



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>6</sup> :</b>  <b>A61F 2/00</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 98/49968</b>  <b>(43) International Publication Date:</b> 12 November 1998 (12.11.98)
<b>(21) International Application Number:</b> PCT/US98/08694  <b>(22) International Filing Date:</b> 30 April 1998 (30.04.98)  <b>(30) Priority Data:</b> 08/850,203                      2 May 1997 (02.05.97)                      US  <b>(71) Applicant (for all designated States except US):</b> OPTICON MEDICAL INC. [US/US]; Suite 106, 2910 Westown Parkway, West Des Moines, IA 50266 (US).  <b>(72) Inventor; and</b> <b>(75) Inventor/Applicant (for US only):</b> SALAMA, Fouad, A. [-/US]; Suite 106, 2910 Westown Parkway, West Des Moines, IA 50266 (US).  <b>(74) Agent:</b> MCKEE, Bruce, W.; Zarley, McKee, Thomte, Voorhees & Sease, Suite 3200, 801 Grand Avenue, Des Moines, IA 50309-2721 (US).		<b>(81) Designated States:</b> AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, GW, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG).  <b>Published</b> <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>
<b>(54) Title:</b> URINARY CONTROL VALVE  <div data-bbox="303 1220 1292 1792"> </div> <b>(57) Abstract</b>  <p>A disc-like valve element (46) in a control valve (10) includes an outer peripheral ring (44) to which leaf elements (50 &amp; 52) are integrally connected having a thickness which increases uniformly from the entire outer peripheral ring (44) to the axial center forming a conical shaped valve element when in a closed condition. The side of the valve element (46) facing the inlet end of the chamber is preferably flat functioning as a funnel to discharge urine when the valve element is moved to an open condition. The increased thickness at the axial center of the valve element (46) is preferably the result of the side of the valve element (46) facing the outlet end (48) of the valve chamber increasing in thickness from the ring (44) laterally inwardly and longitudinally outwardly to maximize flexibility of the leaf elements (50 &amp; 52) adjacent the ring (44) and sealing at the axial center.</p>		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

<b>AL</b>	Albania	<b>ES</b>	Spain	<b>LS</b>	Lesotho	<b>SI</b>	Slovenia
<b>AM</b>	Armenia	<b>FI</b>	Finland	<b>LT</b>	Lithuania	<b>SK</b>	Slovakia
<b>AT</b>	Austria	<b>FR</b>	France	<b>LU</b>	Luxembourg	<b>SN</b>	Senegal
<b>AU</b>	Australia	<b>GA</b>	Gabon	<b>LV</b>	Latvia	<b>SZ</b>	Swaziland
<b>AZ</b>	Azerbaijan	<b>GB</b>	United Kingdom	<b>MC</b>	Monaco	<b>TD</b>	Chad
<b>BA</b>	Bosnia and Herzegovina	<b>GE</b>	Georgia	<b>MD</b>	Republic of Moldova	<b>TG</b>	Togo
<b>BB</b>	Barbados	<b>GH</b>	Ghana	<b>MG</b>	Madagascar	<b>TJ</b>	Tajikistan
<b>BE</b>	Belgium	<b>GN</b>	Guinea	<b>MK</b>	The former Yugoslav Republic of Macedonia	<b>TM</b>	Turkmenistan
<b>BF</b>	Burkina Faso	<b>GR</b>	Greece	<b>ML</b>	Mali	<b>TR</b>	Turkey
<b>BG</b>	Bulgaria	<b>HU</b>	Hungary	<b>MN</b>	Mongolia	<b>TT</b>	Trinidad and Tobago
<b>BJ</b>	Benin	<b>IE</b>	Ireland	<b>MR</b>	Mauritania	<b>UA</b>	Ukraine
<b>BR</b>	Brazil	<b>IL</b>	Israel	<b>MW</b>	Malawi	<b>UG</b>	Uganda
<b>BY</b>	Belarus	<b>IS</b>	Iceland	<b>MX</b>	Mexico	<b>US</b>	United States of America
<b>CA</b>	Canada	<b>IT</b>	Italy	<b>NE</b>	Niger	<b>UZ</b>	Uzbekistan
<b>CF</b>	Central African Republic	<b>JP</b>	Japan	<b>NL</b>	Netherlands	<b>VN</b>	Viet Nam
<b>CG</b>	Congo	<b>KE</b>	Kenya	<b>NO</b>	Norway	<b>YU</b>	Yugoslavia
<b>CH</b>	Switzerland	<b>KG</b>	Kyrgyzstan	<b>NZ</b>	New Zealand	<b>ZW</b>	Zimbabwe
<b>CI</b>	Côte d'Ivoire	<b>KP</b>	Democratic People's Republic of Korea	<b>PL</b>	Poland		
<b>CM</b>	Cameroon	<b>KR</b>	Republic of Korea	<b>PT</b>	Portugal		
<b>CN</b>	China	<b>KZ</b>	Kazakstan	<b>RO</b>	Romania		
<b>CU</b>	Cuba	<b>LC</b>	Saint Lucia	<b>RU</b>	Russian Federation		
<b>CZ</b>	Czech Republic	<b>LI</b>	Liechtenstein	<b>SD</b>	Sudan		
<b>DE</b>	Germany	<b>LK</b>	Sri Lanka	<b>SE</b>	Sweden		
<b>DK</b>	Denmark	<b>LR</b>	Liberia	<b>SG</b>	Singapore		
<b>EE</b>	Estonia						

TITLE: URINARY CONTROL VALVE

## BACKGROUND OF THE INVENTION

This invention relates to a control valve for a urinary catheter. The  
5 valve replaces the bag commonly used with the catheter allowing discharge of  
urine by manual operation of the valve located outside the urethra.

The valve of this invention also is an improvement on my previous valve  
disclosed in Patent No. 4,968,294, November 6, 1990, and Patent No.  
5,306,226, April 26, 1994. My prior valve included valve elements which  
10 extended laterally across the valve chamber but also towards the inlet end of  
the valve chamber. This valve performed very satisfactorily under normal  
conditions and best with higher urethra pressures. Slight leakage sometimes  
occurs at low pressures. The higher the pressure, the more pressure was  
applied to the valve elements to hold them in sealing engagement against each  
15 other in a closed position. Some urine would remain in the valve chamber  
between the valve elements and the chamber sidewall.

Thus, an improved urinary control valve is desired that will  
remain sealed and leak-proof under low pressure conditions and discharge all  
urine when the valve is opened.

20

## SUMMARY OF THE INVENTION

The urinary control valve of this invention involves a valve body having  
a pair of half chamber sections which interface on opposite sides of a disc-like  
valve element. The valve element is of silicone material and includes a ring  
25 around the outer periphery to which a plurality of leaf elements are connected  
and extend inwardly towards an axial center. Thickness of the leaf elements  
increase uniformly from around the entire outer periphery towards the axial  
center to provide maximum flexibility adjacent the ring and maximum sealing  
between contiguous edges of the leaf elements at the axial center. Preferably,  
30 the increased thickness of the leaf elements at the axial center is result of the  
side elements facing the outlet of the chamber tapering laterally inwardly and  
longitudinally outwardly, thus, complementing the urine pressure on the  
opposite side of the leaf elements to cause them to open towards the chamber  
outlet. While a plurality of leaf elements may be used, two are preferred.

The ring of the disc-like valve element limits propagation of the slit formed between the leaf elements and provides for a stable mounting of the valve element on an annular shoulder formed in one half chamber wall with the outer peripheral edge of the other half chamber wall engaging the opposite side of the ring to limit ring movement. The outer edge of one chamber wall includes an annular rib which is received in an annular groove in the other chamber end edge and thus provides for positive sealing of the chamber wall at the interface of the two chamber half wall sections.

The disc-like valve element is opened by applying pressure to the valve body wall at opposite ends of the slit between the leaf elements. The two points where pressure should be applied are located by positioning an inflation tube on the outside of the chamber wall 90° from the opposite ends of the slit.

The side of the disc-like valve element facing the inlet end of the valve chamber is preferably flat thus allowing the valve leaf elements to function as a funnel when they begin to move to an open position towards the outlet end of the valve chamber thus assuring the valve chamber will be completely emptied when the valve is opened.

The thickness of the disc-like valve element at its axial center can vary from 0.031 inches to 0.095 inches with the thickness at the outer ring varying from 0.015 to 0.079. In each instance the increase is 0.016 inches. The preferred embodiment is 0.075 inches at the axial center and 0.059 at its outer periphery. The thickness of the peripheral ring is uniformly 0.062 inches.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is a fragmentary perspective view of the urinary control valve of this invention in a urinary balloon type catheter.

Figure 2 is a cross-sectional view taken along line 2-2 in Figure 1 of the valve body showing the disc-like valve element therein.

Figure 3 is an enlarged perspective view of the valve element.

Figure 4 is an enlarged fragmentary cross-sectional view of the interface of the valve body half chamber sections at their outer edges with each other and the ring of the valve element as indicated by the line 4-4 in Figure 2.

Figure 5 is an enlarged perspective view of the valve element in its closed condition while Figure 6 is a similar view showing the valve element in an open condition.

Figure 7 is a cross-sectional view taken along line 7-7 in Figure 2 showing the valve element in its closed position.

Figure 8 is a view similar to Figure 7 but showing the valve element in an open condition.

Figure 9 is a cross-sectional view taken along line 9-9 in Figure 8 showing the valve element in an open condition.

5        Figures 10-14 are cross-sectional views taken along 10-10 in Figure 5 illustrating valve elements with leaf elements of different thickness and the direction which the leaf elements move to an open position with Figure 11 representing applicant's preferred embodiment.

10        Figure 15 is a perspective view of an alternate embodiment valve element having three leaf elements in a closed position.

Figure 16 is a view similar to Figure 15 but showing the valve element in an open condition.

### DESCRIPTION OF THE PREFERRED EMBODIMENT

15        The urinary control valve of this invention is generally referred to by the Reference 10 in Figure 1 where it is shown as an integral part of a urinary catheter 12. The catheter 12 includes a tube 14 having a urine passageway 16 including an inlet 18 adapted to receive urine from the bladder. An inflatable balloon 20 is provided for seating and sealing the catheter in the bladder as described in my Patent No. 5,306,226. An inflation passageway 22 extends  
20        along the length of the tube 14 and includes an inflation inlet portion 24 adapted to receive inflation liquid or gas from a pump device 26.

25        The tube 14 is connected to a valve body 28 which includes a pair of chamber half sections 30 and 32 having abutting outer peripheral edges 34 and 36 respectively. As seen in Figure 4, the peripheral edge 36 includes an annular rib 38 received in a groove 40 formed in the annular edge 34 of the other chamber half section 30. The thickness of the peripheral edge 36 is reduced to form a shoulder 42 on which a ring 44 of the valve element 46 rests. The thickness of the edge 34 is sufficient to engage the ring 44 opposite the  
30        shoulder 42 to lock the ring in place and limit it against any movement.

      The chamber half section 32 includes an outlet discharge tube portion 48.

35        The valve element 46 is disc-like in shape and includes a pair of leaf elements 50 and 52 which engage each other along contiguous inner edges 54 and 56 respectively. It is seen that the leaf elements 50 and 52 form a slit 58 which extends diametrically across the valve element. The valve elements 50 and 52 uniformly increase in thickness laterally inwardly and axially

outwardly towards the axial center to form a conical shaped surface facing the outlet end 48 of the valve body 28. This construction provides maximum flexibility for the valve leaf elements 50 and 52 adjacent the ring 44 while providing maximum sealing action at the axial center 60 where movement  
5 towards an open position first occurs.

The ring 44 of the silicone valve element 46 limits propagation of the slit 58 which might otherwise occur through repeated opening and closing operations. The valve element 46 is opened by applying pressure as indicated by the arrows 62 at the diametrical opposite ends of the slit 58. These  
10 pressure points on the valve body are located by the user noting that the inflation tube portion 24 is positioned on the valve body 28 at a point 90° from either end of the diametrical slit 58. When pressure is applied to the ring 44 at opposite ends of the slit 58, the leaf elements 50 and 52 deflect axially outwardly in the direction of increased thickness and take on the shape as  
15 shown in Figures 6, 8 and 9. The leaves 50 and 52 are preferably flat on the inlet side 64 and are tapered on the outlet side 66 as seen in Figure 10 thus allowing the fluid pressure on the inlet side 64 to combine with the natural tendency of the leaf elements to open in the direction of the taper on the outlet side. It is seen in Figure 9 that the leaf elements 50 and 52 form a funnel  
20 opening toward the outlet 48 of the valve body 28 thus assuring the valve body 28 is completely emptied through each operation of the control valve 10.

The valve element 46 in Figure 11 represents applicant's preferred embodiment and has an axial center of thickness of 0.075 inches with an outer thickness adjacent the ring 44 of 0.059 inches. The valve element 46A in  
25 Figure 10 has an axial center thickness of 0.095 inches and an outer edge thickness of 0.079 inches. The valve element 46B of Figure 12 has a center axial thickness of 0.031 inches and an outer leaf element thickness of 0.015 inches. In Figure 13, the valve element 46C has an inner axial thickness of 0.062 inches and an outer leaf thickness of 0.046 inches. The ring 44 thickness  
30 is uniformly 0.062 inches.

The arrows 68 in Figures 10-14 indicate the direction of movement for the leaf elements. While it is preferred that the leaf elements open in the direction of the tapered surface, as seen in Figures 10-13, it is seen in the leaf element 46D in Figure 14 that if a taper is provided on both surfaces, they can  
35 open in either direction. In Figure 13, the arrow 68 indicates that while the leaf elements open in the direction of the taper, they also are opening against the fluid pressure in the valve chamber.

A further embodiment of the disc-like element is shown in Figures 15 and 16 and referred to by the Reference 46E and includes three leaf elements 70, 72 and 74 which engage each other along their contiguous inner edges to form slit portions 76, 78 and 80. With this embodiment, while it is preferred  
5 that pressure as indicated by the arrows 82 be applied at the end of the slits, pressure can be applied anywhere around the periphery of the ring 44 to cause the valve elements to move to an open position.

The silicone used in manufacturing the disc valve element 46 is  
10 manufactured by Bayer Silicone under the name Basilone LSR 4050 and is available through Quality Synthetic Rubber, Twinsburg, Ohio. The valve body chamber half sections 30 and 32 are also made from silicone material.

It is thus seen that a urinary control valve of simple construction has been provided which assures non-leak operation through a range of fluid pressures from normal to very low pressure. The pressure required to operate  
15 the valve is minimized while the sealing action between the valve leaf elements is maximized by the conical configuration which provides maximum thickness at the axial center and minimal thickness at their peripheral edges where flexing occurs during the opening and closing operation.

What is claimed is:

1. A urinary control valve comprising, a flexible valve body having inlet and outlet openings at opposite ends of a chamber, a valve means extending  
5 laterally across said chamber between said inlet and outlet openings and having an axial center, said valve means having an outer peripheral edge and including a plurality of flexible leaf sections in a common plane and having contiguous inner edges defining a slit, said contiguous inner edges sealingly engaging each other when said valve means is in a closed position and spaced  
10 apart when in an open position, said leaf sections increase in thickness uniformly from the entire outer peripheral edge toward said axial center and said valve means adapted to move to said open position in response to pressure on opposite sides of said valve body and return to said closed position in response to memory of said flexible leaf sections.  
15
2. The urinary control valve of claim 1 wherein said plurality of flexible leaf sections are defined as two flexible leaf sections which have opposed contiguous inner edges which extend substantially across said chamber.
- 20 3. The urinary control valve of claim 1 wherein said plurality of flexible leaf sections are defined as three flexible leaf sections of equal size and shape, said valve means is adapted to move to said open position in response to pressure on opposite sides of said valve means and return to said closed position in response to memory of said flexible leaf sections.  
25
4. The urinary control valve of claim 1 wherein said leaf sections have oppositely facing sides, and one of said sides is flat and the other side is tapered laterally inwardly and axially outwardly to provide said leaf means with increased thickness at its axial center.  
30
5. The urinary control valve of claim 4 wherein said tapered other side faces said outlet end of said chamber.
- 35 6. The urinary control valve of claim 1 wherein said leaf elements have oppositely facing sides which taper laterally inwardly and axially outwardly to provide said leaf means with increased thickness at its axial center.



7. The urinary control valve of claim 1 wherein said flexible leaf sections are positioned in and integral with a ring along its inner peripheral edge, said ring having an outer peripheral edge and opposite sides, and said chamber being defined by a chamber wall which is engaged by said ring outer peripheral edge.

8. The urinary control valve of claim 7 wherein said chamber is formed by a pair of half chamber sections and said valve means is positioned at the intersection of said half chamber sections.

9. The urinary control valve of claim 4 wherein the thickness of said leaf elements at said increased thickness axial center is between 0.031 inch and 0.095 inch.

10. The urinary control valve of claim 6 wherein the thickness of said leaf sections at said increased thickness axial center is between 0.031 inch and 0.095 inch.

11. The urinary control valve of claim 1 wherein said increase in thickness of said leaf sections at said axial center is approximately 0.016 inch.

12. The urinary control valve of claim 1 wherein said outer periphery edge of said leaf sections is approximately 0.059 inches thick and said axial center is approximately 0.075 inches thick.

13. The urinary control valve of claim 7 wherein said ring is thicker than the outer peripheral edge of said leaf sections whereby lateral outward propagation of said slit will be limited.

14. The urinary control valve of claim 1 wherein a urinary tube is connected to said inlet opening of said valve body, and said urinary tube being adapted to be positioned in a urethra.

15. The urinary control valve of claim 4 wherein a urinary tube is connected to said inlet opening of said valve body, and said urinary tube being adapted to be positioned in a urethra, said tapered one side of said leaf sections faces toward said outlet opening in said valve body whereby the direction of said

taper and the urine pressure on said flat side will cause said leaf sections to open towards said outlet opening.

16. The urinary control valve of claim 8 wherein an annular shoulder is  
5 provided in one of said half chamber sections and said valve means is positioned on said annular shoulder.


17. The urinary control valve of claim 8 wherein an annular shoulder is  
provided in one of said half chamber sections and one side of said ring of said  
10 valve means is positioned on said annular shoulder.




18. The urinary control valve of claim 1 wherein said valve means is injection molded silicone material.








15 19. The urinary control valve of claim 17 wherein said half chamber sections include outer peripheral edges, one of said outer peripheral edges includes an outwardly extending annular rib received in an annular groove in the outer peripheral edge of said other half chamber section.



20 20. The urinary control valve of claim 16 wherein said half chamber sections include outer peripheral edges, said one half chamber section outer peripheral edge being reduced in thickness to form said annular shoulder, and said other outer peripheral edge having a thickness allowing it to engage the other side of said ring and said outer peripheral edge of said one chamber half  
25 section to limit movement of said valve means ring within said chamber.

21. The urinary control valve of claim 2 wherein said valve body includes a urinary tube connected to said inlet opening, and an inflation tube is associated with said urinary tube and includes an inflatable balloon at one end  
30 and an inflation inlet opening means at its opposite end, said valve body having an outside wall surface and said opposite end having said inflation inlet opening means being positioned on the outside surface of said valve body at a point midway between the opposite ends of said slit in said valve element to provide a reference for locating said opposite ends of said slit for applying  
35 pressure to said valve body to open said valve means.

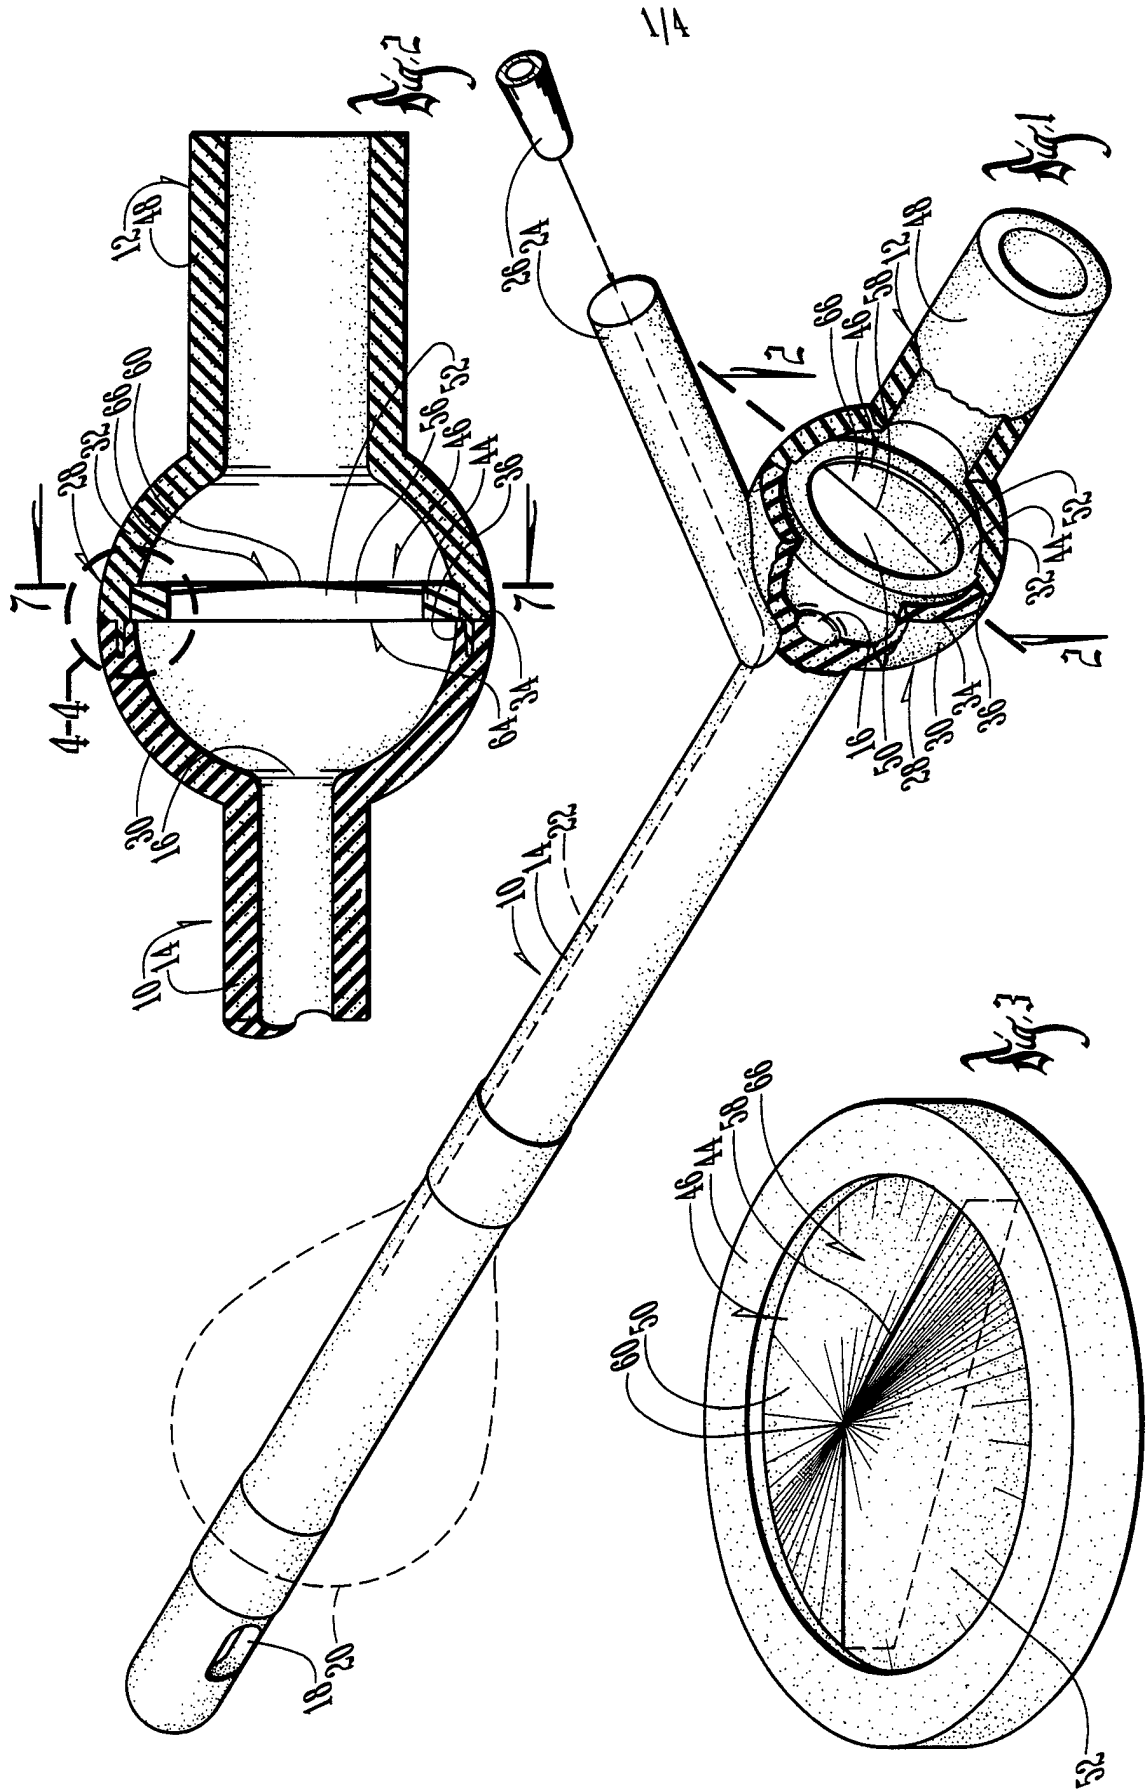

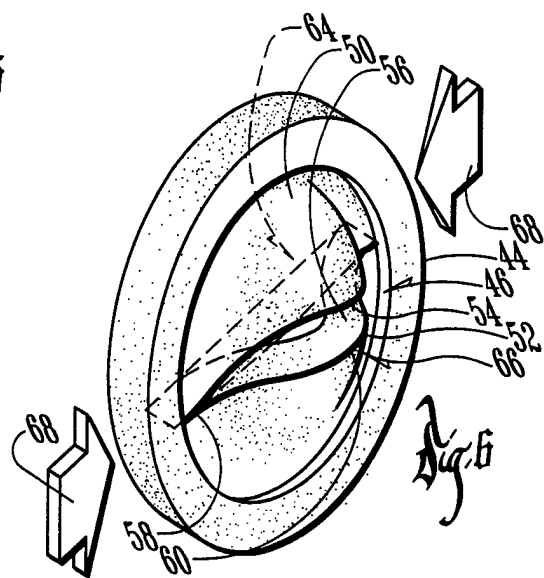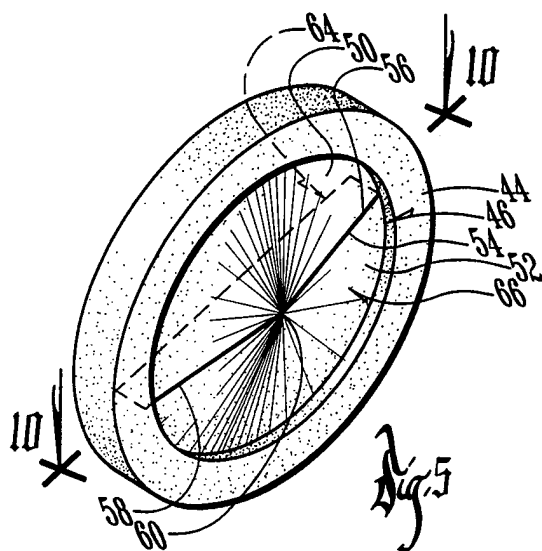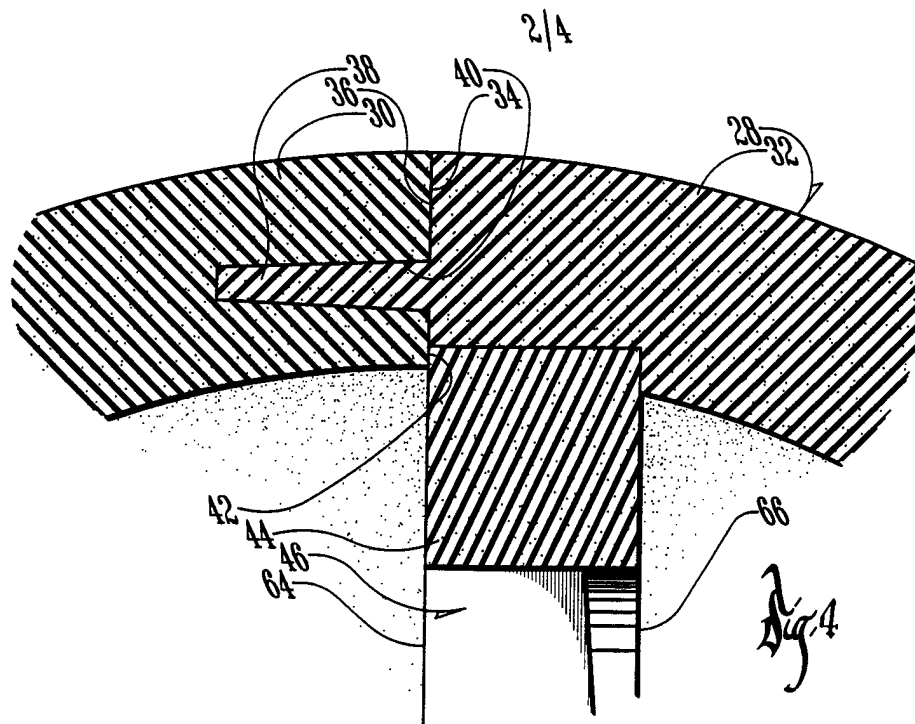

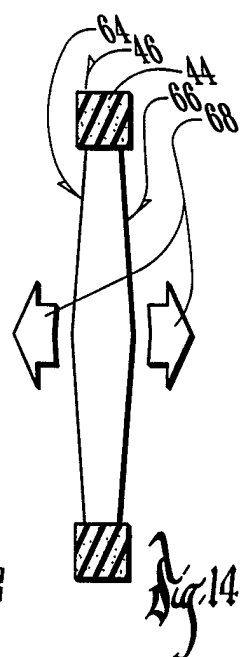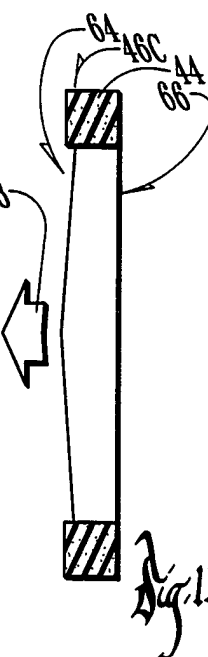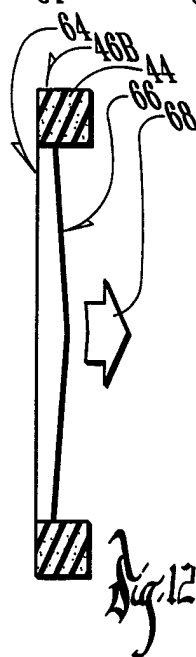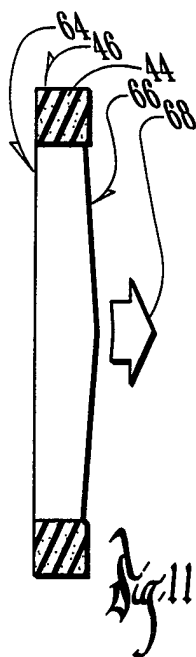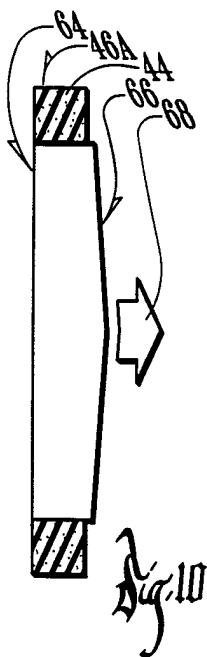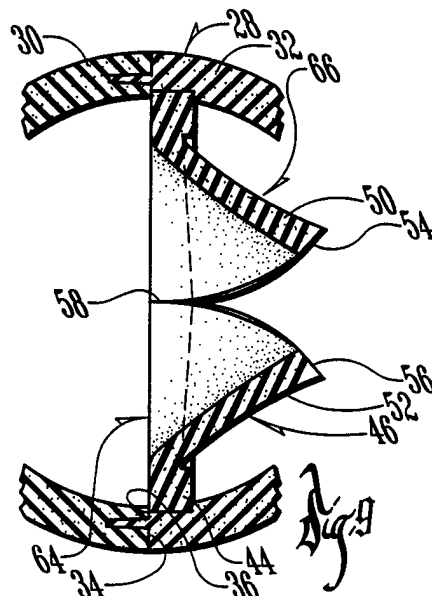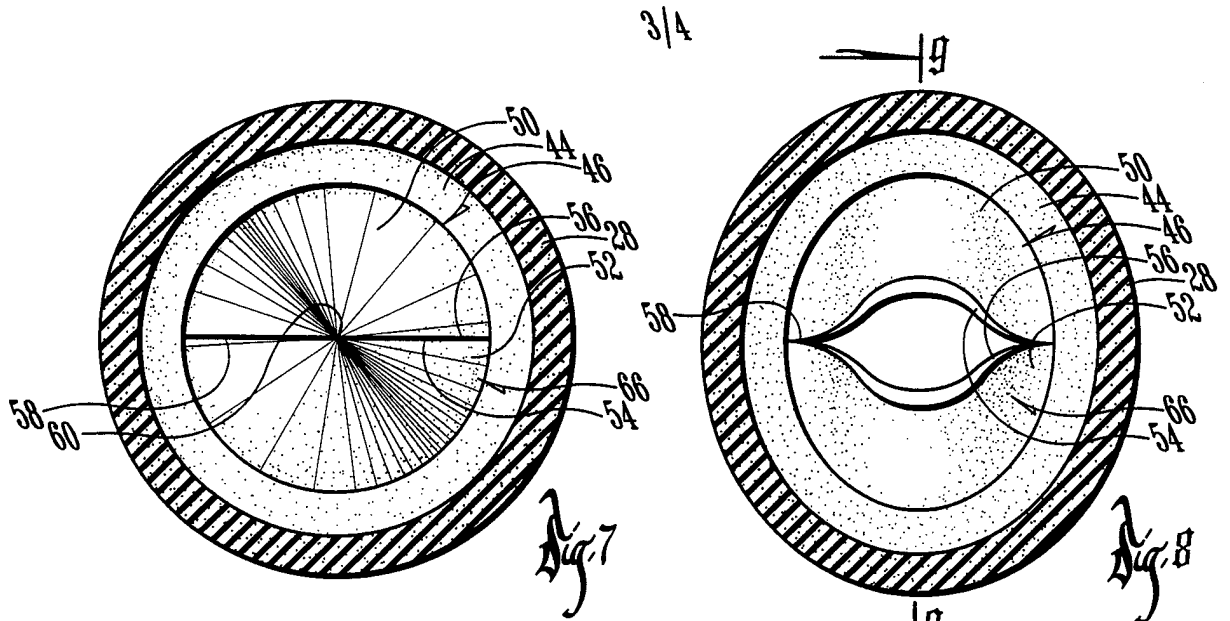

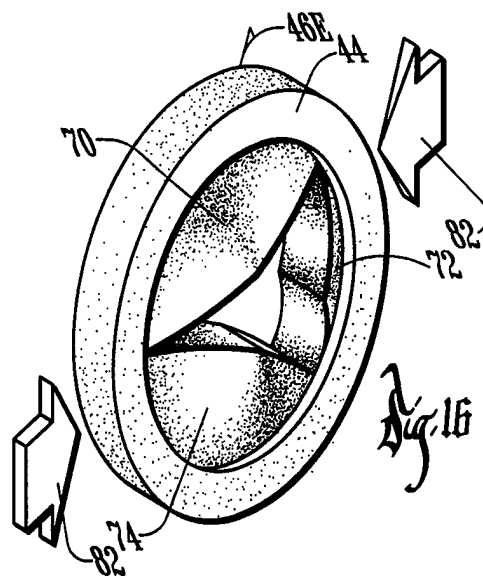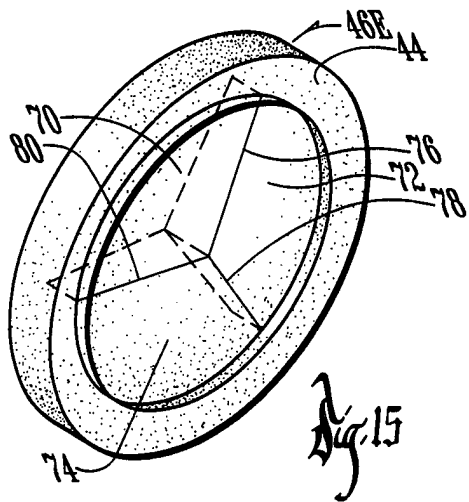

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 98/08694

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61F2/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61F A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 4 968 294 A (SALAMA FOUAD A) 6 November 1990 cited in the application see abstract ---	1
A	US 5 350 363 A (GOODE ROBERTA D ET AL) 27 September 1994 see abstract ---	1
A	US 4 846 784 A (HABER TERRY M) 11 July 1989 ---	
A	US 4 946 449 A (DAVIS JR RICHARD C) 7 August 1990 -----	

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

1 September 1998

Date of mailing of the international search report

10/09/1998

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Sánchez y Sánchez, J

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 98/08694

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 4968294 A	06-11-1990	US 5306226 A US 5634877 A US 5693001 A	26-04-1994 03-06-1997 02-12-1997
US 5350363 A	27-09-1994	US 5538505 A	23-07-1996
US 4846784 A	11-07-1989	AU 616679 B AU 2084388 A EP 0325632 A JP 2500090 T WO 8900030 A	07-11-1991 30-01-1989 02-08-1989 18-01-1990 12-01-1989
US 4946449 A	07-08-1990	NONE	