



(86) Date de dépôt PCT/PCT Filing Date: 2010/03/05

(87) Date publication PCT/PCT Publication Date: 2010/09/10

(45) Date de délivrance/Issue Date: 2017/04/04

(85) Entrée phase nationale/National Entry: 2011/09/06

(86) N° demande PCT/PCT Application No.: EP 2010/052832

(87) N° publication PCT/PCT Publication No.: 2010/100258

(30) Priorité/Priority: 2009/03/06 (EP09305209.0)

(51) Cl.Int./Int.Cl. *A61B 10/02* (2006.01)

(72) Inventeurs/Inventors:

BAUDOUIN, CHRISTOPHE, FR;
ROY, PIERRE, FR;
ELENA, PIERRE-PAUL, FR;
GROUX, HERVE, FR


(73) Propriétaires/Owners:

BAUDOUIN, CHRISTOPHE, FR;
ROY, PIERRE, FR;
ELENA, PIERRE-PAUL, FR;
GROUX, HERVE, FR

(74) Agent: NORTON ROSE FULBRIGHT CANADA
LLP/S.E.N.C.R.L., S.R.L.

(54) Titre : DISPOSITIF PERMETTANT DE REALISER UN ECHANTILLONNAGE DE L'ŒIL

(54) Title: EYE SAMPLING DEVICE

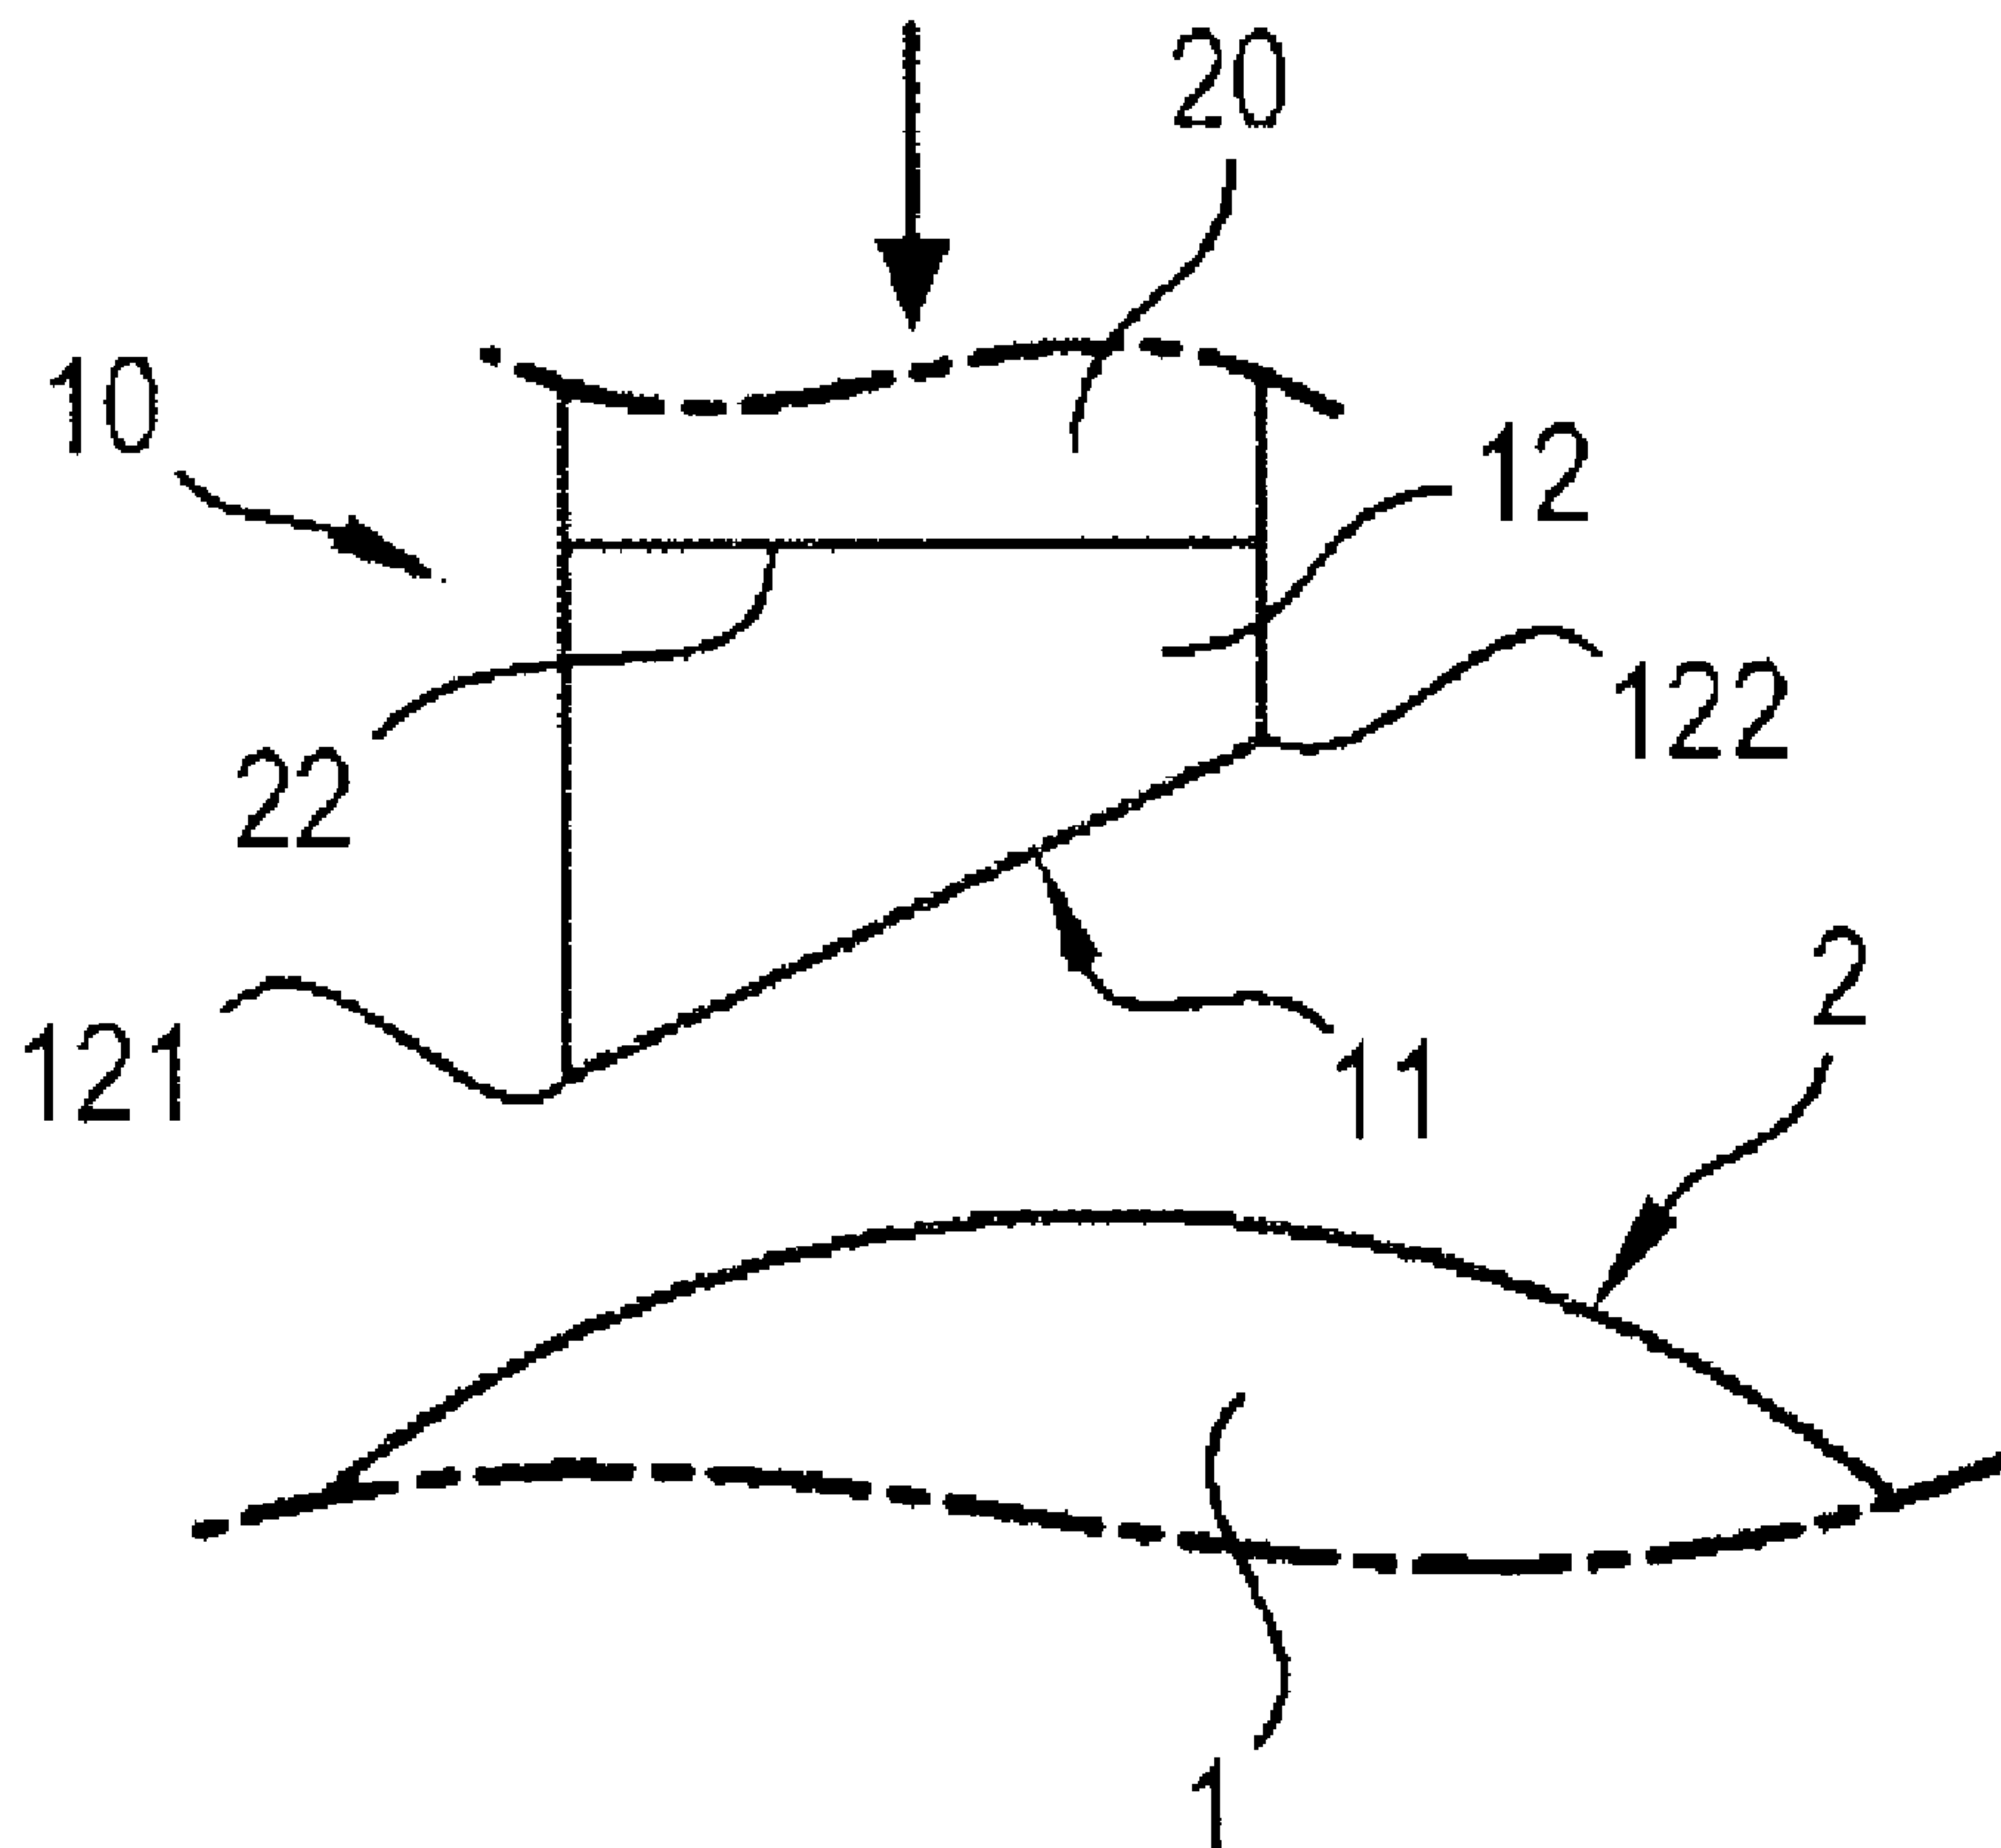

(57) Abrégé/Abstract:

The eye sampling device (10) comprises supporting means (12) comprising a sampling surface (11), the supporting means being elastically deformable between a rest position and a sampling position and conformed so that, upon being used for sampling, the sampling surface applied in the sampling position in a coinciding way onto a sampling area (2), is detached therefrom according to a peeling movement when passing from the sampling position to a rest position.

