



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication: **29.06.2005 Bulletin 2005/26**
(51) Int Cl.7: **G01R 33/28, C07C 69/675, C07C 67/303**
(21) Application number: **04027810.3**
(22) Date of filing: **17.05.2000**

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE

(30) Priority: **19.05.1999 GB 9911681**

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
00929722.7 / 1 179 189

(71) Applicant: **Amersham Health AS**
0401 Oslo (NO)

(72) Inventors:
• **Ardenkjaer-Larsen, Jan Henrik**
205 12 Malmö (SE)
• **Axelsson, Oskar**
205 12 Malmö (SE)

• **Johannesson, Haukur**
205 12 Malmö (SE)
• **Olofsson, Charlotte**
205 12 Malmö (SE)
• **Morgenstjerne, Axel**
205 12 Malmö (SE)
• **Hansson, Georg**
205 12 Malmö (SE)


(74) Representative: **Flechsler, Insa et al**
Amersham plc,
Amersham Place
Little Chalfont, Bucks HP7 9NA (GB)

Remarks:

This application was filed on 24 - 11 - 2004 as a divisional application to the application mentioned under INID code 62.

(54) **Apparatus for hydrogenation**

(57) The present invention provides a hydrogenation apparatus comprising a hydrogenation chamber having a liquid outlet into a conduit leading to a liquid droplet generator inlet to a solvent removal chamber, said hydrogenation chamber having a hydrogen inlet and a solution inlet provided with a further liquid droplet generator, said conduit including a catalyst removal chamber between said hydrogenation chamber and said solvent removal chamber and being provided with a liquid inlet, said solvent removal chamber being provided with a gas outlet and with a liquid outlet.

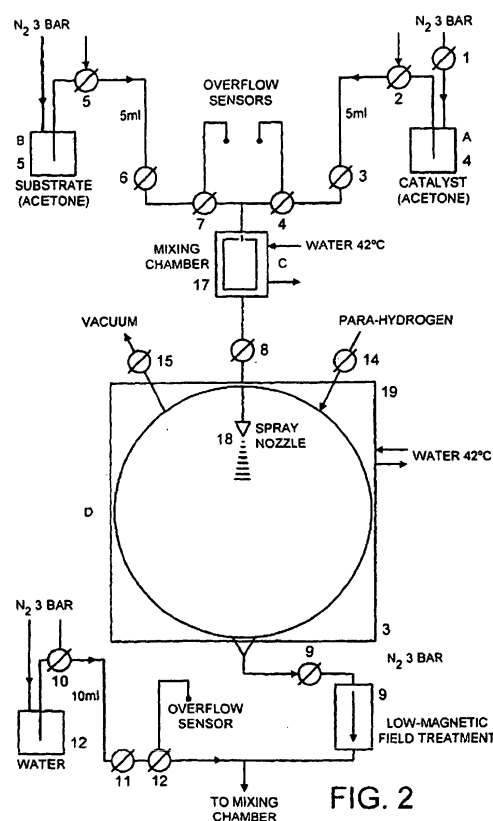

Description

[0001] This invention relates to a process and apparatus for para-hydrogen or ortho-deuterium induced nuclear spin polarization of an unsaturated compound, and more preferably for the preparation of a contrast agent for a magnetic resonance imaging procedure.

[0002] Hydrogen molecules ($^1\text{H}_2$) exist in two different forms, namely para-hydrogen where the nuclear spins are antiparallel and out-of-phase (the singlet state) and ortho-hydrogen where they are parallel or antiparallel and in-phase (the triplet state). At room temperature, the two forms are in equilibrium with an approximately 1:3 ratio of para- to ortho-hydrogen. At 80 K the ratio is about 48:52 and at 20 K it approaches 100:0 (actually about 99.8:0.2).

[0003] In contrast, deuterium (D_2 or $^2\text{H}_2$), where the ^2H nucleus has a nuclear spin (S) of 1 rather than $\frac{1}{2}$, exists in nine different forms, three anti-symmetric para-forms and six symmetric ortho-forms. At ambient temperature, the ratio of ortho-deuterium (o- D_2) to para-deuterium (p- D_2) in an ortho-/para-deuterium mixture is about 2:1, at 60 K it is about 3:1 and at 20 K it is about 98:2. (Deuterium freezes at about 19K).

[0004] In WO99/24080, which is hereby incorporated by reference, it is described how para-hydrogen may be used to catalytically hydrogenate unsaturated compounds, transferring to those compounds the antiparallel proton spins of the para-hydrogen molecule, and transferring nuclear spin polarization from the para-hydrogen deriving protons to non-hydrogen non-zero nuclear spin (i.e. S 0) nuclei in the hydrogenated compound, e.g. ^{13}C or ^{15}N nuclei. In this way, such non-zero spin nuclei may be given a nuclear spin polarization (hyperpolarization) equivalent to that achieved in a kilo Tesla or higher magnetic field. The nuclear magnetic resonance signal emitted by such hyperpolarized nuclei may be used for magnetic resonance imaging in much the same way as has been done with hyperpolarized ^3He -MRI.

[0005] A similar nuclear spin hyperpolarization may likewise be achieved by hydrogenation with deuterium, more particularly with o-deuterium or with hydrogen ($^1\text{H}_2$)/deuterium($^2\text{H}_2$) mixtures, particularly deuterium or hydrogen/deuterium mixtures in which the p/o ratio for hydrogen and the o/p ratio for deuterium are higher than the equilibrium values (1:3 and 2:1) at ambient temperature, e.g. having ratios corresponding to the equilibrium values at temperatures below 80 K, more particularly temperatures below 40 K, especially between liquid helium (4 K) temperatures and 30 K, more especially at temperatures between the melting points of the hydrogen and/or deuterium and 25 K.

[0006] The hydrogenation and/or deuteration, e.g. of an unsaturated bond in a substrate molecule whereby to introduce a ^1H or ^2H atom bound to each of the atoms linked by the unsaturated bond, serves to introduce a hydrogen/deuterium spin distribution into the hydrogenated substrate molecule which is other than the equilibrium distribution at ambient temperature. Where the substrate molecule contains non-zero nuclear spin nuclei (in natural or above natural isotopic abundances), particularly where these non-zero spin (S 0) nuclei are close in the molecular structure of the hydrogenated substrate to the ^1H or ^2H atoms introduced by the hydrogenation, the introduction ^1H or ^2H atoms can induce a nuclear spin distribution in the S 0 nuclei which is other than the equilibrium distribution at ambient temperature. These non-equilibrium nuclear spin distributions for the introduced protons/deuterons and for the S 0 nuclei in the hydrogenated substrate may be harnessed to provide signal enhancement in magnetic resonance imaging (MRI) techniques, including *in vivo* MRI.

[0007] The term "hyperpolarization" is used herein to denote a nuclear spin population distribution for a non-zero nuclear spin imaging nucleus in a hydrogenated substrate which is other than the equilibrium population distribution at ambient to physiological (e.g. 25-40° C) temperatures, more particularly for non-zero nuclear spin imaging nuclei in a hydrogenated substrate a distribution in which the population difference between ground and excited nuclear spin states is greater than the equilibrium population difference.

[0008] By "imaging nuclei" is meant the nuclei in the hydrogenated substrate responsible for the MR signal used in MRI to generate images. Thus, for example, the imaging nucleus might be a ^{13}C or ^{15}N nucleus, generally up to 4 bonds away from a ^1H or ^2H nucleus introduced by hydrogenation of the substrate, or it may be a ^1H or a ^2H nucleus introduced by hydrogenation of a non-symmetric unsaturated substrate. Since the substrate is unsymmetrical the resonance frequencies of the two introduced hydrogens will not be the same.

[0009] While WO99/24080 does describe means by which para-hydrogen hydrogenation may be effected, we have now found that hydrogenation to harness for MRI the p- H_2 and/ or o- D_2 induced hyperpolarization, the hydrogenation reaction is particularly favourably performed by mixing gaseous para-hydrogen and/or ortho-deuterium enriched hydrogen, i.e. where the p:o ratio of $^1\text{H}_2$ is greater than 1:3, particularly greater than 3:7, more particularly greater than 1:1 and/or the o:p ratio of $^2\text{H}_2$ is greater than 3:2, particularly greater than 3:1, more particularly greater than 4:1, with a spray of a solution of the unsaturated compound and a hydrogenation catalyst.

[0010] Viewed from one aspect the invention thus provides a process for the preparation of an MR contrast agent, said process comprising:

- i) obtaining a solution in a solvent of a hydrogenatable, unsaturated substrate compound and a catalyst for the hydrogenation of said substrate compound;
- ii) introducing said solution in droplet form into a chamber containing hydrogen gas (H_2) enriched in para-hydrogen

(p-¹H₂) and/or ortho-deuterium (o-²H₂) whereby to hydrogenate said substrate to form a hydrogenated imaging agent;

iii) optionally subjecting said hydrogenated imaging agent to a magnetic field having a field strength below earth's ambient field strength;

iv) optionally dissolving said imaging agent in an aqueous medium;

v) optionally separating said catalyst from the solution of said imaging agent in said aqueous medium;

vi) optionally separating said solvent from the solution of said imaging agent in said aqueous medium; and

vii) optionally freezing the solution of said imaging agent in said aqueous medium.

[0011] In optional step (iii) of the process of the invention, the hydrogenated imaging agent is subjected to a low magnetic field treatment - this step is desirably effected unless the MR imaging procedure is to use as imaging nuclei deuterons introduced by deuteration with ortho-D₂ (i.e. gas comprising D₂ where the o-D₂:p-D₂ ratio is greater than 2:1). The low field treatment may be effected at any stage following onset of hydrogenation, and indeed the process of the invention may be performed in its entirety in a low field; however it is desirable that the low field treatment occur before water addition (optional step (iv)) in order both to avoid enhancement by the low field of hyperpolarization loss induced by paramagnetic materials which may be present (e.g. as minor impurities, or as dissolved oxygen) in the water and because protons in the water would themselves have a relaxing effect. Accordingly it is preferred that the low field treatment be of the hydrogenation reaction medium (e.g. by placing at least part of the chamber in a low field) and/or of the reaction medium drawn out from the chamber.

[0012] Low field treatment (e.g. at fields below 50 μT, preferably less than 1 μT, most preferably less than 0.1 T) may be achieved by magnetic shielding using commercially available materials, e.g. μ-metal, and may be particularly suitably achieved by disposing some or all of the apparatus used for the process of the invention in a magnetically shielded container such as is described in W099/17304.

[0013] The low magnetic field treatment may alternatively be effected by passage through a twin μ-metal layer tube, capable of giving a field of less than 1 μT, more preferably less than 0.5 μT, most preferably less than 0.1 μT, inside.

[0014] Preferably, the low field treatment may be effected by passage through a magnetically shielded area with a special magnetic field profile. The magnetic screen is a multi-layer tube of μ-metal with the layers arranged so that the sample leaves the earth's magnetic field and enters an area with a field lower than 0.1 μT in just a few ms. The sample is then gradually returned to the earth's magnetic field by a combination of a spiral-shaped tube and a lower degree of magnetic shielding. This effects an efficient transfer of polarization from protons to the hetero-nucleus.

[0015] This cycling of the external magnetic field from "earth-field" to less than 1 μT, preferably about 0.1 μT, and then gradually back again enables polarization to be transferred from protons in the freshly hydrogenated contrast agent to a nucleus within the same molecule with a longer polarization life-time, preferably a ¹³C or ¹⁵N atom. The timing of this process is critical. For the process to work as effectively as possible the sample should leave the earth-field suddenly and then gradually return to earth field. In the present context, "suddenly" means of the order of 1 ms and "gradually" means of the order of 10-10000 ms, preferably 100-1000 ms.

[0016] The magnetic-field screen can be made from μ-metal and can consist of three concentric tubes, for example with diameters of 80, 25 and 12 mm, respectively. At one end of the screen all three layers overlap to give maximal screening and the glass tube is straight and with an inner diameter of, for example 1 mm. From the middle of the screen only the outer layer of screening is kept and the tube spirals out and the inner diameter is increased to, for example 3 mm, to give a more gradual increase in the field. The spiral continues past the screen for a few centimeters.

[0017] The magnetic screen is also equipped with demagnetization coils since the μ-metal is slowly magnetized by external fields, especially in the vicinity of imaging magnets. The demagnetization process involves running AC current of approximately 5 A and 50 Hz through the demagnetization coils and then gradually decreasing the current to zero. The whole process should take between one and a few minutes and preferably be performed on a daily basis. The coils can be made from 1 mm varnished copper wire and can have in total approximately 2000 turns.

[0018] A stopped flow system is where the newly-produced para-hydrogenated product is passed into a resistive magnet (coil) inside a magnetically shielded region. The magnetic screen may be a two-layer tube of μ-metal with such screening capacity that the residual field is less than 0.1 μT when no current is flowing in the coil. Initially, when the sample enters the coil, the current is on to produce a magnetic field of the order of the earth's field. The current is then turned off and then gradually increased back to the original. This effects an efficient transfer of polarization from protons to the hetero-nucleus.

[0019] Most imaging agents will require this low magnetic field treatment for one of two reasons, first that this promotes polarization transfer from the introduced ¹H or ²H nuclei to the imaging nuclei (e.g. ¹³C, ¹⁵N, etc.) and secondly as the treatment transforms the line shape of the MR signal from an anti-phase multiplet with zero integral to a multiplet with a net signal which is good for imaging.

[0020] The hydrogenatable substrate used may be a material such as is discussed in WO99/24080 as a para-hydrogenation substrate. For *in vivo* imaging studies, the substrate is preferably a material which is physiologically tol-

erable both in hydrogenated and unhydrogenated forms. For ^2D -MR studies, the substrate is desirably non-symmetrical about the unsaturated bond which is hydrogenated, especially preferably non-symmetrical within 4 bonds of the unsaturated bond (e.g. $\text{H}_5\text{C}_2\text{OOCCH}_2\text{CH}=\text{CH}-\text{CH}_3$ would be considered to be unsymmetrical within 2 bonds of the ethylenic $\text{C}=\text{C}$ double bond).

[0021] For in vitro or in vivo MR studies of biological or quasi-biological processes or synthetic polymer, e.g. peptide, poly-nucleic acid etc. syntheses, the substrate is preferably hydrogenatable to form a molecule participating in such reactions, e.g. an amino acid, a nucleic acid, a receptor-binding molecule, etc., either a natural such molecule or an analog.

[0022] The solvent used in step (i) of the process of the invention may be any convenient material which serves as a solvent for the substrate and the hydrogenation catalyst. Preferably however it is a volatile organic solvent, e.g. acetone, especially one which is water miscible, especially preferably it is not water, i.e. not $^1\text{H}_2\text{O}$, and especially preferably it is perdeuterated (e.g. $\text{C}^2\text{H}_3\text{OC}^2\text{H}_3$ or d_6 -acetone). Where the imaging agent is for use in in vivo MR investigations, the solvent is preferably physiologically tolerable. Solvent removal (optional process step (vi)) is preferably effected by vacuum, e.g. by spray-flash distillation. Other rapid solvent removal techniques, e.g. affinity techniques, may however be used.

[0023] The solvent is preferably used at or near the minimum quantities required to maintain substrate, catalyst and imaging agent in solution during the hydrogenation reaction. Alternatively, the reaction may be performed directly in water using a water-soluble substrate and a water-soluble catalyst. The process in this case is both simpler and faster as the step of solvent removal is not then required.

[0024] The hydrogenation catalyst is preferably a catalyst as discussed in WO99/24080, e.g. a metal complex, in particular a rhodium complex.

[0025] The enriched hydrogen, which may be pure $^1\text{H}_2$ or $^2\text{H}_2$, or a mixture of $^1\text{H}_2$ and $^2\text{H}_2$ (perhaps containing some HD), optionally containing other gases although preferably free from oxygen or other reactive or paramagnetic gases, may be prepared by cooling hydrogen, i.e. $^1\text{H}_2$, $^2\text{H}_2$ etc., preferably to a temperature below 80 K, more preferably to a temperature below 30 K, still more preferably to a temperature below 22 K, and allowing the nuclear spin states to equilibrate, optionally in the presence of a solid phase equilibration promoter, e.g. Fe_3O_4 , Fe_2O_3 , activated charcoal, etc. The enriched hydrogen is then preferably removed from the equilibrator and optionally stored before use, preferably at a reduced temperature, e.g. 20-80 K. The preparation and storage of enriched hydrogen is described in WO99/24080 the contents of which are incorporated herein by reference.

[0026] For the hydrogenation reaction, enriched hydrogen is filled into a reaction chamber optionally under pressure, e.g. 50 to 100 bar, and the catalyst and substrate solution is introduced in droplet form, e.g. by spraying or atomizing, into this reactor. If desired, the solution may be produced by mixing separate solutions of catalyst and of substrate. To ensure proper mixing, a distributor or a plurality of spray nozzles may be used and the chamber contents may be mixed, e.g. by a mechanical stirrer or by appropriately shaping the chamber walls where there is a flow of reaction mixture in the chamber. The spray nozzles are advantageously of the pneumatic-type where para-hydrogen is used as the atomizing gas. Such nozzles give a better mixing of gas and liquid, smaller droplets and faster spraying than hydrostatic spray nozzles. The process may be performed continuously with a flow reactor, e.g. a loop or tube reactor, or alternatively it may be a batch-wise process. Preferably however there will be a continuous or pulsed flow of enriched hydrogen and solution-spray into the reactor, a continuous or batch-wise removal of liquid solution from the base of the reactor, and a continuous or batch-wise venting of unreacted gas from the reactor. The enriched hydrogen and solution passing into the reactor are preferably temperature-controlled to ensure the gas-droplet phase in the reactor is at the desired temperature. This can be achieved by providing input lines with temperature sensors and heating or cooling jackets.

[0027] Following hydrogenation and any optional, although generally preferred low magnetic field treatment, the imaging agent is preferably mixed with water. The water used is preferably sterile and also preferably essentially free of paramagnetic contaminants. The resultant aqueous solution is then preferably treated to remove the hydrogenation catalyst, e.g. by passage through an ion exchange column, preferably one free of paramagnetic contaminants. The water may be temperature-controlled as may be a mixing chamber where water and imaging agent solutions are mixed so as to ensure the aqueous solution enters the ion exchange column at the appropriate temperature. Strongly acidic, sodium ion charged ion exchange resins such as DOWEX 1 x 2-400 (Dow Chemicals) and Amberlite IR-120 (both available from Aldrich Chemicals) resins may conveniently be used for the removal of typical metal complex hydrogenation catalysts. For fast ion exchange, the resin is preferably cross-linked to only a low degree, e.g. a 2% divinyl benzene cross-linked sulphonated, sodium ion loaded polystyrene resin.

[0028] Removal of the non-aqueous solvent may then conveniently be effected by spray flash distillation - e.g. by spraying the aqueous solution into a chamber, applying a vacuum, and driving the organic solvent free aqueous solution from the chamber using an inert, preferably non-paramagnetic gas, e.g. nitrogen. Indeed in general the flow of liquid components through the hydrogenation apparatus will preferably be effected using applied nitrogen pressure, e.g. 2 to 10 bar.

[0029] The resulting aqueous imaging agent solution may be frozen and stored or alternatively may be used directly in an MR imaging or spectroscopy procedure, optionally after dilution or addition of further solution components, e.g. pH modifiers, complexing agents, etc. Such direct use may for example involve continuous infusion or alternatively injection or infusion of one or more dose units. Bolus injection is particularly interesting.

[0030] The whole process from beginning of hydrogenation to end of solvent removal may conveniently be effected in less than 100 seconds, indeed it is feasible to produce dosage units in as little as 10 to 20 seconds, which is substantially less than T_1 for the imaging nuclei in many of the imaging agents in the contrast media so produced.

[0031] Desirably, the surfaces contacted by the imaging agent during the process of the invention are substantially free of paramagnetic materials, e.g. made of glasses as used for hyperpolarized ^3He containment as discussed in WO99/17304 or gold or a deuterated polymer. Surfaces contacting the non-aqueous solvent (e.g. acetone) should be acetone-resistant and valves may be magnetically controlled with solvent resistant Teflon or silicon parts.

[0032] The process of the invention may conveniently be automated and computer-controlled.

[0033] Viewed from a further aspect the invention provides a hydrogenation apparatus comprising a hydrogenation chamber having a liquid outlet into a conduit leading to a liquid droplet generator inlet (e.g. a spray nozzle) to a solvent removal chamber, said hydrogenation chamber having a hydrogen inlet and a solution inlet provided with a further liquid droplet generator, said conduit including a catalyst removal chamber, e.g. containing an ion exchange resin between said hydrogenation chamber and said solvent removal chamber and being provided, preferably between said hydrogenation chamber and said catalyst removal chamber, with a liquid inlet, e.g. a water inlet, said solvent removal chamber being provided with a gas outlet, e.g. attached to a vacuum source and with a liquid outlet, e.g. to an optional formulation chamber and thence to administration means or to a dose unit receiver, e.g. a syringe, and said hydrogenation apparatus being further provided with magnetic shielding such that the magnetic field within at least part of said hydrogenation chamber and/ or within at least part of said conduit (preferably the part upstream of the liquid (water) inlet) is $<50 \mu\text{T}$, more preferably $<1 \mu\text{T}$, most preferably $<0.1 \mu\text{T}$.

[0034] Clearly, if the process of the invention is performed directly in water using a water-soluble substrate and water-soluble catalyst, then the solvent removal chamber is not required.

[0035] The apparatus of the invention is preferably also provided with reservoirs and mixing chambers appropriate for the materials being fed in, e.g. an enriched hydrogen reservoir, a water reservoir, a reservoir for solutions of hydrogenation catalyst and/or hydrogenatable substrate, reservoirs for further contrast medium components, a mixing chamber for mixing solutions of catalyst and substrate, a mixing chamber for mixing water with the solution exiting the hydrogenation chamber, etc. Likewise the hydrogenation chamber is preferably provided with a vent for removing hydrogen and various of the chambers and reservoirs are preferably provided with nitrogen sources and nitrogen inlets to drive their contents into or through the apparatus. Particularly preferably, the apparatus also includes an enriched hydrogen generator, valves, valve actuators and a computer control for controlling apparatus operation.

[0036] The magnetic shielding is preferably removable so that it can be removed if ^2H -imaging is desired.

[0037] The chambers and conduits of the apparatus of the invention are preferably sealable to prevent ingress of air; moreover, the apparatus is preferably provided with valves and ports arrangeable to permit degassing, in particular to remove surface adsorbed oxygen.

[0038] The water input to the apparatus of the invention is preferably deoxygenated, e.g. by treatment with nitrogen.

[0039] The "chambers" in the apparatus of the invention may have internal cross-sectional areas which are larger than the internal cross-sectional areas of the chamber inlets or outlets (in the flow direction); alternatively the cross-sectional areas in the flow direction may be substantially invariant, i.e. a tube may function as inlet-chamber-outlet.

[0040] The use of homogeneously catalysed "spray-hydrogenation" in the preparation of MR contrast agents is new. Likewise such hydrogenation is new in the preparation of amino acids and pharmaceuticals. The procedure is rapid and efficient and this forms a further aspect of the invention. Viewed from this aspect the invention provides a process for the preparation of an amino acid, a pharmaceutical or an *in vivo* diagnostic agent, characterized in that said process comprises a hydrogenation step in which a solution of a substrate and a hydrogenation catalyst is sprayed into a hydrogen-containing chamber.

[0041] Where the hydrogenation is effected using a gas in which the $^2\text{H}:^1\text{H}$ ratio is in excess of 9:1, using $p\text{-D}_2$, the use of heterogenous catalysis is also contemplated - in this event catalyst removal may involve filtering or other particulate removal techniques.

[0042] The contents of all publications referred to herein are hereby incorporated by reference.

[0043] Embodiments of the process and apparatus of the invention will now be described with reference to the following non-limiting Example and to the accompanying drawings, in which:

Figure 1 is a schematic view of one apparatus according to the invention;
Figure 2 is a schematic view of part of the apparatus of Figure 1;
Figure 3 is a schematic view of a further part of the apparatus of Figure 1; and
Figure 4 is a schematic view of a further aspect of the present invention.

[0044] Referring to Figure 1, hydrogen ($^1\text{H}_2$) from cylinder **1** is fed via tube **2** to a p- $^1\text{H}_2$ generator and thence into hydrogenation chamber **3**. A hydrogenation catalyst solution from reservoir **4** and a hydrogenatable substrate solution from reservoir **5** are fed via lines **6** and **7** to a spray nozzle in chamber **3**. The liquid settling in chamber **3** passes via conduit **8** through a twin μ -metal layered tube **9**, a magnetic shield having an internal field of less than $0.1 \mu\text{T}$, into an ion exchange column **10** and thence to a spray nozzle in the solvent removal chamber **11**. Before the liquid enters the ion exchange column but after it exits the magnetic shielding, water from reservoir **12** is added via tube **13**. Solvent removal chamber **11** is connected via tube **14** to a vacuum pump **15** which serves to remove non-aqueous solvent, e. g. acetone. The liquid remaining in chamber **11** is removed via exit duct **16**.

[0045] Referring to Figure 2, it can be seen that nitrogen (at 3 bar) is used to drive catalyst and substrate solutions from reservoirs **4** and **5** to a water-jacketed mixing chamber **17** and thence to the spray nozzle **18** (which may be pneumatic) in hydrogenation chamber **3** which is provided with a valved hydrogen vent **19**. Alternatively, the dosage and mixing of substrate and catalyst may be controlled by computer controlled pumps (not shown). Nitrogen may be used to drive the liquid collecting in the hydrogenation chamber through the magnetic shielding **9** to mix with nitrogen driven water from reservoir **12**.

[0046] Turning to Figure 3, the solution/water mixture passes into water-jacketed mixing chamber **20** and thence through a 2 to 4 cm long ion exchange column **10** containing 400 mesh sulphonated polystyrene/2% DVB and on to spray nozzle **21** in solvent removal chamber **11**. To ensure complete non-aqueous solvent removal, the chamber **11** is buffered with a cooling trap (not shown) followed by a second volume before the vacuum pump - this relieves the very sudden load otherwise put on the pump. After release from the chamber **11**, the aqueous "contrast medium" is ready for use; alternatively its pH may be buffered and its ion profile adjusted (e.g. to add plasma cations).

[0047] There are two preferred modes of operation; in one the apparatus is used to fill a syringe which is removed and the contrast medium is injected; in the second, the apparatus delivers small doses of contrast medium continuously to a catheter linked to the patient. The second mode allows for easier imaging since the operator can adjust the MR imager to obtain a satisfactory image.

[0048] Referring to Figure 4, the hyperpolarized solution is delivered by the apparatus **30** into a syringe **31**. A 3-way switching valve **32** is connected. The syringe should be positioned vertically with the plunger-handle up to ensure the solution is free of air. By switching the valve **32** the solution can be injected to the transfer tube **33**. A syringe or cavity **34** with determined volume and low friction is connected just before the injection target **35**, and the syringe **34** absorbs the dead space and possible gas bubbles.

EXAMPLE 1

[0049] A solution of (bicyclo[2.2.1]hepta-2,5-diene)-[1,4-bis(diphenylphosphino)butane]-rhodium(I) tetrafluoroborate (93.5mg) in argon-bubbled acetone (5ml) is charged in chamber A and a solution of 2-acetoxy-acrylic acid (110mg, 0.85mmol) in argon-bubbled acetone (5ml) in chamber B. Chamber E is filled with distilled, argon-bubbled water. Ion exchange resin of type sulphonated polystyrene, 2% cross-linked, swelled with water and charged with sodium ions is loaded in the ion-exchange column. Water at 42°C is circulated through the jackets in the set-up. The experiment is started by running a computer program that controls the valves according to scheme 1 as shown in Table 1 below. The program is written in LabView. After the program is finished the sample of aqueous hyperpolarized O-acetyl lactic acid is removed at the bottom of chamber G by a syringe.

[0050] A $3\text{m}^3/\text{hr}$ 2-stage diaphragm pump is used to provide the vacuum and 3 bar of nitrogen is used as the driving pressure.

[0051] The spray nozzles are ordinary commercial oil-burner nozzles, the one in chamber D is specified as 1.5 US gallon/hr with a 60° cone angle, the one in chamber G is 1.0 US gallon/hr with a 80° cone angle.

[0052] The magnetic valves are 8 W, 24 V DC with gaskets of EPDM.

[0053] The magnetic screen is made from two concentric tubes of μ -metal.

Table 1

Valve No. Time/s	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	Comment
0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	Start
1	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	Pressurize
1	0	0	0	0	0	0	0	0	0	1	1	0	0	0	0	0	0	0	Fill water loop until overflow is detected
1	1	1	0	1	1	0	0	0	0	0	0	0	0	0	0	0	0	0	Fill catalyst and substrate loops until overflow is detected
0.2	0	0	0	1	0	1	1	0	0	0	0	0	0	0	0	0	0	0	Add catalyst and substrate to C intermittently
0.2	0	0	1	1	0	0	1	0	0	0	0	0	0	0	0	0	0	0	Loop 15 times
10	0	0	1	1	0	1	1	0	0	0	0	0	0	0	1	0	0	0	Allow pressure to build up in C, evacuate D
10	0	0	0	0	0	0	0	0	0	0	0	0	1	1	0	1	0	0	Fill D with para-hydrogen, evacuate G
12	0	0	1	0	0	1	0	1	0	0	0	0	1	0	0	1	0	0	Spray mixture into D and dry overflow sensors
5	0	0	0	0	0	0	0	1	1	0	0	0	0	0	0	1	0	0	Suck reaction mixture to F
8	0	0	0	0	0	0	0	0	0	0	1	1	0	0	0	1	0	0	Add water and mix
20	0	0	0	0	0	0	0	0	0	0	1	1	1	0	0	1	0	0	Spray into G
3	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	1	1	Increase pressure in G
3	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	1	0	Equilibrate pressure in G with atmosphere
0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	Finished

EXAMPLE 2

[0054] The hyperpolarized solution is delivered by the para-hydrogen contrast agent apparatus to which a tube of length e.g. 50 mm is connected. A 3-way switching valve is connected to this tube, as a syringe. The syringe is placed vertically with the plunger pointing up to ensure the solution is free from air. The bubbles will float to the top and stay there. By switching the valve the solution can be injected into the transfer tube e.g. of length 3200 mm and a diameter of 0.76 mm. This gives a dead-volume of 1.5 ml. Just before the cannula "injection target" (e.g. a venflon or butterfly) a syringe with determined volume and low friction is connected with a 3-way tube. This syringe will collect the dead space and possible gas bubbles from transfer tubes. The plunger of the syringe is prevented from leaving the barrel by a stop-screw. When the syringe is full, the injected solution proceeds by the cannula to the target. Syringes with ground-glass barrel and plunger are suitable for this set-up.


[0055] With the equipment described above it was possible to inject 0.33 ml/s of physiological saline into the tail-vein of a rat.

Claims

1. A hydrogenation apparatus comprising a hydrogenation chamber having a liquid outlet into a conduit leading to a liquid droplet generator inlet to a solvent removal chamber, said hydrogenation chamber having a hydrogen inlet and a solution inlet provided with a further liquid droplet generator, said conduit including a catalyst removal chamber between said hydrogenation chamber and said solvent removal chamber and being provided with a liquid inlet, said solvent removal chamber being provided with a gas outlet and with a liquid outlet.
2. An apparatus as claimed in claim 1 wherein said hydrogenation apparatus is further provided with magnetic shielding such that the magnetic field within at least part of said hydrogenation chamber and/or within at least part of said conduit is $< 50 \mu\text{T}$.
3. An apparatus as claimed in claim 2 wherein said magnetic field is $< 1 \mu\text{T}$.
4. An apparatus as claimed in claim 2 wherein said magnetic field is $< 0.1 \mu\text{T}$.
5. An apparatus as claimed in any one of claims 1 to 4 wherein said conduit is provided with a liquid inlet between said hydrogenation chamber and said catalyst removal chamber.
6. A process for the preparation of an MR contrast agent, said process comprising:
 - i) obtaining a solution in a solvent of a hydrogenatable, unsaturated substrate compound and a catalyst for the hydrogenation of said substrate compound;
 - ii) introducing said solution in droplet form into a chamber containing hydrogen gas (H_2) enriched in para-hydrogen ($p\text{-}^1\text{H}_2$) and/or ortho-deuterium ($o\text{-}^2\text{H}_2$) whereby to hydrogenate said substrate to form a hydrogenated imaging agent;
 - iii) optionally subjecting said hydrogenated imaging agent to a magnetic field having a field strength below earth's ambient field strength;
 - iv) optionally dissolving said imaging agent in an aqueous medium;
 - v) optionally separating said catalyst from the solution of said imaging agent in said aqueous medium;
 - vi) optionally separating said solvent from the solution of said imaging agent in said aqueous medium; and
 - vii) optionally freezing the solution of said imaging agent in said aqueous medium.
7. A process as claimed in claim 6 wherein said field strength in step (iii) is less than $50 \mu\text{T}$.
8. A process as claimed in claim 6 wherein said field strength in step (iii) is less than $1 \mu\text{T}$.
9. A process as claimed in claim 6 wherein said field strength in step (iii) is less than or equal to $0.1 \mu\text{T}$.
10. A process as claimed in claim 6 wherein said field strength in step (iii) is cycled from earth's ambient field strength to a field strength less than $0.1 \mu\text{T}$, then back to ambient field strength again.

EP 1 548 454 A1

11. A process as claimed in claim 10 wherein the first part of the cycle is of the order of ≈ 1 ms and the second part is of the order of 10 - 10000 ms.
12. A process as claimed in any one of the preceding claims wherein said process is carried out directly in water and wherein both said substrate and said catalyst are water-soluble.
13. A process for the preparation of an amino acid, a pharmaceutical or an in vivo diagnostic agent, **characterized in that** said process comprises a hydrogenation step in which a solution of a substrate and a hydrogenation catalyst is sprayed into a chamber containing hydrogen gas enriched in para-hydrogen and/or ortho-deuterium.

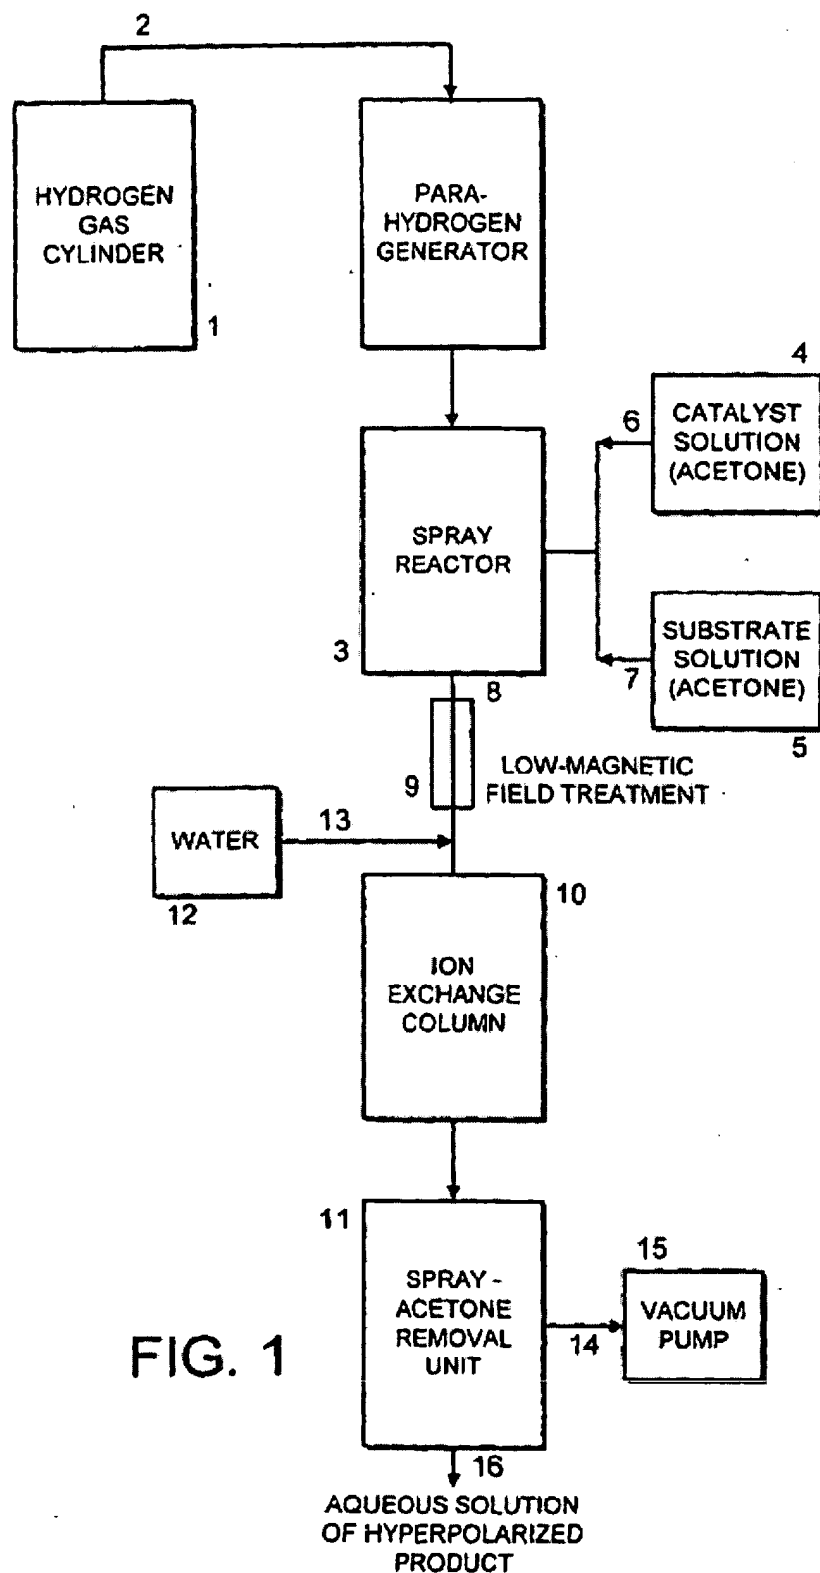

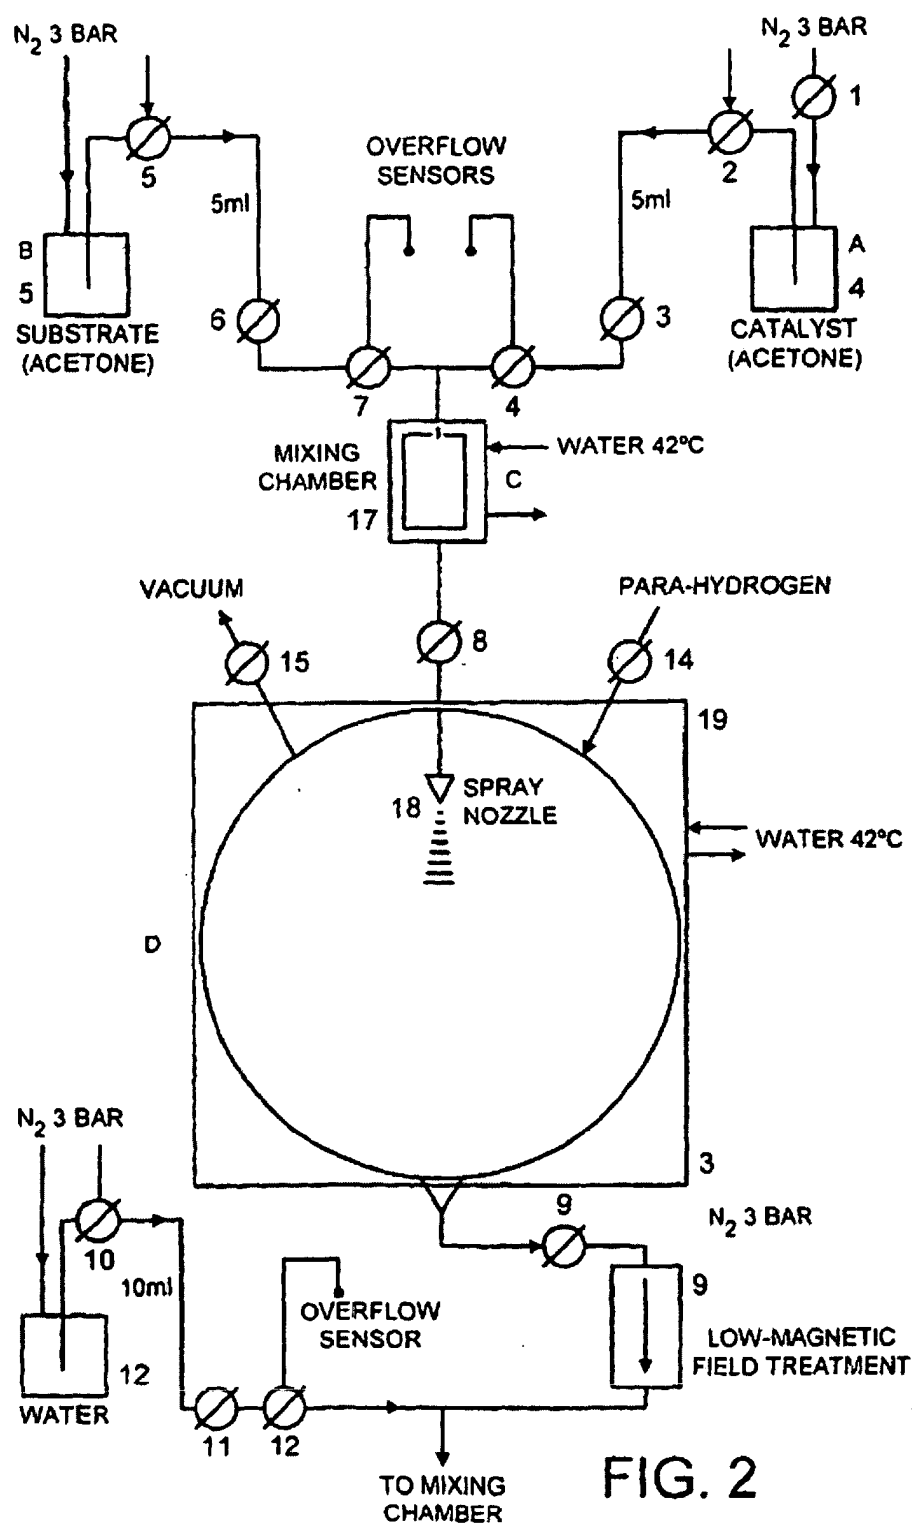


FIG. 2


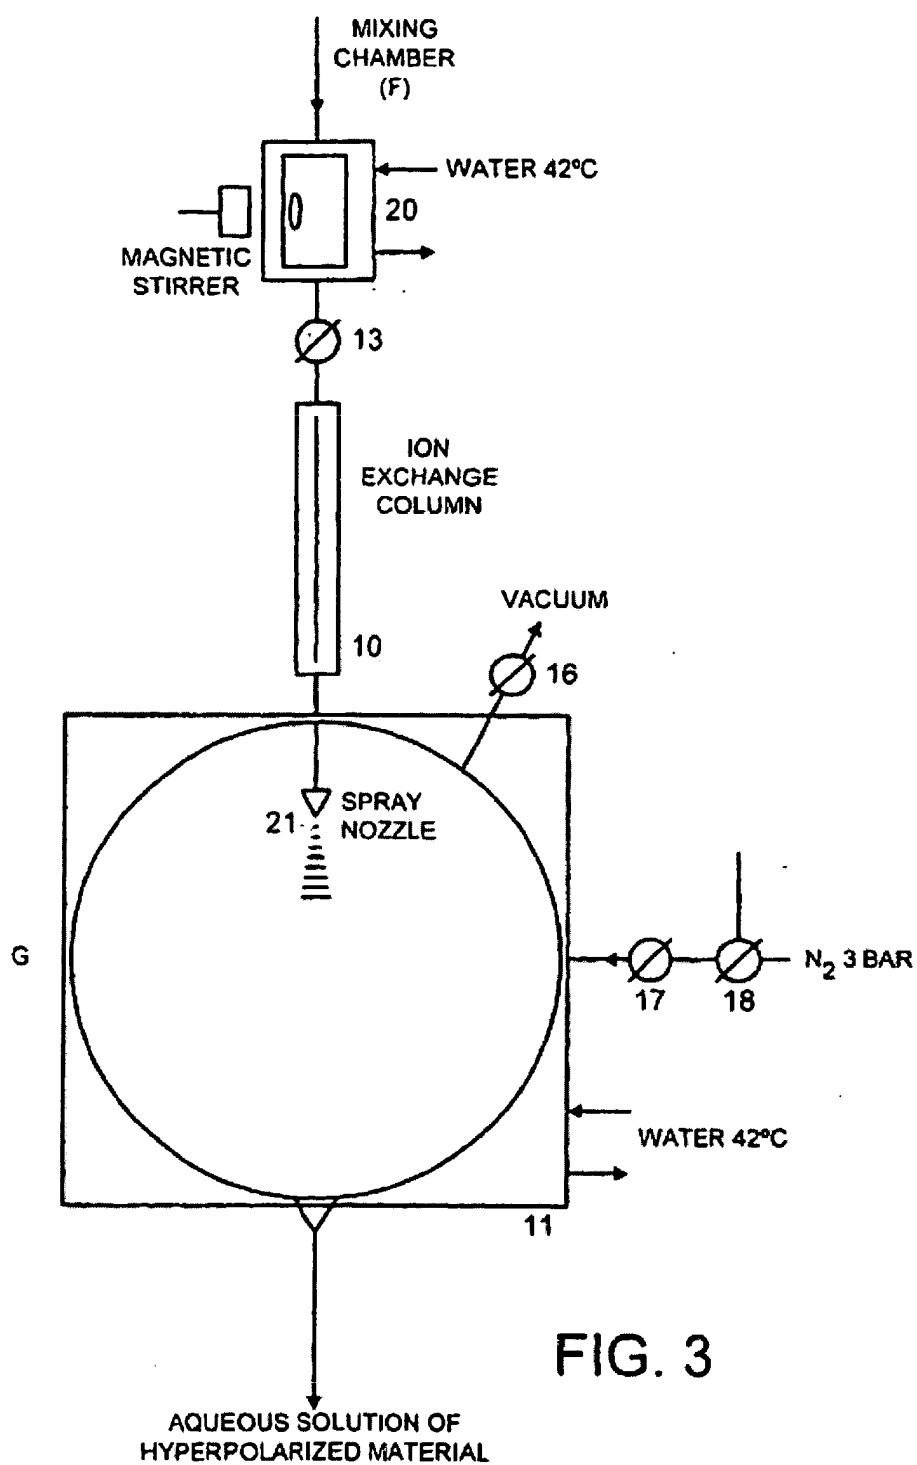


FIG. 3



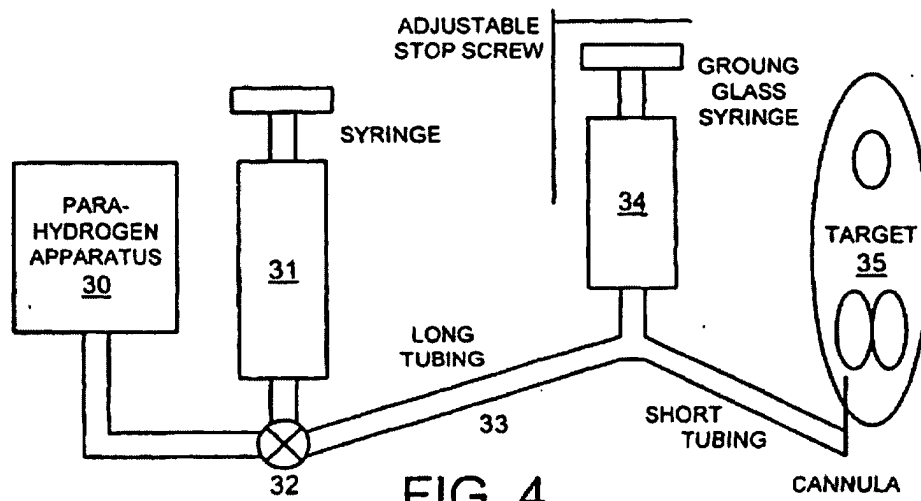

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 04 02 7810

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
X	HARTHUN A ET AL: "The Use of in situ NMR Spectroscopy and Parahydrogen as Tools for Chiral Synthesis" TETRAHEDRON LETTERS,NL,ELSEVIER SCIENCE PUBLISHERS, AMSTERDAM, vol. 36, no. 41, 9 October 1995 (1995-10-09), pages 7423-7426, XP004027014 ISSN: 0040-4039 * the whole document *	1-13	G01R33/28 C07C69/675 C07C67/303 A61K49/18
E	WO 00/40988 A (COOK NEIL ;KNOX PETER (GB); NYCOMED AMERSHAM PLC (GB); AXELSSON OK) 13 July 2000 (2000-07-13) * page 13, line 21 - page 14, line 21 *	1-13	
X	BARKEMEYER ET AL: "Hetero-NMR enhancement via parahydrogen" JOURNAL OF THE AMERICAN CHEMICAL SOCIETY,US,AMERICAN CHEMICAL SOCIETY, WASHINGTON, DC, vol. 117, 1995, pages 2927-2928, XP002094737 ISSN: 0002-7863 * the whole document *	6-13	TECHNICAL FIELDS SEARCHED (Int.Cl.7) A61K G01R C07C
D,P, X	WO 99/24080 A (COCKBAIN JULIAN ;NYCOMED IMAGING AS (NO); JOHANNESON HAUKEUR (SE);) 20 May 1999 (1999-05-20) * example 5 *	6-13	
X	WO 98/30918 A (COCKBAIN JULIAN R M ;NYCOMED IMAGING AS (NO); PETTERSSON STEFAN (S) 16 July 1998 (1998-07-16) * examples * * claims *	6-13	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 25 April 2005	Examiner Dullaart, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

5

EPO FORM 1503 03/82 (P04C01)



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 04 02 7810

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
Y	NATTERER J ET AL: "PARAHYDROGEN INDUCED POLARIZATION" PROGRESS IN NUCLEAR MAGNETIC RESONANCE SPECTROSCOPY,GB,PERGAMON PRESS, OXFORD, vol. 31, no. 4, November 1997 (1997-11), pages 293-315, XP000882257 ISSN: 0079-6565 * page 310; figure 12 * * page 310, paragraph 5.5 - page 311, left-hand column *	6-13	
Y	BROWN, JOHN M. ET AL: "Stereoselective homogeneous hydrogenation of 3-substituted itaconate esters" J. CHEM. SOC., CHEM. COMMUN., no. 3, 1987, pages 181-182, XP002160814 * the whole document *	6-13	
Y	US 4 194 051 A (BACHMAN GERALD L ET AL) 18 March 1980 (1980-03-18) * example III *	6-13	
			TECHNICAL FIELDS SEARCHED (Int.Cl.7)
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 25 April 2005	Examiner Dullaart, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

5

EPO FORM 1503 03/82 (P04/C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 04 02 7810

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

25-04-2005

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 0040988	A	13-07-2000	AU 766923 B2	23-10-2003
			AU 1880300 A	24-07-2000
			CA 2356442 A1	13-07-2000
			EP 1141738 A1	10-10-2001
			WO 0040988 A1	13-07-2000
			JP 2002534687 T	15-10-2002

WO 9924080	A	20-05-1999	AU 1047399 A	31-05-1999
			CN 1306441 A	01-08-2001
			EP 1047455 A1	02-11-2000
			WO 9924080 A1	20-05-1999
			JP 2001522819 T	20-11-2001
			NO 20002429 A	10-05-2000
			RU 2218182 C2	10-12-2003
			US 2004024307 A1	05-02-2004
			US 6574495 B1	03-06-2003
			AU 752308 B2	12-09-2002
			AU 1775399 A	26-07-1999
			AU 8119298 A	04-01-1999
			BR 9813244 A	10-10-2000
			CA 2290808 A1	23-12-1998
			CA 2317526 A1	15-07-1999
			CN 1269015 A	04-10-2000
			CN 1285044 A ,C	21-02-2001
			CN 1527066 A	08-09-2004
			EP 0990168 A1	05-04-2000
			EP 1046051 A1	25-10-2000
			WO 9858272 A1	23-12-1998
			WO 9935508 A1	15-07-1999
			HU 0102093 A2	28-09-2001
			JP 2002508687 T	19-03-2002
			JP 2002501006 T	15-01-2002
			NO 996173 A	15-02-2000
			NO 20003251 A	22-06-2000
			NZ 505151 A	26-11-2002
			RU 2221255 C2	10-01-2004
			US 6278893 B1	21-08-2001
			US 6311086 B1	30-10-2001
			US 6466814 B1	15-10-2002

WO 9830918	A	16-07-1998	AT 256293 T	15-12-2003
			AU 5335298 A	03-08-1998
			DE 69820415 D1	22-01-2004
			DE 69820415 T2	16-09-2004
			EP 0951650 A1	27-10-1999
			WO 9830918 A1	16-07-1998

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 04 02 7810

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

25-04-2005

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9830918 A		JP 2001513661 T	04-09-2001
		US 6453188 B1	17-09-2002

US 4194051 A	18-03-1980	AU 499782 B2	03-05-1979
		AU 1709476 A	02-03-1978
		BE 845454 A1	24-02-1977
		BR 7605568 A	09-08-1977
		CA 1086771 A1	30-09-1980
		CH 624088 A5	15-07-1981
		DE 2638070 A1	10-03-1977
		FR 2322126 A1	25-03-1977
		GB 1501558 A	15-02-1978
		JP 1223604 C	15-08-1984
		JP 52027716 A	02-03-1977
		JP 58050207 B	09-11-1983
		NL 7609340 A	01-03-1977
