

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2015/055715 A1

(43) International Publication Date

23 April 2015 (23.04.2015)

WIPO | PCT

(51) International Patent Classification:

G01N 27/327 (2006.01) G01N 33/487 (2006.01)  
A61B 5/00 (2006.01) G06F 19/00 (2011.01)

(71) Applicant (for US only): ROCHE DIAGNOSTICS OPERATIONS, INC. [US/US]; 9115 Hague Road, Indianapolis, Indiana 46250-0457 (US).

(21) International Application Number:

PCT/EP2014/072114

(72) Inventors: SAMS, Howard; 1518 Prestwick Circle, Carmel, Indiana 46032 (US). STAUBERT, Andreas; Wellering 16, 67098 Bad Duerkheim (DE).

(22) International Filing Date:

15 October 2014 (15.10.2014)

(74) Agents: POREDDA, Andreas et al.; Roche Diagnostics GmbH, Patent Department, Sandhofer Strasse 116, 68305 Mannheim (DE).

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/891,736 16 October 2013 (16.10.2013) US  
61/891,656 16 October 2013 (16.10.2013) US

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.


(71) Applicant (for DE only): ROCHE DIAGNOSTICS GMBH [DE/DE]; Sandhofer Straße 116, 68305 Mannheim (DE).

(71) Applicant (for all designated States except DE, US): F. HOFFMANN-LA ROCHE AG [CH/CH]; Grenzacher Strasse 124, CH-4070 Basel (CH).

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,

[Continued on next page]

(54) Title: COMMUNICATION INTERFACE CLIP FOR A HANDHELD MEDICAL DEVICE

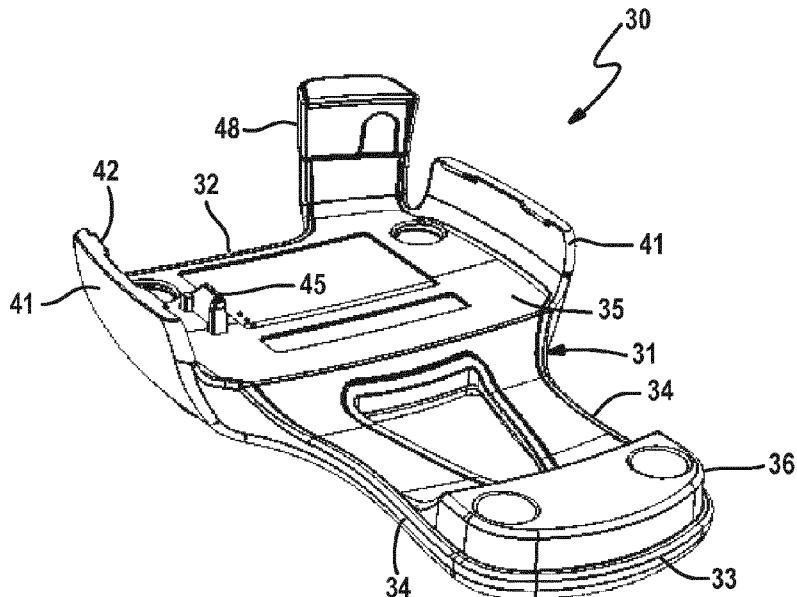

(57) Abstract: A communication interface apparatus is provided for use with a handheld medical test device. The communication interface apparatus is comprised of an attachment member configured to detachably couple to a housing of the medical test device, where the attachment member substantially overlays a rear side of the medical test device. The communication interface apparatus houses an infrared receiver, a secondary transceiver and a controller. The infrared receiver is arranged such that its input port aligns with an output port of an infrared transmitter in the medical test device when the attachment member is coupled to the medical test device.

**FIG. 3**



TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

— *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*

**Published:**

— *with international search report (Art. 21(3))*

## COMMUNICATION INTERFACE CLIP FOR A HANDHELD MEDICAL DEVICE

### FIELD

5 The present disclosure relates to a communication interface apparatus for a handheld medical device having an infrared communication link.

### BACKGROUND

Oral anticoagulation therapy is necessary if a patient has an artificial heart valve, or if they are affected by atrial fibrillation or thrombotic diseases. For 10 patients receiving oral anticoagulation therapy with warfarin, it is important that the dosage is exactly right. The patient's level of coagulation requires regular monitoring, as patients react differently to warfarin, and several factors may interfere with the drugs such as food and other medications. The International Normalized Ratio (INR) is a standardized method of measuring the rate at which 15 blood coagulates. It is very important that patients stay within their target INR range. If a patient's INR is too low, the risk of blood clots increases. If a patient's INR is too high, the risk of internal bleeding increases.

Properly trained patients and/or caregivers are capable of performing reliable INR testing using the patient self-testing model. Handheld blood clot testing 20 meters have enabled patients to implement self-testing. For these patients, self-testing is cost effective and leads to outcomes at least as good as standard INR testing in a specialized clinic. Handheld blood clot testing meters are a sub-category of handheld medical test devices. Other handheld medical test devices are known, like handheld blood glucose meters, lipid testing meters or cardiac 25 marker testing meters.

Despite the success of self-testing, it remains inconvenient for healthcare providers to retrieve test results from the meters used by patients to self-test. An innovative solution is required to address the growing demand from patients for wireless connectivity. Thus, there is a need for means to seamlessly transfer INR 30 or other test results from a handheld medical device wirelessly locally to a

communication hub and/or remotely to a server associated with a healthcare provider.

This section provides background information related to the present disclosure which is not necessarily prior art.

## 5

## SUMMARY

This section provides a general summary of the disclosure, and is not a comprehensive disclosure of its full scope or all of its features.

A communication interface apparatus is provided for use with a handheld medical test device. The communication interface apparatus includes an 10 attachment member that is configured to detachably couple to a housing of the medical test device, where the attachment member substantially overlays a rear side of the medical test device. In an embodiment, the attachment member overlays at least 50%, preferably at least 66%, more preferably at least 75%, more preferably at least 80%, more preferably at least 90%, of the area of the rear side 15 of the medical test device. The communication interface apparatus further includes: an infrared receiver/transceiver, a secondary transceiver, a controller and a power source. The infrared receiver resides in an enclosure of the attachment member and is configured to receive data wirelessly in accordance with a first communication protocol from the infrared transmitter of the medical test 20 device, such that an input port of the infrared receiver aligns with an output port of the infrared transmitter in the medical test device when the attachment member is coupled to the medical test device. The secondary transceiver resides in the enclosure of the attachment member and is configured to transmit data wirelessly in accordance with a wireless second communication protocol, where the first 25 communication protocol differs from the wireless second communication protocol. The controller also resides in an enclosure of the attachment member and operates in a low power mode. The controller periodically transitions from the low power mode to a normal mode and interacts with the infrared receiver in the normal mode to receive data from the medical test device, where the 30 communication interface apparatus consumes more electric power in the normal mode than the low power mode.

In one aspect, the attachment member is further defined by a top edge, a bottom edge and two opposing side edges extending along a planar body between the top edge and the bottom edge. Two clip portions extend outwardly from an opposing side edge of the attachment member and are configured to clip to an outer side surface of the medical test device. More specifically, the housing of the medical test device is formed by an upper shell and a lower shell coupled together and forms a groove where an edge of the upper shell abuts against an edge of the lower shell. Each clip portion of the attachment member includes a tongue that is received in the groove to create a tongue-and-groove joint when the attachment member is coupled to the medical test device.

In another aspect, the attachment member may further include an overhang portion extending outwardly from a top edge of the attachment member and overlays a portion of a top side of the medical test device when the attachment member is coupled to the medical test device, such that the overhang portion encases the infrared receiver and the input port of the infrared receiver faces the top side of the medical test device. A visual indicator may reside in the overhang portion and be electrically connected to the controller, wherein the visual indicator is illuminated while data is transmitted between the meter and the communication interface apparatus.

In yet another aspect, the planar body of the attachment member defines a longitudinal axis extending between the top edge and the bottom edge of the planar body, and the planar body is shaped such that the longitudinal axis is parallel with a horizontal surface upon which the attachment member rests and while the attachment member is coupled to the medical test device.

Additionally, the communication interface further includes a power switch electrically interconnected between the power source and the controller, wherein the power switch is accessible outside of the enclosure to selectively power on and off the communication interface apparatus.

In some embodiments, the communication interface apparatus is configured to communicate data wirelessly via the secondary transceiver to a communication hub, where the communication hub can be configured to plug into a AC power source. In other embodiments, the communication hub is further defined as a

mobile phone. In some cases, the communication interface apparatus may be packaged together with a communication hub as a kit.

In operation, the communication interface apparatus operates in a low power mode and periodically transitions from the low power mode to a normal mode that

5 consumes more electric power than the low power mode. Upon transitioning to the normal mode, the controller interacts with the infrared receiver/transceiver to query the handheld medical device, e.g., a blood clot testing meter. Upon failing to receive a response to the query from the handheld medical device, the communication interface apparatus transitions back to the low power mode. Upon

10 receiving a response to the query from the handheld medical device, the controller interacts with the infrared receiver/transceiver to transmit a request for test results to the handheld medical device. In response to receiving a test result from the handheld medical device, the controller interacts with the secondary transceiver to transmit the test result to the communication hub.

15 Further areas of applicability will become apparent from the description provided herein. The description and specific examples in this summary are intended for purposes of illustration only and are not intended to limit the scope of the present disclosure.

## DRAWINGS

20 The drawings described herein are for illustrative purposes only of selected embodiments and not all possible implementations, and are not intended to limit the scope of the present disclosure.

FIG. 1 is a diagram of a patient administering a self-test;

FIG. 2A is a perspective view of an example medical test device;

25 FIG. 2B is a block diagram depicting the electronic components of the medical test device;

FIG. 3 is a perspective view of a communication interface apparatus for use with the medical test device;

FIG. 4 is a front view of the communication interface apparatus;

FIG. 5 is a rear view of the communication interface apparatus;

FIG. 6 is a block diagram of the electronic components of the communication interface apparatus;

FIG. 7 is a perspective view of the communication interface apparatus  
5 coupled to the medical test device;

FIG. 8 is a front view of the communication interface apparatus coupled to  
the medical test device;

FIG. 9 is a rear view of the communication interface apparatus coupled to the  
medical test device;

10 FIG. 10 is a side view of the communication interface apparatus coupled to  
the medical test device;

FIG. 11 is a top view of the communication interface apparatus coupled to  
the medical test device;

15 FIG. 12 is a cross-sectional view of the communication interface apparatus  
coupled to the medical test device;

FIG. 13 is a fragmentary cross-sectional view of the overhang portion of the  
communication interface apparatus;

FIG. 14 is a diagram depicting a communication interface apparatus in data  
communication with an example communication hub;

20 FIGS. 15A-15C are sequence diagram depicting an example communication  
protocol employed by the communication interface apparatus; and

FIG. 16 is a system diagram for an example independent diagnostic testing  
facility patient services organization.

25 Corresponding reference numerals indicate corresponding parts throughout  
the several views of the drawings. Skilled artisans appreciate that elements in the  
figures are illustrated for simplicity and clarity and have not necessarily been  
drawn to scale. For example, the dimensions of some of the elements in the

figures may be exaggerated relative to other elements to help improve understanding of the embodiments of the present disclosure.

## DETAILED DESCRIPTION

5 Example embodiments will now be described more fully with reference to the accompanying drawings.

FIG. 1 illustrates a patient 2 administering a self-test using a handheld medical device 4. The patient is shown obtaining a blood sample for depositing on a test strip. The test strip is inserted in a strip port of the medical device 4 and a 10 measurement result is determined by the medical device 4. In one embodiment of the instant disclosure, the test strip is inserted in the strip port of the medical device 4 prior to applying the blood sample to the test strip. The medical device 4 can have an integrated heating element to warm the test strip to a pre-determined temperature. When this warm-up process is complete, the medical device 4 can 15 provide an indicator to the operator that he/she can now apply a blood sample to the test strip. The indicator can be, for example, audible, such as a beep, or visual, such as a displayed icon on a screen, or light, or both. In yet another embodiment, the blood sample could be applied to the test strip before or simultaneously with insertion of the test strip into the strip port of the medical device 4.

20 It is desirable that the measurement results obtained by the medical device 4 be transferred seamlessly and typically without further patient intervention to another local computing device, such as a mobile phone 6, tablet or other capable mobile computing device, a laptop computer 7, or a communication hub 8. A communication interface apparatus to facilitate such wireless connectivity is further 25 described below.

FIG. 2A and FIG. 2B further depict an example handheld medical test device 10. In an example embodiment, the medical test device 10 is further defined as a blood clot testing meter which may be used by patients to measure their international normalized ratio (INR) or similar metrics indicative of the clotting 30 tendency or rate at which blood clots. The CoaguChek® XS blood clot testing monitor is an example meter commercially available from Roche Diagnostics. The

CoaguChek® XS system (CoaguChek® XS meter and CoaguChek® XS PT Test strips) quantitatively determines prothrombin time ("PT"), using capillary blood or whole blood from a vein (nonanticoagulated venous whole blood). The system is suited to monitor coagulation values in people who are taking oral anticoagulation 5 medication such as warfarin (vitamin K antagonists, VKAs). The CoaguChek® XS PT Test contains a lyophilized reagent. The reactive components of this reagent consist of thromboplastin and a peptide substrate. When a sample is applied, thromboplastin activates coagulation, which leads to the formation of thrombin. At the same time the meter starts to measure the time. The enzyme thrombin cleaves 10 the peptide substrate, generating an electrochemical signal. Depending on the time elapsed when it first appears, this signal is then converted by means of an algorithm into customary coagulation units (INR, %Quick, seconds) and the result is displayed. While reference is made throughout this application to a blood clot testing meter, the broader aspects of this disclosure pertain to other types of 15 handheld medical devices, such as meters for monitoring blood glucose, lipids, cardiac markers or the like, individually and/or in combination.

With reference to FIG. 2B, the medical test device 10 is comprised generally of a measurement module 22, a processing module 23 and a communication module (COM MOD) 24. During operation, the measurement module 22 20 cooperatively interacts with a test strip inserted into a strip port 12 to determine and display coagulation values, i.e., prothrombin time of a nonanticoagulated venous whole blood sample applied to a test strip. The medical test device 10 can display test results in units equivalent to laboratory plasma measurements, i.e., INR, combination of INR / seconds; or combination of INR / %Quick. The 25 measurement module 22 may include calibration information for the test strips being read by the medical test device 10. Each box of test strips has its own code chip for insertion into the medical test device 10. The code chip contains lot-specific information about its test strips, such as the expiration date and calibration data. Optional liquid controls for the system are also available.

30 As used herein, the term module may refer to, be part of, or include an application Specific Integrated Circuit (ASIC); an electronic circuit; a combinational logic circuit; a field programmable gate array (FPGA); a computer processor that

executes computer readable instructions; other suitable components that provide the described functionality; or a combination of some or all of the above.

The processing module 23 is configured to receive test results that can be customary coagulation units (e.g., INR, INR/seconds; or INR/%Quick) from the 5 measurement module 22 and automatically store the measurement data for subsequent processing. In the example embodiment, each test result (patient test or control) is tagged with identifying information. Identifying information may include but is not limited to a date/time stamp for when the measure was taken, patient ID (and operator ID activated), a serial number for the meter and other 10 information pertaining to the test strip, i.e., lot code, test type like prothrombin time (PT). Of note, each test result measure is also tagged with a unique sequence number assigned by the meter or medical test device 10. In one embodiment, a counter is incremented each time a measurement is taken and the value of the counter is assigned to the test result. The sequence number may be used to 15 retrieve data from the meter as is further described below. Once tagged, the test result is automatically stored in a memory of the medical test device 10. Additionally, the test result can be displayed by the processing module 23 on a display 25. The user interacts with the medical test device 10 using various interface components / interface elements 26 (e.g., buttons, switches, a speaker, a 20 microphone, USB port, etc.) which are also interfaced with the processing module 23. In an exemplary embodiment, the processing module 23 is implemented by a microprocessor and one or more volatile and/or non-volatile memories.

The processing module 23 is also interfaced with the communication module (COM MOD) 24. In an exemplary embodiment, the communication module 24 25 includes an infrared transceiver 27. The infrared transceiver 27 operates to communicate the test result(s) and other data wirelessly via a serial data link to other devices physically separated from the medical test device 10. It is understood that the communication module 24 may further include its own microcontroller, voltage control circuits, etc. Although a few primary components of 30 the medical test device 10 are discussed herein, it is readily understood that other components (e.g., power source) may be needed to implement the medical test device 10.

FIGs. 3-5 depict an example communication interface apparatus 30 designed for use with the handheld medical test device 10. The communication interface apparatus 30 is comprised primarily of an attachment member 31 that detachably couples to the housing of the medical test device 10. The attachment member 31 5 has a planar body that defines a top edge 32, a bottom edge 33 and two opposing side edges 34 and provides at least one enclosure 35 for housing various electronic components as will be further described below.

The shape of the attachment member 31 may take different forms while meeting a few basic requirements. The attachment member 31 is designed so as 10 not to overlap or overlay any buttons, switches, displays or other user interface components / input elements of the medical test device 10, including buttons commonly found on top of a meter. The attachment member 31 should also provide sufficient clearance from the strip port 12 (FIG. 2A) of the medical test device 10 to ensure operability. In addition, the attachment member 31 is typically 15 configured to lay flat on a horizontal surface when coupled to the medical test device 10 as best seen in FIG. 10. That is, the planar body of the attachment member 31 defines a longitudinal axis 39 extending between the top edge 32 and the bottom edge 33 of the planar body and the planar body is shaped such that the longitudinal axis 39 is parallel with a horizontal surface upon which the attachment 20 member 31 rests while the attachment member 31 is coupled to the medical test device 10. In the example embodiment, the attachment member 31 includes a raised portion 36 proximate to the bottom edge 33, where the raised portion 36 has a depth substantially the same as the depth of the enclosure 35 and thereby forms a substantially planar rear surface 37 for level placement on horizontal 25 surfaces such as tables, desks and the like.

In the example embodiment, the attachment member 31 is configured to clip to outer side surfaces of the medical test device 10. More specifically, the attachment member 31 includes two clip portions 41. Clip portions 41 extend outwardly from opposing side edges 34 of the attachment member 31. Each clip 30 portion 41 further includes a tongue 42 that is received in a side surface of the medical test device 10. In this example, the housing of the medical test device 10 is formed by an upper shell and a lower shell coupled together. A groove 43 is formed in the housing where an edge of the upper shell abuts against an edge of

the lower shell and the tongues 42 are sized to fit into the groove 43 as seen in FIG. 12. When clipped together, the tongue 42 and the groove 43 form a tongue-and-groove joint which couples the attachment member 31 along both side surfaces of the medical test device 10. While a particular clip mechanism has been 5 set forth, it is envisioned that other types of fastening mechanisms, such as screws, a hook and loop fastener, magnets, etc., also fall within the scope of this disclosure.

One or more protrusions 45 help to further secure the attachment member 31 to the medical test device 10. The protrusions 45 extend outwardly from a front 10 surface 38 of the attachment member 31. Each protrusion 45 is in turn received into a recess 46 formed in a rear surface of the medical test device 10 as best seen in FIG. 12. In the example embodiment, the recess 46 is part of a latch that opens and closes a panel enclosing a battery compartment. In this way, the design of a pre-existing medical test device does not need to be modified to 15 accommodate the communication interface apparatus 30.

The communication interface apparatus 30 is intended to enhance the wireless connectivity of the medical test device 10 by interfacing the medical test device 10 to another type of wireless data link. To enable such an interface, the communication interface apparatus 30 includes an infrared receiver (or 20 transceiver) whose input port must align with an output port of an infrared transmitter (or transceiver) residing in the medical test device 10 while the attachment member 31 is coupled to the medical test device 10. In the example embodiment, the output port of the infrared transmitter is embedded in the top side of the medical test device 10. Consequently, the attachment member 31 includes 25 an overhang portion 48 which extends outwardly from a top edge of the attachment member 31. The overhang portion 48 encases the infrared receiver and overlays a portion of the top side of the medical test device 10. In this way, the input port of the infrared receiver aligns with the output port of the infrared transmitter found in the medical test device 10. It is readily understood that the 30 infrared transmitter may have different placements in other devices and thus the shape of the attachment member 31 can be altered to accommodate alignment between the infrared components.

FIG. 6 illustrates the electronic components associated with the communication interface apparatus 30. An infrared receiver 61 is disposed in the overhang portion 48 of the attachment member 31 as described above. The infrared receiver (or transceiver) is configured to interface with an infrared transmitter residing in the medical test device. That is, the infrared receiver 61 receives and processes data sent wirelessly in accordance with a first communication protocol, where a suitable communication protocol ensures the integrity and privacy of the transported data over a serial infrared communication link.

To provide visual feedback regarding the progress of any data communication, the overhang portion 48 may also house one or more visual indicators 64 as seen in FIG. 13. In an example embodiment, the visual indicator 64 is implemented by a light emitting diode mounted on a circuit board. At least a portion 131 of the overhang portion 48 is comprised of a transparent material which emits the light from the visual indicator 64. In other embodiments, the visual indicator 64 may be disposed elsewhere on the attachment member 31.

A controller or control module 62 is housed in the primary enclosure 35 provided by the attachment member 31. The controller 62 receives data from the infrared receiver 61 and interacts with a secondary wireless transceiver 63 to transmit the data wirelessly to a local computing device. Conversely, the controller 62 may also receive data from the secondary wireless transceiver 63 and interact with the infrared receiver 61 to transmit the data wirelessly to the medical test device 10. In such an embodiment, the infrared receiver 61 is also able to work as an infrared transceiver to transmit data via infrared connection to the medical test device 10. In one embodiment, the control module 62 is implemented by a single processor. In other embodiments, the control module 62 is comprised of two processors; one processor implements application functions (e.g., converting data between different communication protocols) and a second processor is dedicated to implementing the communication protocol used by the secondary wireless transceiver 63.

In the example embodiment, the secondary transceiver 63 transmits and receives data in accordance with the IEEE 802.15 standard (i.e., the Bluetooth or

Bluetooth Low Energy wireless technology standard). In other embodiments, it is envisioned that the secondary transceiver 63 may transmit and receive data in accordance with other communication protocols operating in the RF spectrum (e.g., IEEE 802.11 standard) or operate in other frequency spectrums, such as 5 cellular or satellite technology. In any case, the secondary transceiver 63 communicates data via a wireless data link to a computing device spatially separated from the communication interface apparatus 30.

A power source 66, such as a battery, is also housed in the primary enclosure 35 provided by the attachment member 31. In one embodiment, the 10 power source 66 provides power to the control module 62 which in turn powers the other electronic components. An on/off (power) switch 65 is electrically interconnected between the control module 62 and the power source 66. The on/off or power switch 65 enables a user to power on and off the communication interface apparatus 30 in order to conserve battery power. In the example 15 embodiment, the on/off or power switch 65 may be implemented by a slide type switch accessible on the rear of the communication interface apparatus 30. While the primary electronic components have been discussed in relation to FIG. 6, it is understood that other electronic components may be employed by the communication interface apparatus 30.

20 FIGs. 7-11 further illustrate the communication interface apparatus 30 when it is coupled to the medical test device 10. Of note, the planar body of the attachment member 31 substantially overlays a rear side of the medical test device 10 but does not otherwise overlap or obstruct other portions of the medical test device 10 including its display, buttons or strip port.

25 FIG. 14 depicts the communication interface apparatus 30 in data communication with an example communication hub 140 while being coupled to the medical test device 10. The communication hub 140 is configured to transmit and receive requests to and from the communication interface apparatus 30 over a wireless data link. Data may be transmitted in accordance with the IEEE 802.15 30 standard although other wireless technology is also contemplated as noted above. The communication hub 140 can in turn process and/or store test results received from the communication interface apparatus 30. More importantly, the

communication hub 140 is typically designed to relay the test results to a remote server (not shown). In an example embodiment, the communication hub 140 is a 2net™ Hub commercially available from Qualcomm Life. In this case, it is envisioned that the communication interface apparatus 30 and the communication hub 140 may be sold together as a kit 142 with or without the medical device. In another example embodiment, the communication hub 140 may be an app on a mobile phone, tablet or other capable mobile computing device, and/or laptop computer. Other implementations for the communication hub 140 are also contemplated by this disclosure.

An example communication protocol between these devices is further described in relation to FIGs. 15A-C. To begin, a user slides the on/off switch of the communication interface apparatus 30 from an 'off' to 'on' position, thereby powering it on. Initially, the communication interface apparatus 30 may enter a low power mode (i.e., sleep mode) to conserve power as indicated at 151. In a low power mode, the controller may be active but other components, such as transceivers, are powered down. At periodic time intervals (e.g., every 1 minute), the communication interface apparatus 30 transitions from the low power mode to a normal mode and begins interacting with the medical device or meter 10. More specifically, the communication interface apparatus 30 wakes-up at 152 and pings the meter 10 at 153 (i.e., sends a wake-up request). In some instances, the meter 10 is powered down and thus does not respond the wake-up request. After failing to receive a response (e.g., within 5 seconds), the communication interface apparatus 30 returns to sleep mode as indicated at 154. This process is repeated until an acknowledgement is received from the meter 10 or the communication interface apparatus 30 is powered down.

When the meter 10 is powered on, it will send an acknowledgement message at 155 in response to the wake-up request received from the communication interface apparatus 30. The communication interface apparatus 30 can then initiate interaction with the meter 10 to obtain available test results. More specifically, the communication interface apparatus 30 sends a request to send last test result at 156. In response to the last result request, the meter 10 sends the last test result at 157 to the communication interface apparatus 30. Each test result is tagged with a unique sequence number (e.g., measurement #512 in Figs

15A-C) which is included in the data sent to the communication interface apparatus 30. During the transmission from the meter 10 to the communication interface apparatus 30, the visual indicator 64 on the communication interface apparatus 30 will be illuminated in a particular manner (e.g., flashing green)

5 indicating data is being transmitted between the meter 10 and the communication interface apparatus 30. In some instances, the data transfer may be interrupted, for example if the patient initiates a new measurement using the meter 10. In this case, the last test result is not sent by the meter 10 and the communication interface apparatus 30 returns to sleep mode after failing to receive a test result.

10 In the example embodiment, the communication interface apparatus 30 is not designed to store test results received from the meter 10. Rather, immediately upon receipt of test results, the communication interface apparatus 30 relays the test result to the communication hub 140 without any involvement by the user. The communication interface apparatus 30 first confirms availability of the

15 communication hub 140 (or otherwise pairs therewith) at 161. During the pairing process, the communication interface apparatus 30 and the communication hub 140 may exchange an authentication token (e.g., a secret PIN). In the event that a data link cannot be established or the communication hub 140 is otherwise unavailable, the communication interface apparatus 30 would return to sleep

20 mode.

At 162, the communication interface apparatus 30 transmits the last test result, including its unique sequence number, to the communication hub 140. During the transmission from the communication interface apparatus 30 to the communication hub 140, the visual indicator 64 on the communication interface apparatus 30 continues to be illuminated in the same manner as noted above (e.g., flashing green).

Test results can be stored at the communication hub 140. Upon receipt of the last test result, the sequence number for the incoming test result (i.e., #512) is compared at 163 to the sequence number for the test result last received and 30 stored (i.e., #509) by the communication hub 140. When the sequence numbers match, the test results stored at the communication hub 140 are in synch with the test results stored on the meter 10. The communication hub 140 sends a reply at

169 to the communication interface apparatus 30 indicating that data transfer is complete. In response to such reply, the communication interface apparatus 30 returns to a sleep mode as indicated at 170. Prior to entering a sleep mode, the visual indicator 64 may be illuminated in a different manner to indicate that all data 5 has been successfully transmitted to the communication hub 140. For example, the visual indicator 64 may be illuminated steady or flashing blue to indicate a successful transmission. Other means for varying the illumination pattern (e.g., solid vs. flashing) are also contemplated by this disclosure. Additionally, the illumination pattern for the visual indicator 64 may be further varied in order to 10 indicate other functions such as successful pairing between devices, startup procedure in progress or weak battery.

On the other hand, when the sequence numbers do not match, the test results stored at the communication hub 140 are not in synch with the test results stored on the meter 10. In this case, the communication hub 140 sends a request 15 for additional test results to the communication interface apparatus 30 at 165. In the example embodiment, the request for additional test result includes a sequence number for the test result being requested, where the value of the sequence number is the sequence number of the test result last received by the communication hub 140 incremented by one (e.g., #510 in FIG. 12). The request 20 for additional test result is forwarded on at 166 to the meter 10.

In response to the request for additional test results, the meter 10 retrieves the applicable test result using the specified sequence number (i.e., #510) and sends the test result via the communication interface apparatus 30 to the communication hub 140 as indicated at 167. Upon receipt of the additional test 25 result at the communication hub 140, the sequence number for the incoming test result (i.e., #510) is again compared at 168 to the sequence number for the test result last received (i.e., #512) and stored by the communication hub 140. The process described above is repeated as shown until the sequence number for the incoming test result matches the sequence number for the test result last received 30 and stored by the communication hub 140. In this way, the test results are transmitted in a defined order so that even if data transmission is interrupted, transmission can be completed at a later time without missing a test result.

When the sequence numbers match, the test results stored at the communication hub 140 are in sync with the test results stored on the meter 10 and the communication hub 140 sends a reply to the communication interface apparatus 30 indicating that data transfer is complete. Again, the visual indicator 5 64 may be illuminated in a manner to indicate that all data has been successfully transmitted to the communication hub 140. The successful data transmission may also trigger the transfer of the data by the communication hub 140 to a remote server, for example associated with a healthcare provider. It is to be understood that only the relevant steps are discussed in relation to FIG. 15 but that other 10 software-implemented instructions may be needed to transmit data between the devices.

In some embodiments, the medical test device 10 and/or the communication hub 140 can be configured to communicate test results to an Independent Diagnostic Testing Facility (IDTF) Patient Services Organization (PSO), like are 15 shown in FIG. 16. Presently operating IDTF PSOs include, for example, CoaguChek® Patient Services (provided by Roche Health Solutions Inc.), mdINR (a Lincare Company), and Alere Home Monitoring, Inc.. Test results can be communicated by the user to the IDTF PSO, e.g. by phoning in the results or entering the result directly in the IDTF PSO internet portal. Test results can also be 20 communicated semi-automatically or automatically to an IDTF PSO by connecting the medical test device 10 to a computing device using an accessory such as, for example, the CoaguChek® XS Connect (Roche Diagnostics), or a cellular access communication hub, such as the Alere™ MobileLink (Alere) or 2net™ Hub (Qualcomm Life) cellular gateway. For more information, reference may be made 25 to Jones, Jay, "Chapter 20 Integration of Point-of-Care Testing into Regional Healthcare Networks." *Point-of-Care Testing: Needs, Opportunity, and Innovation 3<sup>rd</sup> Edition*. Eds. Christopher Price, Andrew St John and Larry Kricka. AACC Press, 2010. Additionally, the CoaguChek® Link Quick Reference Guide (2013) provides clinicians and patients on warfarin therapy with the convenience of a 30 single, secure and easy-to-use website for managing PT/INR testing. See CoaguChek® Link Healthcare Professional's Manual (2013) and CoaguChek® Link User's Manual (2013) (Roche Diagnostics).

IDTF PSOs can operate in a wide range of sequences and actions, and the following scenarios are presented to describe some of the functions of the IDTF PSO. Operation typically begins with a patient manually entering their test results on an internet web site or phoning their test results in using an automated or 5 operator assisted inbound Interactive Voice Response (IVR) system. Healthcare providers can also enter the patients test results using the internet into the IDTF PSO. Once the patient's test results are entered, the results are visible to the patient, healthcare provider, and the IDTF PSO. The test results are evaluated by the IDTF computer system according to HCP/clinic preferences for a notification 10 range. If the test results are within the notification range, an IDTF PSO clinician will phone the patient's healthcare provider and provide an oral notification that the test results are within the notification range, and a facsimile notification will be sent automatically from the IDTF PSO to the HCP. If the test results are not within the notification range, the IDTF PSO automatically sends a facsimile to the healthcare 15 provider notifying the healthcare provider that the patient has performed a test. An outbound Interactive Voice Response (IVR) system, such as Genesys® Angel, notifies patients that are non-compliant in the frequency of their testing such as with a phone call on Tuesdays and Thursdays to remind the patient to test. The outbound IVR receives confirmation on whether the call was received by human 20 voice or voice mail.

IDTF billing identifies billable events based upon billing rules associated with the patient's insurance policy. Billable events not reimbursed by insurance are termed overages that patient has the direct responsibility to pay. The billing events are transferred to the Total Inventory Management System (TIMS) for claims 25 processing with insurance companies and patients. The total inventory management system also permits patients to order consumables such as test strips and lancets on the IDTF internet portal. Other known functions and services may also be provided by the IDTF PSO.

The techniques described herein may be implemented by one or more 30 computer programs executed by one or more processors. The computer programs include processor-executable instructions that are stored on a non-transitory tangible computer readable medium. The computer programs may also include

stored data. Non-limiting examples of the non-transitory tangible computer readable medium are nonvolatile memory, magnetic storage, and optical storage.

Some portions of the above description present the techniques described herein in terms of algorithms and symbolic representations of operations on 5 information. These algorithmic descriptions and representations are the means used by those skilled in the data processing arts to most effectively convey the substance of their work to others skilled in the art. These operations, while described functionally or logically, are understood to be implemented by computer programs. Furthermore, it has also proven convenient at times to refer to these 10 arrangements of operations as modules or by functional names, without loss of generality. It is understood that grouping of operations within in a given module is not limiting and operations may be shared amongst multiple modules or combined into a single module.

Unless specifically stated otherwise as apparent from the above discussion, it 15 is appreciated that throughout the description, discussions utilizing terms such as "processing" or "computing" or "calculating" or "determining" or "displaying" or the like, refer to the action and processes of a computer system, or similar electronic computing device, that manipulates and transforms data represented as physical (electronic) quantities within the computer system memories or registers or other 20 such information storage, transmission or display devices.

Certain aspects of the described techniques include process steps and instructions described herein in the form of an algorithm. It should be noted that the described process steps and instructions could be embodied in software, firmware or hardware, and when embodied in software, could be downloaded to 25 reside on and be operated from different platforms used by real time network operating systems.

The present disclosure also relates to an apparatus for performing the operations herein. This apparatus may be specially constructed for the required purposes, or it may comprise a general-purpose computer selectively activated or 30 reconfigured by a computer program stored on a computer readable medium that can be accessed by the computer. Such a computer program may be stored in a tangible computer readable storage medium, such as, but is not limited to, any

type of disk including floppy disks, optical disks, CD-ROMs, magnetic-optical disks, read-only memories (ROMs), random access memories (RAMs), EPROMs, EEPROMs, magnetic or optical cards, application specific integrated circuits (ASICs), or any type of media suitable for storing electronic instructions, and each 5 coupled to a computer system bus. Furthermore, the computers referred to in the specification may include a single processor or may be architectures employing multiple processor designs for increased computing capability.

The foregoing description of the embodiments has been provided for purposes of illustration and description. It is not intended to be exhaustive or to 10 limit the disclosure. Individual elements or features of a particular embodiment are generally not limited to that particular embodiment, but, where applicable, are interchangeable and can be used in a selected embodiment, even if not specifically shown or described. The same may also be varied in many ways.

## CLAIMS

What is claimed is:

1. A communication interface apparatus (30) for use with a handheld medical test device (10) having an infrared transmitter, comprising:

5 an attachment member (31) providing an enclosure (35) and configured to detachably couple to a housing of the medical test device (10), where the attachment member (31) substantially overlays a rear side of the medical test device (10);

10 an infrared receiver (61) residing in the enclosure (35) and configured to receive data wirelessly in accordance with a first communication protocol from the infrared transmitter (27) of the medical test device (10), where an input port of the infrared receiver (61) aligns with an output port of the infrared transmitter (27) in the medical test device (10) when the attachment member (31) is coupled to the medical test device (10);

15 a secondary transceiver (63) residing in the enclosure (35) and configured to transmit data wirelessly in accordance with a second communication protocol, where the first communication protocol differs from the second communication protocol;

20 a controller (62) residing in the enclosure (35) and that operates in a low power mode (151), wherein the controller (62) is configured to periodically transition from the low power mode (151) to a normal mode (152), and interacts with the infrared receiver (61) in the normal mode (152) to receive data from the medical test device (10), where the communication interface apparatus (30) consumes more electric power in the normal mode (152) than the low power mode (151); and

25 a power source (66) residing in the enclosure (35) and interfaced with the controller (62).

2. The communication interface apparatus (30) of claim 1 wherein the attachment member (31) defines a top edge (32), a bottom edge (33) and two opposing side edges (34) extending along a planar body between the top edge

(32) and the bottom edge (33), and includes two clip portions (41), where each clip portion (41) extends outwardly from an opposing side edge (34) of the attachment member (31) and is configured to clip to an outer side surface of the medical test device (10).

5

3. The communication interface apparatus (30) of claim 2 wherein the attachment member (31) further includes an overhang portion (48) extending outwardly from a top edge (32) of the attachment member (31) and overlays a portion of a top side of the medical test device (10) when the attachment member 10 (31) is coupled to the medical test device (10), wherein the overhang portion (48) encases the infrared receiver (61) and the input port of the infrared receiver (61) faces the top side of the medical test device (10).

4. The communication interface apparatus (30) of claim 3 further comprising a visual indicator (64) residing in the overhang portion (48) and electrically connected to the controller (62), wherein the visual indicator (64) is illuminated while data is transmitted between the medical test device (10) and the communication interface apparatus (30).

20 5. The communication interface apparatus (30) of any one of claims 2 to 4 wherein the planar body of the attachment member (31) defines a longitudinal axis (39) extending between the top edge (32) and the bottom edge (33) of the planar body, and the planar body is shaped such that the longitudinal axis (39) is parallel with a horizontal surface upon which the attachment member (31) rests 25 and while the attachment member (31) is coupled to the medical test device (10).

6. The communication interface apparatus (30) of any one of claims 1 to 5 further comprising a power switch (65) electrically interconnected between the power source (66) and the controller (62), wherein the power switch (65) is 30 accessible outside of the enclosure (35) to selectively power on and off the communication interface apparatus (30).

7. The communication interface apparatus of any one of claims 1 to 6 wherein the secondary transceiver (63) transmits data in accordance with IEEE 802.15 wireless communication standard.

5 8. The communication interface apparatus of any one of claims 1 to 7 wherein the infrared receiver (61) and the secondary transceiver (63) are powered down in the low power mode (151) and powered up in the normal mode (152).

9. The communication interface apparatus (30) of claim 1, comprising:

10 an attachment member (31) having a planar body that defines a top edge (32), a bottom edge (33), two opposing side edges (34) extending between the top edge (32) and the bottom edge (33) and an enclosure (35) therein, wherein the planar body of the attachment member (31) defines a longitudinal axis (39) extending between the top edge (32) and the bottom edge (33) of the planar body and the planar body is shaped such that the longitudinal axis (39) is parallel with a horizontal surface upon which the attachment member (31) rests while the attachment member (31) is coupled to the medical test device (10);

20 an infrared receiver (61) configured to receive data wirelessly in accordance with a first communication protocol, where the infrared receiver (61) is arranged in line-of-sight with an infrared transmitter (27) in the medical test device (10) when the attachment member (31) is coupled to the medical test device (10);

25 a secondary transceiver (63) configured to transmit data wirelessly in accordance with a second communication protocol that differs from the first communication protocol;

a controller (62) interfaced with the infrared receiver (61) and the secondary transceiver (63) and operable to convert data between the first and second communication protocols;

30 a power source (66) interfaced with the controller (62);

a power switch (65) electrically interconnected between the power source (66) and controller (62), where the power switch (65) is actuatable by

a user to selectively power on and off the communication interface apparatus (30);

two clips (41) that extend outwardly from opposing side edges of the attachment member (31) and configured to clip to an outer side surface of the medical test device (10), such that the attachment member (31) substantially overlays a rear side of the medical test device (10) when the attachment member (31) is coupled to the medical test device (10); and

an overhang portion (48) extending outwardly from a top edge (32) of the attachment member (31) and overlays a portion of a top side of the medical test device (10) when the attachment member (31) is coupled to the medical test device (10), wherein the overhang portion (48) encases the infrared receiver (61) and the input port of the infrared receiver (61) faces the top side of the medical test device (10).

10. A system comprising

a communication interface apparatus (30) according to any one of claims 1 to 9 and

a handheld medical test device (10) having an infrared transmitter.

11. The system of claim 10

wherein the housing of the medical test device (10) is formed by an upper shell (13A) and a lower shell (13B) coupled together and forms a groove (43) where an edge of the upper shell (13A) abuts against an edge of the lower shell (13B), and each clip portion (41) of the attachment member (31) of the communication interface apparatus (30) includes a tongue (42) that is received in the groove (43) to create a tongue-and-groove joint when the attachment member (31) is coupled to the medical test device (10).

12. A kit for interfacing with a medical test device (10), comprising

a communication interface apparatus (30) of any one of claims 1 to 9 or a system of any one of claims 10 or 11 and

a communication hub (140) that plugs into a AC power source and is configured to communicate data wirelessly with the secondary transceiver (63) of the communication interface apparatus (30).

5 13. The kit of claim 12, comprising:

a communication interface apparatus (30) configured to detachably couple to a housing of a medical test device (10) and includes

10 an attachment member (31) having a planar body that defines a top edge (32), a bottom edge (33), two opposing side edges (34) extending between the top edge (32) and the bottom edge (33) and an enclosure (35) therein;

15 two clips (41) that extend outwardly from opposing side edges (34) of the attachment member (31) and configured to clip to an outer side surface of the medical test device (10), such that the attachment member (31) substantially overlays a rear side of the medical test device (10) when the attachment member (31) is coupled to the medical test device (10);

20 an infrared receiver (61) configured to receive data wirelessly in accordance with a first communication protocol, where the infrared receiver (61) is arranged in line-of-sight with an infrared transmitter (27) in the medical test device (10) when the attachment member (31) is coupled to the medical test device (10);

25 a secondary transceiver (63) configured to transmit data wirelessly in accordance with a second communication protocol that differs from the first communication protocol;

a controller (62) interfaced with the infrared receiver (61) and the secondary transceiver (63) and operable to convert data between the first and second communication protocols; and

30 a communication hub (140) that plugs into a AC power source and is configured to communicate data wirelessly with the secondary transceiver (63) of the communication interface apparatus (30).

14. The kit of any one of claims 12 to 13 wherein the communication interface apparatus (30) operates in a low power mode (151) and periodically transitions from the low power mode (151) to a normal mode (152) that consumes


more electric power than the low power mode (151), wherein, upon transitioning to the normal mode (152), the controller (62) interacts with the infrared receiver (61) to query the medical test device (10) and

5 wherein, upon failing to receive a response to the query from the medical test device (10), the communication interface apparatus (30) transitions back to the low power mode (151). and



wherein, upon receiving a response to the query from the medical test device (10), the controller (62) interacts with the infrared receiver (61) to transmit a request for test results to the medical test device (10).



10



15. The kit of claim 14 wherein, in response to receiving a test result from the medical test device (10), the controller (62) interacts with the secondary transceiver (63) to transmit the test result to the communication hub (140).

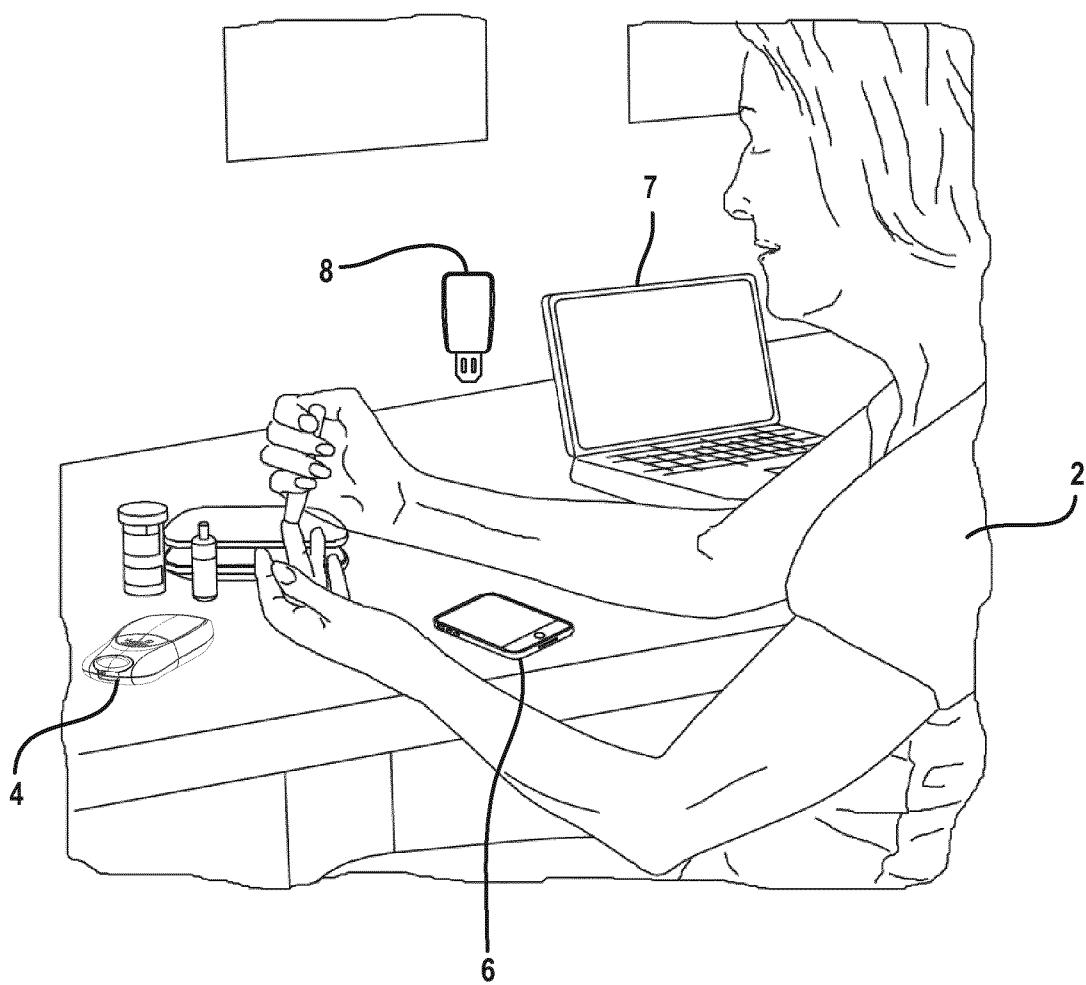


**FIG. 1**

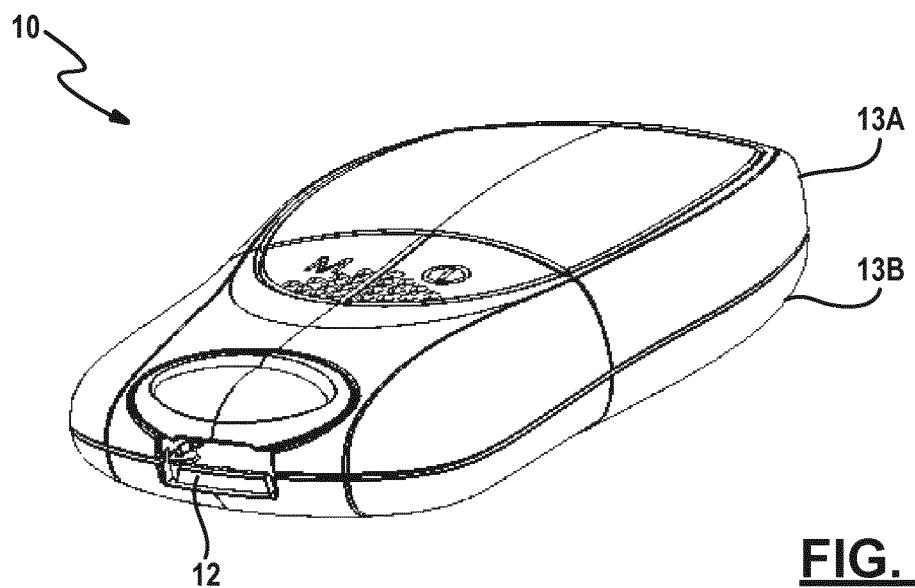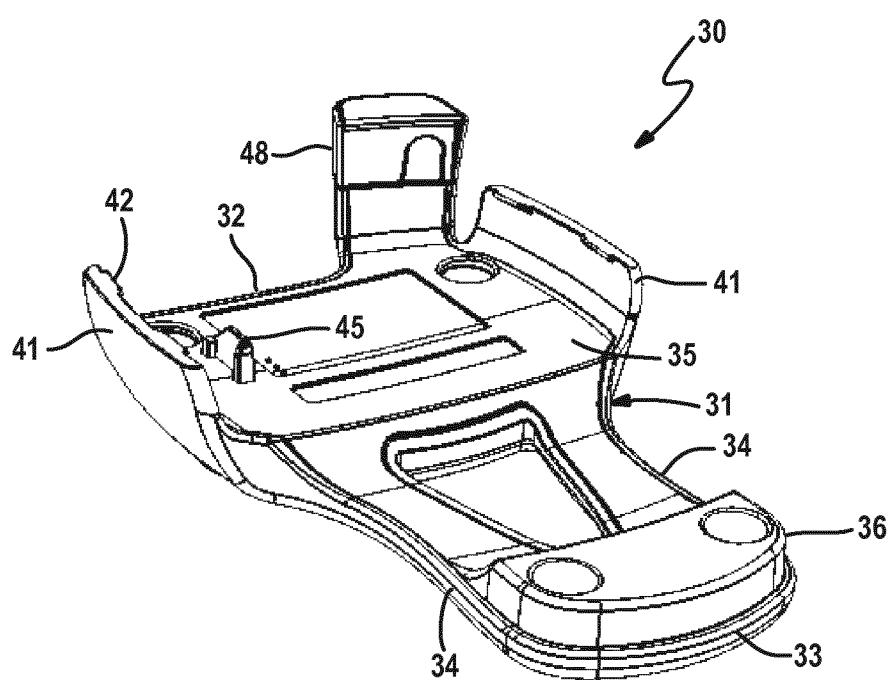
**FIG. 2A****FIG. 3**

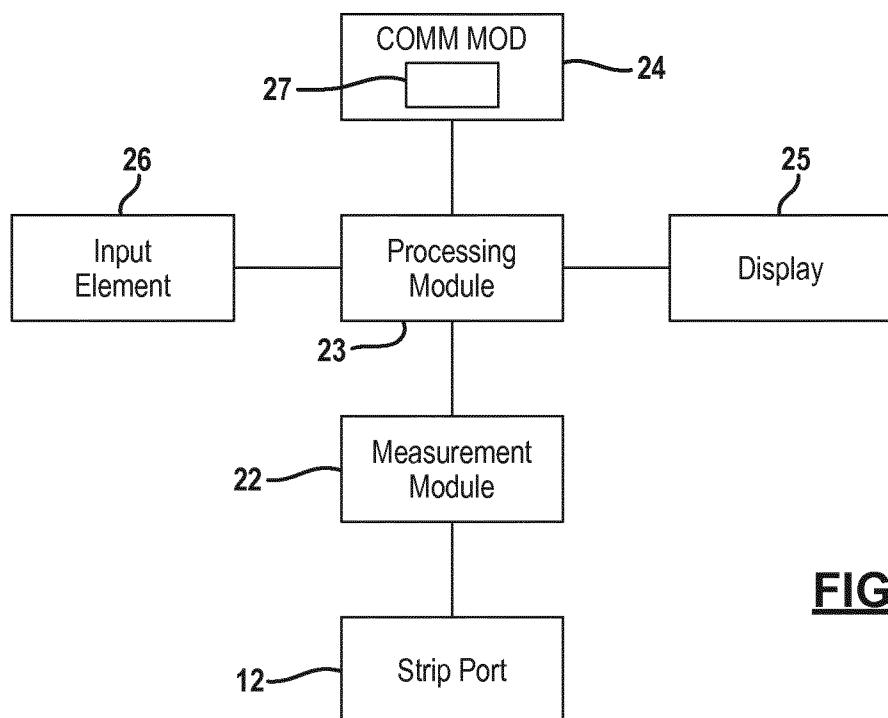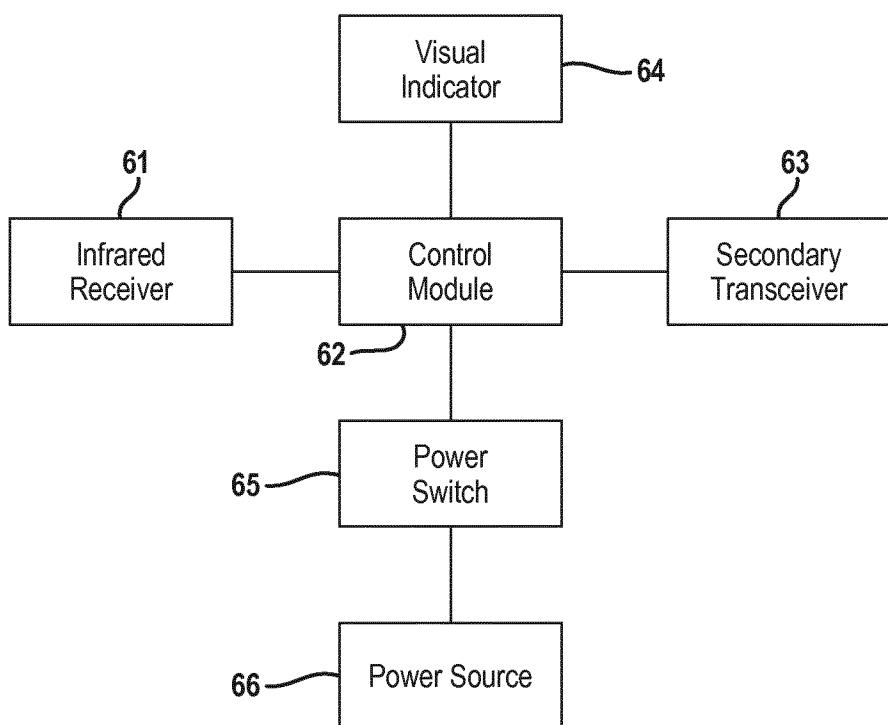**FIG. 2B****FIG. 6**


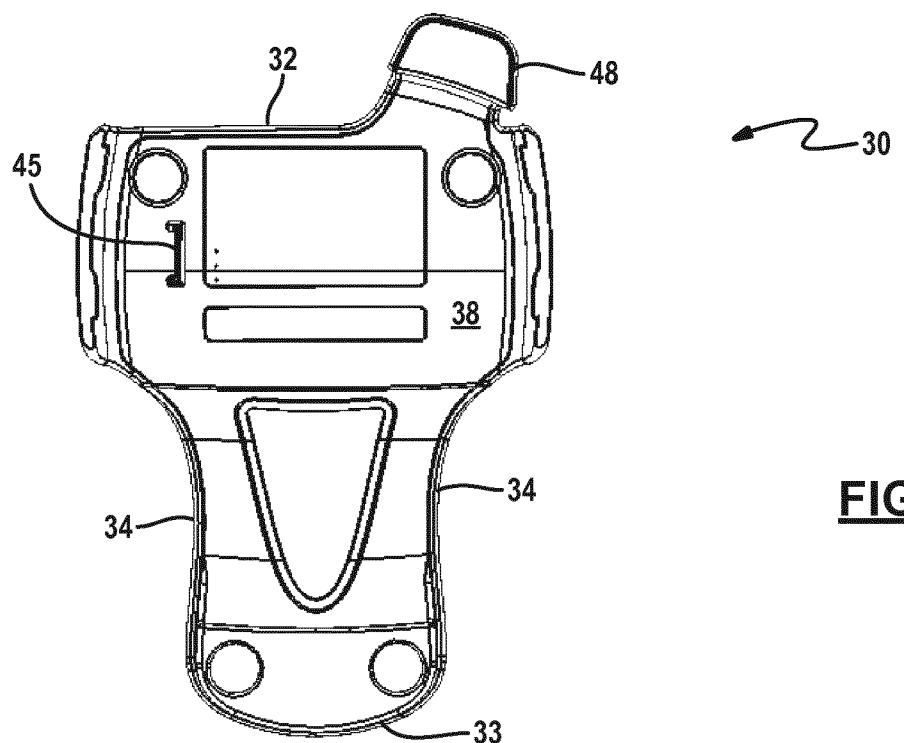
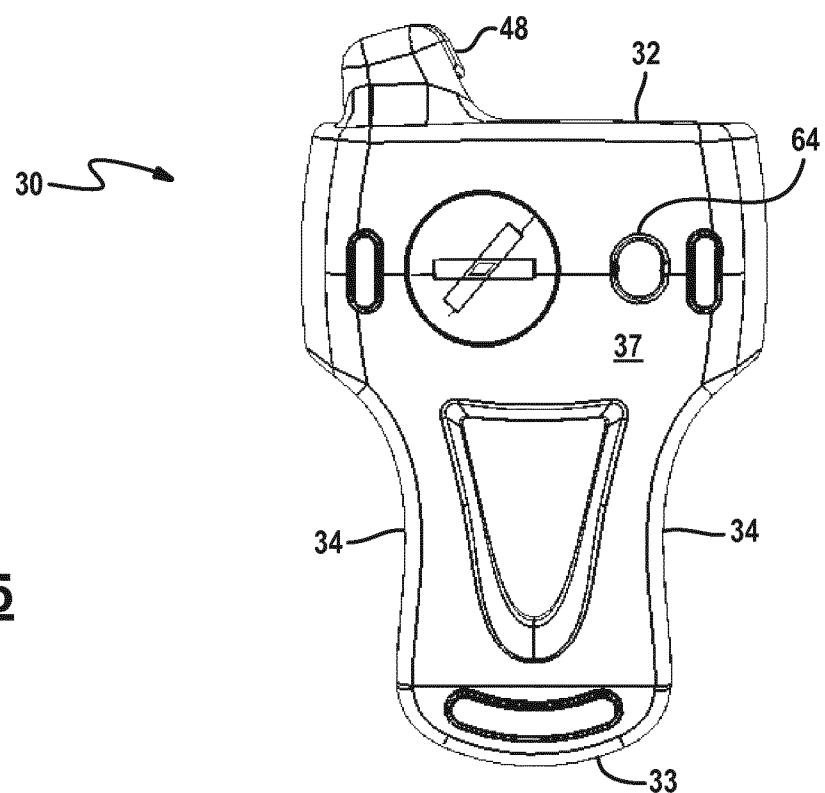
**FIG. 4****FIG. 5**

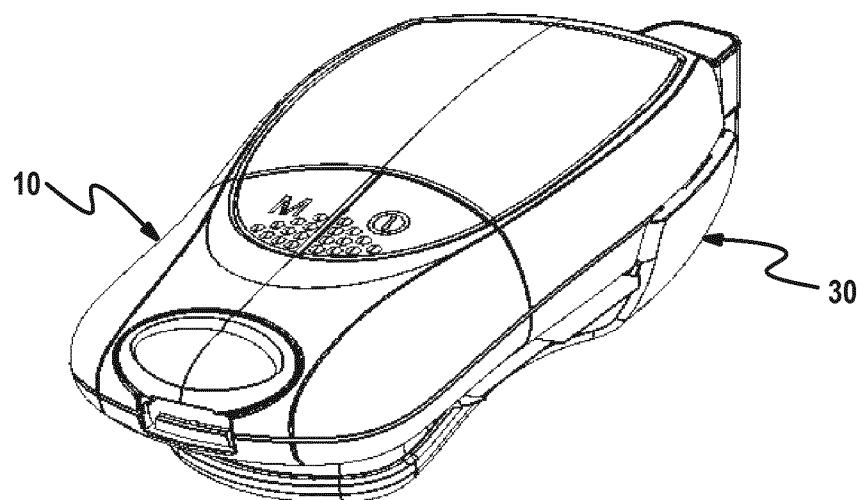


**FIG. 7**

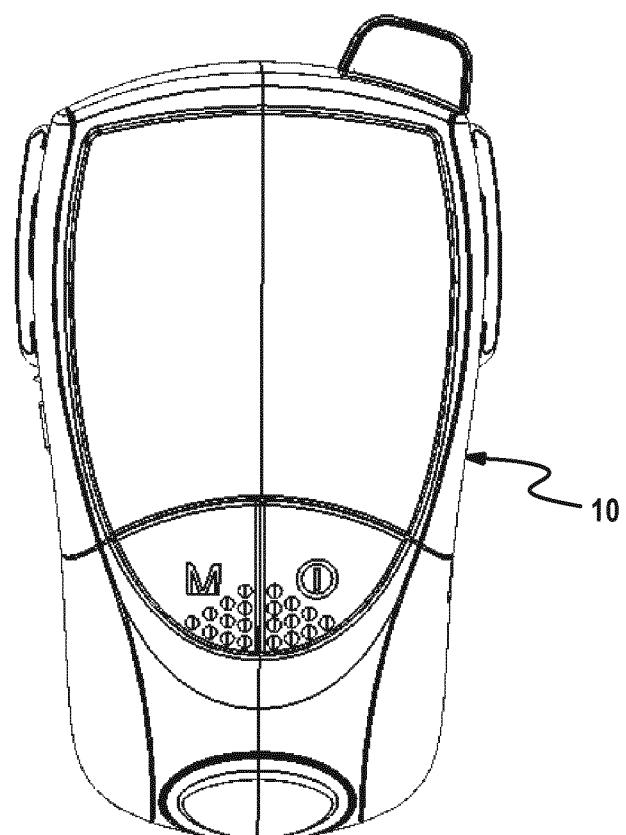


**FIG. 8**

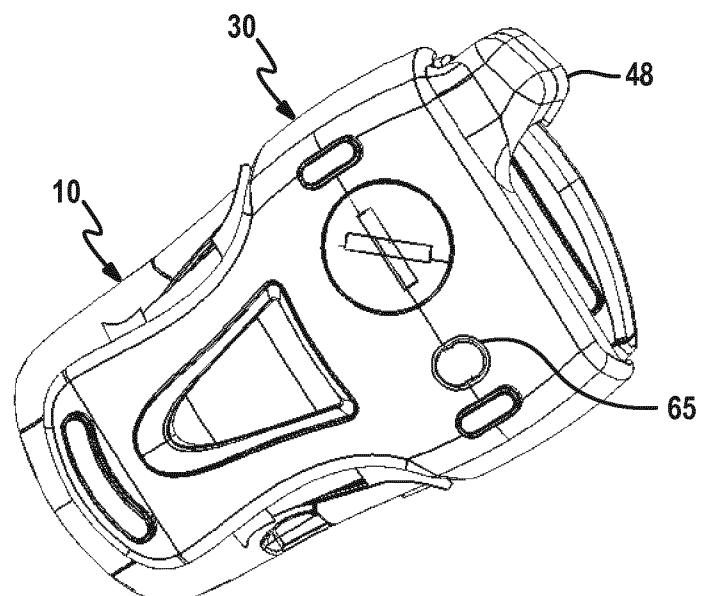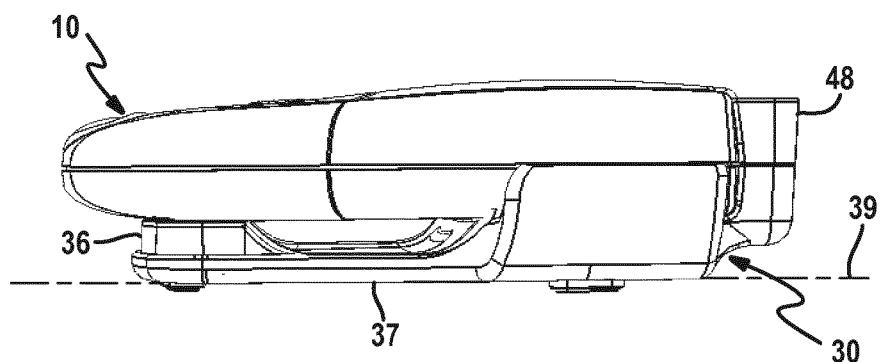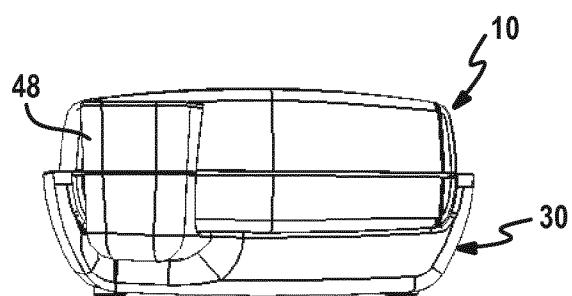
**FIG. 9****FIG. 10****FIG. 11**

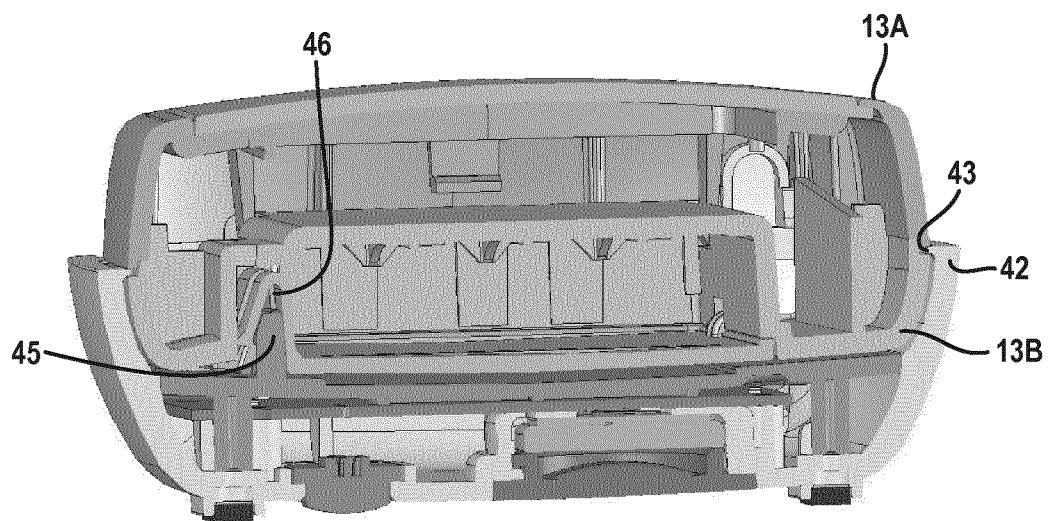


**FIG. 12**

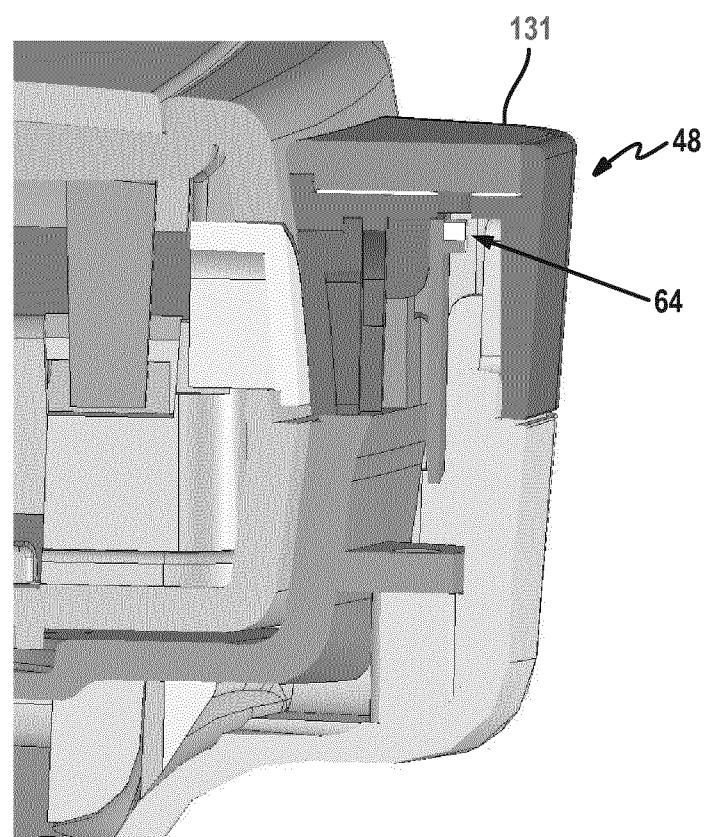



**FIG. 13**

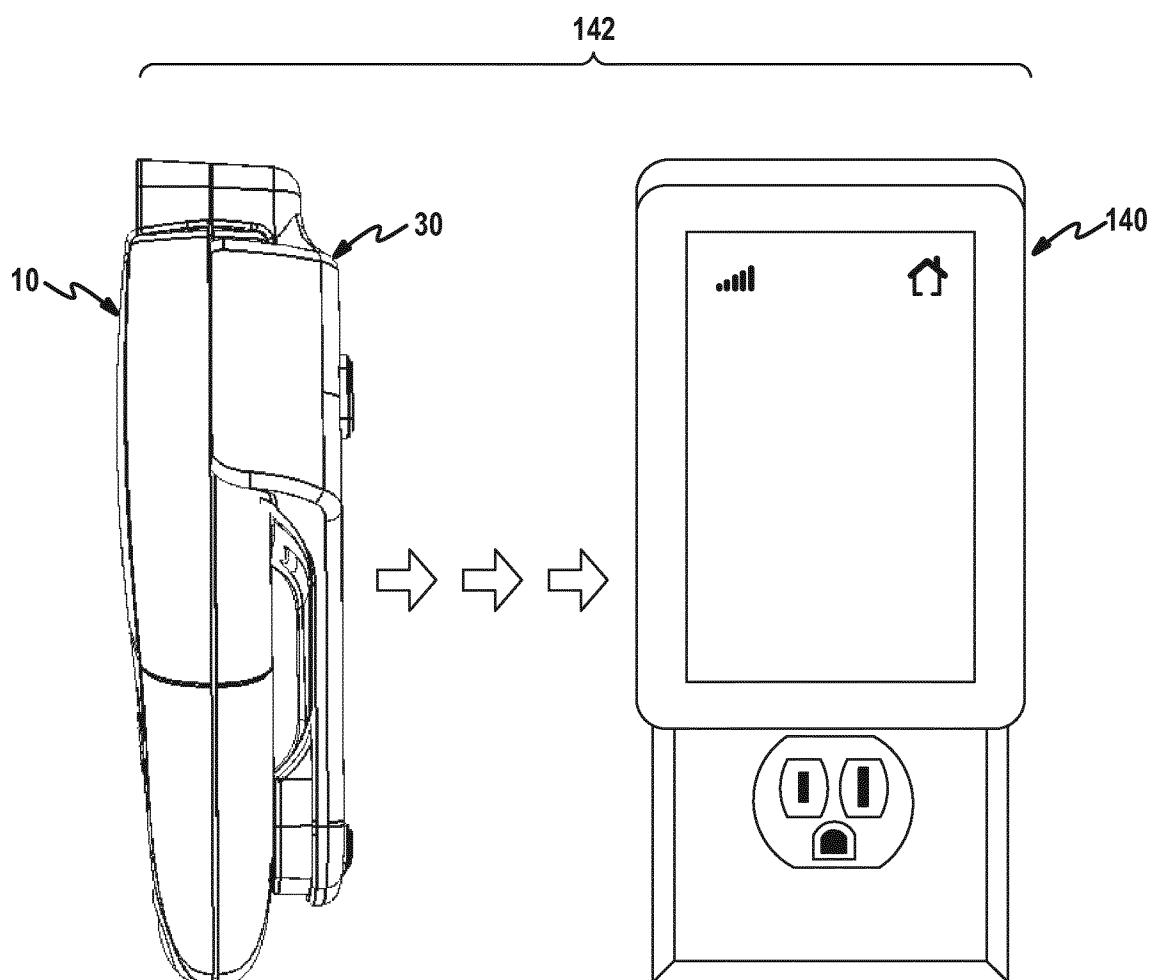

**FIG. 14**

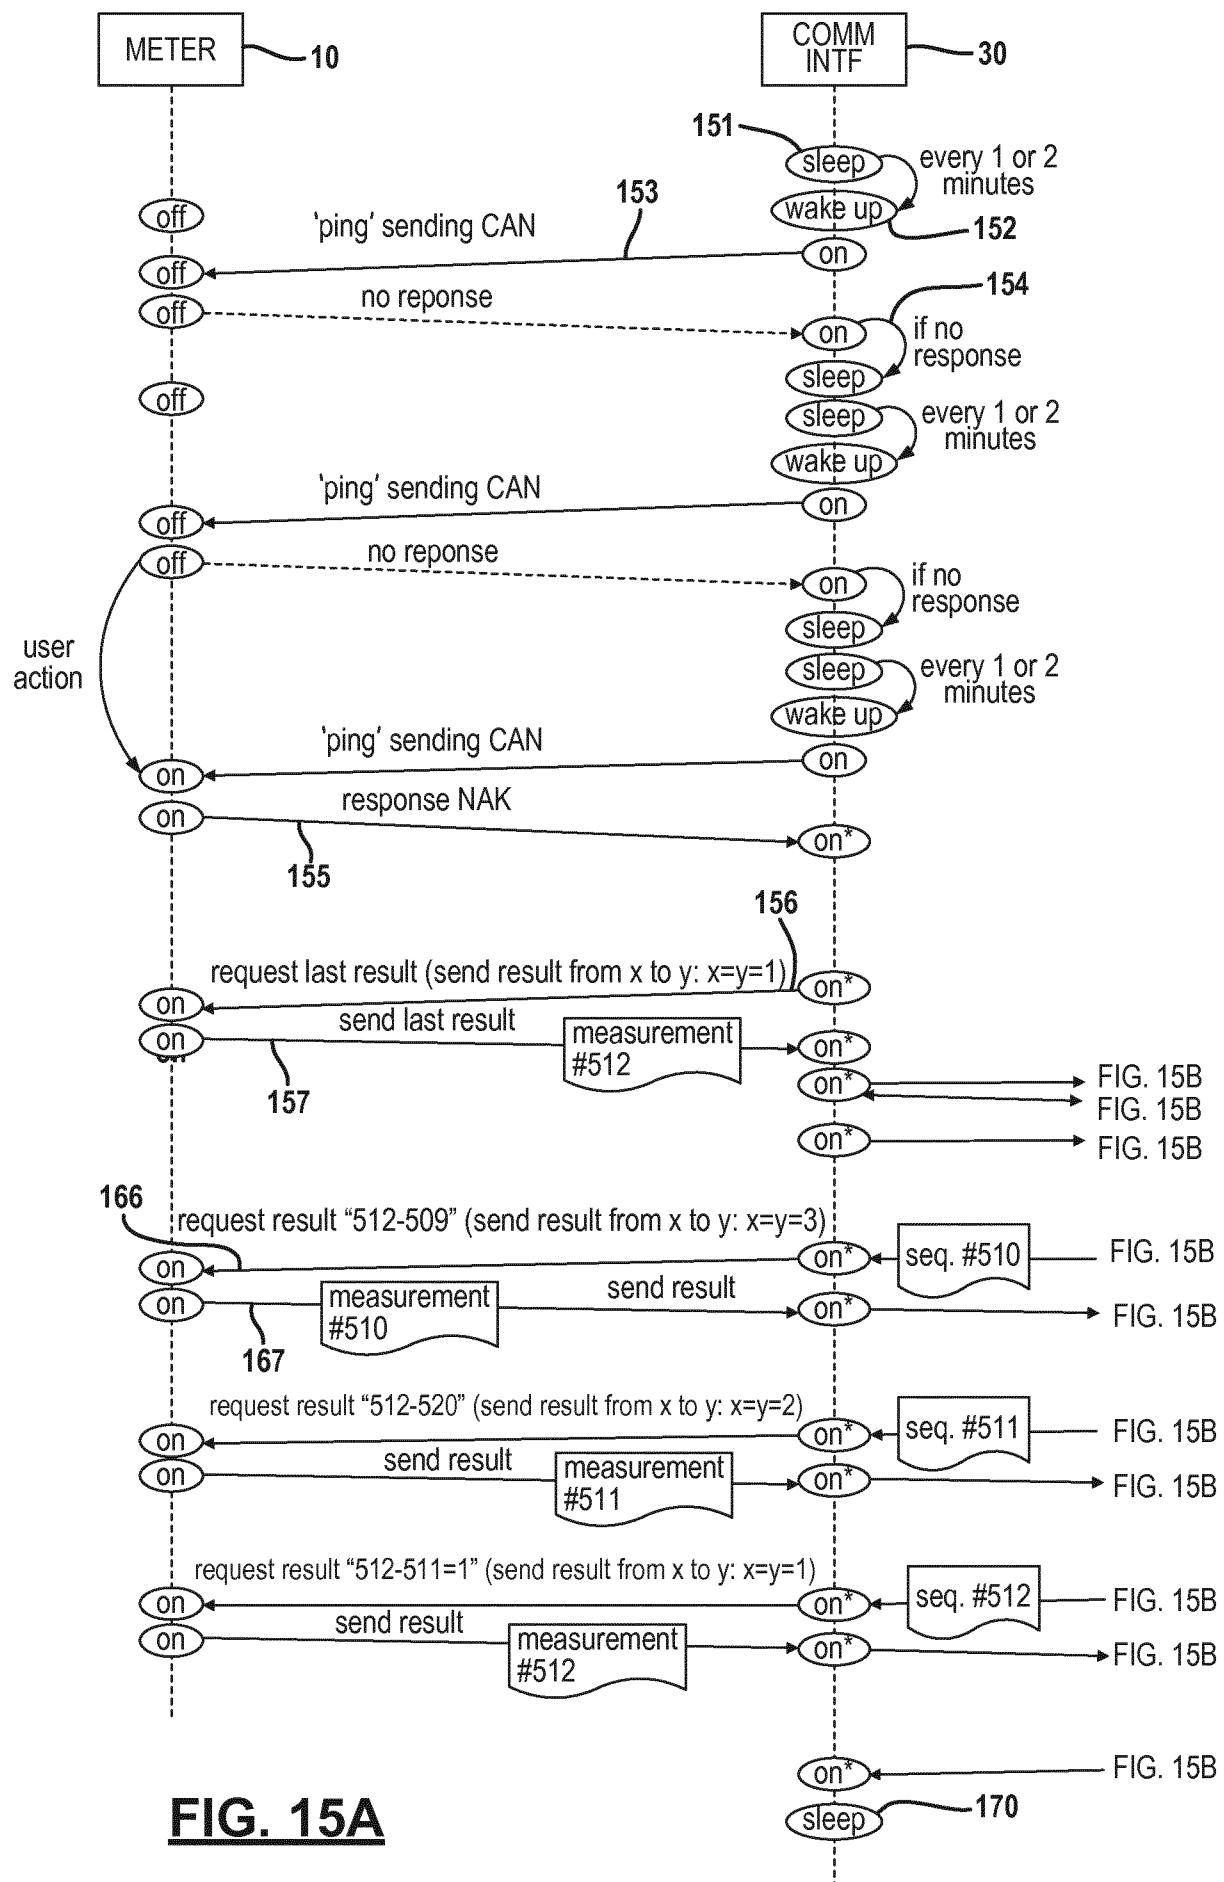**FIG. 15A**

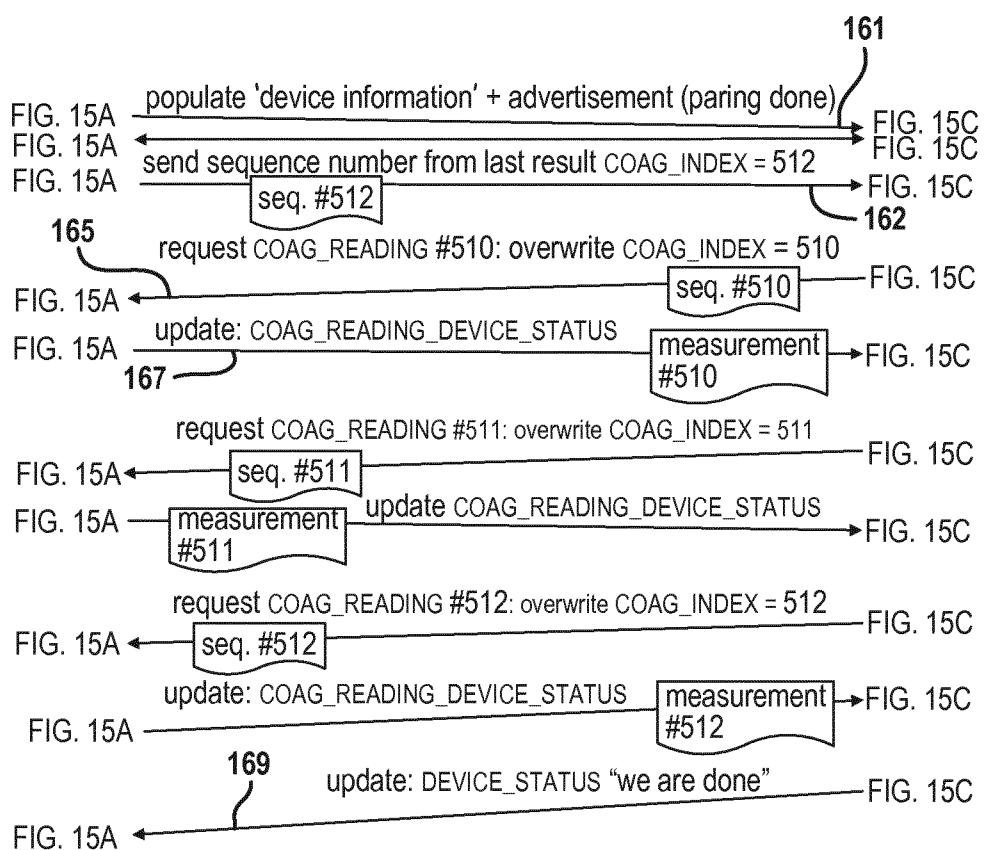**FIG. 15B**

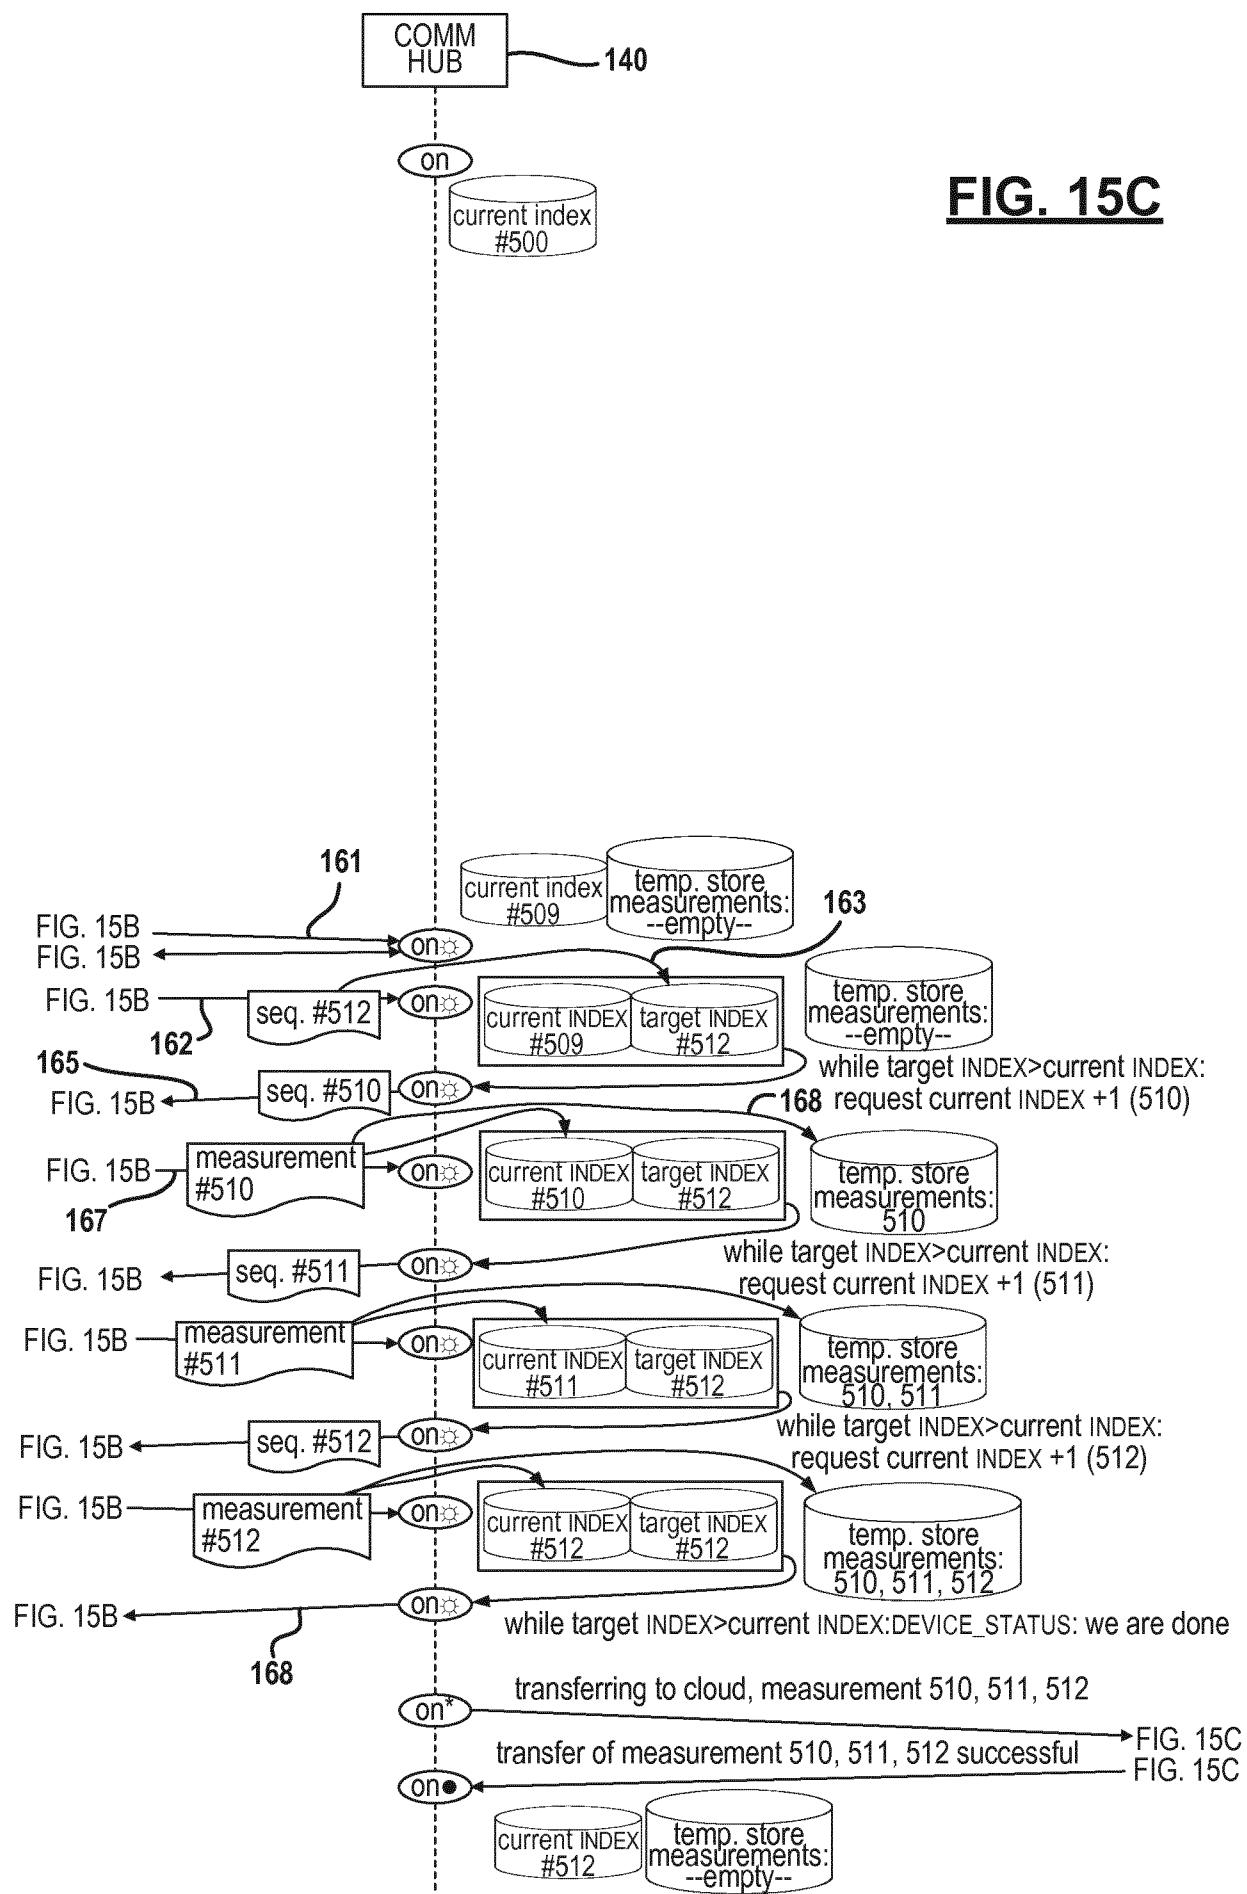

12/13


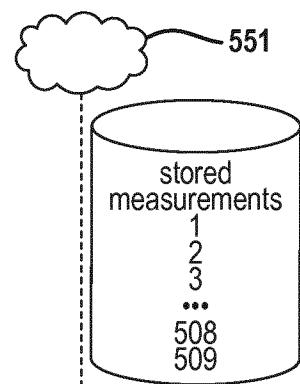
**FIG. 15D**

FIG. 15C → transferring to cloud, measurement 510, 511, 512  
transfer of measurement 510, 511, 512 successful



171

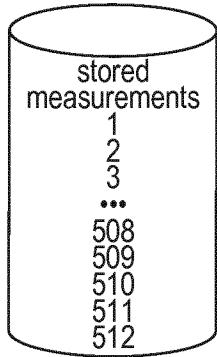

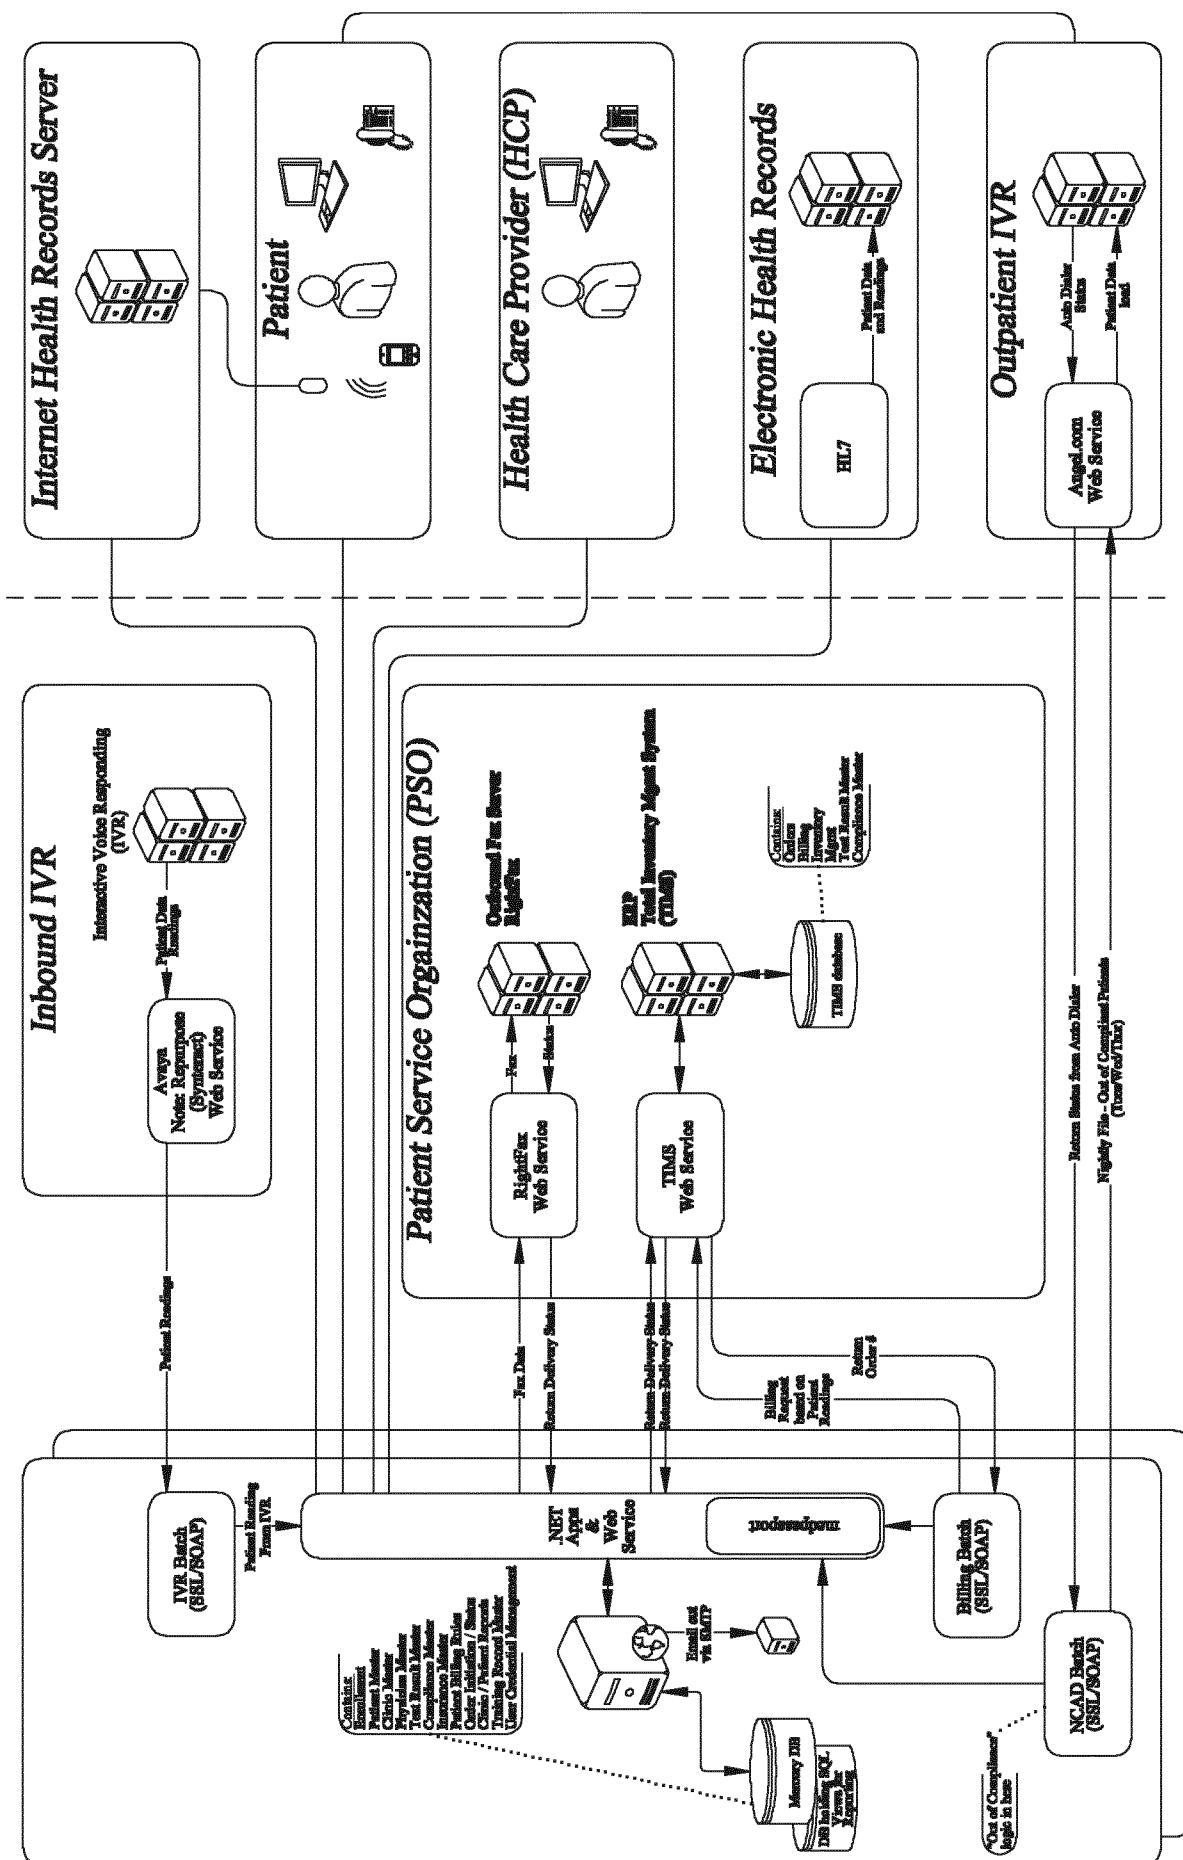


FIG. 15C ←

**FIG. 16**

# INTERNATIONAL SEARCH REPORT

International application No  
PCT/EP2014/072114

**A. CLASSIFICATION OF SUBJECT MATTER**  
INV. G01N27/327 A61B5/00 G01N33/487 G06F19/00  
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
G01N A61B G06F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data, INSPEC, COMPENDEX, BIOSIS

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2011/256024 A1 (COLE JEAN-PIERRE [US] ET AL) 20 October 2011 (2011-10-20)  claims 1-25; figures 1,5 -----	1-8, 10-12, 14,15
A	WO 2011/094075 A2 (MEDTRONIC INC [US]; KIVI GARY P [US]) 4 August 2011 (2011-08-04) abstract -----	1
X	WO 2004/090503 A2 (ABBOTT LAB [US]; CONNOLLY BRIAN E [US]; MACE CHAD H [US]; LAI MARC R [) 21 October 2004 (2004-10-21) the whole document -----	1
A	US 2012/095312 A1 (RAMEY BLAINE EDWARD [IN] ET AL RAMEY BLAINE EDWARD [US] ET AL) 19 April 2012 (2012-04-19) the whole document -----	1-15



Further documents are listed in the continuation of Box C.



See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

Date of mailing of the international search report

12 December 2014

23/12/2014

Name and mailing address of the ISA/  
European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040,  
Fax: (+31-70) 340-3016

Authorized officer

Joyce, David

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/EP2014/072114
---

Patent document cited in search report	Publication date	Patent family member(s)			Publication date
US 2011256024	A1	20-10-2011	NONE		
-----					
WO 2011094075	A2	04-08-2011	US 2011184491 A1	28-07-2011	
			WO 2011094075 A2	04-08-2011	
-----					
WO 2004090503	A2	21-10-2004	CA 2521494 A1	21-10-2004	
			EP 1611500 A2	04-01-2006	
			JP 4403176 B2	20-01-2010	
			JP 2006522346 A	28-09-2006	
			US 2004249999 A1	09-12-2004	
			US 2010076288 A1	25-03-2010	
			US 2010082266 A1	01-04-2010	
			US 2010121168 A1	13-05-2010	
			US 2010309001 A1	09-12-2010	
			US 2014207384 A1	24-07-2014	
			WO 2004090503 A2	21-10-2004	
-----					
US 2012095312	A1	19-04-2012	CA 2809076 A1	19-04-2012	
			CN 103501697 A	08-01-2014	
			EP 2627253 A1	21-08-2013	
			JP 2013545970 A	26-12-2013	
			KR 20130042001 A	25-04-2013	
			US 2012095312 A1	19-04-2012	
			WO 2012049238 A1	19-04-2012	
-----					