



(19) **United States**

(12) **Patent Application Publication**

Brock et al.

(10) **Pub. No.: US 2002/0095175 A1**

(43) **Pub. Date: Jul. 18, 2002**

(54) **FLEXIBLE INSTRUMENT**

(76) Inventors: **David L. Brock**, Natick, MA (US);
Woojin Lee, Hopkinton, MA (US);
Gary Rogers, Wenham, MA (US);
Barry Weitzner, Acton, MA (US)

Correspondence Address:
**Finnegan, Henderson, Farabow,
Garrett & Dunner, L.L.P.**
1300 I Street, N.W.
Washington, DC 20005-3315 (US)

(21) Appl. No.: **10/023,024**

(22) Filed: **Nov. 16, 2001**

Related U.S. Application Data

(60) Continuation-in-part of application No. 09/827,503, filed on Apr. 6, 2001, which is a continuation of application No. 09/746,853, filed on Dec. 21, 2000, which is a division of application No. 09/375,666, filed on Aug. 17, 1999, now Pat. No. 6,197,017, which is a continuation of application No. 09/028,550, filed on Feb. 24, 1998, now abandoned. Continuation-in-part of application No. 09/783,637, filed on Feb. 14, 2001, which is a continuation of application No. PCT/US00/12553, filed on May 9, 2000, which is a non-provisional of provisional application No. 60/133,407, filed on May 10, 1999. Continuation-in-part of application No. PCT/US01/11376, filed on Apr. 6, 2001. Continuation-in-part of application No. 09/827,643, filed on Apr. 6, 2001, which is a non-provisional of provisional application No. 60/257,869, filed on Dec. 21, 2000, and which is a non-provisional of provisional application No. 60/195,264, filed on Apr. 7, 2000, and which is a continuation-in-part of application No. PCT/US00/12553, filed on May 9, 2000. Non-provisional of provisional application No. 60/293,346, filed on May 24, 2001. Non-provisional of provisional application No. 60/279,087, filed on Mar. 27, 2001. Non-provisional of provisional application No. 60/313,496,

filed on Aug. 21, 2001. Non-provisional of provisional application No. 60/313,497, filed on Aug. 21, 2001. Non-provisional of provisional application No. 60/313,495, filed on Aug. 21, 2001. Non-provisional of provisional application No. 60/269,203, filed on Feb. 15, 2001. Non-provisional of provisional application No. 60/269,200, filed on Feb. 15, 2001. Non-provisional of provisional application No. 60/276,151, filed on Mar. 15, 2001. Non-provisional of provisional application No. 60/276,217, filed on Mar. 15, 2001. Non-provisional of provisional application No. 60/276,086, filed on Mar. 15, 2001. Non-provisional of provisional application No. 60/276,152, filed on Mar. 15, 2001. Non-provisional of provisional application No. 60/257,816, filed on Dec. 21, 2000. Non-provisional of provisional application No. 60/257,868, filed on Dec. 21, 2000. Non-provisional of provisional application No. 60/257,867, filed on Dec. 21, 2000. Non-provisional of provisional application No. 60/257,869, filed on Dec. 21, 2000.

Publication Classification

(51) **Int. Cl.⁷** **A61B 17/00**
(52) **U.S. Cl.** **606/205; 606/1**

(57) **ABSTRACT**

A remote control flexible instrument system, employing a shaft which supports a tool, is described in which the has proximal and distal ends with at least a portion thereof extending through a lumen of the human body so as to locate the shaft at an internal target site. A master station including an input device provides control of the instrument situated at a slave station. The master station can control at least one degree-of-freedom of the flexible instrument. A controller intercouples the master and slave stations and is operated in accordance with a computer algorithm that receives a command from the input device for controlling at least one degree-of-freedom of the catheter so as to respond in accordance with action at the input device. The flexible instrument further comprises a controlled flexible segment along the shaft, for controlled bending at the flexible segment to guide the shaft and to dispose the tool at an operative site.

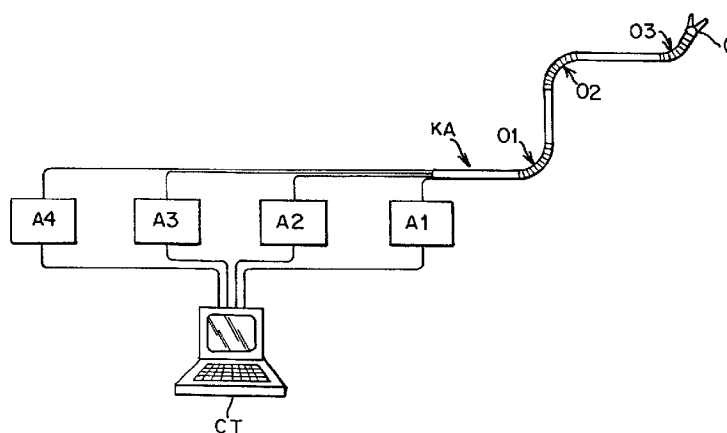




Fig. 1

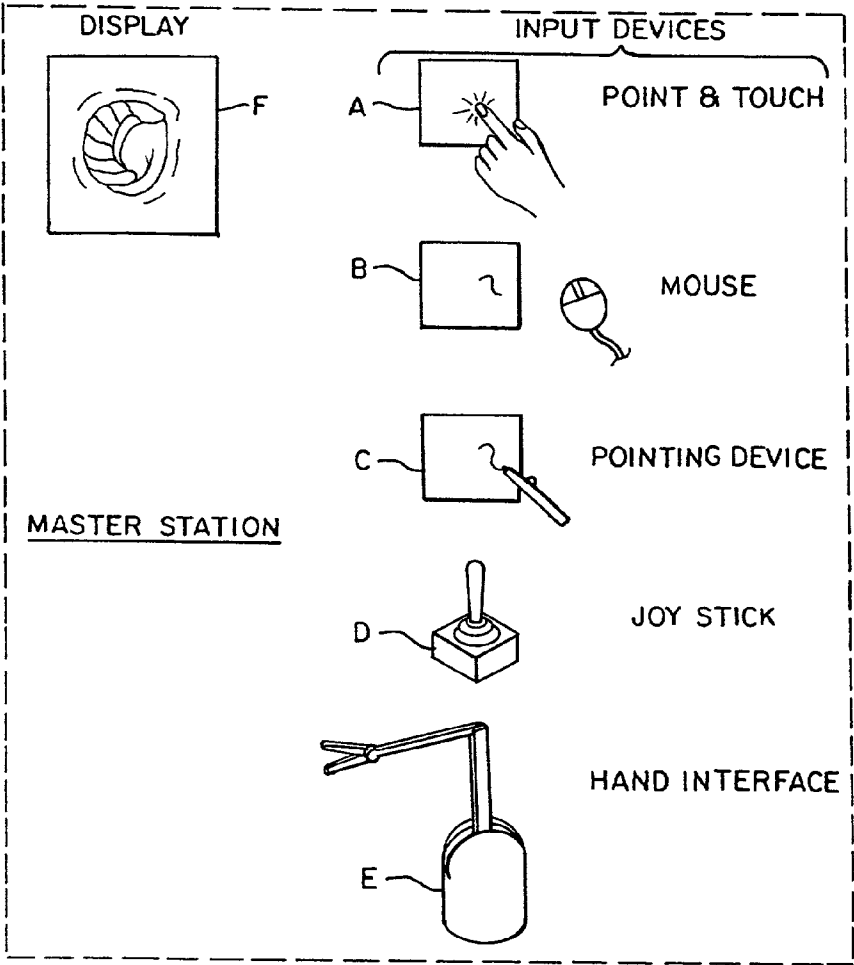


Fig. 2

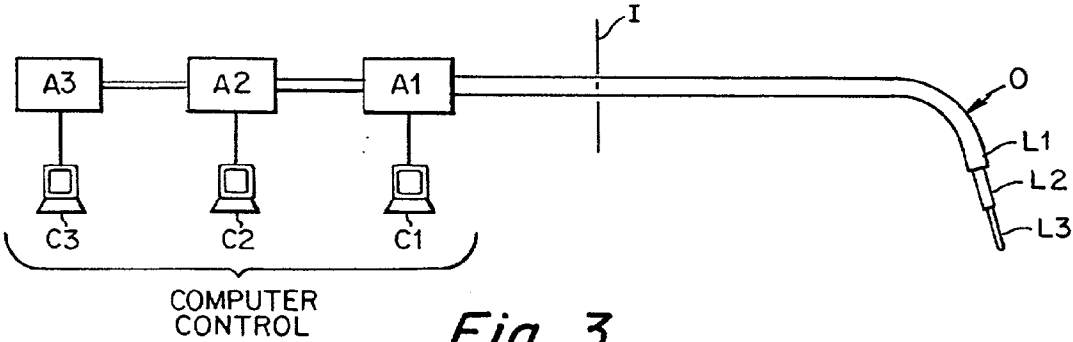


Fig. 3

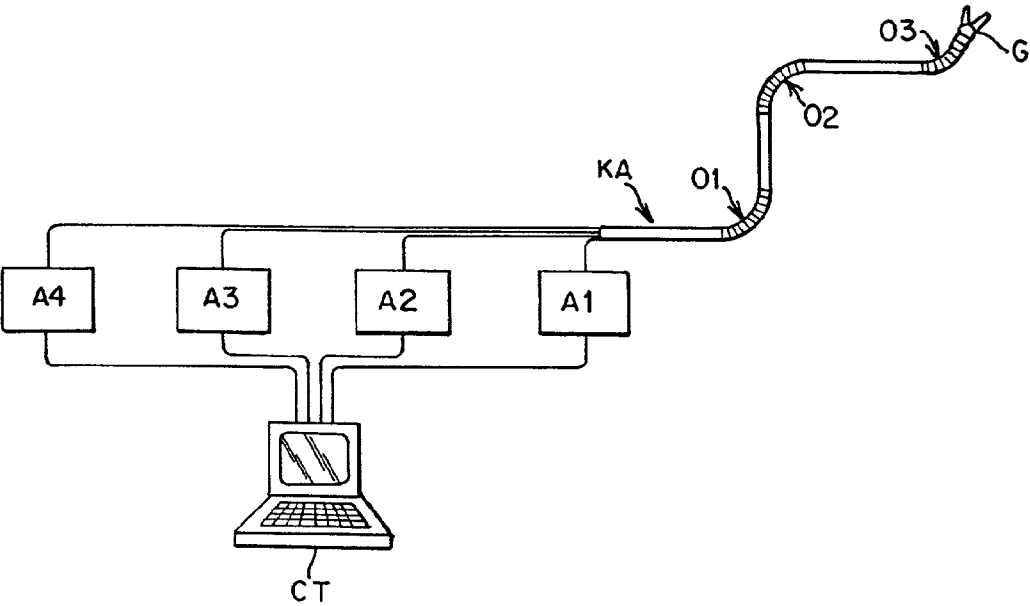


Fig. 3A

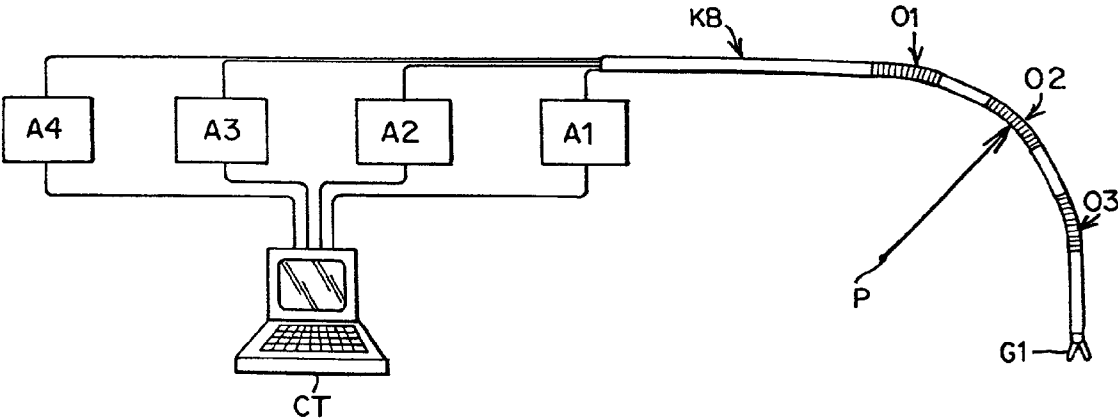


Fig. 3B

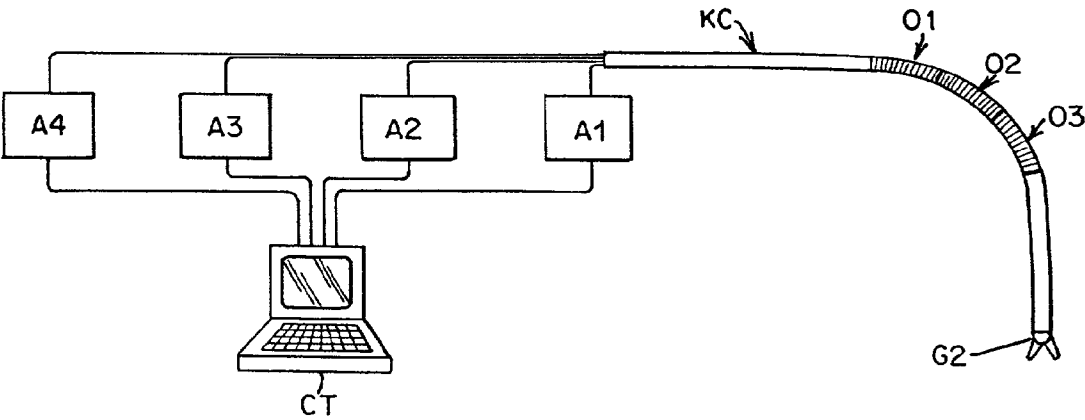


Fig. 3C

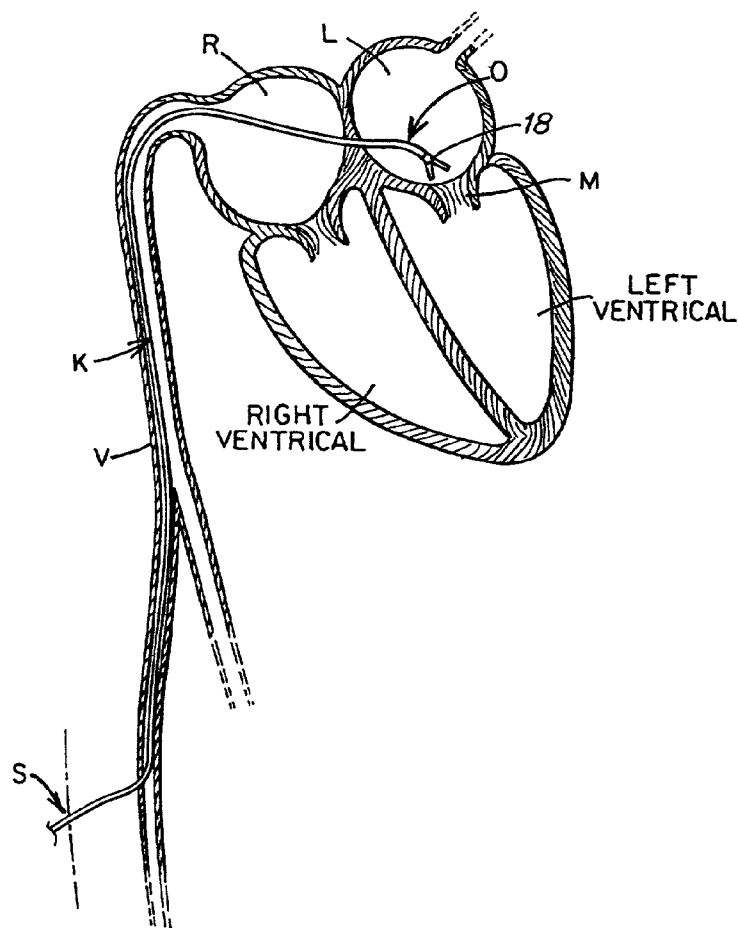


Fig. 4

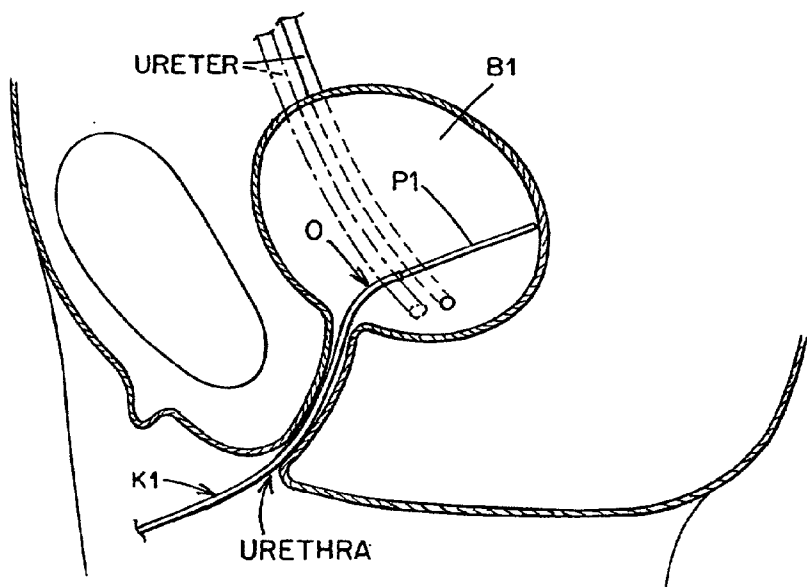


Fig. 5

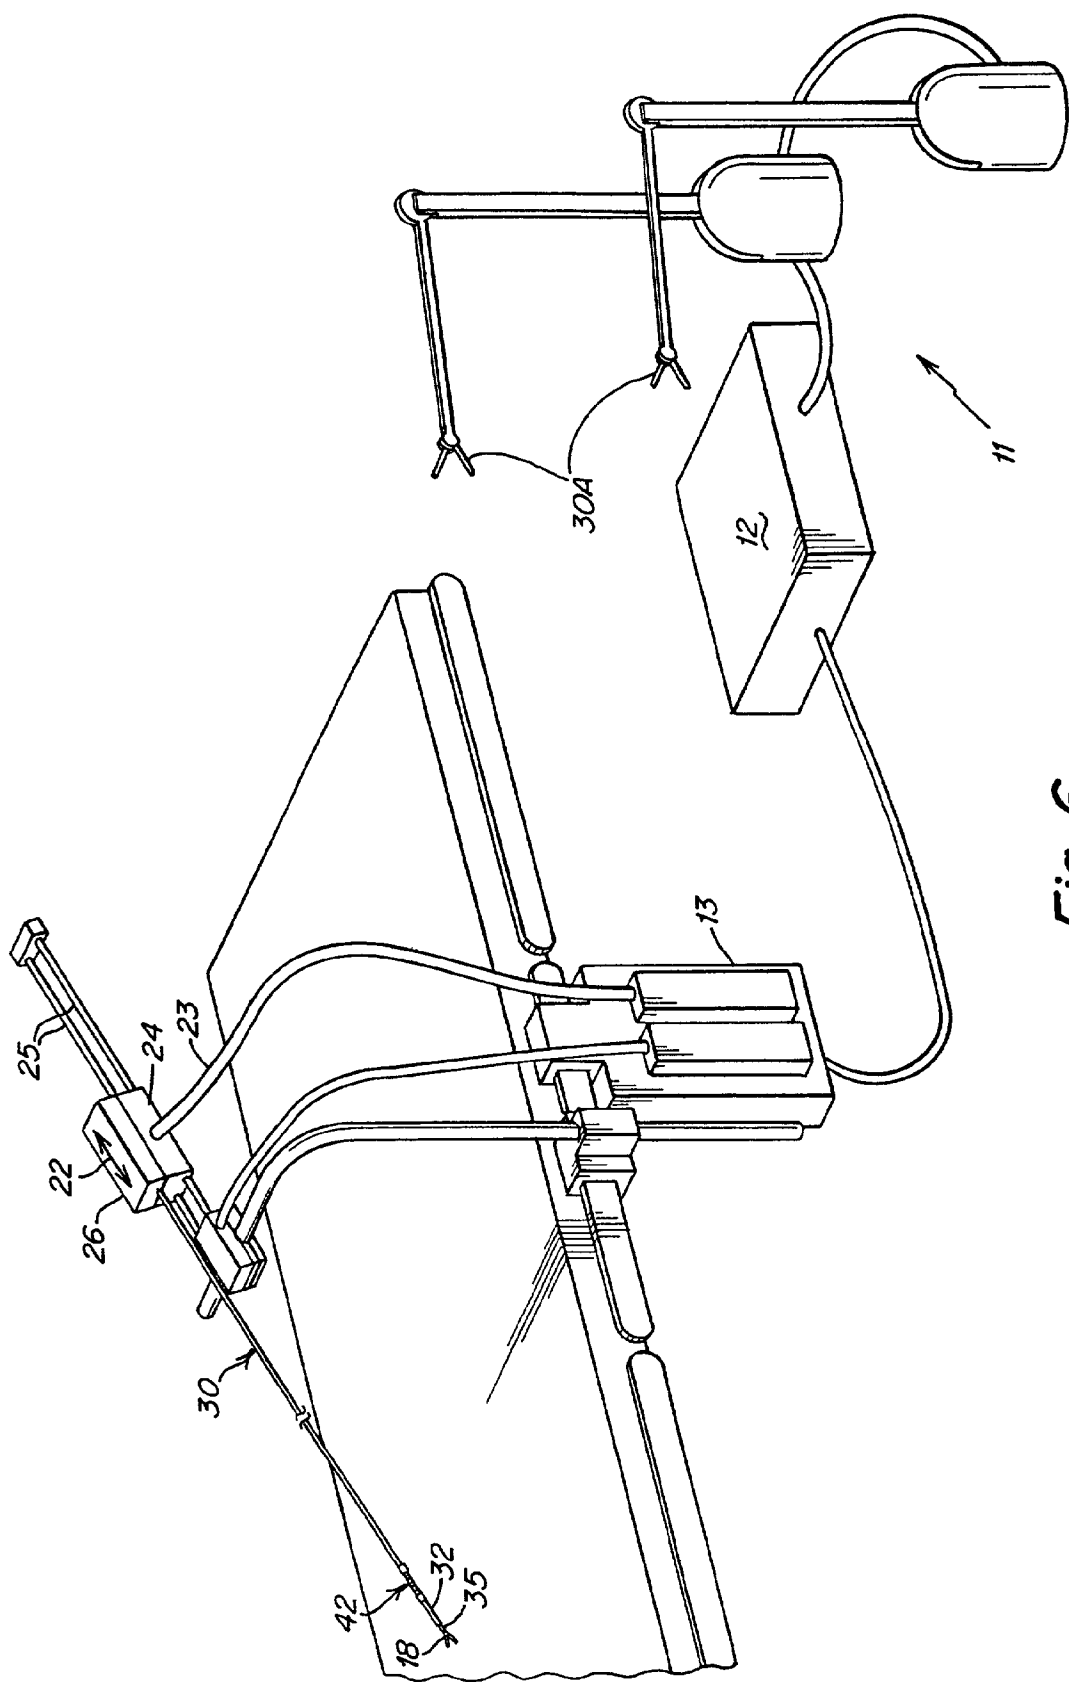
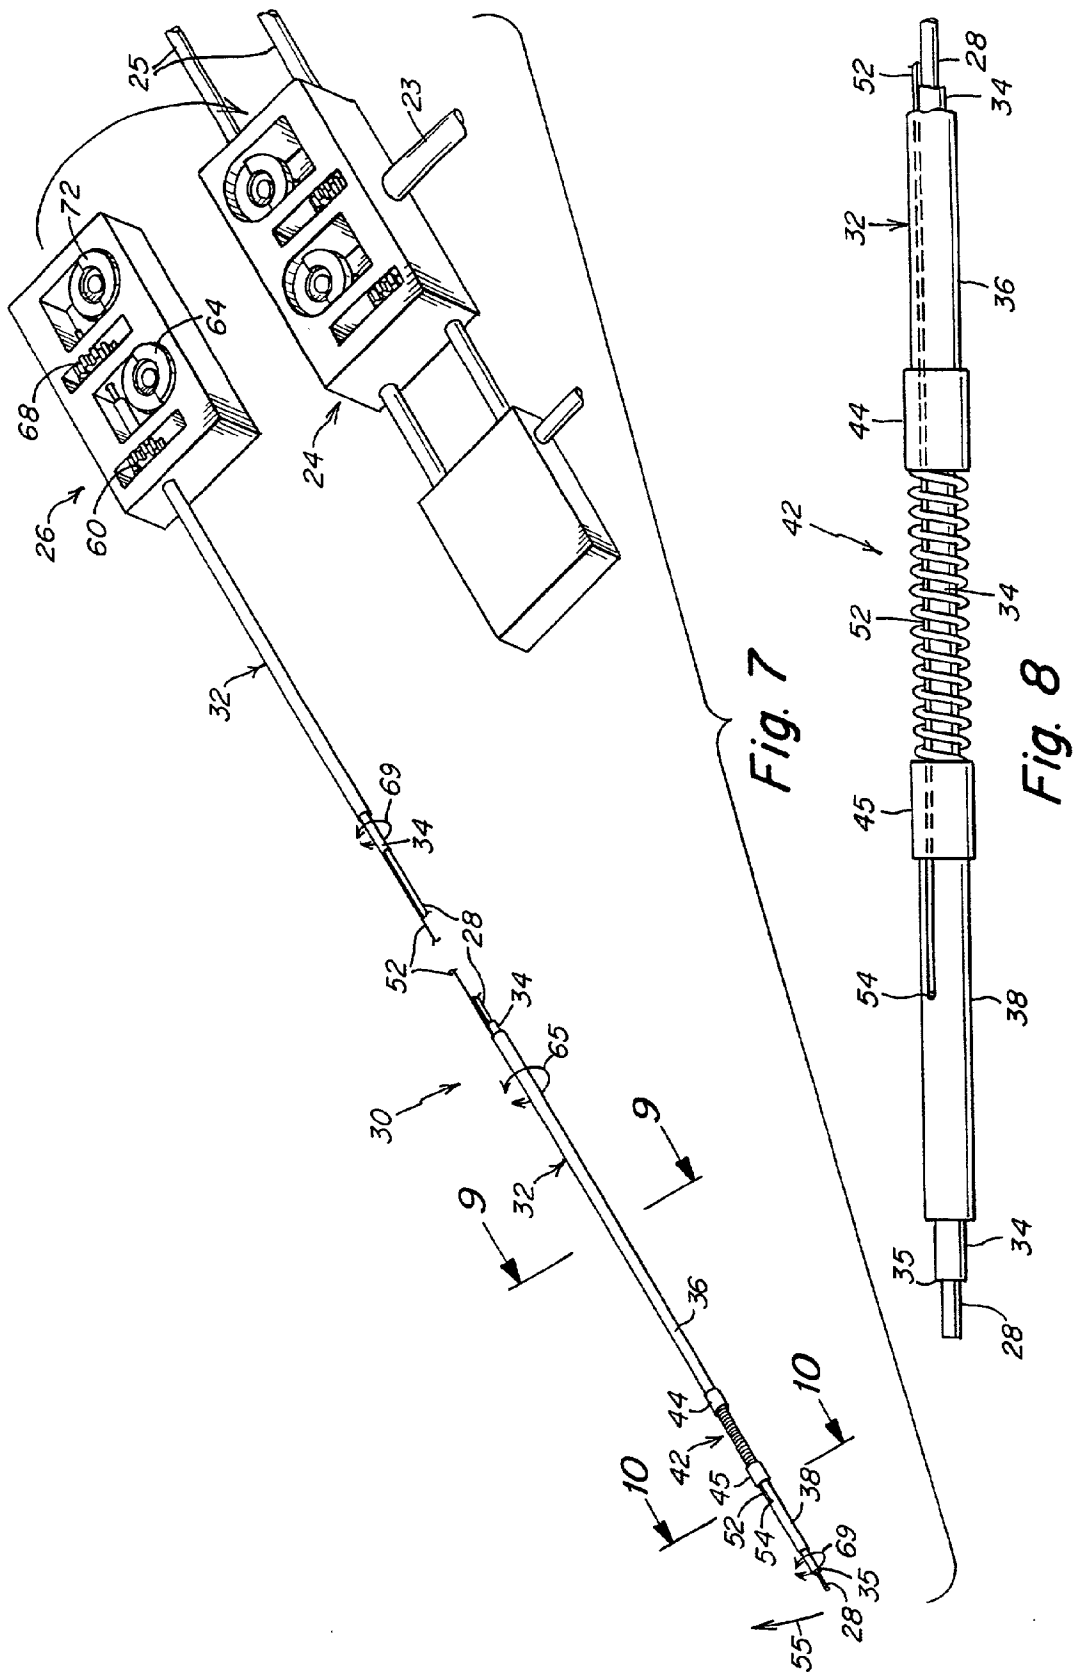


Fig. 6



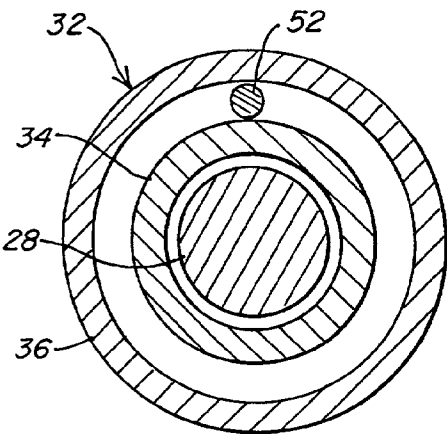


Fig. 9

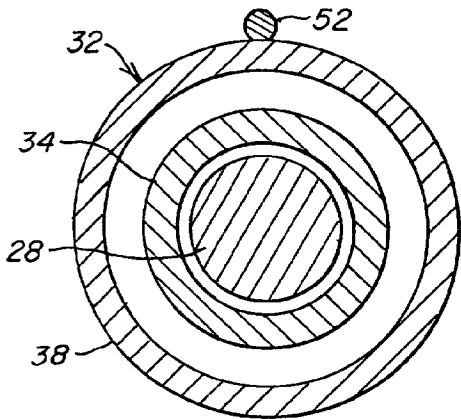


Fig. 10

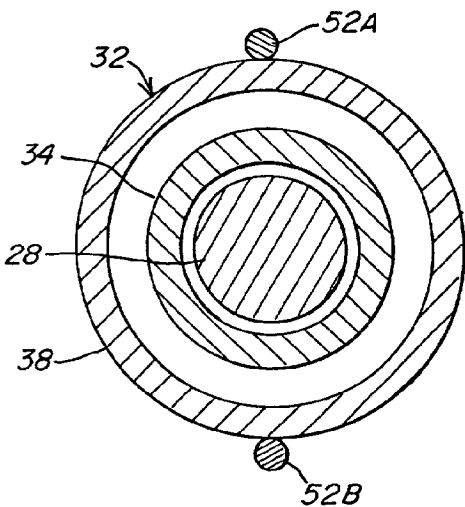


Fig. 11

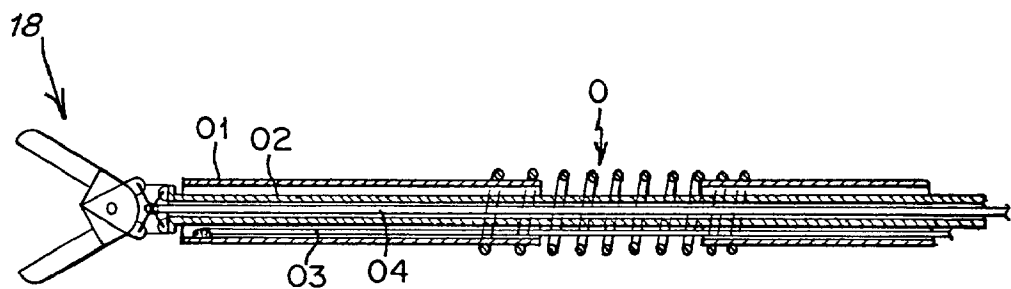


Fig. 12

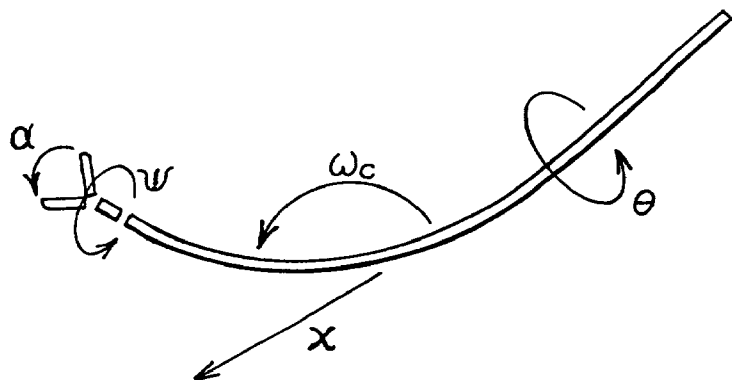


Fig. 13

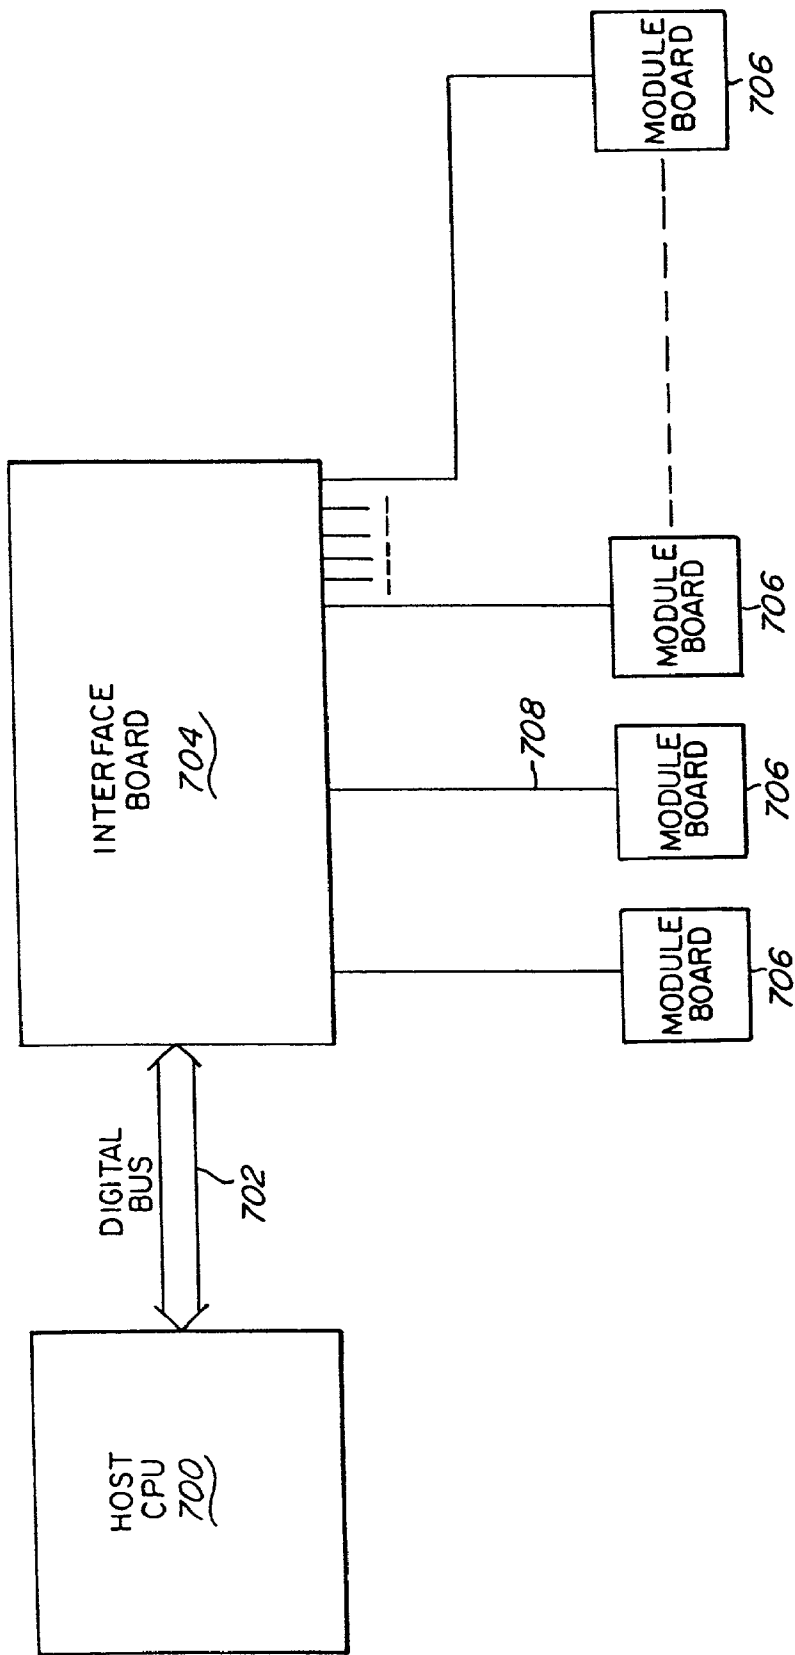


Fig. 14

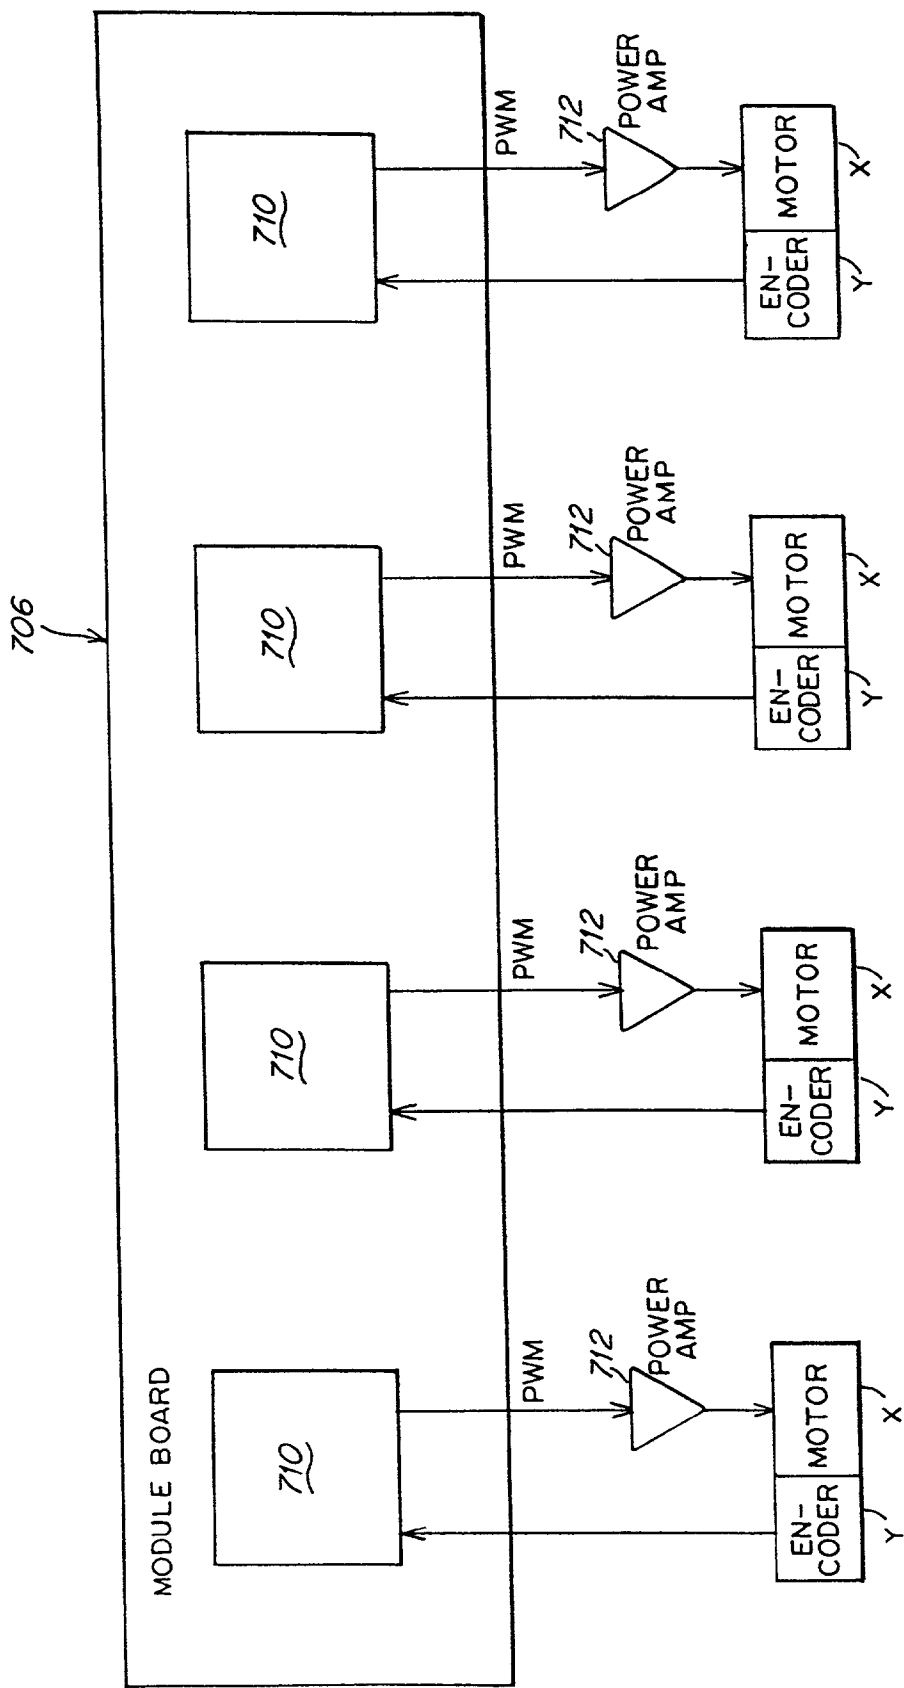


Fig. 15

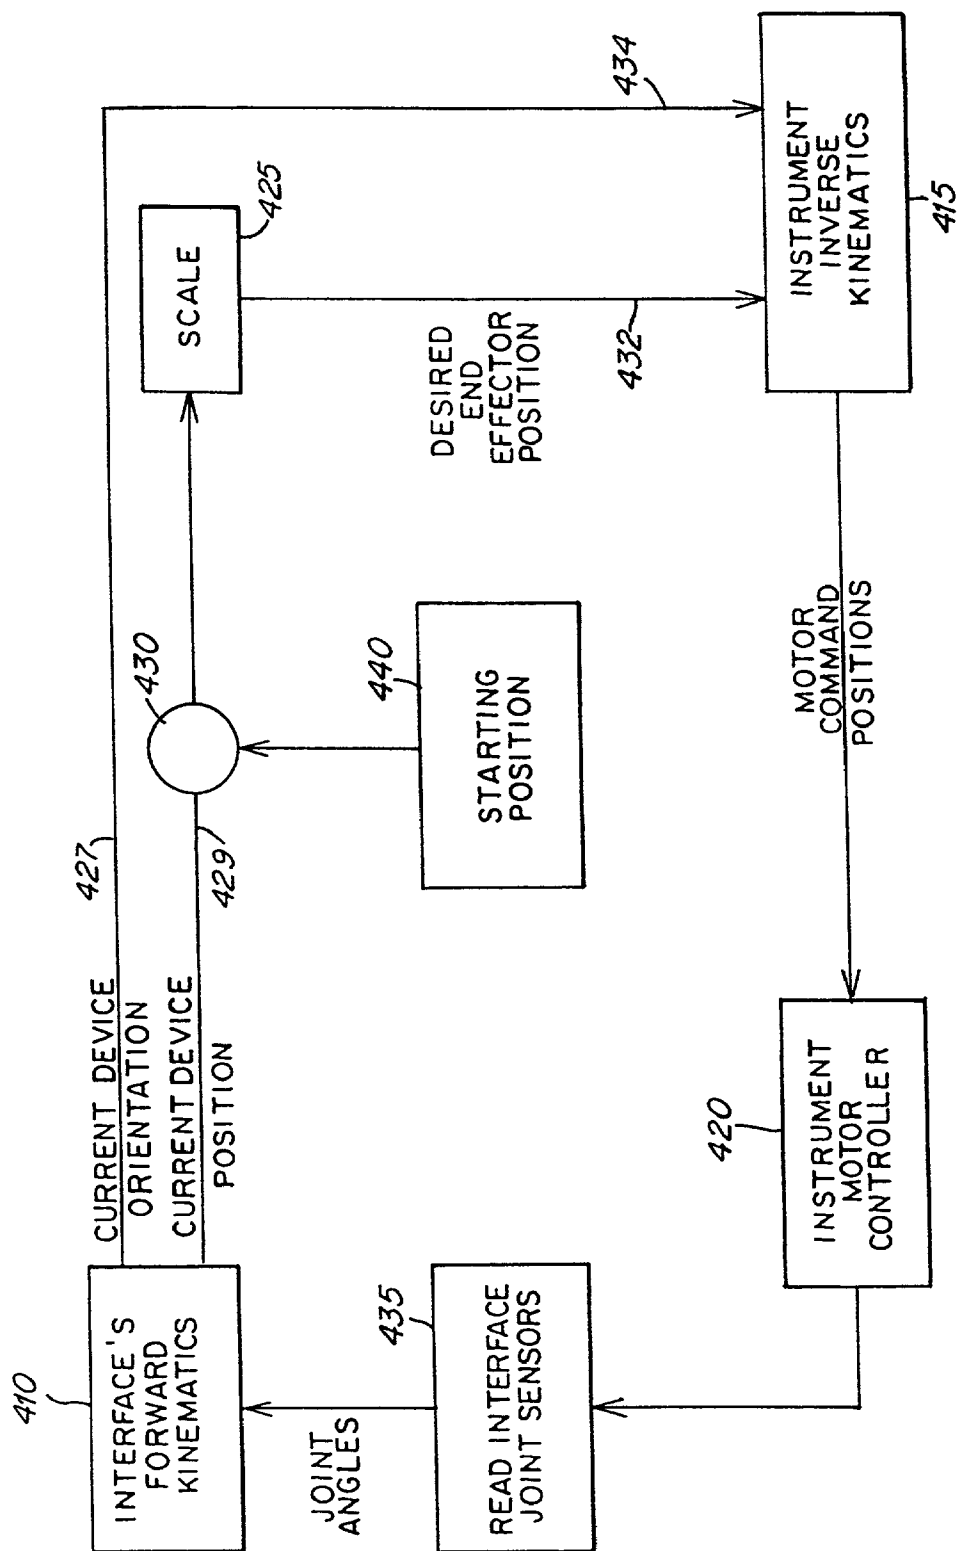


Fig. 16

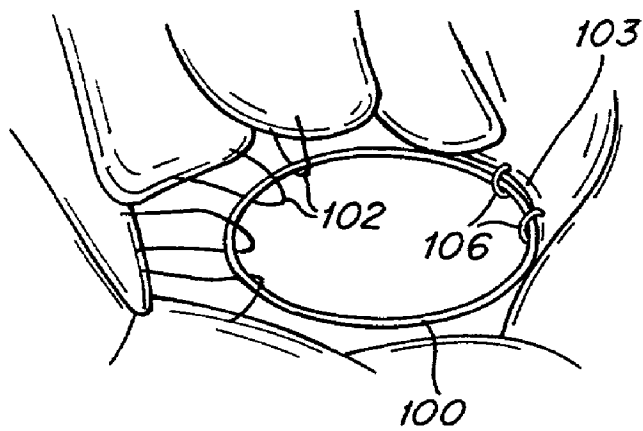


Fig. 17

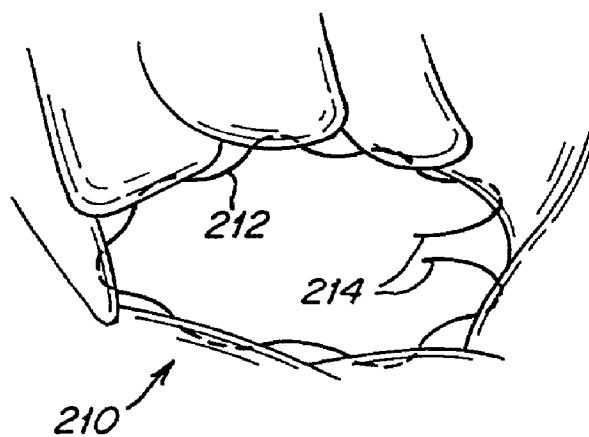


Fig. 18

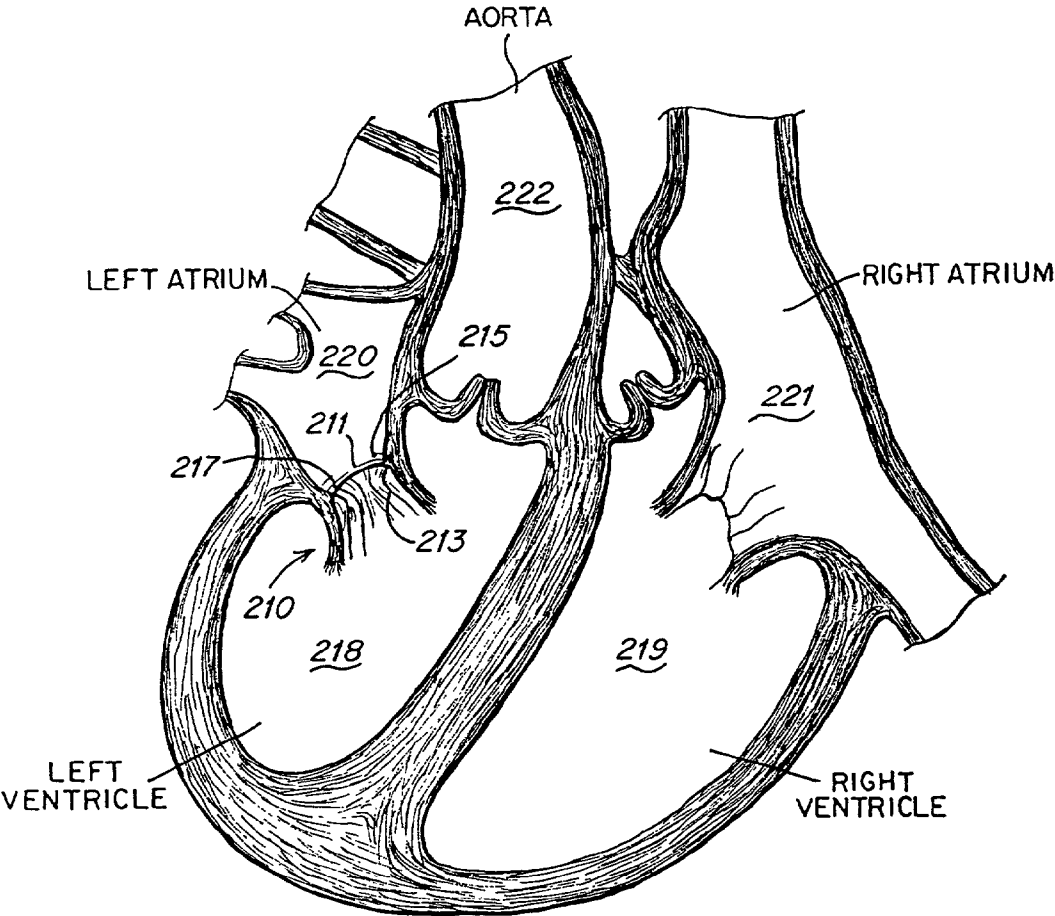


Fig. 19

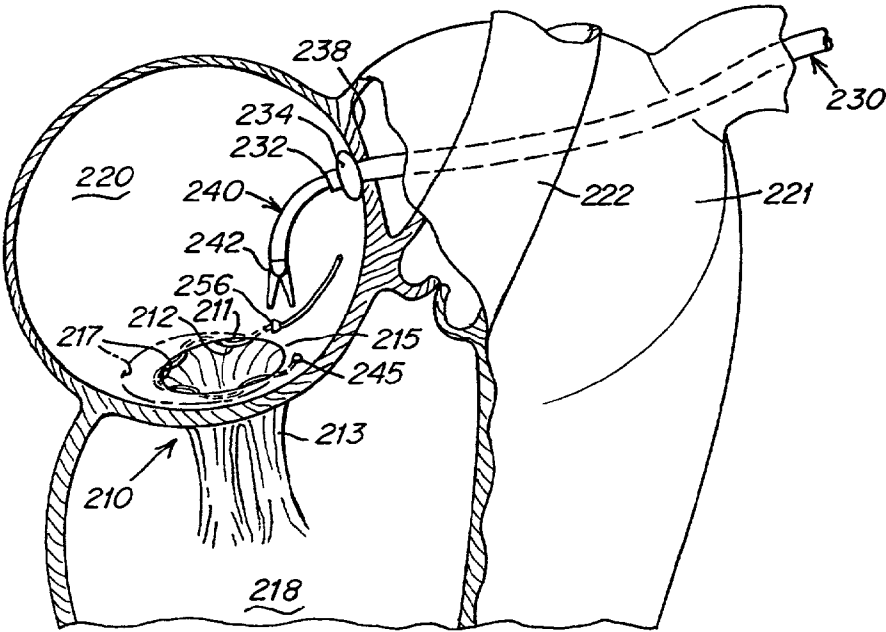


Fig. 20

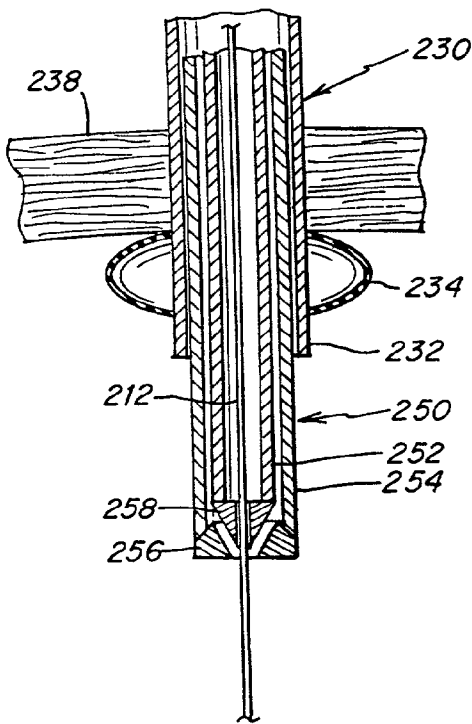


Fig. 21

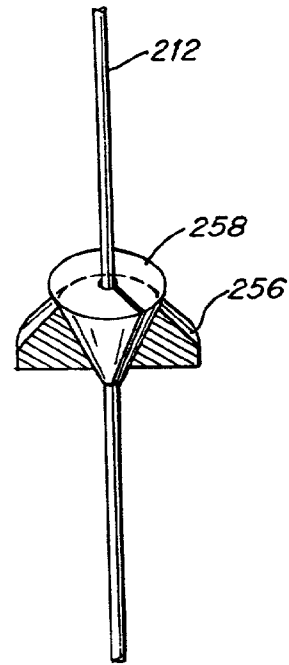


Fig. 22

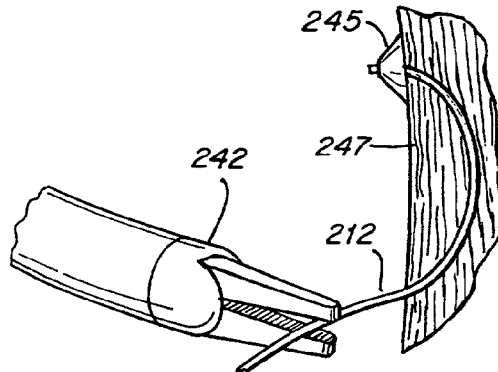


Fig. 23

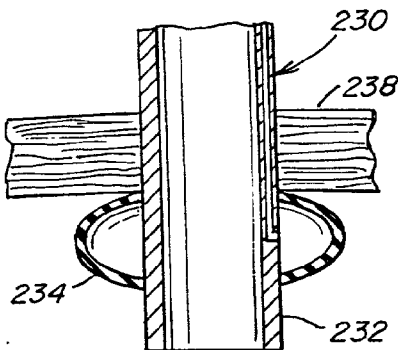


Fig. 24

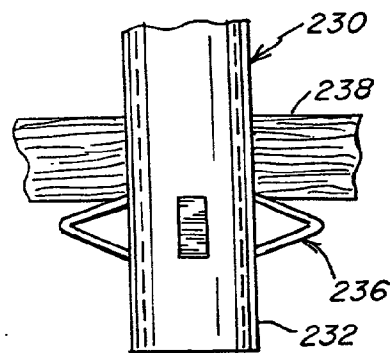


Fig. 25

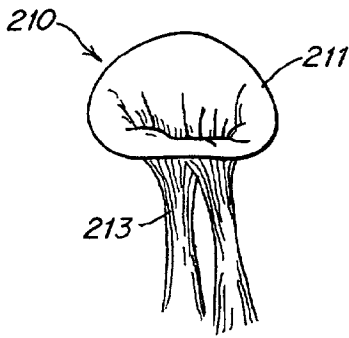


Fig. 26

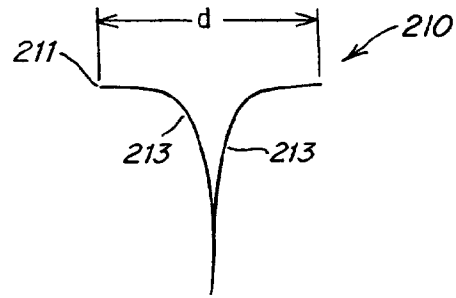


Fig. 27

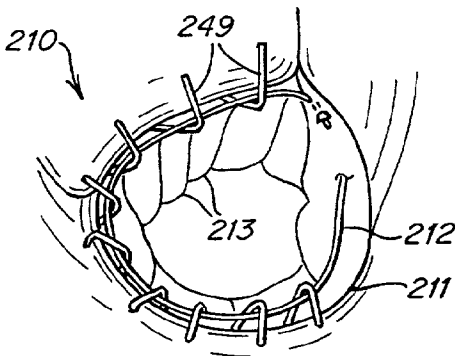


Fig. 28

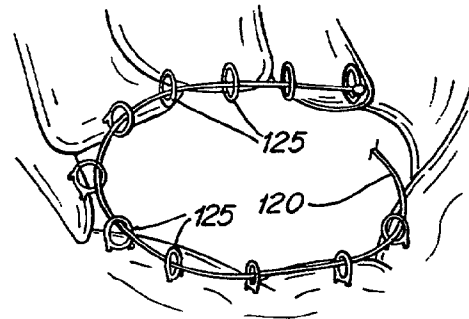


Fig. 29

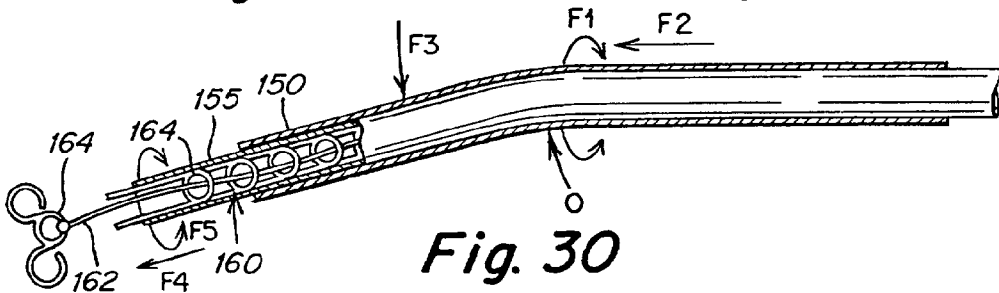


Fig. 30

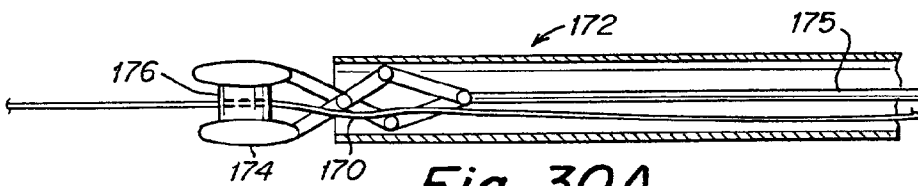


Fig. 30A

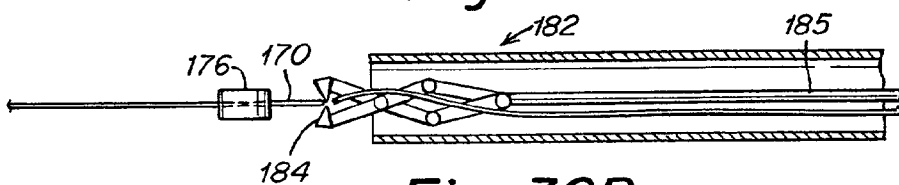


Fig. 30B

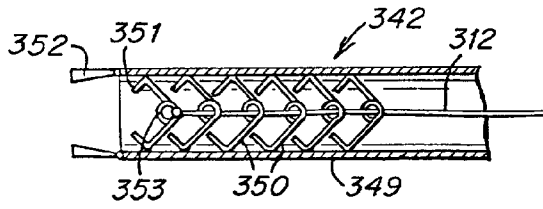


Fig. 31

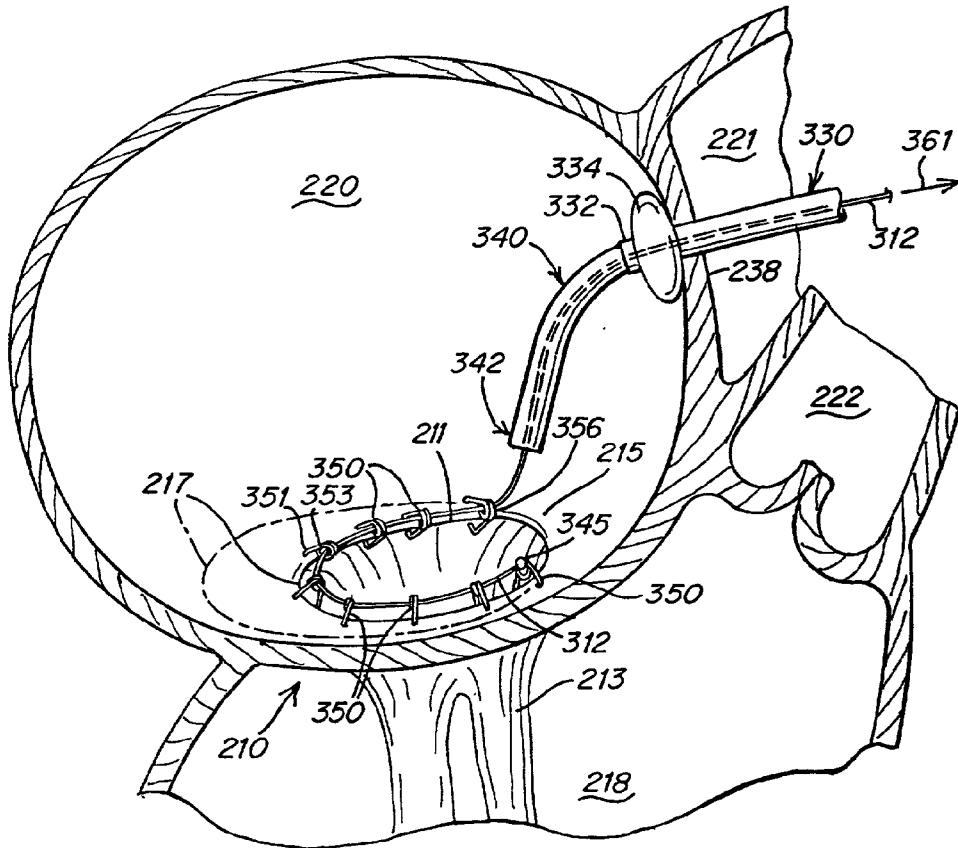


Fig. 32

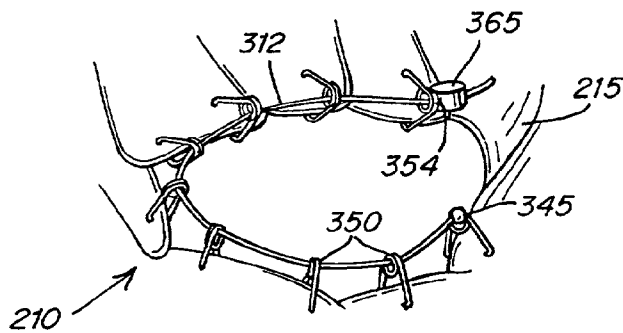


Fig. 33




Fig. 34

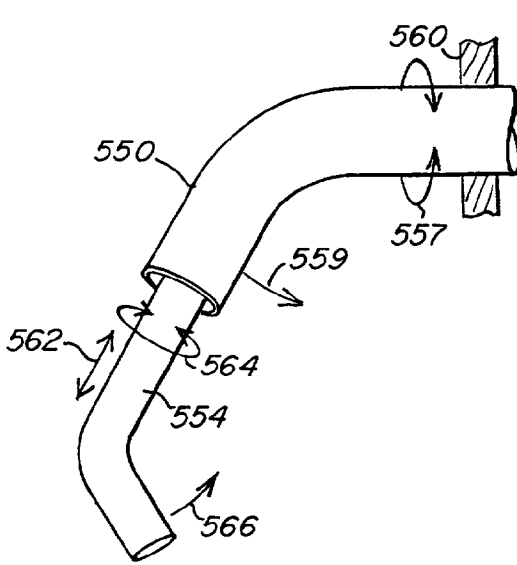


Fig. 35A

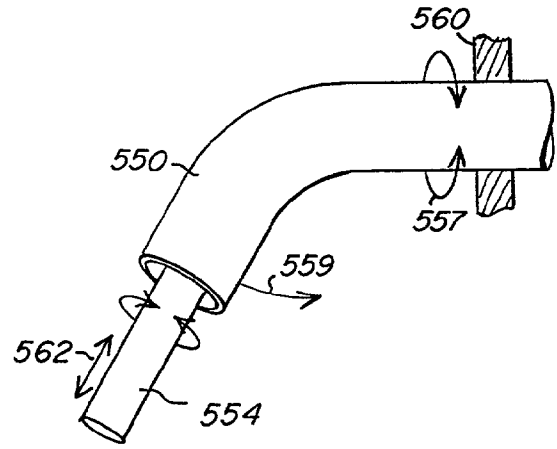


Fig. 35B

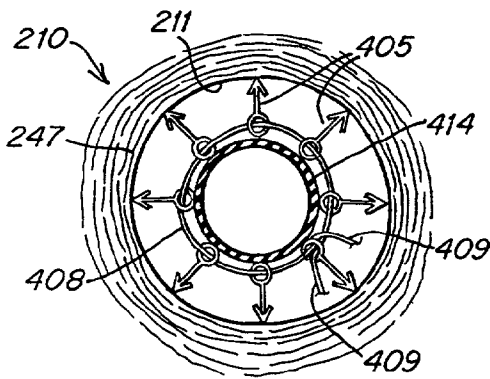


Fig. 36

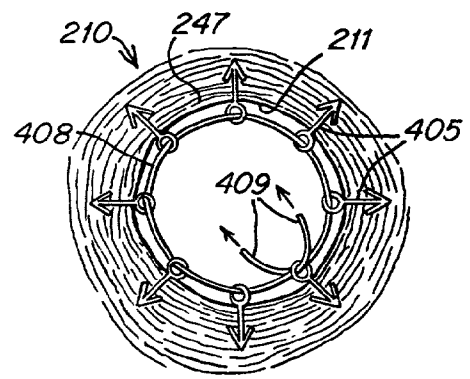


Fig. 37




Fig. 36A

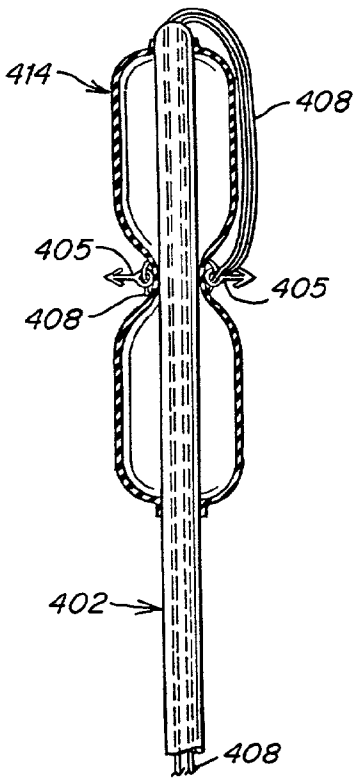


Fig. 38

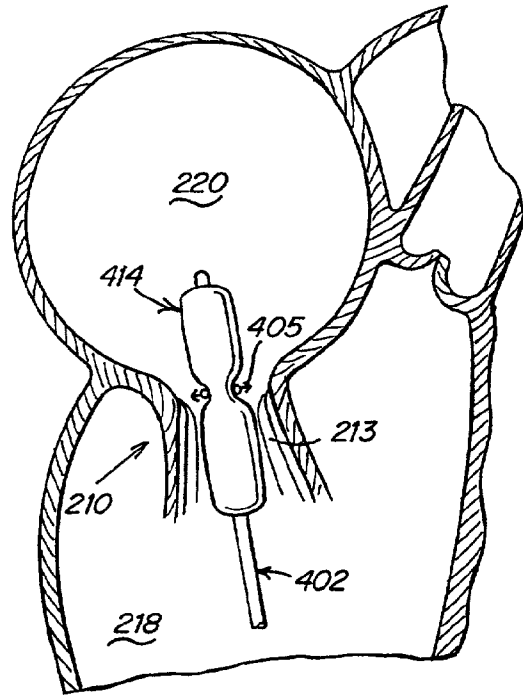


Fig. 39

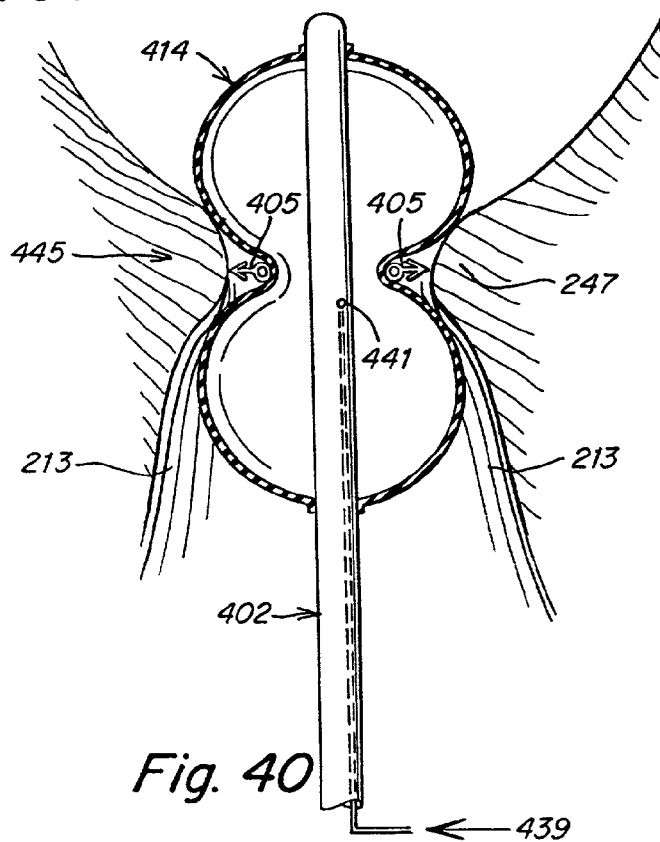


Fig. 40

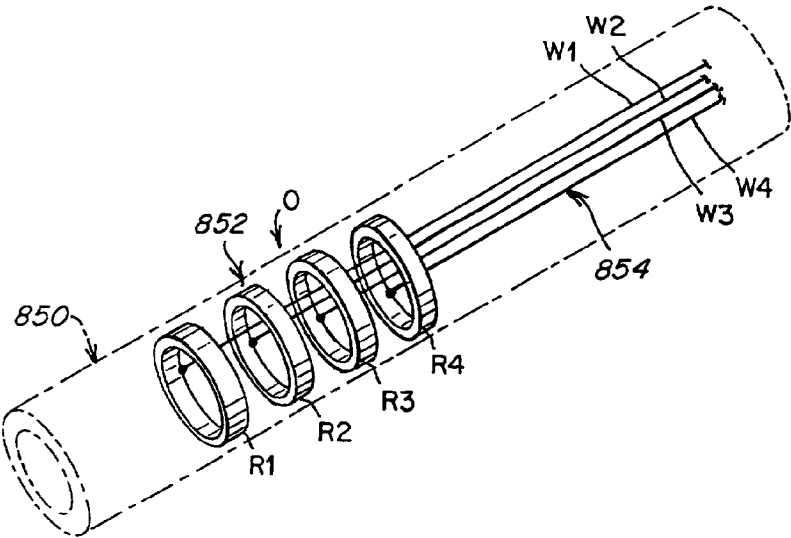


Fig. 41A




Fig. 41B




Fig. 41C

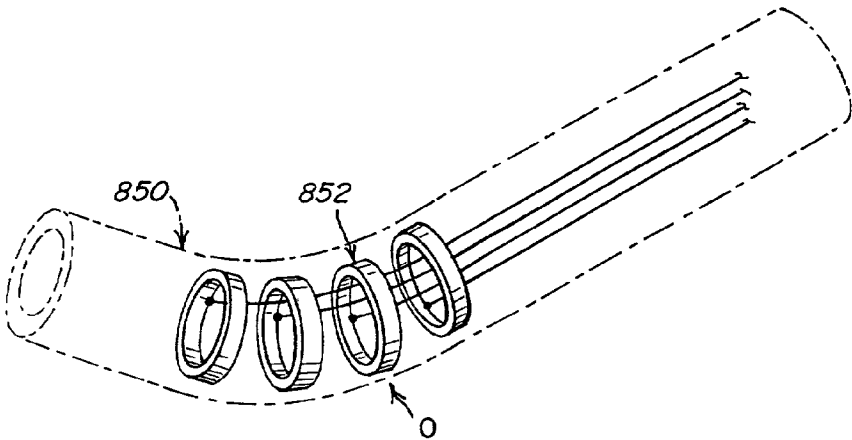
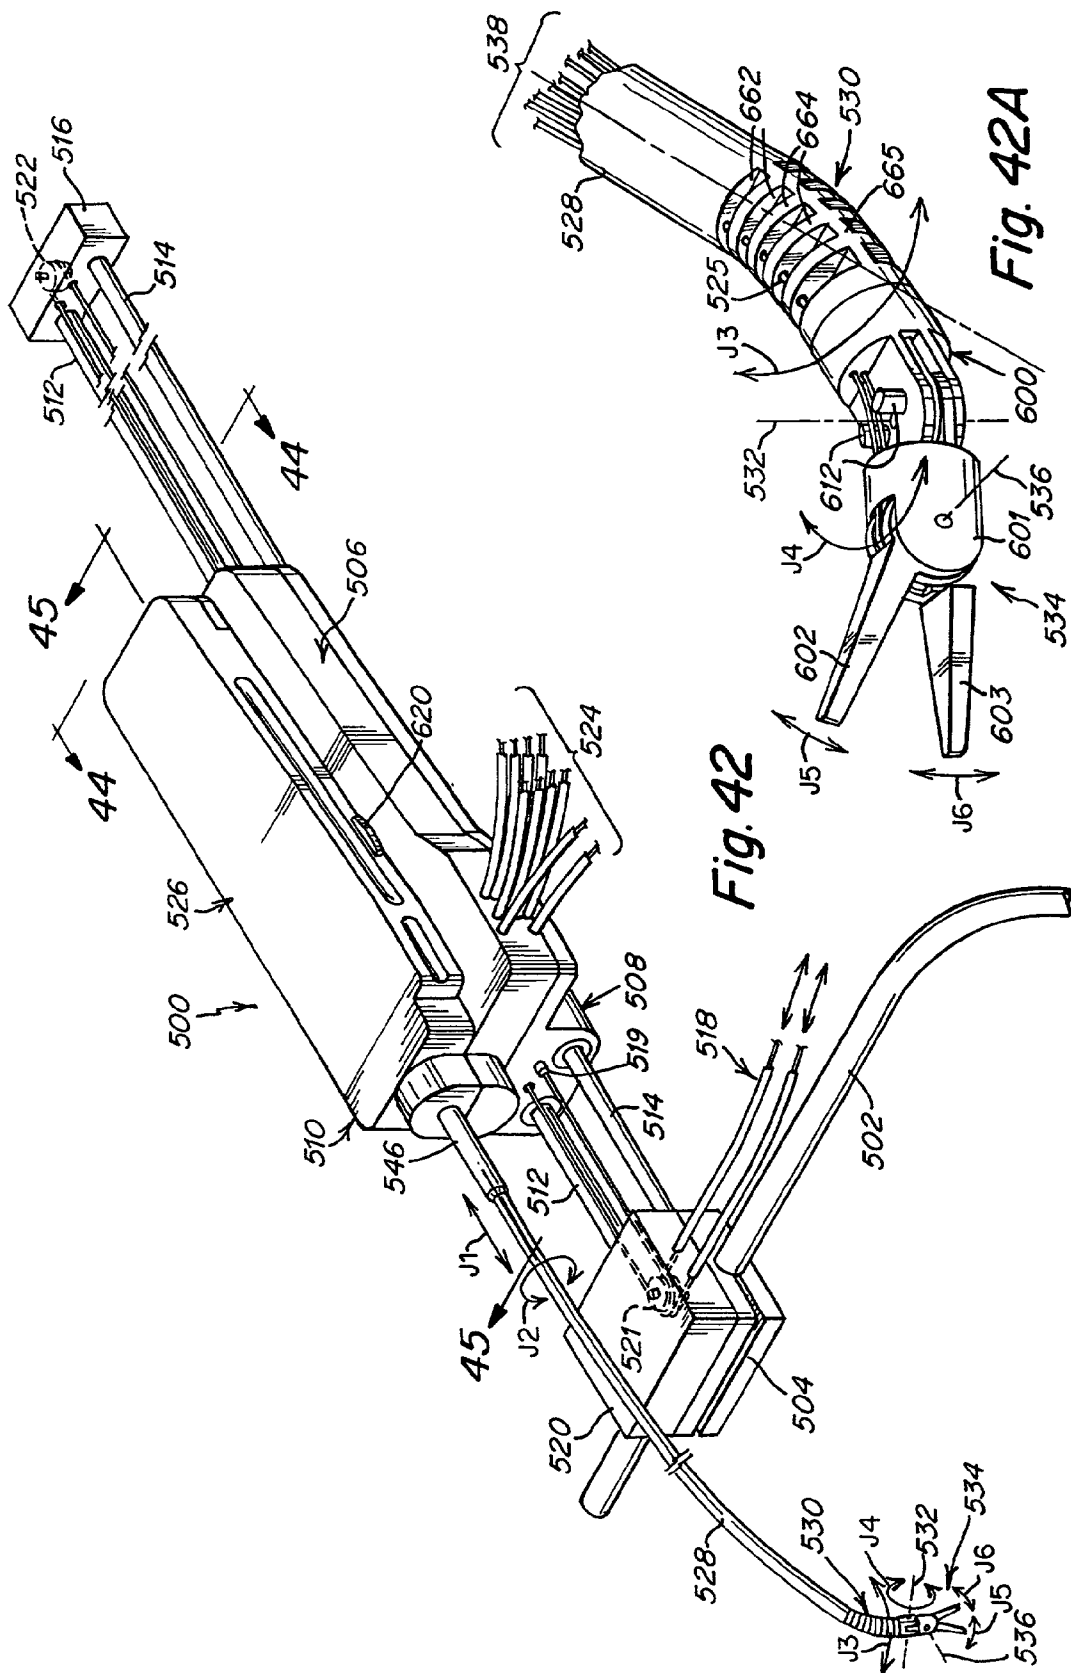
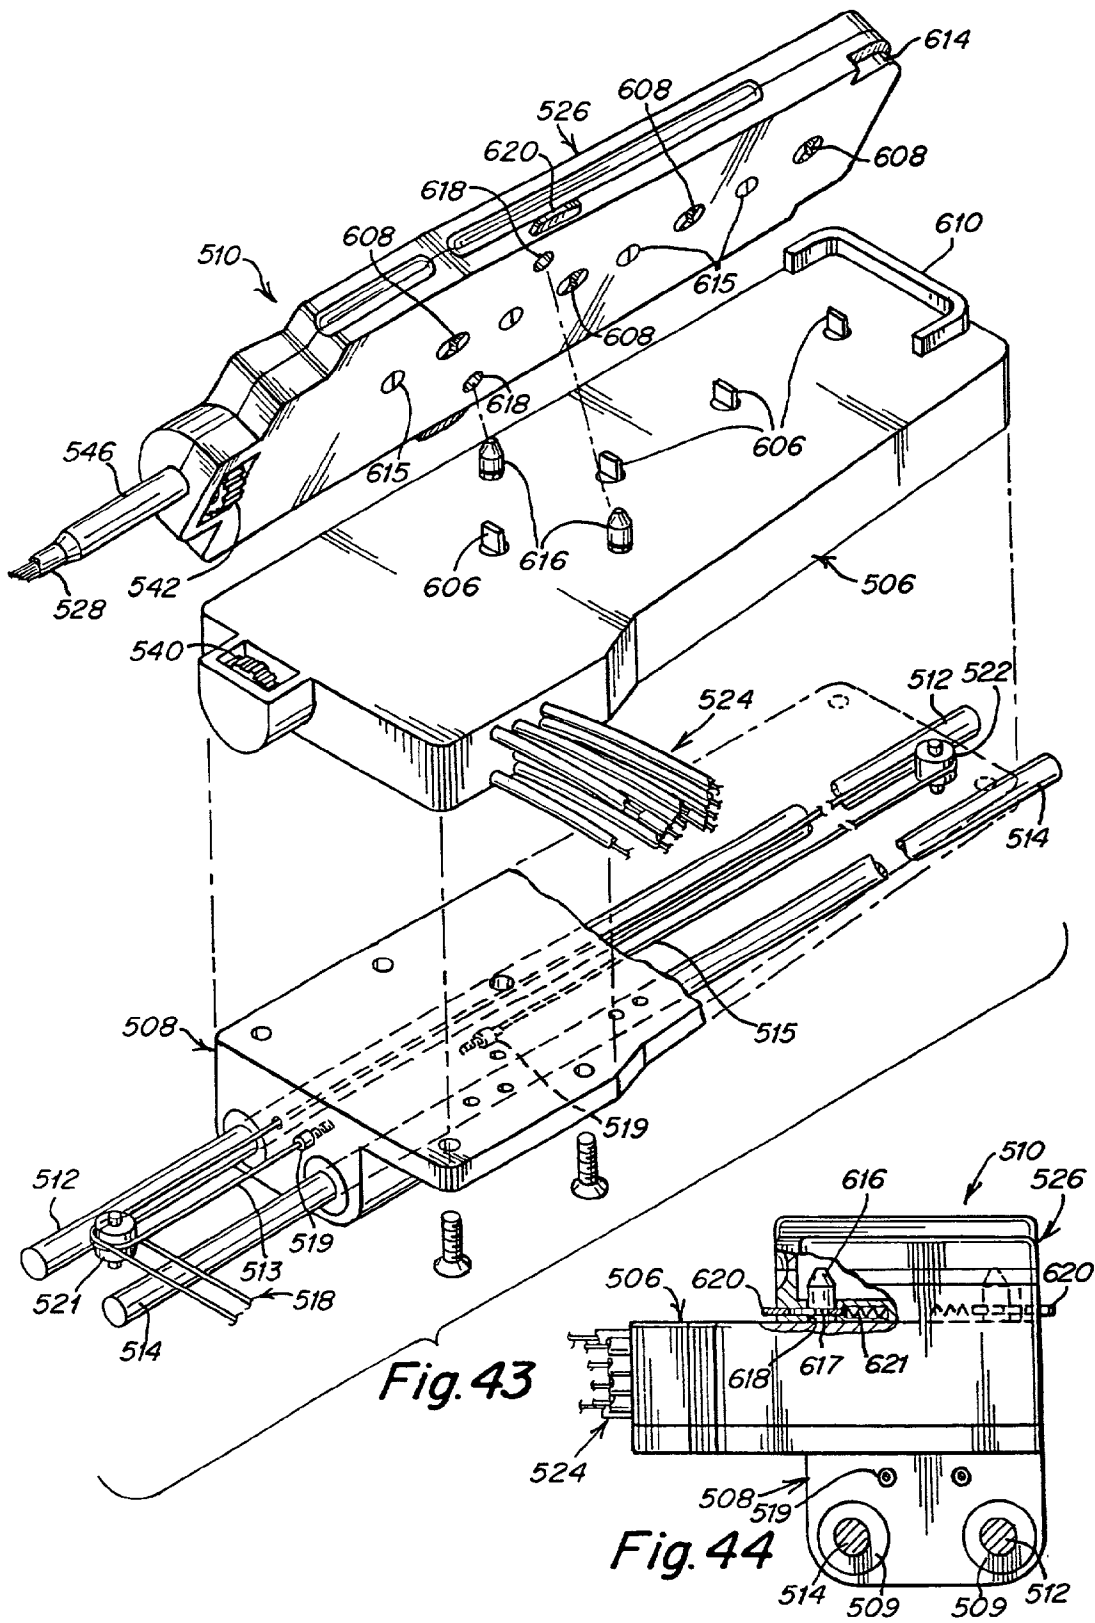
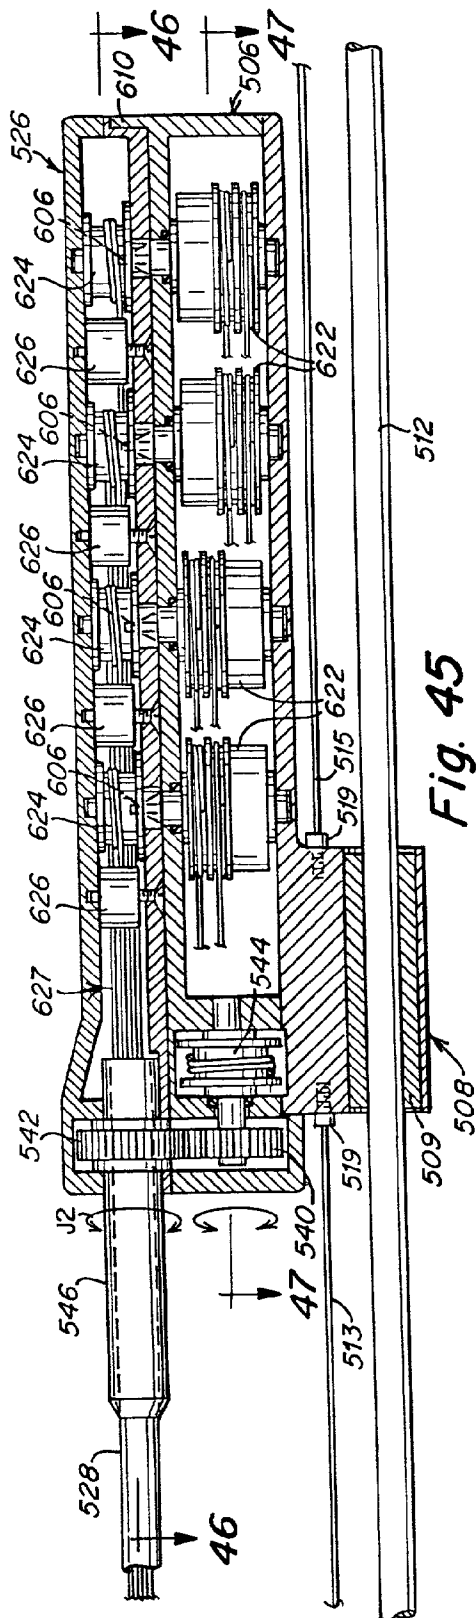
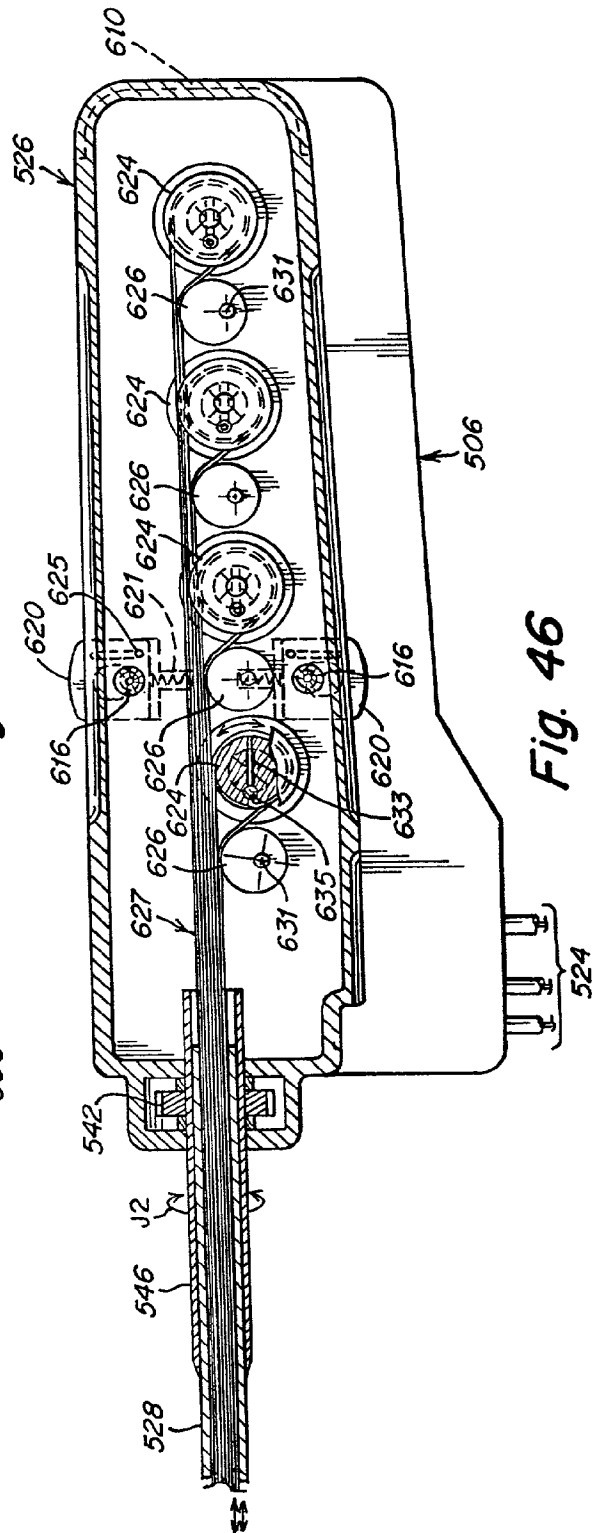


Fig. 41D







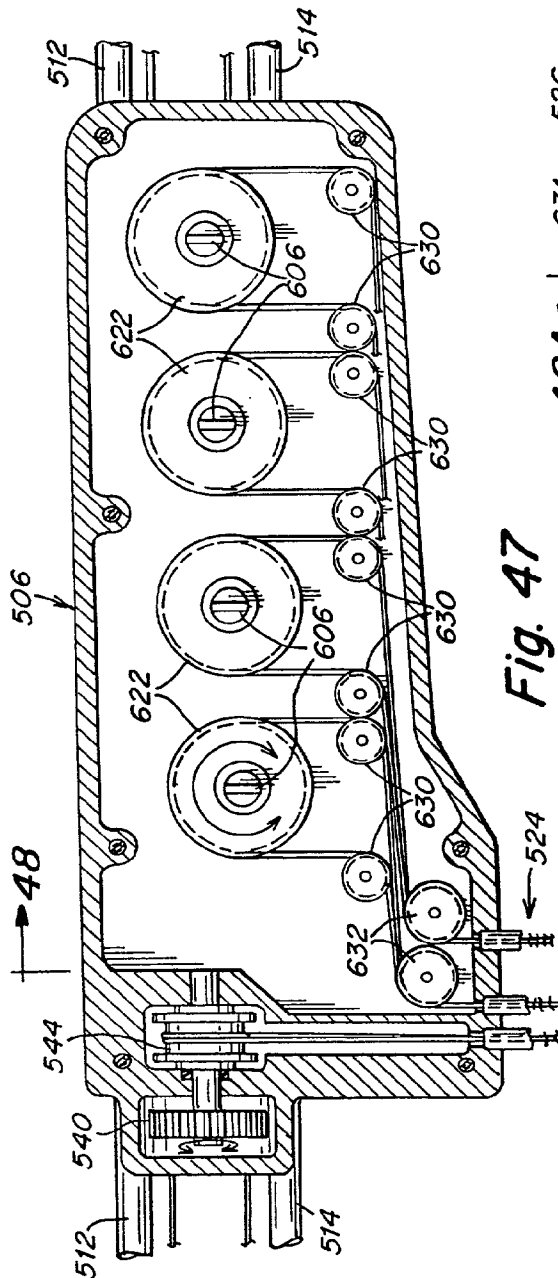


Fig. 47

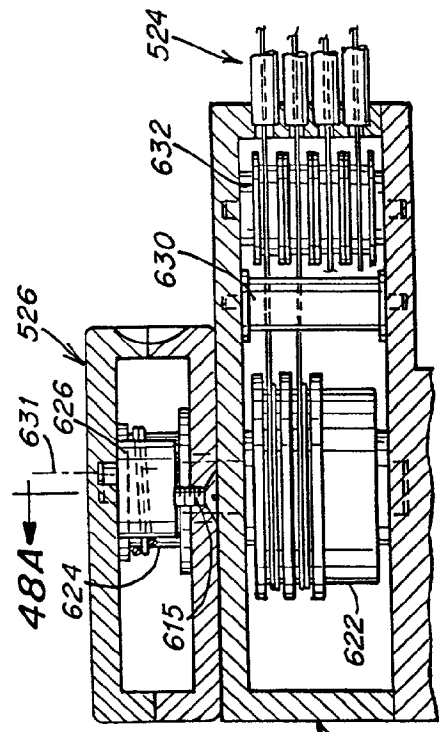


Fig. 48

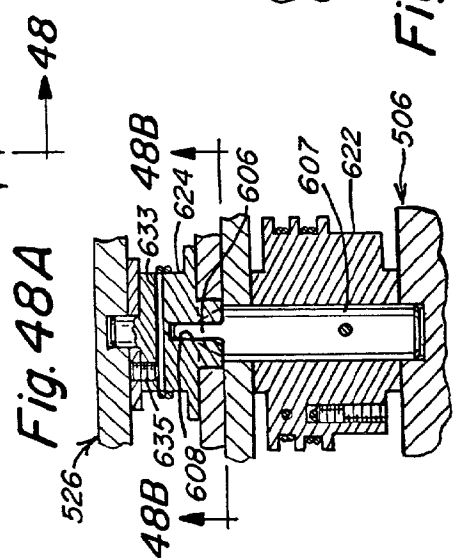


Fig. 48A




Fig. 48B

Fig. 49

FLEXIBLE INSTRUMENT

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part of and claims the benefit of priority from U.S. application Ser. No. 09/827,503, filed Apr. 6, 2001, which is a continuation of U.S. application Ser. No. 09/746,853, filed Dec. 21, 2000, which is a divisional of U.S. application Ser. No. 09/375,666, now U.S. Pat. No. 6,197,017, filed Aug. 17, 1999, which is a continuation of U.S. application Ser. No. 09/028,550 filed Feb. 24, 1998, now abandoned. This application is also a continuation-in-part of and claims the benefit of priority from U.S. application Ser. No. 09/783,637, filed Feb. 14, 2001, which is a continuation of PCT/US00/12553 filed May 9, 2000, which claims the benefit of priority of U.S. provisional patent application Serial No. 60/133,407, filed May 10, 1999, now abandoned. This application is also a continuation-in-part of and claims the benefit of priority from PCT/US01/11376 filed Apr. 6, 2001 which claims priority to U.S. application Ser. No. 09/746,853 filed Dec. 21, 2000 and Ser. No. 09/827,503 filed Apr. 6, 2001. This application is also a continuation-in-part of and claims the benefit of priority from U.S. application Ser. No. 09/746,853 filed Dec. 21, 2000 and Ser. No. 09/827,503 filed Apr. 6, 2001. This application is also a continuation-in-part of and claims the benefit of priority from U.S. application Ser. No. 09/827,643 filed Apr. 6, 2001 which claims priority to, inter alia, U.S. provisional application serial No. 60/257,869 filed Dec. 21, 2000 and U.S. provisional application serial No. 60/195,264 filed Apr. 7, 2000 and is also a continuation-in-part of PCT/US00/12553 filed May 9, 2000 from which U.S. application Ser. No. 09/783,637 filed Feb. 14, 2001 claims priority.

[0002] This application also claims the benefit of priority under 35 U.S.C. §§119 and 120 to U.S. Provisional Application Serial No. 60/293,346 filed May 24, 2001, U.S. Provisional Application Serial No. 60/279,087, filed Mar. 27, 2001, U.S. Provisional Application Serial No. 60/313,496 filed Aug. 21, 2001, U.S. Provisional Application Serial No. 60/313,497 filed Aug. 21, 2001, U.S. Provisional Application Serial No. 60/313,495 filed Aug. 21, 2001, U.S. Provisional Application Serial No. 60/269,203 filed Feb. 15, 2001, U.S. Provisional Application Serial No. 60/269,200 filed Feb. 15, 2001, U.S. Provisional Application Ser. No. 60/276,151 filed Mar. 15, 2001, U.S. Provisional Application Serial No. 60/276,217 filed Mar. 15, 2001, U.S. Provisional Application Serial No. 60/276,086 filed Mar. 15, 2001, U.S. Provisional Application Serial No. 60/276,152 filed Mar. 15, 2001, U.S. Provisional Application Serial No. 60/257,816 filed Dec. 21, 2000, U.S. Provisional Application Serial No. 60/257,868 filed Dec. 21, 2000, U.S. Provisional Application Serial No. 60/257,867 filed Dec. 21, 2000, U.S. Provisional Application Serial No. 60/257,869 filed Dec. 21, 2000.

[0003] The disclosures of all of the foregoing applications and U.S. Pat. No. 6,197,017 are all incorporated herein by reference in their entirety.

[0004] This application further incorporates by reference in its entirety the disclosures of the following U.S. Patent applications which are being filed concurrently on the same date herewith, having the following titles and docket num-

bers: 08491.7013—Surgical Instrument; 08491.7014—Surgical Instrument; 08491.7015—Surgical Instrument; 08491.7016—Surgical Instrument; 08491.7017—Surgical Instrument; 08491.7018—Surgical Instrument; 08491.7019—Surgical Instrument; 08491.0006—Flexible Instrument; 08491.0006—Flexible Instrument; 08491.0007—Flexible Instrument; 08491.0008—Flexible Instrument; 08491.0009—Flexible Instrument; 08491.0010—Flexible Instrument; and 08491.0011—Flexible Instrument.

FIELD OF THE INVENTION

[0005] The present invention relates in general to a remote controlled flexible instrument comprising a flexible shaft, for introduction into a body cavity or body vessel to perform a medical procedure.

BACKGROUND OF THE INVENTION

[0006] Catheters are used extensively in the medical field in various types of procedures, including invasive procedures. Minimally invasive surgery involves operating through small incisions, through which instruments are inserted. These incisions are typically 5 mm to 10 mm in length. Minimally invasive surgery is typically less traumatic than conventional surgery, due, in part, to the significant reduction in incision size. Furthermore, hospitalization is reduced and recovery periods shortened as compared with conventional surgery techniques. Catheters may be tailored to a particular size or form, depending on the incision and the size of the body cavity or lumen.

[0007] Due to the small size of the incision, the bulk of the surgery is not visible. Although the surgeon can have visual feedback from the surgical site via a video camera or endoscope inserted into the patient, or via radiological imaging or ultrasonic scanning, the ability to control the relatively simple laparoscopic instruments remains difficult. Even with good visual feedback, the surgeon's tactile and positional senses are physically removed from the operative site, rendering endoscopic procedures slow and clumsy.

[0008] Current instrumentation, with forceps, scissors, etc., inserted into the body at the end of long slender push rods is not fully satisfactory. The use of such conventional instrumentation increases operative time, and potentially heightens risk. For example, tissue may be injured when the laparoscopic tool moves outside the visual field. Moreover, there are limitations on the type and complexity of procedures that may be performed laparoscopically due, in part, to the limitations on the instruments that are used.

[0009] Development work has been undertaken to investigate the use of robotic work in surgery. Typically, these robotic systems use arms that reach over the surgical table and manipulate surgical instruments. The known robotic systems are large, clumsy to operate and relatively expensive to manufacture. The presence of a robot at the surgical site is problematic particularly when the robot is large and may impede access to the patient during surgery.

SUMMARY OF THE INVENTION

[0010] The present invention features, at least in part, an improved, remote controlled surgical system that does not impede access to the patient during surgery, yet is simple to

operate. The present invention provides a surgical instrument system particularly adapted for a variety of medical procedures, including minimally invasive surgery.

[0011] One aspect of the present invention provides a surgical instrument comprising a shaft having at least one controllably flexible segment and a tool mounted at a distal end of the shaft. The tool is insertable into a subject. The instrument further comprises a shaft mount drivably coupled to the shaft at a proximal end of the shaft where the shaft mount is then drivably coupled to the tool through the shaft. The instrument also comprises a drive unit drivably coupled to the shaft mount. The drive unit is operable from a location remote from the subject to control flexure of the flexible segment so as to control disposition of the tool at an operative site.

[0012] Another aspect of the present invention provides a remotely controllable surgical instrument comprising a user input device for inputting a command. A slave station receives the command from the input device. The user input device is remotely disposed from the slave station. The slave station further comprises a mechanically drivable mechanism comprising a shaft having a proximal end, a distal end supporting a tool and a flexible portion between the proximal and distal ends. An electronic signal link is between the user input device and the slave station receives a the command from the input device being communicated via the link, for controlling bending of the flexible portion so as to controllably position the tool at an operative site of a subject.

[0013] Another aspect of the present invention provides a remotely controllable catheter comprising a tube having a proximal end and a distal end. At least a segment of the tube is controllably flexible. The catheter also comprises a drivable bending mechanism mechanically coupled to and interactive with a controllably flexible segment of the tube. A computer remote from and interconnected to the bending mechanism has a computer for receiving input from the user. The program directs the bending mechanism to controllably flex the flexible segment of the tool according to the user input.

[0014] Another aspect of the present invention provides a catheter comprising a shaft having proximal and distal ends and at least one flexible segment along a length of the shaft. The distal end is insertable within a body cavity or a vessel. A tool is supported at the distal end of the shaft for performing a medical procedure. At least two cables extend along the shaft between the proximal and distal ends. At least one of the cables is associated with the flexible segment to the shaft and at least another of the cables is associated with a tool. An electronic control mechanism is drivably coupled to the cables where the electronic control mechanism is capable of communicating drive signals from a user input device to the cable to affect bending of the flexible segment and operation of the tool.

[0015] One aspect of the present invention provides a medical device comprising disposable mechanically drivable mechanism drivably coupled to a tool via a disposable shaft for insertion into a body vessel or cavity along a selected length of the shaft. The tool is operable to carry out a medical procedure and the shaft is disposable together with the mechanically drivable mechanism. A receiver receives a mechanically drivable mechanism. The medical device further comprises a drive unit coupled to the receiver.

[0016] Another aspect of the present invention provides a medical device comprising a disposable implement comprising a disposable flexible shaft supporting a tool at its distal end for insertion into a subject, and a disposable first drive interface drivably coupled with a tool to the shaft. The medical device further comprises a second drive interface, for drivably coupling the disposable implement with a drive unit. The second drive interface is drivably engageable with a disposable implement via the first drive interface.

[0017] Another aspect of the present invention provides a disposable medical device comprising a disposable flexible shaft having a proximal end and a distal end. A disposable mechanically drivable interface is connected to the proximal end of the shaft. A tool is mounted at the distal end of the shaft. The device further comprises at least one disposable cable drivably interconnected between the mechanically drivable interface in the tool. The mechanically drivable interface is interconnected to a remotely disposed electronic control mechanism which controls drive operation of the device.

[0018] Another aspect of the present invention provides a disposable electronically controlled surgical instrument comprising a disposable flexible elongated shaft having a proximal end and a distal end on which is mounted a tool. The proximal end of the shaft is connected to a mechanically drivable interface. The disposable shaft includes at least one disposable cable drivably interconnected between the mechanically drivable interface and the tool. The mechanically drivable interface is interconnected to a remotely disposed electronic control mechanism which controls drive operation of the device.

[0019] One aspect of the present invention provides a medical device comprising a flexible guide shaft having a distal end disposed at a predetermined location in the subject. The device comprises a flexible inner shaft having a proximal end and a distal end supporting at its distal end a tool. The inner shaft is insertable into the guide shaft so as to dispose a tool at an operative site. The device further comprises a drive unit coupled to the inner shaft for providing controlled actuation of the tool. The drive unit is remote controllably drivable by a user via a manually controllable device.

[0020] Another aspect of the present invention provides a medical device comprising a flexible inner shaft inserted within a flexible guide shaft. A tool is disposed at a distal end of the inner shaft for insertion into a subject. A drive unit is coupled with an inner shaft and a guide shaft independently. The drive unit is capable of independently effecting movement of each shaft to at least one degree of freedom. A user input interface is remote from the drive unit, where the input interface is for remote controllably manipulating the inner and guide shaft.

[0021] Another aspect of the present invention provides a medical device comprising a flexible guide shaft having a distal end disposed at a predetermined location in a subject. A flexible disposable inner shaft has a proximal end and a distal end supporting at its distal end a tool. The inner shaft is insertable to the guide shaft so as to dispose the tool at an operative site. The drive unit is coupled with the inner shaft for providing controlled actuation of the tool and controlled deformation of one or more flexible portions of the inner shaft. The drive unit is remote controllably drivable by the

user via a manually controllable device. The proximal end of the inner shaft includes a mechanically operative element drivably couplable to the drive unit. The mechanically operative element is disposable together with the tool as a unit.

[0022] One aspect of the present invention provides a medical device comprising a mechanically drivable mechanism coupled with a shaft including a flexible segment, where a distal end of the shaft supports a tool insertion into a subject. A drive unit is coupled with a mechanically drivable mechanism and disposed remotely from the sterile field. The drive unit is for intercoupling drive from the drive unit to the drivable mechanism. The drive unit is capable of activating the flexible segment via the mechanically drivable mechanism for actuation of the tool and positioning of the tool at the operative site within the subject.

[0023] Another aspect of the present invention provides an apparatus for use in a body cavity or vessel comprising a catheter having a proximal end and a distal end for placement in the body cavity or vessel. A tool is positioned at the distal end of the catheter. A flexible segment is positioned between the distal and proximal ends of the catheter. Cables extend from a drive unit through the flexible segment. The drive unit is operable from a remote site and capable of bending the flexible segment via the cables for actuation of the tool.

[0024] Another aspect of the present invention provides a remotely driven surgical instrument comprising an elongate flexible shaft having a proximal end and a distal end supporting a surgical tool. The shaft is insertable into a subject for disposition of the tool at an operative site of the subject. An electronically controllable drive unit is mounted in a location remote from the subject. The remote drive unit includes one or more motors drivably interconnected to the proximal end of a flexible shaft by one or more motor driven cables, which are readily drivably interconnectable to and disconnectable from the proximal end of the flexible shaft.

[0025] One aspect of the present invention provides a robotic medical system comprising a flexible instrument having flexible and distal ends with at least one flexible segment extending through a lumen of the human body. The at least one flexible segment is controllably bendable so as to locate a distal end of the shaft at an internal target site. A tool is carried at the distal end of the shaft for performing a procedure. A master station includes an input device. A slave station includes a receiver for the catheter for controlling through the receiver at least one degree of freedom of the catheter. A controller is coupled between the master station and the slave station and is operated in accordance with computer algorithm that receives a command from the input device and for controlling the at least one degree of freedom of the catheter so as to respond in accordance with action at the input device.

[0026] Another aspect of the present invention provides a method of remotely controlling a catheter comprising providing a flexible shaft having a distal end supporting a tool. The shaft includes at least one controlled flexible segment about the distal end capable of controlled bending for positioning the tool at an operative site. The method comprises inserting the shaft into an anatomic lumen where the flexible shaft is adapted to conform to the configuration of the anatomic lumen. The method comprises mechanically

driving, via a drive unit, a cabling system extending through the shaft and the at least one flexible segment. The at least one controlled flexible segment is activated by operating the drive unit from a location remote from the shaft so as to affect bending of the at least one flexible segment and thereby effect positioning of the tool to a target site.

[0027] Another aspect of the present invention provides a flexible instrument system comprising a flexible shaft having a proximal end and a distal end. The distal end supports a tool. The shaft is insertable into a subject so as to dispose the tool at an operative site. A mechanically drivable mechanism is disposed at the proximal end of the shaft. The mechanically drivable mechanism is capable of offering the tool via at least one flexible segment positioned along the shaft. A receiver is supported in a fixed portion of the subject for receiving and storing the shaft via the mechanically drivable mechanism in a position to maintain the tool at the operative site. A computation system receives electrical control signals from a user input device for controlling the shaft.

[0028] Another aspect of the present invention provides a flexible instrument system comprising a medical implement having sufficient flexibility along a length thereof so as to at least flex and conform to a pathway in an anatomic vessel or cavity as the implement is inserted therein. The medical implement comprises a tool for performing a medical procedure and a flexible shaft having proximal and distal ends. The shaft supports the tool at the distal end and is insertable into a subject so as to dispose the tool at an operative site via controlled bending of at least one flexible segment positioned along the shaft. The medical implement also comprises a mechanically drivable mechanism disposed at the proximal end of the shaft. The system comprises a drive unit intercoupled with a medical implement and includes at least a first cable intercoupled with a tool and at least a second cable intercoupled with a shaft for controlling a bend at the at least one flexible segment.

[0029] Another aspect of the present invention provides a flexible instrument system comprising a drive unit for controlling operation of a medical implement. A mechanical actuation system extends from the drive unit. The medical implement has sufficient flexibility to conform to a pathway in an anatomic vessel or cavity as the implement is inserted therein. The medical implement comprises a flexible shaft having proximal and distal ends where the flexible shaft is insertable into a subject so as to dispose the distal end at an operative site. The shaft further comprises at least one controlled flexible segment actuating a controlled bend. The medical implement also comprises a mechanically drivable mechanism disposed at a proximal end of the flexible shaft.

[0030] One aspect of the present invention provides a system for preparing a cardiac valve comprising a flexible guide shaft extending from a site outside a patient to an area about the cardiac valve. A flexible inner shaft supports at its distal end a remotely controlled tool for performing a cardiac repair procedure. The inner shaft is received in the guide shaft for disposing the tool at the area about the cardiac valve. A retainer is positioned at the area of the cardiac valve. The retainer is attached to an annulus of the cardiac valve and is closable via the tool to draw the annulus into a smaller diameter.

[0031] Another aspect of the present invention provides the method of repairing a mitral valve of the heart. The

method comprises extending a guide shaft from a site outside the patient to a site adjacent the mitral valve. The method comprises inserting a fiber through the guide shaft and securing the fiber about an annulus of the mitral valve while the heart is beating. The securing step includes introducing through the guide shaft a flexible inner shaft having a remotely controlled distal tool for securing the fiber about the annulus leaving opposite ends of the fiber exposed. The method for this comprises applying a force to the fiber ends so as to draw the annulus into a tighter diameter.

[0032] Another aspect of the present invention provides a system for remotely repairing a cardiac valve comprising a guide catheter extending through an area of the human body where a distal end of the guide catheter is disposed at an area about the cardiac valve. A fiber extends about a diameter of an annulus of the cardiac valve. The fiber is engaged with a diameter of the annulus and capable of drying the annulus to a smaller diameter. The system comprises a flexible working catheter received by the guide catheter, where the working catheter includes a tool engageable with a fiber. A remote manipulator is controlled from a site remote from the body, for controlling the tool.

[0033] Another aspect of the present invention provides a method of repairing a mitral valve of the heart, comprising extending a guide shaft from a site outside the patient to a site about the mitral valve. The method comprises providing a ring of a first diameter where the ring is deformable and capable of matching a desired predetermined diameter of an annulus of the mitral valve. The ring is engaged with a guide shaft via a flexible inner shaft received by the guide shaft. The ring is secured about the mitral valve annulus while the heart is beating. The securing step includes engaging the ring about a circumference of the annulus via a remotely controlled tool supported at a distal end of the inner shaft. The annulus is drawn into the predetermined diameter.

[0034] Another aspect of the present invention provides a method of repairing a cardiac valve comprising providing a balloon supported on a catheter. A plurality of peripherally disposed anchor pins is supported from an outer surface of the lumen where the anchor pins are tethered to each other. The balloon is passed in a deflated state to an area about the cardiac valve. The method comprises inflating the balloon to thrust the anchor pins into an annulus of the cardiac valve. The tether is tightened to pull the peripherally disposed pins into a smaller diameter.

[0035] Another aspect of the present invention provides a method for repairing a cardiac valve comprising providing a balloon and supporting and passing the balloon in a deflated state to an area about the cardiac valve. A plurality of peripherally disposed anchor pins is disposed and arranged about an outer surface of the balloon. A tether is provided for intercoupling the anchor pins. The balloon is inflated once it is positioned at the area about the cardiac valve, to thrust the anchor pins into a ring defining a base of the cardiac valve. A tether is tightened to pull the peripherally disposed pins into a smaller diameter.

[0036] Another aspect of the present invention provides a system for remotely repairing a cardiac valve comprising a flexible guide shaft extending to an area of the human body so as to locate a distal end thereof at an area about the cardiac valve. A delivery member, for supporting an array of securing pieces at a distal end thereof, extends through the

flexible guide member. The array of securing pieces is intercoupled by a cable. A remote manipulator is controlled from a slight remote from the body, for controlling the delivery member to expel the securing pieces in sequence about the cardiac valve annulus as the valve is functioning. The remote manipulator is capable of controlling a tightening of the cable to draw the annulus into a smaller diameter.

[0037] Another aspect of the present invention provides a flexible instrument system for repairing an anatomic body part comprising a shaft having sufficient flexibility along the length thereof so as to readily flex and conform to a pathway in the anatomy as the shaft is inserted therein. A drivable mechanism is disposed at a flexible end of the shaft controlling a tool supported at a distal end of the shaft. The shaft is insertable into a subject so as to dispose the distal end of the shaft at an internal site of an anatomical body part. A retainer is attached to an annulus at the anatomic body part where the retainer is closable so as to draw the annulus into a smaller diameter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0038] Numerous other objects, features and advantages of the invention should now become apparent upon a reading of the following detailed description taken in conjunction with the accompanying drawings in which:

[0039] FIG. 1 is a simplified block diagram illustrating basic components of a system constructed in accordance with the present invention;

[0040] FIG. 2 illustrates further details of input devices at the master unit;

[0041] FIG. 3 is a schematic diagram illustrating one embodiment of the present invention in which the flexible instrument system includes multiple separate nested catheters;

[0042] FIGS. 3A-3C illustrate different forms of catheter control in accordance with aspects of the present invention;

[0043] FIG. 4 is an illustrative diagram showing the use of the catheter of the present invention in connection with mitral valve repair;

[0044] FIG. 5 is schematic diagram of the catheter system of the present invention as deployed through the urethra for a surgical procedure in the bladder;

[0045] FIG. 6 is a perspective view of one embodiment of a system embodying the catheter apparatus of the present invention;

[0046] FIG. 7 is a more detailed perspective view of the catheter apparatus;

[0047] FIG. 8 is an enlarged view of a portion of the catheter apparatus particularly at the distal end section thereof;

[0048] FIG. 9 is a cross-sectional view through the catheter apparatus as taken along line 9-9 of FIG. 7;

[0049] FIG. 10 is a cross-sectional view through the catheter apparatus as the distal end section thereof, as taken along line 10-10 of FIG. 7;

[0050] FIG. 11 is a cross-sectional view similar to that illustrated in FIG. 9 for an alternate embodiment of the invention depicting dual-direction flexing;

- [0051] FIG. 12 is one design of tool construction in accordance with the present invention employing inner and outer catheters and inner and outer cables;
- [0052] FIG. 13 is a schematic diagram of the tool or mini-tool showing certain parameters relating to position control;
- [0053] FIG. 14 is a block diagram of the controller used with the telerobotic system of this invention;
- [0054] FIG. 15 is a block diagram of further details of the controller particularly details of the module board;
- [0055] FIG. 16 is a block diagram of the control algorithm in accordance with the present invention;
- [0056] FIG. 17 is a schematic diagram illustrating one mechanism for providing mitral valve repair employing a ring mechanism;
- [0057] FIG. 18 illustrates schematically the concept of the present invention in connection with mitral valve repair;
- [0058] FIG. 19 is a diagram of a heart muscle illustrating the position of the mitral valve;
- [0059] FIG. 20 illustrates further detail of the mitral valve construction as well as the catheter and tool used in the procedure;
- [0060] FIG. 21 is a more detailed cross-sectional drawing of the portion of the mechanical member, particularly the means for tightening the retaining means;
- [0061] FIG. 22 shows further details of the structure of FIG. 21;
- [0062] FIG. 23 is a schematic illustration of a section of the mitral valve ring showing the fiber and the securing of one end of the fiber;
- [0063] FIG. 24 illustrates somewhat further detail of a means for retaining the catheter in position;
- [0064] FIG. 25 is a diagram illustrating alternate means for holding the catheter in place;
- [0065] FIG. 26 illustrates a view of a mitral valve;
- [0066] FIG. 27 is a schematic diagram of the mitral valve indicating the ring area and leaflets;
- [0067] FIG. 28 is a schematic illustration showing the mitral valve construction and a mechanical member for retaining and tightening;
- [0068] FIG. 29 is schematic diagram of another technique for mitral valve repair employing a wire to be tightened like a lasso;
- [0069] FIG. 30 is a schematic diagram illustrating a catheter and tool construction containing a tether cable and anchor elements within the inner catheter;
- [0070] FIG. 30A shows a cable termination tool for crimping;
- [0071] FIG. 30B shows a tool for cutting;
- [0072] FIG. 31 illustrates a staple array of the present invention;
- [0073] FIG. 32 illustrates the mitral valve construction as well as the staple apparatus and technique of the present invention;
- [0074] FIG. 33 is an illustration of the staple array when applied and secured to the valve annulus;
- [0075] FIG. 34 is a schematic illustration of an alternate embodiment for the staple array;
- [0076] FIGS. 35A and 35B illustrate another version of the invention wherein the guide catheter is robotic;
- [0077] FIG. 36 schematically represents a system of the present invention for repairing a mitral valve;
- [0078] FIG. 36A shows a pin for anchoring;
- [0079] FIG. 37 illustrates the anchoring system engaged with the mitral valve;
- [0080] FIG. 38 illustrates another version in accordance with the invention employing a balloon with the balloon in a deflated state;
- [0081] FIG. 39 schematically represents portions of the heart muscle and the positioning of the balloon relative to the mitral valve;
- [0082] FIG. 40 illustrates the balloon in its inflated state positioned at the mitral valve;
- [0083] FIGS. 41A-41D depict still another form of catheter in accordance with the present invention;
- [0084] FIG. 42 is a perspective view of another embodiment of the present invention;
- [0085] FIG. 42A is an enlarged detail perspective view of the tool;
- [0086] FIG. 43 is an exploded perspective view of, in particular, the interlocking modules of the flexible instrument system of FIG. 42;
- [0087] FIG. 44 is a partially broken away rear elevational view of the interlocking modules as seen along line 44-44 of FIG. 42;
- [0088] FIG. 45 is a cross-sectional side view through the interconnecting modules and as taken along line 45-45 of FIG. 42;
- [0089] FIG. 46 is a cross-sectional plan view through the instrument module taken along line 46-46 of FIG. 45;
- [0090] FIG. 47 is a cross-sectional plan view taken through the base module of the system of FIG. 42, and as taken along line 47-47 of FIG. 45;
- [0091] FIG. 48 is a cross-sectional end view taken along line 48-48 of FIG. 47;
- [0092] FIG. 48A is a cross-sectional view taken along line 48A-48A of FIG. 48;
- [0093] FIG. 48B is a fragmentary plan view of a drive wheel engagement slot by itself as taken along line 48B-48B of FIG. 48A; and
- [0094] FIG. 49 is a schematic perspective view showing mechanical cabling between the drive unit and the flexible instrument system.

DETAILED DESCRIPTION

[0095] The present invention provides a system for remotely controlling a flexible instrument for use in medical applications, typically for operative or other medical procedures. The flexible instrument comprises a shaft or a tube of sufficient dimensions for passing through a small incision or natural body lumen or cavity and ultimately, for positioning a distal end of the shaft within the body at an internal target (operative) site. The flexible instrument can also support a tool at its distal end to allow more intricate medical procedures. A user or surgeon can control the position of the shaft from a master station, allowing operation from another part of the operating room, or even from another room or another building. In one aspect of the invention, the shaft can comprise one or more flexible segments, which a user can controllably bend, providing finer control in directing the shaft toward the target site. The control can result in, for example, a deflection or turning of the shaft, for guiding this shaft through or within various body cavities or lumens. The controllable bending is also useful for more precise positioning of a distal end of the flexible instrument at a desired operative site.

[0096] Preferably, the flexible instrument is used to perform minimally invasive procedures. "Minimally invasive procedure," refers herein to a surgical procedure in which a surgeon operates through small cut or incision, the small incision being sufficiently necessary to access the operative site. In one embodiment, the incision length ranges from 1 mm to 20 mm in diameter, preferably from 5 mm to 10 mm in diameter. This procedure contrasts those procedures requiring a large cut to access the operative site. Thus, the flexible instrument is preferably used for insertion through such small incisions and/or through a natural body lumen or cavity, if necessary, so as to locate the catheter at an internal target site for a particular surgical or medical procedure. Examples of such minimally invasive procedures include intravascular procedures, such as the repair of a cardiac valve. The introduction of the flexible instrument into the anatomy may be by percutaneous or surgical access to a lumen or vessel, or by introduction through a natural orifice in the anatomy.

[0097] FIG. 1 is a block diagram schematically illustrating the three main components of the remote control system of the present invention. A surgeon or user can input control actuations at master station 1, typically through an input device (not shown). Slave station 3 is separate and remote from the master station and controls the motion of the flexible instrument, in accordance with the user input from master station 1. Master station 1 and slave station 3 may be in relatively close proximity to each other, such as in the same operating room, or can be displaced from each other by miles. Controller 2 provides a telecommunications or electronic communications link coupled between the master station and the slave station. Controller 2 typically includes a computer. Controller 2 receives a command from the input device of master station 1 and relays this command to slave station 3.

[0098] FIG. 6 is a schematic of the remote control system of the present invention. The system includes: (1) A master station comprising a user interface or surgeon's interface 11; (2) A slave station comprising a flexible instrument including shaft 30 which supports tool 18. Shaft 30 is connected

to and is controllable from mechanically drivable mechanism 26, which in turn is engageably received by receiver 24, both of which are mechanically driven by drive unit 13, (alternatively mechanical drive 13); and (3) a controller or computation system 12 to translate a user's commands from user interface 11 to drive unit 13, which then drives the articulations of shaft 30 and tool 18. FIG. 6 illustrates a system where a user or surgeon can control shaft 30 and tool 18 by manipulating interface handles 30A of user interface 11. The movement of handle 30A causes responsive movement of tool 18 through the coordinating action of computation system 12. For example, tool 18 can be a pair of graspers, scissors, staplers, etc. and manipulation of handle 30A can cause the jaws of tool 18 to open and close.

[0099] Surgeon's interface 11 is in electrical communication with computing system 12, which is, in turn, in electrical communication with drive unit 13. In one embodiment, drive unit 13 comprises a plurality of motors. The drive unit 13 is in mechanical communication with shaft 30 via conduit 23, which houses a plurality of mechanical cables driven by the plurality of motors in drive unit 13. In one embodiment, drive unit 13 is solely in mechanical communication with shaft 30. Because of the mechanical communication with shaft 30, the electromechanical components in drive unit 13 are disposed in an area remote from the operative site, and preferably in an area outside the sterile field. Preferably, objects that are difficult to sterilize, e.g. motors or electromechanical components, are kept at a sufficient distance from the patient to avoid contamination. This distance is readily ascertainable by doctors, nurses, and other appropriate medical professionals. In one embodiment, the sterile field has the rest surface of the operating table as its lower boundary. Thus, drive unit 13 is preferably located below the plane of the sterile field, i.e. below the rest surface of the operating table. The patient or subject may be further protected from drive unit 13 with a sterile barrier, such as a sterile cloth. With respect to the drive unit, such as drive unit 13 in FIG. 6, reference is made to co-pending provisional application No. 60/279,087, which is incorporated by reference herein. In accordance with the system of FIG. 6, all of the drive motors in drive unit 13 are disposed away from the sterile field and thus the need for a sterile barrier is eliminated. Furthermore, since all of the motors and electronics are within a single, self-contained unit, design, testing and manufacturing of the system is greatly simplified.

[0100] Accordingly, one aspect of the present invention provides a drive unit capable of remotely driving articulation of a flexible instrument, where the drive unit is remote from the subject and the flexible instrument. The slave station of the present invention employs, to a large part, a mechanical arrangement that is effected remotely and includes mechanical cables and flexible conduits coupling to a remote motor drive unit. This provides the advantage that the instrument is purely mechanical and does not need to be contained within a sterile barrier. The instrument may be autoclaved, gas sterilized or disposed in total or in part.

[0101] In FIG. 6, drive unit 13 mechanically drives the flexible instrument (comprising shaft 30 and tool 18) through conduit 23, receiver 24 and mechanically drivable mechanism 26 (alternatively known as mechanically drivable interface or shaft mount). Conduit 23 houses a plurality of separate mechanical cables to mechanically connect drive

unit 13 with receiver 24. The mechanical cables physically contact and drive the motions of shaft 30 and tool 18. Conduit 23 is engageable and disengageable with drive unit 13, i.e. attachable and detachable (see discussion of FIG. 49, below). Although two conduits 23 are depicted here, it is understood that more or fewer conduits may be used, depending on the particular application. In one embodiment, drive unit 13 comprises a plurality of motors, which drive the mechanical cables extending through conduit 23 and terminating at receiver 24. Receiver 24 interlockably receives mechanically drivable interface 26, which engages a separate set of cables extending through shaft 30 and at least one cable line operating tool 18. Thus, engaging drivable interface 26 with receiver 24 provides a mechanical (physical) connection from drive unit 13 to control certain motions of shaft 30 and tool 18. Receiver 24, which is supported by a carriage, is capable of moving along a linear path represented by the arrow 22 via rails 25.

[0102] Cables in conduit 23 also mechanically drives the translation of receiver 24 along rails 25. The rails, and thus the linear translation extend at an acute angle with respect to the operating table, as well as the subject. This angular arrangement disposes the flexible instrument system in a convenient position over the patient. This arrangement also minimizes the number of components that operate within the sterile field, as drive unit 13 is maintained at a location remote from the sterile field.

[0103] FIG. 49 shows a schematic perspective view of the cabling pathway for mechanically coupling one of an array of motors of a drive unit with a tool supported on a distal end of a shaft. In general, the cabling pathway comprising a plurality of mechanical cables extends from the drive unit to the receiver. Another separate set of mechanical cables connects the mechanically drivable mechanism, situated at a proximal end of the shaft, to the tool and any controlled flexible segments positioned along the shaft. Interlocking the receiver with the mechanically drivable mechanism results in connecting the two separate sets of mechanical cables, thereby extending the cabling pathway from the drive unit to the distal end of the shaft. Thus, each of the mechanically drivable mechanism and the receiver can be considered as a coupler, which interlocks or couples with each other.

[0104] More specifically, FIG. 49 shows drive motor 675 positioned within a drive unit, such as drive unit 13 of FIG. 6. The first cabling pathway comprises a set of cabling, which engages with and extends from drive motor 675 through idler pulley 682. The cables continue through idler pulleys 630 and 632 to drive wheel 622, which resides in receiver 506 (equivalent to receiver 24 of FIG. 6). A second separate set of cables extends about the drive wheel 624, guided by cam 626 and continues through flexible instrument shaft 528. Tool 534 links to shaft 528 via joint 601, which provides a wrist pivot about axis 532 in the direction of arrows J4. The two separate sets of cables are interlocked by interlocking drive wheel 622 of receiver 506 with drive wheel 624 of mechanically drivable mechanism 526 (equivalent to drivable mechanism 26 of FIG. 6). Specifically, the interlocking involves slotting a blade 606 into a corresponding slot within wheel 624 (see further discussion of FIG. 43 below).

[0105] In one embodiment, the interlocking mechanism can comprise a magnetic attachment, where a first series of

magnets in the mechanically drivable mechanism interacts with a second series of magnets in the receiver. Each series of magnets can couple with the mechanical cables.

[0106] FIG. 49 also shows the output of motor 675 at a coupler pulley 677, which is adapted to rotate with an output shaft of the motor. The rotational arrow 680 indicates this rotation.

[0107] For the sake of simplicity, FIG. 49 only illustrates one cabling pathway. It can be appreciated that several other cabling pathways can be constructed and arranged to control other motions of the shaft and tool through other motors of the drive unit.

[0108] Regarding the interface 11, computer system 12 and drive unit 13, reference is also made to co-pending application PCT Serial No. PCT/US00/12553 filed May 9, 2000, and U.S. Provisional Application Serial No. 60/279,087 filed Mar. 27, 2001, both of which are incorporated by reference herein in their entirety.

[0109] A more detailed discussion of the master station, the slave station and computation system or controller 12 is provided below.

[0110] Master Station

[0111] FIG. 2 schematically depicts the components of master station 1. Master station 1 can include any one or a combination of input devices A-E and a display F. Input device A is a point-and-touch device. Input device B is a computer mouse. Input device C is a pointing device that may employ a pen or stylus. Input device D is a joystick. Input device E is a hand interface, that provides finer control of the shaft, or a tool positioned at the distal end of the shaft.

[0112] In one embodiment, input device E features handles that control the motion of the shaft and a tool. Referring back to FIG. 6, the master station features input device 11 comprising handles 30A. Handles 30A are held by the surgeon, who can then torque, translate or rotate catheter member 30 and tool 18 by performing the corresponding motions on handles 30A. A rotation of a handle 30A via rotation of the surgeon's hand can control rotation of, for example, the outer shaft 32 about the co-axis. Flexing or bending of flexible section 42 can be controlled by the surgeon flexing his hand at the wrist and activating flex cable 52, as shown in FIG. 8 (see discussion of FIG. 8, below). A surgeon can manipulate tool 18 by, for example, closing and opening the jaws of handles 30A to simulate opening and closing of jaws of tool 18.

[0113] Reference may also be made to copending application docket number 08491-7018, filed of even date herewith, which discloses other details of a master station input device (master positioner) that may be used in carrying out the control described herein.

[0114] Display F provides a direct video image of the site surrounding the distal end of the shaft. An endoscope supporting a camera is inserted into the body of a subject, providing the video feed of the operative site. The camera can be mounted on or housed at the distal end of the shaft. The camera can provide a view of the operative site, or may be positioned away from the site to provide additional perspective on the surgical operation.

[0115] Other detection systems may be used for providing different images useful in assisting the surgeon in perform-

ing the medical procedure. Thus, various signals may be utilized in conjunction with or in alternative to the video image, such as ultrasound (echocardiography, Doppler ultrasound), angiography, electrophysiology, radiology or magnet resonance imaging (MRI). Also, an audio signal could be used for guiding the shaft. These detection techniques can be operated with the flexible instrument of the present invention to enhance guidance of the shaft to the site as well as manipulation at the site.

[0116] In association with the input devices of FIG. 2, there are various feedback techniques can be used for feeding certain parameters sensed at the slave station back to the master station. The following are parameters that may be sensed, including but not limited to:

- [0117] 1. Force.
- [0118] 2. Position.
- [0119] 3. Vibration.
- [0120] 4. Acoustics, auditory.
- [0121] 5. Visual.
- [0122] 6. Neurological stimulus.
- [0123] 7. Electropotential
- [0124] 8. Biochemical sensing.

[0125] Controller

[0126] As discussed previously, FIG. 6 illustrates a computer system 12, which interfaces the surgeon interface 11 and drive unit 13 of the slave station. The drive unit 13 contains a series of motors that control cables coupled by way of conduit 23 to control certain movements of the catheter apparatus. The controller 12, depicted in FIG. 6 essentially links the slave station to the surgeon interface. The user input device electronically sends commands, which are translated by the controller and sent to drive unit 13. Drive unit 13 then mechanically effects the motion of the shaft, particularly the flexible segment and the tool.

[0127] FIGS. 14 and 15 are block diagrams of an embodiment of a motor control system that may be employed in a drive unit of the present invention. Regarding the master station side, there is at least one position encoder associated with each of the degrees-of-motion or degrees-of-freedom. At least some of these motions are associated with a motor that may be represented by a combination of motor and encoder on a common shaft. Thus, controlling the motor ultimately controls such parameters as a force feedback to the master station. The present system can comprise a multi-axis, high performance motor control system, which can support anywhere from 8 to 64 axes simultaneously using either eight-bit parallel or pulse width modulated (PWM) signals. The motors themselves may be direct current, direct current brushless or stepper motors with a programmable digital filter/commutator. Each motor accommodates a standard incremental optical encoder.

[0128] The block diagram of FIG. 14 represents the basic components of the system. Host computer 700 is connected by digital bus 702 to interface board 704. Host computer 700 can be, for example, an Intel microprocessor based personal computer (PC) at a control station preferably running a Windows NT program communicating with the interface board 704 by way of a high-speed PCI bus 702 (5.0 KHz for

eight channels to 700 Hz for 64 channels) The PC communicates with a multi-channel controller electronic card, providing up to 28 axes of motion control, each with a 1.5 kHz sampling rate. The controller is efficient, scalable and robust.

[0129] Communication cables 708 intercouple interface board 704 to eight separate module boards 706. Interface board 704 can be a conventional interface board for coupling signals between digital bus 702 and individual module boards 706. Each module board 706 includes four motion control circuits 710, as illustrated in FIG. 15. Each circuit 710 can be, for example, a Hewlett-Packard motion control integrated circuit, such as an IC identified as HCTL1 100.

[0130] FIG. 15 depicts a further sub unit of this system, particularly a power amplifier sub unit 712. Power amplifier sub unit 712 is based on National Semiconductor's H-bridge power amplifier integrated circuits for providing PWM motor command signals. Power amplifier 712 is associated with each of the blocks 710, which couples to a motor X. Associated with motor X is encoder Y. Although the connections are not specifically set forth, it is understood that signals intercouple between block 710 and interface 704 as well as via bus 702 to host computer 700.

[0131] The motor control system may be implemented in two ways. In the first method the user may utilize the four types of control modes provided by the motor control sub unit 706: positional control; proportional velocity control; trapezoidal profile control; and integral velocity control. The use of any one of these modes can involve simply specifying desired positions or velocities for each motor, and necessary control actions are computed by motion control IC 710 of the motor control sub unit, thereby greatly reducing the complexity of the control system software. However, in the case where none of the onboard control modes are appropriate for the application, the user may choose the second method in which the servo motor control software is implemented at the PC control station. Appropriate voltage signal outputs for each motor are computed by the PC control station and sent to the motor control/power amplifier unit (706, 712). Even if the computation load is mostly placed on the PC control station's CPU, the use of high performance computers as well as high speed PCI bus for data transfer can overcome this problem.

[0132] FIG. 16 describes the overview of the control algorithm for the present invention, mapping out motions of the catheter to that of the surgeon's interface handle in three-dimensional space. Such precise mapping can create the feel of the tool being an extension of the surgeon's own hands. The control algorithm can assume that both the surgeon's interface as well as the catheter always starts at a predefined position and orientation, and once the system is started, it repeats a series of steps at every sampling. The predetermined positions and orientations, relate to the initial positioning at the master station.

[0133] First, the joint sensors (box 435), which are optical encoders in the present embodiment, of the surgeon's interface system are read, and via forward kinematics (box 410) computation of the interface system, the current positions (see line 429) and orientations (see line 427) of the interface handle can be performed. The translational motion of the surgeon's hand motion is scaled (box 425) whereas the orientations are kept identical, resulting in desired positions (see line 432) and orientations (see line 434) of the catheter's

tool. The results are then inputted into the inverse kinematics algorithms for the catheter's tool, and finally the necessary joint angles and insertion length of the catheter system are determined. The motor controller (box 420) then commands the corresponding motors to positions such that the desired joint angles and insertion length are achieved.

[0134] FIG. 16 provides an initial start position for the handle, indicated at box 440. The output of box 440 couples to a summation device 430. The output of device 430 couples to scale box 425. Initial handle position 440 is established by first positioning the handles at the master station so as to establish an initial master station handle orientation in three dimensional space. Initial handle position 440 is then compared to the current handle position at device 430. The output from device 430 is then scaled by box 425 to provide the desired tool position on line 432 coupled to the catheter inverse kinematics box 415.

[0135] Slave Station

[0136] The slave station comprises a flexible instrument, e.g. a shaft optionally supporting a tool at its distal end, for insertion into a subject. In one embodiment, the flexible instrument is a catheter. "Catheter" as defined herein refers to a shaft adapted for, but not necessarily limited to, insertion into a subject, and more particularly for insertion into natural body lumens, canals, vessels, passageways, cavities or orifices. The shaft is typically tubular, but any elongate shaft may be adaptable for insertion into the subject. The shaft can be solid or hollow. A subject can be a human, an animal, or even individual organs or tissues that are dead or living.

[0137] The introduction of the flexible instrument into the human or animal body, may be by percutaneous or surgical access to a lumen or vessel, or by introduction through a natural orifice in the body. In this regard, examples of natural lumens include body vessels such as a blood vessel (artery, chamber of the heart or vein), urinary system vessels (renal collection ducts, calix, ureter, bladder or urethra), hepatobiliary vessels (hepatic and pancreatic ducts, chyle ducts; common or cystic duct), gastrointestinal tract (esophagus, stomach, small and large intestine, cecum and rectum), gynecological tract (cervix, uterus, fallopian tube or milk ducts and mammary canals of breast), nasopharynx (eustacean tube, sinuses, pharynx, larynx, trachea, bronchus, bronchiole, tear duct) seminal vesicle, spinal canal, or ventricles of the brain. Examples of a natural orifice include oral, rectal, nasal, otic, optic, or urethral orifices.

[0138] The shaft can be constructed from a standard 9 French (2.67 mm diameter) coronary guiding catheter.

[0139] The shaft may support various forms of tools, typically at its distal end. As depicted in FIG. 6, a user can manipulate tool 18 along a single axis of motion where tool 18 is, for example, a grasper, scissors or general mechanism (such as a stapler or clip applier). It is easily understood by those of ordinary skill in the art, however, that tools may be located at a position other than the distal end of the shaft. Preferably the tools aid in carrying out various surgical or medical procedures, including, but not limited to:

- [0140] 1. Grasp;
- [0141] 2. Cut/lyse/puncture;
- [0142] 3. fill/drain;

[0143] 4. Secure (suture, staple, anchor);

[0144] 5. Implant, i.e., any procedure that leaves an object in the body after withdrawal of the flexible instrument;

[0145] 6. Remove;

[0146] 7. Deliver e.g. drug/therapeutic agents;

[0147] 8. Hemostasis;

[0148] 9. Anastomosis;

[0149] 10. Repair/reconstruct;

[0150] 11. Dilate/constrict/occlude;

[0151] 12. Retraction, e.g. backward or inward movement of an organ or part;

[0152] 13. Coagulate;

[0153] 14. Laser application;

[0154] 15. Heat/cool;

[0155] Exemplary objects implanted in a subject include staples, tacks, anchors, screws, stents, sutures, and a variety of other objects implanted by physicians and medical professionals.

[0156] The procedure of delivering (procedure 7, above) can further include delivery of agents including, but not limited to:

[0157] 1. Adhesives.

[0158] 2. Cryonics.

[0159] 3. Drugs.

[0160] 4. Biologic agents.

[0161] 5. Radioactive elements.

[0162] 6. Bullying agents.

[0163] Furthermore, the flexible instrument can be used as a sensor. Parameters that may be sensed include, but are not limited to:

[0164] 1. Force.

[0165] 2. Pressure.

[0166] 3. Electrophysiological signals.

[0167] 4. Chemical, oxygen, Ph, blood gas.

[0168] 5. Temperature.

[0169] 6. Vibration.

[0170] The slave station also comprises a drive unit capable of articulating the flexible instrument, particularly the shaft and the tool. The drive unit is drivably coupled to a receiver for receiving the mechanically drivable mechanism. In one embodiment, this coupling occurs via cables. The drive unit is electronically controllable from the master station, as there is an electronic link between the drive unit and a user input device of the master station.

[0171] When the receiver receives the mechanically drivable mechanism, the drive unit then has a direct pathway for controlling operation of the shaft and tool. If the shaft has a controlled flexible segment, the drive unit is capable of activating or bending the flexible segment via the mechani-

cally drivable mechanism, for actuation of the shaft, the tool and positioning of the tool at an operative site within the subject. In one embodiment, drive unit is capable of bending the flexible segment via a first set of cables which couple the drive unit to the receiver, and a second set of cables which drivably couple the mechanically drivable mechanism to the flexible segment and the tool.

[0172] One aspect of the present invention provides a remote controlled outer (guide) catheter having a distal end disposed at or in an area about an operative site, preferably in the immediate area of an operative site. A coaxial inner (working) catheter nested within the outer catheter can then be used to perform the surgical or medical procedure. Previous surgical procedures involve insertion of a trocar or cannula into the subject at a relatively short depth to provide an opening for receipt of the catheter, which is then guided to the operative site. Typically the catheter is not disposed at the immediate area around the operative or target site. Thus, if the surgeon needs a second catheter, the first catheter must be withdrawn and the second catheter is guided to the target site. Such repeated insertions can aggravate trauma experienced by the patient.

[0173] The feature of the present invention, on the other hand, employs an outer catheter disposed at the target site, which allows more than one shaft to be inserted and withdrawn with minimal irritation or trauma experienced at the passageway leading to the operative site. In one embodiment, the outer catheter housing a coaxial inner catheter is disposed at the target site. The inner catheter can immediately function at the operative site. If a second inner catheter is required, the first inner catheter can be quickly withdrawn through the outer guide catheter and the second inner catheter inserted through the outer catheter with minimal injury to the subject.

[0174] A feature of this aspect of the present invention allows coaxial multiple shafts to be remote controlled independently of each other. FIG. 3 depicts a system of remote controlled coaxial catheters. This system employs three coaxial or nested catheters L1-L3. Dashed line I represents an incision or entry point of the patient. FIG. 3 also illustrates computer controls C1-C3, which are outside of and remote from the patient. "Remote from the patient" refers herein to any location outside the sterile field. Computer controls C1-C3 are associated with corresponding actuators A1, A2 and A3, (i.e. drive units) which in turn are associated with shafts L1-L3, respectively. Thus, in FIG. 3, for example, the controller C1 controls an actuator A1 which, in turn, controls a certain action or movement of the outer shaft L1. Those of ordinary skill in the art would readily appreciate that only one computer can be used with software capable of independently controlling actuators A1-A3. In another embodiment, shafts L1-L3 can be independently controlled by one actuator, which independently drives specific cables leading to each of shafts L1-L3. Ultimately, the present invention allows shafts L1-L3 to be remote controlled independently from each other. For example, shaft L1 can remain stationary while shaft L2 undergoes linear translations or rotations about the co-axis. The distal end of shaft L3 can also carry out these motions as well as a bend or flex independent of shafts L1 or L2. Shaft L2 can be controlled to, for example, provide a rotational movement so as to enable rotation of a distal tool. The control of a tool supported at a distal end of a shaft is

independent of the motions of shafts L1-L3. Alternatively, all shafts L1-L3 can undergo a simultaneous bend or deflection at a single operative segment or flexible segment, labeled as O in FIG. 3.

[0175] FIG. 7 illustrates the outer and inner shafts. In FIG. 7, shaft 30 comprises an outer shaft 32 housing and coaxial with inner shaft 34. Outer shaft 32 and inner shaft 34 extend from and within mechanically drivable interface 26. Interface 26 mechanically couples a drive unit (shown in FIG. 6) with shaft 30. Interface 26 further comprises a series of control elements, such as pulleys 64 and 72, which run cable lines 52 and 28, and gears 60 and 68 for controlling rotation of the shafts.

[0176] The rotation of outer shaft 32 and inner shaft 34 about the co-axis can be controlled independently. Control element 60, or gear 60 in interface 26 encircles outer shaft 30 and controls the rotational position of guide shaft 32 in the direction indicated by rotational arrow 65. Gear 68 in interface 26 encircles inner shaft 34. Control element 68 controls the rotational position of the inner shaft 34 in the direction indicated by rotational arrow 69. Rotational arrows 65 and 69 indicate rotation about the "shaft lumen axis", i.e. the axis tangential to the cross section of the shaft lumen.

[0177] If a tool were supported at the distal end of inner shaft 34, control element 68 would control the rotational position of the tool about the shaft lumen axis as well. If the distal end were flexed, the shaft would curve and rotation of the shaft would cause the tool to trace a circle, and not cause the tool to rotate about its internal axis. As described below, another control can be positioned in the mechanically drivable interface for solely controlling the tool independent of the shaft controls.

[0178] Another aspect of the present invention provides a remote controlled flexible instrument capable of controlled bending, as controlled by a user at a master station. A flexible instrument comprises a shaft having at least one section that is flexible. "Flexible" refers herein to a material that is inherently and sufficiently deformable to readily pass atraumatically through a natural body lumen, cavity, vessel, orifice and the like. In one embodiment, the shaft is sufficiently flexible to readily flex and/or conform to a pathway in an anatomic vessel, lumen, cavity or the like. Non-flexible or rigid catheters can be distinguished from flexible instruments by the following test. By knowing the dimensions of a rigid catheter and the point of entry into the subject, one can calculate the position of the catheter end point inside the subject. In contrast, even if the dimensions and point of entry of a flexible shaft were known, the position of its end point within the subject cannot be calculated with precision because the flexible shaft may bend.

[0179] Flexible instruments of the present invention can also be distinguished from other known catheters that mimic bending motions solely through a series of rigid sections linked by joints. Thus, a "bend" is not the result of a deformation of the catheter material but by the pivoting or rotation of two rigid sections about a joint. In contrast, flexible instruments of the present invention include at least one flexible segment that is bendable without requiring the use of joints. The bending is remotely controlled, allowing deflection at these flexible segments away from the lumen axis of the segment. Bending in this sense is possible by choice of inherent flexibility of the instrument coupled with

an induced deflection at the flexible segment. Inherent flexibility can be achieved by choice of a deformable material, such as. Inherent flexibility can also be achieved by designed construction using a more rigid material, for example carving out segments of the material, i.e. slotting the material, such that the material is sufficiently thin for bending. Of course, the flexible instrument can comprise rotatable or pivotable joints, but the flexible capability is not the result of employing such joints, but by the deformability of the shaft material. In one embodiment, the bending is remotely controlled via a drive unit drivably coupled to the receiver for receiving a mechanically drivable mechanism or shaft mount. The shaft mount is then drivably coupled to the controlled flexible segment, thereby providing a drivable bending mechanism.

[0180] Those of ordinary skill in the art can appreciate that the shaft can be tailored for a particular body lumen. Factors of the shaft construction include resiliency of the walls of the lumen, curvature of the passageway, location of the target site, diameter of the lumen, etc. For example, a shaft for passing through a colon can be, but is not necessarily, manufactured from a material that is less deformable than a shaft for passing through a small, delicate blood vessel. Lumens that present passageways of high curvature may also require a more easily deformable, and thus more flexible, shaft than does a relatively straight lumen. Deformability of the shaft can also be tailored by varying the dimensions, particularly the diameter, of the shaft.

[0181] In this aspect of the invention, a user can controllably bend or flex at least a section of the flexible instrument. In one embodiment, this controlled bend can be provided by a shaft having at least one flexible segment, alternatively a controlled flexible segment. By manipulating controls at the master station, a user can induce a bend in the shaft at the flexible segment. Preferably, the bend at the flexible segment is actuated mechanically, thus distinguishing this aspect of the present invention from prior art catheters where the bends are induced electrically. For example, U.S. Pat. No. 5,238,005 describes a bending mechanism caused by varying the electrical resistance through a catheter material having a negative coefficient. Heating one area of a catheter by increasing its electrical resistance results in contraction of that area, causing the catheter to deflect toward the contracted area. In contrast, the present catheter responds to mechanical forces.

[0182] FIGS. 7 and 8 illustrate one embodiment of a controlled flexible segment. FIG. 7 shows controlled flexible segment 42 residing between proximal end 36 and distal end 38 of shaft 30. It is understood, however, that flexible segment 42 can be positioned on any portion of shaft 30. FIG. 8 provides an expanded view of flexible segment 42 and illustrates one construction of flexible segment 42. Here, flexible segment 42 is constructed by providing inner shaft 34 as a flexible material nested within outer shaft 32. Outer shaft 34 is split into rigid proximal and distal sections 36 and 38, both encircling inner shaft 34. Thus, flexible segment 42 is the gap between proximal and distal sections 36 and 38. Shrink-wrap pieces 44 and 45 extend over the respective facing ends of the proximal and distal shaft sections 36 and 38 and adhere these facing ends to the flexible inner shaft.

[0183] Alternatively, flexible segment 42 may be in the form of a metal coil of diameter similar to the diameter of outer shaft sections 36 and 38.

[0184] Although FIG. 8 illustrates outer shaft 32 as being rigid, it can be appreciated that outer shaft 32 can be constructed of a flexible material as well, although its flexibility is preferably less than that of inner shaft 34.

[0185] Referring to both FIGS. 7 and 8, the bending of flexible segment 42 is controlled through flex wire 52 extending from mechanically drivable mechanism 26 and through flexible segment 42, terminating at point 54 of distal end 38 (see FIG. 8). Flex wire 52 is preferably disposed between inner shaft 34 and outer shaft 32. FIG. 8 shows termination point 54 residing on the outer surface of distal end 38, although conceivably other surfaces of distal end 38 can serve as termination points. The other end wire 52 resides within drivable mechanism 26 on control pulley 64. Turning pulley 64 has the effect of pulling wire 52 in a direction parallel to shaft 30 pointing towards drivable mechanism 26. Because wire 52 is terminated at 54, this pull causes the distal shaft section 38 to deflect in a direction indicated by the arrow 55, as shown in FIG. 7.

[0186] More than one flex wire can be spaced about the circumference of outer shaft 32 to allow bending along multiple directions different from arrow 55 yet orthogonal to shaft 30. For example, FIG. 11 illustrates an embodiment where two cables actuate bending the bending. FIG. 11 is a cross-sectional view of outer shaft 32 receiving inner shaft 34 at termination point 52. Two cables 52A and 52B terminate on outer 32 on opposite sides of distal shaft section 38. Cables 52A and 52B may be manipulated so as to deflect the distal shaft section in opposite directions, in a manner described previously. Those of ordinary skill in the art can readily appreciate that employing multiple cables results in a shaft capable of deflecting in any number of directions.

[0187] If inner shaft 34 supports a tool at its distal end, the bending motions, along with the rotation about the co-axis, serves to place the tool at any place in three-dimensional space. Another control element, i.e. pulley 72 controls cable 28, which extends through the hollow area of inner shaft 34, thereby allowing control of a specific tool operation. Depending on the complexity of the device, one or more cables leading to the tool may be required. In one embodiment, FIG. 12 depicts a distal end of shaft 30, showing operative segment O (e.g. flexible segment 42) and tool 18. FIG. 12 shows two coaxial catheters including an outer shaft O1 (such as outer shaft 32) and inner shaft O2 (such as inner shaft 34). Also disclosed are two stainless steel cables, including outer cable O3 and inner cable O4. Outer shaft O1 provides translational and rotary motion. Outer cable O3, which is disposed between outer and inner shafts O1 and O2, provides the lateral rotation (or yaw motion) of tool 18. Inner shaft O2 rotates tool 18 and inner cable O4 actuates the jaws of tool 18. The tool of FIG. 12 provides a single degree-of-freedom in order to actuate a gripper, scissors or generic mechanism (such as a stapler or clip applier). An example may be a bi-directional gripper 5 mm in length and 2.67 in diameter.

[0188] In one embodiment, the system comprising the flexible instrument comprises tool or mini-tool (18), the operative segment (42), the catheter stem (32, 34), the coupler (24, 26) comprising the mechanically drivable mechanism 26 and the receiver 24, the drive unit (13), the controller (12) and the surgeon's interface (11). The coupler provides a translational degree-of-freedom achieved by

using a sliding mechanism, i.e. rails 25, onto which the coupler is mounted, as illustrated in FIG. 6. The operative or controlled flexible segment provides a number of articulations in order to position and orient tool 18. The catheter (30) has four (4) degrees-of-freedom, i.e. one translation and three rotations, as shown in FIG. 7. A fifth degree-of-freedom may be provided by the actuation of the mini-tool, as tool 18 can provide at least a single axis of motion for a grasper, scissors or general mechanism (such as a stapler or clip applicator). The combination of one translation and two rotations allows the operative segment to arbitrarily position the mini-tool in three dimensional space. A final degree-of-freedom rotates the mini-tool axially.

[0189] The following describes the mathematical mapping of the physician's command input to the motion of the catheter system. FIG. 13 schematically illustrates the various degrees of freedom by which the catheter can be manipulated, particularly the axial and lateral rotations, or the translation motion allowing independent control of the tool position within the surgical space, as well as axial rotation of the tool. For example, the system of FIG. 6 provides a physician with seven independent command inputs, including position (χ_i, γ_i, z_i), orientation ($\theta_i, \omega_i, \psi_i$) and tool grip angle α_i . The controller calculates the position of the five (5) independent degrees-of-freedom of the catheter system, given by ($\chi_c, \theta_c, \omega_c, \psi_c, \alpha_c$), by determining the position (x, y, z) of the tool, given by $\chi = \chi_c + r \cos \omega_c$, $\gamma = -r \sin \omega_c \sin \theta_c$, $z = r \sin \omega_c \cos \theta_c$, $\psi = \psi_c$, $\alpha = \alpha_c$, where $\chi_c, \theta_c, \omega_c, \psi_c, \alpha_c$ are the independent inputs to the catheter system, and r is the distance from the lateral joint to tip of the mini-tool. The resulting position is $\chi_c = \chi - r \cos \psi_c$, $\theta_c = \tan^{-1}(-y/z)$, $\omega_c = \sin^{-1}(z/r \cos \theta_c)$, $\psi_c = \psi$, $\alpha_c = \alpha$. If λ is chosen as a scaling value, the following mapping between command input and independent catheter input is $\chi_c = \lambda \chi_i - r \cos \omega_c \theta_c = \tan^{-1}(-y_i/z_i)$, $\omega_c = \sin^{-1}(\lambda z_i/r \cos \theta_c)$, $\psi_c = \psi_i$, $\alpha_c = \alpha_i$. It is noted that the axial rotation and grip position are scaled.

[0190] FIG. 42 is a perspective view of another embodiment of the slave station for a remote controlled flexible instrument. FIG. 42 depicts flexible instrument system 500 supported from support bracket 502, which extend to the operating table (see FIG. 6). Usually the support bracket is supported from the side of the operating table and may be adjustable in position relative to the operating table, to dispose system 500 in a convenient position over the patient. In one embodiment, bracket 502 is secured to the operating table at one end. The other end of bracket 502 supports the entire flexible instrument by means of a two-piece structure similar to that described in copending U.S. Provisional Applications Serial No. 60/279,087 filed Mar. 27, 2001. A knob may be provided on support base 504, not shown in FIG. 42. Once the support base 504 is fixed to the support bracket 502, then the flexible instrument system is maintained in a fixed position at base 504, providing a stable and steady structure during the medical procedure. Like FIG. 6, system 500 can be positioned at an acute angle with respect to the operating table.

[0191] Flexible instrument system 500 comprises flexible instrument 510 having a shaft 528 extending to mechanically drivable mechanism 526, which interlocks with base (or receiver) 506. Base 506 is supported on carriage 508. Carriage 508 in turn is adapted for linear translation and supported by elongated rails 512 and 514. Rails 512 and 514 terminate at one end via end piece 516, which provides

further support. Support base 504 terminates rails 512 and 514 at their other end. Carriage 508 includes bearings or bushings 509 that support the carriage from rails 512 and 514.

[0192] Flexible instrument system 500 employs two separate cable bundles for mechanically driving the flexible instrument along rails 512 and 514. Pulley 521 (dotted outline), residing within carriage control module 520, receives a first pair of cables 518. Pulley 521 also receives a second set of cable (see cabling sections 513 and 515 of corresponding FIG. 43), which runs through carriage 508 to a further pulley 522 supported by end piece 516. The second set of cables controls the translational motion of carriage 508 and terminates at point 519 (see FIG. 45).

[0193] FIG. 42 also shows a set of cables 524 for driving control elements, e.g. pulleys within receiver 506. These control elements move the shaft and the tool in several degrees-of-freedom. Arrow J1 indicates the linear translation via module 520. Rotational arrow J2 indicates rotation of flexible shaft 528 of flexible instrument 510 about the inner axis parallel with the shaft length. Arrow J3 represents the flexing or bending of flexible shaft 528 at controlled flexible segment 530. In this embodiment, flexible segment 530 is positioned directly adjacent tool 534 at the distal end of shaft 528. Arrow J4 represents the pivot action of a wrist joint, which links tool 534 to shaft 528, about axis 532. In this embodiment, tool 534 is exemplified as a grasper, and arrows J5 and J6 represent the opening and closing actions of the tool jaws. Motions indicated by arrows J2-J6 are controlled from cabling 524 originating at receiver 506.

[0194] FIG. 42A provides an enlarged perspective view of the distal end of shaft 528 including flexible segment 530 and tool 534. Tool 534 comprises upper grip or jaw 602 and lower grip or jaw 603, both supported from link 601. Base 600 is affixed to or integral with flexible shaft 528. Link 601 is rotatably connected to base 600 about axis 532. A pivot pin may be provided for this connection. Upper and lower jaws 602 and 603 are rotatably connected to link 601 about axis 536 and again, a pivot pin can provide this connection.

[0195] FIG. 42A shows eight cables at 538 extending through the hollow inside of shaft 528 for control of tool 534 and flexible segment 530. Two of these cables operate the bend of flexible segment 530, two cables operate one of the jaws 602, two cables operate the other of the jaws 603 and the last two cables operate the wrist action about the axis 532. All of these cables travel through the hollow shaft 528 and through appropriate holes in flexible segment 530, e.g. wire 525, as well as holes in base 600. Each of these pairs of cables operates in concert to open and close jaws, pivot about the wrist, and bend flexible segment 530.

[0196] One pair of cables travels through shaft 528 and through appropriate holes in the base 600, wrapping around a curved surface of the link 601 and then attaching to the link. Tension on this pair of cables rotates the link 601 along with the upper and lower grips or jaws 602 and 603 about axis 532.

[0197] Two other pairs of cables also extend through the shaft 528 and through holes in the base and then pass between fixed posts 612. These posts constrain the cables to pass substantially through axis 532, which defines rotation of link 601. This construction essentially allows free rotation

of link **601** with minimal length changes in the cables passing to jaws **602** and **603**. Thus, the cables actuating jaws **602** and **603** are essentially decoupled from the motion of link **601** and are not effected by any rotation of link **601**. Cables controlling jaw movement terminate on jaws **602** and **603**. These cables permit independent operation of the jaws **602** and **603** in respective clockwise and counter clockwise directions with respect to axis **536**. A similar set of cables is present on the under-side of the link **601** (not shown). Each of the jaws **602** and **603**, as well as the link **601**, may be constructed of metal. Alternatively, link **601** may be constructed of a hard plastic material. Base **600** may also be constructed of a plastic material and may be integral with shaft **528**.

[0198] Bending of flexible segment **530** is provided via diametrically disposed slots **662**, which define spaced ribs **664**. Flexible segment **530** also has a longitudinally extending wall **665** through which cabling may extend, particularly for the operation of the tool. One of the pairs of cables of bundle **538** controlling flexible segment **530** terminates where base **600** intercouple with shaft **528**. This pair of cables works in concert to cause bending as indicated by arrow **J3**, i.e. in a direction orthogonal to the pivoting provided at wrist axis **532**. In FIG. 42A only one cable **525** of two is illustrated.

[0199] FIG. 43 is an exploded prospective view showing carriage **508**, receiver **506** and drivable mechanism **526**. Carriage **508** is adapted for motion along rails **512** and **514**. Pulleys **521** and **522** receive cabling, i.e. cable sections **513** and **515**, which terminate at the carriage base at point **519**. Other sections of this cable extend through an elongated hole or passage within carriage **508**.

[0200] Receiver **506** and drivable mechanism **526** each comprise enclosed housings supporting a plurality of control elements, such as intercouplable drivewheels and associated pulleys or cams. Inter-engaging gears **540** and **542** are supported respectively in the modules **506** and **526**. A pair of cables from bundle **524** engages pulley **544** (see FIG. 45) which, in turn, drives gear **540**, and which further, in turn, drives gear **542** for providing rotation of shaft **528**. Collar **546** is provided at the terminus of the proximal end of shaft **528** for supporting shaft **528**, which is driven by gear **542**. Cabling extending through collar **546** and shaft **528** couple mechanical actions from drivable mechanism **526** through the flexible instrument shaft **528** to the distal end thereof.

[0201] Drivable mechanism **526** interlocks with receiver **506**, providing the mechanical connection that allows the drive unit to run cabling in flexible instrument **510**. Blades **606**, jutting out from the housing of receiver **506**, engage with corresponding slots **608** associated with drivable mechanism **526**. Projecting from the proximal end of receiver **506** is ridge **610**, which is substantially U-shaped and provides another interlocking feature for mating with a similarly shaped slot **614** at the same end of drivable mechanism **526**. Posts **616** protruding from the housing of receiver **506** are adapted to releasably mate with holes **618** in drivable mechanism **526**. Posts **616** and holes **618** to interlock with each other, but may be released from each other via side-disposed buttons **620**, as illustrated in FIG. 46. FIG. 43 also shows the cam locking screws **615**.

[0202] FIG. 44 is a partial broken away rear elevational view of interlocking interfaces as seen along line 44-44 of

FIG. 42. FIG. 44 shows alignment posts **616** each having a groove **617**, which is engaged by the corresponding button **620**. Button **620** is in the form of a plate member biased to a locked position by means of spring **621**. A plate for button **620** has a keyhole slot for receiving and holding post **616** therein. Button **620**, however, may be manually depressed to release posts **616** and enable ready detachment of drivable mechanism **526** from receiver **506**. A retaining pin **625** may also be used to limit the travel of the button between in and out positions.

[0203] FIG. 45 is cross-sectional side view through the interconnecting modules taken along line 45-45 of FIG. 42. FIG. 45 shows details of drive wheels (or pulleys) in the modules **506** and **526**. Four drive wheels **622** are supported within the housing of receiver **506**. Drive wheels **622** receive cabling for controlling the motions of the shaft and the tool, where the cable protrudes from cable bundle **524** in FIG. 43. Each of these pairs of cables is controlled from a corresponding motor, which is part of the drive unit (see discussion of FIG. 49, below).

[0204] FIG. 45 also shows output blades **606**, previously shown in FIG. 43, which extend into corresponding slots **608**. These slots are disposed in respective intergating drive wheels **624** of the drivable mechanism **526**. Blades **606** have a rectangular end construction for engaging with similar rectangular slots **608** associated with the module **526**. FIG. 45 also shows the gears **540** and **542** in engagement to allow drive to occur from bundle **524**.

[0205] FIGS. 45 and 46 show a series of idler cams **626**, one associated with each of drive wheels **624**. FIG. 46 is a plan cross-sectional plan view through receiver **506** as taken along line 46-46 of FIG. 45. FIG. 46 shows the placement of cams **626**. A cable wraps around each of drive wheels **624** and is held in position by its associated cam **626**. FIG. 46 also shows all of the cables running parallel to each other at region **627**, where the cables run from respective drive wheels **624**, through collar **546** and extending down inside shaft **528** to the distal end. With the use of the placement and adjustment of cam **626**, the cables are all directed in a manner to easily couple into shaft **528**.

[0206] Each of cams **626** has an off-center axis **631**. As viewed in FIG. 46, cam **626** may be rotated clockwise to tighten its associated cable. Rotation counterclockwise loosens the tension. Cam locking screws **615** secure cam **626** in an adjusted-to position (see FIG. 48, a cross-sectional view taken along line 48-48 of FIG. 47). FIG. 48A is a cross-sectional view taken along line 48A-48A of FIG. 48. As depicted in FIGS. 46 and 48A, the cable associated with each wheel **624** may be secured in a cable clamping hole **633** via a cable clamping screw **635**. A similar clamping arrangement is associated with wheels **622**. A roll pin fixes each wheel **622** to each spindle **607**.

[0207] FIG. 47 is a cross sectional plan view taken through receiver **506**, as taken along line 47-47 of FIG. 45. The cross-sectional view of FIG. 47 illustrates drive wheels **622** associated with receiver **506**. Drive wheels **622** receive cabling from cable bundle **524**. Each of a pair of idler pulleys **630** are associated with drive wheels **622**. At the very input to receiver **506**, idler pulleys **632** are used for directing the cable to idler pulleys **630** and from there to drive wheels **622**.

[0208] FIG. 48B is a fragmentary plan view of a drive wheel engagement slot by itself as seen along line 48B-48B

of FIG. 48A. The cross-sectional views of FIGS. 48A and 48B illustrate drive wheels 622 within receiver 506 having associated end blades 606. End blade 606 is a screwdriver-type blade that engages a slot previously identified as slot 608 in FIG. 43. This slot 608 is in drive wheel 624 of receiver 526. In FIG. 48B, slot 608 displays a tapered portion. The tapered portion allows easy registration of end blade 606 and slot 608, and thus easy registration between drive wheel 622 and drive wheel 624.

[0209] As described to this point, the bending or deflection of the shaft can be actuated by mechanical means such as a wire extending along a length of the shaft. Thus, actions at the distal end of shafts may be controlled by mechanical elements, such as cables, wires or other tendons.

[0210] Alternatively, actuation of the controlled bending can occur by other means, such as by remote electromagnetic signal couplings. FIG. 41A illustrates shaft 850 having a central lumen. Residing in the central lumen is an operative or controlled flexible segment O, in the form of a plurality of spaced electromagnetic rings 852, separately labeled as R1, R2, R3 and R4. Each of rings R1-R4 is associated with wires 854, similarly labeled as wires W1, W2, W3 and W4. Rings 852, once energized, provide bending of shaft 850 at flexible segment O. FIGS. 41A and 41D are meant to be schematic, while FIGS. 41B and 41C are actual implementations for actuation of the rings by means of coils or windings 853. As illustrated in FIG. 41B, each ring may be electrically energized via a winding 853 associated therewith. FIG. 41B shows a fully wound winding, while FIG. 41C shows a half wound winding. Ring 852 may also have two separate half wound coils on opposite sides thereof. Wires 854 (in pairs) are selectively energized to energize windings 853 on the rings, which in turn, provide either attraction or repulsion of the rings. FIG. 41D illustrates the results of regions of rings 852 being energized to attract or repel adjacent rings. For example, a certain direction of current flow through windings 853 can create an attraction of the coils at the bottom and a repulsion of coils at the top. This cooperative action causes a bending at the operative or controlled flexible segment O.

[0211] The flexible instrument depicted in FIGS. 6 and 7 provides only the distal end as being remotely controlled. It can readily be appreciated that a controlled flexible segment may be provided, not necessarily for action at a target site, but to control certain movements of the catheter to assist in reaching a target site.

[0212] FIGS. 4 and 5 illustrate the advantages of a flexible instrument, particularly a catheter having controlled flexibility via controlled flexible or operative segments, for use in performing a procedure or for guiding the instrument through a natural body lumen. FIG. 4 provides a schematic cross-sectional diagram, illustrating a catheter K for use in mitral valve repair, to be discussed in more detail below. FIG. 4 also shows catheter K supporting a tool 18 for carrying out certain procedures at the mitral valve annulus, also described in further detail below. In FIG. 4, catheter K is shown entering the femoral vein V by a percutaneous access at S. From the femoral vein V, catheter K must bend prior to entering the right atrium R. Catheter K then passes through a septal wall of the heart to the left atrium L, which is directly above the mitral valve M. In this particular embodiment, the operative segment of the catheter K is

illustrated at O and is positioned near the very distal end of the catheter K. Thus, at the sharp, almost 90° bend prior to entering right atrium R, a user can controllably bend catheter K at the operative segment, to perform a procedure with tool 18. Also, the ability to controllably bend catheter K prevents tool 18 from conceivably being trapped within femoral vein V, causing damage to the walls of vein V. In this embodiment, it may be preferable to have at least some length of catheter K constructed of a deformable or flexible material, enabling the catheter to easily pass through the body lumen by essentially conforming to vein configurations, such as that of femoral vein V.

[0213] FIG. 5 provides a schematic cross-sectional diagram illustrating a surgical procedure where catheter K1 enters a natural body orifice, such as the urethra for carrying out procedures in, for example, the bladder. In FIG. 5 catheter K1 is shown extending into bladder B1. In this example, the computer controlled segment, identified as operative or flexible segment O in FIG. 5, is positioned at a more proximal section of catheter K1. Bladder B1, being an open cavity, does not have lumens leading from the urethra that would naturally guide a catheter towards any particular operative site. Upon entering bladder B1, catheter K1 can bend in any direction and not necessarily in the direction of the operative site. In this embodiment, because of the more proximal positioning of operative segment O, a surgeon can controllably bend the distal end of catheter K towards the operative site. In the embodiment shown in FIG. 5, the distal end of the catheter, labeled P1, can be rigid or be "passively" flexible, i.e. made of a flexible material and not necessarily controlled for flexure under remote computer control.

[0214] In the illustration of FIG. 4, the catheter K may be fed through the femoral vein by direct surgeon manipulation, in which case only the operative segment O is under computer control from a master station. Alternatively, the catheter may translate linearly through the vein under remote master station control, where the catheter can have other operative segments disposed at different locations of catheter K. Each of these operative segments can be controlled from a master station for assistance in the guiding of the catheter to a predetermined target site. Thus, the catheter may be inserted manually and also have remote computer control for at least limited linear translation.

[0215] FIGS. 3A-3C show different embodiments of flexible instruments with multiple operative or controllable flexible segments. Shafts having multiple operative segments can be very useful for procedures in a body cavity, as discussed previously, but can also be useful in navigating the shaft through intricate or delicate body lumens. FIGS. 3A-3C schematically illustrate controller CT and a slave portion of the system comprising actuators or drive units A1-A4 and shaft KA, KB or KC having three operative segments O1-O3. In accordance with each of these embodiments, a surgeon inputs commands from a master station to cause certain corresponding movements of the shaft at the slave station. A surgeon's manipulations at the master station are coupled to controller CT where these manipulations are mapped to actions at operative segments O1-O3. Thus, a surgeon, at an appropriate input device, may carry out a first manipulation to control a segment O1, a second different manipulation to control the segment O2 and still a third

manipulation to control the segment O3, either simultaneously or sequentially. A fourth manipulation may control the tool G.

[0216] FIG. 3A shows shaft KA having three operative segments, O1, O2, and O3, and tool G at its distal end. Actuators A1, A2 and A3 are associated respectively with operative segments O1, O2 and O3. Actuator A4 controls tool G. Each of actuators O1-O3 is controlled from controller CT. Operative segments O1, O2 and O3 are spaced a certain distance apart from each other, allowing shaft KA to simultaneously experience controlled bends. This arrangement may be necessary for lumens with multiple bends, or for hard to reach operative sites.

[0217] FIG. 3B, shows catheter KB having tool G1. In this embodiment, three operative segments O1, O2 and O3 are spaced from each other along the length of catheter KB. Segments O1-O3 can be controllably bent to form an arc having an imaginary radius point P. Thus, this arrangement of operative segments can actuate particularly acute bends. In another embodiment, catheter KC in FIG. 3C employs three operative segments O1-O3, which are contiguous. The radius of curvature can be increased.

[0218] It is understood that non-operative segments of the catheter in FIGS. 3A-3C can comprise either a flexible or a rigid material. It can be appreciated that one or more controlled flexible segments can be incorporated in the shaft, depending on the particular application.

[0219] Another aspect of the present invention provides a remote controlled flexible instrument operable within the sterile field, and disposable after use. The sterility of reusable medical instruments and implements are maintained by well-known methods such as exposure to sterile solutions and/or autoclaving. For some medical implements, it can be more cost effective to manufacture them from low cost materials and dispose them after a single use, or use on a single patient. But for certain other medical instruments, its manufacture from low cost materials still results in a costly product due to the intricate nature of the individual parts and the labor required to manufacture complex components.

[0220] It is another feature of the present invention to provide a design for a remote controlled flexible instrument having disposable components, particularly those components that are exposed to the sterile field. The present design allows the use of injection-molded plastic parts. The disposable component can be easily and quickly engaged into and disengaged from a non-disposable, reusable base. The components can be locked onto the base by snapping or interlocking matched parts, without having to thread cable wires or attach any intricate components.

[0221] One aspect of the present invention provides a disposable implement comprising a disposable mechanically drivable mechanism, a disposable shaft extending from the drivable mechanism, and optionally a disposable tool supported on a distal end of the shaft. Referring back to FIG. 7, mechanically drivable mechanism 26 comprising gears 60 and 68 and pulleys 64 and 72, can be manufactured from injection molded plastic, as well as shaft 30 extending from drivable mechanism 26. The sides of pulleys 64 and 72 feature a first semicircular planar disc stepped up from a second matching semicircular planar disc. The sides of the pulleys in receiver base 24 correspondingly match the

stepped up pattern of pulleys 64 and 72. Engaging drivable mechanism 26 onto receiver 24 requires matching and interlocking the respective pulley discs. Thus, the interlocking feature in effect extends the cabling pathway from the first set of cables running from the drive unit to receiver 24, to a second separate set of disposable cables contained within drivable mechanism 26 and shaft 30. No tying or threading of cables is required to engage the disposable portion onto receiver 24.

[0222] Another design for a disposable implement is illustrated in FIG. 42. In FIG. 42, the flexible instrument 510, comprising drive mechanism 526 and shaft 528, can be a single piece disposable unit that is readily engageable and disengageable relative to the base module 506.

[0223] Disposable implement 510 may be considered as comprising a disposable, mechanically drivable mechanism such as the coupler or module 526 interconnected to a tool 534 through an elongated disposable flexible shaft or stem 528. This disposable and flexible implement is mounted so that the mechanically drivable mechanism may be connectable to and drivable from a drive mechanism, such as illustrated in FIGS. 6 and 7. In the illustrated embodiment the drive mechanism may be considered as including the coupler or module 506 and the associated drive motors. The disposable elongated flexible instrument is generally inserted into a body vessel or cavity of a subject along a selected length of the disposable elongated instrument with the elongated flexible instrument being disposable together with the disposable mechanically drivable mechanism.

[0224] The disposable implement is purely mechanical and can be constructed relatively inexpensively thus lending itself readily to being disposable. It may be difficult to make only the tool disposable, due to the intricate nature of the tool parts, which may require the user to perform intricate maneuvers and cable threading into the base of the slave station. Here, the disposable implement, i.e. the tool, shaft and drivable mechanism are manufactured as a single piece disposable unit, thus eliminating the need for intricate instrument or tool exchange procedures.

[0225] Ideally, the base of the slave station, which contacts the disposable implement, is easily cleanable. It is preferred that the disposable implement, which operates within the sterile field, experiences minimal contamination by contacting the slave station. In one embodiment of the present invention, as illustrated in FIG. 43, the interlocking drivable mechanism 526 and receiver 506 features substantially planar surface at the point of contact between the two modules. Regarding receiver 506, the planar surface is easy to clean and the inner intricate pulleys and cabling are protected from contamination by the housing. Regarding mechanically drivable mechanism 526, the housing can be made of injection-molded plastic that is simple to manufacture and is easily disposable.

[0226] One advantage of the present invention is the ease of engaging and disengaging the disposable implement. In a particular medical procedure, a multitude of instrument exchanges may be required, and the system of the present invention is readily adapted for quick and easy instrument exchange. Because the receiver is maintained in a fixed position, the surgeon can easily exchange instruments by readily decoupling at the modules 506 and 526. The ease of exchanging instruments lends to the portability of the slave

station. This portable nature of the slave unit comes about by virtue of providing a relatively simple flexible instrument in combination with an adaptor (module 506, module 520, carriage 508 and associated components) for supporting the flexible instrument. Overall, the slave station is of a relatively small configuration. Because the slave unit is purely mechanical, and is decouplable from the drive unit, the operator can readily position the slave unit. Once in position, the slave unit is then secured to the support, and the mechanical cabling of the slave unit is then attachable to the drive unit. This makes the slave unit both portable and easy to position in place for use.

[0227] FIG. 49 shows an embodiment where pulley 677 is readily manually decouplable from motor 675. For this purpose pulley 677 may be a two-piece pulley arrangement comprising a coupler spindle and a coupler disk with the coupler disk secured to the output shaft of the motor. This enables the entire assembly to be disconnected at the motor so that the flexible instrument system 500 with its flexible instrument 510 may be positioned relative to the patient, independent of any coupling with the drive motors. Once the system illustrated in FIG. 42 is in place, then the coupling of the cables can be made at pulley 677 to provide drive to the flexible instrument system.

[0228] Another aspect of the present invention provides a system for repairing a cardiac valve, such as a mitral valve. Current mitral valve repair techniques, either open or minimal access, require the surgeon to place the patient on cardiopulmonary bypass and stop the heart. The left atrium is then opened and exsanguinated to allow the surgeon to perform the repair. This aspect of the present invention provides a minimally invasive mitral valve annuloplasty technique featuring the following advantages: (1) peripheral venous access; (2) the heart can continue to beat during the repair; and (3) assessment of the correction of valve incompetence in real-time using, for example, Doppler ultrasound guidance.

[0229] In one embodiment, the present cardiac valve repair system employs a guide shaft extending from a site outside a patient to an area about the cardiac valve. The guide shaft receives a flexible inner shaft for disposing a tool at the area about the cardiac valve, where the tool is supported at the distal end of the guide shaft. Preferably, the inner shaft has a relatively small diameter enabling percutaneous intravascular and endoscopic surgery. Even more preferably, the inner shaft, and optionally the guide shaft, is capable of accessing the mitral valve from the peripheral circulation, eliminating the need for incisions through the chest wall. In one embodiment, the inner shaft can have a diameter ranging from 8 to 15 French (2.5-5.0 mm). The outer catheter may be constructed from a standard 9 French coronary guide catheter, having a diameter of 2.67 mm and a wall thickness of 0.1 mm. In other embodiments, the inner catheter can have an outer diameter of 1.1 mm and an inner diameter of 0.09 mm. In yet another embodiment, the braided stainless steel cables are 0.63 mm in diameter and are capable of transmitting 178 Newtons (40 lbs. approx.).

[0230] A feature of this aspect of the present invention is that the percutaneous access to the mitral valve can be accomplished on a beating heart, eliminating the risks associated with cardiopulmonary bypass (CPB). To enable a procedure on the beating heart, preferably the procedure can

be performed under physiologic conditions. The physician may monitor the procedure by, for example, transesophageal echocardiography, instead of a video image. This technique enables real-time assessment of the correction of the mitral valve regurgitation (MR) during the procedure, further enabling intra-operative provocative cardiac testing, with preload and afterload challenges and cardiac pacing all under trans-esophageal echo and trans-thoracic ultrasound guidance to optimize repair.

[0231] The tool can be remote controlled, as described herein, and can be designed for use in any procedure of the cardiac valve repair process. For example, a first set of tools is capable of percutaneous mitral valve annuloplasty. This represents a paradigm shift in management of disease from MIS and open surgical to intraluminal interventions. While this catheter-based intervention is described in connection with mitral annuloplasty, the technique can also be applied to other structures such as, by way of example and not limiting, the biliary tree, the genitourinary tract and intraventricular neurosurgery.

[0232] The system further includes a retainer at the area of the cardiac valve, where the retainer is attached to an annulus of the cardiac valve. As will be described in greater detail below, the retainer is closeable via the tool to draw the annulus into a smaller diameter.

[0233] In one embodiment, a trans-septal guide catheter is used to guide and support an inner catheter. The guide catheter is introduced by percutaneous access, and allows the clinician to access the left atrium via the venous circulation, i.e. through the heart wall (see FIG. 4). The guide catheter may be non-robotic, i.e. simply manipulated manually by the surgeon. Alternatively, the guide catheter may be robotically controlled from surgeon manipulations at an input device of the master station.

[0234] Once access to the left atrium is established, the inner catheter is threaded into the left atrium through the guide catheter. The inner catheter contains attachment anchors for deployment at desired points around the mitral valve annulus. A remote controlled 5-degree-of-freedom tool and wrist can be utilized to precisely reach the annulus. Ultrasound may be used to visualize the system and guide the anchor positioning and placement. This ultrasound may be trans-esophageal ultrasound or trans-thoracic ultrasound, for example. Furthermore, electrophysiologic signals of the heart may be used to aid in precisely locating the position of the tool at the fibrous mitral valve annulus.

[0235] There is now described a number of techniques employing the catheter apparatus of the present invention. These techniques are described herein primarily in connection with mitral valve repair.

[0236] FIG. 19 is a schematic representation of the heart muscle showing the left ventricle 218, the right ventricle 219, the left atrium 220, the right atrium 221 and the aorta 222. Between the left atrium and the left ventricle, blood flow is from the left atrium through the mitral valve 210 to the left ventricle 218. FIG. 26 illustrates an expanded view of a mitral valve at 210 including annulus 211 and leaflets 213. FIG. 27 illustrates schematically the leaflets 213 of the mitral valve 210 with the mitral valve annulus 211. As a heart muscle ages, it is typical for the annulus of the mitral valve 210, illustrated in FIG. 19 at 211, to expand in

diameter causing problems with the leaflets **213**. If the leaflets fail to close properly, regurgitation may result, causing leakage by the mitral valve in the reverse direction and resulting in improper blood flow through the heart. Thus, mitral valve repair involves, at least in part, shrinking the diameter of the annulus to allow the leaflets to operate properly.

[0237] In one embodiment, threading or sewing a ring about the annulus reduces the annulus diameter, where the ring is closeable. The annulus comprises relatively tough tissue just above the top of leaflets. As viewed in **FIG. 19**, the opposite end of the annulus at **217** tends to expand outwardly. **FIG. 19** illustrates an area at the annulus of the mitral valve (that annulus being at the top in **FIG. 19**) identified as trigone area **215**, where the valve ring is more rigid and remains stationary. Because this area is relatively stable and rigid, it is thus difficult to contract, and most of the expansion of diameter of the ring occurs away from the trigone area. This, again, is illustrated in **FIG. 20** by the positions shown in solid and in dotted outline.

[0238] **FIG. 20** shows schematically parts of the heart such as the left atrium **220** and the left ventricle **218**, with the mitral valve **210** disposed therebetween. **FIG. 20** illustrates the annulus of the mitral valve in solid position, at a smaller diameter where the leaflets operate properly. The dotted outline **217** represents the expanded diameter of the base of the mitral valve, the state at which mitral valve leakage can occur.

[0239] To carry out the technique of the present invention, a guide catheter **230** is employed, such as a transseptal atrial guide catheter. The access for catheter **230** is via the vena cava to the right atrium **221**. This access may be from above via the jugular vein or below by way of the femoral vein. A puncture is made in the wall **238** of the right atrium into the left atrium **220**, allowing distal end **232** of catheter **230** to pass into the left atrium **220**.

[0240] **FIG. 17** illustrates one method of shrinking the diameter of the annulus. **FIG. 17** shows a metal wire ring **100** in place about the mitral valve annulus. The ring **100** may be initially secured at the trigone area **103** of the mitral valve annulus. The technique illustrated in **FIG. 17** may rely upon a catheter apparatus, such as depicted in **FIGS. 6 and 7** herein with an operative segment. At least limited linear translation of the catheter may be accomplished with an apparatus similar to that described in **FIG. 6**, although a guide catheter may also be manually inserted at least partially by the surgeon through percutaneous access via the femoral vein. The ring **100**, although depicted in a ring configuration in **FIG. 17**, can be first inserted through the catheter in a straightened configuration. The metal wire or ring **100** is preferably constructed of a material such as Nitinol. The characteristics of this material include the ability to retain its form or to be stretched to a straight position. Once the material is passed through the catheter, it can spring back to its ring configuration. The surgeon preferably matches the configuration of the ring, particularly as to its size, to provide a proper fit for the particular mitral valve that is being repaired.

[0241] Once the straightened wire **100** has passed through the catheter, it assumes the position shown in **FIG. 17**. The ring, once in place, is secured to the annulus via wire clips **106** and/or sutures **102**. By drawing on these sutures with the

tool, the diameter of the mitral valve annulus is reduced so that it conforms to the size of the wire loop **100**. As with other techniques described herein, the control is supplemented by visual considerations such as with the use of ultrasound or electrophysiological feedback.

[0242] **FIG. 18** provides another embodiment of the present invention employing a catheter system for mitral valve repair. **FIG. 18** provides a schematic representation of a ring **210** of a cardiac valve, such as a mitral valve. Fiber **212** is looped about or sewn around the annulus (base) of the valve. A number of different types of stitches may be used. The fiber may be a thread or a wire. In the embodiment of **FIG. 18**, the fiber is actually sewn through the annulus of the valve. After the fiber is sewn in this manner, tension is applied to ends **214** of the fiber. The tightening reduces the diameter of the ring, brings the valve leaflets into their proper position so as to avoid valve regurgitation.

[0243] **FIG. 20** also illustrates a balloon **234** that may be supported at the distal end **232** of the catheter **230**. Once the catheter **230** is in place, balloon **234** is inflated to further support the guide catheter in place with the end **232** extending slightly into left atrium **220**. Once balloon **234** is inflated or opened, it can be snugged back against the septal wall **238** between left atrium **220** and right atrium **221**. The inner diameter of the catheter **230** may be on the order of approximately 5 mm in diameter. **FIG. 24** shows an enlarged view of catheter **230**, with its end **232** and the associated balloon **234** holding catheter **230** in place.

[0244] As an alternate to the use of a balloon **234**, a malecot **236** may be used. This is a mechanical device with expandable wings, as illustrated in **FIG. 25** and associated with catheter **230** so as to hold the end **232** of the catheter in place relative to the septal wall **238**.

[0245] **FIG. 20** also illustrates a flexible catheter **240** with its associated tool **242** extending from the guide catheter **230**. Tool **242** may be a pair of jaws operable for threading or sewing fiber. These jaws can be controlled externally at a user interface by a surgeon. With regard to flexible catheter **240**, reference is made to co-pending provisional application, U.S. Ser. No. 60/269,200, as well as pending application PCT serial No. PCT/US00/12553, filed Nov. 16, 2000, both documents of which are hereby incorporated by reference herein.

[0246] In **FIG. 23** reference is also made to the fiber **212** and an end piece **245** that is secured to one end of the fiber **212**. Fiber **212** is shown sewn through wall **247**. **FIG. 23** also schematically illustrates the tool **242** engaging the fiber **212**.

[0247] After guide catheter **230** is in place with the balloon **234** inflated to secure it in position, flexible catheter **240** is threaded through guide catheter **230** to a position just about the mitral valve, as illustrated in **FIG. 20**. Fiber **212** may also, at the same time, be threaded through the catheter member **230** with end piece **245** being accessible for being secured to the valve ring. As illustrated in **FIG. 20**, the beginning position of the threading or sewing of the fiber **212** is at a position close to or at the trigone area **215** of mitral valve **210**.

[0248] After a single threading or sewing has occurred, such as in **FIG. 23**, then the jaws of tool **242** loop stitch the fiber **212**, which may be a small but rigid wire, about the

mitral valve in the manner illustrated in **FIG. 18**. Staples **249** may also be employed for holding the wire in place.

[0249] **FIGS. 21 and 22** illustrate another embodiment to secure an end of fiber **212**. In this embodiment, the end of fiber **212** is pulled so as to close the diameter of the base ring of the mitral valve. **FIG. 21** illustrates guide catheter member **230** at its end **232**, being held in place against the septal wall **238** by balloon **234**. Flexible catheter **240** with its tool **242** has been withdrawn from catheter member **230**. Double-walled structure **250** comprises coaxially arranged inner and outer tubes **252** and **254**. Fiber **212** extends through these tubes and carries therealong a securing piece **256** and a retaining button **258**. The inner tube **252** is adapted to engage the retaining button **258** and the outer tube **254** is adapted to engage the securing piece **256**. **FIG. 22** shows securing piece **256** and retaining button **258**, along with the fiber **212**.

[0250] Initially, once the threading through the base of the valve ring is completed, the outer tube **254** engages securing piece **256** moving it downwardly in the view of **FIG. 21** while the fiber **212** is held in position. This tightens the securing piece **256** against the other side of the trigone area **215**, of **FIG. 20**. Once the diameter of the ring has been tightened, inner tube **252** is moved downwardly to engage retaining button **258**. Button **258** grabs fiber or wire **212** and at the same time retaining button **258** engages and interlocks with the securing piece **256**. In this way, both ends of the threaded fiber or wire **212** are secured roughly at the positions illustrated in **FIG. 20**. The pulled fiber **212** causes the mitral valve ring to draw into a smaller diameter such as the position shown in solid, rather than the in-dotted position of **FIG. 20**.

[0251] Once the securing piece and the retaining button are firmly held to the wire **212**, then the member **250** may be withdrawn through the guide catheter **230**. The flexible catheter member **240** may then be reinserted with a different tool such as a pair of scissors for cutting the exposed end of the fiber **212**.

[0252] Another possible technique for reducing the annular diameter involves a loop of cable that extends through hooks or anchors placed in the annulus, as illustrated in **FIG. 29**. **FIG. 29** shows the cable or wire **120** and schematically illustrates the anchors at **125**. In this technique the valve is reduced through a "lasso" technique, in which the cable exerts an equal force on all of the anchors. This technique uses an articulate catheter preferably inserted through a guide catheter, such as illustrated hereinbefore, to place the anchors one at a time into the mitral valve annulus. The cable onto which the anchors are suspended provides the closing force when tensioned by the operator.

[0253] In one embodiment, the flexible instrument comprises a guide catheter **150**, as illustrated in the diagram of **FIG. 30**. Inner catheter **155** houses an anchor and cable system depicted generally at **160**, including tensioning cable **162** and anchors **164**. Five degrees-of-freedom are provided: (1) rotary, (2) linear, (3) flexure motion with regard to the guide catheter **150** as well as (4) linear and (5) rotary motion with regard to the inner catheter **155**.

[0254] Guide catheter **150** may be approximately 8 French in diameter with a computer controlled flexible end portion, illustrated in **FIG. 30** as operative segment O. A computer

controls three degrees-of-freedom with regard to the guide catheter **150**, along with two degrees-of-freedom of inner catheter **155**. Refer to **FIG. 30** and the corresponding motions F1-F5.

[0255] **FIG. 30** depicts anchors **164** as having a loop and two legs, although other anchor designs can be readily contemplated. The legs of each anchor **164** may curl outwards. Once anchors **164** are deployed from the constraint of the inner catheter, they curl outwardly. The curling motion of the anchor legs secures them to the fibrous tissue of the mitral valve annulus. Preferably the anchors are fabricated from a super-elastic material such as Nitinol.

[0256] A tensioning cable, such as the cable or wire **162** illustrated in **FIG. 30** may pass through each of the loops of the anchor. This allows an equal force to be placed on each anchor and prevents the anchors from becoming loose in the bloodstream. The tensioning cable passes back through the robot inner catheter and out of the patient. The final tension is adjusted manually by the surgeon (or by computer) to optimize the annular size under direct visualization. Also, within the inner catheter is preferably disposed a deployment wire used to advance and fire the anchors into the annulus wall.

[0257] **FIGS. 30A and 30B** depict a cable termination tool set. This set comprises two catheters used to: (1) crimp the end of the tether cable once the tension is placed on the annulus; and (2) cut off the remaining cable at the end of the procedure. Both of these catheters may use a fourbar linkage or other system.

[0258] **FIG. 30A** shows a crimp tool **172** having a pair of jaws **174** that can be used to crimp member **176** about the tether cable **170**. Thus, the first catheter **172**, which may be referred to as a cable crimper, holds the crimp element **176** in the jaws **174** with the tether cable **170** pre-threaded through the crimp element and catheter shaft. The tensioning of the cable may be performed under ultrasound guidance. Although one tether cable **170** is shown in **FIG. 30A**, opposite ends of the tether that come from the mitral valve site preferably extend through the crimp element **176**. Once the tether cable is tensioned, so as to bring the mitral valve into its proper diameter, then the crimp element **176** is actuated by the cable crimper **172** illustrated in **FIG. 30A**. Once the proper tension is achieved, the crimper is actuated by applying tension on the push-pull drive cable **175** and by closing the crimp element at the jaws **174** so that the crimp element crimps the tether cable **170** in the proper position and at the proper tension.

[0259] After the crimping or securing step, then the cable crimper is removed and the cutting catheter **182** is introduced as also illustrated in **FIG. 30B**. This catheter is also introduced over the tether cable **170** and through the guide catheter. It is advanced up to the crimp, and severs the cable with its jaws **184** by tensioning the push-pull drive cable **185**. The procedure is now completed and the system catheters are then removed.

[0260] As indicated previously, the proximal end of the catheter is comprised of a disposable coupling mechanism that engages a drive mechanism, such as is shown in **FIGS. 6 and 7**. For this purpose, the coupler, identified in **FIGS. 6 and 7** as couplers **24** and **26** are adapted for disengagement therebetween. One coupler section may be considered as

transmitting motion to the guide catheter while the other coupler section may be considered as transmitting motion to the inner catheter and the drive cable. This involves the mechanical coupling of the guide catheter with the coupler so that actions of the guide catheter are controllable from the mechanical control elements of the coupler.

[0261] In one embodiment, a drive unit is coupled with the inner shaft and the guide shaft independently, the drive unit capable of independently effecting movement of each shaft to at least one degree of freedom.

[0262] For each coupler element, rotary disks transmit motion from the remotely controlled drive system to the catheter articulations. By way of example, in a first coupler element, a horizontal disk may drive the distal flexure. Another element may include disks, which control the axial and/or rotary positions of the inner catheter and, for example, the advance of the anchors. All of the coupling elements are mounted on a slider or sliders, which allows independent control of the linear advance of the outer and inner catheters. Again, refer to FIGS. 6 and 7. The catheter system including the inner and outer portions, as well as the proximal coupling element are disposable and mount removably to the drive member.

[0263] In accordance with the technique, such as described in FIG. 29, when the last anchor is in place, the inner robot catheter and deployment wire are removed. The physician can manually (or under computer control) adjust the tension in the cable and thus the diameter of the mitral valve after the first element of the cable termination system is threaded over the cable and through the robot guide catheter. Since this procedure is performed on a beating heart, the annular size can be optimized under direct ultrasound guidance. Once the mitral valve annulus has been precisely adjusted, a cable termination system, such as the one depicted in FIGS. 30A and 30B, clamps and cuts the cable. This completes the mitral valve repair procedure.

[0264] Another feature of the present invention provides a system for closing the base of a cardiac valve, such as a mitral valve. The closing can occur primarily by a stapling technique in which staples are attached to the valve ring or annulus to draw the annulus into a smaller diameter. In this way the leaflets are then more appropriately positioned for opening and closing.

[0265] FIG. 31 illustrates a staple array comprising delivery system 342 including storage housing 349 for a plurality of staples 350. Each of staples 350 is a surgical staple movably mounted within housing 349. Cable or wire 312 interconnects and loops through each of staples 350. Each staple 350 includes a pair of pointed ends 351 and center loop 353. The staple 350 at the most distal end of housing 351 (i.e. nearest the exit of housing 351) has cable 312 attached fixedly at loop 353, to prevent losing staples in the subject. For the remaining staples, cable or wire 312 freely loops through center loop 353. A release mechanism, not illustrated in FIG. 31, but which may be a standard design, can be used to move staples 350, one at a time, out of the housing 349. FIG. 31 also schematically illustrates a clamping mechanism 352 at the distal end of housing 349, for closing each of staples 350 as they exit housing 349.

[0266] FIG. 32 illustrates another method for repairing a mitral valve, featuring the use of staples to secure a ring to

the mitral valve annulus. As will be described in further detail, a tether cable or filament is threaded through an array of staples or anchors via a first inner catheter. Once the attachment anchors are placed around the annulus, the first inner catheter is removed and a second inner catheter is disposed in the guide catheter. This second inner catheter allows the clinician to apply tension to the cable to reduce the mitral valve annulus circumference, in effect, pulling on a lasso. The annuloplasty is monitored by real-time echocardiographic quantitation of regurgitant flow attenuation, with and without after-load reduction. The clinician monitors the cardiac physiology for resolution of regurgitation. When the hemodynamics are optimized, still a further inner catheter device may be used so as to place a stop or crimp on the cable. Still another inner catheter device may be used to cut the cable. These latter two inner catheter devices may be robotic or non-robotic catheters.

[0267] FIG. 32 features mitral valve 210 with trigone area 215. Guide catheter 330 accesses the vena cava and passes to the right atrium 221. This access may be from above via the jugular vein or below by way of the femoral vein. A puncture is made in septal wall 238 separating right atrium 221 from left atrium 220, allowing distal end 332 of guide catheter 330 to access left atrium 220.

[0268] Balloon 334 may be supported at distal end 332 of guide catheter 330. Once guide catheter 330 is positioned at a desired location, balloon 334 is inflated to secure guide catheter 330 to the wall with end 332 extending into the left atrium. Once balloon 334 is inflated, it can be snugged back against the septal wall between left atrium 220 and right atrium 221. The inner diameter of the catheter 330 may be on the order of approximately 5 mm in diameter. As an alternative to balloon 334, a malecot may be used, i.e. a mechanical device having expandable wings capable of securing catheter 330 against septal wall 238.

[0269] Guide catheter 330 coaxially nests flexible catheter 340 and its associated staple delivery system 342. With regard to this catheter construction, reference is made to a co-pending provisional application, Serial No. 60/269,200 filed Feb. 15, 2001, as well as pending application PCT serial No. PCT/US00/12553, filed Nov. 16, 2000, both of which are incorporated by reference herein in their entirety.

[0270] After balloon 334 is inflated to secure guide catheter 330 in position, flexible inner catheter 340 is threaded through guide catheter 330 to a position just above mitral valve 210, as illustrated in FIG. 32. Delivery system 342, associated with inner catheter 340, also passes through catheter 330, holding fiber 312 and staples 350 to an area about the mitral valve.

[0271] FIG. 32 also illustrates fiber 312 tracing a circumference about annulus 211, terminating at two end locations 345 and 356. The area traced by fiber 312 and where the stapling occurs is at a ring of relatively tough tissue just above the top of leaflet 213. The area not traced by fiber 312 is valve trigone area 215, which is relatively fixed and not easily contracted. Thus, the repair of the mitral valve, involving decreasing diameter 217 from dotted line to solid line, occurs away from trigone area 215.

[0272] Flexible catheter 340 is manipulated to cause a stapling about annulus 211 of mitral valve 210. The releasing of each staple is controlled by a mechanism preferably

within flexible catheter **340** and operable from a user interface station remote from the subject. Once all of the stapling has occurred, wire **312** is pulled in the direction of arrow **361** in **FIG. 32**. This pulling causes a closure of valve annulus **211**, as desired. Once the clinician is satisfied that the repair is complete, the cable **312** is then locked off with a crimp, such as illustrated at **365** in **FIG. 33**. This crimp may be facilitated by the insertion of a different catheter member **340** within the catheter **330**, all while the cable **312** is held in the proper cinched-down position.

[0273] A plurality of staples **350** having loops **353** encircling fiber **312**, secures fiber **312** to the annulus of the mitral valve, terminating at points **345** and **356**. The procedure of looping fiber **312** and stapling can be performed via remote control from a master station under surgeon control with multiple degrees-of-freedom of the tool so as to accurately locate the implant fiber **312** and staples **350**.

[0274] Fiber **312** is fixedly secured to end staple **350** at point **345**. The remaining staples are free to glide along fiber **312**. When all the staples are secured about the annulus, fiber **312** may be cinched down under ultrasonic guidance, watching for a reduction or elimination of the valve regurgitation. Once adequate tension has been placed on the cable **312**, tension can be maintained without disengaging the closure system. This allows the clinician to monitor the patient for some period of time to confirm that the repair has taken place. Once the clinician is satisfied with the repair, the cable can be locked off with a crimp or by some other technique and the cable may then be cut.

[0275] Another feature of the present invention is that the technique can be performed under physiologic conditions. The physician can monitor the procedure by, for example, transesophageal echocardiography, instead of a video image. The aforementioned "lasso" technique enables real-time assessment of the correction of the mitral valve regurgitation (MR) as the "lasso" is tightened. This enables performance of intra-operative provocative cardiac testing, with preload and afterload challenges and cardiac pacing all under transesophageal echo and trans-thoracic ultrasound guidance to optimize repair.

[0276] **FIG. 33** illustrates an expanded view of the finished repair region. A staple **350** is fixedly attached to fiber **312** at position **345**. Pulling cable **312** through various loops **353** of staples **350** causes pulling of the annulus into a smaller diameter, thus closing the valve from an initially larger diameter, dotted outline **217**, to a smaller diameter, solid outline in **FIG. 32** at **217**.

[0277] An alternate embodiment of a staple is illustrated in **FIG. 34**. Staple **362** may be an elastic-like staple, such as a nitinol staple. Staple **362** is normally biased to a closed position. A delivery system employs rod **364**, or the like, to hold staple **362** open. As the rod is moved longitudinally to the array, each staple in sequence is sprung closed. Such an arrangement would avoid the necessity of a clamping mechanism **352** as illustrated in **FIG. 31**.

[0278] **FIGS. 35A and 35B** illustrate other embodiments of an outer catheter **550** and an inner catheter **554** extending through septal wall **560**. These embodiments illustrate the outer (guide) catheter as a robotic catheter. It is understood that the instrument embodiments of **FIGS. 20 and 32** may also encompass systems where the guide shaft is robotic. In

FIG. 30, the guide catheter is also robotic. In **FIGS. 35A and 35B**, arrow **557** indicates rotation of outer catheter **550**, and arrow **559** indicates flexing of outer catheter **550**. In **FIGS. 35A and 35B**, inner catheter **554** can experience linear motion along the co-axis (arrow **562**) and rotational motion (arrow **564**). The outer catheter **550** may also be capable of independent linear translation. **FIG. 35A** illustrates inner catheter **554** as being capable of a controlled flex or bend, i.e. inner catheter **554** has a controlled flexible segment. Thus, the inner catheter of **FIG. 35A** is capable of deflecting in the direction of arrow **566**.

[0279] **FIG. 38** illustrates another embodiment of a catheter. Catheter **402** supports dumbbell-shaped balloon **414**. As illustrated in **FIG. 39**, catheter **402** can be introduced into the left ventricle **218** directed upwardly with balloon **414** disposed at mitral valve **210**. The mitral valve **210** separates the left ventricle **218** from the left atrium **220**. As shown in **FIG. 39**, associated with the mitral valve is a ring of relatively tough tissue (the annulus) just above the top of valve leaflets **213**.

[0280] **FIG. 36** shows a cross-sectional view of the use of catheter **402** and balloon **414** for mitral valve repair. **FIG. 36** shows the plurality of peripherally disposed anchor pins **405**. **FIG. 36A** shows each anchor pin comprising a piercing end **426** and a loop end **428**. A fiber or tether **408**, as illustrated in **FIGS. 36 and 37** extends through each of the loop ends **428** and has its ends at **409** free to extend through the catheter **402** to an external site where the tether can be tightened, as will be described in further detail hereinafter.

[0281] **FIG. 37** also shows the position wherein pins **405** have been inserted into wall **247**, which is a section of the ring of the mitral valve just above the leaflets. Pulling tether ends **409** together can close the ring, thus pulling loop ends **428** into a smaller diameter. This smaller diameter reduces the diameter of the ring of the mitral valve so as to minimize or prevent valve regurgitation.

[0282] Initially, **FIGS. 38 and 39** illustrates balloon **314** positioned at a desired location and in a deflated state. **FIG. 38** illustrates pins **405** disposed about a center section of balloon **414**. In the rest or deflated position as illustrated in **FIG. 38**, the pins disposed at their most inner diameter. This innermost diameter state is also represented in the cross-sectional view of **FIG. 36**. Tether **408** may extend by way of catheter **402** to an external site where it can be operated, e.g. outside the body.

[0283] Once the catheter and balloon are in place, such as illustrated in **FIG. 39**, the balloon is inflated by a balloon inflation lumen in the direction of arrow **439** in **FIG. 40**. Arrangements for inflating balloons are well known and are practiced, for example, in the angioplasty field. Inflation pressure may be coupled by way of the port **441** to the interior of balloon **414** causing the balloon to expand. In **FIG. 40** the balloon is shown only partially expanded. When fully expanded, the anchor pins **405** extend to the ring just above the leaflets as indicated at **445** in **FIG. 40**. The corresponding cross-sectional view is shown in **FIG. 37**, depicting the anchor pins **405** penetrating and anchoring the tissue. **FIG. 37** illustrates a placement of tether ends **409**. As the trigone portion of the base ring of the mitral valve is the most stable portion of the ring, it is preferred that tether ends **409** leave the loop at approximately the trigone area. In this way the drawing in of the diameter of the ring is more effective.

[0284] After the anchors are seated, as illustrated in FIG. 37, tether 408 can be tightened, thereby pulling the tissue together so as to repair the mitral valve and reduce or eliminate valve regurgitation.

[0285] Several different techniques may be used for guiding the catheter 402. For example, transesophageal ultrasound or transthoracic ultrasound may be employed. Also, radiopaque dye fluoroscopy or electrophysiologic techniques may be employed for positioning of the catheter.

[0286] The tether can be placed about the mitral valve and tightened by using coaxial inner and outer catheters. The concepts illustrated in FIGS. 39 and 40 may be practiced either with or without robotic control.

[0287] The aforementioned techniques for guiding the catheter may also be used for monitoring the effectiveness of the technique of the present invention. By monitoring the positioning of the balloon, one can assure that the ends of the tether are preferably at the trigone area. Also, as the tether is tightened, the surgeon may monitor the mitral valve activity to determine whether the valve base ring has closed properly so as to reduce or eliminate valve regurgitation. Tether ends may be secured by knotting the ends thereof so as to hold the tether in a closed position.

[0288] The techniques described herein may also be applied in other medical procedures involving repair of other anatomic body members. For example, the techniques described in FIGS. 17-40 may be used in closing, tightening, or constricting other anatomic conduits including, but not limited to, lumens, valves, or sphincters. One example is in connection with drawing the sphincter into a smaller diameter. This smaller diameter is particularly useful in controlling "acid reflux" by constricting an expanded sphincter that couples between the stomach and esophagus. By tightening the sphincter, stomach acids are restricted to the stomach and don't pass back toward the esophagus. Access for such a technique may be via the patient's mouth. Of course, the techniques of the invention may also be applied in virtually any other medical procedures performed internally on the patient.

[0289] The present invention provides a relatively simple system, both in the construction and in its use. The capability to decouple components at the drive unit and the receiver results in a readily portable and readily manually insertable flexible instrument system that can be handled quite effectively by the surgeon or assistant when it is to be engaged with the patient. Only a minimal number of components are positioned within the sterile field, enabling facile manipulation about the surgical site. An advantage of the system of the present invention is the decoupling nature of the system. In the system of the present invention, the instrument, drive unit and controller are inherently decoupled (attachable and detachable). The decouplable design enables the slave station to be readily portable. The instrument can be maintained as sterile but the drive unit need not be sterilized.

[0290] The instrument of the present invention is relatively small because the actuators are not housed in any articulating structure in the system of this invention. Because the actuators are remote, they may be placed under the operating table or in another convenient location and out of the sterile field. Because the drive unit is fixed and stationary, the motors may be arbitrary in size and configu-

ration. Finally, the design allows multiple, specialized instruments to be coupled to the drive unit, allowing a user to design the instrument for particular surgical disciplines.

[0291] Having now described a limited number of embodiments of the present invention, it should now be apparent to those skilled in the art that numerous other embodiments and modifications thereof are contemplated as falling within the scope of the present invention.

1. A surgical instrument comprising:

a shaft having at least one controllably flexible segment and a tool mounted at a distal end of the shaft, the tool being insertable into a subject;

a shaft mount drivably coupled to the shaft at a proximal end of the shaft, the shaft mount being drivably coupled to the tool through the shaft; and

a drive unit drivably coupled to the shaft mount, the drive unit being operable from a location remote from the subject to control flexure of the flexible segment so as to control disposition of the tool at an operative site.

2. The instrument of claim 1, wherein the shaft, the shaft mount, and the tool are constructed and arranged as a single piece disposable unit.

3. The instrument of claim 1, further comprising a receiver intercoupled with the drive unit, the shaft mount being readily mountable on the receiver for drivable intercoupling of the shaft mount with the drive unit.

4. The instrument of claim 3, wherein the drive unit is engageable with and disengageable from the receiver, the drive unit being portable.

5. The instrument of claim 1, wherein the shaft mount and the receiver are engageable with and disengageable from each other.

6. The instrument of claim 1, wherein the shaft, the shaft mount, and the tool are constructed and arranged as a single piece portable unit.

7. The instrument of claim 1, including a cabling pathway extending from the drive unit to the flexible segment, for actuation of controlled bending at the flexible segment by the drive unit.

8. The instrument of claim 1, including a cabling pathway extending from the drive unit to the tool, for actuation of the tool by the drive unit.

9. The instrument of claim 8, wherein the shaft supports the tool via a wrist, the wrist being pivotable.

10. The instrument of claim 1, wherein the flexible segment comprises a series of slots defining spaced ribs.

11. The instrument of claim 1, further comprising a receiver for engaging the shaft mount, the receiver supported by a carriage slideably engaging rails controlled to translate the shaft toward and away from the operative site.

12. The instrument of claim 1, wherein the shaft is an inner shaft, the instrument further comprising a guide shaft for coaxially receiving the inner shaft, the guide shaft capable of disposing the tool at the operative site.

13. The instrument of claim 12, wherein the guide shaft also has at least one flexible segment, the bending of which is remotely controllable.

14. The instrument of claim 1, wherein the shaft is remote controllably drivable by a user via a manually controllable input device remote from the subject.

15. A remotely controllable surgical instrument, comprising:

- a user input device, for inputting a command;
- a slave station for receiving the command from the input device, the user input device being remotely disposed from the slave station, the slave station further comprising a mechanically drivable mechanism comprising a shaft having a proximal end, a distal end supporting a tool and a flexible portion between the proximal and distal ends; and

an electronic signal link between the user input device and the slave station, the command from the input device being communicated via the link for controlling bending of the flexible portion so as to controllably position the tool at an operative site of a subject.

16. The instrument of claim 15, further comprising a plurality of motors coupled to the controller and drivably coupled to the shaft, for controlling at least one degree of freedom of the flexible segment.

17. The instrument of claim 15, further comprising cables extending between the proximal and distal ends of the shaft.

18. The instrument of claim 17, wherein the electronic signal link activates the cables to effect flexure of the shaft at the flexible segment.

19. The instrument of claim 15, wherein the shaft is an inner shaft, the instrument further comprising an outer shaft.

20. The instrument of claim 15, wherein said master station includes a user interface manipulated by a user, and the electronic signal link is provided by a computer system responsive to the user interface manipulations, and the slave station further comprises a drive unit coupled from the computer system to the shaft for controlling actuation of the shaft.

21. A remotely controllable catheter comprising:

- a tube having a proximal end and a distal end, at least a segment of the tube being controllably flexible;
- a drivable bending mechanism mechanically coupled to and interactive with the controllably flexible segment of the tube; and
- a computer remote from and interconnected to the bending mechanism, the computer having a program receiving input from a user, and the program directing the bending mechanism to controllably flex the flexible segment of the tube according to the user input.

22. The catheter of claim 21, wherein:

the bending mechanism comprises a cable extending from the flexible segment and a motor mechanism;

the motor mechanism is interconnected to the computer; and

the cable being driven by the motor mechanism to direct bending of the flexible portion according to the user input.

23. The catheter of claim 21, further comprising a user input device interconnected to the computer, the user input device being remotely mounted relative to the tube and adapted to receive the user input, the program processing the commands capable of directing movement of the bending mechanism according to the user input.

24. A catheter, comprising:

- a shaft having proximal and distal ends and at least one flexible segment along a length of the shaft, the distal end being insertable within a body cavity or vessel;

a tool supported at the distal end of the shaft for performing a medical procedure;

at least two cables extending along the shaft between the proximal and distal ends, at least one of the cables associated with the flexible segment of the shaft and at least another of the cables associated with the tool;

an electronic control mechanism drivably coupled to the cables, the electronic control mechanism capable of communicating drive signals from a user input device to the cables to effect bending of the flexible segment and operation of the tool.

25. The catheter of claim 24, wherein the flexible segment comprises a deformable material, at least one of the cables exerting a pulling or pushing force on the flexible portion of the shaft to effect controlled deformational bending of the flexible portion of the shaft.

26. The catheter of claim 24, wherein the shaft is an inner shaft and the catheter further comprises an outer shaft, the inner shaft being coaxially insertable into the outer shaft.

27. The catheter of claim 24, wherein the flexible segment comprises a coiled section.

28. The catheter of claim 26, wherein the at least one cable associated with the flexible segment is operable to bend the shaft at the flexible segment.

29. The catheter of claim 28, wherein the at least one cable is secured to an outer surface of the shaft between the flexible segment and the distal-most point of the shaft.

30. The catheter of claim 29, wherein the at least one cable extends along the shaft from the secured point to the proximal end.

31. The catheter of claim 28, wherein the at least one cable extends between the inner and outer shafts along the proximal shaft section.

32. The catheter of claim 28, wherein the proximal end of the shaft extends to a mechanically drivable mechanism comprising a first control element for controlling the at least one cable to bend the distal end of the shaft at the flexible segment.

33. The catheter of claim 32, further comprising a second control element that controls rotation of the outer shaft about the co-axis.

34. The catheter of claim 33, further comprising a third control element that controls rotation of the inner shaft about the co-axis.

35. The catheter of claim 34, further comprising a fourth control element associated with an actuating link to control rotation of the tool.

36. The catheter of claim 32, wherein the mechanically drivable mechanism, the shaft and the tool are constructed as a single piece unit that is disposable.

37. The catheter of claim 32, wherein the mechanically drivable mechanism engages a receiver which is supported by a carriage, the carriage slideably engaging rails to translate the catheter to and from the subject.

38. The catheter of claim 24, further comprising a user interface, wherein the electronic control mechanism couples the user interface to a drive unit remote from the body cavity or vessel, the drive unit capable of mechanically driving the at least two cables.

39. The catheter of claim 38, wherein manipulations at the user interface control operation of the tool.

40. The catheter of claim 39, wherein the tool comprises a pair of jaws and the user interface manipulations control the opening and closing of the jaws.

* * * * *