US00D710501S

(12) United States Design Patent

Hayman et al.

(10) Patent No.: US D710,501 S
(45) Date of Patent: ** *Aug. 5, 2014

(54) **RECEPTOR HOLDING DEVICE**

(71) Applicant: **Zuma Dental, LLC**, Los Angeles, CA (US)

(72) Inventors: **Robert Hayman**, Los Angeles, CA (US); **Ekram Khan**, League City, TX (US); **Michael Paloian**, Cold Spring Harbor, NY (US); **Anthony Orchard**, Wantagh, NY (US)

(73) Assignee: **Zuma Dental, LLC**, Los Angeles, CA (US)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **14 Years**

(21) Appl. No.: **29/449,990**

(22) Filed: **Mar. 15, 2013**

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/161**

(58) **Field of Classification Search**
USPC D24/158–161, 185, 186, 152, 176, 177; D8/394, 396; 378/38–40, 169–170, 378/177, 180, 191, 205
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D246,798	S	*	12/1977	Jermyn	D24/161
4,484,342	A	*	11/1984	Allison et al.	378/168
D283,157	S	*	3/1986	Maldonado et al.	D24/161
5,289,522	A	*	2/1994	Kanbar et al.	378/170
D370,732	S	*	6/1996	Smith	D24/176
5,652,779	A	*	7/1997	Levy et al.	378/170
D406,892	S	*	3/1999	Warren	D24/161
6,592,256	B2	*	7/2003	Da Rold et al.	378/168
D537,943	S	*	3/2007	Schmulenson	D24/158
7,871,199	B2	*	1/2011	Szommer	378/170
8,016,483	B2	*	9/2011	Steward, Jr.	378/170
8,573,844	B2	*	11/2013	Steward et al.	378/170
2006/0245549	A1	*	11/2006	Calderwood et al.	378/191
2010/0027756	A1	*	2/2010	Hof	378/170
2011/0299663	A1	*	12/2011	Steward, Jr.	378/170

* cited by examiner

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Quan & Associates; Nancy N. Quan; Christopher N. Quan

(57) **CLAIM**


The ornamental design for a receptor holding device, as shown and described.

DESCRIPTION

FIG. **1** is a back and side perspective view of receptor holding device embodying our new design;
FIG. **2** is a front and side perspective view thereof;
FIG. **3** is front view thereof;
FIG. **4** is a back view thereof;
FIG. **5** is a top view thereof;
FIG. **6** is a right side view thereof;
FIG. **7** is a bottom view; and,
FIG. **8** is a left side view thereof.

The break lines in the drawing views indicate that a specific length of the receptor holding device forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

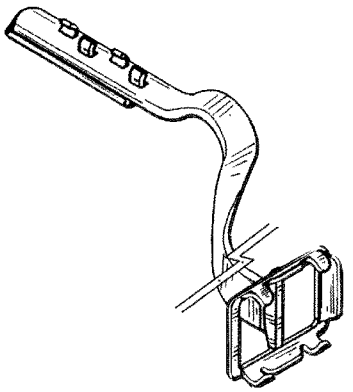

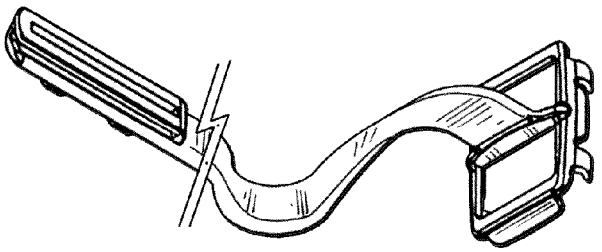


Fig.1

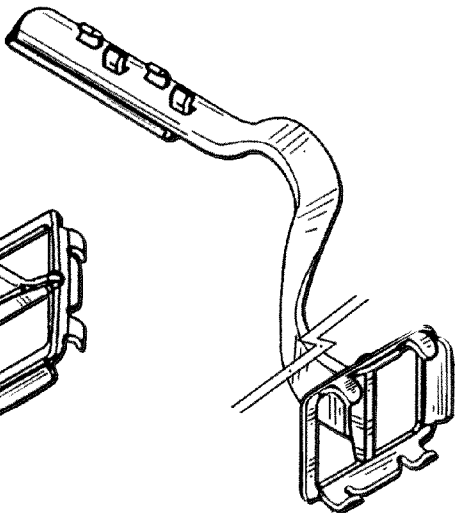


Fig.2

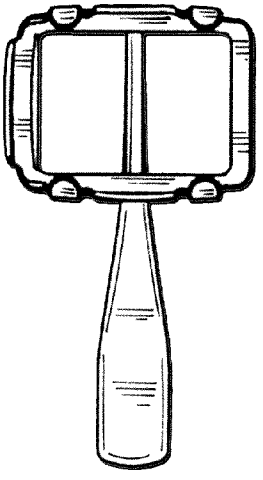


Fig.3

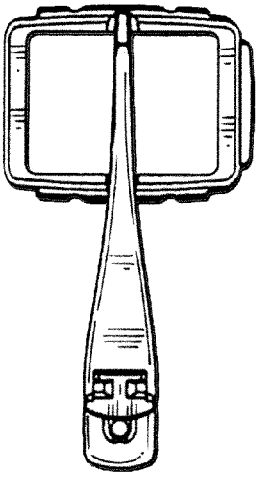


Fig.4

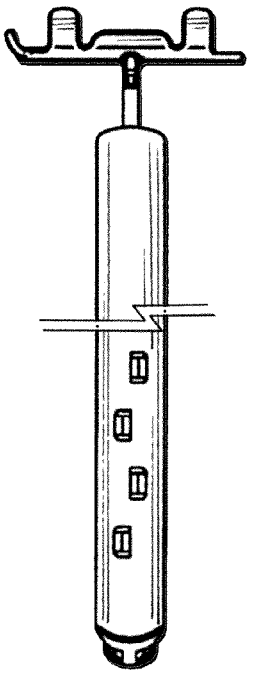


Fig.5

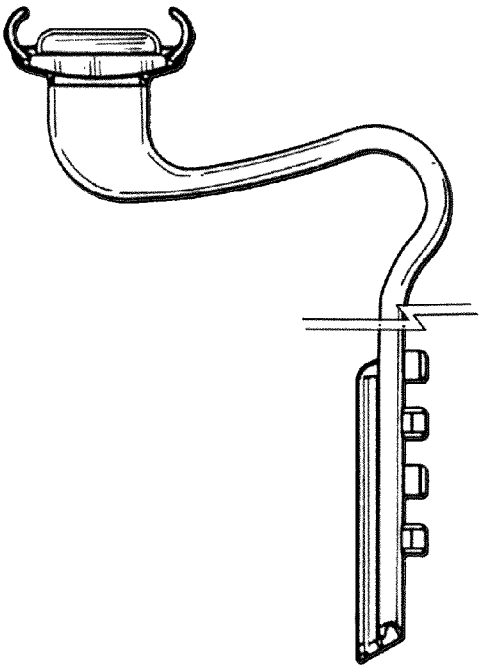


Fig.6

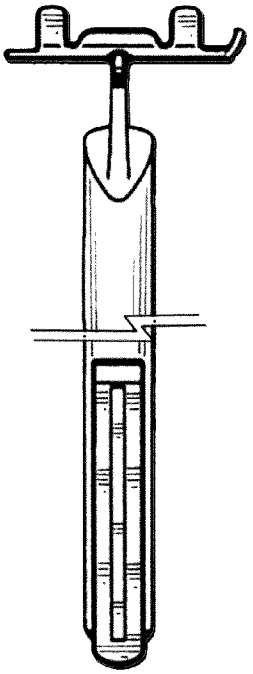


Fig.7

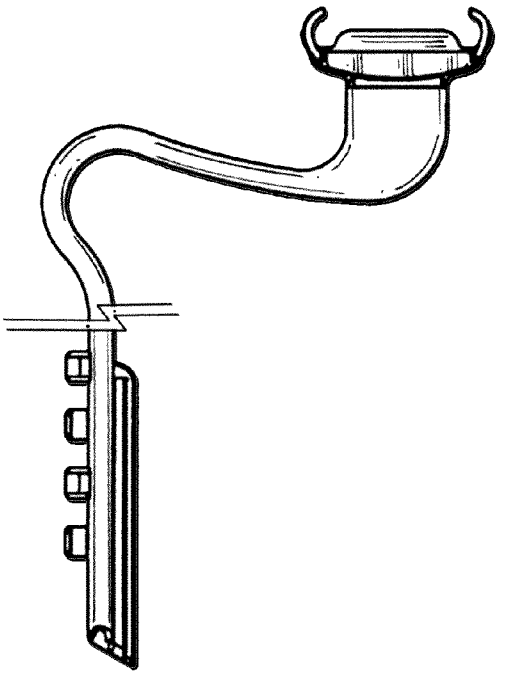


Fig.8