



(51) International Patent Classification:

A61N 5/10 (2006.01) A61G 7/10 (2006.01)  
A61B 6/04 (2006.01) A61B 5/055 (2006.01)

(21) International Application Number:

PCT/EP2017/077982

(22) International Filing Date:

01 November 2017 (01.11.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(71) Applicant: **ELEKTA LTD.** [GB/GB]; Linac House, Flem-  
ing Way, CRAWLEY RH10 9RR (GB).

(72) Inventors: **MINOZ, Alain**; Svartvikslingen 112, 167 39  
BROMMA (SE). **ELDERED, Kjell**; Kvarnbacken 10, 131  
50 SALSTJÖ-DUVNÄS (SE).

(74) Agent: **GROTH & CO KB**; P.O. Box 6107, 102 32  
STOCKHOLM (SE).

(81) Designated States (unless otherwise indicated, for every  
kind of national protection available): AE, AG, AL, AM,  
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,  
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,  
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,  
HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,  
KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,  
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,  
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,  
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,  
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every  
kind of regional protection available): ARIPO (BW, GH,  
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,  
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,  
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,

(54) Title: INDICATOR ARRANGEMENTS AND METHODS FOR SUCH ARRANGEMENTS

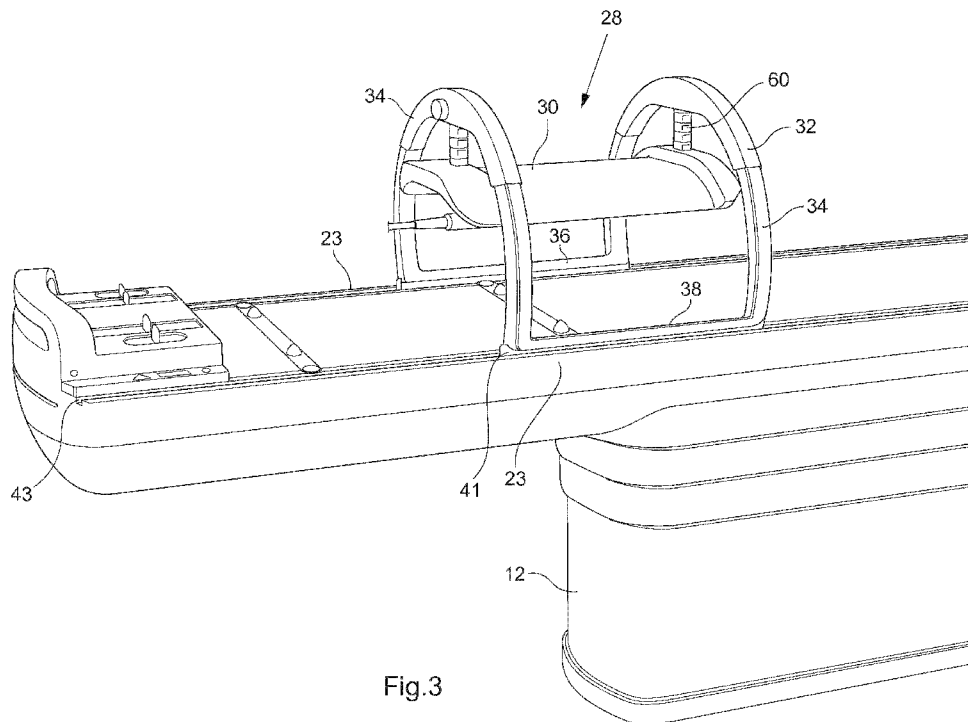


Fig.3

(57) Abstract: The invention relates to a position indicator for a system for moving a patient in a non-invasive therapy system, wherein the system for moving includes a patient support arranged outside a treatment space of a medical apparatus of the non-invasive therapy system, a treatment table arranged inside the treatment space in the medical apparatus, and a patient bed movable in a longitudinal direction from the patient support to the treatment table and back by means of activation of a transferring mechanism, wherein the position indicator comprises a number of light emitting elements arranged in the patient support and each being arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions for treatment equipment.



EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,  
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,  
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,  
KM, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

- *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))*
- *of inventorship (Rule 4.17(iv))*

**Published:**

- *with international search report (Art. 21(3))*

## Indicator arrangements and methods for such arrangements

### Technical field

The present invention relates to medical devices, and particularly to systems and devices for moving  
5 a patient to and from a magnetic resonance imaging system or a combined magnetic resonance  
imaging and radiotherapy system.

### Background

In medical non-invasive therapy system in particular radiotherapy systems, such as conventional  
linear accelerators or MR Linac systems, the patient anatomy being treated or imaged should be  
10 aligned with the radiation isocentre as accurate as possible for each and every set up and each  
treatment fraction. One source of potential inaccuracy in the alignment is the repositioning of the  
bed on which the patient rests. As many medical systems require the patient to be placed into an  
enclosed and confined space, hereinafter called treatment bore, the patient must be set up for  
treatment outside the treatment bore and then transported into the treatment bore for the medical  
15 treatment to begin. Therefore, the bed must be movable between these two locations and  
positionable to a high degree of accuracy as misalignment during set up may entail that the patient  
will need to be removed from the medical radiotherapy system and realigned before treatment can  
commence, and thus wasting time and resources.

It is also of very high importance that the patient positioning is as stable as possible during the  
20 movement as well during the treatment or imaging. Hence, the position of the bed in treatment bore  
in the medical radiotherapy system must be very stable. The process of moving the bed from its  
support outside the medical radiotherapy system into the treatment bore inside the medical  
radiotherapy system itself requires careful alignment with the treatment table of the system as well  
as high degree of stability.

25 Furthermore, it is also important that the process for patient set up and of moving the bed from its  
support outside the medical radiotherapy system into the treatment space inside the medical  
radiotherapy system is secure for the patient and easy to handle for the medical staff. The risk of  
patient injuries must be minimized during movement as well as during treatment in order to provide  
as high patient security as possible and minimize risk for patient movements during treatment.

30 Moreover, in medical non-invasive therapy systems, in particular in MR Linac systems, it is of very  
high importance that all material in the treatment bore or treatment volume is known and taken into

account in the planning system. As all material will absorb radiation dose, it is important to reduce the material present in the treatment bore as much as possible and it is also important that the positions of material structures are known.

5 It is further of very high importance that equipment having a position relatively the patient such as the coil frame as well as patient supporting structures including head support and support for the feet are positioned accurately on the table top or patient support. The operator must install the coil frame on table top at a certain position and there may be around 100 different positions. This is usually performed manually, which is time-consuming and also may entail positioning errors.

10 Due to the delivered radiation and performed imaging inside the bore, no electronic equipment can be used in the table top for indicating the position of, for example, the coil frame on the table top. On one hand, the imaging will most likely be influence and disturbed and, on the other hand, the radiation will likely shorten life-span of and/or destroy the electronic equipment.

15 In summary, there is a number of important factors to take into account when designing a movable bed and treatment table for use in medical radiotherapy systems, such as MR Linac systems. It is of particular importance to make sure that the equipment such as the coil frame, as well as the patient, is positioned very accurate. The accuracy require a very reliable positioning of the coil frame and the patient on the patient bed. In addition, there is a need for providing good quality imaging when tracking the patient. When using magnetic resonance imaging systems for this it is thus important to position the coil in a stable and accurate position while at the same time ensuring a good and  
20 efficient handling of the system during set up.

### **Summary of the invention**

An object of the present invention is to provide a user and patient friendly movable bed and treatment table for use in medical radiotherapy systems, such as MR Linac systems.

25 Another object is to provide a more efficient handling of the a medical radiotherapy systems, such as MR Linac system, during set up

These and other objects are fulfilled by the present invention as defined by the independent claims. Preferred embodiments are defined by the dependent claims.

Non-invasive therapy system may refer to a medical apparatus and include at least a magnetic resonance imaging system or a radiotherapy system or any combination thereof.

According to an aspect of the present invention, there is provided a position indicator for a system for moving a patient in a non-invasive therapy system, wherein the system for moving includes a patient support arranged outside a treatment space of a medical apparatus of the non-invasive therapy system, a treatment table arranged inside the treatment space in the medical apparatus, and a patient bed movable in a longitudinal direction from the patient support to the treatment table and back by means of activation of a transferring mechanism, wherein the position indicator comprises a number of light emitting elements arranged in the patient support and each being arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions for treatment equipment.

10 In embodiments of the present invention, the light emitting elements are arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions, in a longitudinal direction, where the treatment equipment is to be positioned at the patient support.

According to another embodiments of the present invention, the patient support is provided with a number of position markers and the position indicator comprises at least one light emitting element arranged at each position marker, wherein a position marker is lit up when a corresponding light emitting element is instructed to emit light.

15 In other embodiments of the present invention, the position markers includes a transparent or semi-transparent material and are arranged on a longitudinal edge part of the patient support and wherein the light emitting elements are arranged to individually emit light towards a respective position marker.

Further embodiments of the present invention comprises position markers including a transparent or semi-transparent material and wherein the light emitting elements are arranged to emit light towards a respective position marker.

25 According to embodiments of the present invention, the light emitting elements are arranged in an upper surface of the patient support.

In accordance with other embodiments of the present invention, the light emitting elements are arranged in a guide rail of the patient support.

In embodiments of the present invention, the light emitting elements are arranged to, upon receiving activation signals, to emit light according to a predetermined sequence and/or color.

30 In embodiments of the present invention, the treatment equipment includes a coil arrangement including an anterior coil and a support stand, the support stand resting on the patient bed adjacent

to longitudinal edges of the patient bed and being slidable along the patient bed in a longitudinal direction, wherein the light emitting elements are arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions where the coil arrangement should be positioned at along the patient support.

5 According to embodiments of the present invention, the treatment equipment includes patient positioning devices arranged to be positioned at the patient support, wherein the light emitting elements are arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions, in a longitudinal direction, where the patient positioning device should be positioned at the patient support.

10 In embodiments of the present invention, the light emitting elements are arranged to, upon receiving activation signals, to emit light according to a predetermined sequence and/or color, wherein a certain predetermined sequence and/or color is associated with a certain treatment equipment.

According to a further aspect of the present invention, there is provided a method for indicating a position in a system for moving a patient in a non-invasive therapy system, wherein the system for moving includes a patient support arranged outside a treatment space of a medical apparatus of the non-invasive therapy system, a treatment table arranged inside the treatment space in the medical apparatus, a patient bed movable in a longitudinal direction from the patient support to the treatment table and back by means of activation of a transferring mechanism, wherein the method  
15 comprises activating a position indicator comprising a number of light emitting elements arranged in the patient support, each being arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions for treatment equipment.  
20

According to embodiments of the present invention, the method further includes activating a position indicator comprising a number of light emitting elements arranged in the patient support, each being arranged to receive activation signals instructing a receiving light emitting element to emit light to indicate positions, in a longitudinal direction, where the treatment equipment it to be positioned at the patient support.  
25

In embodiments of the present invention, the patient support is provided with a number of position markers and the position indicator comprises at least one light emitting element arranged at each position marker, wherein the method comprises lighten up a position marker by instructing a  
30 corresponding light emitting element to emit light.

Further embodiments of the present invention comprises position markers provided with a transparent or semi-transparent material and are arranged on a longitudinal edge part of the patient support, wherein the method comprises individually emitting light towards a position marker from a corresponding light emitting element.

- 5 In accordance with embodiments of the present invention, the method further comprises providing activation signals to instruct the light emitting elements to emit light according to a predetermined sequence and/or color.

According to embodiments of the present invention, the treatment equipment includes a coil arrangement including an anterior coil and a support stand, the support stand resting on the patient  
10 bed adjacent to longitudinal edges of the patient bed and being slidable along the patient bed in a longitudinal direction, wherein the method further comprises providing activation signal to the light emitting elements instructing a receiving light emitting element to emit light to indicate positions, in a longitudinal direction, where the coil arrangement is to be positioned at the patient support.

In embodiments of the present invention, the treatment equipment includes patient positioning  
15 devices arranged to be positioned at the patient support, further comprising providing activation signals to the light emitting elements instructing a receiving light emitting element to emit light to indicate positions, in a longitudinal direction, where the patient positioning device is to be positioned at the patient support.

According to embodiments of the present invention, the method further comprises providing  
20 activation signals to the light emitting elements instructing a light emitting element to emit light according to a predetermined sequence and/or color, wherein a certain predetermined sequence and/or color is associated with a certain treatment equipment.

Preferred embodiments of the invention will now be described in relation to the drawings.

### **Brief description of the drawings**

25 For a better understanding of the present invention, and to show more clearly how it may be carried into effect, reference will now be made, by way of example, to the following drawings, in which:

Fig. 1 shows a plan view of a system in which the present invention can be used;

Fig. 2 shows a side view of the system in which the present invention can be used;

Fig. 3 shows a perspective view of the system in which the present invention can be used;

Fig. 4 shows a detailed view of the system shown in Fig. 3;

Fig. 5 shows a detailed view of a of an embodiment of the present invention; and

Fig. 6 shows a detailed view of another embodiment of the present invention.

## Description

5 With reference first to Fig. 1 – 3, a system in which the present invention can be used will be described. Figure 1 shows a plan view of a system 10 and Figure 2 shows a side view of the system of Figure 1. The system 10 comprises a patient support 12, a treatment table 14, and a bed 16 which is movable between the patient support 12 and the treatment table 14. The treatment table 14 is schematically shown in Figures 1 and 2 and may form part of any medical treatment system but is particularly suitable for use in MR Linac radiotherapy systems. Hence, in embodiments of the present invention, the system 10 is arranged at a MR Linac radiotherapy system having radiation heads and radiation sources for generating beams of therapeutic radiation emanating from the radiation heads. One or more collimating elements (e.g. a Multi-leaf collimator in the Linac part) are provided for shaping the beam to conform to a desired cross-section. The radiation heads may be mounted on a rotatable gantry, and controlled to rotate around the patient while directing the radiation towards the axis of rotation and the target within the patient. The target thus receives radiation from multiple angles and a higher dose than the surrounding healthy tissue. The extent of the treatment area 18, i.e. the volume in which the radiation beam operates, is illustrated schematically in Figures 1 and 2.

15 The patient support 12 may comprise a mechanism for altering the height of the support, for example, between a first height and second height. For example, the first (lower) height may be at a level suitable to allow the patient to climb on to the bed 16, while the second (higher) height is a level equal to the height of the treatment table 14 and allows the bed 16 to move between the support 12 and the treatment table 14.

20 The bed 12 may be moved in a direction along its longitudinal axis between the support 12 and the treatment table 14 in a manner to be described in more detail below. Those skilled in the art will appreciate that any suitable mechanism may be used for moving the bed 16. For example, the bed 16 may be moved by a pulley/belt system, a rack and pinion system, a conveyor belt, etc.

25 As described above, it is important that the bed can be smoothly transferred or moved between the support 12 and the treatment table 14 so that once on the table 14 the bed is correctly aligned within the system, which in many radiotherapy systems is crucial. In order to ensure that the bed 16 is correctly aligned during initial set-up and treatment, the system 10 may comprise guide elements

20a, 20b, 20c, 20d, arranged on an upper surface of the support 12. Alternatively, guide tracks may be arranged on an upper surface of the support 12 and treatment table 14 and corresponding guide rails may be arranged on the patient bed 16 such that the bed 16 can slide seamlessly between the support and the table.

5 In the illustrated embodiment, the patient support comprises four pairs of guide elements. However, fewer or more guide pairs may be provided without departing from the scope of the invention. The guide pairs may be uniformly spaced, along the edges of the support 12 so as to prevent the bed 16 from moving significantly in the lateral direction (i.e. up and down the page in Figure 1, and Figure 2).

10 In the embodiment illustrated in Figure 1 and 2, the guide elements are rollers which move over the edge of the bed 16 as the bed is moved in the direction along its longitudinal axis. However, those skilled in the art will appreciate that any suitable guiding element which provides a low friction surface along which the bed can travel without sticking may be provided as an alternative. Further, guides need not be identical, and a mix of different guides may be provided in the same system without departing from the scope of the invention.

15 The treatment table 14 may comprise a plurality of guide elements 24a, 24b, 24c, 24d, on an upper surface of the table, similar to the guide elements on the support 12.

With reference now to Fig. 3, a treatment equipment, such as a MR coil arrangement, arranged at the system 10 will be described. The MR coil arrangement 28 includes an anterior coil 30 and a support stand 32 is arranged to be slidable along the patient bed 16 in a longitudinal direction when  
20 a patient is placed on the bed 16. The support stand 32 rests on the patient bed 16 and is arranged adjacent to longitudinal edges 23 of the patient bed 16 and include rails 41 being arranged to be slidable in grooves or guide tracks 43 provided in the patient bed 16. The coil arrangement 28 may further comprise a height adjustment mechanism 60 for adjusting the height of the anterior coil 30 above the patient bed 16. The height adjustment mechanism 60 may enable an operator to adjust  
25 the height of the anterior coil 16 parallel to a plane defined by the patient bed 16 as indicated in figure 3 or it may enable an operator to adjust the anterior coil 16 in an oblique manner (not shown) as seen in relation to the plane defined by the patient bed 16.

Fig. 4 and 5 shows more detailed views of the patient support 12 and the patient bed 16. Position markers 55 are provided on the patient bed 16 arranged as numbers along an edge of the patient  
30 bed 16. In this embodiment, a position indicator 50 is arranged as an array of light emitting elements 51, in this example light emitting diodes, on upper surface 56 of the patient support 12. The array of light emitting elements 51 is arranged such that each light emitting element is in line with a

corresponding position marker 55 on the patient bed 16 when the bed 16 is placed in an end position or home position outside the treatment area 18 (see Fig. 3). According to an embodiment, shown in Fig. 5, the light emitting element 51 are arranged beneath an edge part 57 shaped as a hollow elongated part along longitudinal direction of the patient support 12. The edge part 57 includes transparent areas 58, each being aligned with a corresponding position marker 55 and a corresponding light emitting element 51, when the patient bed is placed in the end position. The light emitting elements 51 are each arranged to receive activation signals instructing a receiving light emitting element 51 to emit light to indicate a position of, for example, the coil arrangement 28. However, other parts such as a head pillow, neck support, feet support for the patient may also be indicated by the light emitting elements 51.

In embodiments, the light emitting elements 51 are arranged to upon receiving activation signals to emit light according to a predetermined sequence and/or color. Thereby, for example, the position of a certain treatment equipment such as the coil arrangement or patient position device, e.g. feet, knee or neck support devices, can be indicated by a light emitting element 51 emitting light according to a first specific sequence and/or color, a position of a neck support with another light emitting element 51 emitting light according to a second specific sequence and/or color, and a position of a feet support with yet another light emitting element 51 emitting light according to a third specific sequence and/or color.

In embodiments, the light emitting elements 51 are controlled by a computer unit (not shown) to receive instructions or activation signal to, for example, emit light to indicate a position of a coil arrangement 28, emit light according to a predetermined sequence, and/or emit light according to a specific color.

With reference now to Fig 6, a further embodiment of the present invention will be discussed. In this embodiment, position markers 55 are provided on the patient bed 16 arranged along an edge part of the patient bed 16. A position indicator 60 is arranged as an array of light emitting elements 61, in this example light emitting diodes, on upper surface 56 of the patient support 12. The array of light emitting elements 51 is arranged such that each light emitting element 51 is in line with a corresponding position marker 55 on the patient bed 16 when the bed 16 is placed in an end position or home position outside the treatment area 18 (see Fig. 3). According to this embodiment, shown in Fig. 6, the light emitting element 51 are arranged in a guide rail 62 of the patient support 12 in which rails 63 of the patient bed 16 moves. The position markers 55 are made of a transparent or semi-transparent material, or are arranged as openings or holes in an elongated part 65 of the patient bed

16. When a light emitting element 51 receives an activation signal or instructions to emit light, it will emit light towards the respective position marker 55.

Although the above description relates to embodiments that is in the light of the present knowledge considered to be the most preferable, it is clear to a person skilled in the art that the invention can

5 be modified in many different ways within the scope defined by the appended claims.

10

15

20

## CLAIMS

1. A position indicator (50; 60) for a system for moving a patient in a non-invasive therapy system, wherein said system for moving includes a patient support (12) arranged outside a  
5 treatment space of a medical apparatus of the non-invasive therapy system, a treatment table (14) arranged inside the treatment space in the medical apparatus, and a patient bed (16) movable in a longitudinal direction from the patient support to the treatment table and back by means of activation of a transferring mechanism, wherein said position indicator comprises a number of light emitting elements (51; 61) arranged in said patient support (12)  
10 and each being arranged to receive activation signals instructing a receiving light emitting element (51; 61) to emit light to indicate positions for treatment equipment (28).
2. The position indicator (50; 60) according to claim 1, wherein said light emitting elements (51; 61) are arranged to receive activation signals instructing a receiving light emitting element  
15 (51) to emit light to indicate positions, in a longitudinal direction, where said treatment equipment (28) is to be positioned at said patient support (12).
3. The position indicator according to claim 1 or 2, wherein said patient support (12) is provided with a number of position markers (55) and said position indicator (50; 60) comprises at least  
20 one light emitting element (51; 61) arranged at each position marker (55), wherein a position marker (55) is lit up when a corresponding light emitting element (51; 61) is instructed to emit light.
4. The position indicator according to claim 1 – 3, wherein said position markers (55) includes a  
25 transparent or semi-transparent material and wherein said light emitting elements (51; 61) are arranged to emit light towards a respective position marker (55).
5. The position indicator according to claim 4, wherein said position markers (55) are arranged  
30 on a longitudinal edge part (58) of said patient support (12) and wherein said light emitting elements (51; 61) are arranged to individually emit light towards a respective position marker (55).

6. The position indicator according to claim 1 – 5, wherein said light emitting elements (51) are arranged in an upper surface (56, 58) of the patient support (12)
- 5 7. The position indicator according to claim 1 – 5, wherein said light emitting elements (61) are arranged in a guide rail (62) of said patient support (12).
8. The position indicator according to any one of preceding claims, wherein said light emitting elements (51; 61) are arranged to, upon receiving activation signals, to emit light according to a predetermined sequence and/or color.
- 10 9. The position indicator according to any one of preceding claims, wherein the treatment equipment includes a coil arrangement (28) including an anterior coil (30) and a support stand (32), the support stand (32) resting on the patient bed (16) adjacent to longitudinal edges (23) of said patient bed (16) and being slidable along the patient bed (16) in a longitudinal direction, wherein said light emitting elements (51; 61) are arranged to receive activation signals instructing a receiving light emitting element (51; 61) to emit light to indicate positions where said coil arrangement (28) should be positioned at along said patient support (12).
- 15 10. The position indicator according to any one of preceding claims, wherein the treatment equipment includes patient positioning devices arranged to be positioned at said patient support (12), wherein said light emitting elements (51; 61) are arranged to receive activation signals instructing a receiving light emitting element (51; 61) to emit light to indicate positions where said patient positioning device (28) should be positioned at along said patient support (12).
- 20 11. The position indicator according to claim 8, wherein said light emitting elements (51; 61) are arranged to, upon receiving activation signals, to emit light according to a predetermined sequence and/or color, wherein a certain predetermined sequence and/or color is associated with a certain treatment equipment.
- 25 12. A method for indicating a position in a system for moving a patient in non-invasive therapy system, wherein said system for moving includes a patient support (12) arranged outside a treatment space of a medical apparatus of the non-invasive therapy system, a treatment table (14) arranged inside the treatment space in the medical apparatus, a patient bed (16)
- 30 35

movable in a longitudinal direction from the patient support to the treatment table and back by means of activation of a transferring mechanism, wherein said method comprises:

activating a position indicator (50; 60) comprising a number of light emitting elements (51; 61) arranged in said patient support (12), each being arranged to receive activation signals instructing a receiving light emitting element (51; 61) to emit light to indicate positions for treatment equipment (28).

5

13. The method according to claim 12, including activating a position indicator (50; 60) comprising a number of light emitting elements (51; 61) arranged in said patient support (12), each being arranged to receive activation signals instructing a receiving light emitting element (51; 61) to emit light to indicate positions, in a longitudinal direction, where said treatment equipment (28) it to be positioned at said patient support (12).

10

14. The method according to claim 12 or 13, wherein said patient support (12) is provided with a number of position markers (55) and said position indicator (50; 60) comprises at least one light emitting element (51; 61) arranged at each position marker (55), comprising lightening up a position marker (55) by instructing a corresponding light emitting element (51; 61) to emit light.

15

15. The method according to claim 13 or 14, wherein said position markers (55) includes a transparent or semi-transparent material and are arranged on a longitudinal edge part (58) of said patient support (12), comprising individually emitting light towards a position marker (55) from a corresponding light emitting element (51; 61).

20

16. The method according to any one of claims 12 – 15, further comprising providing activation signals to instruct said light emitting elements (51; 61) to emit light according to a predetermined sequence and/or color.

25

17. The method according to any one of claims 12 – 16, wherein the treatment equipment includes a coil arrangement (28) including an anterior coil (30) and a support stand (32), the support stand (32) resting on the patient bed (16) adjacent to longitudinal edges (23) of said patient bed (16) and being slidable along the patient bed (16) in a longitudinal direction, further comprising providing activation signal to said light emitting elements (51; 61) instructing a receiving light emitting element (51; 61) to emit light to indicate positions, in a

30

longitudinal direction, where said coil arrangement (28) it to be positioned at said patient support (12).

5 18. The method according to any one of claims 12 – 17, wherein the treatment equipment includes patient positioning devices arranged to be positioned at said patient support (12), further comprising providing activation signals to said light emitting elements (51; 61) instructing a receiving light emitting element (51; 61) to emit light to indicate positions, in a longitudinal direction, where said patient positioning device (28) should be positioned at said patient support (12).

10

19. The position indicator according to claim 16, further comprising providing activation signals to said light emitting elements (51; 61) instructing a light emitting element (51; 61) to emit light according to a predetermined sequence and/or color, wherein a certain predetermined sequence and/or color is associated with a certain treatment equipment.

15

20

25

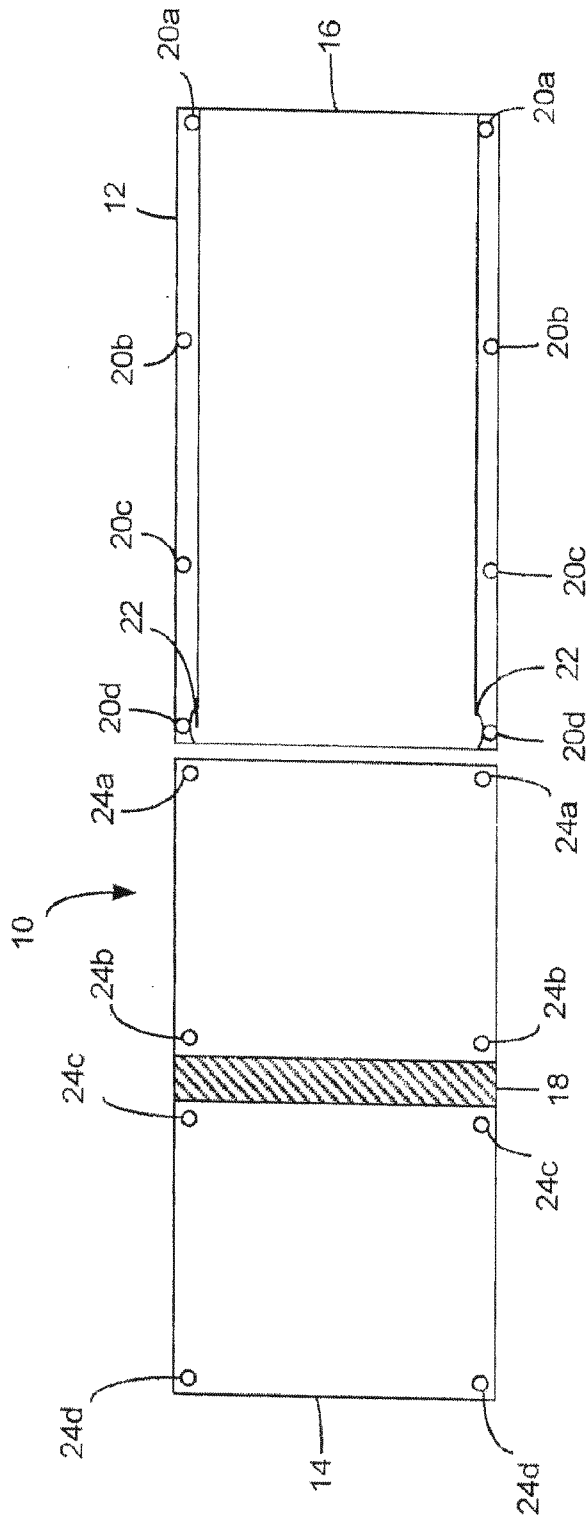


Fig.1

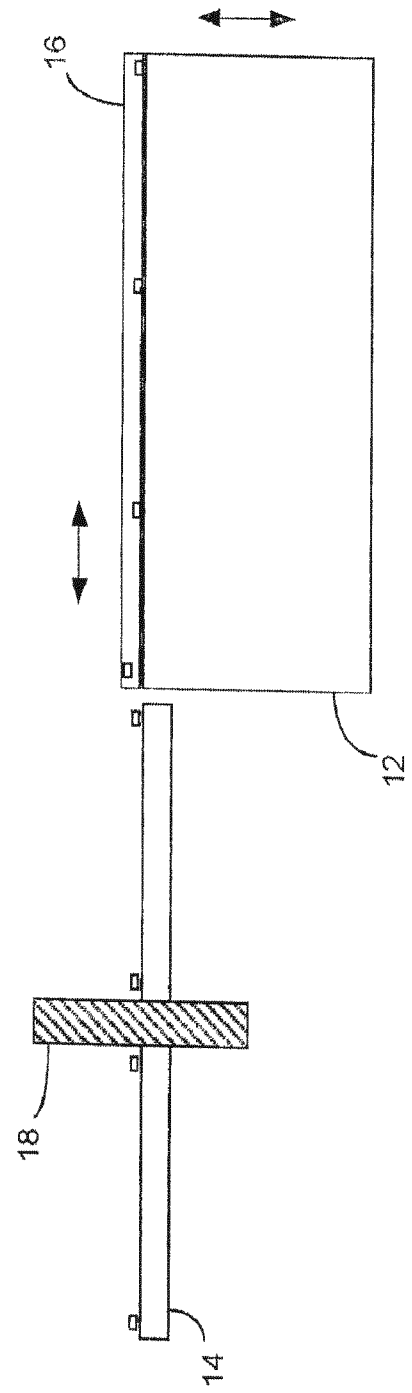


Fig.2

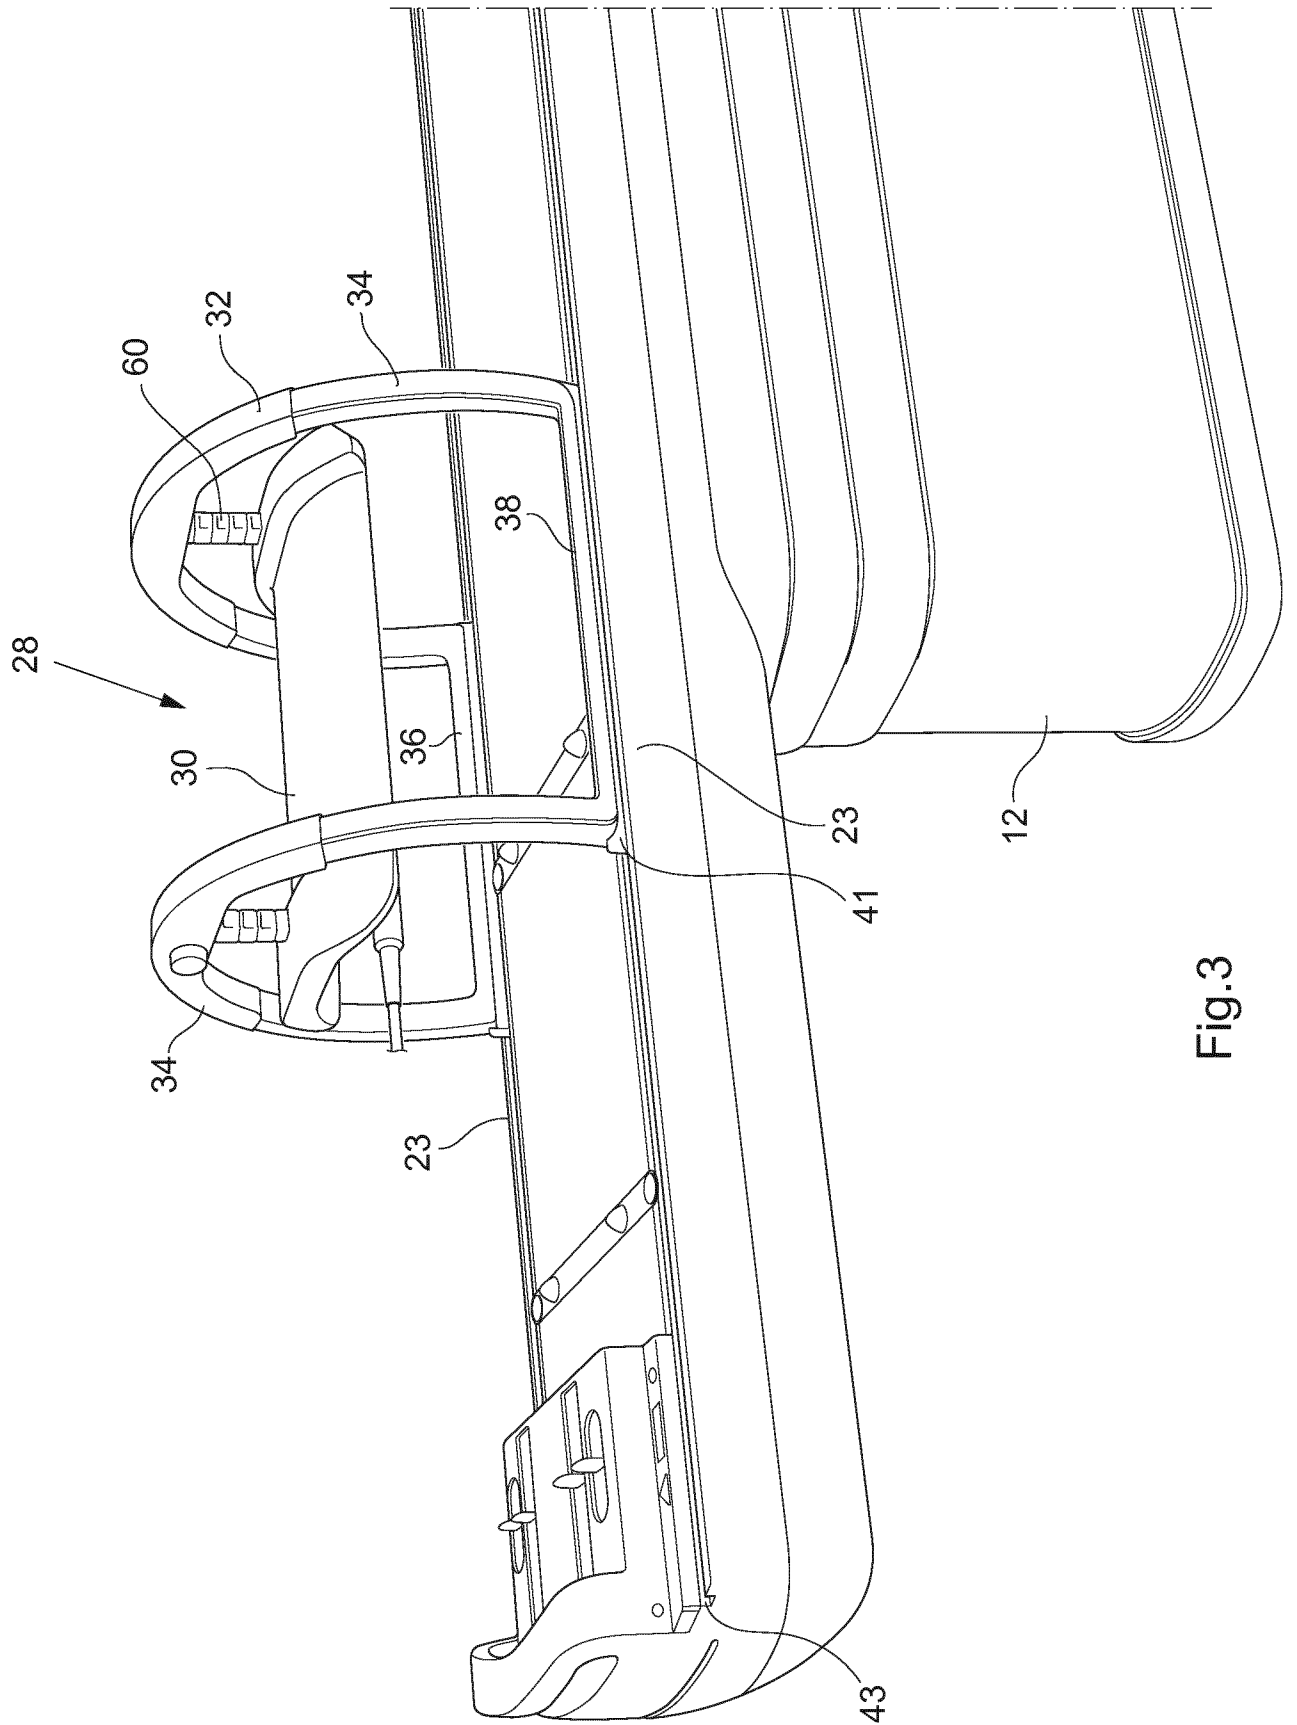
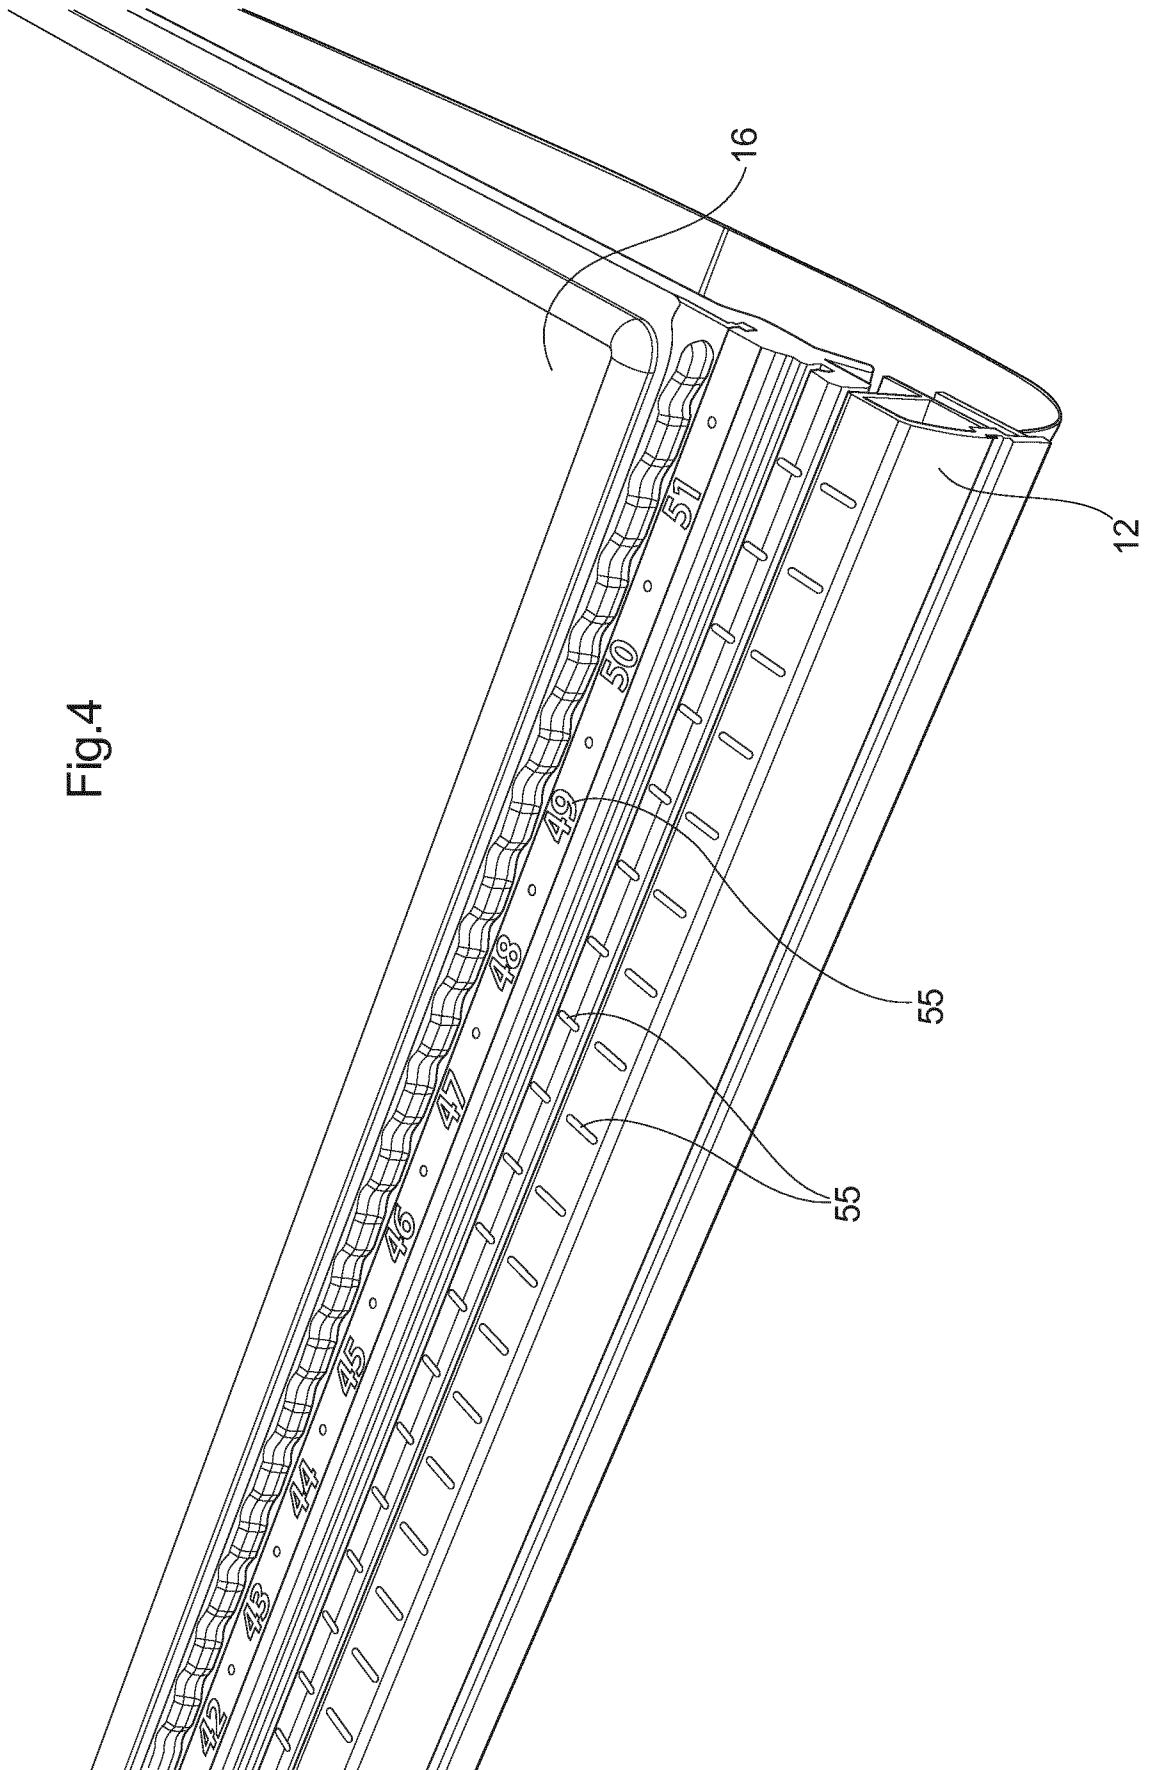


Fig.3

Fig.4



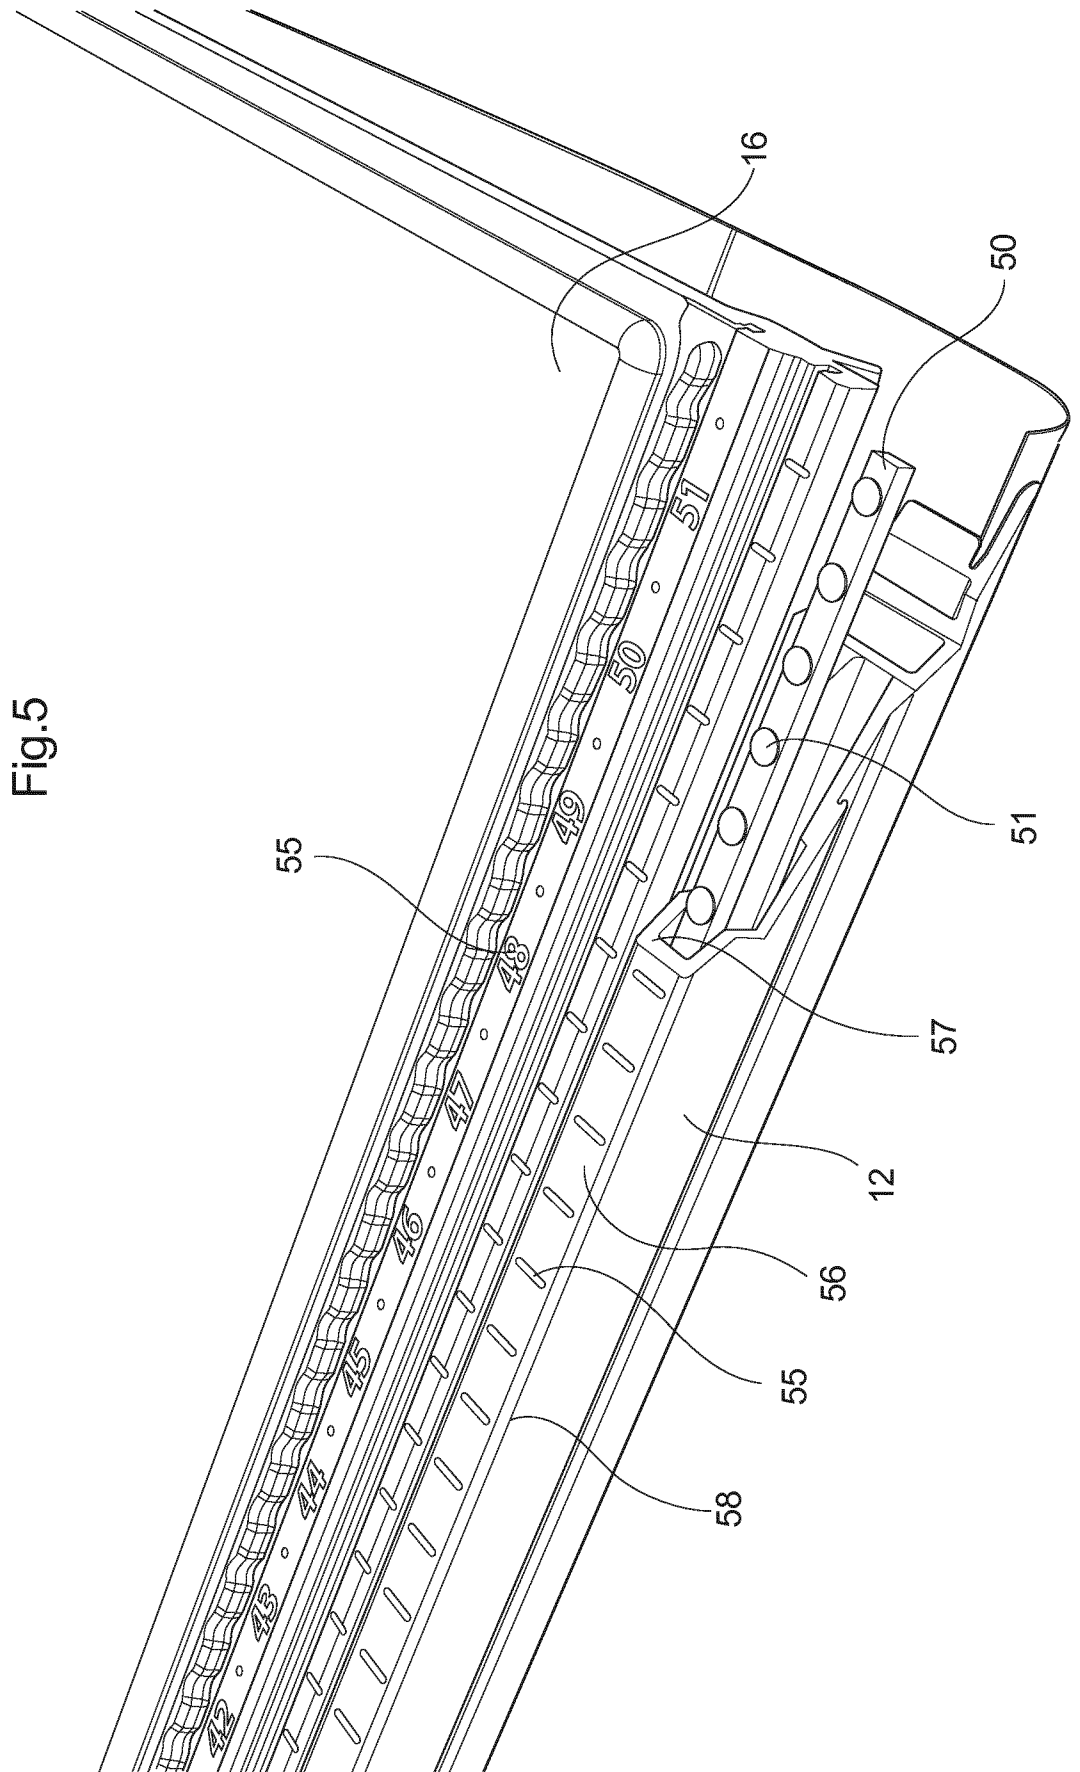


Fig.5

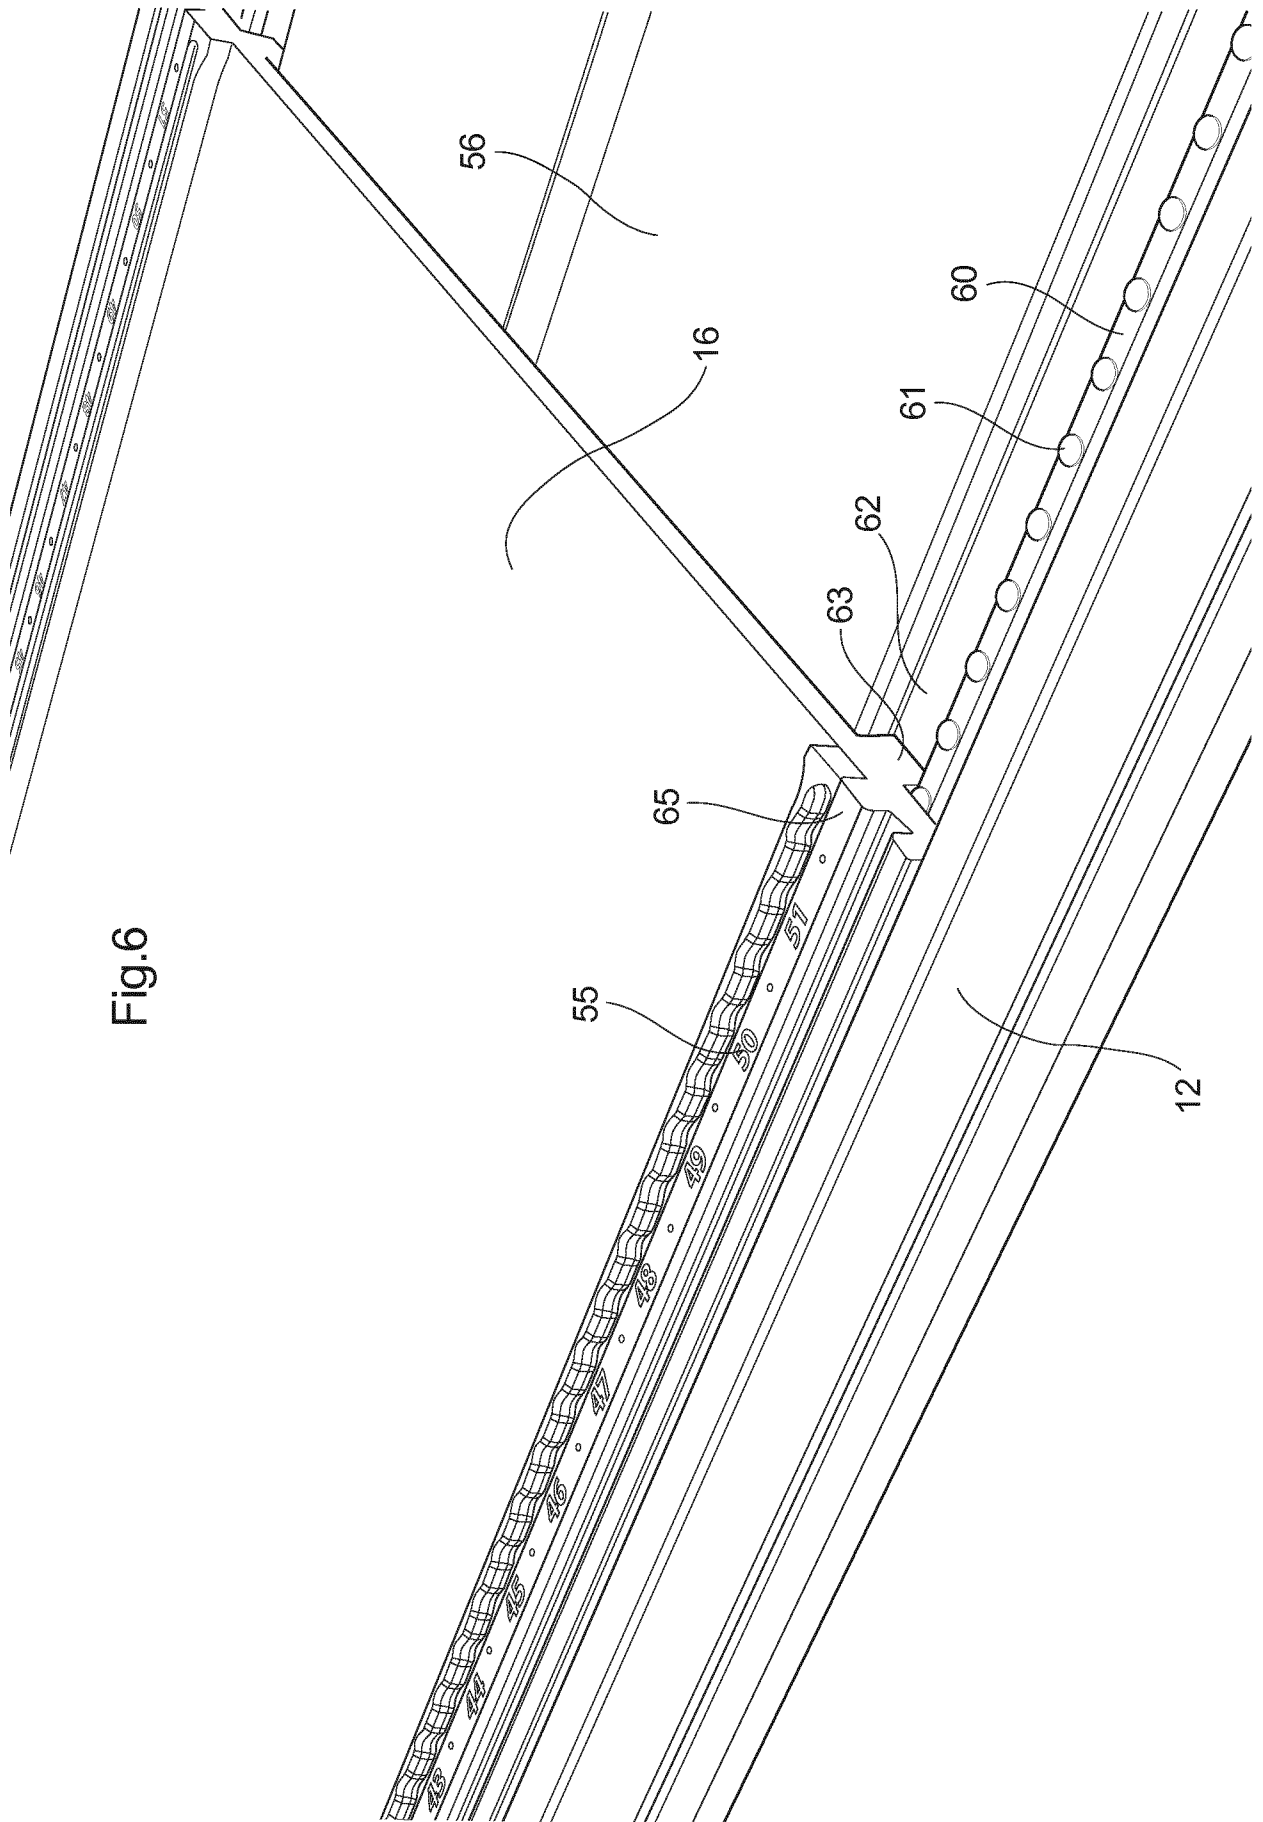


Fig.6

INTERNATIONAL SEARCH REPORT

International application No  
PCT/EP2017/077982

A. CLASSIFICATION OF SUBJECT MATTER  
INV. A61N5/10 A61B6/04 A61G7/10 A61B5/055  
ADD.  
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED  
Minimum documentation searched (classification system followed by classification symbols)  
A61N A61B A61G  
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)  
EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 2006/126108 A1 (KONINKL PHILIPS ELECTRONICS NV [NL]; CUMPSON PATRICK T [US]; PETOT BRA) 30 November 2006 (2006-11-30)	1-8, 12-16
A	page 5, line 23 - page 8, line 27; claims 1-7; figures 1-4	9-11, 17-19
Y	EP 2 881 033 A1 (MEDICAL INTELLIGENCE MEDIZIN TECHNIK GMBH [DE]) 10 June 2015 (2015-06-10)	1-8, 12-16
A	paragraphs [0001] - [0008]; figures 1,2	9-11, 17-19
Y	US 2008/204017 A1 (TAKAMORI HIROMITSU [JP] ET AL) 28 August 2008 (2008-08-28) abstract; figures 2,3,7	8,16
	----- -/--	

Further documents are listed in the continuation of Box C.

See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search  2 July 2018	Date of mailing of the international search report  10/07/2018
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer  Kajzar, Anna

## INTERNATIONAL SEARCH REPORT

International application No  
PCT/EP2017/077982

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 066 915 A (OMORI KATSUHISA [JP] ET AL) 19 November 1991 (1991-11-19) abstract; figures 3,4 -----	9-11, 17-19
A	US 2012/126815 A1 (HAHN HEINZ [DE]) 24 May 2012 (2012-05-24) abstract -----	9-11, 17-19

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2017/077982

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
WO 2006126108	A1	30-11-2006	CN 101179989 A	14-05-2008
			EP 1901652 A1	26-03-2008
			US 2008194942 A1	14-08-2008
			WO 2006126108 A1	30-11-2006
-----				
EP 2881033	A1	10-06-2015	EP 2881033 A1	10-06-2015
			GB 2520965 A	10-06-2015
			US 2015150740 A1	04-06-2015
			US 2018133080 A1	17-05-2018
-----				
US 2008204017	A1	28-08-2008	CN 101185572 A	28-05-2008
			JP 5348870 B2	20-11-2013
			JP 5620969 B2	05-11-2014
			JP 2008149118 A	03-07-2008
			JP 2013059646 A	04-04-2013
			US 2008204017 A1	28-08-2008
-----				
US 5066915	A	19-11-1991	DE 4020477 A1	10-01-1991
			JP H0394734 A	19-04-1991
			US 5066915 A	19-11-1991
-----				
US 2012126815	A1	24-05-2012	CN 102565731 A	11-07-2012
			US 2012126815 A1	24-05-2012
-----				