



(12) **United States Design Patent**  
**Tanaka et al.**

(10) **Patent No.:** **US D958,680 S**  
(45) **Date of Patent:** **\*\* Jul. 26, 2022**

(54) **WARMER FOR AN OPTICAL ANALYZER**

(71) Applicant: **FUJIFILM Corporation**, Tokyo (JP)

(72) Inventors: **Kunihiko Tanaka**, Kanagawa (JP);  
**Yutaka Senda**, Kanagawa (JP)

(73) Assignee: **FUJIFILM Cornoration**, Tokyo (JP)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/767,677**

(22) Filed: **Jan. 25, 2021**

(30) **Foreign Application Priority Data**

Jul. 28, 2020 (JP) ..... 2020-015660 D

(51) **LOC (13) Cl.** ..... **10-05**

(52) **U.S. Cl.**  
USPC ..... **D10/102; D24/231; D24/216**

(58) **Field of Classification Search**

USPC ..... D10/96-103, 65-80, 61; D24/216, 232,  
D24/186, 217, 224, 226, 227, 2, 29, 230,  
D24/231; D16/237, 250, 130, 136, 199  
CPC ..... G01N 35/025; G01N 35/00871; G01N  
35/1009; G01N 35/02; G01N 35/00712;  
G01N 2035/00891; G01N 2035/1025;  
G01N 2035/0091; G01N 2035/0441;  
G01N 2035/0446; G01N 2035/0494;  
G01N 35/00722; G01N 35/1004; G01N  
11/00; G01N 9/00; G01N 7/00; G01N  
5/00; B01L 7/52; B01L 7/00; B01L  
2300/0829; B01L 2300/1844; B01L  
2300/1816; C12Q 1/00; C12Q 2304/00;  
G02B 21/34; G02B 17/06; G02B  
27/0025; G02B 25/007; G02B 13/22

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D421,653 S \* 3/2000 Purcell ..... D24/231  
D607,569 S \* 1/2010 Yukikado ..... D24/186

D714,459 S \* 9/2014 Develon ..... D24/216  
D728,818 S \* 5/2015 Burroughs ..... D24/230  
D730,537 S \* 5/2015 Burroughs ..... D24/226  
D865,218 S \* 10/2019 Mathers ..... D24/232  
D932,929 S \* 10/2021 Stone ..... D24/216  
D941,491 S \* 1/2022 Klein ..... D24/232

(Continued)

**FOREIGN PATENT DOCUMENTS**

CN 304542751 \* 9/2017  
CN 306108058 \* 6/2020

(Continued)

**OTHER PUBLICATIONS**

FUJIFILM , Wako Toxinometer ET-7000/E Expansion Module,  
[online]retrieved Mar. 21, 2022,available from <https://www.fishersci.com/shop/products/toxinometer-et-7000-e-expansion-module/12333045> (Year: 2022).\*

(Continued)

*Primary Examiner* — Keli L Hill

*Assistant Examiner* — Sara S Sahnneh

(74) *Attorney, Agent, or Firm* — Sughrue Mion, PLLC


(57) **CLAIM**

The ornamental design for a warmer for an optical analyzer,  
as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a warmer for an optical  
analyzer, showing the new design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a top view thereof; and,  
FIG. 7 is a bottom view thereof.

**1 Claim, 7 Drawing Sheets**

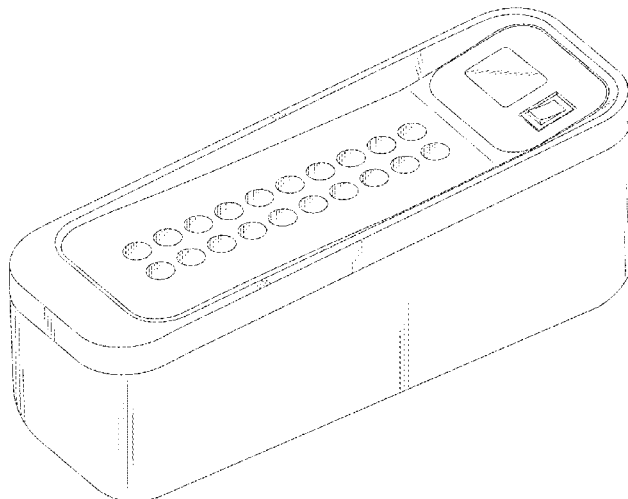

## References Cited

|                   |        |                  |              |
|-------------------|--------|------------------|--------------|
| D942,646 S *      | 2/2022 | Mathers .....    | D24/232      |
| 2013/0004954 A1 * | 1/2013 | Bianchessi ..... | G01N 21/6428 |
|                   |        |                  | 435/6.12     |
| 2014/0273181 A1 * | 9/2014 | Abbott .....     | G02B 17/06   |
|                   |        |                  | 359/398      |
| 2018/0106788 A1 * | 4/2018 | Rossi .....      | G01N 21/314  |
| 2019/0143333 A1 * | 5/2019 | Zhang .....      | B01L 7/00    |
|                   |        |                  | 422/52       |

|    |                |   |         |
|----|----------------|---|---------|
| EM | 002412593-0001 | * | 2/2014  |
| EM | 002874412-0001 | * | 11/2015 |
| EM | 008323257-0002 | * | 12/2020 |
| KR | 300740101.0000 | * | 2/2013  |
| KR | 300807266.0000 | * | 11/2014 |

FUJIFILM ,Toxinometer MT-6500, [online]retrieved Mar. 23, 2022,available from <https://diagnostic-wako.fujifilm.com/asia/products/b-glucan-test/toxinometer-mt6500.html> (Year: 2022).\*

FUJIFILM , $\mu$ TASWako i30 , [online]retrieved Mar. 23, 2022,available from <https://diagnostic-wako.fujifilm.com/asia/products/hcc-risk-biomarkers/utawako-i30.html> (Year: 2022).\*

Thomas Scientific, Test Tube Heater, Date first available from Wayback Machine Nov. 28, 2020, [online]retrieved Mar. 24, 2022, available from [wayback https://www.thomassci.com/scientific-supplies/Test-Tube-Heater](http://www.thomassci.com/scientific-supplies/Test-Tube-Heater) (Year: 2020).\*

\* cited by examiner

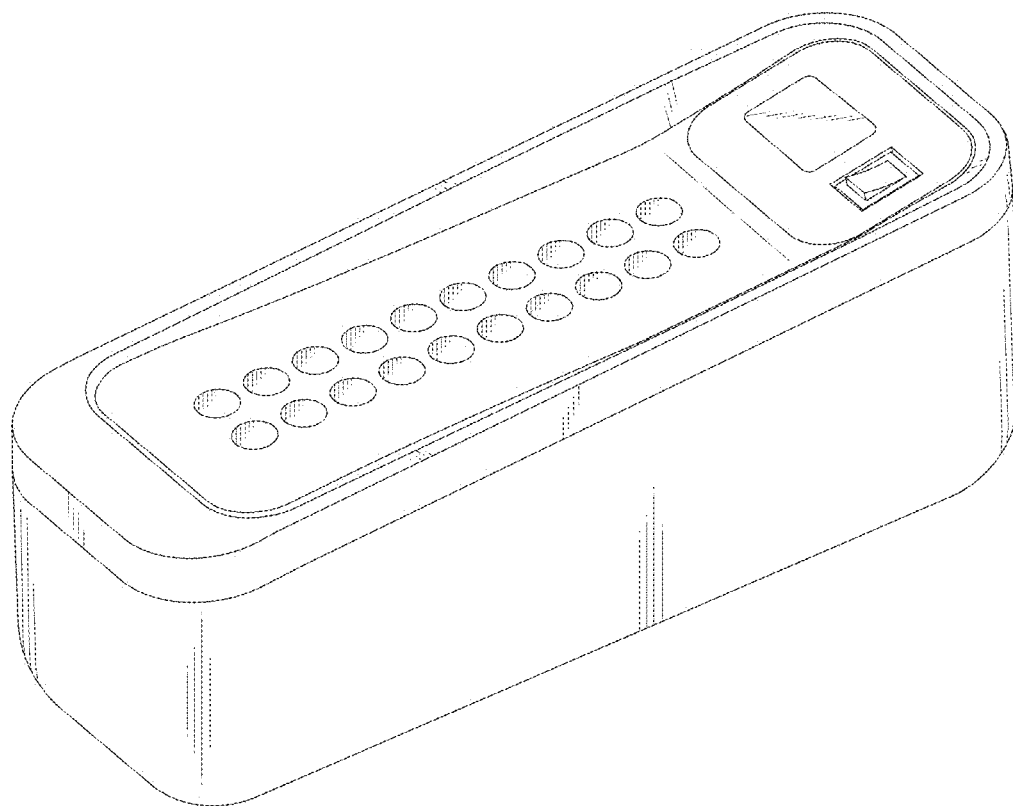


FIG. 1

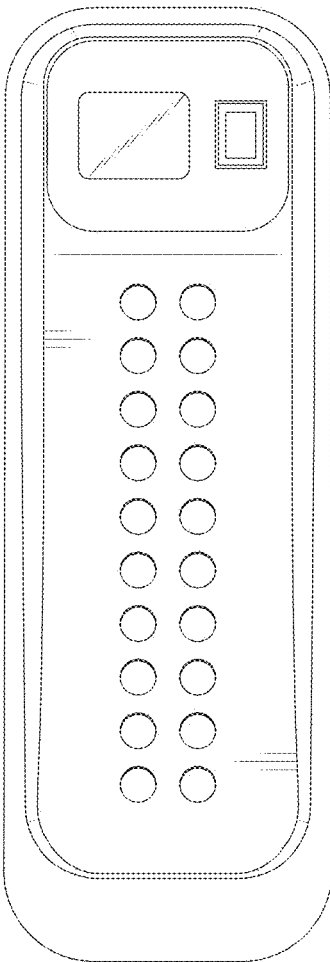


FIG. 2

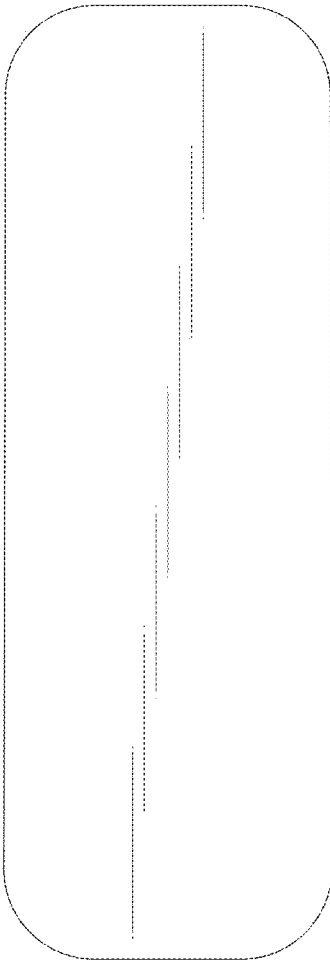


FIG. 3

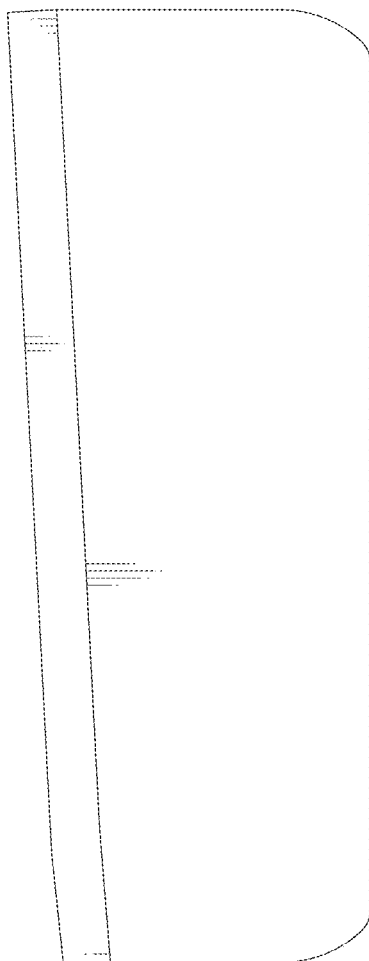


FIG. 4

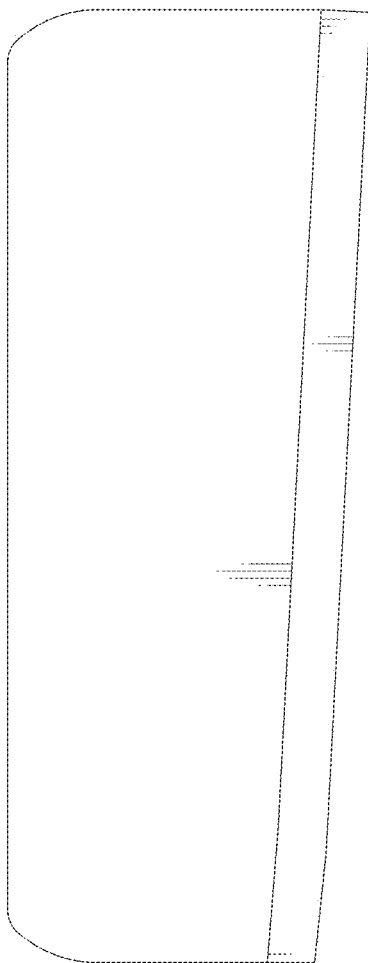


FIG. 5

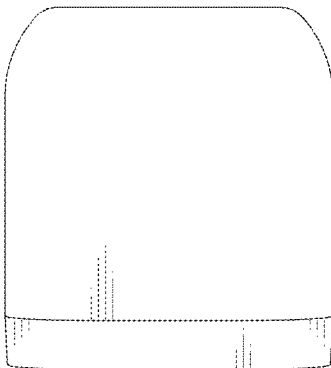


FIG. 6

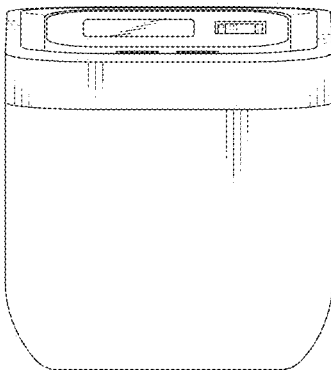


FIG. 7