



(51) International Patent Classification:
A61F 5/00 (2006.01)

(21) International Application Number:
PCT/IL2020/051162

(22) International Filing Date:
09 November 2020 (09.11.2020)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
16/699,451 29 November 2019 (29.11.2019) US

(71) Applicant: **ALLEVETIX MEDICAL LTD.**, [IL/IL]; 2
HAESHEL STREET, CAESAREA INDUSTRIAL PARK
SOUTH, 3088900 CAESAREA (IL).

(72) Inventor: **KALFON, Ziv**; Ein Hod, Builg./ 7, 3089000 Ein
Hod (IL).

(74) Agent: **BRONSTEIN, Rafi**; Daltan Consulting Ltd., P.O.
BOX 1146, 4410002 KFAR SAVA (IL).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, IT, JO, JP, KE, KG, KH, KN,

KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO,
NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW,
SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: IMPLANTABLE ANCHORING DEVICE AND METHODS OF USE

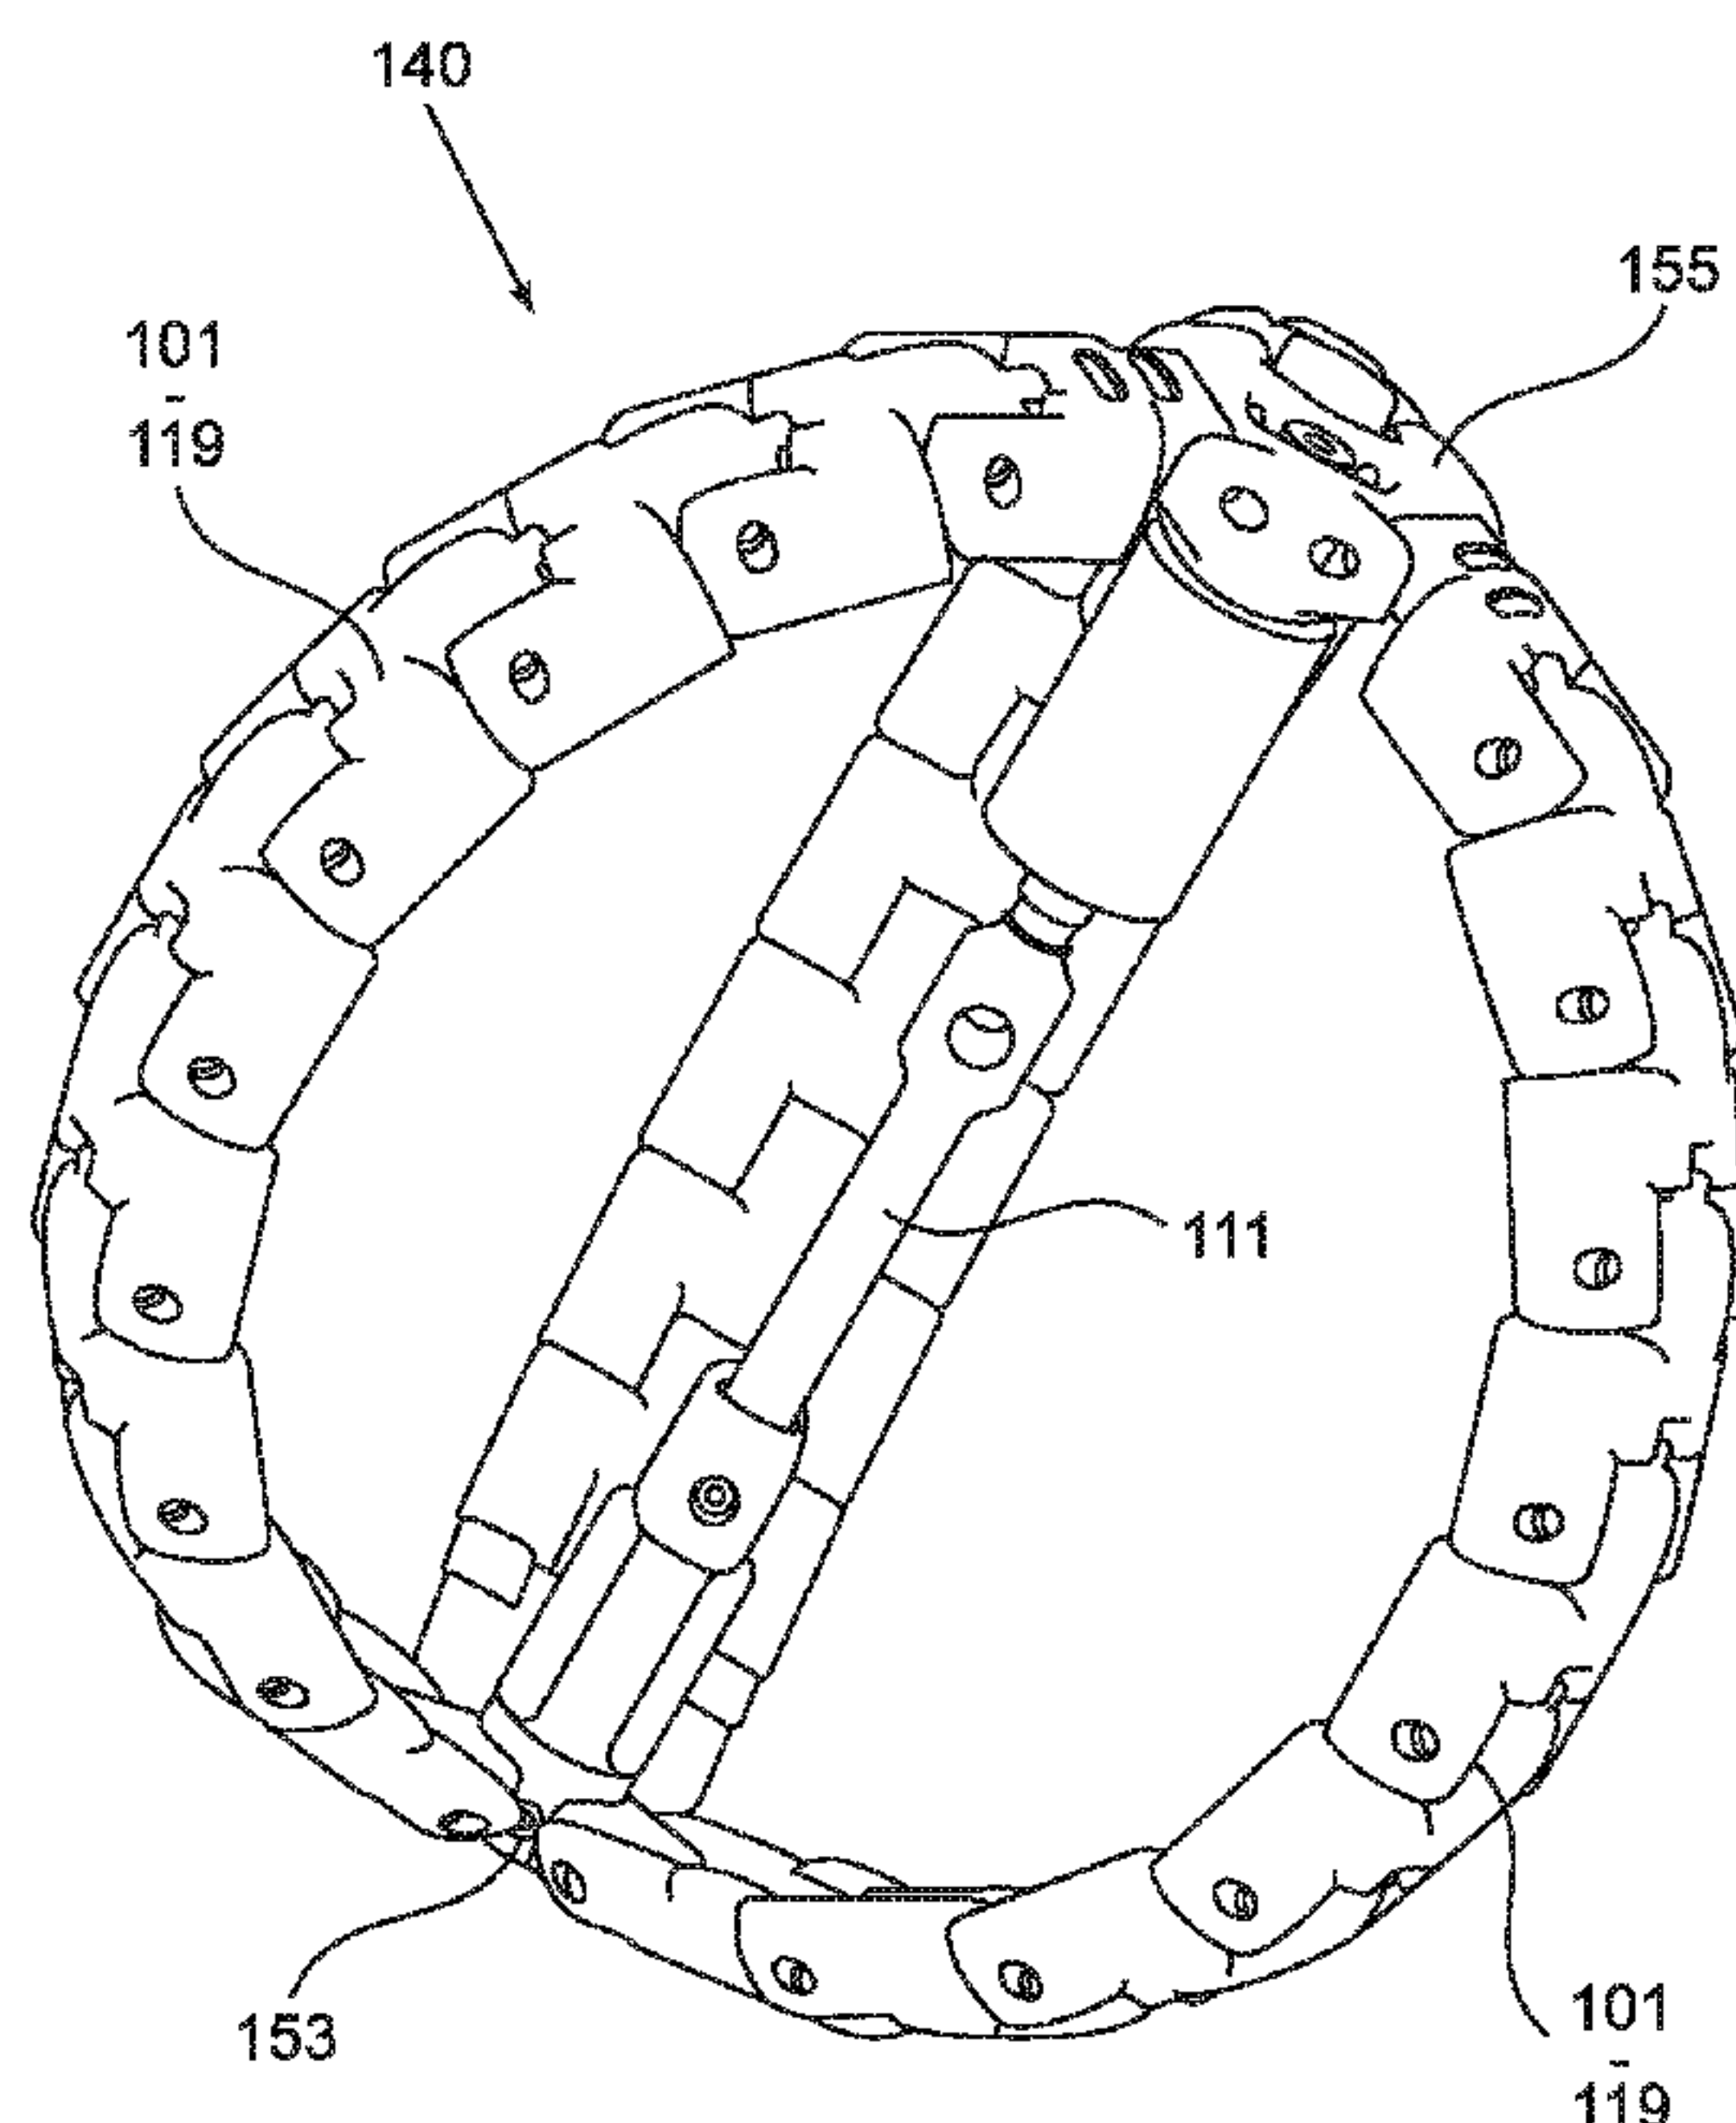


FIG. 1E

(57) Abstract: A method of using an implantable device provides an im-
plantable device including a plurality of arcs. Each arc contains a multiplic-
ity of links. The implantable device further includes a device closure pin, a
lock-in unit attached and located between the three arcs, and a quick-release
unit attached and located between three arcs. The plurality of arcs, the lock-
in unit, and the release unit form a closed contour. The closed contour of the
implantable device, in a rigid state is a three-dimensional shape.

- 1 -

IMPLANTABLE ANCHORING DEVICE AND METHODS OF USE

TECHNICAL FIELD

[0001] The present disclosure generally relates to a device that is inserted into a body cavity using intraoral procedures and positioned within a body cavity by a deformation of the shape and rigidity of the device.

BACKGROUND OF THE DISCLOSURE

[0002] Several medical procedures require placement of a medical device in the lumen of a human or animal body and in particular, in the stomach. Once inserted, the movement of the inserted medical device has to be constrained, and this is achieved by the use of anchors. U.S. Pat. No. 9,636,245 to Chamorro describes a gastrointestinal device including a proximal element configured to reside in the stomach and a distal element configured to reside in an intestine, where the proximal element is configured to resist migration over time. US Pat. Application No. 2008/0058840 to Albrecht describes an alternative proximal element for placement within a hollow body organ. The proximal element includes a member having a first shape for delivery to the hollow body and a second shape for implantation therein. The member has sufficient rigidity in its second shape to exert an outward force against an interior of the hollow body to bring together two substantially opposing surfaces of the hollow body. US Pat. Application No. 2012/0095385 to Domingues describes a gastric balloon that is introduced in the stomach. The balloon occupies space in the stomach, thereby leaving less room for food and creating a feeling of satiety for the patient. U.S. Pat. No. 6,994,715 to Gannoe discloses expandable and space-occupying devices that are inserted into the stomach of a patient and may be maintained within the stomach by anchoring or otherwise fixing the device to the stomach wall. Patent Cooperation Treaty Publication No. 2007/076021 to Haller describes a gastrointestinal device, which is a bag stuffed with digestive resistant

- 2 -

or indigestible material. The bag is located in the gastric lumen in a compacted configuration. The bag is then manipulated into, or allowed to assume, a second expanded configuration sufficiently large to maintain the bag within the stomach and not to be passed through the pylorus and into the intestines. The examples of implants described in the listed above patents suffer from certain drawbacks when inserted within a lumen of the human body and do not provide the long term required implantation stability.

SUMMARY

[0003] This current disclosure describes an implantable device including at least three (plurality) of arcs with each arc including a multiplicity of links. The implantable device is configured to be in either of two states; a flexible state in at least one plane of the device or a rigid state in all other planes of the device. In the rigid state, the device has a three-dimensional curved shape. The implantable device includes at least but not limited to: device closure pin; a lock-in unit; a quick-release unit; a plurality of arcs where each arc includes a multiplicity of links connected to two other links or a link on one side and either a lock-in unit or release unit on an opposing side. The implantable device is inserted into a body cavity using intraoral procedures. During insertion, the device closure pin is attached only at one side and, in one example, to the quick release unit, and the implantable device is in a flexible state. The flexibility of the implantable device affords the device the ability to follow the contours of the body orifice and facilitates the insertion of the device with minimal patient discomfort. The implantable device is releasably connected to the intraoral insertion equipment at the lock-in unit. After insertion of the implantable device into the human body and placement of the implantable device in the target body cavity, the device closure pin is pulled into the lock-in unit and locked into place. The device closure pin is now attached at both ends of the pin and transforms the implantable device into a rigid state. In the rigid state, the implantable

- 3 -

device has a three-dimensional curved shape such as a sphere or an ellipsoid providing anchoring features and preventing mobility of the implantable device in the body cavity.

[0004] In one example, a functional unit providing a body-related function is attached to the release unit. An example of a functional unit is an intragastric sleeve adapted to reduce the intake of food items in the intestine.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] FIG. 1A is an example of an implantable device consisting of two arcs and multiple links and configured to be flexible in at least one plane;

[0006] FIG. 1B is an example of an implantable device consisting of two arcs and multiple links just before being configured to be rigid in all planes;

[0007] FIG. 1C is an example of an implantable device consisting of two arcs and multiple links and configured to be rigid in all planes;

[0008] FIG. 1D is an example of an implantable device consisting of three arcs and multiple links;

[0009] FIG. 1E is an example of an implantable device consisting of three arcs and multiple links and shown in a rigid state;

[00010] FIG. 2A is an example of a link of the implantable device;

[00011] FIG. 2B is an example of a top view of a link of the implantable device;

[00012] FIG. 2C is an example of a side view cross-section of a link of the implantable device at cut line NN from FIG. 2B;

- 4 -

[00013] FIG. 3A is an example of device closure pin attached to a release unit;

[00014] FIG. 3B is an example of a side view of a device closure pin attached to a release unit;

[00015] FIG. 3C is an example of a back view of a device closure pin attached to a release unit;

[00016] FIG. 4A is an example of device closure pin attached to a receptacle;

[00017] FIG. 4B is an example of a side view of a device closure pin attached to a receptacle;

[00018] FIG. 4C is an example of a top view of a device closure pin attached to a receptacle;

[00019] FIG. 5A is an example of a method of use of the implantable device consisting of two arcs and multiple links in the rigid state to constrain movement of the device in a body cavity;

[00020] FIG. 5B is an example of a method of use of the implantable device consisting of three arcs and multiple links in the rigid state to constrain movement of the device in a body cavity;

[00021] FIG. 6A is an example of a wave anchor in a folded configuration; and

[00022] FIG. 6B is an example of a wave anchor in an extended configuration.

DETAILED DESCRIPTION

[00023] In the following detailed description, reference is made to the accompanying drawings, which form a part hereof. In the drawings, similar symbols typically identify similar components, unless context dictates otherwise. The illustrative examples described in the detailed description, drawings, and claims are not meant to be limiting. Other examples may be utilized, and other changes may be made, without departing from the spirit or scope of the subject matter presented here. It will be readily understood that the aspects of the present disclosure, as generally described herein, and illustrated in the figures, can be arranged, substituted, combined, and designed in a wide variety of different configurations, all of which are explicitly contemplated and make part of this disclosure. This disclosure is drawn, among other things, to a device that is inserted into a human or animal body using intraoral procedures and positioned within a body cavity by a change of the shape and rigidity of the device.

[00024] In examples/patents of the implantable devices described above, the proximal element is in contact with the pylorus. The proximal element has a rounded shape, and as a result, it exerts an expansion force on the pylorus, which extends the pylorus opening over time and dislodges the proximal element. Such implants suffer from migration within a lumen of a human or animal body and do not provide the long term required implantation stability. It is desirable to have a proximal element which does have a three-dimensional curved shape that could be in contact with walls of the stomach, the shape large enough and does not slide into the pylorus and provides the long term required implantation stability.

[00025] FIG. 1A is an example of an implantable device consisting of two arcs and multiple links and configured to be flexible in at least one plane. The implantable device includes at least but not limited to; a lock-in unit 103; a quick-release unit 105 a multiplicity of links 101, 113, 115, 117, 119 (collectively 101 – 119 or 101) where each link 101 is connected to two other links 101 or to a link 101, 113, 115, 117, 119 on one side and either a lock-in unit 103 or a release unit 105 on an opposing side. The implantable device is inserted into a body cavity using intraoral procedures. During

- 6 -

insertion, the flexibility of the implantable device affords the device the ability to follow the contours of the body orifice and facilitates insertion with minimal discomfort to the patient. The implantable device connects to delivery or insertion equipment at lock-in unit 103. In one example, a functional unit providing a body-related function is attached to a quick-release unit 105. An example of a functional unit is an intragastric sleeve adapted to reduce the intake of food items in the intestine.

[00026] FIG. 1B is an example of an implantable device, including two arcs and multiple links just before being configured to be rigid in all planes. The implantable device is transformed from a flexible state as described in FIG. 1A to a rigid state as described in FIG. 1C by pulling a cord 121 attached to a device closure pin 111 (FIG. 1B) and passing through lock-in unit 103. Device closure pin 111 follows cord 121 into lock-in unit 103, where a locking mechanism holds the device closure pin 111 in place. The locked-in device closure pin 111 exerts a force on the implantable device links 101- 119, constricting the relative movement of the links and transitioning the implantable device to a rigid state. The transition of the implantable device from a rigid state to a flexible state facilitates removal of the implantable device from the body cavity. Removal of release pin 123 from device closure pin 111, releases the device closure pin 111 from the release unit 105 and transitions or transforms the implantable device to a flexible state. After transitioning the implantable device to a flexible state, it is removed from the body cavity with intraoral procedures. Examples of materials for manufacturing the links 101 include but are not limited to: Titanium; Stainless steel; Cobalt, Chrome, Nitinol alloy, thermoset plastics and similar materials or composition of said materials.

[00027] Additionally, a Teflon™ (polytetrafluoroethylene) coating or overcoat enhances the atraumatic properties of the links 101-119 surfaces. (The surfaces are considered "atraumatic" because they do not cause trauma to the body.) Examples of materials for the device closure pin 111 and the release pin 123 include but are not limited to; Stainless steel; Titanium; Cobalt, Chrome, Nitinol alloy, thermoset plastics and similar materials or composition of said materials. In one example, links 101 of the implantable device are manufactured using additive manufacturing processes, for example, 3D printing. Links 101, lock-in unit 103, quick- release unit 105, and interconnecting pins are manufactured

- 7 -

concurrently and in a connected manner so that at the additive manufacturing cycle results in a connected closed contour of links 101- 119, lock-in unit 103, and quick release unit 105.

[00028] Hence, described in one example is an implantable device including a multiplicity of links 101-119; a device closure pin 111; a lock-in unit 103 attached and located between two links 117, 119; a release unit 105 attached and located between two links 113, 115. The multiplicity of links 101 - 119, lock-in unit 103 and release unit 105 construct a closed contour; and wherein the implantable device is in a flexible state when the device closure pin 111 is coupled to the lock-in unit 103 or the quick-release unit 105 and rigid state when the device closure pin 111 is attached to both the lock-in unit 103 and quick-release unit 105.

[00029] FIG. 1C is an example of a side view of the implantable device in the rigid state 135, where the closed contour and device closure pin 111 form a figure eight. In an alternative example an implantable device comprising; a plurality of links 101 - 119 constructing a closed loop wherein a link 101, 113, 115, 117 is connected to two other links 101 - 119; a device closure pin 111; wherein the implantable device is flexible when only one side of device closure pin 111 is attached to a link 101 - 119 and rigid when both sides of the device closure pin 111 is attached to a link 101 - 119. In a further example the closed contour of an implantable device in a rigid state 135 is oval and is configured to follow the shape of two arcs 125, 127 and two interconnecting sections 131, 133 where the absolute radius of the two arcs sections 125, 127 is at least 5 times larger the absolute radius of the interconnecting sections 131, 133. The radius of each of the arcs sections 125, 127 is of opposite sign. In a further example, the closed contour of an implantable device in a rigid state is oval and comprised of two arcs 125, 127 and two interconnecting sections 131, 133, where the two interconnecting sections 131, 133 are substantially straight. In a further example, the closed contour of an implantable device in a rigid state has a shape of figure eight comprised of two arcs and two connected interconnecting sections. The resulting shape of the implantable device in a rigid state which is in contact with the pylorus is substantially straight and hence does not exert an expanding force on the pylorus, ensuring the long term stability of the implanted device.

- 8 -

[00030] FIG. 1D is an example of an implantable device consisting of three arcs and multiple links. FIG. 1D illustrates implantable device 140 in a first or flexible state. Implantable device 140 consists of three arcs 142, 144, and 146, and each arc includes multiple links 101-119. Arcs 142, 144, and 146 with multiple links 101 - 119 are configured to be sufficiently flexible for an intraoral introduction into a recipient body. The implantable device 140 includes at least but not limited to; a lock-in unit 148; a quick-release unit 155; a multiplicity of links 101- 119. Each link 101 - 119 connects to two other links 101 - 119 or a link 101 - 119 on one side and either a lock-in unit 153 or a quick-release unit 155 on an opposing side. The implantable device 140 in a first or flexible state is inserted into a body cavity using intraoral procedures. During insertion, the flexibility of the implantable device affords the implantable device 140 the ability to follow the contours of the body orifice. It facilitates insertion with minimal discomfort to the patient. The implantable device 140 is connected to delivery or insertion equipment at lock-in unit 153. In one example, a functional unit providing a body-related function is attached to a quick-release unit 155. An example of a functional unit is an intragastric sleeve adapted to reduce the intake of food items in the intestine.

[00031] FIG. 1E is an example of an implantable device consisting of three arcs and multiple links and is shown in a rigid state. The implantable device 140 in the first configuration is in a flexible state. In the second configuration or rigid state, implantable device 140 forms a closed contour wherein the three arcs 142, 144, and 146, lock-in unit 153, and quick-release unit 155 construct a closed three-dimensional curved shape device. The closed three-dimensional curved shape of implantable device 140 could be one of a group of shapes consisting of a sphere or an ellipsoid.

[00032] All links (101- 119) surfaces are atraumatic surfaces made of Titanium. Additionally, a Teflon™ (polytetrafluoroethylene) coating or overcoat enhances the atraumatic properties of the links 101-119 surfaces. Usually, the links (101, 113, 115, 117, 119) are fabricated using additive manufacturing processes.

[00033] FIG. 2A is an example of an implantable device link (FIG. 1A numerals 101 - 119.) A link 101-119 includes an attachment axis 203 and a pin cavity 201. The attachment axis 203 is configured to connect to a pin cavity 201 in a second link creating

- 9 -

a closed contour composed of a multiplicity of links 101 - 119 where each link 101 - 119 is connected to two other links 101 - 119 or to a link 101 on one side and either a lock-in unit (FIG. 1B reference numeral 103 and FIG. 1E reference numeral 153) or release unit (FIG. 1B reference numeral 105 and FIG. 1E reference numeral 155) on an opposing side. FIG. 2B is an example of a top view of a link 101 of the implantable device. FIG. 2C is an example of a side view cross-section of a link of the implantable device at cut line N-N from FIG. 2B. Link 101 includes an attachment axis 203 and a pin cavity 201. The link further includes an inclined side 205. In the flexible state of the implantable device, one link 101 connects to a second link 101, where the axis 203 of one link 101 is inserted in the pin cavity 201 of a second link 101. The links 101 are free to move around the axle defined by their axis 203. The relative movement of the links 101 around the axle provides the required flexibility along one plane of an implantable device in the flexible state. In the constrained state inclined side 205 of one link 101 is pressed against the opposing side 211 of adjacent connecting link 101. The shape of the contour of the implantable device in the constrained state is determined by the relative angle of the inclined side 205 of one link 101, and the opposing side 211 of the adjacent link 101, which is in contact with said inclined side 205. In a further example, the aforementioned relative angle varies from link to link to configure a specific size shape of the closed contour of the implantable device in the rigid state.

[00034] Support recess 207 or 209 come into contact with support recess 209 or 207 of an adjacent link at a maximum preset angle and provide a constraint on the relative motion of the link 101 in the flexible state. The links comprise at least a base 220 (FIG. 2A); one or more connecting pins 203 and one or more vias 201. All links (FIG. 1A 101 - 119 and FIG. 2A 101) comprising the implantable device and pins 203 and pinholes 205 are manufactured concurrently so that a pin 203 of one link 101 is situated in a pinhole 205 of an adjacent link 101 or lock-in unit (FIG. 1A 103 and FIG. 1E 153) or quick release unit (FIG. 1A 105 and FIG. 1E 155) and providing a closed contour of links 101, lock-in unit (FIG. 1A 103 and FIG. 1E 153) and quick release unit (FIG. 1A 105 and FIG. 1E 155) at the end of the additive manufacturing cycle.

- 10 -

[00035] As illustrated in the example, the links consist of at least a base 220; one or more connecting axis 203 and one or more holes 201. Base 220 and a connecting axis 203 of one link (FIG. 1B -1E 101 - 119) which is located in a pinhole 201 of a second link (FIG. 1B-1E. 101 - 119) are fabricated concurrently using additive manufacturing processes.

[00036] FIG. 3A is an example of a device closure pin 111 attached to a release unit 105 (or 155). The top side of device closure pin 111 is configured as a snap-in segment. The snap-in segment includes a recess 305 and a conical tip 309. In a further example, when the implantable device is in a flexible state, a cord (FIG. 1B - 121) is connected to the top part of the conical tip 309. Pulling the cord (FIG. 1B - 121) pulls the device closure pin 111 into a receptacle (FIG. 4 - 401) where it is locked in place due to the recess 305. The device closure pin 111 further includes one or more quick-release pinholes 307. FIG. 3B is an example of a side view of a device closure pin attached to a release unit. The device closure pin 111 further includes an attachment pin 315 and attachment pin cavity 311, which correspond to a link's (FIG. 2A - 101) attachment pin (FIG. 2C - 203) and attachment pin cavity (FIG. 2C - 201). The pins are used to attach links on either side of the device closure unit. The device closure unit 105/155 further includes a quick release housing 301 and second pinhole 303. A device attachment pin is inserted into the quick release housing 301 and held in place by insertion of a quick release pin (FIG. 1B - 123) through the second pinhole 303 and quick release pinhole 307 in the device closure pin 111. Before insertion in the body, the device closure pin 111 is attached to the quick-release unit 105/155. The effective length of the device closure pin 111 is adjusted by a choice through which quick-release pinhole 307 the quick-release pin (FIG. 1B - 123) will pass through and lock the device pin 111 in place. The effective length of the device closure pin 111 determines the contour shape when the implantable device is in the rigid state. In a further example, the contour shape is configured to be essentially flat for at least one link on either side of the quick release unit 105. Sleeve connection pin 321 is the anchor point for a cord connecting the implantable device to an intestine sleeve. FIG. 3C is an example of a back view of a device closure pin attached to a release unit.

[00037] FIG. 4A is an example of device closure pin 111 attached to a receptacle 401.

FIG. 4B is an example of a side view of a device closure pin 111 attached to a receptacle

- 11 -

401 and FIG. 4C is an example of a top view of a device closure pin attached to a receptacle 401. In one example a receptacle 401 includes an outer ring 403 a plurality of spokes 405 which terminate short of the center of the receptacle 401 and enable the conical tip 309 of the device closure pin 111 to traverse the receptacle 401 and then lock the device closure pin 111 in place by extending into the device closure pin recess 305. Examples of materials for manufacturing the receptacle include but are not limited to; stainless steel Titanium; Stainless steel; Cobalt, Chrome, Nitinol alloy, thermoset plastics, and similar materials; or composition of said materials.

[00038] Closure pin 111 includes a conical tip 309 configured for insertion and lock-in into a receptacle 401 with an outer ring 403 and one or more spokes 405 and in, a further example the receptacle 401 is structured as slotted spring washer and configured to receive and hold a snap-in segment of device closure pin 111.

[00039] FIG. 5A is an example of a method of use of an implantable device in the rigid state 135 to constrain implantable device movement in a body cavity. In one example, the implantable device in the rigid state 135 is fixed in the stomach 511. An intestine sleeve 505 is attached with the sleeve cord 501 to the implantable device in the rigid state 151 and inserted into the intestine 513. In a further example, the intestine sleeve 505 includes a wave anchor 503, which positions the intestine sleeve in place.

[00040] FIG. 5B is an example of a method of use of the implantable device consisting of three arcs and multiple links in the rigid state to constrain movement of the implantable device in a body cavity. In the rigid state, the shape of implantable device 140 has a closed three-dimensional curved shape contour. Three arcs 142, 144, and 146 of device 140 open and anchor device 140 within stomach 511. Arcs 142, 144, and 146 of device 140 could be in contact with walls of stomach 511. The three-dimensional curved shape contour of unit 140 supports the almost constant location of unit 140 within the stomach.

[00041] FIG. 6A is an example of the wave anchor 503 in a folded configuration and FIG. 6B is an example of the wave anchor in an expanded configuration.

[00042] Several examples have been described. Nevertheless, it will be understood that various modifications may be made without departing from the spirit and scope of the method. Accordingly, other examples are within the scope of the following claims:

- 12 -

I claim:

1. An implantable device comprising:

at least three arcs transformable from a first flexible state to a second rigid state;

a device closure pin;

a lock-in unit attached and located at one end of the three arcs;

a quick-release unit attached and located at an opposite end of the three arcs; and

wherein the coupling of a device closure pin to one of the lock-in unit or the quick-release unit the device is in the first flexible state and when the device closure pin is attached to both the lock-in unit and the quick-release unit the device is in the second rigid state.

2. The implantable device of claim 1, wherein in the second rigid state the at least three arcs, lock-in unit and release unit construct a closed three-dimensional curved shape.

3. The implantable device of claim 2, wherein the closed three-dimensional curved shape is one of a group of shapes consisting of a sphere or an ellipsoid.

4. The implantable device of claim 1, wherein all link surfaces are atraumatic surfaces comprised of titanium and wherein the atraumatic surfaces of the links further include a polytetrafluoroethylene coating or overcoat.

5. The implantable device of claim 4, wherein each of the links consist of at least a base; an attachment axis and one or more pinholes and the links are fabricated using additive manufacturing processes.

6. The implantable device of claim 5, wherein a base and attachment axis of one link which is located in a pinhole of a second link are fabricated concurrently using additive manufacturing processes.

7. The implantable device of claim 1, wherein the device closure pin includes a conical tip

- 13 -

configured for insertion and lock-in into a receptacle.

8. The implantable device of claim 1, wherein the release unit includes an extractable pin attaching the device closure pin to the release unit, and removal of the extractable pin releases the device closure pin from the release unit.

9. The implantable device of claim 1, wherein a closed contour of the implantable device in a rigid state is a three-dimensional curved shape including three arcs and two interconnecting sections where the two interconnecting sections are substantially straight.

10. An implantable device comprising:

- a multiplicity of links forming three arcs constructing a closed three-dimensional curved shape wherein each link is connected to two other links; and

- a device closure pin including a snap-in segment; and

- a lock-in unit attached and located at one end of three arcs;

- a quick-release unit attached and located at an opposite end of three arcs; and

- wherein the implantable device is flexible when the device closure pin is attached to one of a lock-in unit or a quick-release unit and rigid when both sides of the device closure pin are attached to a lock-in unit and a quick-release unit and; and

- wherein the device closure pin includes a receptacle with a slotted spring washer configured to receive and hold a snap-in segment of the device closure pin.

11. The implantable device of claim 10, wherein the lock-in unit includes a receptacle structured as a slotted spring washer and configured to receive and hold a snap-in segment of the device closure pin.

12. The implantable device of claim 10, wherein the device closure pin includes at least one quick-release pinhole and an extractable pin attaching the device closure pin to a lock-in unit or a release unit.

- 14 -

13. The implantable device of claim 10, wherein a closed curved three-dimensional state of the implantable device is sufficiently large to prevent the implantable device from passing a pylorus.

14. A method of using an implantable device, comprising:

providing an implantable device including at least three arcs, a device closure pin, a lock-in unit attached and located at one end of at least three arcs, and a quick-release unit attached and located at an opposite end of at least three arcs; and

constructing the at least three arcs, lock-in unit and quick-release unit in a closed rigid configuration, wherein the closed rigid state of the implantable device is a three-dimensional curved shape; and

wherein the implantable device three-dimensional curved shape comprises at least three arcs and two interconnecting sections with each interconnecting section connecting at least three arcs.

15. The method of claim 14 further comprising attaching the device closure pin to both the lock-in unit and release unit and holding the implantable device in a rigid state.

16. The method of claim 14, wherein providing at least three arcs consisting of a multiplicity of links and where all link surfaces are atraumatic surfaces made of titanium, and wherein the atraumatic surfaces of the links further include a polytetrafluoroethylene coating or overcoat.

17. The method of claim 14, wherein the implantable device is in a flexible state when the device closure pin is coupled to at least one of the lock-in unit or the quick-release unit and in a rigid state when the device closure pin is attached to both the lock-in unit and the quick-release unit.

18. A method of employing an implantable device, comprising:

providing an implantable device including a multiplicity of arcs with each arc being a flexible straight element; a device closure pin, a lock-in unit attached and located between three arcs, and a quick-release unit attached and located between three arcs; and

- 15 -

constructing the multiplicity of arcs, lock-in unit and release unit in a closed state, wherein the closed state of the implantable device, in a rigid state, is a three-dimensional curved shape; and wherein the implantable device shape is comprised of at least three arcs and two interconnecting sections.

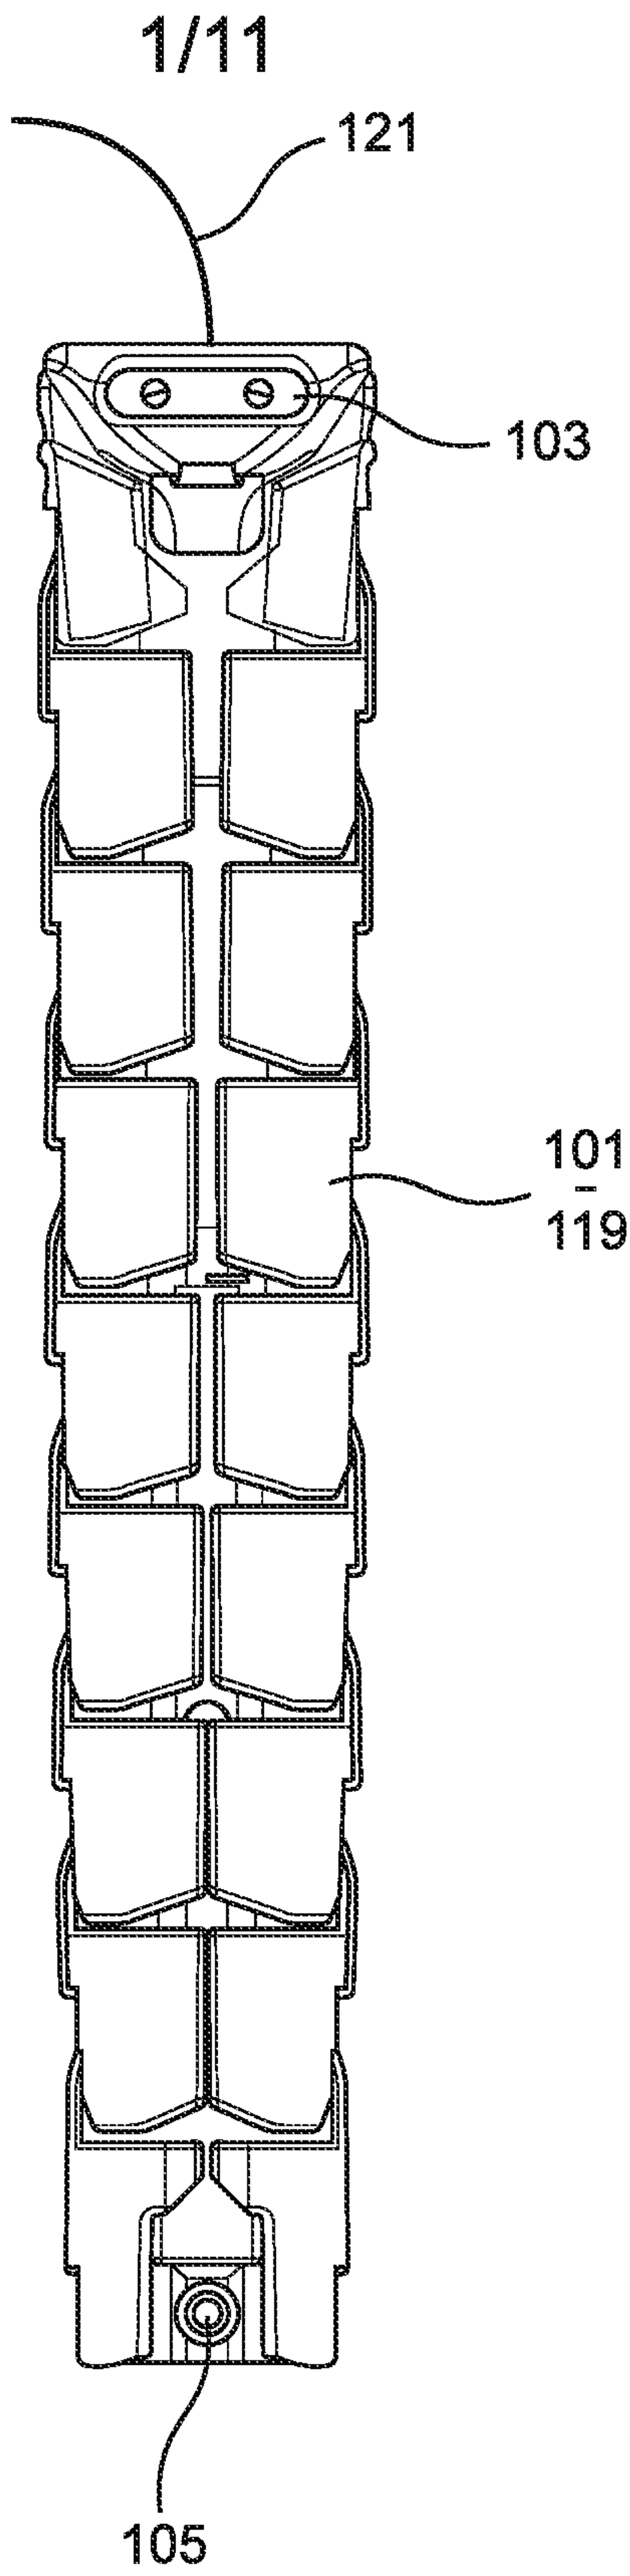


FIG. 1A

2/11

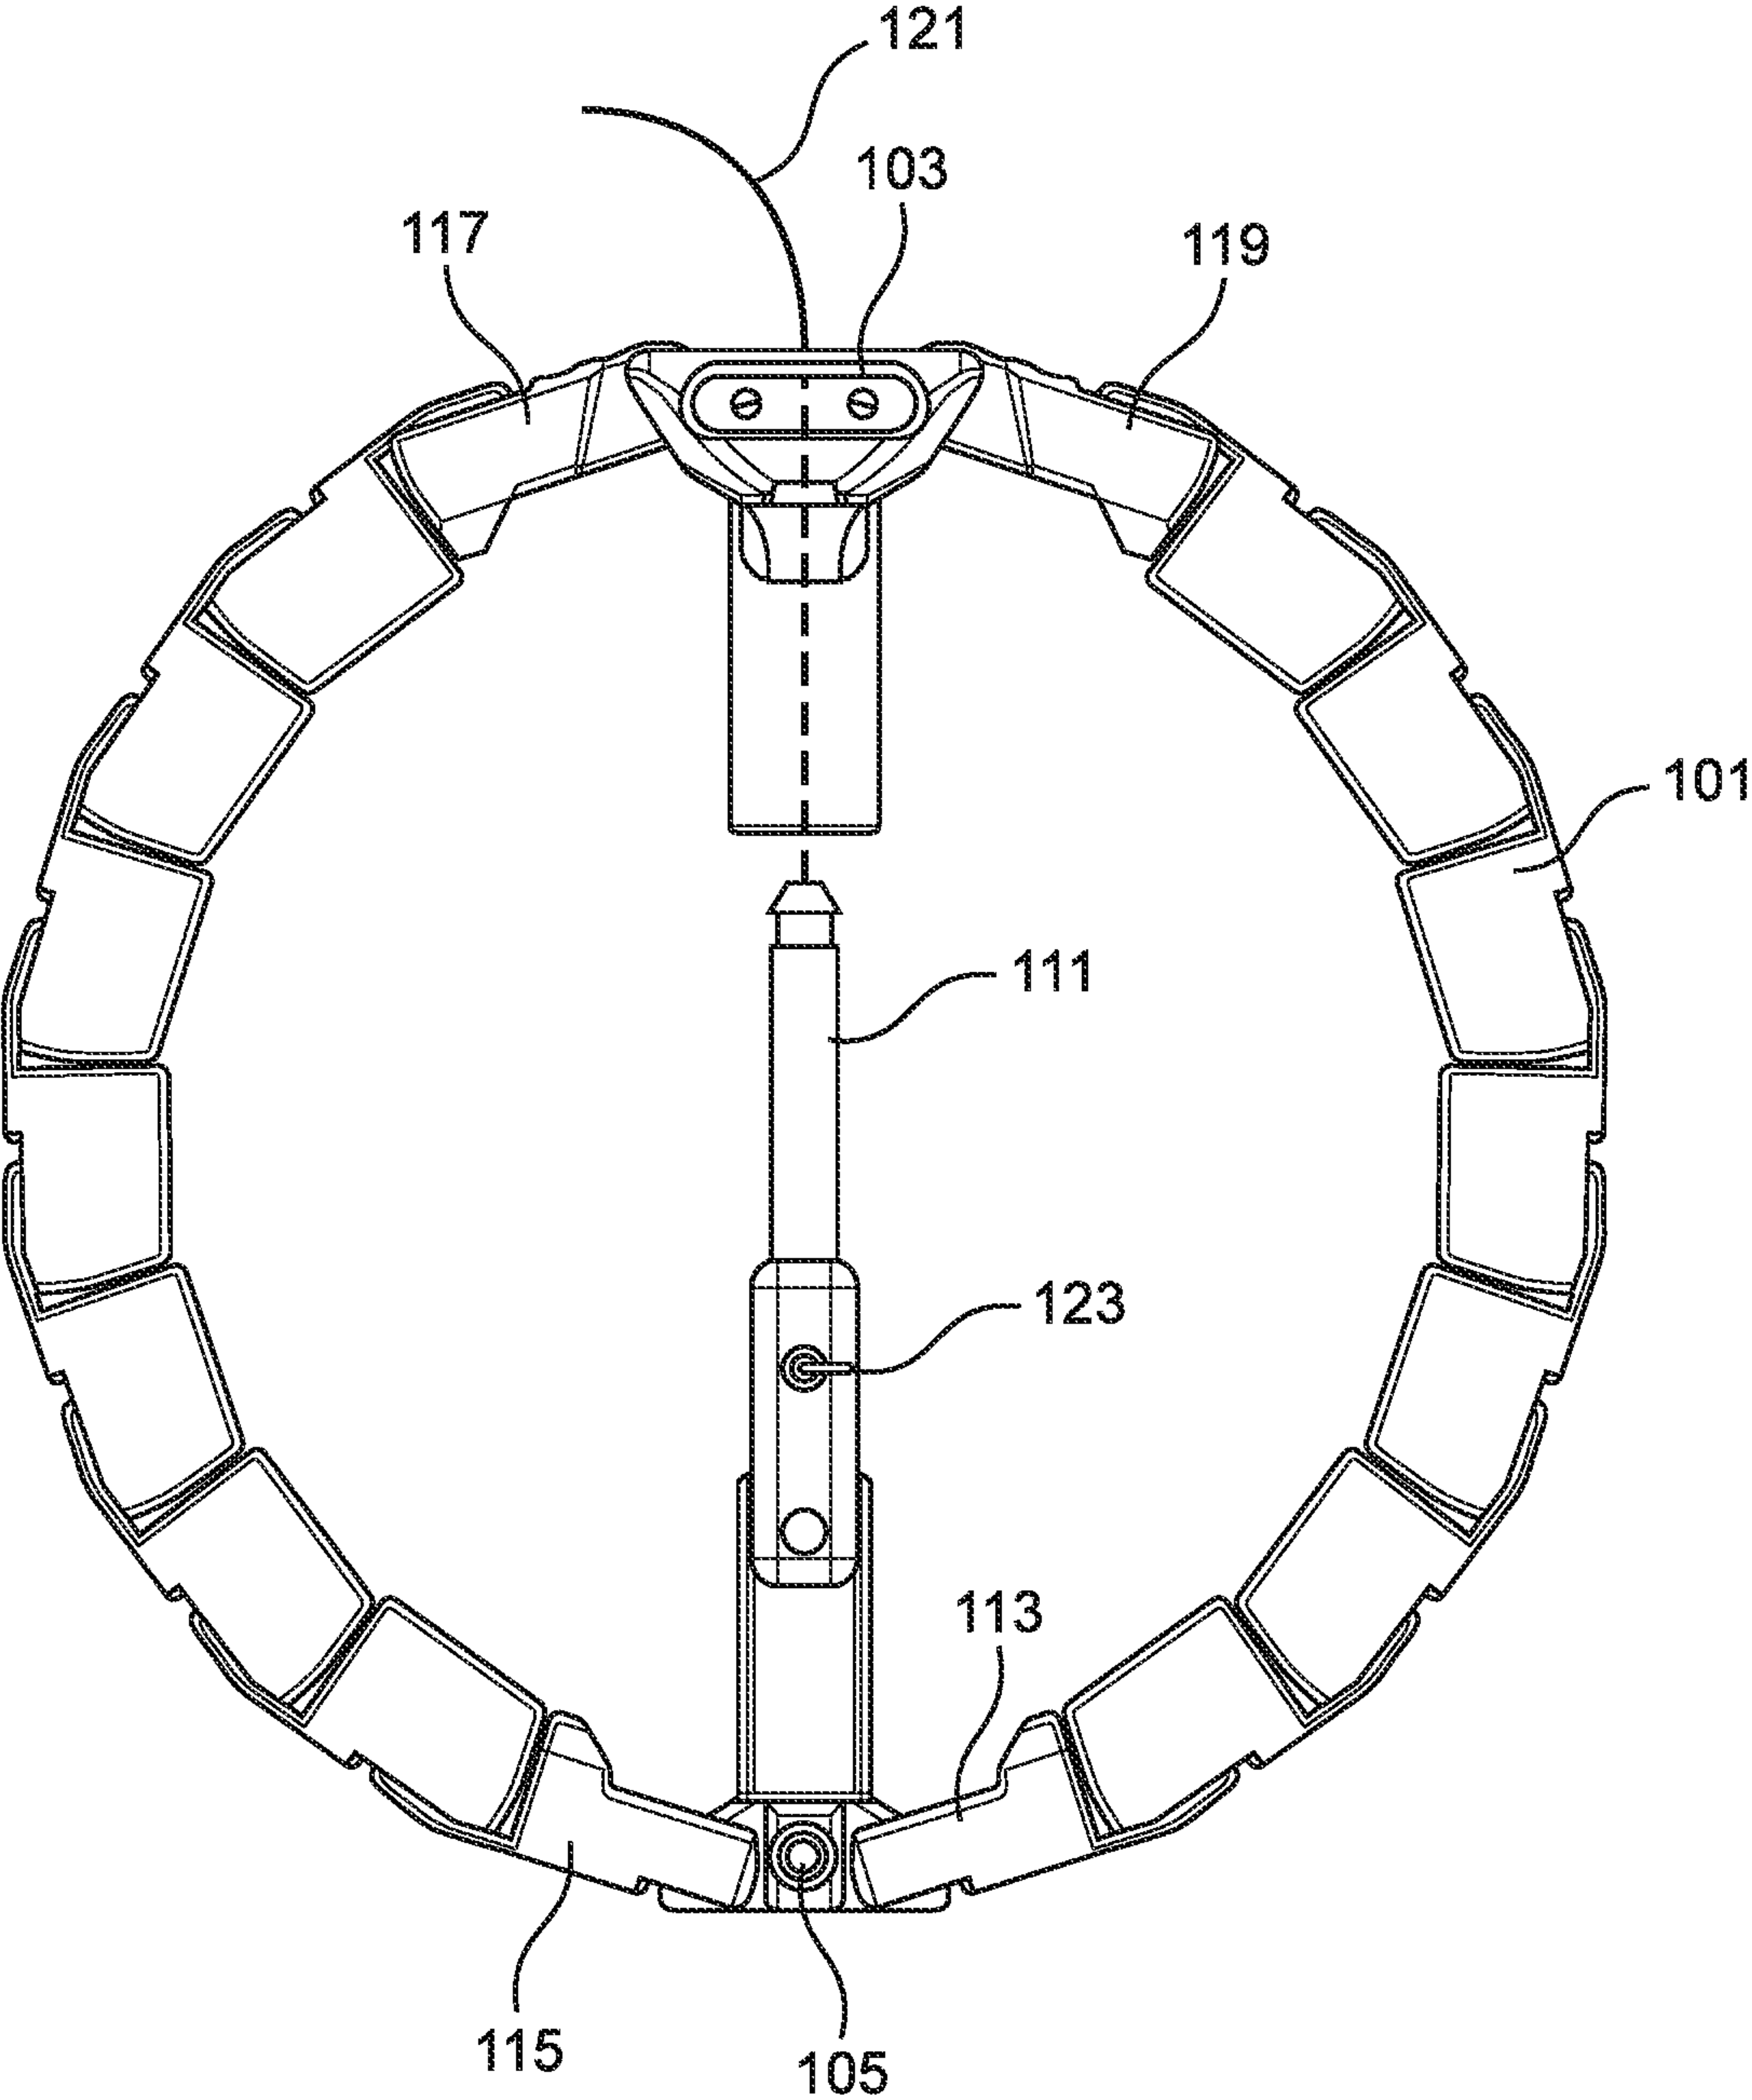


FIG. 1B

3/11

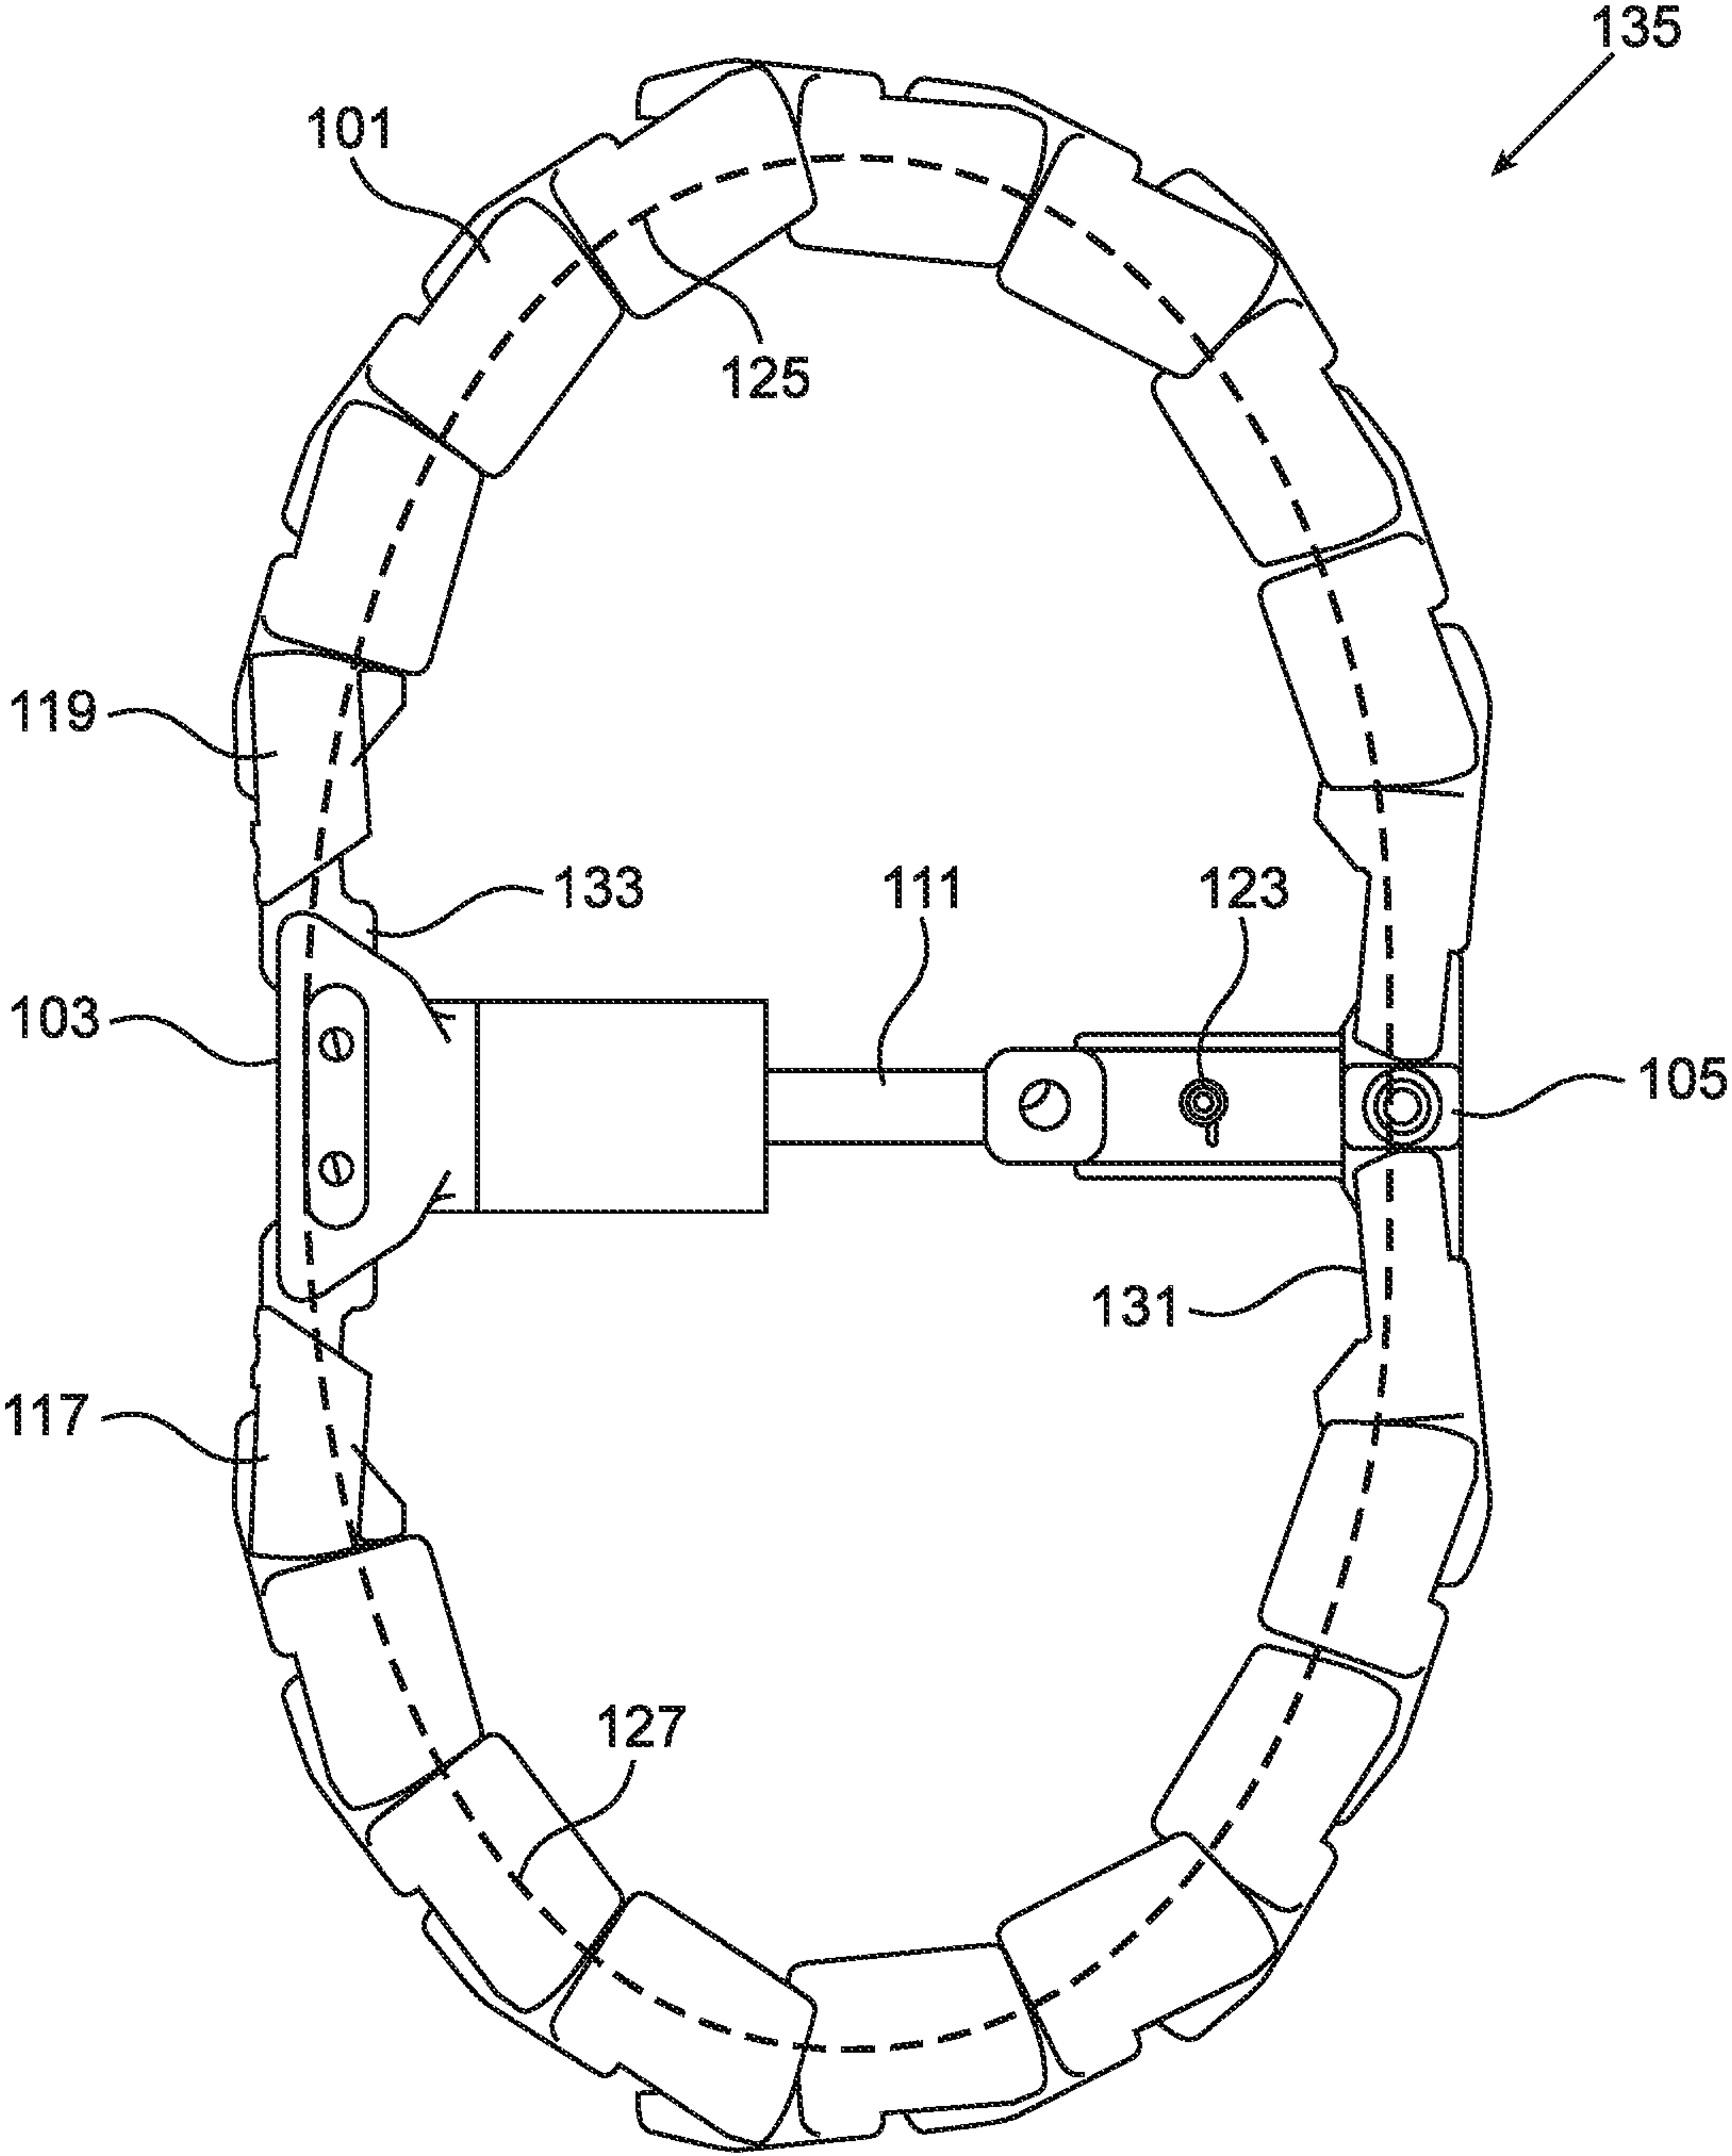


FIG. 1C

4/11

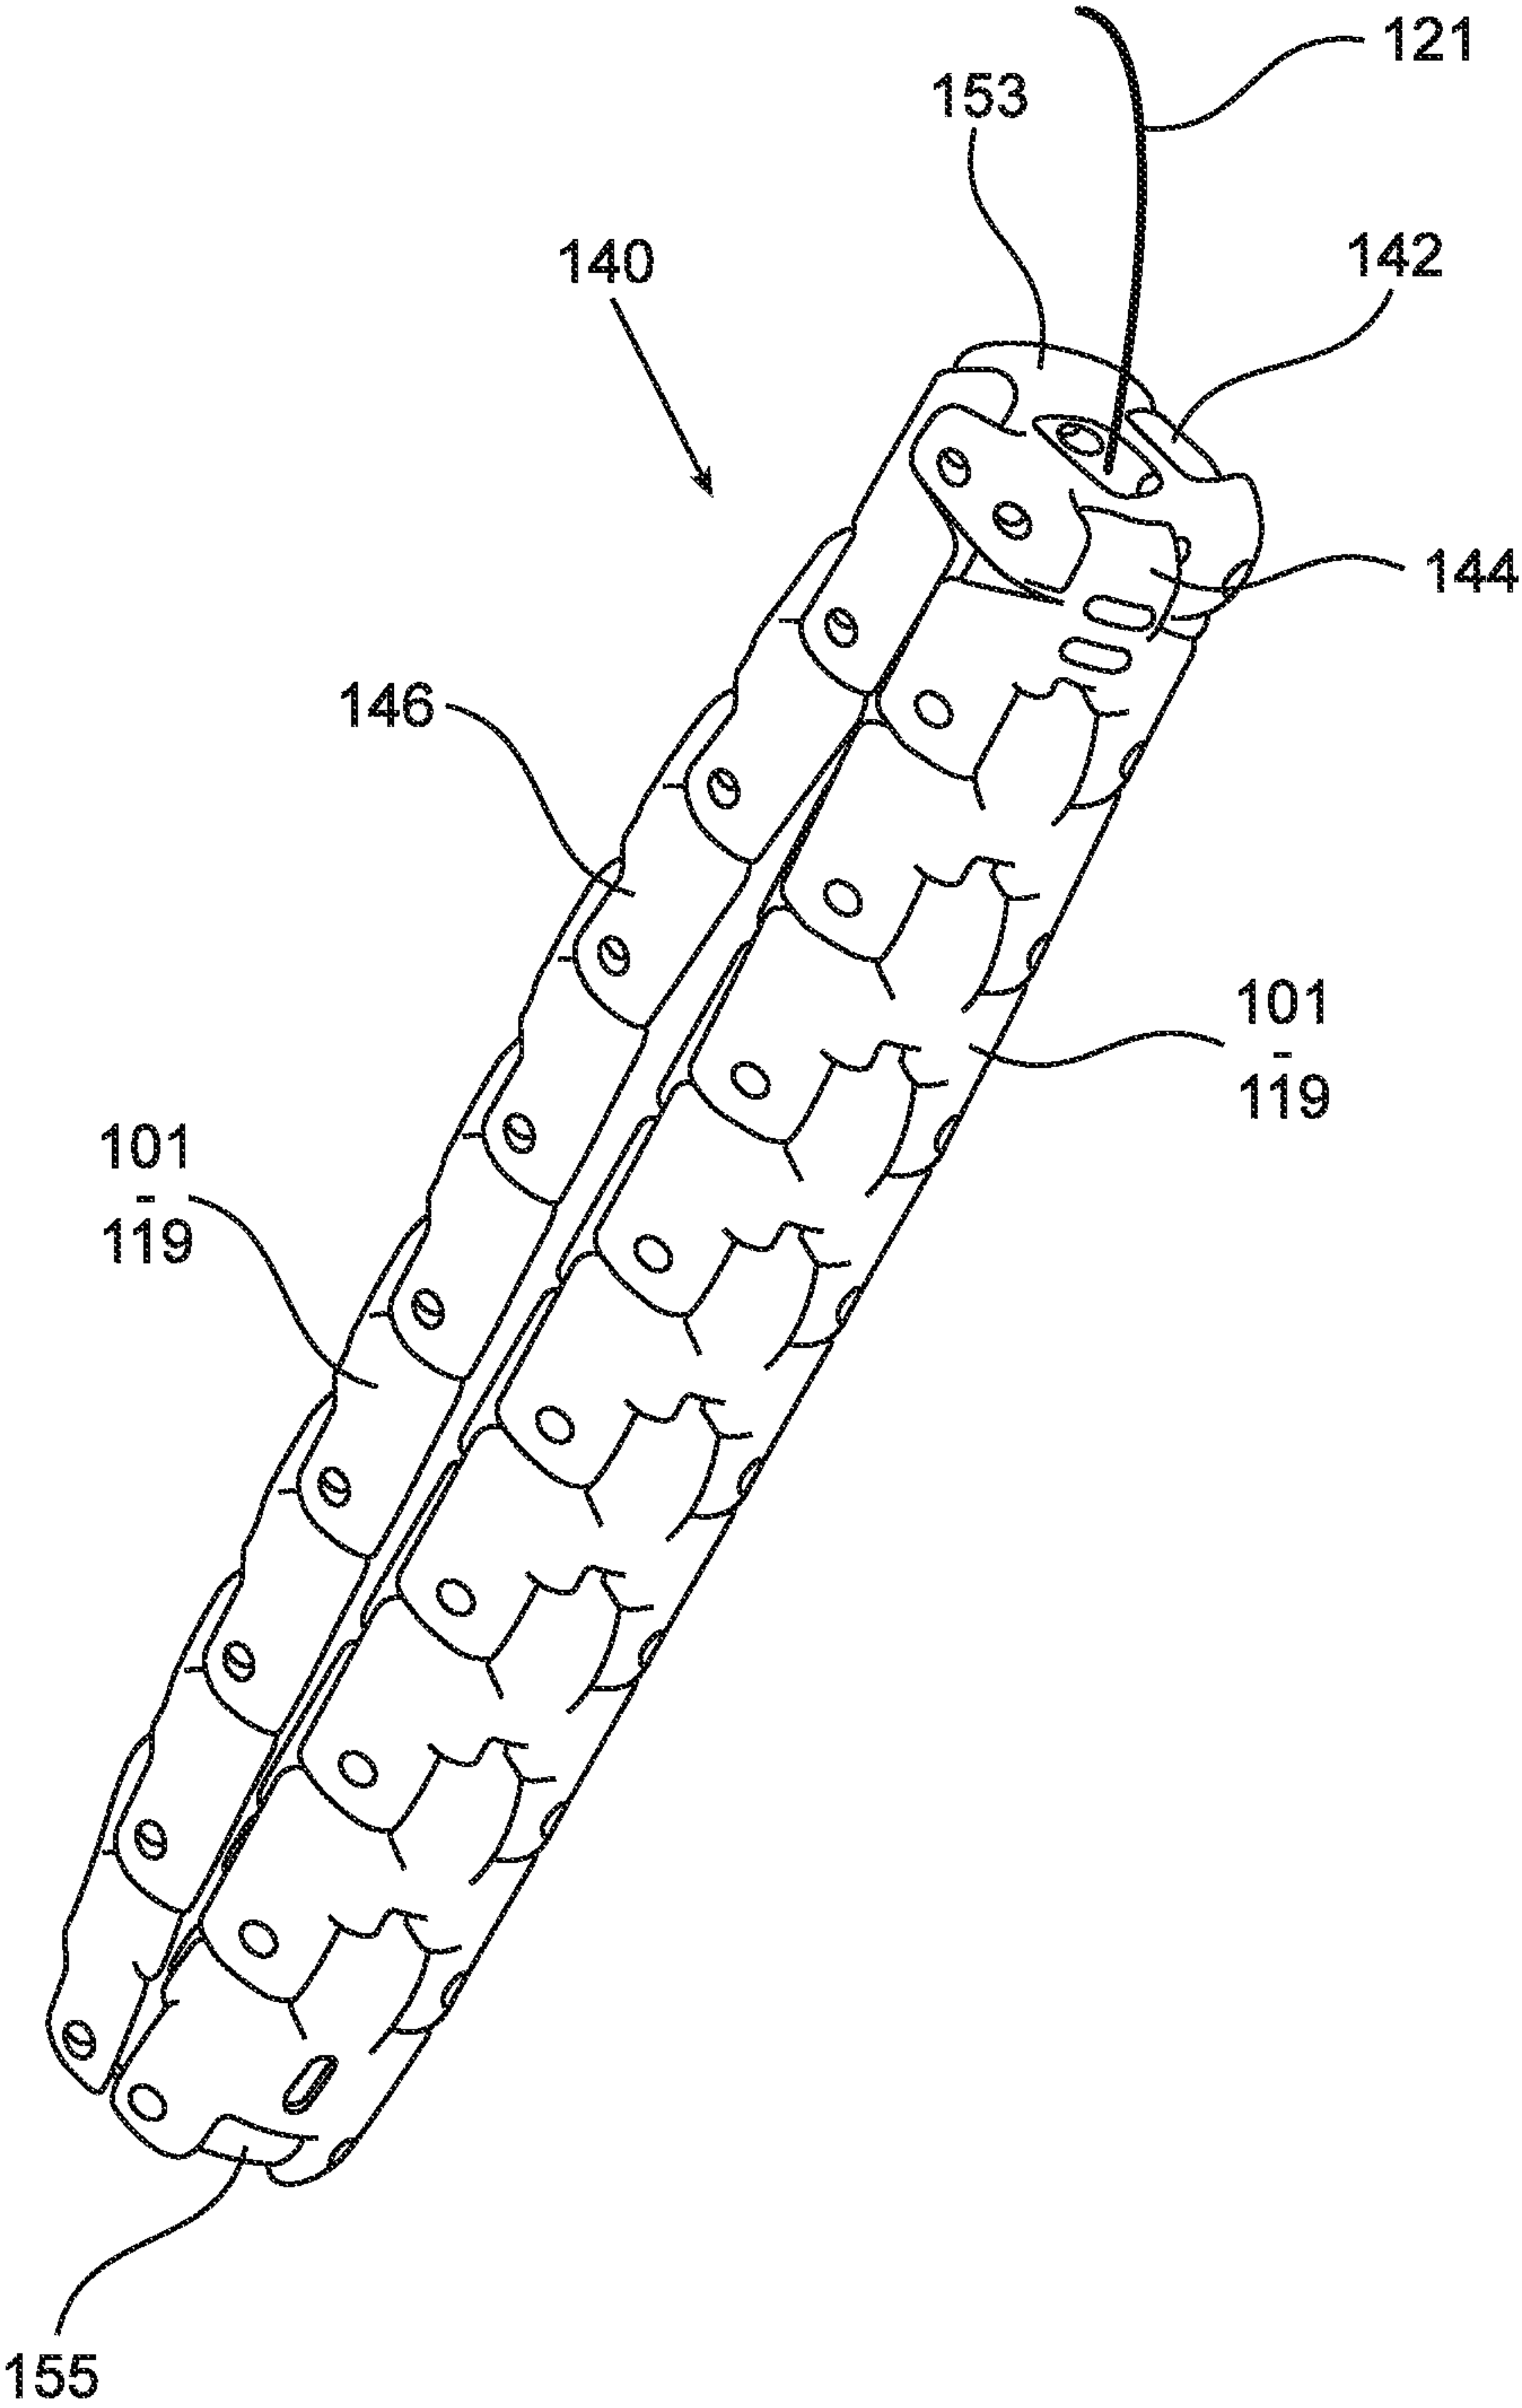


FIG. 1D

5/11

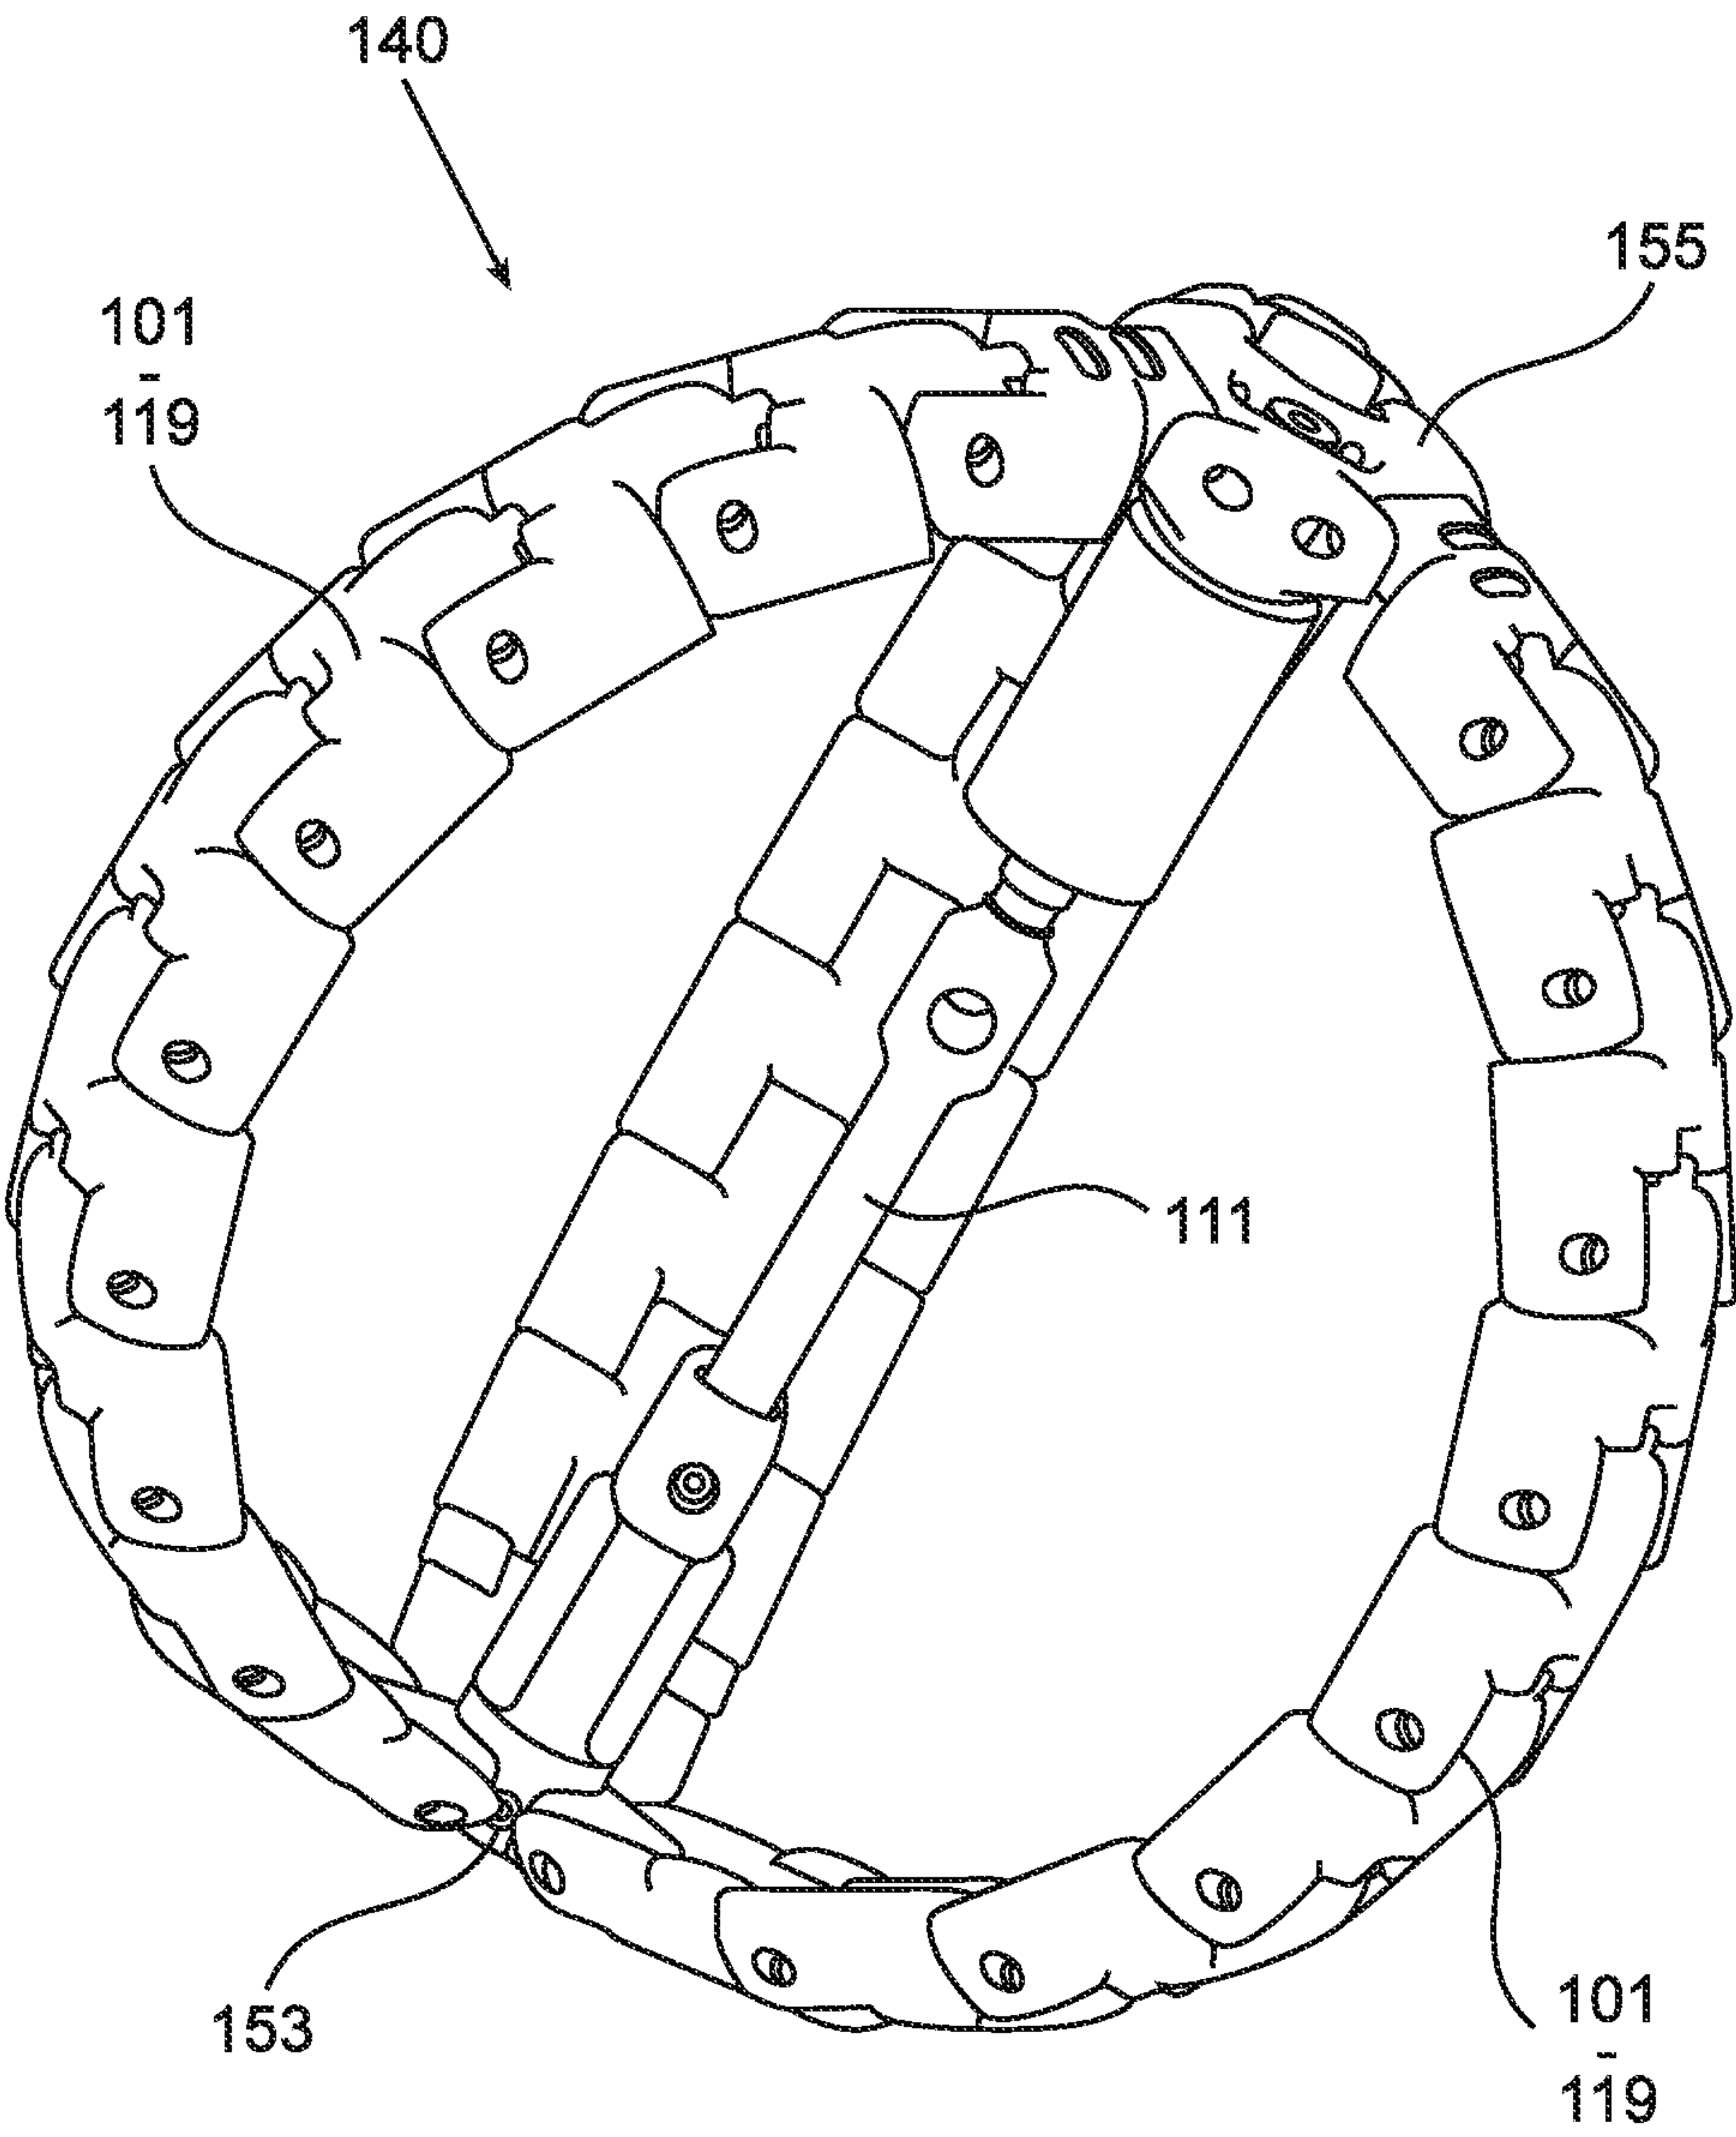


FIG. 1E

6/11

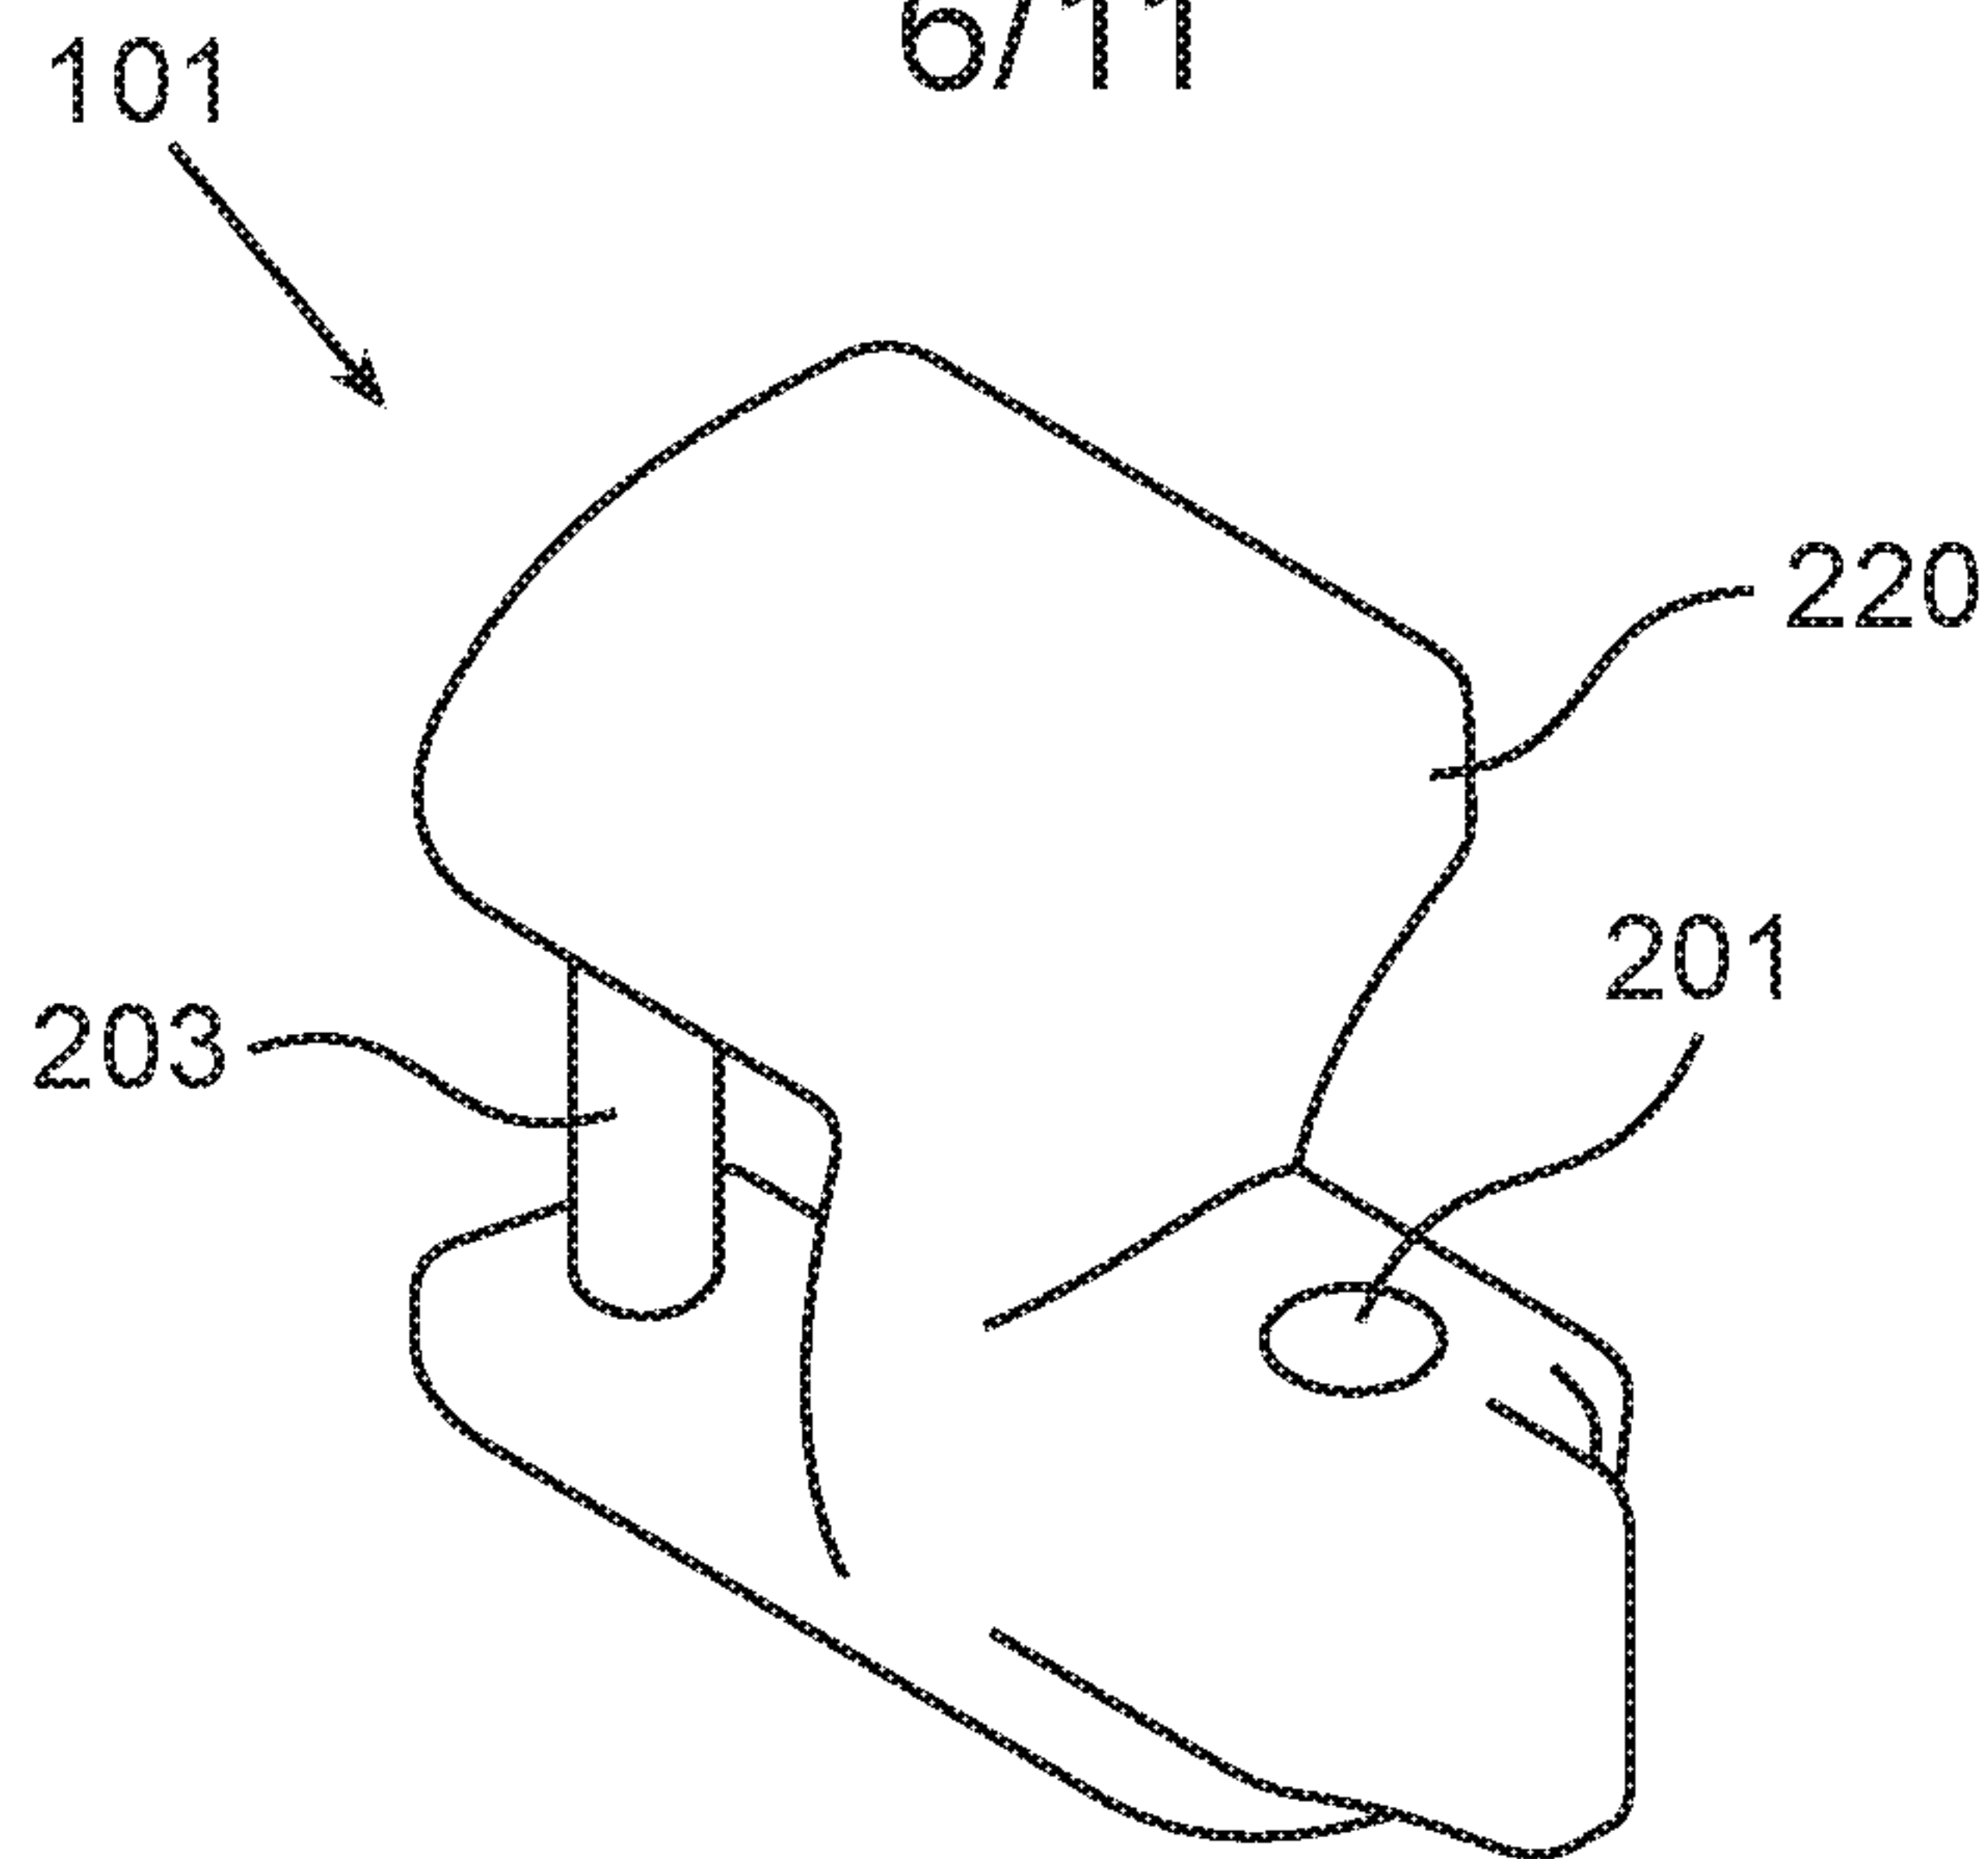


FIG. 2A

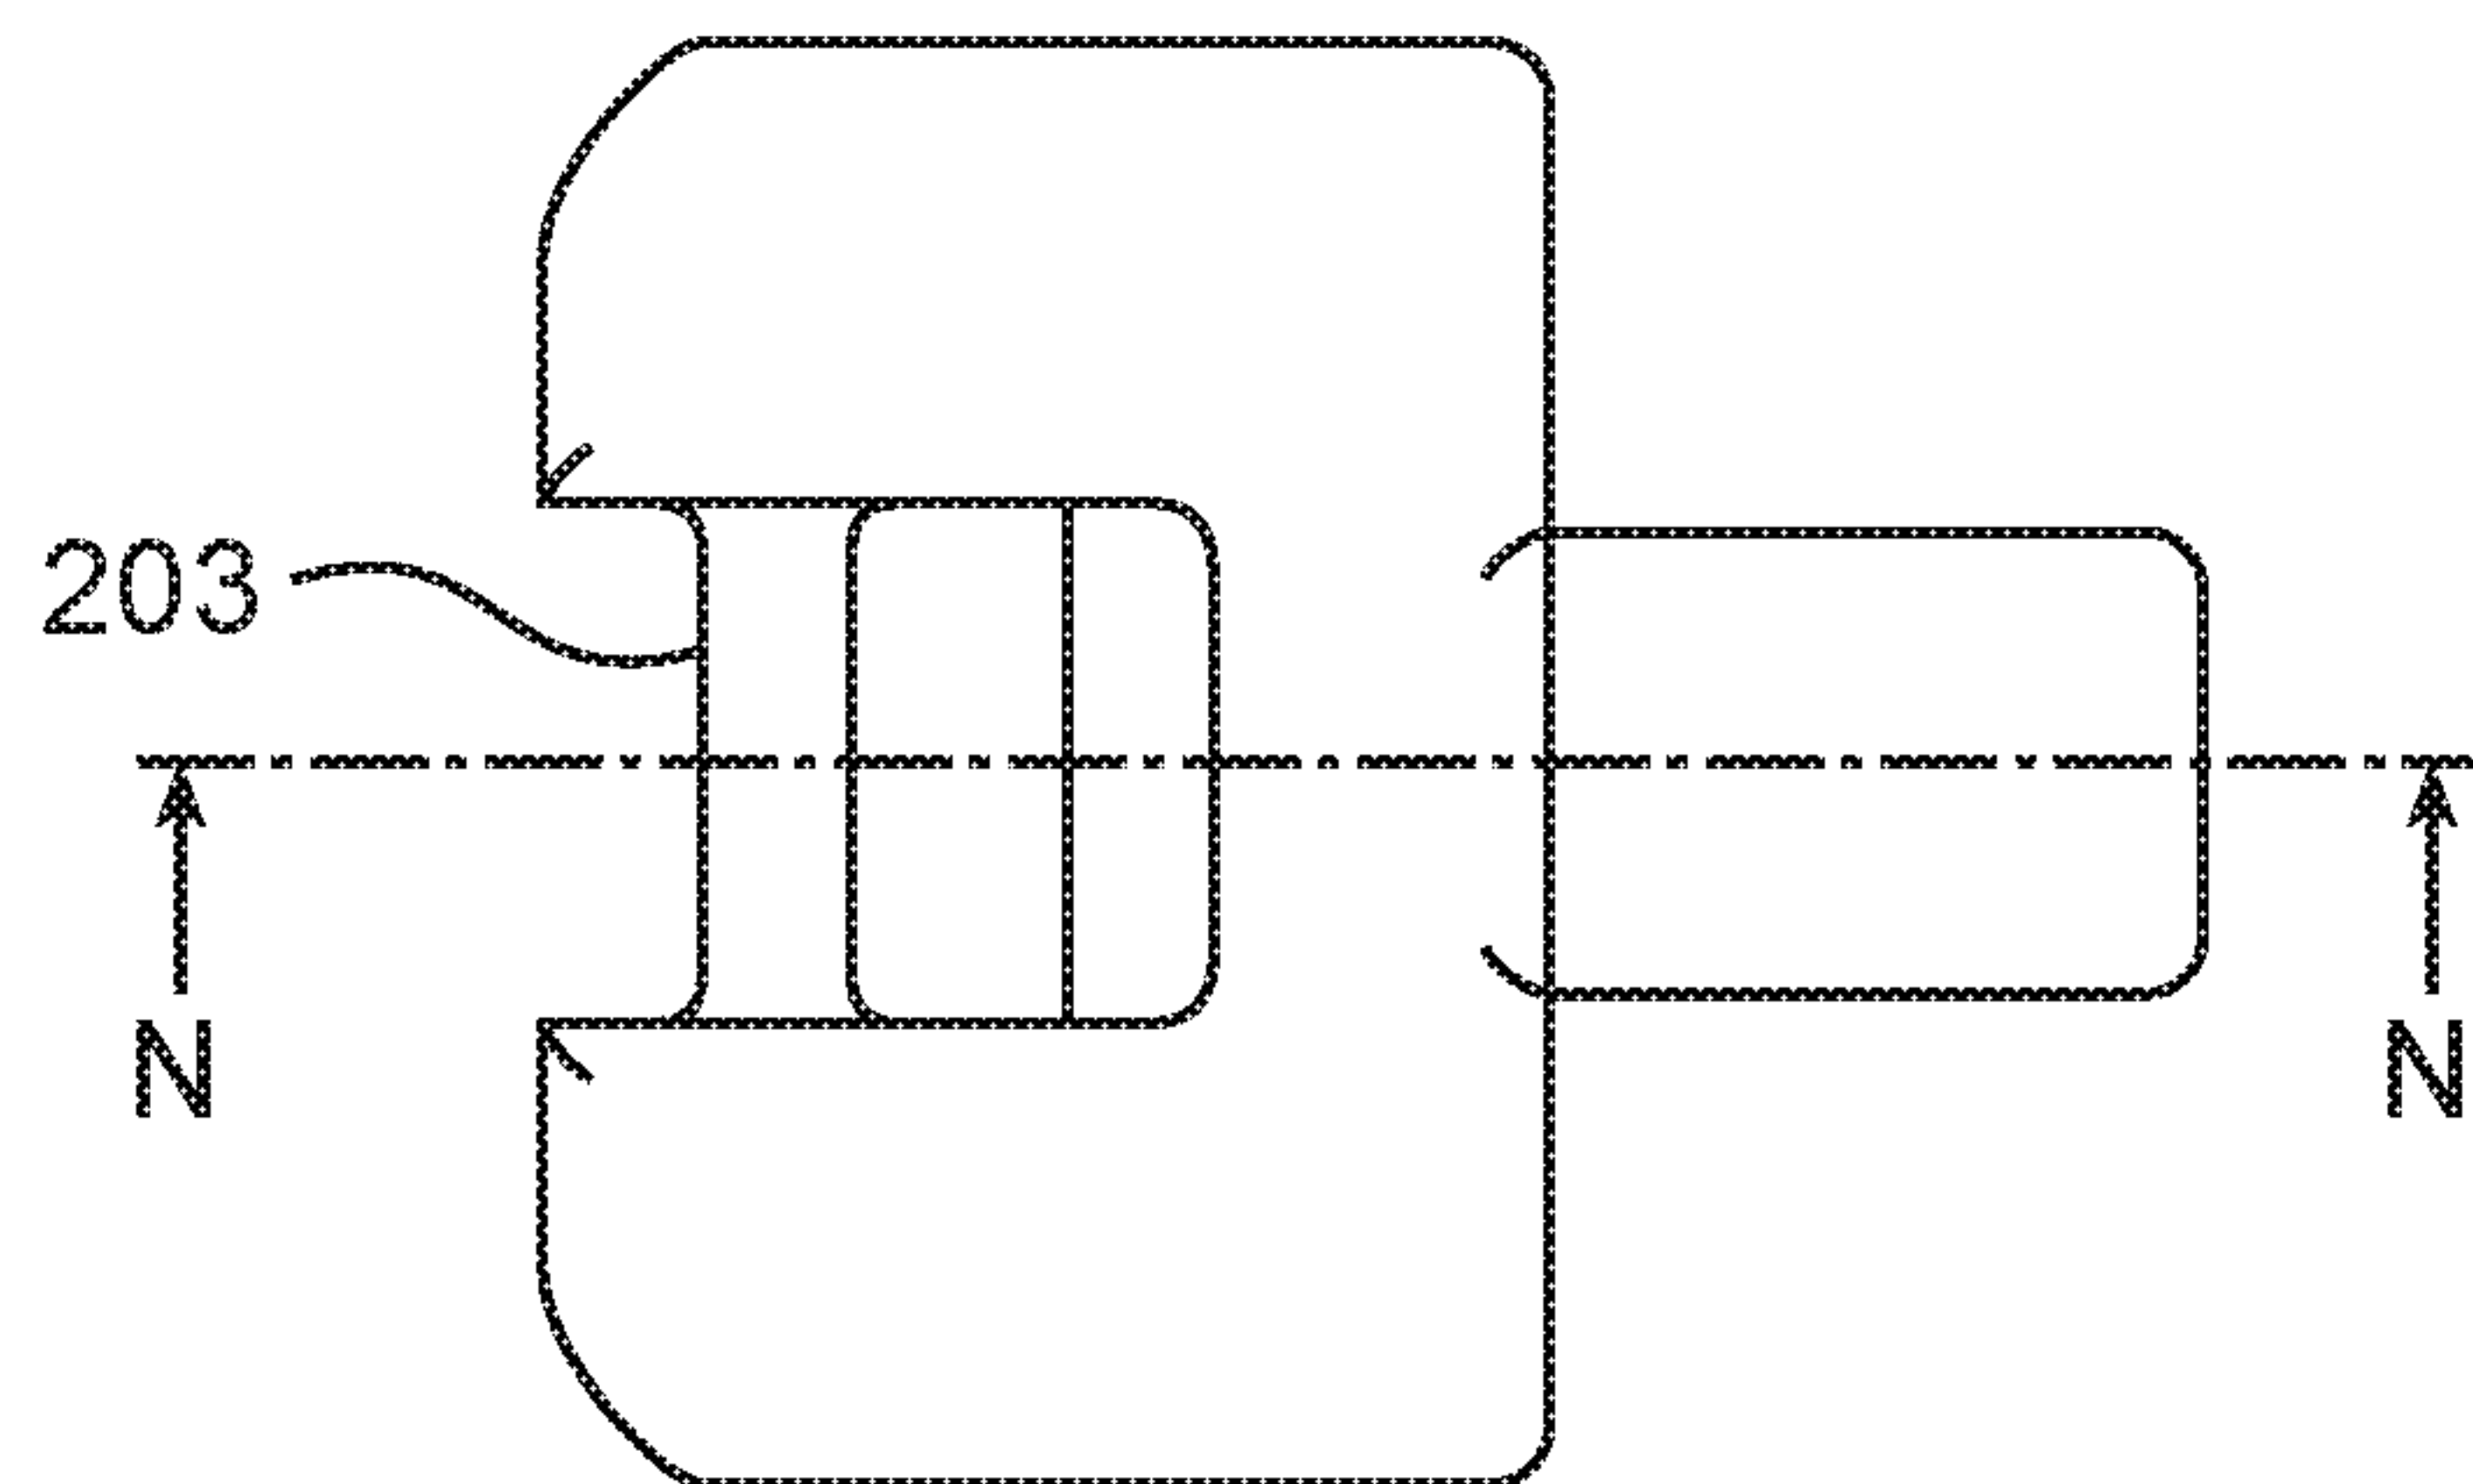


FIG. 2B

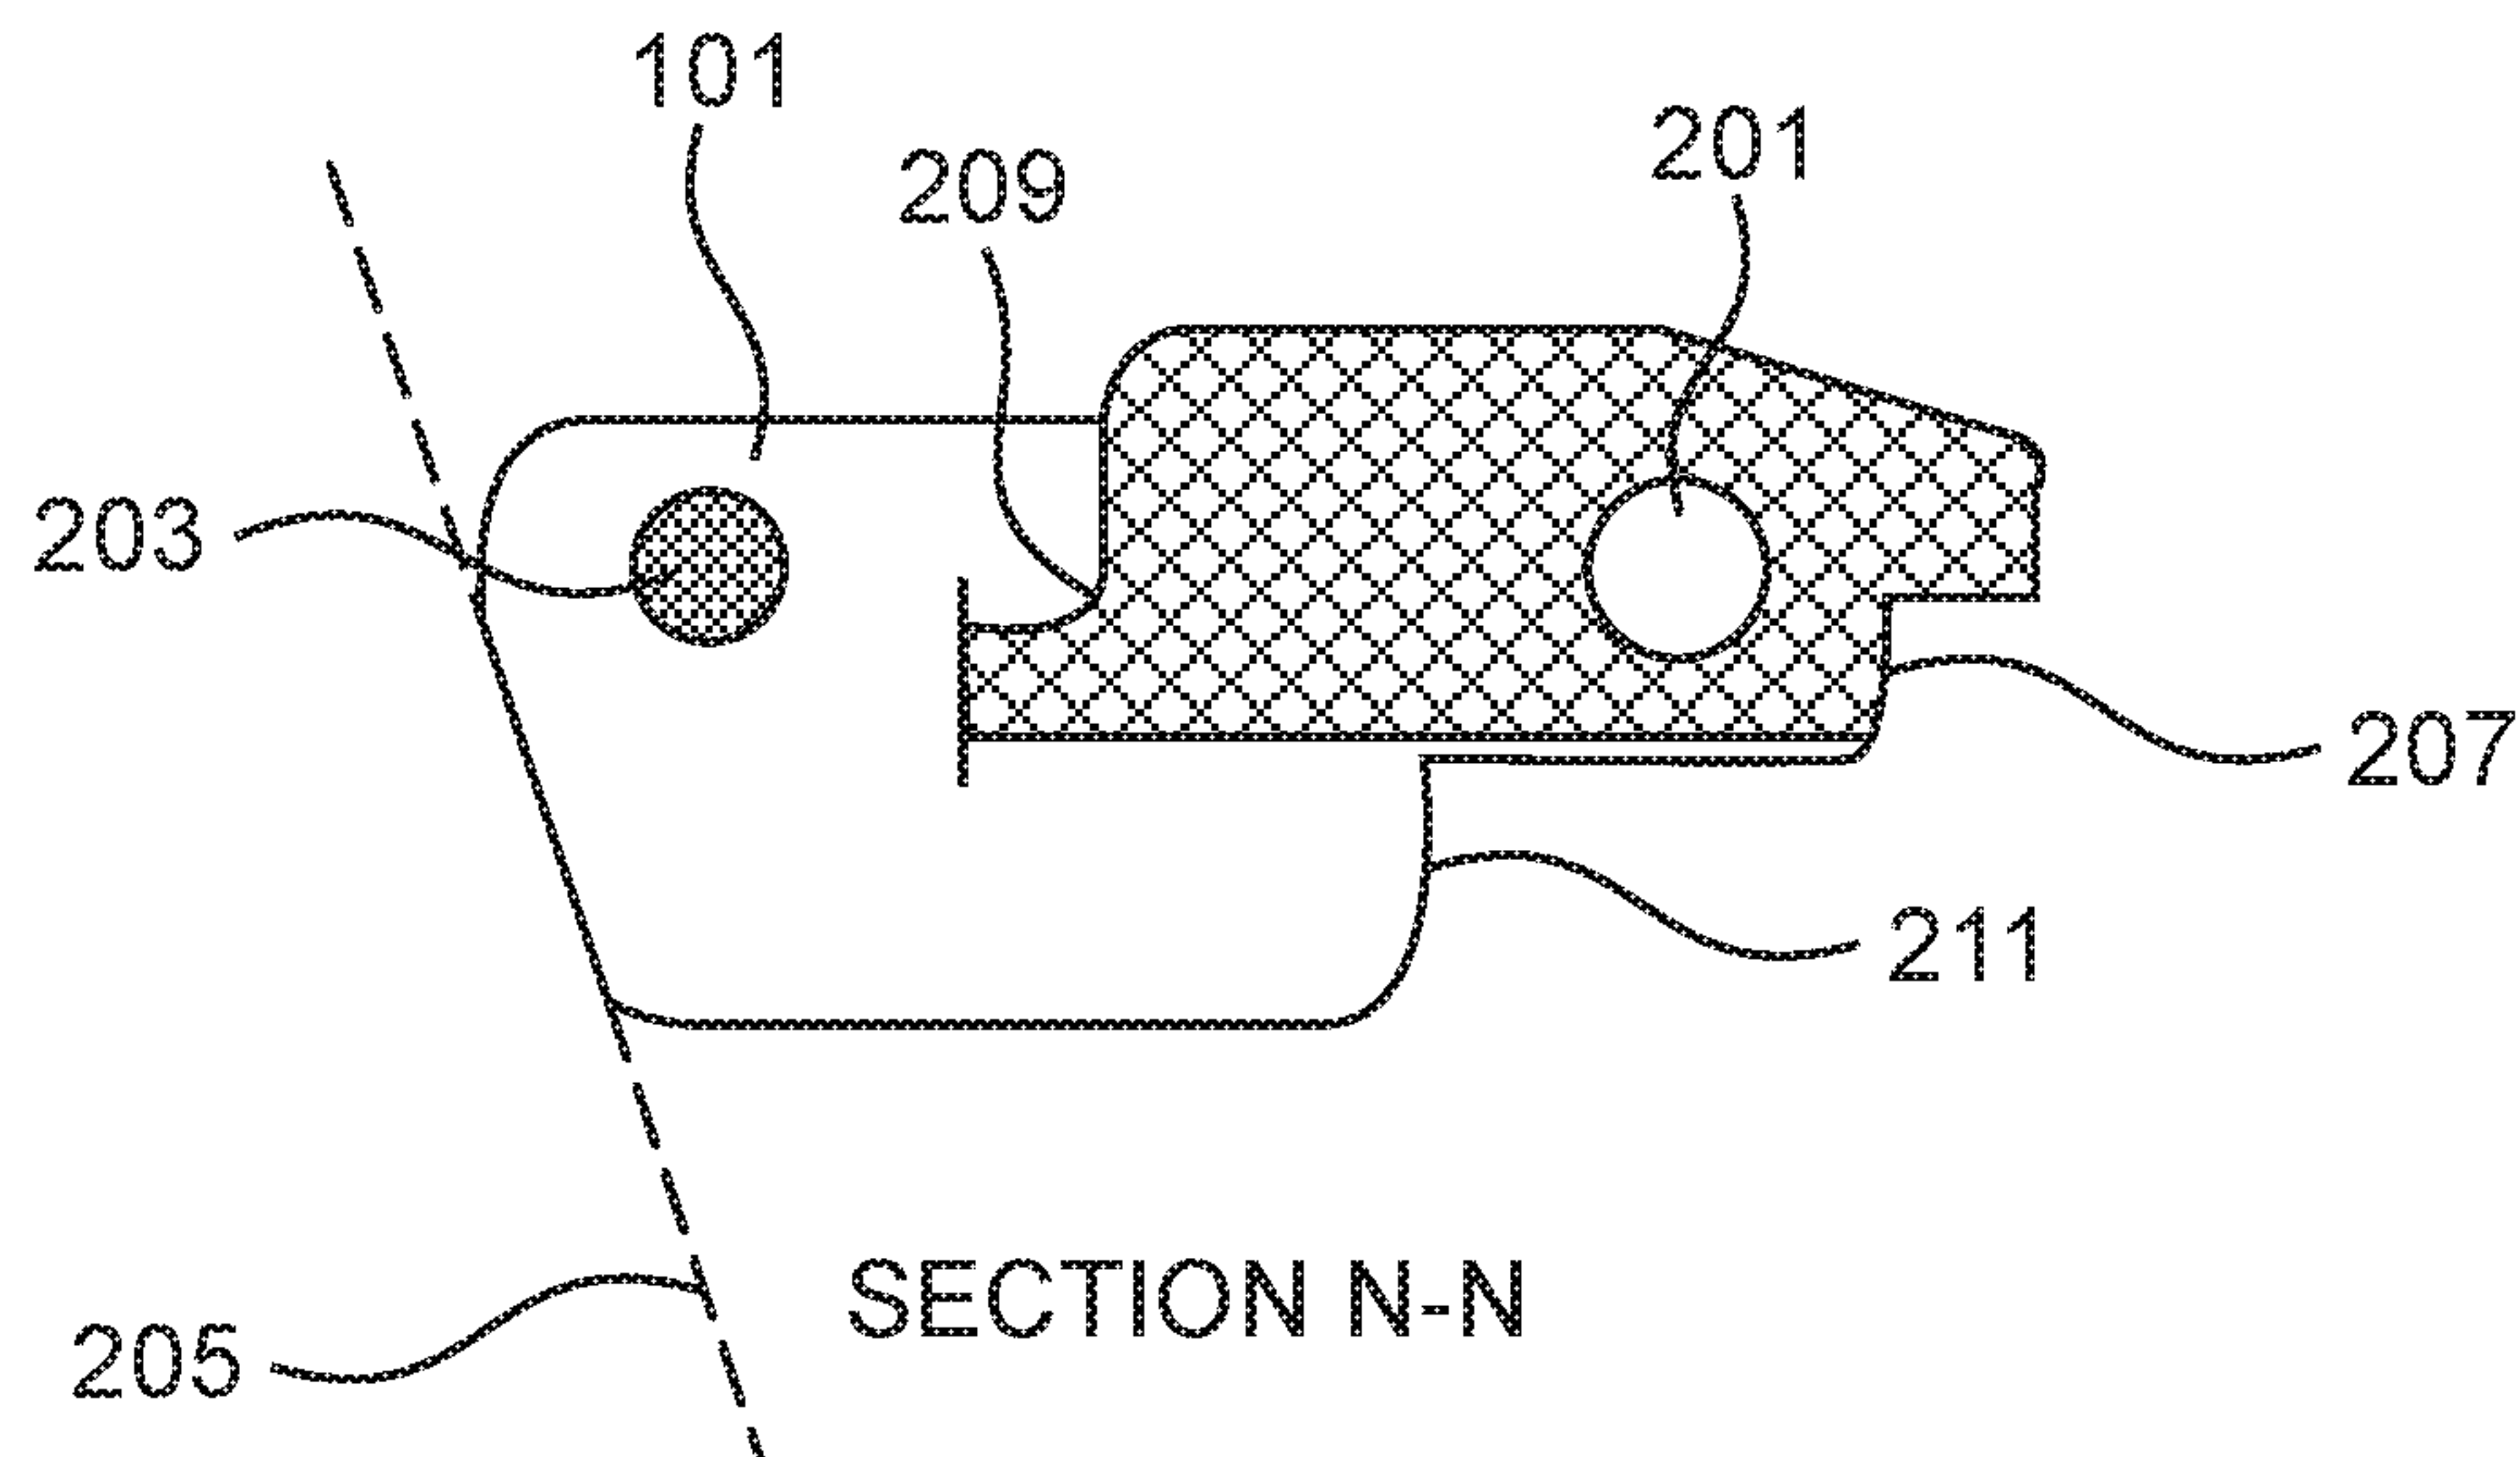


FIG. 2C

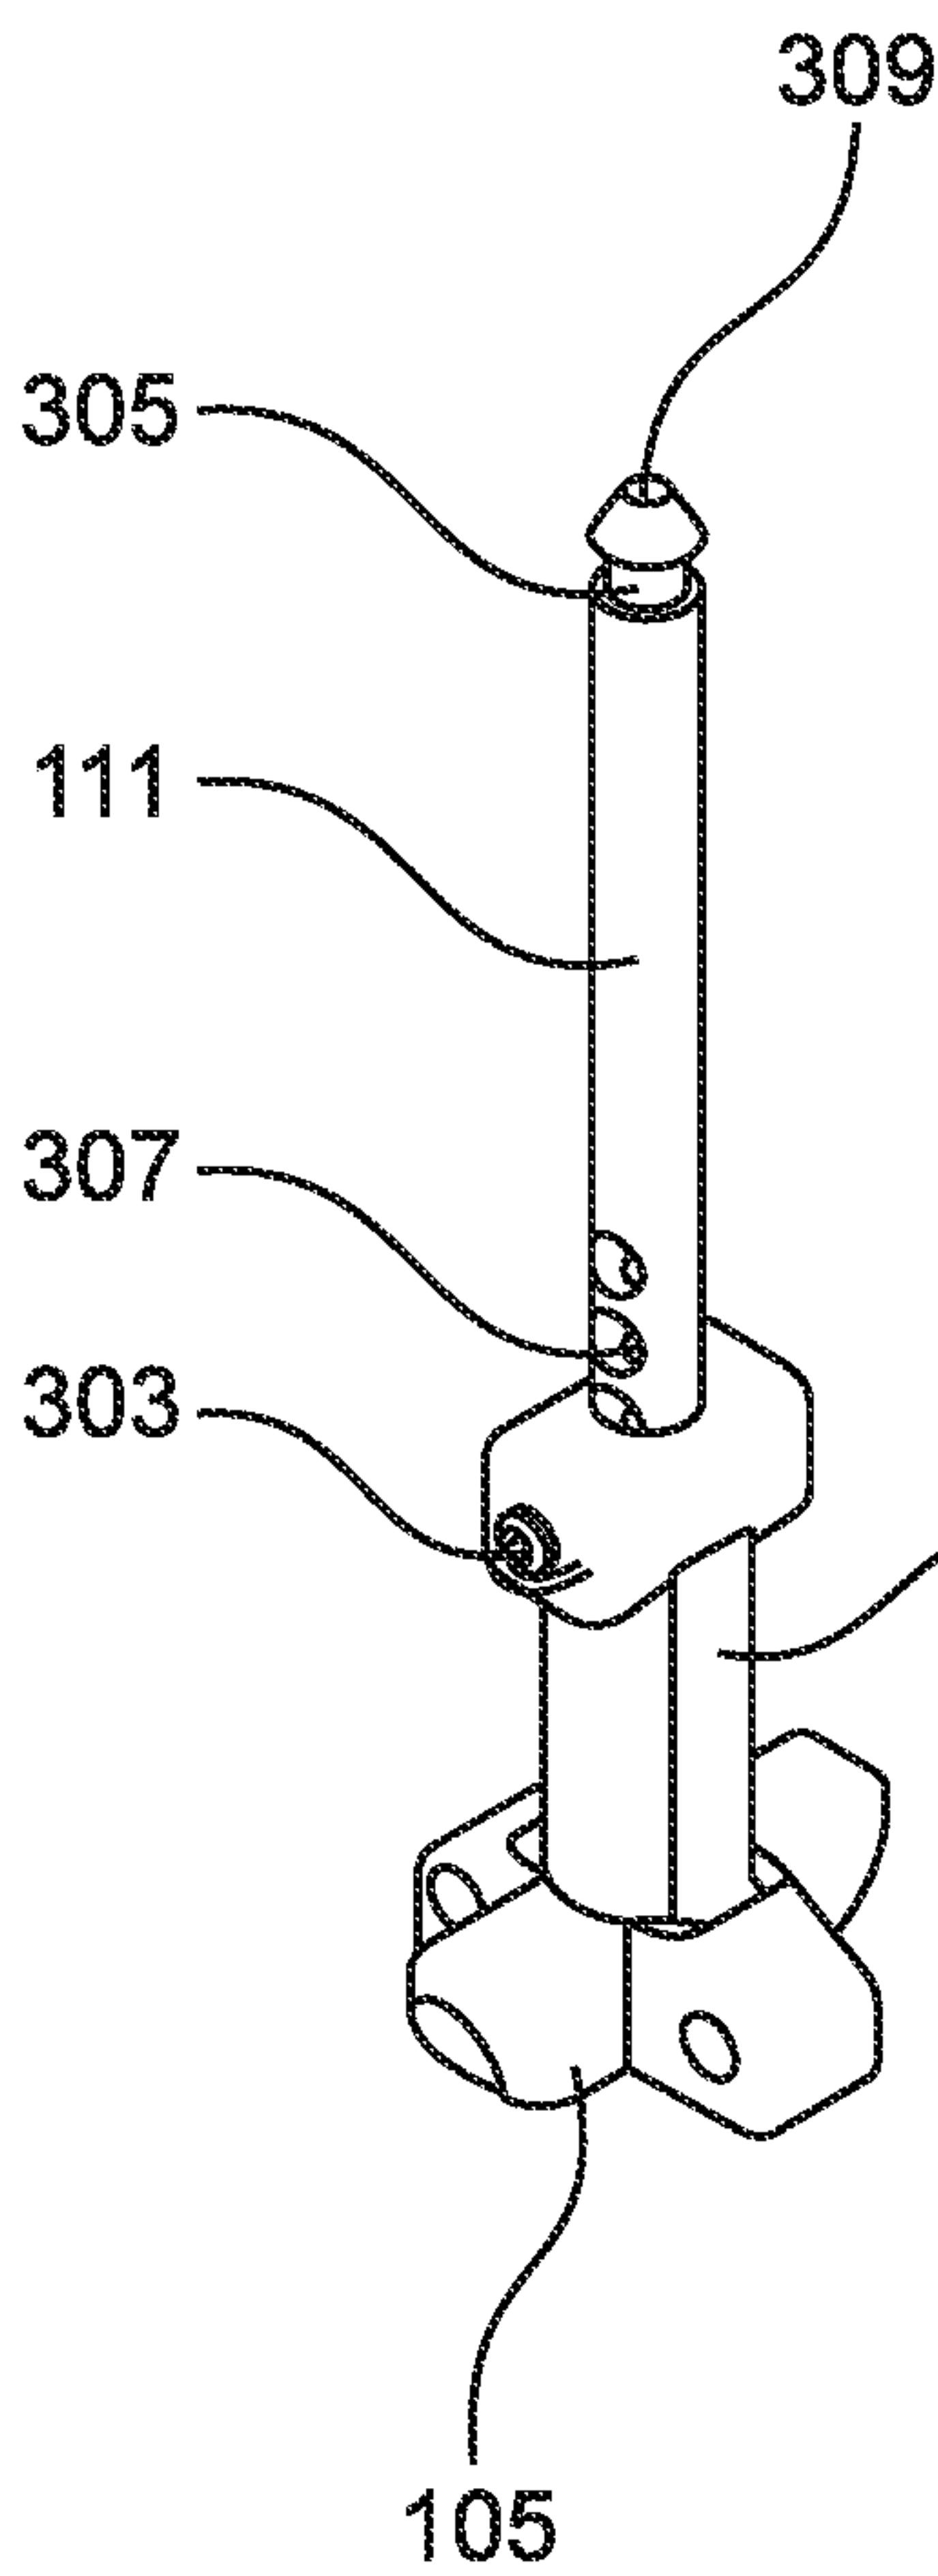


FIG. 3A

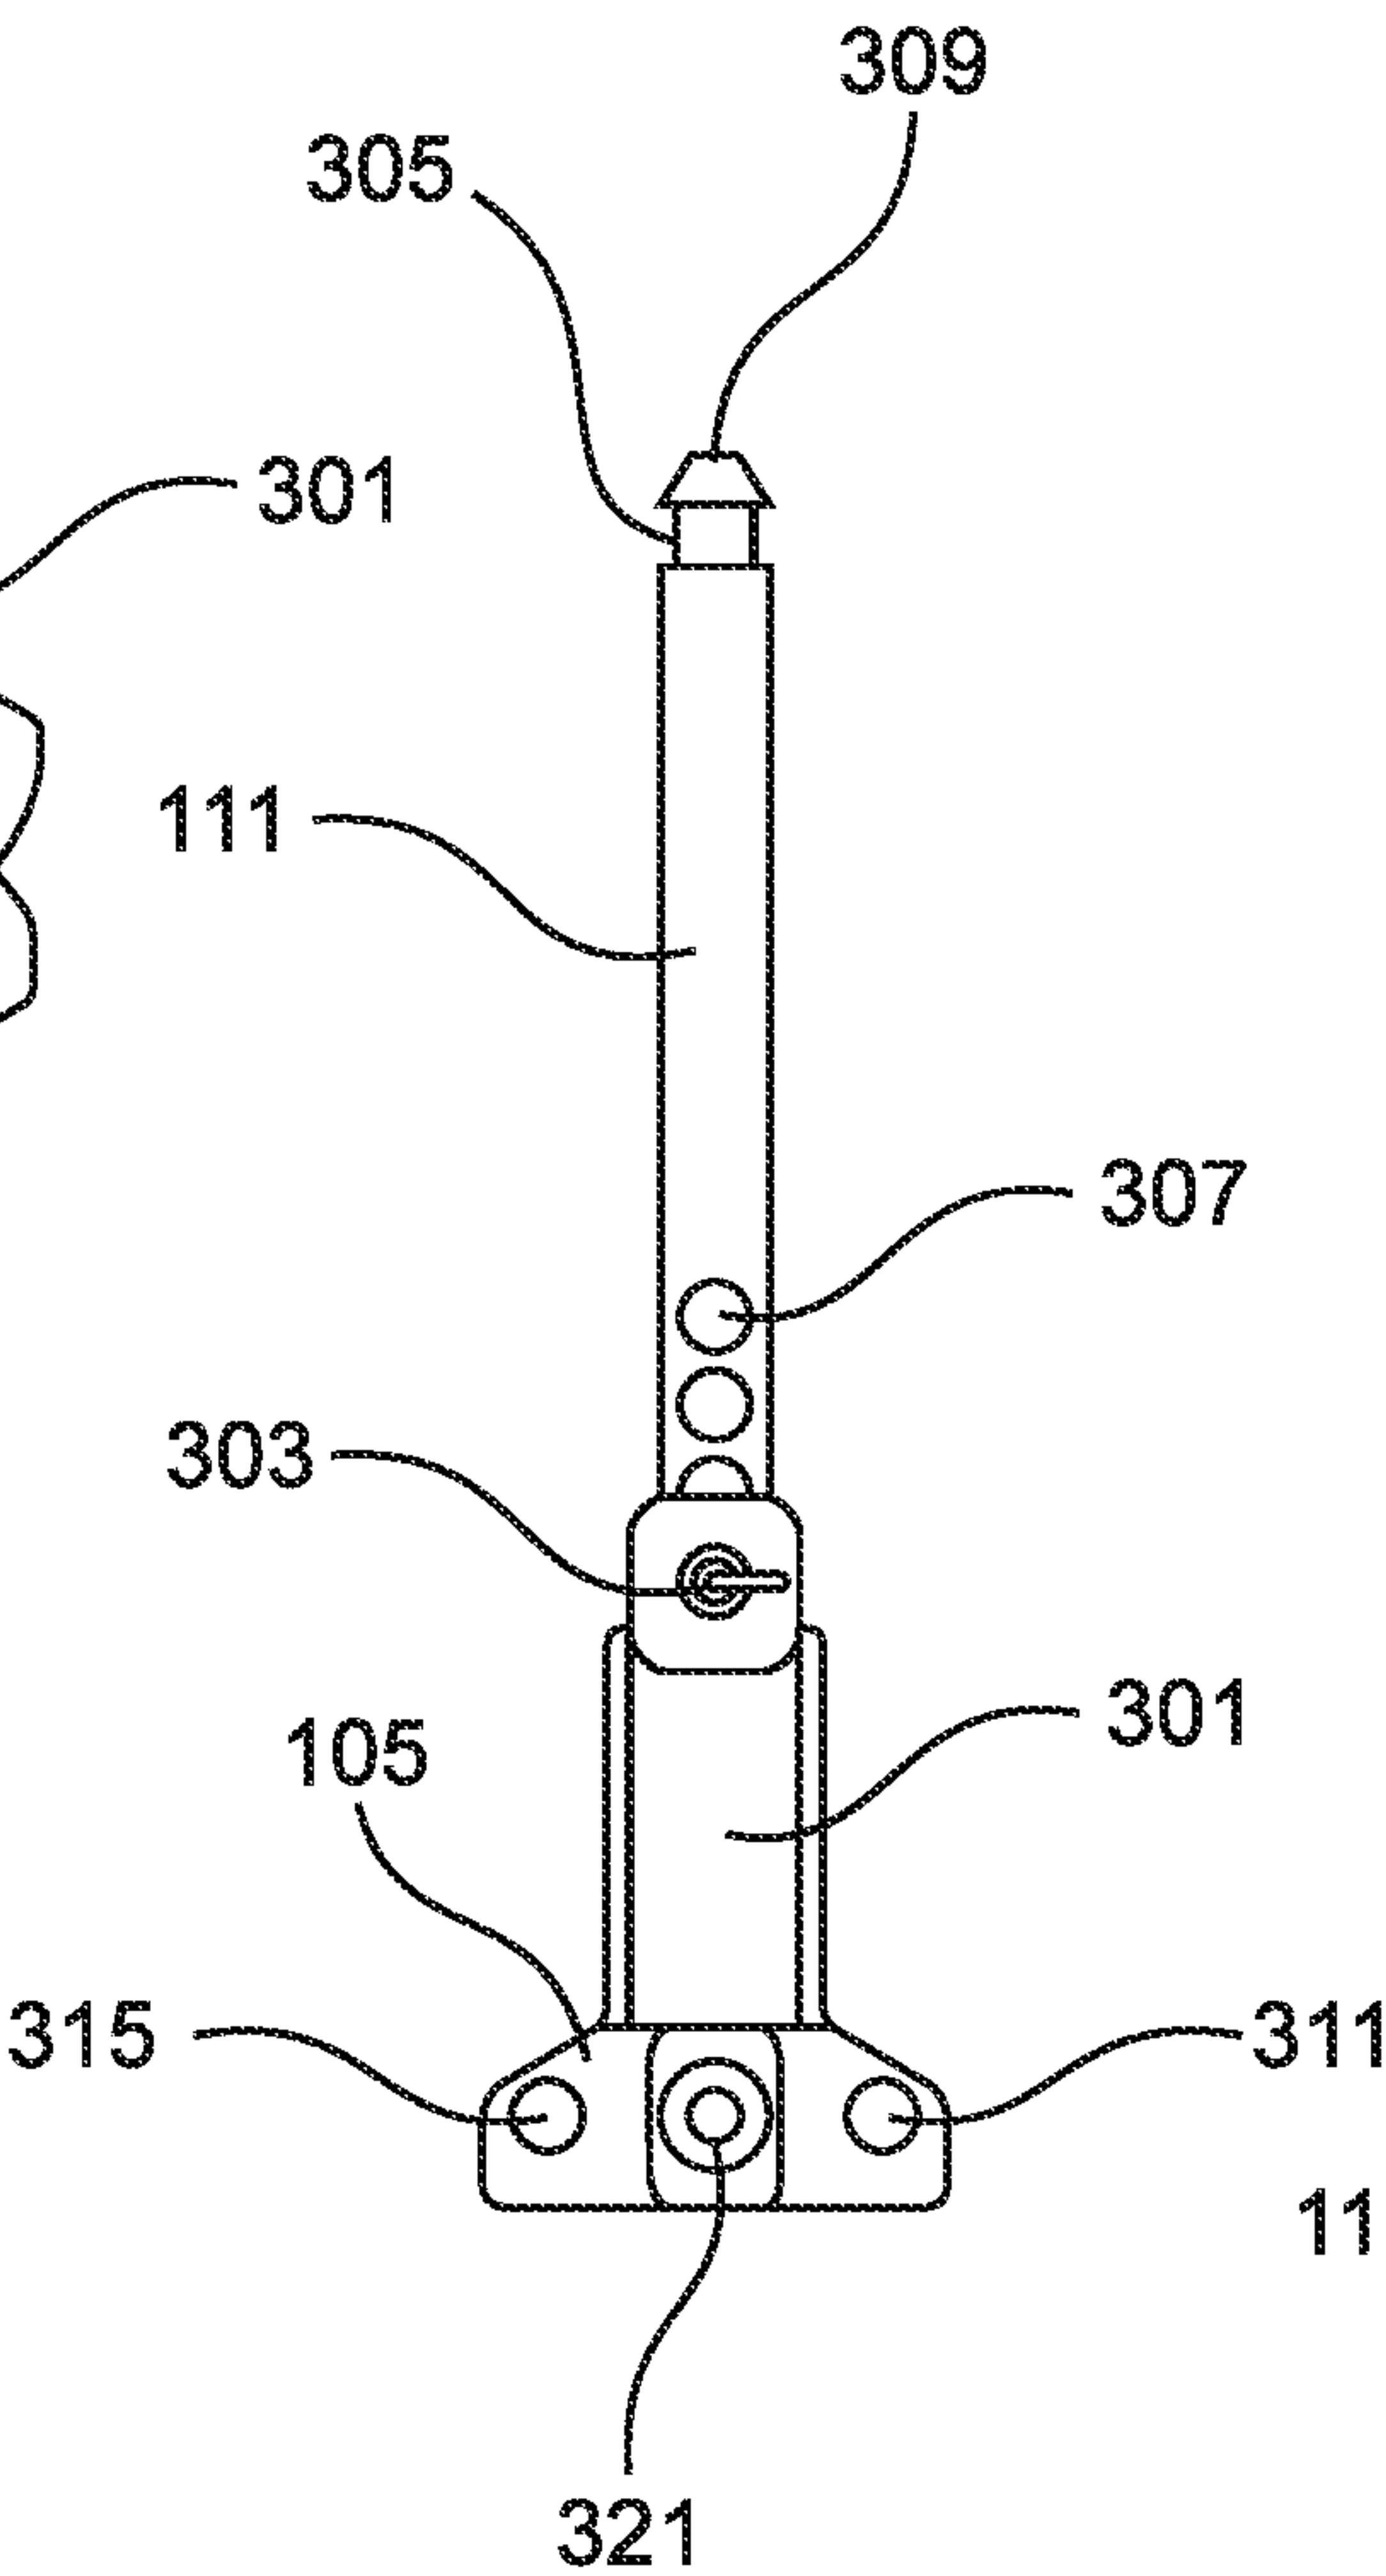


FIG. 3B

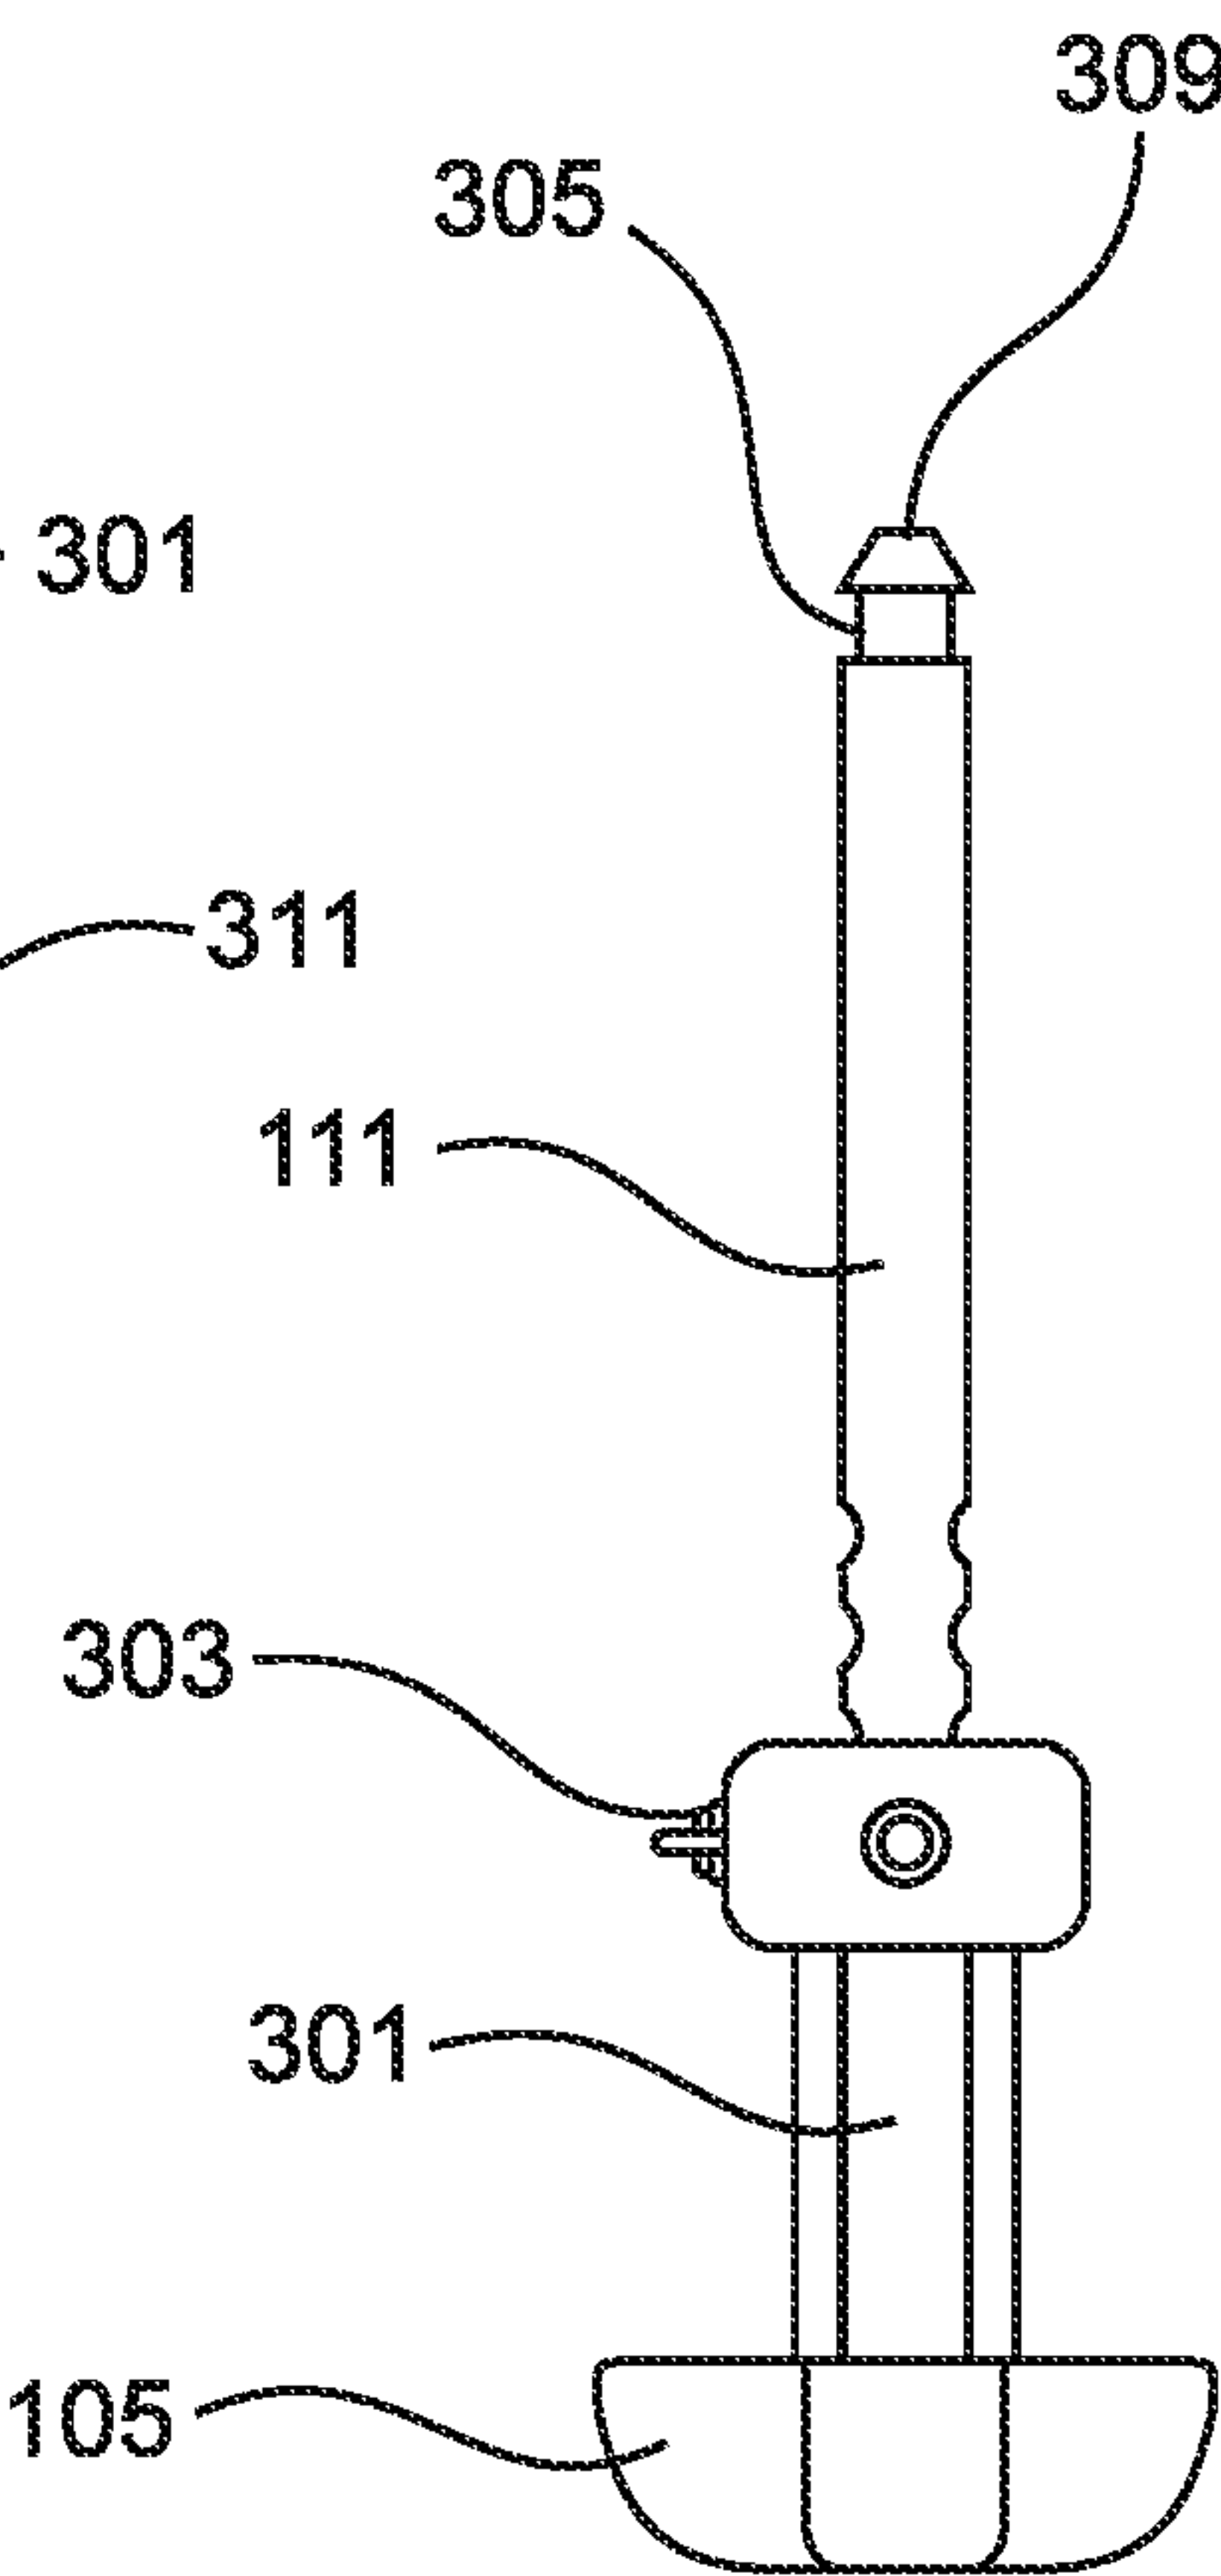


FIG. 3C

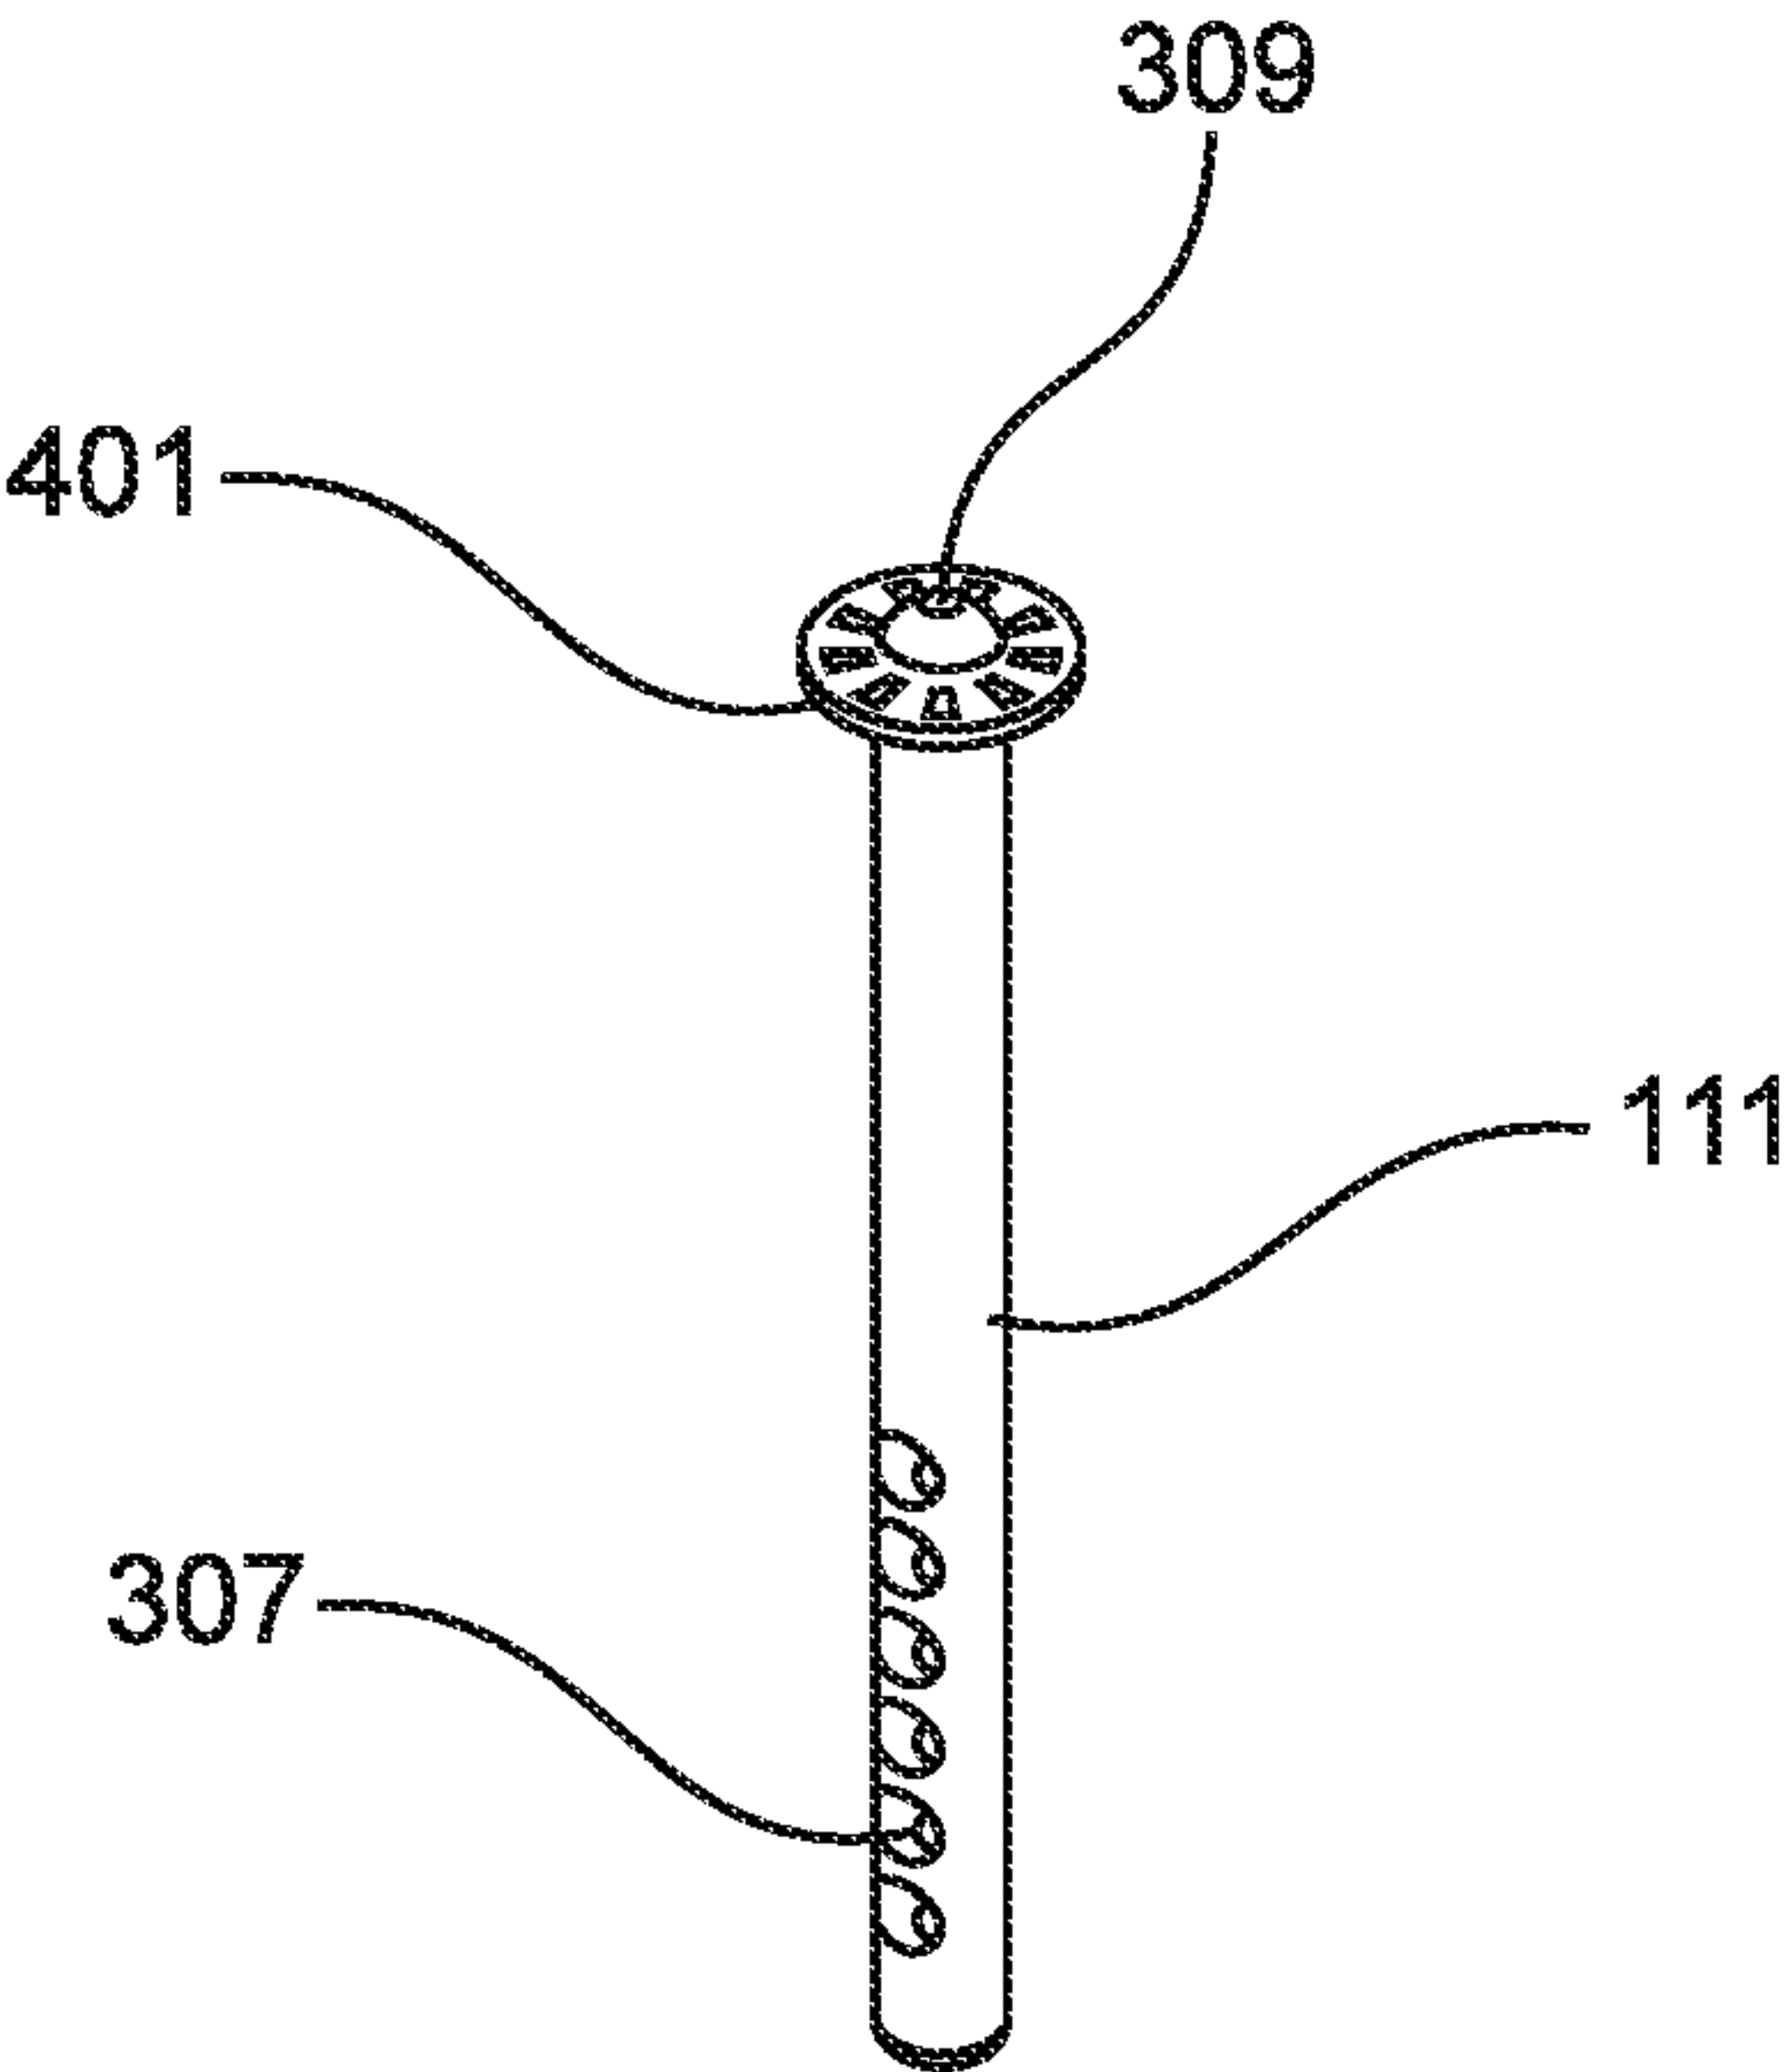


FIG. 4A

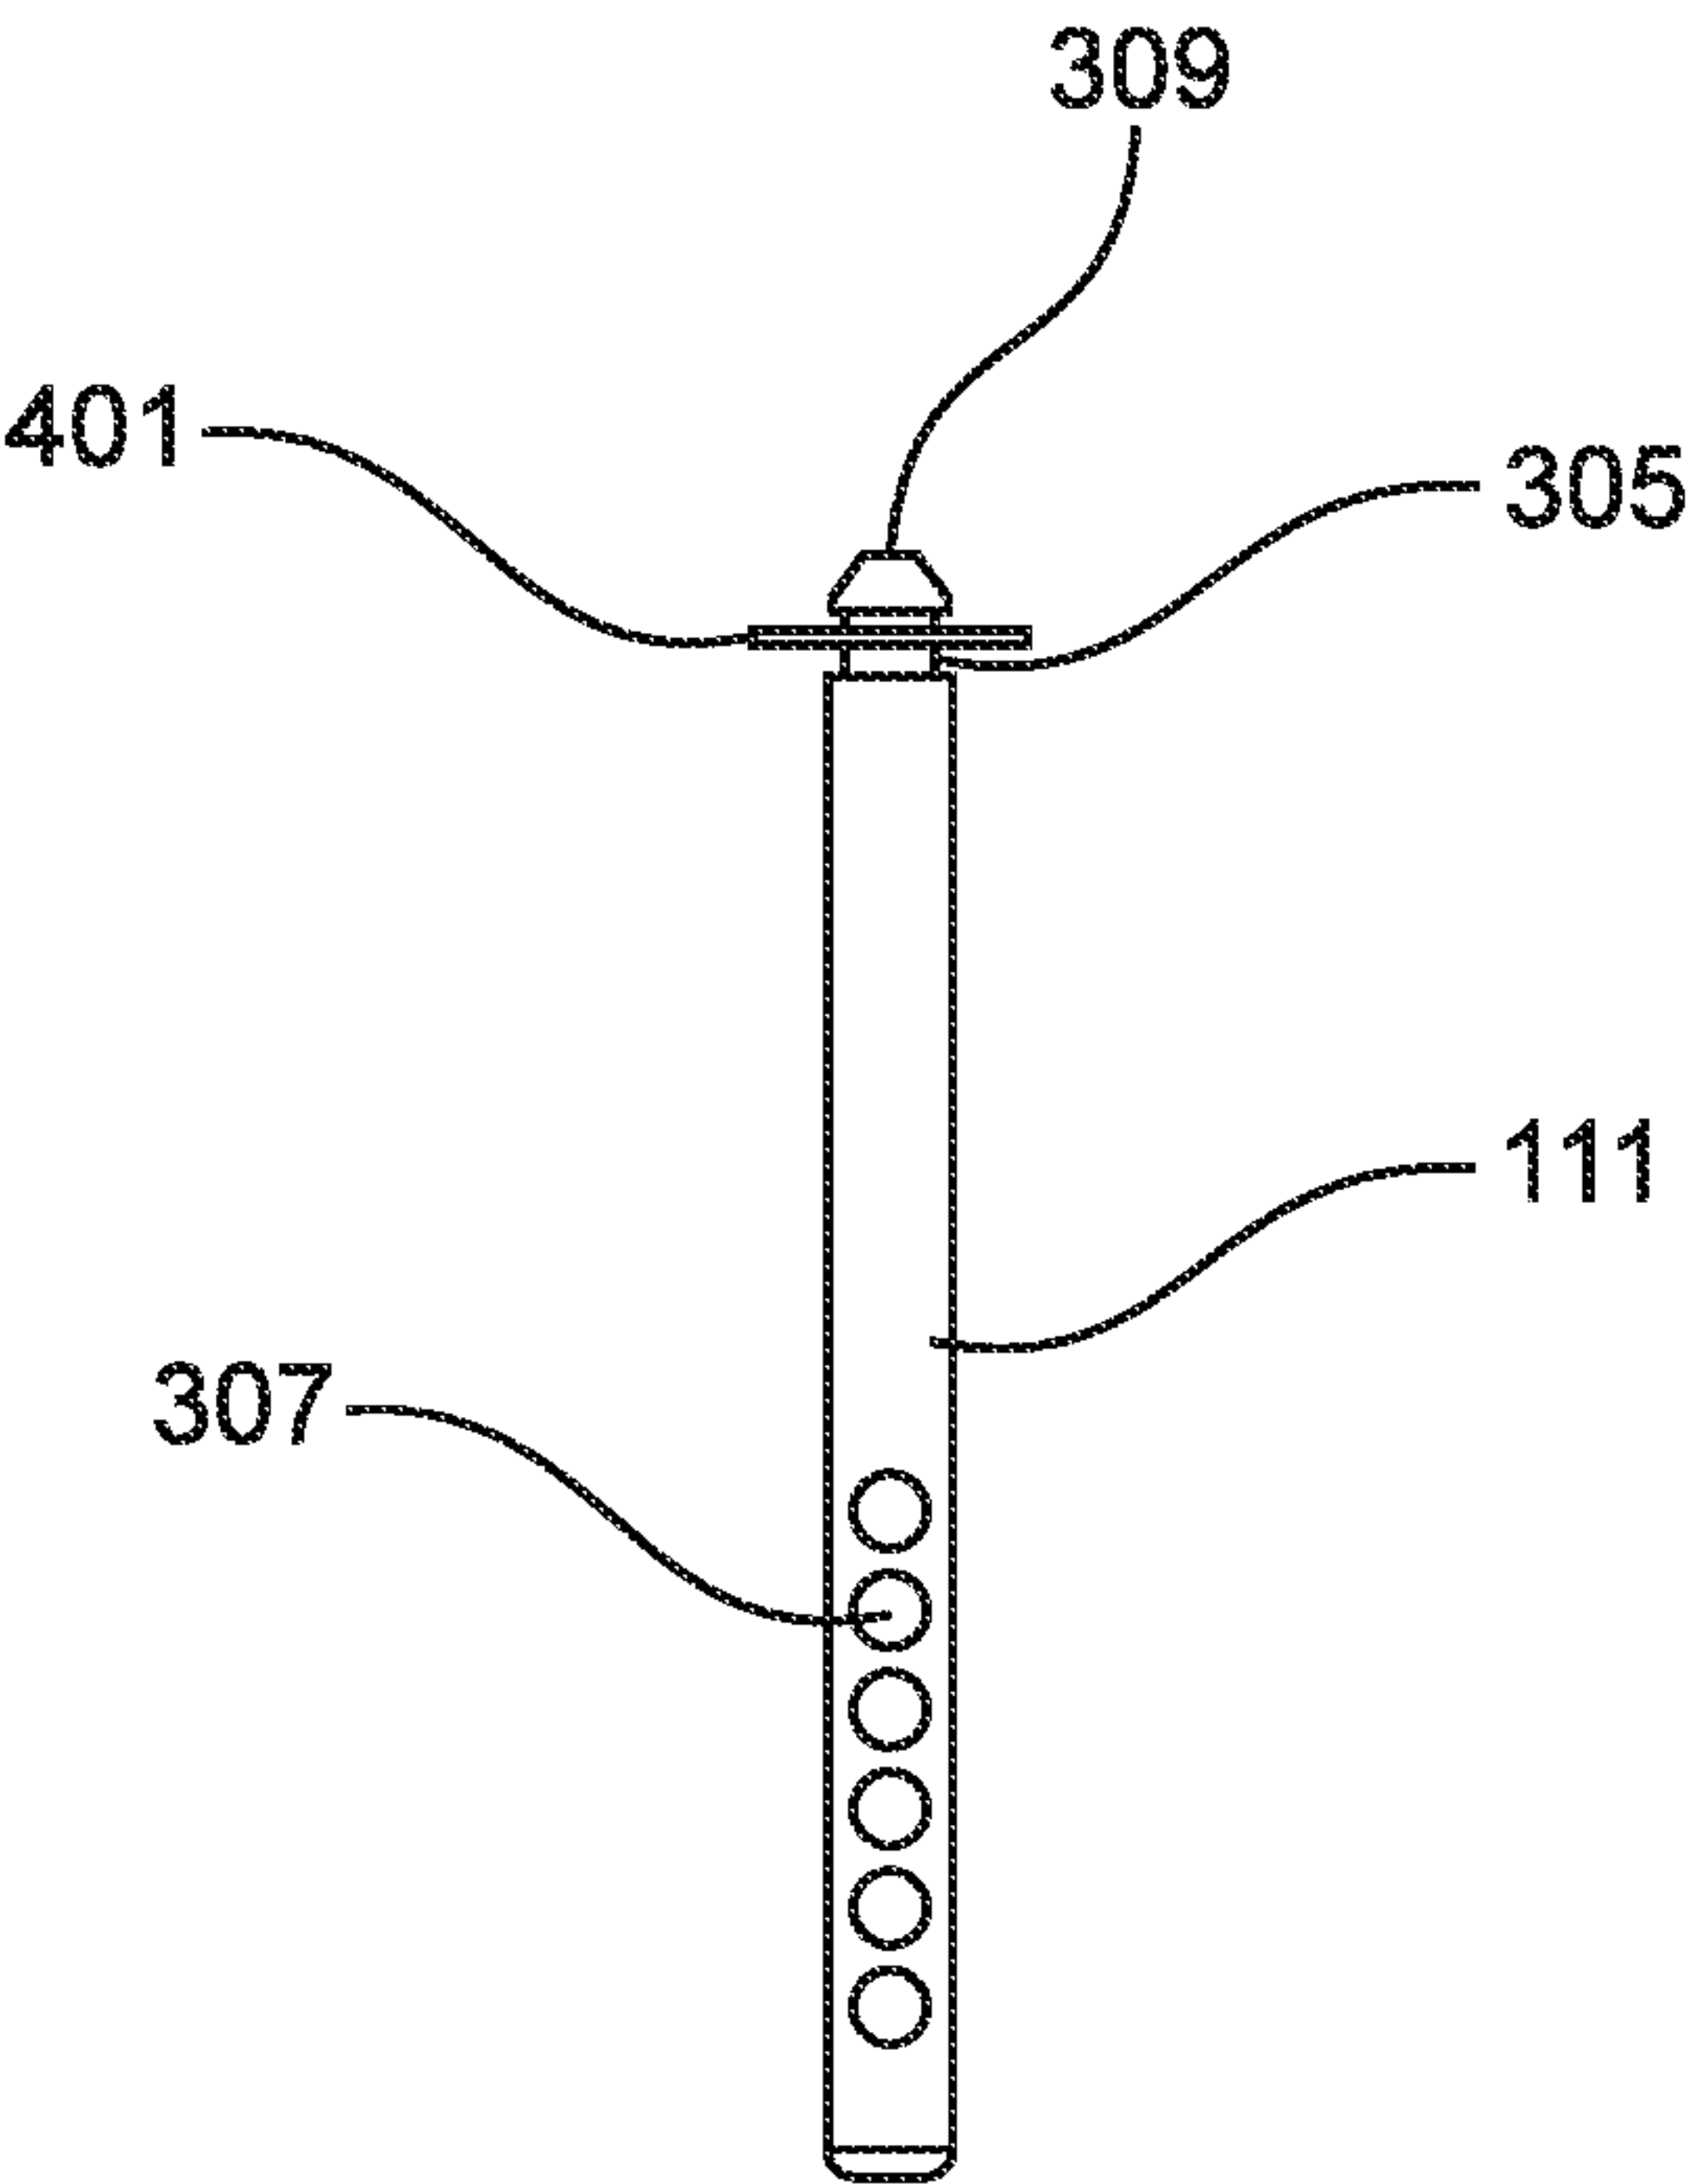


FIG. 4B

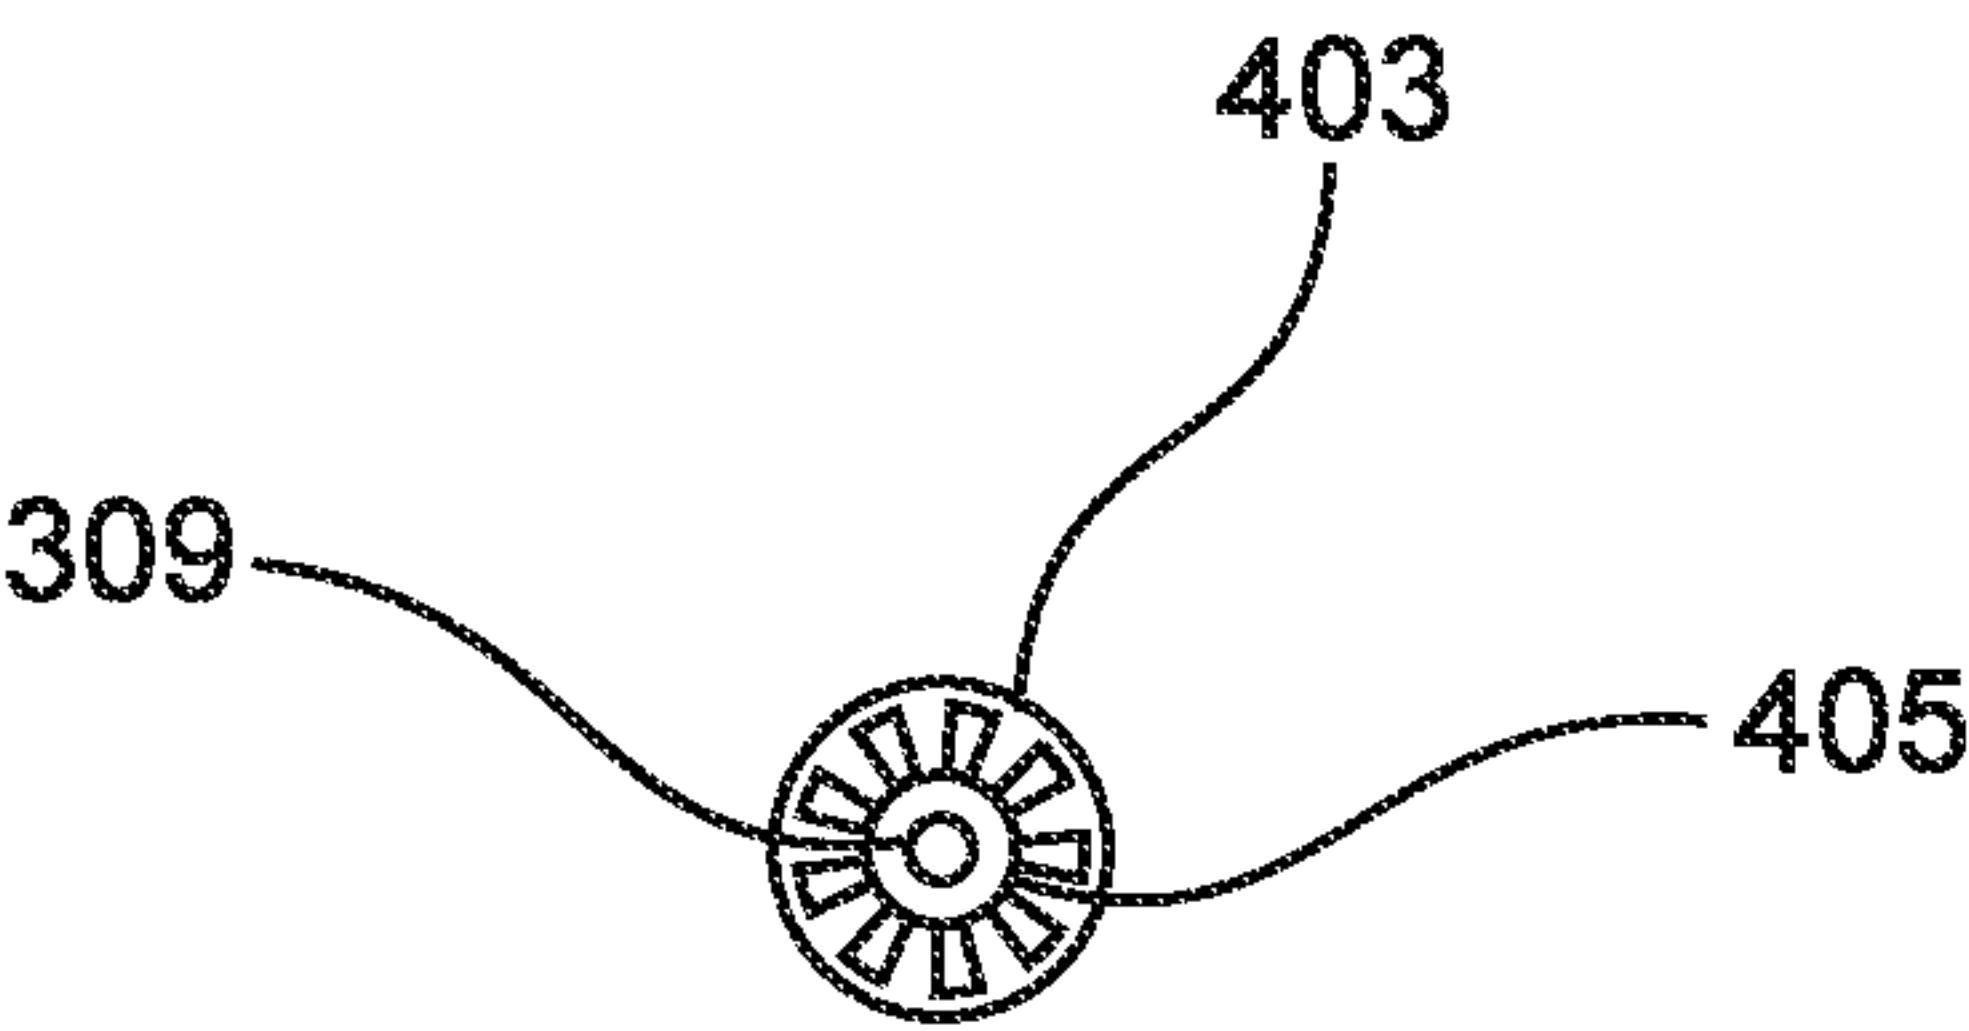


FIG. 4C

9/11

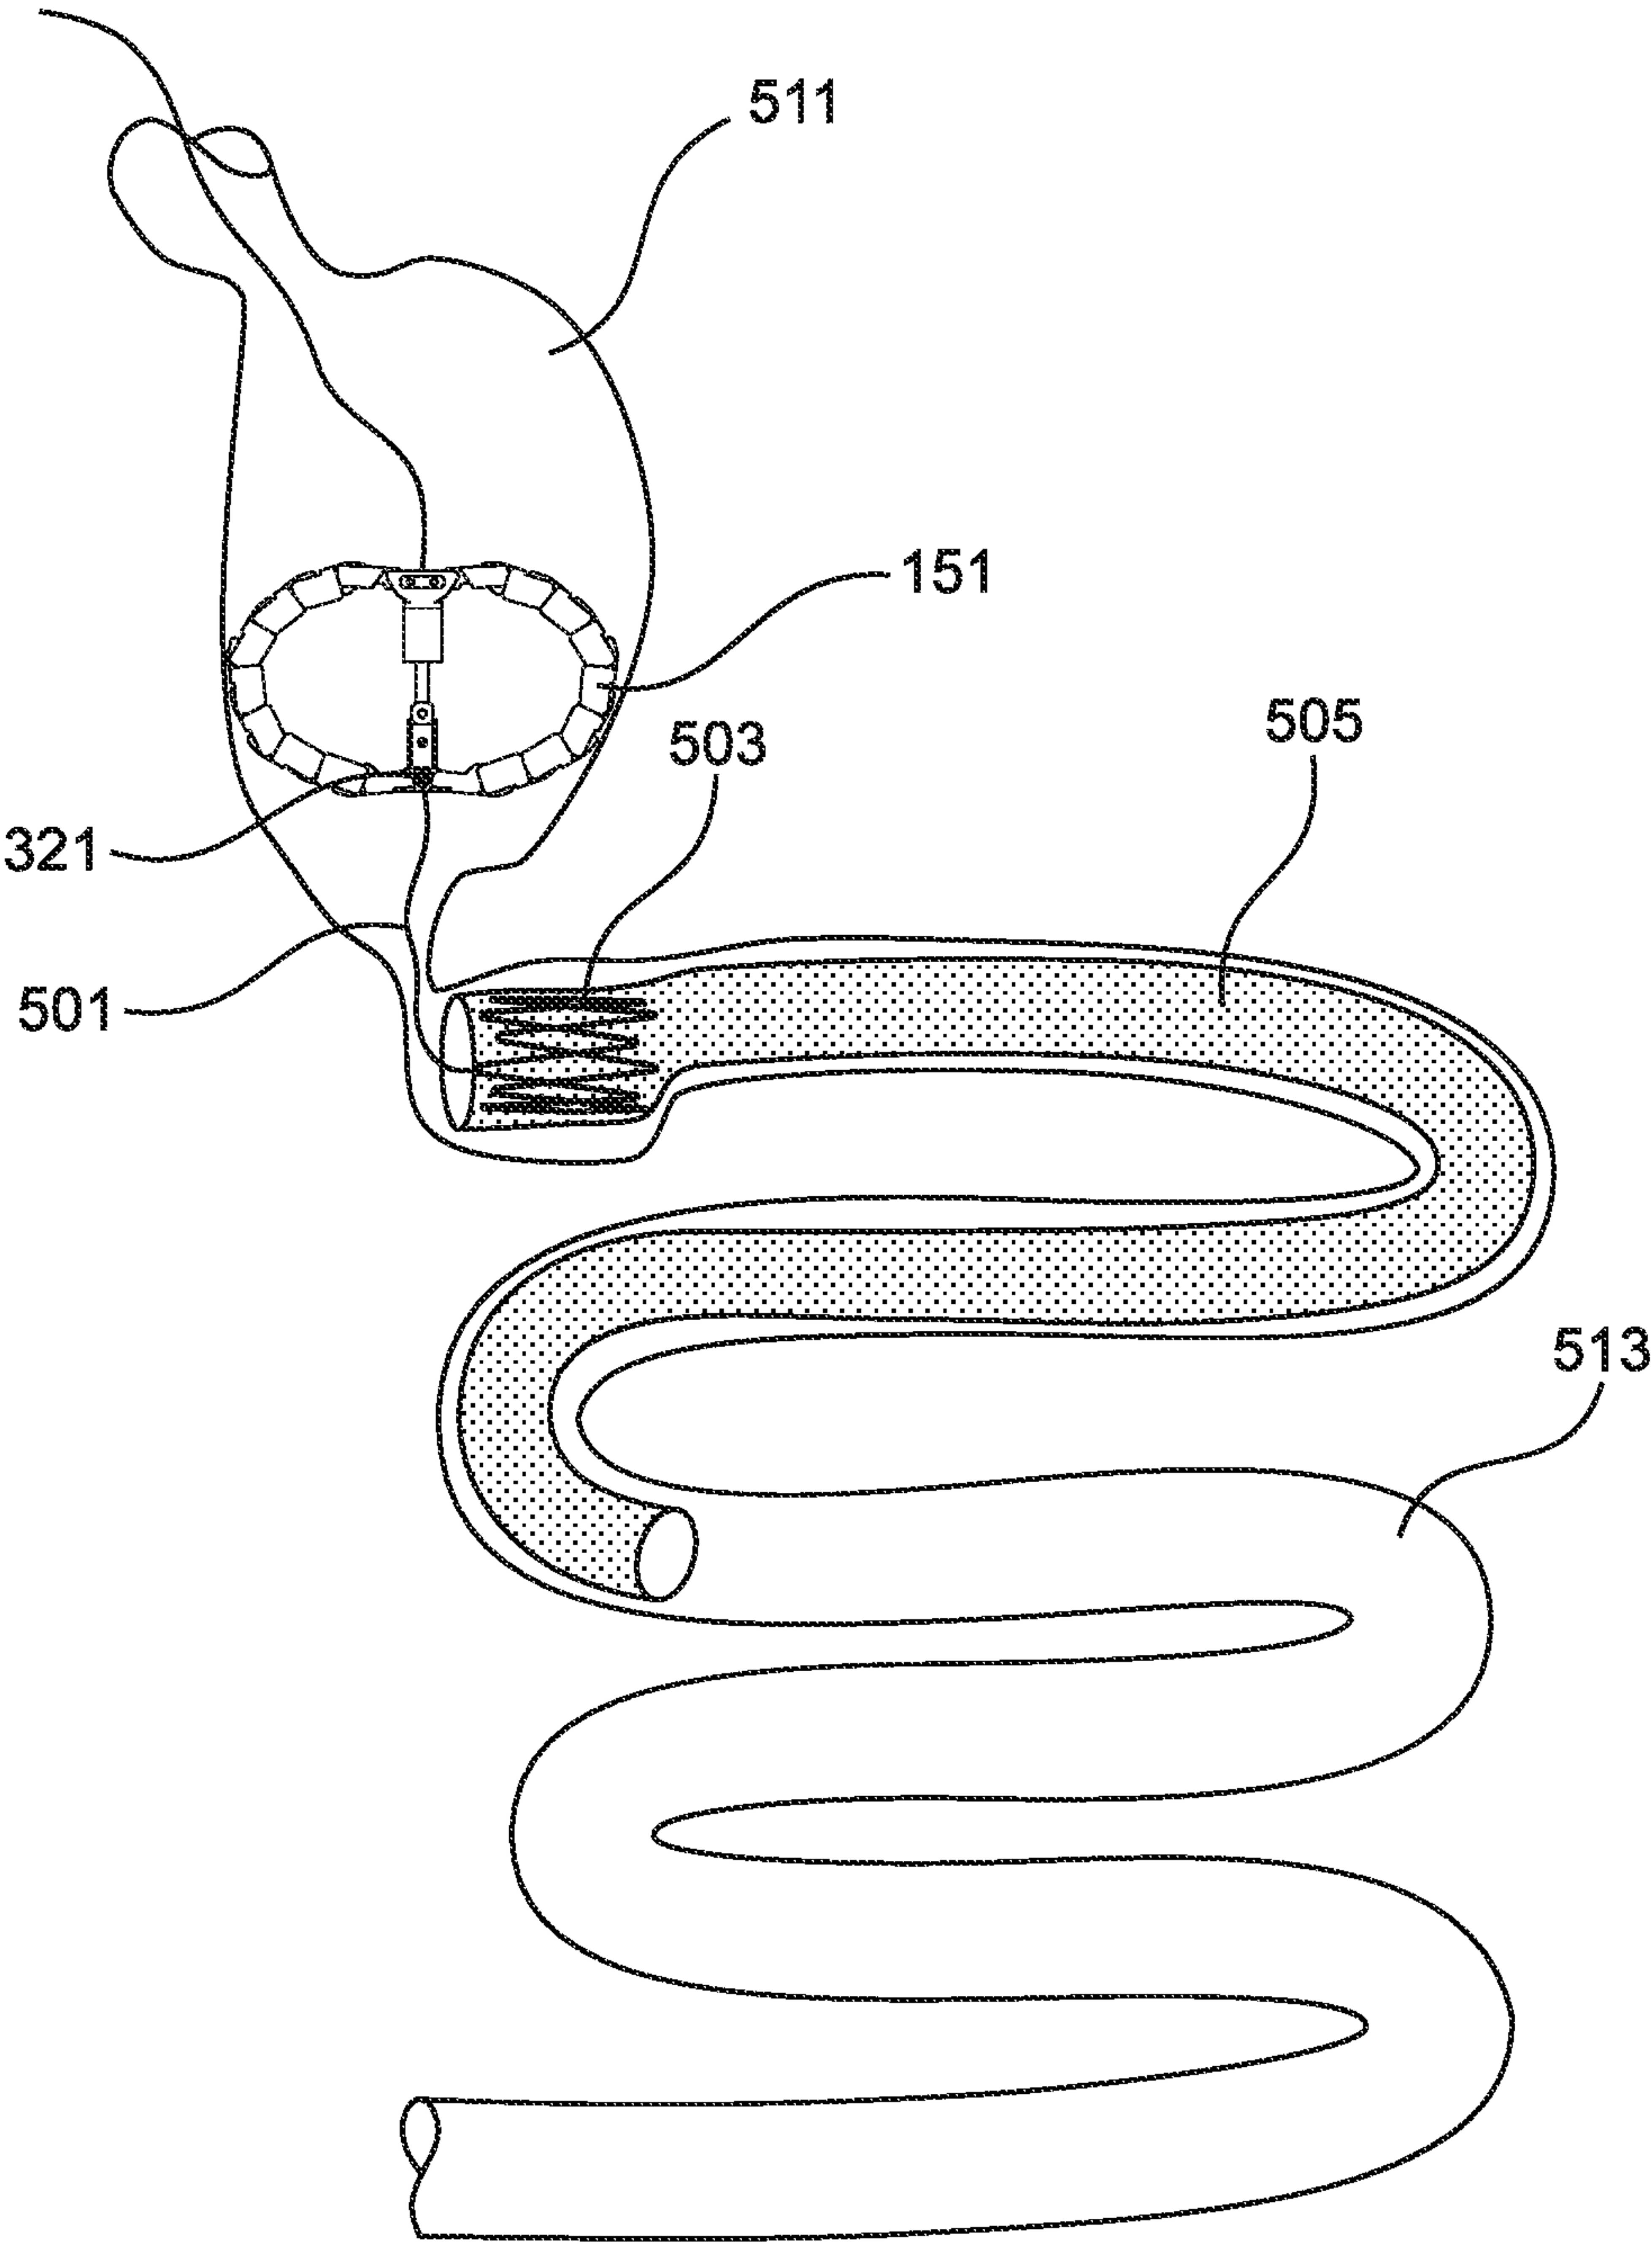


FIG. 5A

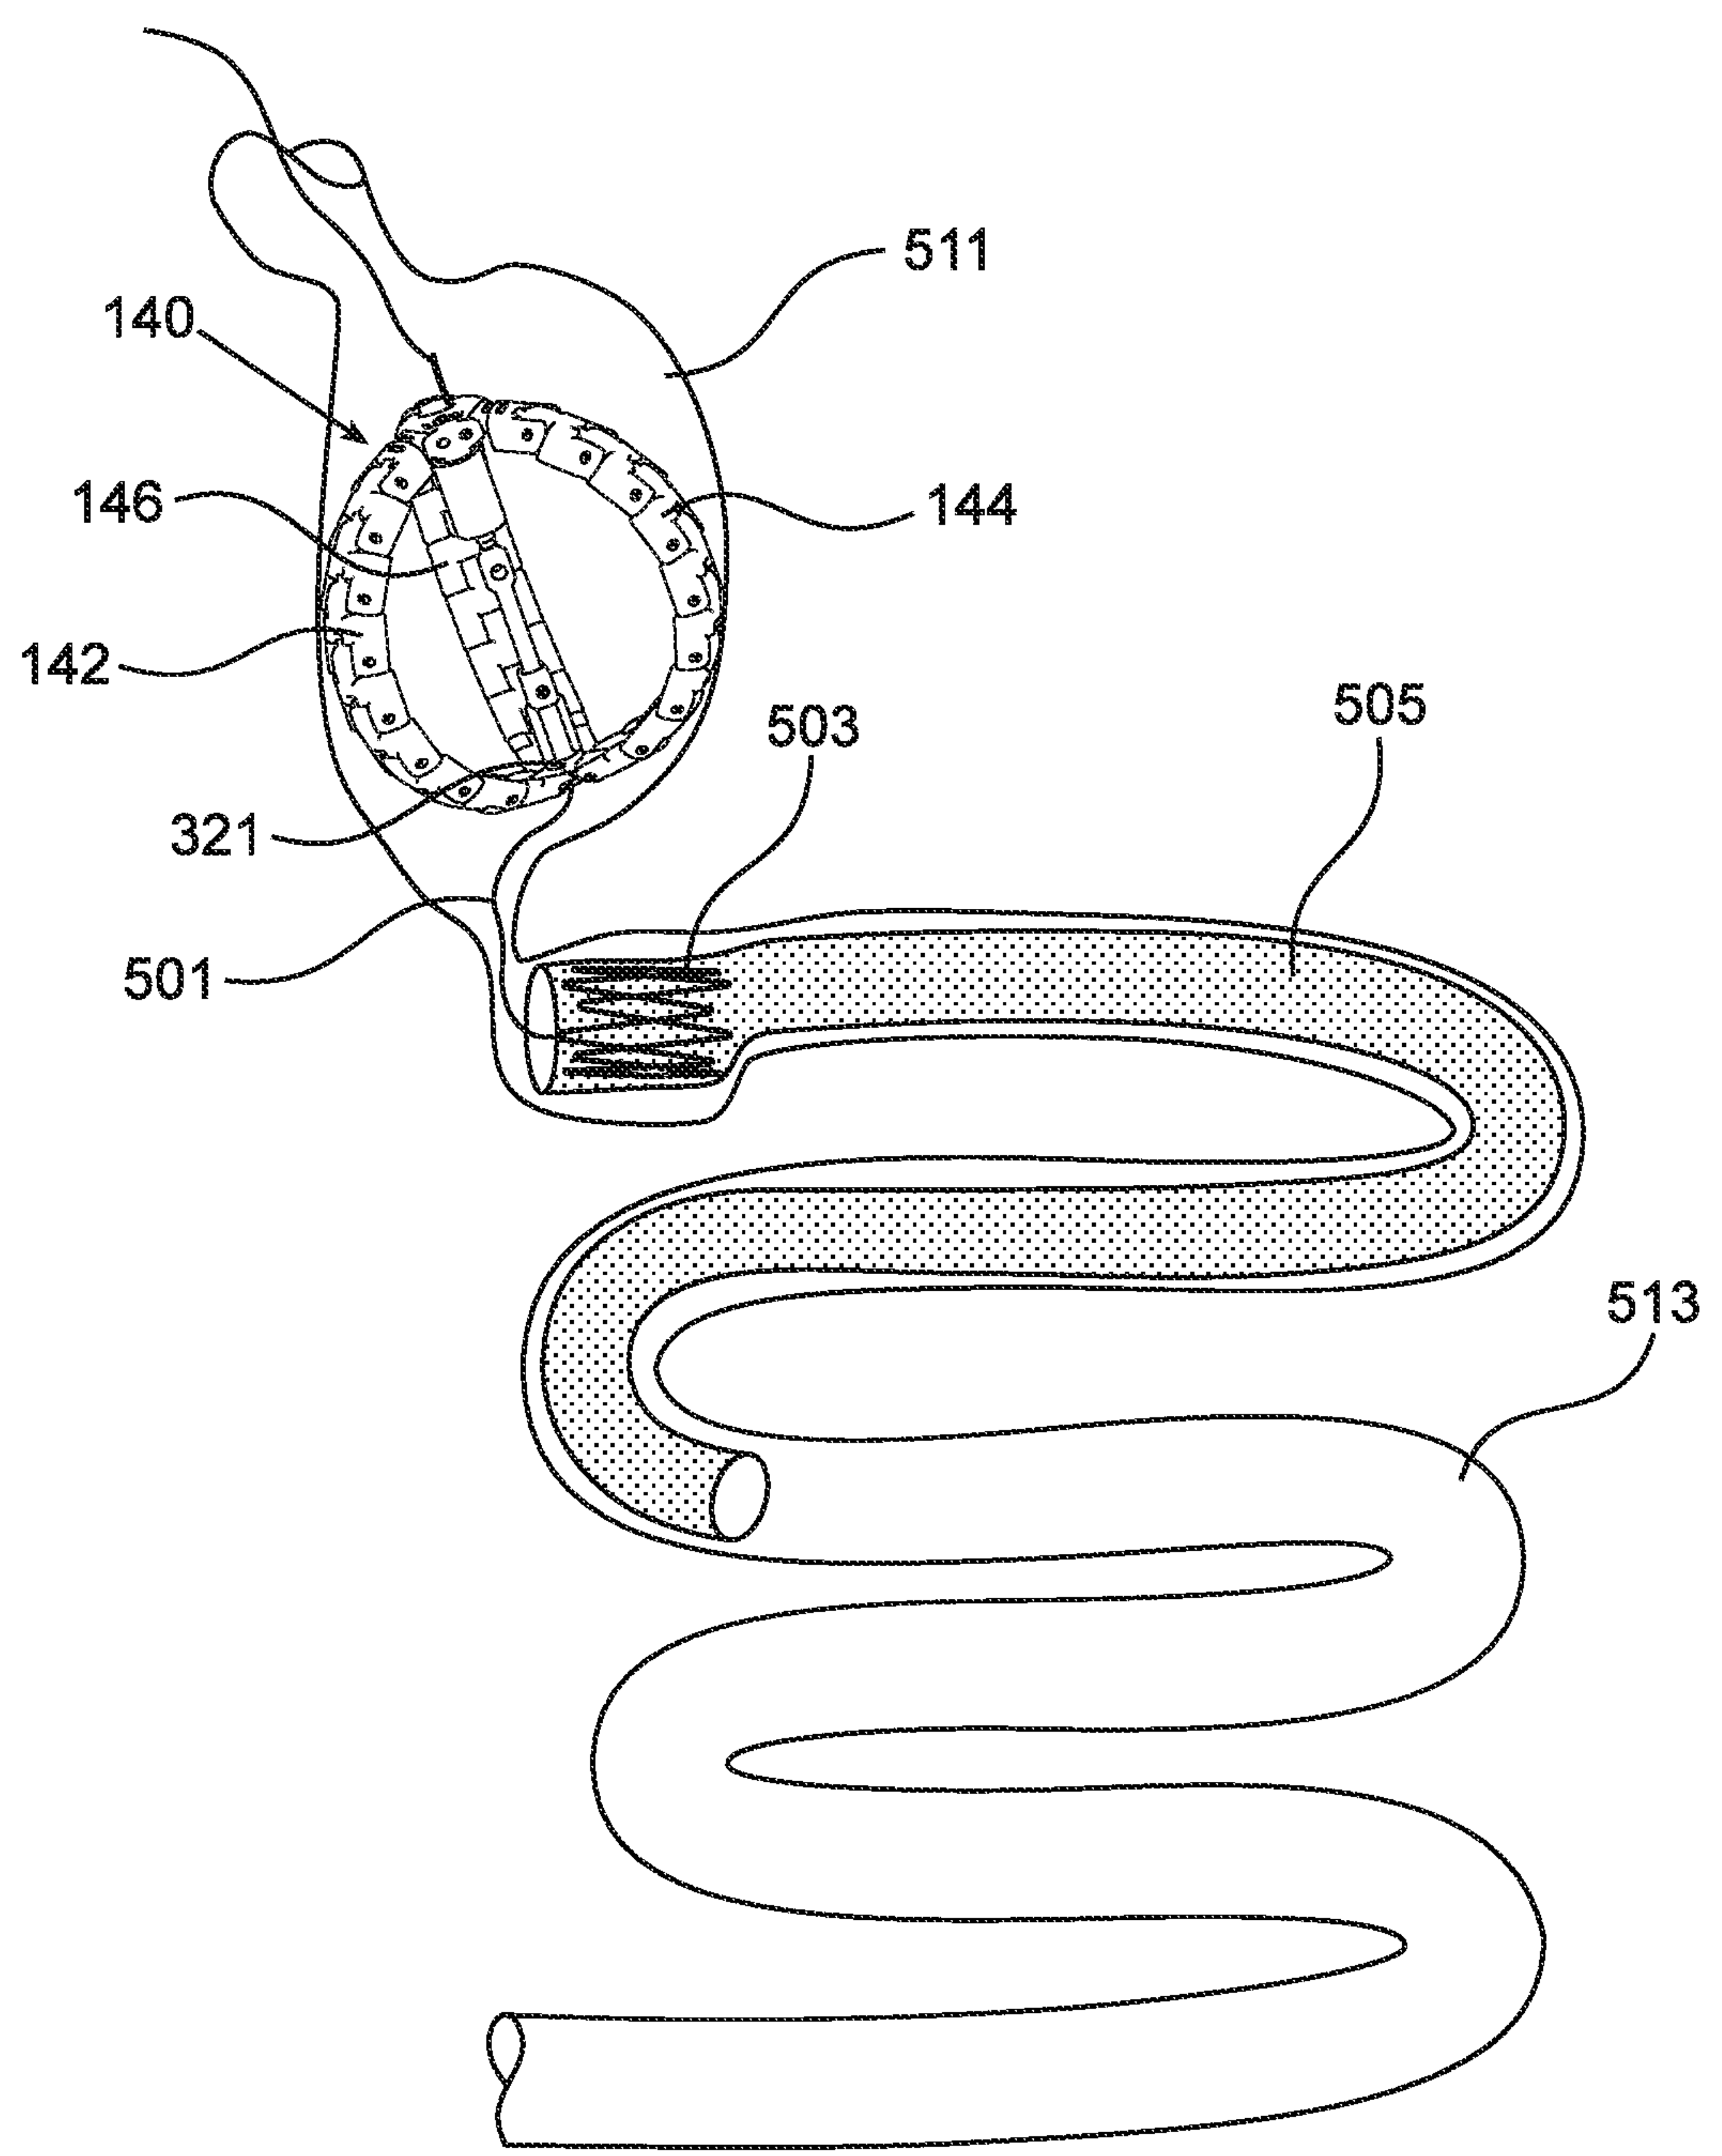


FIG. 5B

11/11

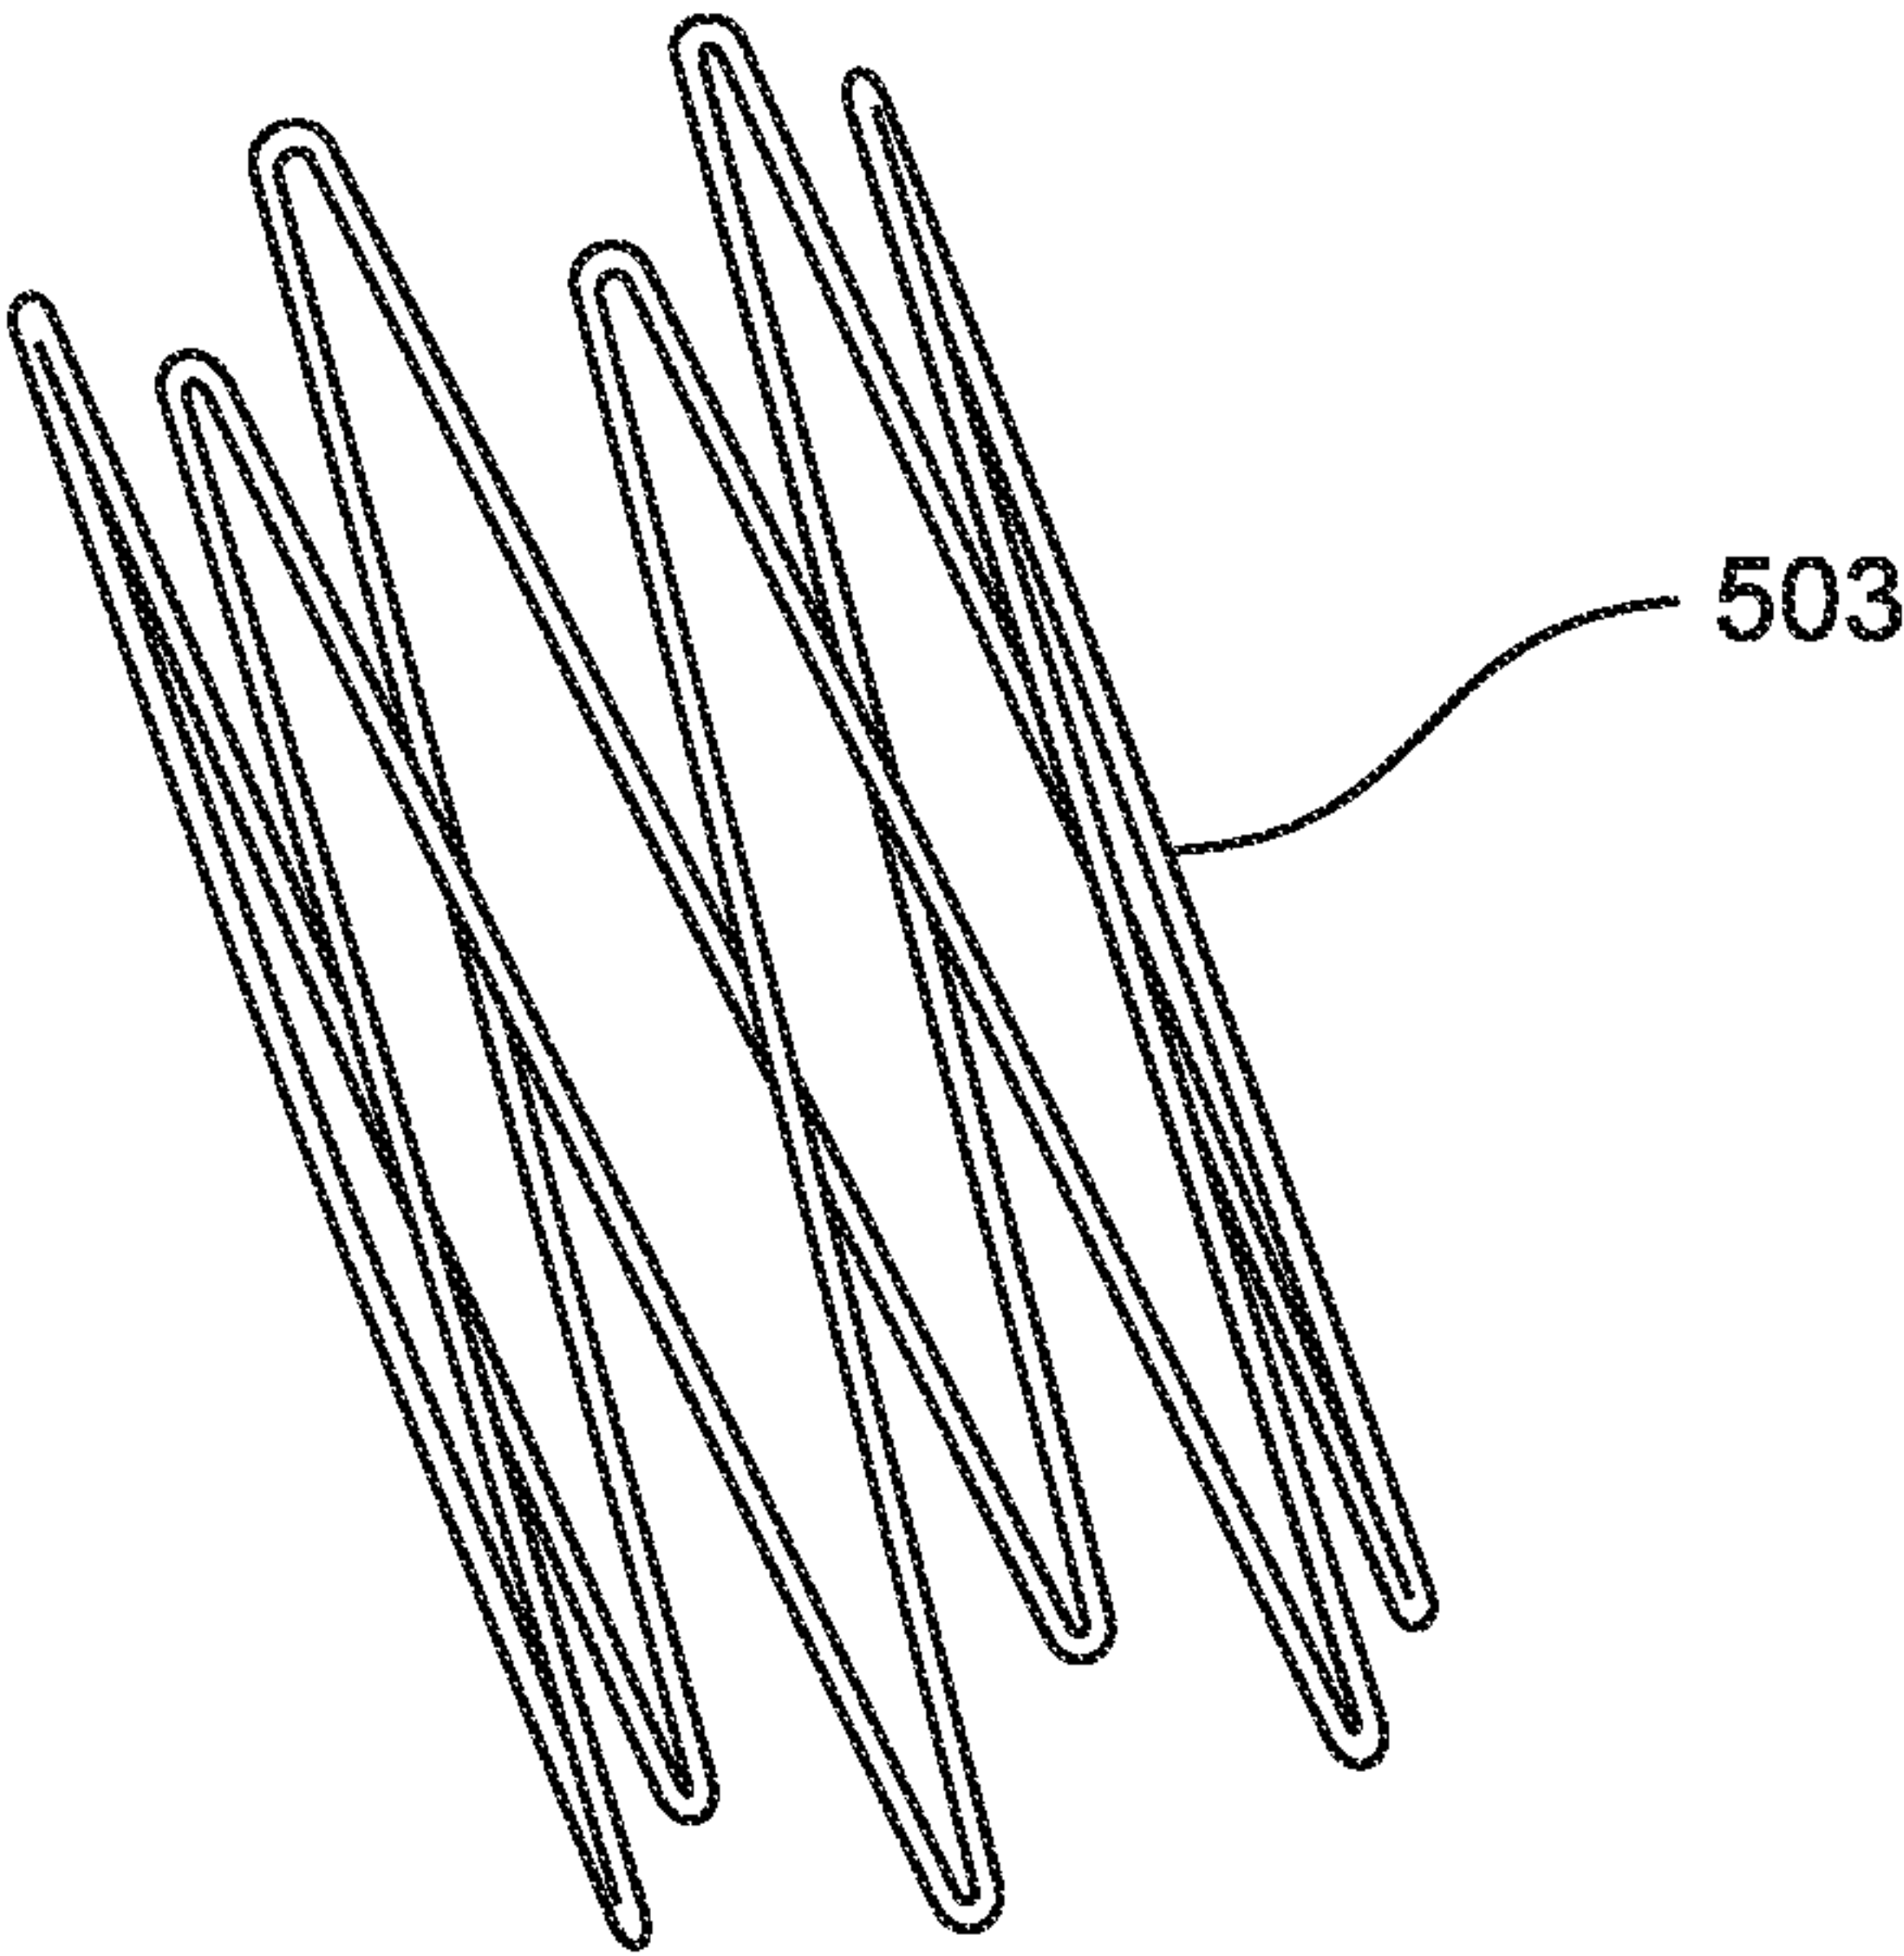


FIG. 6A

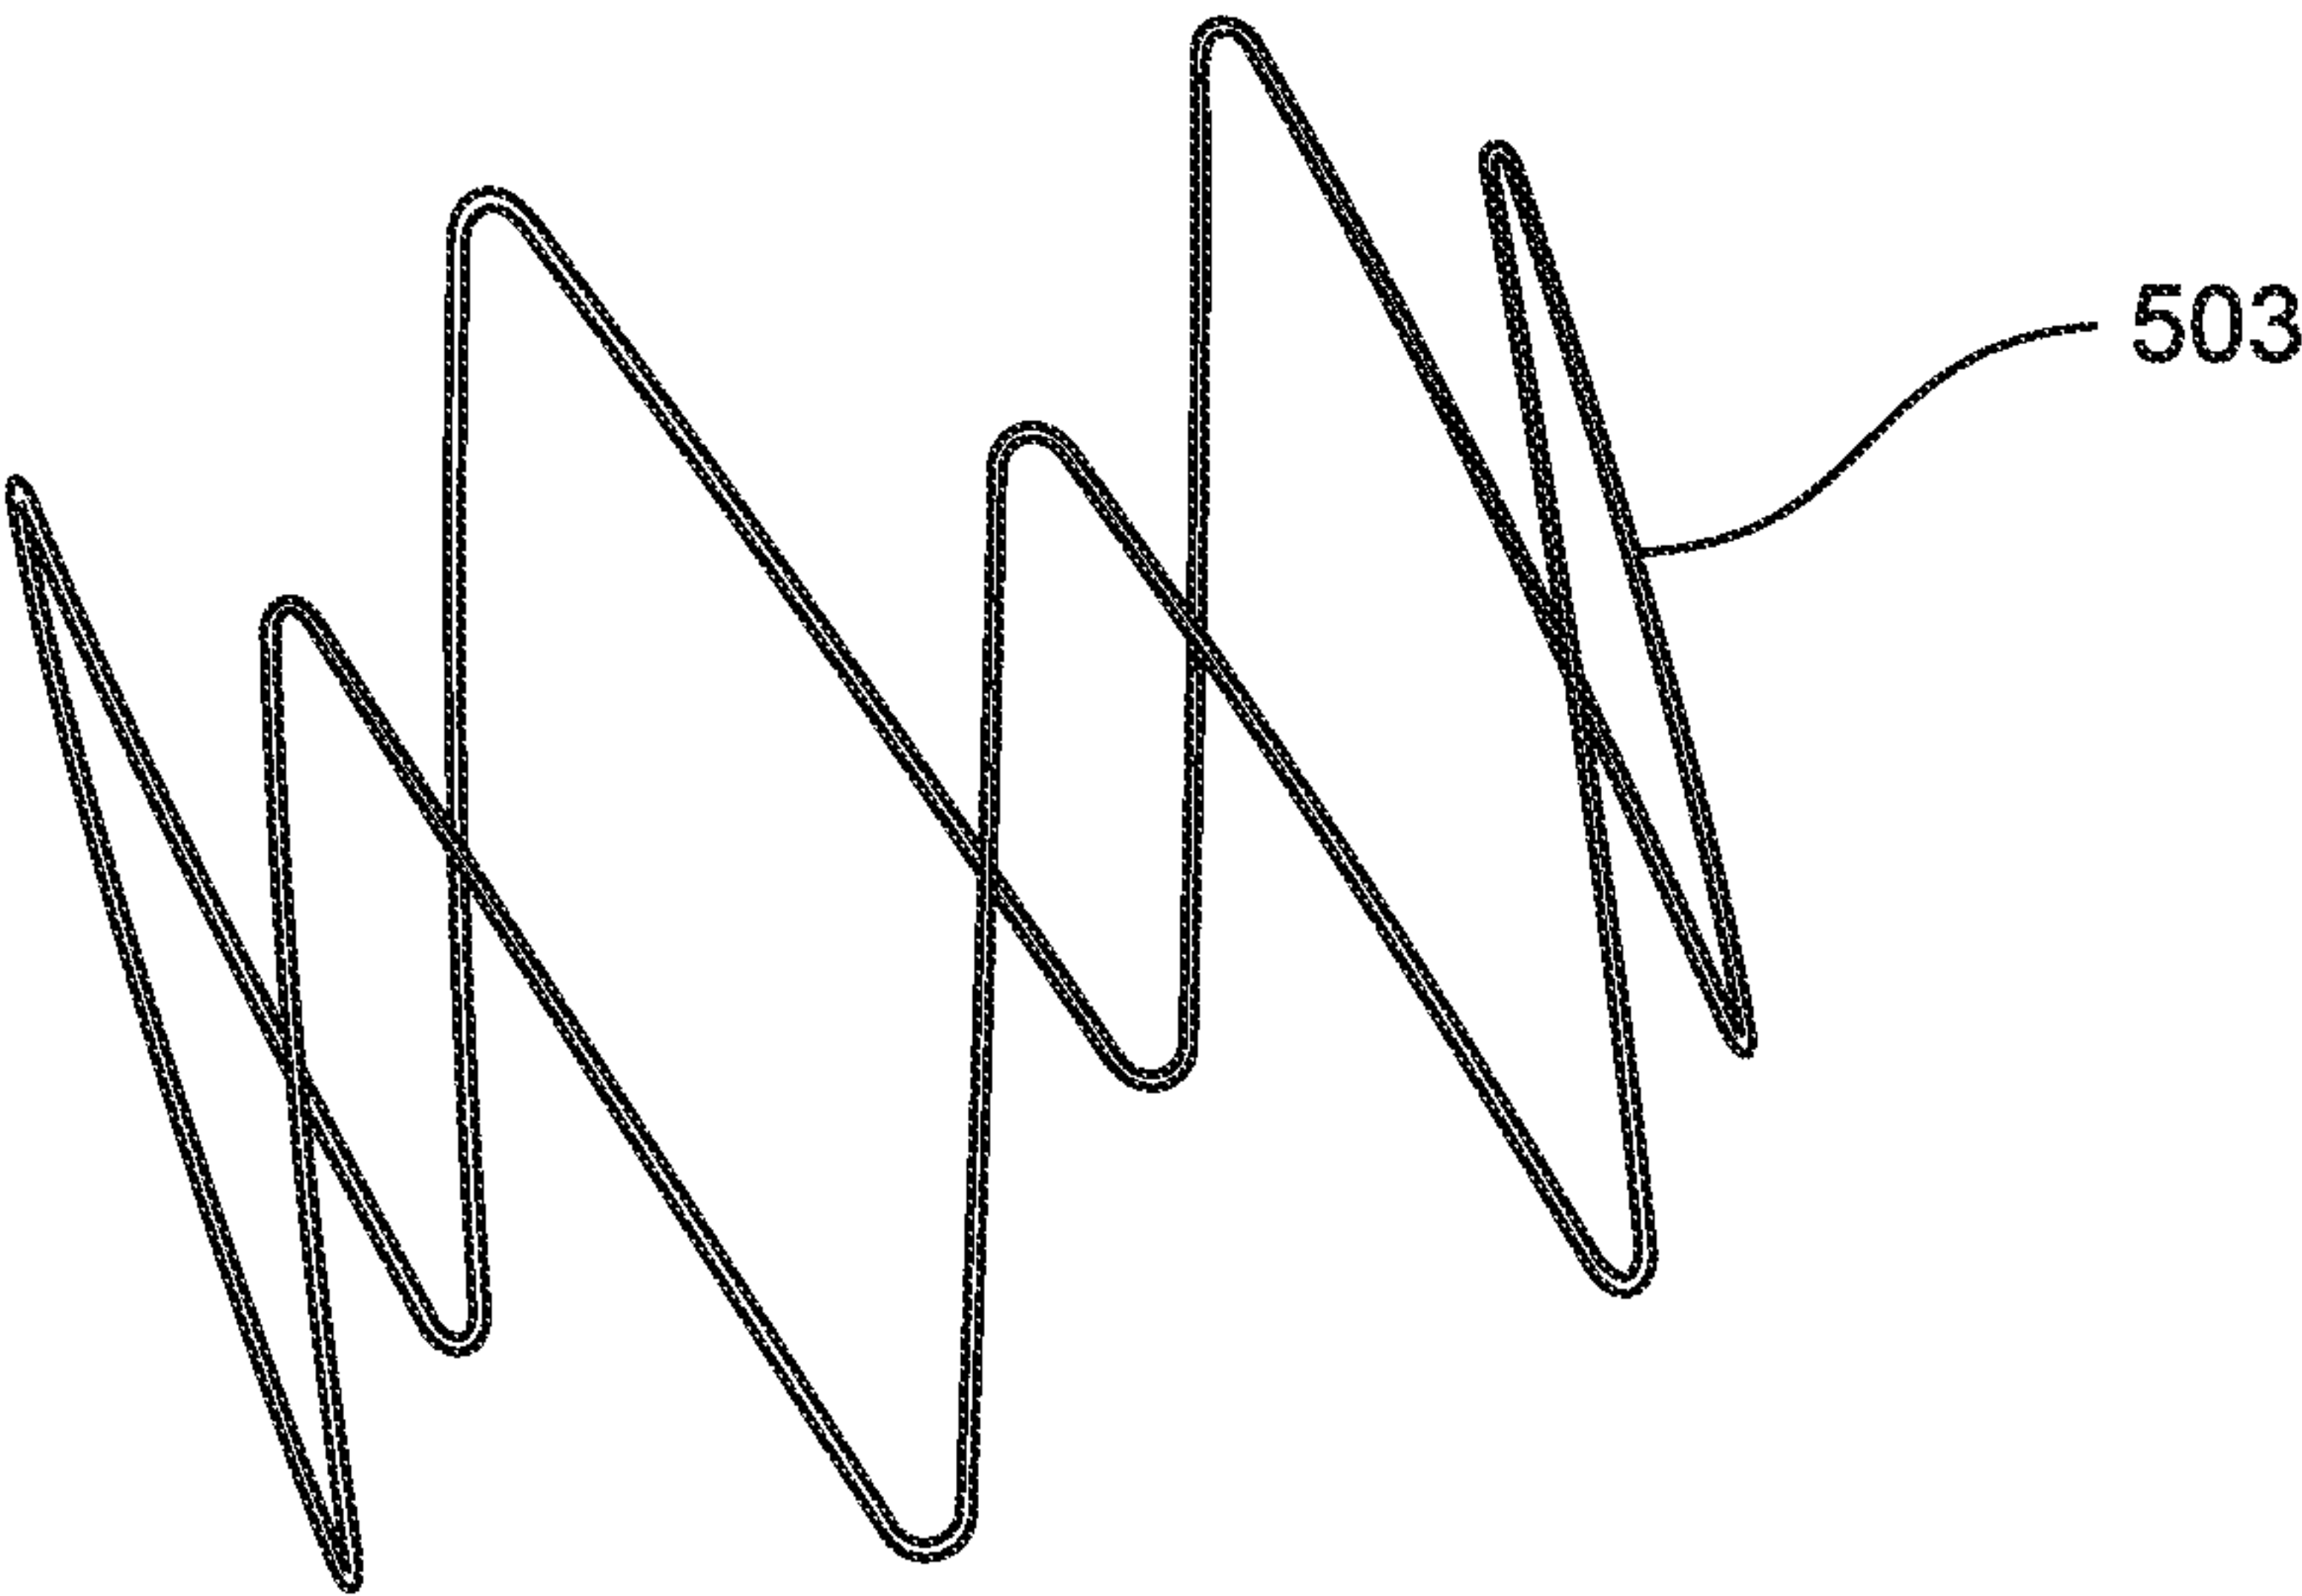


FIG. 6B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/IL2020/051162

A. CLASSIFICATION OF SUBJECT MATTER IPC (20210101) A61F 5/00 CPC (20130101) A61F 5/0036, A61F 5/0076, A61F 5/0013 According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) IPC (20210101) A61F 5/00 CPC (20130101) A61F 5/0036, A61F 5/0076, A61F 5/0013 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) Databases consulted: Esp@cenet, Google Patents, SIMILARI Search terms used: intragastric, anchoring, arcs, implant, sphere, pin, links, rigid, flexible, struts		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2019201181 A1 ALLIUM MEDICAL SOLUTIONS LTD. [IL] 04 Jul 2019 (2019/07/04) The whole document	1-18
Y	US 2017281383 A1 BINMOELLER KENNETH F. et al. 05 Oct 2017 (2017/10/05) The whole document	1-18
A	US 2014350693 A1 BOSTON SCIENT SCIMED INC. [US] 27 Nov 2014 (2014/11/27) The whole document	1-18
A	US 2012095385 A1 ALLERGAN INC. [US] 19 Apr 2012 (2012/04/19) The whole document	1-18
☐ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents: "A" document defining the general state of the art which is not considered to be of particular relevance "D" document cited by the applicant in the international application "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family		
Date of the actual completion of the international search 14 Jan 2021		Date of mailing of the international search report 17 Jan 2021
Name and mailing address of the ISA: Israel Patent Office Technology Park, Bldg.5, Malcha, Jerusalem, 9695101, Israel Email address: pctoffice@justice.gov.il		Authorized officer Kimchi Barry Telephone No. 972-73-3927235

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report			Publication date	Patent family member(s)			Publication Date
US	2019201181	A1	04 Jul 2019	US	2019201181	A1	04 Jul 2019
				US	10368976	B2	06 Aug 2019
				CN	111601573	A	28 Aug 2020
				EP	3735207	A1	11 Nov 2020
				US	2019201182	A1	04 Jul 2019
				US	10631971	B2	28 Apr 2020
				US	2020100888	A1	02 Apr 2020
				US	2020170775	A1	04 Jun 2020
				WO	2019135212	A1	11 Jul 2019
US	2017281383	A1	05 Oct 2017	US	2017281383	A1	05 Oct 2017
				BR	PI0518726	A2	02 Dec 2008
				BR	PI0712468	A2	31 Jul 2012
				BR	PI0915286	A2	16 Feb 2016
				CA	2588901	A1	08 Jun 2006
				CA	2588901	C	25 Nov 2014
				CA	2631934	A1	05 Jul 2007
				CA	2652419	A1	06 Dec 2007
				CA	2652419	C	05 Sep 2017
				CA	2693259	A1	22 Jan 2009
				CA	2693259	C	17 Apr 2018
				EP	1817072	A2	15 Aug 2007
				EP	1817072	A4	02 Dec 2009
				EP	1817072	B1	27 Mar 2013
				EP	1968685	A2	17 Sep 2008
				EP	1968685	A4	02 Jul 2014
				EP	1968685	B1	29 Aug 2018
				EP	2026713	A2	25 Feb 2009
				EP	2026713	A4	26 Jul 2017
				EP	2178474	A1	28 Apr 2010

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
	EP 2178474	B1	20 May 2015
	EP 2313034	A2	27 Apr 2011
	EP 2313034	A4	12 Dec 2012
	EP 2313034	B1	23 Sep 2015
	ES 2416295	T3	31 Jul 2013
	ES 2552821	T3	02 Dec 2015
	HK 1157252	A1	29 Jun 2012
	JP 2008521550	A	26 Jun 2008
	JP 2009524447	A	02 Jul 2009
	JP 2009538218	A	05 Nov 2009
	JP 2013048905	A	14 Mar 2013
	MX 2007006419	A	11 Mar 2008
	MX 2008014939	A	10 Dec 2008
	MX 2010014323	A	03 Mar 2011
	PL 1817072	T3	29 Nov 2013
	PT 1817072	E	04 Jul 2013
	US 2005192614	A1	01 Sep 2005
	US 7931693	B2	26 Apr 2011
	US 2006178691	A1	10 Aug 2006
	US 8147561	B2	03 Apr 2012
	US 2007293885	A1	20 Dec 2007
	US 8585771	B2	19 Nov 2013
	US 2012172999	A1	05 Jul 2012
	US 8603186	B2	10 Dec 2013
	US 2011190684	A1	04 Aug 2011
	US 8623095	B2	07 Jan 2014
	US 2009187206	A1	23 Jul 2009
	US 9060835	B2	23 Jun 2015
	US 2013178782	A1	11 Jul 2013
	US 9072861	B2	07 Jul 2015
	US 2013165842	A1	27 Jun 2013

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		US 9352126 B2	31 May 2016
		US 2017181877 A1	29 Jun 2017
		US 10369035 B2	06 Aug 2019
		US 2011137227 A1	09 Jun 2011
		US 2014100513 A1	10 Apr 2014
		US 2014114228 A1	24 Apr 2014
		US 2015305906 A1	29 Oct 2015
		US 2017156908 A1	08 Jun 2017
		US 2017181878 A1	29 Jun 2017
		WO 2006060049 A2	08 Jun 2006
		WO 2006060049 A3	23 Apr 2009
		WO 2007075396 A2	05 Jul 2007
		WO 2007075396 A3	26 Feb 2009
		WO 2007139920 A2	06 Dec 2007
		WO 2007139920 A3	14 Aug 2008
		WO 2008148047 A2	04 Dec 2008
		WO 2008148047 A3	28 Jan 2010
		WO 2009012335 A1	22 Jan 2009
		WO 2010003097 A2	07 Jan 2010
		WO 2010003097 A3	07 Apr 2011
US 2014350693 A1	27 Nov 2014	US 2014350693 A1	27 Nov 2014
		US 9180036 B2	10 Nov 2015
		AT 464866 T	15 May 2010
		AT 466545 T	15 May 2010
		AU 2003213058 A1	27 Oct 2003
		AU 2003217401 A1	27 Oct 2003
		AU 2003286613 A1	13 Aug 2004
		CN 1575155 A	02 Feb 2005
		CN 1307951 C	04 Apr 2007
		CN 1713870 A	28 Dec 2005

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		CN 1713870 B	08 Dec 2010
		CN 1713871 A	28 Dec 2005
		CN 1713871 B	24 Nov 2010
		CN 101810521 A	25 Aug 2010
		CN 101810521 B	13 May 2015
		CN 101810524 A	25 Aug 2010
		CN 101810524 B	01 Mar 2017
		DE 60332492 D1	17 Jun 2010
		DE 602004026695 D1	02 Jun 2010
		EP 1420730 A2	26 May 2004
		EP 1420730 B1	13 Apr 2016
		EP 1492477 A1	05 Jan 2005
		EP 1492477 B1	13 Apr 2016
		EP 1492478 A1	05 Jan 2005
		EP 1492478 B1	07 Sep 2016
		EP 1585460 A1	19 Oct 2005
		EP 1585460 B1	05 May 2010
		EP 1603488 A2	14 Dec 2005
		EP 1603488 B1	21 Apr 2010
		EP 2191795 A1	02 Jun 2010
		EP 2210570 A1	28 Jul 2010
		EP 2210570 B1	16 Jul 2014
		EP 2397113 A1	21 Dec 2011
		EP 2397113 B1	23 Sep 2015
		EP 2397113 B8	04 Nov 2015
		EP 3042630 A1	13 Jul 2016
		EP 3085334 A1	26 Oct 2016
		EP 3130320 A1	15 Feb 2017
		EP 3130320 B1	13 Jun 2018
		ES 2343793 T3	10 Aug 2010
		ES 2343800 T3	10 Aug 2010

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
	ES	2483791 T3	07 Aug 2014
	ES	2575354 T3	28 Jun 2016
	JP	2005522269 A	28 Jul 2005
	JP	4426852 B2	03 Mar 2010
	JP	2005522268 A	28 Jul 2005
	JP	4511194 B2	28 Jul 2010
	JP	2006512986 A	20 Apr 2006
	JP	4550591 B2	22 Sep 2010
	JP	2006520670 A	14 Sep 2006
	JP	4704331 B2	15 Jun 2011
	JP	2005500127 A	06 Jan 2005
	JP	4790212 B2	12 Oct 2011
	JP	2011200661 A	13 Oct 2011
	JP	5407048 B2	05 Feb 2014
	US	2003040804 A1	27 Feb 2003
	US	6675809 B2	13 Jan 2004
	US	2003040808 A1	27 Feb 2003
	US	6845776 B2	25 Jan 2005
	US	2004153167 A1	05 Aug 2004
	US	7097665 B2	29 Aug 2006
	US	2003199989 A1	23 Oct 2003
	US	7111627 B2	26 Sep 2006
	US	2004172142 A1	02 Sep 2004
	US	7121283 B2	17 Oct 2006
	US	2004158331 A1	12 Aug 2004
	US	7146984 B2	12 Dec 2006
	US	2004172141 A1	02 Sep 2004
	US	7152607 B2	26 Dec 2006
	US	2005004681 A1	06 Jan 2005
	US	7354454 B2	08 Apr 2008
	US	2005267499 A1	01 Dec 2005

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		US 7628821 B2	08 Dec 2009
		US 2008269797 A1	30 Oct 2008
		US 7833280 B2	16 Nov 2010
		US 2006287734 A1	21 Dec 2006
		US 7892292 B2	22 Feb 2011
		US 2004138761 A1	15 Jul 2004
		US 7981162 B2	19 Jul 2011
		US 2012016287 A1	19 Jan 2012
		US 8177853 B2	15 May 2012
		US 2010100109 A1	22 Apr 2010
		US 8337566 B2	25 Dec 2012
		US 2012022430 A1	26 Jan 2012
		US 8337567 B2	25 Dec 2012
		US 2010016988 A1	21 Jan 2010
		US 8568488 B2	29 Oct 2013
		US 2011153030 A1	23 Jun 2011
		US 8784354 B2	22 Jul 2014
		US 2014094734 A1	03 Apr 2014
		US 8845753 B2	30 Sep 2014
		US 2011270410 A1	03 Nov 2011
		US 8992457 B2	31 Mar 2015
		US 2014142720 A1	22 May 2014
		US 9107727 B2	18 Aug 2015
		US 2014364792 A1	11 Dec 2014
		US 9138340 B2	22 Sep 2015
		US 2013310727 A1	21 Nov 2013
		US 9254214 B2	09 Feb 2016
		US 2015202039 A1	23 Jul 2015
		US 9358144 B2	07 Jun 2016
		US 2015320580 A1	12 Nov 2015
		US 9788984 B2	17 Oct 2017

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		US 2016022464 A1	28 Jan 2016
		US 9844453 B2	19 Dec 2017
		US 2015342772 A1	03 Dec 2015
		US 9872786 B2	23 Jan 2018
		US 2016113799 A1	28 Apr 2016
		US 10080677 B2	25 Sep 2018
		US 2003199990 A1	23 Oct 2003
		US 2003199991 A1	23 Oct 2003
		US 2004117031 A1	17 Jun 2004
		US 2008208356 A1	28 Aug 2008
		US 2009299487 A1	03 Dec 2009
		US 2010298631 A1	25 Nov 2010
		US 2012271217 A1	25 Oct 2012
		US 2013296764 A1	07 Nov 2013
		US 2018104079 A1	19 Apr 2018
		WO 03017882 A2	06 Mar 2003
		WO 03017882 A3	20 Nov 2003
		WO 03086246 A1	23 Oct 2003
		WO 03086247 A1	23 Oct 2003
		WO 03086247 A9	10 Jun 2004
		WO 2004064685 A1	05 Aug 2004
		WO 2004080336 A2	23 Sep 2004
		WO 2004080336 A3	16 Dec 2004
US 2012095385 A1	19 Apr 2012	US 2012095385 A1	19 Apr 2012
		CA 2814502 A1	19 Apr 2012
		CA 2814502 C	24 Jul 2018
		EP 2627291 A2	21 Aug 2013
		EP 2629708 A2	28 Aug 2013
		EP 2629708 B1	20 Jul 2016
		EP 2629709 A2	28 Aug 2013

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
	EP 2629709	B1	07 Dec 2016
	EP 2629710	A1	28 Aug 2013
	EP 2629710	B1	14 Sep 2016
	EP 2629711	A2	28 Aug 2013
	EP 2629711	B1	30 Dec 2015
	EP 2629712	A2	28 Aug 2013
	EP 2629712	B1	20 Jul 2016
	EP 2629713	A2	28 Aug 2013
	EP 2629713	B1	27 Dec 2017
	EP 2629714	A2	28 Aug 2013
	EP 2629714	B1	30 Dec 2015
	EP 2629715	A2	28 Aug 2013
	EP 2629715	B1	06 Jan 2016
	EP 2629716	A2	28 Aug 2013
	EP 2629716	B1	13 Jul 2016
	EP 2629717	A2	28 Aug 2013
	EP 2629717	B1	14 Sep 2016
	EP 3023081	A1	25 May 2016
	EP 3111898	A1	04 Jan 2017
	EP 3305254	A1	11 Apr 2018
	ES 2562035	T3	02 Mar 2016
	ES 2565348	T3	04 Apr 2016
	ES 2566498	T3	13 Apr 2016
	ES 2593753	T3	13 Dec 2016
	ES 2594484	T3	20 Dec 2016
	ES 2596729	T3	11 Jan 2017
	ES 2605368	T3	14 Mar 2017
	ES 2605488	T3	14 Mar 2017
	ES 2618256	T3	21 Jun 2017
	ES 2662346	T3	06 Apr 2018
	US 2012095494	A1	19 Apr 2012

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		US 8864840 B2	21 Oct 2014
		US 2013035711 A1	07 Feb 2013
		US 8870966 B2	28 Oct 2014
		US 2012095484 A1	19 Apr 2012
		US 8920447 B2	30 Dec 2014
		US 2012095496 A1	19 Apr 2012
		US 8956380 B2	17 Feb 2015
		US 2012095495 A1	19 Apr 2012
		US 9095405 B2	04 Aug 2015
		US 2012095499 A1	19 Apr 2012
		US 9198790 B2	01 Dec 2015
		US 2012323160 A1	20 Dec 2012
		US 9398969 B2	26 Jul 2016
		US 2012095492 A1	19 Apr 2012
		US 9463107 B2	11 Oct 2016
		US 2012191125 A1	26 Jul 2012
		US 9498365 B2	22 Nov 2016
		US 2013289466 A1	31 Oct 2013
		US 9539133 B2	10 Jan 2017
		US 2013296765 A1	07 Nov 2013
		US 9668901 B2	06 Jun 2017
		US 2015094753 A1	02 Apr 2015
		US 9681974 B2	20 Jun 2017
		US 2015272761 A1	01 Oct 2015
		US 2016331568 A9	17 Nov 2016
		US 9795498 B2	24 Oct 2017
		US 2015142044 A1	21 May 2015
		US 9801747 B2	31 Oct 2017
		US 2015150700 A1	04 Jun 2015
		US 9895246 B2	20 Feb 2018
		US 2015209169 A1	30 Jul 2015

INTERNATIONAL SEARCH REPORT
Information on patent family members

International application No.
PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		US 9895247 B2	20 Feb 2018
		US 2016030219 A1	04 Feb 2016
		US 9956105 B2	01 May 2018
		US 2013281911 A1	24 Oct 2013
		US 10070980 B2	11 Sep 2018
		US 2012089170 A1	12 Apr 2012
		US 2012089172 A1	12 Apr 2012
		US 2012095384 A1	19 Apr 2012
		US 2012095483 A1	19 Apr 2012
		US 2012095497 A1	19 Apr 2012
		US 2014025100 A1	23 Jan 2014
		US 2017065444 A1	09 Mar 2017
		US 2017143523 A1	25 May 2017
		US 2017258617 A1	14 Sep 2017
		US 2019008669 A1	10 Jan 2019
		WO 2012051108 A2	19 Apr 2012
		WO 2012051108 A3	05 Jul 2012
		WO 2012051108 A4	23 Aug 2012
		WO 2012054293 A1	26 Apr 2012
		WO 2012054296 A2	26 Apr 2012
		WO 2012054296 A3	12 Jul 2012
		WO 2012054297 A2	26 Apr 2012
		WO 2012054297 A3	02 Aug 2012
		WO 2012054297 A4	20 Sep 2012
		WO 2012054410 A2	26 Apr 2012
		WO 2012054410 A3	02 Aug 2012
		WO 2012054411 A2	26 Apr 2012
		WO 2012054411 A3	28 Jun 2012
		WO 2012054413 A2	26 Apr 2012
		WO 2012054413 A3	21 Jun 2012
		WO 2012054413 A4	09 Aug 2012

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/IL2020/051162

Patent document cited search report	Publication date	Patent family member(s)	Publication Date
		WO 2012054414 A2	26 Apr 2012
		WO 2012054414 A3	28 Jun 2012
		WO 2012054514 A2	26 Apr 2012
		WO 2012054514 A3	12 Jul 2012
		WO 2012054519 A2	26 Apr 2012
		WO 2012054519 A3	02 Aug 2012
		WO 2012054522 A2	26 Apr 2012
		WO 2012054522 A3	05 Jul 2012
		WO 2012054598 A2	26 Apr 2012
		WO 2012054598 A3	07 Sep 2012
		WO 2014055766 A1	10 Apr 2014