

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2014/028062 A1

(43) International Publication Date

20 February 2014 (20.02.2014)

(51) International Patent Classification:

A61F 2/915 (2013.01) A61F 2/82 (2013.01)

(21) International Application Number:

PCT/US2013/033141

(22) International Filing Date:

20 March 2013 (20.03.2013)

94103 (US). **ANUKHIN, Boris**; 1268 El. Rancho Drive, Santa Cruz, California 95060 (US). **TROLLSAS, Mikael**; 5989 Hosta Lane, San Jose, California 95124 (US). **SCHWARTZ, Lewis B.**; 340 Oakdale, Lake Forest, Illinois 60045 (US).

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

13/584,678 13 August 2012 (13.08.2012) US

(74) Agents: **LUPKOWSKI, Mark** et al.; Squire Sanders (US) LLP, 275 Battery Street, Suite 2600, San Francisco, California 94111 (US).

(71) Applicant: **ABBOTT CARDIOVASCULAR SYSTEMS INC.** [US/US]; 3200 Lakeside Drive, Santa Clara, California 95054 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(72) Inventors: **PAPP, John E.**; 33998 Linda Rosea Road, Temecula, California 92592 (US). **HOSSAINY, Syed Faiyaz Ahmed**; 29885 Bellow View, Hayward, California 94544 (US). **NGO, Michael H.**; 704 Villa Centre Way, San Jose, California 95128 (US). **ABUNASSAR, Chad**; 255 Dolores Street, Apt. #2, San Francisco, California

[Continued on next page]

(54) Title: SEGMENTED SCAFFOLD DESIGNS

(57) Abstract: Segmented scaffolds composed of disconnected scaffold segments with overlapping end rings are disclosed. Scaffolds with at least one discontinuous link are also disclosed.

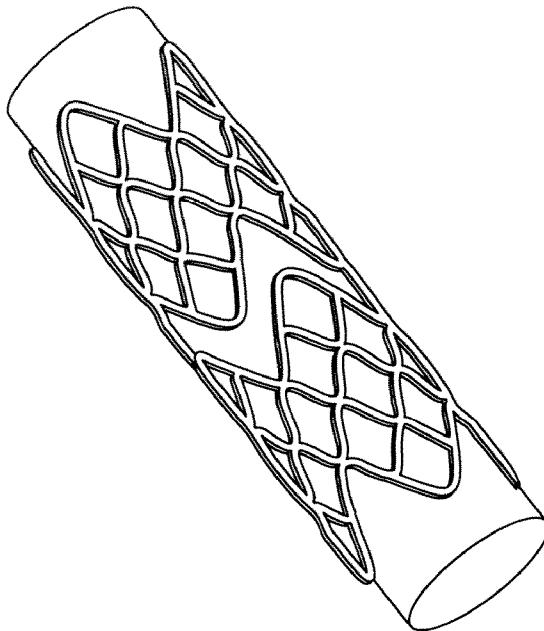


FIG. 11



**(84) Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

**Published:**

- with international search report (Art. 21(3))
- with amended claims (Art. 19(1))

## SEGMENTED SCAFFOLD DESIGNS

### BACKGROUND OF THE INVENTION

#### Field of the Invention

5 This invention relates to methods of treatment of blood vessels with polymeric medical devices, in particular, stent scaffolds.

#### Description of the State of the Art

This invention relates to radially expandable endoprostheses, that are adapted to be implanted in a bodily lumen. An “endoprosthesis” corresponds to an artificial 10 device that is placed inside the body. A “lumen” refers to a cavity of a tubular organ such as a blood vessel. A stent is an example of such an endoprosthesis. Stents are generally cylindrically shaped devices that function to hold open and sometimes expand a segment of a blood vessel or other anatomical lumen such as urinary tracts and bile ducts. Stents are often used in the treatment of atherosclerotic stenosis in 15 blood vessels. “Stenosis” refers to a narrowing or constriction of a bodily passage or orifice. In such treatments, stents reinforce body vessels and prevent restenosis following angioplasty in the vascular system. “Restenosis” refers to the reoccurrence of stenosis in a blood vessel or heart valve after it has been treated (as by balloon angioplasty, stenting, or valvuloplasty) with apparent success.

20 Stents are typically composed of scaffolding that includes a pattern or network of interconnecting structural elements or struts, formed from wires, tubes, or sheets of material rolled into a cylindrical shape. This scaffold or scaffolding gets its name because it physically holds open and, if desired, expands the wall of the passageway. Typically, stents are capable of being compressed or crimped onto a catheter so that 25 they can be delivered to and deployed at a treatment site.

Delivery includes inserting the stent through small lumens using a catheter and transporting it to the treatment site. Deployment includes expanding the stent to a larger diameter once it is at the desired location. Mechanical intervention with stents has reduced the rate of acute closure and restenosis as compared to balloon angioplasty.

5       Stents are used not only for mechanical intervention but also as vehicles for providing biological therapy. Biological therapy uses medicated stents to locally administer a therapeutic substance. The therapeutic substance can also mitigate an adverse biological response to the presence of the stent. A medicated stent may be fabricated by coating the surface of either a metallic or polymeric scaffold with a  
10      bioresorbable polymeric carrier that includes an active or bioactive agent or drug. Polymeric scaffolding may also serve as a carrier of an active agent or drug by incorporating a drug throughout the scaffolding material.

The stent must be able to satisfy a number of mechanical requirements. The stent must have sufficient radial strength so that it is capable of withstanding the structural loads, 15 namely radial compressive forces, imposed on the stent as it supports the walls of a vessel. This structural load will change as a function of time as the vessel heals, undergoes positive remodeling, or adapts to the presence of the stent. Once expanded, the stent must adequately provide lumen support during a time required for treatment in spite of the various forces that may come to bear on it, including the cyclic loading induced by the  
20      beating heart. In addition, the stent must possess sufficient flexibility with a certain resistance to fracture.

Stents implanted in coronary arteries are primarily subjected to radial loads, typically cyclic in nature, which are due to the periodic contraction and expansion of vessels as blood is pumped to and from a beating heart. Stents implanted in peripheral  
25      blood vessels, or blood vessels outside the coronary arteries, e.g., iliac, femoral, popliteal, renal and subclavian arteries, however, can undergo significant nonpulsatile forces and

must be capable of sustaining both radial forces and crushing or pinching loads. These stent types are implanted in vessels that are closer to the surface of the body, and may be close to joints. Because these stents are close to the surface of the body, they are particularly vulnerable to crushing or pinching loads, which can partially or completely 5 collapse the stent and thereby block fluid flow in the vessel.

The superficial femoral artery (SFA), in particular, can subject a scaffold to various nonpulsatile forces, such as radial compression, torsion, flexion, and axial extension and compression, which place a high demand on the mechanical performance of implants.

10 Thus, in addition to high radial strength, stents or scaffolds for peripheral vessels such as the SFA, require a high degree of crush recovery. The term “crush recovery” is used to describe how the scaffold recovers from a pinch or crush load, while the term “crush resistance” is used to describe the minimum force required to resist a permanent deformation of a scaffold.

15 Stents made from biostable or non-bioerodible materials, such as metals, have become the standard of care for percutaneous coronary intervention (PCI) as well as in peripheral applications, such as the superficial femoral artery (SFA), since such stents have been shown to be capable of preventing early and late recoil and restenosis. In the SFA, where the artery undergoes extensive movement, self expanding stents made from 20 materials such as Nitinol are the standard of care.

However, in many treatment applications, the presence of a stent in a body is necessary for a limited period of time until its intended function of, for example, maintaining vascular patency and/or drug delivery is accomplished. Moreover, it is believed that biodegradable scaffolds allow for improved healing of the anatomical 25 lumen since they allow the vessel to return to its natural state as compared to metal stents, which may lead to a reduced incidence of late stage thrombosis. In these cases,

there is a desire to treat a vessel using a polymer scaffold, in particular a bioerodible polymer scaffold, as opposed to a metal stent, so that the prosthesis's presence in the vessel is for a limited duration.

There are numerous challenges to overcome when developing a polymer scaffold, particularly in peripheral blood vessels, or blood vessels outside the coronary arteries in which a stent is subjected to both radial forces and nonpulsatile forces. One way of addressing the adverse effects of nonpulsatile forces is to implant stents as a series of disconnected segments. In this way, the transmission of nonpulsatile forces along the stent are reduced or eliminated.

## 10 SUMMARY OF THE INVENTION

Embodiments of the present invention include a segmented scaffold comprising: two or more radially expandable disconnected scaffold segments arranged end to end, wherein each segment includes two or more undulating cylindrical rings composed of struts, and wherein rings at an end of each segment comprise peak undulations projecting longitudinally outward from the end of the segment and comprise valley undulations extending longitudinally toward the segment, and wherein the peak and valley undulations of adjacent rings overlap.

Embodiments of the present invention include a method of delivering a scaffold: providing a segmented scaffold crimped over a delivery balloon, the segmented scaffold comprising two or more radially expandable disconnected scaffold segments arranged end to end, wherein each end of the segments comprises undulating cylindrical rings composed of struts and wherein undulations of adjacent segments overlap; and expanding the scaffold segments to a deployment diameter, wherein the undulations of the adjacent segments overlap at the deployed diameter.

25 Embodiments of the present invention include a radially expandable scaffold segment comprising: two or more connected undulating cylindrical rings composed of

struts, wherein the undulating rings of each segment form a plurality of diamond-shaped cells with two pairs of opposing vertices, one pair being longitudinally aligned and one pair being circumferentially aligned, and wherein alternating diamonds around at least one end ring are omitted to form peak and valley undulations along the at least 5 one end ring with a longitudinal length that is a longitudinal length of the diamond-shaped cells.

Embodiments of the present invention include a scaffold comprising: a plurality of scaffold segments in a crimped reduced configuration; and at least one discontinuous linking element between adjacent segments comprising a discontinuity located between 10 the adjacent segments.

Embodiments of the present invention include a method of modifying a scaffold comprising: providing a scaffold in a crimped reduced configuration, wherein the scaffold comprises longitudinal scaffold segments and linking elements connecting adjacent scaffold segments; and creating a discontinuity in at least one linking element 15 between at least one set of adjacent segments.

#### INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference, 20 and as if each said individual publication or patent application was fully set forth, including any figures, herein.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 depicts an exemplary stent scaffold.

FIG. 2 depicts an exemplary scaffold pattern which shows schematically the forces 25 acting on the scaffold.

FIG. 3A depicts an exemplary scaffold segment of a segmented scaffold.

FIG. 3B depicts a close-up view of a portion of the scaffold segment in FIG. 3A illustrating various features.

FIG. 4 depicts a segmented scaffold composed of a plurality of axial segments from FIG. 3A.

5 FIG. 5 depicts scaffold segments of a segmented scaffold mounted over a balloon in a folded configuration.

FIG. 6 is a schematic illustration of a segmented scaffold with segments illustrating the reduced diameter of unsupported sections of the vessel wall between the segments.

10 FIG. 7 depicts a flattened view of an exemplary scaffold segment 400 similar to the segment depicted in FIG. 3A.

FIG. 8 depicts an exemplary segment based on the segment of FIG. 7 in which alternating diamonds are omitted one end and in-line diamonds are removed on the other end.

15 FIG. 9 depicts an exemplary segment based on the segment of FIG. 7 in which alternating diamonds are omitted one end and off-set diamonds are removed on the other end.

FIG. 10 depicts two in-line segments of FIG. 8 that are interlinked.

FIG. 11 depicts a three-dimensional view of two interlinked segments.

20 FIG. 12 depicts interlinked segments in a crimped state with about 50% ring overlap or engagement of the end rings.

FIG. 13 depicts interlinked segments in a crimped state with about 100% ring overlap or engagement of the end rings.

FIG. 14 depicts an expanded view of the interlinked scaffolds of FIG. 10.

25 FIG. 15 depicts an image of a deployed segmented scaffold with large segment to segment gaps.

Fig. 16 depicts deployed segmented scaffolds of which the left-most segment is rotated relative to the middle segment resulting in a non-uniform gap.

Fig. 17 depicts a schematic of part of the interlink area of the crimped segmented scaffold of FIG. 13.

5 FIG. 18A depicts an interlinked region of crimped interlinked segments.

FIG. 18B depicts an expanded view of one of the peak undulations.

FIG. 19 depicts a portion of an end ring of a segment with a head portion and body portion.

FIG. 20 depicts a portion of an end ring of a segment with a head portion and body  
10 portion.

FIG. 21 depicts a close-up view of a discontinuous linking element between scaffold segments.

FIG. 22 depicts a two-dimensional projection of adjacent scaffold segments that are all disconnected.

15 FIG. 23 depicts a two-dimensional projection of adjacent scaffold segments that include both intact and discontinuous linking elements.

FIG. 24 depicts a close-up view of a region between scaffold segments, like those shown in FIG. 3A.

20 FIG. 25 depicts a close-up view of a portion of a scaffold like the one shown in FIG. 1.

FIG. 26 depicts a pattern which is pattern from FIG. 1 with one discontinuous linking element and one intact linking element between each ring.

FIG. 27 depicts a pattern which is the pattern from FIG. 1 with one discontinuous linking element and one intact linking element at every third segment gap.

25 FIG. 28 depicts a segmented scaffold, which is the scaffold from FIG. 4 with two intact linking elements and two discontinuous linking elements between each segment.

FIG. 29 is an image of interlinked segmented scaffold in a deployed state from a bench test.

FIG. 30 depicts images of an interlinked segmented scaffold composed of two segments.

5 FIG. 31 depicts images of interlinked segmented scaffolds composed of three in-line segments.

FIG. 32 depicts images of an interlinked segmented scaffold composed of three off-set segments.

10 FIG. 33 depicts images of an interlinked scaffold segmented composed of six in-line segments.

#### DETAILED DESCRIPTION OF THE INVENTION

Coronary arteries refer generally to arteries that branch off the aorta to supply the heart muscle with oxygenated blood. Peripheral arteries refer generally to blood vessels outside the heart. In both coronary artery disease and peripheral artery disease, the arteries become hardened and narrowed or stenotic and restrict blood flow. In the case of the coronary arteries, blood flow is restricted to the heart, while in the peripheral arteries blood flow is restricted leading to the kidneys, stomach, arms, legs, feet, and brain. The narrowing is caused by the buildup of cholesterol and other material, called plaque, on the inner walls of the vessel. Such narrowed or stenotic portions are often referred to as lesions. Arterial disease also includes the reoccurrence of stenosis or restenosis that occurs after an angioplasty treatment. Although there are probably several mechanisms that lead to restenosis of arteries, an important one is the inflammatory response, which induces tissue proliferation around an angioplasty site. The inflammatory response can be caused by the balloon expansion used to open the vessel, or if a stent is placed, by the foreign material of the stent itself.

A stent, a stent scaffold, or scaffold includes a plurality of cylindrical rings connected or coupled with linking elements. When deployed in a section of a vessel, the cylindrical rings are load bearing and support the vessel wall at an expanded diameter or a diameter range due to cyclical forces in the vessel. Load bearing refers to 5 the supporting of the load imposed by radial inwardly directed forces. Structural elements, such as the linking elements or struts primarily serve to maintain stability and connectivity between the rings. For example, a stent may include a scaffold composed of a pattern or network of interconnecting structural elements or struts.

FIG. 1 illustrates a portion of an exemplary prior art stent or scaffold pattern 10 100 shown in a flattened view. The pattern 100 of FIG. 1 represents a tubular scaffold structure so that an axis A-A is parallel to the central or longitudinal axis of the scaffold. FIG. 1 shows the scaffold in a state prior to crimping or after deployment. Pattern 100 is composed of a plurality of ring struts 102 and link struts 104. The ring struts 102 form a plurality of cylindrical rings, for example, rings 106 and 108, arranged about the 15 cylindrical axis A-A. The rings have an undulating or sinusoidal structure with alternating crests or peaks 116 and troughs or valleys 118. The rings are connected by the link struts 104. The scaffold has an open framework of struts and links that define a generally tubular body with gaps 110 in the body defined by rings and struts. A cylindrical tube may be formed into this open framework of struts and links by a laser 20 cutting device that cuts such a pattern into a thin-walled tube that may initially have no gaps in the tube wall.

The structural pattern in FIG. 1 is merely exemplary and serves to illustrate the basic structure and features of a stent or scaffold pattern. A stent such as stent 100 may be fabricated from a polymeric tube or a sheet by rolling and bonding the sheet to form 25 the tube. A tube or sheet can be formed by extrusion or injection molding. A stent pattern, such as the one pictured in FIG. 1, can be formed on a tube or sheet with a

technique such as laser cutting or chemical etching. The stent can then be crimped onto a balloon or catheter for delivery into a bodily lumen.

The width and/or radial thickness of the struts in a scaffold may be 80 to 400 microns, or more narrowly, 100 to 250 microns, 140 to 180 microns, 200 to 400 5 microns, 140 to 160 microns, or 300 to 350 microns. The thickness and width can be different. For example, the width can be at or about 350 microns (e.g.,  $\pm$  10 microns) and the thickness can be at or about 300 microns (e.g.,  $\pm$  10 microns).

Semicrystalline polymers such as poly(L-lactide) (PLLA) with glass transition temperature (Tg) above human body temperature may be suitable as materials for a 10 totally bioresorbable scaffold since they are relatively stiff and strong at the conditions of the human body. However, they tend to be brittle at these conditions. These polymer systems exhibit a brittle fracture mechanism in which there is little plastic deformation prior to failure. As a result, a stent fabricated from such polymers can be vulnerable to fracture during fabrication and use of a scaffold, i.e., crimping, delivery, 15 deployment, and during a desired treatment period post-implantation.

Embodiments of the present invention are applicable to endovascular treatment of coronary and peripheral disease in coronary arteries and various peripheral vessels including the superficial femoral artery, the iliac artery, and carotid artery. The embodiments are further applicable to various stent types, such as self-expandable and 20 balloon expandable stents. The embodiments are further applicable to various stent designs including scaffolding structures formed from tubes, wire structures, and woven mesh structures. Embodiments also applicable to different materials that are permanent implants such as polymers and metals like Nitinol, Algeloy, stainless steel and cobalt chrome.

25 In general, the initial clinical need for a bioresorbable scaffold is to provide mechanical/structural support to maintain patency or keep a vessel open at or near the

deployment diameter. The scaffold is designed to have sufficient radial strength or vessel wall support for a period of time. The vessel wall support provided by the stent allows the stented segment of the vessel to undergo healing and remodeling at the increased diameter. Remodeling refers generally to structural changes in the vessel 5 wall that enhance its load-bearing ability.

A period of vessel wall support is required in order to obtain permanent positive remodeling and vessel healing and hence maintenance of vessel patency. As the polymer of the stent degrades, the radial strength of the scaffold decreases and the load of the vessel is gradually transferred from the scaffold to the remodeled vessel wall. In 10 addition to the decline in radial strength, the degradation of the scaffold also causes a gradual decline in the mechanical integrity, i.e., connectivity of struts and the size and shape of the overall scaffold structure. The struts gradually resorb and disappear from the vessel.

The amount of movement experienced by a peripheral scaffold in the peripheral 15 artery is greater than what a coronary scaffold experiences in the coronary artery. A peripheral scaffold can be subjected to a high degree of flexing, axial elongation/compression, pinching, bending, and torsion after implantation. Axial stresses on the scaffold can arise from the axial compression and extension, flexural stresses are imposed by lateral flexing, crushing forces are imparted by pinching, while 20 helical stress can arise from torsional forces.

Such stresses are propagated along the length of the scaffold and can impart significant forces throughout the scaffold structure. The forces can cause failure in ring struts, resulting in a decrease or loss in vessel wall support provided by the scaffold. Such forces can be transmitted along the length of the scaffold by link struts that 25 connect rings.

Link strut breakage is not inherently deleterious to either performance or safety. Bench testing and animal study results suggest that scaffold properties of radial strength, crush recovery, and crush resistance are primarily attributable to the mechanical/structural integrity of the rings in the scaffold and not the links.

5 Strut breakage can lead to release of fragments in the blood and tissue irritation from broken strut fragments. Fragment release could result in thrombosis. Broken fragments can be mechanically injurious to the vessel leading to tissue irritation or even vessel dissection and perforation.

FIG. 2 depicts the exemplary scaffold pattern 100 which shows schematically 10 the forces acting on the peripheral scaffold. Line A-A represents the cylindrical axis of the stent. The arrows around the edges represent the forces acting on the scaffold during delivery and after deployment. Arrows 111 represent bending, arrows 112 represent radial compression, and arrows 114 represent axial compression. Bending occurs during delivery through tortuous anatomy and after deployment.

15 Radially compressive forces on the scaffold are caused by the push back of the vessel walls on the scaffold. Axial compressive forces in the SFA arise due to movement of a leg such as during walking or bending of the leg. In the SFA, the axial compressive forces can be considerable as the vessel is compressed up to 7% or more and relaxed repeatedly up to one million cycles/year.

20 Cracks in the scaffold occur when it is subjected to a sufficiently high force such as resulting from bending during delivery or repetitive forces after deployment that cause fatigue. These cracks can cause a loss of radial strength or separation of struts of the scaffold that drift downstream of the scaffold.

A crack in the ring strut may cause a reduction or loss of radial strength, while a 25 crack in the link is less damaging to the scaffold in terms of radial strength, crush resistance, and crush recovery. It is believed that if the axial forces on the scaffold

were reduced, the occurrence of ring cracks would be significantly reduced. When axial forces that travel through the links to the ring struts are reduced, then the potential for ring strut fractures are also reduced.

The various embodiments of the present invention are directed to peripheral 5 scaffolds that are subjected to significant nonpulsatile forces upon implantation. Embodiments are further directed to methods and systems for delivering such peripheral scaffolds. The embodiments of the scaffold designs are directed to reducing or eliminating strut fracture and breakage during use of the scaffold.

The embodiments are also directed to implanting such scaffolds in areas or 10 vessels where there is no significant vessel movement such as coronary, iliac, renal etc.

The segmented scaffolds disclosed herein have advantages over non-segmented scaffolds. For example, segmented scaffolds offer a substantial cost savings over conventional stent manufacturing by reducing the number of lengths of scaffolds needed in a product. In addition, the segmented scaffold segments with the disclosed 15 diamond pattern have substantially higher radial strength (more than double that of a conventional stent) over conventional stent patterns which provides improved vessel holding open ability. This can be useful in highly calcified anatomy.

Various embodiments include a scaffold composed of axial scaffold segments that are not connected by link struts. Embodiments of such a scaffold include two or 20 more radially expandable axial scaffold segments arranged axially end to end. The axial segments, in particular, axially adjacent segments are not connected by any physical structure or material of the scaffold. The axial segments, however, may be indirectly in contact through another structure such as a support member or a sheath. The axial segments may further be connected by structures not part of structure from 25 which the scaffold segments are formed, such as a tube.

In general, upon deployment of the scaffold segments, forces subjected on one axial segment cannot be transmitted to other axial segments through linking struts as such forces are by linking struts of a scaffold shown in FIG. 1. The axial segments may be composed of a plurality of interconnected struts. Forces subjected to a segment can 5 be transmitted between struts within the segment, but not between segments.

In some embodiments, the axial segments are composed of one or more cylindrical rings of struts. A cylindrical ring may be composed of undulating struts having crests and troughs. The cylindrical rings of struts that are adjacent in a segment are connected. The rings may be connected by link struts. Alternatively, the rings may 10 be directly connected to one another without link struts. The number of rings in a segment may be one or any number greater than one. In some embodiments, a segment can have 1 or more, 2 or more, 1 to 6 rings, 1 to 3 rings, 2 to 6 rings, or 2 or 3 rings.

Upon deployment, the axial segments remain intact for a period of time and maintain a ring shape at or near the deployed diameter. Since the axial segments are 15 not connected, they are uncoupled which prevents transmission of axial compression between segments. The decoupled axial segments retain sufficient radial strength to support the vessel at or near the deployed diameter. The decoupling of the axial segments reduces stress, for example, from axial compression that causes fracture of ring struts. The reduced ring strut fracture helps maintain the radial strength and the 20 crush recovery and resistance to broken off struts of the scaffold floating down the vessel as emboli. The decoupling of rings reduces or prevents propagation of fracture of rings due to bending of the scaffold structure along its axis.

In some embodiments, a scaffold with disconnected axial segments can be fabricated by forming the axial segments separately. For example, a scaffold pattern 25 can be cut into a thin-walled tube having an axial length the same as the desired axial segment. Alternatively, a scaffold can be fabricated by laser cutting a tube and then

axial segments can be formed cutting the scaffold into disconnected axial segments by cutting link struts between segments or cutting the link struts between segments off entirely. Unless otherwise specified, scaffold segments or segments refer to disconnected scaffold segments or segments.

5        The stability of an axial segment depends on the length of the axial segment. The stability is inversely related to the length of the axial section. The susceptibility to fracture from nonpulsatile forces, however, is directly related to the length of the axial section. The length of the axial segments should be large enough so that it has a desired stability, while having reduced fracture arising from nonpulsatile forces.

10       The radial strength and radial stiffness of a scaffold or scaffold segment increases with the degree of connectivity of a scaffold. The degree of connectivity refers in part to the number of link struts between rings and the length of the link struts: more link struts and shorter link struts tend to increase strength and stiffness. The increase in strength and stiffness from increase in link struts has practical limitations  
15       for the Fig. 1 type designs. As the number of links is increased, the width of each ring strut is reduced to accommodate for the extra link when in the crimped state.

20       The stiffer the scaffold, the more susceptible the scaffold is to fracture. In the present embodiments, since compressive forces are not transmitted along an entire scaffold length, the scaffold segments can be made with a higher connectivity than a scaffold that does not have disconnected axial segments.

25       In the scaffolds such as the one depicted in FIG. 1, the crests of the axial rings are axially aligned or approximately axially aligned. The stiffness of the axial segments of such a scaffold can be increased by increasing the number of link struts between axially adjacent peaks of adjacent rings. Every pair of aligned peaks between adjacent rings can be connected, every other pair of aligned peaks can be connected, or every third pair of aligned peaks can be connected by a link strut.

In some embodiments, the axial segments may be composed of rings arranged such that the crests in one ring are axially aligned or almost axially aligned with the troughs in an adjacent ring. The rings are connected by at least one link strut between an aligned crest and trough. Stiffness is greatest with a link strut between each aligned 5 crest and trough. Greater flexibility is introduced by having fewer than every aligned crest and trough connected by a link strut. For example, only every other aligned crest and trough can be connected, or only every third aligned crest and trough can be connected by a link strut. Additionally, the length of the link struts in the axial segments can be adjusted to modify the stiffness of the axial segment. Decreasing the 10 length of the links increases both the radial strength and radial stiffness of the axial segment since the number of rings per segment length is maximized. Alternatively the ring crests on one ring can be aligned with the ring crests of adjacent rings. In this case, when the scaffold is crimped, the link does not occupy space between ring struts. This allows for the maximizing of ring strut width which results in higher radial strength.

15 Such a pattern may also be described as a plurality of rings composed of diamond-shaped elements formed of struts. The elements of the rings are connected at circumferentially aligned vertices of the diamond-shaped elements. Axially adjacent rings are connected at axially aligned vertices either by a short link strut or at the intersection of vertices of elements of adjacent rings.

20 FIG. 3A depicts an exemplary axial segment 320 viewed in a flattened configuration composed of a plurality of rings of undulating struts with crests and troughs. Line A-A is the longitudinal axis of the axial segment. An exemplary ring 322 has crests 324 and troughs 326. As shown in FIG. 3A, every crest in ring 322 is connected to every trough in adjacent ring 328 by a short link strut 330. The 25 arrangement of rings 322 and rings 328 forms a plurality of rings 329 of diamond-

shaped elements 331 formed of struts. The diamond-shaped elements 331 of the rings are connected at circumferentially aligned vertices of the diamond-shaped elements.

L<sub>s</sub> is the length of the axial segment. L<sub>s</sub> may be 3 to 6 mm, 6 to 8 mm, 8 to 10 mm, 10 to 12 mm, or greater than 12 mm in an as cut or as fabricated configuration. L<sub>s</sub> increases when the segment is crimped to a decreased diameter and then decreases when expanded from a crimped configuration. Length change is affected by the number of peaks in a ring and the width of the diamonds. The length change (increases or decreases) with the number of peaks and (increases or decreases) with the width of the diamonds.

FIG. 3B depicts a close-up view of a portion 339 of axial segment 320 illustrating various features. As shown in FIG. 3B, L<sub>r</sub> is the length of a ring strut, for example, strut 332 between a crest and trough in a ring and W<sub>rs</sub> is the width of the ring strut. L<sub>l</sub> is the length of short link strut 330 that connects crests and troughs of adjacent rings and W<sub>ls</sub> is the width of the link strut.  $\theta$  is the angle at the longitudinal vertex of the diamond shaped cells, i.e., between struts 332 and 334 in a ring that intersects at a crest or trough.  $\varphi$  is the angle between struts 332 and 336 which are joined by short link strut 330 and a diamond-shaped cell. H<sub>c</sub> is the height of the diamond-shaped cell and W<sub>c</sub> is the width of the diamond-shaped cell.

$\theta$  may be 90 degrees, 90 to 95 degrees, 95 to 100 degrees, 100 to 110 degrees, or greater than 110 degrees.  $\theta$  may be 90 degrees, 85 to 90 degrees, 80 to 85 degrees, 70 to 80 degrees, or less than 70 degrees.  $\varphi$  may be 90 degrees, 85 to 90 degrees, 80 to 85 degrees, 70 to 80 degrees, or less than 70 degrees.  $\varphi$  may be 90 degrees, 90 to 95 degrees, 95 to 100 degrees, 100 to 110 degrees, or greater than 110 degrees.

Exemplary values for  $\theta$  and  $\varphi$  are about 70 and 110 degrees, respectively. Values in this range tend to reduce segment shortening from crimping to deployment. Other exemplary values for  $\theta$  and  $\varphi$  are about 110 and 70 degrees, respectively. Values

in this range tend to increase segment's radial strength and crush resistance. Another variable that affects the angles above is the lased tube diameter and the final deployed diameter. Generally, for polymers, the lased tube diameter is slightly larger than the final deployed diameter.

5 The segments can include radiopaque marker embedded within holes in the scaffold segment to aid in visualization of the implanted scaffold. In some embodiments, the markers are embedded in holes in the short link struts 330 of FIG. 3A. In other embodiments, the markers are embedded in holes in ring struts 332 of FIG. 3B.

When a scaffold segment is crimped, the  $L_s$  increases which is caused by 10 bending at the vertices of the diamond-shaped elements. Specifically, when the scaffold segment is crimped,  $\theta$  decreases and  $\varphi$  increases. When a scaffold segment is deployed, the  $L_s$  shortens which is caused by bending at the vertices of the diamond-shaped elements corresponding to an increase in  $\theta$  and a decrease in  $\varphi$ .

The segment properties of radial strength and stiffness can be modified through 15 adjustment of the as-cut geometrical parameters of the diamond-shaped elements. For example, radial strength and stiffness is increased by increasing  $H_c$  which results in a decrease in  $W_c$  and also corresponds to a decrease in  $\varphi$  and an increase in  $\theta$ .

In some segment design embodiments, the diamond-shaped elements are 20 square-shape or approximately square-shaped in the as-cut condition. In such embodiments,  $\varphi$  is the same or approximately the same as  $\theta$ . For example,  $ABS(\varphi - \theta)$  may be 2 or about 2 degrees or less than 2 degrees.

In other segment design embodiments, the diamond-shaped elements can be 25 taller or greater in the circumferential direction or,  $H_c > W_c$  and  $\varphi > \theta$ . In such embodiments, the  $\theta - \varphi$  may be greater than 2 degrees, 2 to 4 degrees, 4 to 8 degrees, greater than 8, about 3 degrees, about 4 degrees, or about 5 degrees.

$L_l$  may be less than 10% or 10% to 20%, 20% to 30%, 30 to 40%, or greater than 40% of a ring strut length between a crest and a trough. Exemplary link struts may have a length of less than 0.01 in, 0.01 to 0.02 in, 0.02 to 0.04 in, 0.04 to 0.06 in, or greater than 0.06 in. In some embodiments, adjacent rings are connected at an 5 intersection of the opposing crests and troughs such that a length of the link strut is effectively the width of the intersection and  $L_l$  is zero.

FIG. 4 depicts a segmented scaffold 340 composed of a plurality of axial segments 341 to 347, from FIG. 3A. The delivery of a scaffold composed of decoupled or disconnected axial segments can be achieved by disposing the axial segments over a 10 catheter delivery balloon. The axial segments can be arranged end to end and spaced apart on a single balloon or multiple balloons arrange end to end. The axial segments may be crimped over the balloon to a reduced diameter configuration to allow for delivery of a vascular system to a treatment site.

Generally, stent crimping is the act of affixing a radially expandable scaffold or 15 stent to a delivery catheter or delivery balloon so that it remains affixed to the catheter or delivery balloon until the physician desires to deliver the stent at the treatment site. Delivery balloons may be compliant, semi-compliant, or noncompliant and are made from PEBAK, nylon, or other type of common balloon material. Examples of such crimping technology which are known by one of ordinary skill in the art include a roll 20 crimper; a collet crimper; and an iris or sliding-wedge crimper. In the sliding wedge or iris crimper, for example, adjacent pie-piece-shaped sections move inward and twist toward a scaffold in a cavity formed by the sections, much like the leaves in a camera aperture.

FIG. 5 depicts a projection of axial segments 351, 352, and 353 disposed over a 25 balloon 350 in a deflated configuration. Axial segments are crimped tightly over the balloon in a reduced diameter configuration. A crimped configuration generally may

correspond to the inner surface of the segments in contact with the outer surface of a balloon. The axial segments are spaced apart by a distance, size, or width Lg, which is the gap between segments. Lg can change during inflation and deployment of the segments to a deployed diameter due to movement of the segments and axial

5 contraction or shortening of the segments. Lg at deployment should be large enough to avoid interference or contact of the segment ends during bodily movements. Lg at deployment should be large enough so that there is axial stability and the support of the vessel is continuous. In exemplary embodiments, the segments when deployed are spaced apart by 0.5 to 2mm, or more narrowly, 0.5 to 1 mm, 1 to 2 mm, 2 to 3 mm.

10 The required Lg is determined by the anatomy that the segmented scaffold will be deployed in to, i.e., in the SFA it will need to be greater than for the Iliac where vessel compression and bending are virtually zero. In general, Lg is higher for anatomies with higher vessel compression and bending.

Factors that influence a desired Lg at deployment include the axial compression

15 in the vessel, bending of the vessel, and stability in presence of side branches coming off of a segment of the vessel where the scaffold is implanted.

When compressive loads are placed on the scaffold the axial compression may occur predominantly between segments. Generally, it is important to allow for the decrease in the spacing of the segments during compression and loading. Therefore, Lg

20 at deployment should be large enough so that the segments do not contact or interfere with each other during axial compression. The Lg at deployment can be selected to allow for an axial compression of zero, below 7%, or 7 to 15%, or for example, about 13%.

The bending of a vessel with implanted segments results in a decrease in the Lg

25 at the concave or inner side of the bend with the gap widening toward the convex or outer side of the bend. The segments at the inner side of the bend can interfere or make

contact with each other if the initial gap is not wide enough. The Lg at deployment can be selected to allow for bending of 20 to 30 degrees or less than 30 degrees, or about 30 degrees. In this case, a 3mm gap reduces to 0.8 mm at the inner side of the gap.

The scaffold segments may be deployed in a vessel that includes a side branch 5 and a gap between segments that overlap this side branch. In this case, Lg can be the width of the side branch or greater or less than the width of the side branch. To maintain axial stability of a segment of a segmented scaffold over a side branch, the length of a segment needs to be longer than the side branch so that the radially supported length of the segment is typically 1.5 times the segment diameter when 10 deployed. This diameter:length ratio can be less than a 1:1 ratio, a 1:1 ratio, a 1:1.5 ratio or a 1:2 ratio or greater. The ratio is dependent among other things on the size of the nonpulsatile forces at the delivery site. For example, the Lg at deployment can be less than 2 or 3 mm.

The diamond pattern disclosed herein tends to maximize the relative friction 15 between the vessel wall and the segments. With this and the high radial and axial rigidity of the diamond pattern, endothelialization of the segments may be sped up and vessel irritation may be reduced. With quick endothelialization, the scaffold/vessel wall becomes a composite structure which in itself enhances the radial strength and hence crush resistance of the vessel/scaffold composite. With most, if not all of the 20 movement transferred to the gaps between the segments, the design utilizes the natural flexibility of the vessel walls to handle any compression, bending and torsional movements.

In some embodiments, a single high radial strength and stiff scaffold segment, such as described above, may be implanted at an implant site. Implanting a single 25 segment without additional segments may be useful in treatments involving vessels that

do not undergo axial compression, torsion, or bending. Examples include the Iliac and Renal artery.

During deployment at a lesion site of a conventional balloon expandable stent or scaffold, the balloons generally start to expand at the proximal and distal ends first, 5 producing a dog bone shape. As pressure is increased, the balloon expands in the center, expanding the scaffold in the center also.

With the segmented scaffold which can include several short scaffolds on a single balloon, the balloon can expand in a similar manner, i.e., expanding at the proximal and distal ends first, followed by expansion of a center section. Expansion at 10 the ends first has the tendency to push the segments axially towards the center of the balloon which decreases the segment to segment gap. The gap may be decreased to the point that the segments collide with each other. This movement of the individual segments axially along the balloon during deployment, therefore, can change the segment to segment gap to an undesirably small size which can result in interference of 15 the segments. Additionally, the segment to segment spacing will not necessarily be the same between all segments. A reduced gap or zero gap may be acceptable where nonpulsatile forces are virtually zero.

In pre-clinical animal studies, bioabsorbable polymer disconnected segmented scaffolds have been shown to have high radial strength and fracture resistance. The 20 sections of the artery along the segments are held open at a desired diameter. However, in some cases, the sections of the artery at the gaps between the segments are not held open to the same degree as along the segments. There appears to be “sagging” or focal restenosis of the vessel wall inward into the artery lumen at the gaps between segments. For example, in a case where the gaps between the segments were on the order of 5mm, 25 sagging or focal restenosis was observed.

FIG. 6 is an image of bench tested segmented scaffold showing segment 352 and a portion of segments 351 and 353. The sections of vessel wall 372 along the segments are supported at a diameter of the segments. Sections 374 of the vessel wall along gaps 360 between the segments sag inward toward the lumen.

5 Embodiments of the present invention include segmented scaffolds and delivery thereof that reduce or prevent the vessel sagging between the segments while maintaining high radial strength and fracture resistance.

10 Embodiments of the present invention include deploying a segmented scaffold in a manner that the ends of the adjacent scaffolds segments overlap or are interlinked. The segments that are overlapped or interlinked are disconnected and are not in contact. The segment ends overlap. Therefore, there no gap between segments that is a strip or band with no support that completely encircles the vessel wall. Equivalently, there is no longitudinal position without support from a segment between the ends of adjacent segments that extends completely around the circumference of the vessel wall or 15 scaffold.

Embodiments also include segmented scaffold segments in a crimped reduced state with ends of the adjacent scaffolds segments that overlap or are interlinked. The crimped scaffold segments can be crimped over a delivery balloon to allow balloon assisted delivery of the segments to a deployed state in a vessel. The scaffold segments 20 are interlinked in a manner that upon expansion of the segments to a deployed state, the deployed segments are interlinked as described.

25 Although specific embodiments are described herein, the embodiments generally apply to segmented scaffold made up of segments composed of struts forming a plurality of circumferential undulating rings, the undulations include peaks and valleys, as exemplified above. Undulating can refer to, but is not limited to, to a wave-like appearance or form. The wave-like appearance can be smooth, such as

sinusoidal from, or jagged, such as a zigzag form. The ends of the segments, therefore, include an undulating ring also with peaks and valleys. A peak or valley undulation refers generally to the portion of an undulation or wave on either side of a peak or valley. The peak undulations project longitudinally outward or away from the end of 5 the segment and the valley undulations extend longitudinally inward or toward the segment.

The interlinking of two adjacent scaffold segments with the above general structure is described with respect to the peak undulation and valley undulation of neighboring end rings of adjacent segments. The peak undulations of a first ring 10 overlap or extend into the valley undulation of an adjacent ring. Likewise, the peak undulations of the adjacent ring overlap or extend into the valleys of the first ring. The degree of overlap or interlinking can be described in terms degree of extension of the peak undulations into the valley undulations.

The peak and valley undulations in the crimped state are compressed close to 15 one another relative to the expanded or deployed state. The segments described are provided in the crimped state with the interlinking of the neighboring rings of adjacent segments. The degree of overlap may be greater in the crimped state than the deployed state since the degree of overlap may decrease as the segments are expanded.

Interlinked segmented scaffolds can be formed using the scaffolds segments 20 described, for example, in FIGs. 3A-B and 4. FIG. 7 depicts a flattened view of another exemplary scaffold segment 400, like segment 320 depicted in FIG. 3A. Line A-A represents the longitudinal axis of the segment. Segment 400 has an end ring 401 of diamond cells made up of two undulating rings connected at peaks, one of which is undulating end ring 402 composed of peaks 404 and valleys 406. Peak undulations 408 25 are composed of struts 408A and 408B which extend from two adjacent valleys and meet at a peak. Valley undulations 410 are composed of struts 410A and 410B which

extend from two adjacent peaks and meet at a valley. Peak undulations project longitudinally outward from the segment and valley undulations extend longitudinally inward into the segment. The height or length of the valley and peak undulations is one half the longitudinal width of a diamond,  $W_c/2$ .

5        A segmented scaffold can be provided in a deployed state with scaffold segments such as segment 400 that are arranged with interlinking of adjacent end rings. The peak undulations 408 can overlap or interlink with the valley undulations 410.

However, for the segment 400 such a deployed configuration may be difficult or impossible to achieve in practice. Specifically, the peak undulations may not fit into 10 the valley undulations in a desired crimped state since the angle at the valley is very small in the crimped state. Additionally, even if the peak undulation overlaps the valley in a crimped state, the degree of overlap at crimping is small compared to the length decrease of the segment from the crimped to deployed state. When the segments are deployed, from the crimped to deployed state, the degree of overlap will decrease 15 and may disappear when the segments are deployed.

Embodiments further include segmented scaffolds with segments that are modified to have valley undulations with a greater length or height which allow overlap in the crimped state and overlap when the segments are deployed. The degree of potential overlap is higher relative to the length change of a segment from the crimped 20 state to a deployed state. In such embodiments, the length of the potential overlap of ends of segments can be at or about the longitudinal length of cells of the pattern. Specifically with respect to the exemplary segment 400, the length of the potential overlap is at or about the longitudinal length of a diamond cell of the segment.

Embodiments include segments which are a modification of the segments as 25 described with an end ring of diamonds and undulating end ring of struts. The modification includes omitting diamonds of the diamond end ring at one or both ends.

In particular, alternating diamonds may be omitted from one or both ends of a segment.

Omitting diamonds refers to removing the struts forming every other peak undulation.

For example, struts 408A and 408B in FIG. 7 may be omitted.

The resulting segment has an end ring with peak and valley undulation that 5 provides a greater potential overlap. The degree of shortening upon expansion is unchanged. Therefore, when the modified scaffold segments that are interlinked in the crimped state are expanded to the deployed state, there is significant overlap remain in the deployed state.

FIG. 8 depicts an exemplary segment 420 based on segment 400 of FIG. 7 in 10 which alternating diamonds are omitted at each end. Equivalently, every other peak undulation is omitted on both ends of the segment. Specifically, every other pair of struts 408A and 408B are omitted. In addition, the diamonds that are omitted at opposite ends are longitudinally aligned or opposite from one another or “in-line” diamonds are omitted. Thus, the embodiment in FIG. 8 will be referred to as an “in-line segment.” The modified segment, therefore, has an end ring with an undulating, 15 zigzag structure in which the length of a “zig” and “zag” or from a valley to a peak is twice the length of a side of a diamond of a diamond cell. The longitudinal length of a peak or valley undulation is the longitudinal length of a diamond cell.

As shown in FIG. 8, segment 420 has an undulating end ring 421 composed of 20 peaks 424 and valleys 426. Peak undulations 428 are composed of pairs of in-line struts, (428A, 428B) and (428C, 428D) which extend from two adjacent valleys and meet at a peak. Valley undulations 430 are composed of pairs of in-line struts (430A, 430B) and (430C, 430D) which extend from two adjacent peaks to a valley. Each of the two inline struts is the length of a side of the diamond cells.

25 Peak undulations project longitudinally outward from the segment and valley undulations extend longitudinally inward into the segment. As is shown below, the

maximum potential length of overlap is one half the longitudinal width of a diamond,  $1/2 W_c$ . For the in-line segment, the peaks (and valleys) of the end rings are longitudinally aligned. As shown in FIG. 8, the minimum width of segment 420 is the longitudinal width of a diamond cell,  $W_c$ .

5 FIG. 9 depicts an exemplary segment 450 based on segment 400 of FIG. 7 in which alternating diamonds are omitted at both ends of the segment. Specifically, every other pair of struts 408A and 408B is omitted. Segment 450 differs from segment 420 of FIG. 8 in that omitted diamonds at one end are not longitudinally aligned with omitted diamonds at the other end. The diamonds omitted at one end are 10 circumferentially off-set by one diamond cell. The embodiment in FIG. 9 will be referred to as an “off-set segment.” An alternate embodiment is omitted diamonds every third or every fourth diamond around the circumference of the end ring.

As shown in FIG. 9, segment 450 has an undulating end ring 451 composed of peaks 454 and valleys 456. Peak undulations 458 are composed of two pairs of in-line 15 struts, as described in FIG. 8, which extend from two adjacent valleys and meet at a peak. Valley undulations 460 are composed of pairs of inline struts, as described in FIG. 8, which extend from adjacent peaks to a valley. Peak undulations project longitudinally outward from the segment and valley undulations extend longitudinally inward into the segment. As shown below, the potential overlap is one half the 20 longitudinal width of a diamond,  $1/2 W_c$ . As shown in FIG. 9, the minimum width of segment 450 is twice the longitudinal width of a diamond cell,  $2 \times W_c$ . Also, as shown in FIG. 9, the peaks at one end are longitudinally aligned with the valleys at the other end, for example, peak 454 is longitudinally aligned with valley 462.

FIG. 10 depicts two in-line segments 470 and 474 which are interlinked. End 25 ring 472 of segment 470 is interlinked with end ring 476 of segment 474. For example, peak undulation 478 of segment 470 projects into valley undulation 480 of segment 474.

Each peak of the interlinking peak undulation (e.g., peak 479) is longitudinally aligned with the each valley of the interlinked valley undulation (e.g., valley 481).

There are various ways of defining the degree of overlap or interlinking of the segments. For example, the percent overlap of interlinking of peak undulation 478 with 5 valley undulation 480 can be calculated from, L, the one half width of a diamond cell and the length of the overlap of the peak undulation 478 with the valley undulation 480, L': %overlap = L' / L x 100%. The degree of overlap at deployment may be 5 to 70%, or more narrowly, 5 to 20%, 20 to 30%, 30 to 40%, 40 to 50%, 50 to 60%, and 60 to 70%.

10 As shown in FIG. 10, there is a gap 482 between end rings 472 and 476 of segments 470 and 474, respectively. However, the gap has an undulating profile that follows the interlinking profile of end rings 472 and 476. As a result, there is no longitudinal position completely around a vessel wall that is not supported. FIG. 11 depicts a three-dimensional view of two interlinked segments.

15 In order for deployed segments to have overlap, the segments are provided in a crimped state with a degree of overlap. The degree of overlap is selected so that upon expansion or deployment to a target diameter, the deployed segments have a desired amount of overlap. The degree of overlap at crimping may be 50 to 100%, or more narrowly, 50 to 60%, 60 to 70%, 70 to 80%, 80 to 90%, or 90 to 100%. This overlap 20 may be such that at the gap 482, the axial space between ring struts from a first segment to the ring struts of a second segment is the same as the ring strut spacing within the segments. This will provide a continuous uniform vessel support at the segments and across the segment gap also. In addition, gap 482 may be less than the width of a diamond, the same as the width of a diamond, or more than the width of a diamond.

25 FIG. 12 depicts a side view of interlinked segments 490 and 494 with omitted end ring diamonds in a crimped state with about 50% ring overlap or engagement of the

end rings. For example, a peak undulation with a peak 492 is shown to be overlapping or engaged within the valley undulation with a valley 496. The opening of the diamond cell 498 is shown to have a deformed shape due to the crimped state.

FIG. 13 depicts interlinked segments 500 and 504 with omitted end ring 5 diamonds in a crimped state with about 100% ring overlap or engagement of the end rings. For example, a peak undulation with a peak 502 is shown to be overlapping or engaged within the valley undulation with a valley 506. The opening of the diamond cell 508 is shown to be reduced significantly due to the crimped state.

The crimped interlinked segments of FIGs. 12 and 13 demonstrate how the 10 undulations of the modified rings allow both crimping to a reduced profile and interlinking at crimped and deployed states. FIG. 14 depicts an expanded view of the interlinked scaffolds of FIG. 10. Peak undulation 520 is composed of a first portion made up of pairs of struts 524A and 524B and a second portion composed of pairs of struts 522A and 522B. Likewise, valley undulation 526 is composed of a first portion 15 made up of pairs of struts 530A and 530B and a second portion composed of pairs of struts 528A and 528B.

When the segment is crimped, the struts that make up the peak and valley 20 undulations bend inward. However, as shown in FIGs. 12 and 13, the first portion 524 and the second portion 522 of the peak undulation 520 bend inward to different degrees at pivot points 523A and 523B. The second portion 522 of the peak undulation bends inward to a greater degree than the first portion 524, which is within the valley undulation.

Likewise, the first portion 530 and the second portions 528 of the valley 25 undulation 526 bend inward to different degrees at points 529A and 529B, as shown in FIGs. 12 and 13. The first portion 530 of the valley bends inward to a greater degree than the second portion 528. The closely spaced struts of the first portion cannot

accommodate overlap of the peak undulation of the adjacent segment, but allows for reduction of the segments to a low profile or low diameter configuration. The struts of the second portion 528 of the valley undulation are spaced apart sufficiently to allow overlap of the first portion 524 of the peak undulation of the adjacent segment. In 5 another embodiment, pivot points 523A and 523B may be closer together. This would result in less room needed for the interlink in the crimped state. Alternatively, the diamonds at the interlink and several rows in from the interlink could be adjusted in shape to accomplish a looser or tighter interlink fit in the crimped state. In addition the diamonds could be axially shorter, axially the same or axially longer near the end or at 10 the end of the segments.

The modified segmented scaffolds disclosed with alternating diamonds removed could be deployed in configurations that are not optimum or undesirable. These configurations may result develop during deployment from the crimped state. A non-optimum configuration includes segments with excessive segment to segment gaps 15 in the deployed state so that the vessel is not supported adequately in the segment gaps. In such a configuration there is no overlap of the end rings or the degree of overlap of the rings is low, for example, less than 20 or 30%. FIG. 15 depicts an image of a deployed segmented scaffold with large segment to segment gaps.

In other non-optimum configurations segments may collide as the vessel is 20 axially compressed as would happen in the Superficial Femoral Artery. Collisions can result from a configuration in which the peaks and valleys of adjacent segments are not longitudinally aligned, in contrast to segments 470 and 474 in FIG. 10. Such a configuration can result from rotation of a segment during deployment. Fig. 16 depicts deployed segmented scaffolds of which the left-most segment is rotated relative to the 25 middle segment resulting in a non-uniform gap at “X”. As a result, the segment gap is nonuniform circumferentially.

Therefore, there is a need for a way to insure that the segment gap is consistent between all segments, not excessive, and also uniform circumferentially.

Fig. 17 depicts a schematic of part of the interlink area of the crimped segmented scaffold of FIG. 13. A peak undulation 554 of segment 550 is disposed in 5 between peak undulations 556 and 558 of segment 552 such that there is an overlap of approximately 100% between the two segments. Peak undulation 554 is made up of struts 560 and 562, the sides of a diamond cell, which extend from opposing vertices of the cell to meet at peak 564. The outer side wall surface or profile of the struts 560 and 562 is straight and smooth so that when the segments are deployed there is no 10 interaction between the surfaces of the adjacent scaffolds that influences the relative positions of the adjacent segments.

FIGs. 18A-B and FIGs. 19-20 depict embodiments of segments that are modified to maintain a consistent segment gap which is not excessive and also reduce or prevent rotation during deployment which results in a nonuniform gap 15 circumferentially.

FIG. 18A depicts an interlinked region of crimped interlinked segments 570 and 572. FIG. 18B depicts an expanded view of one of the peak undulations. The peak undulations of the end rings of segments 570 and 572 include head portion 578 and body portion 580. Head portion 578 in the region of peak 574 has an overhang 580 on 20 either side of peak 574 along struts 582 and 584 that extend from peak 574 to vertices 576 and 577, respectively. The overhangs 580 are situated between peak 574 and the vertices 576 and 577. The side wall surface between peak 574 and the vertices extends inward at the overhang 580 on either side of the peak undulation to form interlocking surfaces 586A and 586B.

25 A shown in FIG. 18A, peak undulation 590 is disposed between peak undulations 592 and 594. The overhangs of the head portion of peak undulation 590

are disposed past the overhangs of peak undulations 592 and 594 such that the interlocking surfaces of peak undulation 590 are engaged or in contact or can engage or make contact when the segments are expanded.

When crimped, the adjacent segments are mechanically held in a constant or 5 fixed relationship to each other both circumferentially and longitudinally. The adjacent segments are held through engagement of the interlocking surfaces of the head portions of the end rings. The adjacent rings overlap longitudinally a consistent amount.

Additionally, the segments are radially locked into place by the mechanical engagement of the head portions.

10 In addition, the crimped segments can move around tight bends in a vessel during delivery to the lesion site. Bending is accommodated at each segment to segment connection by a longitudinal space 596 between the head of each peak undulation and the side walls 598 of the end ring of the adjacent segment.

During balloon inflation, the diamond pattern will open up, for example, as 15 shown in FIG. 30, which shows an exemplary deployment of a segmented scaffold. In FIG. 30, each segment shortens and opens independently of other segments. This is in contrast to deployment of segments 570 and 572 of FIG. 18A. During the initial stages of inflation the several heads at the ends of each segment will stay mechanically engaged behind the heads of the adjacent segment, thus holding the segment to segment 20 relationship. As the segments are expanded further, the heads will move further apart circumferentially, as shown by arrows 599 in FIG. 18A, until they finally pass by each other with no more engagement near the fully deployed diameter. As a result, the natural longitudinal shortening of the diamonds in the segments and also the balloon lengthening which tends to increase the segment to segment gap during deployment 25 have less of a contribution to the final segment to segment gap.

Therefore, the mechanical restraint during deployment provides several advantages. The segment to segment longitudinal relationship is maintained intact for a longer period of time, for example, for a longer period of time during deployment. This results in controlled and consistent final segment to segment gaps. In addition, the 5 segment to segment circumferential relationship is maintained intact for a longer period of time. This results in less circumferential rotation of individual segments and thus a reduction in segment to segment collisions during vessel longitudinal compression. Reduction of collisions results in a reduced risk of vessel irritation, strut fracture, and emboli production.

10 FIGs. 19 and 20 depict alternative head designs. FIG. 19 depicts a portion 600 of an end ring of a segment with a head portion 602 and body portion 604. Line A-A is the longitudinal axis of the segment and line B-B is the circumferential direction. Overhangs 606 extend outward from body 604 with an angle  $A_H$  with respect to line B-B, rotated toward the segment. This alternate head design enhances the longitudinal 15 mechanical wedging interlocking effect of adjacent segments.

FIG. 20 depicts a portion 610 of an end ring of a segment with a head portion 612 and body portion 614. Line A-A is the longitudinal axis of the segment and line B-B is the circumferential direction. Overhangs 616 extend outward from body portion 614 with an angle  $B_H$  with respect to line B-B, rotated away from the segment. The 20 edges of the overhang at the head and body have radii of curvature  $R_1$  and  $R_2$ , respectively.  $R_1$  will always be slightly less than  $R_2$  so that in the crimped state the  $R_2$  of one segment will have clearance at  $R_1$  to the struts of the adjacent segment.  $R_2$  may be 1%, 10%, 20%, 50%, 100% or greater than 100% of the height of one side of the head from strut 614.

25 The alternate head design in FIG. 20 changes the mechanical characteristics of the head to head interaction. As  $R_1$  and  $R_2$  are varied, the diameter at which the

interlocked heads separate is changed. This results in changes in segment spacing at final deployment.

The scaffold segments may be crimped tightly on a delivery balloon using a crimping apparatus such as an iris crimper. The crimping process may include two stages, 5 a pre-crimping process and a final crimp process. In the pre-crimp process, the diameter of the scaffold segments are reduced to a diameter between the initial diameter and the balloon diameter prior to loading the scaffold segments on the balloon. The diameter of the segments can be reduced to the balloon diameter or 1 to 5 % greater than the balloon diameter. For example, the pre-crimping process can crimp segments from a diameter of 10 about 0.3 in to about 0.06 in.

The reason for the pre-crimp processes is to reduce the size of the scaffold segments to allow greater accuracy of loading the segments on the balloon with the desired degree of overlap or interlinking. A detailed discussion of a pre-crimping process for segmented scaffolds can be found in U.S. Patent Application No. 13/441,756.

15 In the pre-crimping process, the scaffold segments in an as-fabricated condition are placed over a mandrel and arranged end to end. The scaffold segments are spaced apart axially. The distance between the segments may be such that when the segments are reduced to the pre-crimp diameter the segments do not make contact with each other. For example, the scaffold segments are placed over a stepped mandrel. The mandrel with the 20 scaffold segments is loaded into the pre-crimper, for example, an iris crimper and crimped to the pre-crimp diameter. The pre-crimped scaffold segments may further be placed inside a protective sheath disposed in an outer surface of the each scaffold segment.

The pre-crimped segments may then be loaded onto a balloon in a deflated state. The segments are placed over the balloon and arranged so that adjacent segments have 25 a certain degree of overlap, for example, between 50 and 100%, or more narrowly, 50 to 60%, 60 to 70%, 70 to 80%, 80 to 90%, or 90 to 100%. The segments and balloon

are then crimped down with pressure. The pressure may be applied at multiple steps with a dwell period between steps to achieve segment retention on the balloon. The balloon may be removed from the crimper one or more times, the removed segments pushed together to obtain a desired overlap and placed back into the crimper. Pressure 5 may be applied to the balloon during the final stages of the crimp process to enhance the scaffold retention to the balloon in the crimped state. When the catheter is removed from the crimper a protective sheath may be placed over the scaffold segments.

Further embodiments of the present invention reduce or eliminate torsional or extension-compression forces on the rings of a scaffold and additionally address the 10 sagging of vessel walls between scaffold segments. The embodiments can include scaffolds that are composed of segments that are not connected by linking elements or are connected by some linking elements.

In these embodiments, a scaffold having a plurality of segments in a crimped reduced configuration has at least one discontinuous linking element between adjacent 15 segments. The scaffold can be crimped over a delivery balloon. The discontinuous linking elements extend from end of adjacent segments, however, do not connect the adjacent segments due to a discontinuity in the linking element located between the adjacent segments. Since the discontinuous linking elements do not connect the adjacent elements, the propagation of forces between the adjacent rings is reduced or 20 eliminated. As a result, the scaffold is more fatigue and fracture resistant. Additionally, since the discontinuous link is structurally intact except for the discontinuity, the link can help support the lumen wall between segments once the scaffold is deployed in a vessel.

FIG. 21 depicts a close-up view of a discontinuous linking element 700 between 25 scaffold segment 702 and scaffold segment 704. Discontinuous linking segment 700 includes a portion 706 connected to segment 702 and a portion 708 that is connected to

segment 704. Linking strut 700 has a discontinuity, gap, or space 710 with a length  $L_{disc}$  between the free ends of portion 706 and 708.  $L_{disc}$  may be very small, for example, between 1 and 5 microns. In general, the width may be 2 to 5, 5 to 10, 10 to 50 microns, or greater than 50 microns.

5 In some embodiments, the scaffold has no linking elements between adjacent segments that connect adjacent segments with only discontinuous linking elements between segments so that all segments are disconnected. Adjacent segments may have 1, 2, 3, 4, 5 or more discontinuous linking elements between adjacent segments. FIG. 22 depicts a two-dimensional projection of adjacent scaffold segments that are 10 disconnected. As shown in FIG. 22, scaffold segments 710, 712, and 714 are arranged end to end. Discontinuous linking elements 716 and 718 are between segments 710 and 712. Discontinuous linking elements 720 and 722 are between segments 712 and 714.

15 In other embodiments, the scaffold includes adjacent segments that are connected by at least one intact linking element. Therefore, adjacent scaffold segments are connected by at least one intact linking element and also include at least one discontinuous linking element.

FIG. 23 depicts a two-dimensional projection of adjacent scaffold segments that include both intact and discontinuous linking elements. As shown in FIG. 23, scaffold 20 segments 730, 732, and 734 are arranged end to end. Scaffold segments 730 and 732 are connected by intact linking element 736 and scaffold segments 732 and 734 are connected by intact linking element 742. Discontinuous linking element 738 is between scaffold segments 730 and 732. Discontinuous linking element 740 is between scaffold segments 732 and 734.

25 In some embodiments, the intact linking elements can be frangible or designed to fail. Frangible linking elements have weakened portions that facilitate fracture or

breaking of the linking element after the scaffold is deployed. Prior to fracture, the frangible linking element provides stability to the scaffold during crimping and for a time after deployment. However, at some time after deployment the frangible linking elements fracture or break at the weakened portion, disconnecting scaffold segments 5 which then prevents transfer of forces between segments. Features that facilitate fracture include a narrowed portion of the linking element, such as notch, or holes through a linking element. Scaffolds disclosing frangible linking elements with various types of weakened portions are disclosed in US2011/0066225 and US2012/0065722.

10 The scaffold segments can have any structure or pattern. For example, the scaffold segments can have the structure of a plurality of rings composed of diamond-shaped elements formed of struts such as the exemplary scaffold segment depicted in FIG. 3A. Additionally, the segments can have a structure composed of cylindrical undulating or sinusoidal rings with alternating crests or peaks with the rings connected by linking elements, as depicted in FIG. 1.

15 FIG. 24 depicts a close-up view of a region between segments 750 and 752, like those shown in FIG. 3A. The segments are shown in an expanded configuration rather than in a crimped configuration for ease of illustration. As shown, two discontinuous linking elements 754 and two intact linking segments 756 are disposed between segments 750 and 752. The number and arrangement of the intact and discontinuous 20 linking elements is exemplary and any number and arrangement of linking elements between the ends of the segments is possible. In the example shown, one end of a linking element is connected to a trough of segment 750 and the other end is connected to a peak of segment 752. Alternatively, one end of a linking element can be connected to a peak of segment 750 and the other end may be connected to a trough of segment 752. In another alternative, segments 750 and 752 can be rotated relative to one 25 another by one cell and one end of a linking element can be connected to the peak (or

trough) of one segment and the other end of the linking element can be connected to the peak (or trough) of the other segment.

FIG. 25 depicts a close-up view of a portion 760 of a scaffold like the one shown in FIG. 1. As shown in FIG. 25, two linking elements are between ring 762 and 5 764, a discontinuous linking element 766 and an intact linking element 768.

Alternatively, both rings can be discontinuous linking elements so that the two rings are disconnected.

The scaffold of FIG. 1 is not designed specifically for use as a segmented scaffold, i.e., there are no pre-defined segments as in the segments of FIG. 3A. 10 However, sets of rings can be identified as segments, where a set is one or more rings, e.g., rings 106 and 108 in FIG. 1. Discontinuous linking elements can be between every ring, every other ring, every third ring, etc., to form segments of one ring, two rings, three rings, etc. Segments can be connected by including at least one intact linking element. Segments can be disconnected by having no intact linking elements. 15 Segments can be disconnected on both ends.

FIG. 26 depicts pattern 770 which is pattern 100 from FIG. 1 with one discontinuous linking element and one intact linking element between each ring. FIG. 27 depicts pattern 772 which is pattern 100 from FIG. 1 with one discontinuous linking element and one intact linking element at every third segment gap, as shown by the 20 arrows. The segments consist of three rings.

In some embodiments, the disconnected linking elements may be arranged in a pattern along the length of the scaffold. Between the first end and second end of the scaffold, the disconnected linking elements may be offset circumferentially from one segment gap to the next. For example, the discontinuous linking elements can form a 25 helical pattern. Offsetting the discontinuous linking elements tends to make the scaffold more stable once implanted. FIG. 28 depicts segmented scaffold 780, which is

scaffold 340 from FIG. 4 with two intact linking elements and two discontinuous linking elements between each segment. Discontinuous linking elements 781-786 are offset circumferentially from gap to gap to form a helical pattern.

A scaffold with discontinuous linking elements can be formed from a scaffold 5 with intact linking elements in a crimped reduced configuration. Scaffolds such as pattern or scaffold 100 in FIG. 1, pattern or scaffold 780 of FIG. 28 (with all linking elements intact) can be formed by laser machining a tube in an expanded configuration. The scaffold may then be crimped or pre-crimped to a reduced configuration. The discontinuous linking elements can be formed by laser cutting the selected linking 10 elements.

The laser cutting can be performed with the scaffold crimped over a delivery balloon. Alternatively, the laser cutting can be performed with the scaffold crimped over a mandrel or some other support to prevent damage of the balloon by the laser. The scaffold may then be removed from the support and crimped over a delivery 15 balloon. In another alternative, the scaffold may be crimped over delivery balloon with a protective sheath over the balloon to protect the balloon from the laser cutting. After laser cutting to create the discontinuous links, the protective sheath can be removed from the balloon by allowing a slight recoil in the scaffold and pulling off the sheath.

A further aspect of the present invention is variation of width of linking 20 elements along the longitudinal axis. The variation in linking elements can include variation of width of intact linking elements and discontinuous linking elements. Certain sections of scaffold may be more susceptible to fracture from radial compression, torsion, flexion, and axial extension and compression. It is expected that the susceptibility to strut fracture depends on strut width. Therefore, the width of 25 linking struts can account for the difference in the forces along the axis of the scaffold.

In these embodiments, the width of linking elements at segment gaps at the ends of a scaffold can be greater or less than the widths in a middle section. In an exemplary embodiment, the width of the linking elements at gaps at the two ends, gaps 790 and 791 and gaps 794 and 795 can be greater than the widths of the linking elements in 5 gaps 792 and 793. The larger strut widths can be 10 to 100% larger, or more narrowly, 10 to 30%, 20 to 50%, or 40 to 80% larger.

The scaffold segments of the present invention can be made from variety of biodegradable polymers including, but not limited to, poly(L-lactide) (PLLA), polymandelide (PM), poly(DL-lactide) (PDLLA), polyglycolide (PGA), 10 polycaprolactone (PCL), poly(trimethylene carbonate) (PTMC), polydioxanone (PDO), poly(4-hydroxy butyrate) (PHB), and poly(butylene succinate) (PBS). The scaffold segments can also be made from random and block copolymers of the above polymers, in particular, poly(L-lactide-co-glycolide) (PLGA) and poly(L-Lactide-co-caprolactone) PLGA-PCL. The scaffold can also be made of a physical blending of the above 15 polymers. The scaffold segments can be made from PLGA including any molar ratio of L-lactide (LLA) to glycolide (GA). In particular, the stent can be made from PLGA with a molar ratio of (LA:GA) including 85:15 (or a range of 82:18 to 88:12), 95:5 (or a range of 93:7 to 97:3), or commercially available PLGA products identified as having 20 these molar ratios. High strength, semicrystalline polymers with a Tg above body temperature include PLLA, PGA, and PLGA.

“Radial strength” is the ability of a stent to resist radial compressive forces, relates to a stent's radial yield strength and radial stiffness around a circumferential direction of the stent. A stent's “radial yield strength” or “radial strength” (for purposes of this application) may be understood as the compressive loading, which if exceeded, 25 creates a yield stress condition resulting in the stent diameter not returning to its unloaded diameter, i.e., there is irrecoverable deformation of the stent. When the radial

yield strength is exceeded the stent is expected to yield more severely as only minimal additional force is required to cause major deformation. “Stress” refers to force per unit area, as in the force acting through a small area within a plane. Stress can be divided into components, normal and parallel to the plane, called normal stress and shear stress, 5 respectively. Tensile stress, for example, is a normal component of stress applied that leads to expansion (increase in length). In addition, compressive stress is a normal component of stress applied to materials resulting in their compaction (decrease in length). Stress may result in deformation of a material, which refers to a change in length. “Expansion” or “compression” may be defined as the increase or decrease in 10 length of a sample of material when the sample is subjected to stress.

As used herein, the terms “axial” and “longitudinal” are used interchangeably and refer to a direction, orientation, or line that is parallel or substantially parallel to the central axis of a stent or the central axis of a tubular construct. The term “circumferential” refers to the direction along a circumference of the stent or tubular 15 construct. The term “radial” refers to a direction, orientation, or line that is perpendicular or substantially perpendicular to the central axis of the stent or the central axis of a tubular construct and is sometimes used to describe a circumferential property, i.e., radial strength.

“Strain” refers to the amount of expansion or compression that occurs in a 20 material at a given stress or load. Strain may be expressed as a fraction or percentage of the original length, i.e., the change in length divided by the original length. Strain, therefore, is positive for expansion and negative for compression.

“Strength” refers to the maximum stress along an axis which a material will 25 withstand prior to plastic deformation and then fracture. The ultimate strength is calculated from the maximum load applied during the test divided by the original cross-sectional area.

“Modulus” may be defined as the ratio of a component of stress or force per unit area applied to a material divided by the strain along an axis of applied force that result from the applied force. For example, a material has both a tensile and a compressive modulus.

5 The underlying structure or substrate of an implantable medical device, such as a stent can be completely or at least in part made from a biodegradable polymer or combination of biodegradable polymers, a biostable polymer or combination of biostable polymers, or a combination of biodegradable and biostable polymers. Additionally, a polymer-based coating for a surface of a device can be a biodegradable polymer or 10 combination of biodegradable polymers, a biostable polymer or combination of biostable polymers, or a combination of biodegradable and biostable polymers.

Examples:

FIG. 29 is an image of an interlinked segmented scaffold in a deployed state from a bench test. The middle segment is an off-set segment. As shown from the 15 figure, there is no axial section all the way around the vessel wall that is not supported by a segment. Additionally, there is no sagging of the vessel wall inward the lumen in between the segments as is shown for the segmented scaffolds in FIG. 6. The vessel wall in FIG. 29 appears to be supported uniformly at the scaffold diameter along the entire length of the segmented scaffold.

20 FIG. 30 depicts images of an interlinked segmented scaffold composed of two segments. Diamonds are omitted only from one end of each segment. The uppermost image depicts the interlinked segments in a fully crimped state over a delivery balloon. The middle image depicts the interlinked segments in a semi-expanded state. The nonuniform or uneven expansion at the ends is due to the characteristic behavior of 25 delivery balloons of inflating first at the ends. The degree of engagement of the segments increases from the crimped to the semi-expanded state. The uneven

expansion causes sliding of the segments together which increases the engagement. The bottom image is the fully expanded scaffold showing the interlinking of the segments.

FIG. 31 depicts images of interlinked segmented scaffolds composed of three in-line segments. The uppermost image depicts the three interlinked segments in a fully crimped state over a delivery balloon. The next two images depict the three interlinked segments undergoing uneven expansion. The next two images depict the three interlinked segments close to full expansion. The bottom image is the fully expanded scaffold showing the interlinking of the middle segment with the end segments. The end segments were observed not so slide on the balloon during the uneven expansion.

FIG. 32 depicts images of an interlinked segmented scaffold composed of three off-set segments. The uppermost image depicts the three interlinked segments in a fully crimped state over a delivery balloon. The next two images depict the three interlinked segments undergoing uneven expansion. The next two images depict the three interlinked segments close to full expansion. The bottom image is the fully expanded scaffold showing interlinking of the middle segment with the end segments. The end segments were observed not so slide on the balloon during the uneven expansion. The segments end tips were in-line at full expansion.

FIG. 33 depicts images of an interlinked scaffold segmented composed of six in-line segments. The uppermost image depicts the five interlinked segments in a fully crimped state over a delivery balloon. The next two images depict the five interlinked segments undergoing uneven expansion. The fourth image depicts the five interlinked scaffolds close to full expansion. The bottom image is the fully expanded scaffold showing the interlinking adjacent segments. The segments were observed not so slide on the balloon during the uneven expansion.

While particular embodiments of the present invention have been shown and described, it will be obvious to those skilled in the art that changes and modifications can be made without departing from this invention in its broader aspects. Therefore, the appended claims are to encompass within their scope all such changes and modifications  
5 as fall within the true spirit and scope of this invention.

## WHAT IS CLAIMED IS:

1. A segmented scaffold comprising:

two or more radially expandable disconnected scaffold segments arranged end to end,

5 wherein each segment includes two or more undulating cylindrical rings composed of struts, and

wherein rings at an end of each segment comprise peak undulations projecting longitudinally outward from the end of the segment and comprise valley undulations extending longitudinally toward the segment, and

10 wherein the peak and valley undulations of adjacent rings overlap.

2. The scaffold of claim 1, wherein the overlap comprises that for each adjacent ring the peak undulations extending between the valley undulations.

3. The scaffold of claim 1, wherein the segments are in a reduced crimped state for delivery into a vessel.

15 4. The scaffold of claim 1, wherein the segments are in a reduced crimped state over a delivery balloon.

5. The scaffold of claim 1, wherein the undulating rings of each segment form a plurality of diamond-shaped cells, wherein at each end alternating diamonds around the rings are omitted to form peak and valley undulations having a longitudinal length that is a longitudinal length of a diamond-shaped cell.

20 6. The scaffold of claim 5, wherein the diamonds omitted at one end are longitudinally aligned with diamonds omitted at an opposite end.

7. The scaffold of claim 5, wherein the diamonds omitted at one end are not longitudinally aligned with diamonds omitted at the other end and are off-set circumferentially.

8. The scaffold of claim 1, wherein the peak undulations comprise a head portion at a peak of the peak undulation including an interlocking side wall surface extending circumferentially from the peak undulation, wherein the interlocking side wall surface of one ring is configured to engage a corresponding interlocking side wall surface of an adjacent ring when the segments are in a crimped state.

5 9. A method of delivering a scaffold:

providing a segmented scaffold crimped over a delivery balloon, the segmented scaffold comprising two or more radially expandable disconnected scaffold segments arranged end to end,

10 wherein each end of the segments comprises undulating cylindrical rings composed of struts and wherein undulations of adjacent segments overlap; and expanding the scaffold segments to a deployment diameter, wherein the undulations of the adjacent segments overlap at the deployed diameter.

10. The method of claim 9, further comprising placing the crimped segmented scaffold  
15 at a treatment site in a vessel.

11. The method of claim 10, wherein no longitudinal position at the treatment site completely around a vessel wall is unsupported by a scaffold segment.

12. A radially expandable scaffold segment comprising:

two or more connected undulating cylindrical rings composed of struts,  
20 wherein the undulating rings of each segment form a plurality of diamond-shaped cells with two pairs of opposing vertices, one pair being longitudinally aligned and one pair being circumferentially aligned,  
and

25 wherein alternating diamonds around at least one end ring are omitted to form peak and valley undulations along the at least one end ring with a longitudinal length that is a longitudinal length of the diamond-shaped cells.

13. The segment of claim 12, wherein the alternating diamonds are omitted around both end rings.
14. The segment of claim 13, wherein peaks of the undulations along one end ring are longitudinally aligned with peaks of the undulations along an opposite end ring.
- 5 15. The segment of claim 13, wherein peaks of the undulations at one end ring are longitudinally aligned with valleys of the undulations along an opposite end ring.
16. The segment of claim 13, wherein the diamonds omitted at one end are longitudinally aligned with diamonds omitted at an opposite end.
17. The segment of claim 13, wherein the diamonds omitted at one end are not longitudinally aligned with diamonds omitted at an opposite end, the omitted diamonds at the opposite end being off-set circumferentially.
18. The segment of claim 13, wherein the peak undulations of the at least one end ring comprise a head portion at a peak of the peak undulation including an interlocking side wall surface extending circumferentially from the peak undulation, wherein the 15 interlocking side wall surface is configured to engage a corresponding interlocking side wall surface of an adjacent ring when the segments are in a crimped state
19. A scaffold comprising:
  - a plurality of scaffold segments in a crimped reduced configuration; and
  - at least one discontinuous linking element between adjacent segments
- 20 20. The scaffold of claim 19, wherein the plurality of segments are positioned over a delivery balloon.
21. The scaffold of claim 19, wherein the scaffold comprises no linking elements that connect the adjacent segments.
- 25 22. The scaffold of claim 19, wherein the discontinuity is less than 10% of the length of the discontinuous linking elements.

23. The scaffold of claim 19, wherein the discontinuous linking elements between different adjacent segments are circumferentially offset.
24. The scaffold of claim 19, wherein discontinuous linking elements between different adjacent segments are circumferentially off-set such that the intact linking elements are arranged in a helical pattern from a first end of the scaffold to a second end of the scaffold.
- 5 25. The scaffold of claim 19, further comprising at least one intact linking element that connects adjacent segments.
26. The scaffold of claim 25, wherein the intact linking elements comprise a weakened portion that facilitates fracture of the intact linking element upon deployment of the scaffold.
- 10 27. A method of modifying a scaffold comprising:
  - providing a scaffold in a crimped reduced configuration, wherein the scaffold comprises longitudinal scaffold segments and linking elements connecting adjacent scaffold segments; and
  - 15 creating a discontinuity in at least one linking element between at least one set of adjacent segments.
28. The method of claim 27, wherein the discontinuity is created by laser cutting through the at least one linking elements.

**AMENDED CLAIMS**  
**received by the International Bureau on 21 September 2013 (21.09.2013)**

1. (amended) A segmented scaffold comprising:  
two or more radially expandable and disconnected polymer scaffold segments arranged end to end, wherein each segment includes two or more undulating cylindrical rings composed of struts, and  
wherein
  - a ring at an end of a first segment comprises peak undulations projecting longitudinally outward from the end of the segment,
  - a ring at an end of a second segment, arranged end to end with the first segment, comprises valley undulations disposed adjacent the ring of the first segment, and
  - wherein the peak and valley undulations overlap each other.
2. (amended) The scaffold of claim 1, wherein the overlap comprises each peak undulation extending between a pair of valley undulations.
3. (amended) The scaffold of claim 1, wherein the first and second segments are in a reduced crimped state for delivery into a vessel.
4. (amended) The scaffold of claim 1, wherein the first and second segments are in a reduced crimped state over a delivery balloon.
5. (Original) The scaffold of claim 1, wherein the undulating rings of each segment form a plurality of diamond-shaped cells, wherein at each end alternating diamonds around the rings are omitted to form peak and valley undulations having a longitudinal length that is a longitudinal length of a diamond-shaped cell.
6. (Original) The scaffold of claim 5, wherein the diamonds omitted at one end are longitudinally aligned with diamonds omitted at an opposite end.

7. (amended) The scaffold of claim 5, wherein the diamonds omitted at one end are not longitudinally aligned with diamonds omitted at the other end such that the omitted diamonds are off-set circumferentially.
8. (amended) The scaffold of claim 1, wherein the peak undulations comprise a head portion at a peak of the peak undulation including an interlocking side wall surface extending circumferentially from the peak undulation, wherein the interlocking side wall surface of the ring of the first segment is configured to engage a corresponding interlocking side wall surface of the ring of the second segment when the first and second segments are in a crimped state.
9. A method of delivering a scaffold:
  - providing a segmented scaffold crimped over a delivery balloon, the segmented scaffold comprising two or more radially expandable disconnected scaffold segments arranged end to end, wherein each end of the segments comprises undulating cylindrical rings composed of struts and wherein undulations of adjacent segments overlap; and
  - expanding the scaffold segments to a deployment diameter, wherein the undulations of the adjacent segments overlap at the deployed diameter.
10. The method of claim 9, further comprising placing the crimped segmented scaffold at a treatment site in a vessel.
11. The method of claim 10, wherein no longitudinal position at the treatment site completely around a vessel wall is unsupported by a scaffold segment.
12. A radially expandable scaffold segment comprising:
  - two or more connected undulating cylindrical rings composed of struts,
  - wherein the undulating rings of each segment form a plurality of diamond-shaped cells with two pairs of opposing vertices, one pair being longitudinally aligned and one pair being circumferentially aligned,
  - and

wherein alternating diamonds around at least one end ring are omitted to form peak and valley undulations along the at least one end ring with a longitudinal length that is a longitudinal length of the diamond-shaped cells.

13. The segment of claim 12, wherein the alternating diamonds are omitted around both end rings.

14. The segment of claim 13, wherein peaks of the undulations along one end ring are longitudinally aligned with peaks of the undulations along an opposite end ring.

15. The segment of claim 13, wherein peaks of the undulations at one end ring are longitudinally aligned with valleys of the undulations along an opposite end ring.

16. The segment of claim 13, wherein the diamonds omitted at one end are longitudinally aligned with diamonds omitted at an opposite end.

17. The segment of claim 13, wherein the diamonds omitted at one end are not longitudinally aligned with diamonds omitted at an opposite end, the omitted diamonds at the opposite end being off-set circumferentially.

18. The segment of claim 13, wherein the peak undulations of the at least one end ring comprise a head portion at a peak of the peak undulation including an interlocking side wall surface extending circumferentially from the peak undulation, wherein the interlocking side wall surface is configured to engage a corresponding interlocking side wall surface of an adjacent ring when the segments are in a crimped state

19. A scaffold comprising:  
a plurality of scaffold segments in a crimped reduced configuration; and  
at least one discontinuous linking element between adjacent segments comprising a discontinuity located between the adjacent segments.

20. The scaffold of claim 19, wherein the plurality of segments are positioned over a delivery balloon.
21. The scaffold of claim 19, wherein the scaffold comprises no linking elements that connect the adjacent segments.
22. The scaffold of claim 19, wherein the discontinuity is less than 10% of the length of the discontinuous linking elements.
23. The scaffold of claim 19, wherein the discontinuous linking elements between different adjacent segments are circumferentially offset.
24. The scaffold of claim 19, wherein discontinuous linking elements between different adjacent segments are circumferentially off-set such that the intact linking elements are arranged in a helical pattern from a first end of the scaffold to a second end of the scaffold.
25. The scaffold of claim 19, further comprising at least one intact linking element that connects adjacent segments.
26. The scaffold of claim 25, wherein the intact linking elements comprise a weakened portion that facilitates fracture of the intact linking element upon deployment of the scaffold.
27. A method of modifying a scaffold comprising:  
providing a scaffold in a crimped reduced configuration, wherein the scaffold comprises longitudinal scaffold segments and linking elements connecting adjacent scaffold segments; and  
creating a discontinuity in at least one linking element between at least one set of adjacent segments.

28. The method of claim 27, wherein the discontinuity is created by laser cutting through the at least one linking elements.

1 / 22

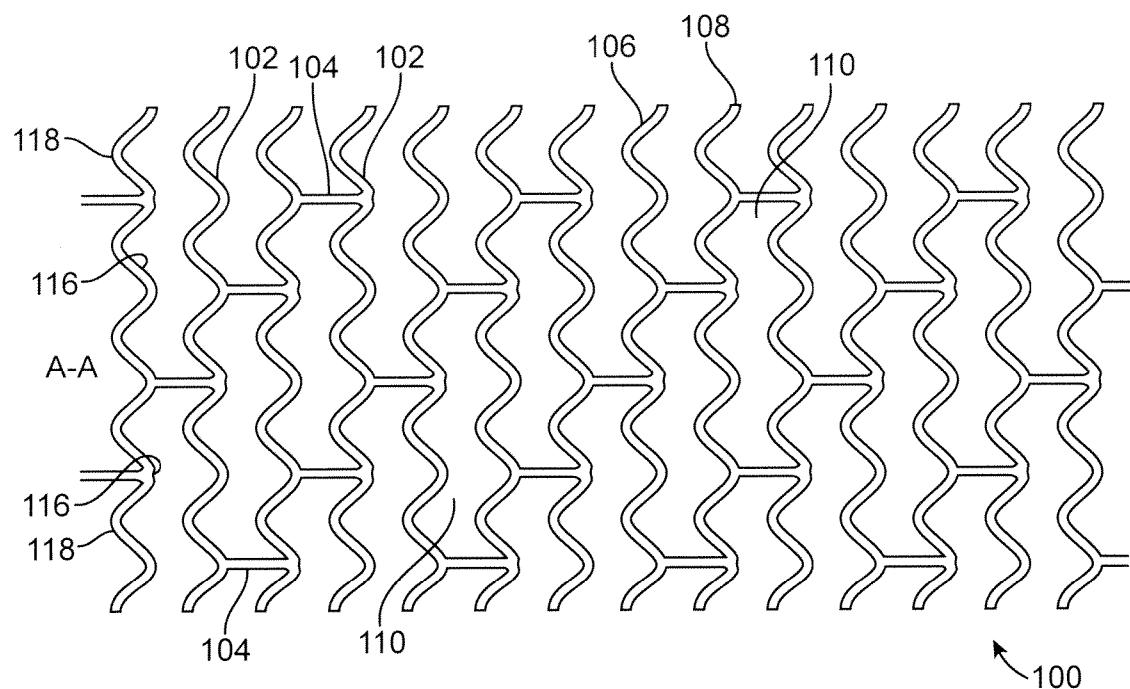


FIG. 1

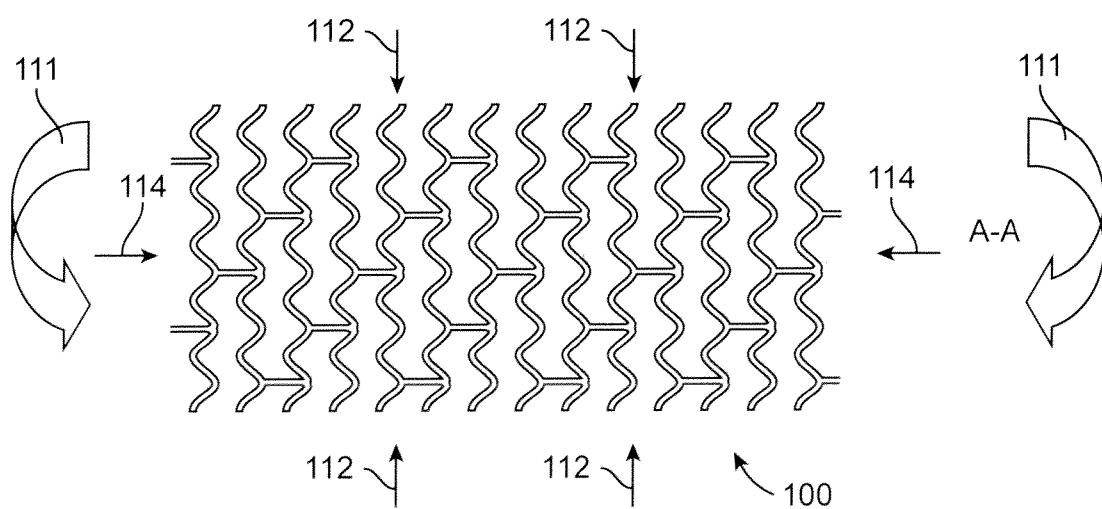


FIG. 2

2 / 22

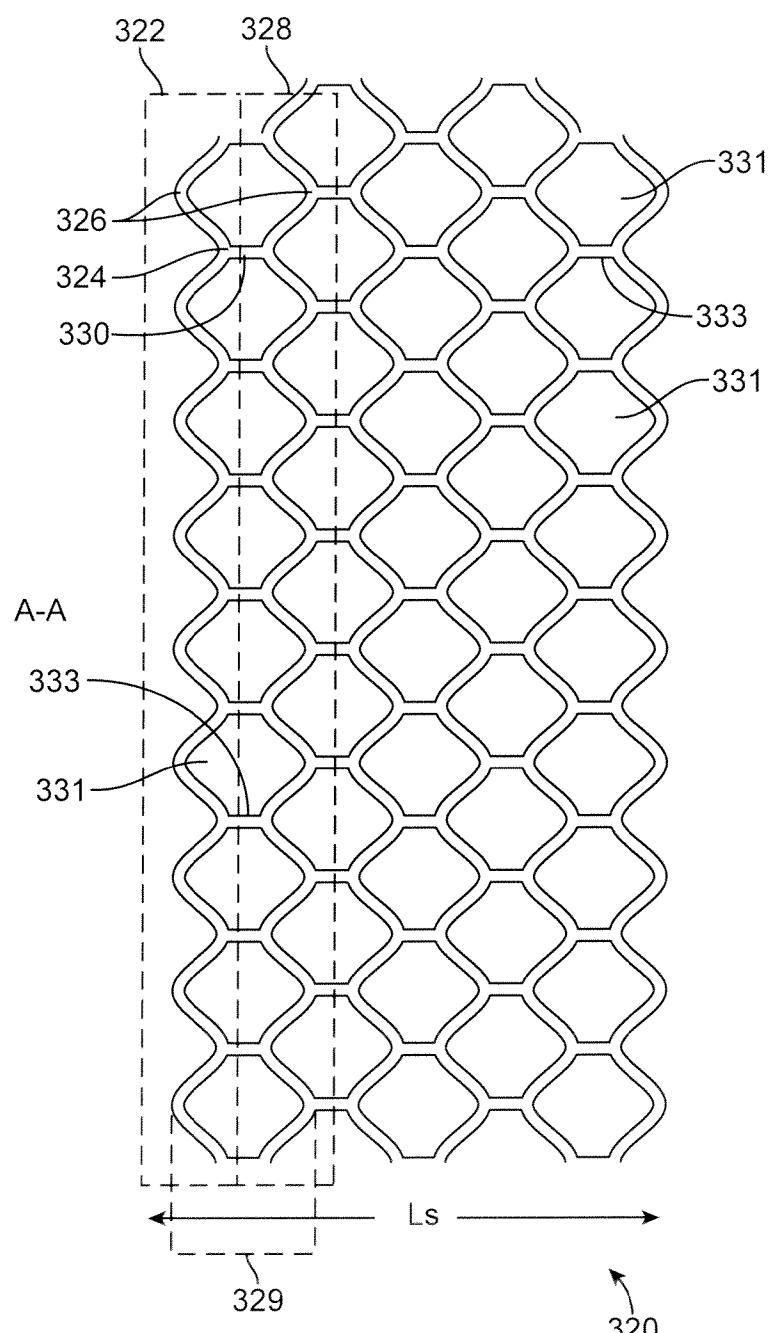


FIG. 3A

3 / 22

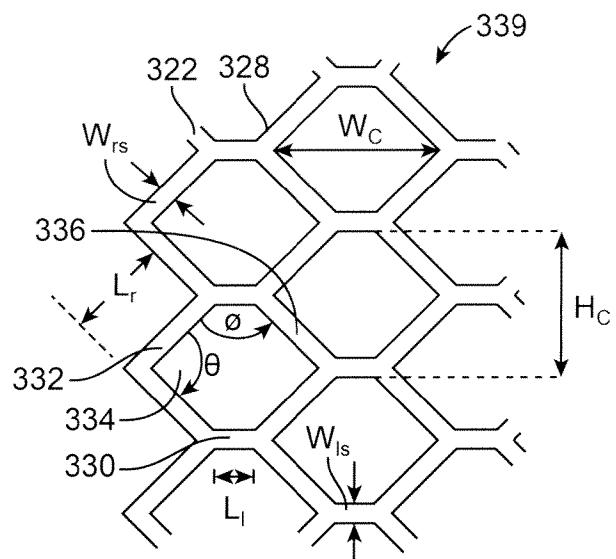


FIG. 3B

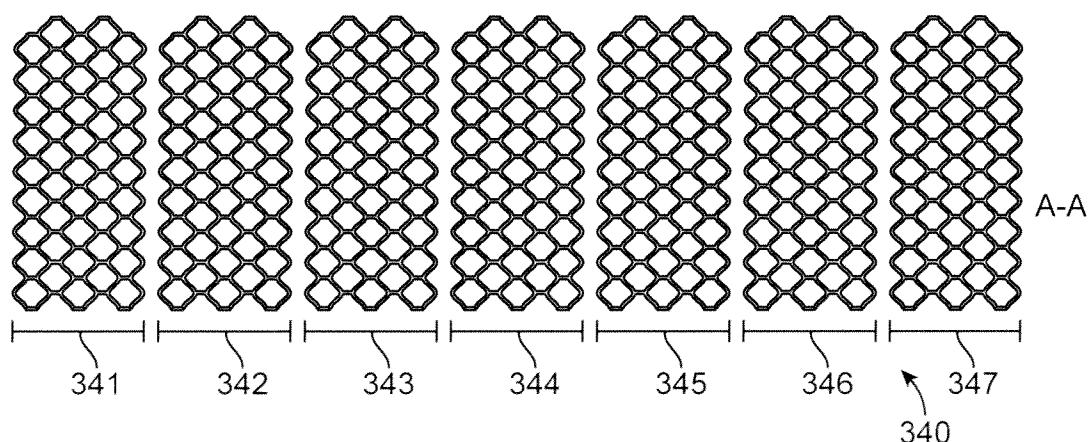


FIG. 4

4 / 22

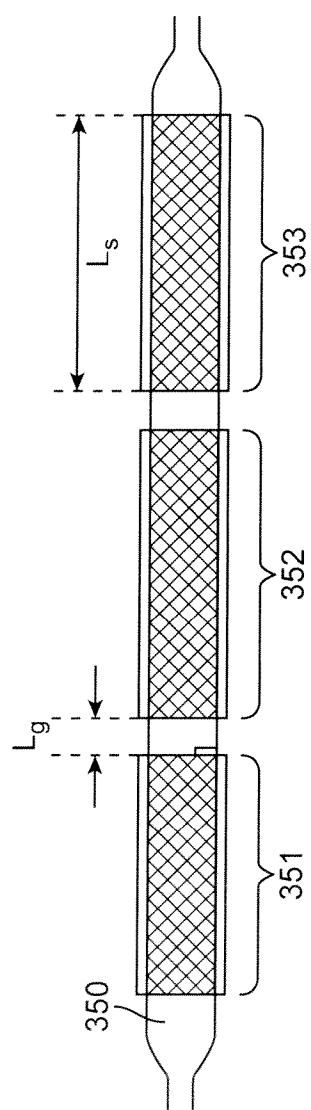


FIG. 5

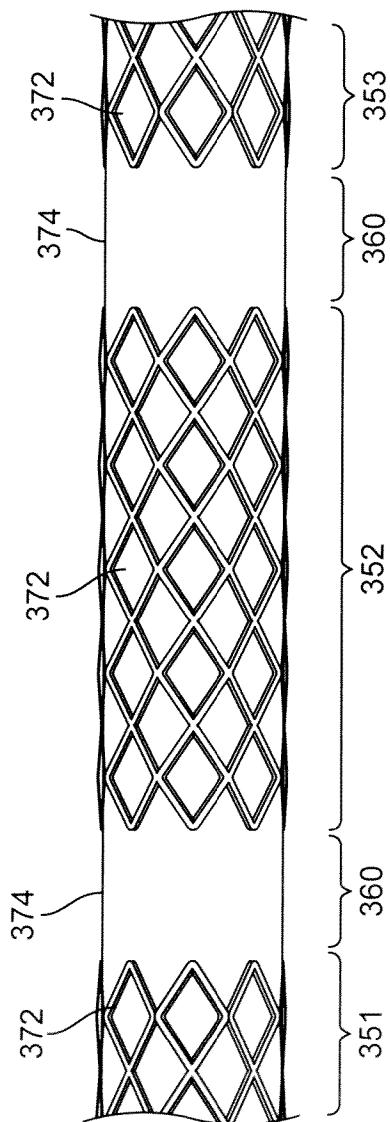


FIG. 6

5 / 22

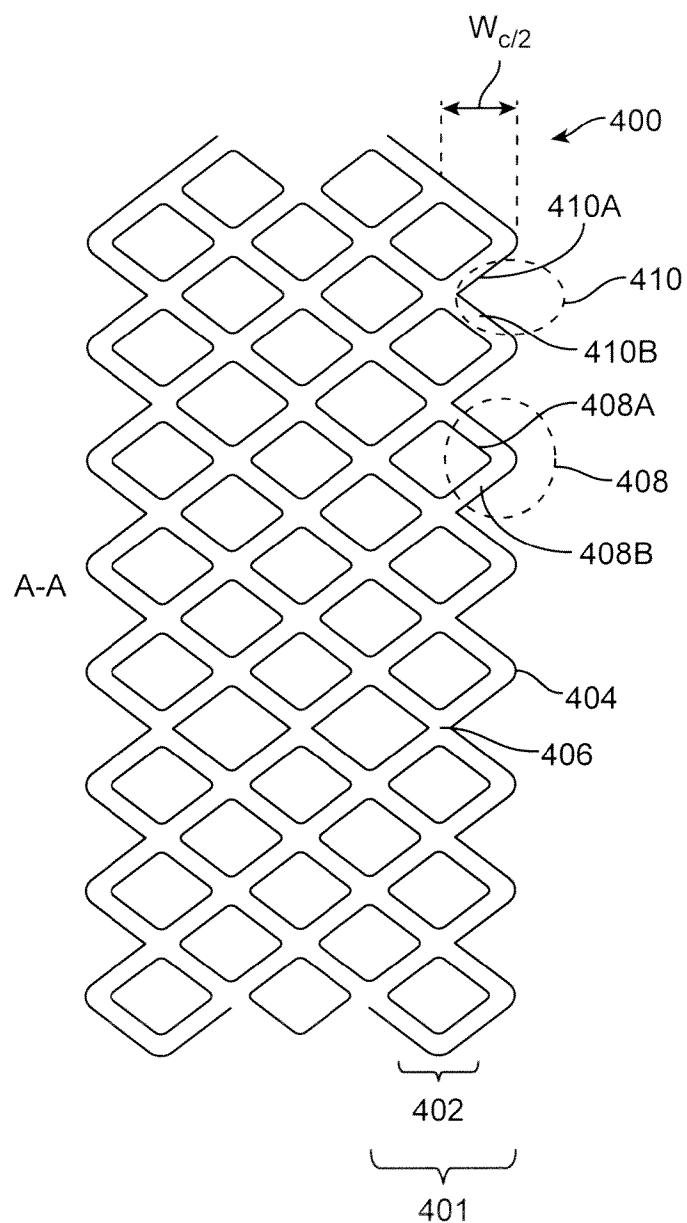


FIG. 7

6 / 22

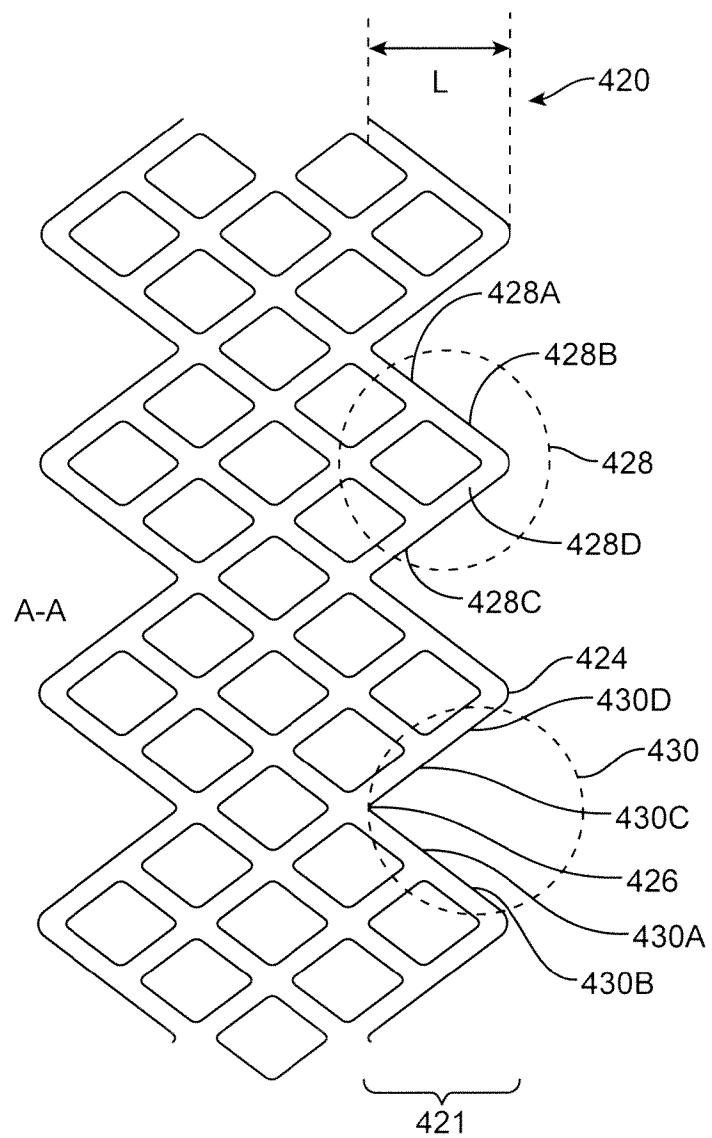


FIG. 8

7 / 22

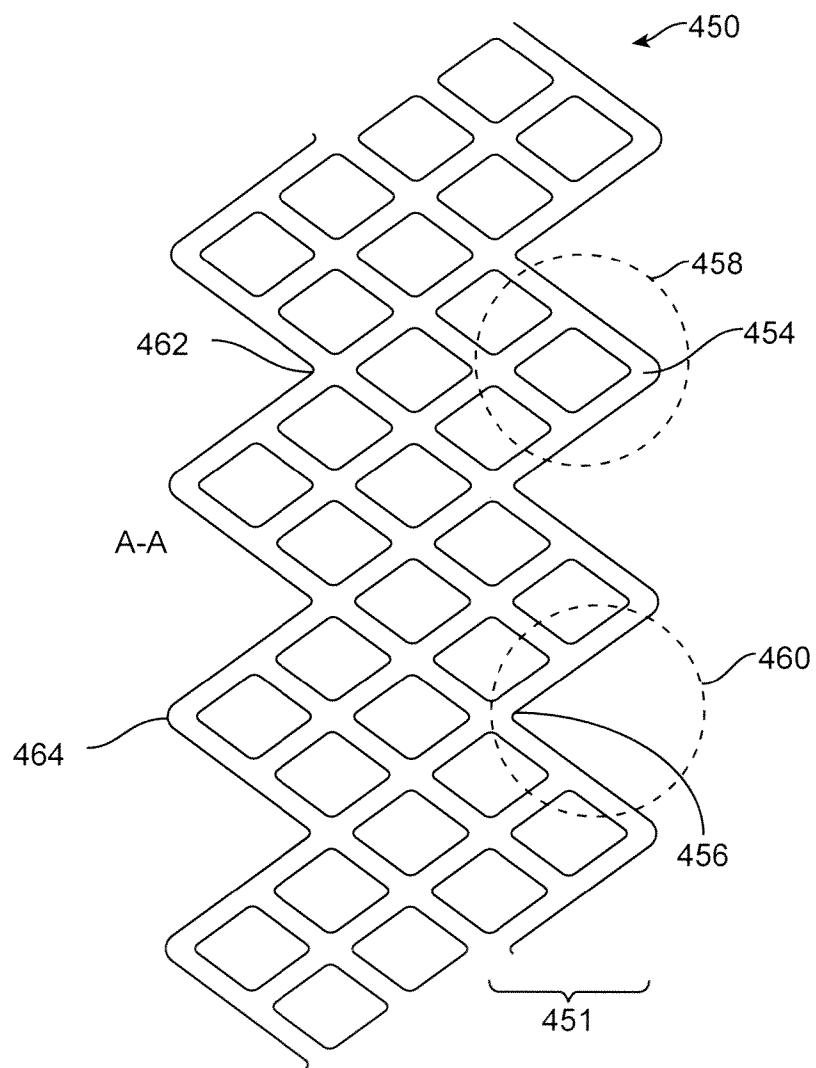


FIG. 9

8 / 22

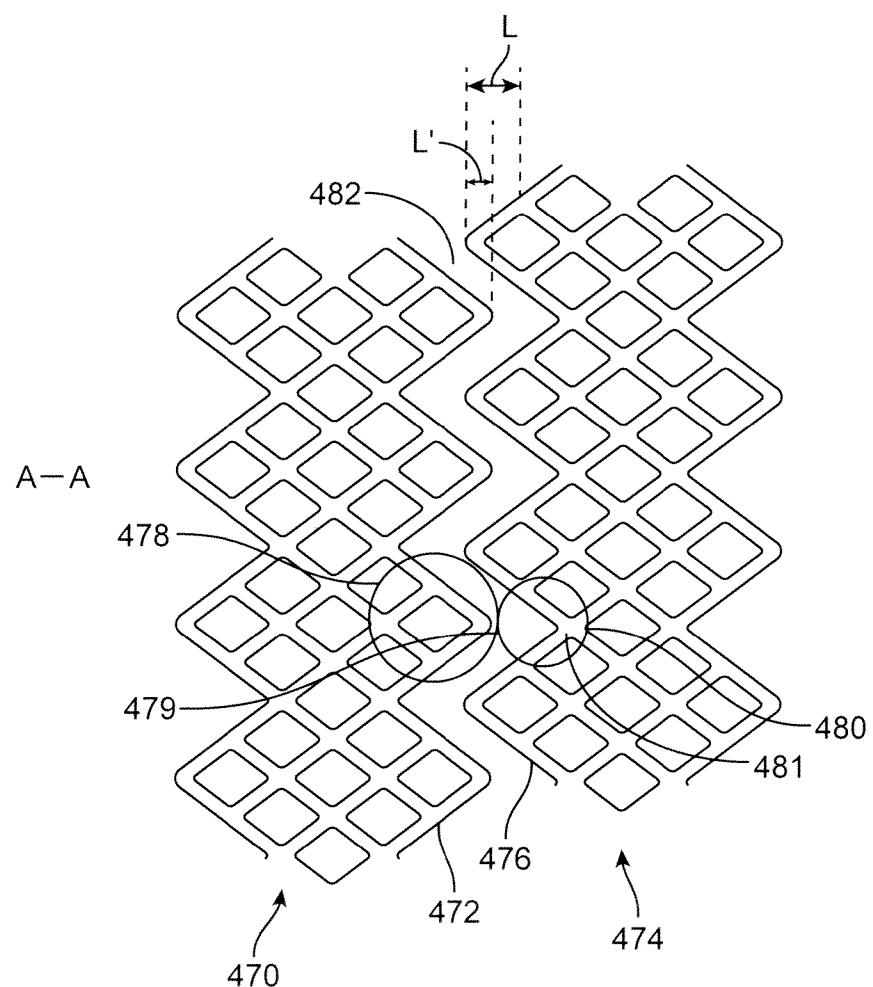


FIG. 10

9 / 22

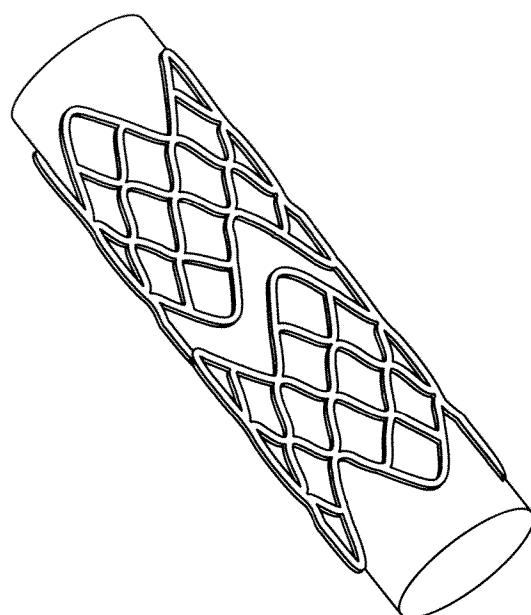


FIG. 11

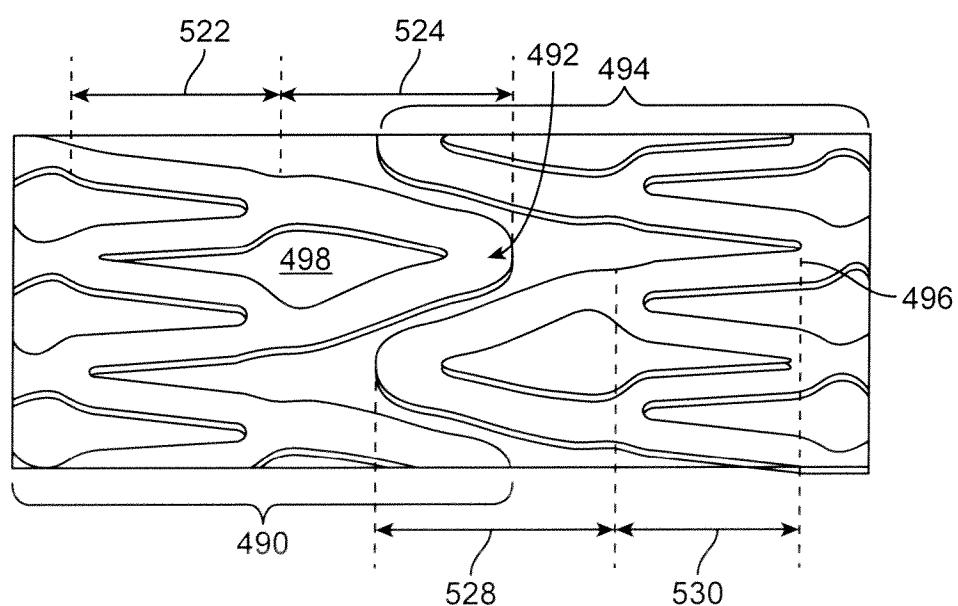


FIG. 12

10 / 22

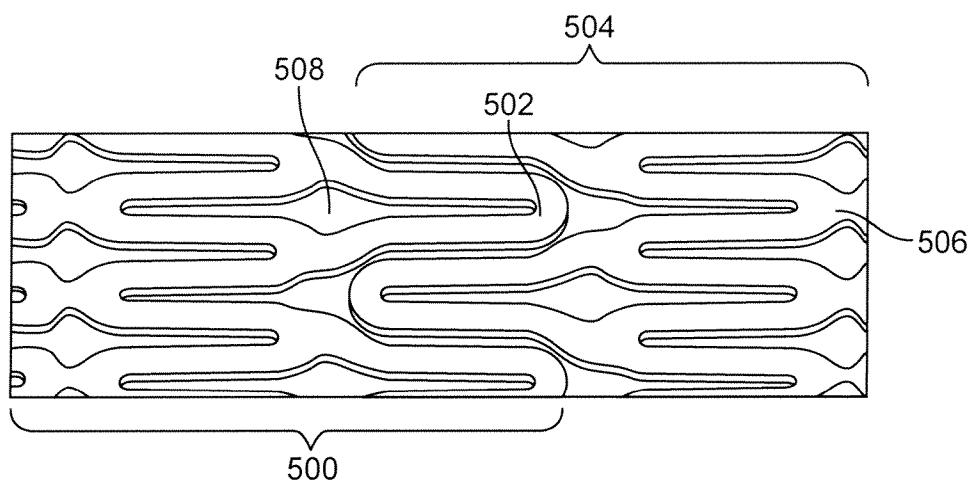


FIG. 13

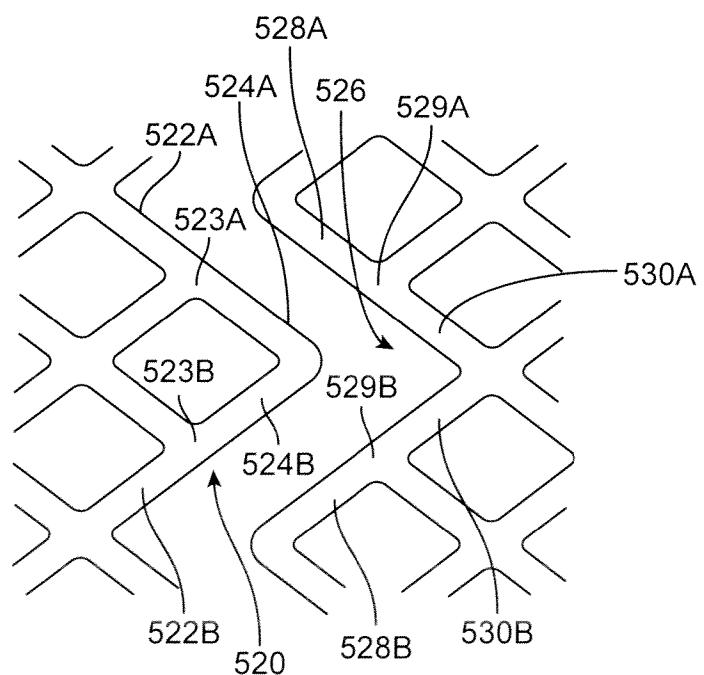


FIG. 14

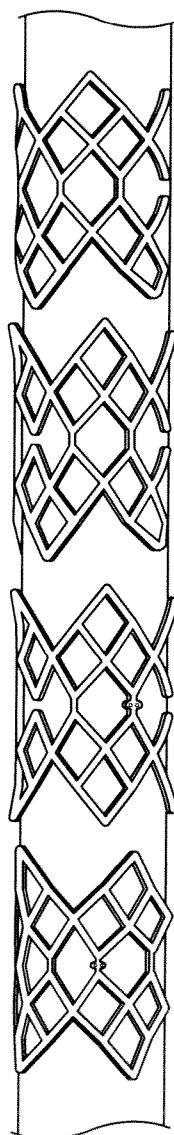


FIG. 15



FIG. 16

12 / 22

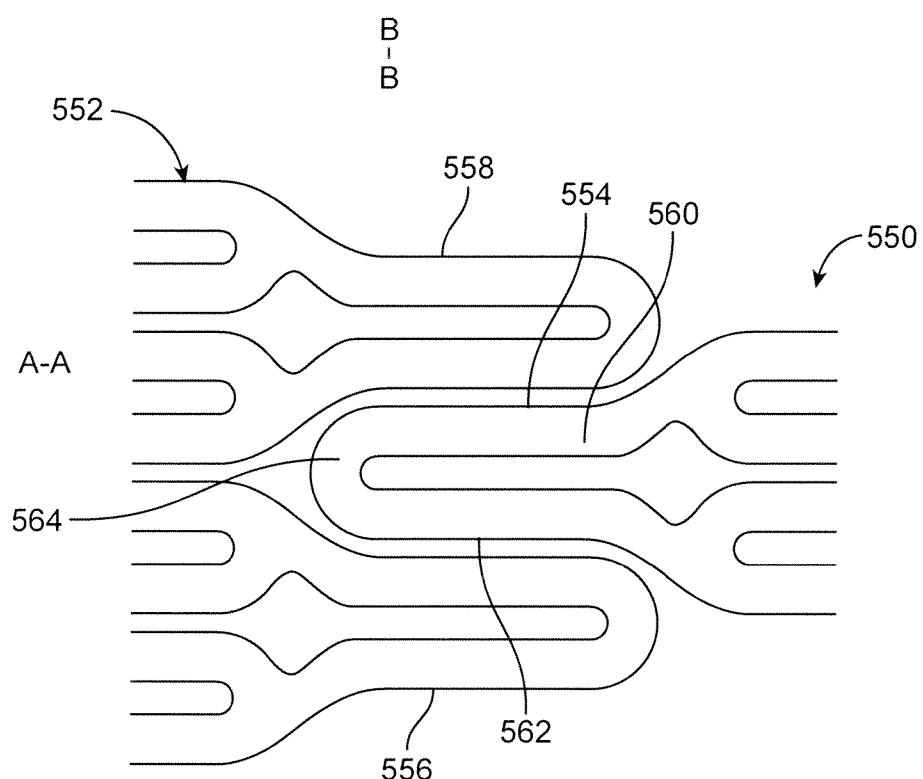


FIG. 17

13 / 22

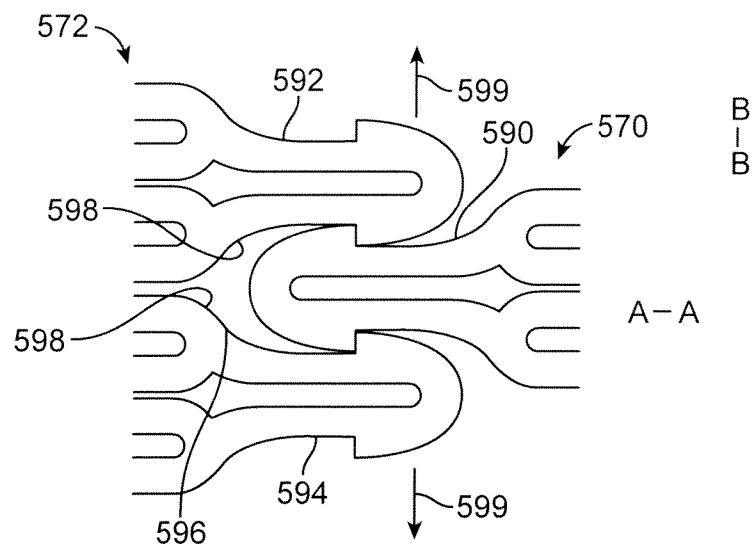


FIG. 18A

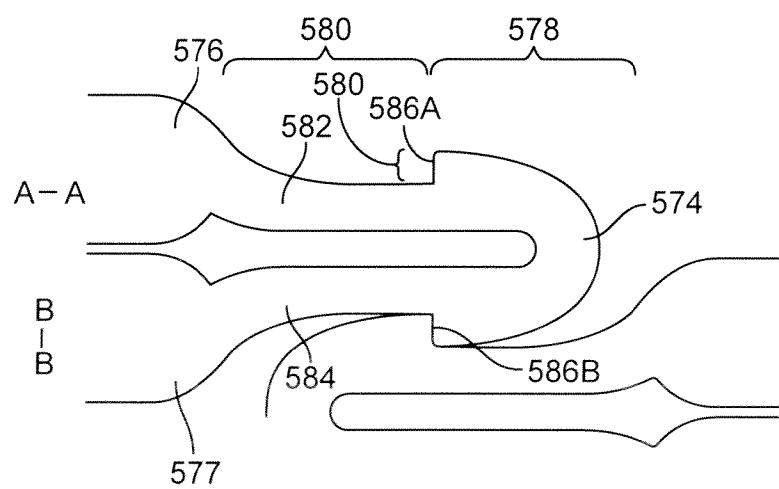


FIG. 18B

14 / 22

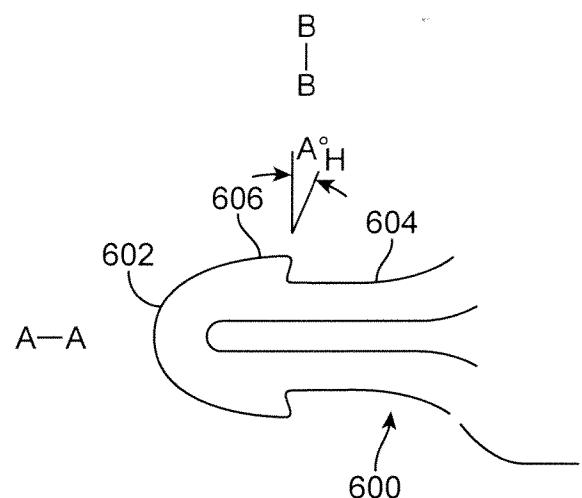


FIG. 19

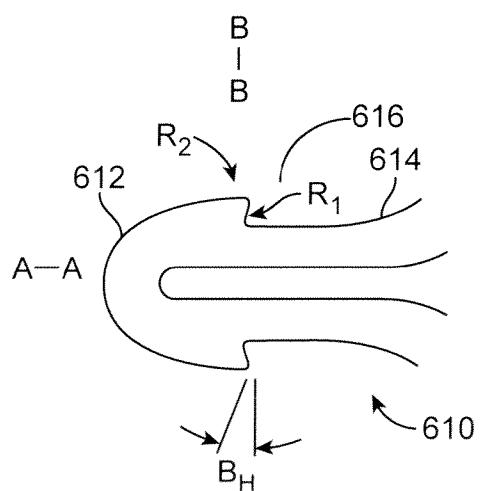


FIG. 20

15 / 22

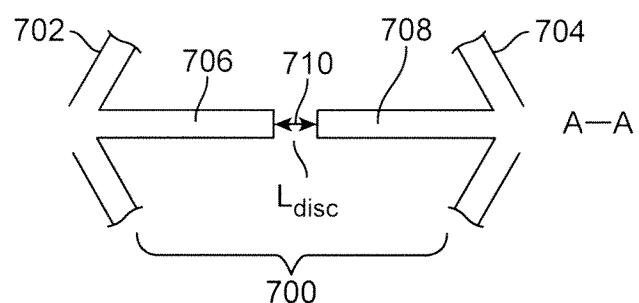


FIG. 21

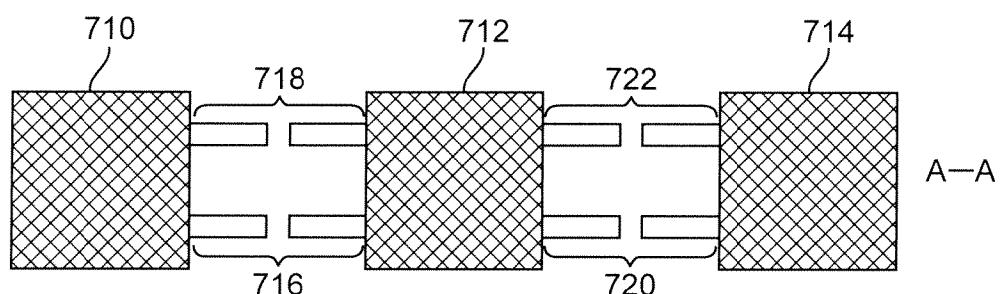


FIG. 22

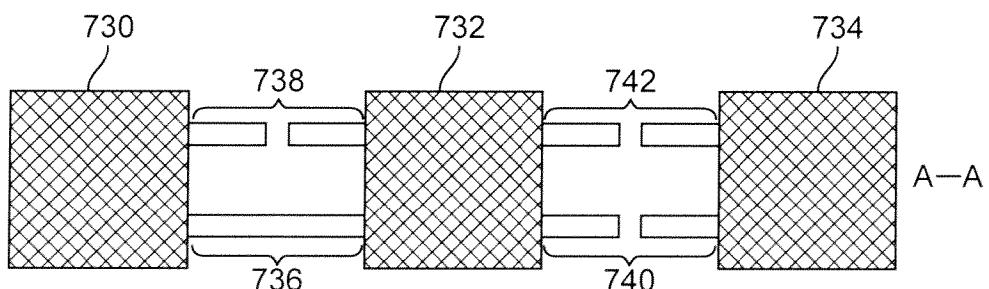


FIG. 23

16 / 22

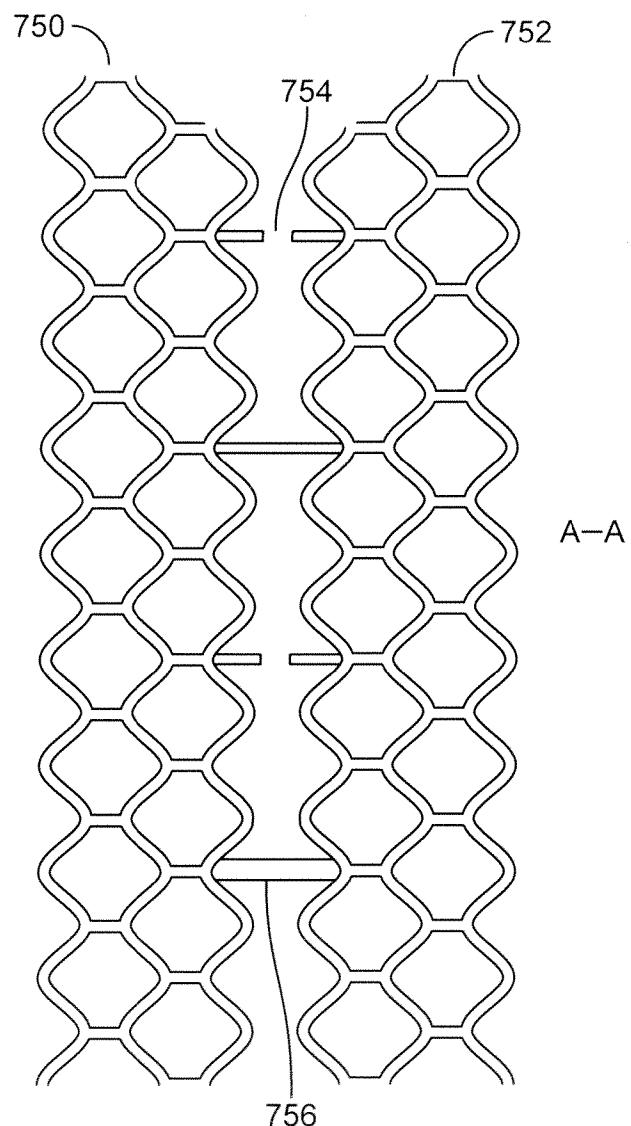


FIG. 24

17 / 22

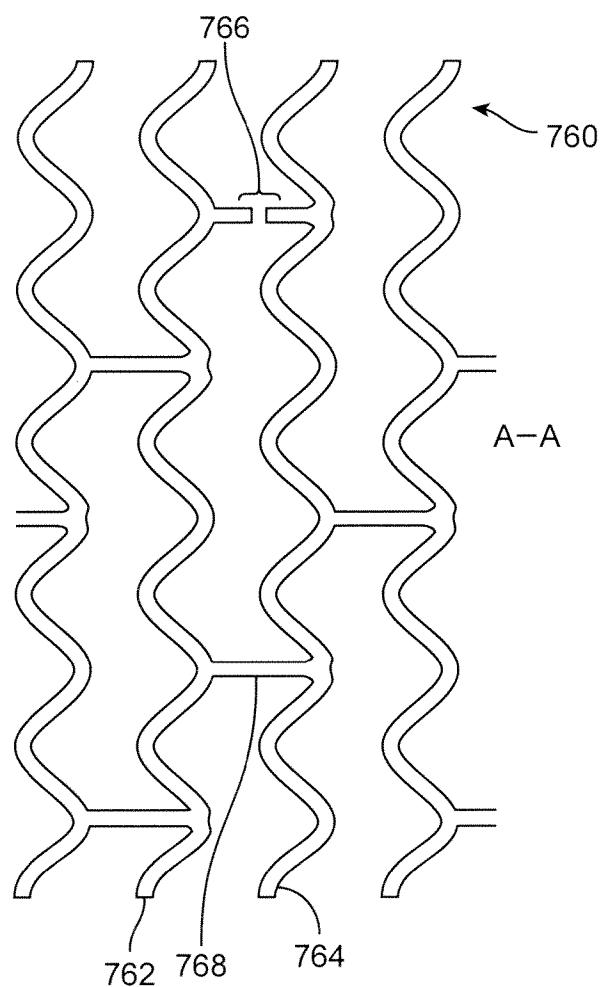


FIG. 25

18 / 22

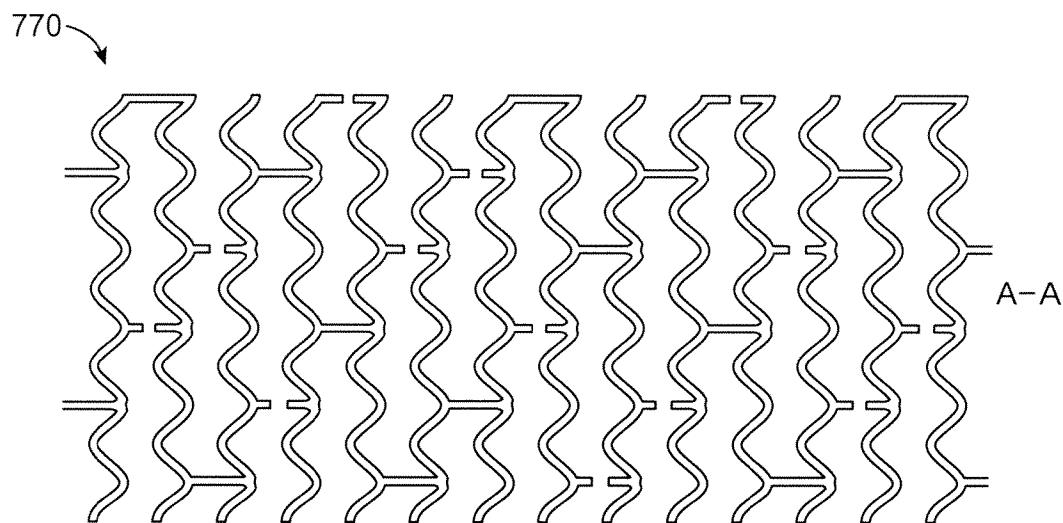


FIG. 26

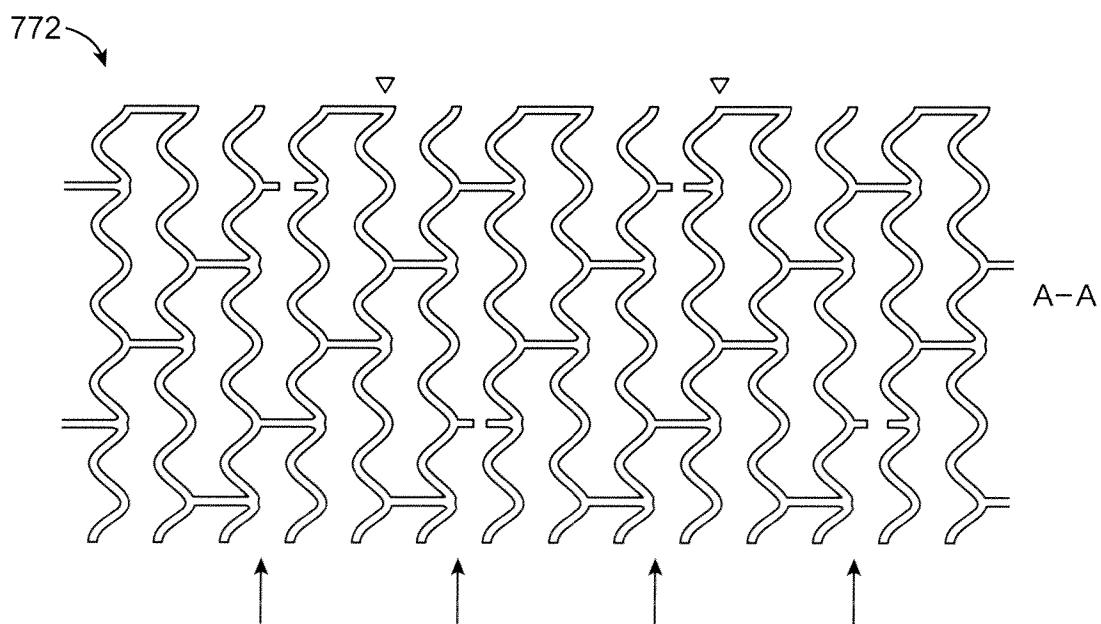


FIG. 27

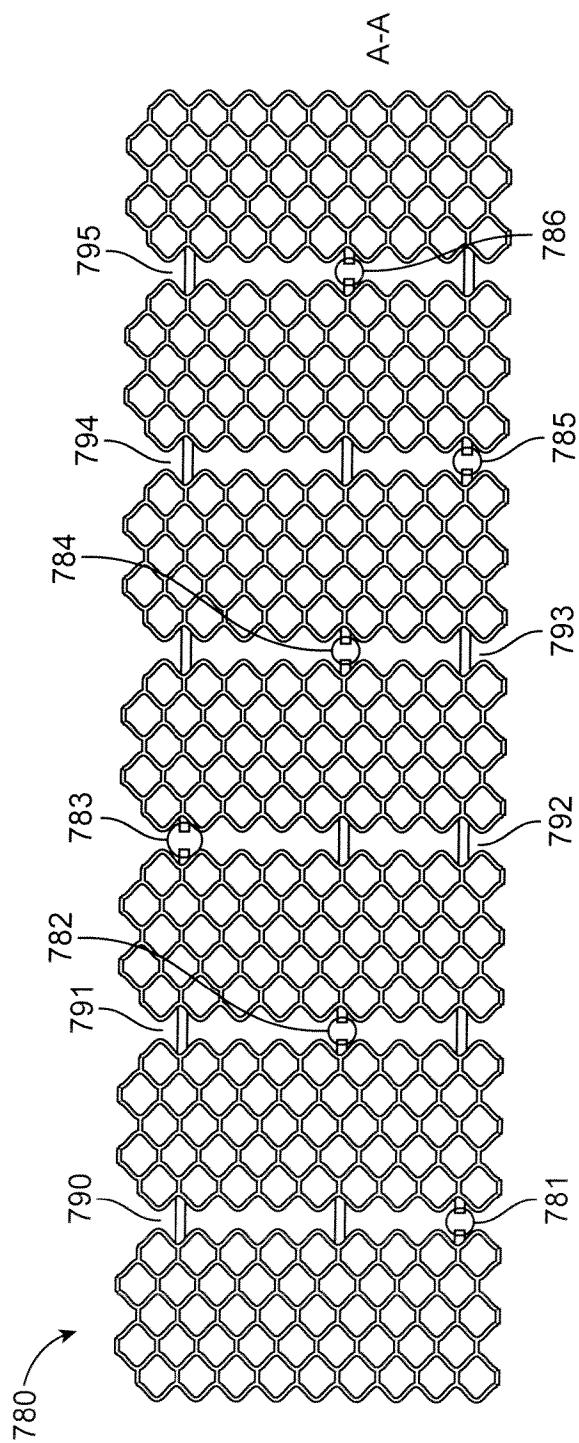


FIG. 28

20 / 22

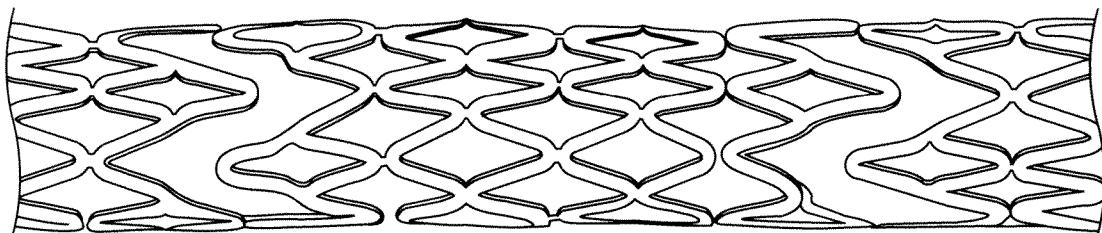


FIG. 29

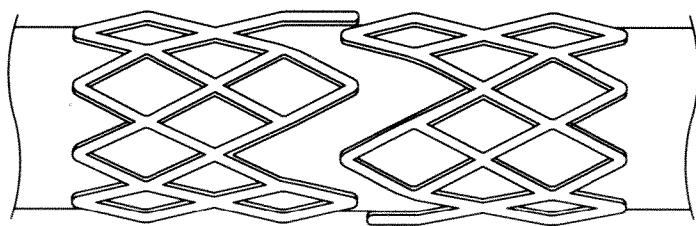
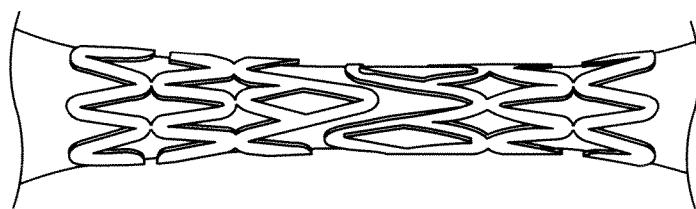



FIG. 30

21 / 22

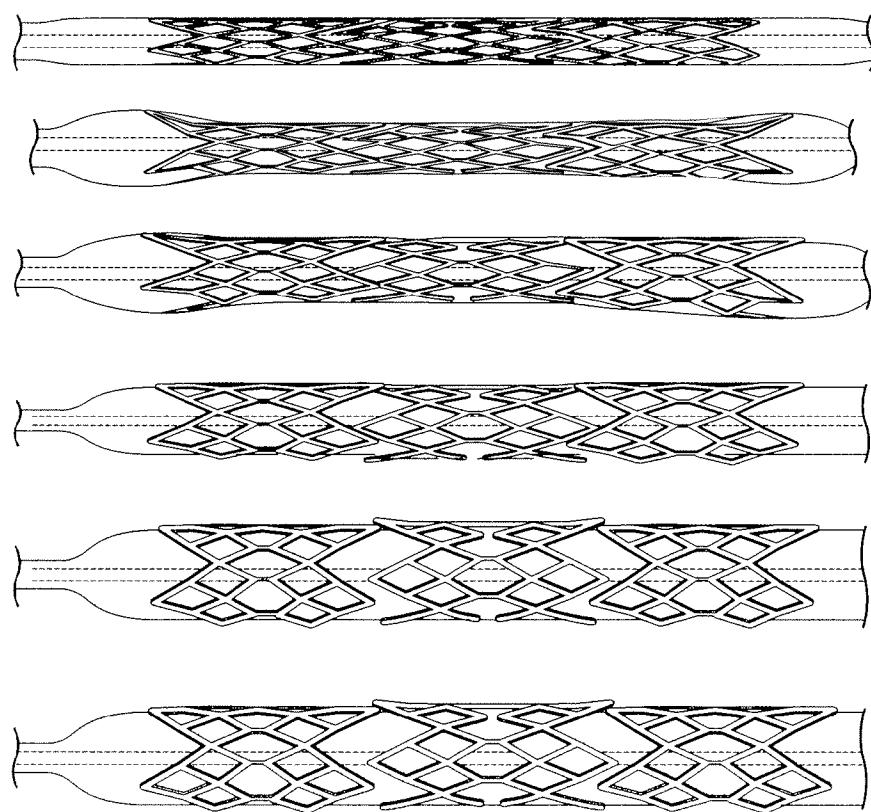


FIG. 31

22 / 22

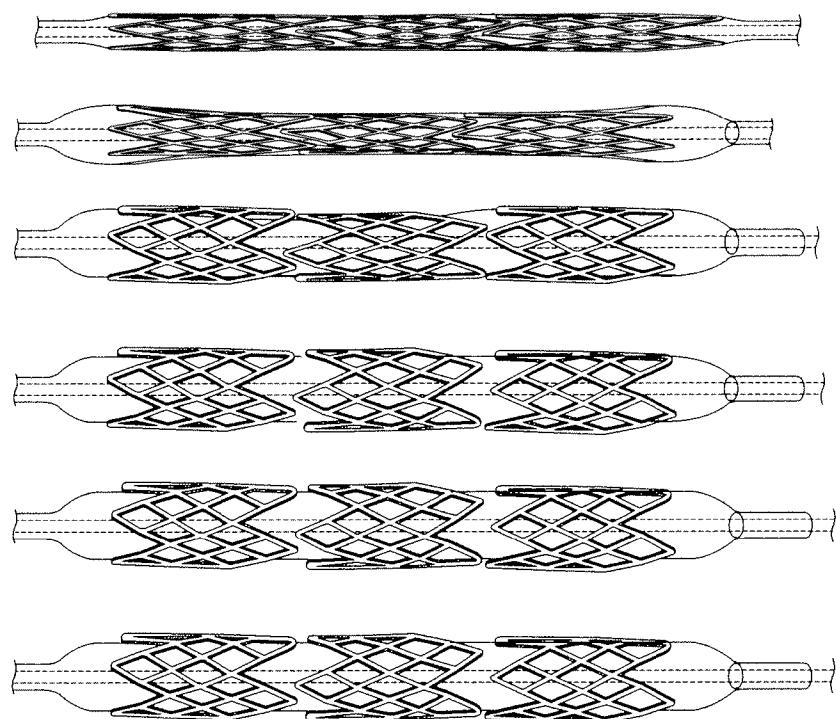


FIG. 32

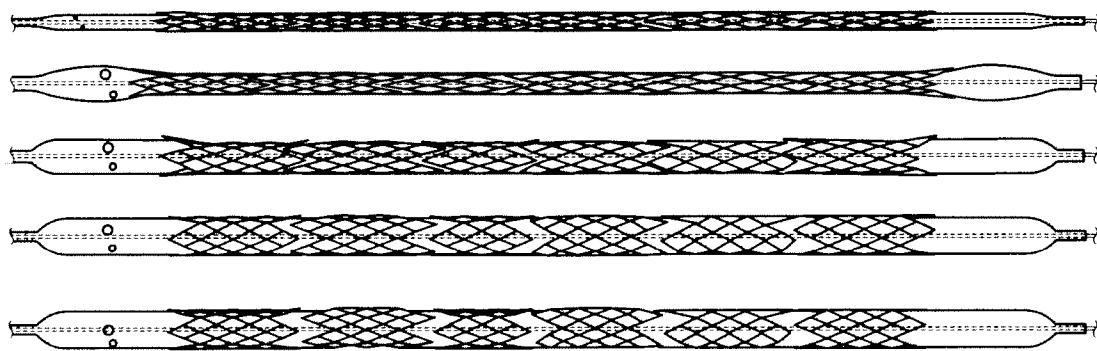


FIG. 33

# INTERNATIONAL SEARCH REPORT

International application No  
PCT/US2013/033141

**A. CLASSIFICATION OF SUBJECT MATTER**  
INV. A61F2/915 A61F2/82  
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
A61F

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 03/053284 A1 (WHITE GEOFFREY H [AU]) 3 July 2003 (2003-07-03) figures 2b, 4,8,12,15b page 13, line 32 - page 16, line 22 -----	1-8, 12-28
X	US 2004/186551 A1 (KAO STEPHEN [US] ET AL) 23 September 2004 (2004-09-23)	1-4,8, 19-24
A	paragraph [0044] - paragraph [0045]; figures 1,7, 11b, 18c, 22a paragraphs [0046], [0050], [0062] paragraph [0076] -----	12-18, 27,28
X	WO 03/022178 A1 (CATHNET SCIENCE HOLDING AS [DK]; ANDERSEN ERIK [DK]; WEN NING [FR]) 20 March 2003 (2003-03-20) page 10, line 8 - page 11, line 26; figure 1 -----	1-4,8, 19-24
A		12-18, 27,28



Further documents are listed in the continuation of Box C.



See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
28 May 2013	06/06/2013

Name and mailing address of the ISA/  
European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040,  
Fax: (+31-70) 340-3046

Authorized officer

Mary, Céline

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US2013/033141

### Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1.  Claims Nos.: **9-11**  
because they relate to subject matter not required to be searched by this Authority, namely:  
**Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery**
2.  Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3.  Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

### Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1.  As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2.  As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3.  As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4.  No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

#### Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/US2013/033141
---

Patent document cited in search report	Publication date	Patent family member(s)			Publication date
WO 03053284	A1 03-07-2003	US 2005182477 A1 WO 03053284 A1			18-08-2005 03-07-2003
US 2004186551	A1 23-09-2004	US 2004186551 A1 US 2008208311 A1 US 2008208318 A1 US 2009264979 A1 US 2013060321 A1			23-09-2004 28-08-2008 28-08-2008 22-10-2009 07-03-2013
WO 03022178	A1 20-03-2003	AT 430537 T CN 1575154 A CN 101779993 A EP 1427353 A1 EP 2085051 A1 JP 5017320 B2 JP 2005501654 A JP 2009240796 A US 2004243217 A1 US 2009248137 A1 WO 03022178 A1			15-05-2009 02-02-2005 21-07-2010 16-06-2004 05-08-2009 05-09-2012 20-01-2005 22-10-2009 02-12-2004 01-10-2009 20-03-2003