

(43) International Publication Date
3 November 2016 (03.11.2016)(51) International Patent Classification:
A61F 2/24 (2006.01)(74) Agents: **KAISER, Annemarie** et al.; Edwards Lifesciences, One Edwards Way, Irvine, CA 92614 (US).(21) International Application Number:
PCT/US2016/029769

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(22) International Filing Date:
28 April 2016 (28.04.2016)

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

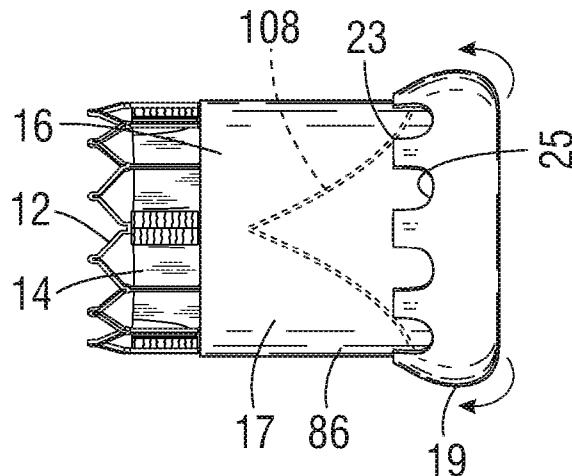
(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
62/154,610 29 April 2015 (29.04.2015) US
15/140,387 27 April 2016 (27.04.2016) US(71) Applicant: **EDWARDS LIFESCIENCES CORPORATION** [US/US]; One Edwards Way, Irvine, CA 92614 (US).**Published:**(72) Inventors: **PELLED, Itai**; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US). **SHERMAN, Elena**; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US). **GOLDBERG, Eran**; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US). **RUPP, Kevin D.**; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US). **NIR, Noam**; Edwards Lifesciences, One Edwards Way, Legal Department, Irvine, CA 92614 (US).

— with international search report (Art. 21(3))

(54) Title: LAMINATED SEALING MEMBER FOR PROSTHETIC HEART VALVE

FIG. 19F

(57) Abstract: The present disclosure relates to laminated sealing members for prosthetic valves and methods of making the same. In a representative embodiment, an implantable prosthetic valve that is radially collapsible to a collapsed configuration and radially expandable to an expanded configuration comprises an annular frame having an inflow end and an outflow end, a leaflet structure positioned within the frame and secured thereto, and a laminate sealing member comprising an encapsulating material. The laminate sealing member has a main portion that encapsulates at least a portion of the frame and an end portion extending from the inflow end of the frame, and the end portion of the laminate sealing member is folded to form a cuff adjacent the inflow end of the frame and secured to the main portion of the laminate sealing member.

LAMINATED SEALING MEMBER FOR PROSTHETIC HEART VALVE

FIELD

[001] The present disclosure relates to implantable prosthetic valves and, more particularly, to laminated sealing members for prosthetic valves and methods of making the same.

BACKGROUND

[002] Known prosthetic valves include a frame with a valvular structure mounted therein, an inner skirt or sealing member secured to the inside of the frame, and an outer skirt or sealing member secured to the exterior of the frame. The inner and outer skirts frequently must be secured to the frame by suturing or stitching the fabric of the respective skirts to the frame. Such suturing must often be done by hand, increasing the cost and time required to produce a prosthetic valve. Accordingly, improvements to skirts for prosthetic valves are desirable.

SUMMARY

[003] Certain embodiments of the disclosure concern laminated sealing members for prosthetic heart valves and methods of making the same. In one representative embodiment, an implantable prosthetic valve that is radially collapsible to a collapsed configuration and radially expandable to an expanded configuration comprises an annular frame having an inflow end and an outflow end, a leaflet structure positioned within the frame and secured thereto, and a laminate sealing member comprising an encapsulating material. The laminate sealing member has a main portion that encapsulates at least a portion of the frame and an end portion extending from the inflow end of the frame, and the end portion of the laminate sealing member is folded to form a cuff adjacent the inflow end of the frame and secured to the main portion of the laminate sealing member.

- 2 -

[004] In another representative embodiment, a method of making a prosthetic heart valve comprises positioning a first layer about a mandrel, positioning a radially expandable frame over the first layer, and positioning a second layer over the radially expandable frame. The method further comprises fusing the first and second layers to form a monolithic laminate sealing member such that at least a portion of the frame is encapsulated within the laminate sealing member, and folding an end portion of the laminate sealing member and securing it to a main portion of the laminate sealing member to form a cuff adjacent an inflow end of the frame.

[005] In another representative embodiment, a transcatheter heart valve comprises a radially expandable frame having an inflow end, an outflow end, and a laminate sealing member comprising a non-fabric inner layer positioned inside of the frame, a non-fabric outer layer positioned outside of the frame, and a fabric layer positioned between the non-fabric inner layer and the non-fabric outer layer. The non-fabric inner and outer layers are fused to one another such that the fabric layer and at least a portion of the frame are encapsulated therebetween. The laminate sealing member further comprises a main portion adjacent the frame and an end portion extending from the inflow end of the frame, the end portion being folded to form a cuff adjacent the inflow end of the frame and secured to the main portion of the laminate sealing member.

[006] The foregoing and other objects, features, and advantages of the disclosure will become more apparent from the following detailed description, which proceeds with reference to the accompanying figures.

BRIEF DESCRIPTION OF THE DRAWINGS

[007] FIGS. 1-3 illustrate an exemplary embodiment of a prosthetic valve including a laminate sealing member

[008] FIGS. 4-10 illustrate an exemplary frame of the heart valve of FIG. 1.

[009] FIGS. 11-15B illustrate another embodiment of a frame for use with a prosthetic heart valve.

[010] FIG. 16 illustrates a cross-sectional profile of the frame of FIG. 4, showing a general tapering from the outflow end to the inflow end.

[011] FIG. 17 is a cross-sectional view of the prosthetic heart valve of FIG. 2 taken along line 17-17.

[012] FIG. 18 is a cross-sectional view of the prosthetic heart valve of FIG. 1 taken along line 18-18.

[013] FIGS. 19A-19F illustrate a method of forming a laminate sealing member on the frame of a prosthetic heart valve, according to one embodiment.

[014] FIG. 20 is a flow chart of a method for forming a laminate sealing member on the frame of a prosthetic heart valve, according to one embodiment.

[015] FIG. 21 is a side elevation view illustrating another embodiment of a sealing member.

[016] FIG. 22 is a perspective view of the sealing member of FIG. 21 folded to form a cuff.

[017] FIG. 23 is a perspective view illustrating the main portion of the sealing member of FIG. 21 secured to a frame and the end portion extending distally from the frame.

[018] FIG. 24 is a perspective view illustrating the end portion of the sealing member of FIG. 21 folded and secured to the frame to form a cuff.

DETAILED DESCRIPTION

[019] The present disclosure concerns embodiments of implantable prosthetic devices and, in particular, implantable prosthetic valves, and methods for making such devices. In one aspect, a prosthetic device includes encapsulating layers that extend over a fabric layer and secure the fabric layer to another component of the device. In particular embodiments, the prosthetic device comprises a prosthetic heart valve, and can be configured to be implanted in any of the native heart valves. In addition, the prosthetic heart valve can be, for example, a transcatheter heart valve, a surgical heart valve, or a

minimally-invasive heart valve. The prosthetic valve also can comprise other types of valves implantable within other body lumens outside of the heart or heart valves that are implantable within the heart at locations other than the native valves, such as trans-atrial or trans-ventricle septum valves.

[020] FIGS. 1-3 show various views of a prosthetic heart valve 10, according to one embodiment. The illustrated valve is adapted to be implanted in the native aortic annulus, although in other embodiments it can be adapted to be implanted in the other native annuluses of the heart. The valve 10 can have four main components: a stent, or frame, 12, a valvular structure 14, and a laminate sealing member 16.

[021] The valvular structure 14 can comprise three leaflets 40, collectively forming a leaflet structure, which can be arranged to collapse in a tricuspid arrangement, as best shown in FIG. 2. The lower edge of leaflet structure 14 desirably has an undulating, curved scalloped shape (suture line 108 shown in FIG. 19F tracks the scalloped shape of the leaflet structure). By forming the leaflets with this scalloped geometry, stresses on the leaflets are reduced which, in turn, improves durability of the valve. Moreover, by virtue of the scalloped shape, folds and ripples at the belly of each leaflet (the central region of each leaflet), which can cause early calcification in those areas, can be eliminated or at least minimized. The scalloped geometry also reduces the amount of tissue material used to form leaflet structure, thereby allowing a smaller, more even crimped profile at the inflow end of the valve. The leaflets 40 can be formed of pericardial tissue (e.g., bovine pericardial tissue), biocompatible synthetic materials, or various other suitable natural or synthetic materials as known in the art and described in U.S. Pat. No. 6,730,118.

[022] The bare frame 12 is shown in FIG. 4. The frame 12 can be formed with a plurality of circumferentially spaced slots, or commissure windows, 20 (three in the illustrated embodiment) that are adapted to mount the commissures of the valvular structure 14 to the frame, as described in greater detail below. The frame 12 can be made of any of various suitable plastically-expandable materials (e.g., stainless steel, etc.) or self-expanding materials (e.g., Nitinol) as known in the art. When constructed of

a plastically-expandable material, the frame 12 (and thus the valve 10) can be crimped to a radially compressed state on a delivery catheter and then expanded inside a patient by an inflatable balloon or equivalent expansion mechanism. When constructed of a self-expandable material, the frame 12 (and thus the valve 10) can be crimped to a radially compressed state and restrained in the compressed state by insertion into a sheath or equivalent mechanism of a delivery catheter. Once inside the body, the valve can be advanced from the delivery sheath, which allows the valve to expand to its functional size.

[023] Suitable plastically-expandable materials that can be used to form the frame 12 include, without limitation, stainless steel, a nickel based alloy (e.g., a cobalt-chromium or a nickelcobalt-chromium alloy), polymers, or combinations thereof. In particular embodiments, frame 12 is made of a nickel-cobalt-chromium-molybdenum alloy, such as MP35N™ (tradename of SPS Technologies), which is equivalent to UNS R30035 (covered by ASTM F562-02). MP35N™/UNS R30035 comprises 35% nickel, 35% cobalt, 20% chromium, and 10% molybdenum, by weight. It has been found that the use of MP35N to form frame 12 provides superior structural results over stainless steel. In particular, when MP35N is used as the frame material, less material is needed to achieve the same or better performance in radial and crush force resistance, fatigue resistances, and corrosion resistance. Moreover, since less material is required, the crimped profile of the frame can be reduced, thereby providing a lower profile valve assembly for percutaneous delivery to the treatment location in the body.

[024] Referring to FIGS. 4 and 5, the frame 12 in the illustrated embodiment comprises a first, lower row I of angled struts 22 arranged end-to-end and extending circumferentially at the inflow end 13 of the frame; a second row II of circumferentially extending, angled struts 24; a third row III of circumferentially extending, angled struts 26; a fourth row IV of circumferentially extending, angled struts 28; and a fifth row V of circumferentially extending, angled struts 32 at the outflow end 15 of the frame. A plurality of substantially straight axially extending struts 34 can be used to interconnect the struts 22 of the first row I with the struts 24 of the second row II. The fifth row V of

angled struts 32 are connected to the fourth row IV of angled struts 28 by a plurality of axially extending window frame portions 30 (which define the commissure windows 20) and a plurality of axially extending struts 31. Each axial strut 31 and each frame portion 30 extends from a location defined by the convergence of the lower ends of two angled struts 32 to another location defined by the convergence of the upper ends of two angled struts 28. FIGS. 6, 7, 8, 9 and 10 are enlarged views of the portions of the frame 12 identified by letters A, B, C, D and E, respectively, in FIG. 4.

[025] Each commissure window frame portion 30 mounts a respective commissure of the leaflet structure 14. As can be seen each frame portion 30 is secured at its upper and lower ends to the adjacent rows of struts to provide a robust configuration that enhances fatigue resistance under cyclic loading of the valve compared to known cantilevered struts for supporting the commissures of the leaflet structure. This configuration enables a reduction in the frame wall thickness to achieve a smaller crimped diameter of the valve. In particular embodiments, the thickness T of the frame 12 (FIG. 4) measured between the inner diameter and outer diameter is about 0.48 mm or less.

[026] The struts and frame portions of the frame collectively define a plurality of open cells of the frame. At the inflow end of the frame 12, struts 22, struts 24, and struts 34 define a lower row of cells defining openings 36. The second, third, and fourth rows of struts 24, 26, and 28 define two intermediate rows of cells defining openings 38. The fourth and fifth rows of struts 28 and 32, along with frame portions 30 and struts 31, define an upper row of cells defining openings 40. The openings 40 are relatively large and are sized to allow portions of the leaflet structure 14 to protrude, or bulge, into and/or through the openings 40 when the frame 12 is crimped in order to minimize the crimping profile.

[027] As best shown in FIG. 7, the lower end of the strut 31 is connected to two struts 28 at a node or junction 44, and the upper end of the strut 31 is connected to two struts 32 at a node or junction 46. The strut 31 can have a thickness S1 that is less than the thicknesses S2 of the junctions 44, 46. The junctions 44, 46, along with junctions 64, can prevent full closure of openings 40. The geometry of the struts 31, and junctions 44, 46

and 64 can assist in creating enough space in openings 40 in the crimped state to allow portions of the leaflets to protrude (i.e., bulge) outwardly through openings. This allows the valve to be crimped to a relatively smaller diameter than if all of the leaflet material is constrained within the crimped frame.

[028] The frame 12 is configured to prevent or at least minimize possible over-expansion of the valve at a predetermined balloon pressure, especially at the outflow end portion of the frame, which supports the leaflet structure 14. In one aspect, the frame is configured to have relatively larger angles 42a, 42b, 42c, 42d, 42e between struts. The larger the angle, the greater the force required to open (expand) the frame. This phenomenon is schematically illustrated in FIGS. 15A and 15B. FIG. 15A shows a strut 32 when the frame 12 is in its compressed state (e.g., mounted on a balloon). The vertical distance d_1 between the ends of the struts is greatest when the frame is compressed, providing a relatively large moment between forces F_1 and F_2 acting on the ends of the strut in opposite directions upon application of an opening force from inflation of the balloon (or expansion of another expansion device). When the frame expands radially, the vertical distance between the ends of the strut decreases to a distance d_2 , as depicted in FIG. 15B. As the vertical distance decreases, so does the moment between forces F_1 and F_2 . Hence, it can be seen that a relatively greater expansion force is required as the vertical distance and the moment between the ends of the strut decreases. Moreover, strain hardening (stiffening) at the ends of the strut increases as the frame expands, which increases the expansion force required to induce further plastic deformation at the ends of the strut. As such, the angles between the struts of the frame can be selected to limit radial expansion of the frame at a given opening pressure (e.g., inflation pressure of the balloon). In particular embodiments, these angles are at least 110 degrees or greater when the frame is expanded to its functional size, and even more particularly these angles are at least 120 degrees or greater when the frame is expanded to its functional size.

[029] In addition, the inflow and outflow ends of a frame generally tend to over-expand more so than the middle portion of the frame due to the “dog boning” effect of the

balloon used to expand the valve. To protect against over-expansion of the leaflet structure 14, the leaflet structure desirably is secured to the frame 12 below the upper row of struts 32, as best shown in FIG. 1. Thus, in the event that the outflow end of the frame is over-expanded, the leaflet structure is positioned at a level below where over-expansion is likely to occur, thereby protecting the leaflet structure from over-expansion.

[030] In a known valve construction, the leaflets can protrude outwardly beyond the outflow end of the frame when the valve is crimped if the leaflets are mounted too close to the distal end of the frame. If the delivery catheter on which the crimped valve is mounted includes a pushing mechanism or stop member that pushes against or abuts the outflow end of the valve (for example, to maintain the position of the crimped valve on the delivery catheter), the pushing member or stop member can damage the exposed leaflets that extend beyond the outflow end 15 of the frame 12. Another benefit of mounting the leaflets at a location spaced from the outflow end 15 of the frame 12 is that when the valve is crimped on a delivery catheter, the leaflets 40 do not protrude beyond the outflow end 15 of the frame 12 in the axial direction. As such, if the delivery catheter includes a pushing mechanism or stop member that pushes against or abuts the outflow end of the valve, the pushing mechanism or stop member can contact the end of the frame 12, and not leaflets 40, so as to avoid damage to the leaflets.

[031] Also, as can be seen in FIG. 5, the openings 36 of the lowermost row of openings in the frame 12 are relatively larger than the openings 38 of the two intermediate rows of openings. This allows the frame, when crimped, to assume an overall tapered shape that tapers from a maximum diameter D_1 at the outflow end of the valve to a minimum diameter D_2 at the inflow end of the valve, as shown in FIG. 16 and further described in U.S. Patent Publication No. 2012/0123529. When crimped, the frame 12 has a reduced diameter region extending along a portion of the frame adjacent the inflow end of the frame, indicated by reference number 174, which generally corresponds to the region of the frame covered by the cuff 21 of the laminated sealing member 16, further described below. The diameter of region 174 is reduced compared to the diameter of the upper portion of the frame such that the cuff 21 need not increase the overall crimp profile of

the valve. When the valve is deployed, the frame can expand to the cylindrical shape shown in FIG. 4. In one example, the frame of a 26-mm valve, when crimped, had a diameter D_1 of 14 French at the outflow end of the valve and a diameter D_2 of 12 French at the inflow end of the valve.

[032] FIGS. 11 and 12 show an alternative frame 50 that can be incorporated in the valve 10. The frame 50 comprises multiple rows of circumferentially extending, angled struts 52 that are connected to each other at nodes, or connecting portions, 54 and 56. The uppermost row of struts 52 are connected to an adjacent row of struts by a plurality of axially extending struts 58 and commissure window frame portions 60. Each commissure frame portion 60 defines a slot or commissure window 62 for mounting a respective commissure of the valvular structure, as described in U.S. Patent Publication No. 2012/0123529. In particular embodiments, the thickness T of the frame 50 is about 0.45 mm or less. FIGS. 13 and 14 are enlarged views of the portions of the frame 50 identified by letters A and B, respectively, in FIG. 12.

[033] The laminate sealing member 16 can include a main portion 17 extending from the proximal end of the fourth row IV of angled struts 28 (i.e., from about the height of the commissure windows 20), and an end portion 19 extending from the inflow end 13 of the frame 12, as shown in FIGS. 1-3. In the illustrated embodiment, the end portion 19 can be folded back on itself and secured to the main portion 17 to form a cuff 21 adjacent the inflow end 13 of the frame 12, as shown in FIGS. 1-3, and 18. The end portion 19 can include a plurality of circumferentially spaced apart extension portions or projections 23 that can be secured to the main portion 17 by, for example, heat bonding, adhesive, and/or suturing, as further described below. The laminate sealing member 16 can seal against the tissue of the native valve annulus, helping to reduce paravalvular leakage past the prosthetic valve 10. In some embodiments, the cuff 21 can billow open such that it defines a pocket in the laminate sealing member 16 extending circumferentially around the inflow end 13 of the frame 12 when the prosthetic valve is implanted in a native valve annulus. Alternatively, the end portion 19 can lie relatively flush against the main portion 17, as desired.

[034] The laminate sealing member 16 can comprise inner and outer encapsulating layers 84, 86, respectively (also referred to as “inner and outer layers”), as shown in FIGS. 17 and 18. In particular embodiments, the encapsulating layers 84, 86 comprise a non-fabric polymer layer or film. In some embodiments, the laminate sealing member 16 can also include a reinforcing layer, such as a fabric or textile layer 18 situated adjacent the frame 12 between the encapsulating layers 84, 86. The encapsulating layers 84, 86 can be fused, bonded, or otherwise secured to each other through the openings in the frame 12, which effectively encapsulates corresponding portions of the frame 12 and the fabric layer 18 to secure these components in their assembled state shown in FIGS. 1-3.

[035] In the embodiment shown, the inner and outer encapsulating layers 84, 86 can be coextensive along the axial length of the main portion 17 of the laminate sealing member 16. In other words, the encapsulating layers 84, 86 can both extend distally from about the level of the commissure windows 20 to the inflow end of the frame to completely or substantially encapsulate the corresponding portion of the frame 12 and the fabric layer 18, as shown in FIG. 18. In the illustrated embodiment, the inner layer 84 can terminate at or near the inflow end 13 of the frame 12, while the outer layer 86 can extend beyond the inflow end to form the end portion 19 of the laminate sealing member 16 and, hence, the cuff 21. Thus, in the illustrated embodiment, the inner layer 84 forms an inner skirt of the sealing member and the outer layer 86 forms an outer skirt of the sealing member. In alternative embodiments, the inner and/or outer layers 84, 86 can extend along any proportion of the main portion 17 or the end portion 19 of the laminate sealing member 16, as desired. For example, in some embodiments the inner and outer layers 84, 86 can be coextensive along both the main portion 17 and the end portion 19 of the laminate sealing member 16. In further alternative embodiments, the outer layer 86 can terminate at the inflow end 13 of the frame 12, while the inner layer 84 can continue beyond the inflow end 13 to form the cuff 21.

[036] In some embodiments, the layers 84, 86 can be such that they only encapsulate selected portions of the frame 12 and the fabric layer 18. Also, although in the illustrated

embodiment the inner and outer layers 84, 86 are tubular or cylindrical in shape, the inner and outer layers 84, 86 need not extend along the respective inner and outer surfaces of the frame 12 in the circumferential direction through 360 degrees. In other words, the inner and outer layers 84, 86 can have a cross-sectional profile (in a plane perpendicular to the axis of the lumen of the valve) that is not a complete circle.

[037] As stated above, the laminate sealing member 16 can comprise a reinforcing layer, such as the fabric layer 18. The fabric layer 18 can comprise, for example, any of various woven fabrics, such as gauze, polyethylene terephthalate (PET) fabric (e.g., Dacron), polyester fabric, polyamide fabric, or any of various non-woven fabrics, such as felt. The thickness of the fabric layer can vary, but can be less than 6 mil, and desirably less than 4 mil, and even more desirably about 2 mil. Traditionally, fabric skirts have been secured to frames using sutures. In contrast, in the illustrated embodiment, fabric layer 18 desirably is secured to the frame 12 without sutures and instead is secured to the frame 12 with the inner and/or outer encapsulating layers 84, and 86 (see, e.g., FIGS. 17 and 18).

[038] The fabric layer 18 of the prosthetic valve can serve several functions. In particular embodiments, for example, the fabric layer 18 primarily functions to strengthen the laminate sealing member 16 to resist tearing. In this manner, the leaflet structure 14 can be anchored to the frame 12 by sutures without tearing the laminate sealing member 16. In addition, the fabric layer 18, in cooperation with the encapsulating layers 84, 86, can help decrease (or prevent) paravalvular leakage past the prosthetic valve when in the expanded configuration.

[039] Alternatively, the reinforcing layer can comprise one or more layers or films formed from any of various semi-crystalline polymeric materials or thermoplastics having aligned or partially aligned (e.g., parallel) molecular chains. Such materials can exhibit anisotropic mechanical properties, such as increased mechanical strength along the longitudinal direction of the molecular chains. Suitable semi-crystalline polymeric materials can include, for example, PTFE, PET, polypropylene, polyamide,

polyetheretherketone (PEEK), etc., layers or films of which can be situated between and encapsulated by the encapsulating layers to reinforce the laminate sealing member 16.

[040] The encapsulating layers 84, 86 can be made of any suitable biocompatible material. In one example, the encapsulating layers 84, 86 can be formed using an electrospinning process. In other examples, the encapsulating layers 84, 86 can be formed using any other suitable method including, for example, dip coating, spray coating, or melt-spinning. The biocompatible material may be a non-absorbable polymeric material (i.e., a material that does not dissolve once implanted in the body). Examples of such materials include, without limitation, expanded polytetrafluoroethylene (ePTFE), unexpanded porous PTFE, polyester or expanded PTFE yarns, PTFE, ultrahigh molecular weight polyethylene (UHMWPE), other polyolefins, composite materials such as ePTFE with PTFE fibers, or UHMWPE film with embedded UHMWPE fibers, polyimides, silicones, polyurethane, hydrogels, fluoroethylpolypropylene (FEP), polypropylfluorinated amines (PFA), other related fluorinated polymers, or various combinations of any of these materials. In particular embodiments, the encapsulating layers 84, 86 are formed from respective tubes made of a suitable polymeric material (e.g., ePTFE tubes or UHMWPE tubes) that are bonded to each other when subjected to heat treatment, as described in detail below.

[041] Microporous expanded polytetrafluoroethylene (ePTFE) tubes can be made by a number of well-known methods. Expanded PTFE is frequently produced by admixing particulate dry polytetrafluoroethylene resin with a liquid lubricant to form a viscous slurry. The mixture can be poured into a mold, typically a cylindrical mold, and compressed to form a cylindrical billet. The billet can then be ram extruded through an extrusion die into either tubular or sheet structures, termed extrudates in the art. The extrudates comprise an extruded PTFE-lubricant mixture called “wet PTFE.” Wet PTFE has a microstructure of coalesced, coherent PTFE resin particles in a highly crystalline state. Following extrusion, the wet PTFE can be heated to a temperature below the flash point of the lubricant to volatilize a major fraction of the lubricant from the PTFE extrudate. The resulting PTFE extrudate without a major fraction of lubricant is known

in the art as dried PTFE. The dried PTFE can then be either uniaxially, biaxially, or radially expanded using appropriate mechanical apparatus known in the art. Expansion is typically carried out at an elevated temperature, e.g., above room temperature but below 327 degrees C., the crystalline melt point of PTFE. Uniaxial, biaxial, or radial expansion of the dried PTFE causes the coalesced, coherent PTFE resin to form fibrils emanating from nodes (regions of coalesced PTFE), with the fibrils oriented parallel to the axis of expansion. Once expanded, the dried PTFE is referred to as expanded PTFE (“ePTFE”) or microporous PTFE.

[042] UHMWPE is made up of very long chains of polyethylene, with molecular weight numbering in the millions, usually between 2 and 6 million. It is highly resistant to corrosive chemicals, has extremely low moisture absorption and a very low coefficient of friction. It is self-lubricating and highly resistant to abrasion. UHMWPE is processed using compression molding, ram extrusion, gel spinning, and sintering. UHMWPE is available commercially as a powder, in sheets or rods, and as fibers.

[043] Referring to FIGS. 19A-19E and 20, an exemplary method for forming the prosthetic valve 10 will now be described. Although the use of ePTFE is described below, it is merely exemplary in nature and is not intended as a limitation. It is to be understood that other materials such as UHMWPE, polyurethane composite materials, or any other non-absorbable polymeric materials described above can be used.

[044] First, as depicted in FIG. 19A, an inner layer 84 comprising a flat piece of ePTFE material or an ePTFE tube can be placed or wrapped on a mandrel 100. Second, as depicted in FIG. 19B, a frame 12 can be placed over the inner layer 84 such that the inner layer 84 extends from approximately the commissure windows 20 to the inflow end 13 of the frame 12, although it will be appreciated that other configurations are possible. Third, as depicted in FIG. 19C, the fabric layer 18 can be placed over the frame 12. The fabric layer 18 can be in the form of a sheet of fabric material that is tightly wrapped around the outer surface of the frame 12. However, in alternative embodiments, the fabric layer 18 may also be situated inside the frame 12 (e.g., placed on the inner layer 84 before placement of the frame 12 on the inner layer 84). In the illustrated

embodiment, the fabric layer 18 may have an axial length that is shorter than the inner and outer layers 84, 86 to facilitate bonding of the inner and outer layers 84, 86 at their respective ends to encapsulate the frame 12 and fabric layer 18 therebetween.

[045] Fourth, as depicted in FIG. 19D, the outer layer 86 comprising a flat piece of ePTFE material or an ePTFE tube can be placed or wrapped over the fabric layer 18. In the illustrated embodiment, the outer layer 86 can have a proximal portion 87 and a distal portion 89, wherein the distal portion 89 can have a diameter that is greater than the diameter of the proximal portion 87. The extension portions 23 of the outer layer 86 can be formed on the distal portion 89 (e.g., by laser cutting) before or after placement of the outer layer 86 on the mandrel 100, as desired. As shown in FIG. 19E, layers of PTFE tape 92 can then be wrapped around one or both ends of the outer layer 86 to help secure the position of the outer layer 86 to the underlying layers of the assembly and to the mandrel 100 during subsequent processing.

[046] An alternative way to encapsulate the frame with a polymer is by using an electrospinning technique. Electrospinning uses an electrical charge to draw very fine (typically on the micrometer or nanometer scale) fibers from a liquid.

[047] The assembly shown in FIG. 19E can now undergo an encapsulation process whereby the assembly is subjected to heat and/or pressure to cause the inner and outer layers 84, 86 to bond to each other through the openings in the frame 12 proximally and distally of the fabric layer 18 (see FIG. 18) to encapsulate the frame 12 and the fabric layer 18 therebetween. Depending on the porosity of the weave of the fabric layer 18, the layers 84, 86 can bond to each other through the fabric layer 18. During this step, the entire outer surface of the assembly on the mandrel 100 can be tightly wrapped with a suitable material (e.g., PTFE tape) to apply pressure to the various layers of the assembly such that the layers 84, 86 form a monolithic laminate sealing member 16. The entire assembly, including the mandrel 100, can be transferred to an oven where the inner and outer layers 84, 86 are sintered by being heated to a predetermined temperature. In one implementation, for example, the inner and outer layers 84, 86 are sintered by being heated to a temperature above 327 degrees C, the crystalline melt point of PTFE. In

some embodiments, bonding between the inner and outer layers 84, 86 can be facilitated by the use of one or more adhesives, such as polyurethane.

[048] During the sintering process the ePTFE is restrained against uniaxial, biaxial, or radial contraction. Sintering can cause at least a portion of the crystalline PTFE to change from a crystalline state to an amorphous state. The conversion from a highly crystalline structure to one having an increased amorphous content can lock the node and fibril microstructure, as well as its orientation relative to the axis of expansion, and provide a dimensionally stable tubular or sheet material upon cooling.

[049] After the sintering process, the assembly is removed from the oven and allowed to cool. The material wrapped around the assembly, as well as tape layers 92, can now be removed. Any portions of the inner and outer layers 84, 86 that extend beyond the desired dimensions of the laminate sealing member 16 can be trimmed. If desired, selected portions of the inner and outer layers 84, 86 can be removed to facilitate crimping of the valve for delivery into a patient. Any of various suitable techniques and mechanisms can be used to selectively remove portions of layers 84, 86, such as laser cutting. For example, portions of the inner and outer layers 84, 86 that cover selected openings in the frame 12 can be cut or otherwise removed to minimize the amount of material in the valve, which can facilitate crimping of the valve to a relatively small diameter.

[050] Referring to FIG. 19F, after the encapsulating layers 84, 86 have been bonded together to form the laminate sealing member 16, the end portion 19 of the laminate sealing member 16 can be folded over to form the cuff 21, and the extension portions 23 can be secured to the main portion 17 of the laminate sealing member 16. In some embodiments, the extension portions 23 can be attached to the main portion 17 by heat bonding (e.g., in combination with an optional additional polymer such as polyurethane to promote bonding between the ePTFE layers, with process temperatures adjusted as necessary). In some embodiments, the extension portions 23 can be attached to the main portion by suturing. In some embodiments, the end portion 19 and/or the extension portions 23 can include a reinforcing fabric layer to facilitate suturing of the end portion

19 to the main portion 17. In some embodiments, the cuff 21 can be secured to the main portion via heat bonding, an adhesive, and/or suturing.

[051] In particular embodiments, the cuff 21 is secured to the main body 17 only along the uppermost edges of the extension portions 23 and the U-shaped upper edge portions 25 defining the gaps are not secured to the frame. Thus, the cuff 21 can form a pocket having openings defined by the U-shaped edges 25.

[052] In an alternative embodiment, the fabric layer 18 can be pre-formed in a tubular or cylindrical configuration. In this embodiment, the fabric layer 18 can be positioned on the frame 12 by first partially crimping the frame 12 to a diameter smaller than the diameter of the fabric layer 18. The fabric layer 18 can then be placed over the partially crimped frame, and the frame can be expanded back to its functional size. The fabric layer 18 desirably is sized such that the expanded frame 12 applies at least some outward radial pressure against the fabric layer 18 to assist in retaining the fabric layer 18 on the frame 12. The frame and fabric layer assembly can then be placed onto inner layer 84 (already on the mandrel), and encapsulated following the process described above. In another embodiment, the fabric layer 18 can be placed on the inside of the frame 12. For example, the fabric layer 18 can be in the form of a sheet of material that is wrapped around inner layer 84 prior to placing the frame 12 on the mandrel 100. Alternatively, the fabric layer 18 can have a tubular configuration and can be positioned onto inner layer 84 prior to placing the frame 12 on the mandrel 100.

[053] After encapsulation, the frame 12 can be removed from the mandrel 100 and the leaflet structure 14 can be attached to the fabric layer 18 and/or the frame 12 using sutures or other suitable techniques or mechanisms. In the illustrated embodiment shown in FIG. 2, for example, the leaflets 40 are secured to one another at their adjacent sides to form commissures 48. Each commissure 48 can be secured to a corresponding commissure window 20 of the frame 12, as described in U.S. Patent Publication No. 2012/0123529. The lower, or inflow, end portion of the leaflets 40 can be sutured to the fabric layer 18 of the laminate sealing member 16 along a suture line 108 that tracks the curvature of the scalloped lower edge of the leaflet structure, as shown in FIG. 19F. The

fabric layer 18 can provide the strength required to retain the sutures without tearing the laminate sealing member 16. Any suitable suture, such as an Ethibond suture, can be used to secure the leaflets 40 to the fabric layer 18 of the laminate sealing member 16 along suture line 108.

[054] In certain embodiments, the lower edges of the leaflets 40 can be secured to the fabric layer 18 via a thin PET reinforcing strip (not shown), as disclosed in U.S. Pat. No. 7,993,394. As described in U.S. Pat. No. 7,993,394, the reinforcing strip can be sutured to the lower edges of the leaflets. The reinforcing strip and the lower edges of the leaflets can then be sutured to the laminate sealing member 16 along suture line 108. The reinforcing strip desirably is secured to the inner surfaces of the leaflets 40 such that the lower edges of the leaflets become sandwiched between the reinforcing strip and the laminate sealing member 16 when the leaflets and the reinforcing strip are secured to the laminate sealing member. The reinforcing strip enables a secure suturing and protects the pericardial tissue of the leaflet structure from tears.

[055] As noted above, the conventional method for securing a fabric skirt to a frame involves manually suturing the fabric skirt to the frame. In contrast, the illustrated embodiment relies on the inner and outer layers 84, 86 to secure the fabric layer 18 in place relative to the frame. As can be appreciated, this technique for securing the fabric layer 18 to the frame can significantly reduce the amount of labor required to assemble a valve. The use of layers 84, 86 provides other advantages as well. For example, the outer layer 86, when formed from ePTFE or UHMWPE, has a porous microstructure that facilitates tissue in-growth from surrounding tissue after the valve is implanted. When formed of ePTFE, UHMWPE, or other suitable polymers, the laminate sealing member 16 can exhibit lower blood permeability than conventional fabric skirts, especially in the period immediately following implantation, which can help to reduce paravalvular leakage.

[056] In addition, the inner and outer layers 84, 86 can protect the leaflets 40 during crimping and facilitate even and predictable crimping of the valve. When a prosthetic valve is placed in a crimping apparatus to radially compress the valve to a smaller

diameter for insertion into a patient, the leaflets of the valve are pressed against the inner surface of the metal frame and portions of the tissue can protrude into the open cells of the frame between the struts and can be pinched due to the scissor-like motion of the struts of the frame. If the valve is severely crimped to achieve a small crimping size, this scissor-like motion can result in cuts and rupture of the tissue leaflets. To protect the leaflets during crimping, it is known to place a deformable material around the valve to prevent direct contact between the hard surface of the jaws of the crimping apparatus and the valve. The deformable material can protrude into the open cells, thereby preventing the leaflets from entering this space and being pinched by metal struts of the frame.

Layers 84, 86 function in a manner similar to this deformable material to protect leaflets from being pinched during crimping. As such, the disclosed valve 10 can be placed in a crimping apparatus without an additional protective layer of material surrounding the valve. Due to the presence of layers 84, 86, the valve 10 can be crimped onto the balloon of a balloon catheter in an even and predictable manner that forms a very ordered structure of balloon-leaflets-frame (from inward to outward). Additionally, inner layer 84 can prevent direct contact between the leaflets 40 and the frame 12 during working cycles of the valve (i.e., as the valve leaflets open and close in response to blood pressure) to protect the leaflets against damage caused by contact with the frame.

[057] Moreover, as noted above, the fabric layer 18 can be any of various woven or non-woven fabrics, such as a gauze, PET cloth, or felt. PET or other fabrics are substantially non-elastic (i.e., substantially non-stretchable and non-compressible). As such, in known prosthetic valves, the skirt can wrinkle after expansion from the crimped diameter. In the illustrated embodiment, the fabric layer 18 can be tightly compressed against the frame by layers 84, 86 such that when the valve is expanded to its functional size from the crimped state, the fabric layer 18 can recover to its original, smooth surfaces with little or no wrinkling.

[058] The encapsulation process is described above in the context of securing a fabric layer to the frame of an expandable transcatheter heart valve within a laminate sealing member. The fabric layer typically is more durable than the ePTFE layers and, therefore,

the fabric layer reinforces the ePTFE layers where they undergo stresses from cyclic loading of the valve. However, in alternative embodiments, the valve can be formed without the fabric layer to permit crimping of the valve to a smaller delivery diameter. The ePTFE layers 84, 86, and the cuff 21 can serve as the primary sealing mechanism that prevents paravalvular leakage around or through the frame of the valve. In other embodiments, the fabric layer 18 can be used to reinforce only selected portions of the layers 84, 86, such as those portions of layers 84, 86 subject to greatest loading, while the remaining portions of layers 84, 86 do not contain a fabric layer or fabric layer.

[059] It should be noted that the encapsulation process can be utilized to secure a fabric or woven or non-woven textile element to other components of a prosthetic valve. For example, surgical valves (valves which are typically implanted via open-heart surgery) include several components that are covered with a cloth or fabric material. Known surgical valves typically have a sewing ring and one or more stent components, each of which are covered with a cloth member. The cloth member typically is wrapped around the valve component and the longitudinal edges of the cloth member are manually stitched to each other to secure the cloth member around the valve component. As can be appreciated, the time and labor required to secure such cloth members to the components of the valve can be significantly reduced by employing an encapsulation technique as described herein.

[060] FIG. 20 schematically illustrates a representative method of encapsulating a frame of a prosthetic valve to form a laminate sealing member. At block 202, an inner layer comprising, for example, ePTFE, can be positioned over a mandrel.

[061] At block 204, a frame can be positioned on the mandrel over the inner layer.

[062] At block 206, an outer layer comprising, for example, ePTFE, can be positioned on the mandrel over the frame.

[063] At block 208, the inner and outer layers can be fused to one another to create a laminate sealing member encapsulating at least a portion of the frame therebetween.

[064] At block 210, an end portion of the laminate sealing member can be folded up and secured to a main portion of the laminate sealing member to form a cuff. The laminate sealing member can optionally include a fabric or textile layer located between the inner and outer layers adjacent the inside or outside of the frame, as described above.

[065] FIGS. 21-24 illustrate another embodiment of a sealing member 300 including a main portion 302, an intermediate portion 304, and an end portion 306. In the illustrated embodiment, the main portion 302 can have a diameter D_M corresponding substantially to an inner diameter of an expanded frame 308. In the illustrated embodiment, the end portion 306 can have a diameter D_E that is equal to or greater than an outer diameter of the expanded frame 308, and the intermediate portion 304 can have a diameter that increases or flares in a longitudinal direction of the sealing member from the diameter D_M of the main portion 302 to the diameter D_E of the end portion 306. Thus, in the illustrated embodiment, the intermediate portion can have a frustoconical shape.

[066] The end portion 306 of the sealing member 300 can be folded (e.g., along the interface 316 between the intermediate portion and the end portion and the interface 318 between the main portion and the intermediate portion) and secured to the main portion 302, as shown in FIGS. 21 and 22. During the assembly process, the sealing member can be secured to the inside of the frame 308 such that the main portion 302 is adjacent an inner surface of the frame and the end portion 306 extends distally from an inflow end 310 of the frame 308. The end portion 306 can then be folded upwardly and around the inflow end 310 of the frame and attached to the main portion 302 (through the frame) and/or to the exterior of the frame 308 to form a cuff 312 adjacent the inflow end 310 of the frame. In this manner, the sealing member 300 can combine the functions of conventionally separate inner and outer skirts into a single unitary sealing member. This can reduce the amount of material around the inflow end of the valve, thereby reducing the crimped profile of the valve, along with flow disturbances or obstructions created by the sealing member when inserted into a native heart valve. Use of the sealing member described herein can also reduce the time and labor required to assemble a valve over known valve skirts.

[067] In the illustrated embodiment, the end portion 306 can include tabs or projections 314, which can be secured to the main portion 302 of the sealing member and/or to the exterior of the frame members by, for example, stitching, adhesive, heat bonding, etc. The projections 314 can aid in folding the end portion 306 to form the cuff 312, thereby reducing the need for complex shaping of the sealing member. In some embodiments, the main portion 302 can also include tabs or projections.

[068] The sealing member 300 may be made from any of various woven fabrics such as PET, polybutylene terephthalate (PBT), UHMWPE, polypropylene, natural fibers such as silk, etc. The fabric may be woven or braided into the final shape of the sealing member 300. Alternatively, the sealing member 300 may be formed from a tubular piece of material, such as by application of heat or by shape setting. The projections 314 can be created by, for example, cutting sections of material from the end portion 306. Additionally, it should be understood that the shape of the sealing member 300 can be applicable to any of the sealing members described herein.

[069] In some embodiments, the properties of the fabric may be varied along the length of the sealing member. For example, yarns in the fabric of the main portion 302 may be set at an angle (e.g., 45 degrees) such that the fabric of the main portion can more easily elongate and/or foreshorten during crimping and expansion of the frame.

[070] In some embodiments, a fabric sealing member (e.g., the sealing member 300) can be laminated with or encapsulated between one or more layers or films of ePTFE (e.g., 0.000020 inch to 0.001 inch Aeos® ePTFE material available from Zeus Industrial Products, Inc.). For example, one or more layers of ePTFE can be applied to at least one surface of the sealing member to reduce the permeability of the sealing member. This can reduce the amount of blood leakage through the sealing member, especially in the time period immediately following implantation. The smooth surface of the one or more ePTFE layers can also improve the durability of the tissue leaflets contacting the ePTFE layers, and can reduce or prevent the exposure of broken yarns or filaments in the underlying fabric, improving yields during manufacturing of the heart valves. The number and thickness of the one or more ePTFE layers, along with other parameters

including the internodal distance, porosity, etc., of the ePTFE, can be varied according to the particular properties desired. In alternative embodiments, one or more layers of ePTFE are applied to both surfaces of a sealing member (e.g., sealing member 300) before it is assembled onto a frame.

General Considerations

[071] For purposes of this description, certain aspects, advantages, and novel features of the embodiments of this disclosure are described herein. The disclosed methods, apparatus, and systems should not be construed as being limiting in any way. Instead, the present disclosure is directed toward all novel and nonobvious features and aspects of the various disclosed embodiments, alone and in various combinations and sub-combinations with one another. The methods, apparatus, and systems are not limited to any specific aspect or feature or combination thereof, nor do the disclosed embodiments require that any one or more specific advantages be present or problems be solved.

[072] Although the operations of some of the disclosed embodiments are described in a particular, sequential order for convenient presentation, it should be understood that this manner of description encompasses rearrangement, unless a particular ordering is required by specific language set forth below. For example, operations described sequentially may in some cases be rearranged or performed concurrently. Moreover, for the sake of simplicity, the attached figures may not show the various ways in which the disclosed methods can be used in conjunction with other methods. Additionally, the description sometimes uses terms like “provide” or “achieve” to describe the disclosed methods. These terms are high-level abstractions of the actual operations that are performed. The actual operations that correspond to these terms may vary depending on the particular implementation and are readily discernible by one of ordinary skill in the art.

[073] As used in this application and in the claims, the singular forms “a,” “an,” and “the” include the plural forms unless the context clearly dictates otherwise.

Additionally, the term “includes” means “comprises.” Further, the terms “coupled” and

“associated” generally mean electrically, electromagnetically, and/or physically (*e.g.*, mechanically or chemically) coupled or linked and does not exclude the presence of intermediate elements between the coupled or associated items absent specific contrary language.

[074] In the context of the present application, the terms “lower” and “upper” are used interchangeably with the terms “inflow” and “outflow”, respectively. Thus, for example, the lower end of the valve is its inflow end and the upper end of the valve is its outflow end.

[075] As used herein, the term “proximal” refers to a position, direction, or portion of a device that is closer to the user and further away from the implantation site. As used herein, the term “distal” refers to a position, direction, or portion of a device that is further away from the user and closer to the implantation site. Thus, for example, proximal motion of a device is motion of the device toward the user, while distal motion of the device is motion of the device away from the user. The terms “longitudinal” and “axial” refer to an axis extending in the proximal and distal directions, unless otherwise expressly defined.

[076] In view of the many possible embodiments to which the principles of the disclosure may be applied, it should be recognized that the illustrated embodiments are only preferred examples and should not be taken as limiting the scope of the disclosure. Rather, the scope of the disclosure is defined by the following claims.

What is claims is:

1. An implantable prosthetic valve that is radially collapsible to a collapsed configuration and radially expandable to an expanded configuration, the prosthetic valve comprising:
 - an annular frame having an inflow end and an outflow end;
 - a leaflet structure positioned within the frame and secured thereto; and
 - a laminate sealing member comprising an encapsulating material, the laminate sealing member having a main portion that encapsulates at least a portion of the frame and an end portion extending from the inflow end of the frame;wherein the end portion of the laminate sealing member is folded to form a cuff adjacent the inflow end of the frame and secured to the main portion of the laminate sealing member.
2. The assembly of claim 1, wherein the laminate sealing member comprises a first tubular layer positioned on the inside of the frame and a second tubular layer positioned on the outside of the frame, the first and second tubular layers being fused together to encapsulate corresponding portions of the frame.
3. The assembly of claim 2, wherein the first tubular layer, the second tubular layer, or both extend from the inflow end of the frame to form the cuff.
4. The assembly of claims 2 or 3, further comprising a reinforcing layer positioned adjacent the frame and encapsulated between the first and second tubular layers.
5. The assembly of claim 4, wherein the leaflet structure is sutured to the reinforcing layer.
6. The assembly of claim 4, wherein the reinforcing layer comprises a fabric.

7. The assembly of claim 4, wherein the reinforcing layer comprises a semi-crystalline polymeric material.

8. The assembly of any preceding claim, wherein the end portion of the laminate sealing member comprises extension portions secured to the main portion of the laminate sealing member.

9. The assembly of any preceding claim, wherein the end portion of the laminate sealing member is secured to the main portion of the laminate sealing member by heat bonding.

10. The assembly of any preceding claim, wherein the end portion of the laminate sealing member is secured to the main portion of the laminate sealing member by suturing.

11. The assembly of any preceding claim, wherein the laminate sealing member comprises a non-absorbable polymer selected from expanded polytetrafluoroethylene, unexpanded porous polytetrafluoroethylene, ultrahigh molecular weight polyethylene, or any combination thereof.

12. A method of making a prosthetic heart valve, comprising:
positioning a first layer about a mandrel;
positioning a radially expandable frame over the first layer;
positioning a second layer over the radially expandable frame;
fusing the first and second layers to form a monolithic laminate sealing member such that at least a portion of the frame is encapsulated within the laminate sealing member; and
folding an end portion of the laminate sealing member and securing it to a main portion of the laminate sealing member to form a cuff adjacent an inflow end of the

frame.

13. The method of claim 12, wherein the fusing further comprises:
 - applying pressure to force the second layer and the first layer into contact with one another; and
 - heating the first and second layers so that they fuse together to form the laminate sealing member encapsulating the frame.
14. The method of claims 12 or 13, further comprising positioning a reinforcing layer adjacent the frame between the first and second layers.
15. The method of claim 14, wherein the reinforcing layer comprises at least one of a fabric material, a textile material, or a semi-crystalline polymeric material.
16. The method of any of claims 12-15, wherein securing the end portion of the laminate sealing member to the main portion of the laminate sealing member further comprises heat bonding the end portion of the laminate sealing member to the main portion of the laminate sealing member.
17. The method of any of claims 12-16, wherein securing the end portion of the laminate sealing member to the main portion of the laminate sealing member further comprises suturing the end portion of the laminate sealing member to the main portion of the laminate sealing member.
18. The method of any of claims 12-17, wherein securing the end portion of the laminate sealing member to the main portion of the laminate sealing member further comprises securing extension portions of the end portion of the laminate sealing member to the main portion of the laminate sealing member.
19. The method of any of claims 12-18, further comprising situating a

valvular structure within the frame and securing the valvular structure to the laminate sealing member and the frame.

20. A transcatheter heart valve, comprising:

a radially expandable frame having an inflow end, an outflow end, and a laminate sealing

member comprising:

a non-fabric inner layer positioned inside of the frame;

a non-fabric outer layer positioned outside of the frame; and

a fabric layer positioned between the non-fabric inner layer and the non-fabric

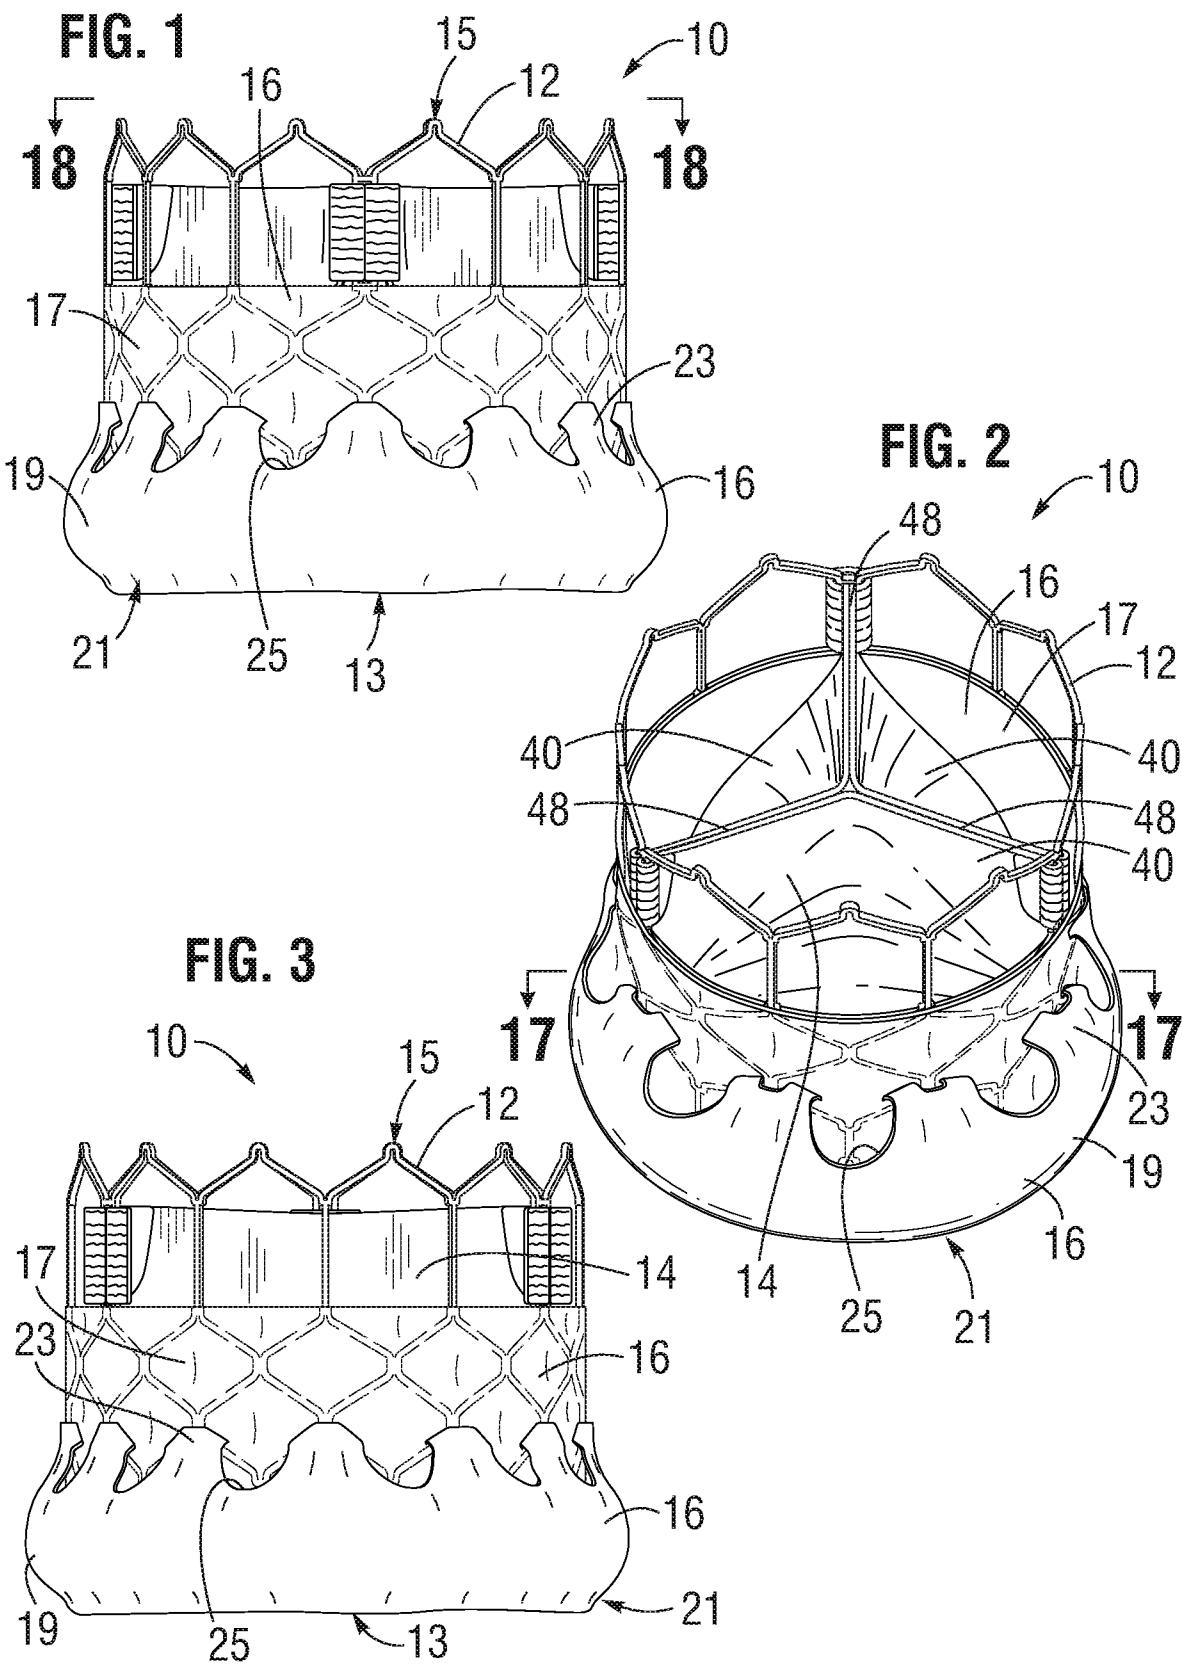
outer layer, the non-fabric inner and outer layers being fused to one another such that the

fabric layer and at least a portion of the frame are encapsulated therebetween;

wherein the laminate sealing member further comprises a main portion adjacent the frame

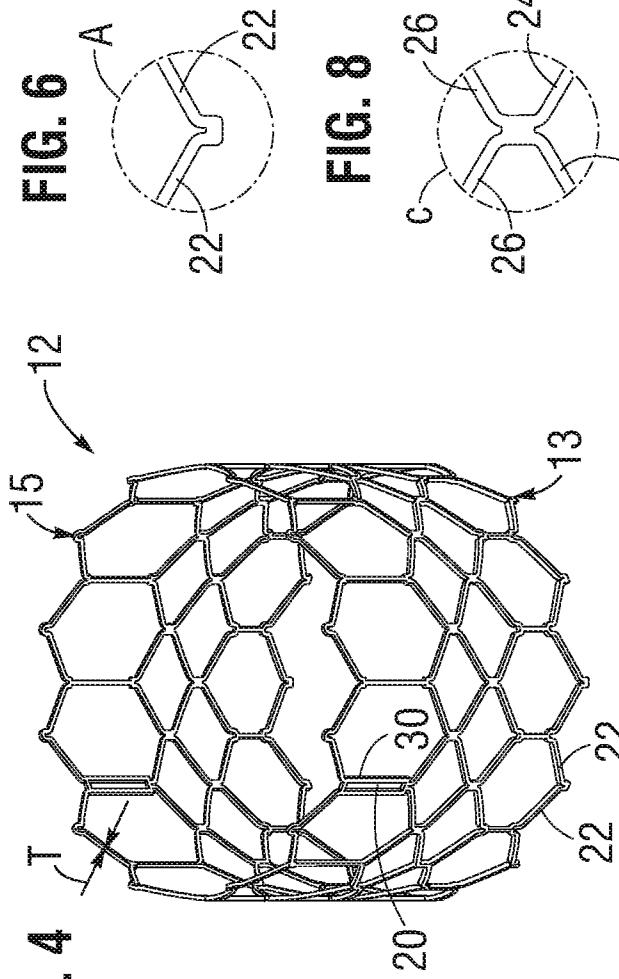
and an end portion extending from the inflow end of the frame, the end portion being folded to form a cuff adjacent the inflow end of the frame and secured to the main portion of the laminate sealing member.

1/9

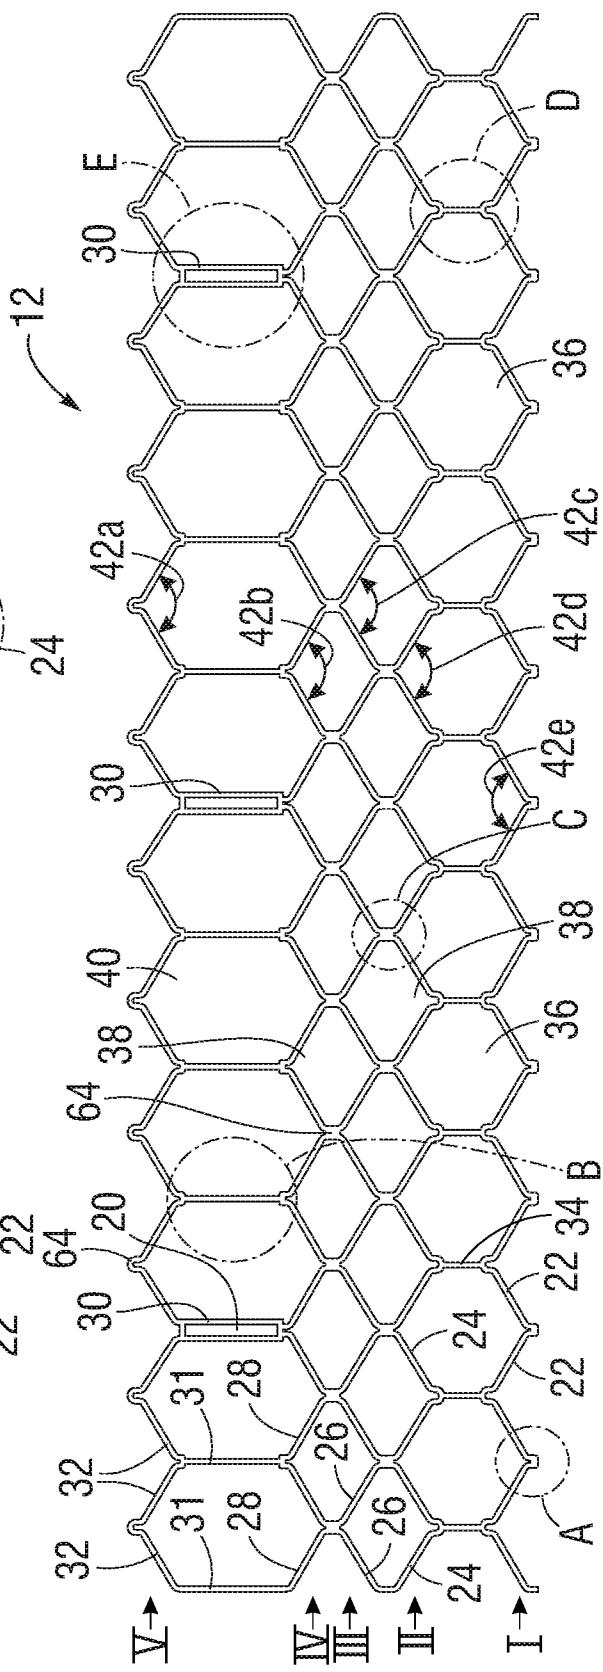


2/9

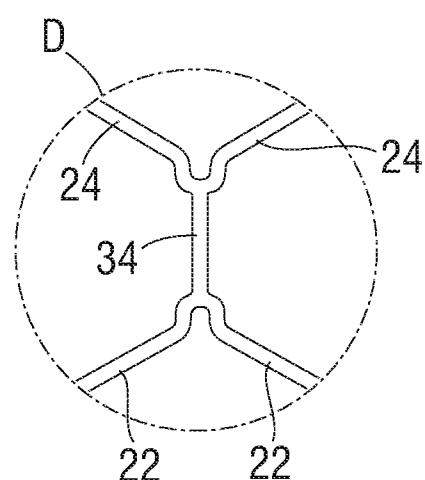
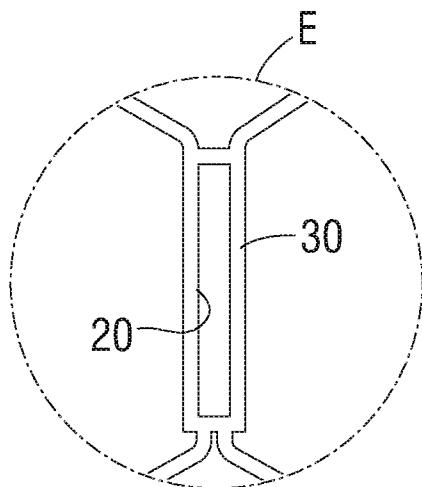
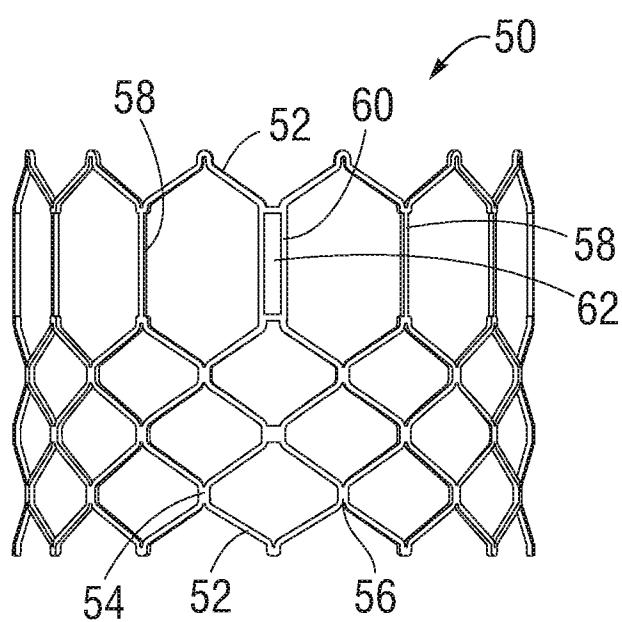
FIG. 4 T 15 12 FIG. 6



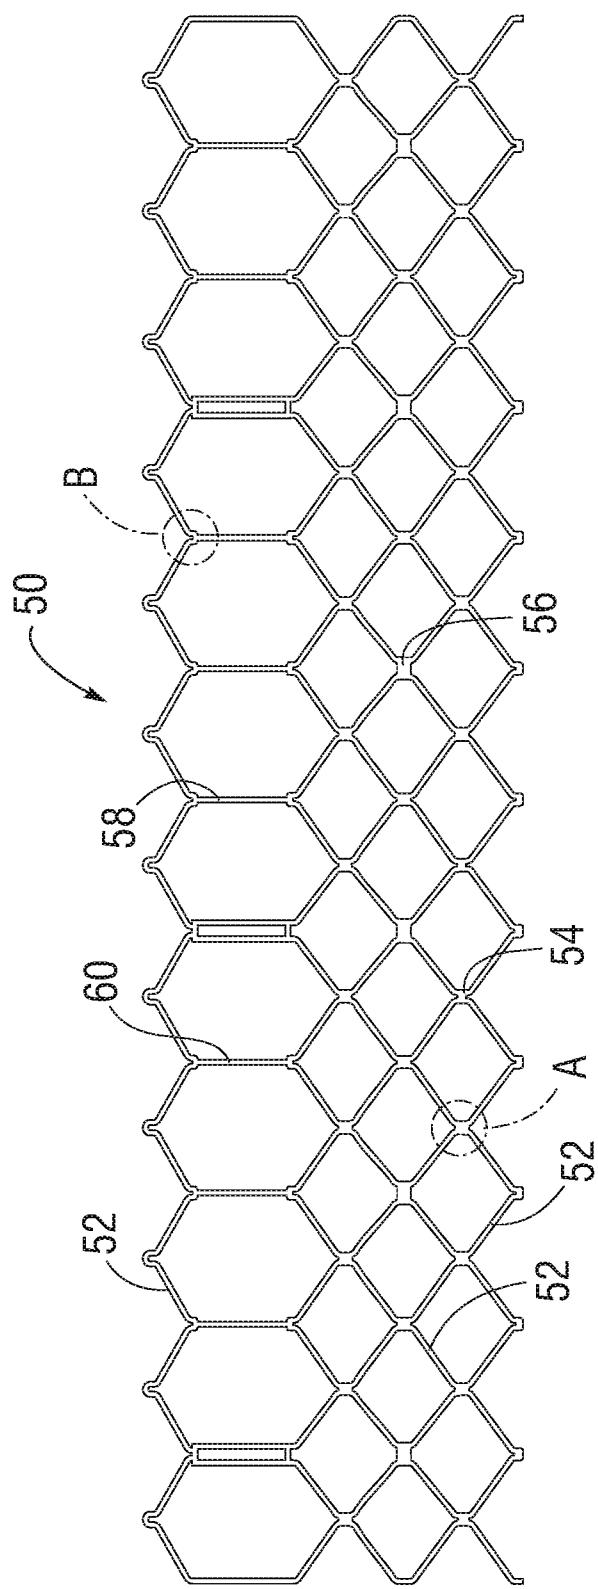
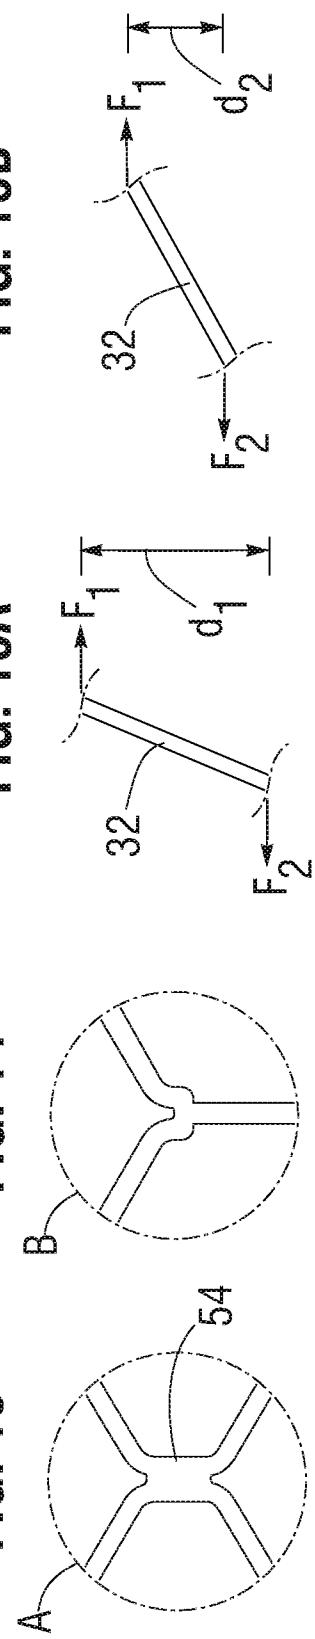
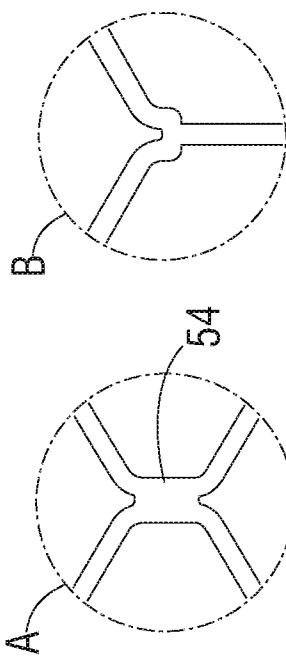
୬୮



3/9

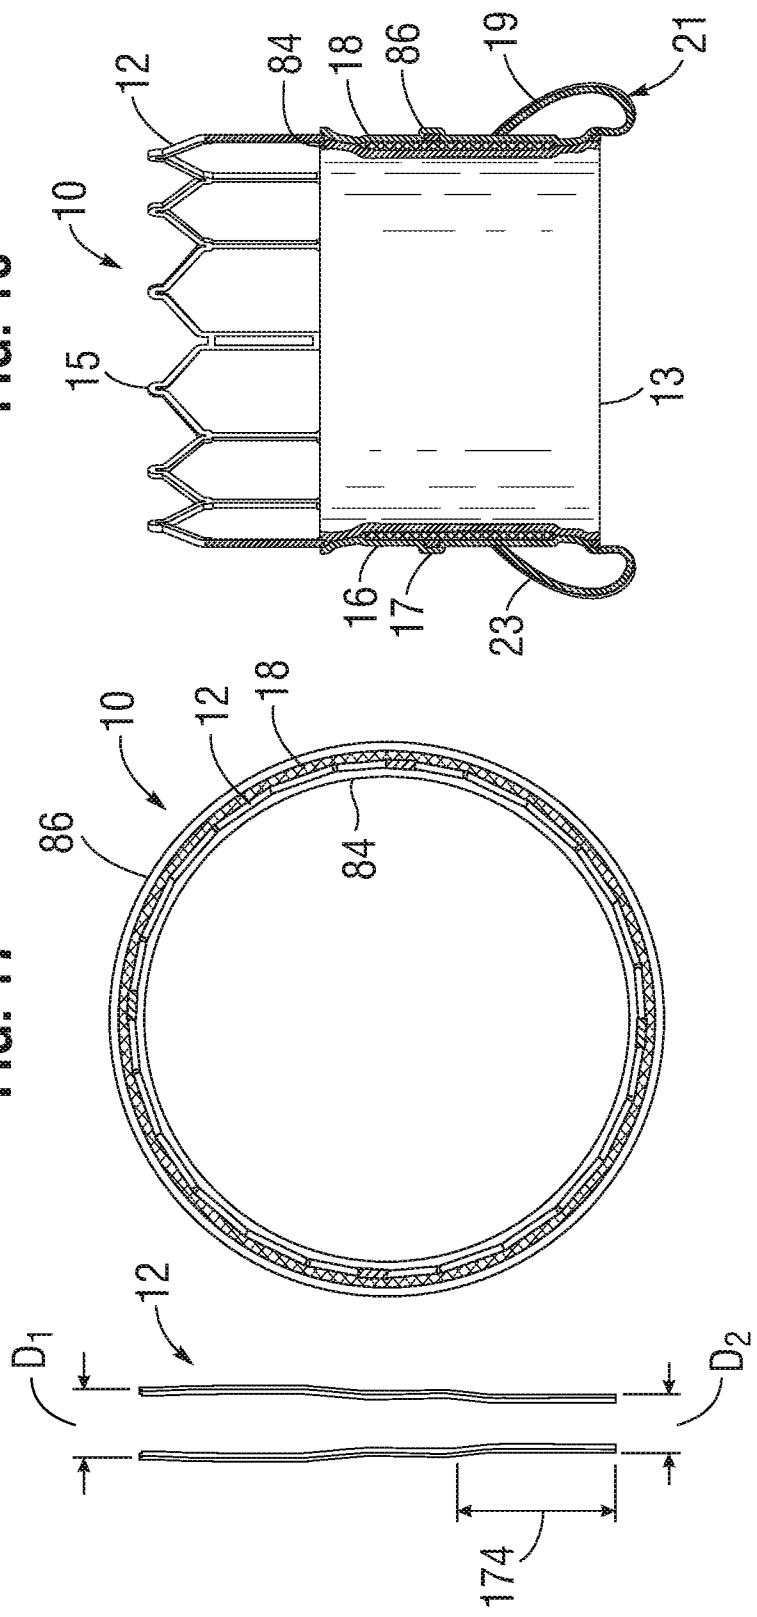
FIG. 9**FIG. 10****FIG. 11**

4/9

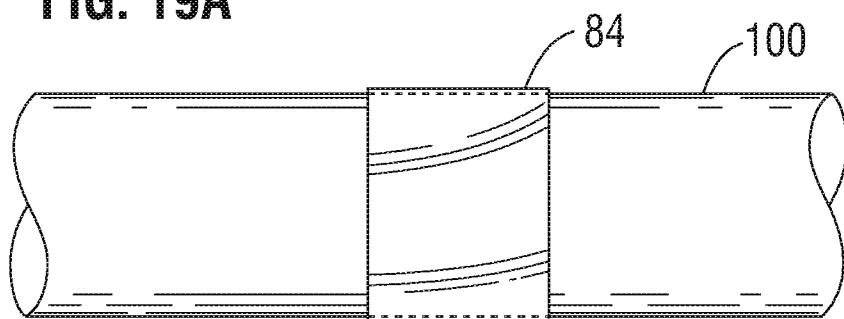
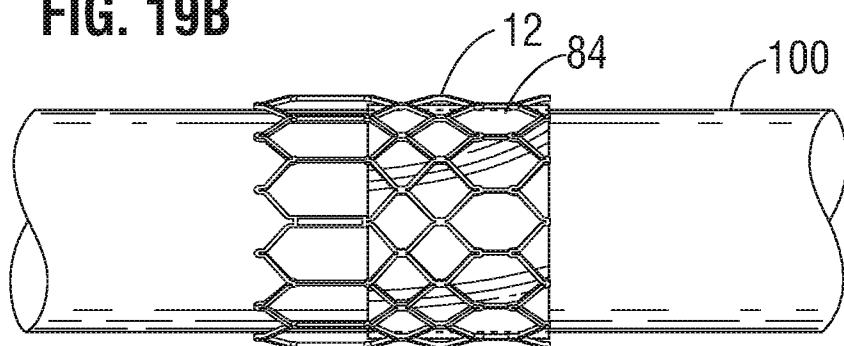
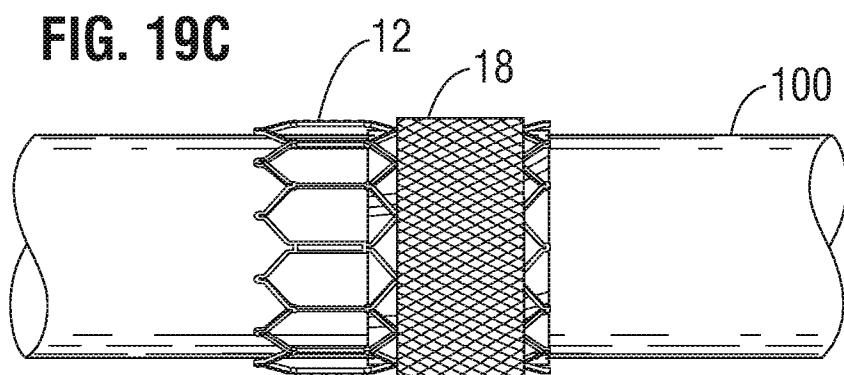
FIG. 12**FIG. 15A** **FIG. 15B****FIG. 14**

5/9

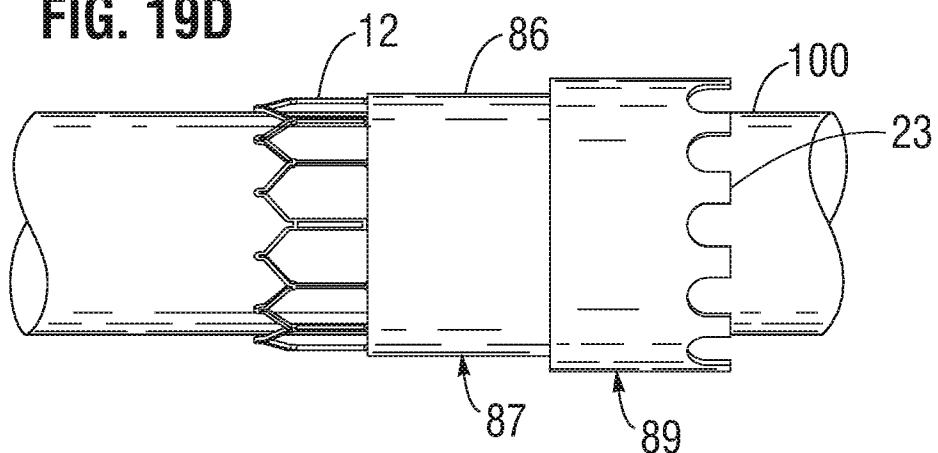
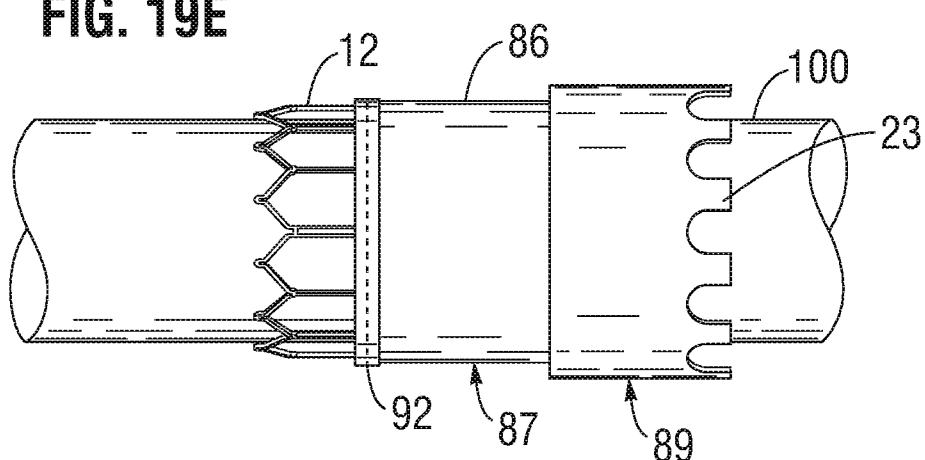
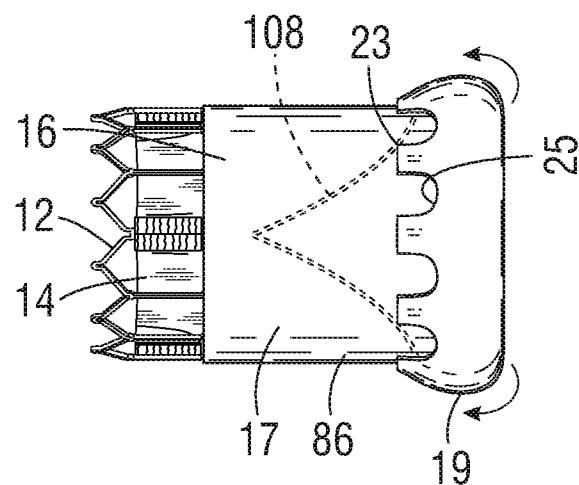
FIG. 16
FIG. 17
FIG. 18



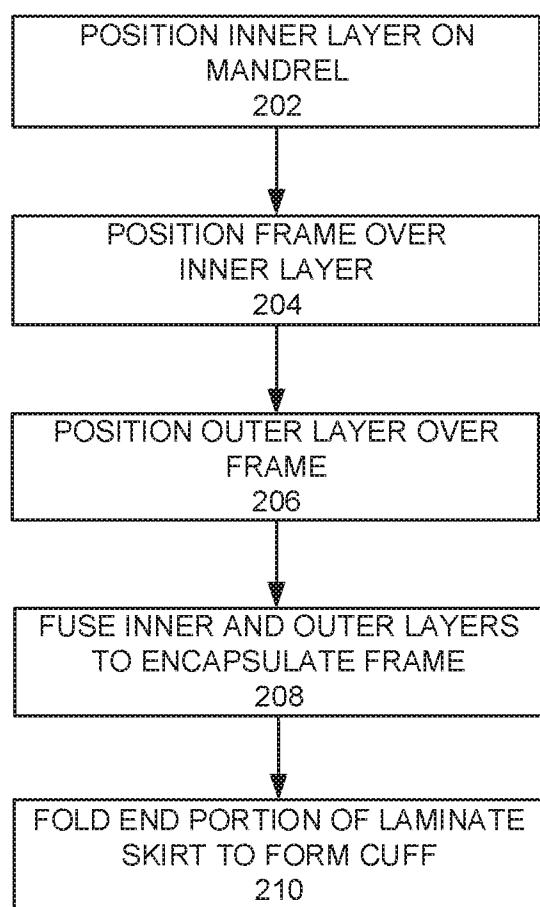
6/9

FIG. 19A**FIG. 19B****FIG. 19C**

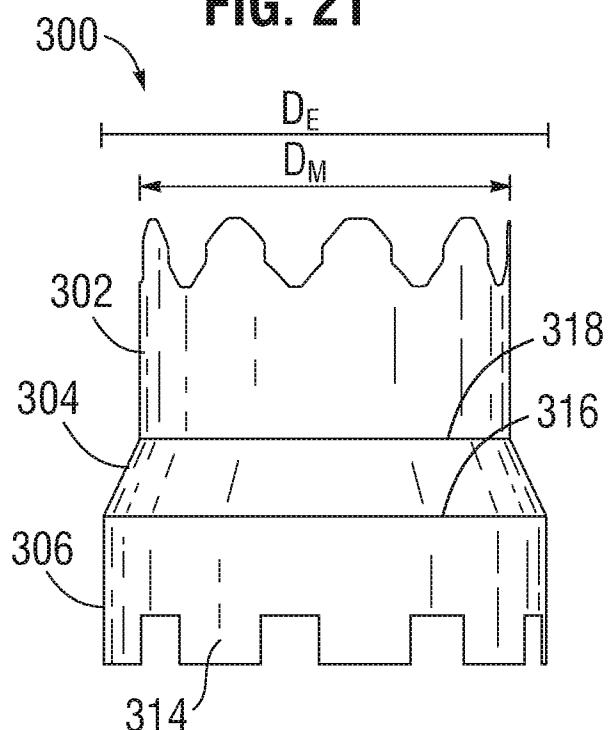
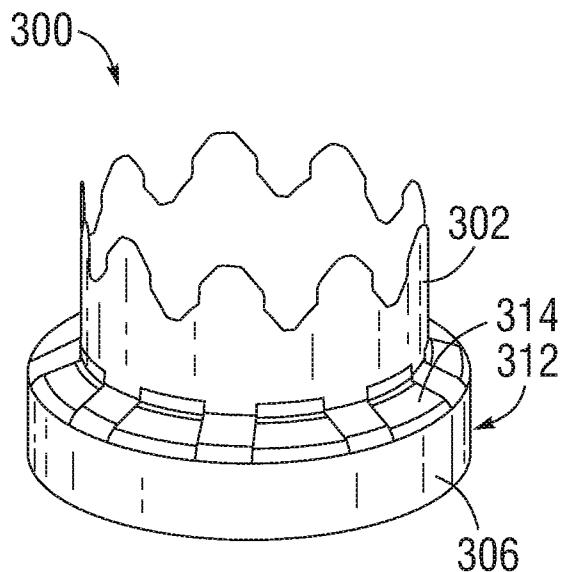
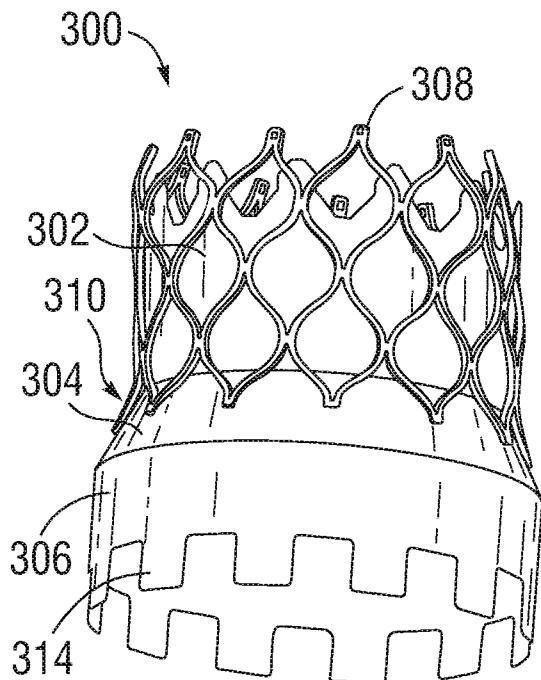
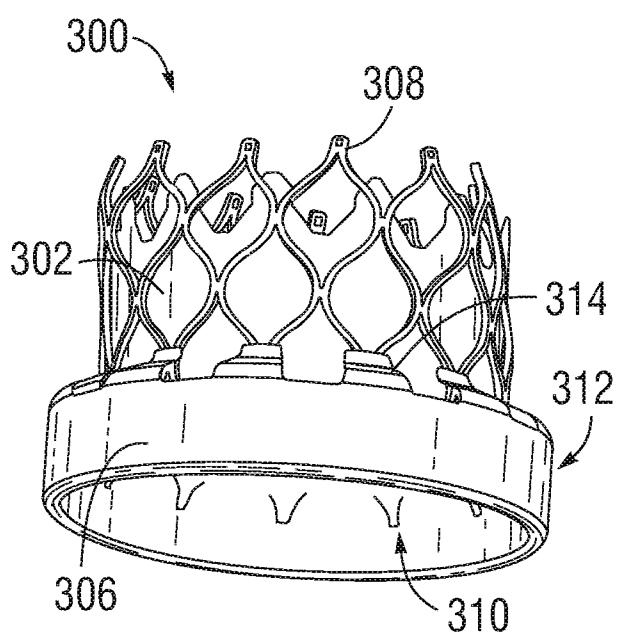
7/9

FIG. 19D**FIG. 19E****FIG. 19F**

8/9

**FIG. 20**

9/9

FIG. 21**FIG. 22****FIG. 23****FIG. 24**

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2016/029769

A. CLASSIFICATION OF SUBJECT MATTER

A61F 2/24(2006.01)I

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61F 2/24Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Korean utility models and applications for utility models
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)
eKOMPASS(KIPO internal) & Keywords: heart valve, sealing, encapsulation, cuff, skirt, fold, reinforce

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2014-0209238 A1 (EDWARDS LIFESCIENCES CORPORATION) 31 July 2014 See paragraphs [0034]–[0059]; claims 1–21; figures 1–6.	1–7, 12–15, 20
Y	US 2012-0123529 A1 (LEVI, T. et al.) 17 May 2012 See paragraphs [0051]–[0087]; claims 1–21; figures 1–56.	1–7, 12–15, 20
A	US 8403983 B2 (QUADRI, A. et al.) 26 March 2013 See column 6, line 7 – column 15, line 23; figures 1–13.	1–7, 12–15, 20
A	US 2013-0338765 A1 (ST. JUDE MEDICAL, INC.) 19 December 2013 See the whole document.	1–7, 12–15, 20
A	US 2014-0277402 A1 (SYMETIS SA) 18 September 2014 See the whole document.	1–7, 12–15, 20

 Further documents are listed in the continuation of Box C. See patent family annex.

- * Special categories of cited documents:
 "A" document defining the general state of the art which is not considered to be of particular relevance
 "E" earlier application or patent but published on or after the international filing date
 "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
 "O" document referring to an oral disclosure, use, exhibition or other means
 "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
 "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
 "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
 "&" document member of the same patent family

Date of the actual completion of the international search
29 July 2016 (29.07.2016)Date of mailing of the international search report
08 August 2016 (08.08.2016)Name and mailing address of the ISA/KR
International Application Division
Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea
Facsimile No. +82-42-481-8578

Authorized officer

Han, Inho

Telephone No. +82-42-481-3362



INTERNATIONAL SEARCH REPORTInternational application No.
PCT/US2016/029769**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.: because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.: because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. Claims Nos.: 8-11,16-19 because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2016/029769

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2014-0209238 A1	31/07/2014	CA 2835947 A1 CN 103732183 A EP 2709563 A1 US 2012-0296418 A1 US 8945209 B2 WO 2012-162228 A1	29/11/2012 16/04/2014 26/03/2014 22/11/2012 03/02/2015 29/11/2012
US 2012-0123529 A1	17/05/2012	AU 2011-312034 A1 AU 2011-312034 B2 CA 2813419 A1 CN 103237524 A CN 103237524 B EP 2624785 A2 JP 2013-543406 A WO 2012-048035 A2 WO 2012-048035 A3	02/05/2013 08/10/2015 12/04/2012 07/08/2013 20/01/2016 14/08/2013 05/12/2013 12/04/2012 19/07/2012
US 8403983 B2	26/03/2013	AU 2009-295960 A1 CA 2749026 A1 CN 102292053 A EP 2367505 A1 EP 2901966 A1 JP 2012-504031 A JP 2014-230797 A US 2010-0082094 A1 US 2013-0131788 A1 US 2013-0131793 A1 US 2013-0184813 A1 US 8894702 B2 WO 2010-037141 A1	01/04/2010 01/04/2010 21/12/2011 28/09/2011 05/08/2015 16/02/2012 11/12/2014 01/04/2010 23/05/2013 23/05/2013 18/07/2013 25/11/2014 01/04/2010
US 2013-0338765 A1	19/12/2013	AU 2009-271573 A1 AU 2009-271573 B2 EP 2299938 A2 EP 2815723 A1 EP 2815724 A1 EP 2815725 A1 EP 2815725 B1 JP 2011-528256 A JP 5379852 B2 US 2011-0098802 A1 US 2014-0350663 A1 US 2014-0350665 A1 US 2014-0350667 A1 US 2015-0216654 A1 US 2015-0216663 A1 US 8808356 B2 US 9220594 B2 US 9289296 B2	21/01/2010 11/09/2014 30/03/2011 24/12/2014 24/12/2014 24/12/2014 06/04/2016 17/11/2011 25/12/2013 28/04/2011 27/11/2014 27/11/2014 27/11/2014 06/08/2015 06/08/2015 19/08/2014 29/12/2015 22/03/2016

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2016/029769

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		WO 2010-008548 A2 WO 2010-008548 A3	21/01/2010 20/05/2010
US 2014-0277402 A1	18/09/2014	CA 2703665 A1 EP 2205183 A1 EP 2679198 A1 JP 2011-500241 A JP 2013-255843 A JP 2015-027557 A JP 5603776 B2 JP 5657076 B2 JP 5905948 B2 US 2011-0022157 A1 US 8647381 B2 WO 2009-053497 A1	30/04/2009 14/07/2010 01/01/2014 06/01/2011 26/12/2013 12/02/2015 08/10/2014 21/01/2015 20/04/2016 27/01/2011 11/02/2014 30/04/2009