

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
9 December 2010 (09.12.2010)

PCT

(10) International Publication Number
WO 2010/141921 A1(51) International Patent Classification:
C02F 1/40 (2006.01)(21) International Application Number:
PCT/US2010/037545(22) International Filing Date:
4 June 2010 (04.06.2010)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/184,759 5 June 2009 (05.06.2009) US
61/235,664 20 August 2009 (20.08.2009) US
61/349,680 28 May 2010 (28.05.2010) US(71) Applicant (for all designated States except US): **INTE-
GENX INC.** [US/US]; 5720 Stoneridge Drive, Suite 300,
Bldg. B, Pleasanton, CA 94588 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **JOVANOVIĆ, Stevan, B.** [US/US]; 723 Hazel Street, Livermore, CA 94550 (US). **NIELSEN, William, D.** [US/US]; 3860 Sophist Dr., San Jose, CA 95132 (US). **COHEN, David, S.** [US/US]; 2911 Crestmoor Dr., San Bruno, CA 94066 (US). **RECKNOR, Michael** [US/US]; 6153 Castle Drive, Oakland, CA 94611 (US). **VANGBO, Mattias** [US/US]; 36704 2nd St., Fremont, CA 94536 (US). **VAN GELDER, Ezra** [NL/US]; 532 Georgia Ave, Palo Alto, CA 94306 (US). **MAJLOF, Lars** [SE/US]; 4855 Atherton Avenue, Ste. 200, San Jose, CA 95130 (US). **EL-SISSI, Omar** [US/US]; 40120 Sentinel Drive, Fremont, CA 94539 (US).(74) Agents: **ROY, Madhuri** et al.; Wilson Sonsini Goodrich & Rosati, 650 Page Mill Road, Palo Alto, CA 94304-1050 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: UNIVERSAL SAMPLE PREPARATION SYSTEM AND USE IN AN INTEGRATED ANALYSIS SYSTEM

(57) Abstract: The invention provides a system that can process a raw biological sample, perform a biochemical reaction and provide an analysis readout. For example, the system can extract DNA from a swab, amplify STR loci from the DNA, and analyze the amplified loci and STR markers in the sample. The system integrates these functions by using microfluidic components to connect what can be macrofluidic functions. In one embodiment the system includes a sample purification module, a reaction module, a post-reaction clean-up module, a capillary electrophoresis module and a computer. In certain embodiments, the system includes a disposable cartridge for performing analyte capture. The cartridge can comprise a fluidic manifold having macrofluidic chambers mated with microfluidic chips that route the liquids between chambers. The system fits within an enclosure of no more than 10 ft³, and can be a closed, portable, and/or a battery operated system. The system can be used to go from raw sample to analysis in less than 4 hours.

WO 2010/141921 A1

**UNIVERSAL SAMPLE PREPARATION SYSTEM
AND USE IN AN INTEGRATED ANALYSIS SYSTEM**

CROSS-REFERENCE

[0001] This application is related to USSN 61/184,759 filed June 5, 2009 and USSN 61/235,664, filed August 20, 2009, which are incorporated herein by reference in their entirety for all purposes.

STATEMENT AS TO FEDERALLY SPONSORED RESEARCH

[0002] This invention was made with Government support under Contract No. 2004*H838109*000 awarded by the Central Intelligence Agency. The Government may have certain rights in this invention.

BACKGROUND OF THE INVENTION

[0003] Sample preparation is a ubiquitous problem in biological analytical systems. The issue of providing sufficiently purified targets from diverse raw sample types to reliably perform downstream analytical assays is pervasive and covers cell biology, genomics, proteomics, metabolomics, food biology, molecular diagnostics, and many other biological and medical assays. While many advances in sample preparation have been made the chief solution has been to develop reagents that are used manually or in robotic systems that use rectilinear stages or multi-axis arms to manipulate samples.

[0004] Microfluidics and nanofluidics allow miniaturized sample volumes to be prepared for analysis. Advantages include the nanoscale consumption of reagents to reduce operating costs and full automation to eliminate operator variances. Microfluidic sample preparation can either interface with existing or future detection methods or be part of a completely integrated system. In the present application, methods and apparatuses are disclosed that integrate full volume sample preparation with volumes over 10 mL with microliter and smaller volumes for sample preparation and analysis.

[0005] Starting from the sample, the present invention can be applied to concentrate, and pre-separate components for further processing to detect and classify organisms in matrices comprising aerosol samples, water, liquids, blood, stools, nasal, buccal and other swabs, bodily fluids, environmental samples with analysis by ELISA, PCR or other nucleic acid amplification techniques, single molecule detection, protein arrays, mass spectroscopy, and other analytical methods well known to one skilled in the art.

[0006] Microfluidic nucleic acid purification can be performed to prepare the sample for nucleic acid assays. For DNA analysis, PCR amplification is one current method. Microarray DNA, RNA and protein analysis also requires extensive sample preparation before the sample can be applied to the microarray for reaction and readout.

[0007] Samples can be obtained by a wide variety of substrates and matrices. The matrix may contain complex mixtures including inhibitory compounds such as hemes, indigo, humic acids, divalent cations, and proteins *etc* that interfere with DNA-based amplification. Aerosols can contain large amounts of molds, metals, and soils humic and other acids that all interfere with PCR amplification—the gold standard.

[0008] Early work showed that as few as three seeded organisms could be detected from diluted samples of soil extracts followed by PCR amplification of two 16S ribosomal gene fragments. Low-melting-temperature agarose has been used to extract DNA from soil samples for 16S and 18S rDNA PCR amplification using universal primers. Spun separation gels in column format can be used, such as Sephadex columns. Multistep purifications such as organic extractions combined with Sephadex columns were developed. Bead beating was found to be an effective way to prepare samples for high numbers of organisms and grinding in liquid nitrogen to detect low numbers of organisms. While these methods are effective they were best suited for research laboratory environments.

[0009] Solid phase extractions to columns, beads, and surfaces can be used to purify DNA before DNA analysis. Proteinase K followed by a Qiagen QIA Amp silica-gel membrane columns and IsoCode Stix, an impregnated membrane-based technology, followed by heating, washing and a brief centrifugation were compared for *B. anthracis* Sterne vegetative cells in buffer, serum, and whole blood and spores in buffer and found to work well.

[0010] A variety of separations can be performed using the devices and methods of the invention. For example, the devices and methods of the invention can be used to perform chromatography, phase-based or magnetic-based separation, electrophoresis, distillation, extraction, and filtration. For example, a microfluidic channel or a capillary can be used for chromatography or electrophoresis. As well, beads, such as magnetic beads can be used for phase-based separations and magnetic-based separations. The beads, or any other surfaces described herein, can be functionalized with binding moieties that exhibit specific or non-specific binding to a target. The binding can be based on electrostatics, van der Waals interactions, hydrophobicity, hydrophilicity, hydrogen bonding, ionic interactions, as well as partially covalent interactions like those exhibited between gold and sulfur. In preferred embodiments, the devices and methods of the invention utilize immunomagnetic separations.

[0011] Immunomagnetic separation (IMS) is a powerful technology that allows targets to be captured and concentrated in a single step using a mechanistically simplified format that employs paramagnetic beads and a magnetic field (see Grodzinski P, Liu R, Yang J, Ward MD. Microfluidic system integration in sample preparation microchip-sets - a summary. Conf Proc IEEE Eng Med Biol Soc. 2004;4:2615-8., Peoples MC, Karnes HT. Microfluidic immunoaffinity separations for bioanalysis. J Chromatogr B Analyt Technol Biomed Life Sci. 2007 Aug 30., and Stevens KA, Jaykus LA. Bacterial separation and concentration from complex sample matrices: a review. Crit Rev Microbiol. 2004; 30(1):7-24.). IMS can be used to capture, concentrate, and then purify specific target antigens, proteins, toxins, nucleic acids, cells, and spores. While IMS as originally used referred to using an antibody, we generalize its usage to include other specific affinity interactions including lectins, DNA-DNA, DNA-RNA, biotin-streptavidin, and other affinity interactions that are coupled to a solid phase. IMS works by binding a specific affinity reagent, typically an antibody or DNA, to paramagnetic beads which are only magnetic in the presence of an external magnetic field. The beads can be added to complex samples such as aerosols, liquids, bodily fluids, or food. After binding of the

target to the affinity reagent (which itself is bound to the paramagnetic bead) the bead is captured by application of a magnetic field. Unbound or loosely bound material is removed by washing with compatible buffers, which purifies the target from other, unwanted materials in the original sample. Because beads are small (about 1 nm to about 1 μ m) and bind high levels of target, when the beads are concentrated by magnetic force they typically form bead beds of between 1 nL and 1 μ L, thus concentrating the target at the same time it is purified. The purified and concentrated targets can be conveniently transported, denatured, lysed or analyzed while on-bead, or eluted off bead for further sample preparation, or analysis.

[0012] Immunomagnetic separations are widely used for many applications including the detection of microorganisms in food, bodily fluids, and other matrices. Paramagnetic beads can be mixed and manipulated easily, and are adaptable to microscale and microfluidic applications. This technology provides an excellent solution to the macroscale-to-microscale interface: beads are an almost ideal vehicle to purify samples at the macroscale and then concentrate to the nanoscale (100's of nL) for introduction into microfluidic or nanofluidic platforms. Immunomagnetic separations are commonly used as an upstream purification step before real-time PCR, electrochemiluminescence, and magnetic force discrimination.

[0013] The ability to move fluids on microchips is a quite important. This invention describes technologies in sample capture and purification, micro-separations, micro-valves, -pumps, and -routers, nanofluidic control, and nano-scale biochemistry. A key component of the technology is Micro-robotic On-chip Valves (MOVE) technology (an example of which is shown in **Figure 1**) and its application to miniaturize and automate complex workflows. Collectively the MOVE valves, pumps, and routers and the instrumentation to operate them can be referred to as a microchip fluid processing platform.

[0014] The heart of the microchip fluid processing platform technology are MOVE pumps, valves, and routers that transport, process, and enable analysis of samples. These novel externally actuated, pneumatically-driven, on-chip valves, pumps, and routers, originally developed in the Mathies laboratory at the University of California at Berkeley (U. C. Berkeley) (Grover, W.H. A. M. Skelley, C. N. Liu, E. T. Lagally, and R. M. Mathies. 2003. *Sensors and Actuators* B89:315-323; Richard A. Mathies et al., United States Patent Application, 20040209354 A1 October 21, 2004; all of which are herein incorporated by reference in their entirety) can control fluidic flow at manipulate volumes from 20 nL to 10 μ L.

[0015] The MOVE valves and pumps (**Figure 1**) can combine two glass and/or plastic microfluidic layers with a polydimethyl siloxane (PDMS) deformable membrane layer that opens and closes the valve, and a pneumatic layer to deform the membrane and actuate the valve. The microfluidic channel etched in the top glass fluidic wafer is discontinuous and leads to a valve seat which is normally closed (**Figure 1A**). When a vacuum is applied to the pneumatic displacement chamber by conventional-scale vacuum and pressure sources, the normally closed PDMS membrane lifts from the valve seat to open the valve (**Figure 1B**). **Figure 1C** shows a top view of the valve a similar scale as the other panels.

[0016] Three microvalves can be used to make a micropump on a microchip to move fluids from the Input area to the Output area on Microchip A. The fluids are moved by three or more valves. The valves

can be created actuation of a deformable structure. In some implementations a valve seat is created and in other embodiments no valve seat may be needed. **Figure 2** shows MOVE devices from top to bottom: valve, router, mixer, bead capture. Self-priming MOVE pumps (**Figure 2**, top) are made by coordinating the operation of three valves and can create flow in either direction. Routers are made from three or more MOVE valves (**Figure 2**, top middle panel). Mixing has been a holy grail for microfluidics: MOVE mixers (**Figure 2**, bottom middle panel) rapidly mix samples and reagents. MOVE devices work exquisitely with magnetic beads to pump or trap sets of beads (**Figure 2**, bottom panel).

[0017] The normally closed MOVE valves, pumps, and routers are durable, easily fabricated at low cost, can operate in dense arrays, and have low dead volumes. Arrays of MOVE valves, pumps, and routers are readily fabricated on microchips. Significantly, all the MOVE valves, pumps, and routers on a microchip are created at the same time in a simple manufacturing process using a single sheet of PDMS membrane—it costs the same to make 5 MOVE micropumps on a microchip as to create 500. This innovative technology offers for the first time the ability to create complex micro- and nanofluidic circuits on microchips.

[0018] Patents and applications which discuss the use and design of microchips include US 7,312,611, issued on December 25, 2007; US Patent 6,190,616, issued on February 20, 2001; U.S. Patent 6,423,536, issued on July 23, 2002; US patent 10,633,171 March 22, 2005; US Patent 6,870,185, issued on March 22, 2005 US Application No. US 2001-0007641, filed on January 25, 2001; US Application US20020110900, filed on April 18, 2002; US patent application 20070248958, filed September 15, 2005; US patent application US 20040209354, filed on December 29, 2003; US patent application US2006/0073484, filed on December 29, 2003; US20050287572, filed on May 25, 2005; US patent application US20070237686, filed on March 21, 2007; US 20050224352 filed on November 24, 2004; US 20070248958, filed on, September 15, 2005; US 20080014576, filed on February 2, 2007; and, US application US20070175756, filed on July 26, 2006; all of which are herein incorporated by reference in their entirety.

SUMMARY OF THE INVENTION

[0019] The invention provides a system that can process a raw biological sample, perform a biochemical reaction and provide an analysis readout in multiplex. For example, the system can extract DNA from a swab, amplify STR loci from the DNA, and analyze the amplified loci and STR markers in the sample. The system integrates these functions by using microfluidic components to connect what can be macrofluidic functions. In one embodiment the system includes a sample purification module, a reaction module, a post-reaction clean-up module, a capillary electrophoresis module and a computer. In certain embodiments, the system includes a disposable cartridge for performing analyte capture. The cartridge can comprise a fluidic manifold having macrofluidic chambers mated with microfluidic chips that route the liquids between chambers. The system fits within an enclosure of no more than 10 ft³. and can be a closed, portable, and/or battery operated system. The system can be used to go from sample to analysis in less than 4 hours.

[0020] In one aspect, this invention provides a system that fits within an enclosure of no more than 10 ft³, the system comprising: (a) a sample preparation module adapted to capture an analyte from a non-microfluidic volume on a capture particle and route the captured analyte through a microfluidic channel; (b) a reaction module comprising a reaction chamber in fluidic communication with the microfluidic channel adapted to immobilize the captured analyte and perform a biochemical reaction on the analyte in a non-microfluidic volume to produce a reaction product; (c) and an analysis module in fluidic communication with the reaction chamber adapted to perform an analysis on the reaction product. In one embodiment, the system is configured to capture the analyte, perform a biochemical reaction on the analyte, and perform an analysis on the product in less than 4 hours, in less than 3 hours, or even in less than 2 hours. In one embodiment, the system further comprises a data analysis module configured to receive data about the analysis from the analysis module and comprising executable code that transforms the data and outputs a result of the analysis. In another embodiment, the system further comprises a processing module in fluidic communication with the reaction chamber and the analysis module and adapted to (1) route the reaction product through a second microfluidic channel into a non-microfluidic processing chamber; (2) process the reaction product and (3) route the processed reaction product into the analysis module. In one particular embodiment, the system fits within an enclosure of no more than 8 ft³, no more than 5 ft³ or no more than 2 ½ ft³. In another embodiment of the system, the sample preparation module is adapted to release the analyte from a cell. In another embodiment of the system, the capture particle is a magnetically responsive capture particle and a reaction module comprises a source of magnetic force configured to immobilize the captured analyte. In another embodiment of the system, the reaction module is adapted to perform thermal cycling. In another embodiment of the system, the system is a closed system and/or battery operated.

[0021] In another aspect, this invention provides a system comprising a cartridge cover, a cartridge and a pneumatic manifold wherein the cartridge can be releaseably engaged with the cartridge cover and the pneumatic manifold, wherein the cartridge comprises one or more pneumatically actuated valves and one or more microfluidic channels, wherein the pneumatic manifold and the cartridge cover are each fluidically connected to at least one pressure source, and wherein the pneumatic manifold and the cartridge cover are each adapted to control fluid flow within the cartridge. In one embodiment, the pneumatic manifold is adapted to actuate the pneumatically actuated valves and the cartridge cover is adapted to apply pressure to one or more chambers in the cartridge.

[0022] In another aspect, this invention provides a system comprising: (a) a disposable cartridge comprising at least one set of fluidic chambers including a sample chamber, a mixing chamber and a thermal cycling chamber in fluid communication with each other, and a reagent card comprising reagents for performing a chemical reaction involving thermal cycling, wherein the reagent card is configured to be carried on the cartridge in a closed configuration and to be moved into fluid communication with the at least one set of fluidic chambers; (b) an actuator assembly configured to move fluids between chambers when the cartridge is engaged with the actuator assembly; (c) a thermal cycler configured to cycle temperature in the thermal cycling chamber when the cartridge is engaged with the actuator assembly; (d) a capillary

electrophoresis assembly configured to accept a sample from cartridge when the cartridge is engaged with the actuator assembly and to perform capillary electrophoresis on the sample; and (e) a computerized control system configured to control the actuator assembly, the thermal cycler and the capillary electrophoresis assembly.

[0023] In another aspect, this invention provides a cartridge comprising: (a) a fluidic manifold comprising a fluidic side and a reagent card side wherein the fluidic manifold comprises: (i) at least one set of fluidic chambers, each chamber comprising a port on the fluidic side; (ii) at least one of thermal cycling chamber comprising at least one port; (iii) at least one of exit port; (iv) a slot on the reagent card side adapted to engage a reagent card, wherein the slot comprises a plurality of slot channels comprising cannulae on the reagent card side and communicating between the two sides; (b) at least one microfluidic chip comprising: at least one fluidic circuit; (ii) a plurality of ports in fluid communication with the fluidic circuit; (iii) at least one pneumatically activated diaphragm valve configured to regulate fluid flow within the fluidic circuit; wherein the at least one chip is engaged with the fluidic manifold so that the ports in the at least one chip are in fluid communication with the ports of the chambers and the slot channels wherein each fluidic chamber is in fluid communication with at least one other fluidic chamber and each cannula is in communication with a fluidic chamber; and (c) a reagent card engaged with the slot, wherein the card comprises a plurality of reagent chambers comprising reagents, each aligned with at least one of the cannulae and adapted to take a first engagement position wherein the reagent chambers are not punctured by the cannulae and a second engagement position wherein the reagent chambers are punctured by the cannulae, thereby putting the reagent chambers in fluid communication with the fluidic circuit. In one embodiment the reagents comprise reagents for performing PCR. In another embodiment, the reagents comprise primers for amplifying a plurality of short tandem repeats. In another embodiment, the at least one set of fluidic chambers is a plurality of sets of fluidic chambers. In yet another embodiment the cartridge is such that the fluidics manifold further comprises at least one auxiliary fluidic channel on the fluidic side of the manifold, the at least one chip is a plurality of chips and fluidic circuits in each of the plurality of chips are in fluidic communication with fluidic circuits of at least one other chip through the auxiliary fluidic channel. In this embodiment, the cartridge can further comprise a gasket between the chips and the manifold, wherein the gasket seals the channels on the manifold. In another embodiment of the cartridge, the fluidic chambers comprise a distribution chamber, a capture chamber, a sample chamber, and a clean-up chamber. In another embodiment of the cartridge, at least one fluidic chamber comprises magnetically responsive particles. In another embodiment of the cartridge, the at least one set of fluidic chambers is at least 4 sets or at least 8 sets. In another embodiment of the cartridge, the chips comprise at least one diaphragm valve.

[0024] In another aspect, the invention provides a system comprising: (a) a pneumatic assembly comprising: (i) a pneumatic manifold adapted to removably engage the cartridge on the fluidic side, wherein the pneumatic manifold comprises a plurality of pneumatic ports configured to engage pneumatic channels in the at least one microfluidic chip and activate the diaphragm valves; and (ii) a pressure source configured to supply positive or negative pressure to the pneumatic channels; (b) a cartridge activation assembly adapted to

engage the cartridge on the reagent card side; wherein the cartridge activation assembly comprises: (i) a reagent pneumatic manifold comprising a pneumatic side and reagent card side, wherein the reagent pneumatic manifold comprises reagent pneumatic manifold channels communicating between the two sides and comprising a cannula on the reagent card side; (ii) a pressure source configured to supply positive or negative pressure to the reagent pneumatic manifold channels; and (iii) a clamp configured to move the reagent card from the first engagement position to the second engagement position, wherein clamping results in the cannulae of the reagent pneumatic manifold puncturing the reagent chambers and putting the reagent chambers in communication with the pressure source; (c) a thermal cycler configured to cycle temperature in the at least one thermal cycling chamber when the cartridge is clamped; (d) a capillary electrophoresis assembly comprising: (i) at least one separation channel fluidically engaged with the exit port when the cartridge is clamped; and (ii) an optical sub-assembly configured to detect signal from the at least one separation channel; and (e) a computerized control system configured to control pneumatic assembly, the cartridge activation assembly, the thermal cycler and the capillary electrophoresis assembly. In one embodiment of this system, clamping seals the chamber ports and the slot channels with the at least one microfluidic chip. In another embodiment of this system, the cartridge activation assembly further comprises at least one heater configured to heat at least one of the fluidic chambers when the reagent pneumatic manifold is engaged with the cartridge. In another embodiment of this system, the cartridge activation assembly further comprises movable magnets configured to move into and out of a position wherein the magnets exert a magnetic force on at least one fluidic chamber. In another embodiment of this system, the cartridge activation assembly further comprises sensors configured to detect the presence of a sample in a sample chamber of the fluidic manifold. In another embodiment of this system, the thermal cycler comprises a Peltier device. In one embodiment the system is comprised in a portable case. In one specific embodiment, the case has an internal volume of no more than 10 ft³ or no more than 2 ½ ft³. In a related embodiment of system, the invention provides for an article in computer readable form comprising code for the operating system.

[0025] In another aspect the invention provides a method comprising: producing, from a sample comprising at least one cell comprising DNA, a computer file identifying a plurality of STR markers in the DNA, wherein the method is performed in less than 4 hours. In one embodiment the method is performed in less than 3 hours. In another embodiment the method is performed in less than 2 hours. In a related embodiment, the producing comprises extracting the DNA from the at least one cell, amplifying the STR markers from the DNA, performing capillary electrophoresis on the amplified markers, detecting the amplified markers, and performing computer analysis on the detected amplified markers to identify the markers. In one embodiment, the plurality of STR markers is at least 5 STR markers. In another embodiment the plurality of markers are CODIS STR markers. In a related embodiment, the plurality of STR markers is at least 5, 10, or 13 CODIS STR markers. In these embodiments, the at least one cell can be a plurality of cells. In some embodiments, the sample is a forensic sample. In specific embodiments, the

method is performed at the site of a sample collection. The sample can comprise blood, or can comprise a cheek swab. The method can be carried out by any system described herein.

[0026] In a related aspect, the invention provides a system configured to perform a method, wherein the method comprises: producing, from a sample comprising at least one cell comprising DNA, a computer file identifying a plurality of STR markers in the DNA, wherein the method is performed in less than 4 hours.

[0027] In another aspect, this invention provides a method comprising: (a) providing a system comprising: (i) a disposable cartridge comprising at least one set of fluidic chambers including a sample chamber, a mixing chamber and a thermal cycling chamber in fluid communication with each other, and a reagent card comprising reagents for performing a chemical reaction involving thermal cycling, wherein the reagent card is configured to be carried on the cartridge in a closed configuration and to be moved into fluid communication with the at least one set of fluidic chambers; (ii) an actuator assembly configured to move fluids between chambers when the cartridge is engaged with the actuator assembly; (iii) a thermal cycler configured to cycle temperature in the thermal cycling chamber when the cartridge is engaged with the actuator assembly; (iv) a capillary electrophoresis assembly configured to accept a sample from cartridge when the cartridge is engaged with the actuator assembly and to perform capillary electrophoresis on the sample; and (v) a computerized control system configured to control the actuator assembly, the thermal cycler and the capillary electrophoresis assembly; (b) moving of the reagent card into fluid communication with at least one set of fluidic chambers; (c) providing a sample comprising a nucleic acid molecule to a sample chamber; and (d) operating the system to amplify and detect at least one nucleic acid sequence in the sample. In one embodiment the time it takes to go from step (b) to step (d) is less than 4 hours. In one embodiment, the method comprises providing each of a plurality of samples to a different sample chamber. In another embodiment, the method comprises amplifying and detecting a plurality of nucleic acid sequences in the sample. In a related embodiment, the plurality of nucleic acid sequences comprise short tandem repeats (STRs). In a specific embodiment, the short tandem repeats comprise a plurality of Combined DNA Index System (CODIS) markers. In another embodiment the CODIS markers comprise a plurality of markers selected from AMEL, D3S1358, THO1, D21s11, D18s51, D5s818, D13s317, D7s820, D16s539, CSF1PO, vWA, D8S1179, TPOX and FGA. In one embodiment, the system comprises: (a) a pneumatic assembly comprising: (i) a pneumatic manifold adapted to removably engage the cartridge on the fluidic side, wherein the pneumatic manifold comprises a plurality of pneumatic ports configured to engage pneumatic channels in the at least one microfluidic chip and activate the diaphragm valves; and (ii) a pressure source configured to supply positive or negative pressure to the pneumatic channels; (b) a cartridge activation assembly adapted to engage the cartridge on the reagent card side; wherein the cartridge activation assembly comprises: (i) a reagent pneumatic manifold comprising a pneumatic side and reagent card side, wherein the reagent pneumatic manifold comprises reagent pneumatic manifold channels communicating between the two sides and comprising a cannula on the reagent card side; (ii) a pressure source configured to supply positive or negative pressure to the reagent pneumatic manifold channels; and (iii) a clamp configured to move the reagent card from the first engagement position to the second engagement position, wherein

clamping results in the cannulae of the reagent pneumatic manifold puncturing the reagent chambers and putting the reagent chambers in communication with the pressure source; (c) a thermal cycler configured to cycle temperature in the at least one thermal cycling chamber when the cartridge is clamped; (d) a capillary electrophoresis assembly comprising: (i) at least one separation channel fluidically engaged with the exit port when the cartridge is clamped; and (ii) an optical sub-assembly configured to detect signal from the at least one separation channel; and (e) a computerized control system configured to control pneumatic assembly, the cartridge activation assembly, the thermal cycler and the capillary electrophoresis assembly. In another embodiment, the system is any system named herein. In one embodiment, the sample is a forensic sample. In a related embodiment, the sample is selected from a buccal swab, blood, hair or semen. In another embodiment, the sample is a raw sample. In some embodiments, the method further comprises transporting the system to a forensic site.

[0028] In another aspect, the invention provides an optical system comprising: (a) a plurality of optically transparent channels; (b) a light source configured to direct to the plurality of optically transparent channels; (c) a dispersive element that disperses light passing through the optically transparent channels in a wavelength dependent manner; and (d) a detector configured to receive the dispersed light. In one embodiment the plurality of optically transparent channels comprises at least eight capillaries. In another embodiment the optically transparent channels are aligned in a first plane and the dispersive element disperses light along a second plane, wherein the first plane and the second plane are different. In another embodiment, the first plane is orthogonal to the second plane.

[0029] In another aspect, the invention provides an optical system comprising: (a) an excitation source configured to direct excitation light to an object; (b) a carrier for an object, wherein the object emits light other than excitation light when excited by the excitation energy; (c) a rejection filter configured to filter out excitation energy and to allow transmission of the emitted light; (d) an imaging lens configured to focus the emitted light; (e) a dichroic mirror substantially transparent to the excitation energy and configured to reflect emitted light to a detector; (f) a focusing system comprising at least one lens configured to focus light reflected from the dichroic mirror; and (g) a photodetector (CCD camera) configured to receive the reflected light. In one embodiment of the optical system, the excitation light comprises light of a wavelength between 0.3 microns and 1 micron. In another embodiment, the carrier comprises an array of capillary tubes and the object comprises a fluorescent species. In another embodiment, the mirror reflects emitted light and an angle between about 5 degrees and about 10 degrees off an incident angle. In another embodiment, the dichroic mirror further comprises a portion that transmits substantially all light. In another embodiment, the focusing system comprises at least one folding mirror. In another embodiment, the photodetector comprises a CCD camera. In a related embodiment, the optical system can further comprise a prism located between the object and the imaging lens.

[0030] In another aspect, the invention provides an optical system comprising: (a) an array of capillary tubes aligned substantially parallel and substantially in a plane; (b) an excitation assembly comprising an

excitation source and configured to deliver excitation light from the excitation source to the array, wherein the light delivery assembly is configured (i) to deliver a thin band of light that covers the array and (ii) to deliver the light to the array at an angle other than 90 degrees to the plane; (c) a collection lens configured to collect light emitted from the array by objects in the array excited by the excitation light; wherein the excitation assembly and the collection lens are configured with respect to the array so that excitation light passing through the array substantially avoids collection by the collection lens. In one embodiment, the angle is between about 10 degrees and about 85 degrees.

[0031] In another aspect, the invention provides an instrument comprising: (a) a microfluidic component comprising a plurality of intersecting microfluidic channels and at least one controllable valve configured to regulate flow of fluid between the intersecting channels; and (b) a non-microfluidic component comprising a plurality of non-microfluidic chambers, wherein each non-microfluidic chamber is fluidically connected to at least one of the microfluidic channels; wherein the instrument is configured to flow fluid from at least one non-microfluidic chamber into another non-microfluidic chamber through a microfluidic channel and flow is regulated by at least one valve. In one embodiment of the instrument, the plurality of non-microfluidic chambers comprises at least three chambers and the at least one valve selectively directs fluid from one chamber to either of the at least two other chambers. In another embodiment, the instrument further comprises a pump to pump fluid from a non-microfluidic chamber into a microfluidic channel. In another embodiment of the instrument the at least one valve is a diaphragm valve. In a related embodiment, the pump is a diaphragm pump comprising a series of three diaphragm valves. In another embodiment, the microfluidic component comprises a monolithic device. In another embodiment, the combination of the microfluidic component and the non-microfluidic component define a fluidic circuit and the instrument comprises a plurality of fluidic circuits. In another embodiment, the non-microfluidic component further comprises a particulate capture agent. In another embodiment, the particles are responsive to a magnetic field and the instrument further comprises a magnet configured to immobilize the particles. In another embodiment, the invention provides a device comprising a plurality of non-microfluidic chambers fluidically connected to a common microfluidic channel.

[0032] In another aspect, the invention provides a method comprising: (a) providing a device comprising: (i) a microfluidic component comprising a plurality of intersecting microfluidic channels and at least one controllable valve configured to regulate flow of fluid between the intersecting channels; and (ii) a non-microfluidic component comprising a plurality of non-microfluidic chambers, wherein each non-microfluidic chamber is fluidically connected to at least one of the microfluidic channels; wherein the instrument is configured to flow fluid from at least one non-microfluidic chamber into another non-microfluidic chamber through a microfluidic channel and flow is regulated by at least one valve; and wherein a first non-microfluidic chamber comprises a first volume of sample comprising an analyte; (b) providing an amount of particulate capture agent in the first non-microfluidic chamber to bind a selected amount of analyte from the sample; (c) moving the particulate capture agent bound to the analyte through a microfluidic channel in the microfluidic device to a second non-microfluidic chamber; (d) contacting the particulate

capture agent bound to the analyte with a reagent in a second non-microfluidic chamber; and (e) performing a chemical reaction on the analyte using the reagent. In one embodiment of the method the contacting comprises flowing the reagent from a third non-microfluidic chamber through a microfluidic channel in the microfluidic device into the second non-microfluidic chamber. In another embodiment of the method, the particles are response to magnetic force and the method further comprises immobilizing the particulate capture agent bound to the analyte in the instrument with a magnetic force. In another embodiment, the method comprises suspending the particulate capture agent bound to the analyte in the instrument in a volume at least an order of magnitude smaller than the sample volume.

[0033] In another aspect, the invention provides a method comprising: (a) performing a first chemical reaction on an analyte in a first chamber which is a non-microfluidic chamber to produce a first reaction product; and (b) moving the first reaction product through a microfluidic channel into a second chamber which is a non-microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product.

[0034] In another aspect, the invention provides a method comprising: (a) performing a first chemical reaction on an analyte in a first chamber which is a non-microfluidic chamber to produce a first reaction product; and (b) moving the first reaction product through a microfluidic channel into a second chamber which is a microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product. In a related aspect of the invention, provided herein is a method comprising: (a) performing a first chemical reaction on an analyte in a first chamber which is a microfluidic chamber to produce a first reaction product; and (b) moving the first reaction product through a microfluidic channel into a second chamber which is a non-microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product. In one embodiment, the methods of these related aspects comprise cleaning the first reaction product before moving it to the second chamber. In another embodiment, the methods of these related aspects comprise at least once, moving a reaction product through a microfluidic channel into a subsequent non-microfluidic chamber and performing a subsequent chemical reaction on the reaction product to create a subsequent reaction product. In another embodiment, the methods of these related aspects comprise at least once and before moving a reaction product into a non-microfluidic chamber, moving a reaction product through a microfluidic channel into a microfluidic chamber and performing a subsequent chemical reaction on the reaction product to create a subsequent reaction product.

[0035] In another aspect of the invention, provided herein is a device comprising: (a) a sample channel having a channel inlet and a channel outlet; (b) an electrophoresis capillary having a capillary inlet and a capillary outlet, wherein the capillary comprises an electrically conductive medium and is in communication with the sample channel at a point of connection; (c) an anode and a cathode configured to apply a voltage across the capillary inlet and capillary outlet, wherein one of the anode or cathode comprises a forked electrode wherein the forks are in electrical communication with the sample channel on different sides of the

point of connection; and (d) a second electrode in electrical communication with the sample channel substantially opposite the point of connection. In one embodiment of the device, the second electrode is comprised as a third fork in the forked electrode.

INCORPORATION BY REFERENCE

[0036] All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

BRIEF DESCRIPTION OF THE DRAWINGS

[0037] The novel features of the invention are set forth with particularity in the appended claims. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying drawings of which:

[0038] **Figure 1** depicts an example of a microscale on-chip valve (MOVE).

[0039] **Figure 2** shows a MOVE microvalve, a microrouter, a MOVE mixer, and bead capture on microchips.

[0040] **Figure 3** shows a fluidic cartridge with MOVE microvalves.

[0041] **Figure 4** shows a fluidic cartridge with ports to a microfluidic microchip with microvalves.

[0042] **Figure 5** shows a microfluidic microchip with MOVE valves that controls flows in a cartridge.

[0043] **Figure 6** shows a cartridge connected to reaction chamber and detector with downstream MOVE pumps and reagents.

[0044] **Figure 7** shows a temperature control device that can thermal cycle and incorporates magnetic capture, pinch clamps and the capability of cycling seven reactions simultaneously.

[0045] **Figure 8** shows a temperature control device that can thermal cycle and incorporates magnetic capture, pinch clamps and the capability of cycling seven reactions simultaneously.

[0046] **Figure 9** shows PowerPlex16 STR (Short tandem repeat) amplification reaction performed in a passive, Teflon (PTFE) based Tube reaction chamber.

[0047] **Figure 10** shows purification of DNA from 25 uL of blood at 69', 23.5', 10.5', and 4.5'; yield in ng is shown on the bars.

[0048] **Figure 11** shows a schematic of using microvalves to capture beads on a microchip.

[0049] **Figure 12** shows bead capture from a cartridge on a microchip using a MOVE microvalve.

[0050] **Figure 13** shows bead capture from a cartridge on a microchip using a MOVE microvalve.

- [0051] **Figure 14** shows a capture and reaction microchip using MOVE microvalves.
- [0052] **Figure 15** shows a capture and reaction microchip using MOVE microvalves.
- [0053] **Figure 16** shows a four module assembly.
- [0054] **Figure 17** shows an example of STR reactions on microchips.
- [0055] **Figure 18** shows a universal sample preparation workflow to prepare nucleic acids and toxins.
- [0056] **Figure 19** shows purification of samples in a cartridge using paramagnetic beads.
- [0057] **Figure 20** shows an integrated pneumatic manifold to operate the MOVE microvalves in cartridge.
- [0058] **Figure 21** shows a cartridge mounted on a computer controlled apparatus.
- [0059] **Figure 22** shows a cartridge mounted on a computer controlled apparatus.
- [0060] **Figure 23** shows a reagent distribution manifold based on MOVE technology that can distribute five reagents to five extraction / isolation or other devices.
- [0061] **Figure 24** shows a reagent distribution manifold based on MOVE technology that can distribute five reagents to five extraction / isolation or other devices.
- [0062] **Figure 25** shows a distribution manifold with sample loops and MOVE microvalves.
- [0063] **Figure 26** shows a pneumatic manifold, top panel shows the top side and the lower panel the bottom side.
- [0064] **Figure 27** shows detection of *E. coli* by immunomagnetic separation, followed by alkaline lysis and PEG-facilitated capture on magnetic beads, and analyzed by real-time PCR.
- [0065] **Figure 28** shows application of a cartridge with three chambers that can be used to construct genomic libraries and other applications.
- [0066] **Figure 29** shows the workflow to prepare genomic libraries using the cartridge.
- [0067] **Figure 30** shows a forked injector for microchip based electrophoresis.
- [0068] **Figure 31** shows sample stacking with a forked injector.
- [0069] **Figure 32** shows a forked injector coupled to MOVE microvalves.
- [0070] **Figure 33** shows a forked cathode injector coupled with a MOVE microchip.
- [0071] **Figure 34** shows a photograph of a microchip with the forked injector.
- [0072] **Figure 35** shows a photograph of a microchip with the forked injector.
- [0073] **Figure 36** shows an electropherogram of a single color from a DNA sequencing trace from a forked cathode injector.

- [0074] **Figure 37** shows STR separations on a forked cathode injection system.
- [0075] **Figure 38** shows a forked cathode with MOVE microfluidics for shuttle loading.
- [0076] **Figure 39** shows an integrated system for nucleic acid isolation, amplification(s), separation and detection.
- [0077] **Figure 40** depicts a device with a cartridge, microfluidic microchip, and a magnet.
- [0078] **Figure 41** depicts a microfluidic microchip with a fluidics layer, an elastomeric layer, and a pneumatics layer.
- [0079] **Figure 42** depicts a fluidics layer made of two layers of material.
- [0080] **Figure 43** depicts a fluidics layer made of a single layer of material.
- [0081] **Figure 44** depicts a reaction scheme for amplifying mRNA.
- [0082] **Figure 45** shows a microfluidic microchip with MOVE valves that controls flows in a cartridge.
- [0083] **Figure 46** shows a forked electrode.
- [0084] **Figure 47** shows a forked electrode, a forked electrode with a wire run electrode, and a forked electrode with a cannular electrode.
- [0085] **Figure 48** shows sample injection into a separation channel.
- [0086] **Figure 49** shows a device for mating a separation capillary with injection tubing.
- [0087] **Figure 50** shows a device for mating separation capillaries with four injection tubings.
- [0088] **Figure 51** shows a thermocycler with an Ultem pinch clamp.
- [0089] **Figure 52** shows a diagram indicating movement of reagents between components of a four channel parallel processing device.
- [0090] **Figure 53** shows a four-channel parallel reagent delivery device: the Chip C microchip design is shown on the top left, a fluidic manifold is shown on the bottom left, and the fabricated and assembled device is shown on the right.
- [0091] **Figure 54** shows a four-channel sample preparation device on the left and a four-channel sample preparation device mounted on a monolithic pneumatic manifold on the right.
- [0092] **Figure 55** shows MOVE microchip designs of the four-channel sample preparation device.
- [0093] **Figure 56** shows IdentiFiler STR profiles of DNA samples prepared on the four-channel sample preparation device, where STR amplifications were performed using fast protocols (1.5 hrs) on a STR Reaction subsystem thermocycler.

- [0094] **Figure 57** shows a four-channel post amplification device combined with an Chip A microchip with a fluidics manifold: the Chip A microchip design is shown on the left, the fabricated microchip is shown in the center, and the assembled fluidic manifold and microchip is shown on the right.
- [0095] **Figure 58** shows a post-amplification STR clean-up subsystem with the post-amplification device.
- [0096] **Figure 59** shows the Chip E microchip design, which can be used in the post-amplification device.
- [0097] **Figure 60** shows a diagram of a mixer.
- [0098] **Figure 61** shows a diagram of a mixer.
- [0099] **Figure 62** shows results of using a mixer to lyse cells.
- [00100] **Figure 63** depicts components of an integrated analysis system.
- [00101] **Figure 64** depicts hardware components of an integrated analysis system.
- [00102] **Figure 65** depicts software components of an integrated analysis system.
- [00103] **Figure 66** depicts consumable components of an integrated analysis system.
- [00104] **Figure 67** depicts documentation components of an integrated analysis system.
- [00105] **Figure 68** shows a picture of an encased integrated analysis system.
- [00106] **Figure 69** shows a schematic of an encased integrated analysis system.
- [00107] **Figure 70** shows a schematic of an encased and portable integrated analysis system.
- [00108] **Figure 71** shows a schematic of an encased and portable integrated analysis system and a polymer injection system.
- [00109] **Figure 72** shows a schematic of an optical detection system and pneumatic system.
- [00110] **Figure 73** shows a diagram of an integrated analysis system.
- [00111] **Figure 74** shows a schematic of a cartridge cover and pneumatic components.
- [00112] **Figure 75** shows a schematic of a cartridge cover, cartridge, pneumatic manifold, and thermocycler.
- [00113] **Figure 76** depicts a cartridge with reagent cassette.
- [00114] **Figure 77** depicts a cartridge with reagent cassette.
- [00115] **Figure 78** depicts a top view of a cartridge with reagent cassette.
- [00116] **Figure 79** depicts a top view of a cartridge without reagent cassette.
- [00117] **Figure 80** depicts a bottom view of a cartridge.

- [00118] **Figure 81** depicts a bottom view of a cartridge with tubes.
- [00119] **Figure 82** depicts a bottom view of a cartridge with tubes.
- [00120] **Figure 83** depicts loading of a cartridge into an encased integrated analysis system.
- [00121] **Figure 84** depicts loading of a cartridge into an encased integrated analysis system.
- [00122] **Figure 85** depicts loading of a cartridge into an encased integrated analysis system.
- [00123] **Figure 86** shows a diagram of a sample analysis procedure.
- [00124] **Figure 87** shows a diagram of a sample analysis procedure.
- [00125] **Figure 88A** shows a timeline of a sample analysis procedure.
- [00126] **Figure 88B** shows a timeline of a sample analysis procedure.
- [00127] **Figure 88C** shows a timeline of a sample analysis procedure.
- [00128] **Figure 89** shows a platform that carries an array of microcapillaries and that comprises an aperture that limits the amount of stray light collected by the optics.
- [00129] **Figure 90** shows an optical assembly.
- [00130] **Figure 91** shows transmission of light through a plurality of capillaries, each forming a separate image.
- [00131] **Figure 92** shows an optical assembly comprising a dichroic mirror (folding mirror 1) that allows transmission of light from the excitation source and a second folding mirror that decreases the footprint of the assembly.
- [00132] **Figure 93** shows the direction of excitation light at an oblique angle to the plane on which an array of capillaries is arranged, such that light passing through the capillaries is not directed normal to the plane where emitted fluorescent light can be collected.
- [00133] **Figure 94** is a top-down view of the configuration of **Figure 93**.
- [00134] **Figure 95** shows an image produced by eight capillary tubes that carry a fluorescent species and that have been excited by light.
- [00135] **Figure 96** shows an injection system for injecting a sample into an electrophoresis capillary.
- [00136] **Figure 96A** shows three electrodes opposite a capillary inside the lumen of tubing. The third electrode is not electrically connected, but is independently electrified.
- [00137] **Figure 96B** shows three electrodes opposite a capillary inside the lumen of tubing. All the electrodes are electrically connected.
- [00138] **Figure 97** shows integrated subsystems.

[00139] **Figure 98 A and B** show embodiments of a device for regulating temperature of electrophoresis capillaries, for example an array of capillaries. The electrically insulating circuit board has a generally S-shaped path for placement of capillaries.

[00140] **Figure 99** shows one embodiment of the optical system for detecting analytes in an array of capillaries.

[00141] **Figure 100** shows 'precious reagent' delivery one embodiment of the placement of 'precious reagent cartridges' in the device.

[00142] **Figure 101** shows the fluidics and pneumatics architecture of a microfluidic chip which is then mated with a fluidics cartridge to form the post amplification module.

[00143] **Figure 102** shows one embodiment of the system enclosure which measure 2 x 2 x 2 ft.

[00144] **Figure 103** shows the fluidics and pneumatics architecture of a microfluidic chip which is then mated with a fluidics cartridge to form the reagent delivery module.

[00145] **Figure 104** shows a portion of a device in which the fluidics layer comprises a plurality of sublayers, in an exploded view. The top or external sublayer 121 is referred to as the "etch" layer and bottom or lower sublayer 122 is referred to as the "via" layer. Fluid traveling in a channel in the etch layer can flow into a conduit in the via layer that faces the elastic layer.

DETAILED DESCRIPTION OF THE INVENTION

[00146] This invention includes devices that incorporate valves, such as microvalves (including but not limited to pneumatically actuated valves and microscale on-chip valves), into their design in order to control the movement of fluid. These devices can be used for the enrichment of a component, for sample preparation, and/or for analysis of one or more components in or from a sample.

[00147] The invention also provides devices for fluid and analyte processing and methods of use thereof. The devices of the invention can be used to perform a variety of actions on the fluid and analyte. These actions can include moving, mixing, separating, heating, cooling, and analyzing. The devices can include multiple components, such as a cartridge, a microfluidic microchip, and a pneumatic manifold.

Microfluidic-Non-Microfluidic Integration

[00148] In one aspect, this invention provides an instrument that uses microfluidic components to integrate functions performed on a non-microfluidic scale. The instrument includes non-microfluidic chambers fluidically connected to each other and to microfluidic chambers through microfluidic channels in a microfluidic device, e.g., a microfluidic chip. The microfluidic device comprises directional control mechanisms, such as valves and pumps, by which fluid can be selectively routed between different chambers and along different channels, and by which a single chamber can communicate with a number of other chambers. These connections and routing mechanisms allow automation of the functions. In certain embodiments, the instrument uses particulate capture agents that can bind an analyte, be immobilized, be

suspended or re-suspended in a desired volume of fluid and be routed to and from chambers through the microfluidic channels. This simplifies in the transition of an analyte from a non-microfluidic environment to a microfluidic environment and back to a non-microfluidic environment. The amount of capture agent can be selected to capture a desired amount analyte from a sample, for example, to concentrate analyte from a dilute sample, to quantitatively capture all or substantially all of an analyte from a sample or to select a portion of an analyte from a more concentrated sample. This allows one to “tune” the amount of analyte used in a reaction and further decreases fluid handling steps. The instrument can comprise a plurality of parallel fluidic circuits by which fluidic operations can be performed in parallel. The integration of microfluidic and non-microfluidic components on the device simplifies sample handling during the performance of chemical reactions (e.g., chemical reaction, biochemical reaction and enzymatic reaction). It also allows size reduction of operations, decreasing the footprint and the total space occupied by the system. Accordingly, the instruments of this invention integrate non-microfluidic and microfluidic environments.

[00149] More specifically, this invention provides instruments that comprise a microfluidic component and a non-microfluidic component in fluid communication with each other. A microfluidic component comprises at least one microfluidic channel. A microfluidic channel generally has a cross sectional area of less than 1 mm^2 or at least one cross-sectional dimension in the range of from about 0.1 microns to about 500 microns, e.g., below about 350 microns. A non-microfluidic component comprises at least one non-microfluidic chamber (open or closed), that is, a chamber that holds a non-microfluidic volume e.g., at least 10 microliters, at least 20 microliters, at least 50 microliters, at least 100 microliters, at least 500 microliters, at least 1 ml, at least 10 ml or at least 100 ml. Accordingly, in the instruments of this invention, a non-microfluidic chamber is in fluid communication with a microfluidic channel. The instruments are adapted to transport fluid samples (e.g., a liquid) from a non-microfluidic chamber into a microfluidic channel and/or from a microfluidic channel into a non-microfluidic chamber or otherwise out of the microfluidic device. In other embodiments the microfluidic devices comprise microfluidic chambers in fluid communication with microfluidic channels. In this case, the instruments are adapted to transport fluid samples between microfluidic chambers and non-microfluidic chambers through microfluidic channels. Fluid moved from a microfluidic channel into a non-microfluidic chamber can be removed from the device.

[00150] Manipulation of the analyte can include a variety of steps. These can include, for example, preparing the analyte for a chemical reaction, mixing with one or more reagents in various sequences, performing a chemical reaction with the analyte, removing wastes and washing. The instrument of this invention can be used to perform these functions by routing analytes, reagents, wastes and wash solutions between compartments. Accordingly, in certain embodiments the instruments of this device comprise a plurality of non-microfluidic chambers connected to each other through microfluidic channels. Fluid can be moved from one chamber to another by any appropriate motive force, for example, continuous pressure or non-continuous pressure (e.g., positive displacement pumps), electroosmotic flow or centrifugation. Pressure can be generated internally (e.g., with on-chip diaphragm valves) or externally. The channels can comprise directional control mechanisms to selectively route fluids between chambers as desired. These

mechanisms can be valves, such as the diaphragm valves described elsewhere in this specification, single use valves such as wax valves or other valves. By opening and closing valves in a proper sequence, analyte, reagents and waste can be routed into appropriate locations. In this way, the microfluidic portion of the instrument is used to route fluids between non-microfluidic environments where various functions can be performed on the analyte.

[00151] The non-microfluidic chambers can comprise capture agents to bind analytes. The capture agents generally comprise a solid substrate and are able to specifically or non-specifically bind analytes. The substrate can assert the binding force, or a molecule having binding properties can be attached to the substrate, for example, an antibody. The capture agent can be a particulate capture agent. Alternatively, the material can be a chromatographic material. In this case, a sample can be passed through the chromatographic material and separated fractions introduced into the microfluidic device. Alternatively, the capture agent can be a monolith. Alternatively, the capture agent can be attached to a surface of the chamber, such as a post, or the chamber surface can be derivatized with a capture molecule.

[00152] The device is further adapted to move particles, such as beads, between a microfluidic channel and a non-microfluidic chamber. The particles can be responsive to magnetic force, electrical forces, or other forces. For example, they can be paramagnetic or magnetic particles. This allows further manipulation of the particles within the device by application of magnetic fields using fixed or movable magnets including electromagnets. The particles can function as a capture agent to capture one or more analytes from a sample. For example, the particles can have specific or non-specific affinity for an analyte. Because the particles are solid, they allow one to transit between non-microfluidic fluid volumes and microfluidic fluid volumes by immobilizing the particles and altering the volume of the fluid in which they are contained. Particles can be immobilized in the non-microfluidic chamber or in the microfluidic device.

[00153] The instrument of this invention can be used to capture a selected amount of an analyte from a sample in a non-microfluidic chamber and transport that amount of analyte from the chamber into a microfluidic channel. Once in the microfluidic channel, the particles can be routed into a non-microfluidic chamber for storage or processing. For example, a non-microfluidic volume of a sample is provided to a chamber. The sample may be, for example, dilute or concentrated with respect to an analyte. By properly calibrating the amount of capture agent and conditions, a selected amount of the analyte can be captured by the capture agent. For example, in a concentrated sample, a small amount of capture agent can be selected so that only a portion of the analyte to be used in a reaction is captured. This allows sampling of a portion of the analyte in the sample volume, e.g., an amount sufficient or appropriate to perform a chemical reaction. Alternatively, in a dilute sample, a greater amount of capture agent can be used so that most or substantially all of the analyte present is captured on the capture agent. This effectively concentrates the analyte. Washing the analyte can remove impurities, effectively purifying the analyte from undesirable components of the sample such as inhibitors, other analytes, etc. The specificity of the capture can also be controlled by adjusting the chemistry to select broader or narrower ranges of analytes, for example longer or short pieces

of DNA, differentiating DNA from RNA, or using affinity reagents with broader or narrower specificity. In some embodiments, multiple analytes may be captured by combining affinity reagents or by using multiple modes of capture either on one type of bead or by mixing multiple bead or particle types. In certain embodiments, the instrument further comprises a detector, e.g., an optical detector, for detecting molecules at some stage of the process.

[00154] A variety of reaction sequences are contemplated. A chemical reaction can be performed on an analyte. Then, the reaction product can be cleaned and subjected to a different chemical reaction. This sequence of cleaning a reaction product and performing a subsequent different reaction can be repeated. In particular, this invention contemplates performing series of biochemical or enzymatic reactions separated by clean-up steps. One example of this is Eberwine chemistry, in which a first chemical reaction, reverse transcription, is followed by a second reaction, second strand synthesis, which is followed by a third reaction, transcription. Before each subsequent reaction, and typically after the last reaction, the product is removed from contaminants in preparation of the next step. In one embodiment, a reaction product in a non-microfluidic chamber is moved through a microfluidic channel to another non-microfluidic chamber. In another embodiment, a reaction product in a non-microfluidic chamber is moved through a microfluidic channel into a microfluidic chamber, e.g., on-chip. In another embodiment, a reaction product in a microfluidic chamber is moved through a microfluidic channel into a non-microfluidic chamber. Accordingly, this invention provides the use of small analyte volumes and small reagent volumes, thereby reducing waste of reagent.

[00155] For example, the instrument can be used to perform chemical reactions on nucleic acids, such as DNA amplification. A non-microfluidic volume of a sample (e.g., several hundred microliters) comprising DNA can be collected in a non-microfluidic chamber of this device. Paramagnetic capture particles can be flowed through microfluidic circuits into the chamber to capture a calibrated amount of nucleic acid. The paramagnetic particles can be held in the chamber by magnetic force and the uncaptured sample can be removed as waste, e.g., through a microfluidic channel. Valves in the microfluidic device can then be configured to route a volume, e.g., a non-microfluidic volume, of wash solution into the chamber. The analyte and particles can be washed, immobilized and the waste can be removed. Then, the particles with captured and purified analyte can be re-suspended in a volume and moved from the chamber through a microfluidic channel into a thermal cycling chamber, which can be a non-microfluidic reaction chamber or a microfluidic reaction chamber. There, the particles can be immobilized and liquid removed. This can concentrate the particles to about the particle volume (e.g., in the nanoliter range). Reagents for performing nucleic acid amplification in an appropriate volume can be routed through a microfluidic channel into the thermal cycling chamber. Under certain conditions, the reaction mixture will elute the nucleic acids from the particles. Accordingly, this invention contemplates contacting reagents for performing a chemical reaction, such as PCR, cycle sequencing, real-time PCR, rolling circle amplification, restriction digestion, RNA fragmentation, protein digestion, etc., with the analyte attached to a particle, without first eluting the analyte from the particle and, e.g., determining concentration and selecting an amount of analyte for mixing with

reagent. This is possible, in part, by properly calibrating the capture agent used to capture analyte, so that an appropriate amount of analyte is already present. After enzymatic reaction or thermal cycling, the product can be moved into a microfluidic channel for clean up, e.g., in a microfluidic chamber or into a non-microfluidic chamber. This can comprise diluting the product to decrease salt concentration. It also can comprise binding the analytes to beads, immobilizing them, and washing them. It can also comprise chromatography, solid phase extraction, or other cleanup methods at microfluidic scale or non-microfluidic scale. At this point, the microfluidic components can route the product to an appropriate location for analysis, e.g., a capillary tube for capillary electrophoresis or the product can be output into a non-microfluidic volume for analysis by an unintegrated system such as a commercial capillary array electrophoresis instrument, mass spectrometer, or other analytical instrument. The microfluidic device also can contain a waste confinement area.

[00156] In certain embodiments, the microfluidic devices of this invention are monolithic devices. In monolithic devices, a plurality of circuits are provided on a single substrate. In the case of devices comprising diaphragm valves, a monolithic device comprises a single elastic layer functioning as a diaphragm for a plurality of valves. In certain embodiments, one actuation channel can operate a plurality of valves on a monolithic device. This allows parallel activation of many fluidic circuits. Monolithic devices can have dense arrays of microfluidic circuits. These circuits function with high reliability, in part because the channels in each circuit are fabricated simultaneously on a single substrate, rather than being made independently and assembled together.

[00157] The fluidic circuits and of these devices can be densely packed. A circuit comprises an open or closed fluid conduit. In certain embodiments, the device can comprise at least 1 fluidic circuit per 1000 mm², at least 2 fluidic circuits per 1000 mm², at least 5 fluidic circuits per 1000 mm², at least 10 fluidic circuits per 1000 mm², at least 20 fluidic circuits per 1000 mm², at least 50 fluidic circuits per 1000 mm². Alternatively, the device can comprise at least 1 mm of channel length per 10 mm² area, at least 5 mm channel length per 10 mm², at least 10 mm of channel length per 10 mm² or at least 20 mm channel length per 10 mm². Alternatively, the device can comprise valves (either seated or unseated) at a density of at least 1 valve per cm², at least 4 valves per cm², or at least 10 valves per cm². Alternatively, the device can comprise features, such as channels, that are no more than 5 mm apart edge-to-edge, no more than 2 mm apart, no more than 1 mm apart, no more than 500 microns apart or no more than 250 microns apart.

Universal Sample Preparation System

[00158] This invention provides a universal sample preparation system. The system is configured to accept a biological sample comprising an analyte in an un-purified form, purify the analyte, perform at least one biochemical reaction on the analyte, and analyze the product of the biochemical reaction.

[00159] The universal sample preparation system can be configured to fit inside a volume of no more than 6 ft³, no more than 7 ft³, no more than 8 ft³, no more than 97 ft³, or no more than 10 ft³. In one specific embodiment, the universal sample preparation system is configured to fit inside a volume of about 8 ft³. In

another specific embodiment, the universal sample preparation system is configured to fit inside a volume of about 10 ft³.

[00160] The universal sample preparation system can comprise the following modules: a sample preparation module, a reaction module, a post-reaction module, an analysis module, and/or a computer module. A sample preparation module can be configured to capture an analyte, e.g., DNA, from a sample that has a non-microfluidic volume, and move the captured analyte into a first microfluidic channel. This can be accomplished using, for example, magnetically-responsive capture particles to concentrate the analyte. The reaction module is fluidly connected to the first microfluidic channel and is configured to perform at least one biochemical reaction on the analyte in a reaction chamber to produce a reaction product. Typically, the analyte in the reaction chamber is concentrated with respect to its concentration in the sample preparation module. A post-reaction module is in fluid communication with the reaction module and is configured to process the reaction product for analysis. The post-reaction module can be configured to move the reaction product through a second microfluidic channel into a non-microfluidic chamber in the post-reaction module. The analysis module is fluidly connected to the reaction module or the post-reaction module and is configured to perform an analysis, such as capillary electrophoresis, on the reaction product. The analysis module generates data about the reaction product. A computer module comprises computer executable code for processing and/or analyzing the data, including formatting the data into a universal format. The system can be further configured to access the Internet, transmit data to an off-site server and receive information from the server.

[00161] An exemplary device is shown in **Figure 6**. **Figure 6** shows a cartridge with integrated microchip (1), temperature modulating device (400), and downstream analysis device (500). In certain embodiments the device comprises a fluid preparation module comprising a cartridge mated or otherwise fluidically connected to a microchip; an off-chip thermal modulation module connected to the fluid preparation module through a fluid transporter with a fluidic channel, such as a tube, through the cartridge, and configured to modulate the temperature in the fluid transporter, wherein the fluid transporter is further fluidically connected to a second microchip with valves and fluidic channels that can selectively route fluid to one or more subsequent devices. This device can be used for thermal cycling or isothermal reactions.

[00162] In one application, the system is configured to prepare, from a biological sample, a CODIS-compatible file for searching a CODIS database. CODIS is a forensic system that presently uses thirteen STR (short tandem repeat) loci as genetic identity markers see, e.g., www.fbi.gov/hq/lab/html/codis1.htm. Information from fewer or more than 13 markers can be used to provide evidence of identity. The sample preparation module extracts DNA from forensic material, captures a predetermined amount of DNA on capture particles e.g. in magnetically responsive particles, and delivers the DNA to a non-microfluidic reaction chamber of a reaction module, where the particles are immobilized, e.g., with a magnetic force. There, reagents for PCR are delivered to the reaction chamber and the STR markers used in CODIS are amplified using PCR. The amplification can be performed using commercially available reagents, such as

those available from Promega (e.g., the PowerPlex product series). This product uses four differently colored fluorescent markers. The PCR products are routed to the post-reaction module and diluted to a proper concentration for capillary electrophoresis. The new product is directed to the analysis module, where capillary electrophoresis is performed. Analytes in the product are detected by fluorescence detection. The data generated is then subjected to an algorithm which generates traces for each fluorescent species. These traces can then be analyzed by computer to identify the markers at the STR loci used in CODIS. Such software is commercially available from, e.g., Life Technologies, such as GeneMapper™ ID-X software or NIST software tools (www.cstl.nist.gov/biotech/strbase/software.htm). Software can convert this data into a file format compatible with CODIS. See, e.g., www.ncjrs.gov/pdffiles1/nij/sl413apf.pdf. The CODIS compatible file can be used to query a forensic database such as the CODIS database. The system can be configured to access the Internet and deliver the file to the appropriate database for analysis and to receive a report from the database indicating the probable matches between the initial sample and an individual.

I. Sample preparation module

[00163] The sample preparation module is configured to capture an analyte from a non-microfluidic volume onto a solid substrate and route the captured analyte through a microfluidic channel into a reaction chamber of the reaction module. The analyte can be captured from a sample in which the analyte is in non-isolated form. An analyte is non-isolated if it is present with other cellular or biomolecular components with which it is naturally associated. These can include for example, cytoplasmic components or viral components. The sample preparation module can be configured to capture and analyte from a raw sample. A raw sample is one in which the analyte is contained within a cell or a virus. For example, blood, a cheek swab and semen are raw samples containing the analyte DNA. In this case, the sample preparation module can comprise materials to lyse cells and extract DNA from the lysate.

[00164] In one aspect a sample preparation device, as shown in **Figure 16**, device 1000 in **Figure 21** and **Figure 22**, and **Figure 54**, comprises a cartridge integrated with a microfluidic microchip that controls movement of the fluid in the cartridge through microvalves and the components to operate the cartridge. The cartridge and/or the compartments therein can be of sufficient size to process one or more milliliter of an input sample in an automated device. The cartridge can process a sample to output a component that can be moved using pressure-driven flow or vacuum modulated by microvalves. The cartridge can provide an interface with a delivery device comprising macroscale samples, such as blood, aerosol liquids, swabs, bodily fluids, swipes, and other liquid, solid, and gas samples. The cartridge can process macroscale sample volumes using microscale sample preparation and analysis. The cartridge can allow for processing of macroscale or large volume samples using microfluidic devices and components have reduced void volumes that allow for reduced loss of materials.

A. Cartridges

[00165] A cartridge, also referred to as a fluidic manifold herein, can be used for a number of purposes. In general, a cartridge can have ports that are sized to interface with large scale devices as well as microfluidic devices. Cartridges or fluidic manifolds have been described in U.S. Patent Publication US20090253181. The cartridge can be used to receive materials, such as samples, reagents, or solid particles, from a source and deliver them to the microfluidic microchip. The materials can be transferred between the cartridge and the microfluidic microchip through mated openings of the cartridge and the microfluidic microchip. For example, a pipette can be used to transfer materials to the cartridge, which in turn, can then deliver the materials to the microfluidic device. In another embodiment, tubing can transfer the materials to the cartridge. In another embodiment, a syringe can transfer material to the cartridge. In addition, a cartridge can have reservoirs with volumes capable of holding nanoliters, microliters, milliliters, or liters of fluid. The reservoirs can be used as holding chambers, reaction chambers (e.g., that comprise reagents for carrying out a reaction), chambers for providing heating or cooling (e.g., that contain thermal control elements or that are thermally connected to thermal control devices), or separation chambers (e.g. paramagnetic bead separations, affinity capture matrices, and chromatography). Any type of chamber can be used in the devices described herein, e.g., those described in U.S. Patent Publication Number 2007/0248958, which is hereby incorporated by reference. A reservoir can be used to provide heating or cooling by having inlets and outlets for the movement of temperature controlled fluids in and out of the cartridge, which then can provide temperature control to the microfluidic microchip. Alternatively, a reservoir can house Peltier elements, or any other heating or cooling elements known to those skilled in the art, that provide a heat sink or heat source. A cartridge reservoir or chamber can have a volume of at least about 0.1, 0.5, 1, 5, 10, 50, 100, 150, 200, 250, 300, 400, 500, 750, 1000, 2000, 3000, 4000, 5000 or more μL . The relative volume of a chamber or reservoir can be about 1, 2, 5, 10, 20, 50, 100, 200, 500, 1000, 2000, 5000, 10000 or more greater than a channel or valve within the microfluidic microchip. The size of the chambers and reservoirs of the cartridge, which can be mated to the microfluidic microchip, can be chosen such that a large volume of sample, such as a sample greater than about 1, 5, 10, 50, 100, 500, 1000, 5000, 10000, 50000 or more μL , can be processed, wherein the flow of fluids for processing the sample is controlled by valves in the microfluidic microchip. This can allow for a reduced amount of sample and reagent loss due to the reduced void volumes in the microfluidic microchip compared to other flow control devices, such as pipettes and large scale valves. The void volume within a microfluidic microchip can be less than 1000, 500, 100, 50, 10, 5, 1, 0.5, 0.1, or 0.05 μL . This can allow for the amount of sample or reagent loss during processing of a sample to be less than 20, 15, 10, 7, 5, 3, 2, 1, 0.5, 0.05 percent.

[00166] A cartridge can be constructed of any material known to those skilled in the art. For example, the cartridge can be constructed of a plastic, glass, or metal. A plastic material may include any plastic known to those skilled in the art, such as polypropylene, polystyrene, polyethylene, polyethylene terephthalate, polyester, polyamide, poly(vinylchloride), polycarbonate, polyurethane, polyvinylidene chloride, cyclic olefin copolymer, or any combination thereof. The cartridge can be formed using any

technique known to those skilled in the art, such as soft-lithography, hard-lithography, milling, embossing, ablating, drilling, etching, injection molding, or any combination thereof.

[00167] As exemplified in **Figure 3** and **Figure 4**, a cartridge (1) can comprise a rectilinear configuration with flat sides. In another embodiment, a cartridge comprises a surface that is curved, rounded, indented or comprises a protrusion. In one embodiment a cartridge has at least one substantially flat surface which is adjacent to a microfluidic microchip. The cartridge is adapted to be fluidically connected with ports in the microchip. For example, openings in the surface of the cartridge can be aligned with ports in the microchip. When the cartridge and microchip are mated to one another, the openings align to create the fluidic connections allowing liquids to pass from the cartridge into the ports of the microchip, which are connected to channels typically having valves that form fluidic circuits.

[00168] In one embodiment a cartridge contains one or more features, including but not limited to a chamber, a port, a channel or a magnet. In one embodiment, microvalves, such as pneumatically actuated valves are combined with the microfluidic cartridge. In some embodiments the microvalves are active mechanical microvalves (such as magnetic, electrical, or piezoelectric thermal microvalves), non-mechanical microvalves (such as bistable electromechanical phase change or rheological microvalves), external microvalves (such as modular or pneumatic), passive mechanical (such as check microvalves or passive non-mechanical (such as capillary microvalves) (Oh et al., A review of microvalves, J. Micromech Microeng. 16 (2006) R13-R39)).

[00169] In another embodiment, pneumatically actuated valves, such as MOVE valves, modulate the flow of air pressure, vacuum, or fluids in a microfluidic microchip 2 or multiple microfluidic microchips. MOVE valves can be microscale on-chip valves, microfluidic on-chip valves or micro-robotic on-chip valves. In one embodiment the flow of air pressure, vacuum, or fluids is regulated by one or more variable pressure pumps, such as solenoid valves or solenoid pumps. In one embodiment, a microfluidic microchip is a structure that contains microchannels and/or microtrenches, where a microchannel is a closed structure and a microtrench is an open structure. In one embodiment a microfluidic microchip is a planar structure. In a related embodiment a microfluidic device comprises a microfluidic microchip with microvalves clustered on one side of a cartridge. In one embodiment (**Figure 3** and **Figure 4**) the cartridge (1) can comprise one or more ports (4, 5, 6, 7, 8, 9) to external fluids, air, or vacuum. Functions of the ports can be for waste (4), reagent entry (5), vent (6), sample input (7), product output (8). The cartridge (1) can contain one or more sample input or reaction chambers, (7) and (3).

[00170] A single chamber within the cartridge, such as a reaction chamber, can have one or more, or at least one, two, or three fluidic connections to a microchip. For example, in **Figure 3** and **Figure 4**, the reaction chamber (3) can have a fluidic connection to the microchip through connection 120, which is at the base of the chamber, and another fluidic connection to the microchip through port (9), which is connected to chamber (3) through a passageway located at the top of the chamber. The top of chamber (3), port (9), and the passageway between chamber (3) and port (9) can be closed from the exterior environment such that

fluids in chamber (3) necessarily are pumped into port (9) when chamber (3) is full and vice versa. Such a chamber or combination of chamber and port can be referred to as a closed chamber. The positioning of the fluidic connections need not necessarily be at the base and top of the chamber, however, fluidic connections at the base and top positions of the chamber allow for reduced trapping of gas in the chamber. Alternatively, reaction chamber (3) can be viewed as a combination of two chambers that are fluidically connected to each other at a top position, which can be within the cartridge, and, where each chamber also has an opening at a base location. The openings at the base locations, also called chamber apertures, can be fluidically connected to port apertures on the microchip. The two fluidic connections can allow for fluids to be directed into and out of the chamber through the microfluidic microchip.

[00171] In another embodiment a device comprises a cartridge comprising at least one pneumatically actuated valve, such as a MOVE valve, located on one or more surfaces or structures in a non-linear manner. A cartridge can comprise one or more pneumatically actuated valves that are located within the cartridge, in a location other than the base of the cartridge.

[00172] Functional elements of a cartridge can include ports, channels, chambers, filters, magnets, or vents, chambers can be collectively referred to as functional elements. In one embodiment, **Figure 4**, the functional elements connect to the microfluidic microchip containing microvalves at junctions 100, 120, 140, 160, and 230. The functional elements can connect with tubing or capillaries inserted into the ports, by a flush connection, or by fittings. In one embodiment a flush connection can comprise a port of a cartridge aligned directly with an aperture of a microfluidic microchip. In one embodiment the cartridge and microfluidic microchip form an integrated module. In another embodiment the cartridge and microfluidic microchip are two separate pieces which are attached together, prior to use.

[00173] A cartridge can comprise at least one chamber, a sample input port, a reagent port, an exit port, a waste port and a magnet. The magnet can be located adjacent to the chamber, so that the magnet force generated by the magnet can attract paramagnetic particles in said chamber to a wall of the chamber. In one embodiment the paramagnetic particles are beads or cells rendered magnetically responsive (e.g., cells comprising hemoglobin that are treated with sodium nitrate). The magnet can be an electric magnet or a permanent magnet, such as a rare earth metal magnet.

[00174] In one embodiment, as exemplified in **Figure 4**, connections or ports (4, 5, 6, 7, 8, and 9) lead to channels in the cartridge (14, 15, 16, 17, 18, and 19) respectively. Ports (4, 5, 6, 7, and 8) show indents to reliably attach a connector or tubing to the indent, such as the indent shown for connection (7) (see the difference in diameter of connection (7) with channel (17)). In one embodiment, the ports or ports can interface with a variety of connector or tubes, such as the capillaries as described in U. S. Patent 6,190,616, U.S. Patent 6,423,536, US Application No. 09/770,412, 1-25-01, US Application No. 60/402,959 or one or more microchips with modular microfluidic ports as described in US Patent 6,870,185 and US application 11/229,065; all of which are herein incorporated by reference in their entirety. In one embodiment, the

modular microfluidic ports enable microchips or capillaries to be reversibly joined without dead volumes or leakage.

[00175] In another embodiment chamber (3) is connected to passageway (9) and to cone (13), leading to junction (120). Chamber (3) can be used for reactions as may any of the channels. In **Figure 4** the cartridge channels lead directly to the apertures of ports on the microchip (2). The channels of the cartridge can interconnect with each other as needed. In some embodiments, at least one channel in a cartridge does not physically connect to a microfluidic microchip. In another embodiment at least one channel in a cartridge is fluidically connected to at least one microchannel in a microfluidic microchip. The connection may or may not utilize an aperture on the microfluidic microchip. An aperture can be an opening or a fitting designed to mate between the microchip and the cartridge. In some embodiments of the invention, the fitting comprises a seal such as a gasket or an o-ring.

B. Microfluidic Devices

[00176] In one embodiment a cartridge and a microfluidic microchip are integrated together to form a single modular device. The cartridge and a microfluidic microchip can be attached by a fluid or by a solid adhesive or mechanically. In one embodiment the adhesive is a polyacrylate, adhesive tape, double-sided tape, or any other adhesive known to one skilled in the art. A cartridge can comprise a feature (12), as exemplified in **Figure 4**, that is capable of wicking a fluid-based adhesive into the junction between a microfluidic microchip and a cartridge. An exemplary In another embodiment a cartridge is attached to a microfluidic microchip with a non-fluidic adhesive layer. Alternatively, the cartridge and microchip can be held together by clips, clamps, or another holding device. The cartridge and microchip can be aligned prior to integration by visual cues, with or without a microscope, or by physical guiding features. Visual cues can include lines or features that are drawn, etched, or otherwise present on the cartridge, the microchip, or both. Physical guiding features include indentations, protrusions, and edges that can be 'keyed' to aid or insure proper assembly.

[00177] In some instances, the microfluidic microchip has diaphragm valves for the control of fluid flow. Microfluidic devices with diaphragm valves that control fluid flow have been described in U.S. Patent No. 7,445,926, U.S. Patent Publication Nos. 2006/0073484, 2006/0073484, 2007/0248958, and 2008/0014576, and PCT Publication No. WO 2008/115626. The valves can be controlled by applying positive or negative pressure to a pneumatics layer of the microchip through a pneumatic manifold.

[00178] In one embodiment, the microchip is a "MOVE" microchip. Such microchips comprise three functional layers – a fluidics layer that comprises microfluidic channels; a pneumatics layer that comprises pneumatics channels and an actuation layer sandwiched between the two other layers. In certain embodiments, the fluidics layer is comprised of two layers. One layer can comprise grooves that provide the microfluidics channels, and vias, or holes that pass from the outside surface to a fluidics channel. A second layer can comprise vias that pass from a surface that is in contact with the actuation layer to the surface in contact with the pneumatic channels on the other layer. When contacted together, these two layers form a

single fluidics layer that comprises internal channels and vias that open out to connect a channel with the fluidics manifold or in to connect a channel with the activation layer, to form a valve, chamber or other functional item. The actuation layer typically is formed of a deformable substance, e.g., an elastomeric substance, that can deform when vacuum or pressure is exerted on it. At points where the fluidic channels or pneumatic channels open onto or are otherwise in contact with the actuation layer, functional devices such as valves, e.g. diaphragm valves, can be formed. Such a valve is depicted in cross section in **Figure 1**. Both the fluidics layer and the pneumatics layer can comprise ports that connect channels to the outside surface as ports. Such ports can be adapted to engage fluidics manifolds, e.g., cartridges, or pneumatics manifolds.

[00179] As shown in **Figure 40**, the microfluidic microchip (103) can be interfaced with the cartridge (101). The microfluidic microchip can have a chamber (105) with an opening that is mated to an opening (117) of the cartridge (101). The chamber can be used for a variety of purposes. For example, the chamber can be used as a reaction chamber, a mixing chamber, or a capture chamber. The chamber can be used to capture magnetic particles such as magnetic beads, paramagnetic beads, solid phase extraction material, monoliths, or chromatography matrices.

[00180] A magnetic component (109) can be positioned such that magnetic particles in the cartridge reservoir (107) and/or the microfluidic chamber (105) are captured against a surface of the microfluidic chamber (105). The magnetic component can generate a magnetic and/or electromagnetic field using a permanent magnet and/or an electromagnet. If a permanent magnet is used, the magnet can be actuated in one or more directions to bring the magnet into proximity of the microfluidic microchip to apply a magnetic field to the microfluidic chamber. In some embodiments of the invention, the magnet is actuated in the direction (111) indicated in **Figure 40**.

[00181] Alternatively, any of a variety of devices can be interfaced with the microfluidic microchip. For example detectors, separation devices (e.g. gas chromatographs, liquid chromatographs, capillary electrophoresis, mass spectrometers, etc), light sources, or temperature control devices can be positioned next to the microfluidic microchip or used in conjunction with the microfluidic microchip. These devices can allow for detection of analytes by detecting resistance, capacitance, light absorbance or emission, fluorescence, or temperature or other chemical or physical measurements. Alternatively, these devices can allow for light to be introduced to a region or area of the microfluidic microchip.

[00182] A microfluidic device can be designed with multiple chambers that are configured for capture of magnetic particles. The multiple chambers and magnetic component can be arranged such that a magnetic field can be applied simultaneously to all chambers, or be applied to each or some chambers independent of other chambers. The arrangement of chambers and magnetic components can facilitate faster or more efficient recovery of magnetic particles. In particular, the arrangement can facilitate recovery of magnetic particles in multiple chambers.

[00183] As shown in **Figure 41**, the microfluidic microchip (103) can be formed of a fluidics layer (203), an elastomeric layer (205), and a pneumatic layer (207). The fluidics layer can contain features such as a

chamber (105), as well as channels, valves, and ports. The channels can be microfluidic channels used for the transfer of fluids between chambers and/or ports. The valves can be any type of valve used in microfluidic devices. In preferred embodiments of the invention, a valve includes a microscale on-chip valve (MOVE), also referred to as a microfluidic diaphragm valve herein. A series of three MOVes can form a MOVE pump. The MOVes and MOVE pumps can be actuated using pneumatics. Pneumatic sources can be internal or external to the microfluidic microchip.

[00184] An example of a MOVE valve is shown in **Figure 1**. A clamshell view of a MOVE valve is shown in **Figure 1A**. A cross-sectional view of a closed MOVE valve is shown in **Figure 1B**. **Figure 1C** shows a top-down view of the MOVE valve. A channel (251) that originates from a fluidic layer can interface with an elastomeric layer (259) by one or more vias (257). The channel can have one or more seats (255) to obstruct flow through the channel when the elastomeric layer (259) is in contact with the seat (255). The elastomeric layer can either be normally in contact with the seat, or normally not in contact with the seat. Application of positive or negative pressure through a pneumatic line (261) to increase or decrease the pressure in a pneumatic chamber (253) relative to the fluidic channel (251) can deform the elastomeric layer, such that the elastomeric layer is pushed against the seat or pulled away from the seat.

[00185] In some embodiments of the invention, a MOVE does not have a valve seat, and fluid flow through the fluidic channel is not completely obstructed under application of positive or negative pressure. This type of valve is useful as a fluid reservoir and as a pumping chamber and can be referred to as a pumping valve. The vacuum that can be applied include extremely high vacuum, medium vacuum, low vacuum, house vacuum, and pressures such as 5 psi, 10 psi, 15 psi, 25 psi, 30 psi, 40 psi, 45 psi, and 50 psi.

[00186] Three MOVE valves in series can form a pump through the use of a first MOVE as an inlet valve, a second MOVE as a pumping valve, and a third MOVE as an outlet valve. Fluid can be moved through the series of MOVes by sequential opening and closing of the MOVes. For a fluid being supplied to an inlet valve, an exemplary sequence can include, starting from a state where all three MOVes are closed, (a) opening the inlet valve, (b) opening the pumping valve, (c) closing the inlet valve and opening the outlet valve, (d) closing the pumping valve, and (e) closing the outlet valve. Since the inlet and outlet valve can have the same structure, a MOVE pump can move fluids in either direction by reprogramming of the sequence of opening inlet or outlet valves.

[00187] The fluidic layer (203) can be constructed of one or more layers of material. As shown in **Figure 42**, the fluidic layer (203) can be constructed of two layers of material. Channels (301, 303, 305) can be formed at the interface between the two layers of material, and a chamber (105) can be formed by complete removal of a portion of one layer of material. The channels can have any shape, e.g., rounded and on one side (301), rectangular (303), or circular (305). The channel can be formed by recesses in only one layer (301, 303) or by recesses in both layers (305). The channels and chambers can be connected by fluidic channels that traverse the channels and chambers shown. Multidimensional microchips are also within the

scope of the instant invention where fluidic channels and connections are made between multiple fluidic layers.

[00188] The thickness (307) of the second layer of material can be of any thickness. In some embodiments of the invention, the second layer has a thickness that minimizes reduction of a magnetic field in the chamber (105) that is applied across the second layer from an external magnetic component or minimizes reductions in heat transfer.

[00189] As shown in **Figure 43**, the fluidic layer (203) can be constructed of a single layer of material. The single layer is then interfaced with an elastomeric layer (205), such that channels (305, 303) and chambers (305) are formed between the fluidic layer and the elastomeric layer.

[00190] The microfluidic microchip can be constructed from any material known to those skilled in the art. In some embodiments of the invention, the fluidics and pneumatic layer are constructed from glass and the elastomeric layer is formed from PDMS. In alternative embodiments, the elastomer can be replaced by a thin membrane of deformable material such as Teflon (PTFE), silicon, or other membrane. The features of the fluidics and pneumatic layer can be formed using any microfabrication technique known to those skilled in the art, such as patterning, etching, milling, molding, embossing, screen printing, laser ablation, substrate deposition, chemical vapor deposition, or any combination thereof.

[00191] Microfluidic devices can be configured so that valves are less sticky. This can be accomplished by coating valve seats and other surfaces over which fluid flows that are likely to come into contact with the elastic layer with low energy material, such a noble metal (e.g., gold) or a perfluorinated polymer (e.g., Teflon). Such devices are described in more detail in U.S. patent application 12/789,186.

[00192] In one embodiment, microchannel circuits are formed on a microfluidic microchip 2, as shown in **Figure 5**, linking sets of microvalves with microchannels. In one embodiment the microvalves are pneumatically actuated valves. In one embodiment the pneumatically actuated valves are MOVE microvalves. In one embodiment, the fluidic path between a cartridge and a microfluidic microchip, such as between chambers, ports, channels, microchannels, and other functional elements can be controlled by opening or closing at least one microvalve. In one embodiment the microvalve is controlled by a microprocessor control such as a computer. A computer can include an input/output controller, or any other components known to one skilled in the art such as memory storage and a processor. In one embodiment, a microvalve is a MOVE valve that is actuated by a pneumatic source, such as through pneumatic ports 10, 20, 30, 40, 50, 60, or 70. In one embodiment the pneumatic source is controlled by at least one solenoid. In one embodiment the solenoid is miniaturized and can be connected to vacuum or pressure sources. In one embodiment the pneumatic source is connected to a pneumatic port using a force such as clamping, springs, pneumatics, or a screw force, optionally with sealing provided by an o-ring.

[00193] In one embodiment **Figure 5** shows a view of the top of a microfluidic microchip (2), this side makes contact with the bottom of cartridge (1). A microvalve 110 controls the fluidic path between

microchannels 101 and 121. A microvalve 130 controls the fluidic path between microchannels 131 and 141. Microvalve (150) controls the fluidic path between microchannels 151 and 152. Microvalve 180 controls the fluidic path between microchannels 181 and 191. Microvalve 200 controls the fluidic path between microchannels 201 and 212. Microvalve 220 controls the fluidic path between microchannels 221 and 231.

[00194] In one embodiment junctions can connect one or more microchannels. **Figure 5** shows the schematic for a microchip that can be mated with the cartridge shown in **Figure 4**. In **Figure 5**, junction 100 connects to single microchannel 101, junction 140 connects to single microchannel 141, junction 160 connects to single microchannel 161, and junction 230 connects to single microchannel 231. Junction 190 connects to two microchannels 191 and 201. Junction 120 connects to three microchannels 121, 131, and 151. In one embodiment more than three microchannels can be connected to a single junction.

[00195] The microchannels can be fabricated by one or more techniques such as photolithography, molding, embossing, casting, or milling. The microchannels can be manufactured in a material such as glass, plastic, polymer, ceramic, gel, metal, or another suitable solid.

[00196] In one embodiment the cartridge is used in a method of sample enrichment comprising: delivery of a sample to a chamber by a sample port and delivery of paramagnetic particles to a chamber by a reagent port. The paramagnetic particles (e.g. paramagnetic beads) bind to at least one component in the sample (such as DNA, RNA, micro RNA, a protein, a lipid, a polysaccharide or other ligand). The paramagnetic particles are attracted to a wall of a chamber by virtue of the magnetic force exerted by a magnet located outside the chamber. The paramagnetic particles are washed with a wash solution delivered to the chamber comprising the paramagnetic particles by a reagent port, and the wash solution is removed by a waste port. A reagent can be added to elute the component of the sample from the paramagnetic particles and output the sample component to another device for further processing or analysis. A preferred embodiment is to output the component of the sample on the paramagnetic particles.

[00197] In one embodiment a device comprising a microfluidic microchip is used in a method of diagnosis. In one embodiment the diagnosis comprises the detection of an infectious agent in a sample. In one embodiment the infectious agent is a bacteria, virus, fungi, mycoplasma or prion. In another embodiment a device comprising a microfluidic microchip is used in a method of diagnosis of a hereditary disease. In one embodiment the hereditary disease is caused by one or more DNA mutations, such mutations include but are not limited, triplet base expansions, base substitution mutations, deletion mutations, addition mutations, nonsense mutations, premature stop codons, chromosomal deletions, chromosomal duplications, aneuploidy, partial aneuploidy or monosomy. In another embodiment a device comprising a microfluidic microchip is used in a method to diagnose cancer or a predisposition to cancer. In another embodiment a device comprising a microfluidic microchip is used in a method to diagnose a hereditary disease such as autism, downs syndrome, trisomy, Tay-sachs, or other hereditary diseases. In some embodiments a sample used for diagnosis in a device comprising a microfluidic microchip is a blood sample, a mucus sample, a lung lavage

sample, a urine sample, a fecal sample, a skin sample, a hair sample, a semen sample, a vaginal sample, or an amniotic sample.

[00198] In another embodiment a device comprising a microfluidic microchip is used to identify the presence of environmental contamination of an agent. In one embodiment the agent is a biological agent such as bacteria, virus, fungi, or mycoplasma in an environmental sample. In another embodiment the agent is a contaminant agent, such as a pesticide, an herbicide, or a fertilizer. In one embodiment the environmental sample is a soil sample, a water sample, an air sample, a meat sample, a vegetable sample or a fruit sample. In another embodiment, the agent is a genetically modified organism.

[00199] In another embodiment a device comprising a microfluidic microchip is used for genotyping, identification of an individual mammal (such as a human), forensics, gene expression, gene modification, microRNA analysis, or ribotyping.

[00200] In another embodiment a device comprising a microfluidic microchip is used in a method comprising molecular biological analysis, including but not limited to polymerase chain reaction (PCR) amplification of nucleic acids in a sample (such as Allele-specific PCR, Assembly PCR, Asymmetric PCR, Colony PCR, Helicase-dependent amplification, Hot-start PCR, Intersequence-specific (ISSR) PCR, Inverse PCR, Ligation-mediated PCR, Methylation-specific PCR Multiplex Ligation-dependent Probe Amplification, Multiplex-PCR, Nested PCR, Overlap-extension PCR, Quantitative PCR Reverse Transcription PCR -PCR, Thermal asymmetric interlaced -PCR, Touchdown PCR, or PAN-AC PCR), isothermal nucleic acid amplifications, (such as Loop-mediated Isothermal Amplification (LAMP); nick displacement amplification; Helicase Dependant Amplification platform (HDA); and the primase-based Whole Genome Amplification platform (pWGA); single primer isothermal amplification (SPIA) and Ribo-SPIA for RNA; strand displacement amplification (SDA); EXPAR [Van Ness J, Van Ness LK, Galas DJ. (2003) Isothermal reactions for the amplification of oligonucleotides. *Proc Natl Acad Sci U S A.* 100:4504-9.]; rolling circle amplification (RCA); transcription-based amplification system (TAS) and its derivatives include self-sustaining sequence replication (3SR), isothermal nucleic acid sequence-based amplification (NASBA), and transcription-mediated amplification (TMA); ligase chain reaction (LCR)), sequencing reactions of DNA or RNA (such as Maxam-Gilbert sequencing, Sanger chain-termination method, Dye-terminator sequencing Emulsion PCR sequencing, massively parallel sequencing, polony sequencing, sequencing by ligation, sequencing by synthesis, or sequencing by hybridization), restriction fragment length polymorphism (RFLP) analysis, single nucleotide polymorphism (SNP) analysis, short tandem repeat (STR) analysis, microsatellite analysis, DNA fingerprint analysis, DNA footprint analysis, or DNA methylation analysis.

[00201] In one embodiment a cartridge employs beads coupled to a binding moiety, including but not limited to a binding receptor, transferrin, an antibody or a fragment thereof (such as an Fc fragment or an Fab fragment), a lectin, or a DNA or RNA sequence. In another embodiment a cartridge comprises a reagent such as an anti-coagulant, a fixative, a stabilization reagent, a preservative or precipitation reagent.

C. Pneumatic Manifold

[00202] A pneumatic manifold can be integrated with any microchip and/or cartridge described herein to facilitate distribution of air pressure or vacuum. The air pressure or vacuum can be used to actuate valves on the microchip. Alternatively, air pressure or vacuum can be supplied to a cartridge such that air pressure or vacuum is provided to microchannels within the fluidics layer of a microchip which can be used to move fluids or gases within the fluidics layer. A pneumatic manifold provides the air pressure or vacuum to operate microvalves on microchip (2) on cartridge (1) of **Figure 3** or operate microvalves in other devices.

[00203] A pneumatic manifold can be used to mate the pneumatic lines of a microfluidic microchip to external pressure sources. The pneumatic manifold can have ports that align with ports on the pneumatics layer of the microfluidic microchip and ports that can be connected to tubing that connect to the external pressure sources. The ports can be connected by one or more channels that allow for fluid communication of a liquid or gas, or other material between the ports.

[00204] The pneumatic manifold can be interfaced with the microfluidic microchip on any surface of the microchip. The pneumatic manifold can be on the same or different side of the microfluidic microchip as the cartridge. As shown in **Figure 40**, a pneumatic manifold (113) can be placed on a surface of the microfluidic microchip opposite to the cartridge. As well, the pneumatic manifold can be designed such that it only occupies a portion of the surface of microfluidic microchip. The positioning, design, and/or shape of the pneumatic manifold can allow access of other components to the microfluidic microchip. The pneumatic manifold can have a cut-out or annular space that allows other components to be positioned adjacent or proximal to the microfluidic microchip. This can allow, for example, a magnetic component (109) to be placed in proximity of a chamber within the microfluidic microchip.

[00205] A pneumatic manifold can be constructed of any material known to those skilled in the art. For example, the cartridge can be constructed of a plastic, glass, or metal. A plastic material includes any plastic known to those skilled in the art, such as polypropylene, polystyrene, polyethylene, polyethylene terephthalate, polyester, polyamide, poly(vinylchloride), polycarbonate, polyurethane, polyvinylidene chloride, cyclic olefin copolymer, or any combination thereof. The pneumatic manifold can be formed using any technique known to those skilled in the art, such as soft-lithography, conventional lithography, milling, molding, embossing, drilling, etching, or any combination thereof.

[00206] The apparatus shown in **Figure 21** and **Figure 22** can incorporate a pneumatic manifold. The apparatus can be used for sample preparation, as described herein, and can incorporate a cartridge. Cartridge (1), labeled 'cube', is attached to manifold (370) with solenoids (1819). The assembly of the cartridge and manifold is mounted on a base plate of the apparatus. The pneumatic manifold can be controlled by an IO controller (1803).

[00207] A gas supply, such as a reservoir that can be maintained at a desired pressure or vacuum, can supply gas to the manifold. The gas supply can be connected to an outside pressure or vacuum source. The

gas supply feeding the gas supply manifold can have a pressure gauge to monitor the inlet pressure. The gas supply can supply gas to multiple components of the system through a gas supply manifold (1821). The gas supply manifold can supply gas to the pneumatic manifold (370) and to individual reagent containers, (1809) and (1807). The line supplying the distribution valve (390) with gas can be regulated by a regulator (1815).

[00208] Reagents and/or sample can also be supplied to the cartridge through the reagent distribution valve (390) that is connected to containers (1809) in a reagent storage region (380) and a bead solution container (1807) that is mounted on a bead mixer (1805). Adapter (1817) can be mounted and/or aligned with the cartridge such that a delivery device, such as a syringe, can deliver a material to the cartridge. The adapter (1817) can be thermally regulated by a heater control (1801). The adapter can have a thermal conductor, such as brass, to distribute heat generated by heater coil or a Peltier device. The adapter can maintain temperature between about 20 to 100, 20 to 75, or 50 to 60 degrees Celsius.

[00209] A magnet assembly (1811) can be positioned adjacent to the cartridge. A magnet (300) of the magnet assembly can be positioned adjacent to the cartridge (1) and moved by an actuator, such that the magnet can exert a magnetic field within the cartridge, or a microchip integrated, mated, or interfaced with the cartridge. The magnetic field can be used to capture paramagnetic or magnetic particles, such as beads, within the cartridge or microchip and separate material bound to the particles from waste materials. Waste from the cartridge and/or microchip can be delivered to a waste container (1813).

[00210] The apparatus shown in **Figure 21** and **Figure 22** can use seven solenoid valves to operate the cartridge (1). The size and complexity of the apparatus can be further reduced with MOVE microvalves. **Figure 23** and **Figure 24** show a reagent distribution device that contains microfluidic microchip 600, which is approximately two inches wide. Solenoid banks 680 and 684 provide connection to full scale external vacuum and pressure through connectors 681, 682, 685, and 686. The solenoids are controlled through electrical junctions 689 and 687. The microfluidic microchip 600, which has MOVE valves, is held in contact with the manifold 700 by attachment 711 using clamp 710. Other methods known to one skilled in the art can be used to connect the microchip to the pneumatics manifold 700.

D. Parallel Processing of Samples

[00211] In some embodiments of the invention, one or more cartridges can be operated simultaneously to allow for parallel processing of samples. **Figure 16** illustrates parallel or ganged operation of multiple cartridges with microvalves on a single pneumatic manifold in swab extraction assembly (800). The manifold (370) distributes regulated vacuum and pressure to operate four cartridges (1), indicated in the figure, using solenoids (680). Solenoids (680) control pressure to the pneumatic layer of a microchip integrated with each cartridge through the pneumatic manifold (370, 380, 390). The pneumatic manifold is formed by a top plate (370), a gasket (380) and a bottom plate (390). The top plate can have channels etched into it. The channels can be sealed by the gasket, which is sandwiched against the top plate by the bottom plate (390). Actuator 310 moves rod 810 to move magnets (320) close to or away from the cartridges (1). Clamps 805 hold cartridges (1) in place.

[00212] In other embodiments of the invention, a single cartridge integrated with a microchip can process multiple samples at one time using parallel channels. For example, the device can be configured to have 4, 8, or even 12 channels. **Figure 14** and **Figure 15** shows an assembled capture and reaction microchip with capillary feed and magnets. This microchip can capture bead solutions and perform, for example, four, STR-PCR reactions simultaneously. **Figure 14** shows a microchip (1201) with a cartridge (1203) adhered to the microchip and tubes (1205, 1207, 1209, 1211, 1213, 1215, 1217, and 1219) leading into and out of the microchip. A total of eight tubes are shown and two tubes are used per parallel reaction. For example, one unit of the parallel processing device is served by tubes 1205 and 1213.

[00213] In an exemplary embodiment, a four-channel sample preparation device combines a four-channel parallel reagent delivery device (**Figure 53**) that meters and delivers reagents simultaneously to all four channels of a single integrated cartridge (**Figure 54**) enabling four samples to be processed simultaneously and rapidly.

[00214] The four-channel parallel reagent delivery device combines a microchip (see **Figure 53**) with a fluidics manifold mounted on a pneumatics control manifold. **Figure 53** shows a sample extraction module comprises a cartridge mated to a microfluidic chip. The cartridge comprises apertures for syringes (6701) and compartments for bead capture of analyte (6702). These compartments are fluidically connected through channels (6703) in a microfluidic chip mated to the undersurface of the cartridge. A reagent distribution cartridge can comprise compartments configured similar to those in **Figure 3**. The two can be fluidically connected, e.g., by tubes, and reagents can be pumped from reagent reservoirs into the chambers on the reagent cartridge and then into the sample extraction module. 4, 8, 12 channel and devices with more channels are contemplated. Reagents are metered, using one of the two different size reagent loops, which can be similar to the sample loops described herein, for each channel, and delivered in parallel to all four channels of the sample preparation device. Delivering reagents simultaneously to all four channels of the sample preparation device using the parallel reagent delivery device can takes <4 minutes, representing a process time saving of >11 minutes as compared to the first generation serial reagent delivery device that took ~15 minutes per four samples processed.

[00215] Bonded pneumatics manifolds can be used to control both the reagent delivery and sample preparation devices by fabricating the manifolds using an adhesive bonding approach; however, these may be prone to delamination over time due to the pneumatic pressures used in the subsystem, and the size and complexity of the manifold. Thermally bonded manifolds can mitigate delamination issues, but may only be a viable approach for relatively small and low complexity manifold designs such as the reagent delivery device. A monolithic manifold made from a single piece of polycarbonate with tubing connecting pneumatic ports to the solenoid control valves can operate the four-channel sample preparation cartridge and has proved to be a viable alternative to bonded pneumatic manifolds. This pneumatic manifold design concept is also being utilized for control of the Chip A microchip on the Post-amplification STR (Short Tandem Repeat) clean-up subsystem.

[00216] Assembly processes for the microchip and fluidic manifold of the four-channel sample preparation cartridge have also been improved. Historically, silicon epoxy can be used to attach the cartridge to its associated MOVE microchip by wicking the adhesive between the microchip and the cube. An inherent lack of control of the movement of the epoxy can allow it to occasionally wick into the ports on either the microchip or the cube creating a blockage in the fluidic pathway rendering the device unusable. This process has been improved by using a double-sided adhesive tape (Adhesives Research ARcare90106) to assemble the fluidic cubes and microchips; this is now the preferred assembly method used for the four-channel reagent delivery cartridge, the sample preparation device, and the post amplification device in the Post-amplification STR clean-up subsystem described below.

[00217] The integrated four-channel sample preparation cartridge with the 069 microchip (see **Figure 55**) was tested. The 069 microchip design is used with the sample extraction cartridge. Other chips, for example the 070 chip is used with the post-amplification cartridge.

[00218] Microchip blockages due to the inadvertent introduction of fibers into the systems and devices described herein can be problematic in microfluidics. To minimize blockages, all reagents with the exception of paramagnetic bead solutions, can be filtered prior to loading and in-line filters used to minimize microchip blockages.

E. Separation and Cleanup

[00219] A variety of separations can be performed using the devices described herein. These separations include chromatographic, affinity, electrostatic, hydrophobic, ion-exchange, magnetic, drag-based, and density-based separations. In some embodiments of the invention, affinity or ion-exchange interactions are utilized to bind materials to solid-phase materials, such as beads. The beads can be separated from fluid solutions using any method known to those skilled in the art.

[00220] Magnetic separation can be used to capture and concentrate materials in a single step using a mechanistically simplified format that employs paramagnetic beads and a magnetic field. The beads can be used to capture, concentrate, and then purify specific target antigens, proteins, carbohydrates, toxins, nucleic acids, cells, viruses, and spores. The beads can have a specific affinity reagent, typically an antibody, aptamer, or DNA that binds to a target. Alternatively electrostatic or ion-pairing or salt-bridge interactions can bind to a target. The beads can be paramagnetic beads that are only magnetic in the presence of an external magnetic field. Alternatively, the beads can contain permanent magnets. The beads can be added to complex samples such as aerosols, liquids, bodily fluids, extracts, or food. After (or before) binding of a target material, such as DNA, the bead can be captured by application of a magnetic field. Unbound or loosely bound material is removed by washing with compatible buffers, which purifies the target from other, unwanted materials in the original sample. Beads can be small (nm to μm) and can bind high amounts of target. When the beads are concentrated by magnetic force they can form bead beds of just nL- μL volumes, thus concentrating the target at the same time it is purified. The purified and concentrated targets can be

conveniently transported, denatured, lysed or analyzed while on-bead, or eluted off the bead for further sample preparation, or analysis.

[00221] Separations are widely used for many applications including the detection of microorganisms in food, bodily fluids, and other matrices. Paramagnetic beads can be mixed and manipulated easily, and are adaptable to microscale and microfluidic applications. This technology provides an excellent solution to the macroscale-to-microscale interface: beads can purify samples at the macroscale and then concentrate to the nanoscale (100's of nL) for introduction into microfluidic or nanofluidic platforms. Magnetic separations can be used as an upstream purification step before real-time PCR, electrochemiluminescence, magnetic force discrimination, magnetophoretic, capillary electrophoresis, field-flow separations, or other separation methods well known to one skilled in the art.

[00222] The devices of the invention can accommodate the use of magnetic beads. For example, beads or bead slurry can be supplied to a port of a cartridge. The beads can be mixed or suspended in solution within the cartridge using pumping, magnetic fields, or external mixers. The beads can then be pumped to desired chambers or reservoirs within the microfluidic device or cartridge. Beads can be captured within a chamber using a magnetic field. Beads in a solution can be captured as the solution travels through the magnetic field, or beads can be captured in a stagnant solution.

[00223] To illustrate methods of use of the cartridge, several examples are contemplated. The first example is processing of nucleic acid from a buccal swab with paramagnetic beads to purify the sample followed by PCR amplification and bead purification of the PCR products. A second example describes performing immunomagnetic separations to purify cells, proteins, or other antigenic material using a binding moiety coupled to beads. A third example describes performing molecular biology to prepare samples for sequencing technologies such as sequencing by synthesis, sequencing by hybridization, or sequencing by ligation. It would be known to one skilled in the art that many different chemistries and biochemistries can be used with the instant invention. These include, but are not limited to, enzymatic reactions, purifications on gels, monoliths, beads, packed beds, surface reactions, molecular biology, and other chemical and biochemical reactions.

[00224] The cartridge with integrated microchip can be formed of any cartridge and microchip described herein. For example, the cartridge and microchip shown in **Figure 3**, **Figure 4**, and **Figure 5**. A movable magnet (300) can be positioned adjacent to the cartridge. The movable magnet can be moved by an actuator (310). The movable magnet can be used to apply a magnetic field within the cartridge or the microchip. In some embodiments, the movable magnet can be used to facilitate gathering or collecting of beads against a wall of a chamber within the cartridge or the microchip.

II. Reaction Module

[00225] The reaction module typically will comprise a reaction chamber fluidically connected to a microfluidic channel and the sample preparation chamber through which the analyte passes. The reaction module can be adapted to place the analyte in a volume, e.g. a non-microfluidic volume, that is smaller than the original sample volume. For example, the reaction module can comprise a chamber in communication with a magnetic force that is adapted to immobilize magnetically responsive particles on which the analyte is captured. The bead bed typically has a volume that is smaller than the original sample volume. The analyte can be released from to particles in the reaction chamber and a biochemical reaction, such as PCR, can be performed on the analyte. The liquid volume in reaction chamber can be a non-microfluidic volume e.g. between 10 and 50 microliters. Accordingly, the use of analyte capture materials that are flowable and immobilizable allows capture, transfer and concentration of the analyte.

[00226] As shown in **Figure 6**, temperature modulator can be fluidically connected to the cartridge and microchip through reaction channel (250). The reaction chamber (250) can be connected at an end (251) to the cartridge. The temperature modulator can be used for thermal cycling the temperature of a reaction channel (250) containing a reaction mixture and a nucleic acid enriched from a sample (collectively referred to as the PCR reaction sample). A control mechanism can be used for controlling the operation of the temperature modulator. An optical assembly can be used to monitor or control the reaction. The optical assembly can introduce or detect light. For example, an optical assembly 410 can be used for performing Real-time PCR or other real-time or end point measurements. In certain embodiments the temperature modulator employs a thermo-coupled Peltier thermoelectric module, a conventional thermoelectric module, hot air, infrared light or microwave. In one embodiment the temperature modulator uses a Peltier thermoelectric module external to the reaction channel to heat and cool the PCR reaction sample as desired. The heating and cooling of the thermoelectric module can be distributed over a region 350. Additional views of the temperature modulator 400 are shown in **Figure 7** and **Figure 8**. **Figure 7** shows the reaction channel 250 in contact with a temperature controlled region 350. The temperature modulator can also include a movable magnet 320 that is positioned by an actuator 330. The movable magnet can be used to capture magnetic particles at position 340, as shown in **Figure 6**. In some embodiments of the invention, the temperature controlled region comprises two parts. The two parts can be parts of a clamshell that are clamped, locked, or held together to maintain thermal contact with the reaction channel 250. One portion of the temperature controlled region, portion 711 of **Figure 8**, can be hinged to the second portion of the temperature controlled region. The temperature controlled regions can have grooved channels for positioning of one or more reaction channels, as shown on the right side of **Figure 7** and in **Figure 8**. The left side of **Figure 7** shows the temperature controlled region in a closed configuration. Additionally, the temperature controlled region can comprise one or more constriction components, shown as 709 and 701 in **Figure 8**. The constricting points can pinch the reaction channel such that a portion of the reaction channel is isolated from another portion of the reaction channel. In some embodiments of the invention, the reaction channel is pinched in two locations such that a body of fluid, such as a reaction mixture, is isolated.

Constriction components 709 and 701 can mate with additional constriction components 707 and 705 to facilitate pinching of the reaction channel.

[00227] Alternatively the temperature modulator can constrict the reaction tubing using a pinch clamp, as shown in **Figure 51**. Use of the pinch clamp, which can be formed of a plastic such as Ultem, can reduce heat transfer to the reaction channel. The reduction in heat transfer can reduce the likelihood that the reaction channel has for being welded closed during thermocycling or temperature regulation. Alternatively, different material tubing can be used as the reaction channel to ensure that the reaction channel can maintain its shape before and after the thermocycling or temperature regulation process. Different material tubing can also be used to reduce rate of evaporation during the temperature modulating process. Example materials include ethylvinyl acetate, silicone, and silanized c-flex tubing.

[00228] The temperature modulating device can modulate temperatures at a rate of 0.5 to over 3 degrees Celsius per second. The heater can utilize about 25 to 100 Watts and a fan, which can be used to cool the temperature modulating device, can produce an air flow rate of at least about 75, 100, 130, 150, 200, 250, or 300 cfm.

[00229] In one embodiment a sample preparation device comprising a cartridge integrated with a microfluidic microchip, which can be used to control the movement of fluid in the cartridge, can be used in conjunction with a temperature modulator 400 as a flow-through PCR thermal cycler. Driving force for moving the fluid can be an external pressure source or an internal pressure source, such as a MOVE valves within the microchip. A flow-through PCR thermal cycler can be used when highly sensitive or high throughput PCR is desired. There are many situations in which one might want to sample air, blood, water, saliva, a cellular sample, or other medium in a sensitive PCR assay. This can be used to detect a variety of biological contaminants including influenza, bacterial pathogens, and any number of viral or bacterial pathogens. Flow-through PCR can allow PCR to be practiced in an automated manner without the need for human interaction. A flow-through PCR system can also serve as an early warning system in HVAC systems of buildings, airplanes, busses, and other vehicles, and can be used in the monitoring of blood, water, or other sample sources for the presence of an infectious agent or a contaminant.

[00230] As shown in **Figure 6**, the flow-through PCR device takes a sample from a collection device, such as a buccal swab, a syringe, an air sampler, fluid sampler or other sampler and delivers it to a sample preparation device 1 (**Figure 6** is not necessarily drawn to scale). The sample is prepared in the preparation device 1, which in some embodiments may include cell lysis, DNA, RNA, or micro RNA enrichment or purification, filtration, or reverse transcription. In one embodiment at least one nucleic acid is enriched. In another embodiment at least one enriched nucleic acid is prepared for PCR by adding the nucleic acid to PCR reagents (such as at least one DNA polymerase, RNA polymerase, dNTPs, buffer or a salt) and primers, (such as assay-specific primers or broadly applicable primer sets for multiple target pathogens). These primers may be chosen to selectively amplify at least one nucleic acid isolated from a specific pathogen (such as a mold, virus, bacteria, parasite or amoeba), gene, other desired nucleic acid, or any combination

thereof. The composition comprising at least one nucleic acid enriched from a sample, PCR reagents and primers is called a PCR reaction sample. In one embodiment, the flowthrough PCR can be used as a continuous flow device while in other embodiments samples are moved into the thermal cycling region and stopped.

[00231] The PCR reaction sample then flows through a reaction channel (250) to a temperature controlled device or region (350). In some embodiments the reaction channel is clear or transparent. In another embodiment the reaction channel is opaque. In one embodiment the reaction channel is a cylinder. In another embodiment the reaction channel's cross section comprises one or more planes forming a shape such as a triangle, square, rectangle, pentagon, hexagon, heptagon, octagon, nonagon, decagon, or other polygon. In one embodiment the volume of PCR reaction sample is such that it takes up a small discrete length of space in the reaction channel, the rest of which is occupied by air, gas, or a non-reactive liquid, such as mineral oil. Air, gas, or a non-reactive liquid can be used to separate individual PCR reaction samples from each other. In one embodiment the temperature controlled region (350) is thermally modulated by one or more modules, including but not limited to thermo-coupled Peltier thermoelectric module, a conventional thermoelectric module, hot air, microwave, or infrared light. In one embodiment the thermal cycler uses Peltier thermoelectric modules external to the tube to heat and cool the sample as desired. In one embodiment a detection module (410) measures fluorescence, luminescence, absorbance or other optical properties to detect a signal emitted from a PCR reaction sample while it is located with a temperature control region, or after it has left a temperature control region. A detection module can comprise a light source (such as a coherent light source or incoherent light source) used to excite a fluorescent dye (such as an intercalating dye, including but not limited to ethidium bromide or Syber green) in a PCR reaction sample, and the excitation light is sensed with a photodetector (such as a CCD, CMOS, PMT, or other optical detector). Detection electronics can evaluate the signal sent from the detection module (410).

[00232] In one embodiment, after the desired number of thermal cycles are complete, the PCR reaction sample is pumped or pushed further down the reaction channel, using pressure or vacuum, exiting the temperature controlled region and passing into a second microfluidic microchip (500). The second microchip (500) can be attached at end (252) to the reaction channel (250). Microfluidic microchip (500) can comprise microvalves (510, 520, 530, and 545). Any three microvalves such as 510, 520, and 530 or 510, 520, and 545 can form a pump. Microchannels 505, 515, 525, and 540 can connect the pumps on the microchip. Downstream devices 535 and 550 can be connected to the microchip. Flow of material to devices (535 and 550) can be controlled by the microvalves, for example, by keeping either valve 530 or 545 closed while pumping or moving fluid. In one preferred embodiment, the downstream device are analytical devices that can be used for performing electrophoresis, mass spectroscopy, or other analytical techniques known to one skilled in the art.

III. Post-Reaction Module

[00233] In certain embodiments, after the biochemical reaction is complete, the reaction product is processed before analysis. The system can include a post-reaction module adapted to process the reaction product. The post-reaction module can comprise a microfluidic device comprising on-device valves and pumps adapted to route a fluid comprising the reaction product through a microfluidic channel into a processing chamber e.g., a non-microfluidic chamber. For example, if the biochemical reaction is DNA amplification, e.g., PCR, and analysis involves e.g. capillary electrophoresis, processing can involve adjusting the salt concentration of the product containing volume. This can involve for example, diluting the reaction product volume.

[00234] In another embodiment multiple reaction channels may be used in parallel to increase sample throughput. In yet another embodiment the system may alert the user when amplification has occurred (a positive result), indicating that the target sequence is present. In one embodiment a reaction channel is used for a single use only, then disposed of. In an alternative embodiment a reaction channels can be used to amplify and detect the presence or absence of PCR amplification products in multiple samples. More than one PCR reaction samples can be loaded at intervals and interspaced with a barrier bolus of gas or liquid to prevent intermixing. In one embodiment samples are spaced apart in a manner so that as one is undergoing thermal cycling another sample is in the detection region undergoing interrogation. It will be obvious to one skilled in the art that the PCR amplification can be replaced by other nucleic acid amplification technologies which may use thermal cycling or be isothermal reactions.

[00235] In other embodiments, the device can perform isothermal reactions such as sandwich assays using affinity reagents such as antibodies or aptamers to determine if cells, proteins, toxins, or other targets are present with the detection module (**Figure 6, 410**) providing a reading of the amount of target present. In these applications, the cartridge 1 may perform an affinity purification such as an IMS purification and then add a secondary antibody that may have a fluorescent label attached. The sample can then move into region 350 where the thermal control is set to optimize the reaction. Detection module (410) can then monitor the reaction. In one embodiment, a plurality of cartridges are ganged to reaction channel (250) and a series of boluses can be readout with detector 410.

IV. Device for Product Analysis (e.g., Capillary Electrophoresis)

[00236] In one embodiment a complete sample-to-answer system is provide, which can comprise microfluidics, requiring coupling all steps together to match volumes and concentrations. Sample analysis using capillary electrophoresis is a standard analytical method that can be used with microfluidic sample preparation methods as described above. Capillary electrophoresis is readily adaptable to microfluidic microchips. In the instant invention, capillary electrophoresis on microchips is combined with MOVE valves

to provide control of samples, process beads to concentrate the samples, and improve the loading and separations.

[00237] **Figure 48** show a sample source 6009 connected to a sample channel 6005, also referred to as a loading channel, that is mated with a separation channel 6011. Two electrodes, 6003 and 6001, can be used to apply an electric field to the separation channel. In some embodiments of the invention, the sample source can pass through a MOVE pump in a microchip used to drive fluid flow within the sample channel. The sample channel can be a microfluidic channel or an injection tubing. The injection tubing can be flexible tubing or another flexible connector. Examples of flexible tubing include polytetrafluoroethylene tubing or silicon tubing. The flexible connector can also connect to another cartridge interfaced with a microchip. Alternatively, the flexible connector can return to the cartridge that it originated from. The separation channel can be a microfluidic channel, capillary tubing, or capillary electrophoresis tubing. The capillary tubing can have an outer diameter of about 150 to 500 microns and an inner diameter of about 10 to 100 microns. The capillary can be polyimide or polytetrafluoroethylene clad. The capillary can be about 2 to 100 cm long. The capillary can be mated to the injection tubing or flexible tubing by first drilling a hole into the injection tubing and then inserting the capillary into the flexible tubing. Alternatively, the capillary can be inserted into the flexible tubing without having to pre-drill the flexible tubing.

[00238] One of the two electrodes, for example electrode 6003, can be a cathode and the other electrode, for example 6001, can be an anode. The cathode can be any cathode, such as a forked cathode, described herein. The anode can be connected to the separation channel using any devices known to those skilled in the art. For example, the separation channel can be joined to a reservoir by an Upchurch fitting, which is in electrical contact with the anode, which can be a metallic electrode.

[00239] In some embodiments of the invention, a stabilizing component, shown at the intersection of a separation capillary and injection tubing in **Figure 49**, can be used to align, seal, and/or protect the connection between the separation capillary and the injection tubing. In some embodiments of the invention, multiple injection tubings are aligned with multiple separation capillaries using a stabilizing component. As shown in **Figure 50**, the stabilizing component can hold four injection tubings, shown as the vertical tubings in the figure, and stabilize the connection with four separation capillaries (not shown).

[00240] Panels 1-6 of **Figure 48** show a process for injecting a sample into a separation channel. In panel 1, no sample is present in the sample channel 6005. In panel 2, sample entering the sample channel from the sample source (6009) is shown. As sample is moved down the sample channel, the sample intersects the separation capillary, as shown in panel 3. The sample can be isolated by boluses of gas upstream and downstream to the sample. Once sample is adjacent to the separation channel, an electric field, which can be between 25 and 500 V/cm, is applied between a first electrode 6003, which can be a cathode or a forked cathode, and a second electrode 6001, which can be an anode. Electrophoresis buffer, shown entering into the sample channel from the sample source, can also enter the sample channel, as shown in panel 3. The voltage potential and/or current between the anode and cathode can drop when an air bolus

passes by the junction between the sample channel and the separation channel, reducing or preventing the injection of air into the separation channel. The voltage potential and/or current drop can be detected to ascertain when the sample and/or electrophoresis buffer is adjacent to the separation channel. Once the electrophoresis buffer is adjacent to the separation channel, as shown in panel 5, the current and/or voltage drop between the anode and cathode can be increased. This can allow for the separation of the analyte in the separation channel, as shown in panel 6, as the electrophoresis buffer provides ions for a high performance separation.

[00241] In one embodiment for STR analysis, the injection process is as follows:

- A. The microfluidic channels can be filled with buffer.
- B. The separation channel can be filled with gel while buffer is pulled across the sample channel, thus sweeping the separation polymer from the cross section formed by the separation and sample channels.
- C. The STR amplified sample (desalted and captured on beads) can be captured on microchip 500, eluted in a low conductivity fluid (water) containing the size standard, and pumped into the sample channel with MOVE technology.
- D. A field can be applied across the cathode and anode, with “pull back” voltage on the sample and waste arms, to drive the sample into the separation channel where it stacks at the head of the separation polymer. As the sample is injected the conductivity of the sample channel can quickly equilibrate with the buffer in the cathode arms providing a single step injection.

[00242] The forked electrode or cathode can be two metallic conductors, as shown in **Figure 46**. The fluid path for a sample to be analyzed, as shown in **Figure 46**, can be along a loading channel. When the location of the sample is adjacent to the separation channel, the forked electrode can be used to inject the sample into the separation channel, as described herein. The conductance of the material in the sample channel can be lower than the conductance of the material in the separation channel, which can be a separation polymer. The difference in conductance can cause sample stacking when an electric field is applied through the forked electrode, which can be a cathode, and a downstream electrode, which can be an anode. The polarity of the forked electrode and the downstream electrode can be reversed such that the forked cathode is the anode and the downstream electrode is the cathode.

[00243] In some embodiments of the invention, an additional electrode can be used to reduce injection of gas into the separation channel or formation of bubbles within the sample loading channel which can lead to loss of the applied field on the separation channel. Injection of gas into the separation channel or formation of bubbles within the sample loading channel can cause inconsistent separation of analytes and can be detected by inconsistent current between the anode and cathode used to apply an electric field to the separation channel. Use of an additional electrode to circumvent or reduce injection of gas or bubbles into

the separation channel is shown in **Figure 47**. The additional electrode can be a single wire run electrode or a cannular run electrode. The increased surface area and/or larger internal diameter of the cannular run electrode can allow for a significant reduction in bubble formation or blockage and/or injection into the separation channel. In some embodiments of the invention, the cannula used for the cannular run electrode and has an inner diameter of at least about 1/64, 1/32, 1/16, 1/8, or 1/4 inches.

[00244] In another embodiment shown in **Figure 96 A and B**, the three-prong electrode arrangement can be used to pre-concentrate analytes before injection. In this method, the outside electrodes are given a charge the same as that of the analyte, and the electrode between them and opposite the electrophoresis capillary is given a charge opposite that of the analyte. For example, in the case of nucleic acids, which are negatively charged, the outside electrodes are given a negative charge and the middle electrode is given a positive charge. This causes the analyte to become concentrated between the flanking electrodes and toward the middle electrode. Then, the charge on the middle electrode is reversed and a voltage is placed across the electrophoresis capillary. This moves the analytes through the capillary tube. The shown electrode configuration for a capillary electrophoresis injector may include a forked electrode and another electrode. Both configurations shown include a forked electrode having two points of contact located distally to the connection with the electrophoresis capillary one electrode directly across from the lumen of the capillary. In one embodiment, the second electrode is a third fork in the forked electrode. In a second embodiment the second electrode is not on the same circuit as the other electrodes. This allows two circuit paths to be employed at the injector. In one method of using the three-electrode arrangement, the sample is moved into place opposite the capillary using the fluidic system. Then, the sample is injected into the capillary using only the middle electrode which is opposite the capillary. Then, the middle electrode is turned off, the flanking electrodes are turned on and are used to electrophorese the analytes through the capillary.

[00245] This invention provides a device for regulating temperature of electrophoresis capillaries, for example an array of capillaries. An embodiment is shown in **Figure 98B**. The electrically insulating circuit board has a generally S-shaped path for placement of capillaries. The generally S-shaped path is broken up into 6 different sections, 12, 14, 16, 18, 20, and 22. These 6 different sections, 12, 14, 16, 18, 20, and 22 separately regulate the temperature in the portion of a capillary in thermal contact with the particular section. Each of the different sections, 12, 14, 16, 18, 20, and 22 is filled with an electrical path that runs back and forth, e.g. in a serpentine shape in that section's area to fill that section's area. This electrical path that runs back and forth is shown in detail in section 22. Although not shown for purposes of clarity in the illustration, the other sections 12, 14, 16, 18, and 20 also are filled with an electrical path that runs back and forth in that section's area to fill that section's area.

[00246] The circuit board also has a row of apertures 10 that run along both sides of the generally S-shaped path for placement of capillaries. The apertures reduce heat transfer between the generally S-shaped path of the circuit board, and a remainder of the circuit board. Because air is a good thermal insulator, heat transfer is reduced between there two parts of the circuit board. The circuit board itself is also a poor thermal

conductor. In another embodiment, instead of rows of apertures, poor thermal conductive material is positioned between these two parts of the circuit board. Such reduction of heat transfer eases thermal regulation of the generally S-shaped path and the capillaries placed on the generally S-shaped path. The apertures serve to reduce the thermal mass of the thermally regulated region to substantially the generally S-shaped path and the capillaries placed on the generally S-shaped path. With less thermal mass, a desired temperature is reached more quickly for the generally S-shaped path and the capillaries placed on the generally S-shaped path.

[00247] The circuit board also includes an aperture 8 along the generally S-shaped path toward the exiting end of the generally S-shaped path. Because of the absence of circuit board material, the aperture 8 facilitates optical interaction with a capillary which is placed over the aperture 8. The aperture 8 allows for fluorescence excitation and detection using an optical configuration such as epi-fluorescent, and various skew illumination schemes.

[00248] The electrical path in various embodiments is a patterned, or etched, conductive trace bonded onto the electrically insulating circuit board. The patterned electrical path may be defined by “subtractive” patterning that removes unwanted conductive material to leave the desired conductive paths, or by “additive” patterning that adds additional conductive material to form the desired conductive paths. The circuit board may have the conductive paths on a single layer circuit board or as part of a multi-layer circuit board.

[00249] Various examples of conductive material in the electrical path are metallic material such as copper, aluminum, silver, or nonmetallic conductive material such as graphite, or conductive ink, but may be any other conductive material.

[00250] In contrast with the conductive material of the electrical path, the circuit board material is nonconductive, commonly a dielectric material.

[00251] Each electrical path creates and defines a thermal area. In one exemplary embodiment, six heating areas, each comprised of approximately 1m of 150um wide copper traces that is folded into the shape needed to generate the heater shapes shown below. Various embodiments vary the length of the trace to shorter or longer than 1m, depending on a length adequate for electrophoretic separation of analytes. Various embodiments widen or narrow the width of the electrical paths, depending on an adequate resistance of the electrical paths to generate adequate heat for thermal regulation of the thermally coupled capillaries. Various embodiments increase or decrease the number of heating areas.

[00252] In some embodiments, an electrical path such as a trace has a width in the range between 0.0001 to 0.5 inches, and a length in the range between 0.25 to 750 inches.

[00253] Performing electrophoresis in a capillary allows the heat to be effectively dissipated through the capillary walls. This allows high voltages to be used to achieve rapid separations.

[00254] **Figure 2** is a top view of a thermal assembly, with a circuit board, electrical paths on the circuit board, a bundle of capillaries, and temperature sensors.

[00255] On a circuit board such as the circuit board shown in **Figure 98A**, electrophoresis capillaries are attached to the generally S-shaped path, such as by adhesive material. In the shown embodiment, a bundle of 8 capillaries are attached. Other embodiments have any other number of capillaries ranging from 1 to a higher number, depending on a particular electrophoresis application's requirements for parallel processing of analytes. The entering end 54 of the capillaries have fanned out ends, to facilitate injection of analytes into the different capillaries. The exiting end 56 of the capillaries remains bundled together in the figure.

[00256] In each of the separately thermally regulated areas or sections of the generally S-shaped path, a temperature sensor is in thermal contact. The temperature sensors shown are 32, 34, 36, 38, 40, and 42. Temperature sensor 42 is in thermal contact not with the capillaries, but the circuit board itself, or alternatively the ambient air. Examples of temperature sensors are thermistors or other temperature-varying resistance, or thermocouples or other temperature-varying voltage source. In another embodiment, the temperature data of the separately thermally regulated sections is not gathered by discrete temperature sensor, but by the electrical paths themselves such as by the resistances of the electrical paths.

[00257] In the shown embodiment, temperature sensors are thermistors that are attached to traces that terminate on a portion of the circuit board outside of the array of thermal insulation apertures. The thermistors are folded down across the capillary array and embedded in the adhesive that bonds the capillary array to the board, to ensure good thermal contact between the thermistors and the capillaries, while minimizing thermal loss from the heaters.

[00258] The temperature data generated by such temperature sensors help to thermally regulate the temperature of the capillaries in thermal contact with the electrical paths. Electrical current through the electrical path deposits thermal energy in the electrical path via Joule heating. The amount of deposited thermal energy varies with the amount of electrical current and resistance of the electrical paths.

[00259] In one embodiment, the invention provides a portable eight-channel integrated automated sample-to-answer DNA forensics device. Such a device accepts buccal swab samples or blood samples; performs STR analysis; and outputs CODIS file ready for interrogation against a database.

[00260] In another embodiment, the invention provides an automated analysis for short term repeats in a sample, wherein the method comprises extracting and purifying a sample comprising an analyte comprising a short term repeat nucleic acid sequence; amplifying the short term repeat nucleic acid sequence; purifying the short term repeat nucleic acid sequence; and performing capillary electrophoresis on purified short term repeat nucleic acid sequence to determine the size of the short term repeat nucleic acid sequence.

[00261] Using standard technologies, the process from biological sample (e.g., cheek swab) to data output of a CODIS file requires more than six hours. This includes DNA extraction, qPCR, DNA normalization, STR amplification with labeled primers, post-reaction sample preparation, CE analysis and data analysis. The system of the present invention can perform this entire process in less than 5 hours, less than 4 hours less than 3 hours or even less than 2 hours.

[00262] In another embodiment, the invention provides an automated analysis for short term repeats wherein the success rate of getting the correct STR from a raw or otherwise unpurified sample is at least 60%, at least 65%, at least 70%, at least 75%, at least 80%, at least 85%, at least 90%, at least 95%, at least 96%, at least 97%, or at least 98%.

A. Detector

[00263] In one aspect, this invention provides an optical system for detecting analytes in an array of capillaries, e.g. an array of 4, an array of 8 or an array of up to 12 capillaries. In this system, the objective lens moves in relation to the capillaries, the excitation source, and the collection optics. As the objective moves, the excitation light passes through a different part of the lens and is focused at a different point in the region of the capillaries. Movement of the objective results in translation of the point of focus so that, so that each capillary can, in turn, be scanned.

[00264] In **Figure 99**, the excitation source of the excitation beam 170 is a solid state laser, the output of which is projected into the capillary 174 using a beam combiner 162 placed at a 45 degree angle in the optical path immediately above the objective 160. In various embodiments the beam combiner comprises a wavelength sensitive reflector or a spatial beam splitter such as a small reflective dot placed on a transparent sheet of glass. The beam combiner is wavelength dependent, which is easier to align than a spatial beam combiner.

[00265] The high numerical aperture objective is used both by the excitation beam 170 on its way to the capillary 174, and by the optical signal of emitted fluorescence from the capillary 174.

[00266] The optical signal of fluorescence emitted from the analytes of the capillary 174 is collimated by the objective 160. The optical signal passes through the wavelength sensitive reflector 162 and impinges on a long pass filter 164 that rejects the portion of the optical signal including the excitation beam 170.

[00267] The fluorescence detection scheme is prism spectrometer based. The optical signal is then projected onto a dispersive prism 166, which serves to change the angle of the rays according to wavelength. This dispersed optical signal is then focused on the plane of the detector 170 using an image forming lens 168, causing different wavelengths of the dispersed optical signal to focus at different locations in the plane of the detector 170. An example of the detector 170 is a CCD camera. An alternative is a CMOS camera or other optical sensors.

[00268] With an array that comprises 30um diameter capillaries, the scan range for the detection device covers +/- 0.8 mm for an eight channel array. This limited scan range minimizes the number of moving parts. Other embodiments widen or narrow the scan range to accommodate a different number of capillaries and/or different number of capillaries. As only the objective 160 moves, the excitation laser beam 170 remains very close to the center of the objective 160, even when the beam 170 is located at the top of the end capillary in the array. The excitation beam 170 impinges on the capillaries at different angles depending on the location of the capillary in the array.

V. Integrated Analysis System with Disposable Cartridge

[00269] The invention provides for an integrated analysis system that can interface with a disposable cartridge that integrates several functions of the system, including sample extraction, thermal cycling, and post-amplification processing. The integrated analysis system and disposable cartridge can be used to analyze a sample obtained from a source and provide information regarding the source. For example, the system and cartridge can be used to extract nucleic acid from a plurality of samples and analyze the extracted nucleic acids for short tandem repeats to obtain genetic information regarding the source.

[00270] An overview of the integrated analysis system and disposable cartridge is shown in **Figure 63**. The integrated analysis system can include hardware, consumables, software, and documentation. As shown in **Figure 64**, the hardware components of the integrated analysis system can include one or more enclosures, electronics, pneumatics, optics, thermocyclers, electrophoresis systems, and cartridge covers. Additional components of the hardware are shown in **Figure 64**. The integrated analysis system can also include one or more control systems, power systems, computers, and displays. As shown in **Figure 65**, the software components of the integrated analysis system can include software providing for a graphical user interface, data analysis, a core, and scripts. The core can be used for the control of the hardware. The scripts can be programs that are run. The programs can correspond to particular analytical procedures.

[00271] As shown in **Figure 66**, the consumables can include one or more capillary arrays, reagent cards, cartridges, and separation polymer cartridges. The reagent cards can include reagents for performing analytical reactions. The cartridge can include chambers for receiving samples and chips having one or more pneumatically actuated valves for controlling fluid transport. Other consumable components are shown in **Figure 66**.

[00272] **Figure 67** shows documentation that can be included with the integrated analysis system. Documentation can include test documentation, manuals, project documentation, requirements and specifications, product documentation, and risk management.

[00273] The integrated analysis system and disposable cartridge can be enclosed in a container having a total volume of less than about 10 ft³, less than about 5 ft³, less than about 3 ft³, less than about 2 ft³, or up to about 1 ft³, such as a Pelican model 1610 case. The pelican case #1610 @ 2.2 ft³ can be used to contain all system parts including user control and spare cartridges. The dimensions of the container can be up to about or about 22 x 17 x 11 inches. The container can have wheels and handles for facilitating transportation of the system. The container can be padded or reinforced such that the system is protected from damage during transportation or use. The container can be securely closed or have one or more alarms to prevent and/or deter unintended entry and/or theft. An example of an encased and integrated analysis system is shown in **Figure 68**. Accordingly, this system incorporates into a suitcase-sized container instrumentation to accept a biological sample and produce an analysis of the genetic content of that sample. The system is multiplexed

and can perform a plurality of operations at once, for example, at least 2, at least 4, at least 6, at least 8, at least 10, or even at least 12, or more samples in parallel. In a specific embodiment, the system can perform 2, 4, 6, or 8 samples in parallel.

[00274] The case load can be <50 kg and can be shipped without protection. No additional packaging may be required, enabling rapid deployment of the device. The lid can be opened and the device can be plugged in upon arrival. The small size and two man lift can enable setup and transfer without need for lift equipment. In some embodiments of the invention, the system includes an internal power source or a power generator. The internal power source can be a battery for powering the system in the absence of an electrical source. The battery can be a rechargeable battery or can be a non-rechargeable battery. The power generator can be a fuel cell, a solar cell, or any other type of power generator known to one skilled in the art.

[00275] The container or case can also have one or more internal enclosures. The internal enclosures can protect hardware from damage or spills. An example of an internal enclosure is shown in **Figure 68**. The internal enclosure has two vents with radial cutouts to allow for air-flow. **Figure 69** shows the system with the internal enclosure (1.0, bottom right) removed from the container, exposing the hardware of the integrated analysis system. **Figure 69** also indicates the location of the optics (4.0), pneumatics (3.0), cartridge (10.0), thermocyclers (5.0), cartridge cover (7.0), reagent card (9.0), and electronics (2.0).

[00276] Under operation, the system may draw hundreds of watts which may need to be exhausted from the chassis. Two rotary fans can draw air through a set of filters and provide sufficient cooling to maintain the internal chassis air temperature within 5°C of ambient with two fans and <10°C with a single fan. Fans can be brushless type to increase life time to >25k-hr.

[00277] The air and temperature control subsystem manages thermal flow within the suitcase enclosure, the thermal cycler, and the CAE. The layout employs a forced-air, internal plenum with inputs at the sides of the Apollo 200 System and outputs filtered air at the front and back of the cartridge to facilitate adequate thermal management and minimize particle introduction.

[00278] Another diagram of an enclosed integrated analysis system is shown in **Figure 70**. **Figure 70** shows a capillary electrophoresis ring for performing separations, a CCD-based detector for detecting analytes, an integrated cassette (combined disposable cartridge with reagent card), pneumatic solenoids, cassette clamp and interface (combined pneumatic manifold and cartridge cover), embedded tablet PC with touch-screen interface, exhaust fan, pneumatic pressure source and ballast, and electronics.

[00279] The computer and control software can integrate the system and provide the electronics interfaces, timing and control. The computer can be an industrial PC running Microsoft XP. Software can be Software control software. The main user interface can be a touch screen panel with auxiliary interface by monitor (VGA or higher res), external keyboard (USB) and mouse (USB) that may not included in the enclosure. A bar code reader (such as Keyence BL-180) and a GPS unit (such as an OEM module based on the Sirf-Star iii Chipset) can be connected via USB to the computer.

[00280] **Figure 71** shows a view of an enclosed integrated analysis system. **Figure 71** shows a touch screen (1.5.1), barcode reader (1.5.2), GPS (1.5.3), case (1.1), power supplies (1.7), chassis and structure (1.2), Internal partitions and baffles (1.3), electronics (2.1-2.5), separation and polymer fill device (6.2), and separation polymer cartridge (11.0). The electronics include a communication controller (2.1), solenoid valve controller (2.2), temperature control (2.3), motor control (2.4), and sensor board (2.5).

[00281] **Figure 72** shows a close-up view of the optics and pneumatics systems of the enclosed and integrated analysis system. The optics include the alignment components and base (4.1), excitation source (4.2), detector (4.3). The pneumatics include the vacuum supply (3.1) and the pressure supply (3.2).

[00282] Industrial grade power supplies can be used to improve the life time of the system. The rating of the power supplies may not be more than 500W. Interconnects that meet vibration standards and are proven to meet long life times can be used.

[00283] Chassis design for mounting subassemblies can include a number of structures which may utilize aluminum castings to reduce weight and cost of high volume parts. Aluminum structures can support subsystems 2, 3,4,5,6 and 11 (**Figure 64**). Structures utilizing sheet metal parts can support subsystems 1.5 and 2. The design can allow for reduced weight and cost while maintaining rigidity and durability to meet vibrations specifications for transportation. Structures can include internal isolation between the enclosure and system/sub-systems.

[00284] Partitions to separate the user manipulated sections, such as the cartridge loading, from the electronics and optics to avoid spillage; and baffles to keep stray light from entering the optics can be made from plastic or aluminum parts.

[00285] The chassis can be designed with a cartridge-handling subsystem. The Cartridge-Handling Subsystem interfaces the chassis with the application-specific cartridge and is located at the front center of the chassis (**Figure 39**). The Cartridge-handling subsystem can be activated when the user pushes the soft button 'Load.' The Cartridge-handling subsystem can accept the cartridge from the user in a cradle similarly to a VCR mechanism which can then be actuated to move the cartridge into the chassis.

[00286] The cartridge will first move away from the user and then down. A top plate can seal the top of the cradle. Fluidic and pneumatic connections can be through the top and bottom of the cartridge through the top plate and a bottom plate both under spring force. All connections can be protected from the environment by the top plate during processing and when stored. The Cartridge-Handling Subsystem and the first cartridge are the highest risk items in the project.

[00287] As the Cartridge-Handling Subsystem completes the cartridge input, both the pneumatics and fluidics are sealed as the cartridge under the spring pressure seats onto miniature 'O-ring' seals on the bottom plate.

[00288] The unit can be constructed to meet standards in transportation vibrations and environmental extreme conditions. The unit can be utilized in a variety of case orientations. The unit can be designed to

function at extreme temperatures and humidity specifications. The unit can be designed to prevent light-leaks.

[00289] The components of the integrated analysis system and disposable cartridge are depicted in **Figure 73**.

[00290] A reagent pneumatic assembly engages the cartridge and can perform a number of functions. A cartridge cover connected to an air supply is shown on the top left portion of the schematic shown on **Figure 73**. A depiction of the cartridge cover is shown in **Figure 74**. **Figure 74** shows the air supply ports for a vacuum source (3.4 Vac) and a pressure source (3.4 Press). The cartridge cover also includes a magnet assembly (7.1), reagent handling interface (7.4) and a heater assembly (7.2).

[00291] The Cartridge cover interfaces with the top of the Cartridge and the Reagent card. It can include several functions: Magnet positioning for magnetic particle capture in the sample extraction process, Heater positioning for the sample extraction lysis process, connection of the Cathode Tubing to feed diluted products to the Electrophoresis System, integration of pressure and vacuum to the Reagent Card, illumination for control of the Sample Loading process and Magnetic Particle re-suspension before Reagent Card activation.

- A. A primary functionality of the Cartridge Cover is to align with the Cartridge, activate the Reagent Card and interface with the Cartridge to provide extended functionality. The functions can include the following, referring to **Figure 74**.
 - A. *Magnet assembly (7.1)*: After lysis the DNA from the sample can be captured on magnetic particles and prepared for further processing by washing to remove contaminants and PCR inhibitors. To provide for the capture and re some or lease of the particles within the Cartridge the Cartridge Cover contains an assembly to facilitate the movement and location of an array of rare earth magnets in respect to the capture chamber on the Cartridge. This assembly consists of a magnet array and a mechanism. Magnets can be moved into and out of position to exert a magnetic force on compartments in the cartridge that can contain paramagnetic beads.
 - B. *Heater assembly (7.2)*: Cell lysis is carried out at elevated temperature, typically 60-80°C. The lysis takes place within the sample chamber which is heated by the Heater assembly. The Cartridge Cover positions the resistive heater around the sample chamber and provides interconnections to the Thermal management component of the Electronics. Temperature feedback is supplied by thermocouples in the heater.
 - C. *Cathode Tubing Connection (7.3)*: After PCR and dilution the sample, now diluted product, is moved to the Cathode Tubing for injection onto the capillary. The

Cathode Tubing is connected through the Cartridge Cover and interfaced with the Cartridge by a low-pressure seal such as a face seal or ferrule type connection. This connection is leak free, clean and low dead volume.

- D. *Reagent Handling (7.4)*: To maximize MOVE valve performance it is sometimes useful to feed the valves with pressurized reagents. Within the Cartridge Cover there are several ports that, when the Reagent Card is activated during system setup, pressurized specific reagent wells. In the same manner, the best scavenging of waste materials is often achieved with vacuum assist. Again, upon Reagent Card activation, specific waste wells may be evacuated to accomplish this. The interface with the Reagent Card is through cannulae, mounted in the Cartridge Cover, that pierce the top seal on the Reagent Card.
- E. *Sample Loading (7.5)*: To facilitate the proper and controlled loading of samples, positive controls, negative controls and allelic ladder the Cartridge Cover can be fitted with sensors and illuminators that work in a closed circuit fashion with the software to monitor and control the activity. Depending on the Cartridge Type and run setup parameters the system can “activate” one or more, e.g., from five to all eight, of the Sample Chambers. A chamber can be activated by illuminating the chamber with an LED or other light source built into the Cartridge Cover. When a swab, FTA punch or control is inserted into the chamber it is detected by an optical sensor built into the Cartridge Cover. The system then turns the illumination off, effectively de-activating the chamber. If a sample is placed into a de-activated chamber the system enters an error mode. The illuminators and sensors are interfaced to the Sensor Board in the Electronics.
- F. *Thermocycler Interface (7.6)*: The Reaction Tubing on the Cartridge is mechanically aligned to the Thermocycler components by the Cartridge Cover.
- G. *Magnetic Particle Re-suspension (7.7)*: Before the Reagent Card is activated the Magnetic Particles can be re-suspended as they may have settled during shipping and storage. The Cartridge Cover can interface a re-suspension device, such as an ultrasonic probe, piezo vibration probe or mixing mechanism, to the Magnetic Particle well of the Reagent Card.

[00292] The cartridge cover can interface with a cartridge, shown within the dashed lines below the cartridge cover on **Figure 73**. The cartridge cover can apply pneumatic pressure to the cartridge and/or be configured to apply a magnetic field and/or heat to one or more components of the cartridge. A depiction of a cartridge interfaced with the cartridge cover and pneumatic manifold is shown in **Figure 75**. **Figure 75** also shows a fan and ducting (5.3) and thermocycling components: thermal plate (5.1), thermoelectric (5.2), and controls (5.4).

[00293] The cartridge, shown in dashed lines on **Figure 73**, can include one or more chambers, fluidic connections, microchips, and/or pneumatically actuated valves. A top view of the cartridge is shown in **Figure 76**, **Figure 77**, **Figure 78**, and **Figure 79**. **Figure 79** shows reagent distribution chambers, capture chambers, sample chambers, and post amplification chambers. The cartridge can also have a receptacle for receiving reagent chambers that are on a reagent card. The reagent card can have a variety of chambers, including reagent chambers (**Figure 76**, 9.0), reaction chambers, and waste chambers. The reagent card (also referred to as a removable reagent cassette) can be manufactured separately from the cartridge. The reagent card can be inserted or interfaced with a reagent card slot (shown in **Figure 79**). The cartridge can be made of a piece of injection-molded plastic. The volume of the chambers, for example the sample chambers, capture chambers, and post amplification chambers can be about or up to about 0.1, 0.2, 0.5, 0.75, 1, 2, 3, 5, or 7 mL. The cartridge can have dimensions of about or up to about 1, 2, 5, 7, 10, 15, or 20 cm in width or height and about or up to about 0.2, 0.5, 0.75, 1, 2, 3, 4, or 5 cm in thickness.

[00294] The Cartridge element consists of several integrated parts. These include a piece that contains reaction chambers and that functions as a fluidic manifold. The chambers, on one side of the piece, communicate with the opposite side of the piece through ports. The opposite, or fluidic side, is engaged with fluidic chips comprising channels and diaphragm valves and pumps that move liquids between reaction chambers and reaction tubing. The chips can be attached to the fluidic side through a gasket. In certain embodiments, the cartridge comprises a plurality of chips. In this case, the fluidic manifold piece can comprise channels that fluidically connect one chip with another. Such channels are depicted, for example, in **Figure 94**. They can be grooves, troughs or other depressions in the surface of the piece that are sealed by a gasket between the underside of the piece and the microfluidic chips. The Reagent Delivery fluidics, Sample extractor fluidics, the Post-amplification fluidics, the top piece, the bottom piece and the Reaction Tubing. The top piece, also referred to as the fluidic manifold, is a plastic assembly and the fluidics are three layer glass MOVE chips that direct and control the flow of reagents through the system. The assembly connects to the pneumatic manifold and interfaces with the Cartridge Cover. The Cartridge facilitates all of the sample processing up to the loading of the amplified, labeled products onto the separation column. The Cartridge contains all the waste it produces and is replaced after each run to avoid contamination.

[00295] The top piece can be a molded plastic part with chambers for the reagent fill, sample extraction particle capture, sample insertion/lysis and product dilution. It also can have a section of silicon tubing used for reactions as well as an interface section for connection to the cathode tubing and an area for interface with the reagent card. For example, the silicon tubing can be used as a thermal cycling reaction chamber that is clamped at both ends during thermal cycling. The piece is made up of several parts. The fluidics components are attached to the bottom of the top piece with double sided adhesive.

[00296] The bottom piece can function as a gasket and seals of the channels molded into the Top Piece and provides a mounting surface and passageways, called vias, to the MOVE fluidic components.

[00297] The reagent delivery fluidics can deliver a preset volume of reagent to the Sample Extractor section facilitating sample processing. This delivery relies on pressurization of the Reagent Card wells which feeds the Reagent distribution fluidic MOVE device. The MOVE device controls the filling and disposition of the reagent chamber in the top piece. Pressurized air is also available for delivery to the Sample extractor section of the Cartridge. The section is comprised of one or more MOVE chips attached to the bottom of the integrated Cartridge bottom piece. The associated manifold and chamber features are connected to the downstream sections through the top piece.

[00298] The sample extractor can include one or more syringe chambers that can be configured to receive one or more samples, such as buccal samples or swabs. In **Figure 76**, the syringe chambers are the row of vertical cylinders that are second from the left. The syringe chambers are also referred to as capture chambers (shown in **Figure 79**). The syringe can be heated by a component on the cartridge or by a component on the cartridge cover.

[00299] Within the Sample extractor the swab/brush/disc is rinsed, the cells are lysed, the DNA is captured on particles, the particles are cleaned and delivered to the Reaction tubing for capture. The fluidics is a three layer glass MOVE chip attached to the integrated Cartridge bottom piece. The MOVE device distributes the flow of reagents from the Reagent distribution section to; the lysis/sample insertion chamber, the capture chamber or the Post-Amplification fluidics.

[00300] The Post Amplification fluidics interfaces with the Sample Extractor section, the Dilution Chamber, the Reaction Tubing and the Cathode Tubing. These fluidics consist of one of more three layer glass MOVE devices attached to the bottom piece. The Post Amplification fluidics control the particle capture from the Sample Extractor section, meter and move premix from the Reagent card to the Reaction tubing, move product from the reaction tubing to the dilution chamber, and meters diluent from the Reagent card to the dilution chamber. It also meters and moves buffer, water and sample to the cathode tubing.

[00301] The cartridge can include reaction tubing (shown in **Figure 77**). The tubes can be interfaced with a temperature controller, such as a thermocycler (shown in **Figure 73**). The tubes can also be interfaced with a magnet (shown in **Figure 73**).

[00302] The Thermocycler module temperature cycles the PCR-STR reactions in the Reaction tubing. It has several distinct components. The Reaction tubing is enclosed in a two piece shell that provides thermal contact and, when fully closed, pinch seals the silicon tubing. The bottom piece of the shell is part of the Cartridge. The top piece of the shell and the thermal control elements are aligned to the bottom piece and the tubing by the Cartridge cover. During particle capture and premix load the shell is in the "open" position; prior to cycling the shell is moved to the "closed" position. In the closed position the top and bottom pieces are in contact with each other which can facilitate thermal communication and pinching of the tubing which limits reaction plug evaporation and movement. Heating and cooling of the assembly is provided by a thermal electric device. The thermal control during cycling is driven by a controller which is managed by the electronics. Feed back is provided by a thermocouple permanently bonding to the top piece of the shell.

[00303] The thermal cycler temperature control can use Software objects and a thermal control board updated to 12-channels. Heating of the BeadStorm sample extraction portion of the DNA Profiling cartridge and of the capillaries of the CAE cartridge can use resistive heating monitored by thermocouples. The STR reactions can use resistive heating and fan cooling as the base case. Peltier/thermoelectric heating and cooling can also be applied as needed for extreme temperature ranges; MBI uses thermoelectric with MOVE microchips in a project with a strategic partner. The air from the thermal cycler can be output to the plenum. Control of temperature can be exerted through the MBI Temperature Control Board controlled by existing Software.

[00304] The chambers can be fluidically connected to a cartridge manifold. The cartridge manifold is shown in **Figure 80**. The manifolds can include one or more channels. These channels can be for swab extractor outputs, reagent distribution, post amplification to thermocycler channels, lysis channels, ethanol channels, waste channels, and bead channels.

[00305] The cartridge manifold can have one or more channels that fluidically connect the chambers on the top layer of the chip to one or more microchips. The cartridge manifold can also fluidically connect one or more microchips to each other, allowing for a fluid in one microchip to be transported to a second microchip. For example, material in the reagent chambers (shown in **Figure 73**) can be transported to the swab syringe (shown in **Figure 73**) by transport through the following components: the reagent distribution manifold section, the reagent distribution chip, the reagent distribution manifold section, the swab extractor manifold section, the swab extractor chip, and the swab extractor manifold section.

[00306] Microchips are shown as square outlines in **Figure 81** and **Figure 82**, which is a view of the base of a cartridge. The chips can be post amplification chips, sample extractor chips, and reagent distribution chips. The chips, also referred to as microchips herein, can have one or more pneumatically actuated valves. The valves can be used to control fluid flow by blocking or opening fluidic passages or providing a driving force for fluid movement. The valves can be controlled by a pneumatic manifold (shown in **Figure 73**). The pneumatic manifold (shown in **Figure 73**) can be similar to any other pneumatic manifold described herein. The pneumatic manifold can be connected to an air and vacuum source.

[00307] The chips can be fluidically connected to each other by channels in the cartridge. The channels in the cartridge can be an alternative to tubes that fluidically connected microchips, as described elsewhere herein. This can reduce the space required for the integrated analysis system and the time required to perform an analysis reaction.

[00308] As shown in **Figure 73**, the reagent card can include reagent chambers for, e.g., lysis, ethanol, bead, waste, syringe, water, ladder, premix, diluent, buffer, and waste chambers. The premix can be any premix described herein. In some embodiments, the premix is a premix for performing a nucleic acid amplification reaction. The reagent chambers can have a volume of about or up to about 0.1, 0.2, 0.5, 0.75, 1, 2, 5, 7, or 10 mL. The chambers can include features or mechanisms for keeping reagents cooled, heated, or mixed. For example, the chambers can include agitators or mixers. The reagent chambers can be sealed

prior to engaging the cartridge. Engaging the reagent card with the cartridge can reversibly or irreversibly place the reagent chambers in fluidic connection with the cartridge. In some embodiments, the cartridge has one or more cannulae that puncture a seal that encloses the reagent chamber. The seal can be a plastic seal or a rubber seal. In some embodiments of the invention, the rubber seal can effectively re-seal the chamber after dis-engagement. Accordingly, the card can be engaged with the cartridge in an inactive configuration. When the cartridge is engaged with a pneumatic manifold, the cover can depress the card into an active position in which the cannulae puncture the reagent chamber on one side and the cover punctures the reagent chambers from another side. This places the reagent chambers in fluid communication with the reaction chamber through channels connected by the microfluidic chips. This also allows positive pressure to be exerted to present reagent to the chips, which pump it to directed locations, as well as allowing vacuum to be exerted to pull waste presented by the chips into waste chambers on the card.

[00309] The card is designed with chambers to accommodate specific fill volumes without entrapping air. Both sides of the chambers are sealed with an elastomeric membrane. This eliminates the need for centrifugation before use. The card is fixed to the Cartridge and locked into a raised “safe” position. This is how the card ships with the Cartridge. In this position the bottom seal is aligned to the cannula on the top of the Cartridge. A safety mechanism assures that the card does not move to the lower “active” position where the cannulae on the Cartridge pierce the reagent cards seals.

[00310] The following are components of the reagent card, referring to **Figure 66**.

- A. *Reagent Set* (9.2): The Reagent Set and Reagent Card loading process and equipment are loaded with reagents adapted for performing the particular chemical reaction desired. For example, they can include reagents for performing STR analysis on one or more CODIS markers. The card can contain the following reagents:
- B. *Diluent* (9.2.1): The diluent is used to lower the salt concentration of the PCR reaction product and introduce a size standard. The size standard in the diluent can have fragments from approximately 60 to 600 bp.
- C. *Wash Solution* (9.2.2): The wash solution is used to clean the magnet particles and facilitate transfer to the Reaction Tubing.
- D. *Lysis Buffer* (9.2.3): The Lysis Buffer is used to lyse the cells in the sample.
- E. *Allelic Ladder* (9.2.4): The Allelic Ladder is included on one type of Cartridge. The Allelic Ladder is used to establish a standard position for all the possible Loci sizes. When used, the Allelic Ladder takes the place of one channel, during the sample loading process this channel may not be loaded with a standard or sample.
- F. *Capture Particles* (9.2.5): The Capture Particles are used to facilitate the isolation, purification and volume reduction of the sample DNA.

- G. *Run Buffer* (9.2.6): The Run Buffer is used as an electrolyte in the electrophoresis process.
- H. *Premix* (9.2.7): The Premix supplies the primers, buffer and enzyme to run the PCR reaction
- I. *Water* (9.2.8): Water is used to prepare the Cathode Tubing for the reaction products.

[00311] A single or set of small, quiet pumps can be used along with ballasts and precision regulators to supply the required pressure and vacuum. The regulators can be factory set and monitored by the system through electronic pressure transducers to assure accurate and predictable pneumatic performance at all times. MOVE valves have very low flow but require well regulated pressure. The Cartridge Fluidics manifold provides primarily for MOVE valves. The Cartridge Cover / Reagents manifold supplies the pressure feed reagents and internal pressurized air requirements of the cartridge as well as vacuum for the waste wells. This is slightly higher flow than the MOVE valves. The Mechanisms manifold is higher flow but usually may not require the same accuracy of regulation.

[00312] The pneumatic manifold provides for the mounting of the Cartridge and the control interface to the MOVE fluidics. The manifold has 3-way solenoids with a delivery port switching between vacuum and pressure. The solenoids are addressed by the Solenoid Valve Controller component of the electronics subsystem. The solenoids are mounted in a manifold that distributes the pneumatics to ports that align with inputs on the bottom of the MOVE microfluidic chips that are part of the Cartridge. This manifold also serves as the alignment and interface component to the cartridge.

[00313] The pneumatic manifold can be integrated into the chassis of the encasement such that the pneumatic manifold can be moved away from underneath the cartridge cover. This can facilitate loading of the cartridge into the integrated analysis system. **Figure 83, Figure 84, and Figure 85** show loading of a cartridge into an integrated an encased analytical system. **Figure 83** shows the pneumatic manifold in a position that is not underneath the cartridge cover. In **Figure 83**, the cartridge is positioned above the pneumatic manifold. **Figure 84** shows the cartridge engaged with the pneumatic manifold. The pneumatic manifold can then be moved or slid to a position such that the cartridge can be engaged with the cartridge cover, as shown in **Figure 85**. **Figure 69** shows the cartridge in a position such that the cartridge is engaged and fluidically connected with the cartridge cover and pneumatic manifold.

[00314] To maximize MOVE valve performance it is sometimes can be useful to feed the valves with pressurized reagents. Within the Cartridge Cover there are several ports that, when the Reagent Card is activated during system setup, pressurized specific reagent wells. In the same manner, the best scavenging of waste materials is often achieved with vacuum assist. Again, upon Reagent Card activation, specific waste wells may be evacuated to accomplish this. This manifold is a mixed manifold of 3-way solenoids

delivering either pressure or vacuum to the output port. The third port is generally vented to atmosphere. The solenoids interface with the Solenoid Valve Controller component of the electronics.

[00315] Pneumatic cylinders are used to move and set a variety of mechanisms within the system. These include the Thermocycler, Cartridge Cover and components within the cover. The mechanism manifold is pressure only, utilizing 3-way solenoids to deliver pressure to the output port and vent to atmosphere with the third port. The solenoids interface with the Solenoid Valve Controller component of the electronics.

[00316] The cartridge cover, cartridge, and pneumatic manifold can be used to extract nucleic acids and perform amplification reactions, as described elsewhere herein. Amplified nucleic acids can be delivered to one or more electrophoresis channels (shown in **Figure 73**) through fluidic connectors (shown in **Figure 73**). The electrophoresis channels can be electrically connected to a cathode and anode. The cathode and anode can be electrically connected to a high voltage controller (shown in **Figure 73**). The electrophoresis channels can be filled with separation polymer using the separation polymer module (shown in **Figure 73**).

[00317] The Electrophoresis hardware consists of the High Voltage Supply and Control, the Separation Polymer Fill Device and the Capillary Array Thermal Control. It also facilitates the mounting of the Capillary array. The thermal control provides precise heating of the capillaries during electrophoresis.

[00318] The cathode is part of the Capillary array and held in place by the Electrophoresis System hardware. The anode is part of the Separation Polymer Fill Module and is connected to the Electrophoresis System hardware. The high voltage control is an MBI HV board switching an OEM high voltage source. This action is managed and monitored by the electronics. High voltage is supplied to the anode electrode while sixteen cathode electrodes (two per channel) are held at ground. Current monitoring is done between the cathodes and ground and is monitored for individual channels on the MBI HV board. The cathode electrodes are part of the Capillary Array and connections are made to the HV system during array installation. The anode electrode is part Separation polymer fill module and the electrical connection to the cathode is through electrode immersion in the separation polymer.

[00319] The Separation polymer fill provides separation polymer to the capillaries through an interface at the anode. It connects to the Electrophoresis System hardware for anode high voltage supply and control. The Separation Polymer Fill Cartridge attaches to the module and supplies pressure and reagent for every run. The system is pressure driven and controlled by solenoids managed by the electronics. Pressure can be monitored by electronic transducers monitored by the Electronics. Safety can be provided by passive and active pressure relief paths.

[00320] The Separation Polymer Cartridge contains the separation polymer, a pressure canister, and a waste receptacle. The assembly is installed in the system before the run. During the run the system uses the pressure to flush the anode and refill it with fresh polymer then forces the polymer into the capillary array.

[00321] The high voltages used in capillary array electrophoresis (CAE) produce substantial thermal loads that can be managed to eliminate the likelihood of thermal runaway, due to Joule heating, disturbing

the electrophoretic process. CAE is generally run at elevated temperature, 40-80°C, producing a requirement of uniform thermal characteristics of the capillaries during the heat producing electrophoresis process. Affective transfer of Joule heating is required along with thermal uniformity to produce predictable, high resolution electropherograms. The heating and physical thermal management of the capillaries resides in the Capillary Array assembly. The interface and control of the temperature is through the Capillary Thermal Control component of the Electrophoresis System and the Temperature Control component of the Electronics.

[00322] The Capillary array includes the anode end connection, cathode tubing and electrical connections, window holder, heater, holder and eight capillaries; it provides for the separation of the labeled products and interfaces with the Electrophoresis System (6.0) and the Optics (4.0). The assembly is reusable and requires replacement by a trained technician at a prescribed interval, likely during regular maintenance. Replacement includes removing the old assembly, connecting the new assembly and aligning the capillaries to the Optics assembly. The anode piece interfaces the capillaries with the Separation Polymer Fill Device (6.2) and the anode electrode (within 6.1). It is also connected to a waste. The cathode tubing provides an interface between the capillaries and the Cartridge (10.0). It is also connected to a waste. The flow-through TREKI injection system utilizes two cathode injection electrodes which are permanently fixed and removed with the assembly. The window holder places and holds the detection window in the optical path and interfaces with the alignment system on the Optics assembly. The eight fused quartz polyamide coated capillaries, when filled with the separation polymer, facilitate the size mediated separation of the labeled products. Windows in the polyamide allow for the excitation and detection of the products as they move through the system. Capillary thermal control is by close contact to a material with high thermal transfer. Temperature control of the assembly is by resistive element and is driven by the Temperature Control electronics (2.3). Feed back is provided by a thermocouple.

[00323] The high voltages used in capillary array electrophoresis (CAE) produce substantial thermal loads that can be managed to eliminate the likelihood of thermal runaway, due to Joule heating, disturbing the electrophoretic process. CAE is generally run at elevated temperature, 40-80°C, producing a requirement of uniform thermal characteristics of the capillaries during the heat producing electrophoresis process. Affective transfer of Joule heating is required along with thermal uniformity to produce predictable, high resolution electropherograms. The system can utilize materials with high thermal transfer characteristics and good thermal uniformity such as aluminum and graphite coupled with powerful, flexible resistive heaters and fine resolution thermal control and monitoring to maintain tight thermal tolerances.

[00324] A detector (shown in **Figure 73**) can be used to observe or monitor materials in the electrophoresis channels. The detector can be a CCD camera-based system, or any other detection system described herein.

[00325] The Optical detector assembly detects the separated labeled products and sends the data to the software. The assembly consists of excitation and collection optics, an excitation source, a prism and a

camera. The excitation source is a DPSS laser which passes through specialized optics which shape the beam into a line. The line is focused on the capillary windows. The emission generated by the excitation of the fluors as they pass through the window area is collected by an objective and passed through a prism which separates the light into its component wavelengths. The output of the prism is focused on a camera which collects data in which the capillary array is in one axis and the emission spectra is in the other. Based on off the shelf reagent kits, the emission spectra can initially be separated into five bands. The number of discrete bands can increase to over seven without changing the physical design.

[00326] The electrophoresis channels and the optical detection assembly, including the detector and light source, can occupy a volume of about or less than about 0.1, 0.2, 0.3, 0.4, 0.5, 0.75, 1, 1.25, 2, or 5 ft³.

[00327] In some embodiments of the invention, the integrated analytical system can include other types of analytical devices. These analytical devices can include devices for performing mass spectrometry, gas chromatography, liquid chromatography, or any other type of analysis described herein.

[00328] The control systems, including the computer and software, can allow for a user to select analysis parameters, control the hardware, and obtain data. The electronics of the instrument are built in a highly modular fashion using distributed micro controllers to handle peripheral control and management tasks, such as temperature control, switching of solenoids, and control of other actuators used in the system. A main "application processor" is responsible for communicating with computer running the user interface, and controlling and coordinating the activities of the system.

[00329] The primary user interface can be a 13" tablet-style, embedded touch screen mounted in the lid of the enclosure. Night mode with severely reduced light emission can be an option for the display. An application-specific GUI can overlay the Software instrument control and analysis software.

[00330] The user can turn on an On/Off switch, scan their fingerprint or enter through the touch screen. For the Standard User, four buttons can be displayed: Insert Cartridge, Load Samples, Start, and Stop. The GUI can be designed to also provide a gateway to an Expert User mode and an Admin Mode for replacement of the CAE cartridge, and instrument calibration and service. In the Expert Mode, the GUI can also provide the user with various options for data analysis and display and output, USB ports and plug in keyboards can also be enabled per the particular usage scenario and device configuration.

[00331] Each peripheral sub system is designed with hardware feedback and safety mechanisms to ensure that the firmware responsible for the operation of the module can determine whether the sub-system is operating properly from an electronics point of view. For example, current through solenoids and motors is monitored to make it possible to determine that the actuator connected and that it is drawing an appropriate amount of current. (It is possible, for instance, to determine whether a DC motor is stalled, running properly, or disconnected from its load simply by correlating the current through the motor to the voltage applied to drive it.)

[00332] Similarly, critical fluidics paths are monitored using optical sensors to determine whether they contain fluid, bubbles or air.

[00333] In certain critical systems, such as temperature control, redundant sensors and hardware over temperature protection are integrated to ensure that firmware errors cannot cause damage to the system. Further, the temperature sensors used for feedback to the control firmware are biased to a tightly controlled voltage that makes it possible to determine whether the sensor is attached or not.

[00334] Redundant interlock circuits are employed to ensure operator safety with regards to high voltage, exposure to fluorescence excitation light and other potential hazards.

[00335] The system uses CAN bus for communication between the micro controllers in the distributed network. (CAN is a robust serial network.) It enables fast and reliable communication of messages between modules, and can be set up enable master-slave control schemes that are highly responsive to real time events in the instrument.

[00336] The control of the instrument can be hierarchical. The user interface computer sends high level commands to the main “applications processor” which translates them to sequences of commands for the individual micro controllers. Each step of such a sequence is executed by sending a message to the appropriate controller. Commands are always acknowledged, either by the returning the requested data or with a specific response indicating the receipt of the command. When a module has completed a command of this latter type, it can send a message to the “applications processor” indicating whether the completion was successful or not. (There are commands defined that let the “applications processor” query for detailed status that may explain any failure.)

[00337] Any node on the CAN network can send a message to any other node at any time. The system uses this to deal with exceptions to normal operations. If for instance, the temperature control module cannot maintain the temperature within given limits, it can send spontaneous error message to the “applications processor” to “inform” it of the problem. Similarly the controller monitoring fluid lines for air or bubbles would send a spontaneous message to enable the appropriate action to be taken by the system (or the user) in response to the problem. Depending on the specifics of the problem, the control application may choose to abort the run, solicit user action, or simply log and ignore the issue.

[00338] When the system is started, all sub-systems run through a basic confidence test to ensure that all parts of the instrument are operating properly. The application can also choose to invoke all or part of this test at the beginning of each experiment. During operation, each module monitors its hardware feedback for signs of errors. If an error is detected, a message to that effect is sent to the “applications processor” which can take appropriate action to mitigate the problem (which may cause it to be escalated to the user via the GUI). All errors and other significant events are logged in non-volatile memory for later retrieval to assist in troubleshooting and maintenance of the instrument.

[00339] Referring to **Figure 64**, the electronic components can include the following: a communications controller (2.1) that communicates with the computer and in turn with other electronics modules to relay and monitor execution of commands; a Solenoid Valve Controller (2.3) that is responsible for operating the MOVE valves to implement various pumping and valve control modes. The controller can also operate solenoids for reagent and waste handling, as well as mechanism operation; a Temperature controller (2.3) that runs the thermoelectric devices to implement thermal cycling and reagent temperature control, as well as resistive heating elements to maintain heated regions (e.g. separations subsystem); a Motor Controller (2.4) that operates magnet mover and other moving elements; a Sensor Board (2.5) that is an analog and digital input device that monitors the state of various sensors within the system.

[00340] Software runs all applications, controls HW and provides GUI functionality. Software is designed for the interfacing and control of instrumentation and automation components. This architecture is simple, flexible, and designed to allow rapid implementation of laboratory protocols. Software utilizes a standardized state machine model that uses XML files, scripted code, and standard libraries to describe the devices needed to carry out a given process. A state machine defines operational logic for a hardware component or software service, defines methods that are externally available, and provides details about current state and data. Initial data analysis is done by MBI software while the final base calling is done by a third party expert system. The data is background subtracted and filtered then spectrally separated into its four or five dye channels. Further filtering is performed before the data is formed into an AB compatible file and the expert software analysis and call is initiated

[00341] Software is composed of four primary sets of code, as follows, referring to **Figure 65**:

- A. *Core* (12.1): A windows service and set of libraries that implement a set of state machines (one for each hardware module). A state machine defines operational logic for a hardware component or software service, defines methods that are externally available, and provides details about current state and data.
- B. *GUI* (12.2): A simple graphical user interface communicates with the core to allowing the operator to run and monitor process scripts.
- C. *Scripts* (12.3): Process scripts constitute the operation logic that controls the hardware to carry out the logic of defined protocols. Scripts are compiled and run dynamically, thus providing great flexibility in modifying the logic of the system.
- D. *Data Analysis* (12.4): Initial data analysis is done by MBI software while the final base calling is done by a third party expert system. The data is background subtracted and filtered, then spectrally separated into its four or five dye channels. Further filtering is performed before the data is formed into an AB compatible file and the expert software analysis and call is initiated.

VI. Example of Operation

[00342] An example of operating the encased and integrated system is shown in **Figure 86** and **Figure 87**.

[00343] After powering on the system and logging on by fingerprint recognition or password, the user can push “Load” on the touch screen display. A cartridge-handling mechanism can open and the user can insert the cartridge into a mechanism which can then seat and automatically connect all liquid and pneumatic interfaces.

[00344] The user can then be prompted to add each sample. Optical barcodes can provide the chain-of-custody for sample identity and connection to associated biometric information such as photo, fingerprint, or iris scan. RFID tags may be used to transfer any associated information. Once the samples are loaded and the user touches “Go”, the user’s interaction can end until the system reports the results.

[00345] The cartridge is then processed by the chassis using reagents on the cartridge. The cartridge can contain all reagents and a positive and negative control. The processing of the samples in the DNA Profiling can take about 1 ¼ hrs. Any biological reaction can be performed in the integrated and enclosed analysis system. For example, SNP analysis or any other analysis reactions described herein can be performed.

[00346] The DNA Profiling cartridge can have four main functional areas held in a frame:

- A. Pre-processing and nucleic acid extraction using a BeadStorm-based device,
- B. STR reaction chambers in tubing,
- C. Microfluidic handling using MOVE micropumps to manipulate precious reagents and post-process microscale samples and,
- D. Reagent and waste storage

[00347] The chassis Pneumatic subsystem, driven by the Control subsystem, controls all fluidic operations on the cartridge including reagent metering and distribution, mixing, and bead-based purifications. The samples are moved into the ‘BeadStorm-based’ area extracts nucleic acids from large volume raw and/or otherwise unprocessed samples including swabs and milliliters of liquid using MOVE microvalves to control pressure-driven flow.

[00348] The Thermal subsystem performs the thermal cycling for STR amplification in the cartridge. The pre-processed samples on beads are moved into the Thermal subsystem and the samples eluted off the beads in STR mix, and thermal cycled. The thermal cycler can be based upon the present MBI thermal cycler. The thermal cycled STR products are then diluted into size standards and pumped by MOVE micropumps to the CAE subsystem.

[00349] The CAE subsystem performs the automated separation of the STR products using capillary array electrophoresis (CAE) on a reusable CAE cartridge in about 45 min. The CAE subsystem on the

chassis can have a high voltage supply and control, heat controller, and a laser-induced fluorescent detector with an imaging system capable of high sensitivity detection and data collection of separated STR products or other fluorescently labeled biomolecules.

[00350] The CAE cartridge performs the actual electrophoretic separation of the labeled products in an array of 12 separation capillaries. The CAE cartridge has the capillary array, anode and cathode assemblies, window holder, and a detection window, attached to a frame containing embedded heating segments. A separation polymer fill device accesses polymer and buffer on the single use DNA Profiling cartridge and replaces the separation polymer through an interface at the anode.

[00351] When the single-base resolution separation is complete, the digital data is processed to remove background and noise, and perform a spectral separation by **MBI's Trace Analyzer**. An expert system based on FSS's IQ3 then processes the data to a CODIS metafile. The metafile is queried against local and remote databases and answer if the sample's identify is produced on the screen in 2 hr after loading.

[00352] The MBI integrated single channel ANDE device can have a run time of three to three and one half hours depending on the run conditions. This includes the sample entry, lysis, extraction, purification, transfer, elution, thermo-cycling of the 16-plex reaction, transfer, dilution, injection, separation and detection of the products (see **Figure 88A**). The biggest single segment of time, the thermo-cycling at 100 minutes, can be significantly reduced. For example, the thermo-cycling time can be reduced to 45 minutes or less. Off system testing has shown good results with cycling times of less than one hour. Combining the intelligent primer design of the PowerPlex with advanced buffer, enzyme and dye chemistries and with efficiencies in the fluidic and separation process can allow for a processing time of less than two and one half hours (see **Figure 88B**). Processing times less than 1 hr may be achieved (see **Figure 88C**).

VII. Optical Detection System

[00353] The invention provides for a systems approach for the implementation of an eight channel capillary fluorescence detection and excitation sub-system.

[00354] Fluorescently labeled molecules are transported through a sieving matrix in the capillaries (200 μm ID and 50-75 μm OD). Four or more different dyes are present in the capillaries and the detector part of the system has to be able to distinguish their individual spectral signatures. Excitation of all dyes is accomplished using a solid state laser operating at 488 nm.

[00355] As shown in **Figure 89**, eight of these capillaries are held in parallel on a glass (or other substrate with similar thermal expansion properties) with epoxy adhesive. The substrate has an aperture that allows the optical system unrestricted access to the top and bottom of the capillaries.

[00356] The main purpose of the aperture is to limit the amount of material that is impinged upon by the excitation beam, which minimizes the background fluorescence of the system.

[00357] The detection system can be comprised of five elements:

- A. An objective with high numerical aperture (NA=0.65) with field of view that is large enough to image the eight capillaries (1.6mm),
- B. A laser rejection filter, capable of suppressing the excitation laser by at least five orders of magnitude.
- C. A dispersive element (a prism) that separates the images of the capillaries by wavelength.
- D. An imaging optic that projects an image of the spectrally dispersed light from the dispersive element onto the detector.
- E. An area detector that is capable of capturing images of the eight parallel, spectrally separated, images of the capillaries at a rate of five to ten images per second.

[00358] Software that is capable of separating the images of the eight capillaries and generating the spectral profile of the contents of the capillary is also an integral part of the system.

[00359] An embodiment of the main part of the optical system is shown in **Figure 90**. The configuration is similar to that of a modern microscope, with an “infinity corrected” design. The objective collects the emitted light from the capillaries and collimates it at its back aperture. A prism is inserted in the collimated path to separate the image of the capillaries into its spectral components. The imaging optic (known as a “tube lens” in a microscope) then projects that spectrally separated image onto the primary focal plane of the detector.

[00360] As shown in **Figure 91**, each capillary forms its own spectrally separated image as is shown in the following image. It shows an “end view” of the optical path projecting each of the capillary images onto the primary image plane.

[00361] Although the components used in the optical path of the detection system are chosen to be low noise, there is still an opportunity for this system to generate, collect and deliver stray light to the main primary focal plane. Much of such light can arrive at that focal plane at angles that are substantially different from that of the desired signal.

[00362] The alternative optical configuration takes advantage of that by inserting an aperture in the primary focal plane. It then images that plane to the detector using a relay optic that effectively suppresses light from outside the desired image of the capillaries. A further refinement on the idea with the aperture, is to place a dichroic mirror, the size of the image, in the primary focal plane. With properly chosen cut on wavelength for the coating, this can reject more than 90% of laser light that may have made it past the laser rejection filter. The mirror is positioned at an angle to direct light toward a detector. **Figure 92** shows the dichroic mirror as folding mirror #1.

[00363] The purpose of folding mirror #2 is primarily to reduce the foot print of the optical path, and to provide an easy way to align the image on the detector. The coating on that mirror could, however, also be of the same kind as that of folding mirror #1, in which case further laser rejection would be possible.

[00364] The detector for the system can comprise any photodetector. In one embodiment, the photodetector is a scientific grade, moderately cooled, two dimensional CCD camera.

[00365] The excitation of the fluorescent dyes in the capillaries can be done using a 488nm solid state laser. The laser is projected onto the capillaries from a direction opposite of the detection system, as shown in **Figure 93**. The capillaries are arrayed substantially in a plane. If light is directed orthogonally to the plane, the excitation light passes through the capillaries and is detected by the optics, interfering with sensitivity of detection. In order to avoid capturing the majority of the laser light in the collection system, the excitation is projected onto the capillaries at an oblique angle with respect to the normal orientation. In this way, the light passing through the capillaries avoids and is not collected by the collection optics.

[00366] The optical model shows how the laser beam is scattered in the capillaries, generating a “plume” of scatter that is outside the capture aperture of the collection optic. (It would be “looking” straight up at the intersection between the laser beam and the capillaries in the image above.)

[00367] **Figure 94** shows the excitation path from above. It shows the laser beam slightly diverging from its source. That is because the system uses either an “Engineered Diffuser” or a Powell lens to convert the Gaussian intensity profile of the laser to a uniformly illuminated line of light. This line is then projected (by the cylindrical lenses) directly onto the capillaries which act as very short focal length cylindrical lenses, effectively focusing the illumination energy inside the themselves.

[00368] **Figure 95** shows a simulated image of the capillaries showing the illumination intensity in pseudo color.

EXAMPLES

Example 1: Operation of a Cartridge for Nucleic Acid Purification

[00369] This example refers to the use of a device comprising a cartridge mated to a microchip. The numbers refer to the cartridge of **Figure 3** and **Figure 4** mated to a microchip with the circuit architecture of **Figure 5**. This sub-assembly also can be fluidically connected other sub-assemblies in the instrument of **Figure 6**. For reference, a cartridge mated with a microchip also is shown in **Figure 40** and **Figure 45**.

[00370] Nucleic acids can be purified from a wide variety of matrices for many purposes including, but not limited to, genotyping, identification, forensics, gene expression, gene modification, microRNA analysis, ribotyping, diagnostics, or therapeutics. The input sample can be a solid, swab, liquid, slurry, aerosol or a gas.

[00371] For molecular diagnostics and forensics, swabs are commonly used. A buccal swab can be taken using a swab with an ejectable tip and the swab ejected into a syringe attached to connection 7 of **Figure 4**. Connection 5 of **Figure 4** leads by tubing or capillary to a reagent manifold that can select a single reagent from multiple reagents by opening a full scale valve or by opening a MOVE valve with the reagents either

under pressure or moved by vacuum. MOVE or other micropumps on microchip 2 of **Figure 4** can also move the fluids or gases.

[00372] In one embodiment, human and other cells in a swab are first lysed using a buffer with a heated chaotropic agent and/or other commercial-off-the shelf (COTS) chemistries in a syringe inserted into port 7. The lysate is transported to a DNA isolation chamber (**Figure 4 #3**) where paramagnetic beads have been added from a reservoir to adsorb nucleic acids onto the beads. A moveable magnet is then actuated to capture the beads onto the side of the isolation chamber where they are washed automatically using a buffer. The purified DNA, still bound to beads, is then pumped through a small diameter tube 250 where multiplexed PCR is performed. Pre-scripted Software automates the complete process. The Software defines a set of communication and command protocols in a standardized automation architecture that is simpler, more flexible, and quicker to implement than other software development approaches. The Software implementation framework is based on core technologies that span multiple operating systems, development languages, and communication protocols. Software drivers wrap individual smart components of the system, greatly reducing the time needed for typical de novo system software development. This makes it relatively straightforward to integrate the operation of multiple system modules (pumps, valves, temperature controllers, I/O controllers, etc.) that are either COM- or .NET-based. Software provides a professional quality software development system for prototyping through product release and maintenance.

[00373] While DNA amplification is useful for positive identification of microorganisms, samples can be obtained from a wide variety of substrates and matrices that contain compounds that are inhibitory to DNA amplification reactions. Raw samples are most often complex mixtures that can include inhibitors such as hemes, metal ions, humic and fulvic acids, chelators, DNases, proteases, and molds. While the initial isolation of target organisms and toxins from the sample matrix by IMS may remove most of these inhibitors, lysed cell components and lysis agents can also need to be removed or diluted from nucleic acid samples so that they do not interfere with successful amplification. Raw samples are otherwise unprocessed samples, and may environmental, biological, and the like.

[00374] In one embodiment, a small volume nucleic acid purification is used. These purification methods can be used with a wide range of samples, such as blood, to aerosols, to buccal swabs. Paramagnetic beads can be used in a disclosed device to purify DNA from various sample sources. In one embodiment a microfluidic microchip can be used to sequence a nucleic acid using magnetic beads and reagents to purify nucleic acid products for sequencing in microscale reactions. In one embodiment, the microfluidic microchip is a 24-channel microfluidic microchip.

[00375] In one embodiment, polyethylene glycol (PEG)-based nucleic acid purification is used on carboxylated magnetic beads. This PEG-facilitated process can produce yields of over 80% from upstream immunomagnetic separations (IMS) captured samples. Development of a universal sample preparation module (USPM) can partly involve porting the PEG-based nucleic acid purification onto a device containing

a cartridge such as the devices shown in **Figure 21** or **Figure 16**. In another embodiment, Agencourt Orapure or Promega DNA IQ chemistries are used in conjunction with a device of the present invention.

Bead dispensation and delivery.

[00376] To purify nucleic acids, paramagnetic beads with different surface chemistries can be mixed in a reagent container. Pressure is then applied to send the reagents to connection 5. MOVE microvalves or other valves may be closed unless referred to as open. To move the paramagnetic beads into the reaction chamber (3), microvalves 180 and 150 are opened. The beads are moved through connection 5 into channel 15 which leads to junction 190 and microchannel 191. Because microvalves 180 and 150 are open and microvalves 200 and 170, and the other microvalves, are closed, an open microfluidic connection is from microchannel 191 through microvalve 180 to microchannel 181 through microchip 152 to open microvalve 150 and microchip 151 to junction 120. Junction 120 leads to cone 13 and chamber 3, which can be filled with beads. The volume of beads supplied to chamber 3 can be controlled by timing the opening of the reagent valves and the microvalves or by filling and emptying a sample loop connected to the microchip or the cartridge.

[00377] Commercial bead based chemistries can be used in the disclosed system, including but not limited to Orapure from Agencourt (Waltham MA) and DNA IQ from Promega (Madison, WI). Orapure uses a carboxylated bead surface and SPRI chemistry while DNA IQ is an example of a silica bead and chaotrophic chemistry. Other embodiments of paramagnetic beads or chemistries to process nucleic acids can be used in conjunction with the disclosed system, including but not limited to beads with oligonucleotides, locked nucleic acids, degenerate bases, synthetic bases, conformation, nucleic acid structures, or other hybridization and specific capture methods.

Filling chamber (3) with beads.

[00378] For Orapure or DNA IQ beads, 450 microliters can be moved into chamber (3) using three fills of a 150 microliter sample loop 630 or 631. A movable magnet 300 attached to actuator 310 can then be moved towards cartridge (1) near the side of 3 to pull the beads to the side of chamber (3). Magnet size and orientation can be adjusted to generate magnetic fields appropriate to specific applications. Pressurized air can then be applied through the reagent manifold with microvalve 180, 150, and 110 open. The opening of microvalve 110 connects from junction 190 which connects to the reagent manifold through junction 120 and microchannels 121 and 101 to connection 100 which leads through channel 14 to connection (4) and to waste. The air can move any remaining liquid through the circuit. Air or other gases can also be used to dry beads, volatilize solvents, or for bubble-enabled mixing (described herein).

Bubbling of gas through chamber (3)

[00379] If microvalves 180, 150, and 220 are open, and all other microvalves closed, the pressure can force air through chamber (3) to channel 9 and down channel 19 to junction 210 through microchannels 211 and 221, through open microvalve 220 and microchannel 231 to junction 230, through channel 16 to

connection 6 which can be a vent. This sequence can bubble air or other gases through chamber (3) and can be used to mix reactions in chamber (3) or to change the gas phase.

Moving liquids and beads from chamber (3) to waste

[00380] Liquids and beads can be moved from reaction chamber (3) or any other location to waste. This can be used to wash beads, flush channels, move liquids or beads to waste. When pressure is applied to connection 6 with microvalves 220 and 110 open, and all other microvalves closed, the pressure can force air through channel 16 to junction 230 to microchannel 231, through open microvalve 220 and microchannels 222 and 221, through junction 210, and channels 19 and 9 into reaction chamber (3) and through junction 120 through microchannel 121, open microvalve 110, microchannel 101, channel 14 and to connection 4.

[00381] The equivalent effect can be obtained by applying vacuum to connection (4) if connection 6 is a vent without any additional control of air pressure. The air pressure or vacuum can move any liquids in chamber (3) to the waste connection 4. When magnet 300 is close to chamber (3), paramagnetic beads can remain on the side of chamber (3) and the result is that the liquid is removed. When magnet 300 is far enough from chamber (3), paramagnetic beads can not remain on the side of chamber (3) and the result is that the liquid and beads are removed.

[00382] To clean paramagnetic beads, the beads are pulled to the side of chamber (3) with magnet 300 (see **Figure 6**) and the liquid removed to waste. 450 microliters of buffer can be dispensed from the reagent manifold and added to chamber (3) by opening microvalves 180 and 150. The beads can be released if desired and then recaptured by moving the magnet 300 and the liquid then removed. This is repeated for a total of three times to produce beads ready to process samples.

Lysis and extraction of nucleic acids from cells on the swab

[00383] A swab can be loaded into a syringe barrel inserted into connection 7 and then be lysed by addition of lysis buffer through reagent connection 5 with microvalves 180 and 170 opened. In some embodiments Orapure or DNA IQ chemistries are used.

Movement of the lysed cellular material to chamber (3) and mixing with beads

[00384] The material in the syringe connected to connection 7 can be moved into chamber (3) by applying pressure to the syringe or by applying vacuum to vent 6. When vacuum is used, microvalves 170, 150, and 220 are opened. The vacuum connects through microchannels 231, 221, 211, and channels 9 and 19 through chamber (3), microchannels 151, 152, 171, and 161 to pull material from connection 7 into chamber (3). When paramagnetic beads are loaded and cleaned in chamber (3), the lysed sample material mixes with the beads in chamber (3) with the magnet is the far position.

Purification of nucleic acids on the beads

[00385] The paramagnetic beads are then incubated with the lysed sample. Continued air or gas flow can aid mixing. The magnet 300 is then moved to the closed position and the beads are captured on the wall of

chamber (3). The sample lysate can then be removed from chamber (3) to waste and multiple volumes of wash solution added according to manufacturers' specifications for the Orapure chemistry or DNA IQ chemistry. The sample components on the beads have now been purified and are ready for reactions in the cartridge or exporting to the sample product connection. In one embodiment the beads are used to enrich a nucleic acid component from a sample.

Exporting samples through the sample product connection 8

[00386] The purified sample components on the beads can be moved to connection 8 by applying pressures on reagent connection 5 with microvalves 180, 150, and 130 open. In one embodiment, connection 8 is connected with reaction channel 250 such as C-flex tubing (Cole Parmer) and additional reactions are performed in the reaction channel.

Multiplexed PCR amplification of STR markers

[00387] DNA amplification can be performed by PCR amplification. The present invention enables PCR reactions as well as many other DNA amplification and modification reactions. The reactions can be performed in chamber (3), in reaction channel 250 attached to connection 8 which can be a tube 250 (**Figure 3, Figure 4, Figure 6**), or in another device or microdevice connected to tube 250. This demonstrates the utility of the sample preparation for DNA reactions including thermal cycling.

Capture of nucleic acid containing beads in a reaction channel

[00388] The purified DNA output through the sample product connection 8 is moved into a reaction channel 250 at end 251 by applied pressure or alternatively through vacuum applied to end 252. An actuator 330 moves a magnet 320 under software control into a position close to bead capture region 340. Fixed magnets of different sizes and shapes (such as rare earth magnets) as well as electromagnets or superconducting magnets can be used. As the solution containing the beads moves through region 340, the magnetic field attracts the beads to the side of the reaction channel and holds them in place. The fluid is then followed by air pressure through reagent connection 5 leaving the beads region 340 in air.

Addition of reagents and movement of samples into reaction region

[00389] Reagents can be added from the reagent manifold as described. In one embodiment, reagents are added from end 252 of reaction channel 250. End 252 is attached to a microfluidic microchip 500 comprising microvalves 510, 520, 530, and 540. Any three microvalves such as 510, 520, and 530 or 510, 520, and 540 can form a pump. Microvalve 530 connects through a microchannel to a downstream device 535, which can connect to tubing leading to a reagent reservoir. Microvalve 540 connects through a microchannel to downstream device 545, which can connect to tubing that leads to a reagent reservoir.

[00390] Reaction mixes (such as at least one DNA polymerase, dNTPs, buffer and a salt) including but not limited to master mixes and primers, (such as assay-specific primers or broadly applicable primer sets for multiple target pathogens), or complete PCR master mixes such as PowerPlex 16 from Promega (Madison,

WI) or IdentiFiler or MiniFiler from Applied Biosystems (Foster City, CA) in reagent reservoir 600 can be delivered by a micropump formed by microvalves 530, 520, and 510 through tubing 610 and microchannels 531, 521, 511, and 512, into end 252 of reaction channel 250, as shown in **Figure 6**. MOVE microvalves can precisely position fluids and move the fluid to region 340 where the reaction mix encounters the beads comprising nucleic acids. Magnet 320 is moved away from reaction channel 250 by actuator 330 which releases the beads from the inner surface of the reaction channel 250. The MOVE microvalves on microchip 500 pump the beads into device 400 with an area of reaction channel 250 forming temperature controlled region 350. The region 350 can be held at isothermal temperatures or thermal cycled or other varied as is well known to one skilled in the art. The region 350 can be a temperature modulator or thermally coupled to a temperature modulator.

[00391] **Figure 7** shows a temperature control device 400 that is capable of thermal modulation using a temperature modulator for heating and cooling to thermocycle the reaction channel. In one embodiment the temperature modulator comprises a Peltier module, infra-red module, microwave module, a hot air module or a light module. In another embodiment a PCR reaction sample is moved inside the reaction channel past one or more constant temperature zones.

[00392] **Figure 9** shows the amplification of PowerPlex 16 STR reactions that have been prepared in a cartridge (1) from buccal swab samples and processed in reaction channel 250 using the temperature control device 400 in **Figure 7**. The STR markers are amplified from standard conditions with Mg optimized for the apparatus 1000.

[00393] The temperature control device 400 can also have a detector 410. The detector can detect optical detection such as absorbance, fluorescence, chemiluminescence, imaging, and other modalities well known to one skilled in the art or measurement such as IR, NMR, or Raman spectroscopy. The detector can comprise a light source is used to excite a fluorescent or luminescent dye in the PCR reaction sample, and the excitation light is sensed with a photodetector (such as a CCD, CMOS, PMT, or other optical detector). In one embodiment the light source is a coherent light source, such as a laser or a laser diode. In another embodiment the light source is not a coherent light source, such as a light emitting diode (LED) or a halogen light source or mercury lamp.

[00394] For nucleic acid amplification, real-time PCR is one example of a nucleic acid assay method that can be performed in tube 250 in temperature controlled region 350 and detected with detector 410.

Example 2: Universal sample preparation

[00395] The previous example illustrated one embodiment in which the disclosed apparatus can be used to prepare samples for analysis and showed one example of STR amplification. Another embodiment involves the use of a Universal Sample Preparation Module (USPM). The USPM device can consist of a sample processing cartridge (1), accompanying apparatus to operate the cartridge, a microprocessor, and

software that can readily be interfaced to downstream analytical devices. In one embodiment the USPM can be tightly integrated with analytical devices to form a modular sample-to-answer system. The cartridge can be configured as a disposable single-use device that can process swabs or liquids (including aerosol samples) for field monitoring processes, or as a reusable, flow-through format for remote operations with rare positives. Target specificity of the USPM is imparted through the use of specific antibodies (that bind selected targets) attached to paramagnetic beads; different cartridges can be supplied with various mixtures of targets.

[00396] A USPM can use a multistep fully automated process to prepare biological samples for downstream analysis. One example in **Figure 18** can use swabs or liquids; the operator can select the sample type and then insert samples into input port(s). The first step can apply immunomagnetic separations (IMS) to capture, concentrate, and purify target molecules from solution onto paramagnetic beads. Targets already tested include cells, spores, viruses, proteins, or toxins. For toxin and protein detection, or for use as a triggering device, the captured targets from the IMS can be exported directly to the downstream analytical device. For nucleic acid detection, the second step can lyse the cells or spores to release the DNA and/or RNA using mechanical or other lysis techniques. The third step, nucleic acid purification, can adsorb, concentrate, and purify the nucleic acids onto a second set of paramagnetic beads and output the beads with nucleic acid, or purified desorbed nucleic acid, for downstream analysis.

[00397] Referring to cartridge (1), the immunomagnetic separation can be performed by using reagent beads that have antibodies or other immunomagnetic, affinity magnetic, or surface chemistry magnetic separations. For example, immunomagnetic beads with antibodies can be added to cartridge (1) to capture, purify, and concentrate cells, viruses, spores, toxins and other biomolecules onto bead.

[00398] Upstream sample processing for the USPM can be done in the sample preparation devices, which can process samples over 0.6 mL in a microfluidic cartridge (1) (**Figure 21**). The sample processing cartridge, about 1 in cubed dimension, (**Figure 3, Figure 21**) was developed to automatically remove collected buccal cells from a swab, lyses the cells, and purifies released cellular DNA on magnetic beads. The bead beds are typically 100 nL and can be used for downstream STR analysis with microfluidics devices or full scale qPCR reactions.

[00399] The sample preparation device uses a MOVE microvalve microchip interfaced with the bottom of the cube (**Figure 3**, arrow labeled 2) to direct pressure-driven flows consisting of fluids, beads, and samples among the reagent and reaction reservoirs. The MOVE microvalves replace conventional valves and tubing between the reservoirs, thereby providing a non-leakable, directable fluid transport and enable miniaturization of the entire cube and sample preparation device.

[00400] This sample preparation device technology has been used to automate DNA extraction from buccal swabs as described above. **Figure 10** shows automated preparation of DNA from 25 uL of blood in the automated sample preparation device using pressure driven flows, vibrational mixing, MOVE valves,

actuated magnets, and magnetic beads. The fully automated process produced DNA ready for STR analysis in less than five minutes.

[00401] An automated system has been developed for capturing, concentrating, and purifying cells, viruses, and toxins from liquid samples (1-10 mL) using magnetic beads coated with antibodies specific to targets of interest. Thus, a variety of targets have been concentrated and purified with this automated system. Using this approach, *E. coli* cells were captured and detected at cell concentrations as low as 15 cells/mL/sample (**Figure 27**). Similar results of greater than 90% capture efficiency were obtained using *Bacillus* spores, Gm⁺ and Gm⁻ vegetative cells, a model virus (bacteriophage fd), SEB, and ovalbumin as targets. Purified samples can be further processed in the sample preparation device (*e.g.*, lysis and nucleic acid purification), moved onto a microchip for analysis, or used with an off-chip PCR/qPCR device.

[00402] IMS capture has been shown to work well in complex samples such as aerosols and in the presence of biological clutter (See U.S. Patent Publication No. 20080014576, herein incorporated by reference in its entirety). For clutter, we showed that up to 10⁵-fold levels of added bacteria produced only a two-fold reduction in capture efficiency. For complex samples, add-back experiments using many different aerosol samples established that aerosol samples reduce the binding of *B. cereus* spores to IMS beads by less than 50%. Therefore, there is less than a two-fold loss of sensitivity in complex, real-world samples.

[00403] IMS has been used to capture, concentrate, and detect toxins. We have developed IMS assays for ovalbumin and SEB, multiplexed the assays, and developed two generations of completely integrated microfluidic systems that automate the IMS assays. Less than 10 ng of SEB can be reliably detected in a one mL samples with no interference from closely related *Staphylococcal* enterotoxins.

[00404] IMS can:

- A. Select target organisms from samples with high backgrounds of interferents (selectivity),
- B. Discriminate between two different strains or species of bacteria (specificity),
- C. Effectively capture cells and toxins across a wide range of concentrations from a wide range of samples (sensitivity, robustness)
- D. Reduce target sample volume significantly, from mL to nL volume

[00405] The instant invention and the apparatus and methods are capable of implementing IMS and coupling it to nucleic acid extractions.

[00406] The next step in the USPM is the lysis of the captured target when it is a cell, virus, prion, or spore. Lysis of spores is particularly challenging. A MagMill or magnetically driven lysis or homogenizing device has been developed for efficient lysis of *Bacillus* and other spores, as well as vegetative cells. The MagMill consists of a rapidly rotating magnet 2000 actuated by a motor 2001 (**Figure 60**) that drives rotation of another magnet 2002 contained within a sample-containing vessel 2003 or compartment (**Figure**

61). The magnet 2002 contained within the sample-containing vessel can have any shape. For example, the magnet can have a bar, spherical, cylindrical, rectangular, oval, hexagonal, or propeller shape. Alternatively, the magnet can have holes through it, such that liquid may be forced through the holes and increase the shear force applied to the sample when the magnet is rotated by a magnetic field. The same basic components can be miniaturized, incorporated into a microfluidic format, or connected to a microfluidic format. The overall effect is analogous to a magnetic stir plate, with the sample being rapidly vortexed within the sample tube. Using magnetically driven sample agitation by MagMill treatment, spore lysis is achieved without silica, zirconia or other beads. Lysis may be accomplished by shear forces generated as the spore passes between the magnet and the vessel walls. The magnet can rotate at a rate of greater than about 10, 50, 100, 150, 200, 250, 500, 750, 1000, 1500, 2000, 2500, 5000, or 10000 rpm.

[00407] This device disrupts spores with similar efficiency as traditional bead beating that employs silica/zirconia beads (**Figure 62**). Spores (3.2×10^7) were lysed in a volume of 1 ml with viability was determined by plating on Tryptic Soy Agar; results are an average of two separate experiments each run with duplicate samples (total n=4). The non-viability of magnetically-driven spore lysates was 93% compared to traditional bead beating (BioSpec beater) lysates using either Zirconia/silica which was 96% or silica beads which was 80%. The same pattern was confirmed by qPCR

[00408] The advantage of using the MagMill (versus traditional bead beating) is that the design is more mechanically robust and thus able to withstand many cycles of use without failure, and samples can be lysed using just the agitation of the magnet in the sample, without the need for inclusion of silica/zirconia beads that have been shown to bind released DNA causing a loss in follow-on detection sensitivity. The basic features of the MagMill can be reconfigured in a miniaturized format that can be integrated into a sample preparation device. The system can potentially be down-sized to fit into a microfluidic microchip. Despite changes in configuration, however, the principle driving lysis, that of a rapidly rotating magnet contained within a sample vessel, remains the same.

**Example 3: Coupling of a sample preparation device
with a microchip-based sample cleanup and separation**

[00409] **Figure 34** and **Figure 35** show a device with a cartridge (2907) and microchip (2901) that was designed to incorporate the Forked Injector design, as shown in **Figure 32**, a gel filling manifold (2903), and associated components. The cartridge is fluidically connected to a pneumatics manifold and tubing (2905). Different configurations of the injector design, separation channel length and separation polymer were tested. **Figure 36** show an electropherogram of an M13 T track injected and separated on a microchip channel using the Forked Cathode injector, with sample detection on a confocal microscope breadboard system. The sample was injected uniformly with short and long DNA fragments represented equally. The results show that an M13 T track DNA ladder can be uniformly injected and single base pair resolution can be obtained out to approximately 330 base pairs in less than 20 minutes. Higher sample signal strengths were obtained

compared to injections using a conventional twin T design. When integrated with a detection system, the microchip is held at a constant 50°C in order to obtain separations with good resolution.

[00410] Using these processes, excellent results were obtained for MOVE integrated, field amplified stacking injections of liquid samples (**Figure 37**). This data was generated with all sample loading, manipulation and injection processes carried out under software control using MOVE microvalves. The data has been minimally processed, color corrected from a detector that uses eight diode channels to four dye traces.

[00411] One embodiment of a microchip that combines the forked cathode with a MOVE sample preparation device is shown in **Figure 38**. This device comprised additional processes that enable integration with the rest of the system, i.e., the sample preparation device (1000 shown in **Figure 22**), the reaction channel (250 shown in **Figure 6**), and the output of the STR purification as described in the STR example. **Figure 38** shows a forked cathode with MOVE fluidics and shuttle sample loading for integration with post amplification STR purification system. The parts are: 1 - Reagent input port, 2- Reagent pump head, 3 - Sample input port, 4 - Size Standard / eluent input port, 5 - Capture valve, 6 - Waste port, 7 - Elution valve, 8 - Sample waste port, 9 - Cathode, 10 - Cathode port, 11 - Sample valve, 12 - Sample port, and 13 - Separation channel. The anode port, which is downstream of the channel, is not shown.

[00412] The sample to be separated is introduced as a bead solution in ethanol. This can be the purified reaction products on beads output as described above. In one embodiment, the sample is an STR reaction. In other embodiments, the sample can be nucleic acid fragments of different lengths produced by other reaction chemistries including DNA sequencing by Sanger chemistry. The solution containing the sample is flowed from the Sample input port to the Sample waste port with the Capture valve and other intervening valves open. The open Capture valve facilitates a slowing of the stream flow and bead capture by a fixed magnet placed above or below the valve. The ethanol solution is completely run through the system followed by air yielding a relatively dry and clean bead bed, with purified products, in the valve. At this point the valve is closed and reopened (in coordination with other valves) to fill it eluent solution from the associated port. For an STR analysis or other analyzes where an internal size standard is needed, the eluent can contain a size standard. The solution is moved between the Elution valve and the Capture valve to facilitate mixing, ending with the solution in the Elution valve. The Sample valve is then opened in coordination with the Elution valve closing to "shuttle" the sample through the sample channel leaving it filled. The sample FASS injection is carried out as previously described. An additional noteworthy function of the device is that in one embodiment the Reagent input port and Reagent pump are used to provide metered STR reaction premix to the reaction channel (250 shown in **Figure 6**) after the swab extraction of DNA on the sample preparation device; in other embodiments, the device can provide other nucleic acid reaction reagents such as cycle sequencing mixture or provide PCR reagents to perform a PCR amplification followed by providing cycle sequencing reagents to perform cycle sequencing with bead-based cleanup reactions integrated as needed. Other chemistries will be apparent to one skilled in the art.

[00413] While preferred embodiments of the present invention have been shown and described herein, it will be obvious to those skilled in the art that such embodiments are provided by way of example only. Numerous variations, changes, and substitutions will now occur to those skilled in the art without departing from the invention. For example, any MOVE valve, pump, router, or other MOVE device described herein can be replaced with any pneumatically actuated valve, pump router or other device. It should be understood that various alternatives to the embodiments of the invention described herein can be employed in practicing the invention. It is intended that the following claims define the scope of the invention and that methods and structures within the scope of these claims and their equivalents be covered thereby.

CLAIMS

WHAT IS CLAIMED IS:

1. A system that fits within an enclosure of no more than 10 ft.³ comprising:
 - (a) a sample preparation module adapted to capture an analyte from a non-microfluidic volume on a capture particle and route the captured analyte through a microfluidic channel;
 - (b) a reaction module comprising a reaction chamber in fluidic communication with the microfluidic channel adapted to immobilized the captured analyte and perform a biochemical reaction on the analyte in a non-microfluidic volume to produce a reaction product; and
 - (c) an analysis module in fluidic communication with the reaction chamber adapted to perform an analysis on the reaction product.
2. The system of claim 1 configured to capture the analyte, perform a biochemical reaction on the analyte, and perform an analysis on the product in less than 4 hours.
3. The system of claim 1 further comprising a data analysis module configured to receive data about the analysis from the analysis module and comprising executable code that transforms the data and outputs a result of the analysis.
4. The system of claim 1 further comprising a processing module in fluidic communication with the reaction chamber and the analysis module and adapted (1) to route the reaction product through a second microfluidic channel into a non-microfluidic processing chamber; (2) process the reaction product and (3) route the processed reaction product into the analysis module.
5. The system of claim 1 wherein the system fits within an enclosure of no more than 8 ft³.
6. The system of claim 1 wherein the system fits within an enclosure of no more than 5 ft³.
7. The system of claim 1 wherein the system fits within an enclosure of no more than 2 ½ ft³.
8. The system of claim 1 wherein the sample preparation module is adapted to release the analyte from a cell.
9. The system of claim 1 wherein the capture particle is a magnetically responsive capture particle and the reaction module comprises a source of magnetic force configured to immobilized the captured analyte.
10. The system of claim 1 wherein the reaction module is adapted to perform thermal cycling.
11. The system of claim 1, wherein the system is a closed system.
12. The system of claim 1, wherein the system is battery operated.

13. A system comprising a cartridge cover, a cartridge and a pneumatic manifold wherein the cartridge can be releaseably engaged with the cartridge cover and the pneumatic manifold,

wherein the cartridge comprises one or more pneumatically actuated valves and one or more microfluidic channels,

wherein the pneumatic manifold and the cartridge cover are each fluidically connected to at least one pressure source, and

wherein the pneumatic manifold and the cartridge cover are each adapted to control fluid flow within the cartridge.

14. The system of claim 13, wherein the pneumatic manifold is adapted to actuate the pneumatically actuated valves and the cartridge cover is adapted to apply pressure to one or more chambers in the cartridge.

15. A system comprising:

a) a disposable cartridge comprising at least one set of fluidic chambers including a sample chamber, a mixing chamber and a thermal cycling chamber in fluid communication with each other, and a reagent card comprising reagents for performing a chemical reaction involving thermal cycling, wherein the reagent card is configured to be carried on the cartridge in a closed configuration and to be moved into fluid communication with the at least one set of fluidic chambers;

b) an actuator assembly configured to move fluids between chambers when the cartridge is engaged with the actuator assembly;

c) a thermal cycler configured to cycle temperature in the thermal cycling chamber when the cartridge is engaged with the actuator assembly;

d) a capillary electrophoresis assembly configured to accept a sample from cartridge when the cartridge is engaged with the actuator assembly and to perform capillary electrophoresis on the sample; and

(e) a computerized control system configured to control the actuator assembly, the thermal cycler and the capillary electrophoresis assembly.

16. A cartridge comprising:

a) a fluidic manifold comprising a fluidic side and a reagent card side wherein the fluidic manifold comprises:

(i) at least one set of fluidic chambers, each chamber comprising a port on the fluidic side;

(ii) at least one of thermal cycling chamber comprising at least one port;

(iii) at least one of exit port;

(iv) a slot on the reagent card side adapted to engage a reagent card, wherein the slot comprises a plurality of slot channels comprising cannulae on the reagent card side and communicating between the two sides;

b) at least one microfluidic chip comprising:

- (i) at least one fluidic circuit;
- (ii) a plurality of ports in fluid communication with the fluidic circuit;
- (iii) at least one pneumatically activated diaphragm valve configured to regulate fluid flow within the fluidic circuit;

wherein the at least one chip is engaged with the fluidic manifold so that the ports in the at least one chip are in fluid communication with the ports of the chambers and the slot channels wherein each fluidic chamber is in fluid communication with at least one other fluidic chamber and each cannula is in communication with a fluidic chamber; and

c) a reagent card engaged with the slot, wherein the card comprises a plurality of reagent chambers comprising reagents, each aligned with at least one of the cannulae and adapted to take a first engagement position wherein the reagent chambers are not punctured by the cannulae and a second engagement position wherein the reagent chambers are punctured by the cannulae, thereby putting the reagent chambers in fluid communication with the fluidic circuit.

17. The cartridge of claim 16 wherein the reagents comprise reagents for performing PCR.
18. The cartridge of claim 17 wherein the reagents comprise primers for amplifying a plurality of short tandem repeats.
19. The cartridge of claim 16 wherein the at least one set of fluidic chambers is a plurality of sets of fluidic chambers.
20. The cartridge of claim 16 wherein the fluidics manifold further comprises at least one auxiliary fluidic channel on the fluidic side of the manifold, the at least one chip is a plurality of chips and fluidic circuits in each of the plurality of chips are in fluidic communication with fluidic circuits of at least one other chip through the auxiliary fluidic channel.
21. The cartridge of claim 20 wherein further comprising a gasket between the chips and the manifold, wherein the gasket seals the channels on the manifold.
22. The cartridge of claim 16 wherein the fluidic chambers comprise a distribution chamber, a capture chamber, a sample chamber, and a clean-up chamber.
23. The cartridge of claim 16 wherein at least one fluidic chamber comprises magnetically responsive particles.
24. The cartridge of claim 16 wherein the at least one set of fluidic chambers is at least 4 sets or at least 8 sets.
25. The cartridge of claim 16 wherein the chips comprise at least one diaphragm valve.

26. A system comprising:

a) a pneumatic assembly comprising:

- (i) a pneumatic manifold adapted to removably engage the cartridge of claim 16 on the fluidic side, wherein the pneumatic manifold comprises a plurality of pneumatic ports configured to engage pneumatic channels in the at least one microfluidic chip and activate the diaphragm valves; and
- (ii) a pressure source configured to supply positive or negative pressure to the pneumatic channels;

b) a cartridge activation assembly adapted to engage the cartridge on the reagent card side; wherein the cartridge activation assembly comprises:

- (i) a reagent pneumatic manifold comprising a pneumatic side and reagent card side, wherein the reagent pneumatic manifold comprises reagent pneumatic manifold channels communicating between the two sides and comprising a cannula on the reagent card side;
- (ii) a pressure source configured to supply positive or negative pressure to the reagent pneumatic manifold channels; and
- (iii) a clamp configured to move the reagent card from the first engagement position to the second engagement position, wherein clamping results in the cannulae of the reagent pneumatic manifold puncturing the reagent chambers and putting the reagent chambers in communication with the pressure source;

c) a thermal cycler configured to cycle temperature in the at least one thermal cycling chamber when the cartridge is clamped;

d) a capillary electrophoresis assembly comprising:

- (i) at least one separation channel fluidically engaged with the exit port when the cartridge is clamped; and
- (ii) an optical sub-assembly configured to detect signal from the at least one separation channel; and

(e) a computerized control system configured to control pneumatic assembly, the cartridge activation assembly, the thermal cycler and the capillary electrophoresis assembly.

27. The system of claim 26 wherein clamping seals the chamber ports and the slot channels with the at least one microfluidic chip.

28. The system of claim 26 wherein the cartridge activation assembly further comprises at least one heater configured to heat at least one of the fluidic chambers when the reagent pneumatic manifold is engaged with the cartridge.

29. The system of claim 26 wherein the cartridge activation assembly further comprises movable magnets configured to move into and out of a position wherein the magnets exert a magnetic force on at least one fluidic chamber.
30. The system of claim 26 wherein the cartridge activation assembly further comprises sensors configured to detect the presence of a sample in a sample chamber of the fluidic manifold.
31. The system of claim 26 wherein the thermal cycler comprises a Peltier device.
32. The system of claim 26 comprised in a portable case.
33. The system of claim 32 wherein the case has an internal volume of no more than 10 ft³.
34. The system of claim 32 wherein the case has an internal volume of no more than 8 ft³.
35. The system of claim 32 wherein the case has an internal volume of no more than 2 ½ ft³.
36. An article in computer readable form comprising code for operating the system of claim 26.
37. A method comprising: producing, from a sample comprising at least one cell comprising DNA, a computer file identifying a plurality of STR markers in the DNA, wherein the method is performed in less than 4 hours.
38. The method of claim 37 wherein the method is performed in less than 3 hours.
39. The method of claim 37 wherein the method is performed in less than 2 hours.
40. The method of claim 37 wherein producing comprises extracting the DNA from the at least one cell, amplifying the STR markers from the DNA, performing capillary electrophoresis on the amplified markers, detecting the amplified markers, and performing computer analysis on the detected amplified markers to identify the markers.
41. The method of claim 37 wherein the plurality of STR markers is at least 5 STR markers.
42. The method of claim 37 wherein the plurality of markers are CODIS STR markers.
43. The method of claim 42 wherein the plurality of STR markers is at least 5, 10, or 13 CODIS STR markers.
44. The method of claim 37 wherein the at least one cell is a plurality of cells.
45. The method of claim 37 wherein the sample is a forensic sample.
46. The method of claim 37 performed at the site of a sample collection.
47. The method of claim 37 wherein the sample comprises blood.
48. The method of claim 37 wherein the sample comprises a cheek swab.
49. The method of claim 37, wherein the method is carried out by a system as described in any of claims 1-15 or 26-35.
50. A system configured to perform a method, wherein the method comprises: producing, from a sample comprising at least one cell comprising DNA, a computer file identifying a plurality of STR markers in the DNA, wherein the method is performed in less than 4 hours.

51. A method comprising:
- a) providing a system comprising:
 - i) a disposable cartridge comprising at least one set of fluidic chambers including a sample chamber, a mixing chamber and a thermal cycling chamber in fluid communication with each other, and a reagent card comprising reagents for performing a chemical reaction involving thermal cycling, wherein the reagent card is configured to be carried on the cartridge in a closed configuration and to be moved into fluid communication with the at least one set of fluidic chambers;
 - ii) an actuator assembly configured to move fluids between chambers when the cartridge is engaged with the actuator assembly;
 - iii) a thermal cycler configured to cycle temperature in the thermal cycling chamber when the cartridge is engaged with the actuator assembly;
 - iv) a capillary electrophoresis assembly configured to accept a sample from cartridge when the cartridge is engaged with the actuator assembly and to perform capillary electrophoresis on the sample; and
 - v) a computerized control system configured to control the actuator assembly, the thermal cycler and the capillary electrophoresis assembly;
 - b) moving of the reagent card into fluid communication with at least one set of fluidic chambers;
 - c) providing a sample comprising a nucleic acid molecule to a sample chamber; and
 - d) operating the system to amplify and detect at least one nucleic acid sequence in the sample.
52. The method of claim 51 comprising providing each of a plurality of samples to a different sample chamber.
53. The method of claim 51 wherein the time it takes to go from step b) to step d) is less than 4 hours.
54. The method of claim 51 comprising amplifying and detecting a plurality of nucleic acid sequences in the sample.
55. The method of claim 54 wherein the plurality of nucleic acid sequences comprise short tandem repeats.
56. The method of claim 56 wherein the short tandem repeats comprise a plurality of Combined DNA Index System (CODIS) markers.
57. The method of claim 56 wherein the CODIS markers comprise a plurality of markers selected from AMEL, D3S1358, THO1, D21s11, D18s51, D5s818, D13s317, D7s820, D16s539, CSF1PO, vWA, D8S1179, TPOX and FGA.
58. The method of claim 51 wherein the system is a system of claim 26.

59. The method of claim 51 wherein the sample is a forensic sample.
60. The method of claim 51 wherein the sample is selected from a buccal swab, blood, hair or semen.
61. The method of claim 51 wherein the sample is a raw sample.
62. The method of claim 51 further comprising transporting the system to a forensic site.
63. An optical system comprising:
- a) a plurality of optically transparent channels;
 - b) a light source configured to direct to the plurality of optically transparent channels;
 - c) a dispersive element that disperses light passing through the optically transparent channels in a wavelength dependent manner; and
 - d) a detector configured to receive the dispersed light.
64. The system of claim 63, wherein the plurality of optically transparent channels comprises at least eight capillaries.
65. The system of claim 63, wherein the optically transparent channels are aligned in a first plane and the dispersive element disperses light along a second plane, wherein the first plane and the second plane are different.
66. The system of claim 65, wherein the first plane is orthogonal to the second plane.
67. An optical system comprising:
- a) an excitation source configured to direct excitation light to an object;
 - b) a carrier for an object, wherein the object emits light other than excitation light when excited by the excitation energy;
 - c) a rejection filter configured to filter out excitation energy and to allow transmission of the emitted light;
 - d) an imaging lens configured to focus the emitted light;
 - e) a dichroic mirror substantially transparent to the excitation energy and configured to reflect emitted light to a detector;
 - f) a focusing system comprising at least one lens configured to focus light reflected from the dichroic mirror; and
 - g) a photodetector (CCD camera) configured to receive the reflected light.
68. The optical system of claim 63 wherein the excitation light comprises light of a wavelength between 0.3 microns and 1 micron.

69. The optical system of claim 67 wherein the carrier comprises an array of capillary tubes and the object comprises a fluorescent species.
70. The optical system of claim 67 wherein the mirror reflects emitted light and an angle between about 5 degrees and about 10 degrees off an incident angle.
71. The optical system of claim 67 wherein the dichroic mirror further comprises a portion that transmits substantially all light.
72. The optical system of claim 67 wherein the focusing system comprises at least one folding mirror.
73. The optical system of claim 67 wherein the photodetector comprises a CCD camera.
74. The optical system of claim 67 further comprising a prism located between the object and the imaging lens.
75. An optical system comprising:
- a) an array of capillary tubes aligned substantially parallel and substantially in a plane;
 - b) an excitation assembly comprising an excitation source and configured to deliver excitation light from the excitation source to the array, wherein the light delivery assembly is configured (i) to deliver a thin band of light that covers the array and (ii) to deliver the light to the array at an angle other than 90 degrees to the plane;
 - c) a collection lens configured to collect light emitted from the array by objects in the array excited by the excitation light;
- wherein the excitation assembly and the collection lens are configured with respect to the array so that excitation light passing through the array substantially avoids collection by the collection lens.
76. The optical system of claim 75 wherein the angle is between about 10 degrees and about 85 degrees.
77. An instrument comprising:
- a) a microfluidic component comprising a plurality of intersecting microfluidic channels and at least one controllable valve configured to regulate flow of fluid between the intersecting channels; and
 - b) a non-microfluidic component comprising a plurality of non-microfluidic chambers, wherein each non-microfluidic chamber is fluidically connected to at least one of the microfluidic channels;
- wherein the instrument is configured to flow fluid from at least one non-microfluidic chamber into another non-microfluidic chamber through a microfluidic channel and flow is regulated by at least one valve.
78. The instrument of claim 77 wherein the plurality of non-microfluidic chambers comprises at least three chambers and the at least one valve selectively directs fluid from one chamber to either of the at least two other chambers.

79. The instrument of claim 77 further comprising a pump to pump fluid from a non-microfluidic chamber into a microfluidic channel.
80. The instrument of claim 77 wherein at least one valve is a diaphragm valve.
81. The instrument of claim 80 wherein the pump is a diaphragm pump comprising a series of three diaphragm valves.
82. The instrument of claim 77 wherein the microfluidic component comprises a monolithic device.
83. The instrument of claim 77 wherein the combination of the microfluidic component and the non-microfluidic component define a fluidic circuit and the instrument comprises a plurality of fluidic circuits.
84. The instrument of claim 77 wherein the non-microfluidic component further comprises a particulate capture agent.
85. The instrument of claim 84 wherein the particles are responsive to a magnetic field and the instrument further comprises a magnet configured to immobilize the particles.
86. A device comprising a plurality of non-microfluidic chambers fluidically connected to a common microfluidic channel.
87. A method comprising:
- a) providing a device comprising:
 - i) a microfluidic component comprising a plurality of intersecting microfluidic channels and at least one controllable valve configured to regulate flow of fluid between the intersecting channels; and
 - ii) a non-microfluidic component comprising a plurality of non-microfluidic chambers, wherein each non-microfluidic chamber is fluidically connected to at least one of the microfluidic channels;wherein the instrument is configured to flow fluid from at least one non-microfluidic chamber into another non-microfluidic chamber through a microfluidic channel and flow is regulated by at least one valve;
 - and wherein a first non-microfluidic chamber comprises a first volume of sample comprising an analyte;
 - b) providing an amount of particulate capture agent in the first non-microfluidic chamber to bind a selected amount of analyte from the sample;
 - c) moving the particulate capture agent bound to the analyte through a microfluidic channel in the microfluidic device to a second non-microfluidic chamber;

d) contacting the particulate capture agent bound to the analyte with a reagent in a second non-microfluidic chamber; and

e) performing a chemical reaction on the analyte using the reagent.

88. The method of claim 87 wherein contacting comprises flowing the reagent from a third non-microfluidic chamber through a microfluidic channel in the microfluidic device into the second non-microfluidic chamber.

89. The method of claim 87 wherein the particles are response to magnetic force and the method further comprises immobilizing the particulate capture agent bound to the analyte in the instrument with a magnetic force.

90. The method of claim 87 comprising suspending the particulate capture agent bound to the analyte in the instrument in a volume at least an order of magnitude smaller than the sample volume.

91. A method comprising:

a) performing a first chemical reaction on an analyte in a first chamber which is a non-microfluidic chamber to produce a first reaction product; and

b) moving the first reaction product through a microfluidic channel into a second chamber which is a non-microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product.

92. A method comprising:

a) performing a first chemical reaction on an analyte in a first chamber which is a non-microfluidic chamber to produce a first reaction product; and

b) moving the first reaction product through a microfluidic channel into a second chamber which is a microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product.

93. A method comprising:

a) performing a first chemical reaction on an analyte in a first chamber which is a microfluidic chamber to produce a first reaction product; and

b) moving the first reaction product through a microfluidic channel into a second chamber which is a non-microfluidic chamber and performing a second chemical reaction on the first product to create a second reaction product.

94. The method of any of claims 91-93 comprising cleaning the first reaction product before moving it to the second chamber.

95. The method of any of claims 91-93 further comprising, at least once, moving a reaction product through a microfluidic channel into a subsequent non-microfluidic chamber and performing a subsequent chemical reaction on the reaction product to create a subsequent reaction product.

96. The method of any of claims 91-93 further comprising, at least once and before moving a reaction product into a non-microfluidic chamber, moving a reaction product through a microfluidic channel into a microfluidic chamber and performing a subsequent chemical reaction on the reaction product to create a subsequent reaction product.

97. A device comprising:

- a) a sample channel having a channel inlet and a channel outlet;
- b) an electrophoresis capillary having a capillary inlet and a capillary outlet, wherein the capillary comprises an electrically conductive medium and is in communication with the sample channel at a point of connection;
- c) an anode and a cathode configured to apply a voltage across the capillary inlet and capillary outlet, wherein one of the anode or cathode comprises a forked electrode wherein the forks are in electrical communication with the sample channel on different sides of the point of connection; and
- d) a second electrode in electrical communication with the sample channel substantially opposite the point of connection.

98. The device of claim 97 wherein the second electrode is comprised as a third fork in the forked electrode.

1/76

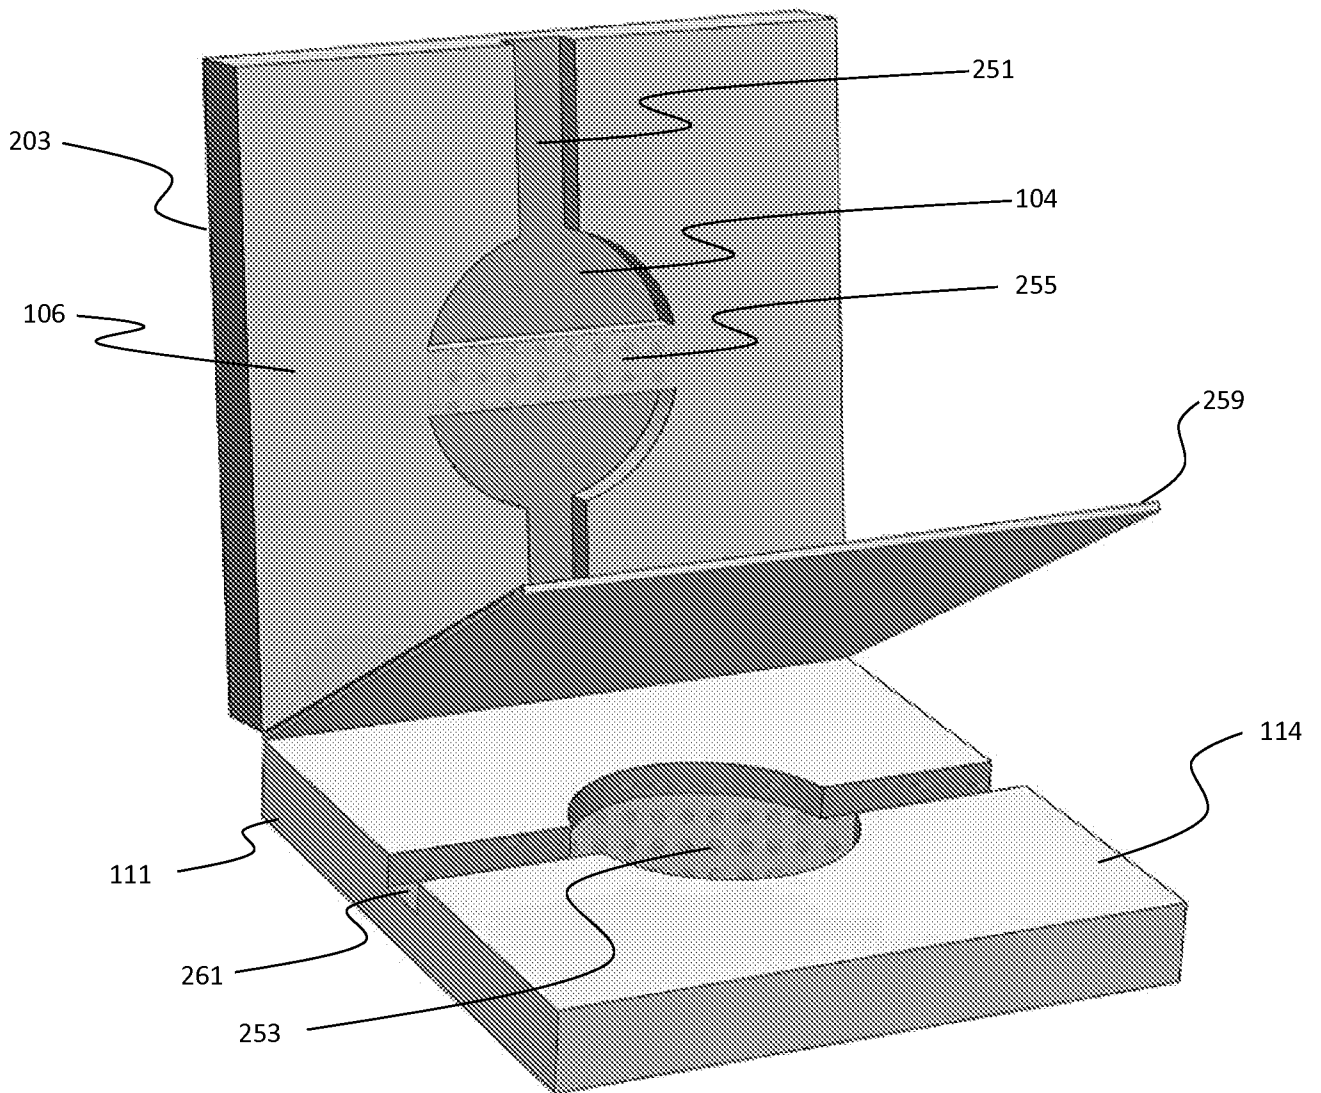


Figure 1A

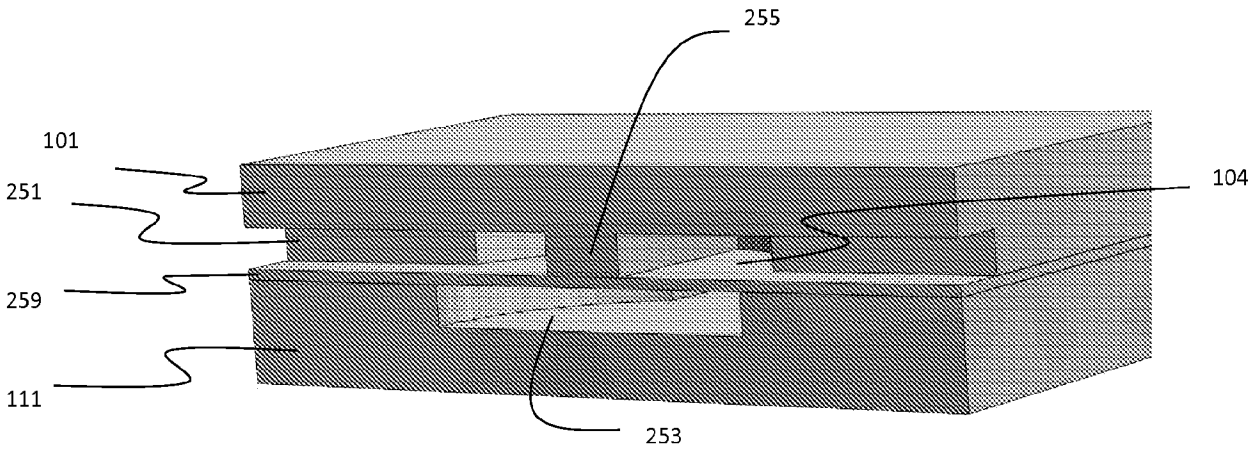


Figure 1B

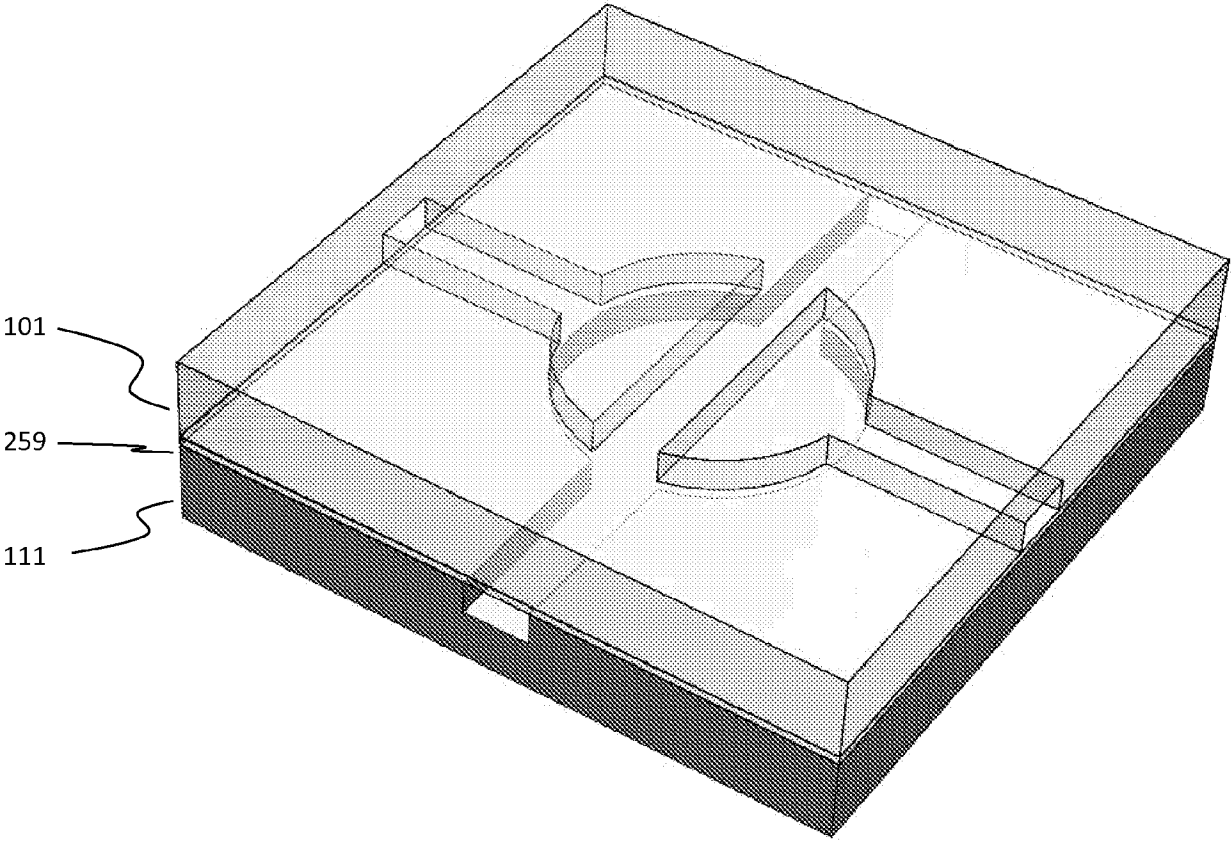


Figure 1C

4/76

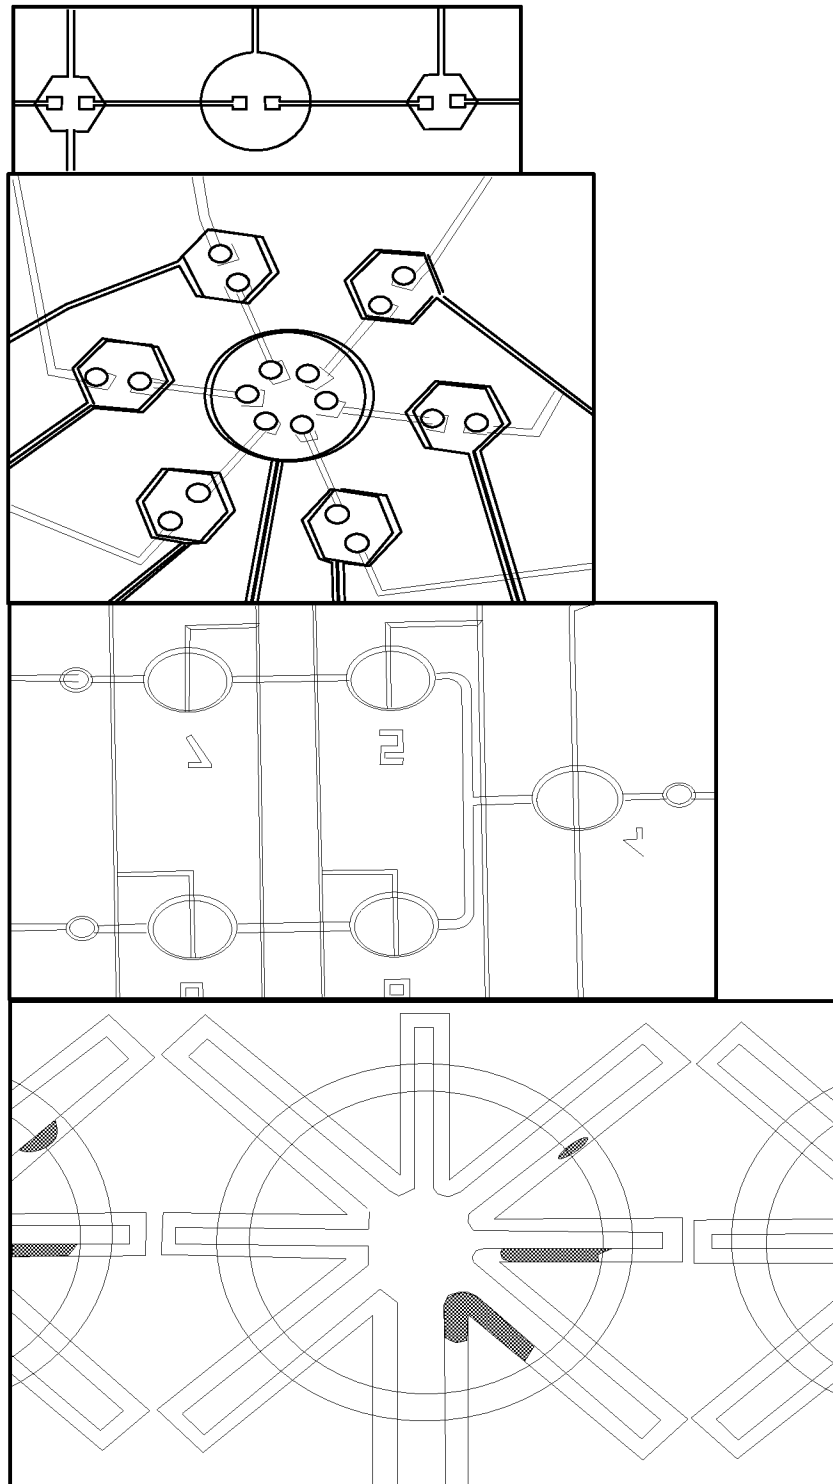


Figure 2

5/76

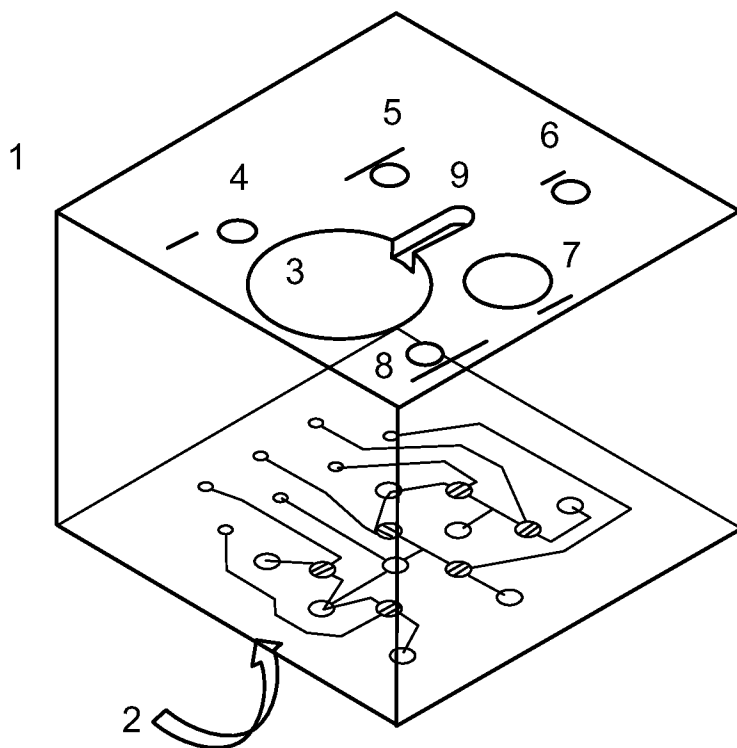


Figure 3

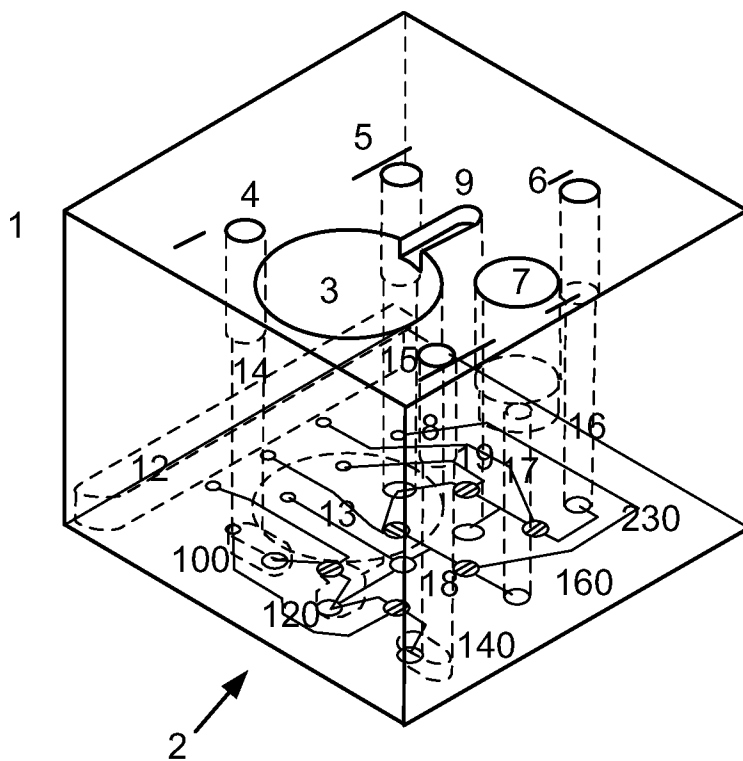


Figure 4

6/76

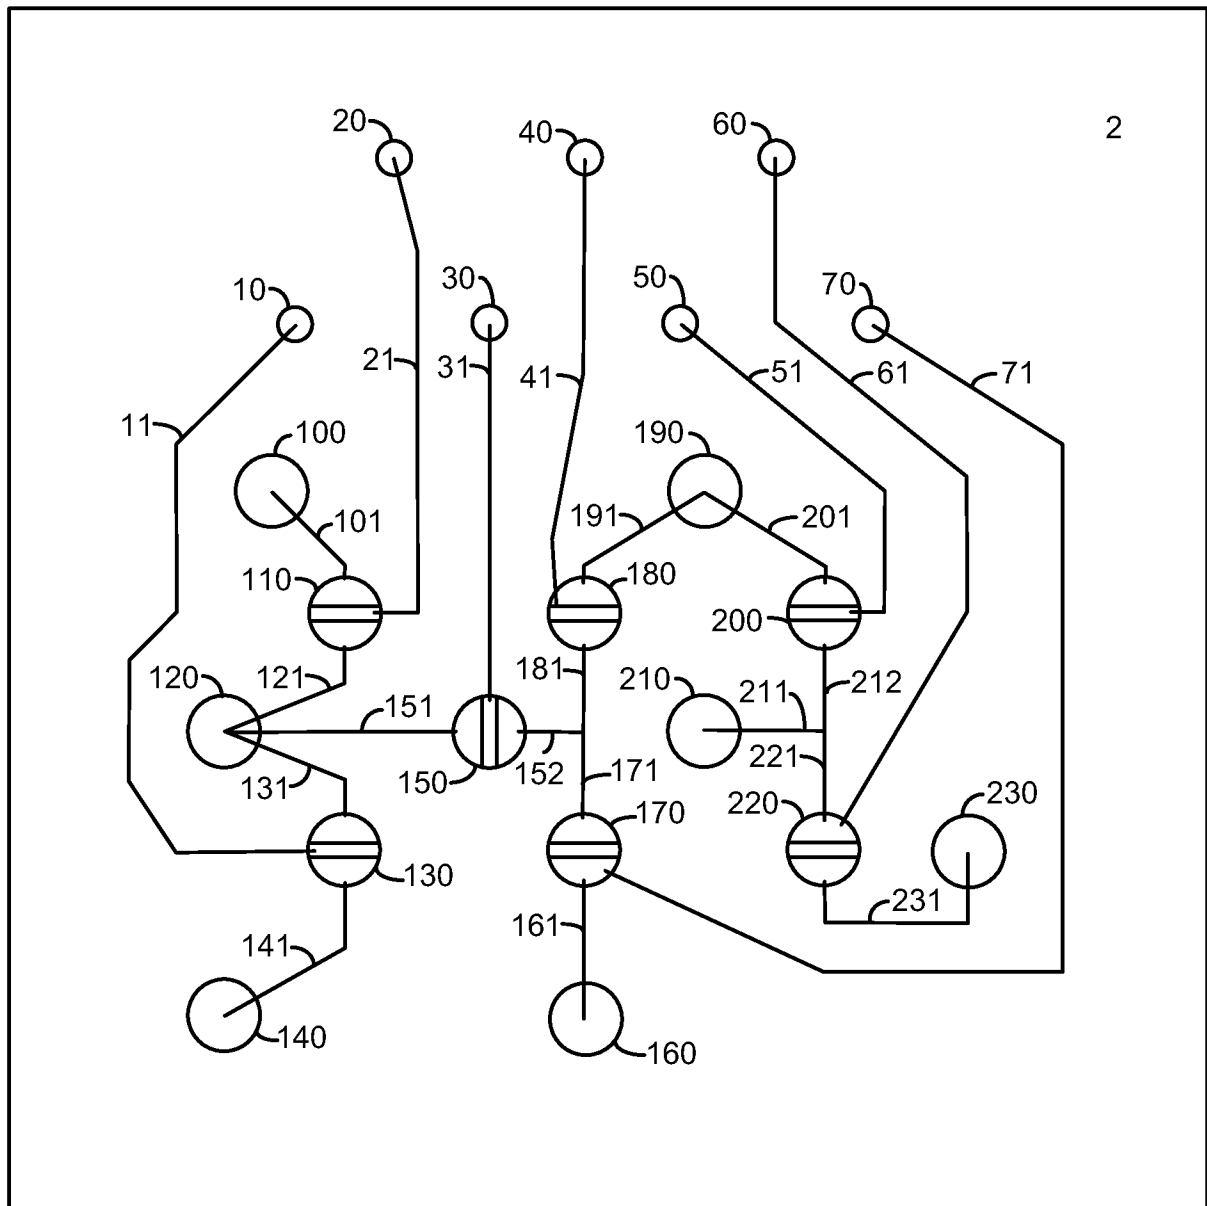


Figure 5

7/76

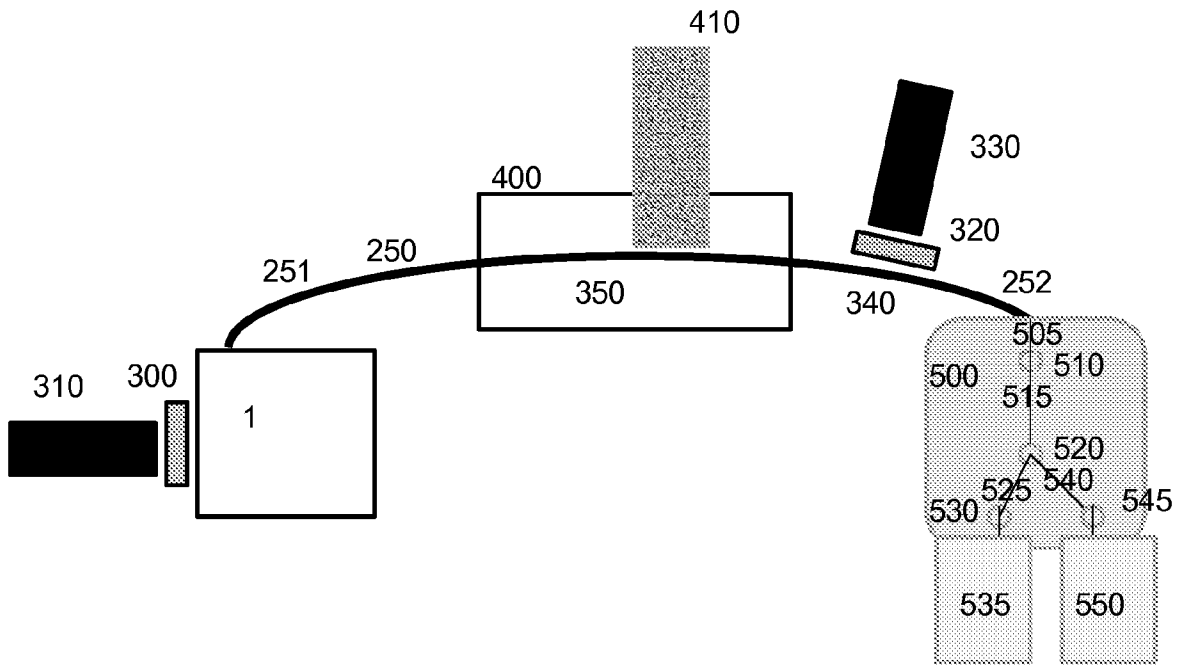


Figure 6

8/76

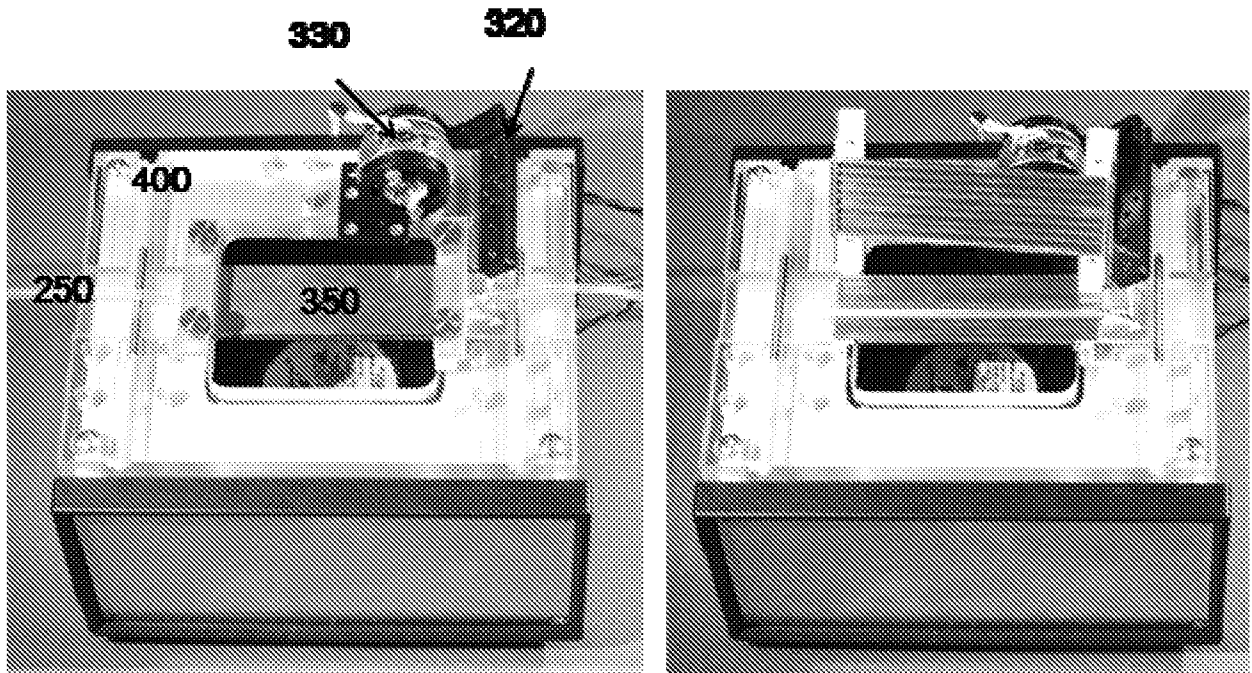


Figure 7

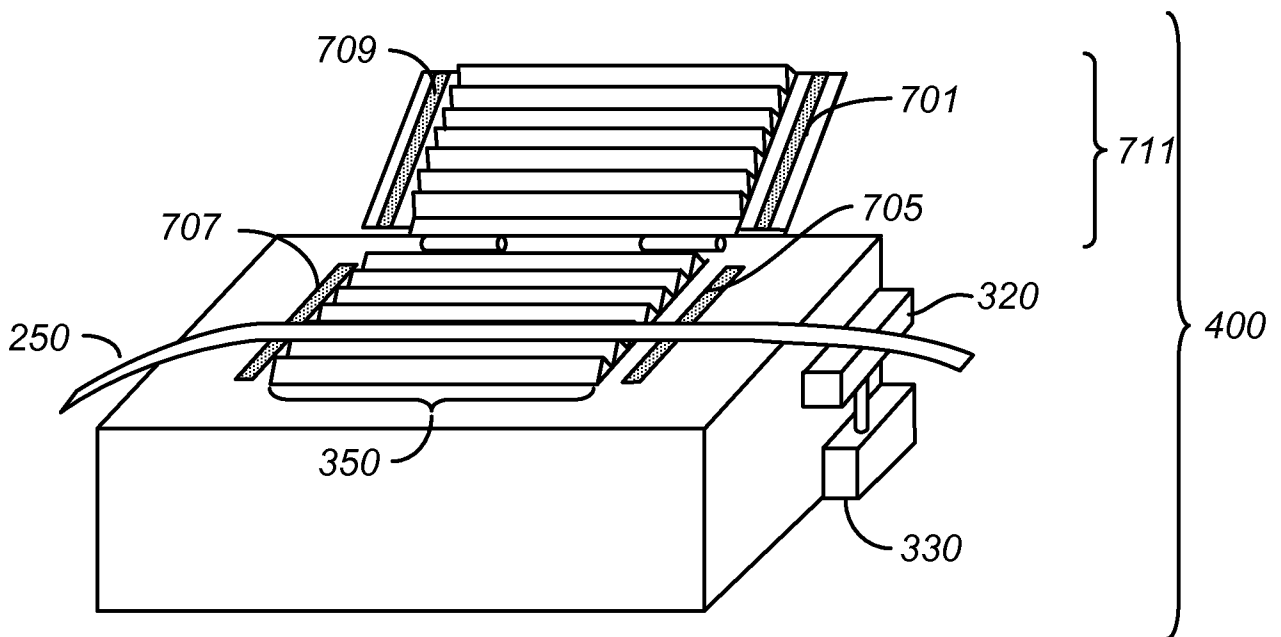


Figure 8

REPLACEMENT SHEET

9/76

PowerPlex 16 reaction amplified in Teflon based Reaction Chambers on an MBI Thermocycling Subsystem device with separation and detection on the MegaBACE1000

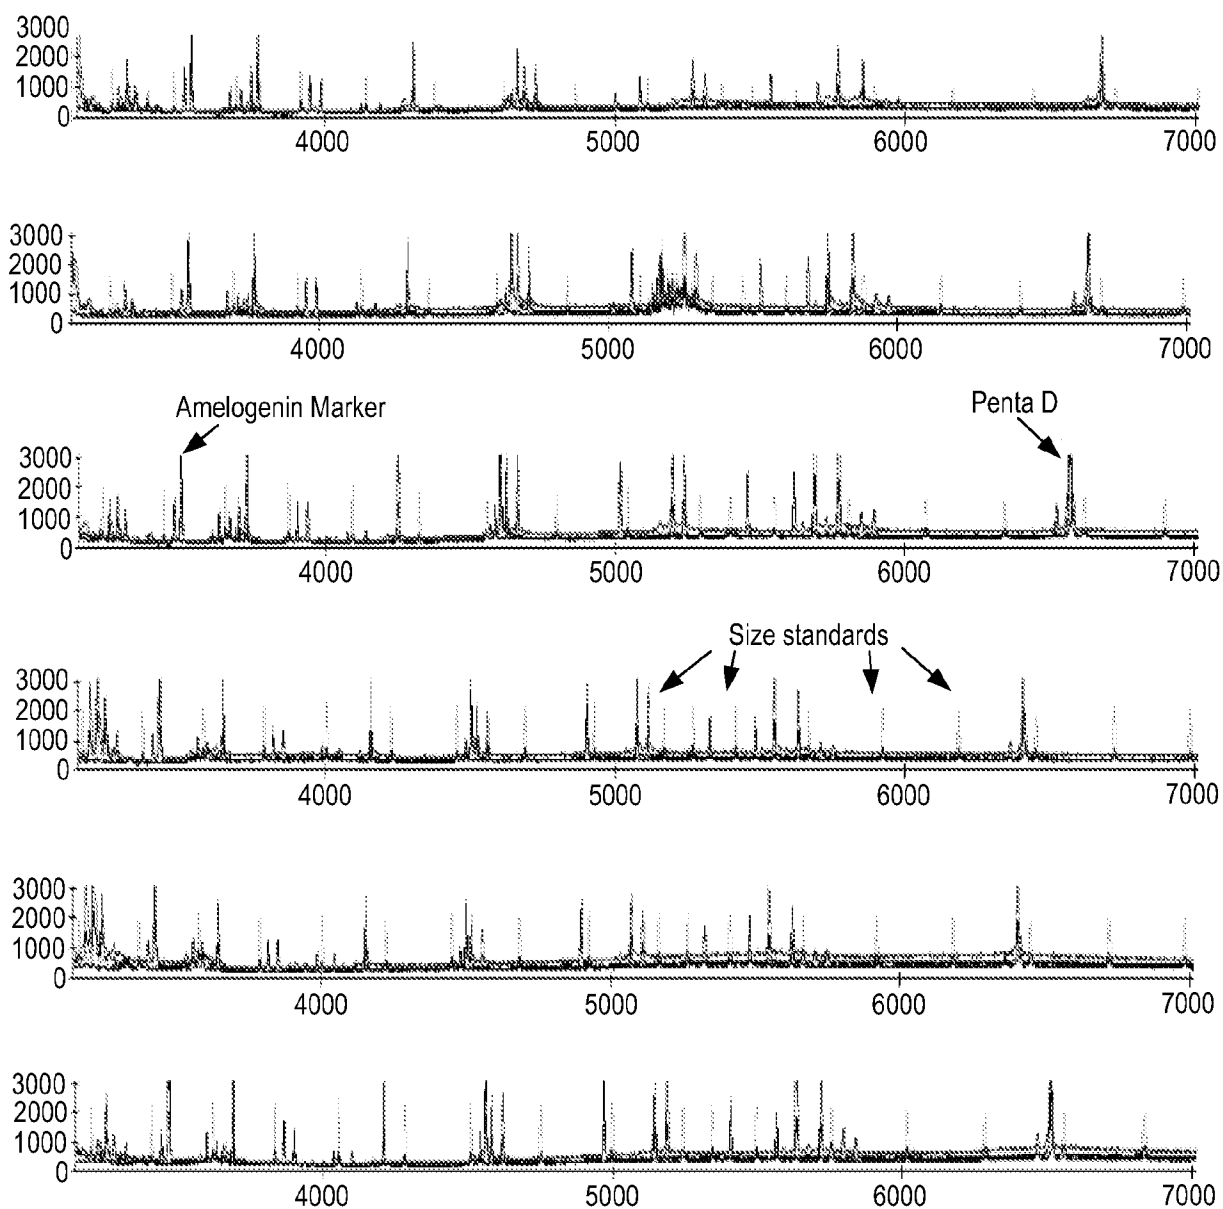


Figure 9

10/76

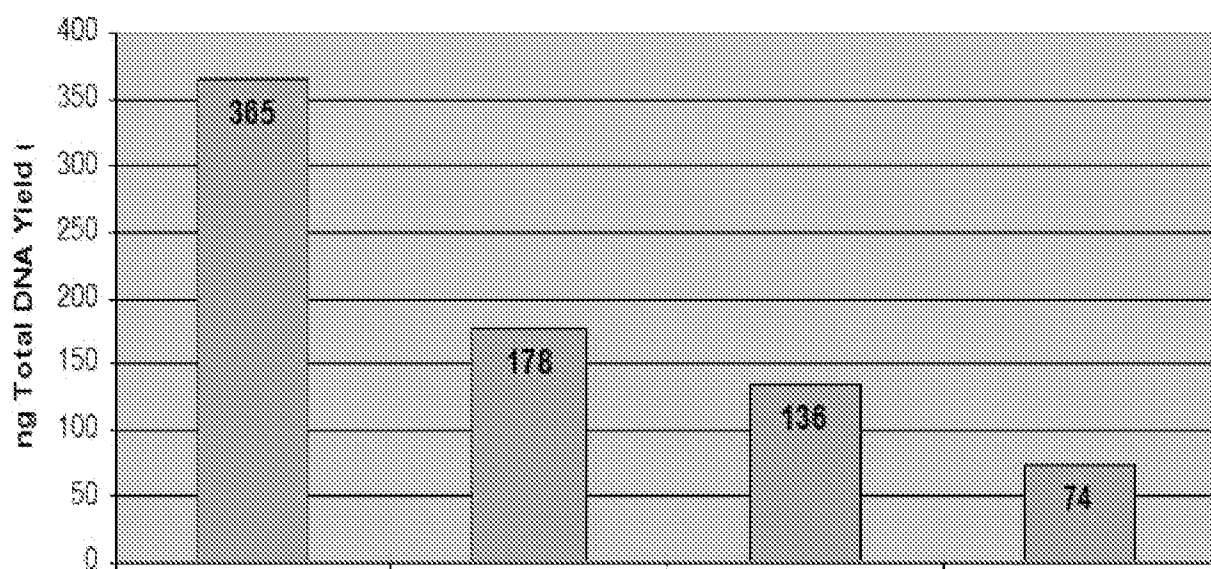


Figure 10

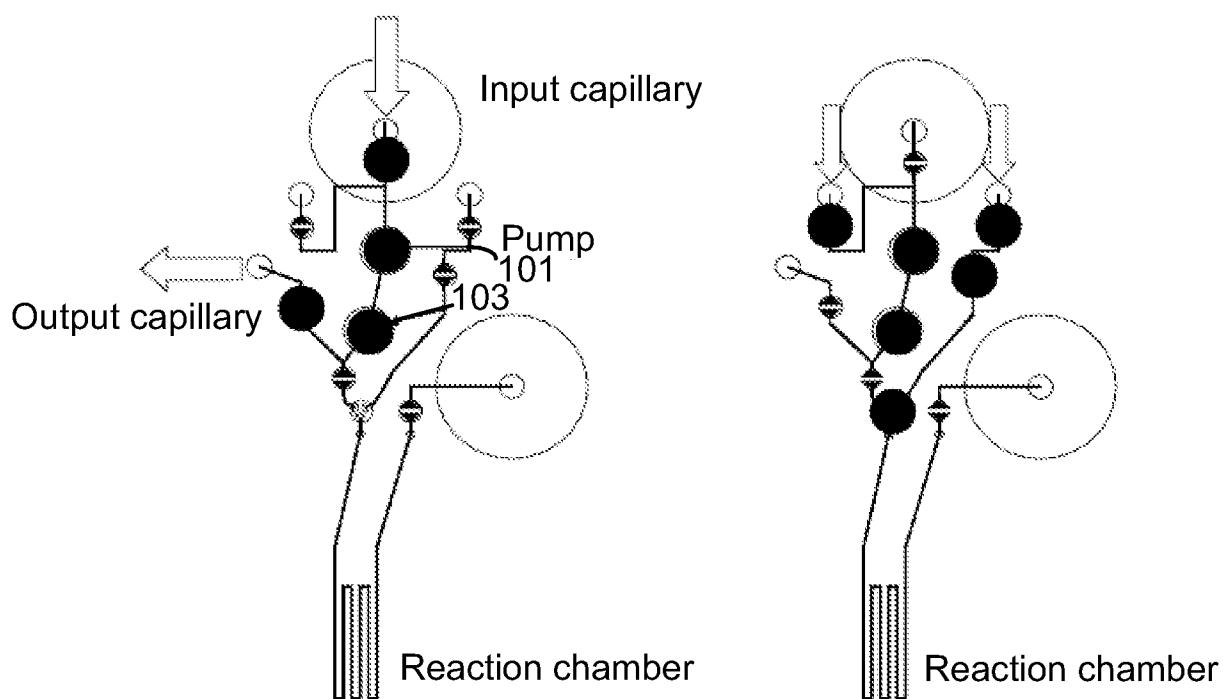


Figure 11

11/76

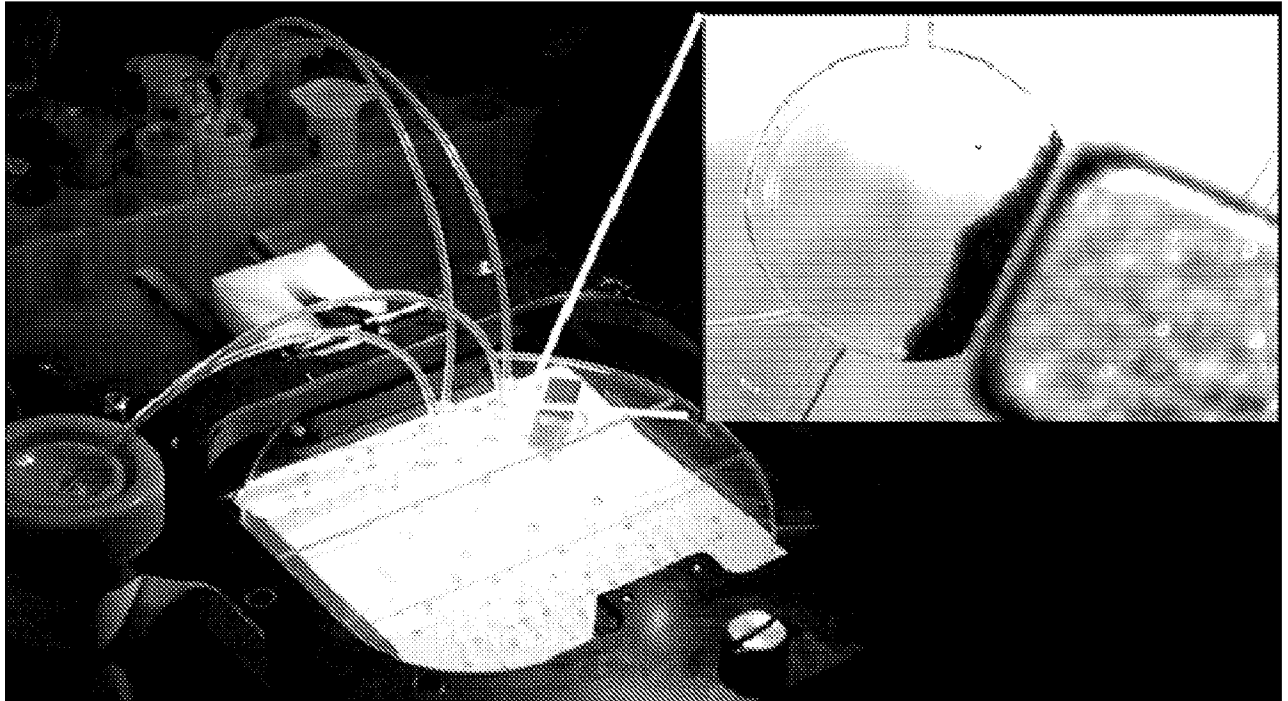


Figure 12

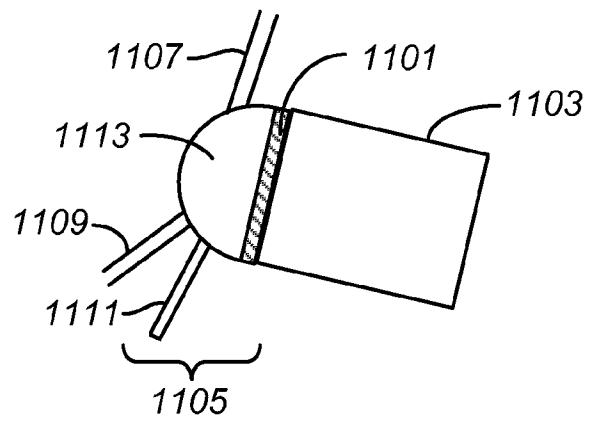


Figure 13

12/76

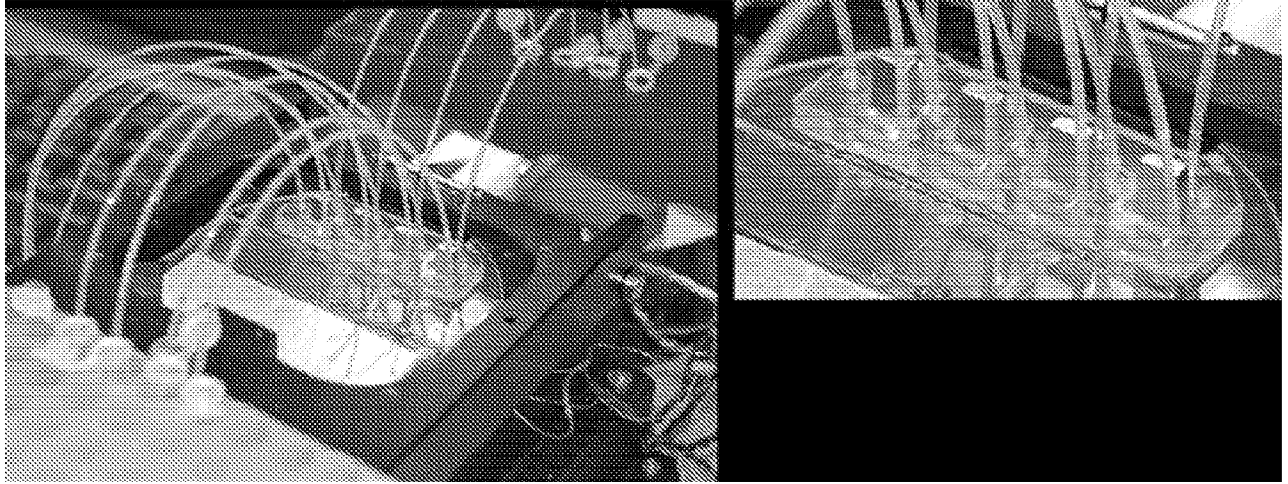


Figure 14

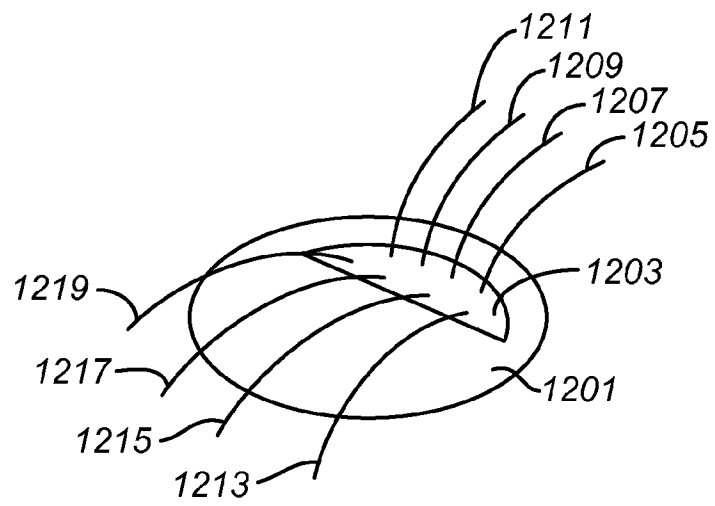


Figure 15

13/76

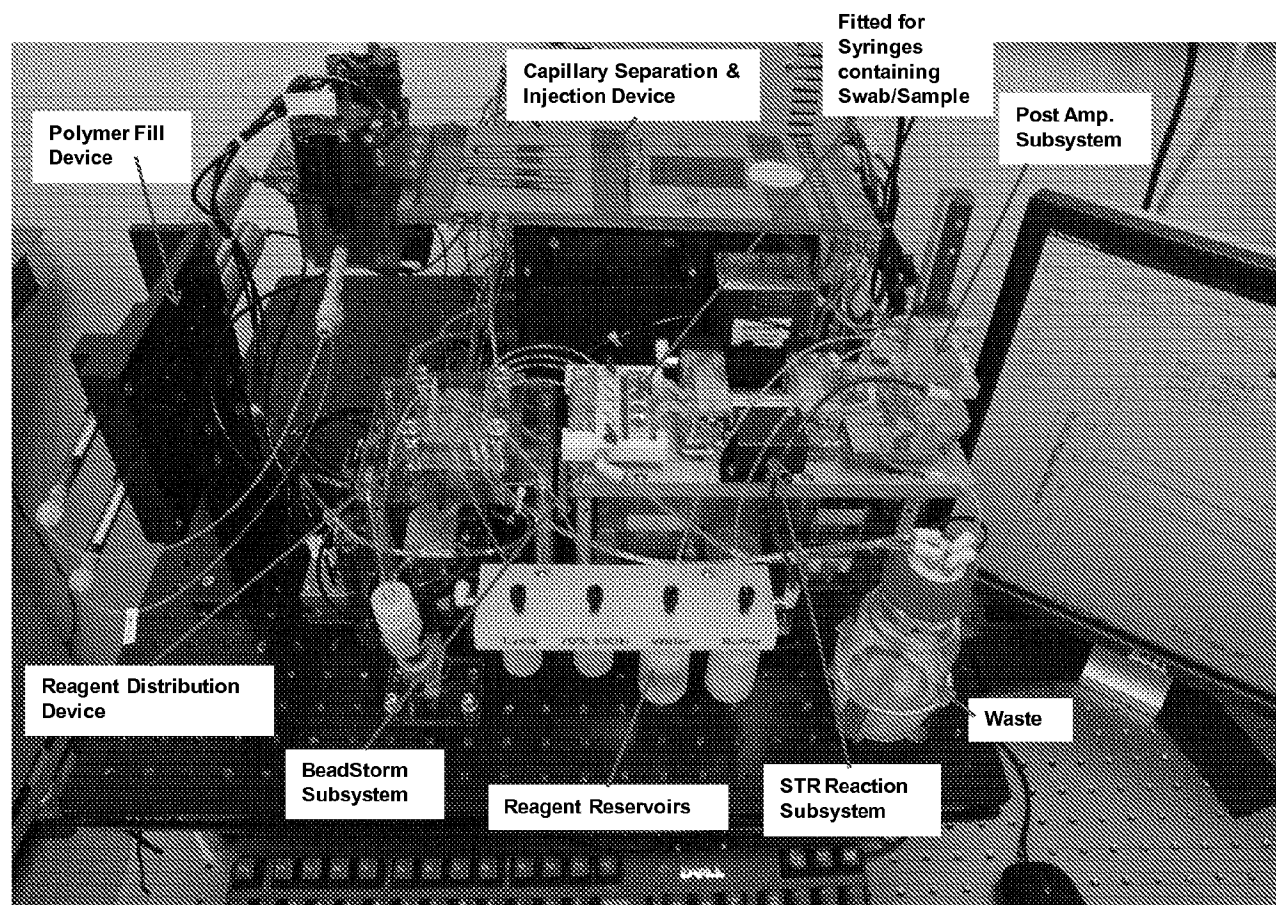


Figure 16

14/76

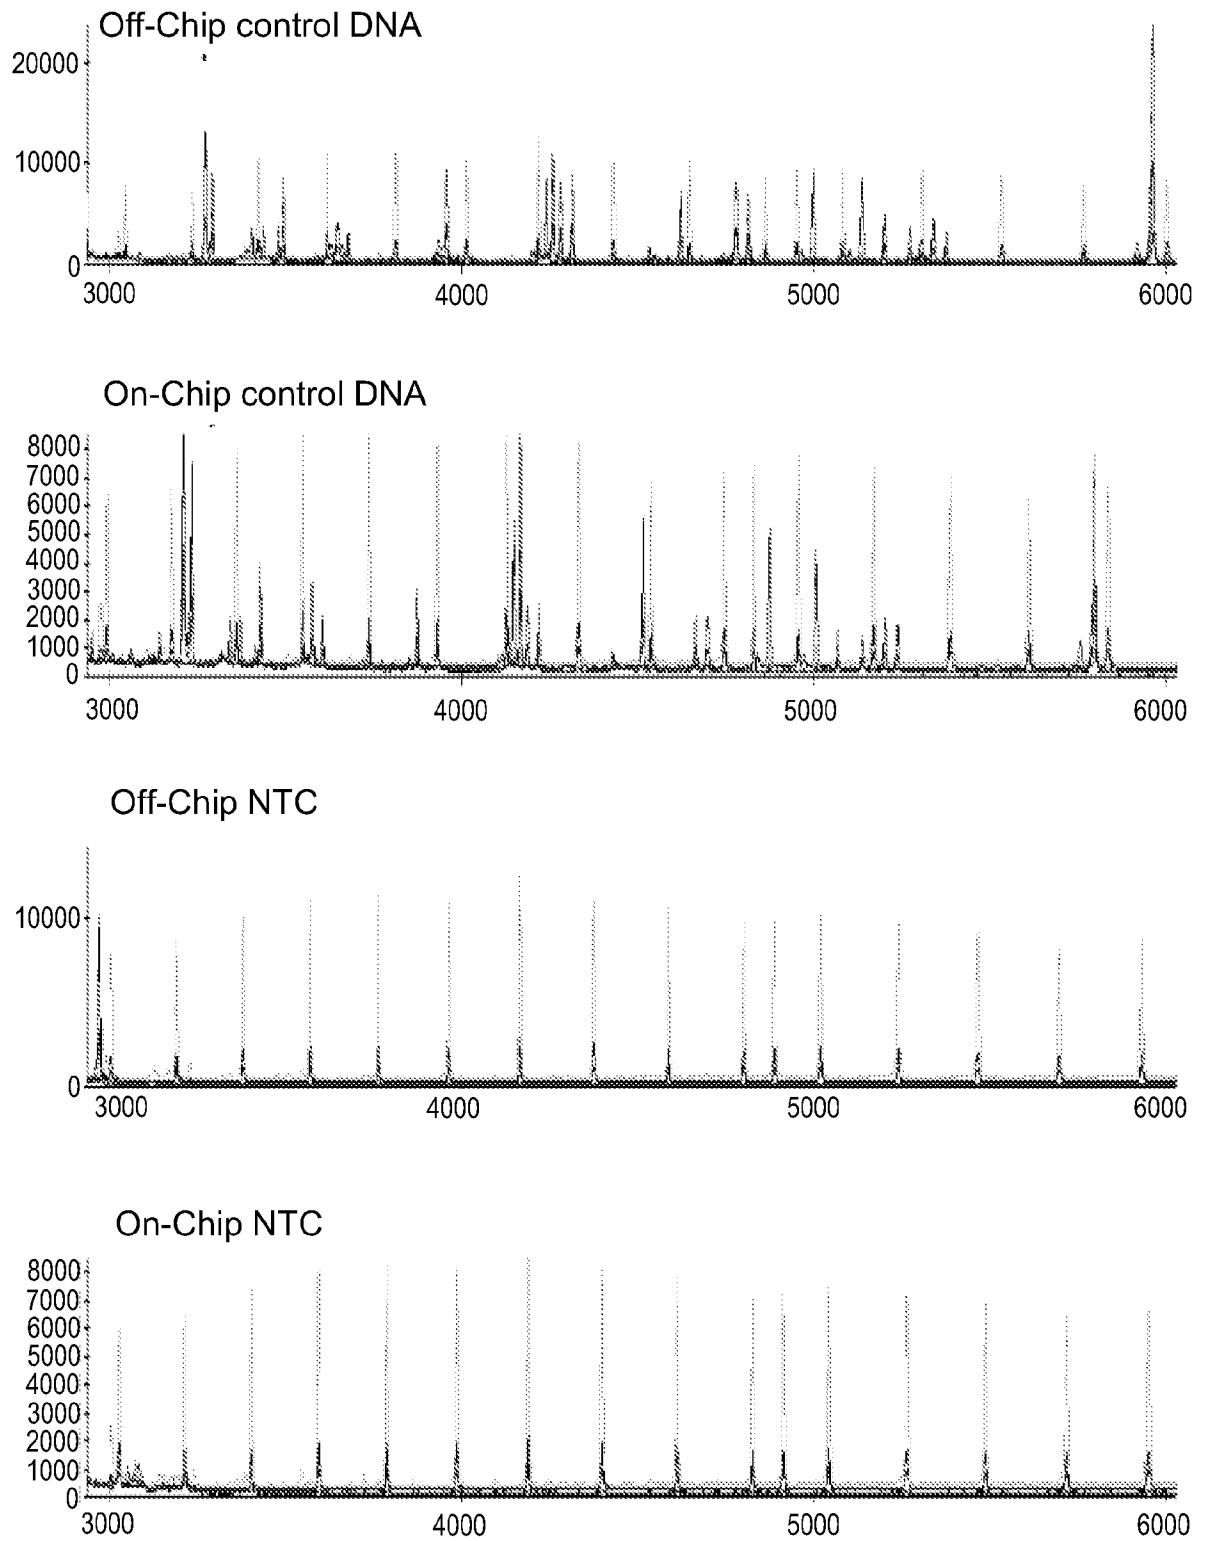


Figure 17

15/76

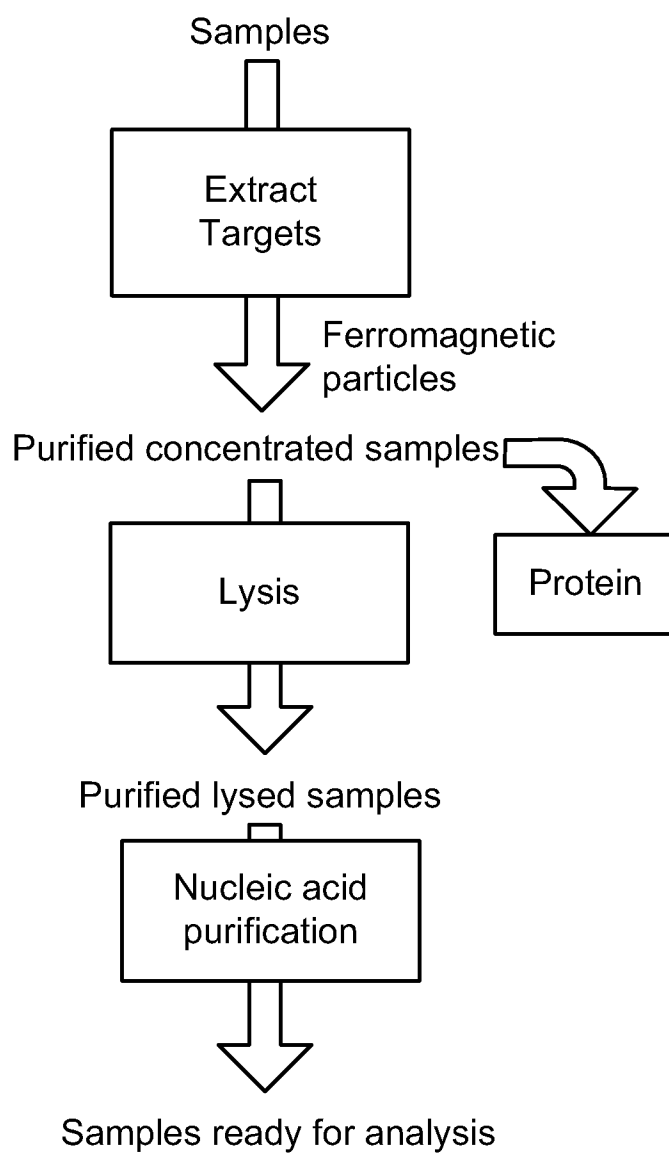


Figure 18

16/76

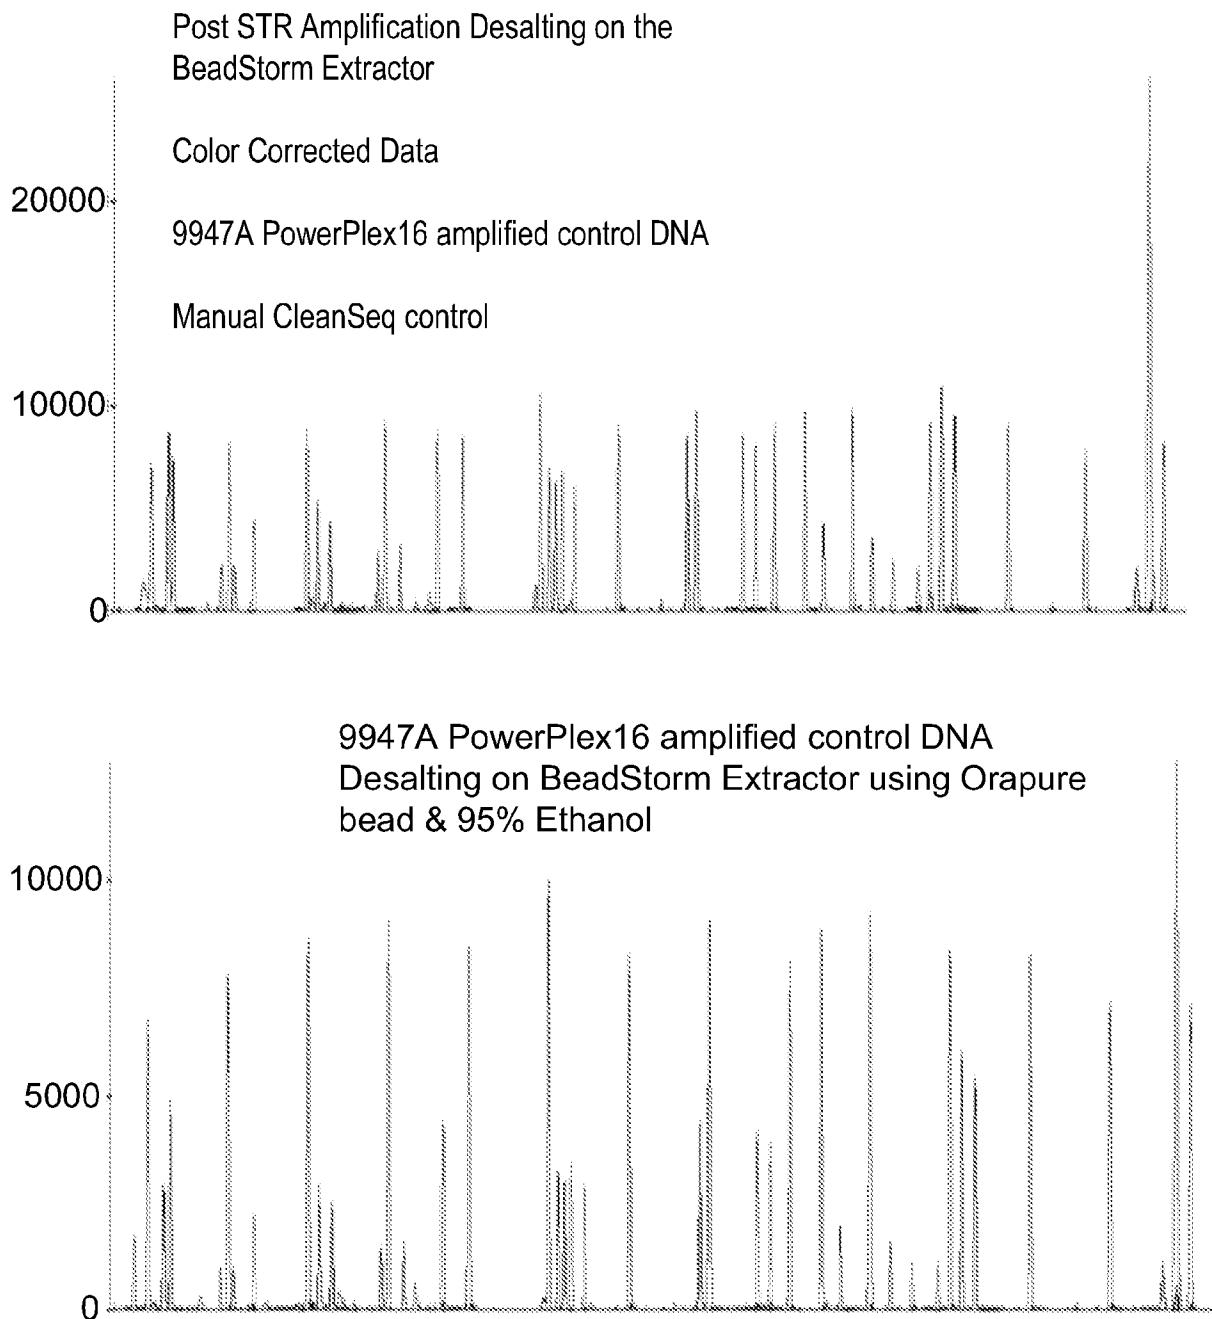


Figure 19

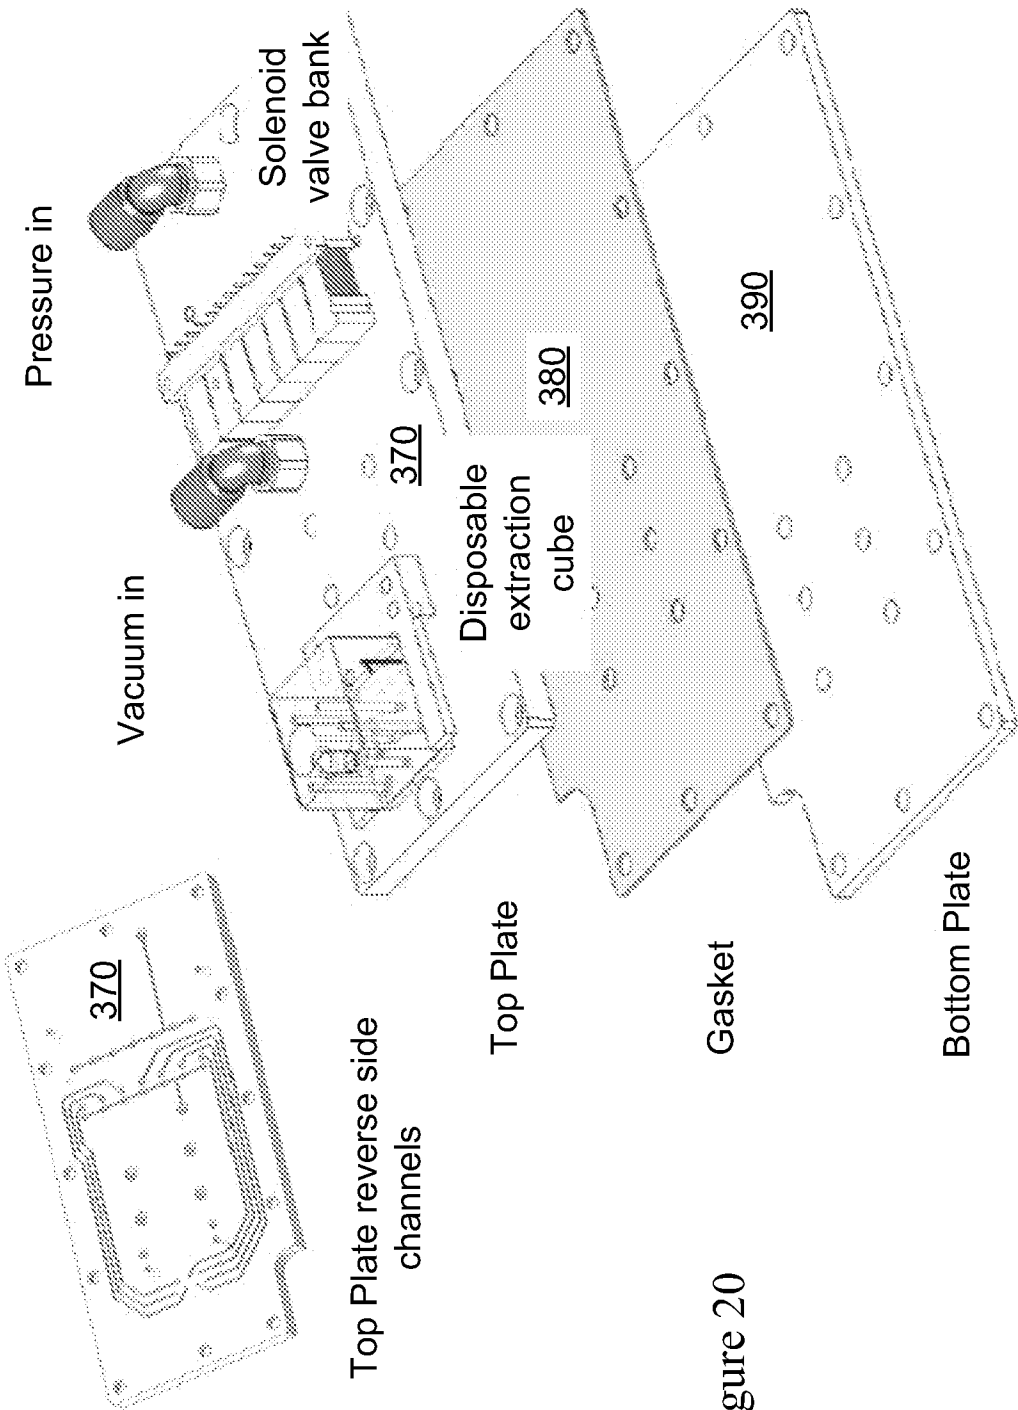


Figure 20



Figure 21

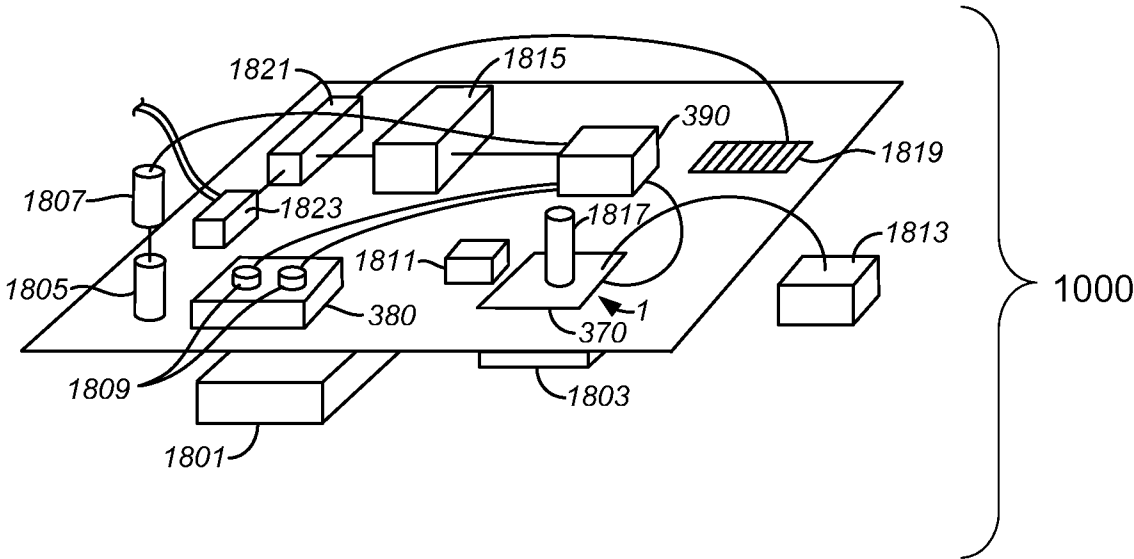


Figure 22

20/76

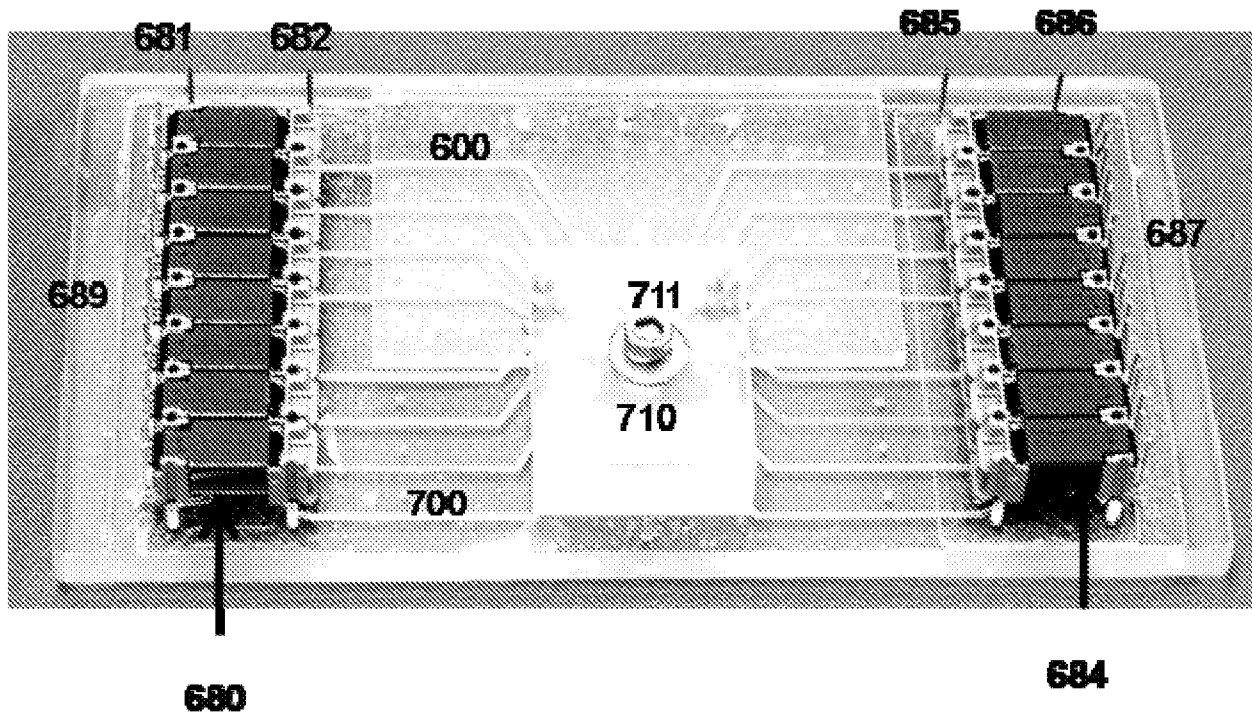


Figure 23

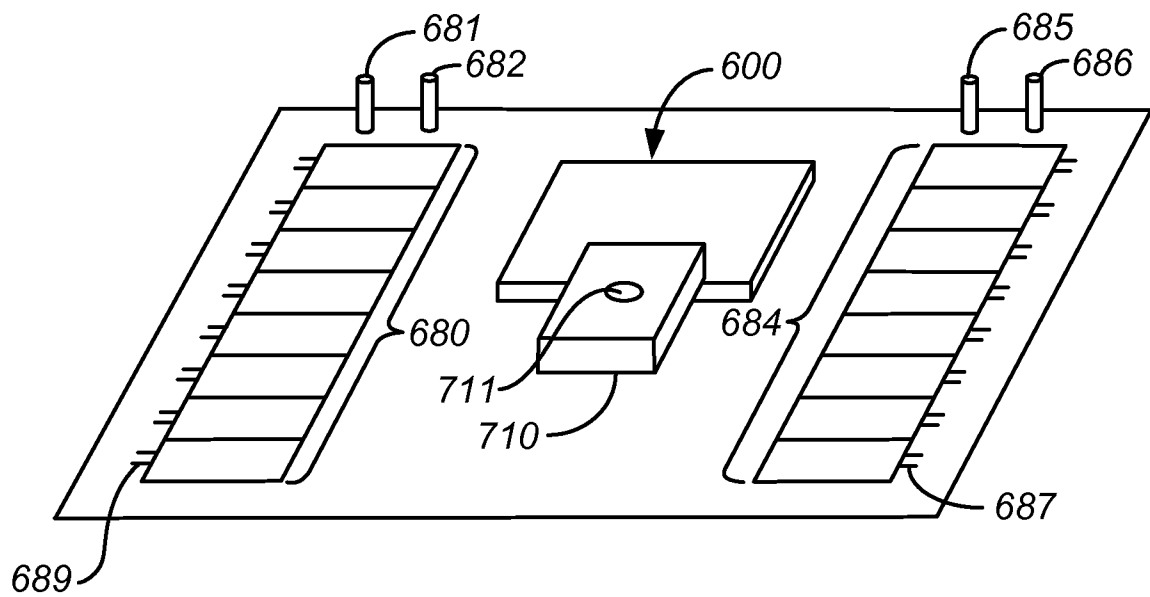


Figure 24

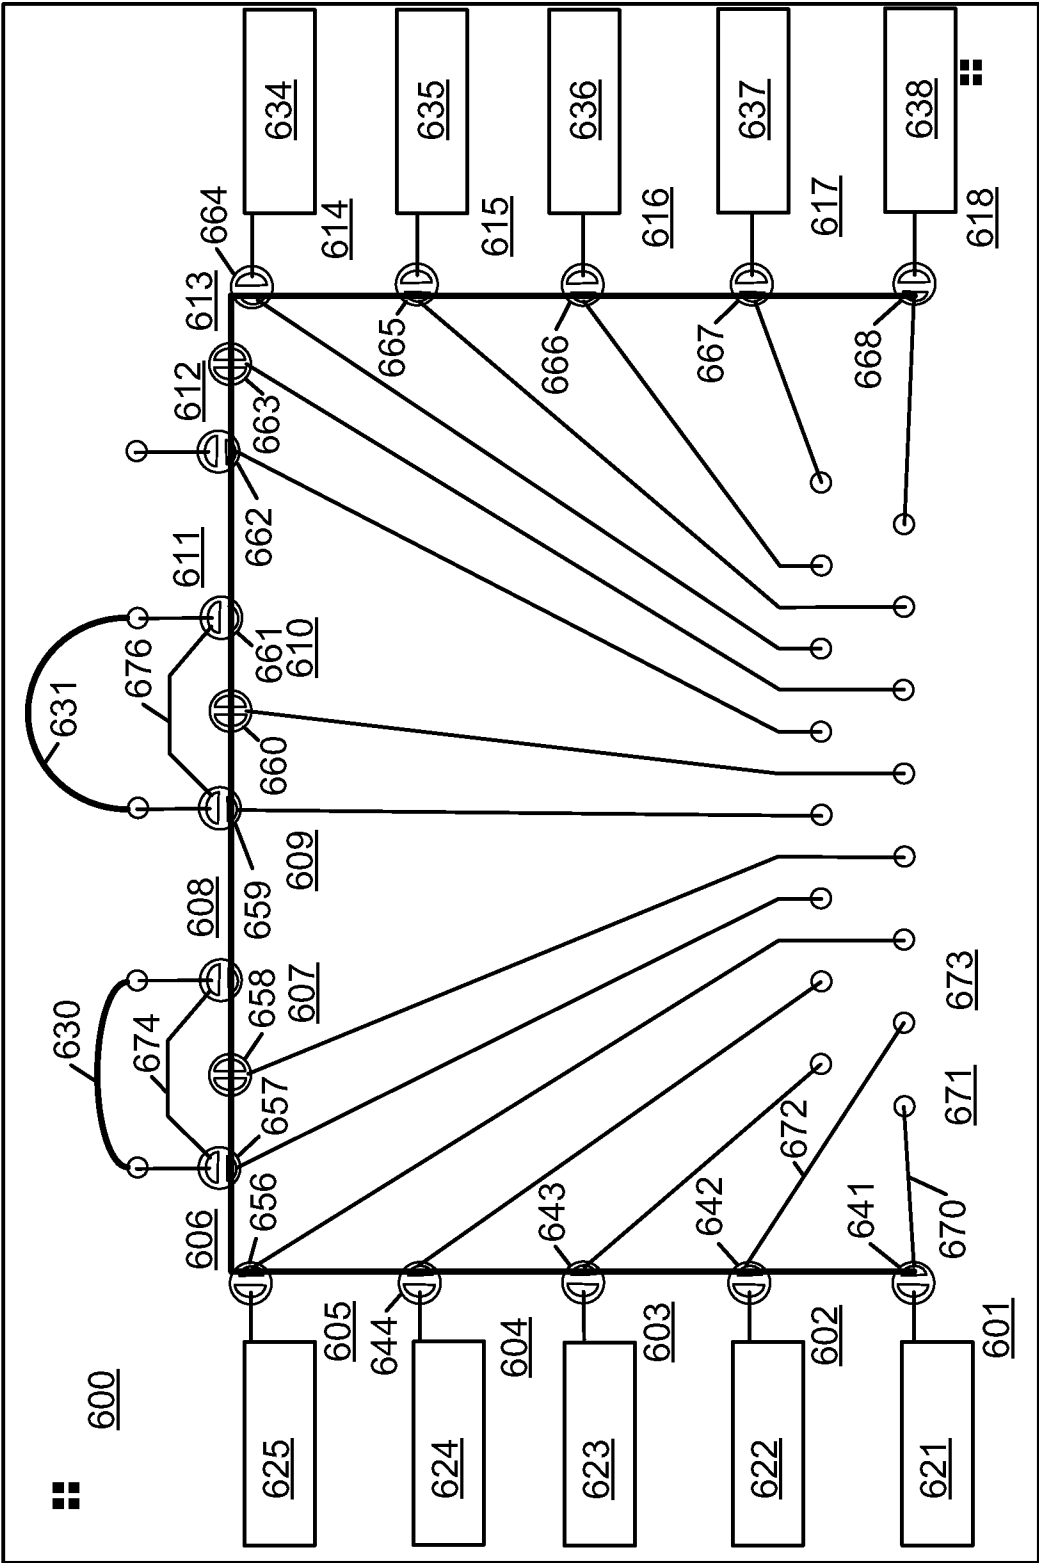


Figure 25

22/76

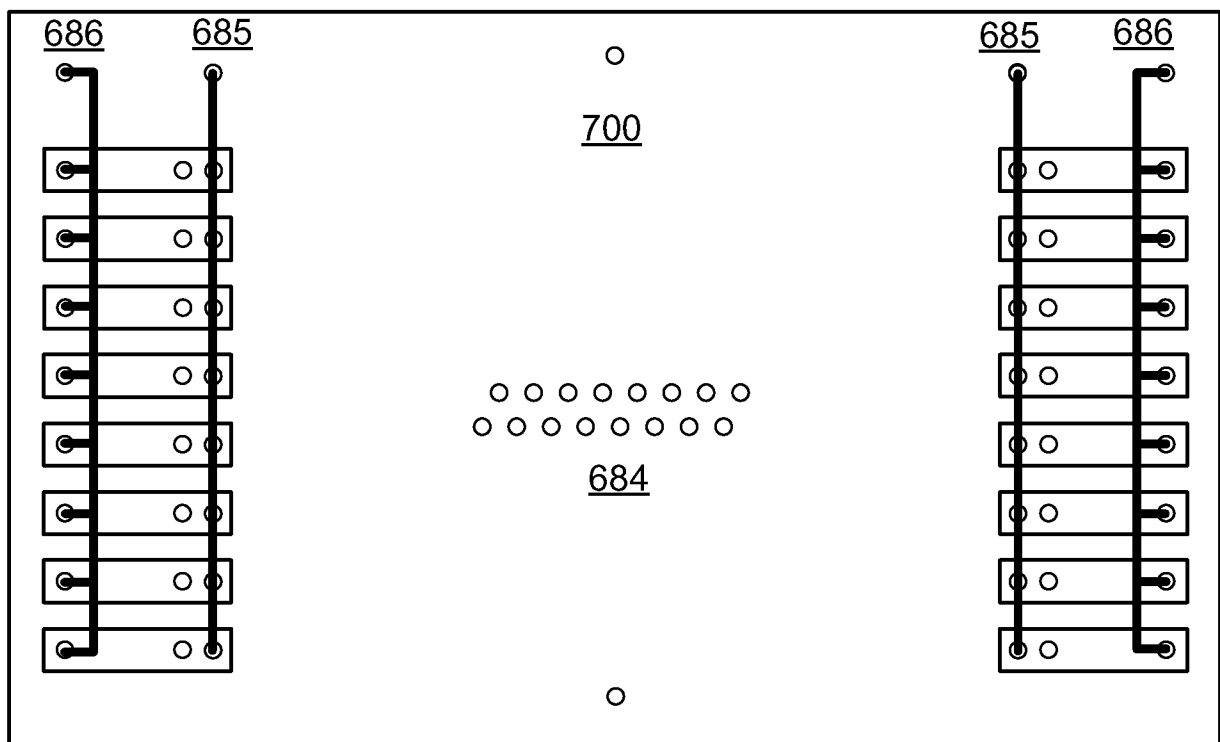
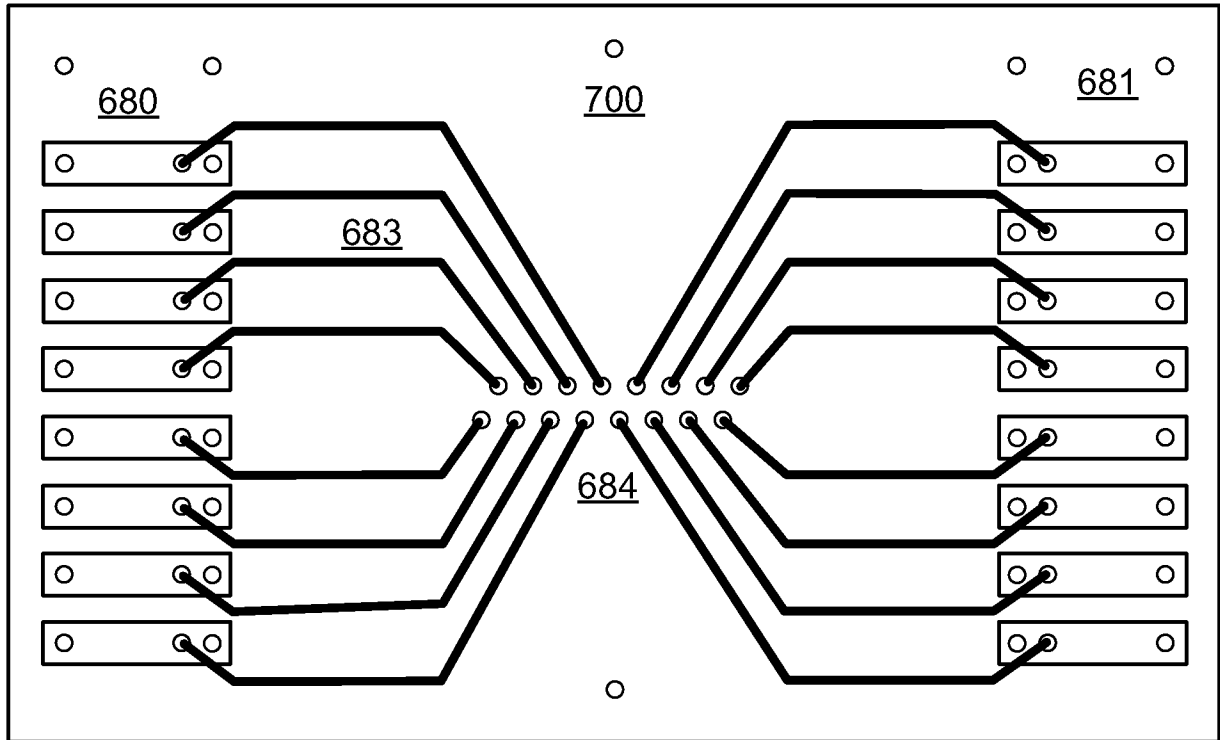


Figure 26

23/76

E. coli Detection by IMS
with subsequent NaOH Lysis & Bead-based DNA Purification

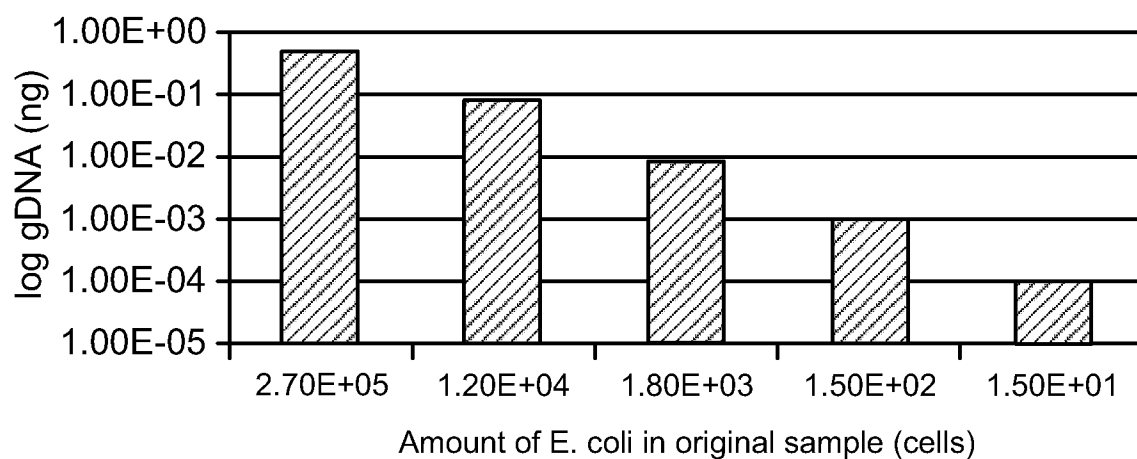


Figure 27

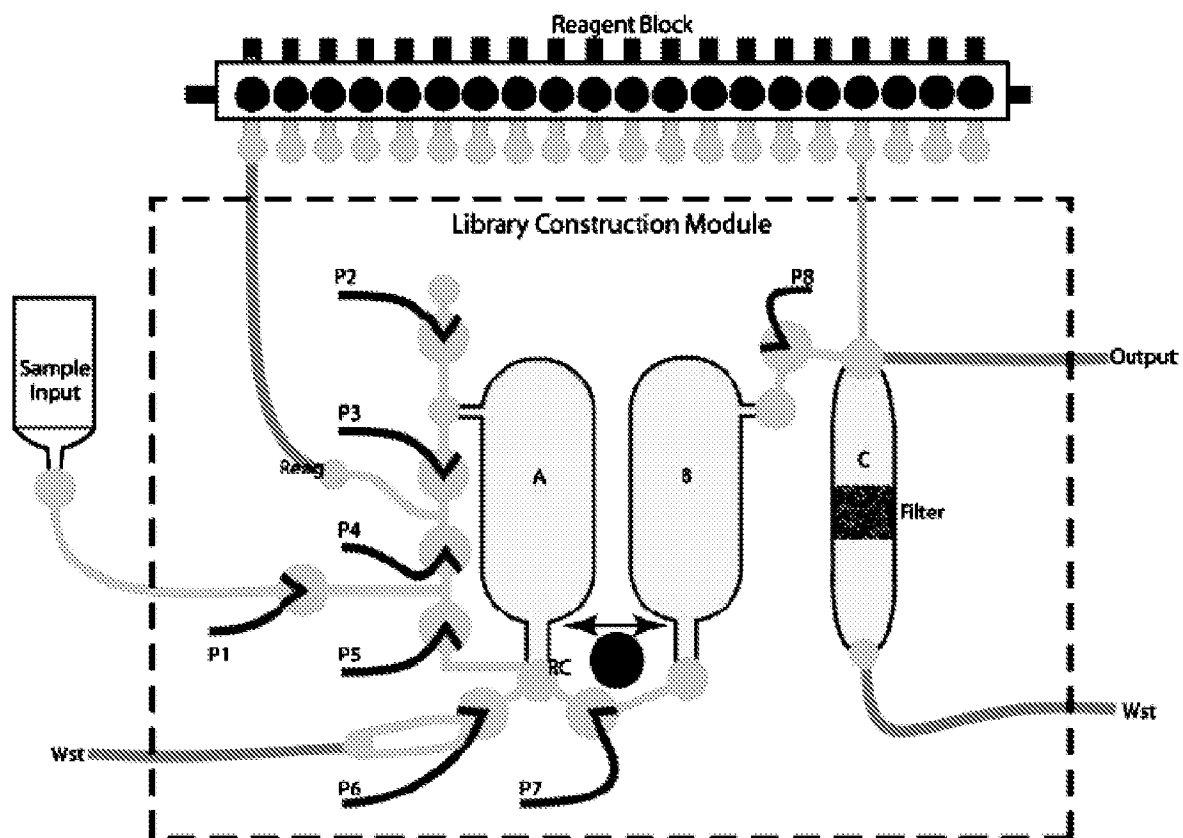


Figure 28

24/76

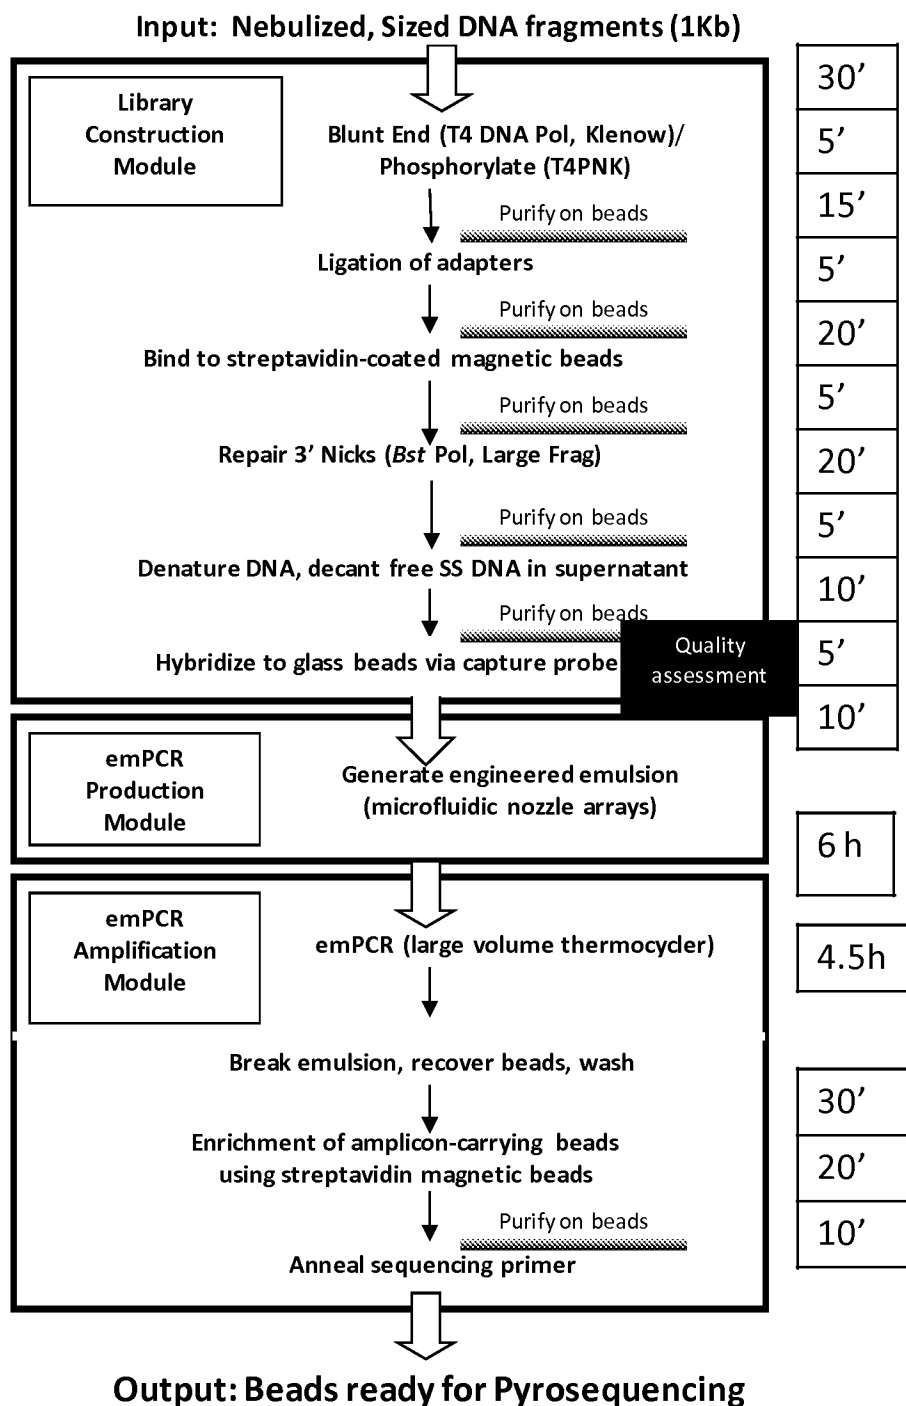


Figure 29

25/76

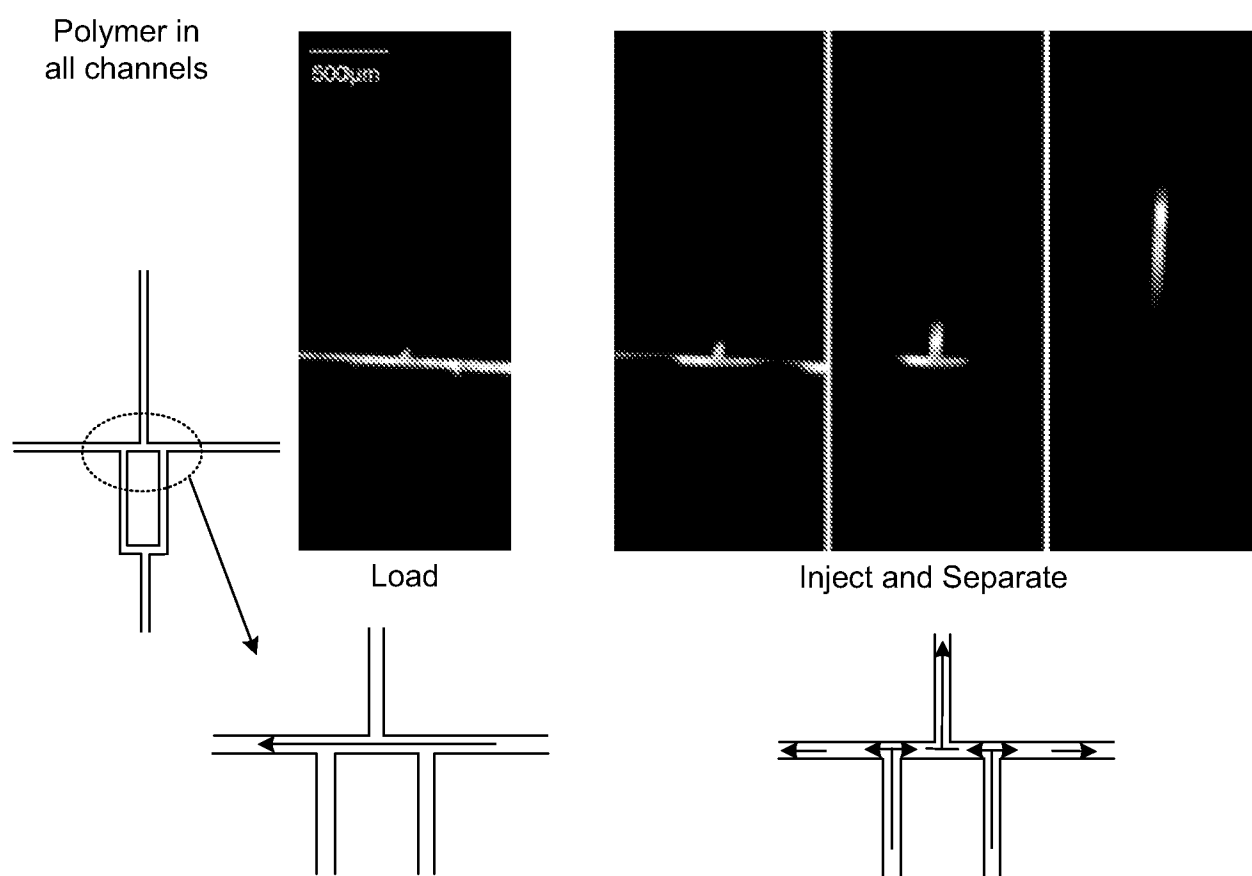


Figure 30

26/76

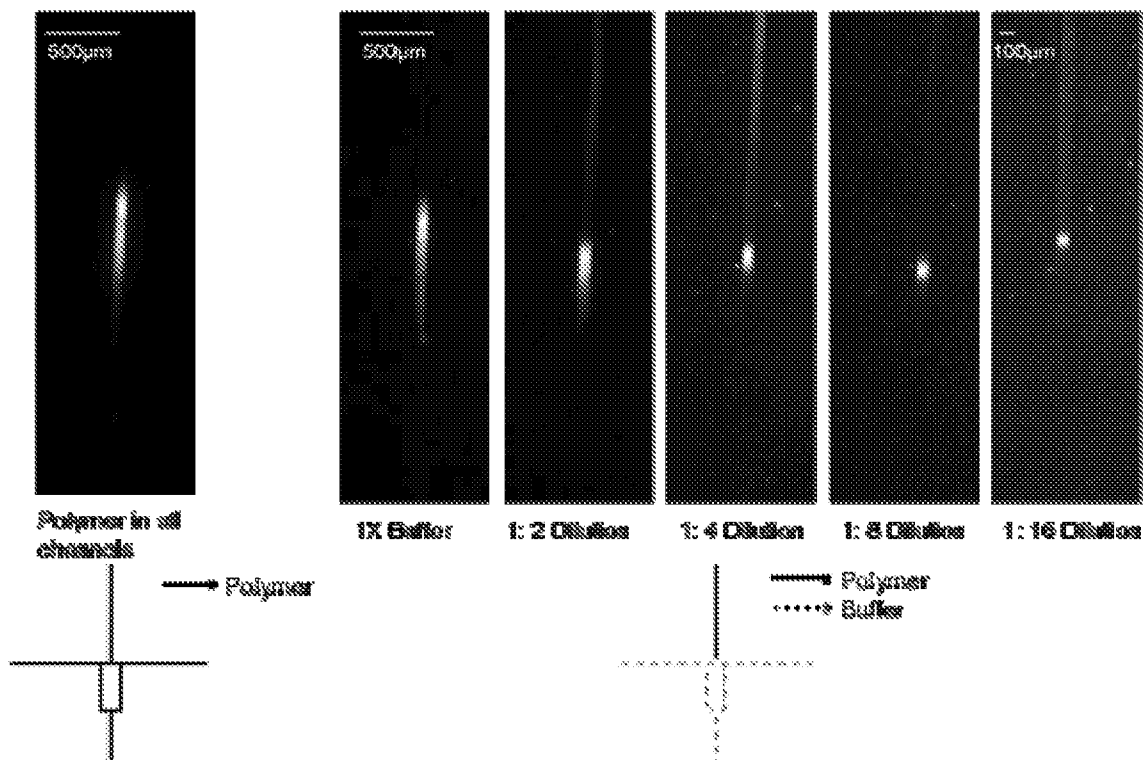


Figure 31

27/76


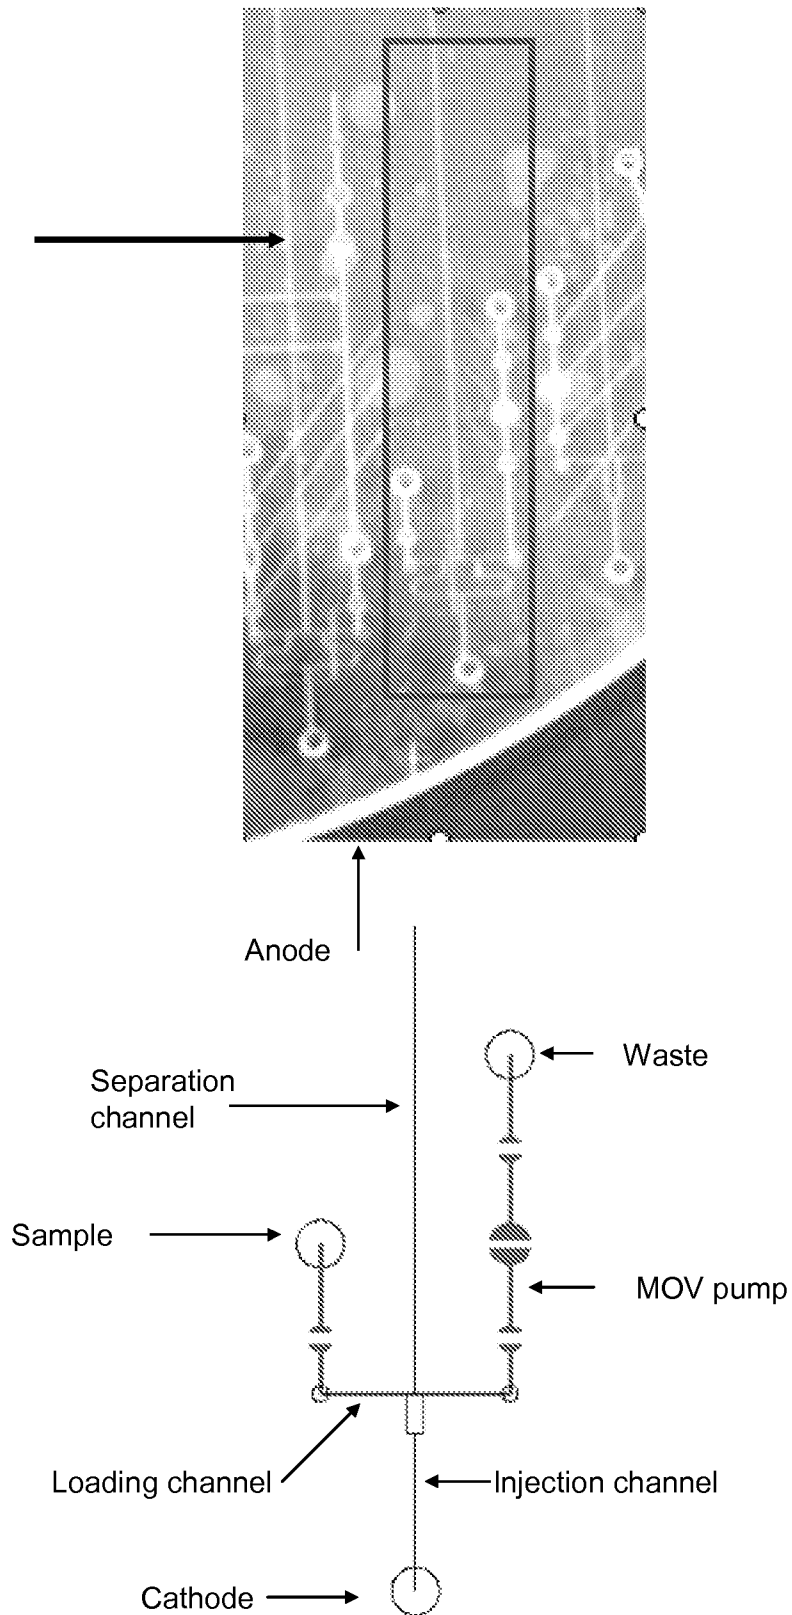



Figure 32

28/76


STR Sample Loading



Initiate sample
pumping across
loading channel



Pump
through-stroke




Complete pump
loading

Polymer
filled
Channel


STR Sample Injection

Initiate Injection



Apply high
voltage across
cathode and
anode

Electrophoresis



Apply high
voltage across
cathode and
anode

Figure 33

29/76

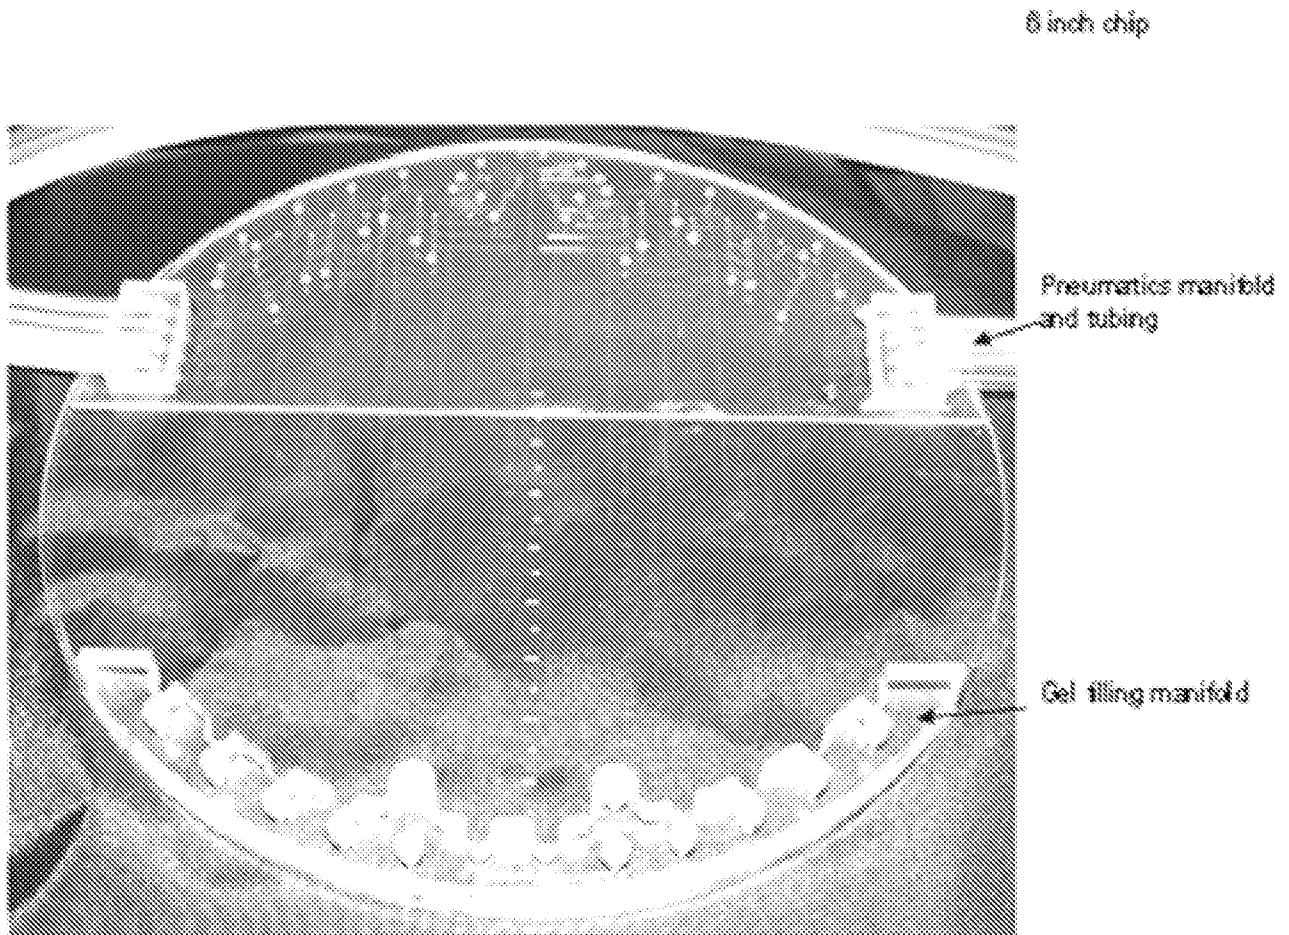


Figure 34


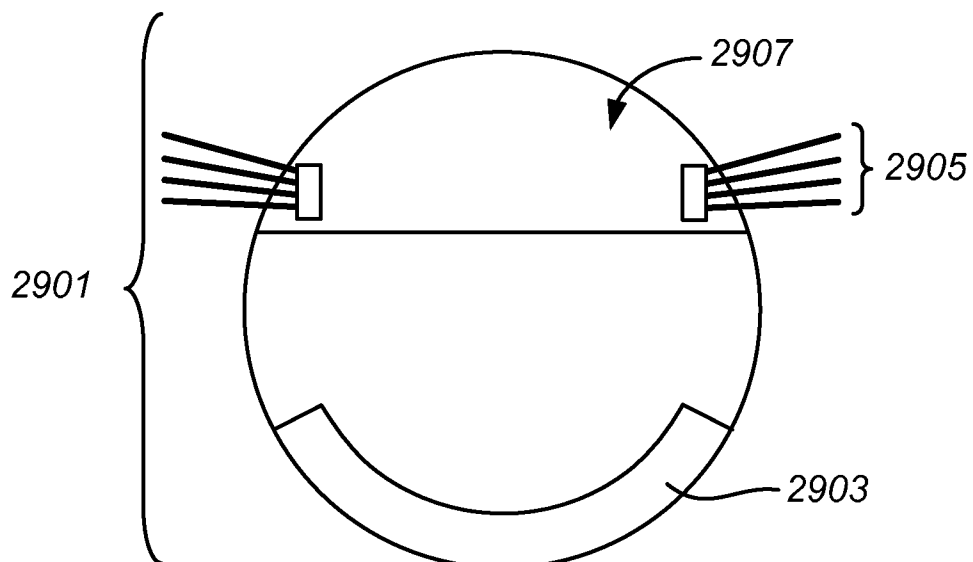


Figure 35

500um sample plug, separated using 125 v/cm on LPA polymer. DNA fragments detected after 6.5 cm of separation

Time: the first peak comes out at ~2min and the last peak here at ~ 6.5 mins

Signal intensity: peaks 100-500 counts

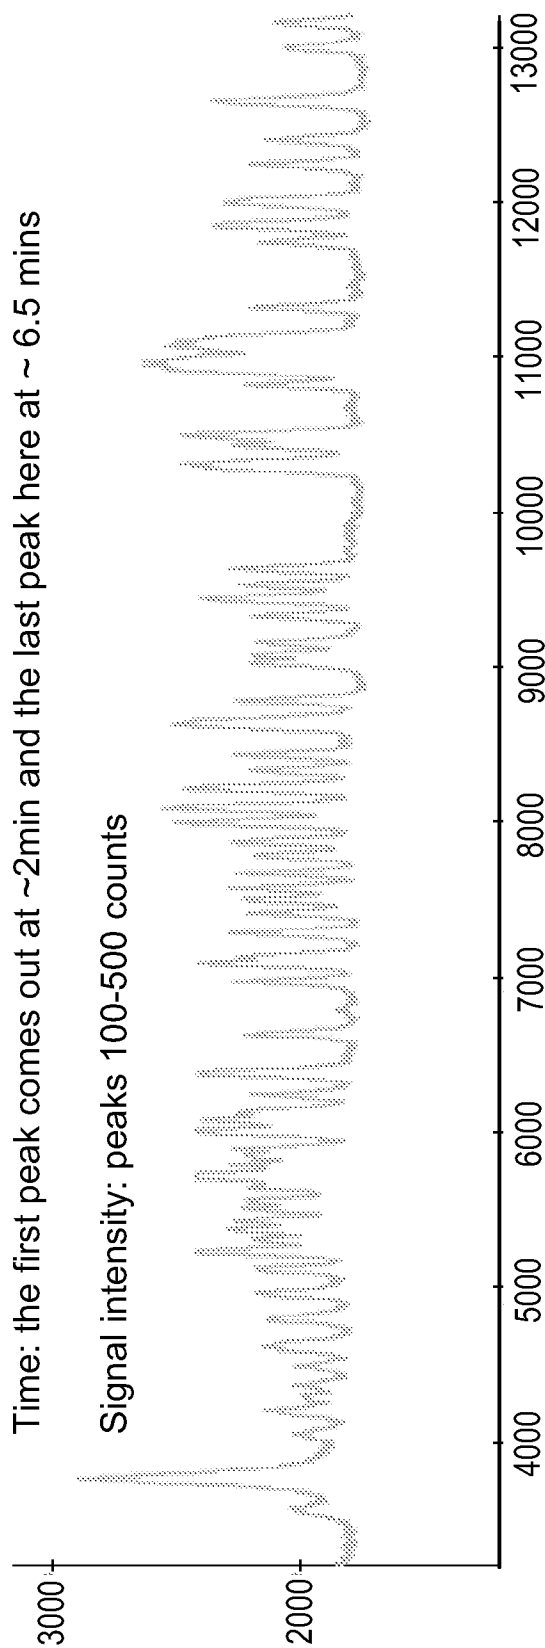

30/76

Figure 36

31/76

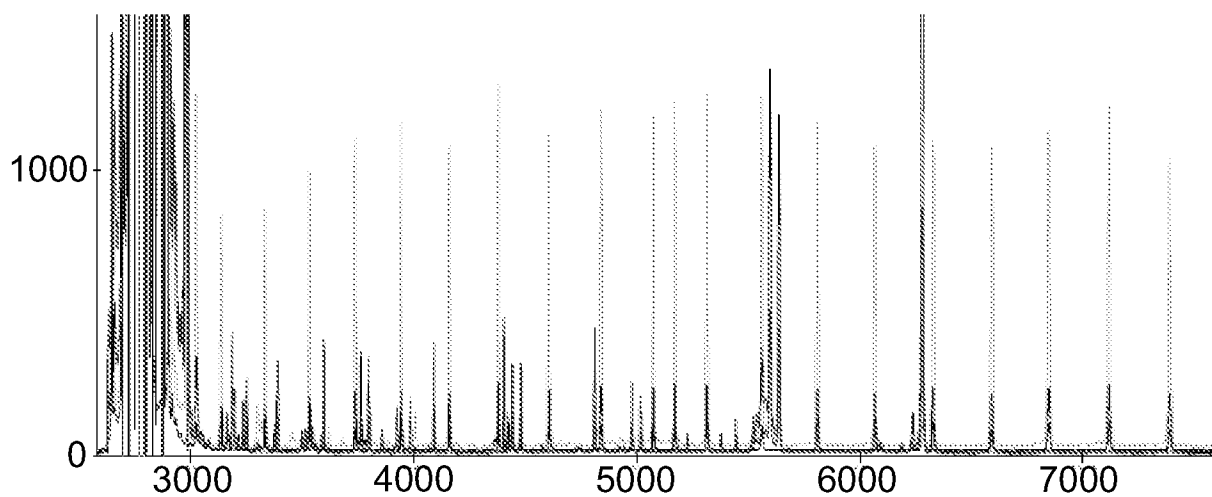
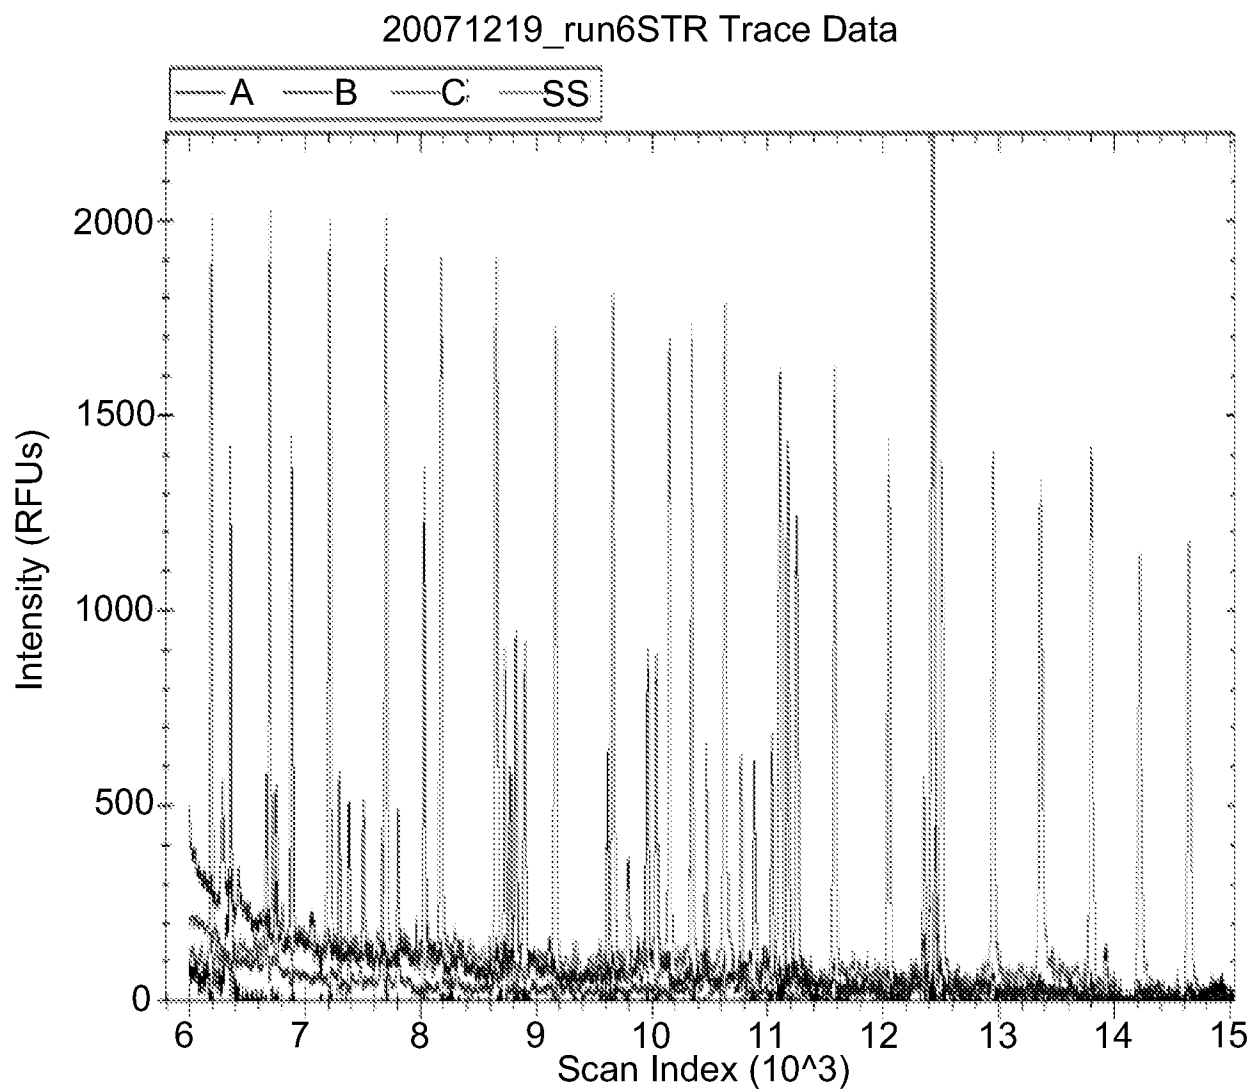


Figure 37

32/76

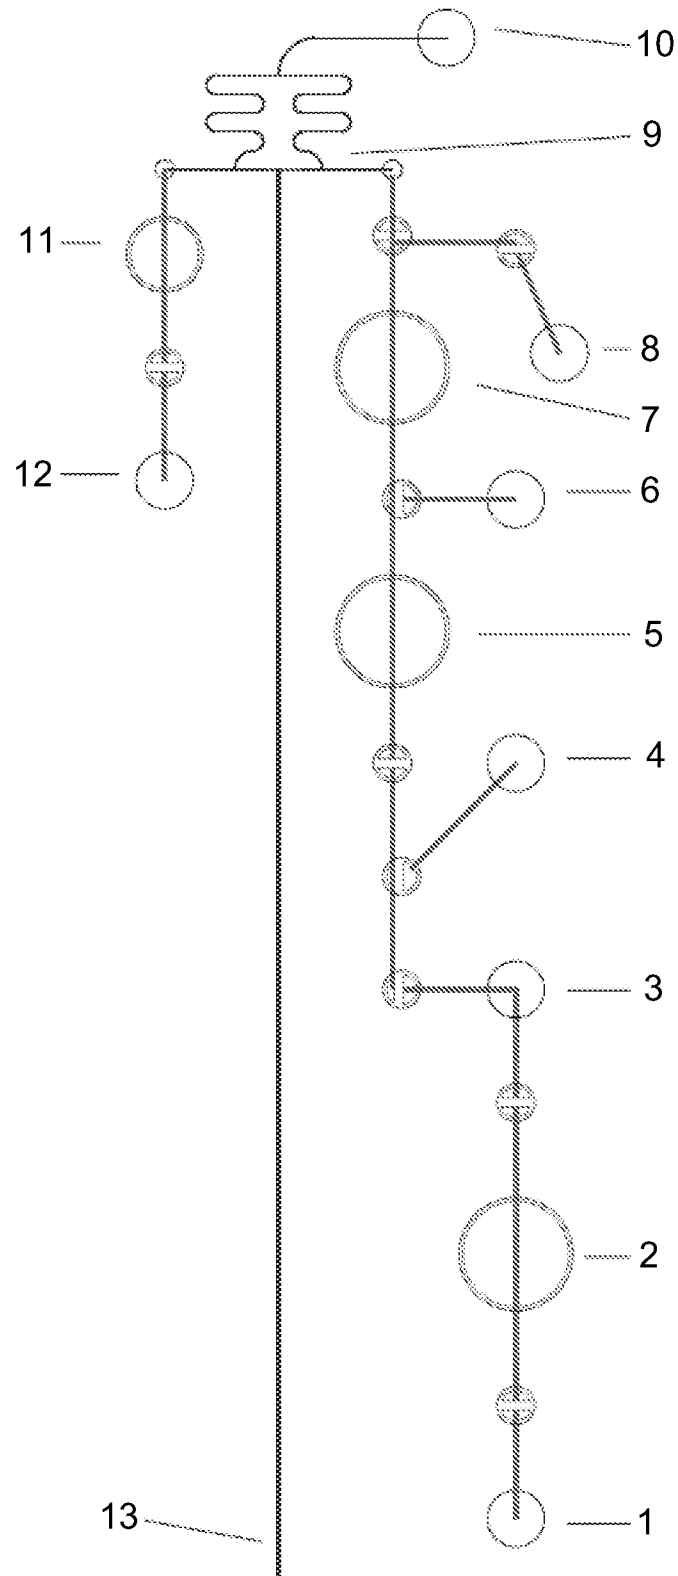


Figure 38

33/76

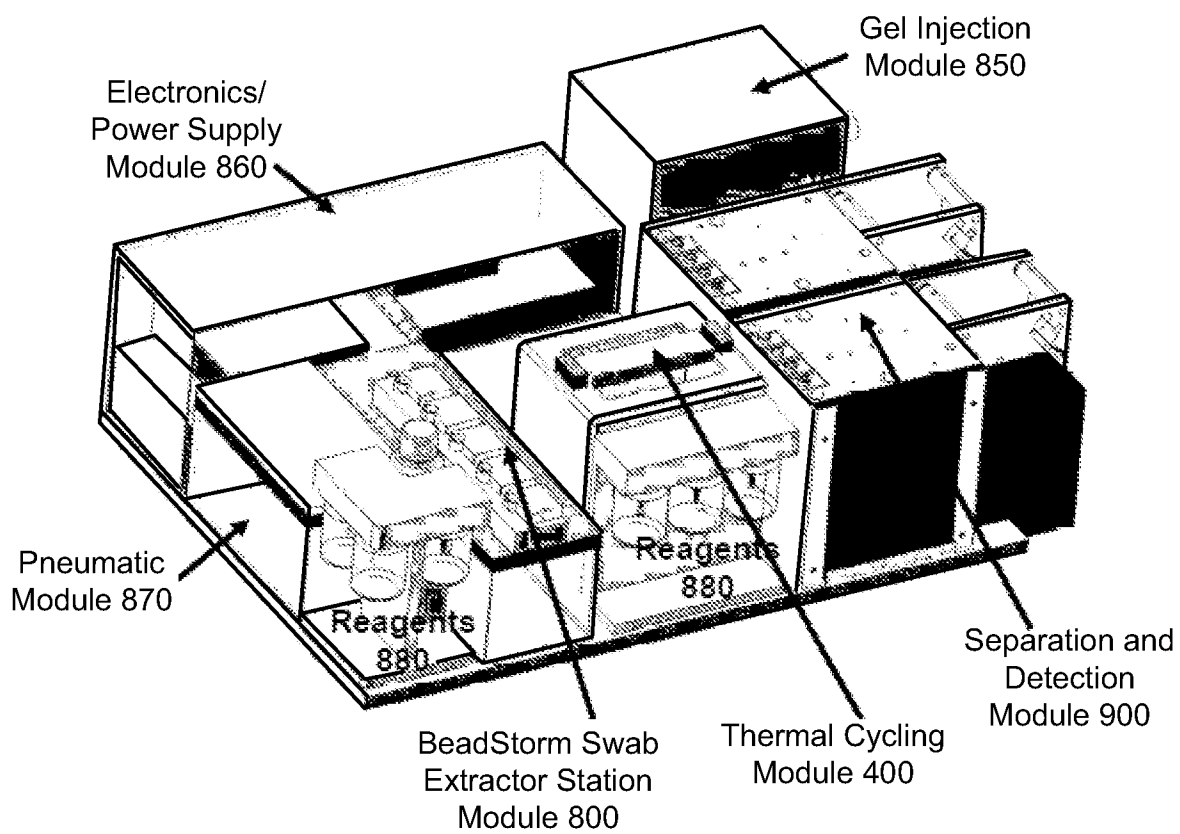


Figure 39

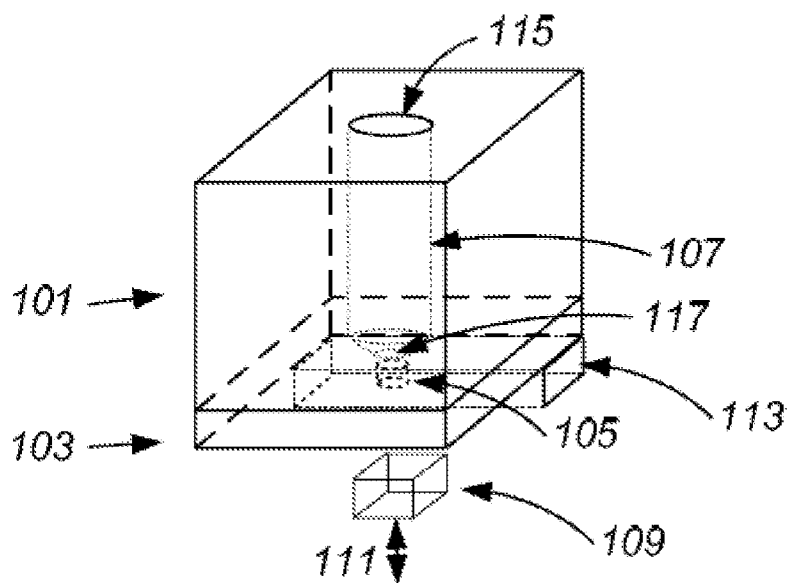


Figure 40

34/76

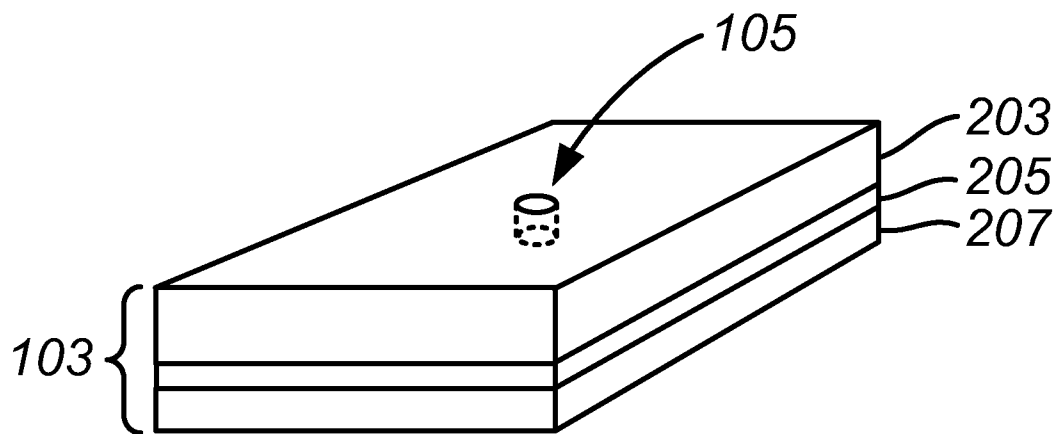


Figure 41

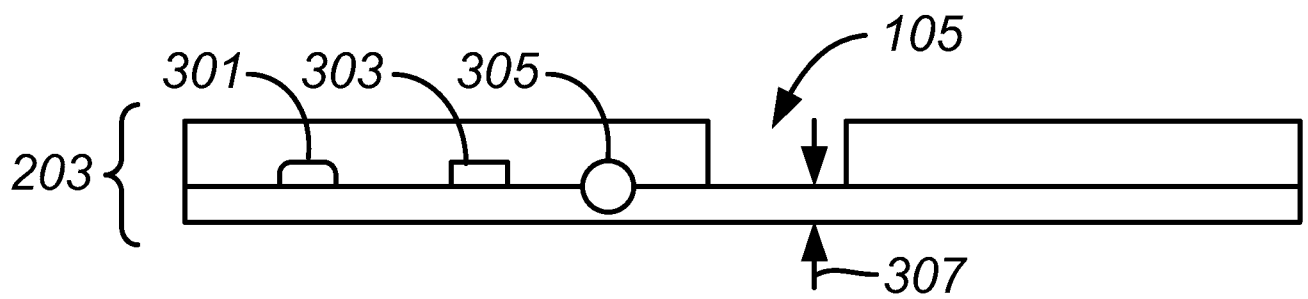


Figure 42

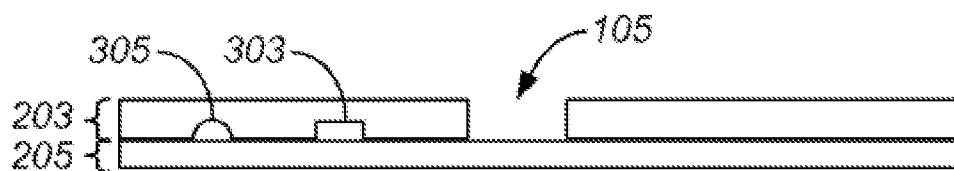


Figure 43

35/76

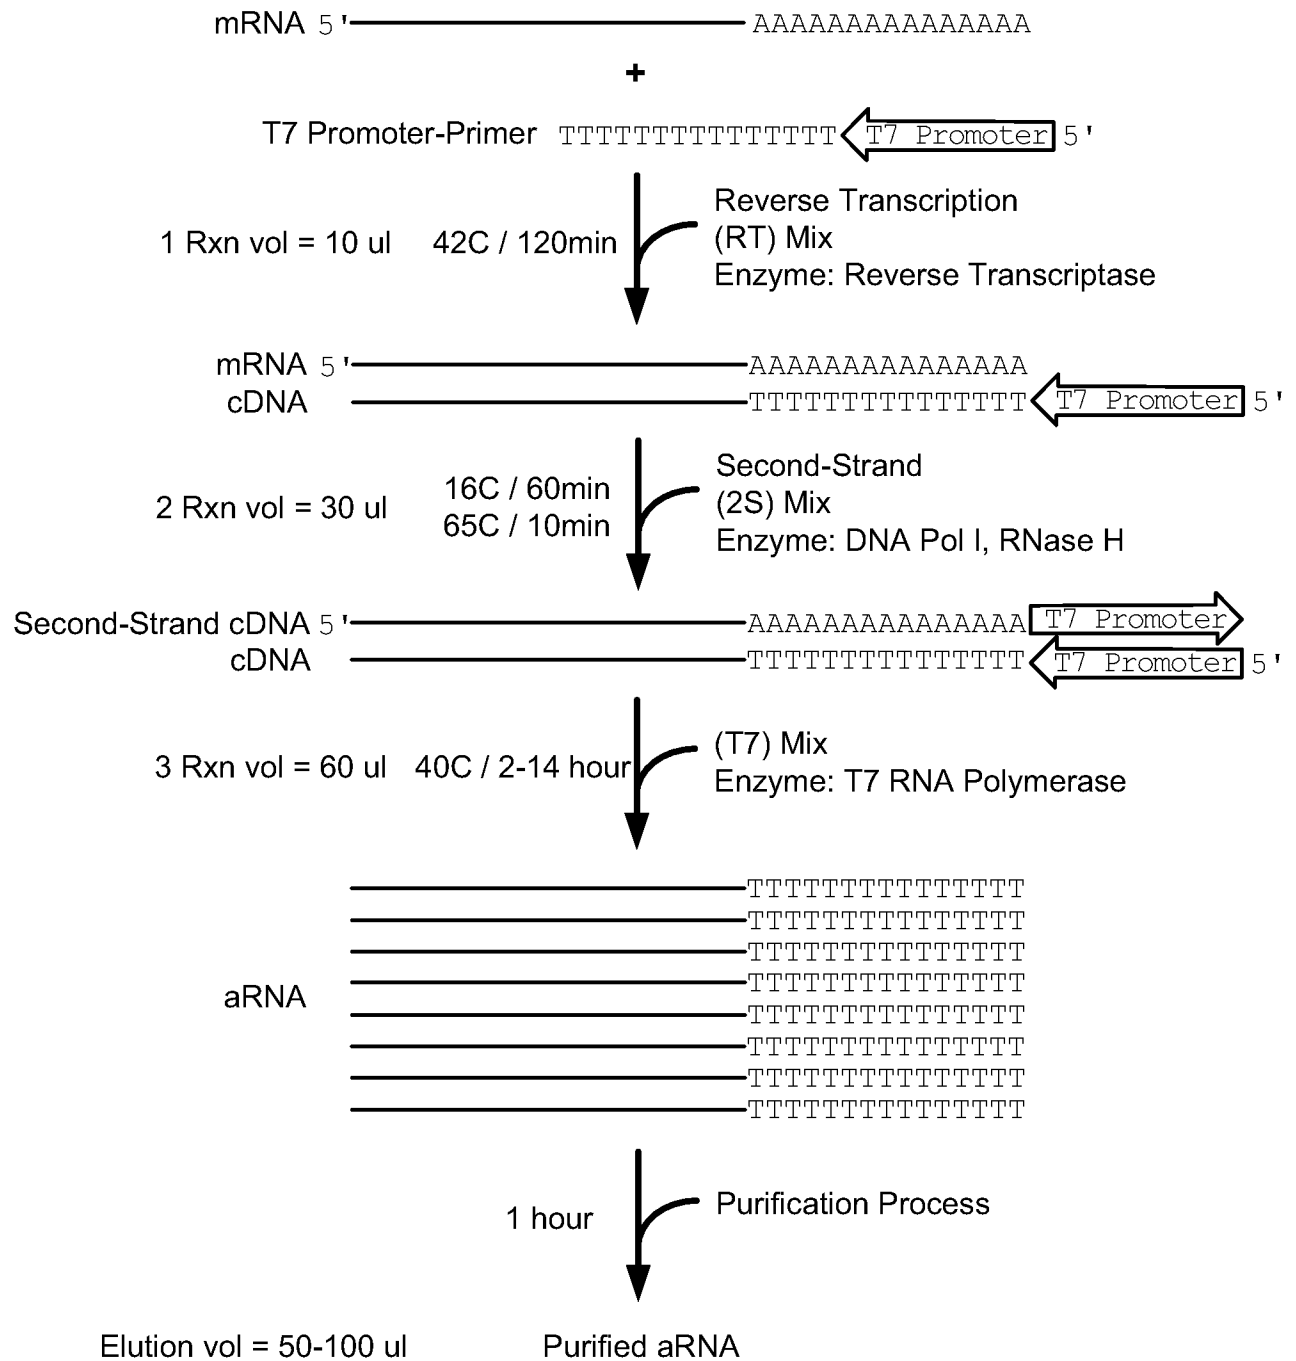


Figure 44

36/76

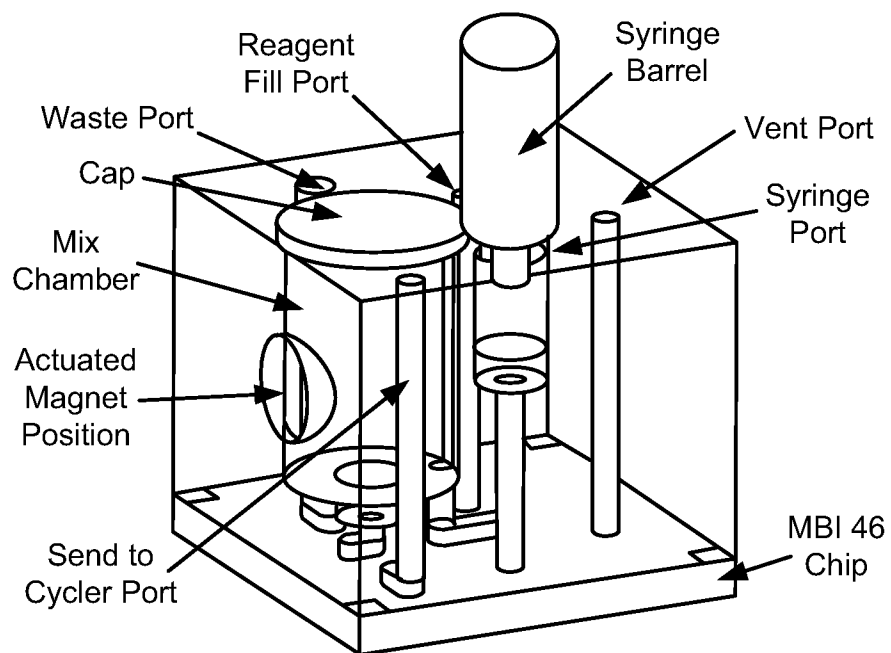


Figure 45

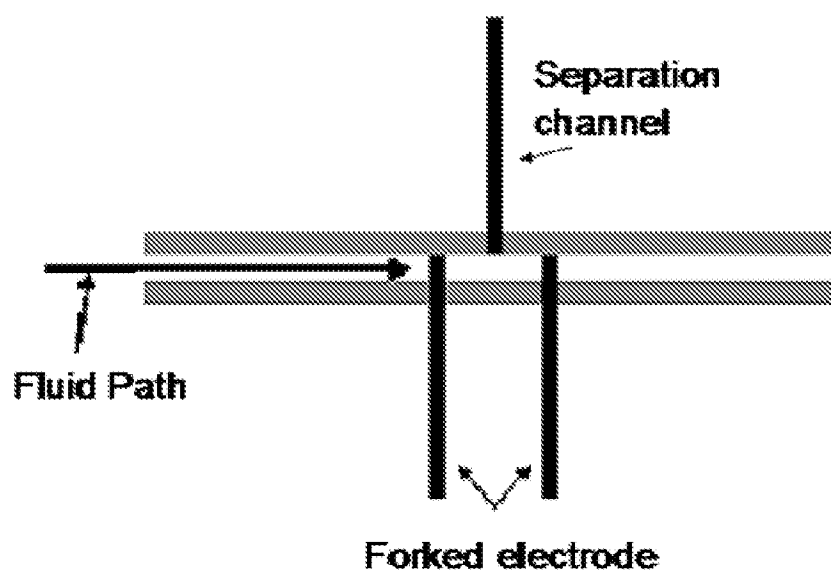


Figure 46

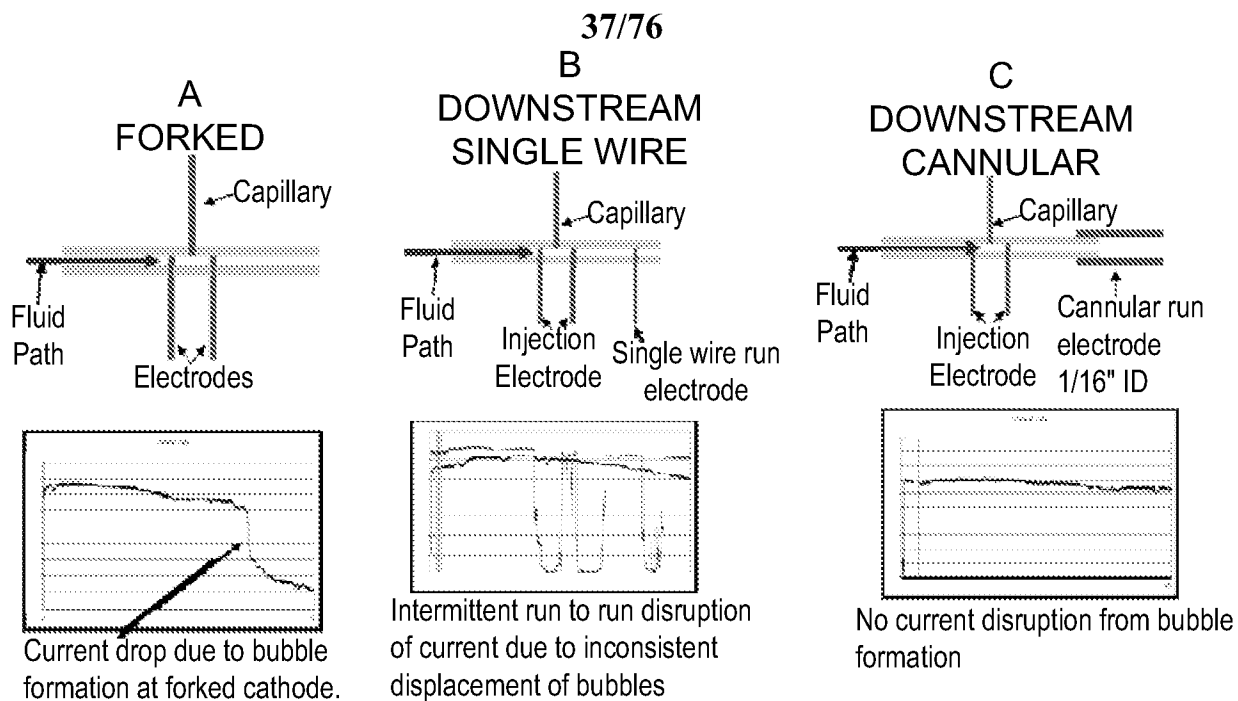


Figure 47

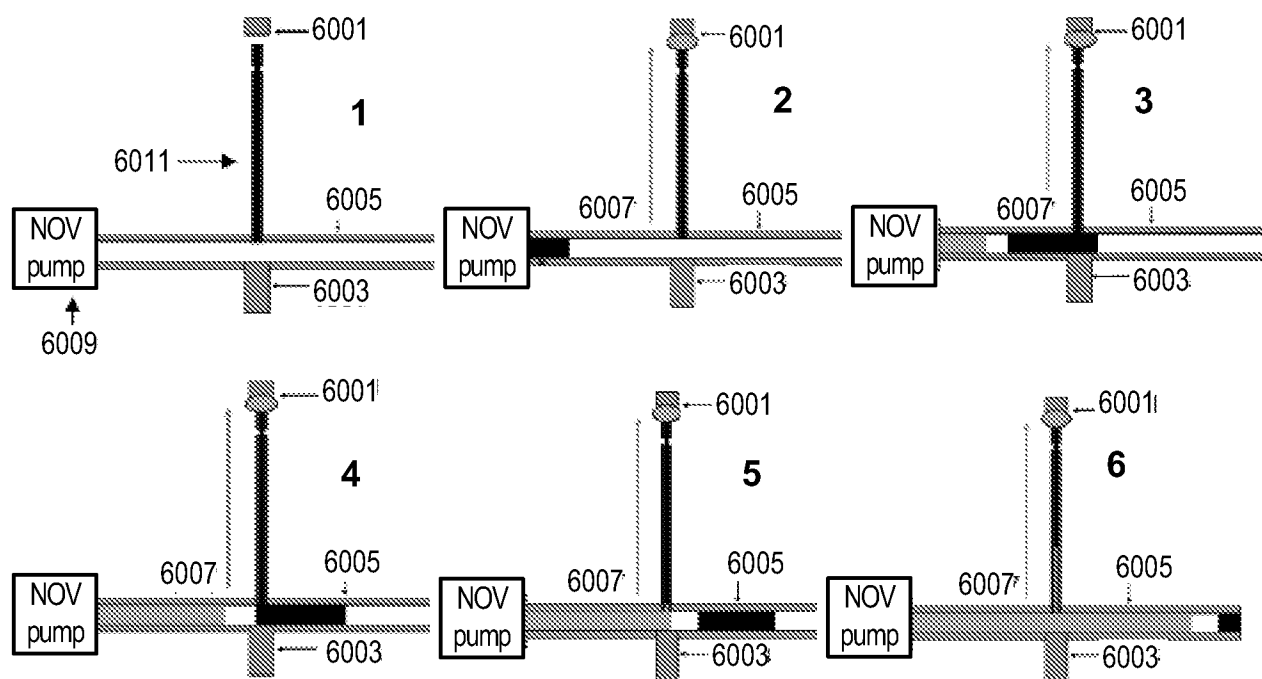


Figure 48

38/76

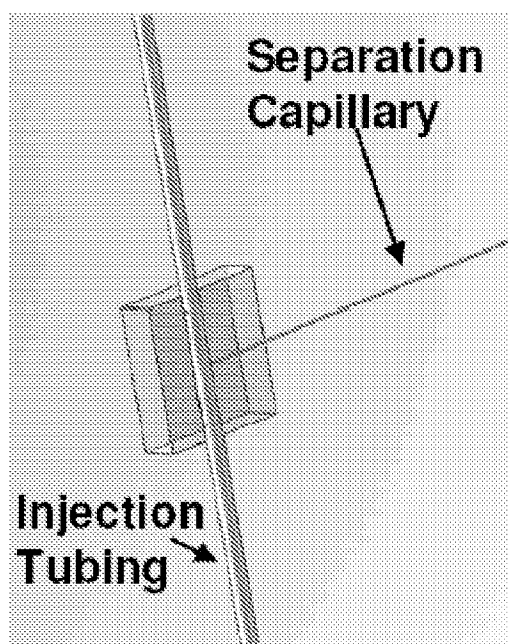


Figure 49

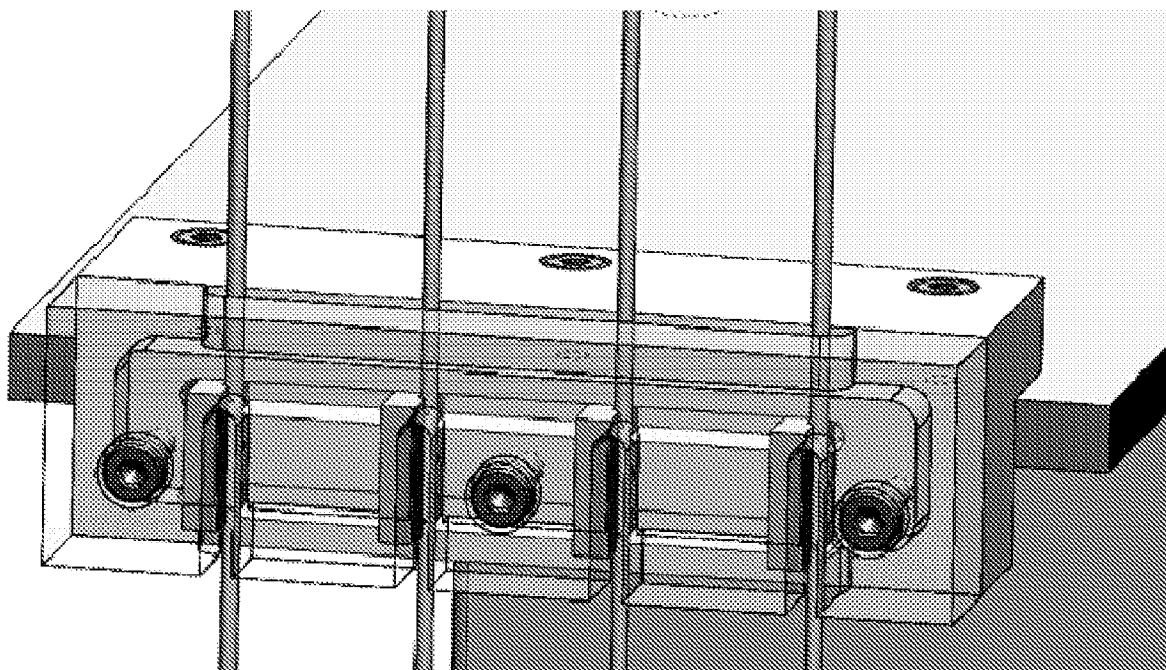


Figure 50

39/76

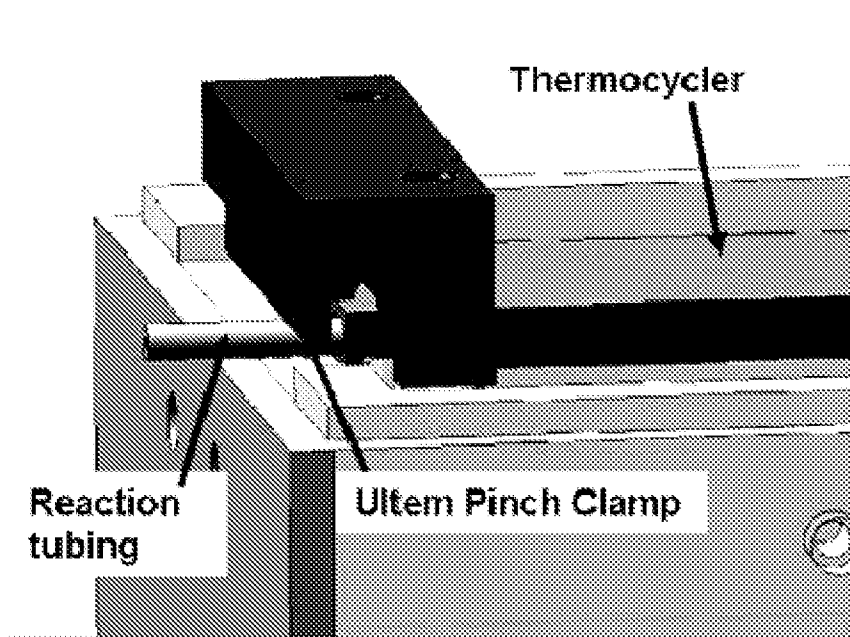


Figure 51



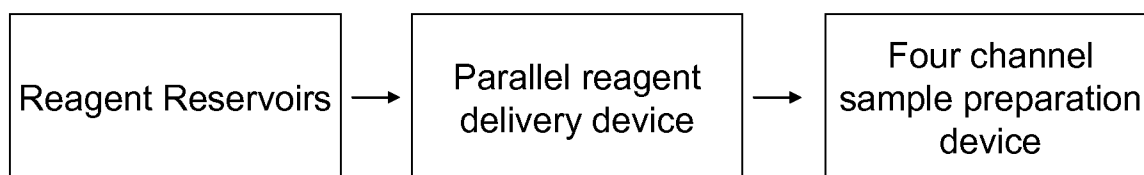


Figure 52

40/76

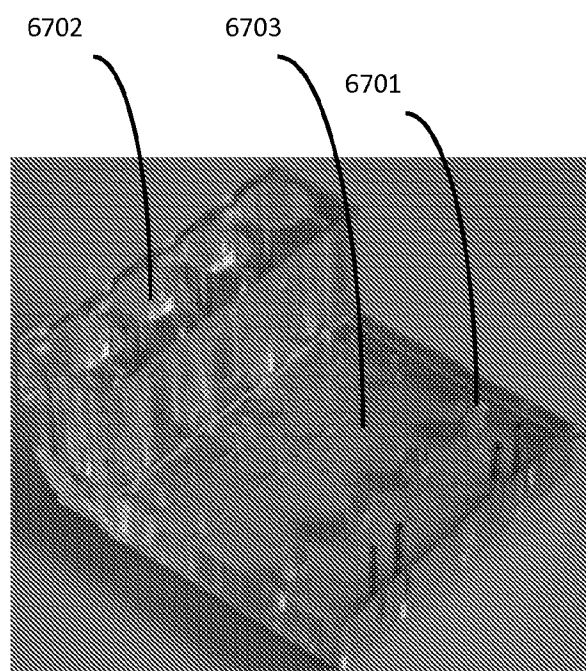

Sample Extraction

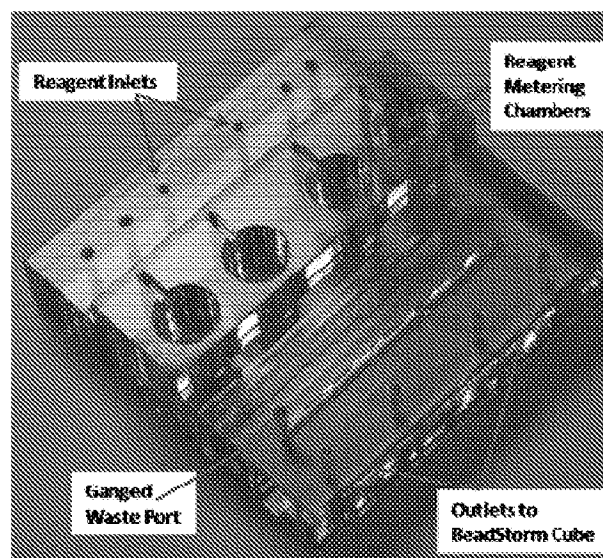

Reagent Distribution

Figure 53

41/76

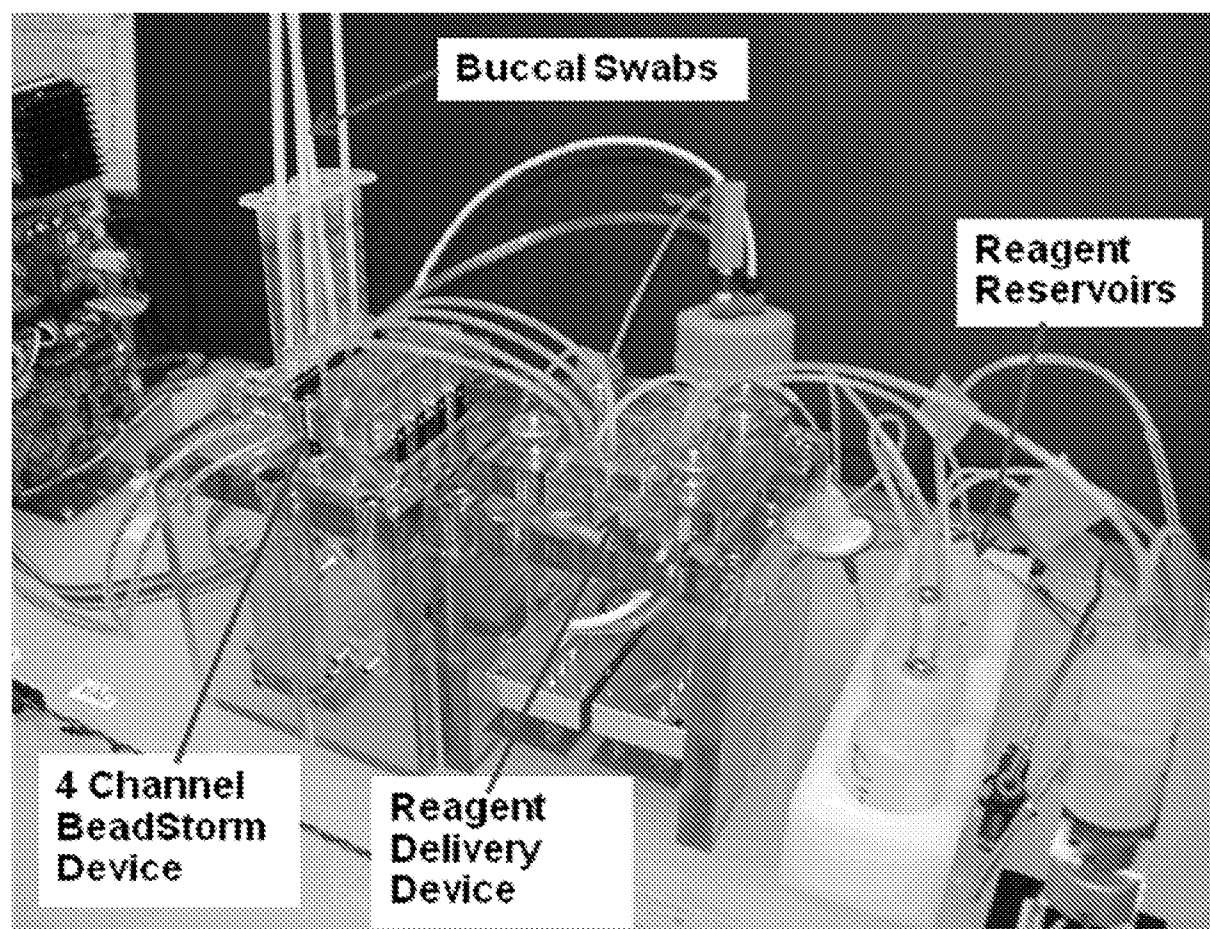


Figure 54

42/76

MBI069

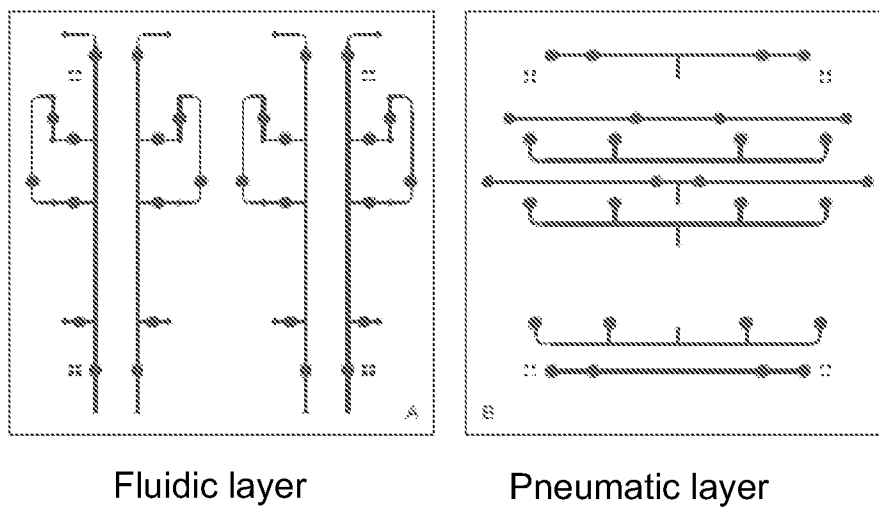


Figure 55

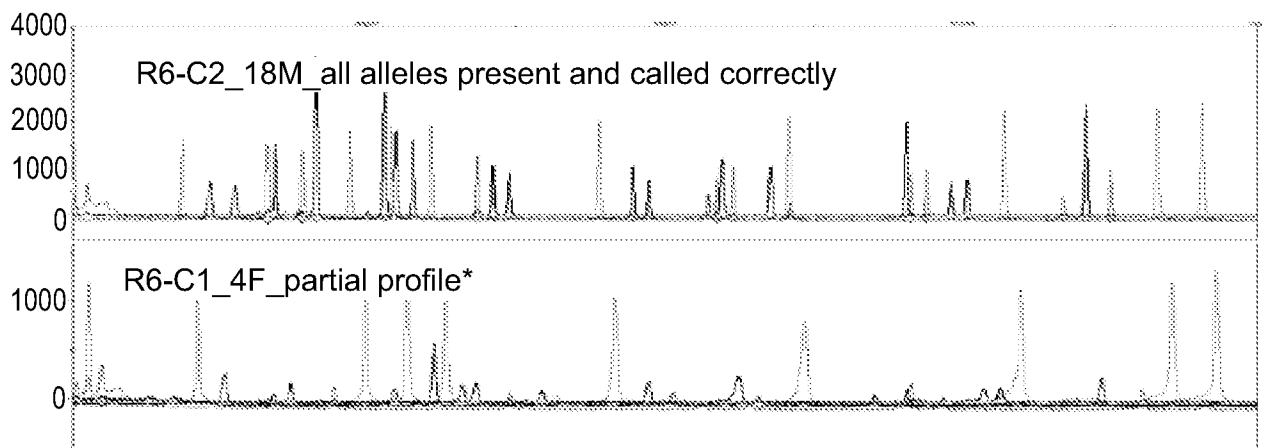


Figure 56

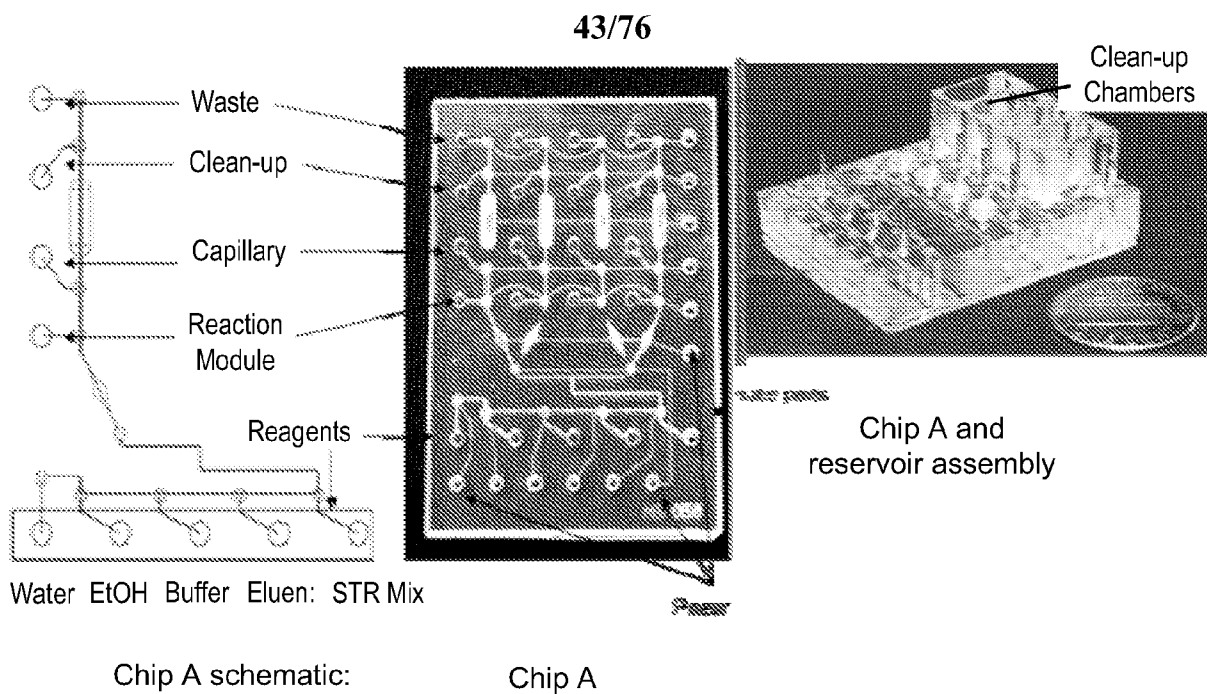


Figure 57

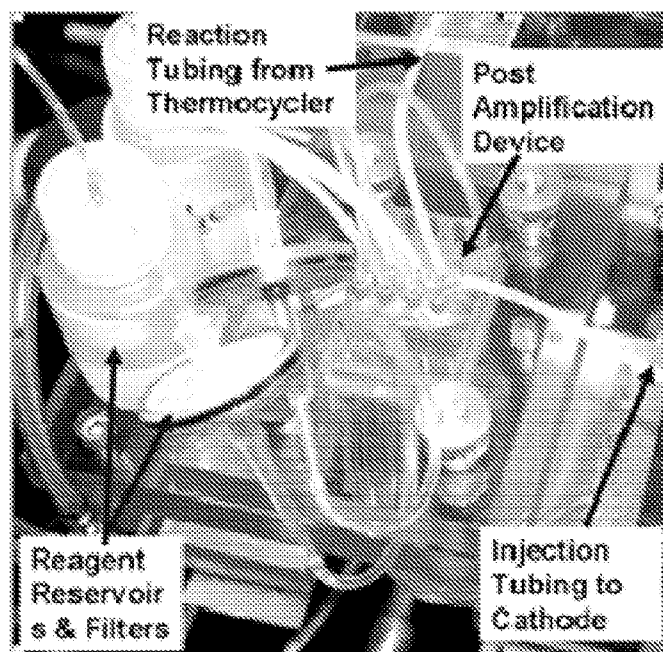


Figure 58

44/76

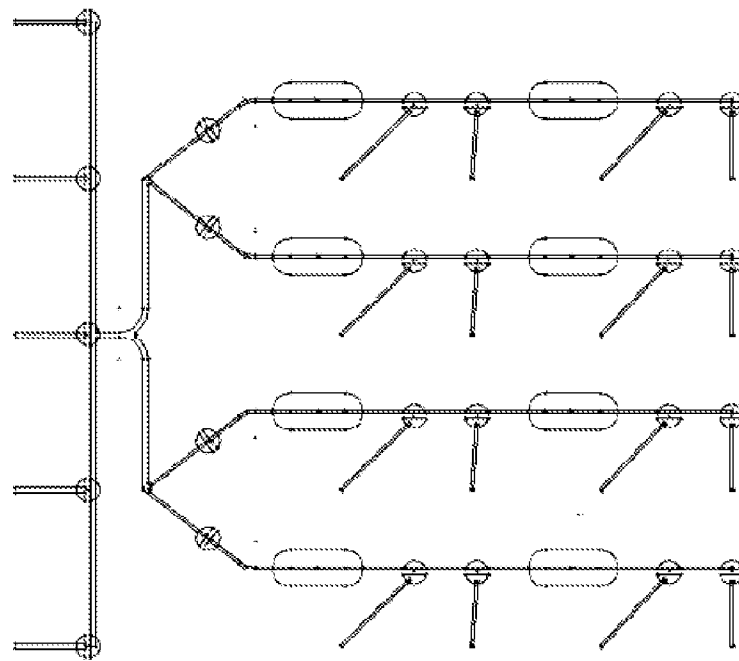


Figure 59

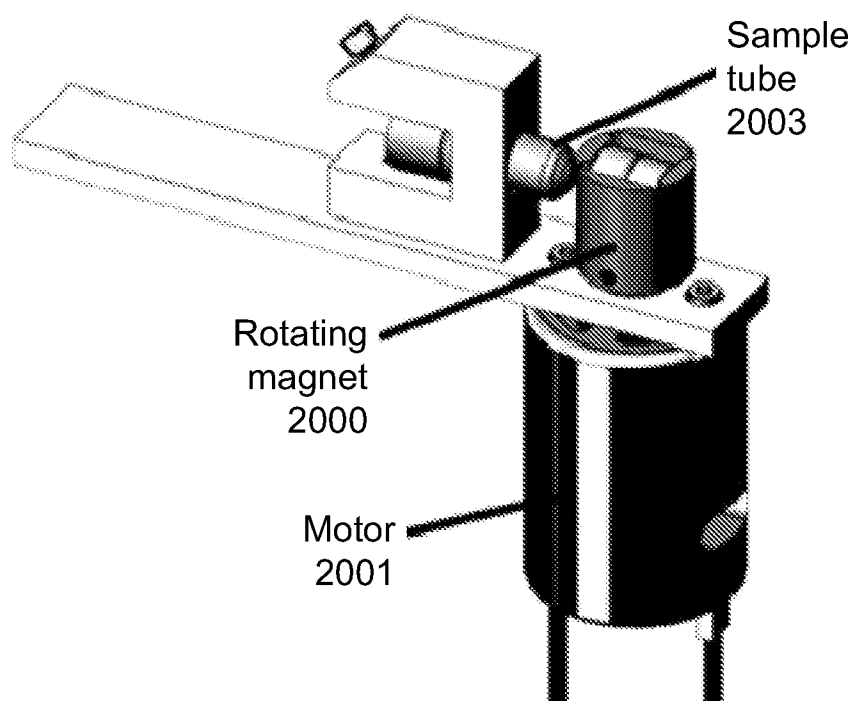


Figure 60

45/76

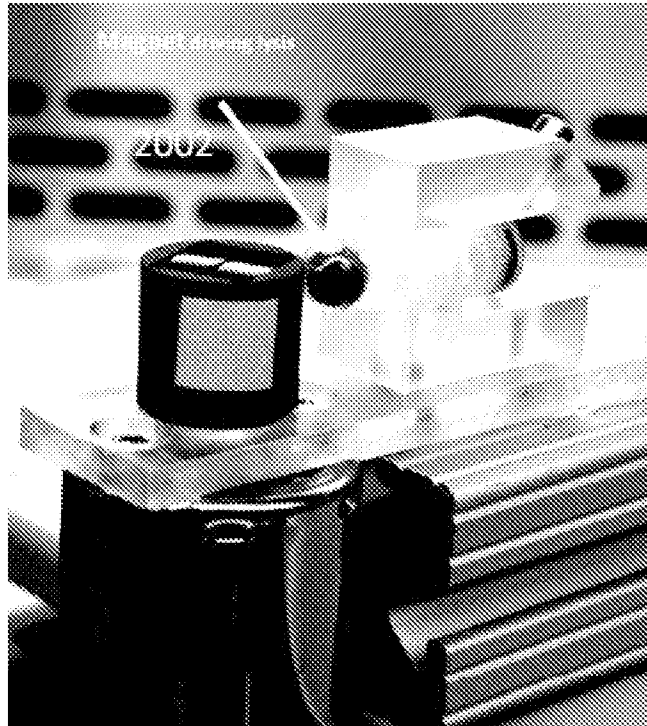


Figure 61

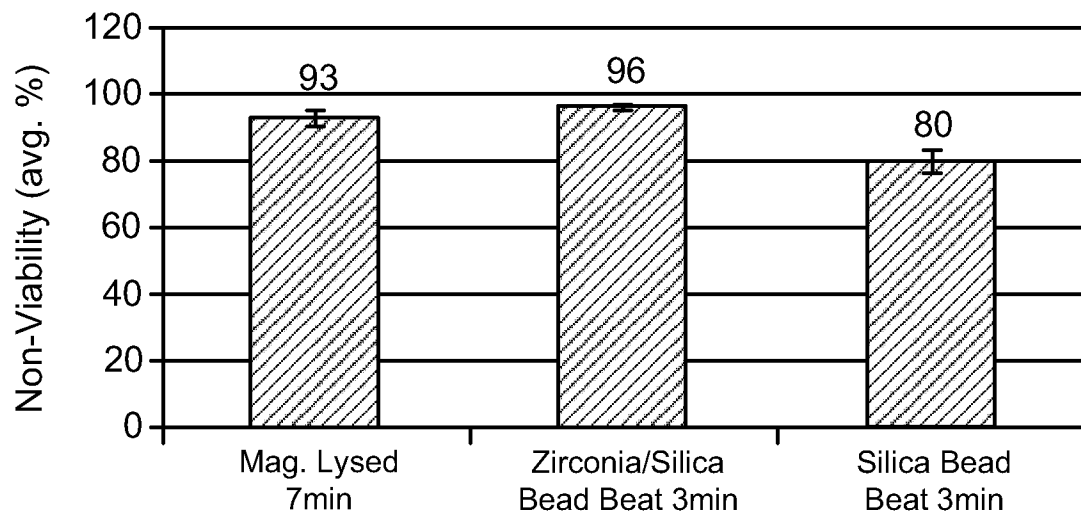


Figure 62

46/76

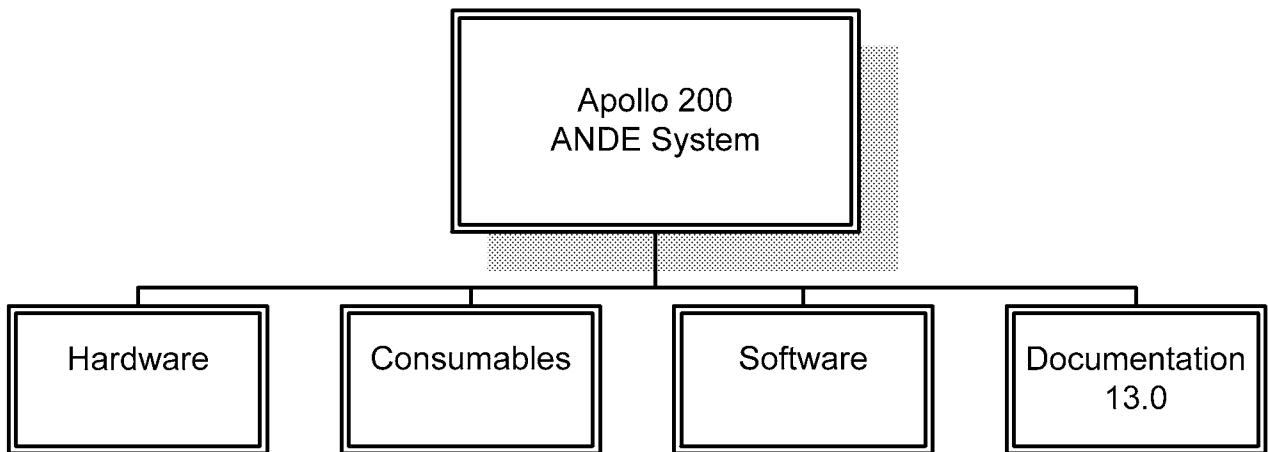


Figure 63

47/76

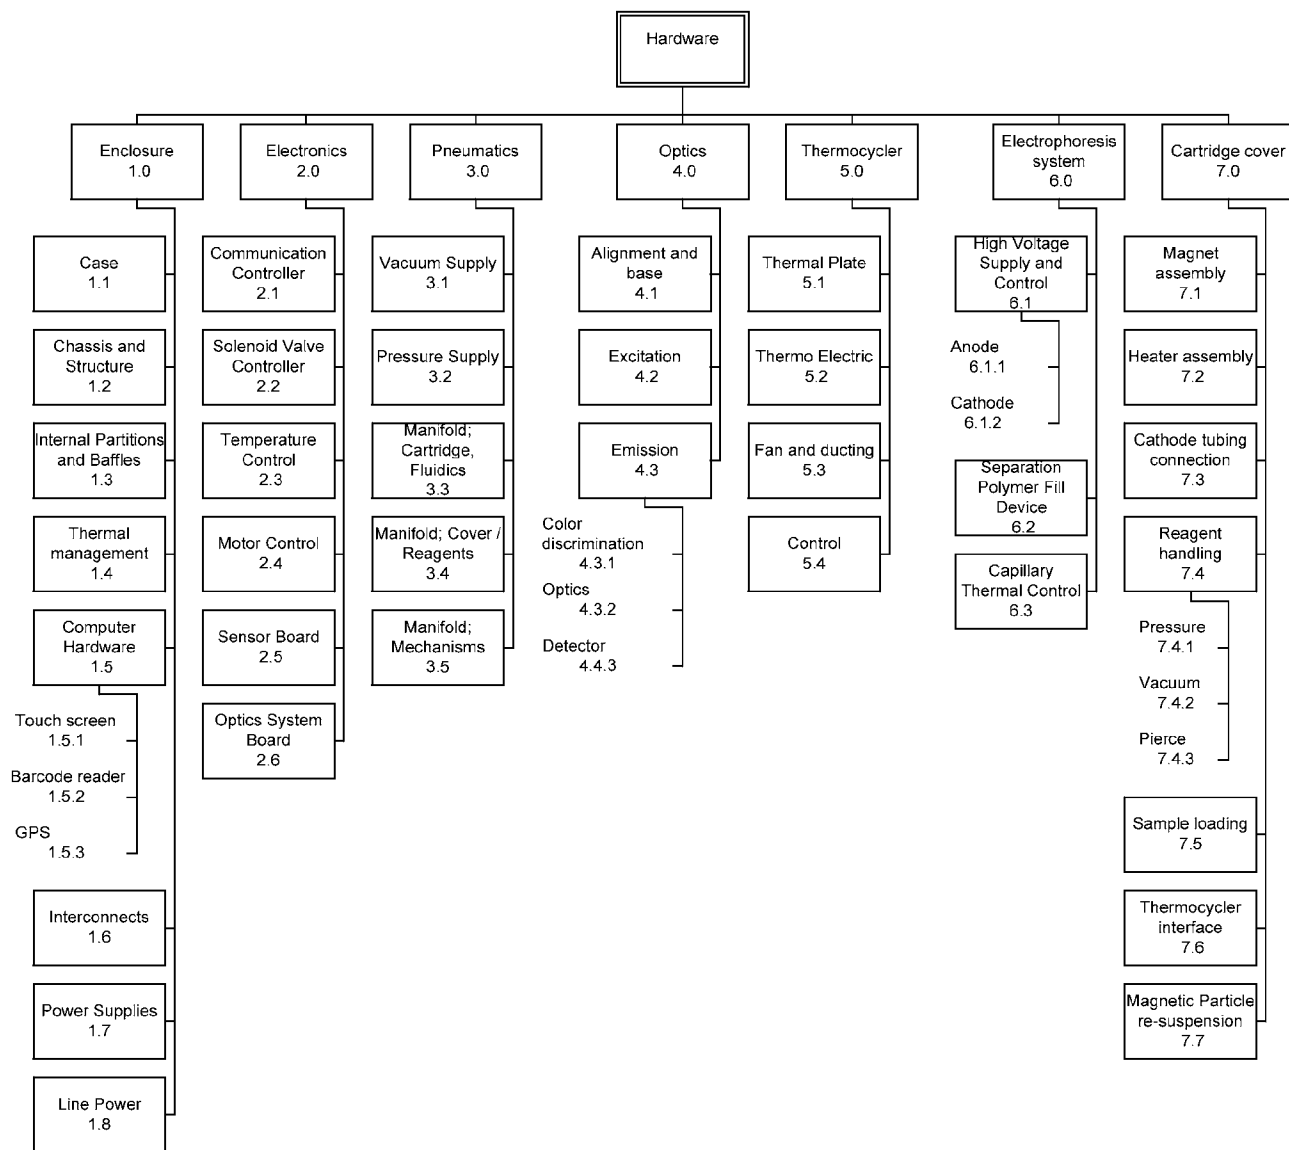


Figure 64

48/76

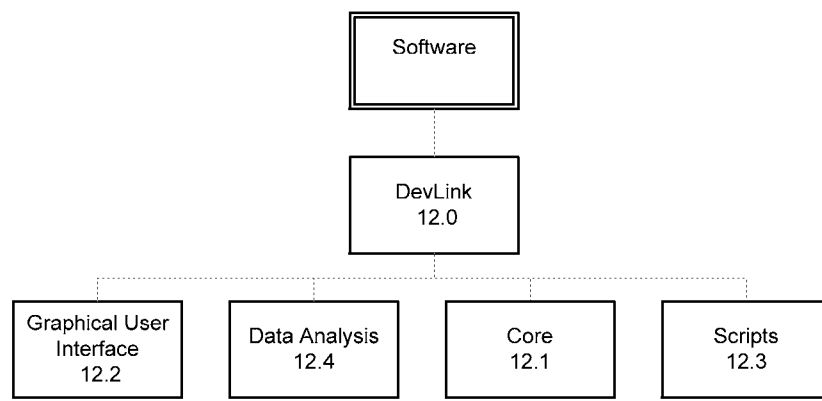


Figure 65

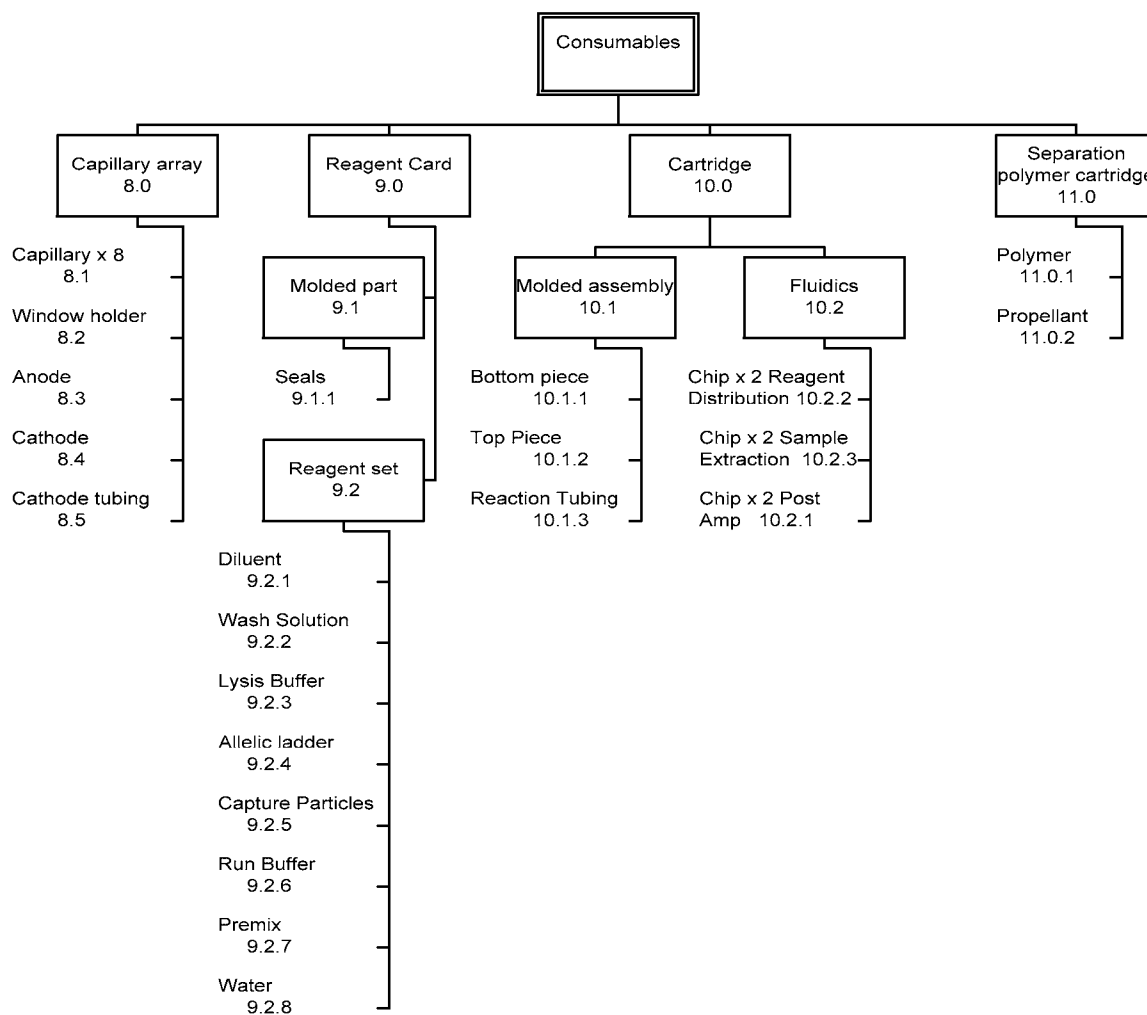


Figure 66

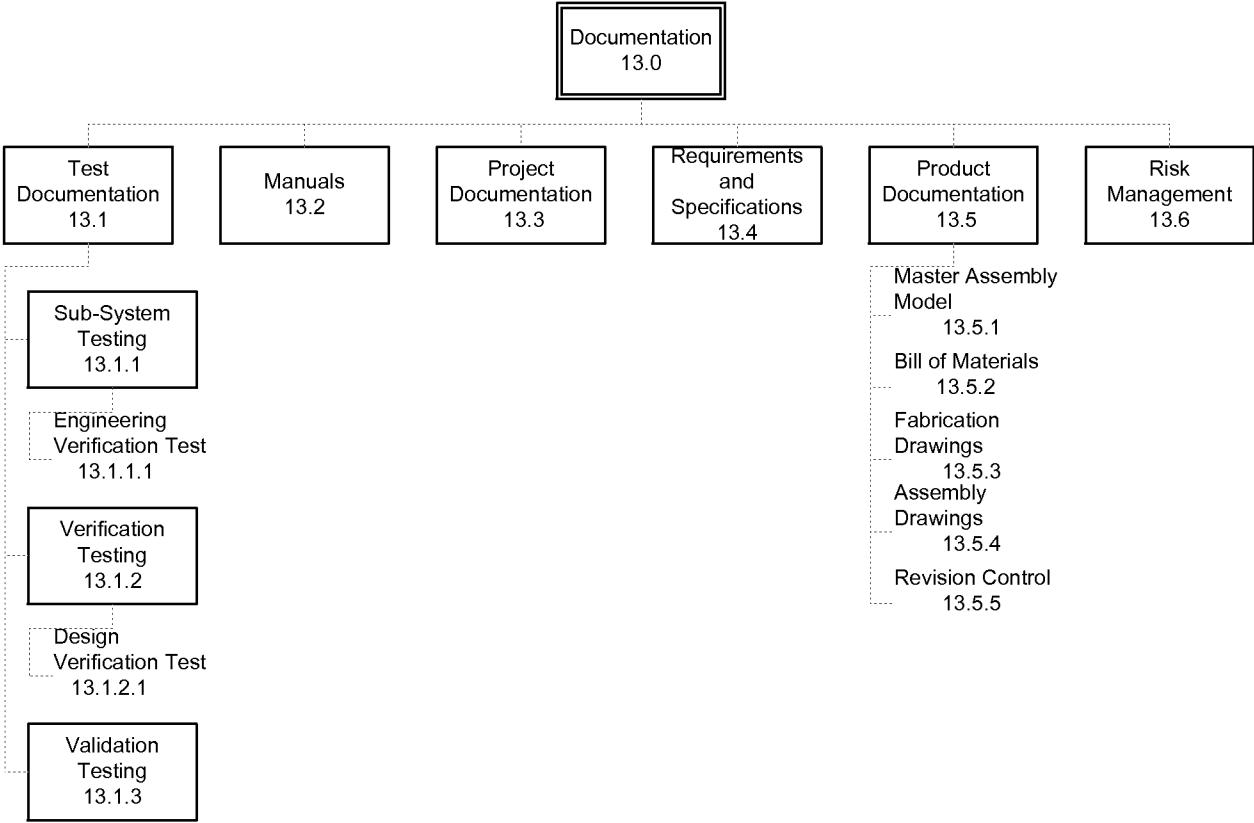


Figure 67

50/76

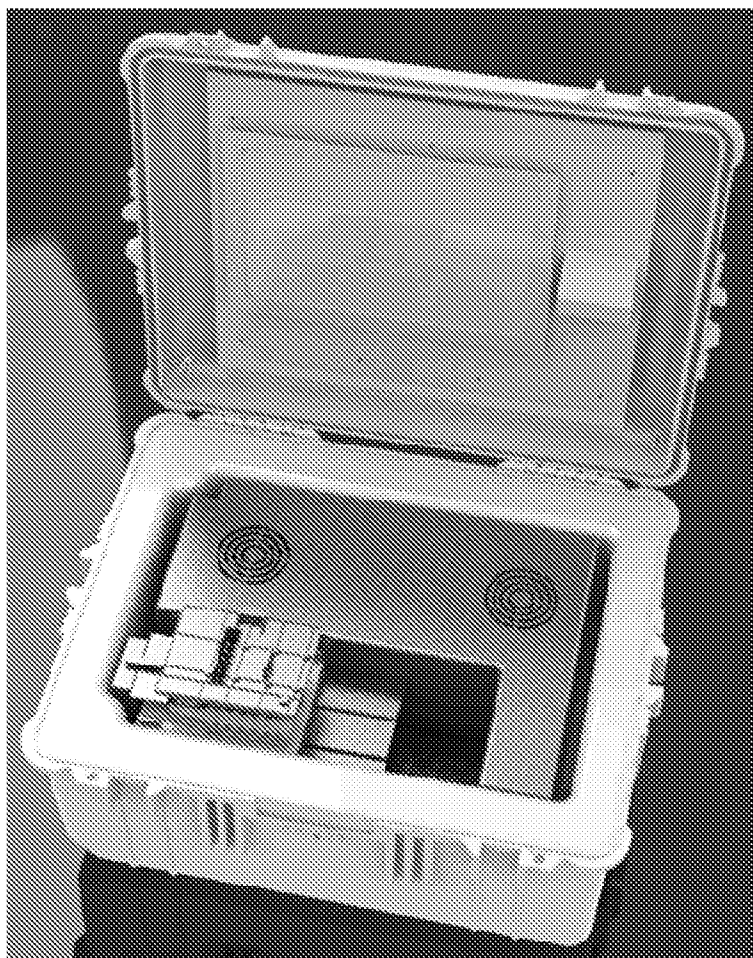


Figure 68

51/76

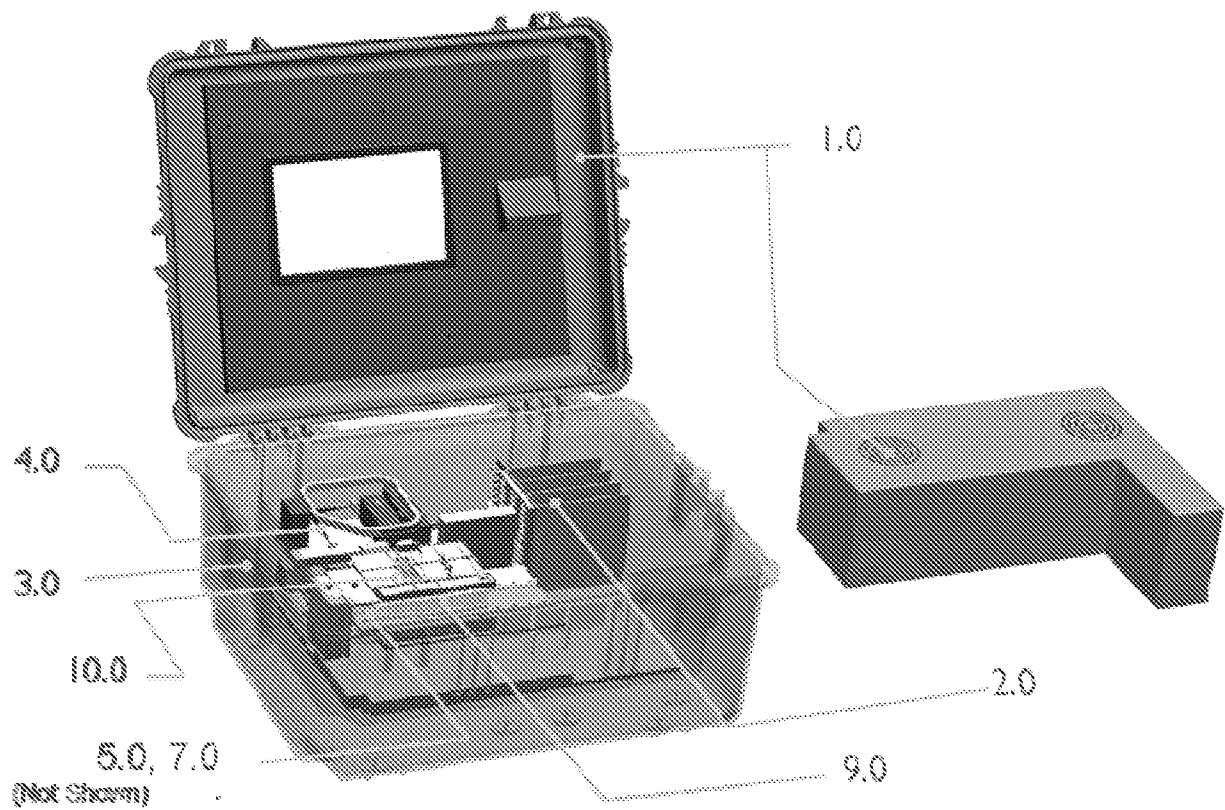


Figure 69

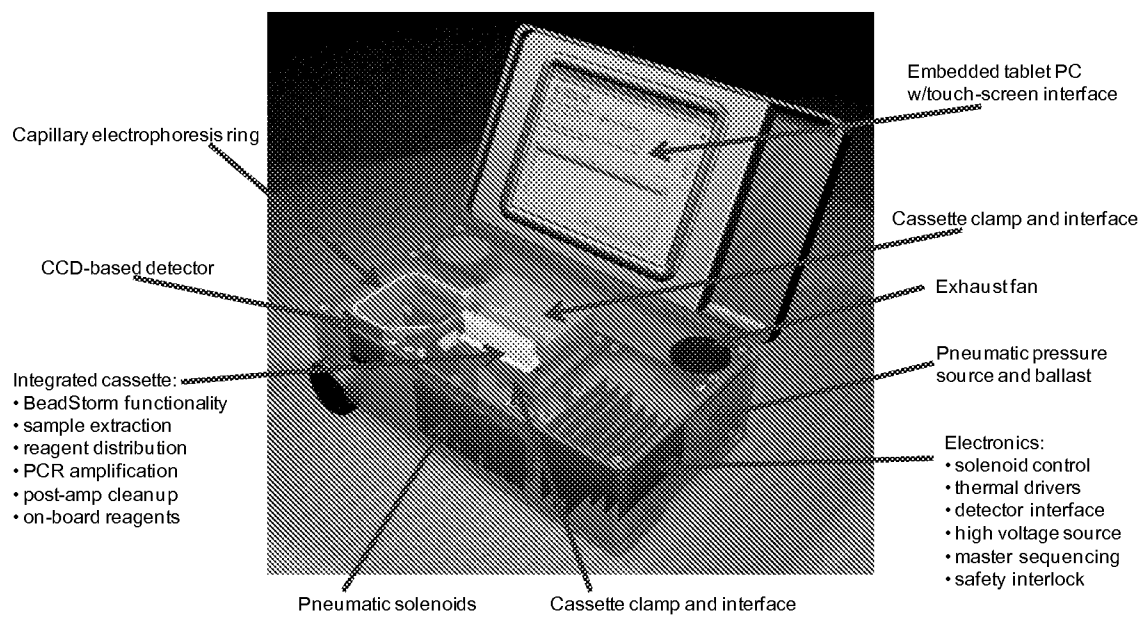


Figure 70

52/76

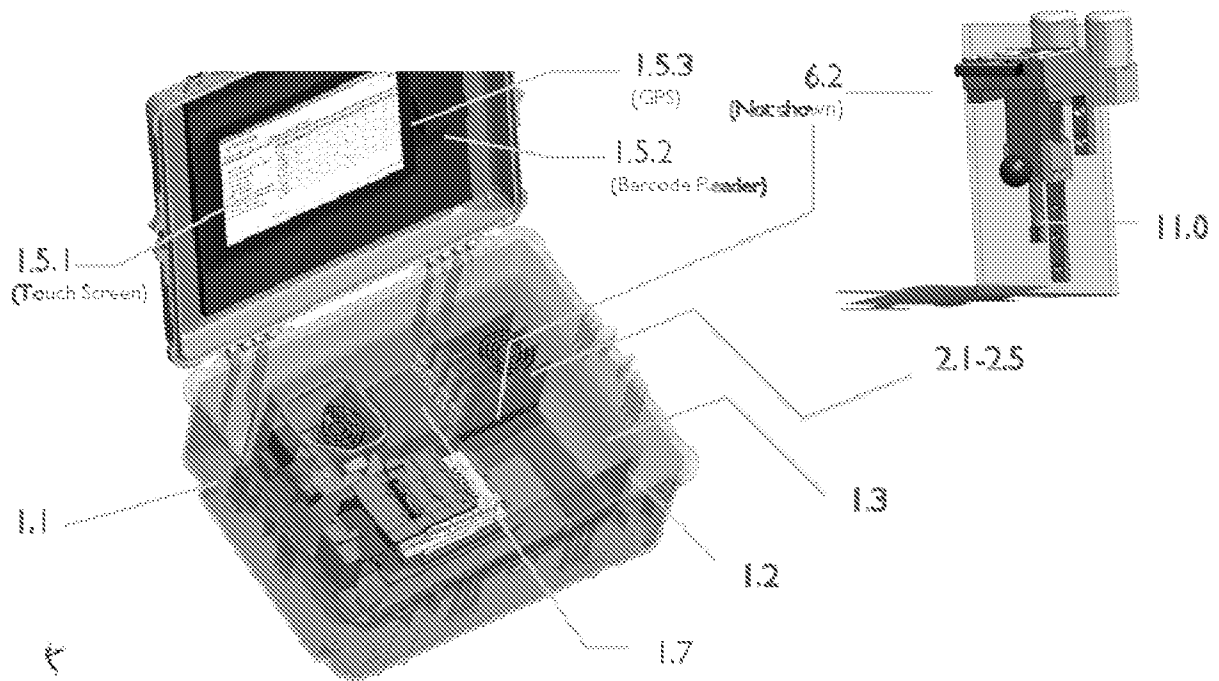


Figure 71

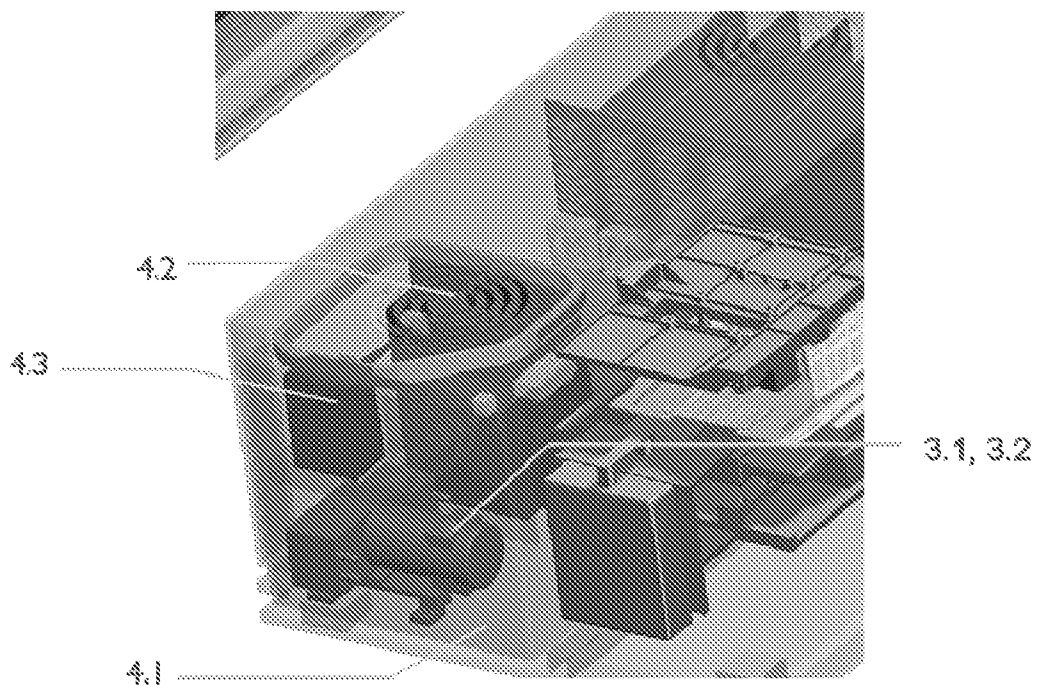


Figure 72

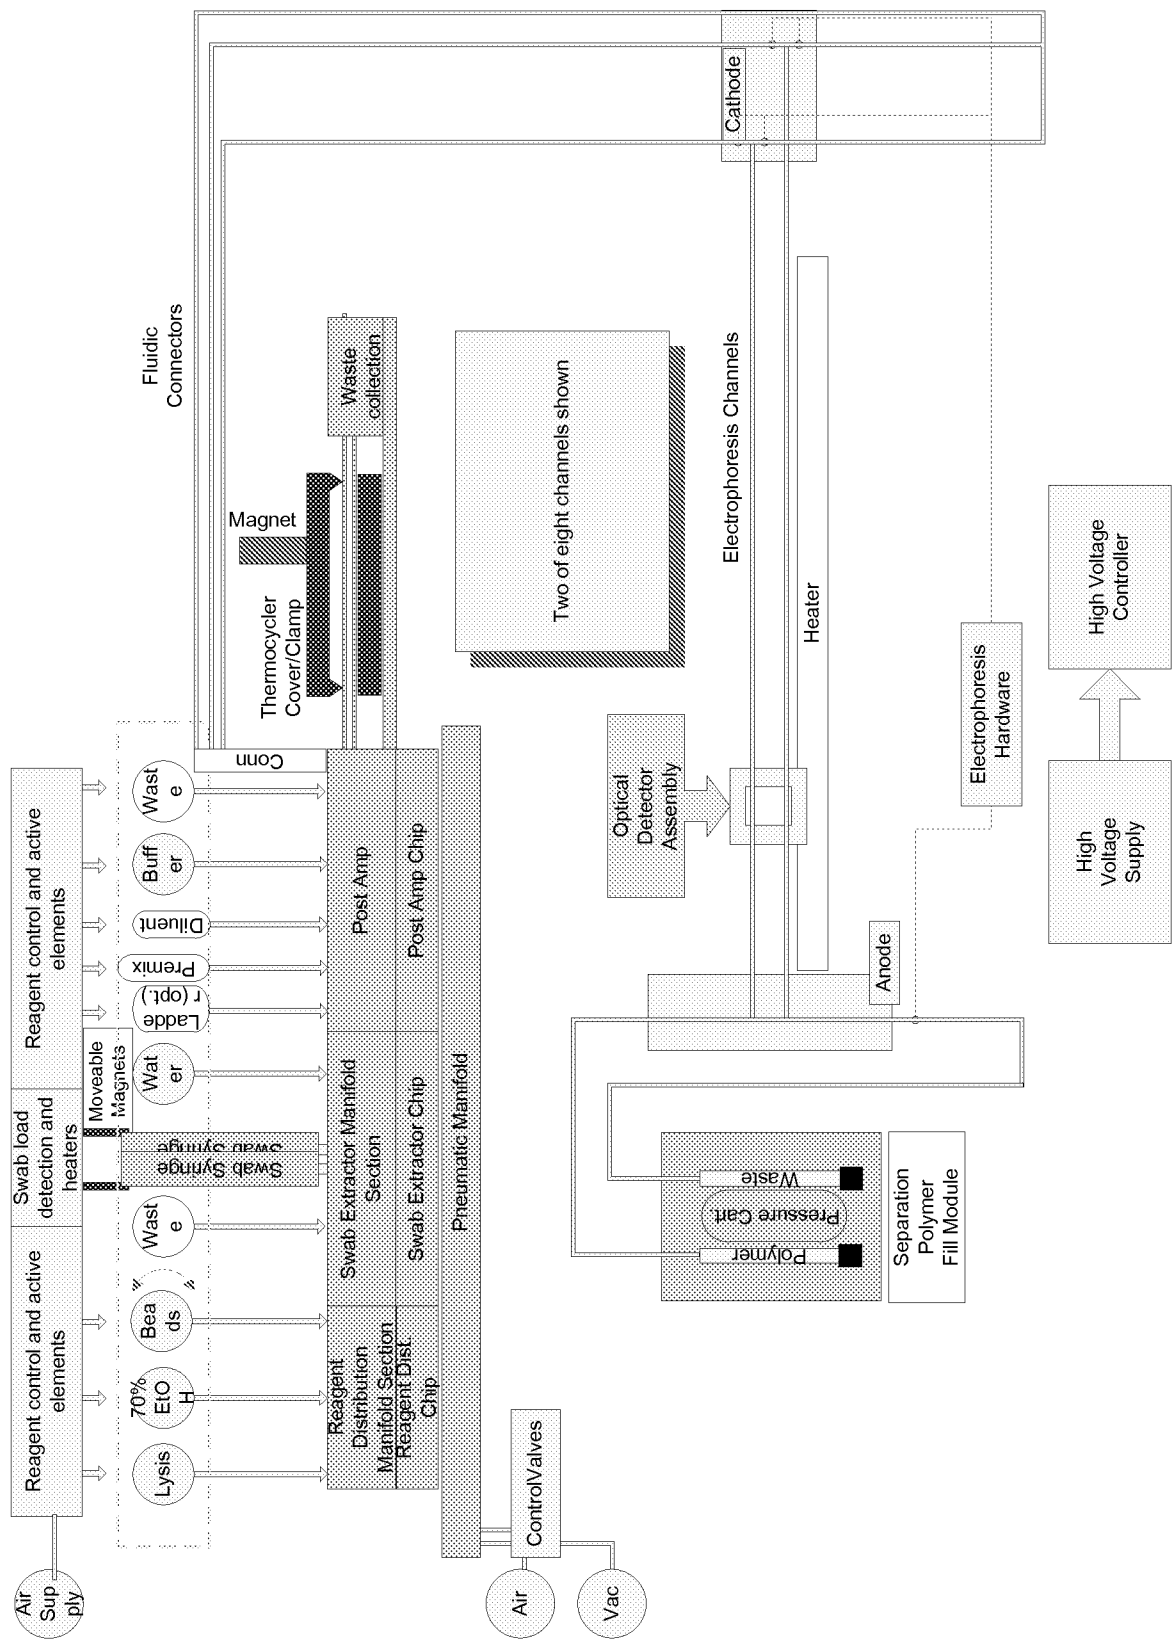


Figure 73

54/76

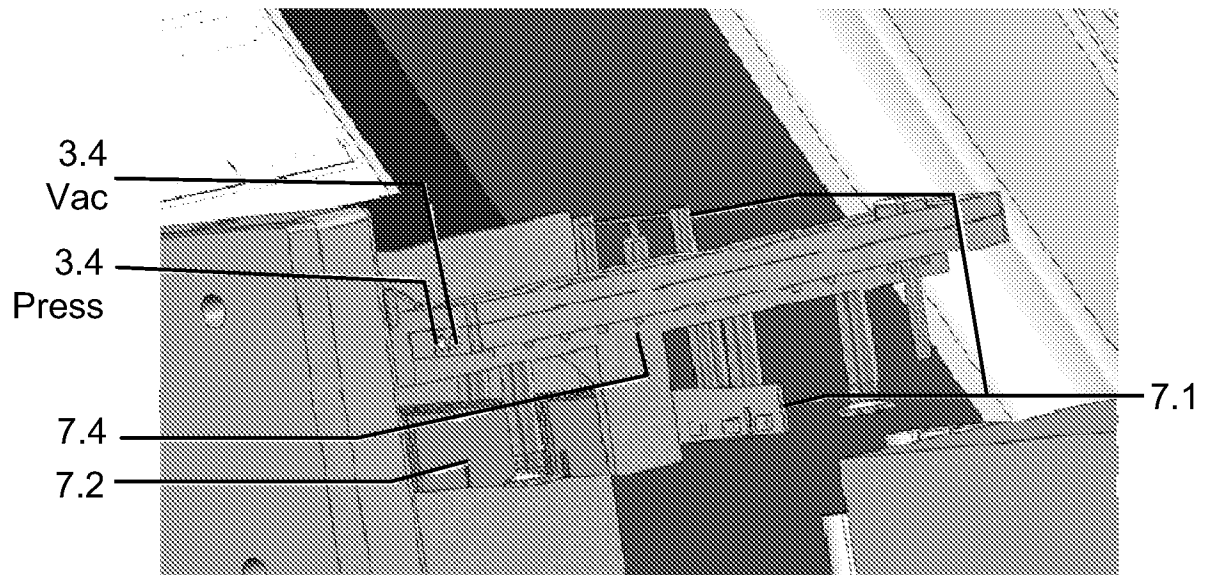


Figure 74

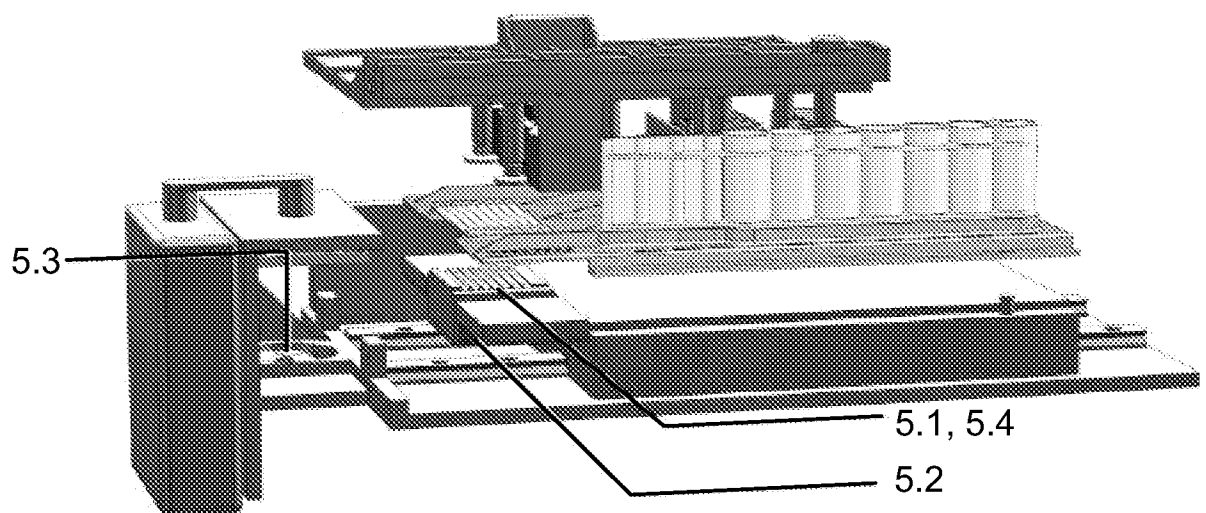


Figure 75

55/76

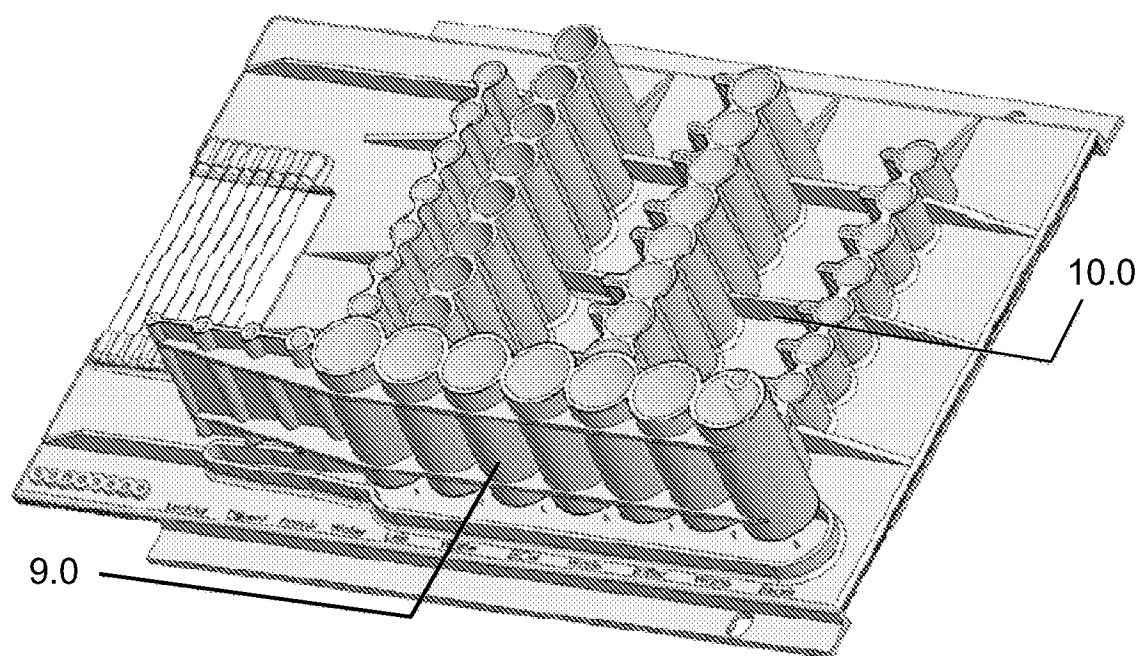


Figure 76

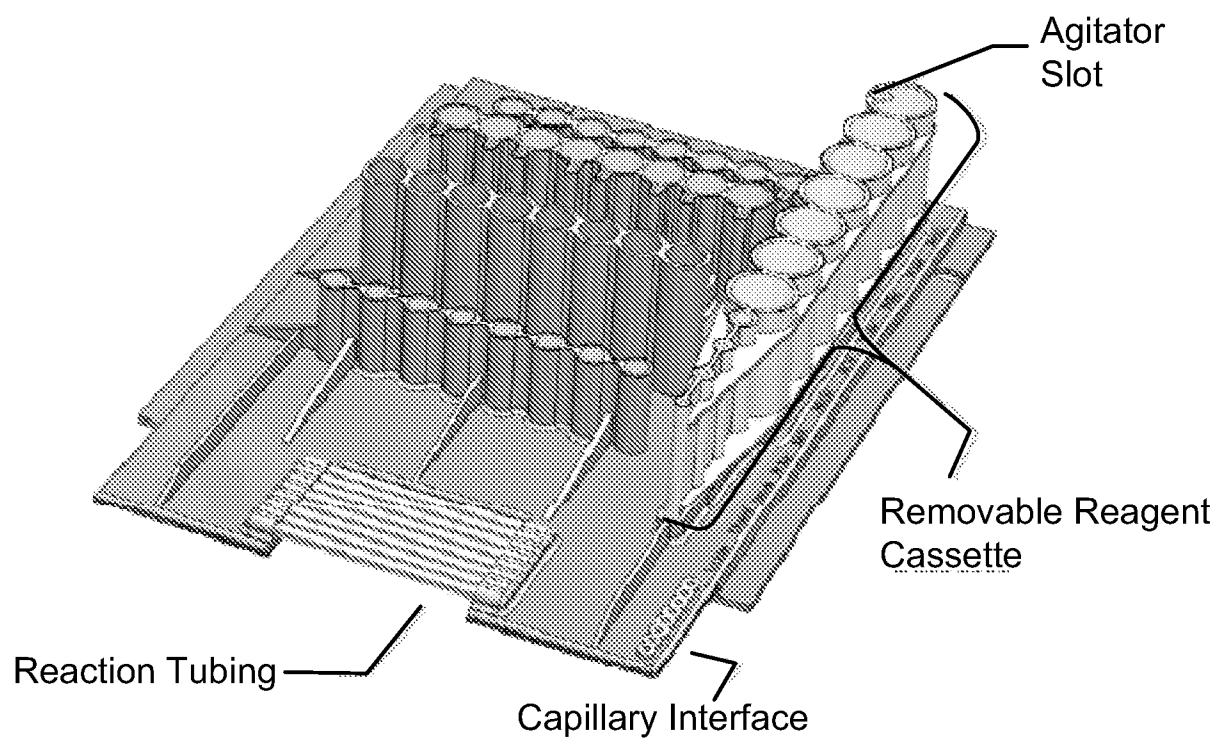


Figure 77

56/76

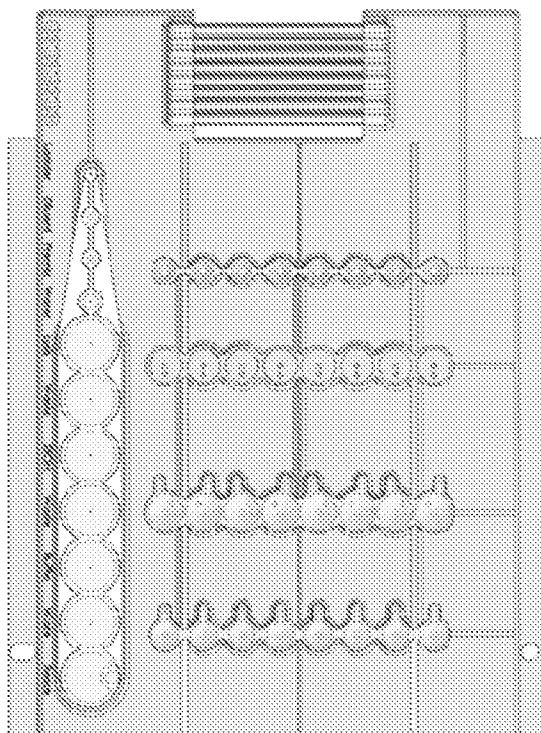


Figure 78

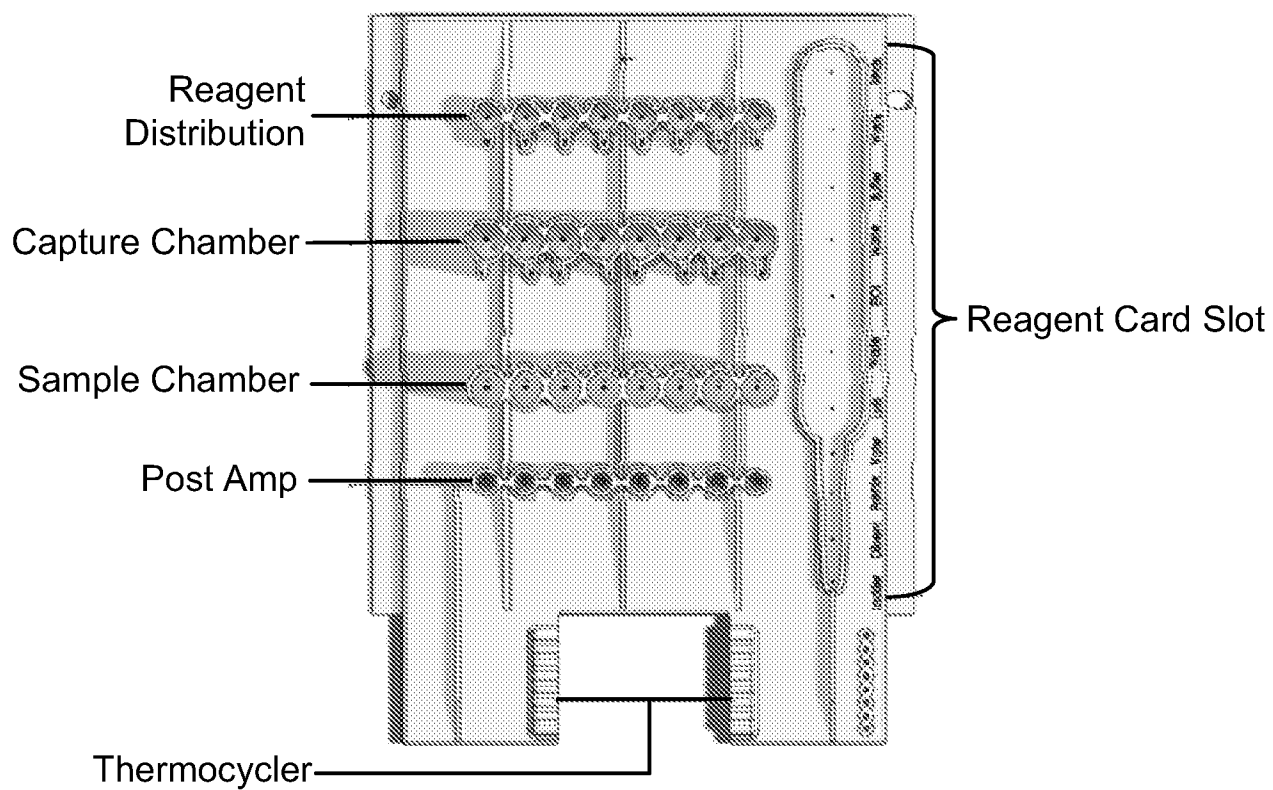


Figure 79

57/76

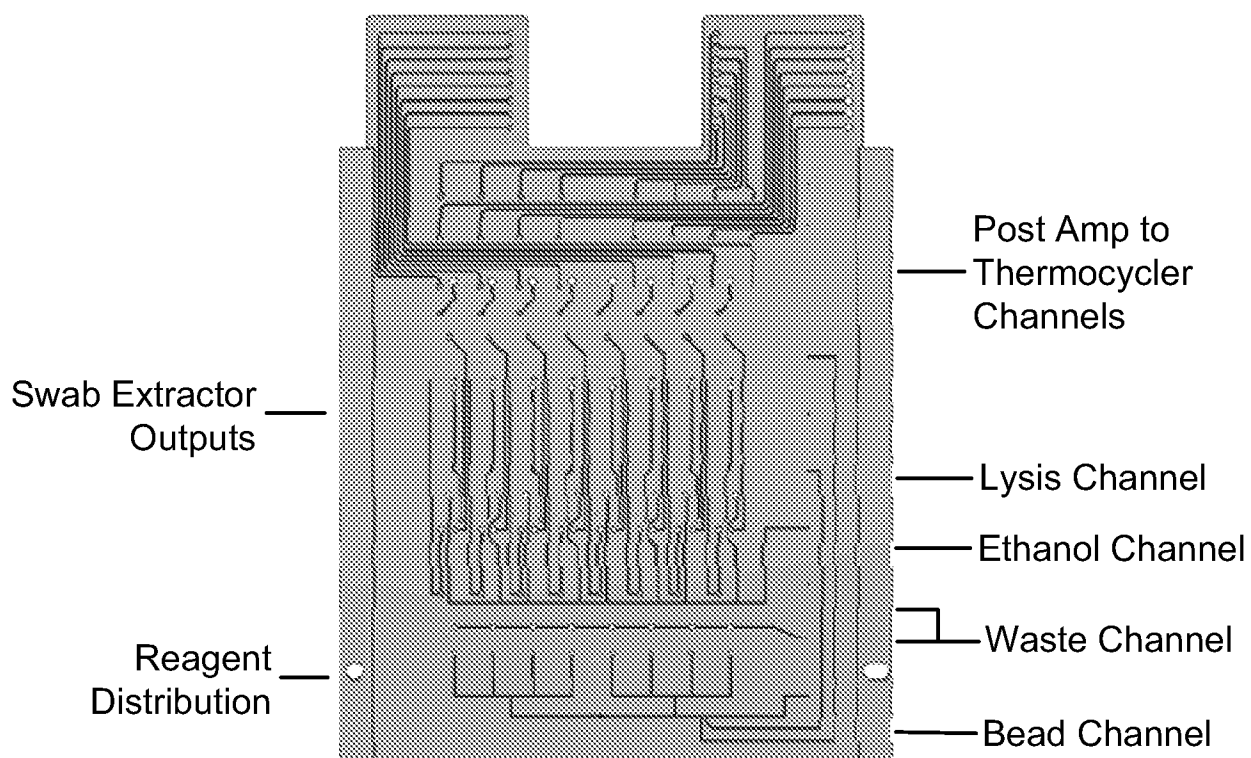


Figure 80

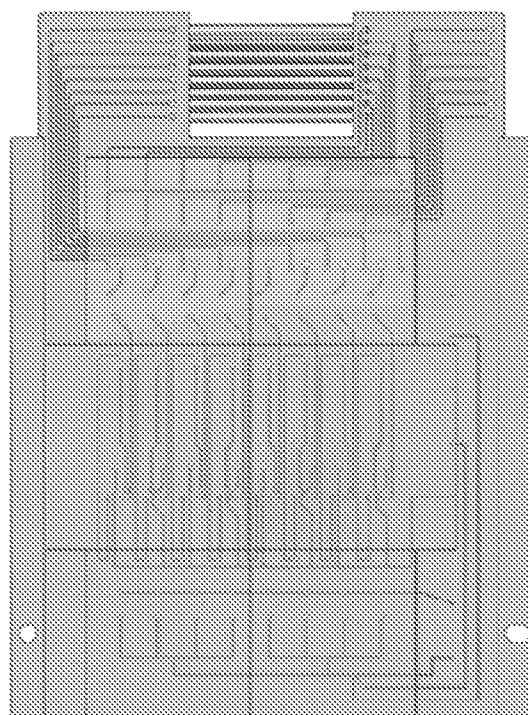


Figure 81

58/76

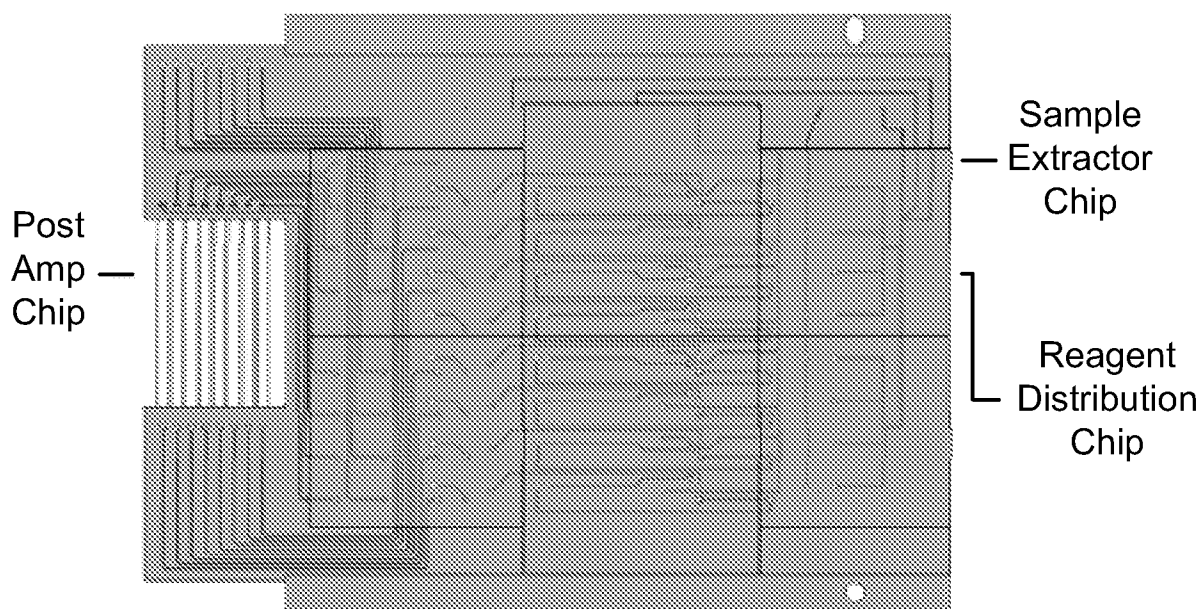


Figure 82

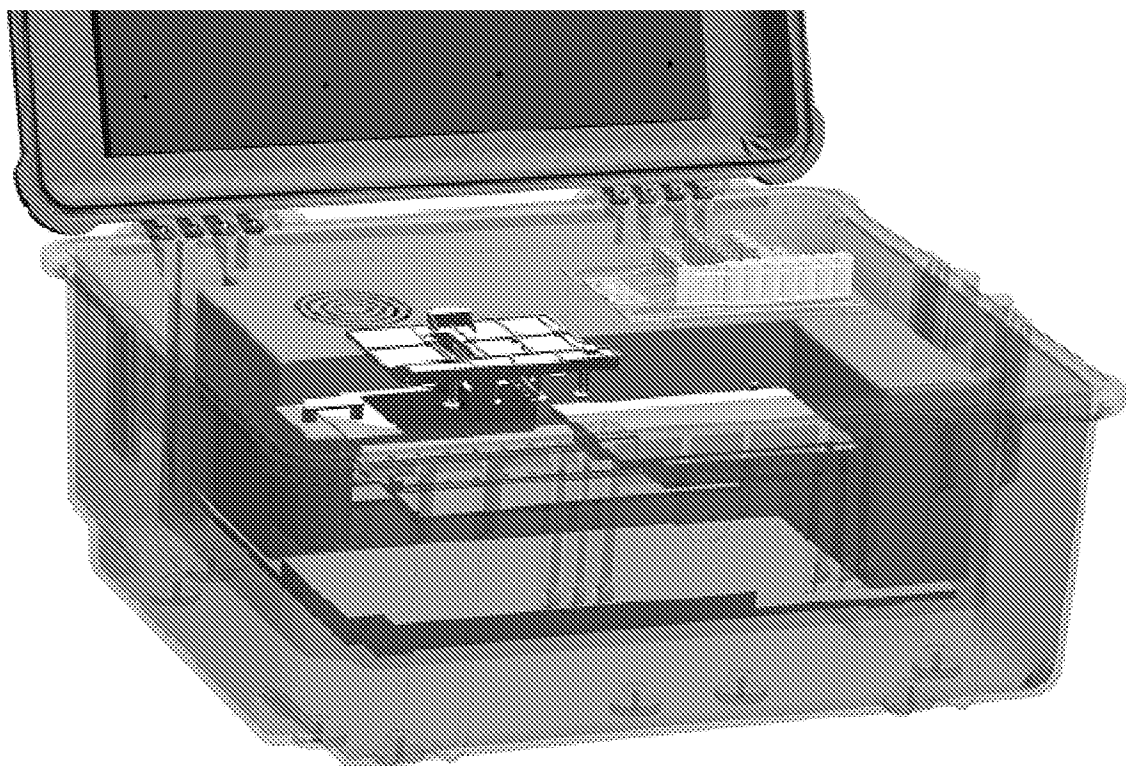


Figure 83

59/76

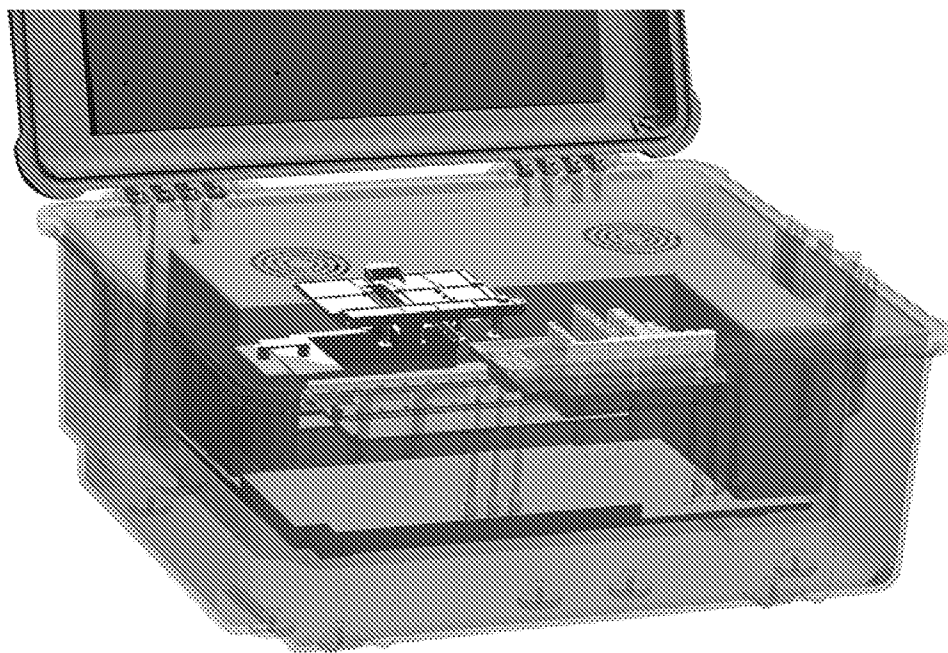


Figure 84

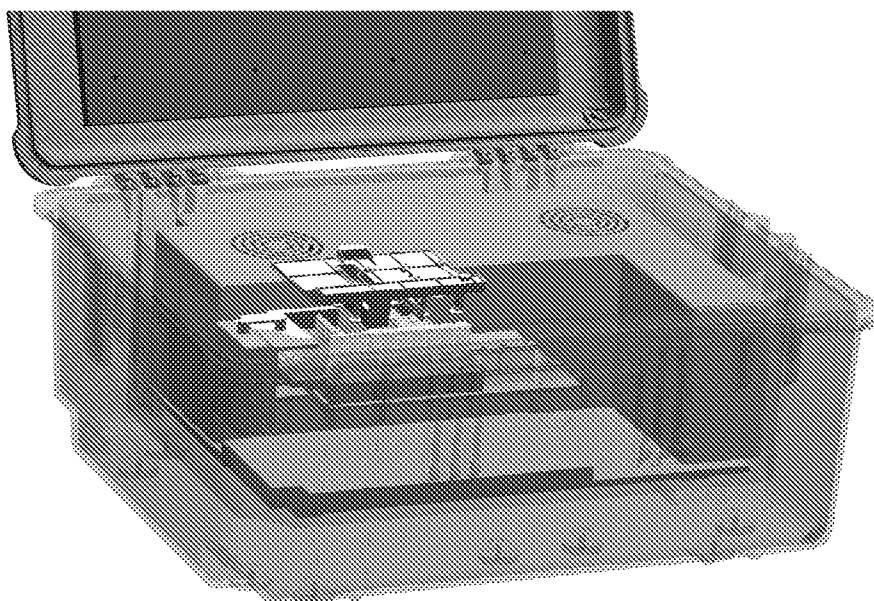


Figure 85

60/76

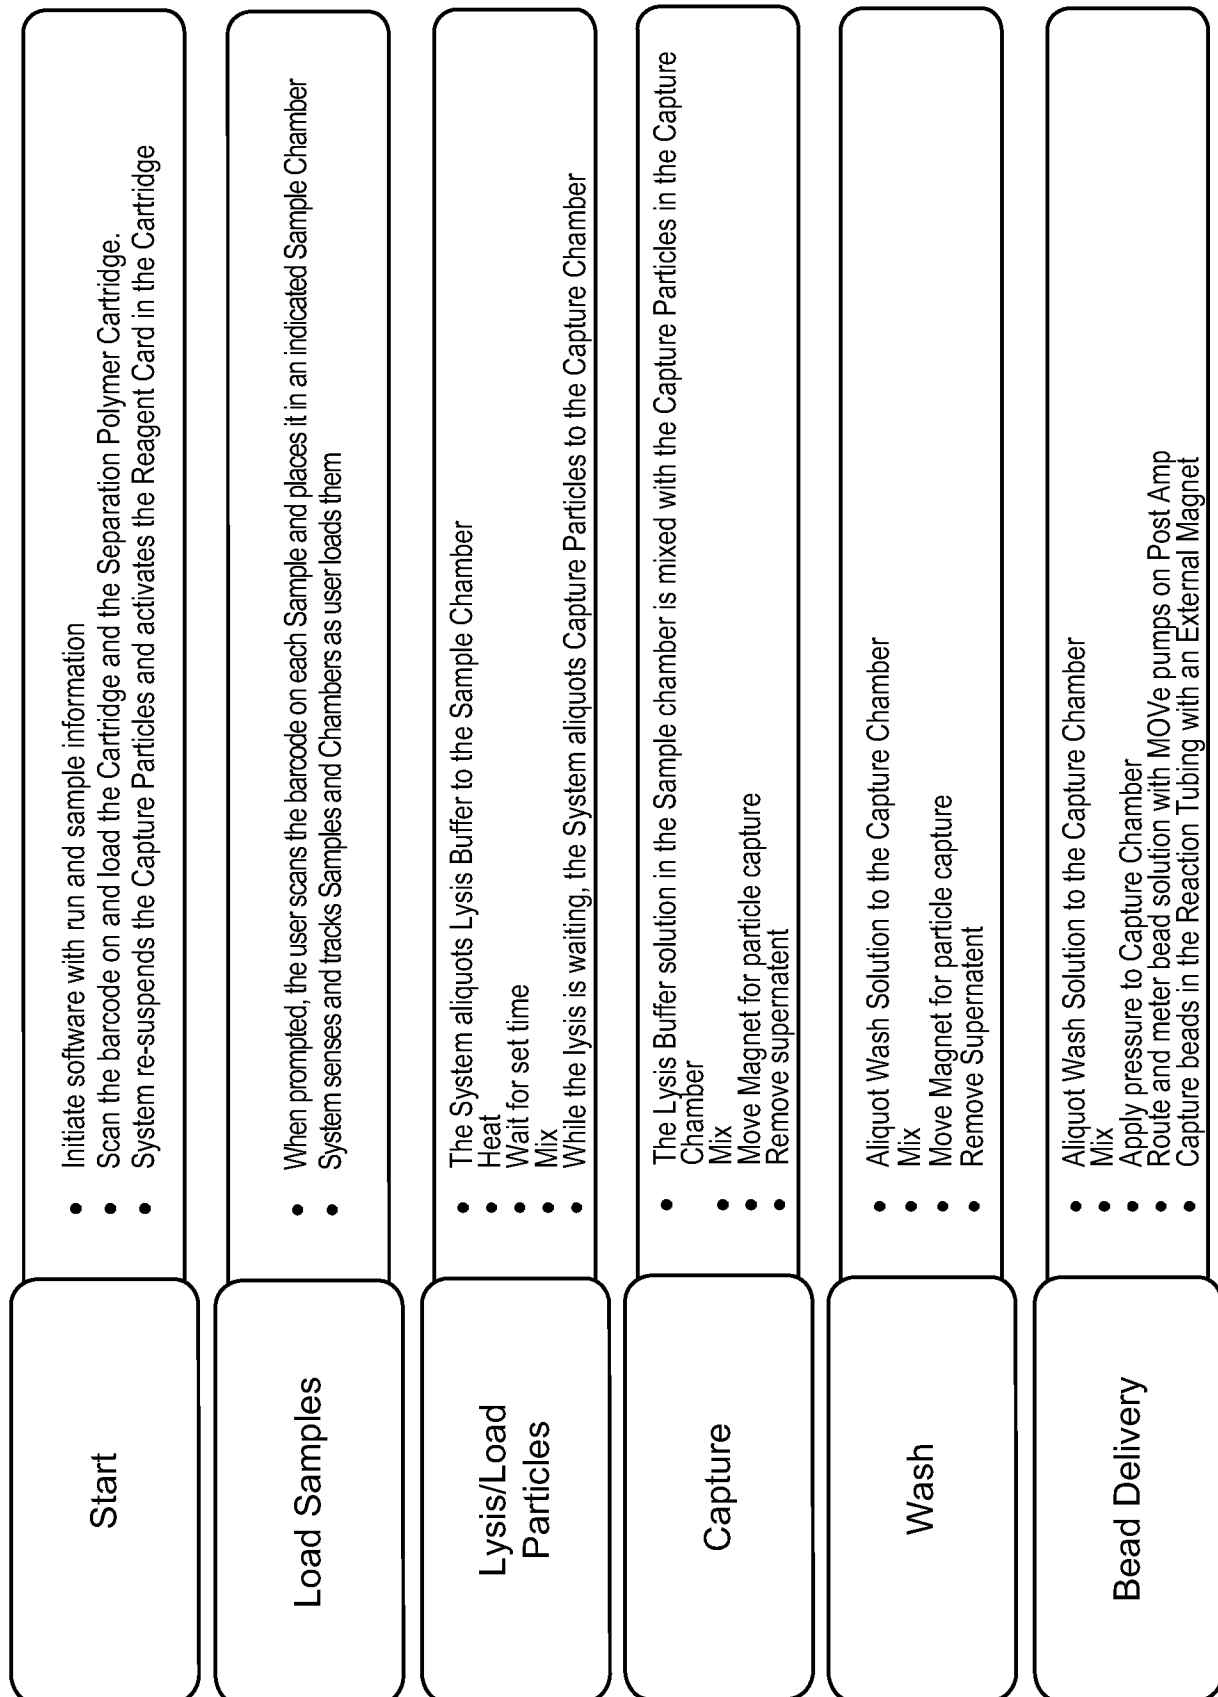


Figure 86

61/76

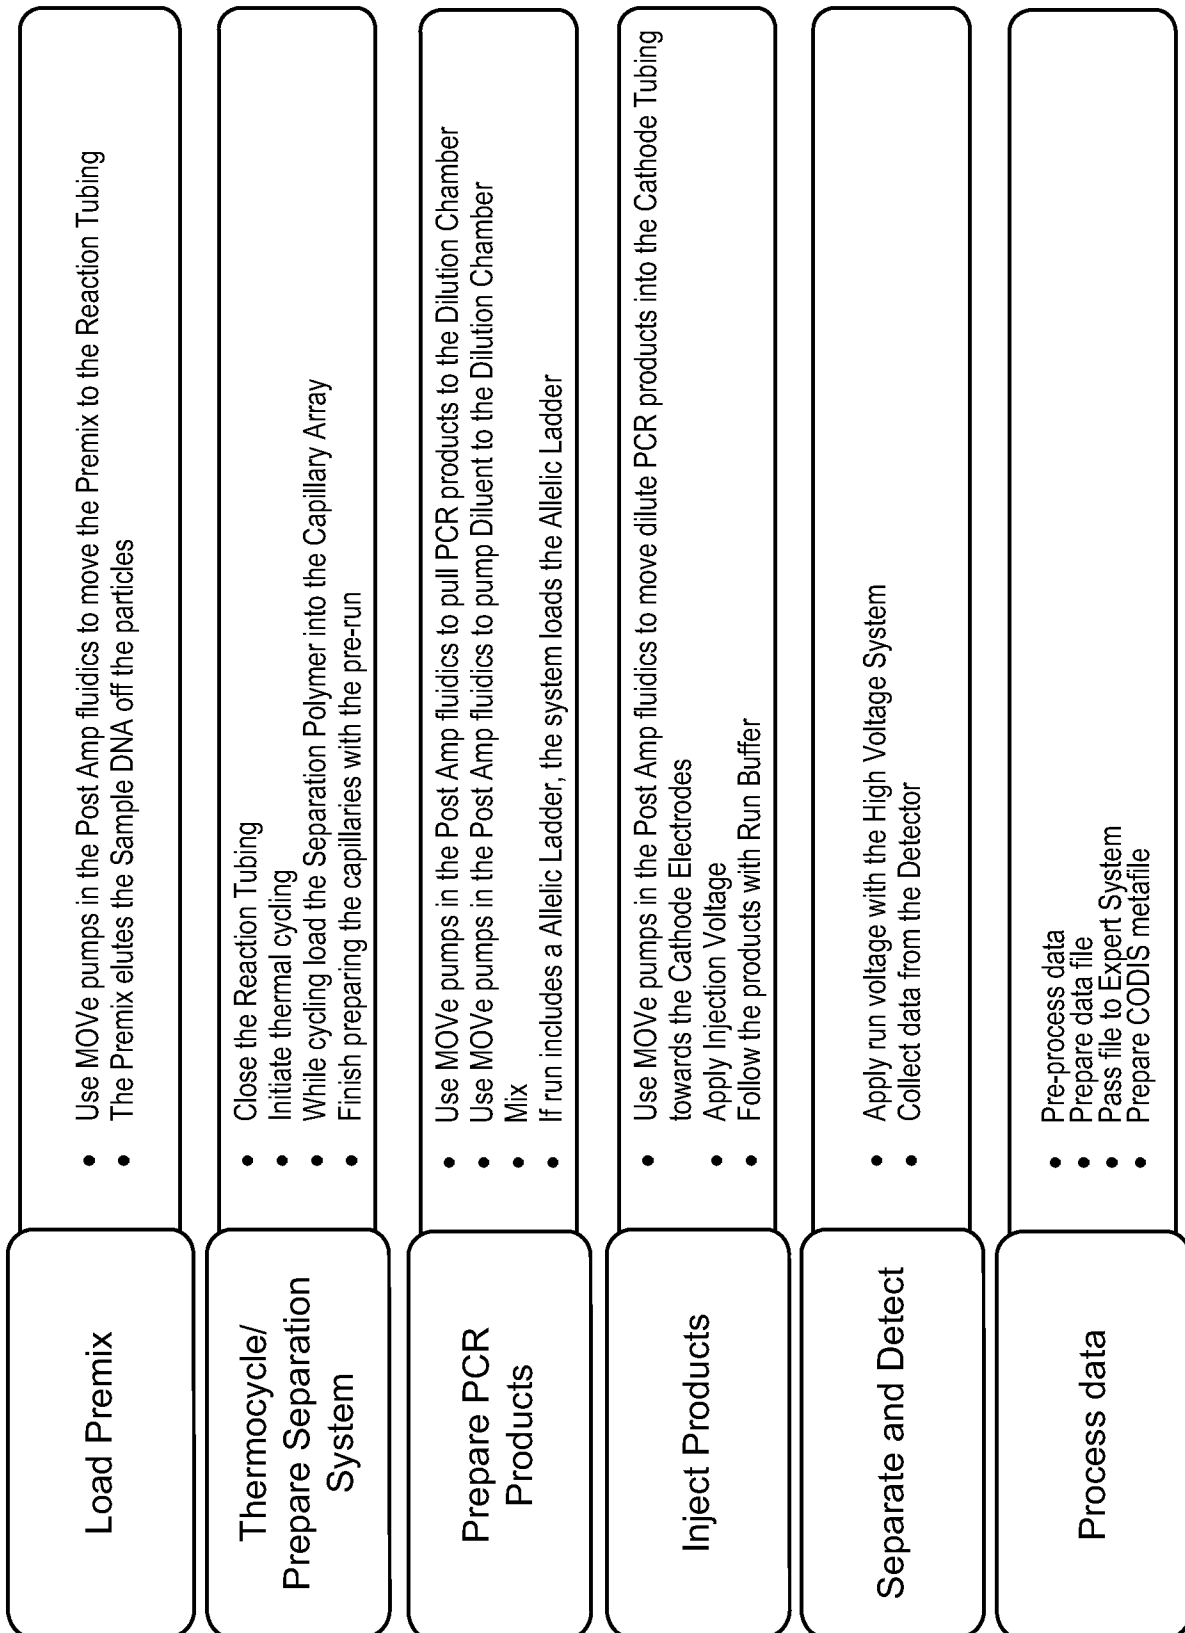


Figure 87

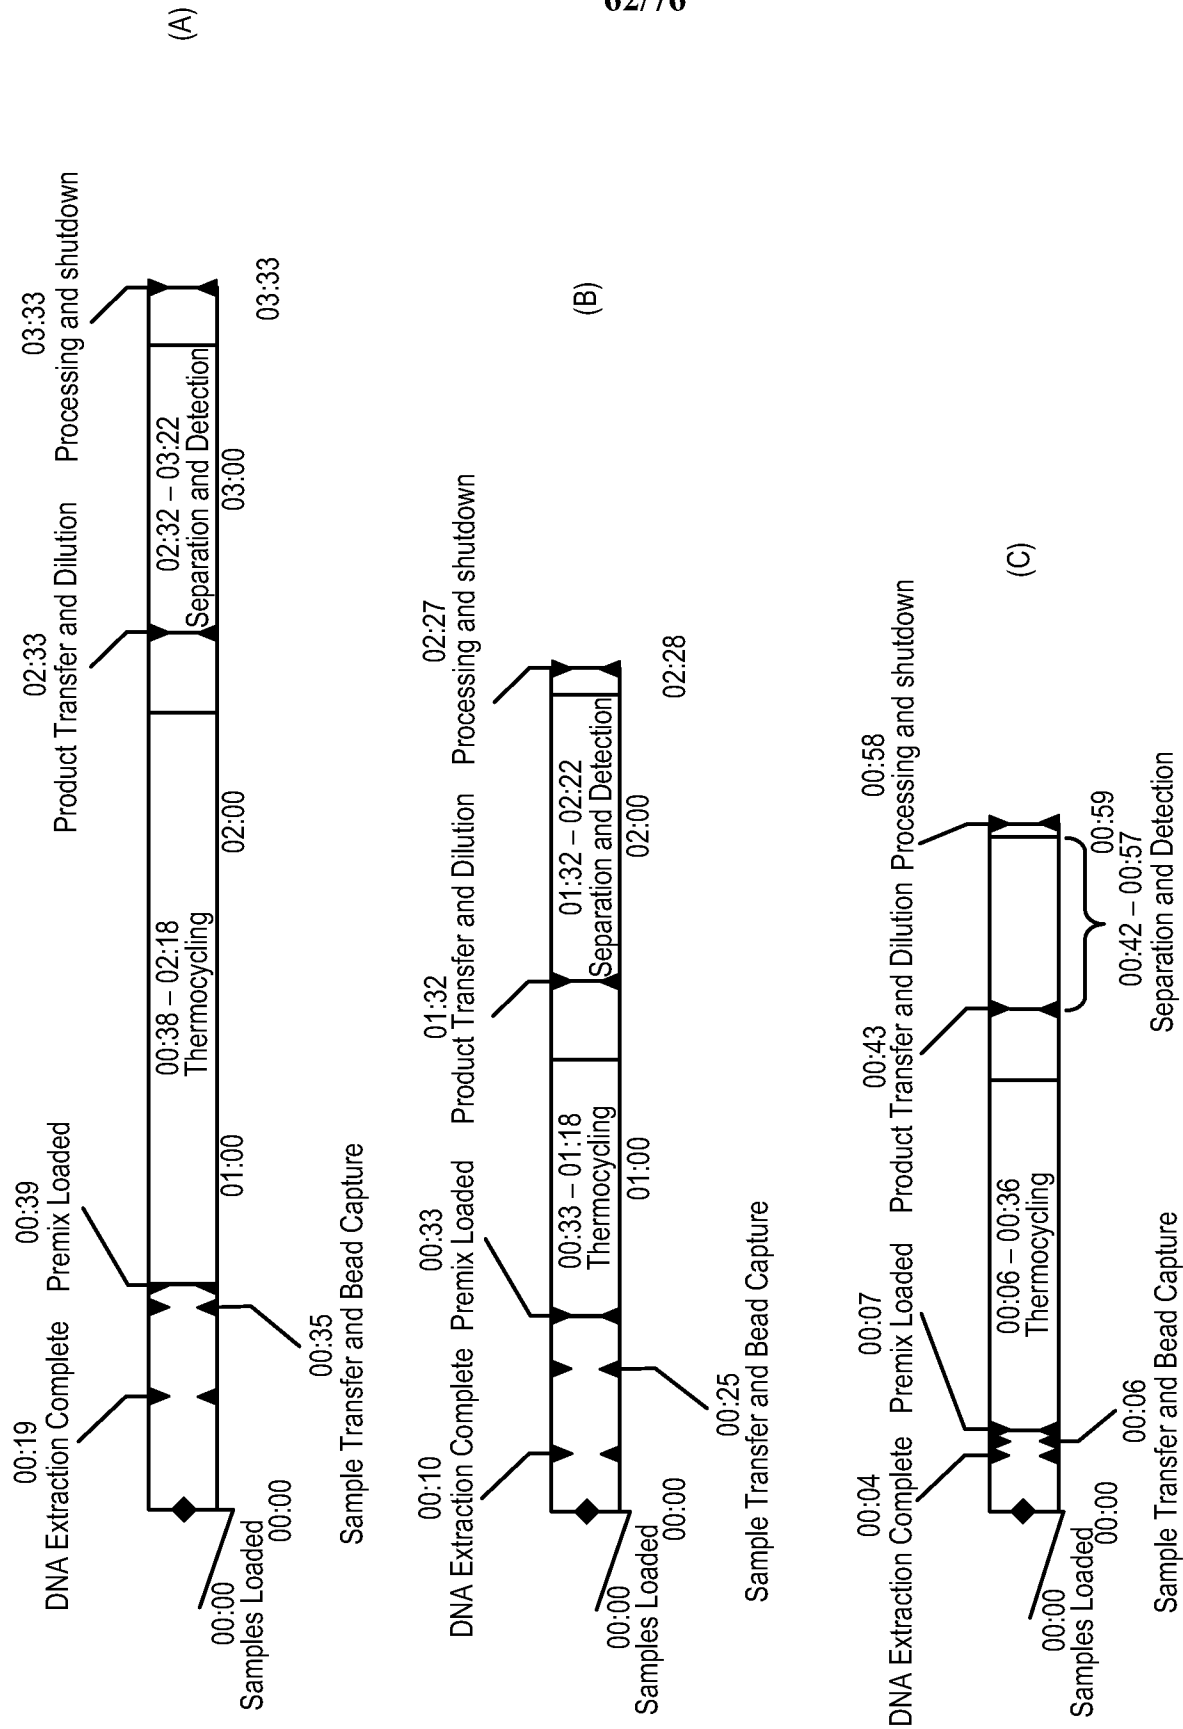


Figure 88

63/76

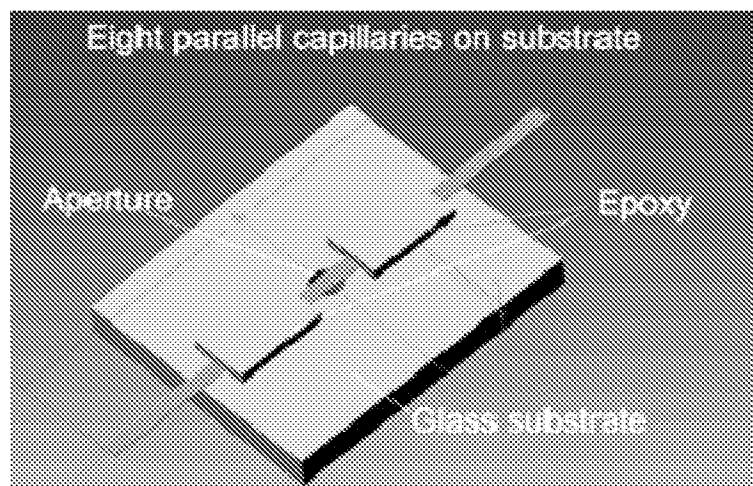


Figure 89

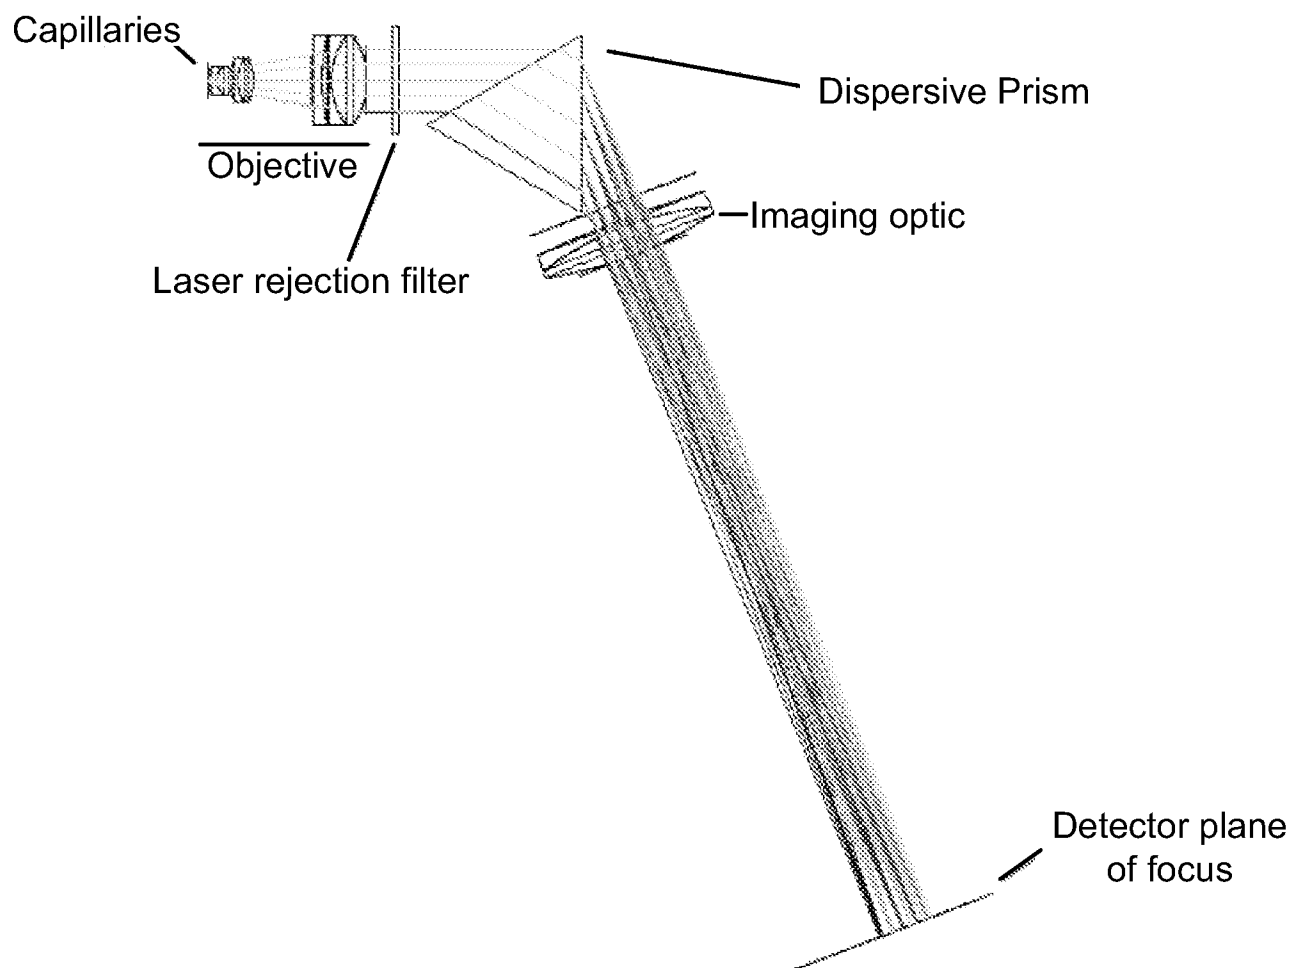


Figure 90

64/76

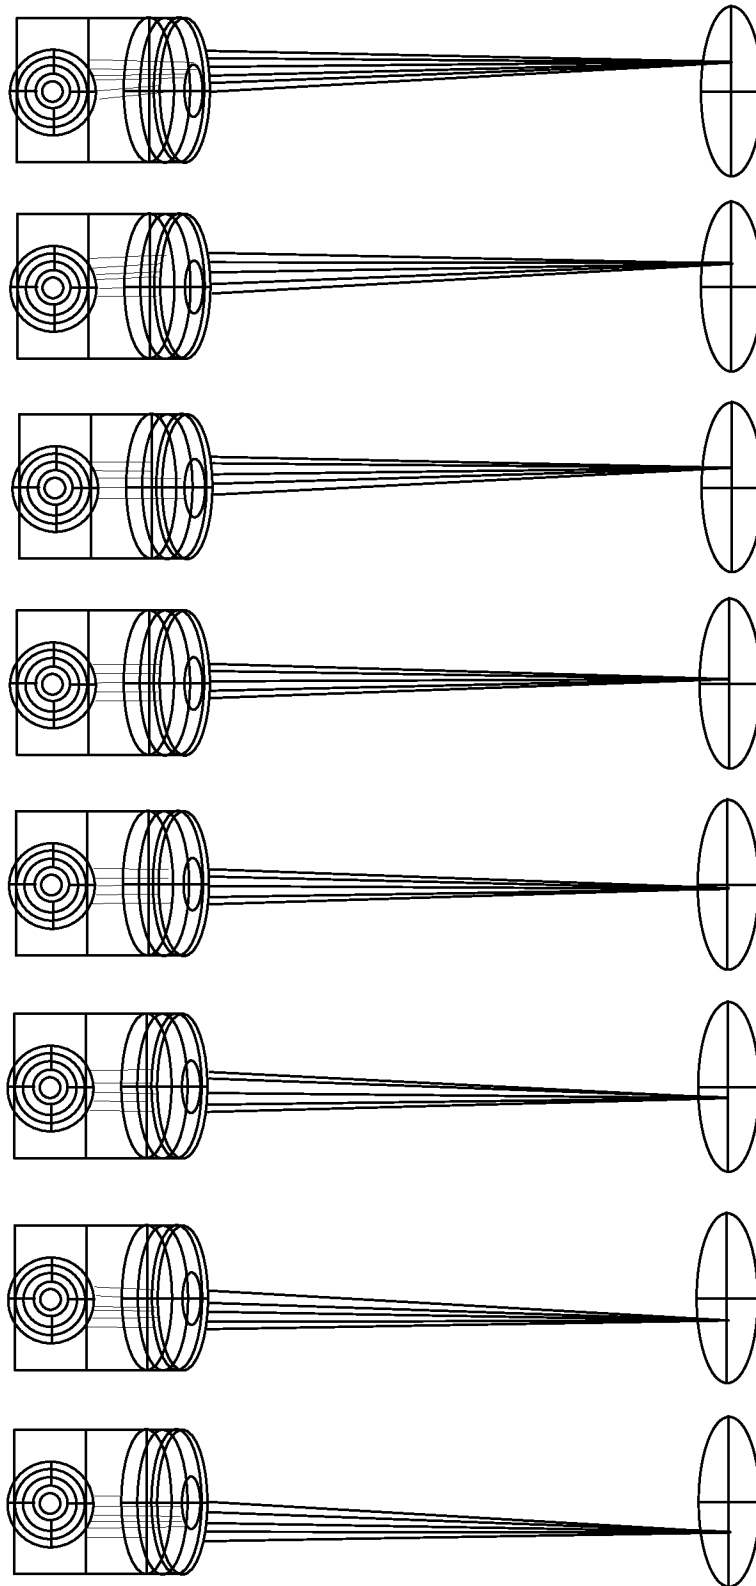


Figure 91

65/76

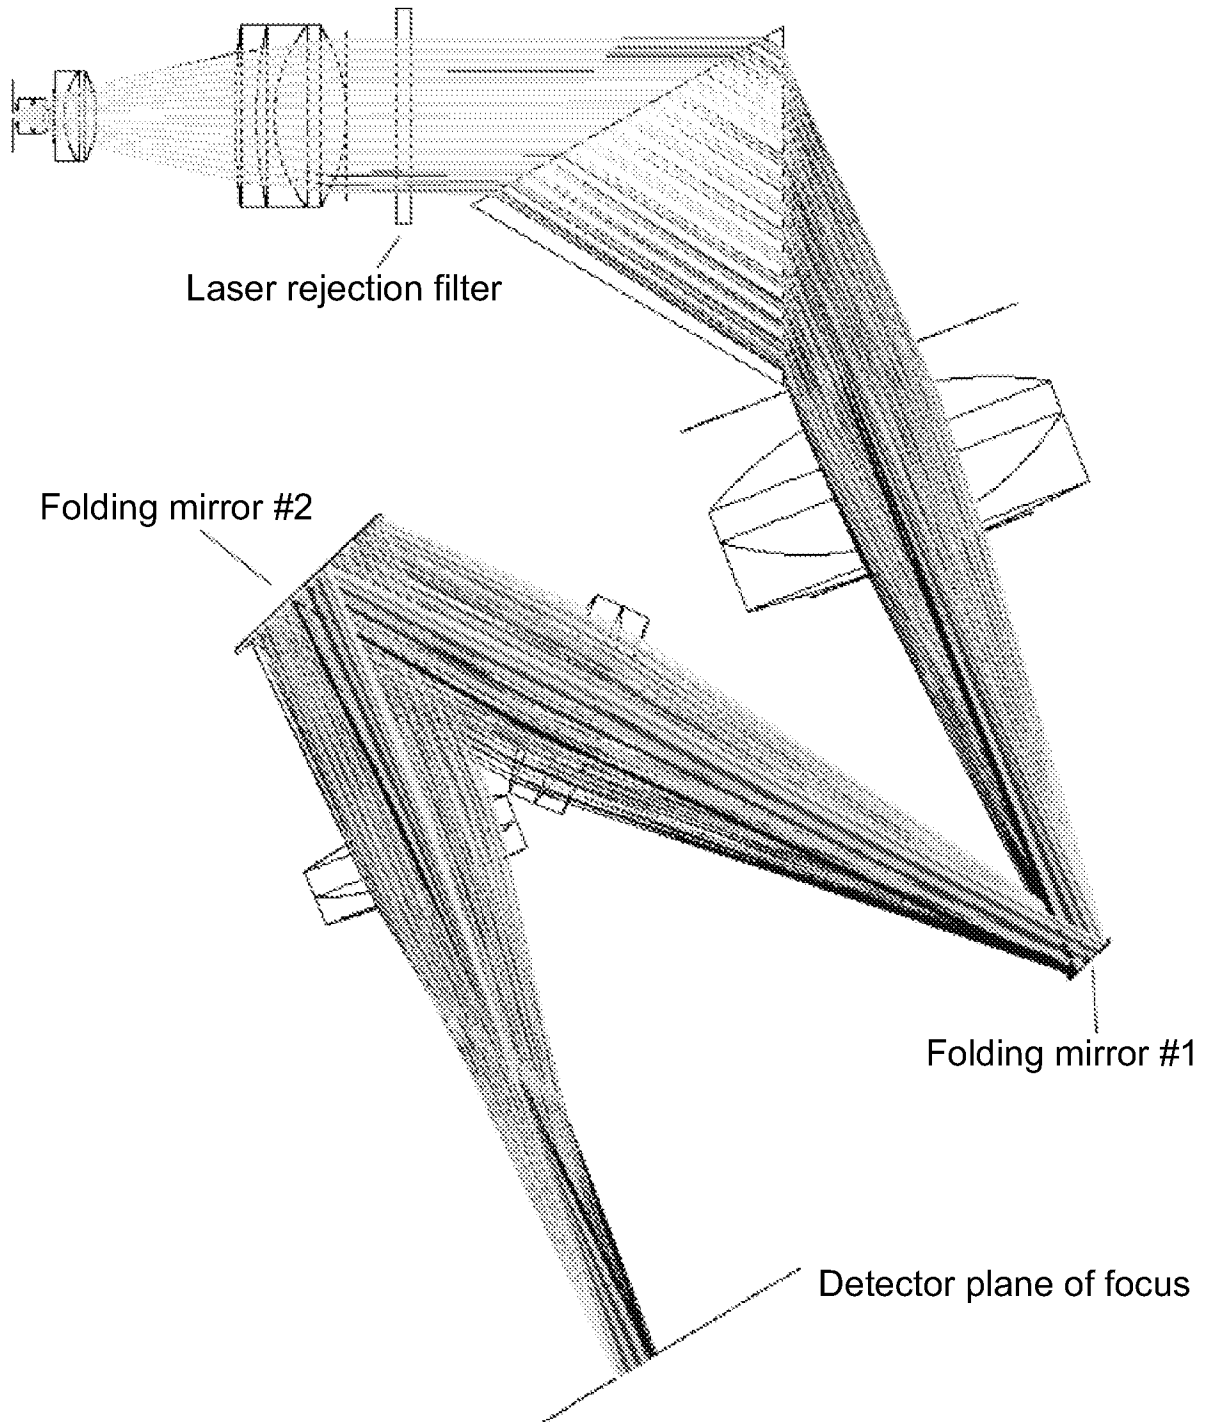


Figure 92

66/76

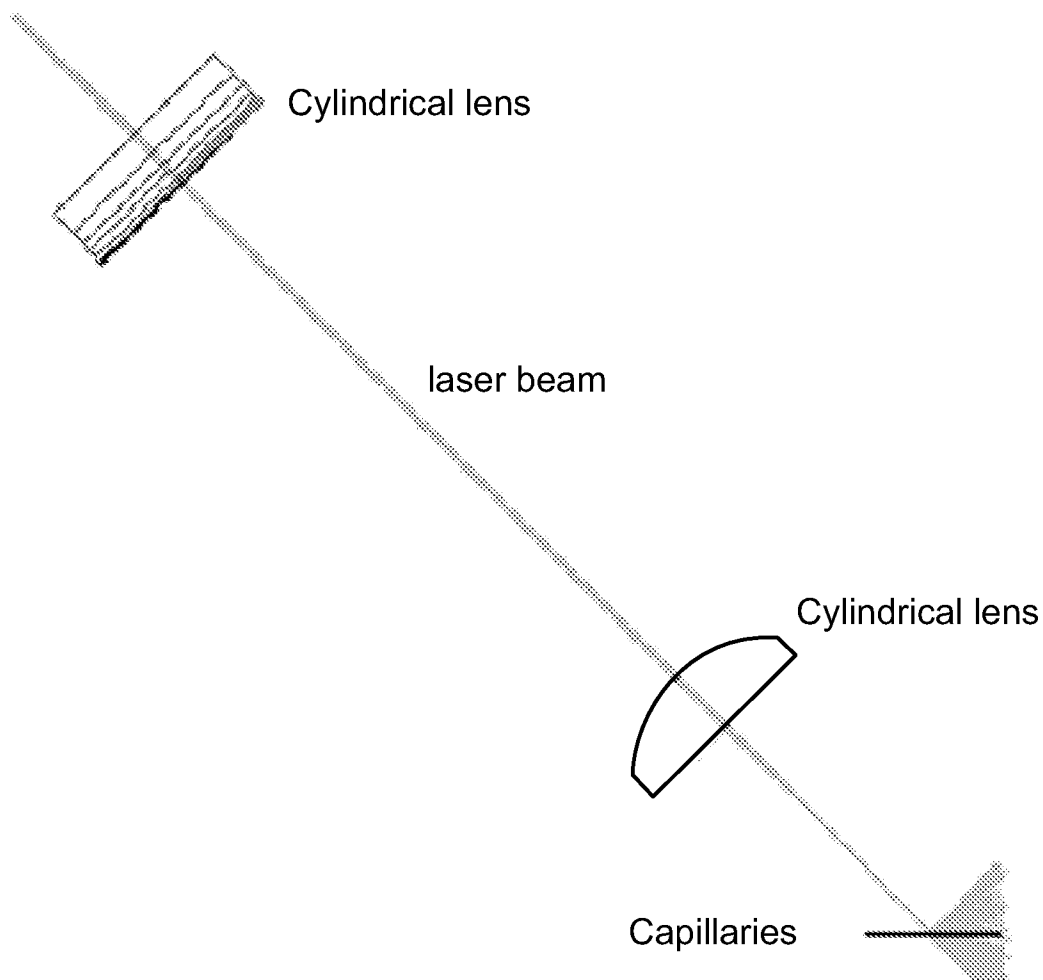


Figure 93

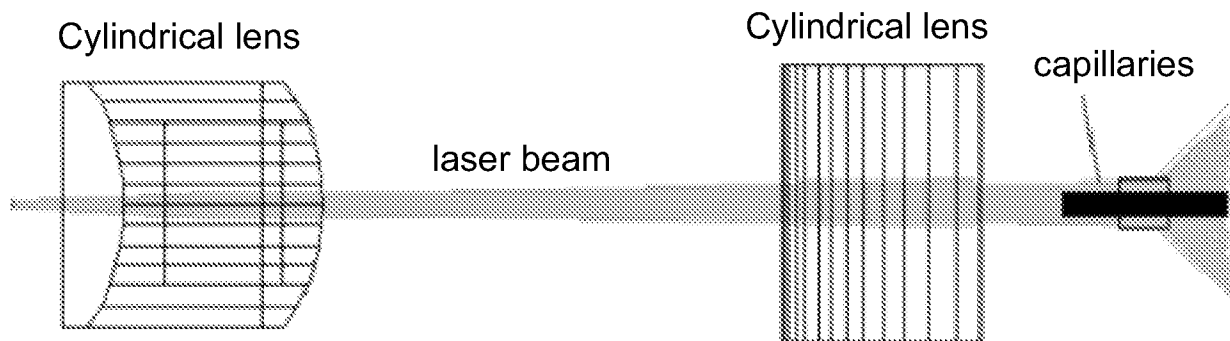


Figure 94

67/76

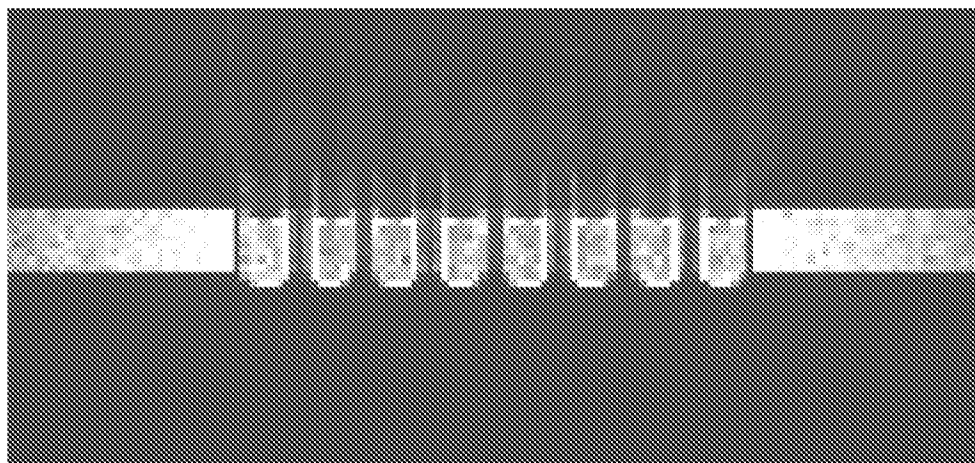


Figure 95

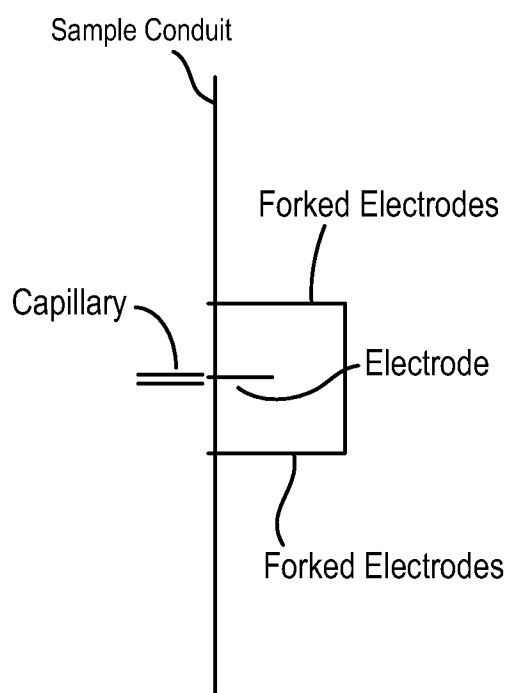


Figure 96A

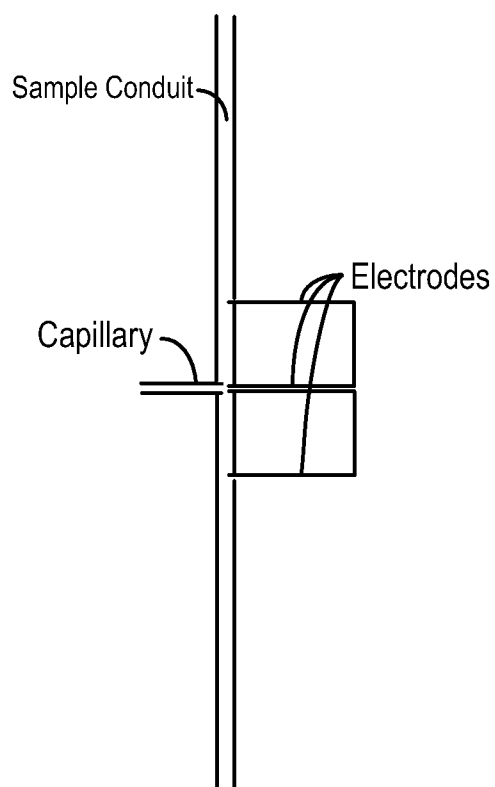


Figure 96B

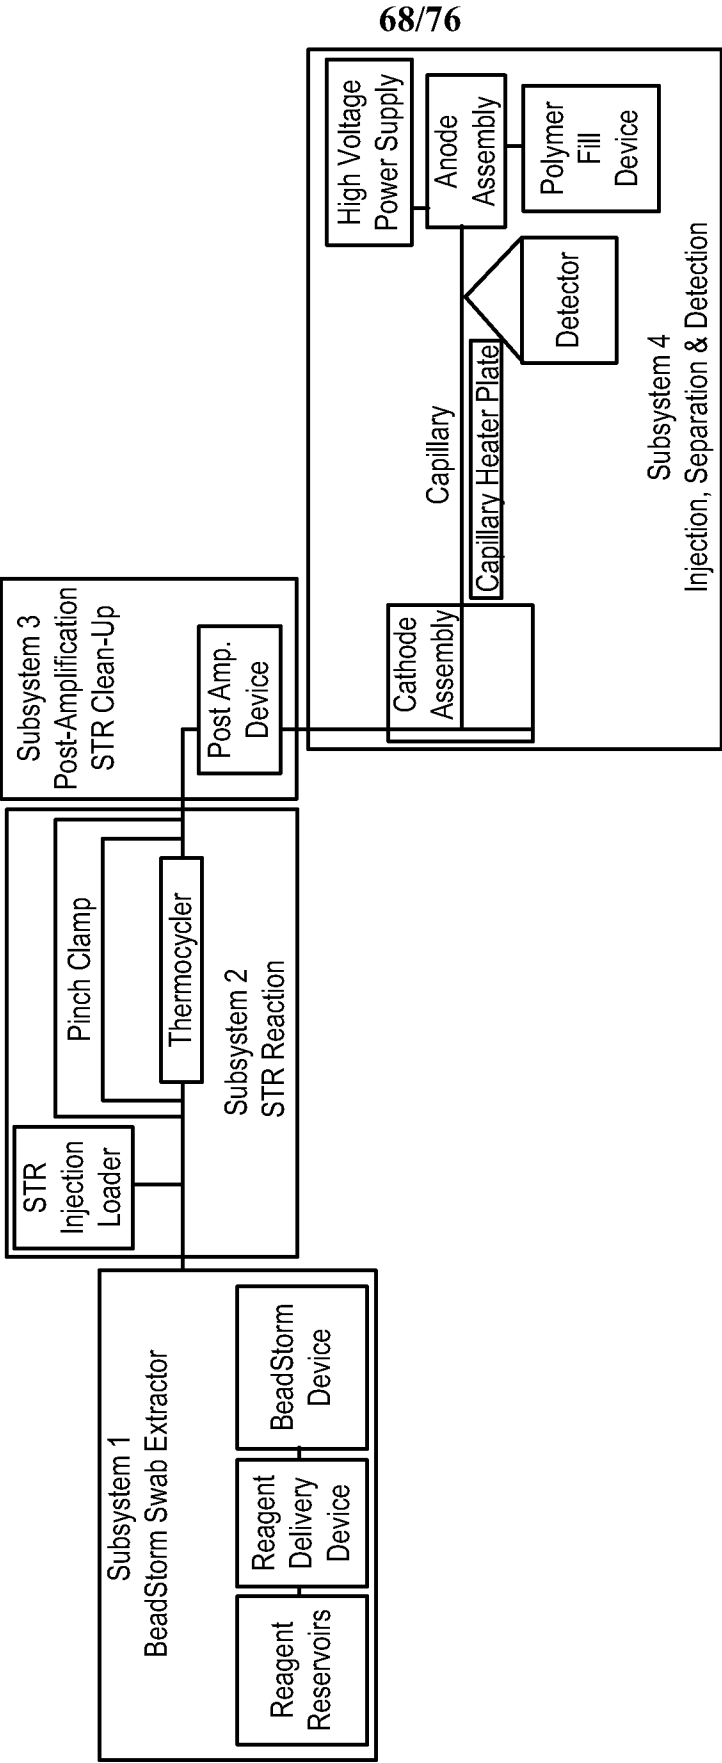


Figure 97

69/73

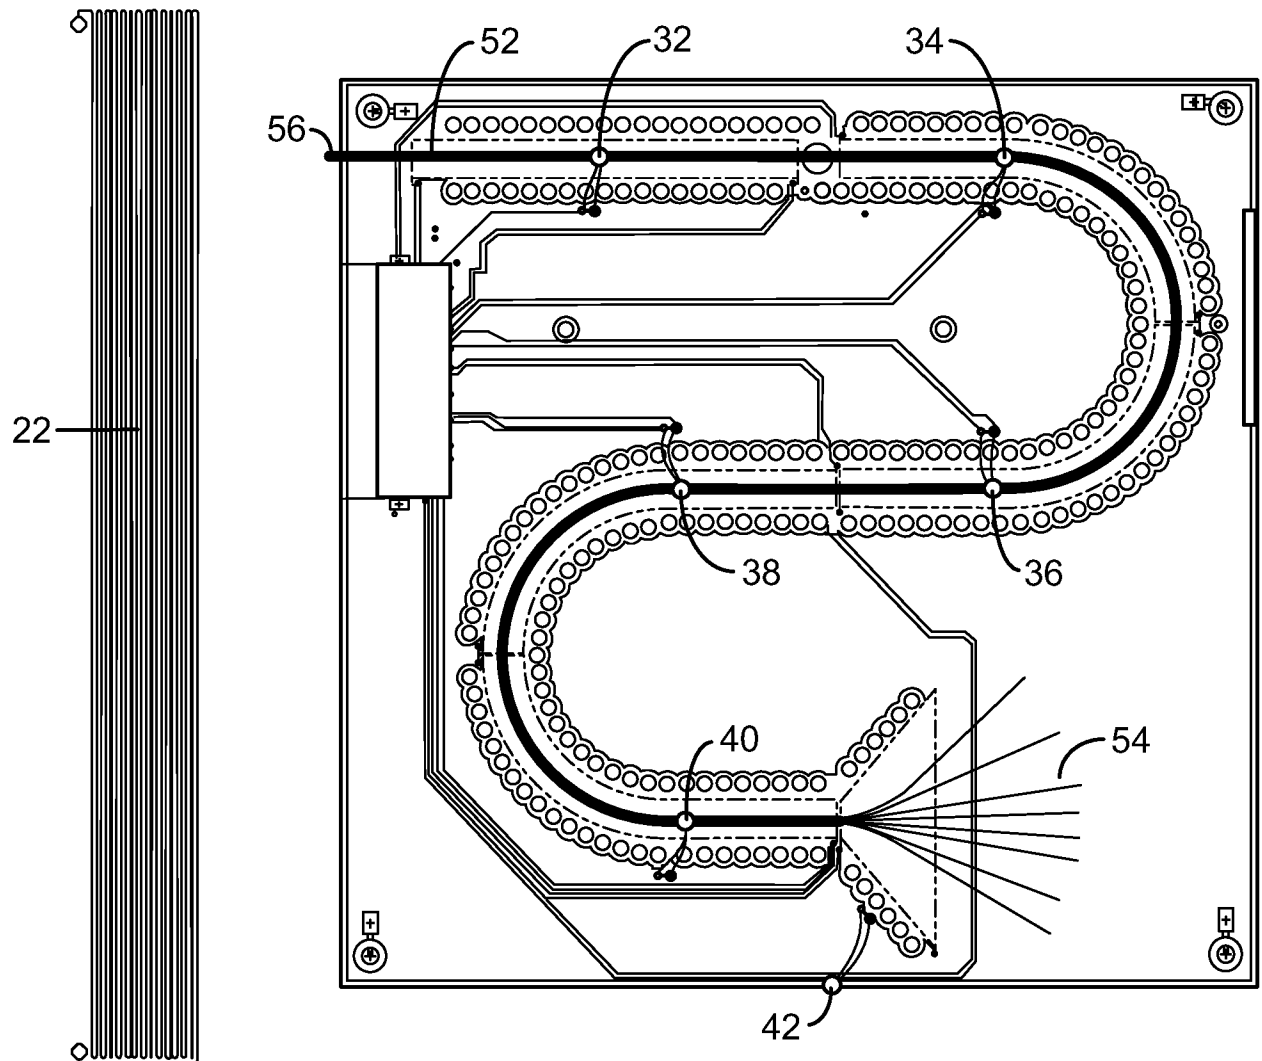


Figure 98A

70/76

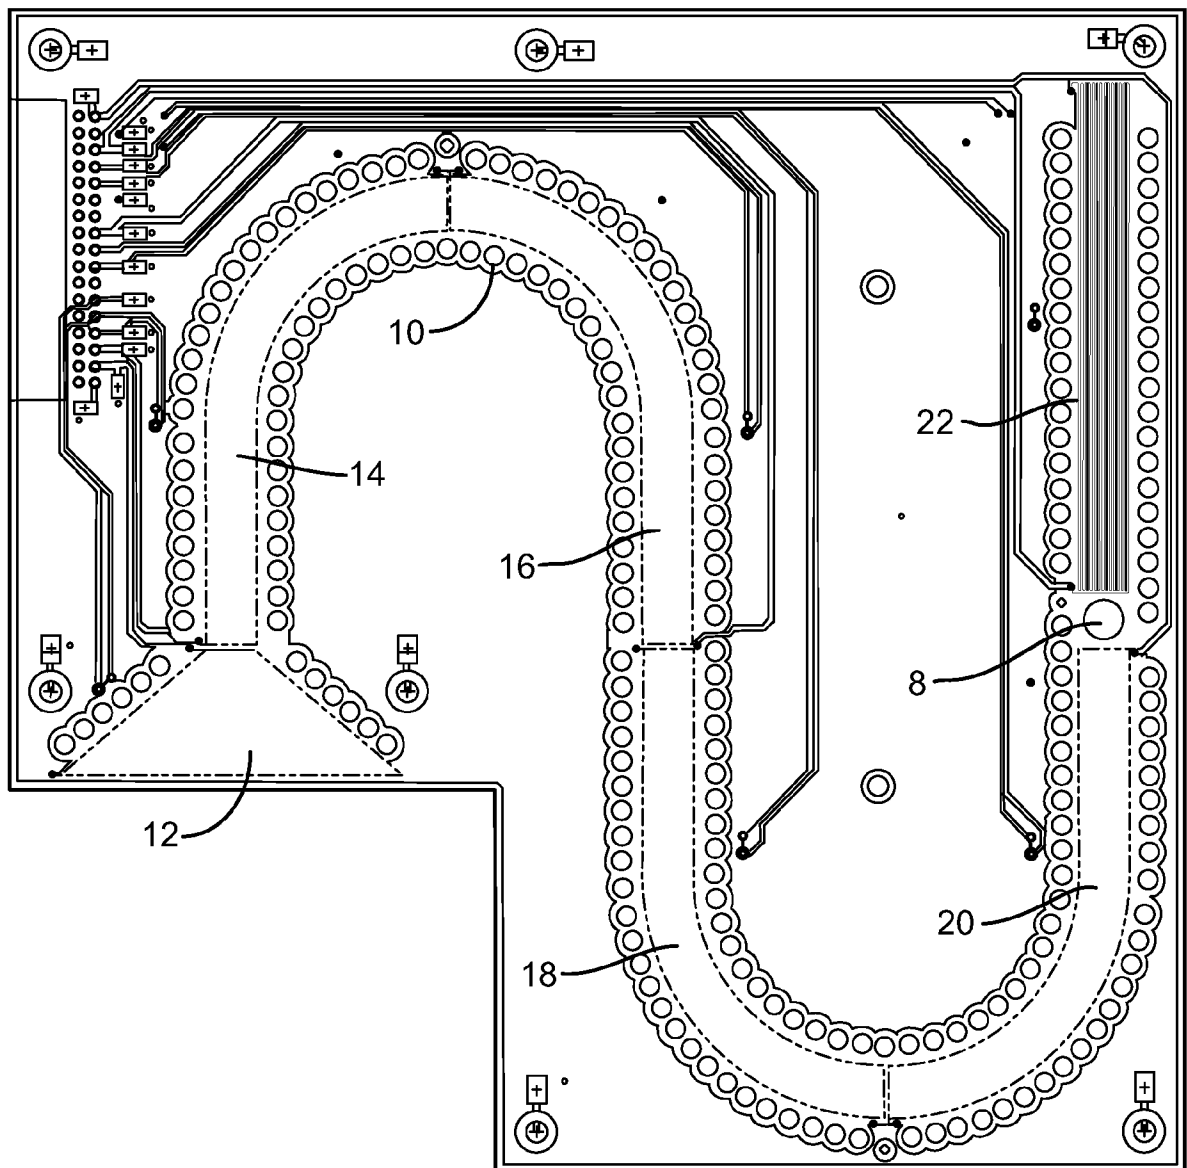


Figure 98B

71/76



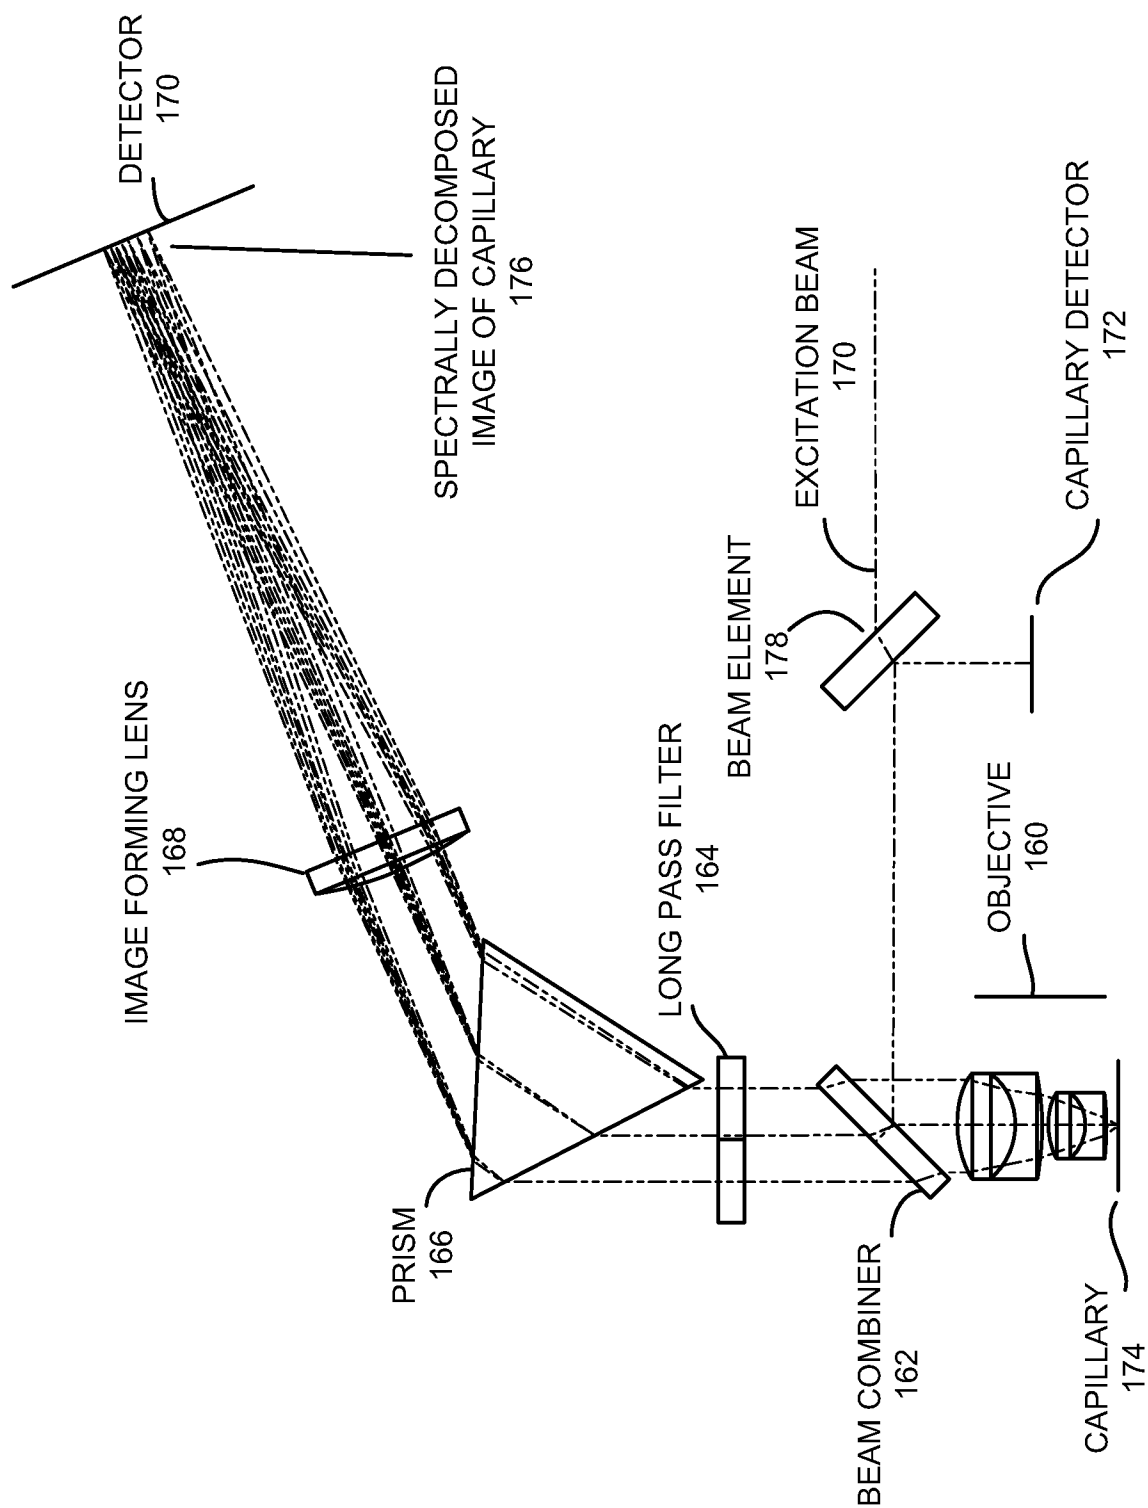


Figure 99

72/76

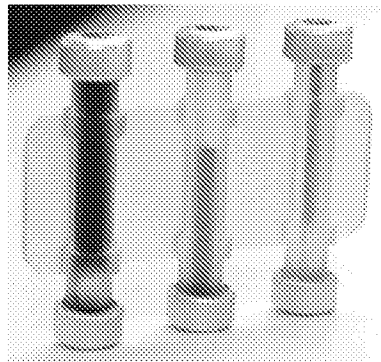


Precious Reagent Cartridge

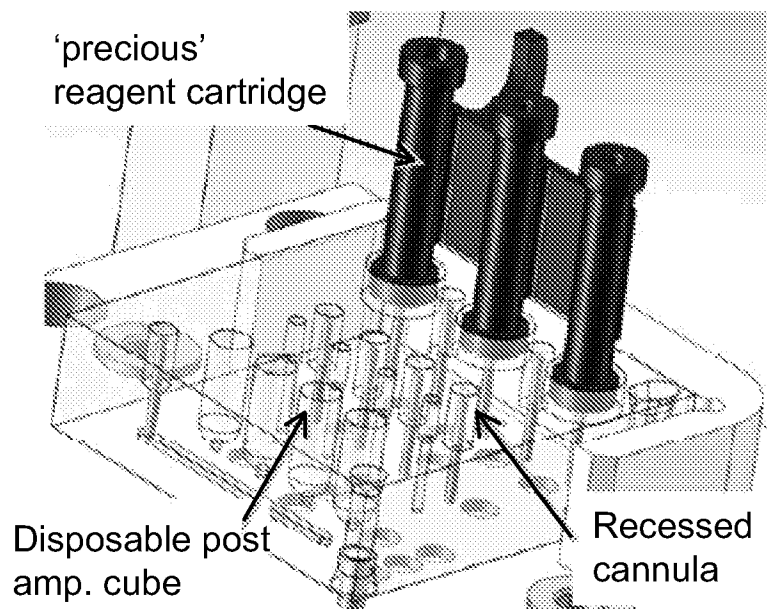

'precious' reagent cartridge

Disposable post amp. cube

Recessed cannula

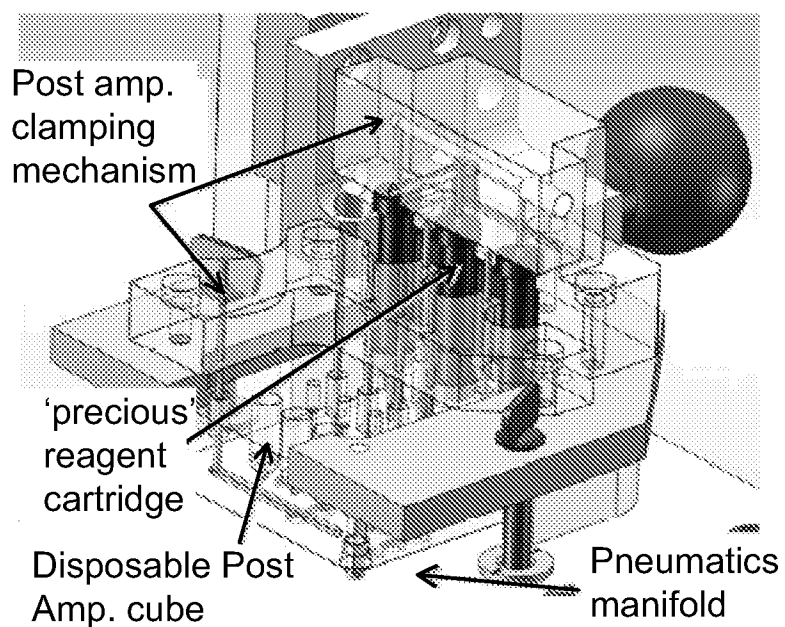

Post amp. clamping mechanism


'precious' reagent cartridge

Disposable Post Amp. cube

Pneumatics manifold

Figure 100

73/76

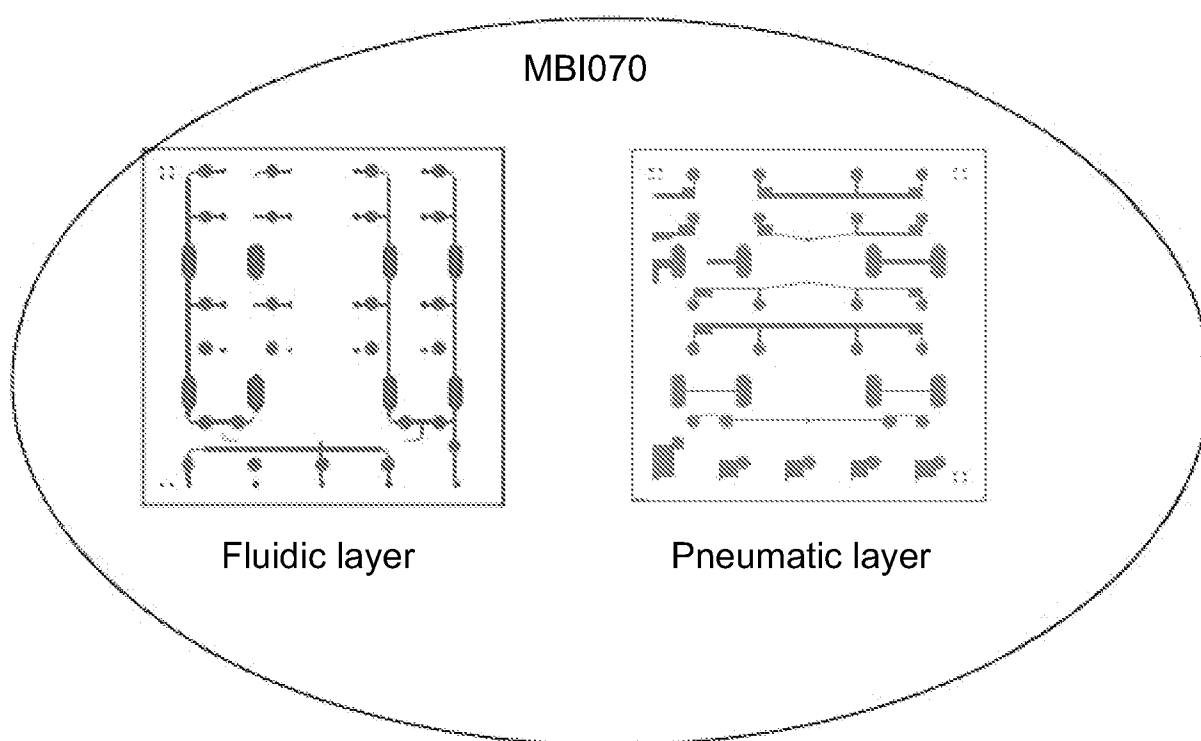

Post-amp Chip Architecture

Figure 101

74/76



System with Enclosure

Footprint = 2 x 2 x 2 ft

Figure 102

75/76

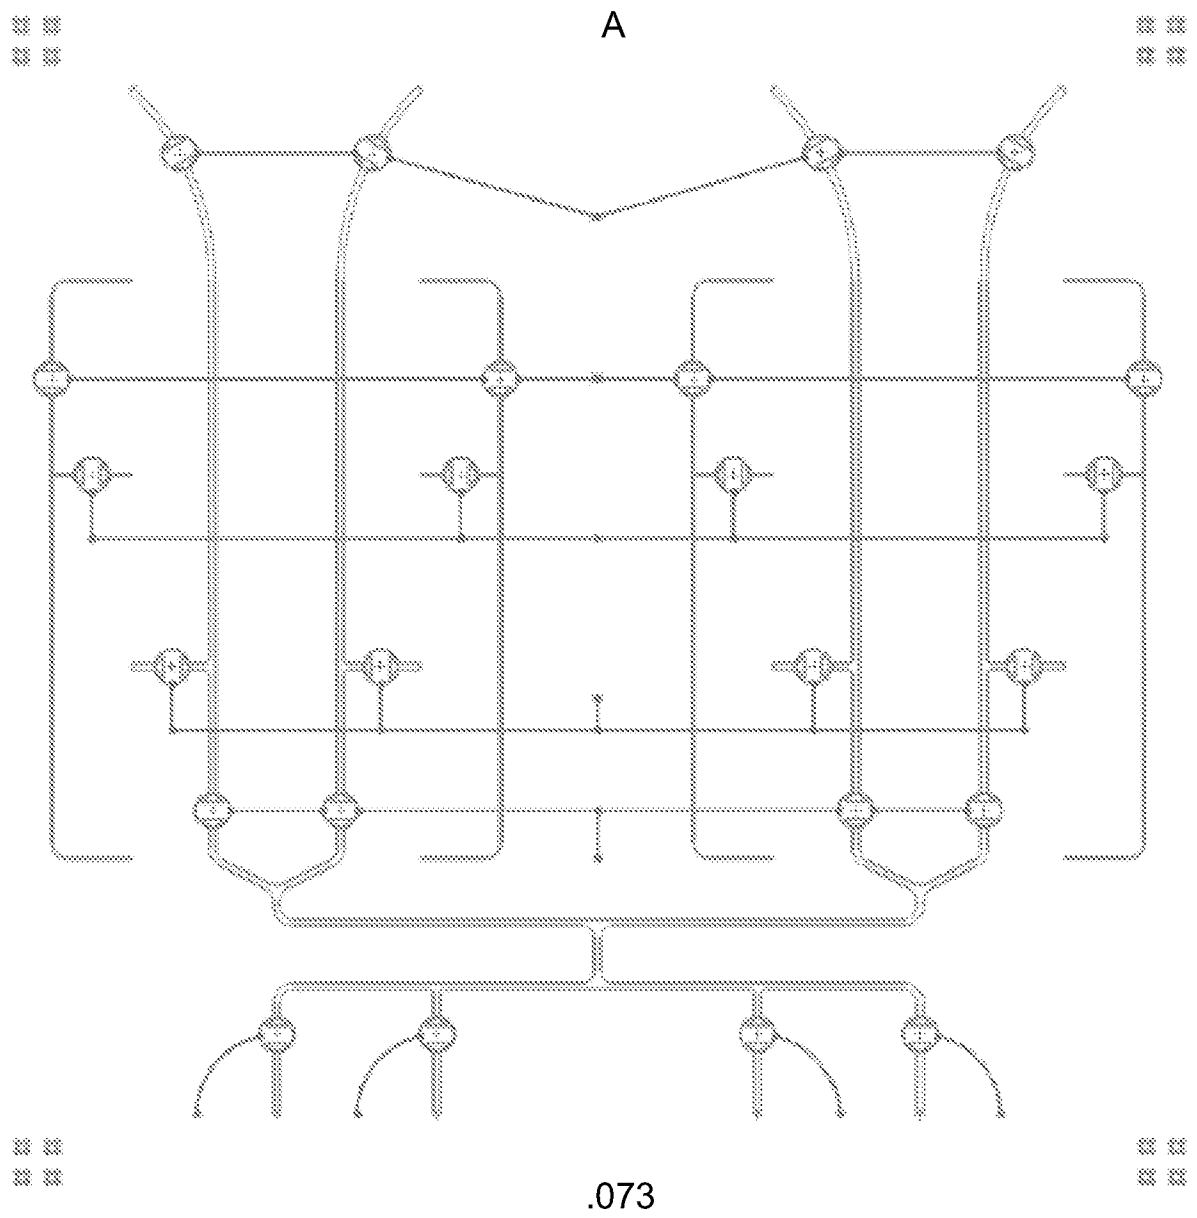


Figure 103

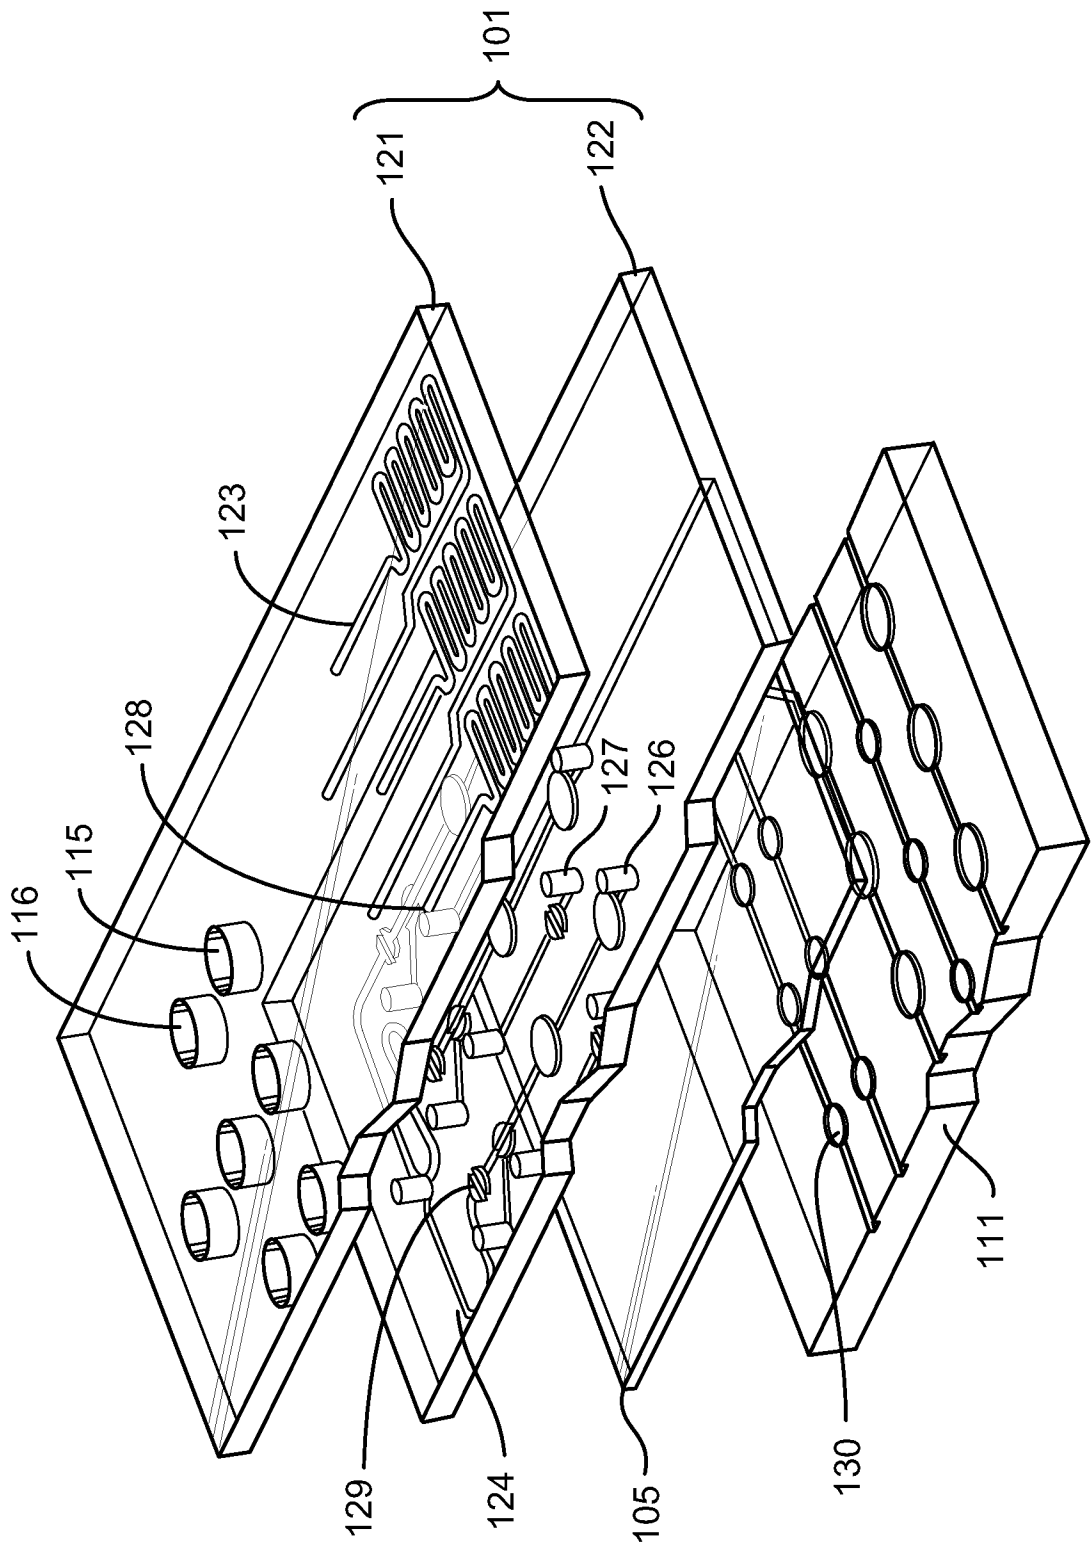


Figure 104

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 10/37545

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - C02F 1/40 (2010.01)

USPC - 204/601

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8): C02F 1/40 (2010.01)

USPC: 204/601

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

USPC: 204/600,450;600/583;606/139

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

PubWEST (PGPB,USPT,USOC,EPAB); Google Scholar (Articles and patents)

Search terms used: microfluidic channel analyte valve pump diaphragm (capture OR immobilize) (intersect OR intersecting) batter\$
monolith\$ circuit fluid sequential "ft.sup.3"

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2008/0014576 A1 (JOVANOVIĆ et al.) 17 January 2008 (17.01.2008), entire document, especially: para [0059]-[0064], [0082], [0107], [0115], [0129]-[0139], [0158]	1-12, 49, 77-96
Y	US 2007/0034025 A1 (PANT et al.) 15 February 2007 (15.02.2007), para [0045]	1-12, 49
Y	US 2005/0241941 A1 (PARCE et al.) 3 November 2005 (03.11.2005), para [0010]	77-90
Y	US 2008/0281090 A1 (LEE et al.) 13 November 2008 (13.11.2008), para [0008], [0024], [0209]	91-96
Y	US 2008/0164155 A1 (PEASE et al.) 10 July 2008 (10.07.2008), para [0136]	11, 81
A	US 2005/0161669 A1 (JOVANOVIĆ et al.) 28 July 2005 (28.07.2005), entire document	1-12, 49, 77-96

☐ Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

28 September 2010 (28.09.2010)

Date of mailing of the international search report

06 OCT 2010

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-3201

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 10/37545

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

Please see Supplemental Box

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
Group I: claims 1-12, 49, and 77-96

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

Box III: Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This application contains the following inventions or groups of inventions which are not so linked as to form a single general inventive concept under PCT Rule 13.1. In order for all inventions to be examined, the appropriate additional examination fees must be paid.

Group I: Claims 1-12, 49 and 77-96, drawn to a system and method that fits within an enclosure comprising sample preparation module adapted to capture an analyte from a non-microfluidic volume, reaction module comprising a reaction chamber in fluidic communication with the microfluidic and analysis module in fluidic communication with the reaction chamber.

Group II: Claims 13-36, 49 and 51-62, drawn to a system comprising a cartridge cover, a cartridge and a pneumatic manifold wherein the cartridge can be releasably engaged with the cartridge cover and the pneumatic manifold.

Group III: Claims 37-50, drawn to a method comprising producing, from a sample comprising at least one cell comprising DNA, a computer file identifying a plurality of STR markers in the DNA.

Group IV: Claims 63-76, drawn to an optical system comprising a plurality of optically transparent channels, light source and a detector.

Group V: Claims 97-98, device comprising, electrophoresis capillary inlet and outlet; anode and a cathode forked electrode.

The inventions listed as Groups I-V do not relate to a single general inventive concept under PCT Rule 13.1 because, under PCT Rule 13.2, they lack the same or corresponding special technical features for the following reasons:

The technical feature of Group I is the sample preparation module, non-microfluidic volume, microfluidic module, which is not present in Group II-V

The technical feature of Group II is the cartridge cover, a cartridge and a pneumatic manifold, which is not present in Groups I, and III-V.

The technical feature of Group III is the computer file identifying a plurality of STR markers in the DNA, which is not present in Groups I-II and IV-V.

The technical feature of Group IV is an optical system, which is not present in Groups I-III and V

The technical feature of Group V is electrophoresis capillary; and anode and a cathode forked electrode, which is not present in Groups I-III and IV

Therefore, the unity of invention is lacking between Groups I-V under PCT Rule 13.1.