



(12) **United States Design Patent**
McCracken et al.

(10) **Patent No.:** **US D1,002,000 S**
(45) **Date of Patent:** **** Oct. 17, 2023**

(54) **NASAL MASK AND TUBE IN COMBINATION**

(56) **References Cited**

(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,
Eindhoven (NL)

(72) Inventors: **Chris McCracken**, Harrison City, PA
(US); **Lloyd Spencer**, Pittsburgh, PA
(US); **Oisin O’Muircheartaigh**,
Cambridge, MA (US); **Justin Shinn**,
Pittsburgh, PA (US); **Justin Rothermel**,
Pittsburgh, PA (US); **Dave Ignaczak**,
Monroeville, PA (US); **Jonathan**
Grashow, Cheswick, PA (US); **Richard**
Haibach, Verona, PA (US)

U.S. PATENT DOCUMENTS

D704,329 S * 5/2014 Collazo D24/110.4
D708,736 S * 7/2014 Judson D24/110.5
D770,036 S * 10/2016 Walls D24/110.4
D787,662 S * 5/2017 Guney D24/110.4
D797,921 S * 9/2017 Huang D24/110.4
10,080,856 B2 * 9/2018 McLaren A61M 16/06
D857,190 S * 8/2019 Siew D24/110.4
D861,857 S * 10/2019 Huang D24/110.4

(Continued)

OTHER PUBLICATIONS

Nuance tube assembly, posted at thecpapshop.com, first available Aug. 27, 2019, retrieved, Aug. 30, 2022, online, URLhttps://www.1800cpap.com/nuance-cpap-mask-gel-cushion-replacement-1 (Year: 2019).*

(Continued)

Primary Examiner — Mary Shannon Malley
Assistant Examiner — Michelle Marquart Christeon

(73) Assignee: **KONINKLIJKE PHILIPS N.V.**,
Eindhoven (NL)

(**) Term: **15 Years**

(21) Appl. No.: **29/762,357**

(22) Filed: **Dec. 16, 2020**

(57) **CLAIM**

The ornamental design for a nasal mask and tube in combination, as shown and described.

(30) **Foreign Application Priority Data**

Jun. 16, 2020 (EM) 008006399

(51) **LOC (14) Cl.** **29-02**

(52) **U.S. Cl.**

USPC **D24/110.4**

(58) **Field of Classification Search**

USPC D24/110, 110.1–110.5, 127, 129;
D29/108

CPC A61M 16/0622; A61M 16/0616; A61M
16/0816; A61M 16/08; A61M 16/0633;
A61M 16/06; A61M 16/0666; A61M
2210/0618; A61M 16/0683; A61M
16/0605; A61M 16/0875; A61M
2208/0618; A61M 2208/0208; B63C
11/205; B63C 11/16

See application file for complete search history.

DESCRIPTION

FIG. 1 is a perspective view showing a nasal mask and tube in combination;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a right side elevational view thereof;


FIG. 5 is a left side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines in the figures show portions of the nasal mask and tube in combination that form no part of the claimed design.

1 Claim, 5 Drawing Sheets

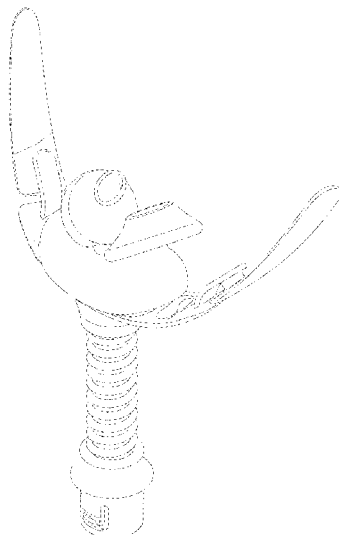

(56)

References Cited

U.S. PATENT DOCUMENTS

D894,372 S * 8/2020 Larrow D24/110.4
D901,003 S * 11/2020 Gardiola D24/110.4
D930,148 S * 9/2021 Dantanarayana D24/110.1
2014/0000614 A1* 1/2014 Chang A61M 16/0666
128/205.25
2014/0299134 A1* 10/2014 Matula A61M 16/0666
128/205.25
2016/0151596 A1* 6/2016 Slight A61M 16/06
128/207.18
2019/0151592 A1* 5/2019 Bornholdt A61M 16/0666

OTHER PUBLICATIONS

Swift Fx Nasal Assembly, posted at thecpapshop.com, first available Sep. 5, 2011, retrieved, Aug. 30, 2022, online, URL:<https://www.thecpapshop.com/resmed-swift-fx-nasal-pillow-cpap-mask-headgear> (Year: 2011).*

Rio Nasal Assembly, posted at cpap.com, first available May 6, 2018, retrieved, Aug. 30, 2022, online, URL:<https://www.cpap.com/productpage/3b-medical-rio-ii-nasal-pillow-cpap-mask-all-sizes> (Year: 2018).*

Swift LT Apparatus, posted at respshop.com, first available Jul. 11, 2014, retrieved, Aug. 30, 2022, online, URL:<https://www.respshop.com/cpap-masks/nasal-pillows/resmed-swift-lt-nasal-pillow-cpap-mask-p-118.html> (Year: 2014).*

* cited by examiner

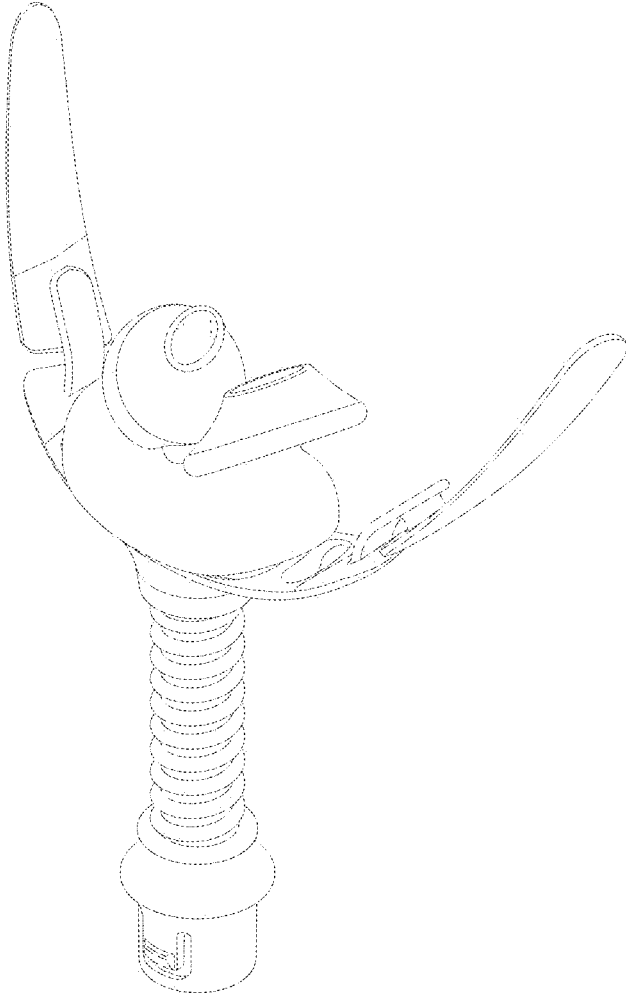


FIG. 1

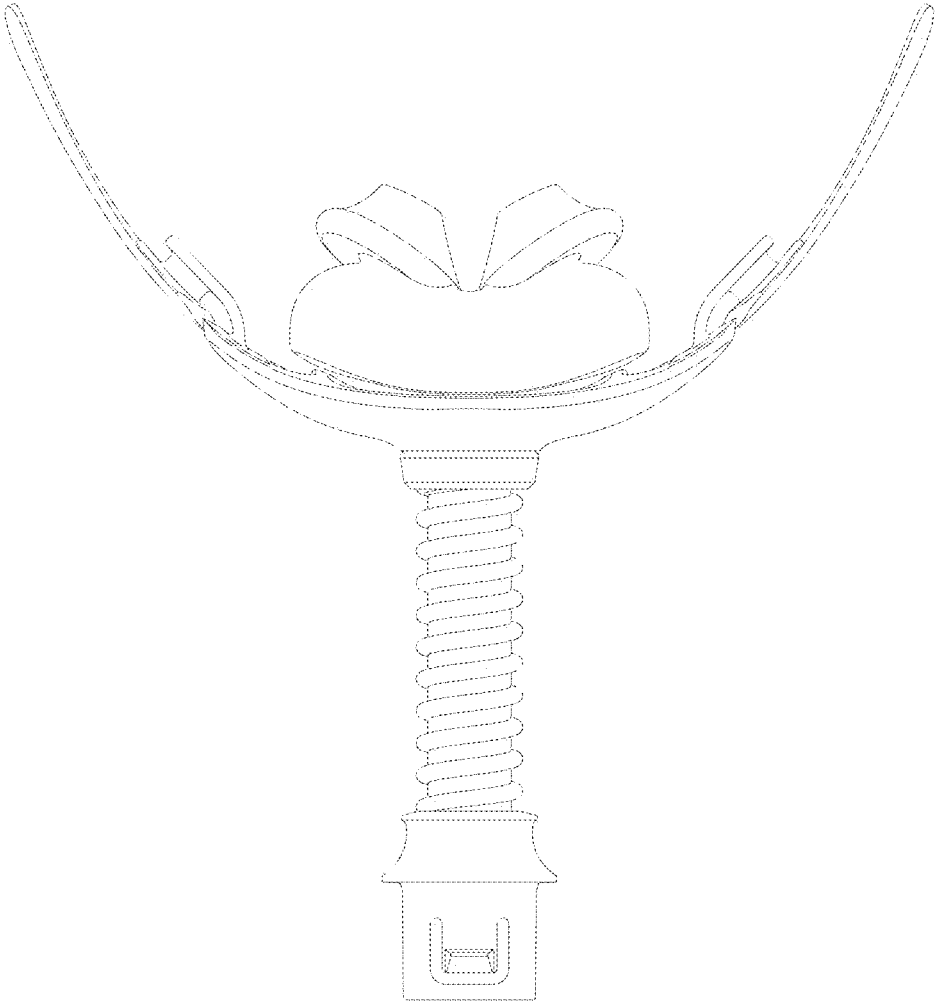


FIG. 2

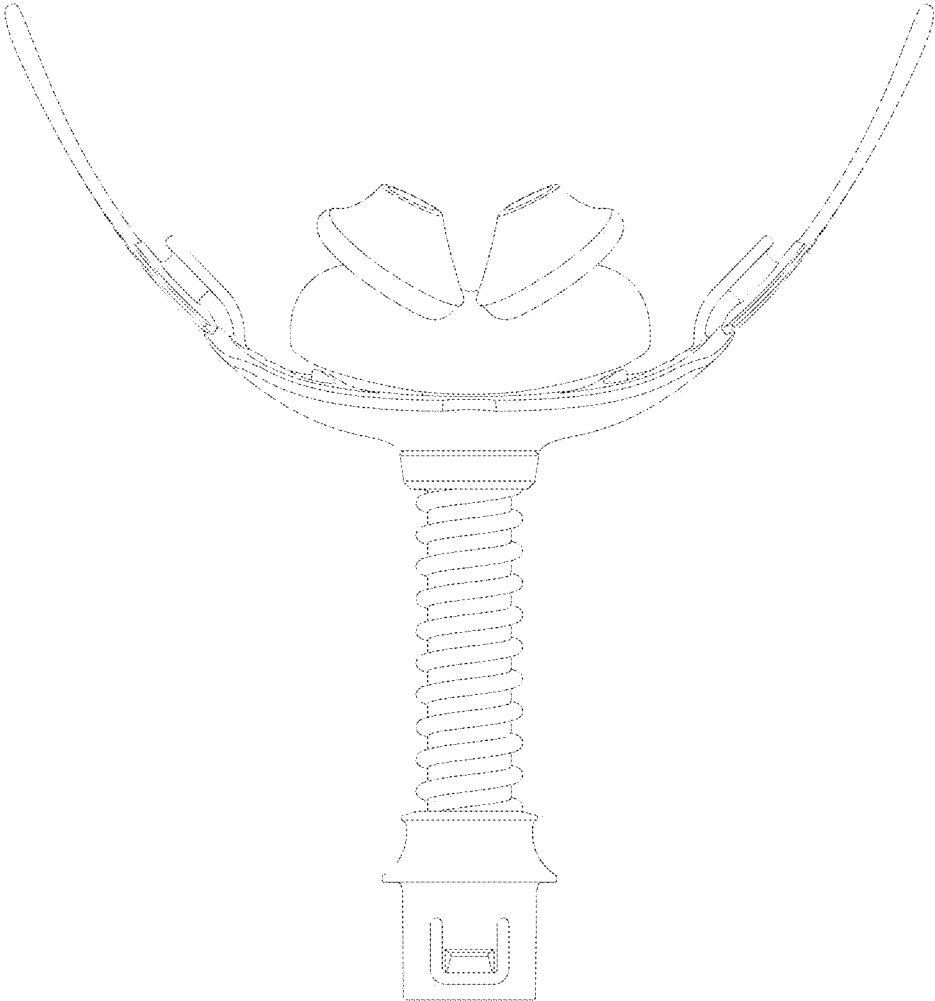


FIG. 3

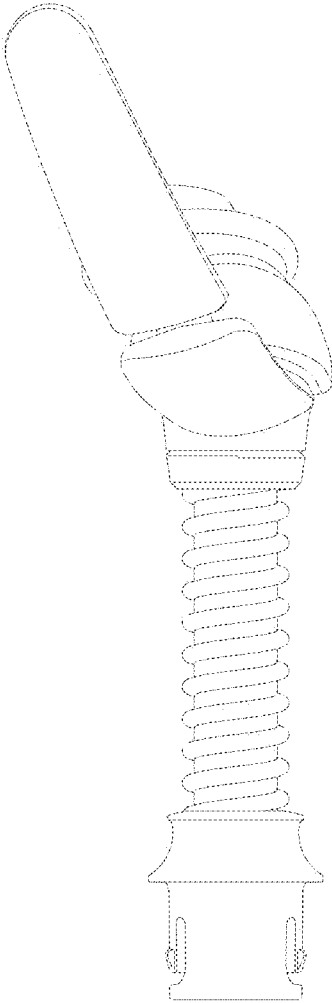


FIG. 4

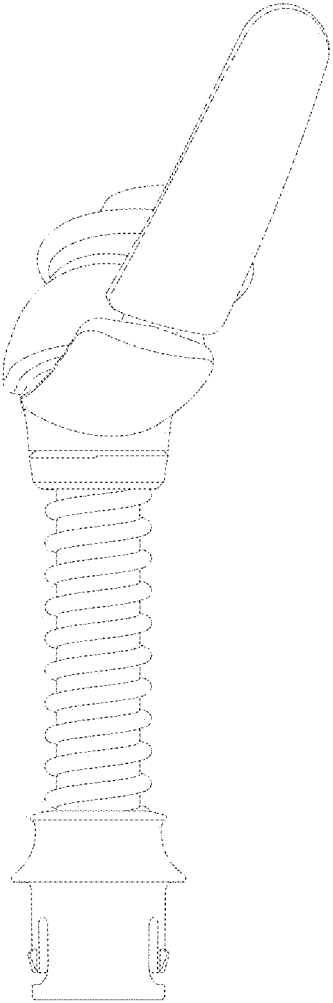


FIG. 5

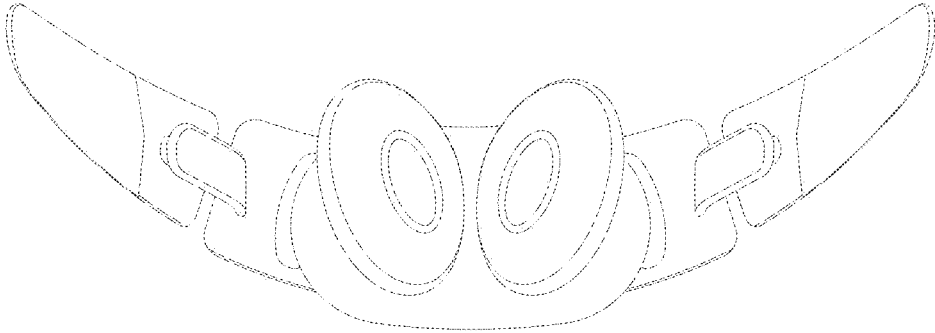


FIG. 6

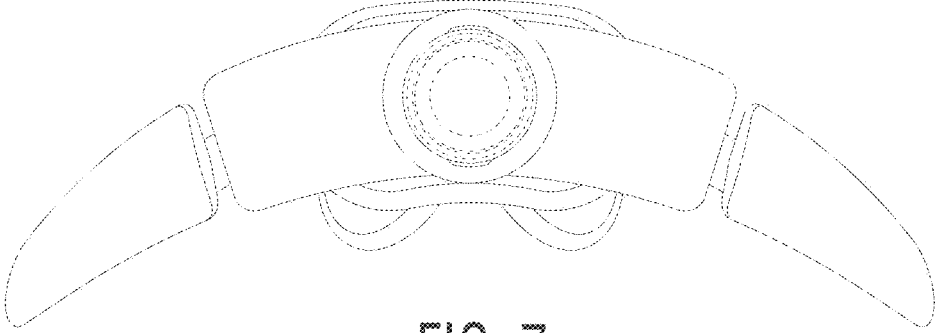


FIG. 7