

**(12) STANDARD PATENT**  
**(19) AUSTRALIAN PATENT OFFICE**

(11) Application No. **AU 2013336675 B2**

(54) Title  
**Crimping method for bioresorbable stents**

(51) International Patent Classification(s)  
**A61F 2/958** (2013.01) **A61F 2/915** (2013.01)

(21) Application No: **2013336675** (22) Date of Filing: **2013.10.24**

(87) WIPO No: **WO14/064183**

(30) Priority Data

(31) Number	(32) Date	(33) Country
<b>61/718,549</b>	<b>2012.10.25</b>	<b>US</b>

(43) Publication Date: **2014.05.01**

(44) Accepted Journal Date: **2017.10.26**

(71) Applicant(s)  
**Arterial Remodeling Technologies, SA**

(72) Inventor(s)  
**Vial, Beatrice;Van Der Leest, Machiel**

(74) Agent / Attorney  
**Davies Collison Cave Pty Ltd, Level 15 1 Nicholson Street, MELBOURNE, VIC, 3000, AU**

(56) Related Art  
**WO 2002/066095 A2**  
**US 2011/0295201 A1**  
**WO 2008/011028 A1**  
**US 2010/0063571 A1**  
**US 2012/0079706 A1**  
**US 2012/0010693 A1**  
**US 2012/0261858 A1**  
**US 8062465 B1**  
**US 6063092 A**  
**US 7731740 B2**



- (51) **International Patent Classification:**  
*A61F 2/958* (2013.01) *A61F 2/915* (2013.01)
- (21) **International Application Number:**  
PCT/EP2013/072247
- (22) **International Filing Date:**  
24 October 2013 (24.10.2013)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**  
61/718,549 25 October 2012 (25.10.2012) US
- (71) **Applicant:** ARTERIAL REMODELING TECHNOLOGIES, SA [FR/FR]; 3 rue de Verdun, F-78590 Noisy Le Roi (FR).
- (72) **Inventors:** VIAL, Béatrice; 16 rue du Château Grillot, F-70100 Chargey les Gray (FR). VAN DER LEEST, Machiel; 7 rue de l'Abbé de l'Epée, F-75005 Paris (FR).
- (74) **Agents:** STARCK-LOUDES, Anne-Caroline et al.; Becker & Associés, 25 rue Louis le Grand, F-75002 Paris (FR).
- (81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,


BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

**Published:**

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) **Title:** CRIMPING METHOD FOR BIORESORBABLE STENTS

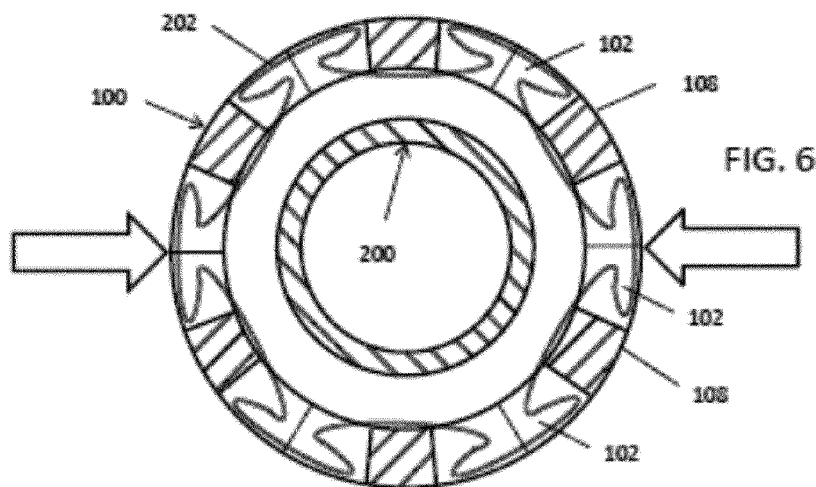

(57) **Abstract:** The present patent application relates to a method of crimping a tubular stent having a stent lumen onto an inflatable balloon of a stent delivery catheter.

## CRIMPING METHOD FOR BIORESORBABLE STENTS

### Field of the invention

5

The present invention relates to a method for crimping a vascular stent onto a stent delivery catheter. The crimping method disclosed is particularly advantageous for crimping a bioabsorbable or bioresorbable polymeric vascular stent onto an inflatable balloon of a stent delivery catheter.

10

### Background of the Invention

In recent decades, vascular stenting has become an important therapy for treating occlusive vascular disease, including coronary artery disease, carotid artery disease and peripheral artery disease. A stent, also known as a vascular scaffold, is a tubular structure that is used, sometimes in conjunction with an angioplasty balloon catheter, to open up a stenosis or narrowing in a blood vessel and to hold the blood vessel open to allow improved blood flow. Stents are also used to treat strictures or narrowings in body passages other than blood vessels. Vascular stents are typically grouped into two general categories: balloon expandable stents and self-expanding stents. The bioresorbable vascular stent used in the present invention can be considered to be a hybrid of these two types. The bioresorbable vascular stent is heat treated to have a shape memory that makes the stent expand toward its deployed diameter. This behavior is temperature dependent. Above the glass transition temperature  $T_g$  of the stent material, the stent expands quickly, but at body temperature, the stent expands more slowly. An inflatable balloon is therefore used to accelerate the deployment of the stent, but even after deployment, the stent will continue to expand slightly, which assists in apposing the stent struts to the vessel wall. The stent could therefore be considered to be a balloon-assisted self-expanding stent or a self-apposing balloon expandable stent. For the crimping process however, the bioresorbable vascular stent can be treated much like a balloon expandable stent.

30

Typically, a balloon expandable stent is mounted on a stent delivery catheter by crimping (i.e. squeezing) the stent onto an inflatable balloon located near the distal end of the catheter.

Specialized crimping devices and automated machines have been devised for crimping stents onto balloon catheters. See, for example: U.S. Patent 8,141,226; PCT International Application WO 2004/019768 and U.S. Patent Application 2002/0138966. Where allowed, these and all patents and patent applications referred to herein are hereby incorporated by reference. The stent crimping devices described in these patents can be modified for use with the crimping method of the present invention by adding controlled heating and cooling the crimp head.

Most balloon expandable stents used today are metal stents. However, there is an emerging field of bioabsorbable or bioresorbable polymeric vascular stents. The terms *bioabsorbable* and *bioresorbable* are used interchangeably in the medical device industry to describe a material that, after implantation in the body, breaks down over time and is absorbed or resorbed by the surrounding tissues. Typical materials for bioabsorbable or bioresorbable stents include polylactic acid (PLA) and polyglycolic acid (PGA) polyglactin (PLAGA copolymer). Additional stent materials suitable for the present invention are described in U.S. Patent 7,731,740 and PCT International Application WO 2005/096992. In general, a polymer with a glass transition temperature (T<sub>g</sub>) of at least 45°C is preferred.

Polymeric vascular stents present particular challenges in stent crimping. U.S. Patent 7,743,481 describes an apparatus and method that are particularly adapted for crimping polymeric vascular stents. This stent crimping apparatus can be modified for use with the crimping method of the present invention by adding controlled heating and cooling.

Various methods have been devised for crimping balloon expandable stents that involve a step of inflating the balloon on the catheter during the crimping process. Examples of these methods are described in the following and patent applications: U.S. Patent 5,836,965 (cf. FIG. 3); U.S. Patent 5,976,181; and U.S. Patent 8,123,793 (cf. FIG. 4).

Generally, the methods described in these patent references are not suitable for application to bioabsorbable or bioresorbable polymeric vascular stents. One fundamental difference between metallic stents and polymeric stents is that tubular metallic stents are typically fabricated at a diameter that is just slightly larger than their undeployed or crimped diameter. During the crimping step, the diameter of the stent only needs to be reduced by a small amount. Thus, when the balloon is inflated during the crimping process, it cannot assume its fully expanded diameter because it is constrained by the stent and the crimping apparatus. If

the balloon were to be fully inflated it would impart irreversible plastic deformation to the stent struts, which would be highly deleterious to the stent. On the other hand, tubular polymeric stents are fabricated at a diameter that is close to their deployed or fully expanded diameter. During the crimping process, the diameter of the stent must be reduced from the  
5 deployed or fully expanded diameter to the undeployed or crimped diameter. Elevating the temperature of the polymeric stent at or above  $T_g$  during crimping avoids the problem of irreversible plastic deformation that occurs with metallic stents. Because it takes into account these differences, the crimping method of the present invention is particularly advantageous for crimping a bioabsorbable or bioresorbable polymeric vascular stent onto an inflatable  
10 balloon of the stent delivery catheter.

### **Brief description of the drawings**

FIGURE 1 (FIG. 1) is a photograph of a bioresorbable polymeric vascular stent crimped onto  
15 the balloon of a stent delivery catheter according to the method of the present invention.

FIGURE 2 (FIG. 2) is an enlarged detail photograph of a proximal portion of the inflatable balloon and the vascular stent of FIG. 1, showing a bumper at the balloon cone level that is formed during the crimping process.

20

FIGURE 3 (FIG. 3) is a cross section of a stent crimped onto the balloon of a stent delivery catheter using a prior art crimping method according to U.S. Patent 5,836,965.

FIGURE 4 (FIG. 4) is a cross section of a stent crimped onto the balloon of a stent delivery  
25 catheter using another prior art crimping method according to U.S. Patent 8,123,793.

FIGURE 5 (FIG. 5) is a cross section showing the balloon inflation step of the stent crimping method of the present invention.

30 FIGURE 6 (FIG. 6) is a cross section showing the crimping step of the stent crimping method of the present invention.

FIGURE 7 (FIG. 7) is a cross section photograph showing the final result of the stent crimping method of the present invention.

FIGURE 8 (FIG. 8) is a photograph of a deployed bioresorbable polymeric vascular stent.

FIGURE 9 (FIG. 9) illustrates a deployed vascular stent that was previously crimped  
5 according to prior art methods. The stent is laid out flat to show the uneven deployment of the stent.

FIGURE 10 (FIG. 10) illustrates a deployed vascular stent that was previously crimped  
10 according to the stent crimping method of the present invention. The stent is laid out flat to show the even deployment of the stent.

### **Brief description of the invention**

Inventors herein provide a method of crimping a tubular stent having a stent lumen onto an  
15 inflatable balloon of a stent delivery catheter, the stent having a deployed diameter and a crimped diameter that is smaller than the deployed diameter. This method comprises:

- inserting the inflatable balloon of the stent delivery catheter into the stent lumen of the tubular stent with the inflatable balloon at a deflated diameter and with the tubular stent at approximately the deployed diameter;
- 20 - inflating the inflatable balloon of the stent delivery catheter to an inflated diameter within the stent lumen of the tubular stent;
- crimping the tubular stent to the crimped diameter while maintaining inflation pressure within the inflatable balloon of the stent delivery catheter; and
- deflating the inflatable balloon of the stent delivery catheter while maintaining the tubular  
25 stent at the crimped diameter.

The herein described method can further comprise a step of heating the tubular stent to a temperature at or above the glass transition temperature prior to the crimping step and/or a step of cooling the tubular stent to a temperature below the glass transition temperature after  
30 the crimping step.

In a particular embodiment of the present invention, the inflatable balloon of the stent delivery catheter is inflated within the stent lumen of the tubular stent with an inflation pressure typically between 0.1 to 5 bars or 0.1 to 2.5 bars, preferably of approximately 0.2 to

2.0 bars, prior to the crimping step of the method according to the present invention and maintained at this inflation pressure during the crimping step. Preferably, the method further comprises after the crimping step and prior to the deflating step, a step of increasing the inflation pressure of the inflatable balloon of the stent delivery catheter within the stent lumen  
5 of the tubular stent to an inflation pressure of approximately 3.0 to 7.0 bars while maintaining the tubular stent at the crimped diameter.

In another particular embodiment of the present invention, the method of the invention further comprises prior to inserting the inflatable balloon of the stent delivery catheter into the stent  
10 lumen of the tubular stent, a step of inserting the tubular stent into a crimping machine at approximately the deployed diameter and a step of precrimping the tubular stent to a precrimped diameter that is slightly smaller than the deployed diameter. This method can further comprise after the deflating step, a step of removing the tubular stent and the inflatable balloon of the stent delivery catheter from the crimping machine.

15 A preferred method of the invention comprises:

- prior to inserting the inflatable balloon of the stent delivery catheter into the stent lumen of the tubular stent, inserting a tubular stent formed from a polymer having a glass transition temperature into a crimping machine at approximately the deployed diameter and precrimping  
20 the tubular stent to a precrimped diameter that is slightly smaller than the deployed diameter;
- prior to the crimping step, heating the tubular stent to a temperature at or above the glass transition temperature;
- prior to the crimping step, inflating the inflatable balloon of the stent delivery catheter within the stent lumen of the tubular stent with an inflation pressure typically between 0.1 to  
25 2.5 bars, preferably of approximately 0.2 to 2.0 bars and maintaining this inflation pressure during the crimping step;
- after the crimping step and prior to the deflating step, increasing the inflation pressure of the inflatable balloon of the stent delivery catheter within the stent lumen of the tubular stent to an inflation pressure of approximately 3.0 to 7.0 bars while maintaining the tubular stent at  
30 the crimped diameter and cooling the tubular stent to a temperature below the glass transition temperature; and
- after the deflating step, removing the tubular stent and the inflatable balloon of the stent delivery catheter from the crimping machine.

Another aspect of the invention is an apparatus comprising:

- a tubular stent having a multiplicity of stent struts arranged around a stent lumen of the tubular stent and a multiplicity of interstices between the stent struts, the tubular stent being positioned at an undeployed, crimped diameter; and

- an inflatable balloon positioned within the stent lumen of the tubular stent, the inflatable balloon being positioned at an undeployed, deflated diameter with a wall material of the inflatable balloon arranged into a multiplicity of folds;

wherein the multiplicity of stent struts are evenly distributed around a circumference of the tubular stent and the wall material of the inflatable balloon is evenly distributed around the circumference of the tubular stent.

In the previously described apparatus, the wall material of the inflatable balloon can protrude into the multiplicity of interstices between the stent struts.

In a particular embodiment of the invention, an approximately equal amount of the wall material of the inflatable balloon protrudes into each the multiplicity of interstices between the stent struts.

In another particular embodiment of the invention, the stent can have a proximal end and a distal end and the wall material of the inflatable balloon can be configured to form a proximal bumper of increased diameter positioned beyond the proximal end of the stent and a distal bumper of increased diameter positioned beyond the distal end of the stent.

The multiplicity of stent struts can be each in contact with the wall material of the inflatable balloon. The multiplicity of stent struts can also be configured i) to enclose a multiplicity of closed cells arranged around a circumference of the tubular stent or ii) to enclose a multiplicity of closed cells arranged in rings around a circumference of the tubular stent, a plurality of linking struts connecting adjacent rings of closed cells.

The tubular stent used in the context of the invention typically comprises a bioresorbable material, preferably a bioresorbable polymer. The tubular stent is advantageously formed from a material having a glass transition temperature ( $T_g$ ), advantageously a glass transition temperature ( $T_g$ ) of at least 45°C. Preferably the tubular stent comprises a poly (lactic acid) polymer. Preferably the tubular stent comprises an antiproliferative agent.



## Detailed description of the invention

A prior art method used by applicant for crimping a PLA bioresorbable stent on a semicompliant angioplasty balloon includes the following steps:

1. Loading the PLA stent in a preheated stainless steel crimp head (at or above the polymer glass transition temperature  $T_g$ ) at a pre-crimp diameter of approximately 0.2 mm less than the PLA stent cut component diameter;
2. After a preheating period, the PLA stent diameter is reduced to and maintained at crimp diameter;
3. Immediately after reaching crimp diameter, the PLA stent is cooled down to below  $T_g$  (typically to room temperature) while increasing the balloon pressure, preferably between approximately 3.0 to 7.0 bars, to create bumpers at the balloon cone level.

By contrast, the improved crimping method of the present invention includes the following steps:

1. Loading the PLA stent in a preheated stainless steel crimp head (at or above the polymer glass transition temperature  $T_g$ );
2. Precrimping the stent to a diameter of approximately 0.2 mm less than the PLA stent cut component diameter (which is just enough to grip the stent within the crimp head);
3. After a time delay of approximately 30-180 seconds to allow the stent material to heat up in the crimp head, inserting the balloon of a stent delivery catheter into the lumen of the stent and fully inflating the balloon at a low pressure typically between approximately 0.2 to 5.0 bars (for example 1, 2, 3 or 4 bars), preferably between approximately 0.2 to 2.0 bars;
4. After a sufficient preheating period to heat the stent material to at or above the polymer glass transition temperature  $T_g$ , reducing the diameter of the PLA stent together with the inflated balloon using the crimp head and maintaining the stent at the crimped diameter;
5. Immediately after reaching the crimped diameter, cooling the PLA stent down to below  $T_g$  (typically to room temperature) while increasing the balloon pressure, preferably between approximately 3.0 to 7.0 bars, to create bumpers at the balloon cone level; and
6. Releasing the pressure in the balloon and removing the stent delivery catheter with the stent crimped on the balloon from the crimp head.

The improved crimping method provides a number of advantages over the prior art:

1. Significantly increased stent retention;
2. Increased homogeneity of the crimped stent since the inflated balloon guides the PLA stent in a rubbery state (at around  $T_g$ ), resulting in fewer defects due to crimping;
3. Improved stent expansion since the balloon is pre-fit (in phase) to the final stent diameter
- 5 leading to an increased homogeneity of the expanded stent;
4. Improved guidance of the crimped stent while tracking as the balloon penetrates in between stent struts;
5. Significantly increased tracking time in the artery vasculature over 30 minutes, which is important because, as noted above, PLA stents begin to slowly expand when heated up to
- 10 body temperature ( $37^\circ\text{C}$ ).

FIGS. 8 and 10 illustrate a vascular stent 100 suitable for use with the crimping method of the present invention. The stent 100 is generally manufactured in a tubular configuration, as shown in FIG. 8, but FIG. 10 has been drawn as if the stent 100 has been cut longitudinally

15 along line 1–1 and laid out flat to more clearly illustrate the structure of the stent 100. Preferably, the stent 100 is made from a bioabsorbable or bioresorbable polymer having a  $T_g$  of at least  $45^\circ\text{C}$ . The stent 100 can be manufactured in a many different possible designs. This illustrative embodiment shows a stent 100 with a combination of closed cells 102 for structural strength in the circumferential direction (i.e. radial strength) and open cells 104 for

20 flexibility in the longitudinal direction. Each of the closed cells 102 is bordered by four approximately-linear struts 108 whose ends are joined together to form a diamond, rhombus or lozenge-shaped cell 102. The illustrated stent 100 has six cells 102 in the circumferential direction and four cells 102 in the longitudinal direction. This stent configuration can be envisioned as having four circumferential rings with six closed cells 102 each, which are

25 joined by two linking struts 106 between each pair of adjacent rings. Many other stent, cell and strut configurations are possible. Optionally, the stent 100 may include one or more radiopaque markers 120. Furthermore, the bioresorbable stent may optionally include an antiproliferative agent, such as paclitaxel, sirolimus (rapamycin) or another limus-family drug, in the form of a coating or compounded into the polymer for extended release.

30

FIG. 1 is a photograph of a bioresorbable polymeric vascular stent 100 crimped onto the balloon 202 of a stent delivery catheter 200 utilizing the method of the present invention.

FIG. 2 is an enlarged detail photograph of a proximal portion of the inflatable balloon 202 and

the vascular stent 100 of FIG. 1, showing a proximal bumper 204 and a distal bumper 206 that are formed at the proximal and distal cone portions of the inflatable balloon 202 during the second inflation step of the crimping process. The proximal bumper 204 and distal bumper 206 help to retain the stent 100 on the stent delivery catheter 200 during insertion and advancement of the catheter 200.

FIG. 3 is a cross section of a metallic stent 4 that was crimped onto the balloon 202 of a stent delivery catheter 200 using a prior art crimping method according to U.S. Patent 5,836,965. It is evident that the balloon 202 was folded into wings prior to partially inflating the balloon 202 inside the stent 4 during crimping. Note that the balloon material 202 is not evenly distributed in between the stent struts 108. In some of the interstices between stent struts 108 there is a great deal of redundancy of balloon material 210, whereas in other interstices between stent struts 108 there is essentially no redundancy of balloon material 212. The uneven distribution of the balloon material 202 in between the stent struts 108 can lead to uneven deployment of the stent 4 when the balloon 202 is inflated.

FIG. 4 is a cross section of a metallic stent 12 that was crimped onto the balloon 202 of a stent delivery catheter 200 using another prior art crimping method according to U.S. Patent 8,123,793. In this example, the balloon 202 is irregularly folded underneath the stent 12. As in the above example, the balloon material 202 is not evenly distributed in between the stent struts 108. In some of the interstices between stent struts 108 there is a great deal of redundancy of balloon material 210, whereas in other interstices between stent struts 108 there is essentially no redundancy of balloon material 212. Also note that some of the stent struts 108 are in contact with the balloon material, while others 108' are not. The uneven distribution of the balloon material 202 in between the stent struts 108 can lead to uneven deployment of the stent 100 when the balloon 202 is inflated.

FIG. 9 illustrates a deployed vascular stent 100' that was previously crimped according to prior art methods, such as the examples described above. The stent 100' is laid out flat to show the uneven deployment of the stent 100'. The upper portion 160 represents an area of the stent 100' where there was not enough redundancy of balloon material between stent struts, which causes this area of the stent to be underdeployed. The lower portion 162 represents an area of the stent where there was too much redundancy of balloon material between stent struts, which causes this area of the stent to be overdeployed or overstretched.

Uneven deployment of the stent can compromise the structural strength of the stent 100'. For drug eluting stents, uneven deployment of the stent can cause additional problems. Some areas of the vascular wall where the stent is underdeployed can receive too much antiproliferative drug per surface area, whereas other areas of the vascular wall where the stent is overdeployed may not receive enough of the antiproliferative drug per surface area.

FIG. 5 is a cross section showing the balloon inflation step of the stent crimping method of the present invention. Note that the stent 100 is at or very close to the fully deployed diameter of the stent 100 and the inflated balloon 202 is also at or very close to its nominal inflated diameter. The balloon material 202 is in-phase with the stent struts 108, that is, the balloon material 202 is evenly distributed in between the stent struts 108. Another way to describe this is that there is a 1-to-1 mapping between the balloon material and the circumference of the stent.

FIG. 6 is a cross section showing the crimping step of the stent crimping method of the present invention. During the crimping step, the inflated balloon 202 guides the stent struts 108 from the as-cut stent diameter to the crimped stent diameter and assures an evenly spaced crimped configuration. Note that, during the crimping step, the balloon material 202 remains in-phase with the stent struts 108 and that, although there is redundancy of balloon material 202, the balloon material 202 is evenly distributed in between the stent struts 108. The 1-to-1 mapping between the balloon material and the circumference of the stent is maintained as the diameter of the stent is reduced by crimping. The inflation pressure inside the balloon causes the balloon material 202 to protrude between the stent struts 108 as the diameter of the stent 100 is reduced.

FIG. 7 is a cross section photograph showing the final result of the stent crimping method of the present invention. Each of the stent struts 108 is in contact with the balloon material 202 and the balloon material 202 is evenly distributed in between the stent struts 108. The protrusion or interdigitation of the balloon material 202 between the struts 108 of the stent greatly increases the retention strength of the stent 100 on the stent delivery catheter 200, which is very important for successful delivery and deployment of the stent 100 in a patient's blood vessel. The balloon 202 with the stent 100 crimped onto it has been inserted into a tubular protection sleeve 220 that protects the assembly during packaging, sterilization and handling. In use, the stent delivery catheter 200 is inserted into the patient's vasculature to

2013336675 09 Oct 2017

5 deliver the stent 100 to a stenosis or narrowing in an artery or other vessel. The balloon 202 is inflated to expand the stent 100 and appose it to the vessel wall. The balloon 202 is then deflated and the catheter 200 is withdrawn. The expanded stent 100 holds open the previously stenosed portion of the artery. However, the material of the stent 100 gradually decomposes over a period of months and is resorbed by the surrounding tissues, thus allowing the artery to remodel and return to its normal function. The bioresorbable stent does not leave behind a large amount of foreign material that might cause inflammation, which could lead to restenosis or late stent thrombosis.

0 FIG. 8 is a photograph of a deployed bioresorbable polymeric vascular stent 100 that was previously crimped according to the stent crimping method of the present invention. FIG. 10 illustrates the deployed vascular stent 100 of FIG. 8 with the stent laid out flat to show the even deployment of the stent 100. The stent struts 108 are evenly distributed around the surface area of the stent 100. In contrast to the prior art stent 100' of FIG. 9, the upper portion 5 160 and lower portion 162 of the stent 100 are evenly deployed. If the stent 100 is a drug eluting stent, the antiproliferative drug will be evenly distributed around the inner surface of the vascular wall as well.

0 Throughout this specification and the claims which follow, unless the context requires otherwise, the word "comprise", and variations such as "comprises" and "comprising", will be understood to imply the inclusion of a stated integer or step or group of integers or steps but not the exclusion of any other integer or step or group of integers or steps.

25 The reference in this specification to any prior publication (or information derived from it), or to any matter which is known, is not, and should not be taken as an acknowledgment or admission or any form of suggestion that that prior publication (or information derived from it) or known matter forms part of the common general knowledge in the field of endeavour to which this specification relates.

**THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:**

1. A method of crimping a bioresorbable polymeric tubular stent having a stent lumen onto an inflatable balloon of a stent delivery catheter, the stent having a multiplicity of stent struts evenly distributed around the stent lumen and a multiplicity of interstices between the stent struts, and the stent having a deployed diameter and a crimped diameter that is smaller than the deployed diameter, the bioresorbable polymer having a glass transition temperature (Tg), the inflatable balloon having a wall material arranged into a multiplicity of folds and evenly distributed around the stent lumen, and the method comprising in the following order:
  - inserting the inflatable balloon of the stent delivery catheter into the stent lumen of the tubular stent with the inflatable balloon at a deflated diameter and with the tubular stent at approximately the deployed diameter;
  - heating the tubular stent to a temperature at or above the glass transition temperature of the bioresorbable polymer;
  - inflating the inflatable balloon of the stent delivery catheter to an inflated diameter within the stent lumen of the tubular stent with an inflation pressure between 0.1 to 5 bars ;
  - crimping the tubular stent from the deployed diameter to the crimped diameter while maintaining the inflation pressure within the inflatable balloon of the stent delivery catheter; cooling the tubular stent to a temperature below the glass transition temperature while maintaining or increasing the inflation pressure within the inflatable balloon of the stent delivery catheter; and
  - deflating the inflatable balloon of the stent delivery catheter while maintaining the tubular stent at the crimped diameter.
2. The method of claim 1, wherein the tubular stent comprises a poly (lactic acid) polymer.
3. The method of claim 1 or claim 2, further comprising after the crimping step and prior to the deflating step, increasing the inflation pressure of the inflatable balloon of the stent delivery catheter within the stent lumen of the tubular stent to an inflation

pressure of approximately 3.0 to 7.0 bars while maintaining the tubular stent at the crimped diameter.

4. The method of any one of claims 1-3, further comprising prior to inserting the inflatable balloon of the stent delivery catheter into the stent lumen of the tubular stent, inserting the tubular stent into a crimping machine at approximately the deployed diameter and precrimping the tubular stent to a precrimped diameter that is slightly smaller than the deployed diameter.
5. The method of claim 4, further comprising after the deflating step, removing the tubular stent and the inflatable balloon of the stent delivery catheter from the crimping machine.
6. The method of claim 1, wherein the tubular stent is formed from a bioresorbable polymer having a glass transition temperature and wherein the method further comprises:
  - prior to inserting the inflatable balloon of the stent delivery catheter into the stent lumen of the tubular stent, inserting the tubular stent into a crimping machine at approximately the deployed diameter and precrimping the tubular stent to a precrimped diameter that is slightly smaller than the deployed diameter;
  - prior to the crimping step, heating the tubular stent to a temperature at or above the glass transition temperature;
  - prior to the crimping step, inflating the inflatable balloon of the stent delivery catheter within the stent lumen of the tubular stent with an inflation pressure of approximately 0.2 to 2.0 bars and maintaining this inflation pressure during the crimping step;
  - after the crimping step and prior to the deflating step, increasing the inflation pressure of the inflatable balloon of the stent delivery catheter within the stent lumen of the tubular stent to an inflation pressure of approximately 3.0 to 7.0 bars while maintaining the tubular stent at the crimped diameter and cooling the tubular stent to a temperature below the glass transition temperature; and
  - after the deflating step, removing the tubular stent and the inflatable balloon of the stent delivery catheter from the crimping machine.

7. The method of claim 6, wherein the tubular stent comprises a poly (lactic acid) polymer.



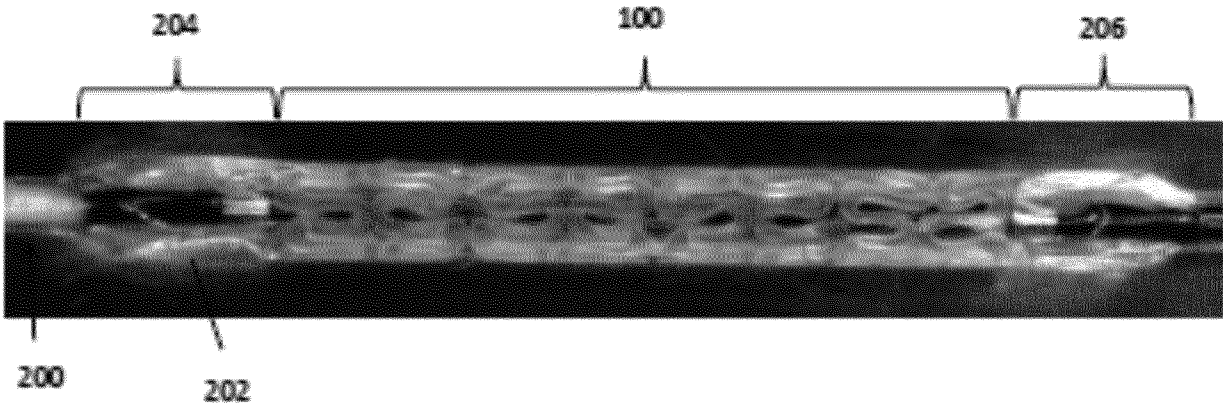


FIG. 1





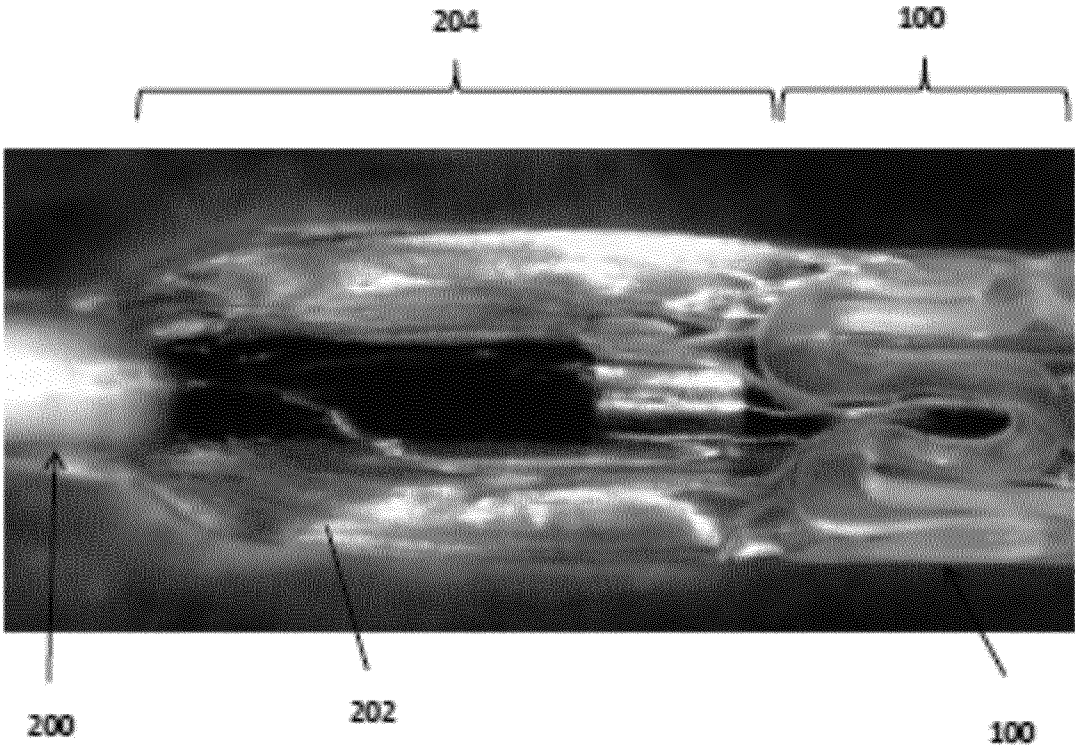


FIG. 2

2/5

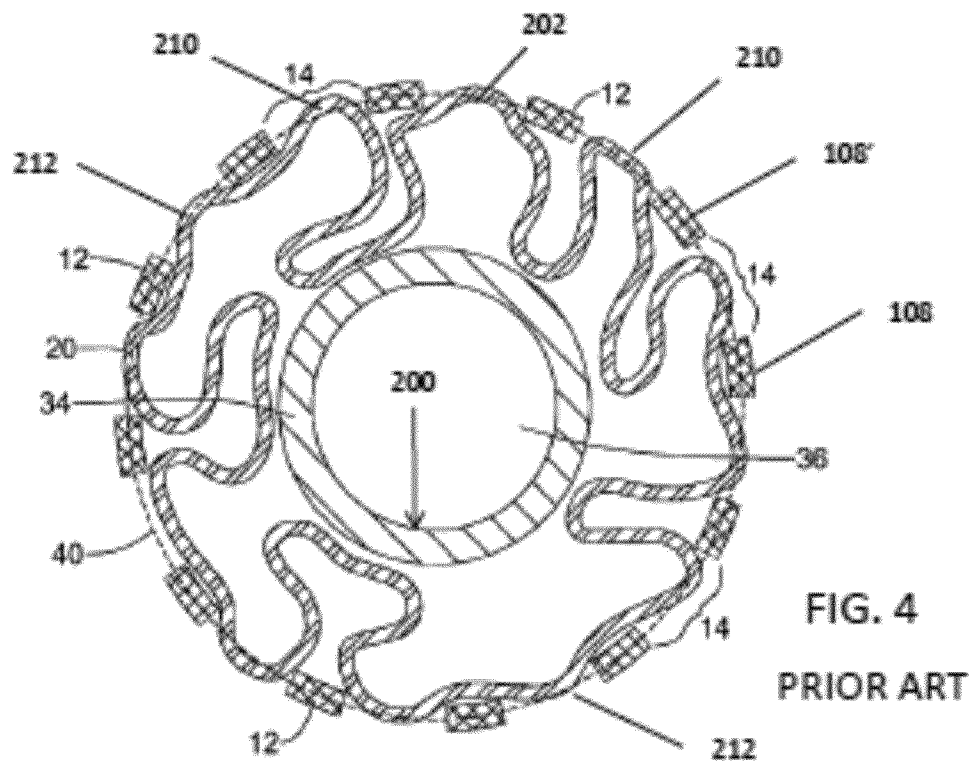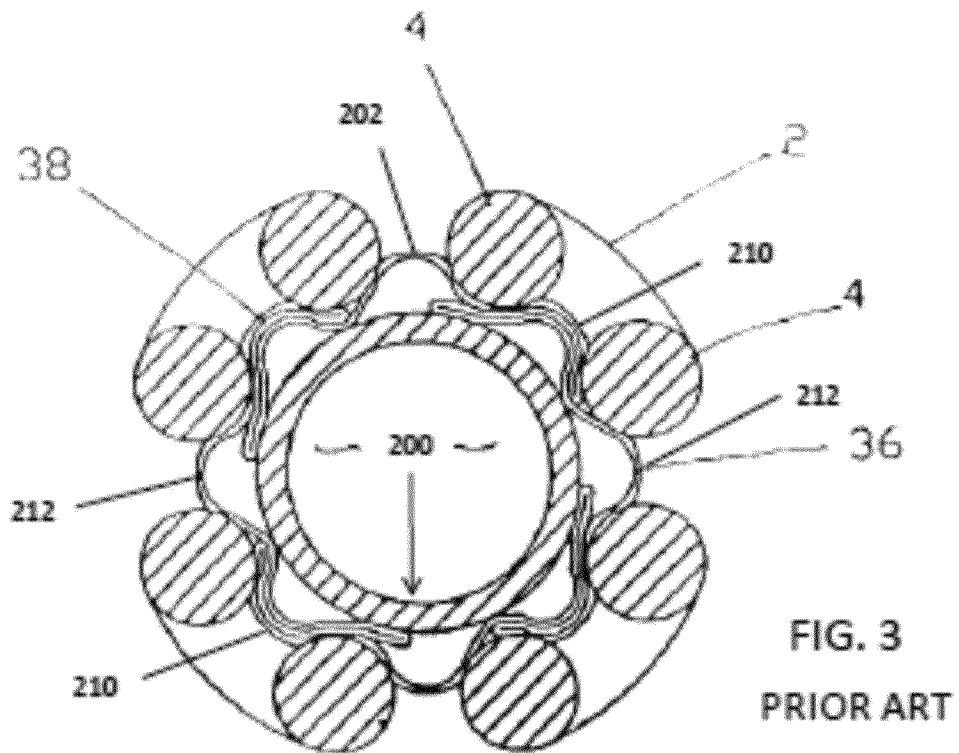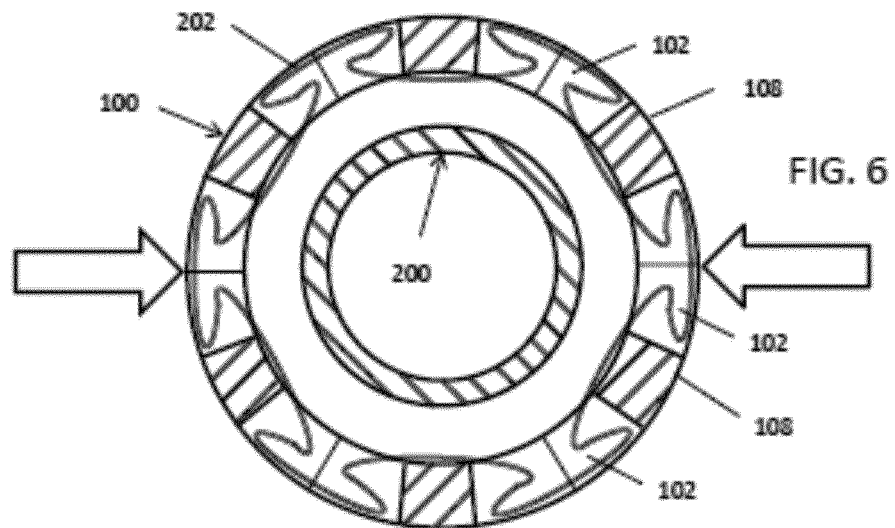

3/5

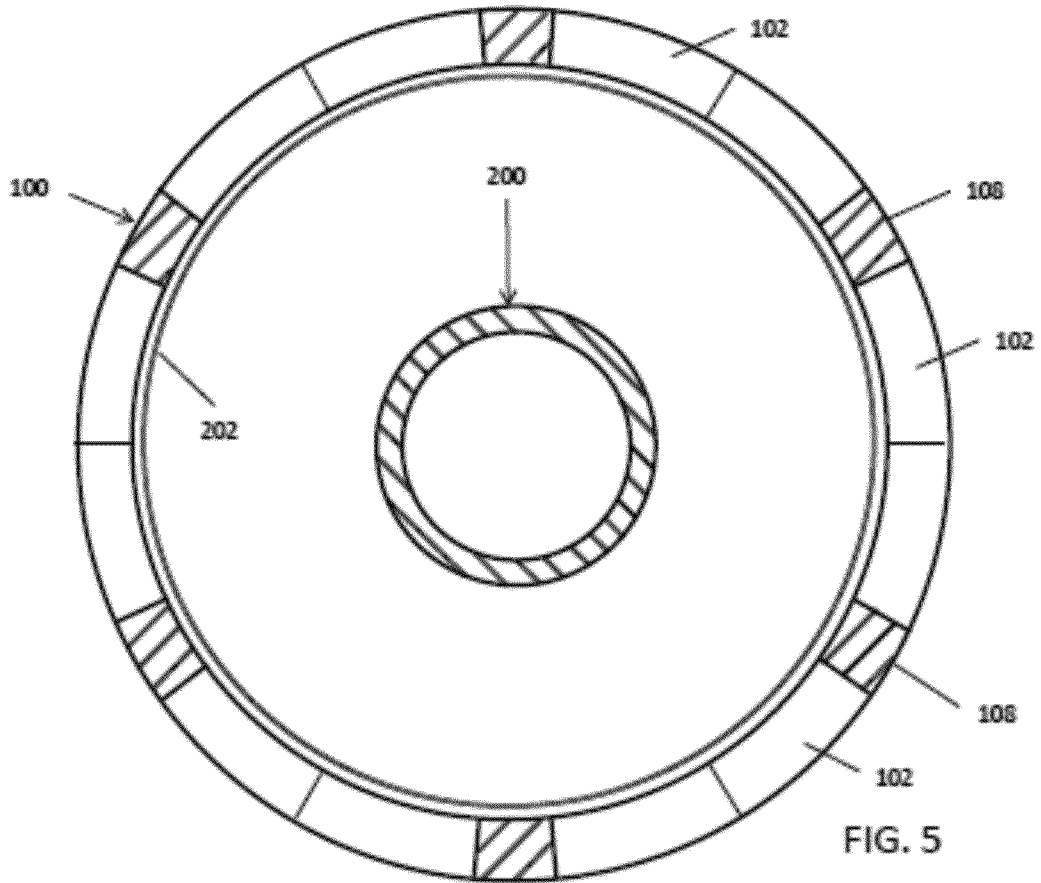

4/5

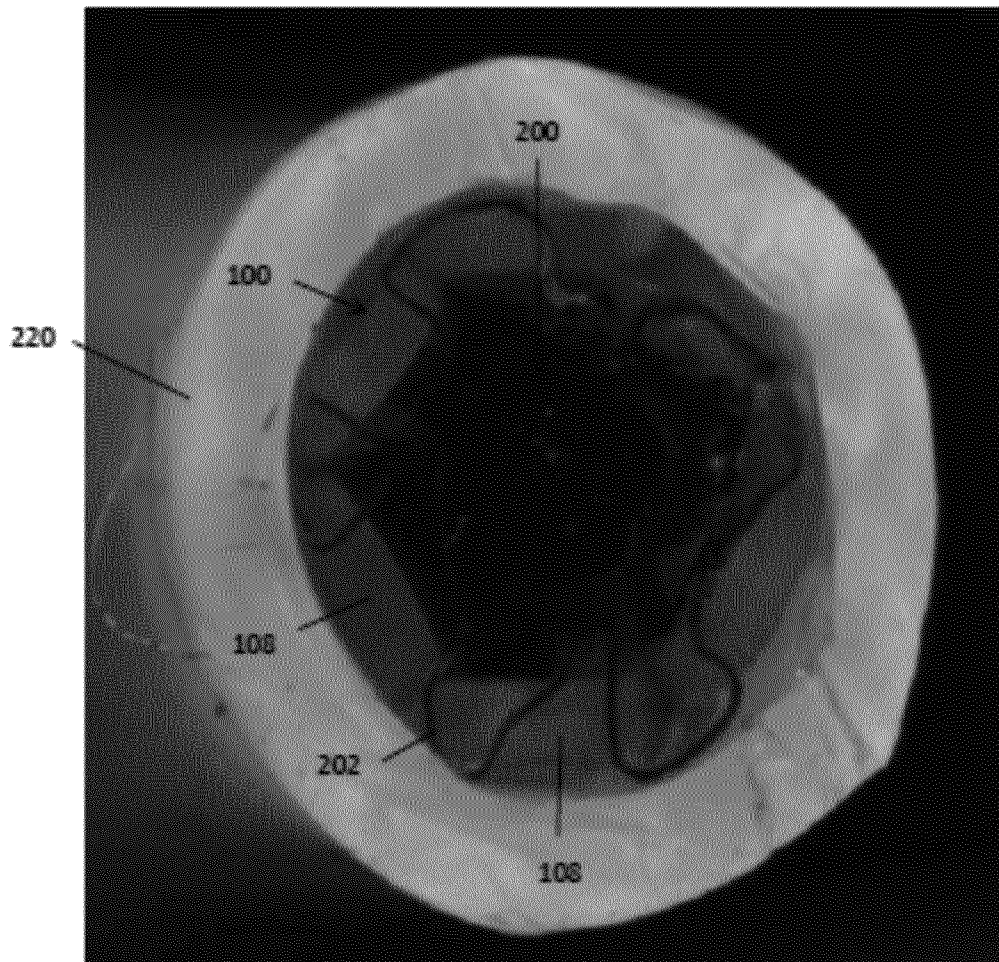


FIG. 7

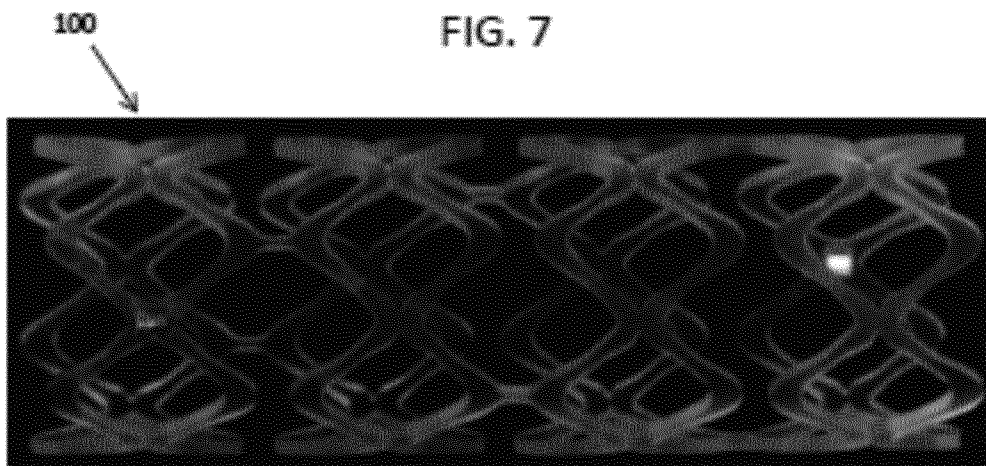


FIG. 8

5/5

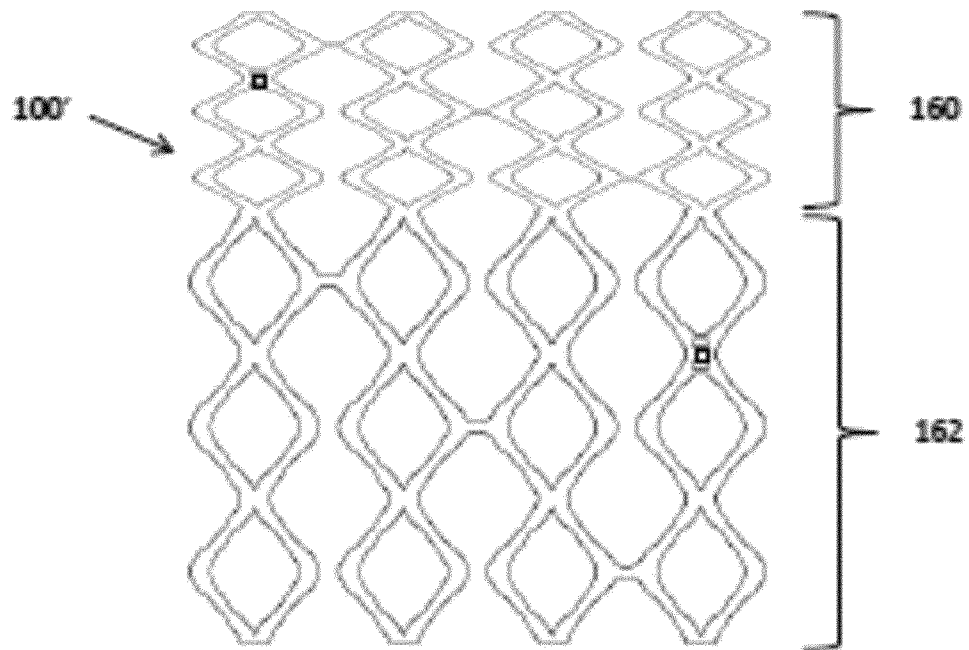


FIG. 9  
PRIOR ART

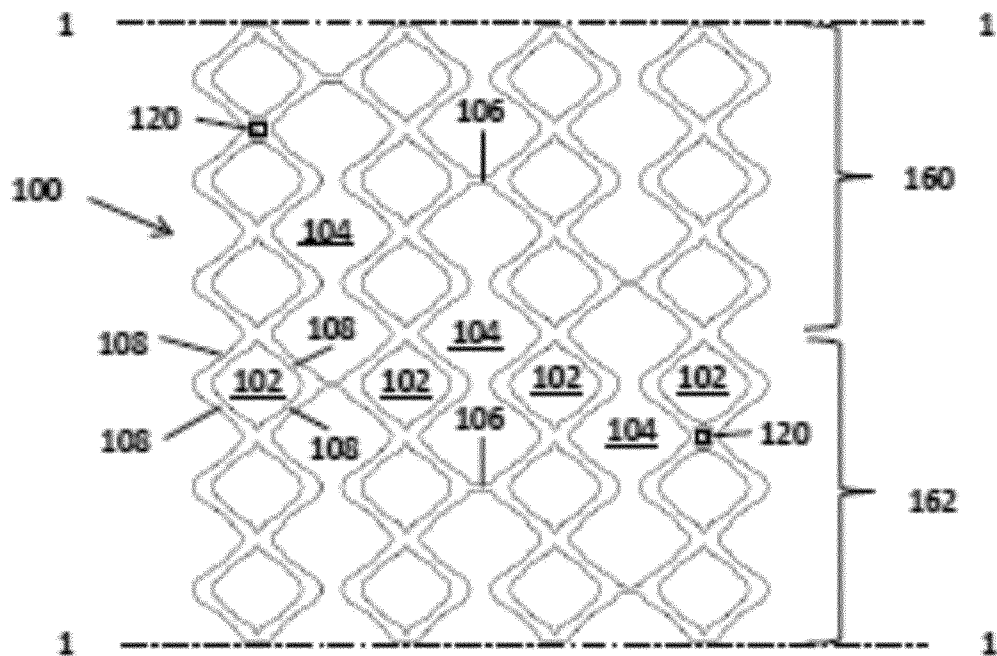


FIG. 10