



(22) Date de dépôt/Filing Date: 1992/07/14

(41) Mise à la disp. pub./Open to Public Insp.: 1993/02/17

(45) Date de délivrance/Issue Date: 2003/04/01

(30) Priorité/Priority: 1991/08/16 (746,446) US

(51) Cl.Int.⁵/Int.Cl.⁵ A61F 9/00


(72) Inventeur/Inventor:
SHIMMICK, JOHN, US

(73) Propriétaire/Owner:
VISX, INCORPORATED, US

(74) Agent: KIRBY EADES GALE BAKER

(54) Titre : METHODE ET APPAREIL PERMETTANT D'APPORTER SIMULTANEMENT DES CORRECTIONS
CYLINDRIQUES ET SPHERIQUES A LA CORNEE

(54) Title: METHOD AND APPARATUS FOR COMBINED CYLINDRICAL AND SPHERICAL EYE CORRECTIONS

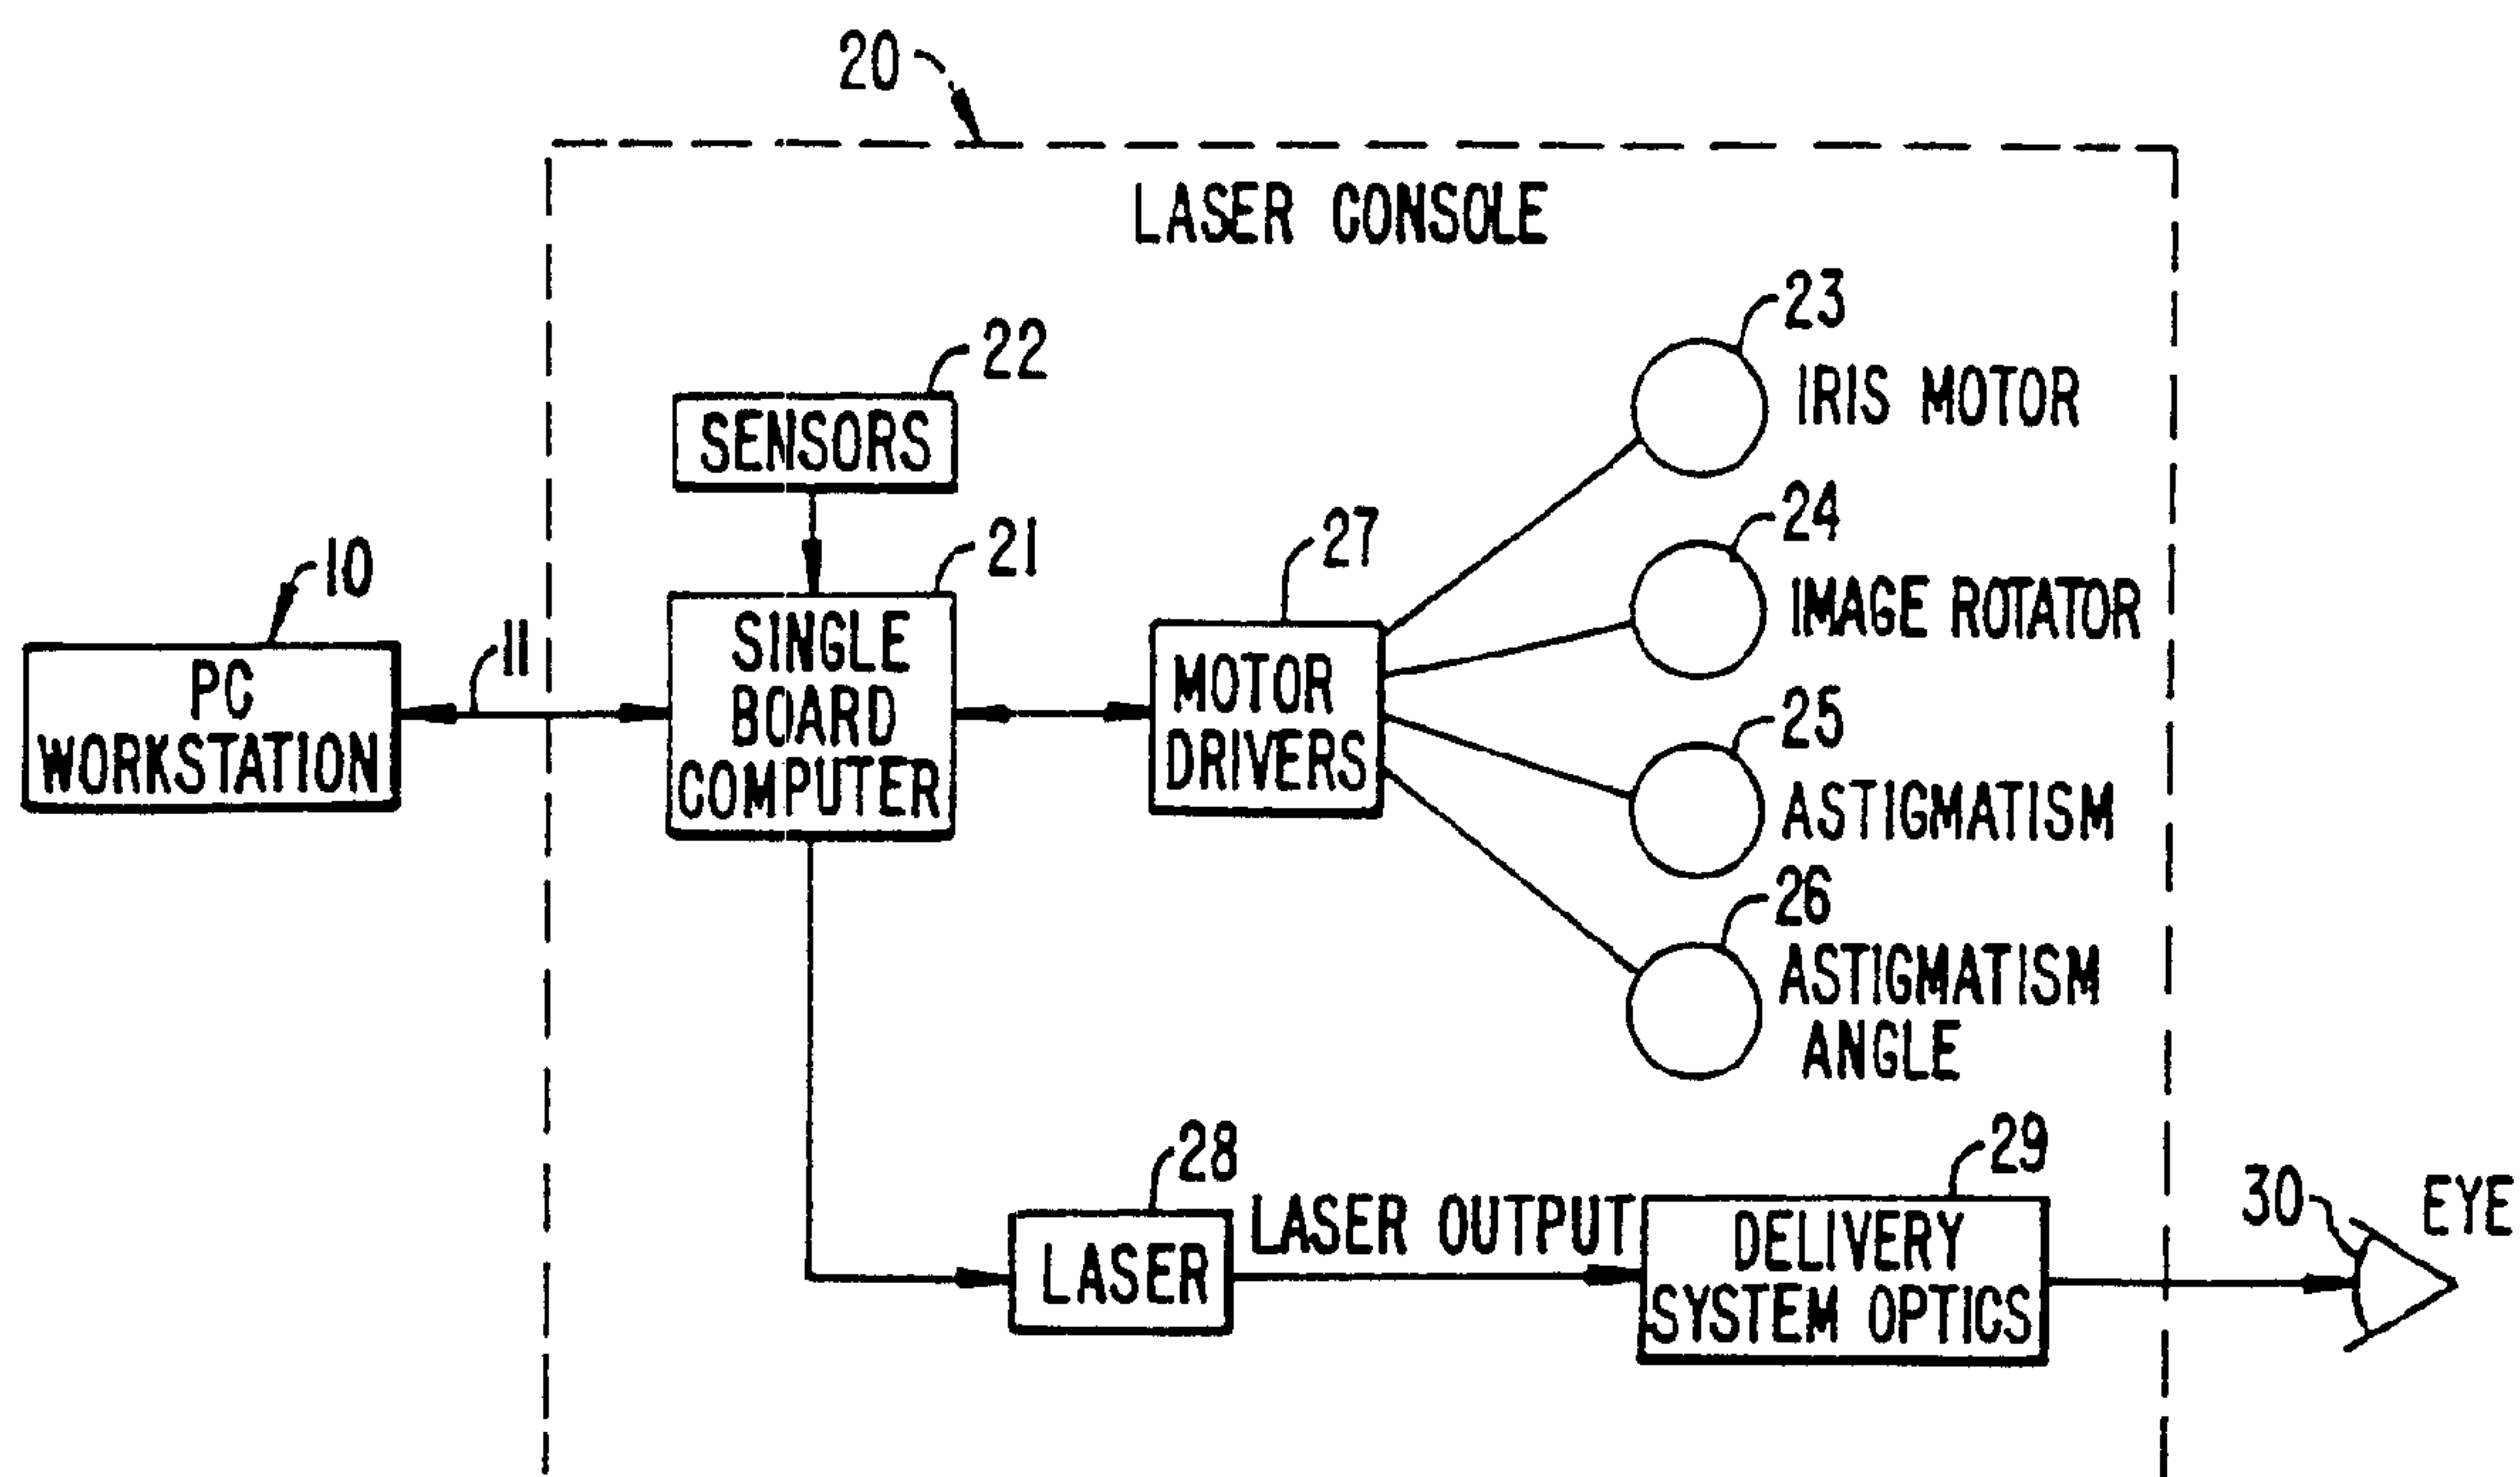

(57) Abrégé/Abstract:

A method for performing concurrent spherical and cylindrical corrections to the corneal surface of the eye to reduce myopia and astigmatism. A laser beam irradiates the corneal surface via a variable diameter iris and a slot produced by a pair of translatable blades. The width of the slot and the diameter of the iris are varied as the laser is pulsed to produce a toric ablation of the corneal surface. Alternatively, the laser beam is passed through a succession of apertures in a tilted variable aperture element to produce toric ablation. The total number of laser pulses required to effect both types of correction is equal to the number required for the spherical correction alone, reducing the laser power and the procedure time. The toric ablation produces no steep end walls as with standard cylindrical ablation procedures, thereby eliminating hyperopic shift and minimizing flattening along the ablated cylinder axis.



ABSTRACT OF THE DISCLOSURE

A method for performing concurrent spherical and cylindrical corrections to the corneal surface of the eye to reduce myopia and astigmatism. A laser beam irradiates the corneal surface via a variable diameter iris and a slot produced by a pair of translatable blades. The width of the slot and the diameter of the iris are varied as the laser is pulsed to produce a toric ablation of the corneal surface. Alternatively, the laser beam is passed through a succession of apertures in a tilted variable aperture element to produce toric ablation. The total number of laser pulses required to effect both types of correction is equal to the number required for the spherical correction alone, reducing the laser power and the procedure time. The toric ablation produces no steep end walls as with standard cylindrical ablation procedures, thereby eliminating hyperopic shift and minimizing flattening along the ablated cylinder axis.

METHOD AND APPARATUS FOR COMBINED CYLINDRICAL
AND SPHERICAL EYE CORRECTIONS

5

BACKGROUND OF THE INVENTION

This invention relates to ophthalmological surgery techniques which employ an ultraviolet laser used to provide photodecomposition of the surface of the cornea in order to correct vision defects.

10

Ultraviolet laser based systems and methods are known for enabling ophthalmological surgery on the surface of the cornea in order to correct vision defects by the technique known as ablative photodecomposition. In such such systems and methods, the irradiated flux density and exposure time of the cornea to the ultraviolet laser radiation are so controlled as to

15 provide a surface sculpting of the cornea to achieve a desired ultimate surface change in the cornea, all in order to correct an optical defect. Such systems and methods are disclosed in the following U.S. patents and patent applications: U.S. Patent No. 4,665,913 issued May 19, 1987 for "METHOD FOR OPHTHALMOLOGICAL SURGERY"; U.S. Patent No. 4,669,466 issued

20 June 2, 1987 for "METHOD AND APPARATUS FOR ANALYSIS AND CORRECTION OF ABNORMAL REFRACTIVE ERRORS OF THE EYE"; U.S.. Patent No. 4,732,148 issued March 22, 1988 for "METHOD FOR PERFORMING OPHTHALMIC LASER SURGERY"; U.S. Patent No. 4,770,172 issued September 13, 1998 for "METHOD OF LASER-

25 SCULPTURE OF THE OPTICALLY USED PORTION OF THE CORNEA"; U.S. Patent No. 4,773,414 issued September 27, 1988 for "METHOD OF LASER – SCULPTURE OF THE OPTICALLY USED PORTION OF THE CORNEA" and U.S. Patent No. 5,108,388 issued April 28, 1992 for "LASER SURGERY METHOD".

In the above-cited U.S. Pat. No. 4,665,913 several different techniques are described which are designed to effect corrections for specific types of optical errors in the eye. For example, a myopic condition, which is typically caused by excessive curvature in the anterior surface of the cornea, is corrected by laser sculpting the corneal surface to flatten the curvature. In addition, an astigmatic condition, which is typically caused by a cylindrical component of curvature departing from the otherwise generally spherical curvature of the surface of the cornea, is corrected by effecting cylindrical ablation about the axis of cylindrical curvature of the eye. Other optical errors can be corrected in a similar fashion.

The technique for providing the flattening of the corneal curvature for myopia error correction involves selectively varying the area of the cornea exposed to the laser beam radiation to produce an essentially spherical surface profile of reduced curvature. This selective variation of the irradiated area may be accomplished in a variety of ways. U.S. Patent No. 4,732,148 cited above discloses the technique of providing a movable opaque element having apertures of various diameters and passing the laser beam through different ones of the apertures in a programmed fashion, starting either with a smallest diameter aperture and progressively increasing the surface area of exposure using apertures of wider diameters, or using the reverse process. Another technique for accomplishing varying areal exposure employs a variable diameter iris for controlling the area of the cornea exposed to the laser beam. Still another technique for providing the flattening of the corneal curvature for myopia error correction involves the use of a laser beam attenuator which varies the energy distribution of the laser beam to sculpt the surface of the cornea in conformance with the varied energy distribution. The attenuator typically includes a positive lens-shaped portion with a laser energy absorbing material and end caps having planar outer surfaces and the same refractive index as the positive portion, which prevents refraction of the laser beam upon passing through the attenuator. This technique is disclosed in U.S. Patent No. 4,838,266, issued June 13, 1989 for "LENS SHAPING DEVICE

USING A LASER ATTENUATOR". The astigmatic cylinder correction is typically performed by providing a pair of movable blades which intercept the laser beam and permit only a rectangular area of the cornea to be exposed to the beam through the width of the slit formed by the confronting edges of the blades, and by controlling the width of the slit in a predetermined manner so that a rectangular area of the cornea of either increasing or decreasing width is exposed to the laser beam. The '466 U.S. patent noted above discloses such a variable width slit mechanism.

In practice, the laser sculpturing ophthalmological surgical system is typically provided with delivery system optics which include both the variable diameter beam shaping element and the variable width slit mechanism in order to afford both myopia and astigmatism corrections. In some patients, there are both myopia and astigmatism defects in the same eye, requiring correction of both errors in order to improve vision. In the past, such compound errors have been corrected in systems having a variable diameter element and a variable width slit mechanism in a sequential fashion, with the astigmatic correction typically being performed first with the slit mechanism, followed by the correction for myopia using the variable diameter element. This has the disadvantage that the length of the operation is maximized, which increases the time that the patient's eye must be completely immobilized. This increases the physical strain and stress on the patient.

In addition, the cylindrical ablations required to correct astigmatic errors normally result in sharp transitions in the cornea at the extreme ends of the sculpted area. It has been observed that the eye responds to such sharp transitions by promoting growth of the epithelium and the stroma to smooth out sharp edges in the surface of the cornea. This has an adverse optical effect, sometimes termed the "hyperopic shift", which causes vision regression and thus reduces the effectiveness of the laser sculpting technique. In addition, such sharp transitions have the potential to induce changes in corneal curvature, such as flattening along the cylindrical axis of ablation. In

the past, attempts have been made to reduce the hyperopic shift by laser sculpting smoothing transition zones. This has been accomplished by manipulating the diameter of a circular aperture at the ends of the slit to form sigmoidal or "s" shaped transition zones. However, therapeutic patients
5 undergoing large area ablations questionable since many of such patents still exhibit hyperopic shifts.

SUMMARY OF THE INVENTION

The invention comprises a method and apparatus for providing
10 both spherical myopic and cylindrical astigmatic corrections to the cornea of an eye which eliminates the sharp transitions at the ends of the cylindrical ablation and which reduces the time required to perform both types of optical error correction.

From a method standpoint, the invention comprises the steps of
15 concurrently correcting myopic sphere and astigmatic cylinder errors in an eye by selective ultraviolet radiation and ablative photodecomposition of the corneal surface in a volumetric removal of corneal tissue and with depth penetration into the stroma to effect toric ablation. The toric ablation is effected by passing the ultraviolet radiation in the form of a laser beam
20 through a slit of varying width and an aperture of varying diameter. Preferably, the slit width is varied from a minimum value to a maximum value, while the aperture diameter is contemporaneously varied from a maximum value to a minimum value. The inverse operation of the slit and the aperture is also effective, though less preferred. Alternatively, the toric ablation is effected by
25 passing the ultraviolet radiation in the form of a laser beam through a variable aperture modulator to produce an elliptical beam profile of variable dimensions. The elliptical beam profile is preferably produced in this embodiment by angularly directing the laser beam at a variable aperture element having a plurality of circular apertures of different diameters, and
30 progressively positioning different ones of the apertures into the path of the

beam. The laser beam encounters a series of elliptical apertures of varying axial dimension, depending on the tilt angle and the aperture diameter.

In another method aspect, the invention comprises a method of changing the anterior surface of the cornea of an eye from initial spherical and cylindrical curvature having myopic and astigmatic optical properties to a subsequent curvature having correctively improved optical properties, which method comprises exposing the surface of the cornea and passing ultraviolet laser radiation through a variable aperture element to selectively ablate the exposed surface of the cornea by photodecomposition, with penetration into the stroma and substantially simultaneous spherical and cylindrical volumetric sculpturing removal of corneal tissue to such penetration depth and profile as to characterize the anterior surface of the cornea with said subsequent curvature.

In a still further aspect of the invention, the invention comprises a method of using an ultraviolet laser to concurrently correct myopic and astigmatic optical errors of an eye, which method comprises the steps of adjusting the intensity of laser beam projection to a level at which laser beam projection onto the exposed surface of the cornea of the eye will result in a corneal tissue ablation per unit time which is a function of a predetermined maximum ablation depth into the stroma of the cornea, and directing the laser beam at the exposed surface of the cornea in a controlled program of circular and rectangular area coverage as a function of time to redefine the exposed surface curvature by volumetric removal of corneal tissue in the course of selective ablative sculpture of the stroma. The step of directing the laser beam at the exposed surface of the cornea is performed by passing the laser beam through an aperture and a slit and varying the diameter of the aperture and the width of the slit to effect toric ablation of the stroma.

More specifically, according to the invention there is provided a system for changing the anterior surface of the cornea of an eye from an initial spherical and cylindrical curvature having myopic and astigmatic optical properties to a subsequent curvature having correctively improved optical properties, the cornea having a surface and a stroma, the system comprising
5 laser for generating a beam of ultraviolet radiation along a path, and a variable aperture device disposed in the path of said beam for exposing the surface of the cornea and permitting the ultraviolet laser radiation to pass through the variable aperture element to selectively ablate the exposed surface of the
10 cornea by photodecomposition, with penetration into the stroma and simultaneous spherical and cylindrical volumetric sculpturing removal of corneal tissue during at least a portion of the selective ablation to such penetration depth and profile as to characterize the surface of the cornea with said subsequent curvature.

15 Accordingly to another aspect of the present invention there is provided a laser eye surgical system for providing elliptical beam cross-sections for spherical astigmatic corrections to a cornea of an eye, said system comprising: (a) a laser for producing a laser beam, said laser positioned so that said laser beam propagates along a beam path;(b) beam shaping means
20 disposed along said beam path of said laser beam for shaping said laser beam by transmitting only a portion of said laser beam having an elliptical cross-section past said beam shaping means, said beam shaping means comprising a mask having a plurality of elliptical apertures having different dimensions from one another, at least some of said elliptical apertures having different
25 sizes from one another; and (c) means for rotatably mounting said mask so that different ones of said apertures of said mask can be positioned along said beam path at different times, wherein said plurality of apertures are dimensioned to enable producing desired elliptic ablations from corneal tissue.

According to yet another aspect of the present invention there is
30 provided an apparatus for performing ophthalmological treatment to improve spherical and cylindrical vision defects by selective ablation of the cornea to

5 b

achieve a volumetric removal of corneal tissue, said apparatus comprising:

(a) laser means for producing an output beam in the ultraviolet portion of the electromagnetic spectrum and for directing said output beam onto the eye

which is to be treated;(b) adjustment means provided in the laser beam path

5 for adjustably determining the laser beam area at impingement upon the

cornea; and (c) control means operative upon said adjustment means for

adjusting the laser beam area at corneal impingement in a controlled manner

in the course of an ophthalmological treatment so that sculpturing action

results from a controlled variation in the area of the cornea that is irradiated

10 and a corresponding controlled variation in the cumulative ablative flux

delivered to different areas of the cornea; characterized in that, for the

treatment of an eye having both spherical and cylindrical curvature defects,

said adjustment means and said control means are adapted and arranged

such that the laser beam can be directed onto the cornea in a controlled

15 program of irradiated area variation which effects simultaneous spherical and

cylindrical volumetric sculpturing removal of corneal tissue thereby enabling

both spherical and cylindrical corrections to be concurrently effected to the

eye.

For a fuller understanding of the nature and advantages of the

20 invention, reference should be had to the ensuing detailed description taken in
conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a block diagram of an ophthalmological laser surgery system for performing the invention;

Fig. 2 is a schematic plan view showing the movable slit and
5 variable diameter aperture;

Fig. 3 is a schematic diagram illustrating the geometry of an elliptical ablation; and

Fig. 4 is a graph showing variation of the minor axis length with correction ratio for different major axis lengths.

10

DESCRIPTION OF THE PREFERRED EMBODIMENTS

Turning now to the drawings, Fig. 1 illustrates a block diagram of an ophthalmological surgery system for performing the invention. As seen in this Fig., a personal computer (PC) work station 10 is coupled to a single
15 board computer 21 of a laser surgery unit 20 by means of a first bus connection 11. PC work station 10 and the subcomponents of laser surgery unit 20 are known components and preferably comprise the elements of the VISX TWENTY/TWENTY EXCIMER LASER SYSTEM available from Visx, Incorporated of Sunnyvale, California. Thus, the laser surgery system 20
20 includes a plurality of sensors generally designated with reference numeral 22 which produce feedback signals from the movable mechanical and optical components in the laser optical system, such as the elements driven by an iris motor 23, an image rotator 24, and astigmatism motor 25 and an astigmatism angle motor 26. The feedback signals from sensors 22 are provided via
25 appropriate signal conductors to the single board computer 21, which is preferably an STD bus compatible single board computer using a type 8031 microprocessor. The single board computer 21 controls the operation of the motor drivers generally designated with reference numeral 27 for operating the elements 23-26. In addition, single board computer 21 controls the operation
30 of the Excimer laser 28, which is preferably an argon-fluorine laser with a 193 nanometer wavelength output designed to provide feedback stabilized fluence

of 160 mJoules per cm^2 at the cornea at the patient's eye 30 via the delivery system optics generally designated with reference numeral 29. Other ancillary components of the laser surgery system 20 which are not necessary to an understanding of the invention, such as a high resolution microscope, a video monitor for the microscope, a patient eye retention system, and an ablation affluent evacuator/filter, as well as the gas delivery system, have been omitted to avoid prolixity. Similarly, the keyboard, display, and conventional PC subsystem components (e.g., flexible and hard disk drives, memory boards and the like) have been omitted from the depiction of the PC work station 10.

10 The iris motor 23 is used to control the diameter of a variable diameter iris schematically depicted in Fig. 2. The astigmatism motor 25 is used to control the separation distance between a pair of cylinder blades 35, 36 which are mounted on a platform 38 for bi-directional translatory motion in the direction of arrows 40, 41. Platform 38 is rotatably mounted on a second platform (not illustrated) and is rotationally driven by astigmatism angle motor 15 26 in a conventional way in order to enable alignment of the slit axis (illustrated in a vertical orientation in Fig. 2) with the cylinder axis of the patient's eye. Iris 32 is driven by iris motor 23 in a known way to change the diameter of the iris opening from a fully opened position (the position 20 illustrated in Fig. 2) to a fully closed position in which the aperture is closed to a minimum diameter of 0.8 mm. It is understood that the variable diameter iris 32 and the cylinder blades 35, 36 are positioned with respect to the output of laser 28 in such a manner as to intercept the beam prior to irradiation of the corneal surface of the patient's eye 30. For the purpose of this application, it 25 may be assumed that iris 32 and cylinder blades 35, 36 are part of the delivery system optics subunit 29 shown in Fig. 1.

 The system of Figs. 1 and 2 is used according to the invention to concurrently effect myopic spherical and astigmatic cylindrical corrections to the surface of the cornea by toric ablation. Toric ablation is effected by 30 controlling the combined movement of the cylinder blades 35, 36 and iris 32 over a desired range of movement. The constant depth contour map of a

The refractive power of an elliptical ablation for treating myopia and myopic cylinder is most easily understood using minus notation for the cylinder. The cylinder axis is located along the major axis of the ellipse, while the refractive power of the cylinder is located along the minor axis. For such an ablation in a flat surface, the spherical refractive power can be calculated from the central depth of ablation, the length of the major axis and the index of refraction of the ablated material. The refractive power along the minor axis can similarly be calculated from the length of the minor axis, the depth of ablation and the index of refraction of the ablated material. The cylindrical power can then be calculated by subtracting the refractive (spherical) power along the major axis from the refractive power along the minor axis. The equations set forth in "Photorefractive keratectomy: A technique for laser refractive surgery" authored by Munnerlyn, et al., J. Cataract Refract Surg - Vol. 18, pages 46-52 (Jan., 1988),

can be used to calculate the ablation geometry in corneal tissue along the major and minor axes of the ellipse. Along the major axis, the length of the major axis, S_{maj} , is substituted for the treatment diameter, and the dioptric correction entered into the equations is the spherical correction. To determine the ablation geometry along the minor axis, the sum of the spherical and cylindrical corrections is entered into the equations as the dioptric correction, and the length of the minor axis, S_{min} , is substituted for the treatment diameter.

30

$$S_{\min} \sim S_{\text{maj}} [D_{\text{cyl}}/D_{\text{sph}} + 1]^{-1/2}.$$

In the above equation, S_{min} is the length of the minor axis, S_{maj} the length of the major axis, D_{cyl} the cylindrical correction and D_{sph} the spherical correction. As noted above, this equation assumes minus notation for the cylindrical portion of the correction.

To be effective clinically, an elliptical ablation must have a sufficiently large minor axis comparable in size to the maximum diameter of the corneal treatment zone. As shown in Fig. 4, which plots varying ratios of cylindrical to spherical corrections for constant major axis length, there are certain practical limits to the maximum ratio of cylindrical to spherical corrections. In particular, for a given major axis length the length of the minor axis decreases as the ratio of cylindrical to spherical correction increases. For example, for a major axis of 6.0 mm (corresponding to a laser capable of producing a maximum treatment diameter of 6.0 mm), the minor axis for equal spherical and cylindrical corrections is 4.25 mm. This suggests that the clinical use of toric ablations to correct refractive cylinder should be limited to patients having at least as much spherical error as cylindrical error (for a 6.0 mm maximum treatment diameter). For larger maximum treatment diameters (e.g., the upper curve in Fig. 4 corresponding to a 7.0 mm treatment diameter), the ratio constraints will be different.

Returning to Fig. 2, in the preferred embodiment toric ablations are produced by relative motion of the cylinder blades 35, 36 while varying the diameter of the iris 32. Initially, the cylinder blades 35, 36 are completely closed and the iris 32 is opened to the maximum desired diameter.

Thereafter, the cylinder blades 35, 36 are progressively opened while the iris 32 is progressively closed by the respective motors 25, 23. As the cylinder blades 35, 36 are opened, the cylindrical component is ablated in the surface of the cornea. As the diameter of iris 32 is closed contemporaneously with the opening of the cylinder blades 35, 36, the spherical component is ablated in the corneal surface. The combined progressive motion of the cylinder blades 35, 36 and the iris 32 produces the toric ablation desired.

As an example, consider the case of a patient with a refraction of -3.0 -2.0 x 175, average keratometry of 44.5D and a desired 6.0 mm treatment zone. The iris 32 is initially imaged to a 6.0 mm diameter, and cylinder blades 35, 36 are initially placed in the closed position and rotated to the desired angular orientation in the plane of Fig. 2. Thereafter, as laser 28 is pulsed the cylinder blades 35, 36 are progressively opened to effect a -2.0D cylindrical correction. At the same time, iris 32 is progressively closed to effect a -3.0D spherical correction.

The preferred embodiment uses laser 28 to ablate a thin layer of tissue from the surface of the cornea with each pulse. The desired ablation depth along each axis can be predetermined by computer control. The iris 32 is programmed to close at a rate which corresponds to the spherical correction, and the cylindrical blades 35, 36 open at a rate corresponding to the cylindrical correction. The transverse displacement of each aperture between pulses corresponds to the change in desired cut depth for the appropriate aperture (i.e., iris 32 or blades 35, 36). The change in desired cut depth is equal to the amount of material removed with each pulse. Thus, for a -3.0 -2.0 x 175 correction, the iris 32 is closed to create a -3.0D ablation while the cylinder blades 35, 36 open to create a -2.0D cylindrical correction. Along the minor axis of the ellipse, the combined effect of the iris 32 and cylinder blades 35, 36 produces a -5.0D ablation, while the major axis of ellipse has a -3.0D ablation.

A significant advantage of the preferred embodiment is that the boundaries of the elliptical ablated area are determined by the combined motion of the iris 32 and the cylinder blades 35, 36. As the simultaneous refractive correction proceeds, the intersection of the cylinder blades and iris mark the outer edge of the ablation. The ratio of the minor to major axes is determined by the relative motion of the iris 32 and the cylinder blades 35, 36. Thus, the exact geometry of the ablated area need not be solved for explicitly, and can be varied depending upon the correction required.

Since the number of laser pulses required to effect the spherical correction will usually be greater than the number of laser pulses required to effect the cylindrical correction (assuming equal treatment values of S in the equations of Munnerlyn et al.), cylinder blades 35, 36 will be fully opened to the 6.0 mm position while the iris 32 is not yet fully closed in the above example. Cylinder blades 35, 36 are left at the 6.0 mm position without further movement while the laser finishes the extra pulses required until iris 32 is fully closed. It should be noted that an alternate method of operating the iris 32 and the cylinder blades 35, 36 is to start with the iris 32 initially closed and the cylinder blades 35, 36 initially opened to the maximum slot width, followed by progressive opening of the iris 32 and progressive closing of the blades 35, 36. If the number of pulses required to effect the spherical correction is greater than that required to effect the cylindrical correction (which will be the case whenever the ratio of cylinder-to-sphere shown in Fig. 4 is less than 1.0 and the programmed treatment diameters are equal), motion of blades 35, 36 must be delayed until the extra number of pulses required for the spherical correction have been produced. Otherwise, the blades 35, 36 will be fully closed before the spherical correction is completed. This alternate method of operation thus requires additional capability in the system of Fig. 1 to delay the operation of the astigmatism motor 25 in the closing direction until the extra number of laser pulses required for the spherical correction have been produced.

While the embodiment employing the iris 32 and cylinder blades 35, 36 described above is preferred, the toric ablation may also be effected by employing a variable aperture laser beam modulator to produce an elliptical beam profile of variable dimensions. This may be done by using a mask rotatably mounted in the beam path and having a plurality of variable dimension elliptical apertures with progressive sizes required to produce the desired toric ablation. Alternatively, the mask may have circular apertures of different diameters, and the mask may be positioned at an angle with respect to the laser beam axis so that each circular aperture provides an elliptical

profile to the laser beam. The apertured mask is progressively re-positioned between pulses of the laser beam so as to vary the area of the corneal surface exposed to the laser beam from a smallest elliptical area to a largest elliptical area (or the reverse). Care must be taken to ensure that the major
5 axis of each ellipse is collinear with the desired axis of cylindrical ablation throughout the surgery, and this requires precise positioning of the cornea with respect to the elliptical axes. This alternative embodiment has the advantage of employing apertured masks which may already be present in an existing system, such as those shown in the above-referenced U.S. Patent No.
10 4,732,148 (particularly Figs. 9 and 24).

As will now be apparent, the invention enables both spherical and cylindrical corrections to be concurrently effected to the eye of a patient, thus eliminating the prior need with variable aperture and slit systems to first perform the one type of correction (usually the astigmatic correction using the
15 slit) followed by the other correction (typically the spherical correction using the variable aperture). This reduces the total number of pulses required to effect both types of correction to simply the number required to perform the spherical correction. Since the laser beam cross section and intensity can vary over time and with repeated pulsing, the invention reduces the likelihood
20 of error in effecting the desired contoured shaping of the corneal surface. In addition, by sculpting the corneal surface using a toric ablation, the steep vertical "walls" with depth equal to the astigmatic ablation depth are not formed at each end of the cylindrical ablation: consequently, there is no need to produce the sigmoidal transition zones, which simplifies the procedure. In
25 addition, the absence of any steep edges in the corneal ablation reduces the tendency of the eye to produce excessive growth of the epithelium over the ablated surface and this reduces the hyperopic shift phenomenon.

It is understood that the invention encompasses various techniques used to prepare the anterior surface of the cornea for the laser
30 based ablation. For example, removal of the epithelium by both surgical scraping and peeling to expose the corneal surface, as well as laser ablation

of the epithelium prior to or contemporaneously with the laser sculpting of the corneal surface, are encompassed by the invention. Thus, the term "corneal surface" refers to the surface to be sculpted to the desired corrective curvature, regardless of whether or not the epithelium or Bowman's membrane
5 (or both) intervene with the actual corneal surface.

While the above provides a full and complete disclosure of the preferred embodiments of the invention, various modifications, alternate constructions and equivalents may be employed as desired. For example, while the invention has been described with specific reference to the system of
10 Figs. 1 and 2, other arrangements may be employed to produce the variable rectangular and circular areal irradiation desired. Therefore, the above description and illustrations should not be construed as limiting the invention, which is defined by the appended claims.

CLAIMS:

1. A system for changing the anterior surface of the cornea of an eye from an initial spherical and cylindrical curvature having myopic and astigmatic optical properties to a subsequent curvature having correctively improved optical properties, the cornea having a surface and a stroma, the system comprising laser for generating a beam of ultraviolet radiation along a path, and a variable aperture device disposed in the path of said beam for exposing the surface of the cornea and permitting the ultraviolet laser radiation to pass through the variable aperture element to selectively ablate the exposed surface of the cornea by photodecomposition, with penetration into the stroma and simultaneous spherical and cylindrical volumetric sculpturing removal of corneal tissue during at least a portion of the selective ablation to such penetration depth and profile as to characterize the surface of the cornea with said subsequent curvature.

2. The system of claim 1 wherein said variable aperture device comprises a slit of varying width and a diaphragm of varying diameter.

3. The system of claim 1 further comprising a modulator for varying the width of the slit from a maximum to a minimum value and the aperture diameter from a minimum to a maximum value.

4. The system of claim 1 further comprising a modulator for varying the width of the slit from a minimum to a maximum value and the aperture diameter from a maximum to a minimum value.

5. The system of claim 4 wherein said modulator produces an elliptical ablation profile of variable dimension.

6. The system of claim 5 wherein the variable aperture device is provided with a plurality of circular apertures; and

wherein the modulator includes means for angularly directing the laser beam at the variable aperture element and means for progressively positioning different ones of the circular apertures in the path of the beam.

7. A laser eye surgical system for providing elliptical beam cross-sections for spherical and astigmatic corrections to a cornea of an eye, said system comprising:

- 5 (a) a laser for producing a laser beam, said laser positioned so that said laser beam propagates along a beam path;
- (b) beam shaping means disposed along said beam path of said laser beam for shaping said laser beam by transmitting only a portion of said laser beam having an elliptical cross-section past said beam shaping means, said beam shaping means comprising a mask having a plurality of elliptical apertures having different dimensions from one another, at least some of said elliptical apertures having different sizes from one another; and
- 10 (c) means for rotatably mounting said mask so that different ones of said apertures of said mask can be positioned along said beam path at different times, wherein said plurality of apertures are dimensioned to enable producing desired elliptic ablations from corneal tissue.
- 15

8. A laser eye surgical system for providing elliptical beam cross-sections for spherical and astigmatic corrections to a cornea of an eye, said system comprising:

20

- (a) a laser for producing a laser beam, said laser positioned so that said laser beam propagates along a beam path;
- 25 (b) beam shaping means disposed along said beam path for shaping said laser beam by transmitting only a portion of said laser beam having an elliptical cross-section past said beam shaping means, said beam shaping means comprising
- (i) a mask having an aperture; and
- 30 (ii) means for rotating said mask about a mask axis that is perpendicular to said beam path.

9. A system according to claim 8 wherein the eye has an astigmatic axis and said mask axis is perpendicular to said astigmatic axis.

10. A system according to claim 8 wherein said aperture is circular.

5 11. A system according to claim 8 wherein said mask has a plurality of circular apertures.

12. A system according to claim 8 wherein said means for rotating rotates said mask so that said aperture remains in said beam path.

10 13. A system for ablating a surface with laser energy, said system comprising:

(a) means for aligning a surface with a laser which is operable to deliver a beam of photo ablative pulses of laser energy along a path to the surface;

15 (b) means for varying a cross-sectional size of the beam by means for shaping the beam into an elliptical form having a major axis and a minor axis, said means for shaping comprising an optical system along said path of the beam, wherein said optical system defines an aperture having a cross-section defining said cross-sectional size of the beam such that the aperture remains in said path while said cross-sectional size varies; and

20 (c) means for adjusting said optical system to select an astigmatic ratio of the major axis to the minor axis of the beam on the surface;

25 thereby forming a time-varying elliptical distribution of intensity on the surface.

14. The system of claim 13 further comprising means for rotating said optical system to select an orientation of said major axis of the time-varying elliptical distribution of intensity on the surface.

30 15. The system of claim 13 wherein said means for varying comprises:

- (a) an adjustable aperture; and
- (b) means for imaging said adjustable aperture onto the surface.

5 16. The system of claim 13 further comprising means for adjusting said optical system to select a second astigmatic ratio on the surface.

17. A system for ablating an area of the cornea of an eye for correcting myopic astigmatism, said system comprising:

- (a) means for fixing an eye relative to a laser;
- 10 (b) means for delivering a beam of photo ablative pulses of laser energy from said laser along a path to the cornea;
- (c) an optical system along said path of the beam and comprising means for varying a cross-sectional size of the beam such that the beam passing through said
- 15 optical system is shaped into an elliptical form having a major axis and a minor axis, wherein said means for varying defines an aperture having a cross-section defining said cross-sectional size of the beam such that the aperture remains in said path while said cross-
- 20 sectional size varies;
- (d) means for adjusting said optical system to select an astigmatic ratio of the major axis to the minor axis of the beam on the cornea; and

25 thereby forming a time-varying generally elliptical distribution of intensity on the cornea.

18. A system of claim 17 further comprising means for rotating said optical system to orient the time-varying elliptical distribution of intensity on the cornea.

30 19. The system of claim 17 wherein said optical system comprises:

- (a) an adjustable aperture, and

- (b) means for imaging said adjustable aperture onto the cornea.

20. The system of claim 17 further comprising means for adjusting said optical system to define a length of said major axis and thereby
5 selecting the astigmatic ratio of the beam on the cornea.

21. The system of claim 17 wherein said laser is an excimer laser.

22. The system of claim 17 wherein said optical system comprises delivery system optics for transmitting the beam from the laser to
10 the cornea so that the beam has a predetermined fluence at the cornea.

23. A laser system for reprofiling a surface, said laser system comprising:

- 15 (a) an excimer laser for generating pulses of laser light along a beam path and at an energy per pulse such that the pulses impinging onto the surface induce photo ablation of the surface, the laser light having dimensions at the surface;
- (b) beam control means for controlling the dimensions of the laser light to create an astigmatic irradiation pattern at the
20 surface said beam control means comprising:
- (1) two cylinder blades defining a slit shaped aperture,
(2) an iris, and
(3) said beam control means disposed along the beam path; and
- 25 (c) adjustment means for shifting an optical means to select an astigmatic ratio for the astigmatic irradiation pattern at the surface.

24. The laser system of claim 23 wherein said excimer laser contains a mixture of gases comprising argon and fluorine for generating 193
30 nanometer laser radiation.

25. The laser system of claim 23 wherein said iris is an adjustable iris for controlling a diameter of the laser light.

26. The laser system of claim 25 wherein an optical means defines an aperture for controlling the diameter of said laser beam applied to
5 said surface.

27. The laser system of claim 25 wherein an optical means includes means for rotating said cylinder blades to orient an astigmatic axis of the astigmatic irradiation pattern at the surface.

28. The laser system of claim 27 wherein said optical means
10 further comprises delivery system optics.

29. A laser eye surgical system for providing spherical myopic and cylindrical astigmatic corrections to a cornea of an eye, said system comprising:

- 15 (a) a laser for producing a laser beam, said laser positioned so that said laser beam propagates along a beam path;
- (b) beam shaping means disposed along said beam path of said laser beam for shaping said laser beam by transmitting only a portion of said laser beam past said beam shaping means, said beam shaping means
20 comprising:
 - (i) means for defining a slit shaped aperture having a slit width;
 - (ii) means for defining a circular shaped aperture having a circular diameter;
 - 25 (iii) means for simultaneously varying said slit width and said circular diameter of said circular shaped aperture.

30. A system according to claim 29 wherein said beam shaping means further comprises means for simultaneously increasing said
30 slit width while decreasing said circular diameter.

31. A system according to claim 29 wherein said beam shaping means further comprises means for simultaneously decreasing said slit width while increasing said circular diameter.

32. A system according to claim 29 wherein

- 5 (a) said means for defining said circular shaped aperture comprises an iris; and
- (b) said means for simultaneously varying said slit width and said circular diameter comprises means for opening and closing said iris.

10 33. A system according to claim 29 wherein said laser is an excimer laser.

34. A system according to claim 29 wherein said laser is an excimer laser containing a gas mixture substantially comprising argon and fluorine gas for generating 193 nonometer laser radiation.

15 35. A system according to claim 29 wherein said slit shaped aperture extends in an extending direction and further comprising means for rotating a first cylinder blade and a second cylinder blade to thereby rotate said extending direction.

20 36. A system according to claim 29 wherein said laser comprises means for producing laser beam pulses having a wavelength of 193 nanometers and a pulse fluence at the cornea that is stabilized by feedback.

37. A system according to claim 29 wherein

- 25 (a) said means for defining said slit shaped aperture comprises a first cylinder blade and a second cylinder blade, said first cylinder blade has a flat first cylinder blade surface, said second cylinder blade has a flat second cylinder blade surface, said flat first cylinder blade surface opposes said flat second cylinder blade surface, said flat first cylinder blade surface is separated from said flat second cylinder blade surface by a separation
- 30

distance equal to said slit width, and

- (b) said means for varying said slit width comprises means for varying said separation distance by moving said flat first cylinder blade surface and said flat second cylinder blade surface towards and away from one another.

5

38. A system according to claim 37 wherein said beam shaping means further comprises means for

10

- (iv) simultaneously increasing said separation distance from a minimum separation distance value to a maximum separation distance value while decreasing said circular diameter from a maximum diameter value to an intermediate diameter value and then

15

- (v) maintaining said separation distance value at said maximum separation distance value while decreasing said circular diameter from said intermediate diameter value to a minimum diameter value.

39. A system according to claim 38 wherein said minimum separation distance value is zero and said minimum diameter value is zero.

20

40. A system according to claim 38 wherein said maximum diameter value and said maximum separation distance value are about six millimeters.

41. A system according to claim 37 wherein said beam shaping means further comprises means for

25

- (iv) maintaining said separation distance at a maximum separation distance value while increasing said circular diameter from a minimum diameter value to an intermediate diameter value and then

30

- (v) simultaneously decreasing said separation

distance from said maximum separation distance value to a minimum separation distance value while increasing said circular diameter from said intermediate diameter value to a maximum diameter value.

5

42. A system according to claim 41 wherein said minimum separation distance value is zero and said minimum diameter value is zero.

43. A system according to claim 41 wherein said maximum diameter value and said maximum separation distance are about six millimeters.

10

44. An apparatus for ablating a surface with laser energy, the apparatus comprising:

(a) a laser operable to deliver a beam of photoablative pulses of laser energy;

15

(b) means for aligning a surface with said laser to deliver a beam of photoablative pulses of laser energy along a path to the surface, the beam having a cross-sectional size;

(c) an optical system disposed along said path, said optical system comprising:

20

(1) a slit having a width, a major dimension, and a minor dimension; and

(2) an iris having a diameter;

(d) means for

25

(1) sending a photoablative pulse from said laser through said optical system to said surface;

(2) changing said width and said diameter; and

(3) sending another photoablative pulse from said laser means through said optical system to said surface.

30

45. The apparatus of claim 44 further comprising means for rotating said slit to thereby rotate said major axis.

46. The apparatus of claim 44 wherein said means for aligning comprises means for aligning a surface of an eye with said laser.

5 47. The method of claim 44 wherein said laser is an excimer laser.

48. A laser system for reprofiling a surface, said laser system comprising:

10 (a) laser means for generating pulses of laser light along a beam path and at an energy per pulse such that the pulses impinging into the surface induce photoablation of the surface, the laser light having dimensions at the surface;

15 (b) optical means including a slit having a width and an iris having a diameter disposed along the beam path for adjusting the dimensions of the laser light along one axis for creating an astigmatic irradiation pattern at the surface; and

20 (c) adjustment means for shifting said optical means by varying said width of said slit and said diameter of said iris to select an astigmatic ratio for the astigmatic irradiation pattern at the surface.

25 49. The laser system of claim 48 wherein said optical means includes an aperture for controlling the diameter of said laser beam applied to said surface.

50. The laser system of claim 48 wherein said laser means is an excimer laser.

51. The laser system of claim 50 wherein said excimer laser is an argon fluoride laser.

52. The laser system of claim 48 wherein said optical means includes means for rotating at least one optical element to orient an astigmatic axis of the astigmatic irradiation pattern at the surface.

53. The laser system of claim 52 wherein said optical means
5 further comprises delivery system optics.

54. Apparatus for performing ophthalmological treatment to improve spherical and cylindrical vision defects by selective ablation of the cornea to achieve a volumetric removal of corneal tissue, said apparatus comprising:

- 10 (a) laser means for producing an output beam in the ultraviolet portion of the electromagnetic spectrum and for directing said output beam onto the eye which is to be treated;
- 15 (b) adjustment means provided in the laser beam path for adjustably determining the laser beam area at impingement upon the cornea; and
- 20 (c) control means operative upon said adjustment means for adjusting the laser beam area at corneal impingement in a controlled manner in the course of an ophthalmological treatment so that sculpturing action results from a controlled variation in the area of the cornea that is irradiated and a corresponding controlled variation in the cumulative ablative flux delivered to different areas of the cornea;

25 characterized in that, for the treatment of an eye having both spherical and cylindrical curvature defects, said adjustment means and said control means are adapted and arranged such that the laser beam can be directed onto the cornea in a controlled program of irradiated area variation which effects simultaneous spherical and cylindrical volumetric sculpturing
30 removal of corneal tissue thereby enabling both spherical and cylindrical corrections to be concurrently effected to the eye.

55. Apparatus according to claim 54 wherein said adjustment means comprises variable aperture means disposed in the path of the laser beam.

56. Apparatus according to claim 55 wherein said variable aperture means comprises a first means defining a variable diameter circular aperture and a second means defining a variable width slit.

57. Apparatus according to claim 56 wherein said first means comprises an iris diaphragm.

58. Apparatus according to claim 56 or 57 including means for adjusting the orientation of said variable width slit in the laser beam.

59. Apparatus according to any one of claims 56, 57 or 58 wherein said control means is arranged to vary the slit width from a minimum to a maximum value and to vary the circular aperture diameter from a maximum to a minimum value.

60. Apparatus according to any one of claims 56, 57 or 58 wherein said control means is arranged to vary the slit width from a maximum to a minimum value and to vary the circular aperture diameter from a minimum to a maximum value.

61. Apparatus according to claim 55 wherein said variable aperture means comprises a variable aperture laser beam modulator producing an elliptical beam profile of variable dimensions.

62. Apparatus according to claim 61 wherein said variable aperture laser beam modulator comprises a mask having a plurality of elliptical apertures of progressively different sizes.

63. Apparatus according to claim 61 wherein said variable aperture laser beam modulator comprises a mask having a plurality of circular apertures of different diameters and means for positioning said mask at an angle with respect to the laser beam so that each mask aperture provides an elliptical profile to the laser beam.

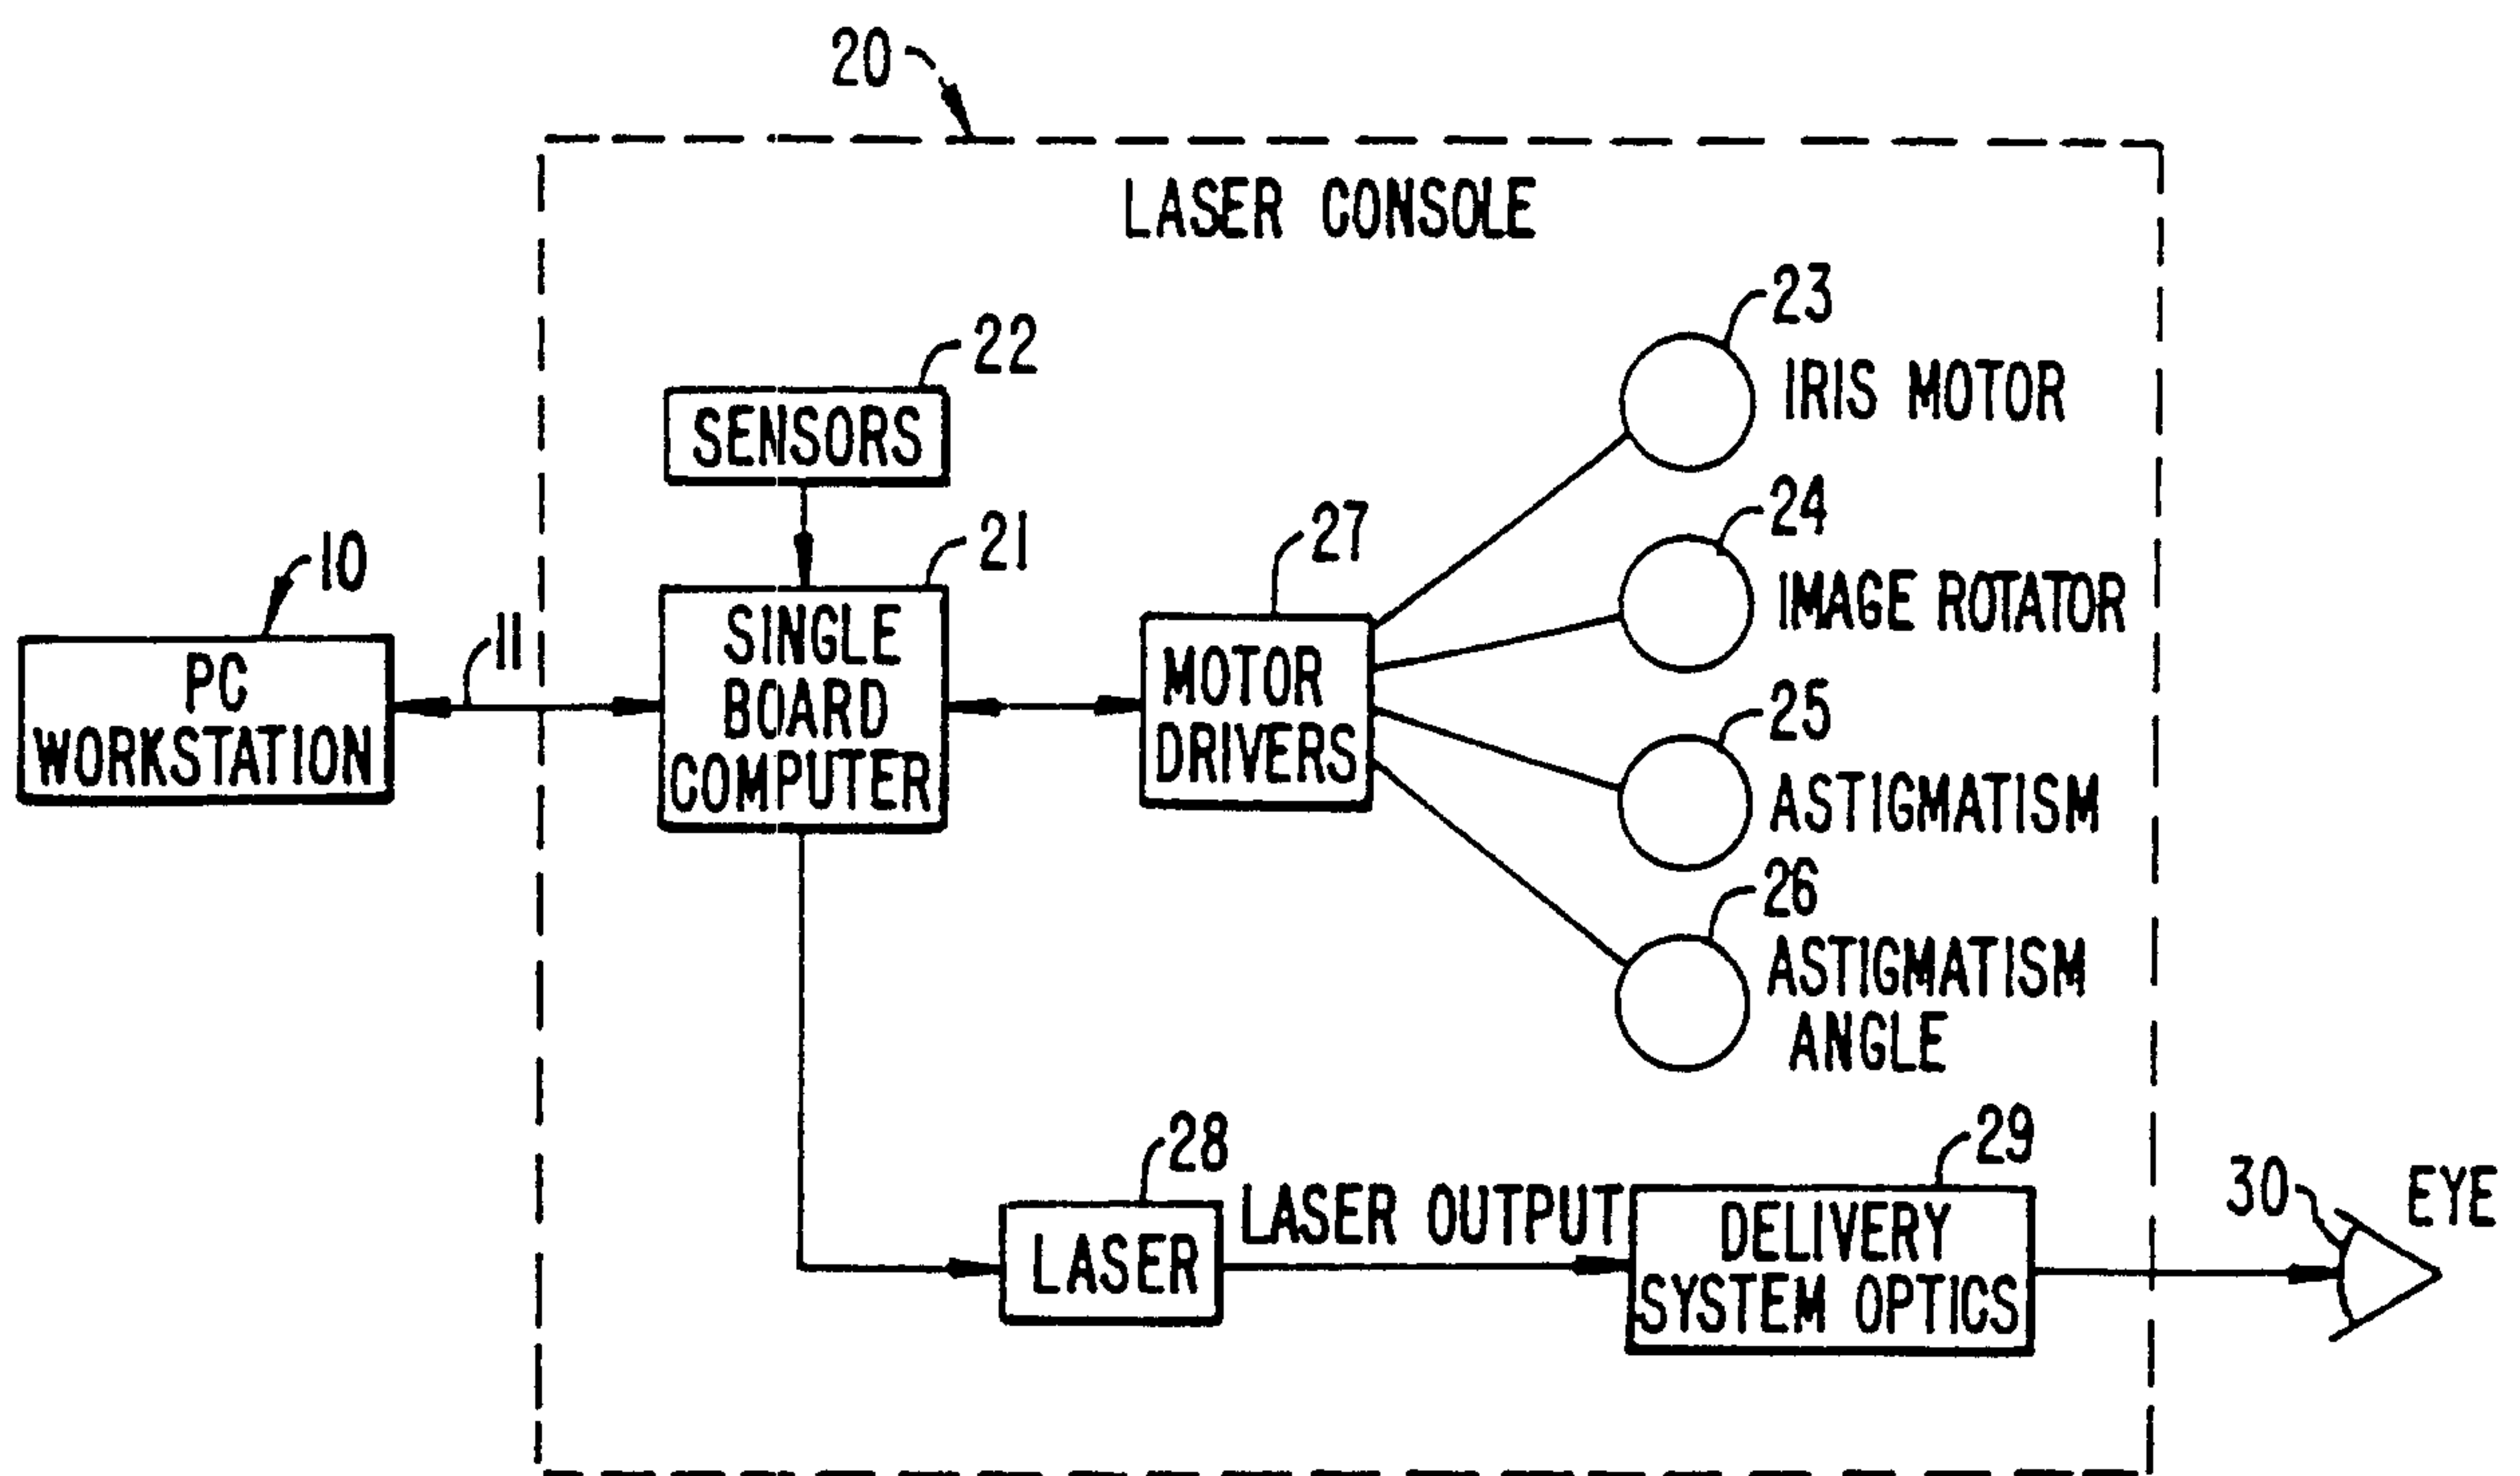


FIG. 1.

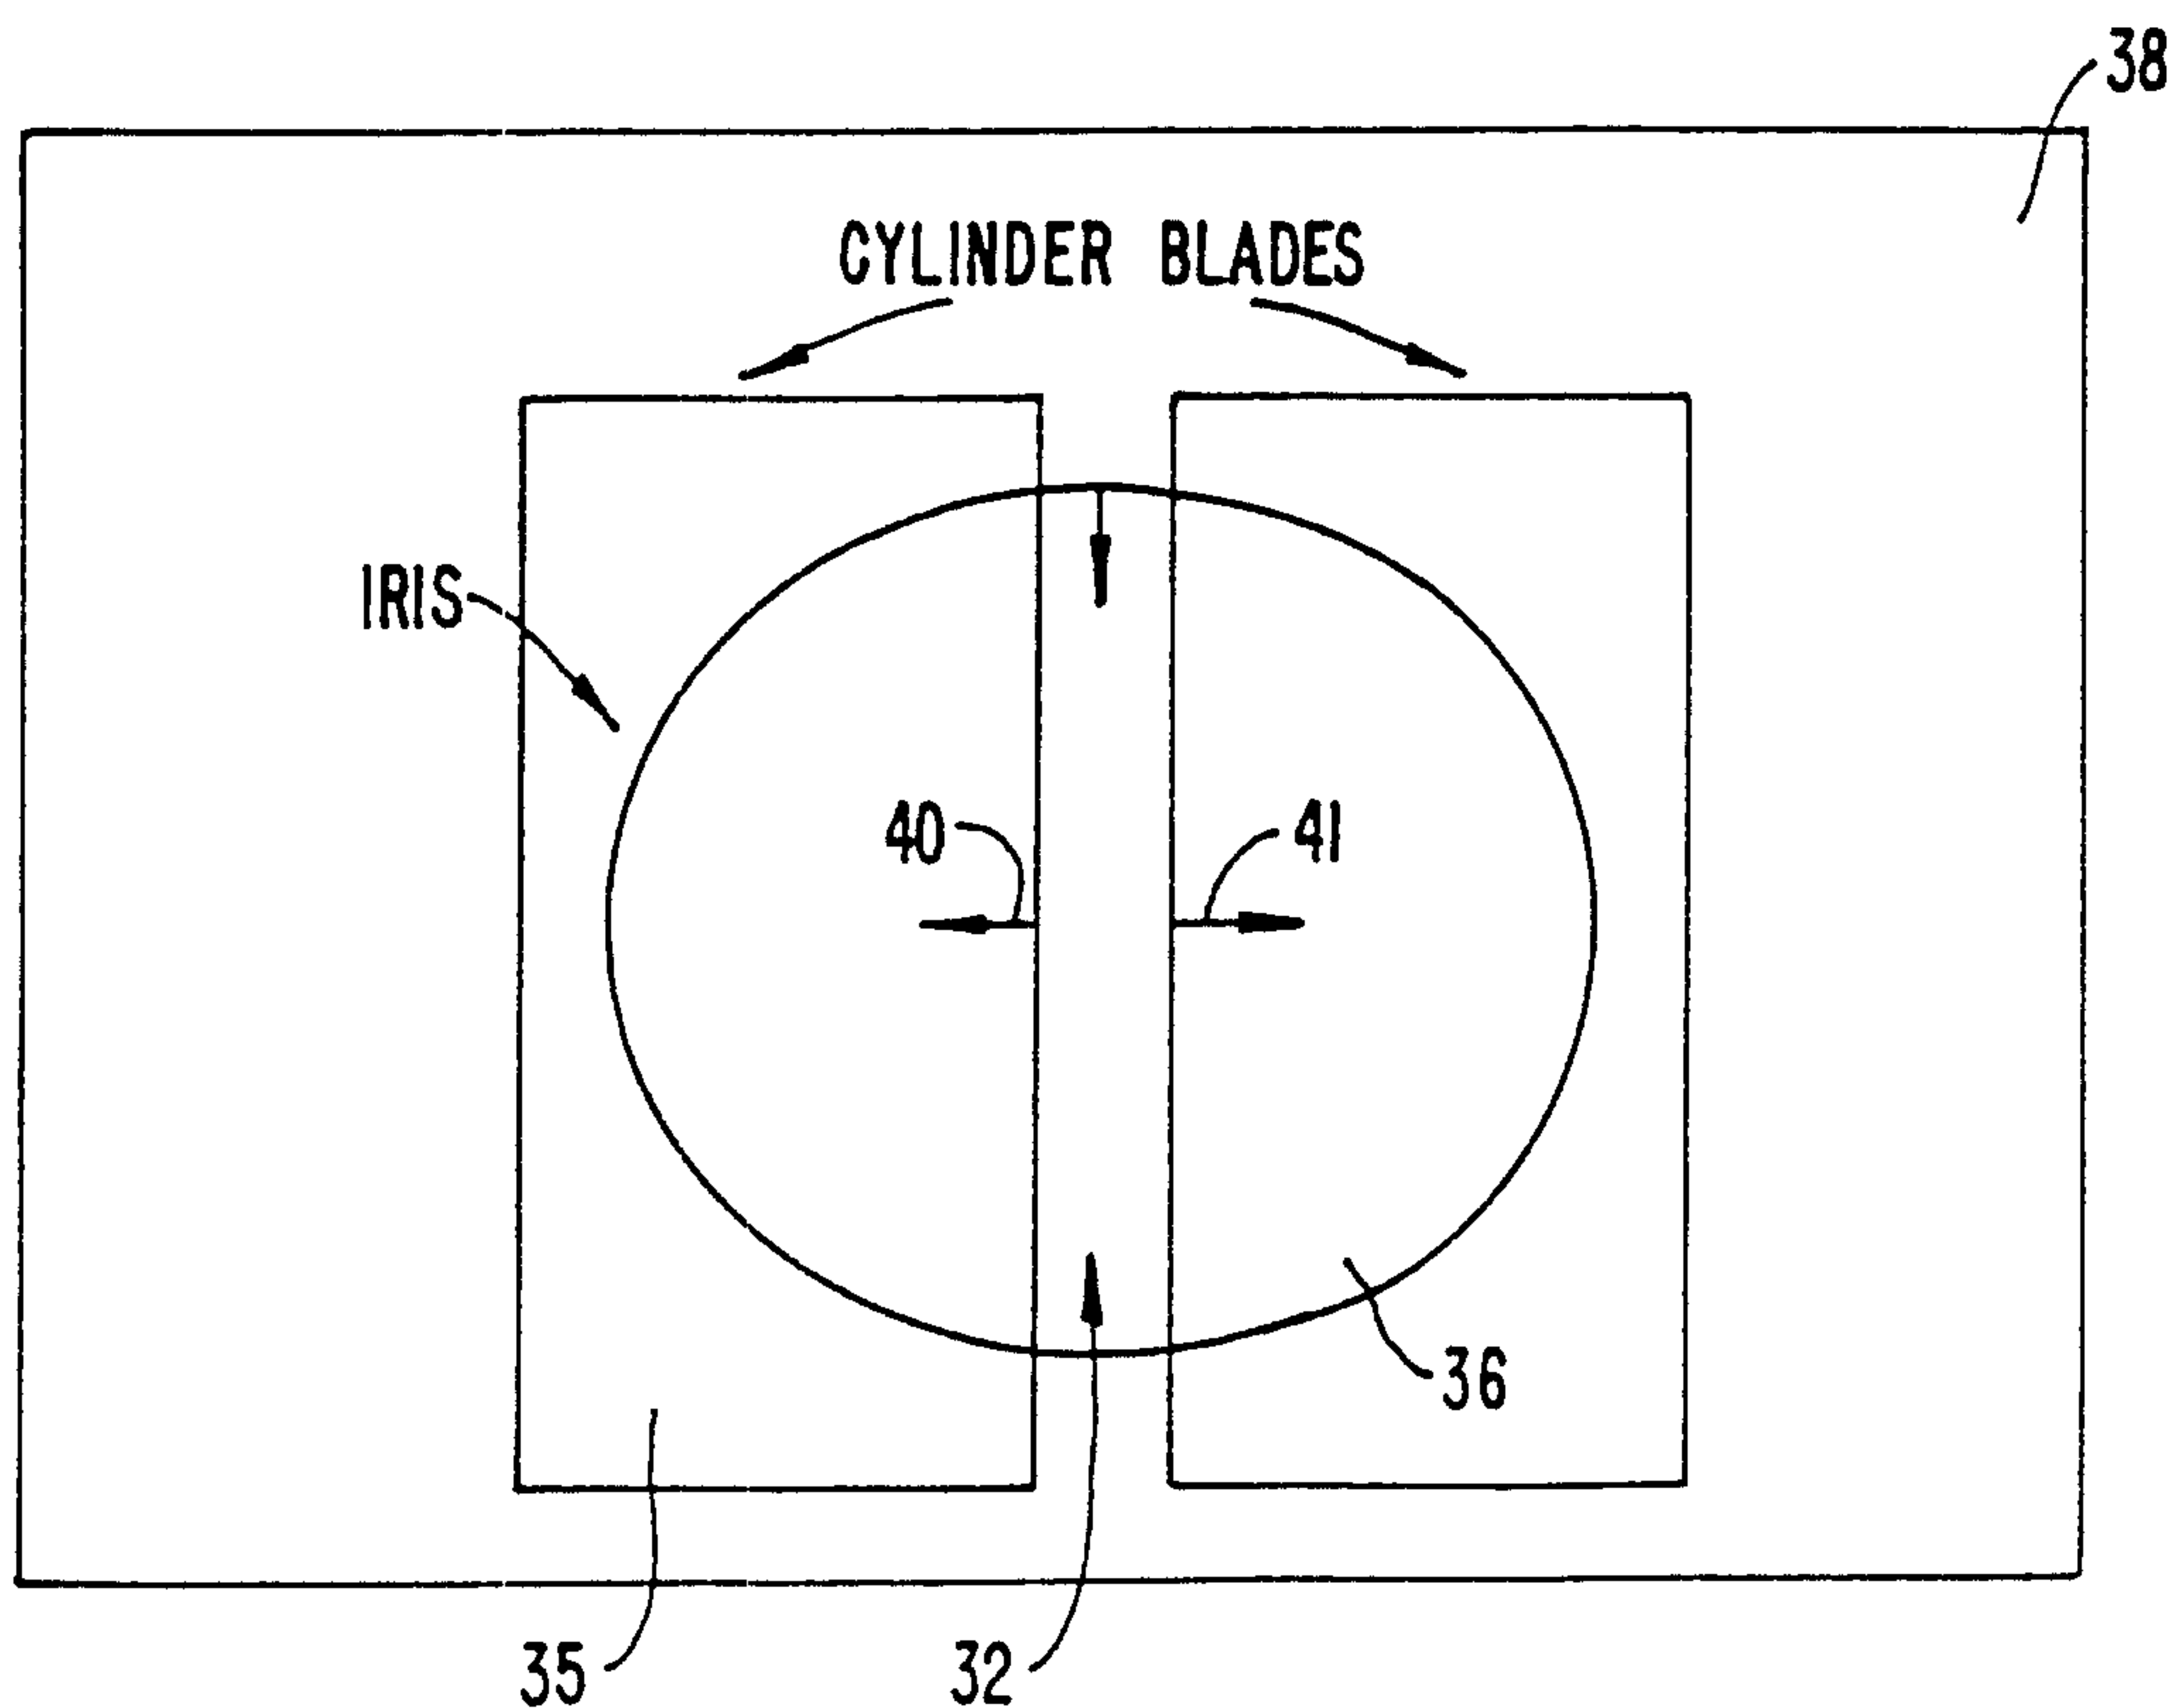


FIG. 2.

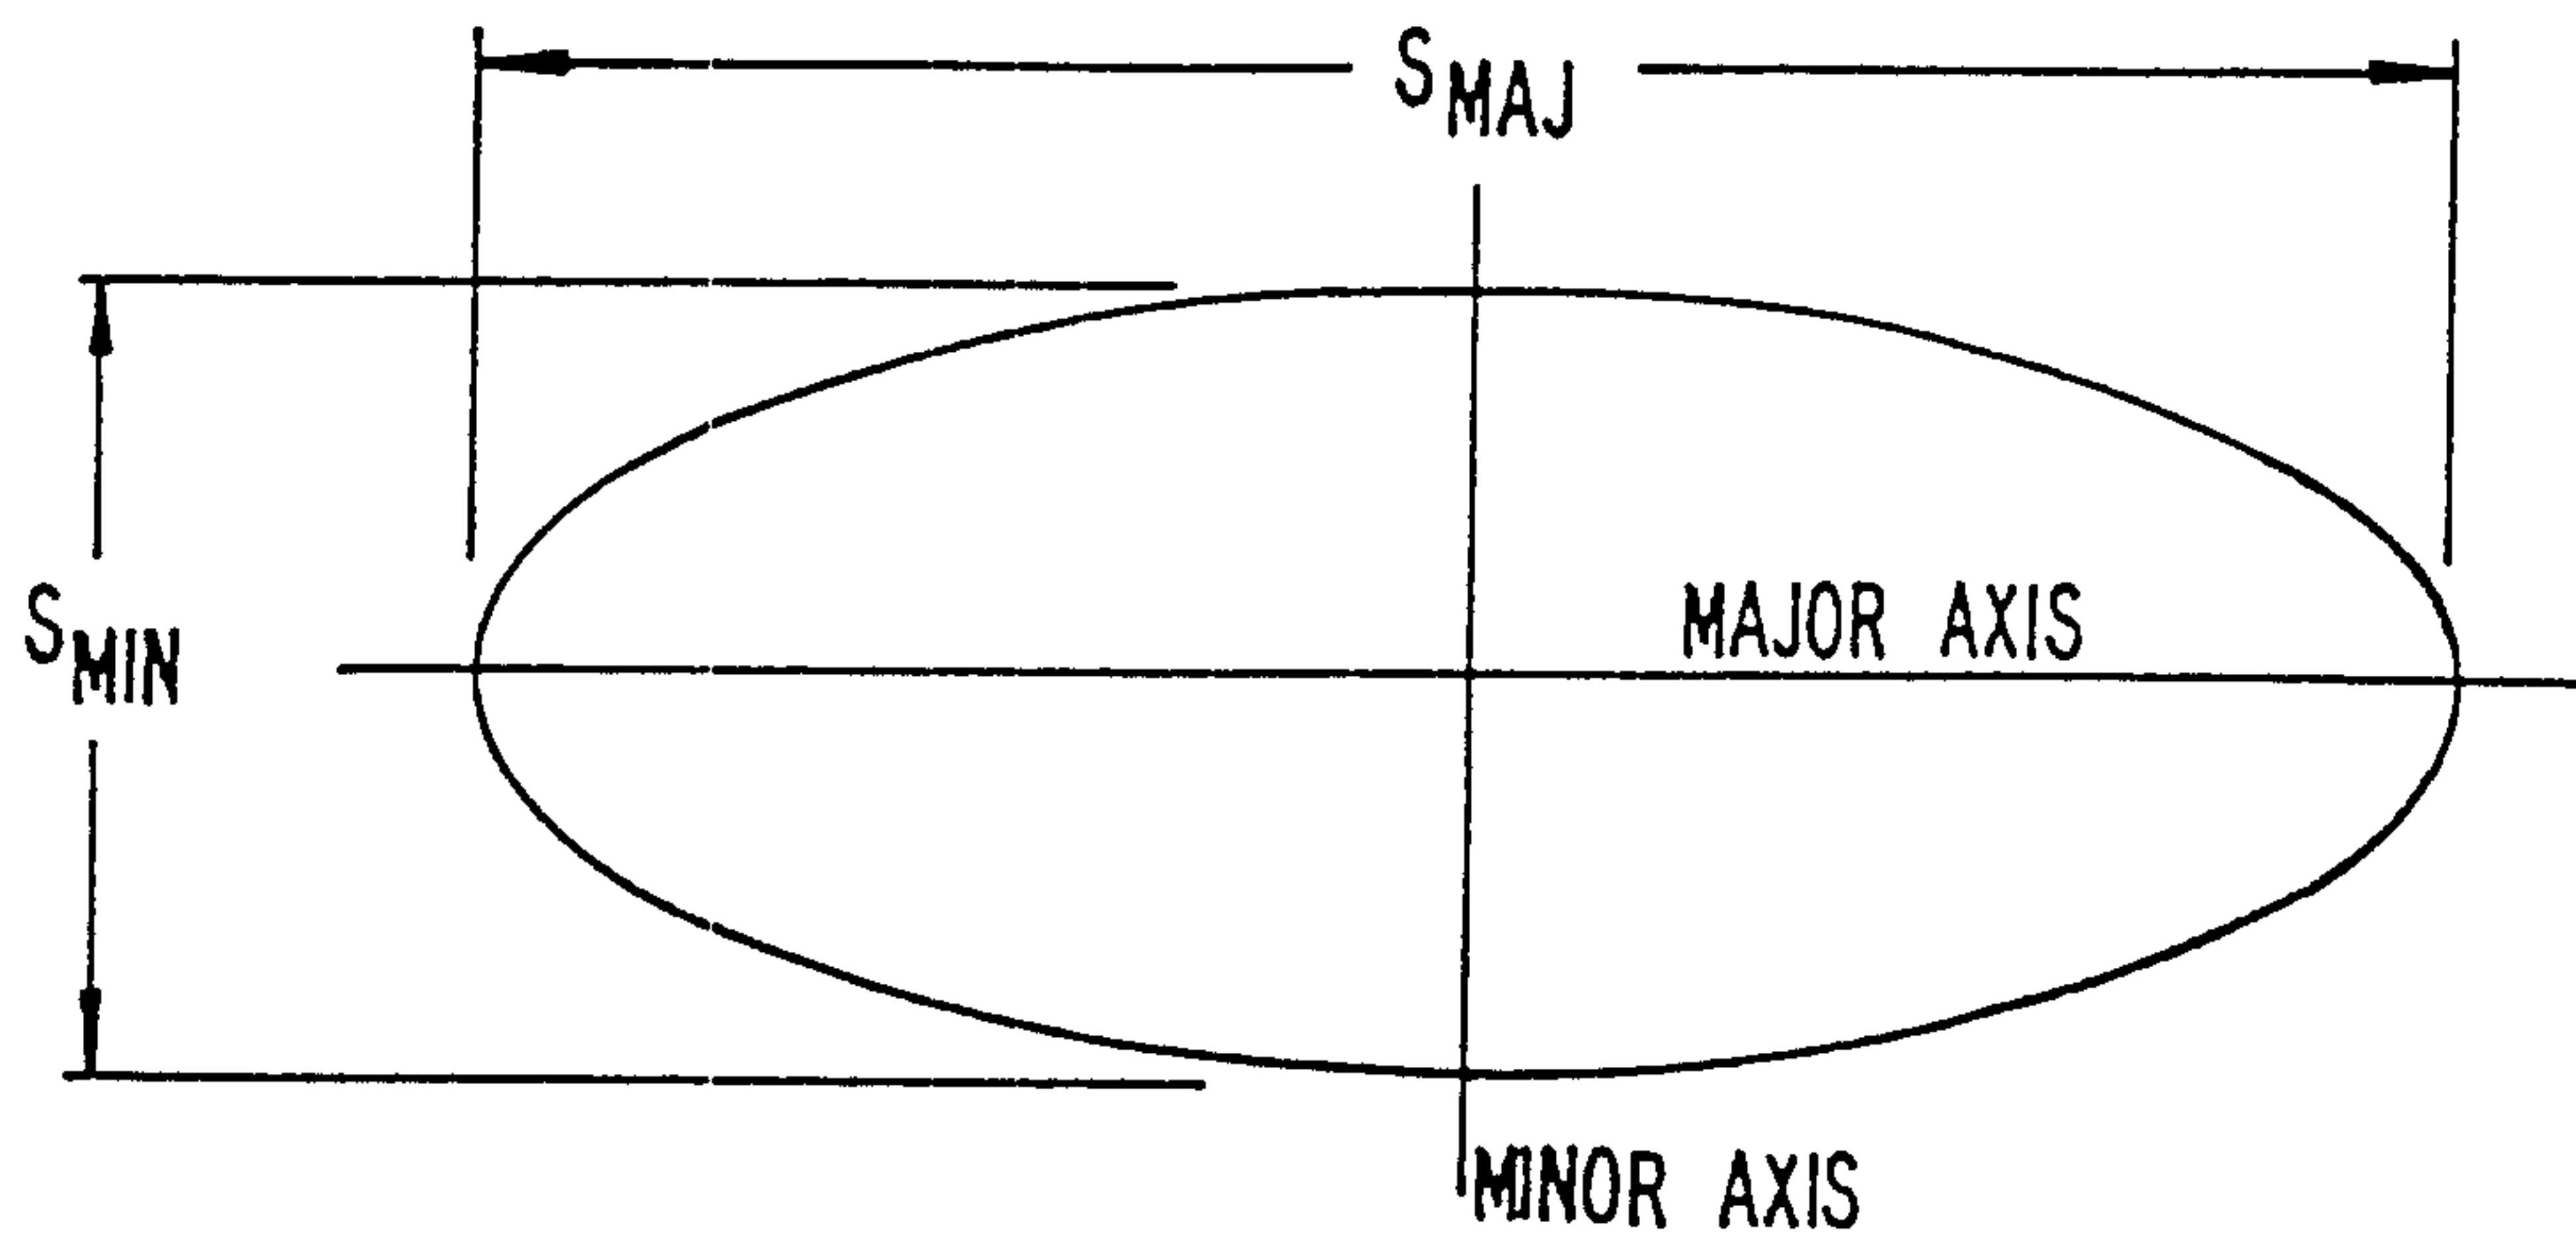


FIG. 3.

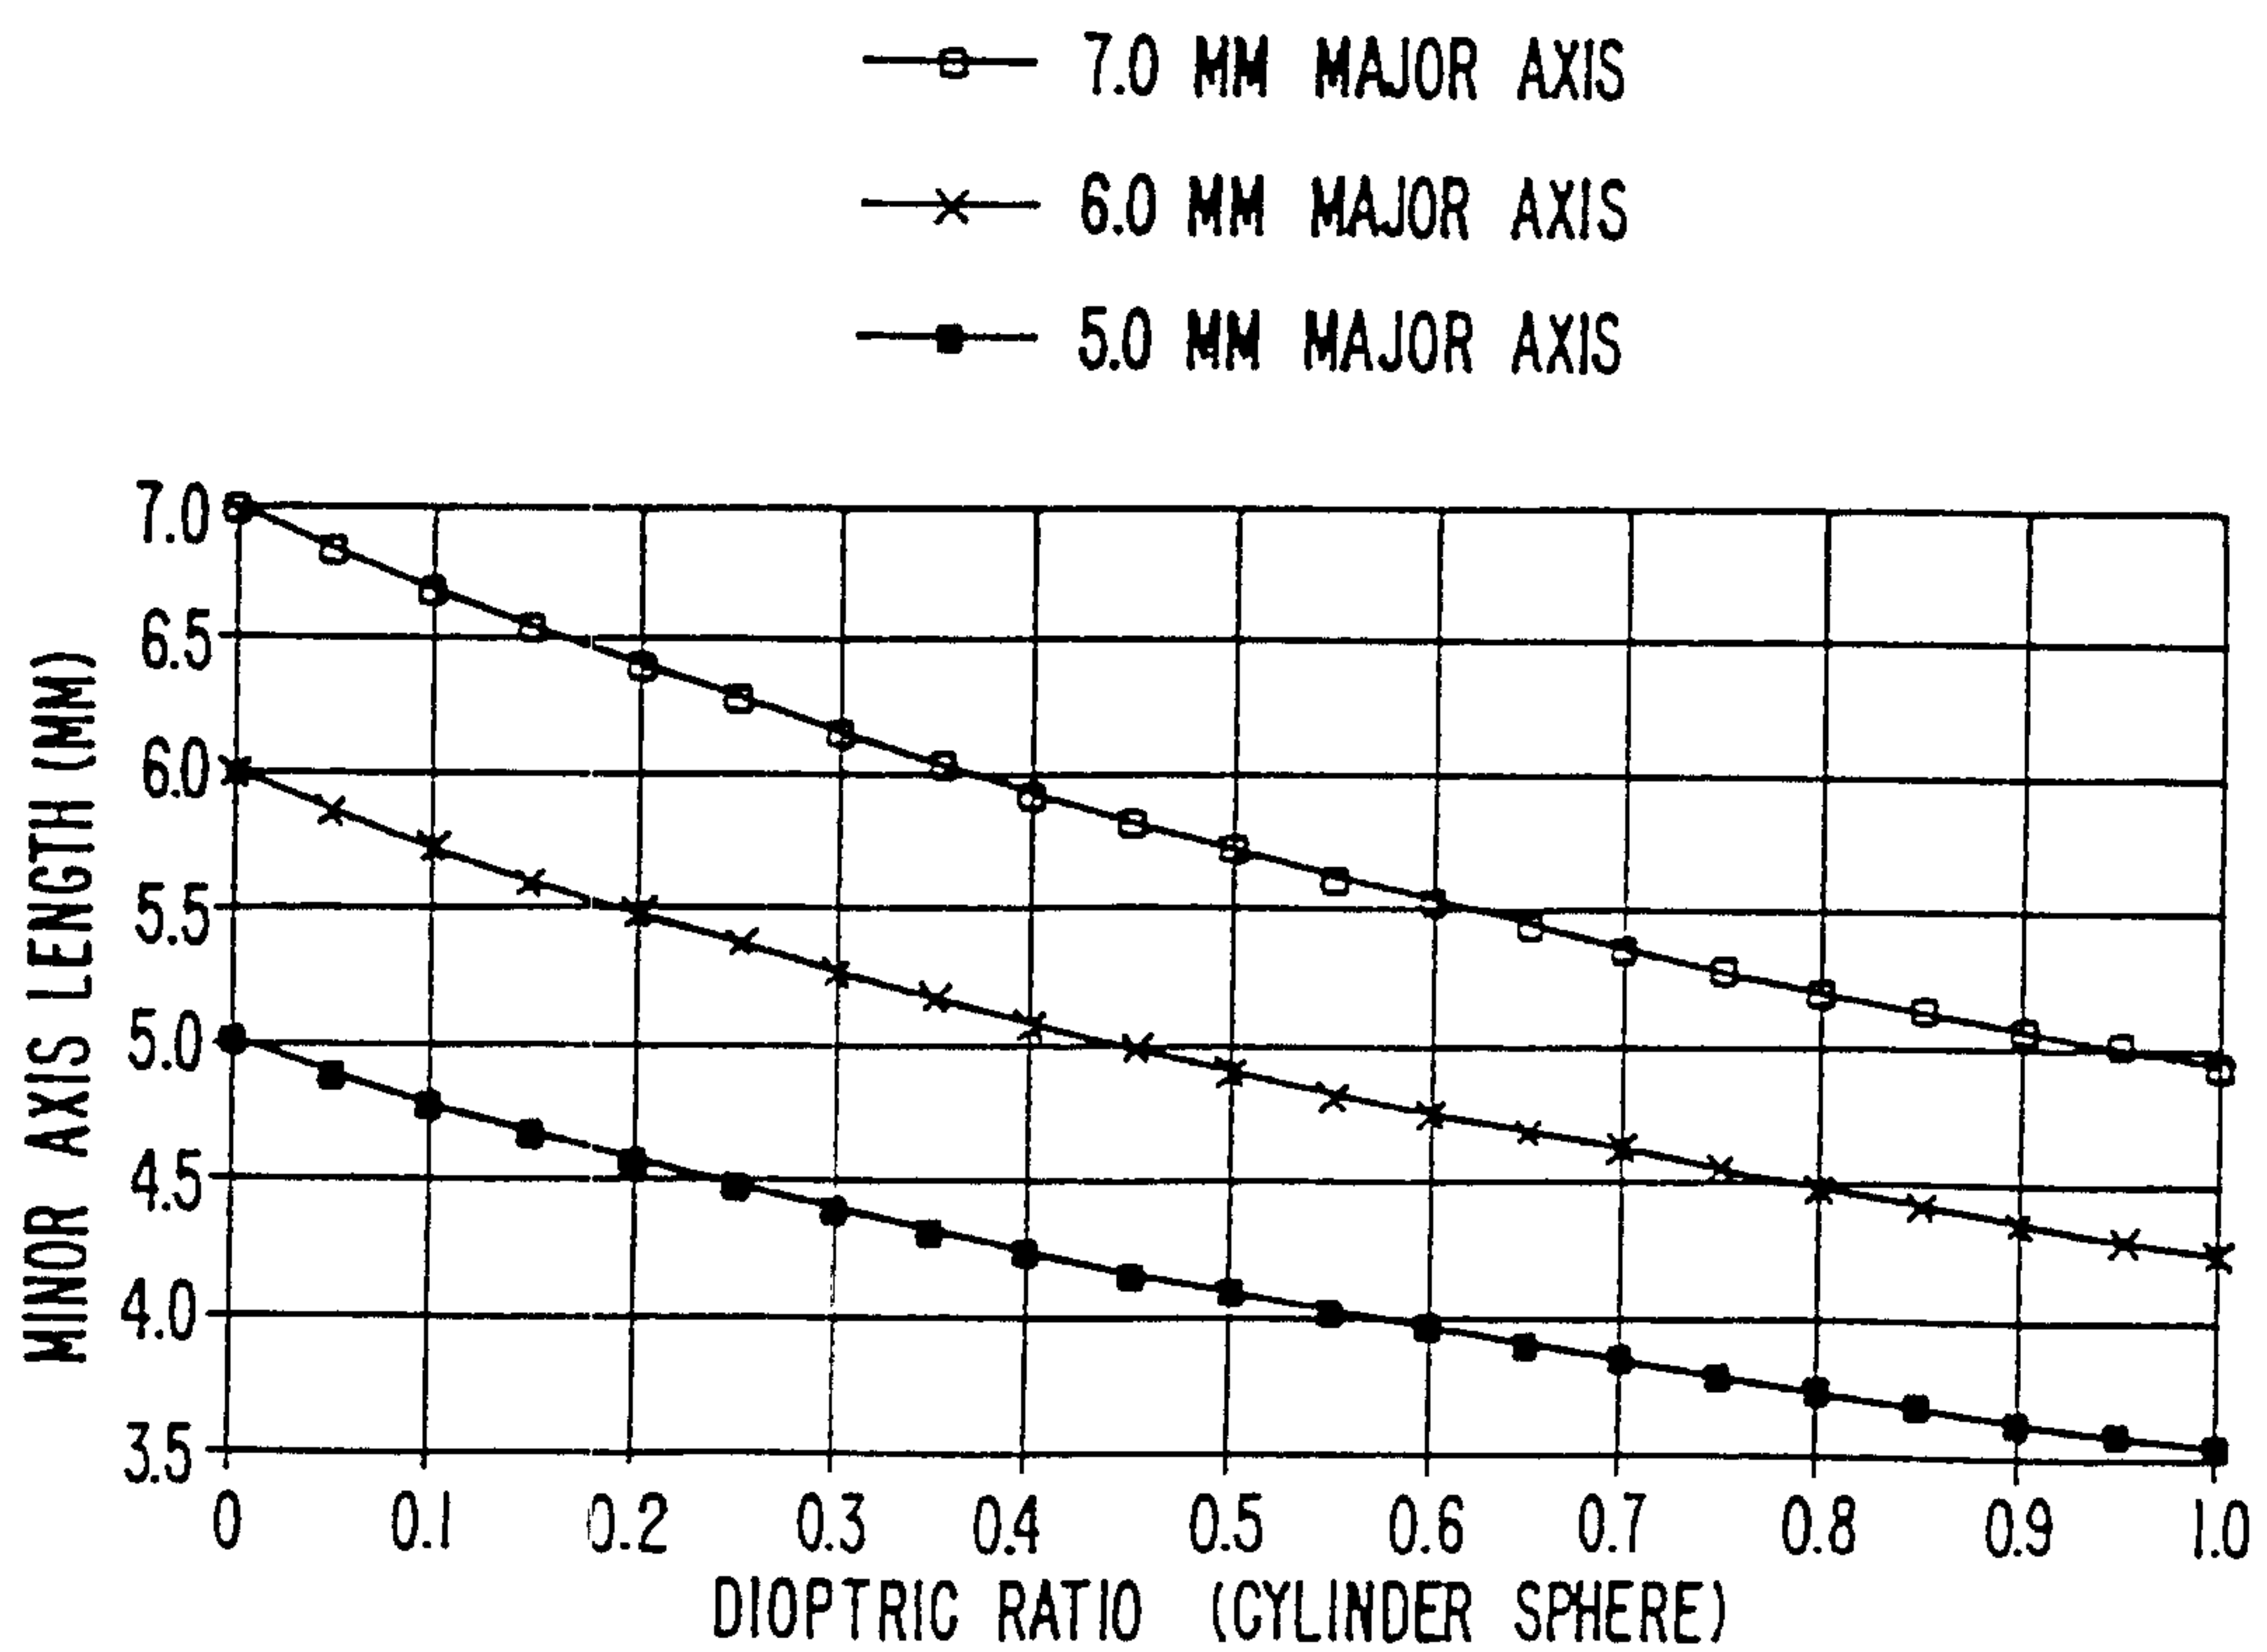


FIG. 4.

