



US00D732058S

(12) **United States Design Patent**
Landis et al.

(10) **Patent No.:** **US D732,058 S**

(45) **Date of Patent:** **** Jun. 16, 2015**

(54) **DISPLAY SCREEN WITH COMPUTER ICON FOR BLOOD GLUCOSE MONITORING**

(71) Applicant: **LifeScan, Inc.**, Milpitas, CA (US)

(72) Inventors: **Jeremy Landis**, New York, NY (US);
Salve Retuta Pascual, Washington, DC (US)

(73) Assignee: **LifeScan, Inc.**, Wayne, PA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/496,566**

(22) Filed: **Jul. 15, 2014**

D563,972 S *	3/2008	Sherry	D14/487
D590,410 S *	4/2009	Wall et al.	D14/486
D594,911 S	6/2009	Hall et al.		
D598,923 S	8/2009	Chen et al.		
D599,810 S *	9/2009	Scalisi et al.	D14/485
D599,814 S *	9/2009	Ogura et al.	D14/489
D606,092 S *	12/2009	Danton	D14/489
D607,467 S *	1/2010	Westermair	D14/486
7,689,585 B2	3/2010	Zeng et al.		
D618,695 S	6/2010	Bennett et al.		
D619,593 S *	7/2010	Fujioka et al.	D14/485
D628,584 S *	12/2010	Umezawa	D14/489
7,913,177 B1 *	3/2011	Smith et al.	715/762
D638,024 S	5/2011	Wall et al.		
D640,285 S *	6/2011	Woo	D14/487
D650,392 S *	12/2011	Glezer et al.	D14/486
D650,790 S *	12/2011	Jeans et al.	D14/488
D654,084 S	2/2012	Joseph		

(Continued)

Related U.S. Application Data

(60) Division of application No. 29/393,126, filed on May 31, 2011, now Pat. No. Des. 709,901, which is a continuation of application No. 13/192,348, filed on Jul. 27, 2011.

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC G06F 3/048; G06F 3/0481; G06F 3/04817
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,034,682 A *	3/2000	Neumann et al.	715/703
6,437,804 B1	8/2002	Ibe et al.		
D502,184 S	2/2005	Glezer et al.		
7,020,847 B1	3/2006	Holzheuer		
7,051,279 B2 *	5/2006	Simonyi	715/705
D525,264 S *	7/2006	Chotai et al.	D14/486
D545,231 S *	6/2007	Waldman	D10/125
D545,324 S *	6/2007	Decombe	D14/485
D554,654 S *	11/2007	Waldeck	D14/486

Primary Examiner — Kevin Rudzinski

(57) **CLAIM**

We claim the ornamental design for a display screen with computer icon for blood glucose monitoring, as shown and described.

DESCRIPTION

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawing(s) will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 illustrates a front view of a display screen with computer icon for blood glucose monitoring showing our new design;


FIG. 2 illustrates a second embodiment thereof;

FIG. 3 illustrates a third embodiment thereof; and,

FIG. 4 illustrates a fourth embodiment thereof.

The broken lines shown in the drawings illustrate portions of the graphical user interface and display screen and form no part of the claimed design.

1 Claim, 4 Drawing Sheets
(4 of 4 Drawing Sheet(s) Filed in Color)

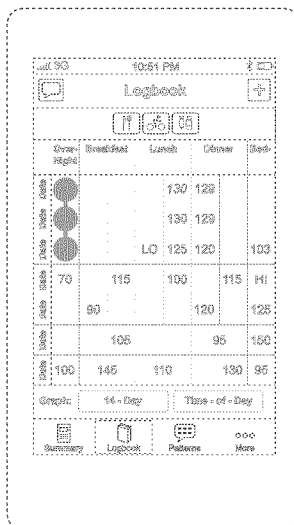

(56)

References Cited

U.S. PATENT DOCUMENTS

D654,925 S *	2/2012	Nishizawa et al.	D14/488	D711,395 S *	8/2014	Hanson et al.	D14/485
D656,946 S	4/2012	Judy et al.		D711,420 S *	8/2014	Agnew	D14/488
D658,204 S	4/2012	Jones		D711,896 S *	8/2014	Hanson et al.	D14/485
D667,022 S	9/2012	Lobosco et al.		8,798,934 B2 *	8/2014	Wei et al.	702/19
D674,404 S	1/2013	Pearcy et al.		8,816,862 B2 *	8/2014	Harper et al.	340/573.1
D681,656 S *	5/2013	Lawrence et al.	D14/486	D714,315 S *	9/2014	Pereira	D14/485
D682,301 S *	5/2013	DiJulio et al.	D14/487	D714,316 S *	9/2014	Pereira	D14/485
D682,304 S *	5/2013	Mierau et al.	D14/488	D714,317 S *	9/2014	Pereira	D14/485
D682,305 S *	5/2013	Mierau et al.	D14/488	D714,320 S *	9/2014	Pereira	D14/485
D693,829 S *	11/2013	Edwards et al.	D14/485	D714,321 S *	9/2014	Pereira	D14/485
D693,836 S *	11/2013	Bouchier	D14/486	D714,322 S *	9/2014	Pereira	D14/485
D693,837 S *	11/2013	Bouchier	D14/486	D714,325 S *	9/2014	Pereira	D14/485
D694,764 S *	12/2013	Talbot et al.	D14/485	2002/0145623 A1 *	10/2002	Decombe	345/734
D694,769 S *	12/2013	Edwards et al.	D14/485	2002/0156814 A1 *	10/2002	Ho	707/514
D697,074 S *	1/2014	Waldman	D14/485	2007/0156742 A1 *	7/2007	Gonzalez	707/102
D698,817 S *	2/2014	Laverack et al.	D14/489	2008/0081653 A1 *	4/2008	Mock et al.	455/518
D699,250 S *	2/2014	Fujii et al.	D14/486	2009/0135186 A1 *	5/2009	Tsubota et al.	345/442
D704,204 S *	5/2014	Rydenhag	D14/486	2009/0228832 A1 *	9/2009	Cheng	715/810
D704,734 S *	5/2014	Wafapoor	D14/489	2009/0276724 A1	11/2009	Rosenthal et al.	
D709,901 S *	7/2014	Landis et al.	D14/486	2010/0105999 A1	4/2010	Dixon et al.	
D710,863 S *	8/2014	Agnew	D14/485	2010/0333029 A1 *	12/2010	Smith et al.	715/834
D711,394 S *	8/2014	Hanson et al.	D14/485	2011/0053121 A1	3/2011	Heaton	
				2011/0264378 A1 *	10/2011	Breton et al.	702/19
				2013/0035575 A1 *	2/2013	Mayou et al.	600/365

* cited by examiner

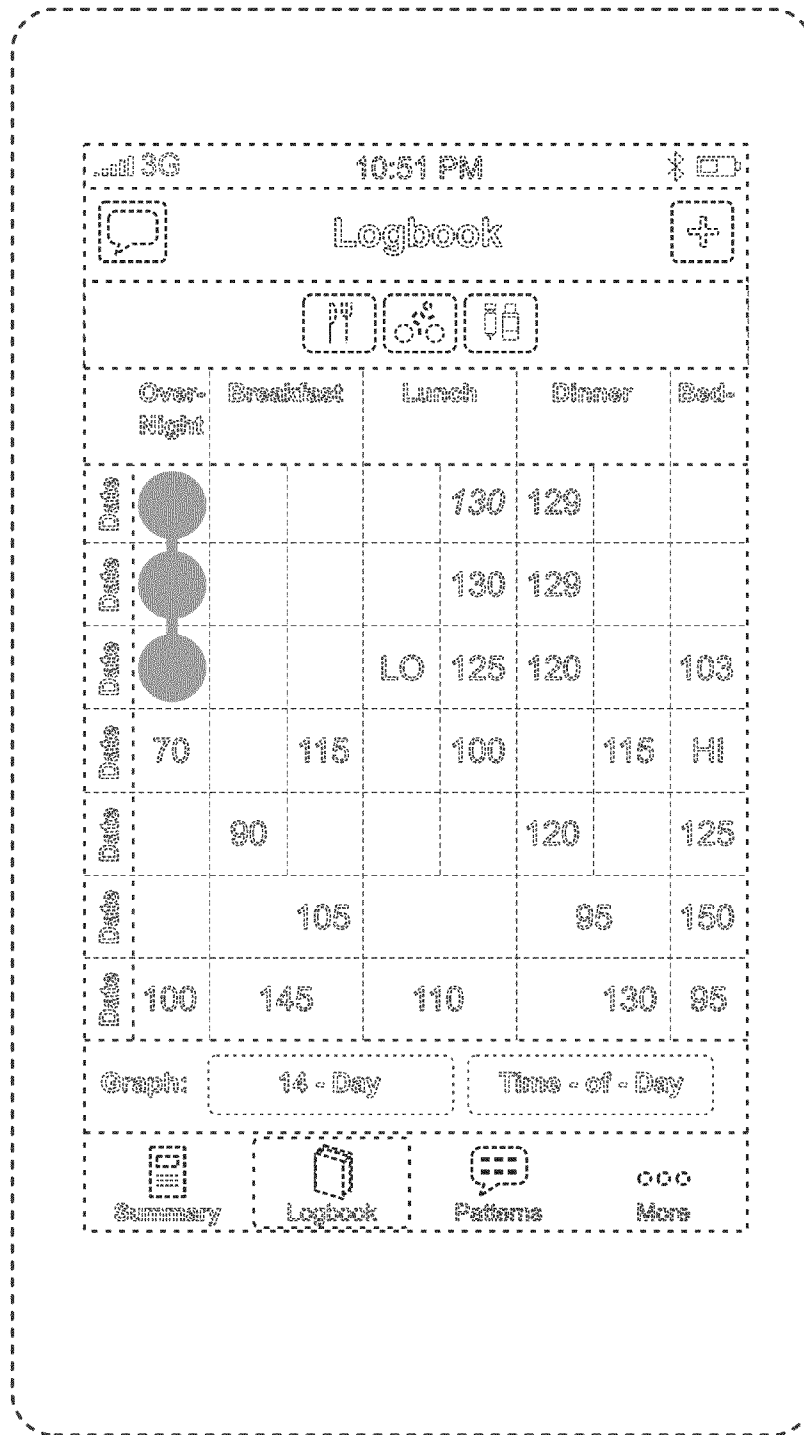


FIG. 1

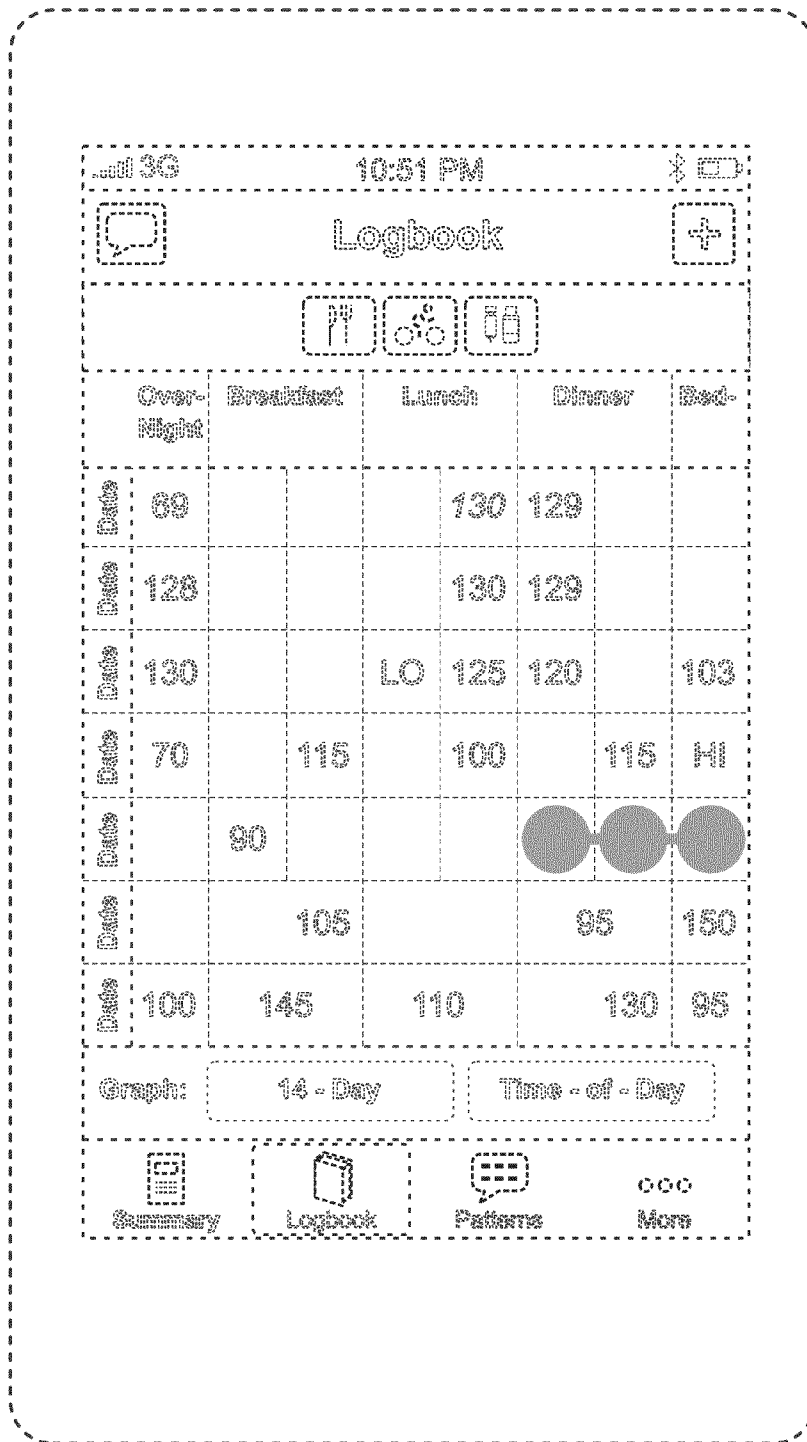


FIG. 2

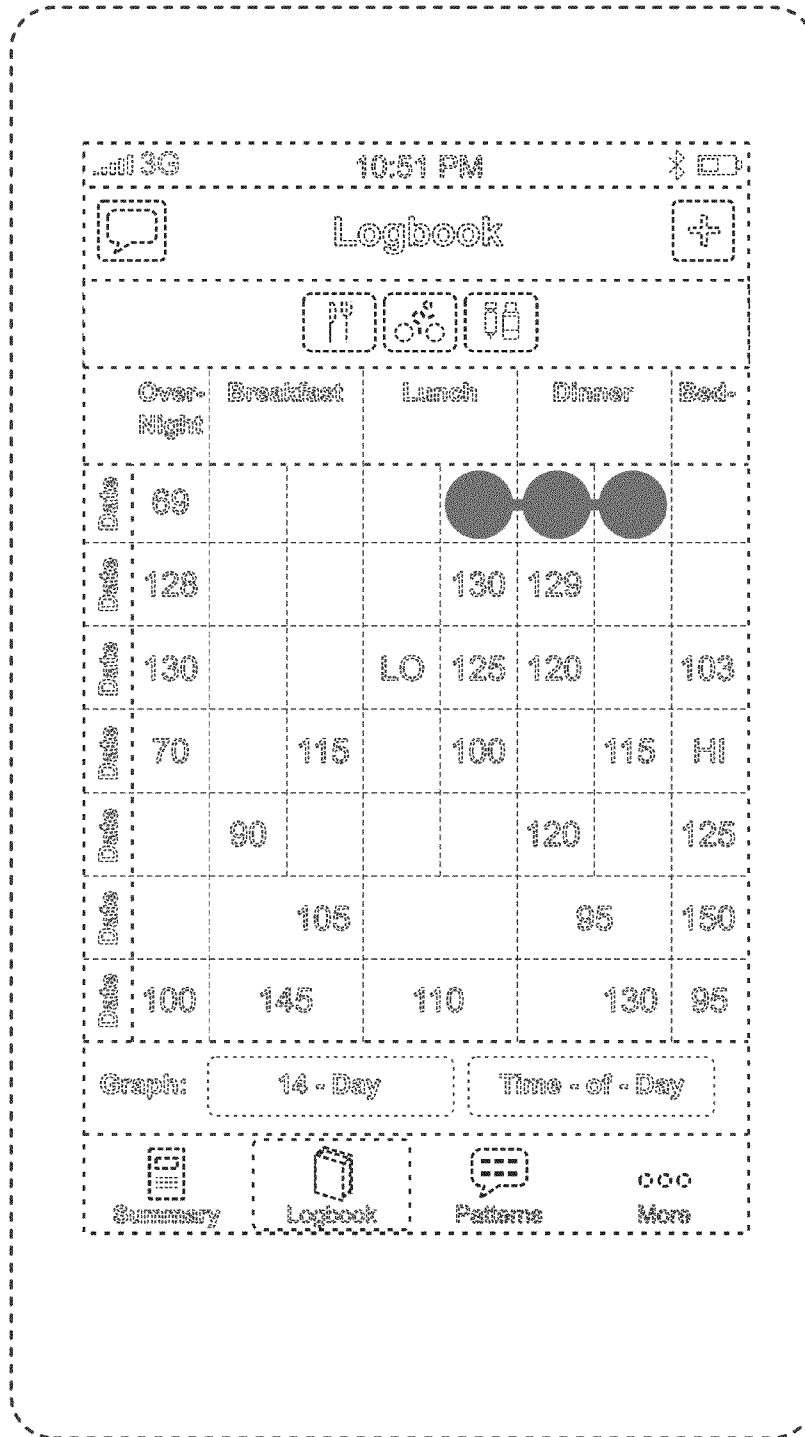


FIG. 3

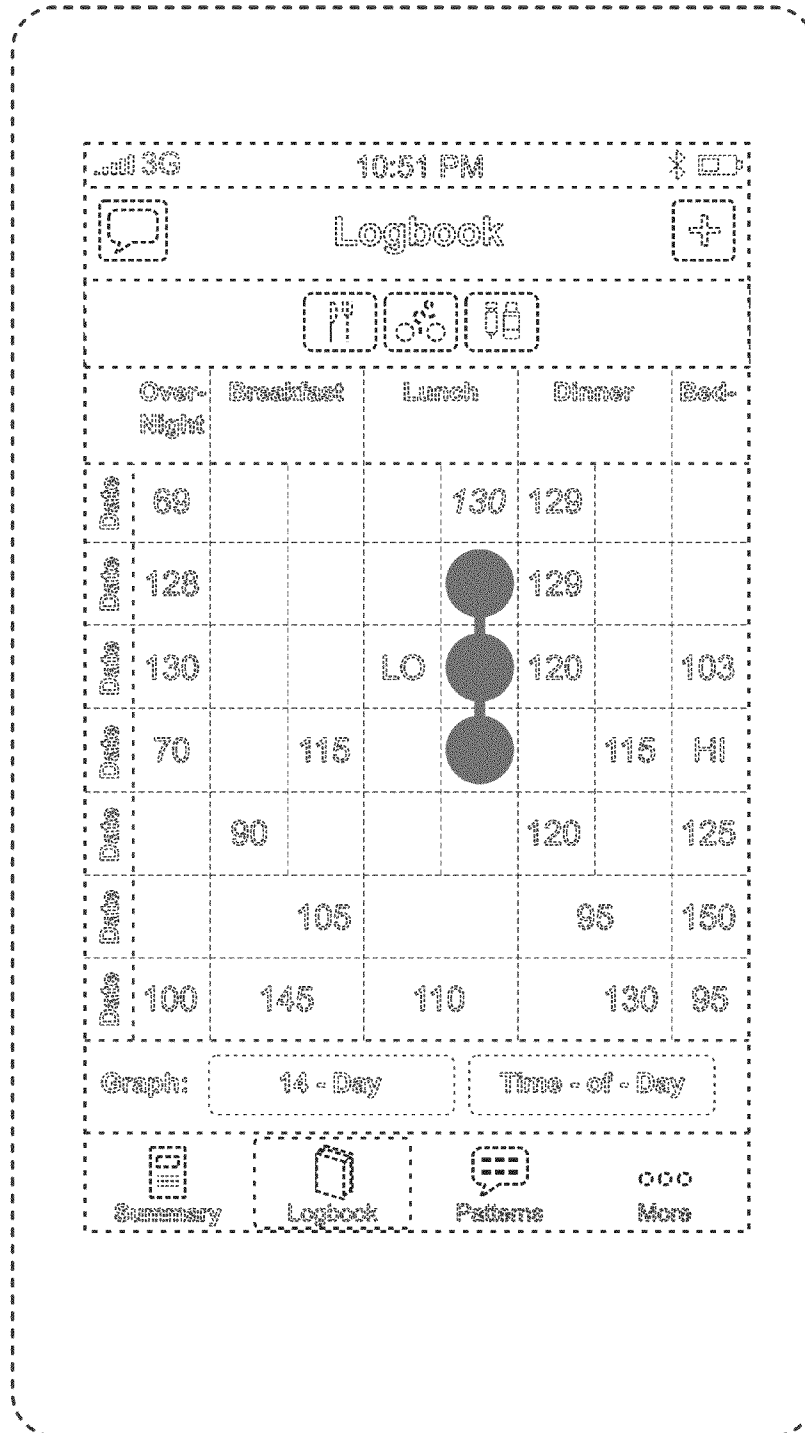


FIG. 4