



(11) **EP 1 586 340 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
08.06.2011 Bulletin 2011/23

(51) Int Cl.:
A61M 1/06 ^(2006.01)

(21) Application number: **05252269.5**

(22) Date of filing: **12.04.2005**

(54) **Breast pump**

Brustpumpe

Pompe à lait

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU MC NL PL PT RO SE SI SK TR**

(30) Priority: **12.04.2004 US 821924**

(43) Date of publication of application:
19.10.2005 Bulletin 2005/42

(73) Proprietor: **Sea Profit (Hong Kong) Limited**
Kwun Tong,
Kowloon (HK)

(72) Inventor: **Yuen, Yat Keung William**
Lam Tin
Kowloon (HK)

(74) Representative: **Brookes Batchellor LLP**
102-108 Clerkenwell Road
London
EC1M 5SA (GB)

(56) References cited:
US-A- 5 542 921 US-B1- 6 547 756
US-B1- 6 673 036

EP 1 586 340 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] This invention relates to a breast pump and, in particular, an electrically operated breast pump for drawing milk from a user.

Background of the Invention

[0002] There are in existence a large number of electrically operated breast pumps, allowing a user, e.g. a mother, to pump milk from her breast. Various pumping mechanisms have been proposed for drawing milk from the mother's breast, including, for example, ones disclosed in US Patent Nos. 6,045,529 and 6,355,012 issued to Nüesch. Such mechanisms are generally speaking rather complicated, and thus costly to manufacture. In addition, most such mechanisms include gear trains which would generate much noise, especially when the motor is operating at a relatively high speed.

[0003] In addition, although a user may, with some existing breast pumps, be able to adjust the pumping cycles, e.g. by varying the number of suction cycles per minute, or adjusting the vacuum level for pumping milk from the user's breast, it is up to the user to decide whether to make such variation or adjustment, and the user may simply have no information on which to decide whether the current pumping rate is suitable or not. In this connection, US Patent No. 6,547,756 issued to Greter et al. discloses a programmable breast pump which may be programmed to generate a number of different milk expression (extraction) sequences, or curves. In this arrangement, a motorized pump is provided with a microprocessor-based controller. Cards, with microprocessor "chips", containing instructions for different suction curves are also included, which may be inserted into the breast pump, so that the instructions in the cards may be read and acted upon by the breast pump. However, as in the case of other adjustable breast pumps discussed above, it is still up to a user to decide whether to change the mode of pumping operation of the breast pump, and a user may not know whether an alternative, and if so which, suction curve should be applied. A further shortcoming associated with conventional electric breast pumps is that the user is provided with no information as to the time required to fill up the milk receptacle, e.g. bottle.

[0004] Such and other shortcomings discussed above are also present in breast pumps disclosed in US Patent No. 6,673,036 issued to Britto which discloses a pump as defined in the preamble of claim 1 and US Patent No. 6,090,065 issued to Giles.

[0005] It is thus an object of the present invention to provide an electric breast pump in which the aforesaid shortcomings are mitigated or at least to provide a useful alternative to the public.

Summary of the Invention

[0006] According to the present invention, there is provided an electric breast pump as defined in the claims.

Brief Description of the Drawings

[0007] A preferred embodiment of the present invention will now be described, by way of example only, with reference to the accompanying drawings, in which:

Fig. 1 is a perspective view of an electric breast pump according to the present invention;

Fig. 2 is an exploded view of the breast pump shown in Fig. 1;

Fig. 3 is a sectional view of the breast pump shown in Fig. 1;

Fig. 4 is a sectional view taken along the line A-A in Fig. 3;

Fig. 5 is a circuit diagram of the breast pump shown in Fig. 1;

Fig. 6 shows part of the circuitry in the breast pump shown in Fig. 1;

Fig. 7 shows a liquid crystal display (LCD) setting in the breast pump shown in Fig. 1;

Fig. 8 is a block diagram of an exemplary microcontroller which may be used in the circuit shown in Fig. 5;

Fig. 9 is an enlarged view showing the engagement between the pump motor and the diaphragm in the breast pump shown in Fig. 1;

Fig. 10 is an enlarged sectional view of part of the breast pump shown in Fig. 3;

Fig. 11 is an enlarged perspective view showing the mechanism for manual adjustment of the level of vacuum in the breast pump shown in Fig. 1;

Fig. 12 shows a first configuration of the manual vacuum adjustment mechanism shown in Fig. 11;

Fig. 13 shows a second configuration of the manual vacuum adjustment mechanism shown in Fig. 11;

Fig. 14 shows an enlarged sectional view of the milk flow sensing mechanism in the breast pump shown in Fig. 1; and

Fig. 15 is a flow chart showing the steps of operation of the breast pump shown in Fig. 1.

Detailed Description of the Preferred Embodiment

[0008] Figs. 1 and 2 show an electrically operated breast pump according to a preferred embodiment of the present invention, generally designated as 10. The breast pump 10 has a hood 12 adapted to be fitted over a breast of a user in an essentially gas-tight manner, for pumping milk from the breast. An insert 12a for contacting the user's breast is received within the hood 12. The insert 12a is made of a soft plastic material, e.g. silicone, to provide comfort to the user during use. The hood 12 is in funnel shape and has a tunnel 14 leading to a con-

nector 16, which fluidly communicates with the hood 12, and with a milk-receiving bottle 18 *via* a valve seat 20, the structure and function of which will be further discussed below.

[0009] The connector 16 is engaged with a head portion 22 which houses most of the operating components of the breast pump 10, as will be clear from the ensuing discussion. On a top surface 24 of the head portion 22 is provided with an ON/OFF button 26 for selectively activating/deactivating the breast pump 10. Also provided on the top surface 24 of the head portion 22 is a liquid crystal display (LCD) 28 for displaying various operation information and data relating to the operation of the breast pump 10. The head portion 22 is connected with a handle 30, which also acts as a battery compartment for housing a number of batteries 32 for powering the breast pump 10. The handle 30 is swivellable relative to the head portion 22 for easy handling. On each side of the handle 30 is provided a PAUSE button 34, allowing a user to temporarily suspend the operation of the breast pump 10 by pressing the button 34 once, and to resume its operation by pressing the button 34 once again. On a side of the head portion 22 is a power jack 36 which allows the breast pump 10 to be powered by an A/C source, possibly *via* a transformer (not shown).

[0010] Fig. 3 shows a sectional view of the breast pump 10. As shown in Fig. 3, provided in a chamber 37 of the connector 16 are two infrared (IR) units 38a, 38b, each including an IR transmitter and an IR receiver. Housed in the head portion 22 is a pump motor 42 for operating a pump diaphragm 44 for generating a low pressure (vacuum) in the breast pump 10. Within the handle 30 is a valve motor 46 for operating a needle valve 48. The valve 48 is pneumatically connected, e.g. *via* a hose (not shown), with a nozzle 50 which is in turn pneumatically connected with the milk-receiving bottle 18.

[0011] Housed in the head portion 22 is a microcontroller 40 for controlling the operation of various electronic and electrical components of the breast pump 10. As shown in Fig. 5, the microcontroller 40 is electrically connected with and controls the operation of the pump motor 42, the valve motor 46, and the LCD display 28. The microcontroller 40 is also connected with and receives instructions and/or signals from the PAUSE buttons 34 and the IR units 38a, 38b. Fig. 6 shows in more detail a circuitry which controls the operation of the valve motor 46, the pump motor 42, and the IR units 38a, 38b, of which only one set 38a is shown here.

[0012] Fig. 7 shows the setting of the LCD display 28, and it can be seen that the LCD display 28 may display such information as the setting being used, the flow-rate (slow, medium, high), battery low, and the remaining time (in minutes) required for filling the bottle 18.

[0013] A microcontroller 40 suitable for use in the breast pump 10 may be one traded by Sino Wealth Microelectronics Corporation Limited, of Hong Kong, under serial number SH6622A, although other similar microcontrollers may also be used. SH6622A is a 4-bit micro-

controller, which integrates a 4-bit CPU core with SRAM, 4K program ROM, timer and I/O Port Fig. 8 shows a block diagram of SH6622A. The CPU of SH6622A contains the following function blocks: Program Counter, Arithmetic Logic Unit (ALU), Carry Flag, Accumulator, Table Branch Register, Data Pointer (INX, DPH, DPM, and DPL), and Stack.

[0014] Fig. 9 shows an enlarged perspective view of the pump motor 42, having an output spindle 51 engaged with an eccentric cam 52 which in turn carries a yoke 54 fixed with the pump diaphragm 44. By way of such an arrangement, rotational movement of the output pin 51 is converted into linear reciprocal movement of the diaphragm 44 in the direction of the bi-directional arrow L-L.

[0015] As can be clearly seen in Fig. 10, fixed to the output spindle 51 of the pump motor 42 is a linkage mechanism 58 comprising six links 60 linked with one another in a hexagonal ring-shaped structure. Each link 60 is swivellable relative to two adjacent links 60 to which it is pivotally hinged. Over the output spindle 51 is also provided with a spring 62 which biases an end pin 64 outwardly, which in turn acts on and biases a lid 66 away from a vent hole 68. The diaphragm 44 is positioned in a chamber 71 which is closeable by the lid 66, a first one-way valve 70, and a second one-way valve 74. The first one-way valve 70 only allows air to enter the chamber 71 from a conduit 72, which is in turn in fluid communication with the hood 12. The second one-way valve 74 only allows air to exit the chamber 71.

[0016] When the motor 42 is not in operation, the linkage mechanism 58 will be biased by the spring 62 to assume the shape and configuration as shown in Figs. 3 and 10. During operation of the pump motor 42, rotation of the output spindle 51 will bring about simultaneous and corresponding rotation of the linkage mechanism 58, whereby the hexagonal ring-shaped structure 58 will "flatten" because of the centrifugal force generated by the rotation, thus retracting the end pin 64 against the outward biasing force of the spring 62. The lid 66 will thus close the vent hole 68. With the vent hole 68 closed by the lid 66, linear reciprocal movement of the diaphragm 44 in the direction of the bi-directional arrow L-L will draw air from the hood 12, through the conduit 72 and the first one-way valve 70, into the chamber 71, and push the air out through the second one-way valve 74, thus generating a lower pressure ("vacuum") in the hood 12 relative to the outside atmospheric pressure, and mimicking a sucking action of a baby on a mother's breast. The sucking/releasing cycle is completed by a releasing action when the motor 42 stops rotation. Upon stopping of the motor 42, the linkage mechanism 58 will, under the biasing force of the spring 62, resume the stable shape and configuration as shown in Figs. 3 and 10, whereupon the lid 66 will be pushed by the end pin 64 away from the vent hole 68, to thereby open the vent hole 68. When the vent hole 68 is opened, air will enter the vent hole 68, and then back into the hood 12, thus releasing the "vacuum" in the hood 12.

[0017] To allow further versatility of the breast pump 10, a manual pressure adjustment mechanism is provided, allowing the user to manually adjust the level of "vacuum" applied during operation of the breast pump 10, to suit individual need in different times. As shown in Fig. 11, the manual pressure adjustment mechanism includes a wheel 80 with a gear 82 in mesh with a pinion 84 on an end of a pin 86 and a valve seat 88. As can be seen in Figs. 10, 12 and 13, the wheel 80 is fixed to the handle 30 for rotational movement. The wheel 80 may be moved by a thumb of a user to rotate relative to the handle 30, about the longitudinal axis of the wheel 80. The valve seat 88 is also fixedly secured to the handle 30. Byway of such an arrangement, and because of the engagement between the gear 82 and the pinion 84, rotation of the wheel 80 will cause the pin 86 to move in or out of a recess 90 in the valve seat 88. In particular, rotation of the wheel 80 in the direction indicated by the arrow F in Fig. 12 will retrieve the pin 86 from the recess 90, whereas rotation of the wheel 80 in the direction indicated by the arrow R in Fig. 13 will insert the pin 86 further into the recess 90.

[0018] The valve seat 88 is made of a thermoplastic elastomer (TPE) or silicone, and when the pin 86 is fully received within the recess 90, the valve seat 88 is fully sealed, whereas air may enter the valve seat 88 if the pin 86 is retrieved from the valve seat 88, and the amount of air allowed to enter the valve seat 88 will depend on the extent to which the pin 86 is retrieved from the valve seat 88. The recess 90 is in fluid communication with a nozzle 92, which is in turn in fluid communication with the hood 12, e.g. via a hose (not shown) connected to the conduit 72, so that the pressure within the hood 12 when such is applied over a breast of a user may be fine-tuned by the user by manually operating the wheel 80.

[0019] When the breast pump 10 is fitted over a breast of a user and the pump motor 42 is activated, the pump diaphragm 44 will reciprocate to generate a lower pressure ("vacuum") in the hood 12, thus stimulating milk ejection reflex and subsequent expression of milk. Milk from the breast of the user will flow into the hood 12 and subsequently into the chamber 37 in the direction of the arrow M. The milk will accumulate in the chamber 37, first blocking the transmission of infrared signals between the transmitter and receiver of the lower IR unit 38a, and subsequently that between the transmitter and receiver of the upper IR unit 38b.

[0020] In the valve seat 20 is a one-way valve 96 which allows milk to enter the bottle 18, but not *vice versa*. Because the hood 12 is at a lower pressure than the bottle 18 during operation of the pumping action of the diaphragm 44, the higher pressure in the bottle 18 will prevent the milk in the chamber 37 from entering the bottle 18, thus allowing the milk level to rise in the chamber 37. It may take several sucking/releasing cycles before the milk level rises to, and blocks the transmission of infrared signals between the transmitter and receiver of, the upper IR unit 38b. When the milk level rises to the upper IR unit

38b, the motor 42 will stop, thus releasing the "vacuum" in the hood 12, in the manner discussed above. In addition, the needle valve 48 will be opened by the valve motor 46, whereby air will exit the bottle 18 via the nozzle 50, and subsequently out of the needle valve 48. The milk in the chamber 37 will thus fall, on its own weight, through the one-way valve 96 into the bottle 18, during the course of which the level of milk in the chamber 37 will fall. The transmission of IR signals between the transmitter and receiver of the upper IR unit 38b will thus resume, and then that between the transmitter and receiver of the lower IR unit 38a will resume.

[0021] As shown clearly in Figs. 4 and 14, above the upper IR unit 38b is a partition 98 which prevents milk from entering the interior of the head portion 22, e.g. when the breast pump 10 is accidentally knocked over. Milk entering the interior of the head portion 22 may damage the movement parts of the breast pump 10, thus shortening its useful life, or necessitating servicing.

[0022] Researches indicate that a baby's feeding is not a single continuous process, but rather a two-phased process in which the baby will initially suckle rapidly, called "stimulation". Once the breast has been sufficiently stimulated, milk begins flowing and the baby will settle into a slower, more relaxed sucking speed for the actual feeding phase, called "expression". The breast pump 10 can mimic the natural feeding pattern of a baby by first exhibiting rapid sucking/releasing actions to stimulate the milk ejection reflex (MER) or "let down". Once milk begins to flow, the breast pump 10 will then exhibit slower and longer sucking/releasing actions which help to maximize milk flow in less time.

[0023] The manner of operation of the breast pump 10 will be further discussed by reference to Fig. 15, which shows a flow chart of the steps of operation of the breast pump 10. Once the breast pump 10 is started (Step 100), the valve motor 46 will be triggered once to close the needle valve 48, which is called "retainer valve" in Fig. 15 (Step 102). A "let down" sequence will be operated in which sucking/releasing actions will be carried out at a speed of 90 cycles per minute at a pressure of 5-7 inch mercury (in Hg) for 30 seconds (Step 104). If no milk flows (Step 106), an "expression" mode will be operated in which sucking/releasing actions will be carried out at a speed of 45 cycles per minute at a pressure of 7-9 in Hg for 30 seconds (Step 108). If there is still no milk flow (Step 110), the microcontroller 40 of the breast pump 10 (hereinafter simply referred to as the "breast pump 10" for simplicity) will determine if this is the first time such occurs since the breast pump 10 is started (Step 112). If not, the breast pump 10 will repeat the above process (Step 114) by carrying out the "let down" sequence again (Step 104). If, however, such a situation has already occurred once in this operation, a sign or symbol alerting the user to seek medical assistance, e.g. to undergo certain milk flow stimulation operation, will be displayed on the LCD display 28 (Step 115), and the breast pump 10 will also cease operation immediately (Step 116). For

carrying out sucking/releasing actions at a frequency of 45 cycles per minute, the pump motor 42 may be activated for 0.8 second, then deactivated for 0.53 second, and then activated for 0.8 second, and so on.

[0024] If milk flows after the "let down" sequence (Step 104) or the "expression" sequence (Step 110), the breast pump 10 will then check whether transmission of IR signals in the lower IR unit 38a is interrupted (Step 118). If so, a timer in the microcontroller 40 will start timing (Step 120). The breast pump 10 will then check whether transmission of IR signals in the upper IR unit 38b is interrupted (Step 122). If so, the timer will stop (Step 124). Because the volume in the chamber 37 between the lower IR unit 38a and the upper IR unit 38b is known, it is possible to thus calculate the rate of flow of milk (in grams per second, g/s) and such is calculated. The valve motor 46 will be triggered once to open the needle valve 48, thus allowing milk in the chamber 37 to fall into the bottle 18. The breast pump 10 will also count the number of times of such triggers of the valve motor 46 as "X" (Step 126).

[0025] The breast pump 10 will then check whether transmission of IR signals in the lower IR unit 38a resumes ("released") within 2.5 seconds (Step 128). If so, the valve motor 46 will be triggered once to close the needle valve 48 (Step 130). If transmission of IR signals in the lower IR unit 38a does not resume ("released") within 2.5 seconds (Step 128), or after the closing of the needle valve 48 (Step 130), the breast pump 10 will then check if transmission of IR signals in the upper IR unit 38b is still blocked in 2.5 seconds (Step 132). If so, the pump motor 42 will stop operation, and the needle valve 48 will be opened once again (Step 134). If transmission of IR signals in the upper IR unit 38b is still blocked (Step 136), the pump motor 42 will stop operation again, and the needle valve 48 will be opened once again (Step 138). If transmission of IR signals in the upper IR unit 38b is still blocked (Step 140), the pump motor 42 will stop, a warning signal will be given on the LCD display 28, and the LCD display 28 will be turned off automatically in 5 minutes, (Step 142), and the operation of the breast pump 10 will also stop automatically (Step 116). Such will prevent the motor 42 from continuing operation when, e.g. the breast pump 10 accidentally topples over.

[0026] If transmission of IR signals in the upper IR unit 38b is not blocked after Step 132, Step 136 or Step 140, the breast pump 10 will operate according to the milk flow rate obtained in Step 126. If the flow rate is between 0.01 to 0.09 g/s (Step 144), the breast pump 10 will switch to "let down" sequence (Step 146) in which sucking/releasing action is carried out at a frequency of 90 cycles per minute at a pressure of 5-7 in Hg, and a sign or symbol indicating low flow rate will be displayed on the LCD display 28 (Step 148). If the flow rate is between 0.1 to 0.24 g/s (Step 150), the breast pump 10 will carry out sucking/releasing action at a frequency of 45 cycles per minute at a pressure of 7-9 in Hg (Step 152), and a sign or symbol indicating medium flow rate will be displayed on the LCD display 28 (Step 154). If the flow rate is 0.25 g/s or above

(Step 156), the breast pump 10 will carry out sucking/releasing action at a frequency of 38 cycles per minute at a pressure of 6-8 in Hg (Step 158), and a sign or symbol indicating high flow rate will be displayed on the LCD display 28 (Step 160).

[0027] According to the present example, the bottle 18 is designed to hold 151.51g of milk, and in each cycle, the milk that enters, and is thus collected by, the bottle 18 is 1.5g. Based on such information, and the frequency at which sucking/releasing action is carried out, the breast pump 10 is able to calculate and display the remaining time required to fill the bottle 18. In this example, it normally requires 101 triggers of the valve motor 46, "X", to fill the bottle 18. Depending on the number of times, "X", the valve motor 46 has already been triggered to open the needle valve 48, the breast pump 10 can calculate the remaining time required for filling up the bottle 18 (Step 162). The remaining time required will be displayed on the LCD display 28 (Step 164).

[0028] If $1.5X > 151.51$ (Step 166), it means that the bottle 18 is filled up, the breast pump 10 will stop (Step 116). If not, the breast pump 10 will check again if transmission of IR signals in the lower IR unit 38a is interrupted (Step 118), and the pumping action will go on again.

[0029] It should be understood that the above only illustrates an example whereby the present invention may be carried out. For example, although the present invention is here described in the context of a "one-pump" model, it is equally applicable to a "two-pump" model, in which a second breast pump is pneumatically connected with the first pump to share in the suction vacuum generated by the pump motor.

[0030] It should also be understood that certain features of the invention, which are, for clarity, described in the context of separate embodiments, may be provided in combination in a single embodiment.

Claims

1. An electric breast pump comprising at least one hood member (12) adapted to be fitted over a breast of a user and a chamber (71) adapted to be in fluid communication with said hood member (12) via a first valve (70); wherein a first motor (42) is operatively associated with a pumping member (44) which is movable to draw air from said hood member (12) into said chamber (37) via said first valve (70); **characterized in that** said chamber (71) has at least a first opening (68) and a closure member (66) operatively associated with said first motor (42); **in that** said closure member (66) is movable between a first position to close said first opening (68) and a second position in which said first opening (68) is open; and **in that** said closure member (66) is at said first position when said first motor (42) is in operation and is at said second position when said first motor (42) is not in operation.

2. A breast pump according to claim 1, **characterized in that** said closure member (66) is biased towards said second position.
3. A breast pump according to claim 2, **characterized in that** said closure member (66) is biased towards said second position by a spring member (62).
4. A breast pump according to any preceding claim, **characterized in that** said first valve is a one-way valve (70).
5. A breast pump according to any preceding claim, **characterized in that** said first motor (46) is engaged with said closure member (66) via at least one ring-shaped structure (60).
6. A breast pump according to claim 5, **characterized in that** said ring-shaped structure (60) is movable between a stable first configuration to which said ring-shaped structure is biased and a second configuration in which said closure member (66) is allowed to occupy said first position
7. A breast pump according to claim 6, **characterized in that** said ring-shaped structure (60) is at said stable first configuration when said first motor (42) is not in operation and at said second configuration when said first motor (42) is in operation.
8. A breast pump according to claim 7, **characterized in that** said ring-shaped structure (60) rotates when said first motor (42) is in operation.
9. A breast pump according to claim 8, **characterized in that** said ring-shaped structure (60) moves from said first configuration to said second configuration by centrifugal force when said ring-shaped structure rotates.
10. A breast pump according to any preceding claim, **characterized in that** said chamber (71) includes at least a second opening closable by a second valve (74).
11. A breast pump according to claim 10, **characterized in that** said second valve (74) is a one-way valve.
12. A breast pump according to claim 10 or claim 11, **characterized in that** said second valve (74) only allows air to exit said chamber.
13. A breast pump according to any preceding claim, **characterized in that** it further includes an adjustment member manually operable to adjust the air pressure in said hood member (12).
14. A breast pump according to claim 13, **characterized in that** said adjustment member includes a third valve member (86) in fluid communication with said hood member (12).
15. A breast pump according to claim 14, **characterized in that** said adjustment member further includes a wheel member (80) manually operable to adjust the amount of air allowed to enter the third valve.
16. A breast pump according to any preceding claim, **characterized in that** it further includes a fourth valve (96) in fluid communication with the hood member (12).
17. A breast pump according to claim 16, **characterized in that** it further includes a second motor (46) for selectively opening or closing said fourth valve (96).
18. A breast pump according to claim 16 or claim 17, **characterized in that**, during operation of said breast pump, said fourth valve (96) is openable to release the vacuum in said hood member (12).
19. A breast pump according to any preceding claim, **characterized in that** it further includes at least one sensing unit (38b) adapted to detect the passing of milk.
20. A breast pump according to claim 19, **characterized in that** it further includes a data processing unit (40) adapted to calculate the rate of flow of milk on the basis of data received from said sensing unit (38b).
21. A breast pump according to claim 19 or claim 20, **characterized in that** said sensing unit (38b) includes at least one infrared (IR) transmitter and an IR receiver adapted to receive IR signals from said IR transmitter.
22. A breast pump according to any one of claims 19 to 21, **characterized in that** it further includes at least a second sensing unit (38a).
23. A breast pump according to claim 22, **characterized in that** said first and second sensing units (38b, 38a) are arranged in series in the path of flow of milk in said breast pump.
24. A breast pump according to claim 23, **characterized in that** a timer is provided for determining the time duration between when passing of milk is detected by said first sensing unit (38b) and when passing of milk is detected by said second sensing unit (38a).
25. A breast pump according to any one of claims 22 to 24, **characterized in that** IR signals transmitted by said IR transmitter are prevented from being received by said IR receiver upon passing of milk ther-

ebetween.

26. A breast pump according to any one of claims 19 to 25, **characterized in that** it further includes a display (28) for visually indicating the general rate of flow of milk into said breast pump.
27. A breast pump according to claim 21, **characterized in that** said data processing unit (40) is adapted to calculate the remaining time required for filling a receptacle of milk associated with said breast pump.
28. A breast pump according to claim 27, **characterized in that** it includes a motor operatively associated with a pumping member, wherein the frequency of movement of said pumping member is adapted to be varied on the basis of the rate of flow of milk calculated by said data processing unit.
29. A breast pump according to claim 28, **characterized in that** the motor is adapted to stop operation when IR signals transmitted by said IR transmitter are prevented from being received by said IR receiver for a predetermined period of time.

Patentansprüche

1. Elektrische Brustpumpe mit wenigstens einem Haubenelement (12), das so ausgebildet ist, dass dieses über eine Brust einer Benutzerin gesetzt werden kann, und einer Kammer (71), die so ausgebildet ist, dass diese über ein erstes Ventil (70) in Fluidkommunikation mit dem Haubenelement (12) steht; wobei ein erster Motor (42) mit einem Pumpelement (44) operativ verbunden ist, welches beweglich ist, um über das erste Ventil (70) Luft aus dem Haubenelement (12) in die Kammer (37) zu ziehen; **dadurch gekennzeichnet, dass** die Kammer (71) wenigstens eine erste Öffnung (68) und ein Verschlusselement (66) hat, das operativ mit dem ersten Motor (42) verbunden ist; dass das Verschlusselement (66) zwischen einer ersten Position zum Schließen der ersten Öffnung (68) und einer zweiten Position, in welcher die erste Öffnung (68) offen ist, bewegbar ist; und dass das Verschlusselement (66) sich in der ersten Position befindet, wenn der erste Motor (42) in Betrieb ist, und sich an der zweiten Position befindet, wenn der erste Motor (42) nicht in Betrieb ist.
2. Brustpumpe nach Anspruch 1, **dadurch gekennzeichnet, dass** das Verschlusselement (66) in Richtung der zweiten Position vorgespannt ist.
3. Brustpumpe nach Anspruch 2, **dadurch gekennzeichnet, dass** das Verschlusselement (66) in Richtung der zweiten Position durch ein Federelement (62) vorgespannt ist.

4. Brustpumpe nach einem der vorhergehenden Ansprüche, **dadurch gekennzeichnet, dass** das erste Ventil ein Einwegventil (70) ist.
5. Brustpumpe nach einem der vorhergehenden Ansprüche, **dadurch gekennzeichnet, dass** der erste Motor (46) mit dem Verschlusselement (66) über wenigstens eine ringförmige Struktur (60) in Eingriff steht.
6. Brustpumpe nach Anspruch 5, **dadurch gekennzeichnet, dass** die ringförmige Struktur (60) zwischen einer stabilen ersten Konfiguration, in welcher die ringförmige Struktur vorgespannt ist, und einer zweiten Konfiguration, in welcher das Verschlusselement (66) die erste Position einnehmen kann, bewegbar ist.
7. Brustpumpe nach Anspruch 6, **dadurch gekennzeichnet, dass** sich die ringförmige Struktur (60) in der stabilen ersten Konfiguration befindet, wenn der erste Motor (42) nicht in Betrieb ist, und sich in der zweiten Konfiguration befindet, wenn der erste Motor (42) in Betrieb ist.
8. Brustpumpe nach Anspruch 7, **dadurch gekennzeichnet, dass** die ringförmige Struktur (60) rotiert, wenn der erste Motor (42) in Betrieb ist.
9. Brustpumpe nach Anspruch 8, **dadurch gekennzeichnet, dass** sich die ringförmige Struktur (60) von der ersten Konfiguration in die zweite Konfiguration durch die Zentrifugalkraft bewegt, wenn die ringförmige Struktur rotiert.
10. Brustpumpe nach einem der der vorhergehenden Ansprüche, **dadurch gekennzeichnet, dass** die Kammer (71) wenigstens eine zweite Öffnung enthält, die durch ein zweites Ventil (74) schließbar ist.
11. Brustpumpe nach Anspruch 10, **dadurch gekennzeichnet, dass** das zweite Ventil (74) ein Einwegventil ist.
12. Brustpumpe nach Anspruch 10 oder Anspruch 11, **dadurch gekennzeichnet, dass** das zweite Ventil (74) durch den Austritt von Luft aus der Kammer erlaubt.
13. Brustpumpe nach einem der vorhergehenden Ansprüche, **dadurch gekennzeichnet, dass** diese ferner ein Einstellelement enthält, das manuell betätigbar ist, um den Luftdruck in dem Haubenelement (12) einzustellen.
14. Brustpumpe nach Anspruch 13, **dadurch gekennzeichnet, dass** das Einstellelement ein drittes Ventilelement (86) in Fluidkommunikation mit dem Hau-

benelement (12) enthält.

15. Brustpumpe nach Anspruch 14, **dadurch gekennzeichnet, dass** das Einstellelement ferner ein Rad-
element (80) enthält, das manuell betätigbar ist, um
den Betrag der Luft einzustellen, die in das dritte
Ventil eintreten darf.
16. Brustpumpe nach einem der vorhergehenden An-
sprüche, **dadurch gekennzeichnet, dass** diese
ferner ein viertes Ventil (96) in Fluidkommunikation
mit dem Haubenelement (12) enthält.
17. Brustpumpe nach Anspruch 16, **dadurch gekenn-
zeichnet, dass** diese ferner einen zweiten Motor
(46) zum selektiven Öffnen oder Schließen des vier-
ten Ventils (96) enthält.
18. Brustpumpe nach Anspruch 16 oder Anspruch 17,
dadurch gekennzeichnet, dass während des Be-
triebs der Brustpumpe das vierte Ventil (96) geöffnet
werden kann, um das Vakuum in dem Haubenele-
ment (12) zu beseitigen.
19. Brustpumpe nach einem der vorhergehenden An-
sprüche, **dadurch gekennzeichnet, dass** diese
ferner wenigstens eine Erfassungseinheit (38b) ent-
hält, die so ausgebildet ist, dass diese den Durch-
gang von Milch detektiert.
20. Brustpumpe nach Anspruch 19, **dadurch gekenn-
zeichnet, dass** diese ferner eine Datenverarbei-
tungseinheit (40) enthält, die so ausgelegt ist, dass
diese die Durchflussmenge von Milch auf Basis der
von der Erfassungseinheit (38b) erhaltenen Daten
berechnen kann.
21. Brustpumpe nach Anspruch 19 oder Anspruch 20,
dadurch gekennzeichnet, dass die Erfassungs-
einheit (38b) wenigstens einen Infrarot (IR)-Trans-
mitter und einen IR-Empfänger enthält, der so aus-
gebildet ist, dass dieser IR-Signale von dem IR-
Transmitter erhält.
22. Brustpumpe nach einem der Ansprüche 19 bis 21,
dadurch gekennzeichnet, dass diese ferner we-
nigstens eine zweite Erfassungseinheit (38a) ent-
hält.
23. Brustpumpe nach Anspruch 22, **dadurch gekenn-
zeichnet, dass** die erste und zweite Erfassungsein-
heit (38b, 38a) in Reihe im Fließweg der Milch in der
Brustpumpe angeordnet sind.
24. Brustpumpe nach Anspruch 23, **dadurch gekenn-
zeichnet, dass** ein Zeitnehmer vorgesehen ist, zum
Bestimmen der Zeitdauer zwischen der Erfassung
des Durchgangs von Milch mittels der ersten Erfas-

sungseinheit (38b) und der Erfassung des Durch-
gangs von Milch mittels der zweiten Erfassungsein-
heit (38a).

25. Brustpumpe nach einem der Ansprüche 22 bis 24,
dadurch gekennzeichnet, dass IR-Signale, die
von dem IR-Transmitter übertragen werden, daran
gehindert werden, beim Durchgang von Milch zwis-
chen beiden, durch den IR-Receiver empfangen zu
werden.
26. Brustpumpe nach einem der Ansprüche 19 bis 25,
dadurch gekennzeichnet, dass diese ferner eine
Anzeige (28) zum visuellen Anzeigen der allgemei-
nen Durchflussmenge von Milch in der Brustpumpe
enthält.
27. Brustpumpe nach Anspruch 21, **dadurch gekenn-
zeichnet, dass** die Datenverarbeitungseinheit (40)
so ausgelegt ist, dass diese die verbleibende Zeit
berechnet, die zum Füllen eines mit der Brustpumpe
verbundenen Milchgefäß benötigt wird.
28. Brustpumpe nach Anspruch 17, **dadurch gekenn-
zeichnet, dass** diese einen Motor enthält, der mit
einem Pumpelement operativ verbunden ist, wobei
die Bewegungsfrequenz des Pumpelements so aus-
gelegt ist, dass diese auf der Basis der durch die
Datenverarbeitungseinheit berechneten Durch-
flussmenge von Milch variiert werden kann.
29. Brustpumpe nach Anspruch 28, **dadurch gekenn-
zeichnet, dass** der Motor so ausgelegt ist, dass die-
ser den Betrieb stoppt, wenn IR-Signale, die von
dem IR-Transmitter übertragen werden, für eine vor-
bestimmte Zeitspanne daran gehindert werden, von
dem IR-Receiver empfangen zu werden.

Revendications

1. Tire-lait électrique comprenant au moins un élément
de capuchon (12) conçu pour être adapté sur un sein
d'une utilisatrice et une chambre (71) conçue pour
être en communication fluïdique avec ledit élément
de capuchon (12) par l'intermédiaire d'une première
vanne (70), dans lequel un premier moteur électrique
(42) est associé fonctionnellement à un élément de
pompage (44) qui peut être déplacé pour aspirer de
l'air à partir dudit élément de capuchon (12) à l'inté-
rieur de ladite chambre (37) par l'intermédiaire de
ladite première vanne (70), **caractérisé en ce que**
ladite chambre (71) comporte au moins une premiè-
re ouverture (68) et un élément de fermeture (66)
associé fonctionnellement audit premier moteur
électrique (42), **en ce que** ledit élément de fermeture
(66) peut être déplacé entre une première position
pour fermer ladite première ouverture (68) et une

- deuxième position dans laquelle ladite première ouverture (68) est ouverte; et **en ce que** ledit élément de fermeture (66) se trouve à ladite première position lorsque ledit premier moteur électrique (42) fonctionne et se trouve à ladite deuxième position lorsque ledit premier moteur électrique (42) ne fonctionne pas.
2. Tire-lait selon la revendication 1, **caractérisé en ce que** ledit élément de fermeture (66) est sollicité vers ladite deuxième position.
 3. Tire-lait selon la revendication 2, **caractérisé en ce que** ledit élément de fermeture (66) est sollicité vers ladite deuxième position par un élément de ressort (62).
 4. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce que** ladite première vanne est une vanne unidirectionnelle (70).
 5. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce que** ledit premier moteur électrique (46) est engagé avec ledit élément de fermeture (66) par l'intermédiaire d'au moins une structure de forme annulaire (60).
 6. Tire-lait selon la revendication 5, **caractérisé en ce que** ladite structure de forme annulaire (60) peut être déplacée entre une première configuration stable vers laquelle ladite structure de forme annulaire est sollicitée et une deuxième configuration dans laquelle ledit élément de fermeture (66) est amené à occuper ladite première position.
 7. Tire-lait selon la revendication 6, **caractérisé en ce que** ladite structure de forme annulaire (60) se trouve à ladite première configuration stable lorsque ledit premier moteur électrique (42) ne fonctionne pas et à ladite deuxième configuration lorsque ledit premier moteur électrique (42) fonctionne.
 8. Tire-lait selon la revendication 7, **caractérisé en ce que** ladite structure de forme annulaire (60) tourne lorsque ledit premier moteur électrique (42) fonctionne.
 9. Tire-lait selon la revendication 8, **caractérisé en ce que** ladite structure de forme annulaire (60) se déplace depuis ladite première configuration vers ladite deuxième configuration par une force centrifuge lorsque ladite structure de forme annulaire tourne.
 10. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce que** ladite chambre (71) comprend au moins une deuxième ouverture pouvant être fermée par une deuxième vanne (74).
 11. Tire-lait selon la revendication 10, **caractérisé en ce que** ladite deuxième vanne (74) est une vanne unidirectionnelle.
 12. Tire-lait selon la revendication 10 ou la revendication 11, **caractérisé en ce que** ladite deuxième vanne (74) permet uniquement à l'air de sortir de ladite chambre.
 13. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce qu'il** comprend en outre un élément de réglage pouvant être actionné manuellement pour régler la pression de l'air dans ledit élément de capuchon (12).
 14. Tire-lait selon la revendication 13, **caractérisé en ce que** ledit élément de réglage comprend un troisième élément de vanne (86) en communication fluide avec ledit élément de capuchon (12).
 15. Tire-lait selon la revendication 14, **caractérisé en ce que** ledit élément de réglage comprend en outre un élément de roue (80) pouvant être actionné manuellement pour régler la quantité d'air admise pour entrer par la troisième vanne.
 16. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce qu'il** comprend en outre une quatrième vanne (96) en communication fluide avec l'élément de capuchon (12).
 17. Tire-lait selon la revendication 16, **caractérisé en ce qu'il** comprend en outre un deuxième moteur électrique (46) destiné à ouvrir ou fermer sélectivement ladite quatrième vanne (96).
 18. Tire-lait selon la revendication 16 ou la revendication 17, **caractérisé en ce que**, au cours du fonctionnement dudit tire-lait, ladite quatrième vanne (96) peut être ouverte pour libérer le vide dans ledit élément de capuchon (12).
 19. Tire-lait selon l'une quelconque des revendications précédentes, **caractérisé en ce qu'il** comprend en outre au moins une unité de détection (38b) conçue pour détecter le passage du lait.
 20. Tire-lait selon la revendication 19, **caractérisé en ce qu'il** comprend en outre une unité de traitement de données (40) conçue pour calculer le débit du lait sur la base des données reçues depuis ladite unité de détection (38b).
 21. Tire-lait selon la revendication 19 ou la revendication 20, **caractérisé en ce que** ladite unité de détection (38b) comprend au moins un émetteur à infrarouge (IR) et un récepteur à infrarouge conçu pour recevoir des signaux infrarouges dudit émetteur à infrarouge.

22. Tire-lait selon l'une quelconque des revendications 19 à 21, **caractérisé en ce qu'il** comprend en outre au moins une deuxième unité de détection (38a).
23. Tire-lait selon la revendication 22, **caractérisé en ce que** lesdites première et deuxième unités de détection (38b, 38a) sont agencées en série sur le trajet de circulation de lait dans ledit tire-lait. 5
24. Tire-lait selon la revendication 23, **caractérisé en ce qu'un** chronomètre est prévu pour déterminer la durée entre le moment où le passage du lait est détecté par ladite première unité de détection (38b) et le moment où le passage du lait est détecté par la deuxième unité de détection (38a). 10 15
25. Tire-lait selon l'une quelconque des revendications 22 à 24, **caractérisé en ce que** les signaux infrarouges transmis par ledit émetteur à infrarouge sont empêchés d'être reçus par ledit récepteur à infrarouge lors du passage du lait entre ceux-ci. 20
26. Tire-lait selon l'une quelconque des revendications 19 à 25, **caractérisé en ce qu'il** comprend en outre un dispositif d'affichage (28) destiné à indiquer visuellement le débit général du lait dans ledit tire-lait. 25
27. Tire-lait selon la revendication 21, **caractérisé en ce que** ladite unité de traitement de données (40) est conçue pour calculer le temps restant qui est requis pour remplir un réceptacle de lait associé audit tire-lait. 30
28. Tire-lait selon la revendication 27, **caractérisé en ce qu'il** comprend un moteur électrique associé fonctionnellement à un élément de pompage, dans lequel la fréquence de mouvement dudit élément de pompage est conçue pour être amenée à varier sur la base du débit du lait calculé par ladite unité de traitement de données. 35 40
29. Tire-lait selon la revendication 28, **caractérisé en ce que** le moteur électrique est conçu pour s'arrêter de fonctionner lorsque les signaux infrarouges émis par ledit émetteur à infrarouge sont empêchés d'être reçus par ledit récepteur à infrarouge pendant une durée prédéterminée. 45

50

55

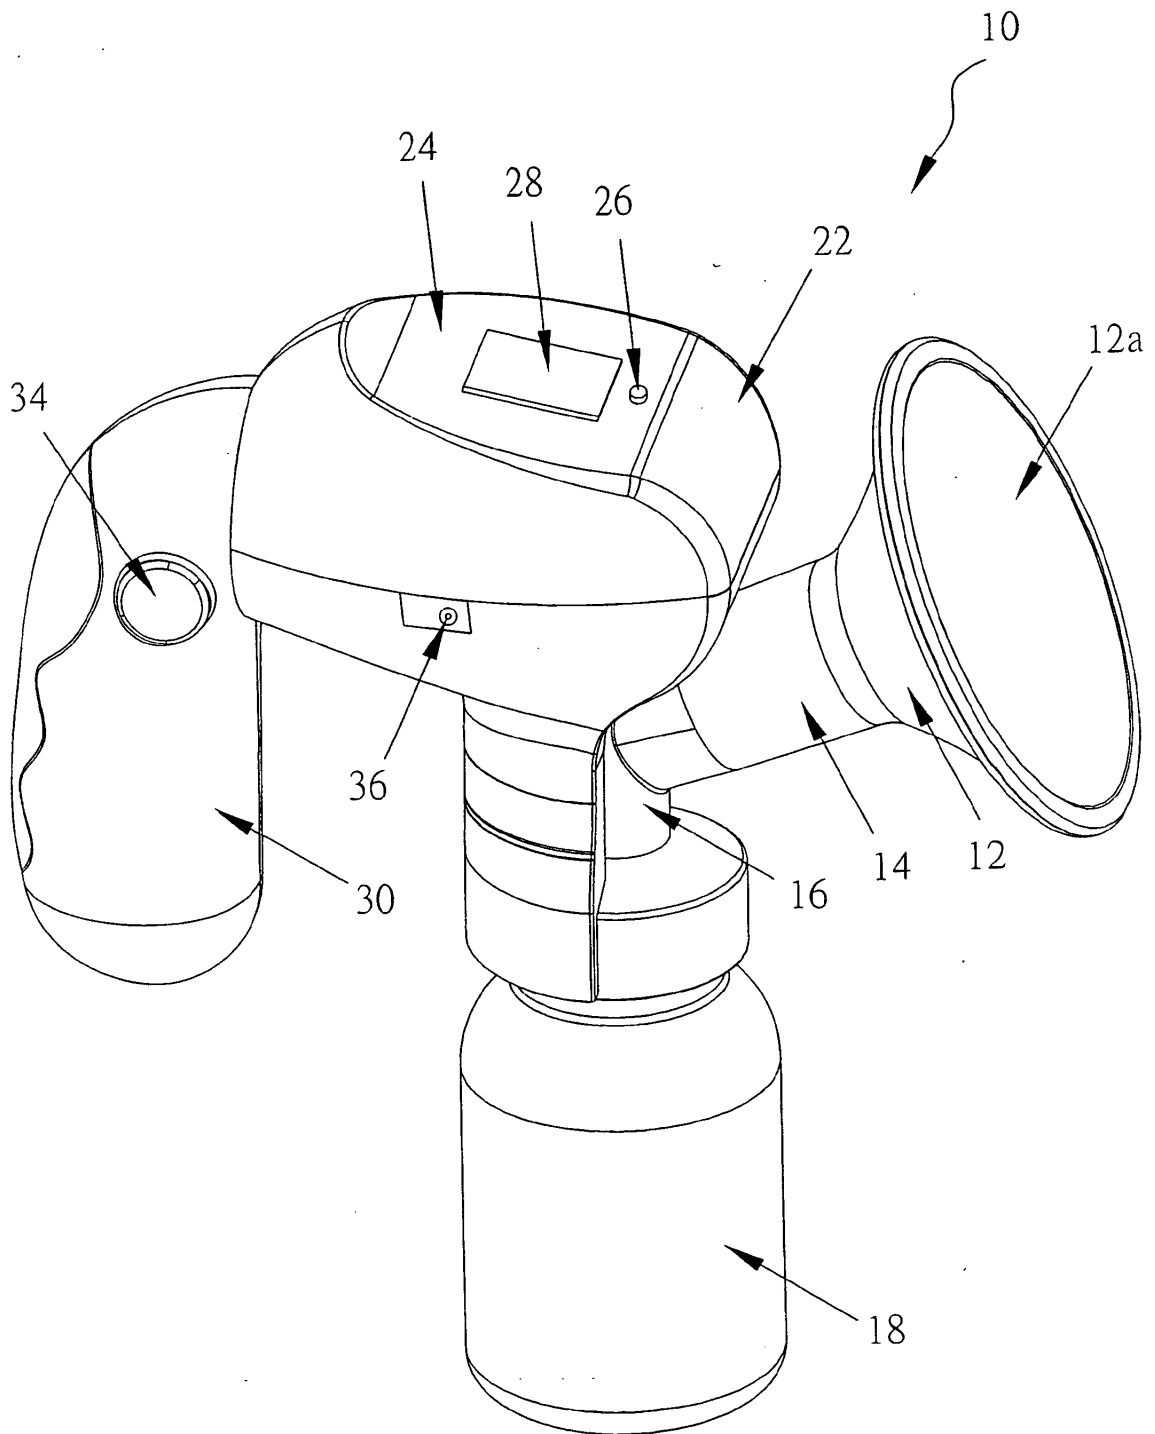
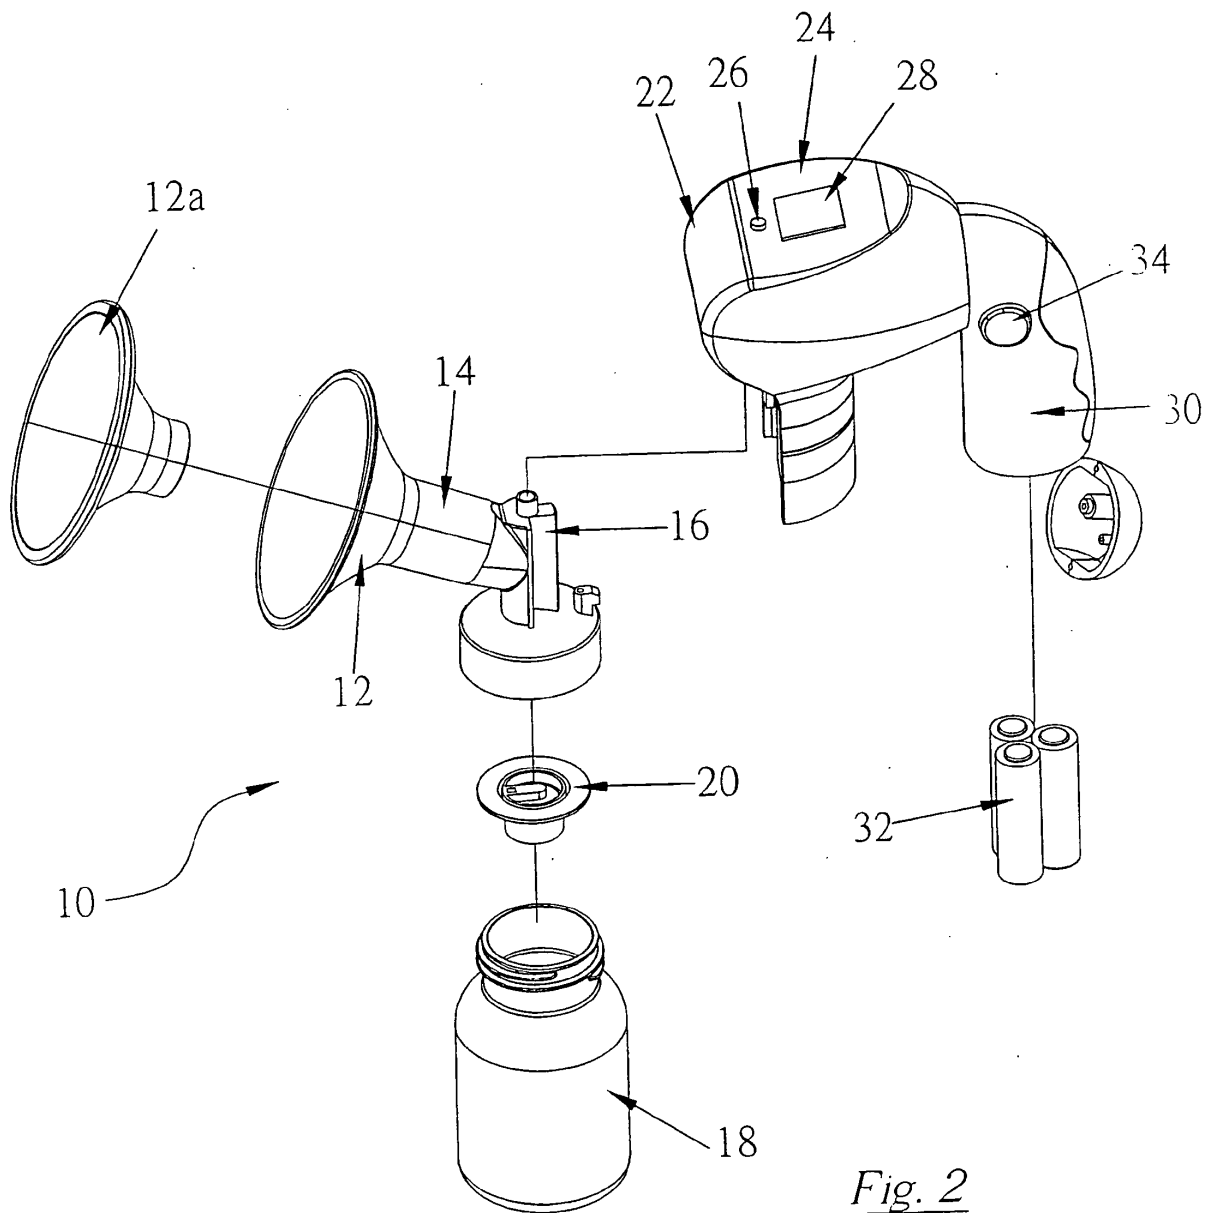


Fig. 1



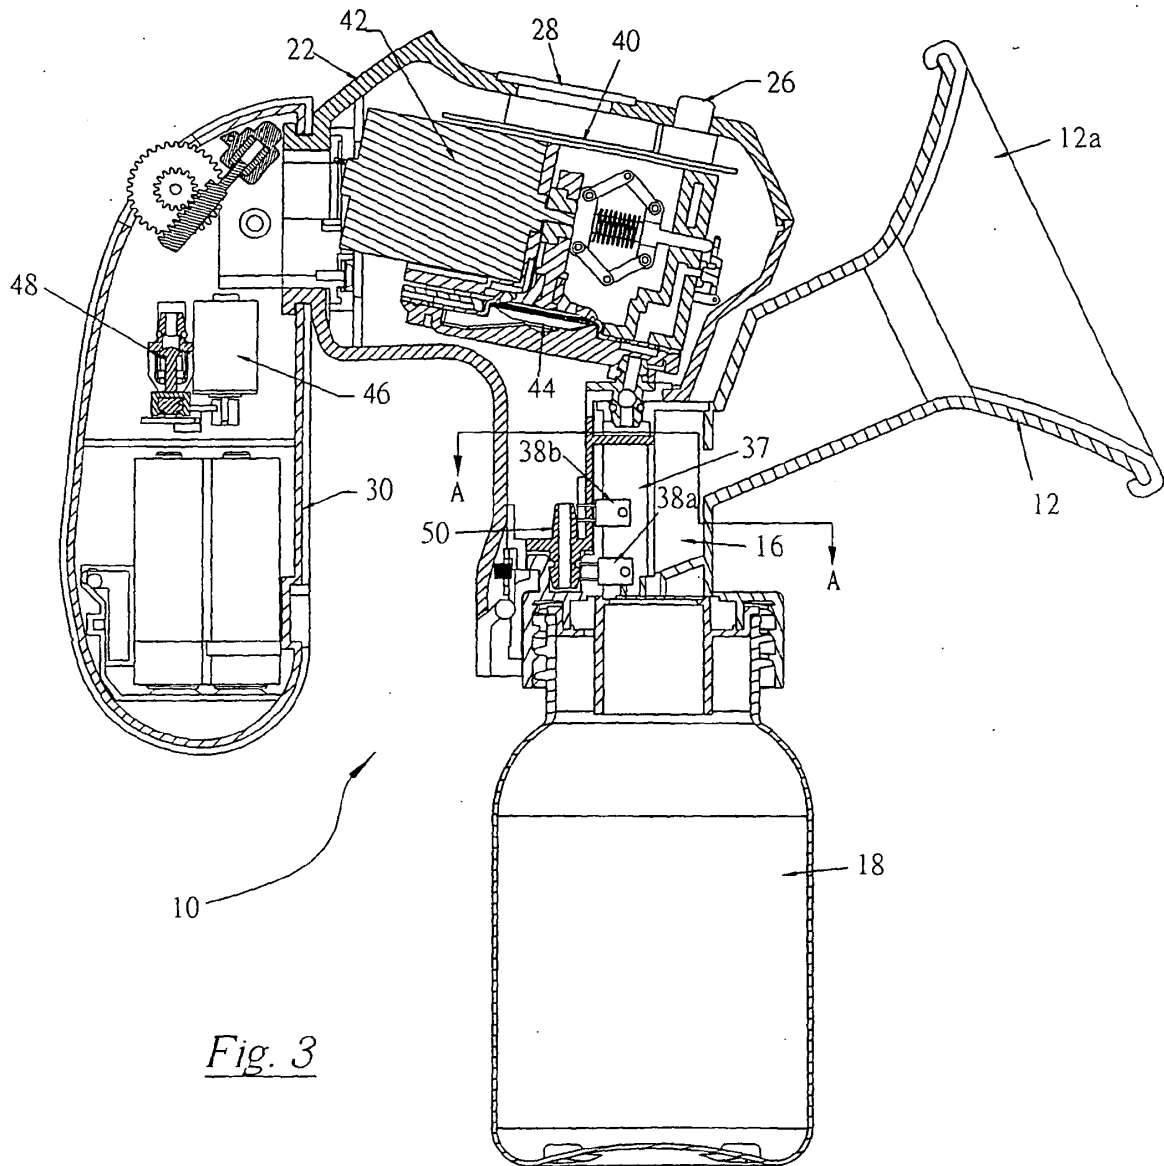
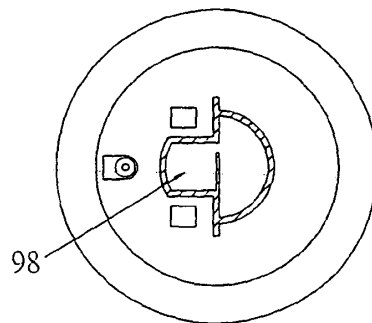


Fig. 3

Fig. 4



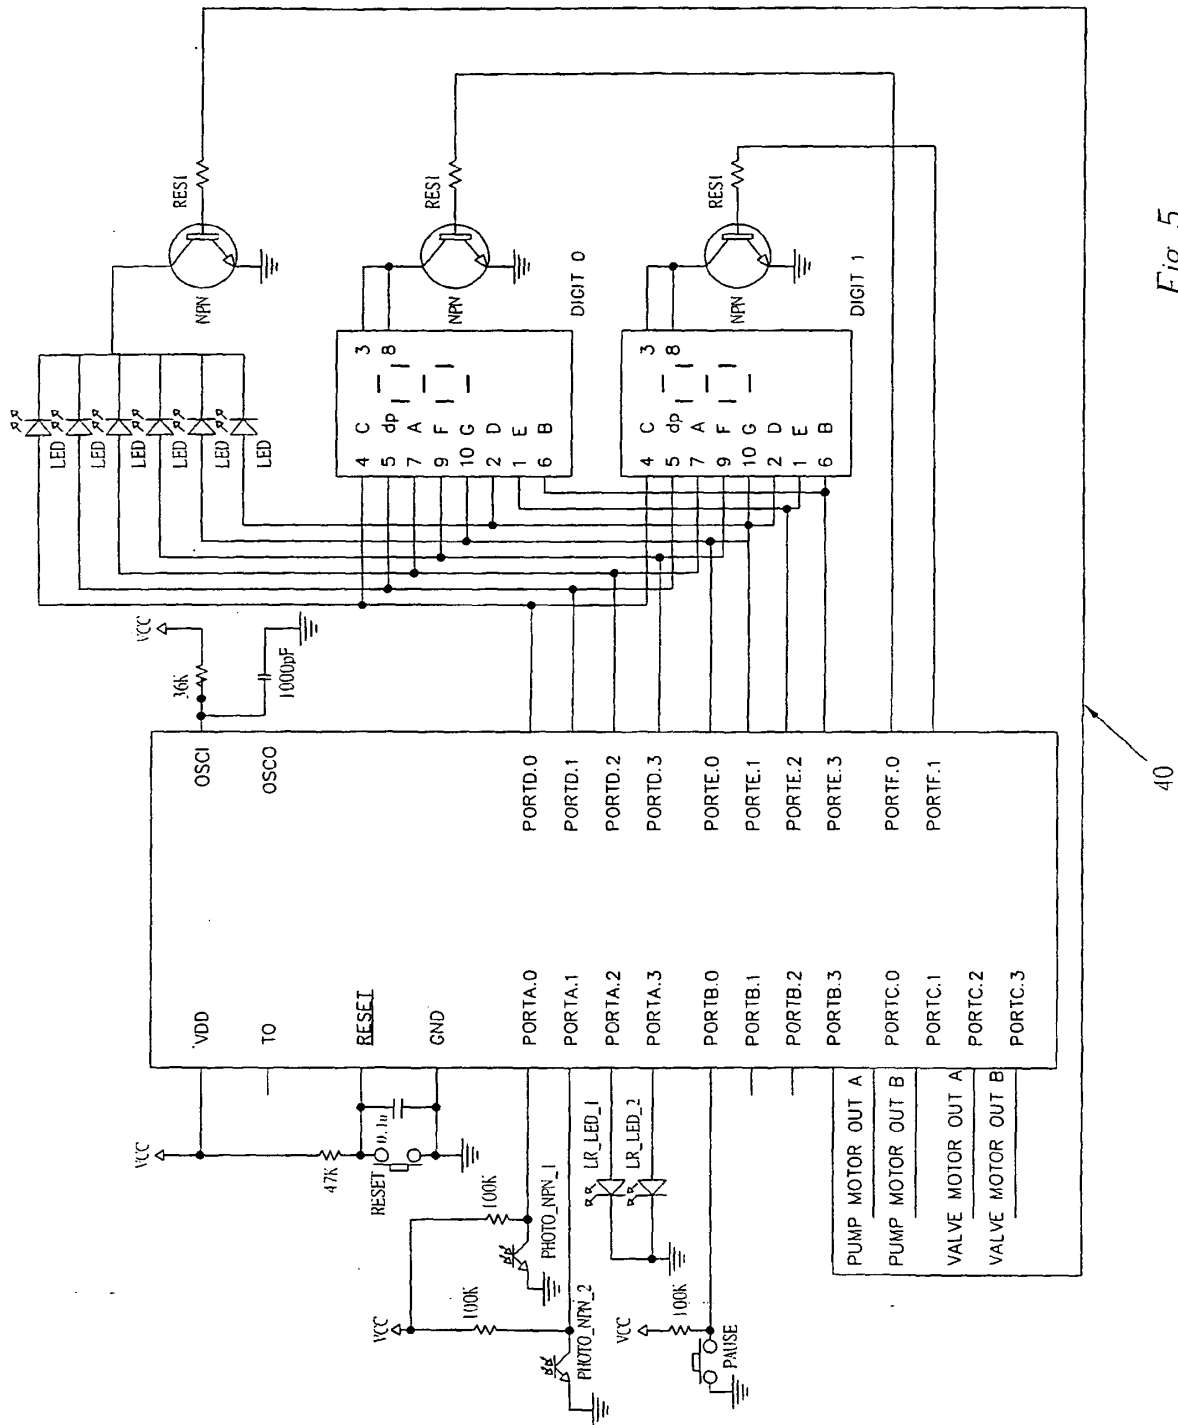


Fig. 5

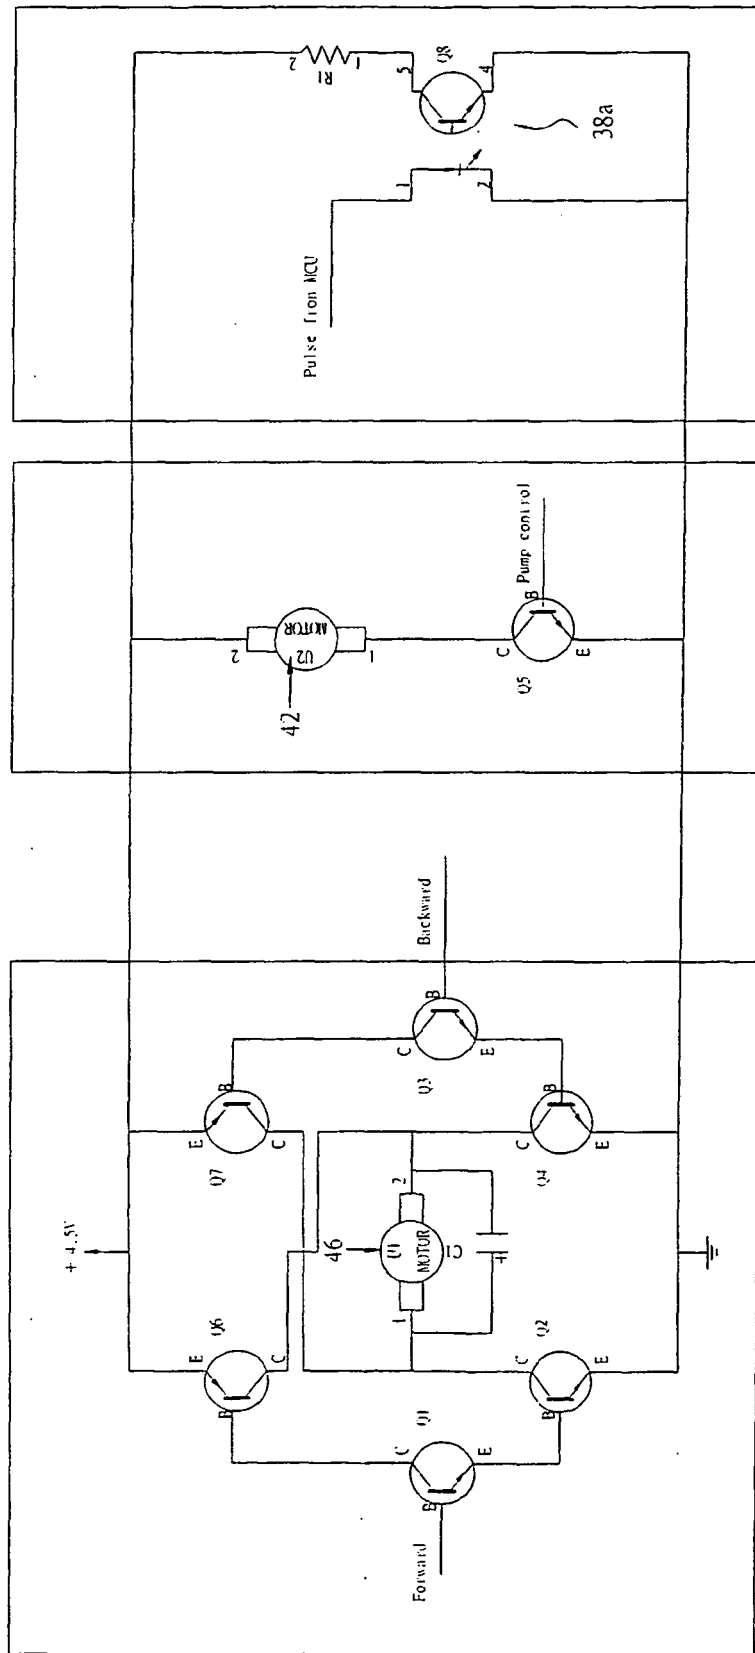


Fig. 6

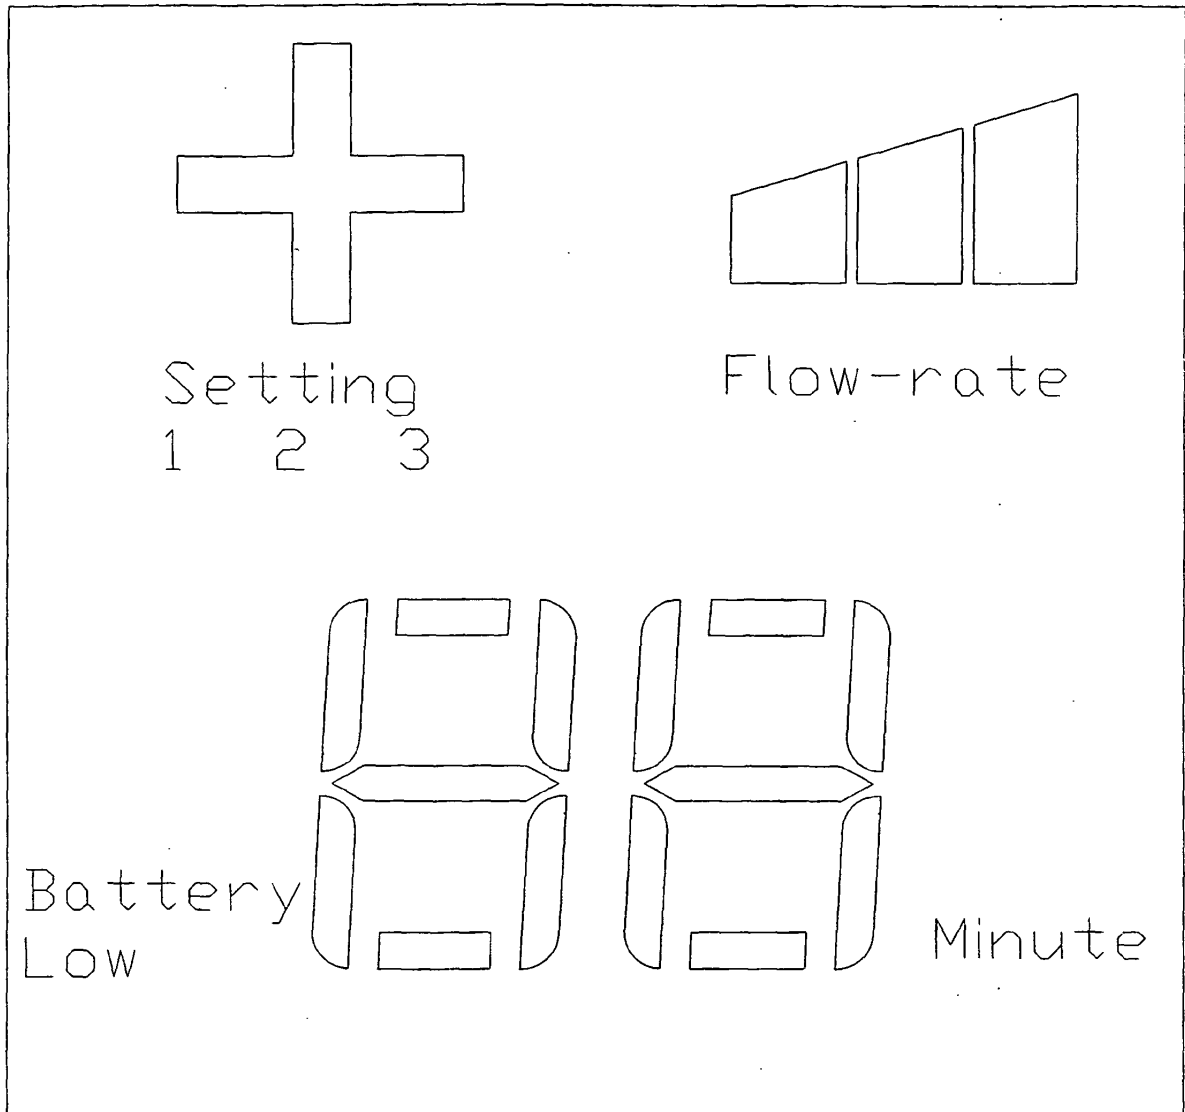


Fig. 7

28

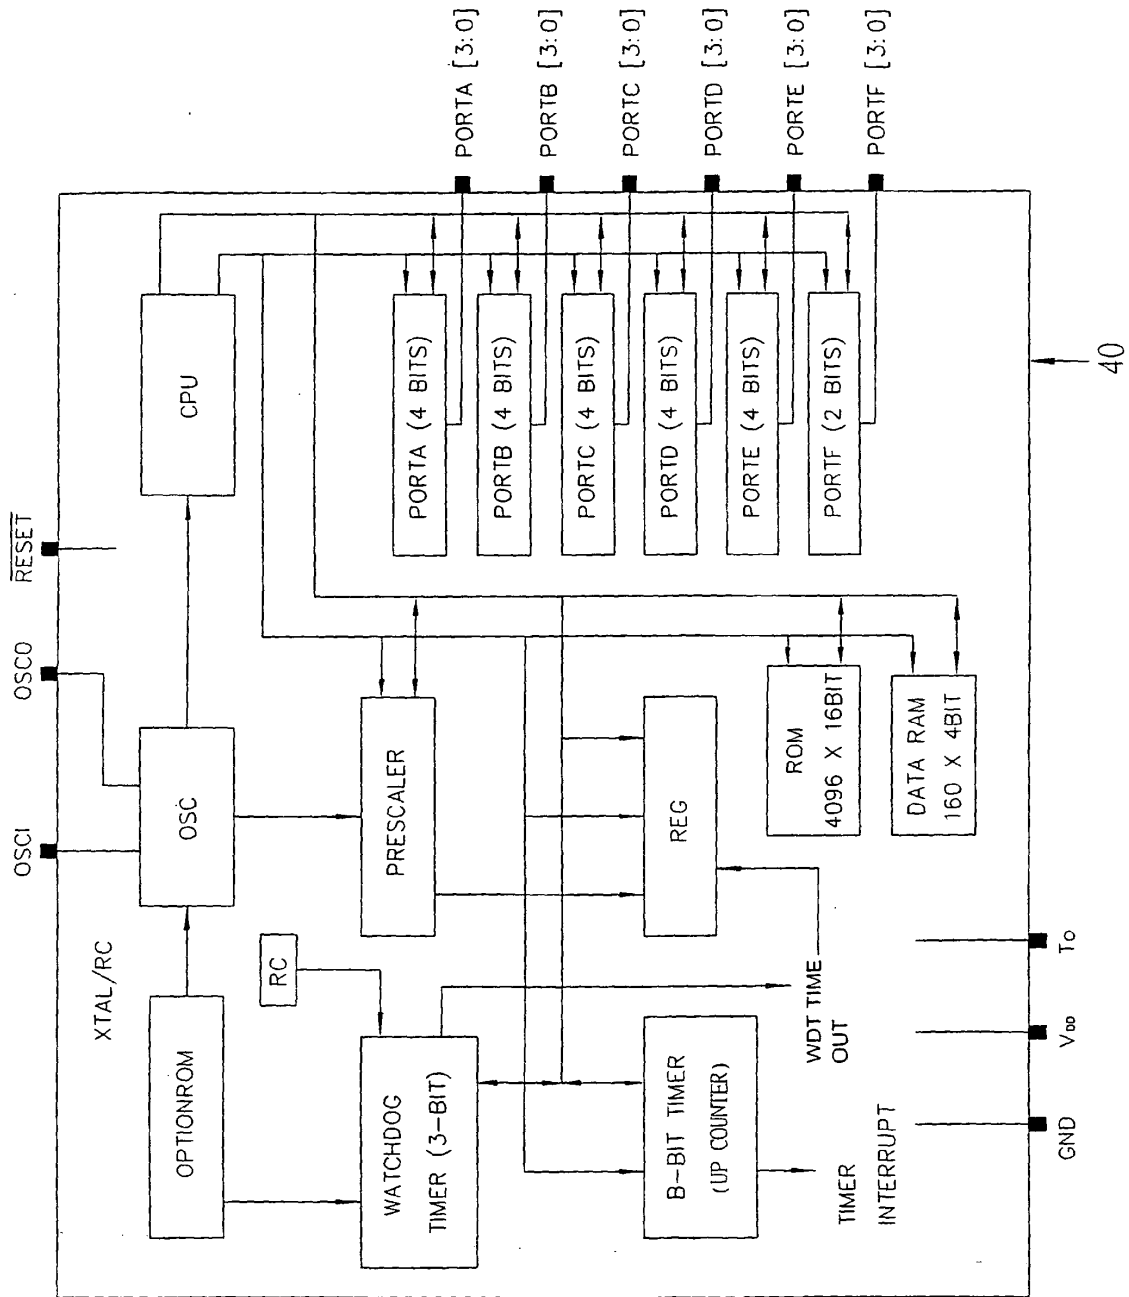


Fig. 8

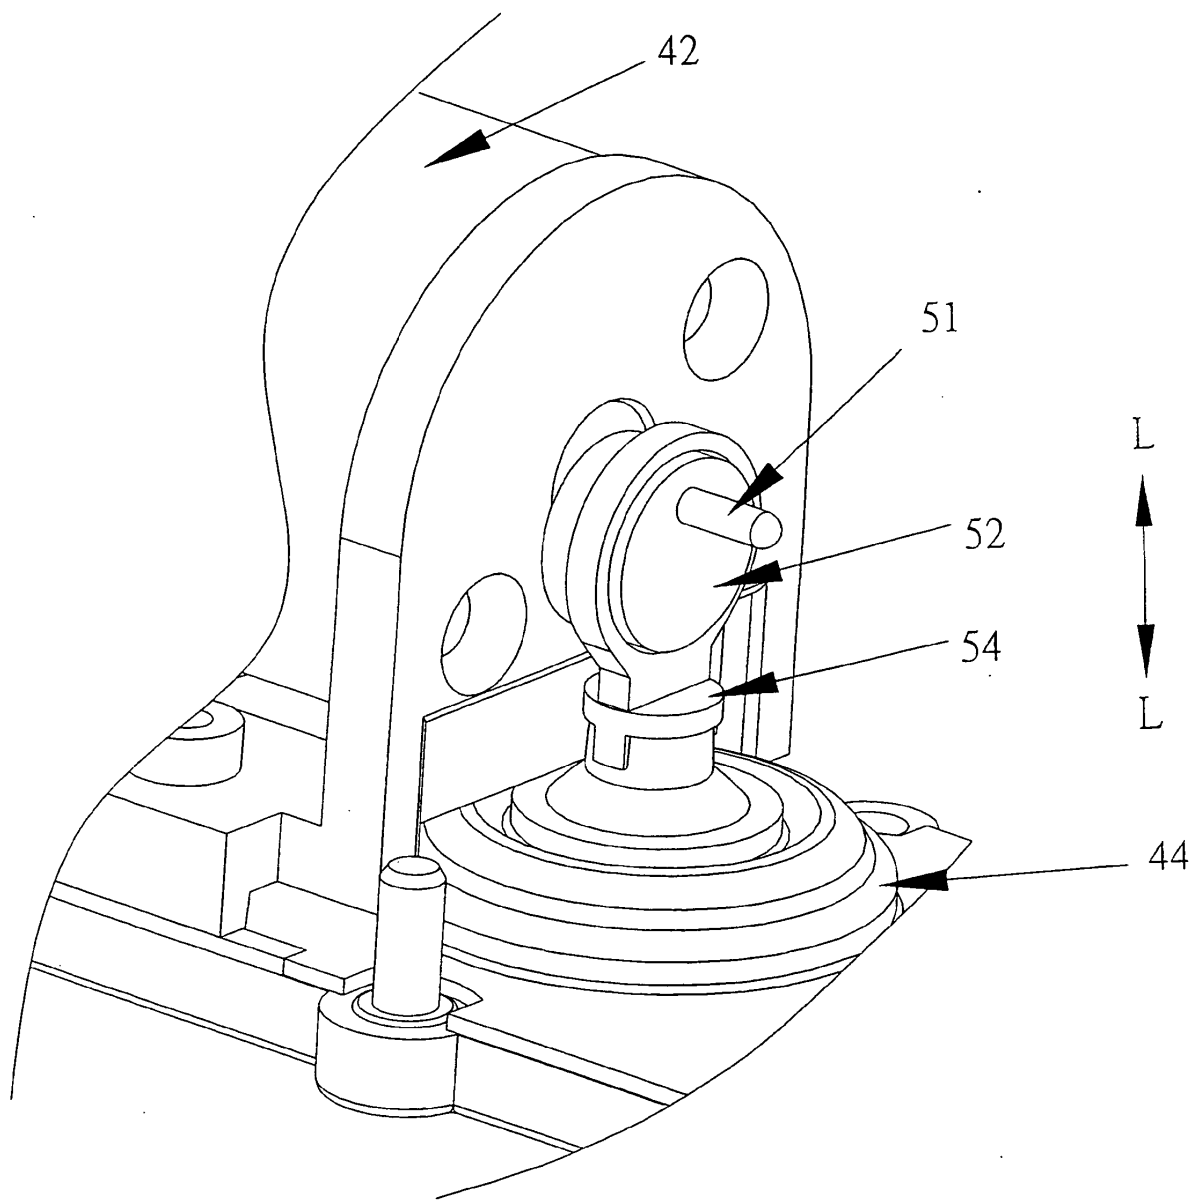


Fig. 9

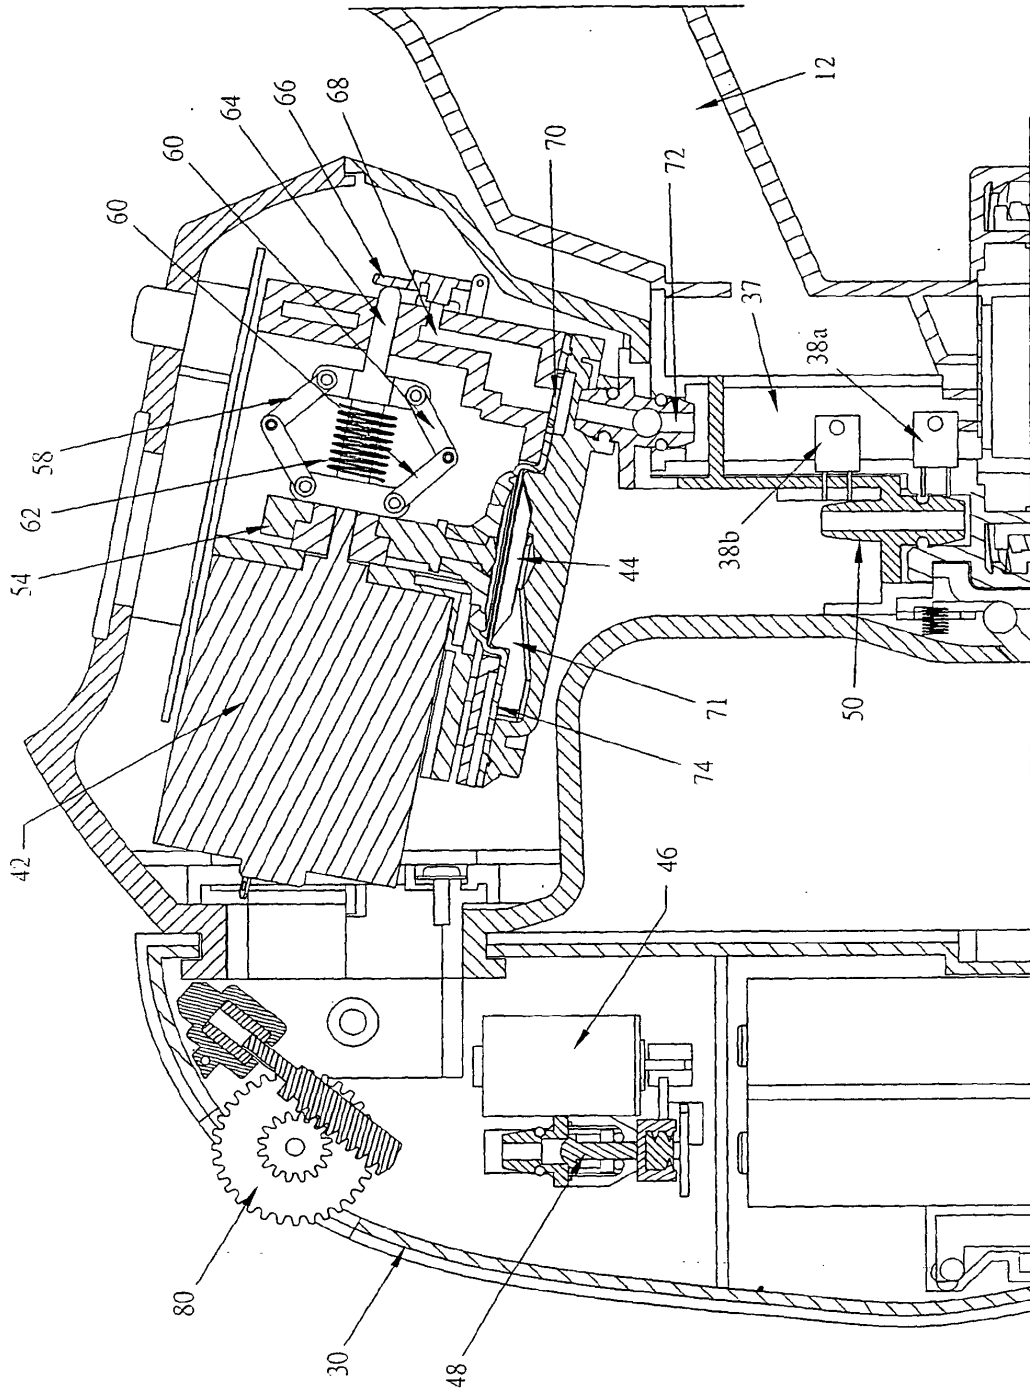


Fig. 10

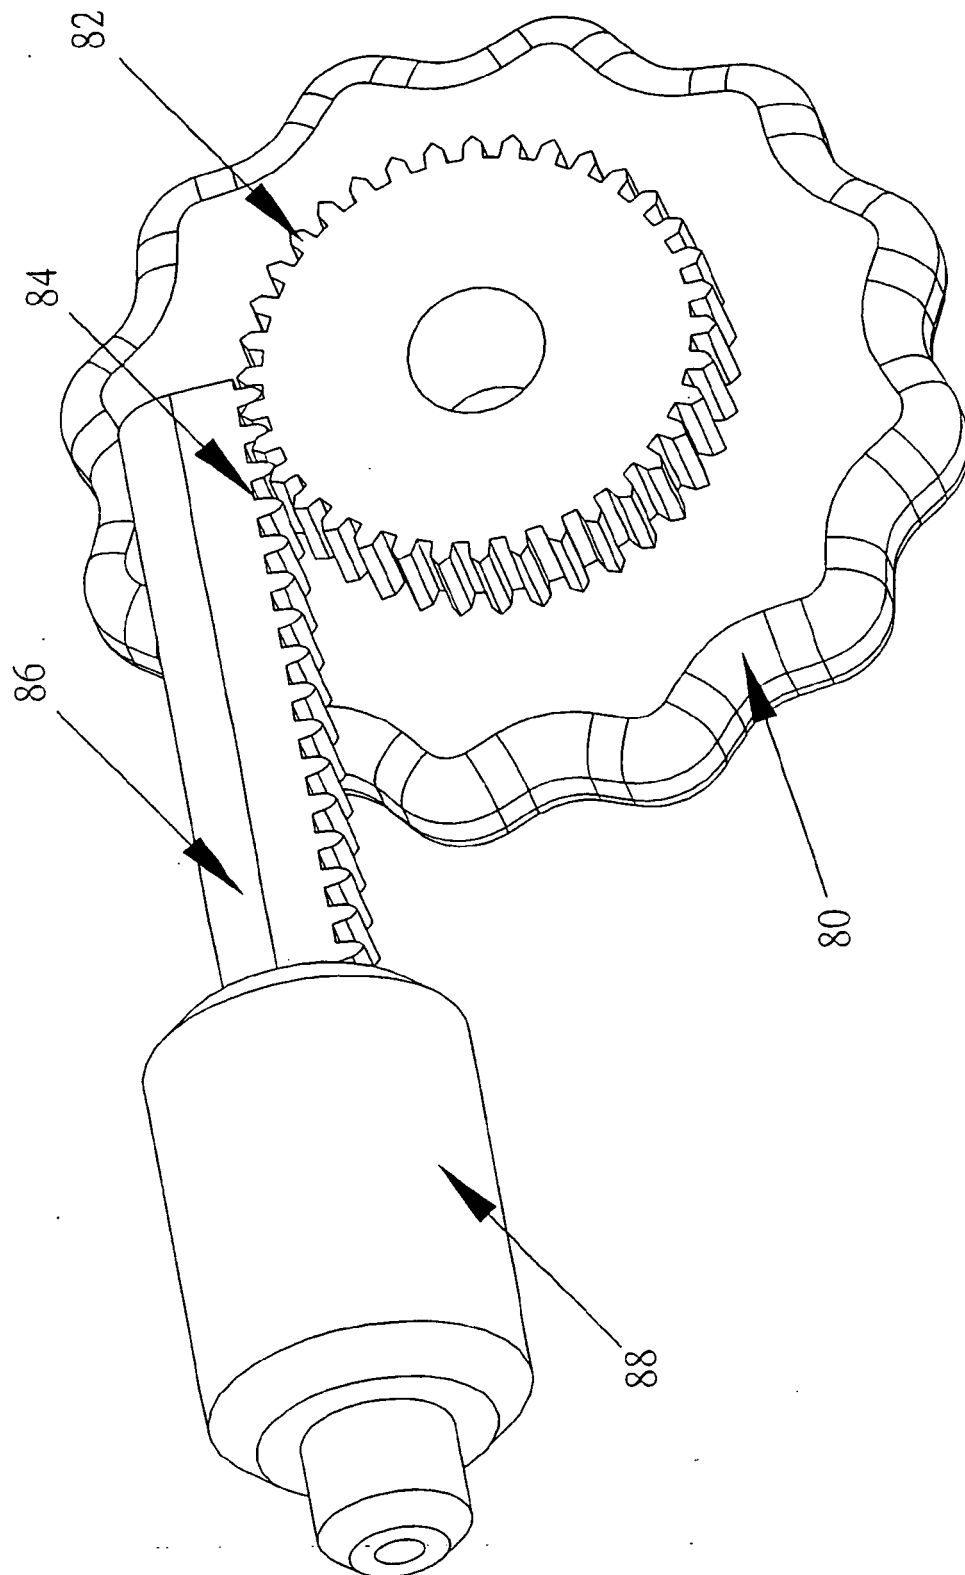


Fig. 11

Fig. 12

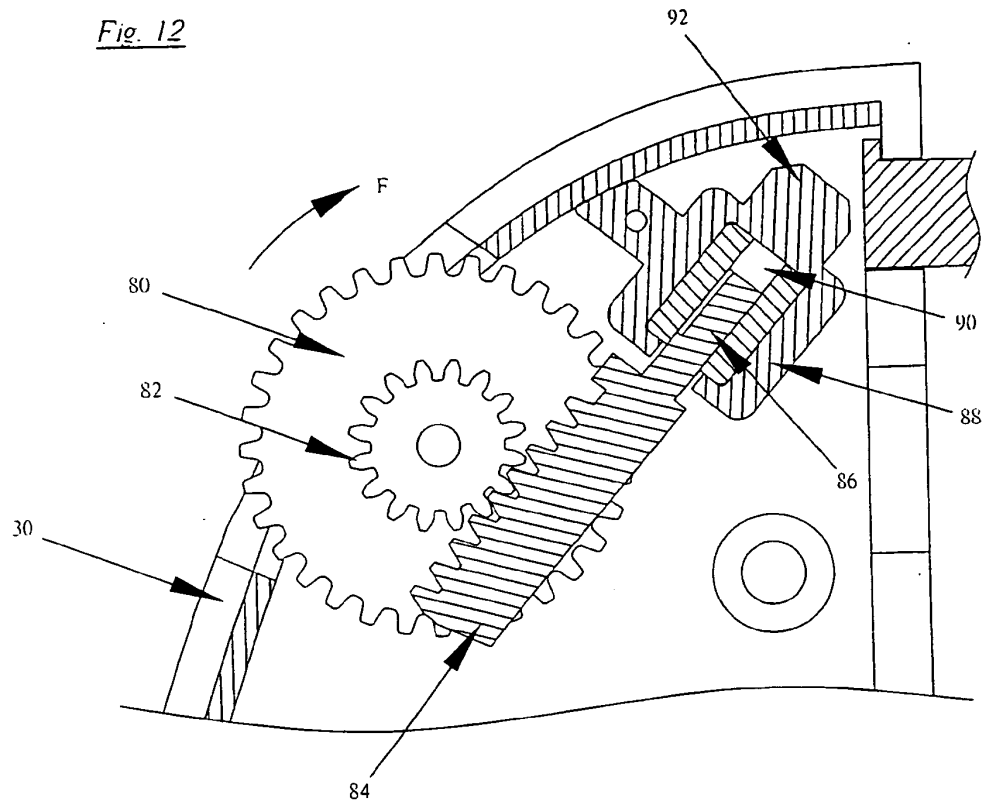
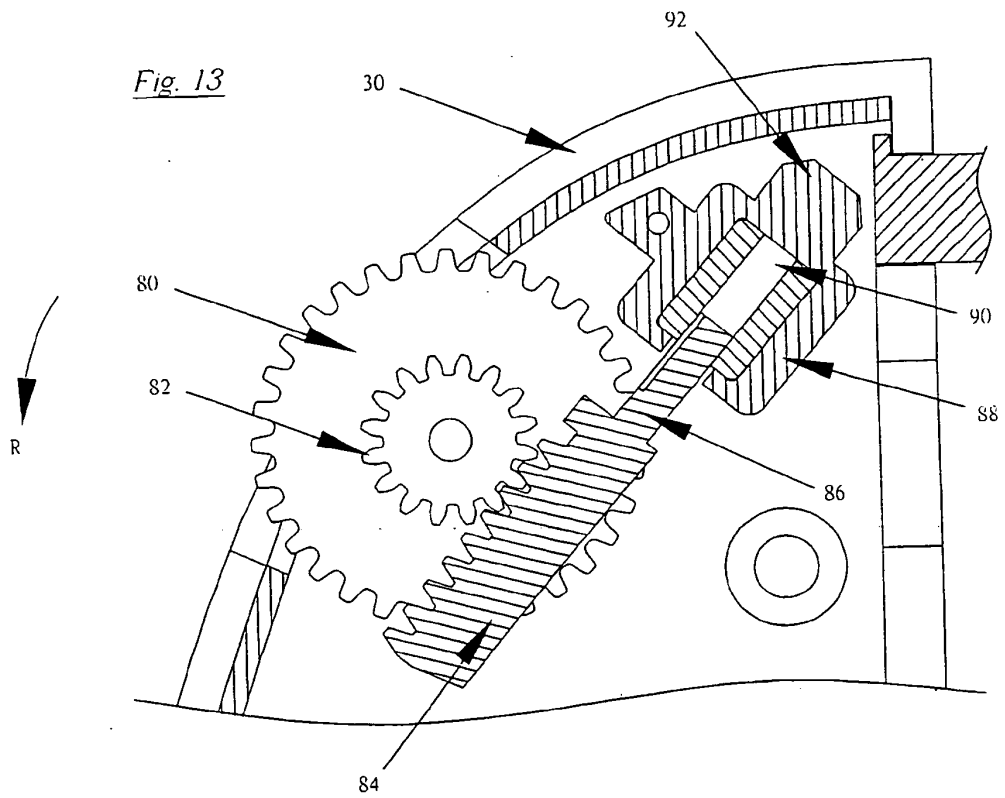


Fig. 13



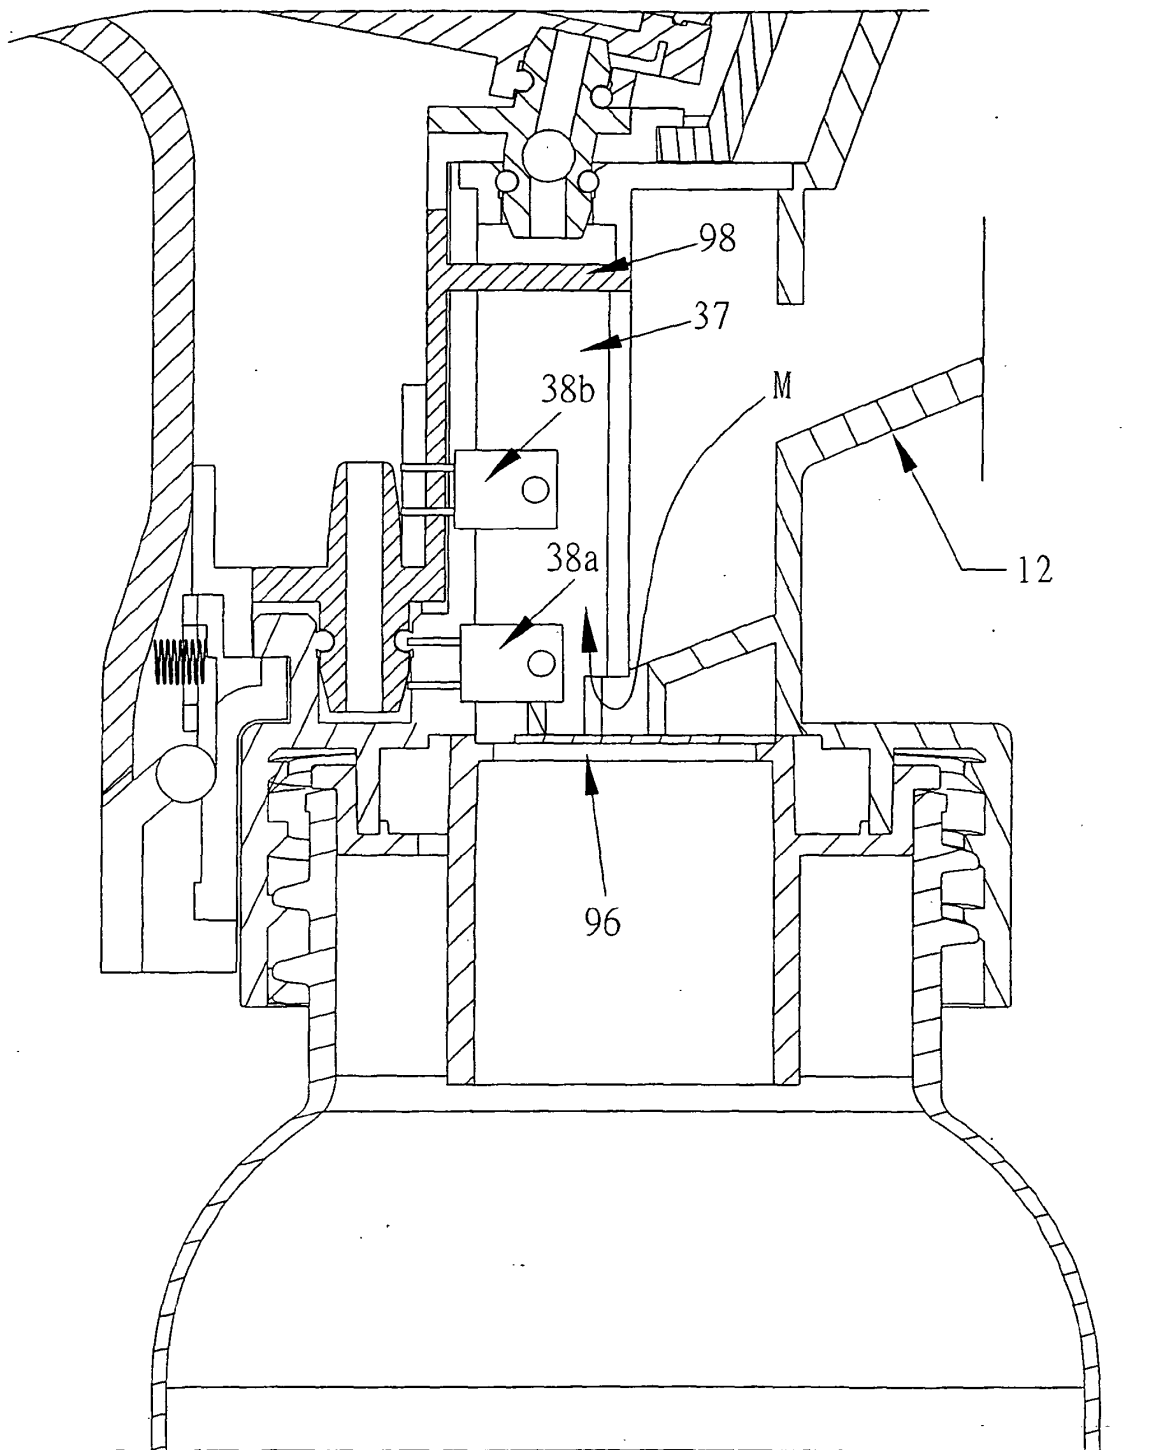


Fig. 14

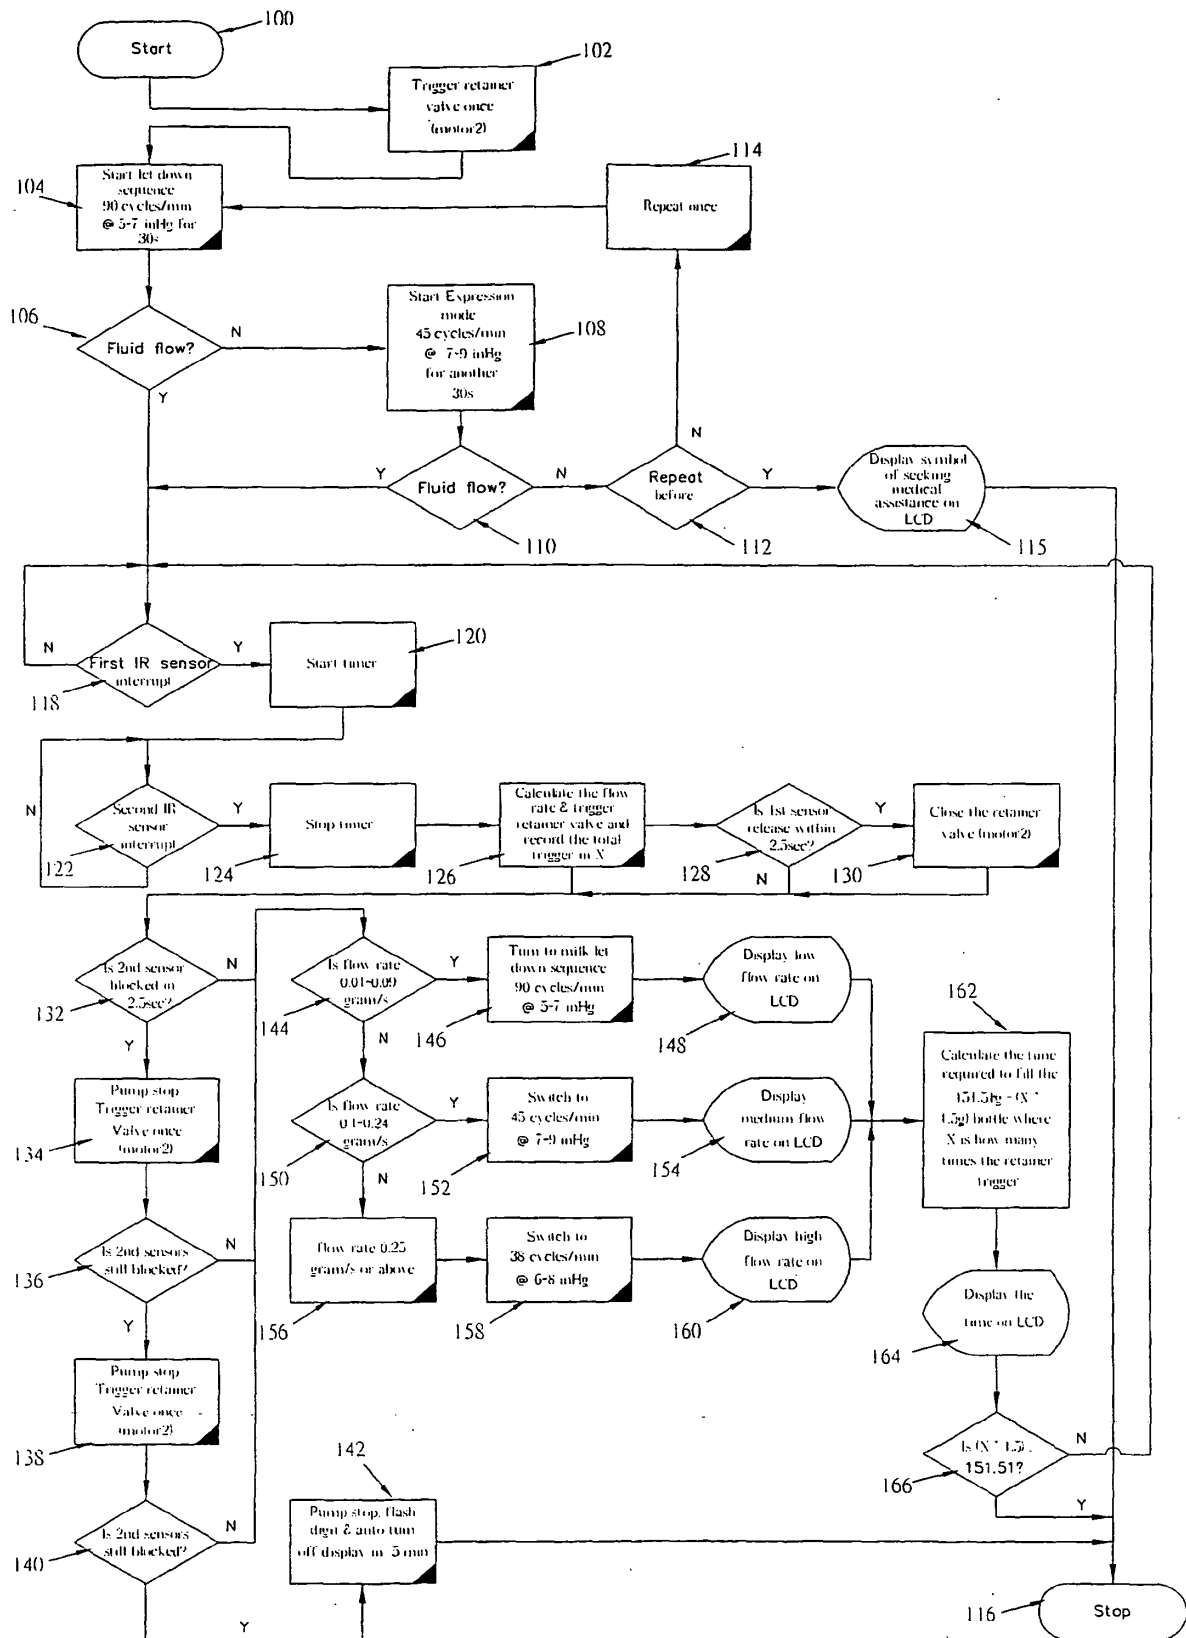


Fig. 15

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6045529 A [0002]
- US 6355012 B [0002]
- US 6547756 B, Greter [0003]
- US 6673036 B, Britto [0004]
- US 6090065 A, Giles [0004]