



US0D1007002S

(12) **United States Design Patent**  
**Jeffrey-Coker et al.**

(10) **Patent No.:** **US D1,007,002 S**

(45) **Date of Patent:** **\*\* Dec. 5, 2023**

(54) **LID FOR A REAGENT CARTRIDGE**

4,090,850 A 5/1978 Chen et al.  
D338,965 S 8/1993 Glanz et al.  
D359,126 S 6/1995 Hovatter  
D387,874 S \* 12/1997 Vila ..... D24/227  
6,096,562 A 8/2000 Bunn et al.  
(Continued)

(71) Applicant: **Singular Genomics Systems, Inc.,** La Jolla, CA (US)

(72) Inventors: **Bandeje Jeffrey-Coker,** Darnestown, MD (US); **Eli N. Glezer,** Del Mar, CA (US); **Anson Hsu,** San Diego, CA (US); **Cory Spivey,** San Diego, CA (US)

**FOREIGN PATENT DOCUMENTS**

CN 200630134998 \* 8/2007  
GB 2560161 A 9/2018  
(Continued)

(73) Assignee: **Singular Genomics Systems, Inc.,** San Diego, CA (US)

**OTHER PUBLICATIONS**

(\*\*) Term: **15 Years**

Axygen® PCR-strips of 8 tubes located at <https://www.mls.be/en/p/tubes-racks-pcr/analysercups-microtubes-pcr-disposables/axxygen-microtubes-pcr-range/axxygen-pcr-range/> last accessed May 5, 2022.  
(Continued)

(21) Appl. No.: **29/869,464**

(22) Filed: **Dec. 30, 2022**

**Related U.S. Application Data**

(63) Continuation of application No. 29/837,498, filed on May 5, 2022, now Pat. No. Des. 979,093.

*Primary Examiner* — Omeed Agilee  
(74) *Attorney, Agent, or Firm* — Mintz, Levin, Cohn, Ferris, Glovsky, Popeo, P.C.; Zachary L. Terranova

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/226; D24/227**

(57) **CLAIM**

The ornamental design for a lid for a reagent cartridge, as shown and described.

(58) **Field of Classification Search**

USPC ..... D24/128, 216, 223–230; D3/203.1, D3/203.3; D19/75, 85, 90; D8/70; D15/127, 139, 140, 141; D9/756–758  
CPC ..... A61B 5/150343; B01D 9/00; B01L 3/06; B01L 3/502; B01L 3/5025; B01L 3/5082; B01L 3/5085; B01L 9/06; A47J 36/2433  
See application file for complete search history.

**DESCRIPTION**


FIG. 1 is a front, top, and right side perspective view of a lid for a reagent cartridge of our design;  
FIG. 2 is a front view thereof;  
FIG. 3 is a rear view thereof;  
FIG. 4 is a right side view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a top view thereof; and,  
FIG. 7 is a bottom view thereof.  
The dash-dash broken lines illustrate portions of the lid for a reagent cartridge that form no part of the claimed design.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,826,347 A \* 3/1958 Schiavo ..... A47G 23/06 206/427  
D242,654 S 12/1976 Rawls  
D243,798 S \* 3/1977 Swartz ..... D24/226

**1 Claim, 3 Drawing Sheets**

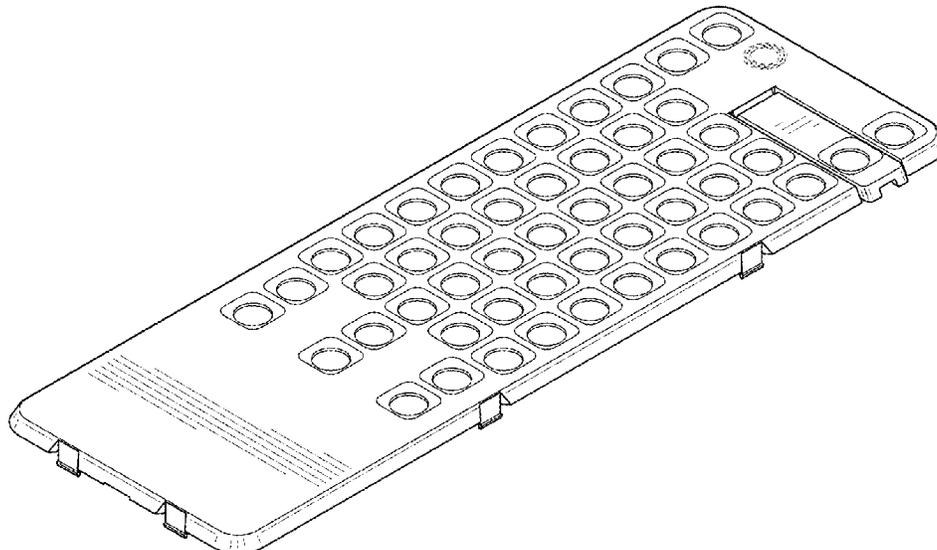

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,190,300 B1 2/2001 Demsia et al.  
6,190,878 B1 2/2001 Pierson et al.  
D438,633 S 3/2001 Miller  
D453,573 S 2/2002 Lafond et al.  
D628,306 S 11/2010 Blanc et al.  
7,854,896 B2 12/2010 Tyndorf et al.  
D632,803 S 2/2011 Motadel et al.  
D634,570 S \* 3/2011 Lin ..... D6/705  
8,182,763 B2 5/2012 Duffy et al.  
D673,293 S 12/2012 Demas et al.  
D674,112 S 1/2013 Demas et al.  
8,361,385 B2 1/2013 Glezer et al.  
D687,567 S 8/2013 Jungheim et al.  
D691,733 S 10/2013 Demas et al.  
D699,370 S 2/2014 Motadel et al.  
8,701,913 B2 4/2014 Pack et al.  
D709,625 S 7/2014 Baum et al.  
D709,718 S \* 7/2014 Snyder ..... D6/682.4  
9,080,207 B2 7/2015 Handique et al.  
D735,881 S 8/2015 Thomas et al.  
9,180,461 B2 11/2015 Edens et al.  
9,260,763 B2 2/2016 Thomas et al.  
9,267,890 B2 2/2016 Kawata et al.  
D759,835 S 6/2016 Baum et al.  
9,408,965 B2 \* 8/2016 Christensen ..... B65D 25/108  
9,488,648 B2 11/2016 Neely et al.  
9,519,000 B2 12/2016 Wilson et al.  
D776,297 S 1/2017 Demas et al.  
9,702,852 B2 7/2017 Lowery et al.  
D808,540 S 1/2018 Johns et al.  
D812,243 S 3/2018 Johns et al.  
9,931,635 B1 4/2018 Ho  
10,071,381 B2 9/2018 Welch et al.  
D840,049 S 2/2019 Schulz et al.  
D840,050 S 2/2019 Schulz et al.  
D840,051 S 2/2019 Schulz et al.  
D843,007 S 3/2019 Schulz et al.  
10,220,392 B2 3/2019 Baum et al.  
10,241,054 B2 3/2019 Williams et al.  
D848,637 S 5/2019 Schulz et al.  
D852,977 S 7/2019 Suchocki et al.  
D854,707 S 7/2019 Jakobsen et al.  
10,335,787 B2 7/2019 Haghgooeie et al.  
10,351,843 B2 7/2019 Belz et al.  
D856,527 S 8/2019 Kaplan et al.  
D857,228 S 8/2019 Kaplan et al.  
D857,229 S 8/2019 Kaplan et al.  
10,377,538 B2 8/2019 Crivelli et al.  
D861,914 S 10/2019 Blake et al.  
D864,412 S 10/2019 Dangelo et al.  
D865,213 S 10/2019 Dangelo et al.  
D865,215 S 10/2019 Dangelo et al.  
D889,685 S 7/2020 Leimkuehler et al.  
D902,431 S 11/2020 Sims et al.  
10,921,336 B2 2/2021 Hansen et al.  
D918,417 S 5/2021 O'Mahony et al.  
D919,115 S 5/2021 Kaplan et al.  
11,000,851 B2 5/2021 Knight  
D928,984 S \* 8/2021 Yoo ..... D24/227  
D932,052 S 9/2021 Zergiebel et al.  
11,199,538 B2 12/2021 Burd et al.  
11,254,942 B2 2/2022 Tian et al.  
11,293,021 B1 4/2022 Bernate et al.  
D954,996 S \* 6/2022 Motadel ..... D24/229  
D959,018 S 7/2022 Livingston et al.  
2004/0238401 A1 12/2004 Greenstein et al.  
2008/0257882 A1 10/2008 Turner  
2011/0236278 A1 \* 9/2011 Motadel ..... B01L 9/543  
422/560  
2013/0030914 A1 1/2013 Ho  
2013/0108522 A1 \* 5/2013 Cohen ..... B01L 9/543  
422/552  
2014/0234182 A1 8/2014 Motadel et al.  
2017/0036207 A1 2/2017 Wright et al.  
2017/0043346 A1 2/2017 Welch et al.

2017/0136467 A1 5/2017 Johns et al.  
2017/0197213 A1 7/2017 Nielsen et al.  
2020/0029003 A1 1/2020 Frank et al.  
2020/0122141 A1 4/2020 Haghgooeie et al.  
2021/0324445 A1 10/2021 Buse et al.  
2022/0080425 A1 3/2022 Bashar et al.  
2022/0112452 A1 4/2022 Garst et al.  
2022/0112508 A1 4/2022 Garst et al.

## FOREIGN PATENT DOCUMENTS

JP D2022-27508 \* 5/2023  
KR 3020190032223 7/2019  
WO WO-2001/060519 A1 8/2001  
WO WO-2020/183195 A1 9/2020  
WO WO-2021/126420 A1 6/2021

## OTHER PUBLICATIONS

Capp 0. 1 and 0.2 ml PCR Strip Tubes, located at <<https://www.capp.dk/product/expellper-strip-tubes>> last accessed May 5, 2022.  
Fischer Scientific—Eppendorf™ PCR Tube Strips and Domed Cap Strips, 0.1 ml, located at <<https://www.fishersci.se/shop/products/eppendorf-0-ml-per-tubes-cap-strips/10146704>> last accessed May 5, 2022.  
Hitachi—Compact CE Sequencer DS3000 located at <<https://www.hitachihihtech.com/global/science/products/bio-systems/sequencer/ds3000.html>> last accessed May 5, 2022.  
Ion 540™ Kit-Chef (2 sequencing runs per initialization) located at <<https://www.thermofisher.com/order/catalog/product/A30011>> last accessed May 5, 2022.  
LabX Ion S5 Semiconductor Sequencer+ Ion Chef System | For Sale | Labx Ad 14035113, located at <[https://www.google.com/imgres?imgurl=https%3A%2F%2Fcheckout.labx.com%2Fpub%2Fmedia%2Fcatalog%2Fproduct%2Fi%2Fm%2Fimg-20220202-09243\\_1\\_058.jpg&imgrefurl=https%3A%2F%2Fwww.labx.com%2Fitem%2Fion-s5-semiconductor-sequencer-ion-chef-system%2F14035113&tbnid=CtQy2sS\\_zECkM&vet=10CK0BEDMtgFqFwoTCPCy84qHpfCFQAAAAAAdAAAAABAD.i&docid=18bcwsY5Nbi5hM&w=1600&h=1200&q=DNA%20sequencer%20reagent%20cartridges&ved=0CK0BEDMtgFqFwoTCPCy84qHpfCFQAAAAAAdAAAAABAD](https://www.google.com/imgres?imgurl=https%3A%2F%2Fcheckout.labx.com%2Fpub%2Fmedia%2Fcatalog%2Fproduct%2Fi%2Fm%2Fimg-20220202-09243_1_058.jpg&imgrefurl=https%3A%2F%2Fwww.labx.com%2Fitem%2Fion-s5-semiconductor-sequencer-ion-chef-system%2F14035113&tbnid=CtQy2sS_zECkM&vet=10CK0BEDMtgFqFwoTCPCy84qHpfCFQAAAAAAdAAAAABAD.i&docid=18bcwsY5Nbi5hM&w=1600&h=1200&q=DNA%20sequencer%20reagent%20cartridges&ved=0CK0BEDMtgFqFwoTCPCy84qHpfCFQAAAAAAdAAAAABAD)> last accessed May 5, 2022.  
MiSeq Reagent Kit v3 located at <<https://www.illumina.com/systems/sequencingplatforms/miseq/products-services.html>> last accessed May 5, 2022.  
NextSeq 500/550 v2.5 Kits located at <<https://www.illumina.com/products/bytype/sequencingkits/cluster-gen-sequencing-reagents>> last accessed May 5, 2022.  
NovaSeq Reagent Kits, Illumina, located at <<https://www.illumina.com/products/bytype/sequencing-kits/cluster-gen-sequencing-reagents/novaseq-reagent-kits.html>> last accessed May 5, 2022.  
Preparing DNA Libraries for Sequencing on the Mi Seq®. (Jan. 2013) located at <<https://content.ilabsolutions.com/wp-content/uploads/2013/04/MiSeq-Preparing-DNA-libraries.pdf>> last accessed Sep. 2, 2022.  
Qiagen—QIAsymphony® DNA Maxi Handbook located at <<https://www.google.com/imgres?imgurl=x-rawimage%3A%2F%2Ffae1930bd2bc06f496a635e47df671c1818eff4edfb5a5123e3a71ff012524a&imgrefurl=https%3A%2F%2Fwww.qiagen.com%2Fde%2Fresources%2Fdownload.aspx%3Fid%3D71390d4f-115f-4368-ba2e-5f6cf7936b21%26lang%3Den&tbnid=9Aa80guT4fgjvM&vet=10CAoQMjyUAWoXChMI8LLzioel9wIVAAAAAB0AAAAAEAQ..i&docid=7suz1oSWWcuBtM&w=1109&h=439&g=DNA%20sequencer%20reagent%20cartridges&ved=0CAoQMjyUAWoXChMI8LLzioel9wIVAAAAAB0AAAAAEAQ/>> last accessed May 5, 2022.  
Qiagen—RNA kit located at <<https://www.qiagen.com/us/products/discovery-and-translationalresearch/dna-rna-purification/rna-purification/total-rna/qiasymphony-rna-kit/>> last accessed May 5, 2022.  
Removable 8 Well PCR Tube Strip located at <<https://www.azenta.com/products/removable-8-well-per-tube-strip>> last accessed May 5, 2022.

(56)

**References Cited**

OTHER PUBLICATIONS

Stellar Scientific—SeeMore 0.2ml Optically Clear PCR Strip Tube with Separate Dome Caps, located at <<https://www.stellarscientific.com/seemore-0-2ml-optically-clear-pcr-strip-tube-withseparate-dome-caps-sterile-125-pack/#&gid=1&pid=1>> last accessed May 5, 2022.  
T320-2 & T320-3 Amplitube™ 8 Tube Strips With Individually Attached Caps, located at <<https://www.simport.com/en/products/224-t320-2.html>> last accessed May 5, 2022.

\* cited by examiner


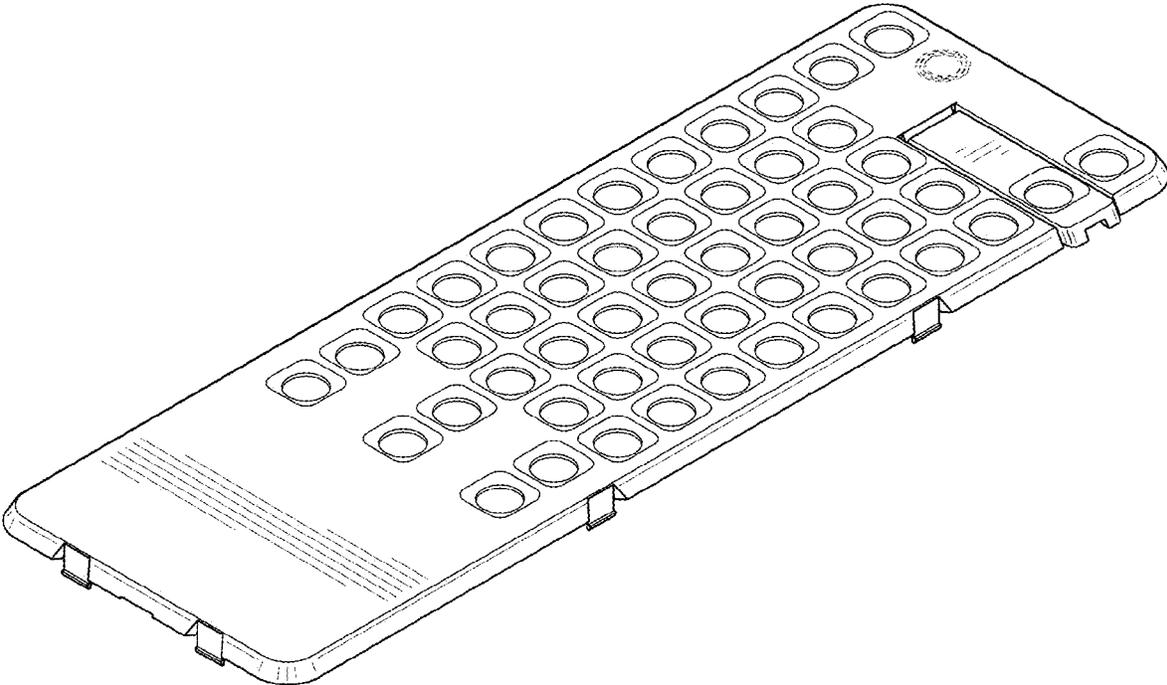


FIG.1




**FIG. 2**



**FIG. 3**



**FIG. 4**



**FIG. 5**

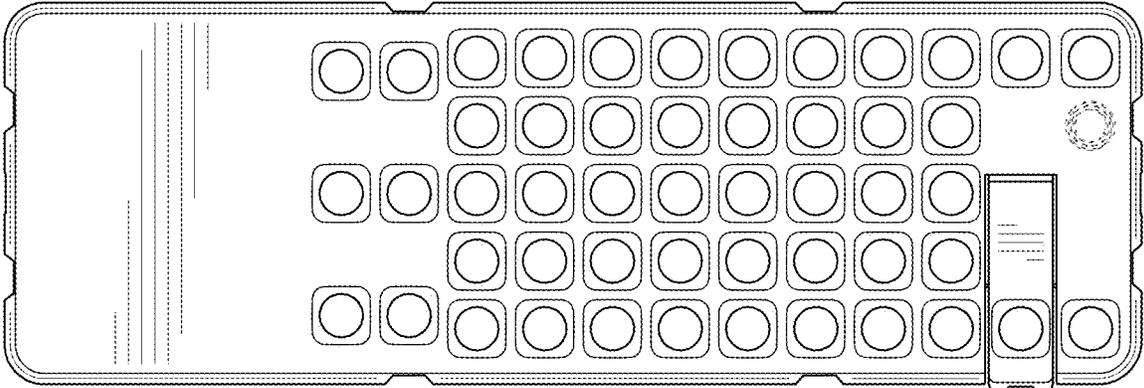


FIG. 6

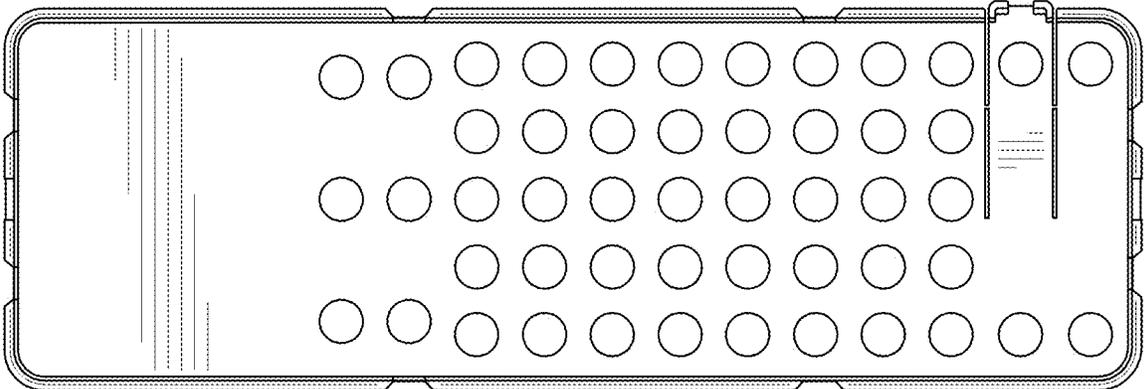


FIG. 7