



(51) International Patent Classification:
G02B 21/00 (2006.01) **G02B 27/24** (2006.01)
G02B 27/22 (2006.01)

(21) International Application Number:
PCT/US2010/052512

(22) International Filing Date:
13 October 2010 (13.10.2010)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/251,237 13 October 2009 (13.10.2009) US
61/381,389 9 September 2010 (09.09.2010) US
12/903,650 13 October 2010 (13.10.2010) US

(71) Applicants (for all designated States except US): **CALIFORNIA INSTITUTE OF TECHNOLOGY** [US/US]; 110 East California Blvd., Pasadena, California 91125 (US). **WU, Jigang** [CN/US]; 301 Verano Place, Irvine, California 92617 (US). **PANG, Shuo** [CN/US]; 307 S. Wilson Ave., Apt. 4, Pasadena, California 91106 (US).

(72) Inventor; and

(75) Inventor/Applicant (for US only): **YANG, Changhuei** [SG/US]; 1269 E. Elizabeth Street, Pasadena, California 91104 (US).

(74) Agent: **MARTINEZ-LEMKE, Sheila**; 110 Pacific Avenue, Suite 240, San Francisco, California 94111 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,

[Continued on next page]

(54) Title: HOLOGRAPHICALLY ILLUMINATED IMAGING DEVICES

(57) Abstract: Embodiments of the present invention relate to holographically illuminated imaging devices including a holographic element for transforming an illumination beam into a focal array of light spots, a scanning mechanism for moving an object across one or more light spots in the focal array of light spots, and a light detector for detecting light associated with the focal array of light spots and generating light data associated with the received light.

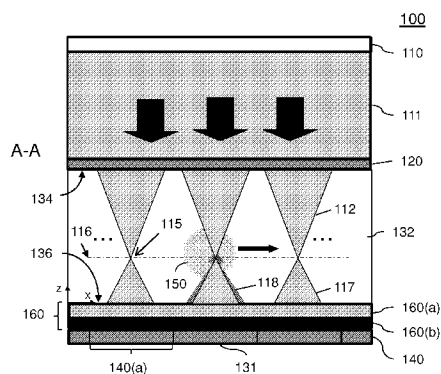


FIG. 2(a)

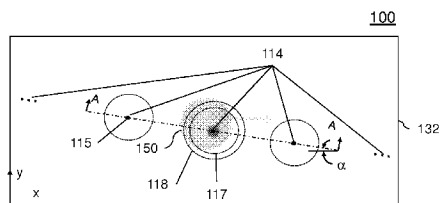


FIG. 2(b)



SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG). **Published:**

— *without international search report and to be republished
upon receipt of that report (Rule 48.2(g))*

HOLOGRAPHICALLY ILLUMINATED IMAGING DEVICES

CROSS-REFERENCES TO RELATED APPLICATIONS

[0001] This is a non-provisional application of and claims priority to U.S. Provisional Patent Application No. 61/251,237 entitled “Approaches for Building Compact Fluorescence Microscopes” filed on October 13, 2009 and to U.S. Provisional Patent Application No. 61/381,389 entitled “Fluorescence Optofluidic Microscope” filed on September 9, 2010. These provisional applications are hereby incorporated by reference in their entirety for all purposes.

[0002] This non-provisional application is related to the following co-pending and commonly-assigned patent applications, which are hereby incorporated by reference in their entirety for all purposes:

- U.S. Patent Application No. 12/398,050 entitled “Optofluidic Microscope Device with Photosensor Array” filed on March 4, 2009.
- U.S. Patent Application No. 12/399,823 entitled “Scanning Illumination Microscope” filed on March 6, 2009.
- U.S. Patent Application No. 12/886,779 entitled “Reflective Focusing and Transmissive Projection Device” filed on September 21, 2010.

BACKGROUND OF THE INVENTION

[0003] Embodiments of the present invention generally relate to sensing and imaging devices. More specifically, certain embodiments relate to holographically illuminated imaging devices used in microscopy and photography.

[0004] Microscopes and other optical microscopy devices are used extensively in modern biomedicine and bioscience. Typically, conventional microscopes include an objective lens, a platform for supporting a specimen, and an eyepiece containing lenses for focusing images. These conventional microscope designs have bulky optics, and have proven to be expensive and difficult to miniaturize. Further, since high resolution objective lenses have a limited field of view, the specimen stage must be moved to increase the scope of the view, which can be time-consuming.

[0005] A conventional confocal laser scanning microscope uses a laser beam to provide light which is focused by an objective lens into a small focal volume at the specimen. Scattered and reflected laser light as well as any fluorescence light from the illuminated spot on the specimen is collected by the objective lens. The collected light is transmitted to a beam splitter which separates out the light of interest and transmits it to a detection apparatus. As the laser scans, an image can be obtained of the specimen. This technique can be time-consuming.

BRIEF SUMMARY OF THE INVENTION

[0006] Embodiments of the present invention relate to holographic illumination in sensing and imaging devices. More specifically, certain embodiments relate to holographically illuminated imaging devices (HIIDs) having a holographic element to transform a planar wavefront from an illumination beam into at least one focal array of light spots in a fluid channel. A fluid flow moves an object through the light spots in the fluid channel. The object alters the light (e.g., fluorophores absorb light and emit light of a different light property). A light detector detects the altered light (e.g., emissions) and generates time varying data which can be used to produce an image of the object. One embodiment includes an HIID with a plurality of focal arrays along the fluid channel at different depths, forming a three-dimensional focal array. This configuration can be used to generate sectional images or three-dimensional images of the object moving through the fluid channel.

[0007] One embodiment is directed to a HIID comprising a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots. The HIID further comprises a scanning mechanism configured to move an object across one or more light spots in the focal array of light spots. The HIID further comprises a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light.

[0008] Another embodiment is directed to a HIID comprising a body defining a fluid channel. The HIID further comprises a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots. The HIID further comprises a beam splitter configured to reflect the focal array of light spots into the fluid channel wherein a flow in the channel moves an object across one or more light spots in the focal array of light spots. The beam splitter is further configured to transmit light altered by the object. The HIID further comprises a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light.

[0009] Another embodiment is directed to a HIID comprising a holographic element configured to transform an illumination beam into a plurality of focal arrays of light spots at different focal planes. The HIID further comprises a scanning mechanism configured to move an object across one or more light spots in the plurality of focal arrays of light spots. The HIID further comprises a light detector configured to receive light associated with the plurality of focal arrays of light spots, and generate light data associated with the received light.

[0010] Another embodiment is directed to a system comprising a HIID and a processor. The HIID includes a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots. The HIID also includes a scanning mechanism configured to move an object across one or more light spots in the focal array of light spots. The HIID also includes a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light. The HIID also includes a processor in communication with the light detector. The processor is configured to receive a signal with light data and generate an image of the object based on the light data.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] **FIG. 1** is a block diagram of components of an HIID system, in accordance with embodiments of the disclosure.

[0012] **FIG. 2(a)** is a schematic drawing of a cross sectional view of components of an HIID employing a microfluidic flow, according to embodiments of the invention.

[0013] **FIG. 2(b)** is a schematic drawing of a partial top view of components of the HIID of **FIG. 2(a)**, according to embodiments of the invention.

[0014] **FIG. 3** is a schematic drawing of components of an HIID having a collection component, according to embodiments of the invention.

[0015] **FIG. 4** is a schematic drawing of components of an HIID having a collection component including a diffraction optical element (DOE) and a beam block, according to embodiments of the invention.

[0016] **FIG. 5** is a schematic drawing of components of an HIID having a reflective design, according to embodiments of the invention.

[0017] **FIG. 6** is a schematic drawing of components of an HIID having multiple focal arrays in series at different depths for sectional imaging or three-dimensional imaging, according to embodiments of the invention.

[0018] **FIG. 7** is a schematic drawing of components of an HIID having multiple focal arrays in series with different differentiating elements for multi-spectral fluorescence or phosphorescence imaging, according to embodiments of the invention.

[0019] **FIG. 8(a)** is a schematic drawing of a setup for off axis recording a holographic element, according to embodiments of the invention.

[0020] **FIG. 8(b)** is a schematic drawing of a setup for inline recording a holographic element, according to embodiments of the invention.

[0021] **FIG. 9** is a block diagram of subsystems that may be present in computer devices that are used in an HIID system, according to embodiments of the invention.

DETAILED DESCRIPTION OF THE INVENTION

[0022] Embodiments of the present invention will be described below with reference to the accompanying drawings. One embodiment includes an HIID having a holographic element for illuminating a fluid channel carrying an object being imaged. The holographic element transforms a planar wavelength of an illumination beam into an array of spherical wavefront or approximately spherical wavefront to form a focal array of tightly confined light spots diagonally extending across the fluid channel. As the object moves past light spots, the light is altered (e.g., fluorophores absorb light and emit light of a different property). A differentiating element transmits the altered light (e.g., emissions) to a light detector which generates time varying data, which is used to generate images (e.g., fluorescent images) of the object.

[0023] Some conventional imaging systems use a lens array to channel uniform light into light spots. The spacing between the light spots is restricted by the diameter of the lens. For example, to create an array of light spots with a spacing of 30 micron using an appropriate lens array, each lens would have about a 30 micron diameter. The numerical aperture of each lens is also limited by the lens diameter.

[0024] The HIID of embodiments does not have these restrictions because it uses a holographic element. A holographic element can represent a series of overlapping effective 'lenses.' The effective 'lenses' can channel an illumination beam into overlapping focal cones and into light spots. Since the focal cones overlap, the spacing between the light spots is not dependent on the diameter of the effective 'lens.' The holographic element can also have a much higher achievable numerical aperture than a lens array and may be capable of generating higher resolution images. Examples of holographic elements that generate light spots can be found in Wu, Jigang, Cui, Xiquan, Zheng, Guoan, Wang, Ying Min, Lee, Lap Man, Yang, Changhui, "Wide field-of-view microscope based on holographic focus grid illumination," Optics Letters, Vol. 35, No. 13, July 1, 2010, which is hereby incorporated by reference in their entirety for all purposes.

[0025] The HIIDs of embodiments of the invention provide one or more advantages. One advantage is that the HIID provides more localized illumination which can improve image resolution. Since the holographic element does not have the same physical restrictions of a lens array, the holographic element may be able to generate tighter focused light spots in a shorter focal length, which can allow for higher resolution images. In a microfluidic flow

application (e.g., an optofluidic microscope), a holographic element may provide tightly focused light spots within the short width of a fluid channel, which can provide better illumination than conventional systems. This improved illumination can result in higher resolution images. In some embodiments, image resolution of less than 0.6 micron can be achieved. Another advantage is that the HIID has more effective usage of a given illumination beam (e.g., excitation light) than conventional imaging devices. The use of a holographic element allows for effective channeling of the light power in an illumination beam into tightly confined light spots. In some embodiments, a holographic element of an HIID may be able to channel up to 47% of an illumination beam into the light spots. Some embodiments may be able to provide a local light intensity at the light spots of values of about $3 \times 10^4 \text{ W/cm}^2$. Another advantage is that the HIID has few components in a simple multi-layered structure that can be fabricated in an on-chip design. Since the HIID can be designed in a multilayered structure, the device can be an on-chip design inexpensively fabricated using standard semiconductor and micro/nanofabrication procedures. A multi-layered on-chip design can also be easily miniaturized. Another advantage is that the HIID can employ microfluidic flow for high throughput analyses and imaging. These microfluidic flow methods can also be highly automated. Another advantage is that an HIID has the flexibility of being designed with a focal plane away from the surface of a fluid channel in a microfluidic flow application. The HIID can be designed to locate the focal plane of the light spots at any arbitrary height within the fluid channel so that the high resolution images can be generated at any arbitrary height. This flexibility is useful as it frees the restriction of having to flow specimens with the objects close to either the channel floor or ceiling for good image acquisition.

[0026] I. HIID System

[0027] FIG. 1 is a block diagram of components of an exemplary HIID system **10**, in accordance with embodiments of the disclosure. The HIID system **10** includes an HIID **100** communicatively coupled to a host computer **200**. Although the illustrated embodiment includes a single HIID **100** and a single host computer **200**, other embodiments may include two or more HIIDs **100** and/or host computers **200**.

[0028] The HIID **100** includes an illumination source **110**, a holographic element **120**, a scanning mechanism **130** and a light detector **140**. The holographic element **120** transforms a wavefront of an illumination beam (shown in **FIG. 2(a)**) by the illumination source **110** into

an array of converging spherical wavefront to form a focal array of light spots **114** (shown in **FIG. 2(b)**) to illuminate an object **150** (shown in **FIG. 2(a)**) being imaged by the HIID **100**. Although many embodiments show an array of converging spherical wavefront, approximately spherical wavefront or other wavefront with well separate structure can be used in other embodiments. The scanning mechanism **130** moves the focal array of light spots relative to the object **150** or move the object **150** relative to the focal array of light spots. The light detector **140** light altered (e.g., blocked, reduced intensity, and/or modified wavelength or other light property) by the object **150**. The light detector **140** generates light data associated with light received by the light detector **140**. Although the illustrated embodiment includes a single illumination source **110**, a single holographic element **120**, a single scanning mechanism **130** and a single light detector **140**, other embodiments may include any suitable number of these components.

[0029] The host computer **200** comprises a processor **210** (e.g., a microprocessor) communicatively coupled to the light detector **140**, a computer readable medium (CRM) **210**, and a display **230**. The processor **200** receives signals with light data from the light detector **140**. The processor **210** executes code stored on the CRM **210** to generate images or otherwise analyze the object **150** using the light data. The images and other output can be shown on the display **230**. Any suitable images can be generated such as photoluminescence images, intensity images, phase images, differential interference contrast (DIC) images, etc. A photoluminescence image can refer to a fluorescence image or a phosphorescence image.

[0030] The illumination source **110** may be a component of the HIID **100** or may be separate from the HIID **100**. The illumination source **110** may be provided by any suitable device(s). Some suitable devices include light-emitting diodes (LED), laser of suitable wavelength, broadband source (e.g., mercury lamp, halogen lamp, etc.) with a suitable filter, etc. Suitable illumination sources are commercially available. The illumination source **110** may be placed in any suitable location to generate the appropriate wavefront at the holographic element **120**. The illumination source **110** may provide an illumination beam of any suitable wavelength, intensity, phase, polarization, spin angular momentum or other light property, and any suitable spatial distribution. In exemplary embodiments, the illumination source **110** provides an illumination beam with the same wavelength, same spatial distribution and/or other light properties, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. In exemplary fluorescence/phosphorescence embodiments, the illumination source **110** provides excitation

light having a first light property (e.g., first wavelength) matching the excitation wavelength of the fluorophores in an object **150** being imaged. The fluorophores are excited by the excitation light and emit light (emissions) of a second light property (e.g., second wavelength). Some examples of suitable excitation light include fluorescence, 2-photon or higher order fluorescence, Raman, second harmonic or higher order, or other emission mechanism that results in emissions at a different wavelength or other different light property than the excitation light.

[0031] As used herein, a holographic element **120** refers to a suitable holographic film/plate/crystal capable of converting an illumination beam **111** (shown in **FIG. 2(a)**) from an illumination source **110** into a focal array of light spots **114** (shown in **FIG 2(b)**). In many illustrated embodiments, the holographic element **120** transforms a wavefront of the illumination beam **111** from the illumination source **110** into an array of spherical wavefront to form a focal array of light spots **114**. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. The holographic element **120** can be made of any suitable materials. Some examples of suitable holographic materials include photographic emulsions, dichromated gelatin, and photoresists. The holographic element **120** can have any suitable dimensions (e.g., 1 mm x 1 mm, 2 mm x 2 mm, 5 mm x 2 mm, 10 mm x 10 mm, 10 mm x 50 mm, etc.). The holographic element **120** can be made using any holographic recording technique capable of encoding (recording) data about the focal array of light spots. Some examples of suitable holographic recording techniques include in-line (Gabor) and off-axis (Leith-Upatnieks). To play back the recording, the holographic element **120** can be illuminated by an illumination beam having the same wavelength, same spatial distribution, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. Use of a holographic element **120** can allow for effective channeling of light power from the illumination source **110** into the light spots **115**.

[0032] The focal array of light spots **114** (shown in **FIG. 2(b)**) can have any suitable number of light spots (e.g., 1, 10, 100, 200, etc.) and can be any suitable array or combination of arrays. Some examples of suitable arrays include a one-dimensional array, a two-dimensional array, a three-dimensional array, and a multiplicity of one-dimensional, two-dimensional, and/or three-dimensional arrays. The arrays can have any suitable orientation or combination of orientations. In some embodiments, a three-dimensional array can be used to

image at different depth positions of the specimen having the object **150** being imaged. For example, **FIG. 6** is an illustration of an embodiment of an HIID **100** having a holographic element **120** generating a three-dimensional focal array of light spots **600** along the longitudinal axis of the fluid channel **132** and at different focal planes through the depth of the fluid channel **132**. In **FIG. 6**, the three-dimensional array **600** is comprised of a plurality of n one-dimensional focal arrays of light spots **114(1)-114(n)** at n different focal planes **116(1)-116(n)** at different depths of the fluid channel **132**. As an object **150** moves through the fluid channel **132**, the light spots illuminate the object **150** at different focal planes and the object **150** alters the light. The light data can be used to generate sectional images of the object **150** at different depths and/or generate three-dimensional images of the object **150**.

[0033] Each light spot **115** can be of any suitable size. Some examples of suitable diameters (FWHM) are 0.4 microns, 0.6 microns, 0.8 microns, 1 micron, etc. In one exemplary embodiment, the light spot diameter is 0.6 microns (FWHM). Any suitable spacing (5 microns, 10 microns, 15 microns, etc.) can be used between the light spots **115**. In one exemplary embodiment, a light spot spacing of 20 microns is used.

[0034] In some embodiments, the holographic element **120** can be replaced by a diffractive optical element (DOE) in the HIID **100**. A DOE refers to any suitable structure capable of diffracting light to generate a desired light pattern such as a focal array of light spots. Some examples of suitable DOEs include a Fresnel Zone plate, diffraction grating, photon sieve, etc. The DOE can be made of any suitable material and may have any suitable dimensions (e.g., 1 mm x 1 mm, 2 mm x 2 mm, 5 mm x 2 mm, 10 mm x 10 mm, 10 mm x 50 mm, etc.). In some cases, using DOEs may be advantageous because they have a comparatively high shelf life. DOEs are also suitable for nanofabrication and semiconductor fabrication technique.

[0035] As used herein, the scanning mechanism **130** refers to a suitable device(s) capable of moving the object **150** being imaged relative to the light spots or the light spots relative the object **150** to substantially illuminate the object **150**. The scanning mechanism **130** can be based on any suitable method including, for example, microfluidic flow methods, optical tweezing methods, and scanning methods (raster scanning, linear scanning, etc.). An example of a scanning mechanism **130** employing a microfluidic flow method includes a fluid channel **132** having a fluid flow with the object **150** being imaged. In another example, the scanning mechanism **130** may include a raster scanning device for raster scanning the

object **150** or specimen stage with the object **150** through the light spots or raster scanning the light spots over the object **150**. The scanning mechanism **130** can be in any suitable location that does not block the light from the illumination source **110**.

[0036] A light detector **140** (e.g., a photosensor) refers to any suitable device capable of detecting light and generating signals with light data. The signals may be in the form of electrical current that results from the photoelectric effect. The light detector can be a single detector, a one-dimensional detector array, or a two-dimensional detector array. Some examples of single detectors include a photo-diode (PD), an avalanche photo-diode (APD) and a photomultiplier tubes (PMT). Some examples of one-dimensional or two-dimensional detector arrays include a charge coupled device (CCD) array, a complementary metal-oxide-semiconductor (CMOS) array, an APD array, a PD array, a PMT array, etc.

[0037] The light detector **140** includes one or more discrete light detecting elements **140(a)** (shown in **FIG. 2(a)**) of any suitable size (e.g., 1-10 microns) and any suitable shape (e.g., circular or square). For example, a CMOS or CCD light detecting element **140(a)** may be 1-10 microns and an APD or PMT light detecting element **140(a)** may be as large as 1-4 mm. The light detecting elements **140(a)** can be arranged in any suitable form such as a one-dimensional array, a two-dimensional array, or a multiplicity of one-dimensional and/or two-dimensional arrays. The arrays can be in any suitable orientation or combination of orientations. In some cases, the light detecting elements **140(a)** can be arranged to correspond to the focal array of light spots **114** (shown in **FIG. 2(b)**). For example, the light detecting elements **140(a)** can have the same form as the focal array of light spots **114** so that one or more light detecting elements **140(a)** corresponds to a light spot.

[0038] The light detecting elements **140(a)** can detect any suitable light data. Light data refers to any suitable information related to the light detected by the light detecting elements **140(a)**. Light data may include, for example, information about the properties of the light detected such as the intensity of the light, the wavelength(s) of the light, the frequency or frequencies of the light, the polarization(s) of the light, the phase(s) of the light, the spin angular momentum(s) of the light, and/or other light properties associated with the light detected by the light detecting elements **140(a)**. Light data may also include the location of the light detecting element **140(a)** associated with the light data and the time that the light was detected by the light detecting element **140(a)**. The light data may be data based on a single time, based on multiple times, or on a time varying basis. In some

embodiments such as the microfluidic flow embodiments, the light data may be time varying data.

[0039] The system **10** also includes a host computer **200** communicatively coupled to the light detector **140**. The host computer **200** comprises a processor **210** (e.g., a microprocessor) coupled to a computer readable medium (CRM) **210** and a display **230**. Alternatively, one or more components of the host computer **200** can be part of the HIID **100**.

[0040] The processor **210** receives signals with light data from the light detector **140** associated with the light received by the light detecting elements **140(a)**. The processor **210** executes code stored on the CRM **220** to perform some of the functions of system **10** such as interpreting the light data from the light detector **142**, performing analyses from the light data and/or generating images from the light data.

[0041] The CRM **220** (e.g., memory) stores code for performing some functions of system **10**. The code is executable by the processor **210**. In one embodiment, the CRM **220** comprises: a) code for interpreting the light data received from the light detector **142**, b) code for performing analyses based on the light data, c) code for generating one or more images from the light data, d) code for displaying one or more images, and e) any other code for performing the functions of system **10**.

[0042] The display **230** is communicatively coupled to the processor **210** to receive output data such as image data. Any suitable display may be used. In one embodiment, the display **230** may be part of the HIID **100**. The display **230** may provide output such as images to a user of the HIID **100**.

[0043] Modifications, additions, or omissions may be made to HIID system **10** without departing from the scope of the disclosure. For example, other embodiments of the HIID system **10** may not include a display **230**. In addition, the components of system **10** may be integrated or separated according to particular needs. For example, the processor **210** may be integrated into the light detector **140** so that the light detector **140** performs all the functions of the processor **210** in some embodiments.

[0044] **II. HIID Configurations**

[0045] Several configurations of HIIDs **100** are described below. The first configuration includes an HIID **100** using a microfluidic flow method as a scanning mechanism **130**. The second configuration adds a collection component **170** for collecting

light for detection by the light detector **140**. The third configuration is a reflective design including a beam splitter. The fourth configuration uses a three-dimensional focal array of light spots to sectionally image the object **150** at different depths. Although the illustrated embodiments of these configurations use microfluidic flow, other scanning mechanisms **130** can be used in these configurations.

[0046] A. Configuration 1

[0047] FIG. 2(a) is a schematic drawing of cross sectional view of components of an HIID **100** employing a microfluidic flow method, according to embodiments of the invention. **FIG. 2(b)** is a drawing of a partial top view of components of the HIID **100** shown in **FIG. 2(a)** taken at the focal plane **116**, according to embodiments of the invention. The drawing in **FIG. 2(a)** is a cross-section A-A of the HIID **100** in **FIG. 2(b)** through a focal array of light spots **114**.

[0048] In **FIGS. 2(a)** and **2(b)**, the HIID **100** includes a multi-layered body **131** with a holographic element **120** and an illumination source **110** providing an illumination beam **111** at the holographic element **120**. The multi-layered body **131** also defines or includes a fluid channel **132** having a fluid flow with the object **150** being imaged. The fluid channel **132** has a first surface **134** and a second surface **136** on opposite sides of the fluid channel **132**. The body **131** also includes an optional differentiating element **160** located outside the second surface **136** of the fluid channel **132** and a light detector **140** located outside the differentiating element **160**.

[0049] In the illustrated embodiment, the holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. In the illustrated embodiment, each volume is hour-glass shaped, forming a focal cone **112** converging to a light spot **115** at the focal plane **116** and spreading to a spreading volume **117**. The array of spherical wavefront forms the focal array of light spots **114**. The focal array of light spots **114** includes light spots **115** collectively extending across the fluid channel **132** or across a portion of the fluid channel **132**. An object **150** moving through the fluid channel **132** can alter (e.g., block, reduce intensity, change wavelength, or otherwise modify a light property) the light. The altered light spreads into an altered light volume **118**.

The differentiating element **160** transmits light altered by the object **150**. The light detector **140** receives light and generates time varying light data based on the received light as the object **150** moves through the fluid channel **132**. A processor **210** (shown in **FIG. 1**) can use the time varying light data to generate images or otherwise analyze the object **150**.

[0050] The HIID **100** also includes an x-axis, a y-axis, and a z-axis. The x-axis and a y-axis lie in the plane of the second surface **136** of the fluid channel **132**. The x-axis lies along a longitudinal axis of the fluid channel **132**. The z-axis is orthogonal to the x-axis and the y-axis.

[0051] In the illustrated example, the body **131** is a multi-layered structure. In other embodiments, the body **131** may be a single, monolithic structure. The layers of the body **131** may include any suitable material or combination of materials having any suitable thickness. The layers of the body **131** may also include any suitable devices (e.g., holographic element **120**, light detector **140**). Although **FIGS. 2(a)** and **2(b)** have certain layers, other embodiments of the invention may integrate, omit, or add one or more layers or change the location of one or more layers in the body **131**. For example, the body **131** may also include a collection component **170** (shown in **FIG. 3**) between the fluid channel **132** and the differentiating element **160** or between the differentiating element **160** and the light detector **140** in some embodiments. As another example, the body **131** may also include a layer (e.g., a protective layer) made of opaque, semi-opaque, or transparent material that lies between the second surface **136** of the fluid channel **132** and the layer with the differentiating element **160** or outside the first surface **134**.

[0052] The fluid channel **132** may have any suitable dimensions. For example, the height of the fluid channel **132** can range from 1-20 microns and the width can range from 10-500 microns in some cases. In one embodiment, the fluid channel **132** may be sized based on the size of the objects **150** being imaged by the HIID **100**. For example, the height of the fluid channel may be sized to be about the diameter of the object **150**.

[0053] In microfluidic flow embodiments, the fluid flow in the fluid channel **132** is generally in the direction of the x-axis along a longitudinal axis of the fluid channel **132**. Any suitable technique may be used for providing fluid flow and particulate transport of the objects **100** in the fluid channel **132** of these embodiments. Some convention techniques include pressure drive flow, electrokinetic transport, discrete droplet translocation via electrowetting, or thermocapilarity techniques. Other techniques may include gravity drive

flow, hydrodynamic focusing, dielectrophoresis, and optical tweezing. Any suitable control device(s) may be used to control the flow of fluid and/or movement of the object **150** through the fluid channel **132**. Some examples of suitable control devices include micropumps, direct current (DC) electrokinetic devices, dielectrophoresis electrodes, and/or hydrodynamic focusing channels.

[0054] The illumination source **110** may be a component of the HIID **100** or may be separate from the HIID **100**. The illumination source **110** may be provided by any suitable device(s). Some suitable devices include light-emitting diodes (LED), laser of suitable wavelength, broadband source (e.g., mercury lamp, halogen lamp, etc.) with a suitable filter, etc. Suitable illumination sources are commercially available. The illumination source **110** may be placed in any suitable location to generate the appropriate wavefront at the holographic element **120**. In the illustrated embodiment, the illumination source **110** provides an illumination beam **111** with the same wavelength, same spatial distribution and/or other light properties, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. In exemplary fluorescence and phosphorescence embodiments, the illumination source **110** provides excitation light having a first light property (e.g., first wavelength) matching the excitation wavelength of the fluorophores in an object **150** being imaged. The fluorophores are excited by the excitation light and emit light (emissions) of a second light property (e.g., second wavelength). Some examples of suitable excitation light include fluorescence, 2-photon or higher order fluorescence, Raman, second harmonic or higher order, or other emission mechanism that results in emissions at a different wavelength or other different light property than the excitation light.

[0055] The holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array of converging spherical wavefront to form a focal array of light spots **114** at the focal plane **116**. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. The holographic element **120** can be made of any suitable materials. The holographic element **120** can have any suitable dimensions (e.g., 1 mm x 1 mm, 2 mm x 2 mm, 5 mm x 2 mm, 10 mm x 10 mm, 10 mm x 50 mm, etc.). The holographic element **120** can be made using any holographic recording technique capable of encoding (recording) data about the focal array of light spots. To play back, the holographic element **120** can be illuminated by a beam having the same wavelength, same

spatial distribution, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**.

[0056] In **FIGS. 2(a)** and **2(b)**, the focal array of light spots **114** includes a one-dimensional array of light spots **115** located at an angle, α with respect to the x-axis. The angle, α can be any suitable angle (e.g., 5 degrees, 10 degrees, ...90 degrees, ...170 degrees, etc.). In many cases, the light spots **115** collectively extend diagonally across the fluid channel **132**. In other cases, the light spots **115** may collectively extend in a direction parallel to the y-axis and across the fluid channel **132**. Any suitable number of light spots **115** can be used (e.g., 1, 10, 50, 100, 500, etc.). In some cases, the number of light spots **115** may be determined by the number of light spots **115** needed to collectively extend across a width of the fluid channel **132** where the objects **150** being examined flow. Although **FIGS. 2(a)** and **2(b)** show the HIID **100** having a single one-dimensional focal array of light spots **114**, other embodiments may have a two-dimensional array, a three-dimensional array, or a combination of one, two, and/or three-dimensional arrays.

[0057] Each light spot **115** can be of any suitable size. Some examples of suitable diameters (FWHM) are 0.4 microns, 0.6 microns, 0.8 microns, 1 micron, etc. In one exemplary embodiment, the light spot diameter is 0.6 microns (FWHM). Any suitable spacing (5 microns, 10 microns, 15 microns, etc.) can be used between the light spots **115**. In one exemplary embodiment, a light spot spacing of 20 microns is used.

[0058] In the illustrated example, the scanning mechanism **130** employs a microfluidic flow method. The scanning mechanism **130** includes the fluid channel **132** defined by the body **131** and the fluid carrying the object **150** through the fluid channel **132**. Although the illustrated embodiment includes a scanning mechanism **130** employing a microfluidic flow method, other methods (e.g., optical tweezing, scanning method, etc.) can be used in other embodiments. For example, one embodiment may have a scanning mechanism **130** that includes a scanning device (e.g., raster scanner, linear scanner, etc.) for scanning the object **150** or specimen stage with the object **150** through light spots **115** or scanning the light spots **115** across or through the object **150**.

[0059] In the illustrated embodiment, the light detector **140** detects light and generates signals with time varying light data about the properties of the light detected. Some examples of light properties that can be detected include intensity, wavelength, frequency, polarization, phase, spin angular momentum, etc. The light detector can be a single detector,

a one-dimensional detector array, or a two-dimensional detector array. Some examples of single detectors include a photo-diode (PD), an avalanche photo-diode (APD) and a photomultiplier tubes (PMT). Some examples of one-dimensional or two-dimensional detector arrays include a charge coupled device (CCD) array, a complementary metal-oxide-semiconductor (CMOS) array, an APD array, a PD array, a PMT array, etc. The light detector **140** may be a monochromatic or a color detector. For example, the light detector **140** may be a color light detector that generates light data that can be used to generate color images.

[0060] The light detector **140** includes an array of discrete light detecting elements **140(a)** of any suitable size (e.g., 1-10 microns) and any suitable shape (e.g., circular or square). The array of light detecting elements **140(a)** may be a one-dimensional array or a two-dimensional array. The array or arrays can be in any suitable orientation or combination of orientations. In the illustrated example, the array is a two-dimensional array of light detecting elements **140(a)** located at an angle, α with respect to the x-axis. Any suitable angle can be used. In the illustrated example, each light detecting element **140(a)** detects light associated with a single light spot **115**. In other cases, each light detecting element **140(a)** may detect light from more than one light spot **115**. Other embodiments may also have a plurality (e.g., 2 x 2 grid, 4 x 4 grid, etc.) of light detecting elements **140(a)** from the two-dimensional array of light detecting elements **140(a)** that detects light from a single light spot **115**.

[0061] In FIGS. 2(a) and 2(b), the object **150** is shown at a time ($t = t_1$) as the object **150** moves through the fluid channel **132** generally in the x-direction. Although the object **150** is shown as a cell, other embodiments may include other suitable object(s). Some examples of suitable objects include biological and inorganic entities. Some examples of biological entities include whole cells, cell components, microorganisms such as bacteria or viruses, cell components such as proteins, etc. Any suitable number of objects **150** may be imaged and/or analyzed using the HIID **100**.

[0062] The body **131** of the HIID **100** may optionally include a differentiating element **160** located outside the second surface **136**. A differentiating element **160** refers to any suitable device(s) (e.g., optical filters) capable of selectively transmitting light having select light properties (e.g., polarization, wavelength, frequency, intensity, phase, spin angular momentum, etc.) while substantially removing light the remaining light by any

suitable method such as reflection, absorption or interference. Some examples of suitable devices include filters (e.g., interference filters, absorption filters, etc.). Any type of filter can be used such as dichroic filters, monochromatic filters, etc. In one embodiment, a polarization filter may be used. In the illustrated embodiment, the differentiating element **160** includes an interference filter **160(a)** and an absorption filter **160(b)**. The interference filter **160(a)** transmits the altered light and removes remaining light from the illumination source **110** by interference. The absorption filter absorbs remaining light from the illumination source **110**. In fluorescence and phosphorescence applications, the differentiating element **160** may be used to transmit emissions from fluorophores in the object **150** and substantially removes excitation light.

[0063] In an exemplary operation, the illumination source **110** provides an illumination beam **111** at the holographic element **120**. The holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure.

[0064] In the exemplary operation, each volume is hour-glass shaped, forming a focal cone **112** converging to a light spot **115** at the focal plane **116** and spreading to a spreading volume **117**. The array of spherical wavefront forms the focal array of light spots **114**. The focal array of light spots **114** is formed at the focal plane **116** in the fluid channel **132**.

[0065] During operation, a fluid, within which the object **150** is suspended, flows through the fluid channel **132**. As the object **150** flows through the fluid channel **132**, the object **150** alters (blocks, reduces intensity, modifies wavelength or other light property or spatial distribution) the light in the fluid channel **132**. **FIGS. 2(a)** and **2(b)** show the object **150** at a specific time ($t = t_1$) proximal a single light spot **115**. At this time, light altered by the object **150** spreads from the site of the single light spot **115** in the form of an altered light volume **118**. Although the illustration shows altered light only originating from the site of a light spots **115**, altered light may also originate from other areas (e.g., focal cones **112** and spreading cones) in other embodiments.

[0066] The differentiating element **160** transmits the altered light (e.g., reduced intensity, altered wavelength, etc.) to the light detecting elements **140(a)**. Light that does not interact with the object **150** is at least partially removed by the differentiating element **160**.

[0067] In the illustrated embodiment, each light detecting element **140(a)** receives light associated a single corresponding light spot **115** in the focal array **114**. In other embodiments, each light detecting element **140(a)** may receive light associated with other light spots **115**. The light detecting elements **140(a)** receive light and generate time varying light data about the light as the object **150** moves through the fluid channel **132**. The processor **210** receives a signal with time varying light data. The processor **210** uses the time varying light data to generate line scans associated with the y-locations of the light detecting elements **140(a)**. Each line scan is associated with a light spot **115**. The time varying light data from the light detecting elements **140(a)** is dependent on the profile of the object **150** as well as its optical properties. The processor **210** can reconstruct an image of the object **150** by appropriately shifting and assembling the line scans, and optionally other data such as rotation, velocity of the object **150**, and changes in shape of the object **150**, etc.

[0068] The HIID **100** can be used to generate any suitable type of image such as a fluorescence image, phosphorescence image, intensity images, phase image, differential interference contrast (DIC) image, etc. The images can be black and white images, grey tone images, color images, etc.

[0069] In one exemplary embodiment, the HIID **100** can be used in fluorescence or phosphorescence imaging (collectively, photoluminescence imaging). The specimen with one or more objects **150** may be prepared by mixing a reagent with the specimen. The reagent may be suitable chemical for attaching (tagging) portions (e.g., molecules of a cell nucleus) of the objects **150** with fluorophores. A fluorophore refers to a component of a molecule which causes the molecule to be fluorescent or phosphorescent. The resulting fluid is introduced into the fluid channel **132** of the HIID **100**. The illumination source **110** provides an illumination beam **111** of excitation light having a first light property (e.g., first wavelength, first polarization, etc.) that can excite the fluorophores in the object **150**. The holographic element **120** transforms the wavefront of the illumination source **110** of excitation light into an array of converging spherical wavefront, nearly spherical wavefront, or other wavefront having a well separated structure to form a focal array of light spots **114** of excitation light. The fluorophores absorb the excitation light and emit light (emissions)

having a second light property (e.g., a second wavelength, a second polarization, etc.). The emissions spread from site of the light spot **115** in the form of an altered light volume **118**. The differentiating element **160** transmits emissions and substantially removes remaining light. The light detector **140** detects light and generates time varying light data associated with the received light as the object **150** flows through the flow channel **132**. The processor **210** receives a signal from the light detector **140** having time varying data and generates one or more fluorescence or phosphorescence images of the object **150** based on the time varying data.

[0070] In one embodiment, the holographic element **120** can be replaced by one or more diffractive optical elements (DOE) (e.g., a Fresnel zone plate (FZP), diffraction grating, photon sieve, etc.) at the same location illuminated by the illumination beam **111**. The DOE diffracts the illumination beam **111** to generate the focal cones **112** and focal array of light spots **114**. The DOE can be made of any suitable material and may have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2 mm, ..., 10mm x 10 mm). Using DOEs may be advantageous because they have a high shelf life. DOEs are also suitable for nanofabrication and semiconductor fabrication technique.

[0071] **B. Configuration 2 - HIID 100 with Collection Component**

[0072] In some embodiments, the HIID **100** includes a collection component **170** for collecting light for detection by the light detector **140**. **FIG. 3** is a schematic drawing of components of an HIID **100** having a collection component **170**, according to embodiments of the invention. The drawing in **FIG. 3** is a cross sectional view of components HIID **100** at a line through a focal array of light spots **114**. In **FIG. 3**, an illumination source **110** provides an illumination beam **111** to a holographic element **120**.

[0073] In **FIG. 3**, the HIID **100** has a multi-layered body **131** including the holographic element **120**. The multi-layered body **131** also defines or includes a fluid channel **132** having a fluid flow with an object **150** being imaged. The fluid channel **132** has a first surface **134** and a second surface **136** on opposite sides of the fluid channel **132**. The body **131** also includes a collection component **170** outside the second surface **136** of the fluid channel **132**, an optional differentiating element **160** located outside the collection component **170**, and a light detector **140** located outside the differentiating element **160**.

[0074] In the illustrated embodiment, the holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array

of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. In the illustrated embodiment, each volume is hour-glass shaped, forming a focal cone **112** converging to a light spot **115** at the focal plane **116** and spreading to a spreading volume **117**. The array of spherical wavefront forms the focal array of light spots **114**. The focal array **114** includes light spots **115** that collectively extend across the fluid channel **132** or across a portion of the fluid channel **132**. An object **150** moving through the fluid channel **132** can alter (e.g., block, reduce intensity, change wavelength, or otherwise modify a light property) light. The altered light spreads in an altered light volume **118**. The collecting component **170** refocuses light transmitted through the second surface **136** into an array of collections spots **119** at an outside surface of the collection component **170**. The differentiating element **160** transmits light altered by the object **150**. The light detector **140** receives light and generates time varying light data based on the received light as the object **150** moves through the fluid channel **132**. A processor **210** (shown in FIG. 1) can use the time varying light data to generate images or otherwise analyze the object **150**. Using a collection component **170** can be advantageous in improving the quality of the light data collected at the light detector **140** which can improve the quality of the images and other analyses performed by the HIID **100**. In fluorescence and phosphorescence applications, a collection component **170** can be advantageous to collect emissions that may be highly scattered and weak.

[0075] The HIID **100** also includes an x-axis and a z-axis. The x-axis lies along a longitudinal axis of the fluid channel **132**. The z-axis is orthogonal to the x-axis.

[0076] In the illustrated embodiment, the body **131** is a multi-layer structure. The layers of the body **131** may include any suitable material or combination of materials having any suitable thickness. The layers of the body **131** may also include any suitable devices (e.g., holographic element **120**, light detector **140**). Other embodiments may integrate, omit, or add one or more layers or change the location of one or more layers in the body **131**. For example, the collection component **170** may be omitted in some embodiments. As another example, the body **131** may also include a protective layer made of opaque, semi-opaque, or transparent material that lies between the second surface **136** of the fluid channel **132** and the layer with the differentiating element **160** or outside the first surface **134**.

[0077] The fluid channel **132** may have any suitable dimensions. For example, the height of the fluid channel **132** can range from 1-20 microns and the width can range from 10-500 microns in some cases. In one embodiment, the fluid channel **132** may be sized based on the size of the objects **150** being imaged by the HIID **100**. For example, the height of the fluid channel may be sized to be about the diameter of the object **150**. The fluid flow in the fluid channel **132** is generally in the direction of the x-axis along a longitudinal axis of the fluid channel **132**. Any suitable technique (e.g., pressure drive flow, electrokinetic transport, discrete droplet translocation via electrowetting, thermocapilarity techniques, gravity drive flow, hydrodynamic focusing, dielectrophoresis, optical tweezing, etc.) may be used for providing fluid flow and particulate transport of the objects **100** in the fluid channel **132**. Any suitable control device(s) (e.g., micropumps, direct current (DC) electrokinetic devices, dielectrophoresis electrodes, hydrodynamic focusing channels, etc.) may be used to control the flow of fluid and/or movement of the object **150** through the fluid channel **132**.

[0078] The illumination source **110** may be a component of the HIID **100** or may be separate from the HIID **100**. The illumination source **110** may be provided by any suitable device(s). Some suitable devices include light-emitting diodes (LED), laser of suitable wavelength, broadband source (e.g., mercury lamp, halogen lamp, etc.) with a suitable filter, etc. Suitable illumination sources are commercially available. The illumination source **110** may be placed in any suitable location to generate the appropriate wavefront at the holographic element **120**. In the illustrated embodiment, the illumination source **110** provides an illumination beam **111** with the same wavelength, same spatial distribution and/or other light properties, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. In exemplary fluorescence and phosphorescence embodiments, the illumination source **110** provides excitation light having a first light property (e.g., first wavelength) matching the excitation wavelength of the fluorophores in an object **150** being imaged. The fluorophores are excited by the excitation light and emit light (emissions) of a second light property (e.g., second wavelength). Some examples of suitable excitation light include fluorescence, 2-photon or higher order fluorescence, Raman, second harmonic or higher order, or other emission mechanism that results in emissions at a different wavelength or other different light property than the excitation light.

[0079] In the illustrated embodiment, the holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** to an array of converging spherical wavefront to form a focal array of light spots **114** at the focal plane

116. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. The holographic element **120** can be made of any suitable materials and have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2mm, ..., 10 mm x 10 mm, etc.). The holographic element **120** can be made using any holographic recording technique capable of encoding (recording) data about the focal array of light spots. To play back, the holographic element **120** can be illuminated by a beam having the same wavelength, same spatial distribution, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**.

[0080] In **FIG. 3**, the focal array of light spots **114** includes a one-dimensional array of light spots **115** located at an angle, α (shown in **FIG. 2(b)**) with respect to the x-axis. The angle, α can be any suitable angle (e.g., 5 degrees, 10 degrees, ...90 degrees, ...170 degrees, etc.). Any suitable number of light spots **115** can be used (e.g., 1, 10, 50, 100, 500, etc.). Although **FIG. 3** has a single one-dimensional focal array of light spots **114**, other embodiments may have a two-dimensional array, a three-dimensional array, or a combination of one, two, and/or three-dimensional arrays.

[0081] Each light spot **115** can be of any suitable size. Some examples of suitable diameters (FWHM) are 0.4 microns, 0.6 microns, 0.8 microns, 1 micron, etc. In one exemplary embodiment, the light spot diameter is 0.6 microns (FWHM). Any suitable spacing (5 microns, 10 microns, 15 microns, etc.) can be used between the light spots **115**. In one exemplary embodiment, a light spot spacing of 20 microns is used.

[0082] In the illustrated example, the scanning mechanism **130** employs a microfluidic flow method. The scanning mechanism **130** includes the fluid channel **132** defined by the body **131** and the fluid carrying the object **150** through the fluid channel **132**. Although the illustrated embodiment includes a scanning mechanism **130** employing a microfluidic flow method, other methods (e.g., optical tweezing, scanning method, etc.) can be used in other embodiments. For example, one embodiment may have a scanning mechanism **130** that includes a scanning device (e.g., raster scanner, linear scanner, etc.) for scanning the object **150** or specimen stage with the object **150** through light spots **115** or scanning the light spots **115** across or through the object **150**.

[0083] In the illustrated embodiment, the light detector **140** detects light and generates signals with time varying light data about the properties of the light detected. Some

examples of light properties that can be detected include intensity, wavelength, frequency, polarization, phase, spin angular momentum, etc. The light detector **140** can be a single detector, a one-dimensional detector array, or a two-dimensional detector array of light detecting elements **140(a)**. Some examples of single detectors include a photo-diode (PD), an avalanche photo-diode (APD) and a photomultiplier tubes (PMT). Some examples of one-dimensional or two-dimensional detector arrays include a charge coupled device (CCD) array, a complementary metal-oxide-semiconductor (CMOS) array, an APD array, a PD array, a PMT array, etc. The light detector **140** may be a monochromatic or a color detector. For example, the light detector **140** may be a color light detector that generates light data that can be used to generate color images.

[0084] The light detector **140** includes an array of discrete light detecting elements **140(a)** of any suitable size (e.g., 1-10 microns) and any suitable shape (e.g., circular or square). The array of light detecting elements **140(a)** may be a one-dimensional array or a two-dimensional array. The array or arrays can be in any suitable orientation or combination of orientations. In the illustrated example, the array is a two-dimensional array of light detecting elements **140(a)** located at an angle, α with respect to the x-axis. Any suitable angle can be used. In the illustrated example, each light detecting element **140(a)** detects light associated with a single light spot **115**. In other cases, each light detecting element **140(a)** may detect light from more than one light spot **115**. Other embodiments may also have a plurality (e.g., 2 x 2 grid, 4 x 4 grid, etc.) of light detecting elements **140(a)** from the two-dimensional array of light detecting elements **140(a)** that detects light from a single light spot **115**.

[0085] In FIG. 3, the object **150** is shown at a time ($t = t_1$) as the object **150** moves through the fluid channel **132** generally in the x-direction. Although the object **150** is shown as a cell, other embodiments may include other suitable object(s) (e.g. biological and inorganic entities). Any suitable number of objects **150** may be imaged and/or analyzed using the HIID **100**.

[0086] The body **131** of the HIID **100** may optionally include a differentiating element **160** located outside the second surface **136**. The differentiating element **160** selectively transmits altered light while substantially removing the remaining light. The differentiating element **160** includes an interference filter **160(a)** and an absorption filter **160(b)**. The interference filter **160(a)** transmits the altered light and removes remaining light

from the illumination source **110** by interference. The absorption filter absorbs remaining light from the illumination source **110**. In fluorescence and phosphorescence applications, a differentiating element **160** may be used to transmit emissions from fluorophores in the object **150** and substantially remove excitation light.

[0087] The collection component **170** refers to a device(s) capable of refocusing light passing through the second surface **136** and associated with each light spot **115** to one or more light detecting elements **140(a)**. By refocusing the altered light, the detection efficiency may be increased. The collection component **170** can include any suitable device or combination of suitable devices. Some examples of suitable devices include a refractive lens or other diffractive elements (e.g., Fresnel zone plate).

[0088] The collection component **170** can refocus light into any suitable light distribution at any suitable plane(s). In some embodiments, the light distribution may be a tightly confined collection spot **119**. In other embodiments, the light distribution may be a wider distribution that can be detected by one or more light detecting elements **140(a)**. The collection component **170** may be in any suitable location. For example, the collection component **170** may be located between the differentiating element **160** and the light detector **140** of the HIID **100** shown in **FIG. 2(a)**. As another example, the collection component **170** can be located between the second surface **136** of the fluid channel **132** and the differentiating element **160** as shown in **FIG. 3**.

[0089] In **FIG. 3**, the collection component **170** refocuses light associated with each light spot **115** into an array of collection spots **119** at the outside surface of the collection component **170**. Light transmitted through the second surface **136** continues spreading until the mid portion of the collection component **170**. At the mid portion, the light no longer spreads and focuses to an array of collection spots **119** on the outer surface of the collection component **170**. Any suitable device or devices (e.g., refractive lenses) may be used to provide for this collection.

[0090] **FIG. 4** is a schematic drawing of components of an HIID **100** having a collection component **170** including a DOE (e.g., Fresnel zone plate, diffraction grating, photon sieve, etc.) **172** and a beam block **174**, according to embodiments of the invention. The drawing is a cross sectional view through a portion of the HIID **100** having a light spot **115** of the focal array of light spots **114**. The diffractive element **172** refers to a device capable of modifying light passing through the second surface **136** into collection spots

119(a) and **119(b)**. A beam block **174** can refer to a suitable device capable of blocking all light. In an exemplary fluorescence or phosphorescence operation, a beam block **174** can be designed to remove the unscattered excitation light.

[0091] In **FIG. 4**, the HIID **100** includes a multi-layered body **131** and an illumination source **110** providing an illumination beam **111**. The body **131** includes a holographic element **120** and defines or includes a fluid channel **132** having a fluid flow with an object **150** being imaged. The fluid channel **132** has a first surface **134** and an opposing second surface **136**. The body **131** also includes the collection component **170** having a DOE **172** and beam block **174**, an optional differentiating element **160**, a light detector **140**, an x-axis, and a z-axis. By using a beam block **174**, the differentiating element **160** in the HIID **100** can be less powerful and potentially smaller so that the HIID **100** having a beam block **174** can be more compact. In these embodiments, the addition of a collection component **170** with a beam block **174** can allow for a more compact HIID **100** and a more compact system **10**.

[0092] In **FIG. 4**, the collection component **170** refocuses the light passing through the second surface **136**. The DOE **172** or holographic elements or a refractive lens focuses the unscattered light (e.g., excitation light) passing through the second surface **136** from the spreading volume **117** to a plane where the beam block **174** is located. The beam block **174** blocks the light focused at the beam block **174**. The DOE **172** focuses the light altered by the object **150** (e.g., emissions) that pass through the second surface **136** from altered light volume **118** into a second collection spot **119(b)** at the detector plane at the outer surface of the collection component **170**.

[0093] In an exemplary operation of an HIID **100** with a collection component **170**, the illumination source **110** provides the illumination beam **111**. The holographic element **120** transforms the wavefront, planar or otherwise, of the illumination source **110** into an array of spherical wavefront, nearly spherical wavefront, or other wavefront having a well separated structure to form a focal array of light spots **114** at the focal plane **116** in the fluid channel **132**. The light spreads in the form of spreading volumes **117**.

[0094] As fluid flows through the fluid channel **132**, the object **150** alters light in the fluid channel **132**. **FIG. 3** shows the object **150** at a specific time ($t = t_1$). The altered light spreads from each site of the light spot **115** in the form of an altered light volume **118**. Although the illustration shows altered light only originating from the site of the light spots

115, altered light may also originate from other areas (e.g., focal cones **112**) in other embodiments. The collection component **170** refocuses light passing through the second surface **136** into an array of collection spots **119**. In some cases, the collection component may have devices such as a beam block **174** that block light that did not interact with the object **150**. The differentiating element **160** removes any light that did not interact with the object **150** and that transmits through the outer surface of the collection component **170**. The differentiating element **160** transmits light altered by the object **150** to the light detecting elements **140(a)**.

[0095] In this exemplary operation, each light detecting element **140(a)** receives light associated with a single corresponding light spot **115** in the focal array **114**. In other embodiments, each light detecting element **140(a)** may receive light associated with other light spots **115**. The light detecting elements **140(a)** receive light and generate time varying light data about the light as the object **150** moves through the fluid channel **132**. The processor **210** receives a signal with time varying light data and uses the time varying light data to generate line scans associated with the y-locations of the light detecting elements **140(a)**. Each line scan is associated with a light spot **115**. The time varying light data from the light detecting elements **140(a)** is dependent on the profile of the object **150** as well as its optical properties. The processor **210** can reconstruct an image of the object **150** by appropriately shifting and assembling the line scans, and optionally other data such as rotation, velocity of the object **150**, and changes in shape of the object **150**, etc.

[0096] The HIID **100** including a collection component **170** can be used to generate any suitable type of image such as a fluorescence image, phosphorescence image, intensity images, phase image, differential interference contrast (DIC) image, etc. For example, the HIID **100** with a collection component **170** can be used in fluorescence or phosphorescence imaging. In this example, the illumination source **110** provides an illumination beam **111** of excitation light having a first light property that can excite fluorophores in the object **150**. In the illustrated embodiment, the holographic element **120** transforms the planar wavefront of the illumination beam **111** of excitation light into an array of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. In the illustrated embodiment, the spherical wavefront are in the form of focal cones **112** converging to a focal array of light spots **114** of excitation light. The fluorophores absorb the excitation light and emit light

(emissions) having a second light property. The emissions spread from site of the light spot **115** in the form of an altered light volume **118**. The collection component **170** refocuses light passing through the second surface **136** into an array of collection spots **119**. The differentiating element **160** transmits emissions and substantially removes remaining light. The light detector **140** detects light and generates time varying light data associated with the received light as the object **150** flows through the flow channel **132**. The processor **210** receives a signal from the light detector **140** having time varying data and generates one or more fluorescence or phosphorescence images of the object **150** based on the time varying data.

[0097] In one embodiment, the holographic element **120** can be replaced by one or more diffractive optical elements (DOE) (e.g., a Fresnel zone plate (FZP), diffraction grating, photon sieve, etc.) at the same location illuminated by the illumination beam **111**. The DOE diffracts the illumination beam **111** to generate the focal cones **112** and focal array of light spots **114**. The DOE can be made of any suitable material and may have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2 mm, ..., 10mm x 10 mm). Using DOEs may be advantageous because they have a high shelf life. DOEs are also suitable for nanofabrication and semiconductor fabrication technique.

[0098] **C. Configuration 3 - Reflective Design with Beam Splitter**

[0099] In some embodiments, the HIID **100** has a reflective design configuration with a beam splitter **190**. A beam splitter **190** refers to an optical device capable of splitting a single beam of light of a particular type into two or more beams of light of different types (e.g., different wavelengths, different polarizations, etc.). In a fluorescence or phosphorescence application, the beam splitter **190** can be designed to reflect excitation light and transmit emitted light (emissions) from fluorophores. The beam splitter **190** can be in any suitable form (e.g., cube, half-silvered mirror, etc.).

[0100] **FIG. 5** is a schematic drawing of components of a reflective design configuration of an HIID **100** having a beam splitter **190** in the form of a cube, according to embodiments of the invention. The drawing in **FIG. 5** is a cross sectional view of the HIID **100** at a line through the focal array of light spots **114**.

[0101] In **FIG. 5**, the HIID **100** includes a multi-layered body **131** defining or including a fluid channel **132** having a fluid flow carrying an object **150** being imaged or otherwise analyzed. The fluid channel **132** has a first surface **134** and a second surface **136**

on opposite sides of the fluid channel **132**. The HIID **100** also includes an x-axis along a longitudinal axis of the fluid channel **132** and a z-axis orthogonal to the x-axis.

[0102] The HIID **100** also includes a beam splitter **190** coupled at a first outer surface to the fluid channel **132**, a holographic element **120** coupled to a second outer surface of the beam splitter **190**, an illumination source **110** providing an illumination beam **111** to the holographic element **120**, and an optional differentiating element **160** outside a third outer surface of the beam splitter **190**. The first and third surfaces are opposing surfaces of the cube of the beam splitter **190**. The beam splitter **190** splits light at a splitting plane **192** located at a 45 degree angle with respect to the x-axis of the fluid channel **132**. In the illustrated embodiment, the beam splitter **190** reflects light with properties of the illumination beam **111** and transmits light having other properties. The HIID **100** also includes a collection component **170** coupled to the outside of the differential element **160** and a light detector **140** coupled to the outside of the collection component **170**.

[0103] In an exemplary operation, the holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. In the exemplary operation, each volume is hour-glass shaped, forming a focal cone **112** converging to a light spot **115** at the focal plane **116** and spreading to a spreading volume **117**. The array of spherical wavefront forms the focal array of light spots **114**. Light from the illumination beam **111** is reflected at the splitting plane **192** of the beam splitter **190** and transmitted through the second surface **136** of the fluid channel **132** to form the focal array of light spots **114** in the fluid channel **132**. A fluid with the suspended object **150** flows through the fluid channel **132**. As the object **150** moves across the focal array **114**, the object **150** alters light from each light spot **115**. The altered light (e.g., fluorescent emissions) from the site of the light spot **115** is transmitted through the splitting plane **192** of the beam splitter **190**. The altered light is in the form of an altered light volume **118**. The differentiating element **160** transmits the altered light and the collection component **170** refocuses light into a collection spot **119** at light detector **140**.

[0104] In the illustrated embodiment, the body **131** is a multi-layer structure having layers of suitable material or combination of materials having any suitable thickness. The

layers of the body **131** may also include suitable devices. In the illustrated embodiment, the body **131** defines or includes a fluid channel **132** having any suitable dimensions. The body **131** also includes the beam splitter **190**, the differentiating element **160**, the collection component **170**, and the light detector **140**. Other embodiments may integrate, omit, or add one or more layers or change the location of one or more layers in the body **131**. For example, the body **131** may also include a layer made of opaque, semi-opaque, or transparent material that lies between the second surface **136** of the fluid channel **132** and the layer with the differentiating element **160** or outside the first surface **134**.

[0105] The fluid channel **132** may have any suitable dimensions. For example, the height of the fluid channel **132** can range from 1-20 microns and the width can range from 10-500 microns in some cases. In one embodiment, the fluid channel **132** may be sized based on the size of the objects **150** being imaged by the HIID **100**. For example, the height of the fluid channel may be sized to be about the diameter of the object **150**. The fluid flow in the fluid channel **132** is generally in the direction of the x-axis along a longitudinal axis of the fluid channel **132**. Any suitable technique (e.g., pressure drive flow, electrokinetic transport, discrete droplet translocation via electrowetting, thermocapilarity techniques, gravity drive flow, hydrodynamic focusing, dielectrophoresis, optical tweezing, etc.) may be used for providing fluid flow and particulate transport of the objects **100** in the fluid channel **132**. Any suitable control device(s) (e.g., micropumps, direct current (DC) electrokinetic devices, dielectrophoresis electrodes, hydrodynamic focusing channels, etc.) may be used to control the flow of fluid and/or movement of the object **150** through the fluid channel **132**.

[0106] The illumination source **110** may be a component of the HIID **100** or may be separate from the HIID **100**. The illumination source **110** may be provided by any suitable device(s). The illumination source **110** may be placed in any suitable location to generate the appropriate wavefront at the holographic element **120**. In the illustrated embodiment, the illumination source **110** provides an illumination beam **111** with the same wavelength, same spatial distribution and/or other light properties, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. In exemplary fluorescence and phosphorescence embodiments, the illumination source **110** provides suitable excitation light having a first light property (e.g., first wavelength) matching the excitation wavelength of the fluorophores in an object **150** being imaged. The fluorophores are excited by the excitation light and emit light (emissions) of a second light property (e.g., second wavelength).

[0107] In the illustrated embodiment, the holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into an array of converging spherical wavefront to form a focal array of light spots **114** at the focal plane **116**. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. The holographic element **120** can be made of any suitable materials and have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2mm, ..., 10 mm x 10 mm, etc.). The holographic element **120** can be made using any holographic recording technique capable of encoding (recording) data about the focal array of light spots. To play back, the holographic element **120** is illuminated by an illumination beam **111** having the same wavelength, same spatial distribution, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**.

[0108] In FIG. 5, the focal array of light spots **114** includes a one-dimensional array of light spots **115** located at an angle, α (shown in FIG. 2(b)) with respect to the x-axis. The angle, α can be any suitable angle (e.g., 5 degrees, 10 degrees, 45, degrees, ..., 170 degrees, etc.). Any suitable number of light spots **115** can be used (e.g., 1, 10, 50, 100, 500, etc.). Each light spot **115** can be of any suitable size. Some examples of suitable diameters (FWHM) are 0.4 microns, 0.6 microns, 0.8 microns, 1 micron, etc. In one exemplary embodiment, the light spot diameter is 0.6 microns (FWHM). Any suitable spacing (5 microns, 10 microns, 15 microns, etc.) can be used between the light spots **115**. In one exemplary embodiment, a light spot spacing of 20 microns is used.

[0109] In the illustrated example, the scanning mechanism **130** employs a microfluidic flow method. The scanning mechanism **130** includes the fluid channel **132** defined by the body **131** and the fluid carrying the object **150** through the fluid channel **132**. Although the illustrated embodiment includes a scanning mechanism **130** employing a microfluidic flow method, other methods (e.g., optical tweezing, scanning method, etc.) can be used in other embodiments. For example, one embodiment may have a scanning mechanism **130** that includes a scanning device (e.g., raster scanner, linear scanner, etc.) for scanning the object **150** or specimen stage with the object **150** through light spots **115** or scanning the light spots **115** across or through the object **150**.

[0110] The light detector **140** detects light and generates signals with time varying light data about the light properties (e.g., intensity, wavelength, frequency, polarization, phase, spin angular momentum, etc.) of the light detected. The light detector **140** can be a single detector, a one-dimensional detector array, or a two-dimensional detector array of light detecting elements **140(a)** (shown in **FIG. 2(a)**). Some examples of single detectors include a photo-diode (PD), an avalanche photo-diode (APD) and a photomultiplier tubes (PMT). Some examples of one-dimensional or two-dimensional detector arrays include a charge coupled device (CCD) array, a complementary metal-oxide-semiconductor (CMOS) array, an APD array, a PD array, a PMT array, etc. In some cases, each light detecting element **140(a)** detects light associated with a single light spot **115**. In other cases, each light detecting element **140(a)** may detect light from more than one light spot **115**. In some cases, a plurality (e.g., 2 x 2 grid, 4 x 4 grid, etc.) of light detecting elements **140(a)** from the two-dimensional array of light detecting elements **140(a)** detects light from a single light spot **115**. The light detector **140** may be a monochromatic or a color detector. For example, the light detector **140** may be a color light detector that generates light data that can be used to generate color images.

[0111] In **FIG. 4**, the object **150** is shown at a time ($t = t_1$) as the object **150** moves through the fluid channel **132** generally in the x-direction. Although the object **150** is shown as a cell, other embodiments may include other suitable object(s) (e.g. biological and inorganic entities). Any suitable number of objects **150** may be imaged and/or analyzed using the HIID **100**.

[0112] The body **131** of the HIID **100** may optionally include a differentiating element **160** outside a third outer surface of the beam splitter **190**. The differentiating element **160** selectively transmits light altered by the object **150** while substantially removing other remaining light. In fluorescence and phosphorescence applications, a differentiating element **160** may be used to transmit emissions from fluorophores in the object **150** and substantially remove excitation light.

[0113] The collection component **170** refers to a device(s) capable of refocusing light associated with each light spot **115** that is transmitted through the differentiating element **160**, into a collection spot **119** at one or more light detecting elements **140(a)** of the light detector **140**. The collection component **170** can include any suitable device or combination of suitable devices (e.g., refractive lens or other diffractive elements). The collection

component **170** can refocus light into any suitable light distribution at any suitable plane(s). In the illustrated example, the light distribution is a tightly confined collection spot **119**. In other embodiments, the light distribution may be a wider distribution that can be detected by a single light detecting element **140(a)** or by a grid of corresponding light detecting elements **140(a)**.

[0114] The beam splitter **190** splits a light beam of a particular type into two or more beams of light of different types (e.g., different wavelengths, different polarizations, etc.). In a fluorescence or phosphorescence application, the beam splitter **190** can be designed to reflect excitation light and transmit emissions. The beam splitter **190** can be of any suitable design form (e.g., cube, half-silvered mirror, dichroic mirrored prism, etc.) including any suitable device(s). In **FIG. 4**, the beam splitter **190** is a cube including two triangular portions. The beam splitter **190** includes a splitting plane **192** at the interface between two triangular portions. In some cases, the splitting plane **192** within the beam splitter **190** may be coated with a dichroic layer which reflects the light of the same type as the illumination beam (e.g., excitation light) and transmit light of other types (e.g., fluorescent emissions).

[0115] In one embodiment, the beam splitter **190** can be a polarized beam splitter. In this embodiment, the illumination beam **111** can be excitation light that is linearly polarized and can be reflected by the polarized beam splitter to form the focal array **114**. In this example, about 50% of the emission may pass through the polarized beam splitter.

[0116] In an exemplary operation, the illumination source **120** provides an illumination beam **111**. The holographic element **120** transforms the planar wavefront of the illumination beam **111** into an array of spherical wavefront to form a focal array of light spots **114**. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. In the exemplary operation, the light is reflected at the splitting plane **192** located at a 45 degree angle with respect to the x-axis of the fluid channel **132** so that the light spots **115** are formed in the fluid channel **132**. As the object **150** moves through the fluid channel **132**, the object **150** alters light from each light spot **115**. The altered light (e.g., fluorescent emissions) from each light spot **115** is transmitted through the splitting plane **192** of the beam splitter **190**. **FIG. 5** shows a single object **150** at a specific time ($t = t_1$) altering light at a single light spot **115**. At this time, light altered by the object **150** spreads from the site of the light spot **115** in the form of an altered

light volume **118**. The differentiating element **160** transmits the altered light and removes other light. At this time, the collection component **170** refocuses light altered by the object **150** at a single collection spot **119** at light detector **140**. The light detecting elements **140(a)** receive light and generate time varying light data about the light as the object **150** moves through the fluid channel **132**. The processor **210** receives a signal with time varying light data and uses the time varying light data to generate line scans associated with the y-locations of the light detecting elements **140(a)**. Each line scan is associated with a light spot **115**. The time varying light data from the light detecting elements **140(a)** is dependent on the profile of the object **150** as well as its optical properties. The processor **210** can reconstruct an image of the object **150** by appropriately shifting and assembling the line scans, and optionally other data such as rotation, velocity of the object **150**, and changes in shape of the object **150**, etc.

[0117] The HIID **100** can be used to generate any suitable type of image such as a fluorescence image, phosphorescence image, intensity images, phase image, differential interference contrast (DIC) image, etc. In a fluorescence or phosphorescence imaging example, the HIID **100** provides an illumination beam **111** of excitation light having a first light property that can excite fluorophores in the object **150**. The holographic element **120** transforms the wavefront of the illumination source **120** of excitation light into an array of spherical wavefront, approximately spherical wavefront or other wavefront having a well separated structure to form a focal array of light spots **114** of excitation light. The excitation light is reflected by the splitting plane **192** to form the focal array of light spots **114** in the fluid channel **132**. The fluid channel **132** has a fluid flow with the object **150** being imaged. The fluorophores absorb excitation light and emit light (emissions) having a second light property different from the first light property. At a specific time ($t = t_1$), an object **150** alters the light from a single light spots **115** as illustrated in **FIG. 5**. The emissions spread from site of the light spot **115** in the form of an altered light volume **118**. In some cases, emissions also spread from the site of the focal cones **112**. The splitting plane **192** transmits the emissions and the collection component **170** refocuses the emissions into a collection spot **119** associated with a light spot **115**. As the object **150** moves through the fluid channel **132**, the light detector **140** detects light and generates time varying light data associated with the received light. The processor **210** receives a signal from the light detector **140** having time varying data and generates one or more fluorescence or phosphorescence images of the object **150** based on the time varying data.

[0118] In one embodiment, the holographic element **120** can be replaced by one or more diffractive optical elements (DOE) (e.g., a Fresnel zone plate (FZP), diffraction grating, photon sieve, etc.) at the same location illuminated by the illumination beam **111**. The DOE diffracts the illumination beam **111** to generate the focal cones **112** and focal array of light spots **114**. The DOE can be made of any suitable material and may have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2 mm, ..., 10mm x 10 mm). Using DOEs may be advantageous because they have a high shelf life. DOEs are also suitable for nanofabrication and semiconductor fabrication technique.

[0119] **E. Configuration 4 – Multiple Focal Arrays**

[0120] The cost and complication of combining multiple HIID **100** illustrated in **FIG. 2(a)** into a single HIID **100** with multiple focal arrays **114** can be relatively minor in many cases. Having multiple focal arrays **114** in a single HIID **100** may provide one or more advantages. HIID **100** with multiple focal arrays **114** multiplexed in parallel can be used in parallel processing to boost throughput. Other HIID **100** can have focal arrays in series to perform more detailed analysis of the same specimen. For example, an HIID **100** with a series of focal arrays each having a differentiating element **160** that passes a different emission light (e.g., light of a different wavelength) can be used to perform multi-spectral fluorescence imaging. As another example, an HIID **100** with a series of focal arrays at different focal planes **116** can be used to generate sectional images and three dimensional images of an object **150** as shown in **FIG. 6**.

[0121] One design approach for combining multiple HIID **100** into a single HIID **100** with multiple focal arrays **114** in series is to employ a long fluid channel **132** through which can flow a specimen with object(s) **150**. The focal arrays **114** can be located separately along the fluid channel **132** to separately image the same specimens. Any suitable spacing between the focal arrays can be used (e.g., 10 microns, 20 microns, etc.).

[0122] **1. Sectional Imaging and Three-dimensional Imaging**

[0123] **FIG. 6** is an illustrated example of an HIID **100** with multiple focal arrays **114** that can be designed by combining multiple HIIDs **100** of **FIG. 2(a)** in series into a single HIID **100** employing a long fluid channel **132**. **FIG. 6** is a schematic drawing of components of an HIID **100** having multiple focal arrays **114** in series at different depths for sectional imaging and/or three-dimensional imaging, according to embodiments of the invention.

[0124] In FIG. 6, the HIID 100 includes a three-dimensional focal array of light spots 600 employing a microfluidic flow for generating sectional images (x-y images of the specimen at different z-values) at different depths through a fluid channel 132 and/or generating three-dimensional images, according to embodiments of the invention. The three-dimensional focal array of light spots 600 is comprised of a plurality of n one-dimensional focal arrays 114(1),...,114(n) (n = 2, 3, 4, 5, etc.) at different focal planes 116(1),...,116(n) at different depths of the fluid channel 132. The plurality of n focal arrays 114(1),...,114(n) are located at n different depths through the fluid channel 132 and at n different x locations along the longitudinal axis of the fluid channel 132. The HIID 100 can be used to take sectional images of an object 150 at different depths associated with the n focal planes 116(1),...,116(n) during a single pass through the fluid channel 132.

[0125] In FIG. 6, the HIID 100 includes a multi-layered body 131 with a holographic element 120 and an illumination source 110 providing an illumination beam 111 at the holographic element 120. The multi-layered body 131 also defines or includes a fluid channel 132 having a fluid flow with the object 150 being imaged. The fluid channel 132 has a first surface 134 and a second surface 136 on opposite sides of the fluid channel 132. The body 131 also includes an optional differentiating element 160 located outside the second surface 136 of the fluid channel 132 and a light detector 140 located outside the differentiating element 160. The differentiating element 160 includes an interference filter 160(a) and an absorption filter 160(b) for removing light having the same light properties as the illumination beam 111.

[0126] In the illustrated embodiment, the holographic element 120 transforms the planar wavefront of the illumination beam 111 from the illumination source 110 into n arrays of converging spherical wavefront. Any suitable number can be used for n (e.g., 1, 5, 10, 100, 200, etc.). In other embodiments, the holographic element 120 may also transform a wavefront, planar or otherwise, from the illumination source 110 into an approximately spherical wavefront or other wavefront having a well separated structure.

[0127] In the illustrated embodiment, each volume is hour-glass shaped, forming a focal cone 112 converging into a light spot 115 and spreading into a spreading volume 117. The n arrays of spherical wavefront form n focal arrays of light spots 114(1),...,114(n) at corresponding focal planes 116(1),...,116(n). Each of the focal arrays 114(1),...,114(n) includes light spots 115 collectively extending across the fluid channel 132 or across a

substantial portion of the fluid channel **132**. Each focal array is located at a different focal plane **116(1),...,116(n)** at different depths through the fluid channel **132**. An object **150** moving through the fluid channel **132** can alter (e.g., block, reduce intensity, change wavelength, or otherwise modify a light property) the light in the fluid channel **132**. The altered light is in the form of altered light volumes **118** (shown in **FIG. 2(a)**). The differentiating element **160** transmits light altered by the object **150**. The light detector **140** receives light and generates time varying light data based on the received light as the object **150** moves through the fluid channel **132**. A processor **210** (shown in **FIG. 1**) can use the time varying light data to generate sectional images of the object(s) **150** at different depths associated with the focal planes **116(1)...116(n)**. Any type of sectional image can be generated such as a fluorescence or phosphorescence image, intensity image, phase image, differential interference contrast (DIC) image, etc.

[0128] The HIID **100** also includes an x-axis, a y-axis, and a z-axis. The x-axis and a y-axis lie in the plane of the second surface **136** of the fluid channel **132**. The x-axis lies along a longitudinal axis of the fluid channel **132**. The z-axis is orthogonal to the x-axis and the y-axis.

[0129] In the illustrated example, the body **131** is a multi-layered structure. In other embodiments, the body **131** may be a single, monolithic structure. The layers of the body **131** may include any suitable material or combination of materials having any suitable thickness. The layers of the body **131** may also include suitable devices (e.g., holographic element **120**, light detector **140**). Although **FIG. 6** has certain layers at certain locations, other embodiments of the invention may integrate, omit, or add one or more layers or change the location of one or more layers in the body **131**. For example, the body **131** may also include a collection component **170** (shown in **FIG. 3**) between the fluid channel **132** and the differentiating element **160** or between the differentiating element **160** and the light detector **140** in some embodiments. As another example, the body **131** may also include a layer (e.g., a protective layer) made of opaque, semi-opaque, or transparent material that lies between the second surface **136** of the fluid channel **132** and the layer with the differentiating element **160** or outside the first surface **134**.

[0130] The fluid channel **132** may have any suitable dimensions. For example, the height of the fluid channel **132** can range from 1-20 microns and the width can range from 10-500 microns in some cases. In one embodiment, the fluid channel **132** may be sized based

on the size of the objects **150** being imaged by the HIID **100**. For example, the height of the fluid channel may be sized to be about the diameter of the object **150**. The fluid flow in the fluid channel **132** is generally in the direction of the x-axis along a longitudinal axis of the fluid channel **132**. Any suitable technique (e.g., pressure drive flow, electrokinetic transport, discrete droplet translocation via electrowetting, thermocapilarity techniques, gravity drive flow, hydrodynamic focusing, dielectrophoresis, optical tweezing, etc.) may be used for providing fluid flow and particulate transport of the objects **100** in the fluid channel **132**. Any suitable control device(s) (e.g., micropumps, direct current (DC) electrokinetic devices, dielectrophoresis electrodes, hydrodynamic focusing channels, etc.) may be used to control the flow of fluid and/or movement of the object **150** through the fluid channel **132**.

[0131] The illumination source **110** may be a component of the HIID **100** or may be separate from the HIID **100**. The illumination source **110** may be provided by any suitable device(s). Some suitable devices include light-emitting diodes (LED), laser of suitable wavelength, broadband source (e.g., mercury lamp, halogen lamp, etc.) with a suitable filter, etc. Suitable illumination sources are commercially available. The illumination source **110** may be placed in any suitable location to generate the appropriate wavefront at the holographic element **120**. In the illustrated embodiment, the illumination source **110** provides an illumination beam **111** with the same wavelength, same spatial distribution and/or other light properties, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**. In exemplary fluorescence and phosphorescence embodiments, the illumination source **110** provides excitation light having a first light property (e.g., first wavelength) matching the excitation wavelength of the fluorophores in an object **150** being imaged. The fluorophores are excited by the excitation light and emit light (emissions) of a second light property (e.g., second wavelength). Some examples of suitable excitation light include fluorescence, 2-photon or higher order fluorescence, Raman, second harmonic or higher order, or other emission mechanism that results in emissions at a different wavelength or other different light property than the excitation light.

[0132] The holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into n arrays of converging spherical wavefront to form n focal arrays of light spots **114(1),...,114(n)** at corresponding focal planes **116(1),...,116(n)** at different depth through the fluid channel **132**. The holographic element **120** can be made of any suitable material(s). The holographic element **120** can have any suitable dimensions (e.g., 1 mm x 1 mm, 2 mm x 2 mm, 5 mm x 2 mm, 10 mm x 10 mm, 10

mm x 50 mm, etc.). The holographic element **120** can be made using any holographic recording technique capable of encoding (recording) data about the focal array of light spots. To play back, the holographic element **120** can be illuminated by a beam having the same wavelength, same spatial distribution, but not necessarily the same intensity, as the reference beam used to record the holographic element **120**.

[0133] In **FIG. 6**, the holographic element forms n one-dimensional focal arrays of light spots **114(1),...,114(n)** at different depths through the fluid channel **132** and at different x locations along the fluid channel **132**. The n one-dimensional focal arrays of light spots **114(1),...,114(n)** form the three-dimensional array of light spots **600**. Any suitable number (e.g., 2, 3, 5, 10, 20, 50, 100, etc.) of one-dimensional focal arrays, n can be used. Each one-dimensional focal array **114(i)** ($i = 1$ to n) is located at an angle, α_i with respect to the x -axis. The angle, α_i may be any suitable angle (e.g., 5 degrees, 10 degrees,...90 degrees, ...170 degrees, etc.). In many cases, all the focal arrays **114(1),...,114(n)** will be located at the same angle, α angle. In some cases, the light spots **115** collectively extend diagonally across the fluid channel **132**. In other cases, the light spots **115** may collectively extend in a direction parallel to the y -axis and across the fluid channel **132**. Although the focal arrays **114** in the illustrated example have three light spots **115**, any suitable number of light spots **115** can be used (e.g., 1, 10, 50, 100, 500, etc.) in other embodiments. In some cases, the number of light spots **115** may be determined by the number of light spots **115** needed to collectively extend across a width of the fluid channel **132** where the object(s) **150** being examined flow.

[0134] Each light spot **115** can be of any suitable size. Some examples of suitable diameters (FWHM) are 0.4 microns, 0.6 microns, 0.8 microns, 1 micron, etc. In one exemplary embodiment, the light spot diameter is 0.6 microns (FWHM). Any suitable spacing (5 microns, 10 microns, 15 microns, etc.) can be used between the light spots **115**. In one exemplary embodiment, a light spot spacing of 20 microns is used.

[0135] In the illustrated example, the scanning mechanism **130** employs a microfluidic flow method. The scanning mechanism **130** includes the fluid channel **132** defined by the body **131** and the fluid carrying the object **150** through the fluid channel **132**. Although the illustrated embodiment includes a scanning mechanism **130** employing a microfluidic flow method, other methods (e.g., optical tweezing, scanning method, etc.) can be used in other embodiments. For example, one embodiment may have a scanning

mechanism **130** that includes a scanning device (e.g., raster scanner, linear scanner, etc.) for scanning the object **150** or specimen stage with the object **150** through light spots **115** or scanning the light spots **115** across or through the object **150**.

[0136] The light detector **140** detects light and generates signals with time varying light data about the light properties of the detected. Some examples of light properties that can be detected include intensity, wavelength, frequency, polarization, phase, spin angular momentum, etc. The light detector **140** can be a single detector, a one-dimensional detector array, or a two-dimensional detector array. Some examples of single detectors include a photo-diode (PD), an avalanche photo-diode (APD) and a photomultiplier tubes (PMT). Some examples of one-dimensional or two-dimensional detector arrays include a charge coupled device (CCD) array, a complementary metal-oxide-semiconductor (CMOS) array, an APD array, a PD array, a PMT array, etc. The light detector **140** may be a monochromatic or a color detector. For example, the light detector **140** may be a color light detector that generates light data that can be used to generate color images.

[0137] The light detector **140** includes a two-dimensional array of discrete light detecting elements **140(a)** (shown in FIG. 2(a)) of any suitable size (e.g., 1-10 microns) and any suitable shape (e.g., circular or square). The array is located at an angle, α with respect to the x-axis. Any suitable angle can be used. Any suitable number of light detecting elements **140(a)** may correspond to a light spot **115**. In FIG. 6, each light detecting element **140(a)** detects light from a single corresponding light spot **115**. In another example, each light detecting element **140(a)** may detect light from more than one light spot **115**. In another example, a plurality (e.g., 2 x 2 grid, 4 x 4 grid, etc.) of light detecting elements **140(a)** may detects light from a single light spot **115**.

[0138] In FIG. 6, the object **150** is shown at a time ($t = t_1$) as the object **150** moves through the fluid channel **132** generally in the x-direction. Although the object **150** is shown as a cell, other embodiments may include other suitable object(s) such as biological entities (e.g., whole cells, cell components, microorganisms such as bacteria or viruses, cell components such as proteins, etc.) and inorganic entities. Any suitable number of objects **150** may be imaged and/or analyzed using the HIID **100**.

[0139] The body **131** of the HIID **100** may optionally include a differentiating element **160** located outside the second surface **136**. The differentiating element **160** selectively transmits altered light while substantially removing the remaining light. The

differentiating element **160** includes an interference filter **160(a)** and an absorption filter **160(b)**. The interference filter **160(a)** transmits the altered light and removes remaining light from the illumination source **110** by interference. The absorption filter absorbs remaining light from the illumination source **110**. In fluorescence and phosphorescence applications, a differentiating element **160** may be used to transmit emissions from fluorophores in the object **150** and substantially remove excitation light.

[0140] In an exemplary operation, the illumination source **110** provides an illumination beam **111**. The holographic element **120** transforms the planar wavefront of the illumination beam **111** from the illumination source **110** into n arrays of converging spherical wavefront. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure.

[0141] In the exemplary operation, each volume is hour-glass shaped, forming a focal cone **112** converging to a light spot **115** at the focal plane **116** and spreading to a spreading volume **117**. The n arrays of converging spherical wavefront forms n focal arrays of light spots **114(1),...,114(n)** at different focal planes **116(1),...,116(n)** at different depths of the fluid channel **132** and at different x locations along the fluid channel **132**. The n focal arrays of light spots **114(1),...,114(n)** form the three-dimensional focal array of light spots **600**.

[0142] During operation, a fluid, within which the object **150** is suspended, flows through the fluid channel **132**. As the object **150** flows through the fluid channel **132**, the object **150** alters (blocks, reduces intensity, modifies wavelength or other light property or spatial distribution) light in the fluid channel **132** as it passes through one or more of the focal arrays **114(1)...114(n)** located at different depths of the fluid channel **132**. The differentiating element **160** transmits the altered light and removes light having the same properties as the illumination beam **111**.

[0143] The light detecting elements **140(a)** (shown in FIG. 2(a)) receive light and generate time varying light data about the light as the object **150** moves through focal arrays at different depths of the fluid channel **132**. The processor **210** receives a signal with time varying light data associated with each of the focal arrays. The processor **210** uses the time varying light data to generate line scans associated with the y -locations of the light detecting elements **140(a)** for each of the focal arrays. The time varying light data is dependent on the profile of the object **150** as well as its optical properties. The processor **210** can reconstruct a

sectional image of the object **150** at a specific depth by appropriately shifting and assembling line scans from time varying data taken by light detecting elements associated with a focal array **114(i)** having a focal plane **116(i)** located at the specific depth. Optionally, other data (e.g., rotation, velocity of the object **150**, and changes in shape of the object **150**, etc.) can also be used to determine the sectional image. The processor **210** can also construct a three-dimensional image of the object **150** based on the sectional images or the time varying data.

[0144] The HIID **100** can be used to generate any suitable type of image such as a fluorescence image, phosphorescence image, intensity images, phase image, differential interference contrast (DIC) image, etc.

[0145] In one exemplary embodiment, the HIID **100** can be used in fluorescence or phosphorescence imaging. The specimen with one or more objects **150** may be prepared by mixing a reagent with the specimen. The resulting fluid is introduced into the fluid channel **132** of the HIID **100**. The illumination source **110** provides an illumination beam **111** of excitation light having a first light property (e.g., first wavelength, first polarization, etc.) that can excite the fluorophores in the object **150**. The holographic element **120** transforms the planar wavefront of the illumination beam **111** of excitation light into n arrays of converging spherical wavefront to form n focal array of light spots **114(1),...,114(n)** of excitation light at n focal planes at different depths through the fluid channel **132** and at different x-locations along the longitudinal axis of the fluid channel **132**. In other embodiments, the holographic element **120** may also transform a wavefront, planar or otherwise, from the illumination source **110** into an approximately spherical wavefront or other wavefront having a well separated structure. As the object moves through the fluid channel **132**, fluorophores in the object **150** absorb excitation light from a proximal light spot **115** at a particular depth. The fluorophores then emit light (emissions) having a second light property (e.g., a second wavelength, a second polarization, etc.). The emissions spread from site of the proximal light spot **115** in the form of an altered light volume **118**. To a lesser extent, the fluorophores may also absorb excitation light from the focal cone **112** and the spreading volume **117**. In this case, the fluorophores from these areas may emit light as well.

[0146] The differentiating element **160** transmits emissions and substantially removes excitation light. The light detector **140** detects light and generates time varying light data associated with the received light as the object **150** flows through the flow channel **132**. The processor **210** receives a signal from the light detector **140** having time varying data. The

processor **220** generates one or more fluorescence or phosphorescence sectional images of the object **150** and/or three-dimensional images of the object **150** based on the time varying data.

[0147] In one embodiment, the holographic element **120** can be replaced by one or more diffractive optical elements (DOE) (e.g., a Fresnel zone plate (FZP), diffraction grating, photon sieve, etc.) at the same location illuminated by the illumination beam **111**. The DOE diffracts the illumination beam **111** to generate the focal cones **112** and focal array of light spots **114**. The DOE can be made of any suitable material and may have any suitable dimensions (e.g., 1 mm x 1mm, 2 mm x 2 mm, ..., 10mm x 10 mm). Using DOEs may be advantageous because they have a high shelf life. DOEs are also suitable for nanofabrication and semiconductor fabrication technique.

[0148] **2. Multi-spectral Fluorescence or Phosphorescence Imaging**

[0149] Another example of an HIID **100** with multiple focal arrays **114** that can be designed by combining multiple HIIDs **100** of **FIG. 2(a)** in series into a single HIID **100** employing a long fluid channel **132** can be used to perform multi-spectral fluorescence or phosphorescence imaging. In one embodiment, an HIID **100** includes multiple focal arrays arranged in a series at different x-locations along the longitudinal axis of the fluid channel **132**. The HIID **100** also includes multiple differentiating elements **160** corresponding to the different focal arrays **114**. Each differentiating element **160** transmits light of a different light property (e.g., wavelength, polarization, etc.). For example, a first differentiating element **160** associated with a first focal array **114** may allow light with a wavelength λ_1 to pass, a second differentiating element **160** associated with a second focal array **114** may allow light with a wavelength λ_2 to pass, a third differentiating element **160** associated with a third focal array **114** may allow light with a wavelength λ_2 to pass, etc. In this example, the HIID **100** can generate fluorescence or phosphorescence images from light of wavelengths, λ_1 , λ_2 , and λ_3 . In some cases, different structures in the object **150** being imaged may emit light have different light properties (e.g., λ_1 , λ_2 , λ_3). In these cases, the HIID **100** may have differentiating elements **160** associated with the different light properties corresponding to the different structures. The HIID **100** can then image the different structures associated with the different light properties.

[0150] **FIG. 7** is a schematic drawing of components of an HIID **100** having multiple focal arrays **114** in series with different differentiating elements **160** for multi-spectral fluorescence or phosphorescence imaging, according to embodiments of the invention. **FIG.**

7 is an another illustrated example of an HIID **100** having multiple focal arrays **114** that can be designed by combining multiple HIIDs **100** of **FIG. 2(a)** in series into a single HIID **100** employing a long fluid channel **132**. In this example, the HIID **100** has five differentiating elements **160(1)-160(5)** corresponding to the five focal arrays **114(1)-114(5)**. Each of the differentiating elements **160(1)-160(5)** transmits light of a different light property. In this way, a single passage of an object **150** through the fluid channel **132** will allow each segment to acquire a spectrally distinct image.

[0151] Embodiments of an HIID **100** including multiple focal arrays in series and corresponding differentiating elements **160** for multi-spectral fluorescence or phosphorescence imaging may have advantages. With conventional microscopes, multi-spectral fluorescence images are typically generated by swapping the chromatic filters between each image acquisition step. As the number of slots in a filter carousel is limited, the acquisition of more than 5 wavelength bands typically requires a carousel swap. With an HIID **100** having a series of focal arrays, the acquisition of multi-spectral images can be implemented automatically by connecting several focal arrays, each sensitive to a particular emission wavelength band, in series. A single passage of an object **150** through the fluid channel **132** generates a complete set of fluorescence or phosphorescence images.

[0152] Modifications, additions, or omissions may be made to any of the configurations of the HIIDs **100** without departing from the scope of the disclosure. In some cases, one or more components of any of the HIIDs **100** may be added to other configurations in other embodiments. For example, the collection component **170** can be added to some configurations. In addition, the components of any of the configurations of the HIID **100** may be integrated or separated according to particular needs. For example, the processor **210** may be integrated into the light detector **140** so that the light detector **140** performs all the functions of the processor **210** in some embodiments.

[0153] III. Fabrication Techniques

[0154] The holographic element **120** can be recorded using any holographic recording technique. One recording method involves interfering a light field **700** through a recording mask having an array of apertures **705** with a collimated reference beam (write beam) **710** via a beam splitter **190**, as shown in **FIG. 8(a)**. A recording mask refers to an array of apertures **705** patterned in a layer of metal film or coating on a substrate such as a glass slide. **FIG. 8(a)** is a schematic drawing of a setup for off-axis recording a holographic element **120**,

according to embodiments of the invention. In the illustrated setup, a beam splitter **190** is used. In this illustration a recording mask is used. In the illustrated example, the apertures may have an aperture size equal to the desired light spot size and the aperture spacing is equal to the desired spacing between light spots in the focal array of light spots. The interference pattern can then be recorded on the holographic element **120**. When the holographic element **120** is illuminated by an illumination beam **111** (shown in **FIG. 2(a)**) propagating in the opposite direction as the original reference write beam, the holographic element **120** will generate an optical conjugate wave that will reconstitute into a focal array of light spots based on the array of apertures **705**.

[0155] Another method is illustrated in **FIG. 8(b)**. **FIG. 8(b)** is a schematic drawing of a setup for inline recording a holographic element **120**, according to embodiments of the invention. In the illustrated embodiment, an incident collimated light beam transmitted through the apertures will interfere with the fairly strong uniform transmission through the metal film/coating (in effect, this serves as the write beam) to create a recordable interference pattern at a short distance away, as shown in **FIG. 8(b)**. The pattern can be recorded by placing the holographic element **120** arbitrarily close to the recording mask **760**. This technique allows recording of holographic elements **120** that can generate holograms with excellent stability since there are no potential drifts between the two interfering components. This method for creating a holographic element **120** for generating light spots is easy and readily scalable for mass-manufacture. Using this method, some embodiments of holographic elements **120** have been recorded to generate light spots **115** with diameters of about 0.60 micron and to have 10% efficiency in channeling of the illumination beam **111**.

[0156] In one embodiment, a silver halide holographic element **120** was recorded using a recording mask **760**. After exposure, the holographic element **120** was developed and bleached to produce a phase hologram. A light spot **115** can then be generated by the holographic reconstruction process, where a conjugated collimated beam **710** is transformed into a light spot **115** by the holographic element **120**. The focal length between the holographic element **120** and the focal plane **116** (shown in **FIG. 2(a)**) is the same as the distance **770** between the recording mask **760** and the holographic element **120** during the recording process.

[0157] The recording mask can be fabricated using any suitable method. In one example, a specialized mask **760** (shown in **FIG. 8(b)**) is made to record a holographic

element **120** of **FIG. 6** with a plurality of n focal arrays **114(1),...,114(n)** at different depths. The recording mask **760** is made by starting with a piece of glass and depositing layers of SU-8 photoresist film or other suitable material layer on the glass in a step fashion. For example, each step can be 2 micron high and 50 micron wide. Any suitable step dimensional can be used in other embodiments. Then, a layer of material (e.g., gold) is deposited, with a suitable thickness (e.g., 200 nm thick), on the structure and mill apertures at the appropriate places with a focused ion-beam machine. The recording mask **760** can then be used to record the holographic element **120**.

[0158] V. Computer devices

[0159] FIG. 9 shows a block diagram of subsystems that may be present in computer devices that are used in system **10**, according to embodiments of the invention. For example, the computer **200** in communication with the HIID **100** may have any suitable combination of components in **FIG. 9**.

[0160] The various components previously described in the Figures may operate using one or more computer devices to facilitate the functions described herein. Any of the elements in the Figures may use any suitable number of subsystems to facilitate the functions described herein. Examples of such subsystems or components are shown in a **FIG. 9**. The subsystems shown in **FIG. 9** are interconnected via a system bus **975**. Additional subsystems such as a printer **974**, keyboard **978**, fixed disk **979** (or other memory comprising computer readable media), display **230**, which is coupled to display adapter **982**, and others are shown. Peripherals and input/output (I/O) devices, which couple to I/O controller **971**, can be connected to the computer system by any number of means known in the art, such as serial port **957**. For example, serial port **977** or external interface **981** can be used to connect the computer apparatus to a wide area network such as the Internet, a mouse input device, or a scanner. The interconnection via system bus allows the central processor **210** to communicate with each subsystem and to control the execution of instructions from system memory **980** or the fixed disk **979**, as well as the exchange of information between subsystems. The system memory **980** and/or the fixed disk **979** may embody a computer readable medium **220**. Any of these elements may be present in the previously described features. A computer readable medium **220** according to an embodiment of the invention may comprise code for performing any of the functions described above.

[0161] In some embodiments, an output device such as the printer 974 or display 230 of the HHD system 10 can output various forms of data. For example, the system 10 can output a fluorescence image of an object 150 or other results of analysis.

[0162] It should be understood that the present invention as described above can be implemented in the form of control logic using computer software in a modular or integrated manner. Based on the disclosure and teachings provided herein, a person of ordinary skill in the art will know and appreciate other ways and/or methods to implement the present invention using hardware and a combination of hardware and software.

[0163] Any of the software components or functions described in this application, may be implemented as software code to be executed by a processor using any suitable computer language such as, for example, Java, C++ or Perl using, for example, conventional or object-oriented techniques. The software code may be stored as a series of instructions, or commands on a computer readable medium, such as a random access memory (RAM), a read only memory (ROM), a magnetic medium such as a hard-drive or a floppy disk, or an optical medium such as a CD-ROM. Any such computer readable medium may reside on or within a single computational apparatus, and may be present on or within different computational apparatuses within a system or network.

[0164] A recitation of “a”, “an” or “the” is intended to mean “one or more” unless specifically indicated to the contrary.

[0165] The above description is illustrative and is not restrictive. Many variations of the disclosure will become apparent to those skilled in the art upon review of the disclosure. The scope of the disclosure should, therefore, be determined not with reference to the above description, but instead should be determined with reference to the pending claims along with their full scope or equivalents.

[0166] One or more features from any embodiment may be combined with one or more features of any other embodiment without departing from the scope of the disclosure. Further, modifications, additions, or omissions may be made to any embodiment without departing from the scope of the disclosure. The components of any embodiment may be integrated or separated according to particular needs without departing from the scope of the disclosure.

[0167] All patents, patent applications, publications, and descriptions mentioned above are hereby incorporated by reference in their entirety for all purposes. None is admitted to be prior art.

WHAT IS CLAIMED IS:

1. A holographically illuminated imaging device, comprising:
a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots;
a scanning mechanism configured to move an object across one or more light spots in the focal array of light spots; and
a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light.
2. The holographically illuminated imaging device of claim 1, further comprising a processor configured to generate an image of the object based on the light data.
3. The holographically illuminated imaging device of claim 1, further comprising:
a differentiating element located between the light detector and the object, and configured to transmit emissions from fluorophores in the object; and
a processor configured to generate a photoluminescent image of the object based on light data.
4. The holographically illuminated imaging device of claim 1, wherein the scanning mechanism comprises a fluid channel having a fluid carrying the object through the fluid channel, the light spots collectively and substantially extending across the fluid channel.
5. The holographically illuminated imaging device of claim 1, wherein the scanning mechanism is a scanning device configured to scan the object relative to the focal array of light spots.
6. The holographically illuminated imaging device of claim 1, further comprising a collection component located between the light detector and the object, and configured to collect light at the light detector.
7. A holographically illuminated imaging device, comprising:

a body defining a fluid channel;
a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots;
a beam splitter configured to reflect the focal array of light spots into the fluid channel wherein a flow in the channel moves an object across one or more light spots in the focal array of light spots, the beam splitter further configured to transmit light altered by the object; and
a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light.

8. A holographically illuminated imaging device, comprising:
a holographic element configured to transform an illumination beam into a plurality of focal arrays of light spots at different focal planes;
a scanning mechanism configured to move an object across one or more light spots in the plurality of focal arrays of light spots; and
a light detector configured to receive light associated with the plurality of focal arrays of light spots, and generate light data associated with the received light.

9. The holographically illuminated imaging device of claim 8, further comprising a processor configured to use the light data to generate one or more sectional images of the object associated with different focal planes.

10. The holographically illuminated imaging device of claim 8, further comprising a processor configured to generate a three-dimensional image of the object based on the light data.

11. The holographically illuminated imaging device of claim 8, further comprising:
a differentiating element located between the light detector and the object, and configured to transmit emissions from fluorophores in the object; and
a processor configured to generate a photoluminescent image of the object based on light data.

12. The holographically illuminated imaging device of claim 8, wherein the scanning mechanism comprises a fluid channel having a fluid carrying the object through the fluid channel, wherein the focal arrays are located along the fluid channel, and wherein the light spots of each focal array collectively and substantially extend across the fluid channel.

13. The holographic illuminated imaging device of claim 8, wherein the scanning mechanism is a scanning device configured to scan the object relative to the plurality of focal arrays of light spots.

14. The holographically illuminated imaging device of claim 8, further comprising a collection component located between the light detector and the object, and configured to collect light at the light detector.

15. A system, comprising:
a holographically illuminated optofluidic imaging device including
a holographic element configured to transform an illumination beam from an illumination source into a focal array of light spots,
a scanning mechanism configured to move an object across one or more light spots in the focal array of light spots, and
a light detector configured to detect light associated with the focal array of light spots, and generate light data associated with the received light; and
a processor in communication with the light detector, the processor configured to receive a signal with light data and generate an image of the object based on the light data.

16. The system of claim 15, further comprising a display for displaying the image generated by the processor.

1/9

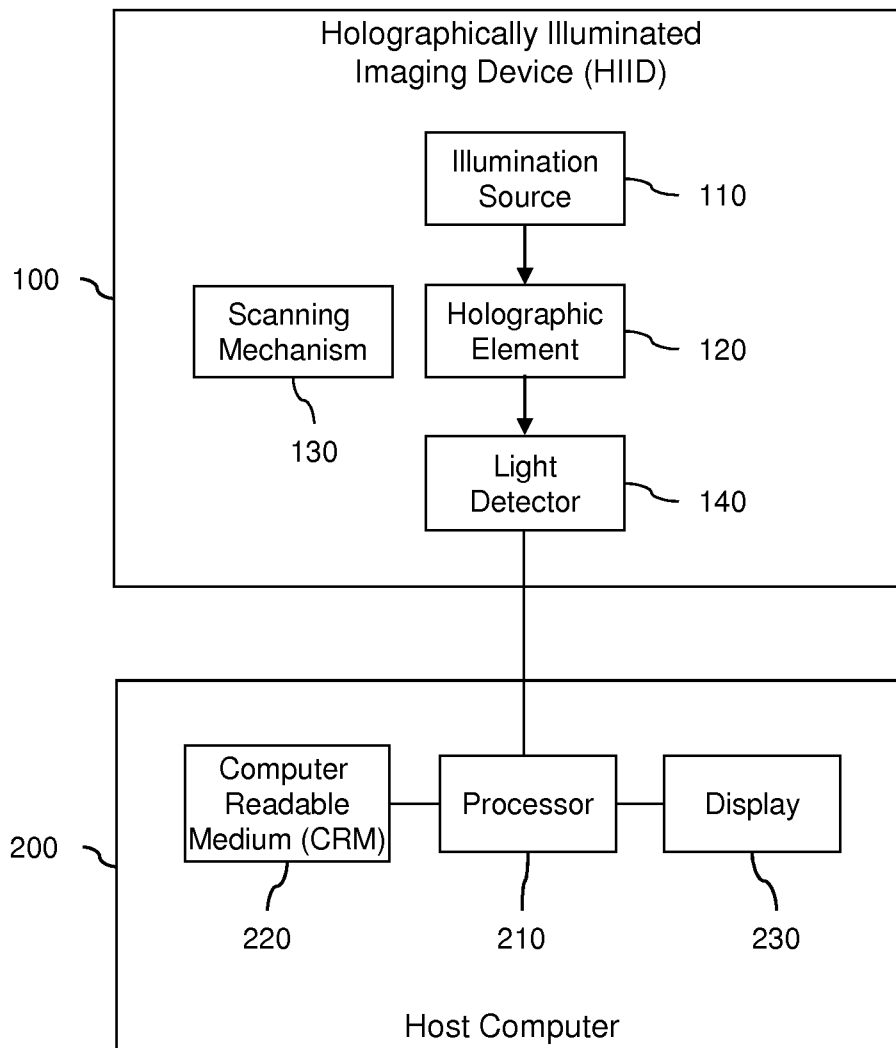
10

FIG.1

2/9

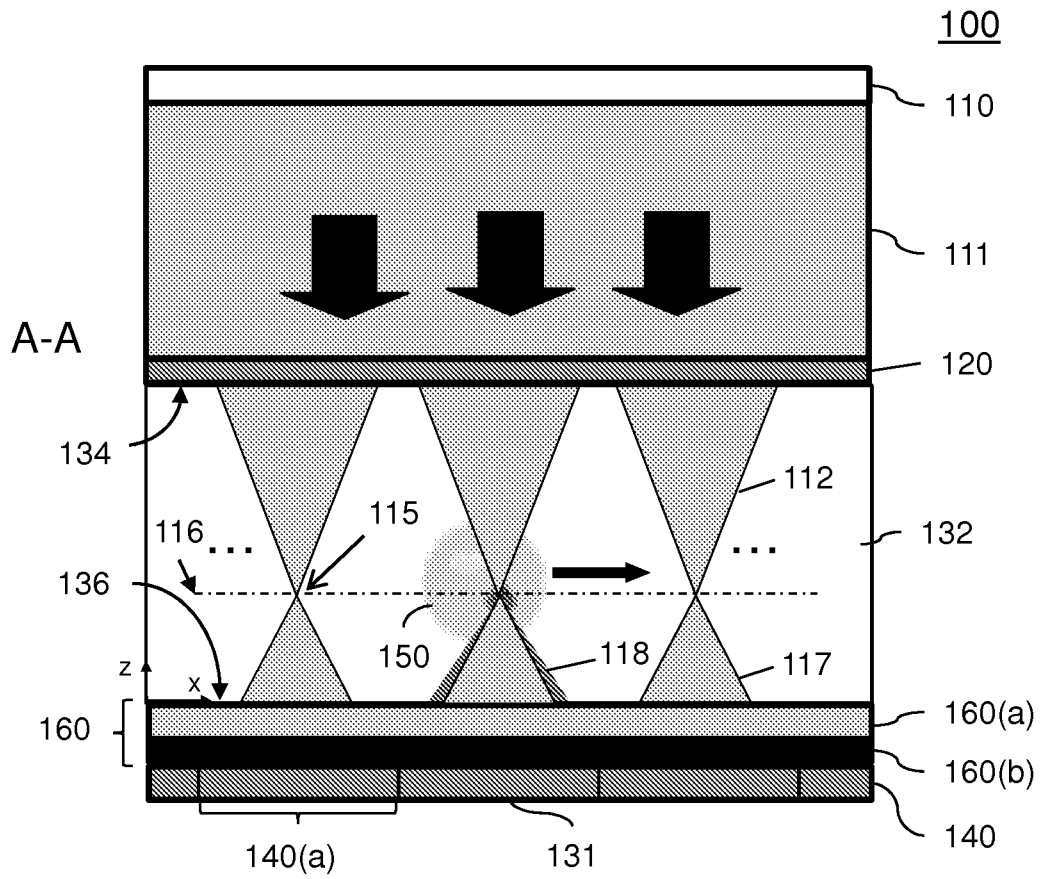


FIG. 2(a)

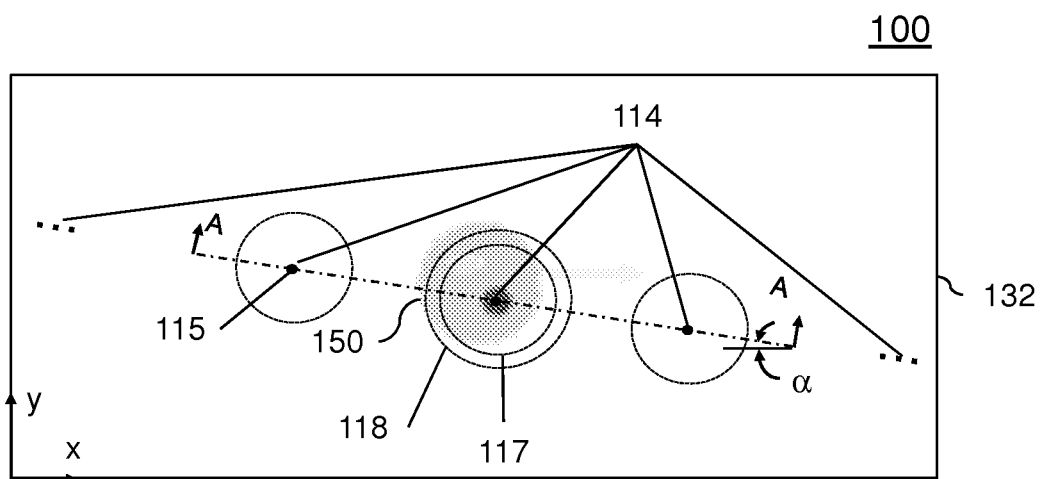


FIG. 2(b)

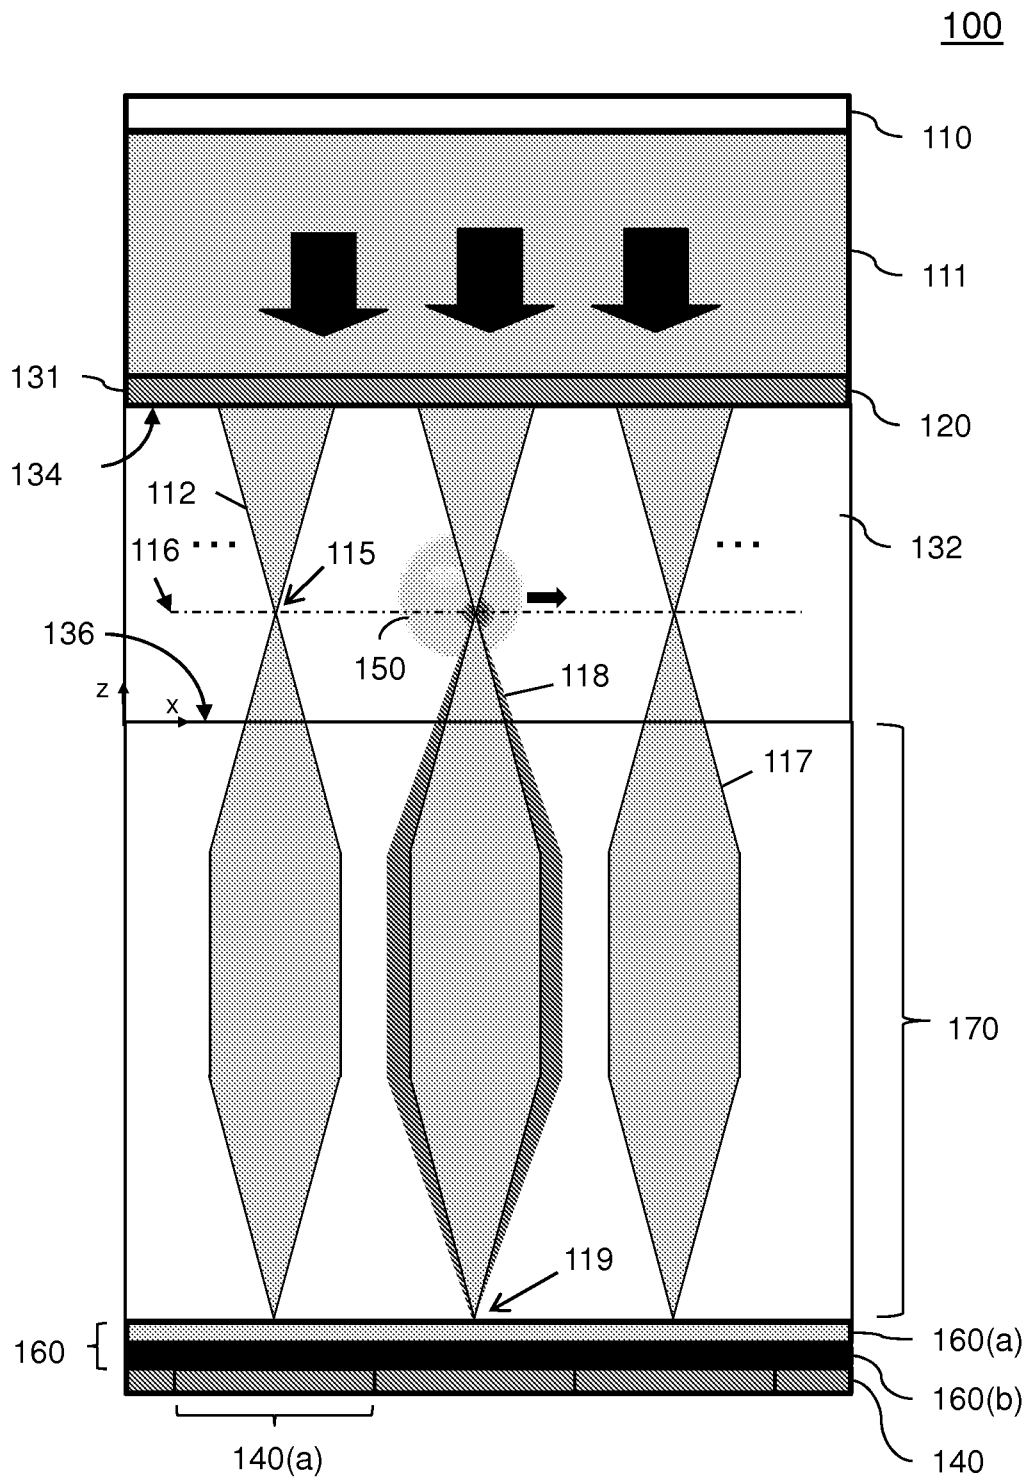


FIG.3

4/9

100

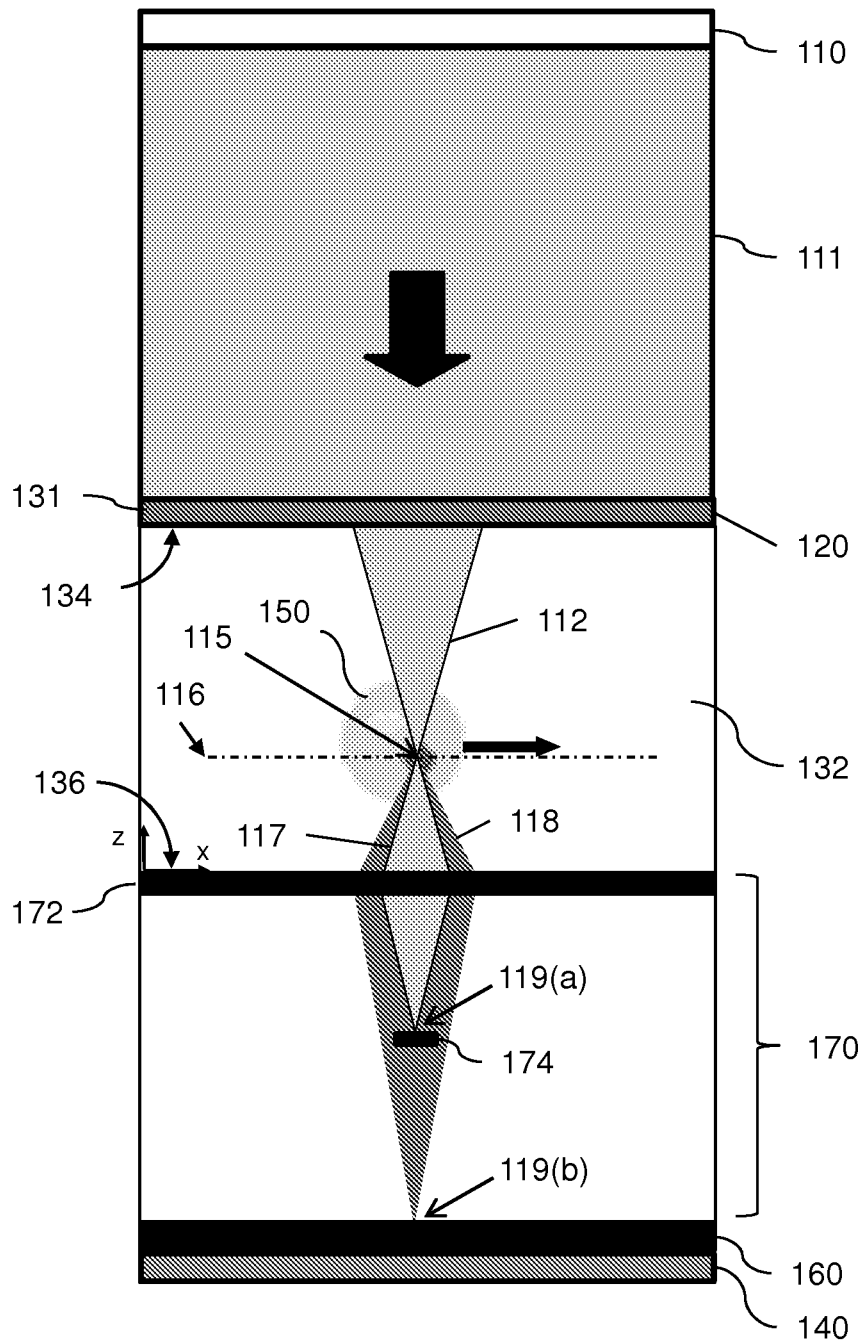


FIG.4

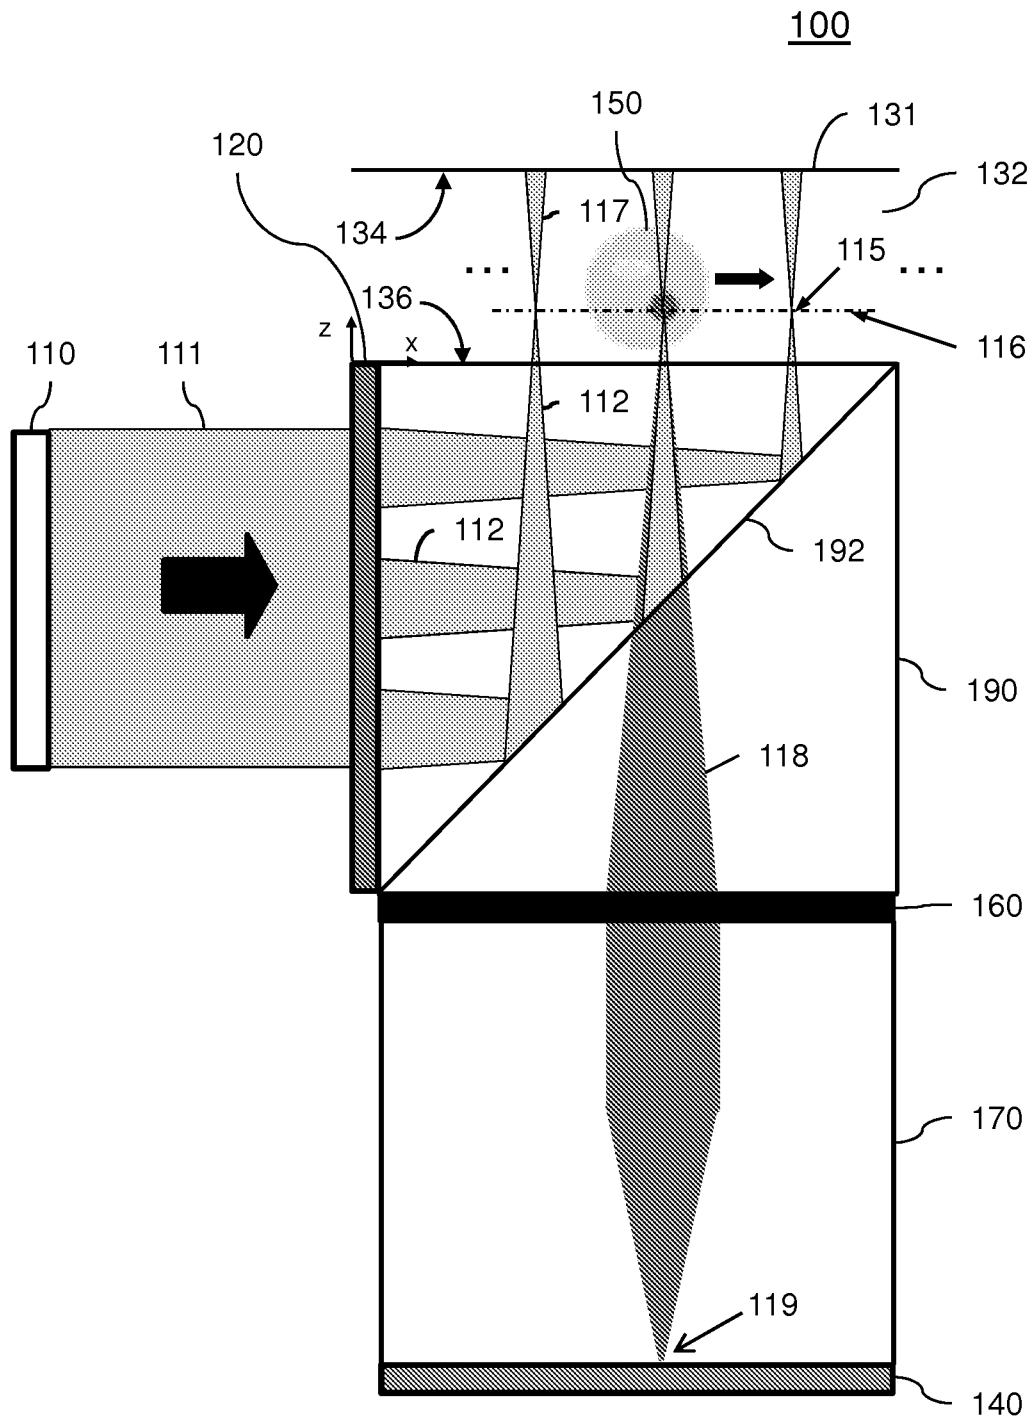


FIG.5

100

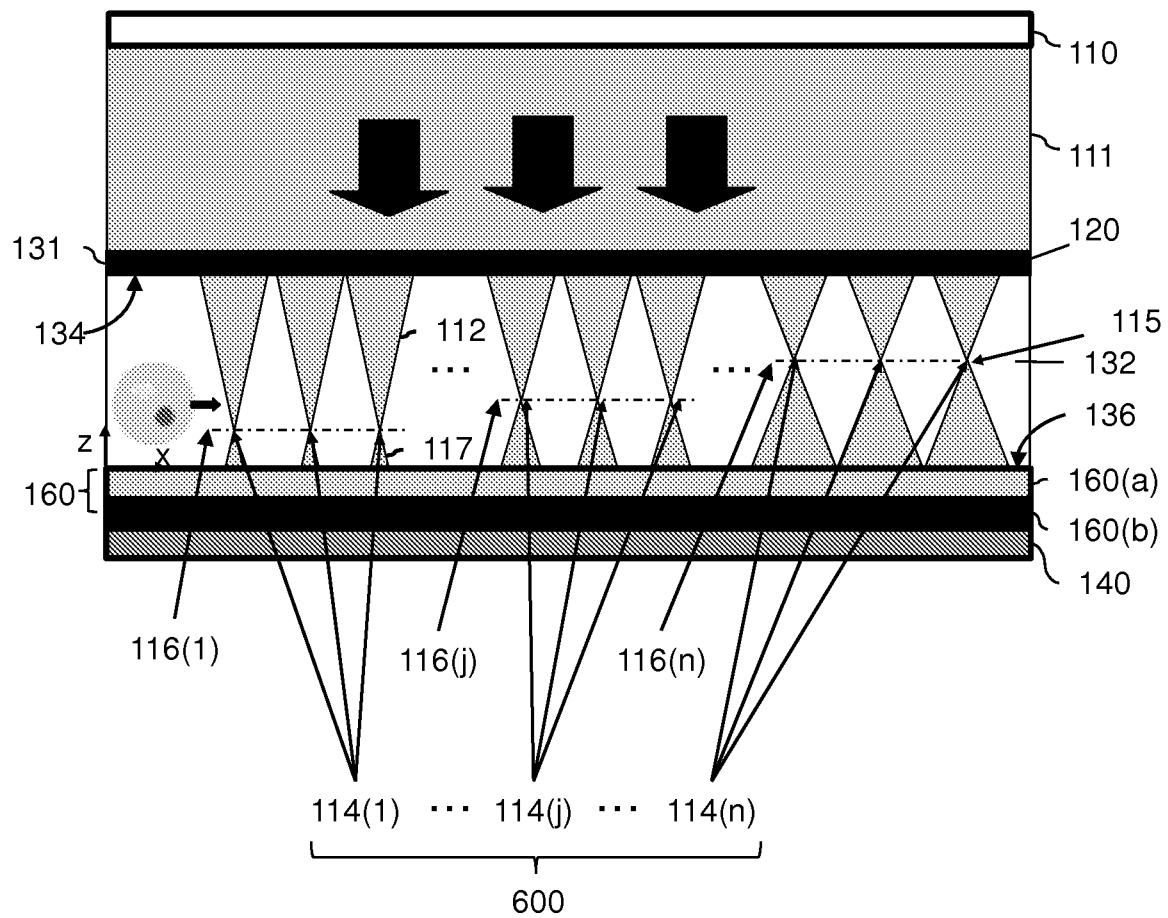


FIG.6

100

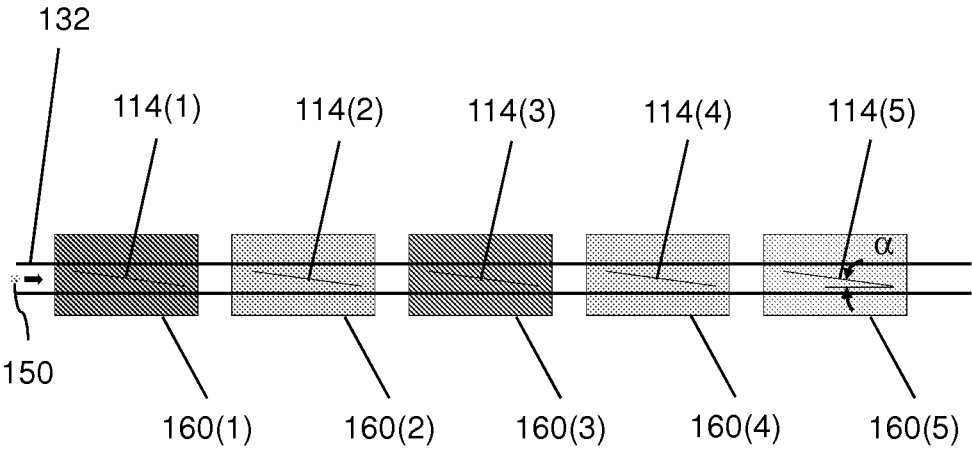


FIG.7

8/9

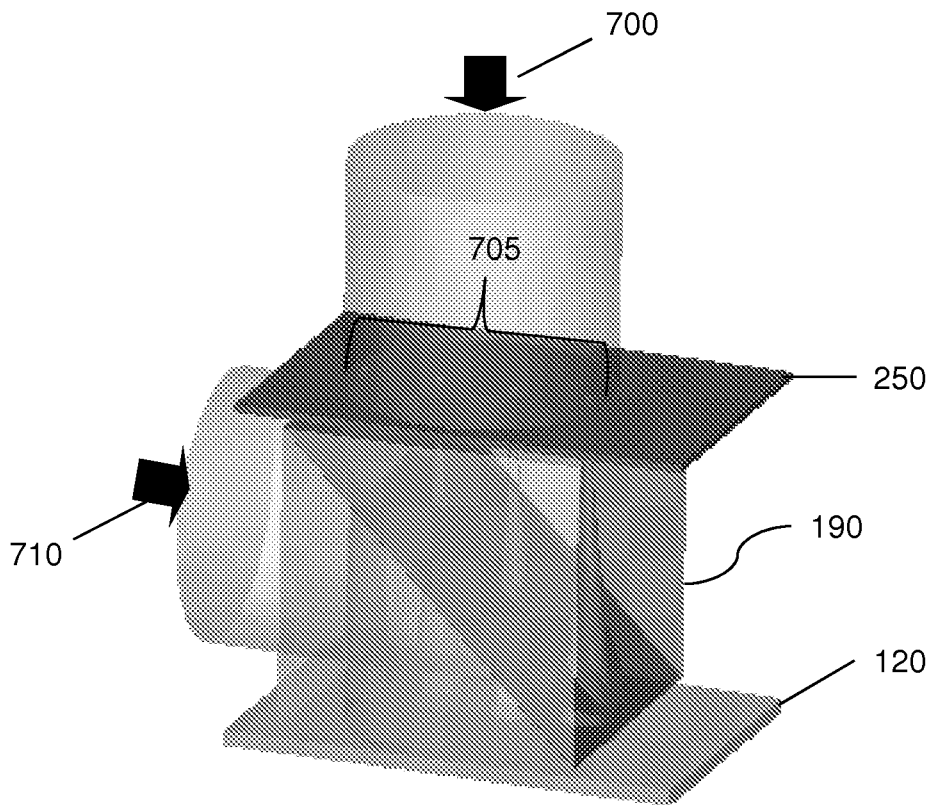


FIG. 8(a)

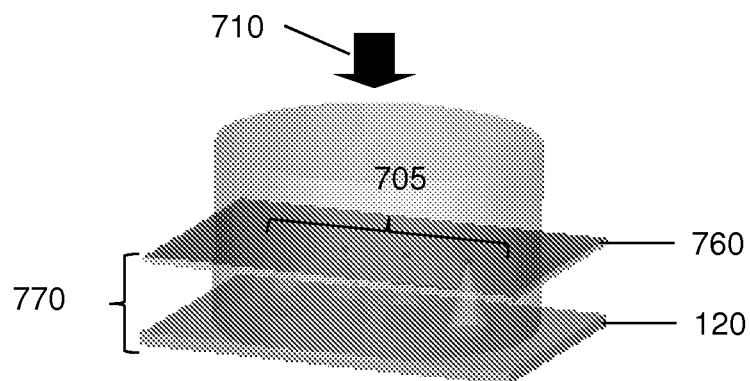


FIG. 8(b)

9/9

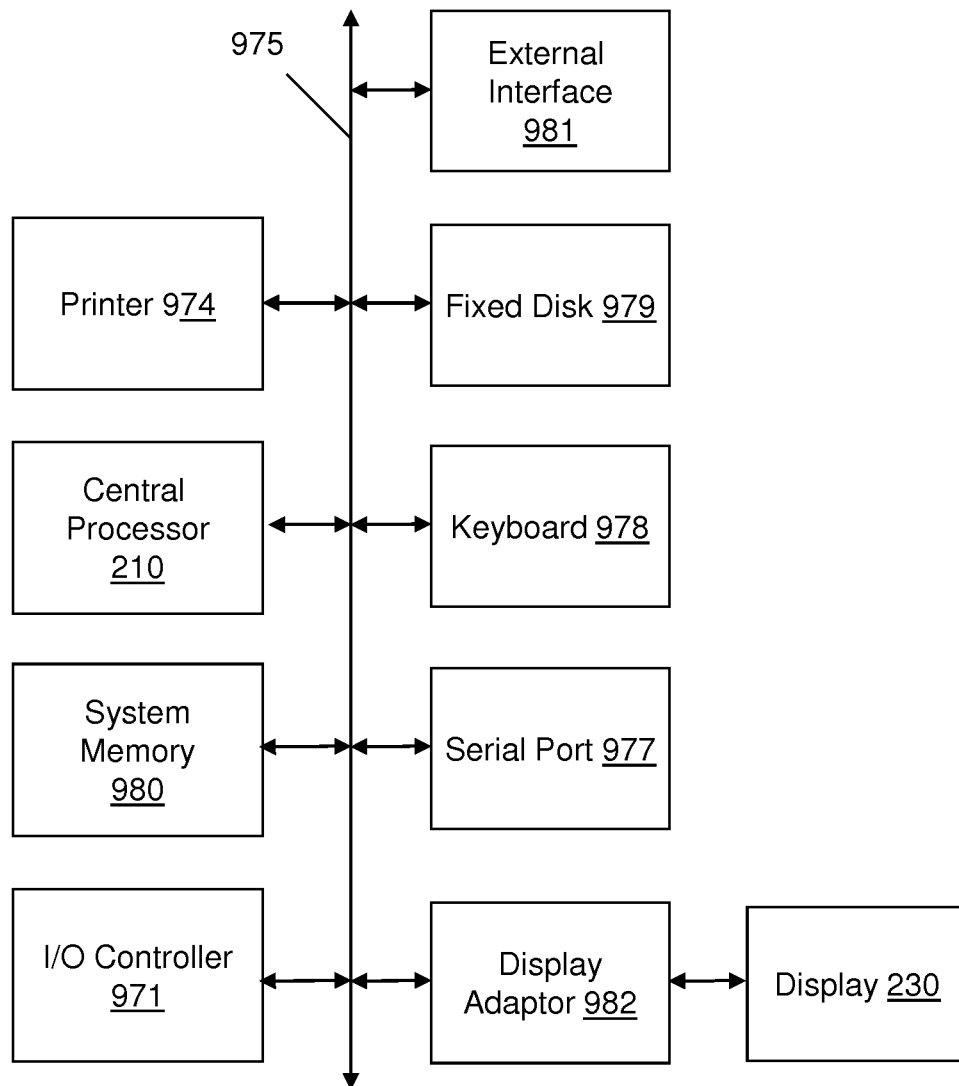


FIG.9