



US00D794662S

(12) **United States Design Patent** (10) **Patent No.:** **US D794,662 S**
Genstler et al. (45) **Date of Patent:** **** Aug. 15, 2017**

(54) **MEDICAL DEVICE CONTROL UNIT
DISPLAY SCREEN WITH GRAPHICAL USER
INTERFACE**

(71) Applicant: **EKOS CORPORATION**, Bothell, WA
(US)

(72) Inventors: **Curtis Genstler**, Snohomish, WA (US);
William Russell Kanz, Woodinville,
WA (US); **Michael George Svob**,
Everett, WA (US); **William Lyle
Richardson**, Duvall, WA (US); **Jeff
Ladwig**, Seattle, WA (US); **Amy
Brumet**, Seattle, WA (US); **Eric Wahl**,
Redmond, WA (US); **David Kalamen**,
Redmond, WA (US); **Stephanie
Seraphina**, Redmond, WA (US); **Alex
Hay**, Bothell, WA (US)

(73) Assignee: **EKOS CORPORATION**, Bothell, WA
(US)

(**) Term: **14 Years**

(21) Appl. No.: **29/503,035**

(22) Filed: **Sep. 22, 2014**

(51) **LOC (10) Cl.** **14-04**

(52) **U.S. Cl.**
USPC **D14/486**

(58) **Field of Classification Search**
USPC D14/485-495
CPC .. G06F 19/3406; G06F 17/246; G06F 3/0482;
G06F 3/04842; G11B 19/025; A61B 5/02
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D238,905 S 2/1976 Sokol
4,006,743 A 2/1977 Kowarski

D247,251 S 2/1978 Napoli
4,312,361 A 1/1982 Nicholson et al.
D264,128 S 4/1982 Barnes et al.
D296,240 S 6/1988 Albright et al.
D330,424 S 10/1992 Davis et al.
(Continued)

FOREIGN PATENT DOCUMENTS

CN 301040544 S 10/2009
CN 301877182 S 4/2012
JP D145667 S 11/2012

OTHER PUBLICATIONS

Plus91 Online, ClinION current patient History Tab, Oct. 13, 2009
[online], [site visited Mar. 21, 2016]. Available from Internet:
<<https://www.youtube.com/watch?v=cdg-9H2RtXs>>.*

(Continued)

Primary Examiner — Karen Kearney

Assistant Examiner — Katherine Holbrow

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson
& Bear LLP

(57) **CLAIM**

The ornamental design for a medical device control unit
display screen with graphical user interface, as shown and
described.


DESCRIPTION

The file of this patent contains at least one drawing/photo-
graph executed in color. Copies of this patent with color
drawing(s)/photograph(s) will be provided by the Office
upon request and payment of the necessary fee.

FIG. 1 is a front view of a medical device control unit
display screen with graphical user interface, showing a first
embodiment of the new design; and,

FIG. 2 is a front view of a second embodiment thereof.

1 Claim, 2 Drawing Sheets
(1 of 2 Drawing Sheet(s) Filed in Color)

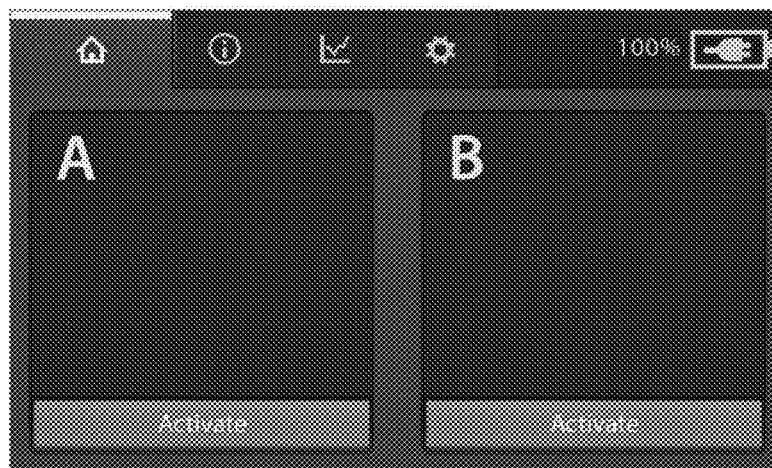

US D794,662 S

Page 2

(56)

References Cited

U.S. PATENT DOCUMENTS

5,461,708 A * 10/1995 Kahn G06T 11/206
345/440
D380,543 S 7/1997 Piontek et al.
D427,574 S * 7/2000 Sawada D14/486
6,493,731 B1 * 12/2002 Jones G06Q 10/10
715/234
D526,655 S * 8/2006 McDougall D14/485
D534,654 S 1/2007 Hayamizu
7,178,109 B2 * 2/2007 Hewson G06F 9/4443
715/742
7,235,063 B2 6/2007 D'Antonio et al.
D555,165 S * 11/2007 Myers D14/487
D564,094 S 3/2008 Hayashi
D564,661 S 3/2008 Hayashi
D574,961 S 8/2008 Kitahara et al.
D578,543 S * 10/2008 Ulm D14/487
D592,754 S 5/2009 Koike et al.
D593,117 S * 5/2009 Lettau D14/488
7,615,030 B2 11/2009 Murphy et al.
D617,332 S * 6/2010 Loken D14/485
D622,841 S 8/2010 Bierman
D630,727 S 1/2011 Petrovic et al.
D637,287 S 5/2011 Mudd et al.
D643,117 S 8/2011 Onuma
D644,649 S * 9/2011 Fullington D14/485
D651,212 S * 12/2011 Bakhreiba D13/164
D658,667 S * 5/2012 Cho D14/486
D659,151 S * 5/2012 Loken D14/485
D664,257 S 7/2012 Patil
D664,985 S 8/2012 Tanghe et al.
D670,714 S * 11/2012 Majeed D14/485
D670,716 S * 11/2012 Majeed D14/485
D670,725 S 11/2012 Mori et al.
D671,552 S 11/2012 Mori et al.
D676,562 S 2/2013 Marzynski
D685,815 S * 7/2013 Bork D14/486
D698,925 S 2/2014 Marzynski
D700,343 S 2/2014 Liu
8,762,880 B2 * 6/2014 Dukhon G06F 17/24
715/781
D709,515 S * 7/2014 Elston D14/485

8,771,186 B2 * 7/2014 Kinsley A61B 5/0205
128/920
D711,001 S 8/2014 Boudier
D714,948 S 10/2014 Vaccarella
D725,784 S 3/2015 Xia et al.
D733,178 S * 6/2015 Omiya D14/486
9,050,123 B2 * 6/2015 Krause A61B 17/32002
D733,720 S * 7/2015 Mueller D14/485
D733,738 S * 7/2015 Omiya D14/486
D734,475 S 7/2015 Ross
D741,351 S * 10/2015 Kito D14/486
D741,871 S * 10/2015 Chung D14/485
D763,298 S * 8/2016 Hoang D14/487
D767,583 S * 9/2016 Xiong D14/485
D767,584 S * 9/2016 Xiong D14/485
D772,252 S * 11/2016 Myers D14/486
D773,491 S * 12/2016 Ahdritz D14/486
D776,688 S * 1/2017 Gamel D14/486
2004/0111195 A1 * 6/2004 Vries G01C 21/20
701/21
2005/0278633 A1 * 12/2005 Kemp G06F 3/0481
715/713
2008/0115064 A1 * 5/2008 Roach G06F 3/04817
715/730
2008/0228526 A1 * 9/2008 Locke A61M 5/1415
705/3
2008/0235872 A1 * 10/2008 Newkirk A61G 7/018
5/600
2008/0290114 A1 11/2008 Cabuz
2013/0073306 A1 * 3/2013 Shlain G06Q 10/06
705/2
2014/0226901 A1 * 8/2014 Spracklen H04N 21/4621
382/167
2015/0095807 A1 * 4/2015 Duncker G06F 17/30873
715/753
2015/0178044 A1 * 6/2015 Ehlen G06F 3/0482
715/728

OTHER PUBLICATIONS

"EkoSonic® MACH4e", EKOS Advertisement, Venous Times, Issue 6, dated Jan. 2010, p. 3.

* cited by examiner

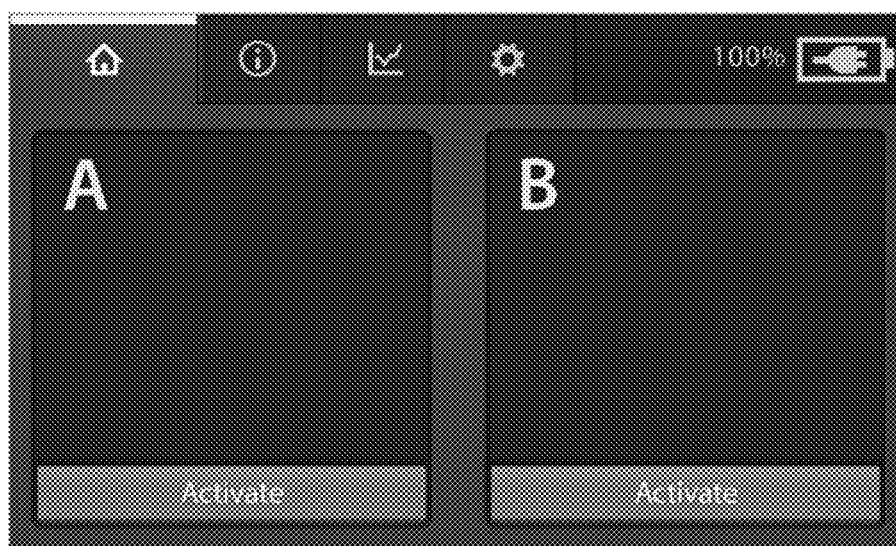
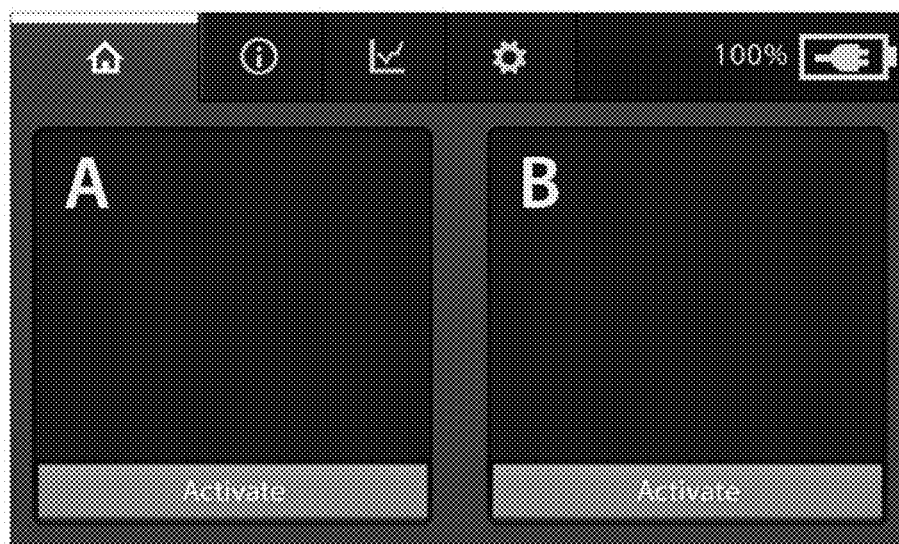


FIG. 1

*FIG. 2*