



US 20080058828A1

(19) **United States**(12) **Patent Application Publication****Reiley et al.**(10) **Pub. No.: US 2008/0058828 A1**(43) **Pub. Date: Mar. 6, 2008**(54) **SYSTEMS AND METHODS FOR TREATING BONE USING EXPANDABLE BODIES**(75) Inventors: **Mark A. Reiley**, Piedmont, CA (US);
Arie Scholten, Fremont, CA (US);
Karen D. Talmadge, Palo Alto, CA (US); **Robert M. Scribner**, Los Altos, CA (US)

Correspondence Address:

Daniel D. Ryan**RYAN, MAKI, MANN & HOHENFELDT, S.C.**

Suite 1900

633 West Wisconsin Avenue**Milwaukee, WI 53203 (US)**(73) Assignee: **Kyphon, Inc.**(21) Appl. No.: **11/977,667**(22) Filed: **Oct. 25, 2007****Related U.S. Application Data**

(60) Division of application No. 11/528,163, filed on Sep. 27, 2006, which is a division of application No. 10/958,600, filed on Oct. 5, 2004, which is a division

of application No. 09/754,451, filed on Jan. 4, 2001, now Pat. No. 6,899,719, which is a continuation of application No. 08/871,114, filed on Jun. 9, 1997, now Pat. No. 6,248,110, which is a continuation-in-part of application No. 08/659,678, filed on Jun. 5, 1996, now Pat. No. 5,827,289, which is a continuation-in-part of application No. 08/485,394, filed on Jun. 7, 1995, now abandoned, which is a continuation-in-part of application No. 08/188,224, filed on Jan. 26, 1994, now abandoned.

Publication Classification(51) **Int. Cl.****A61B 17/58** (2006.01)**A61M 29/00** (2006.01)(52) **U.S. Cl.** **606/94; 606/192; 606/198; 606/92; 606/93**(57) **ABSTRACT**

An expandable device is introduced into a cancellous bone volume of a vertebral body through a percutaneous access path. The expandable device is expanded while disposed within the cancellous bone volume to create a cavity. A filling material including a biomaterial is placed within the cavity.

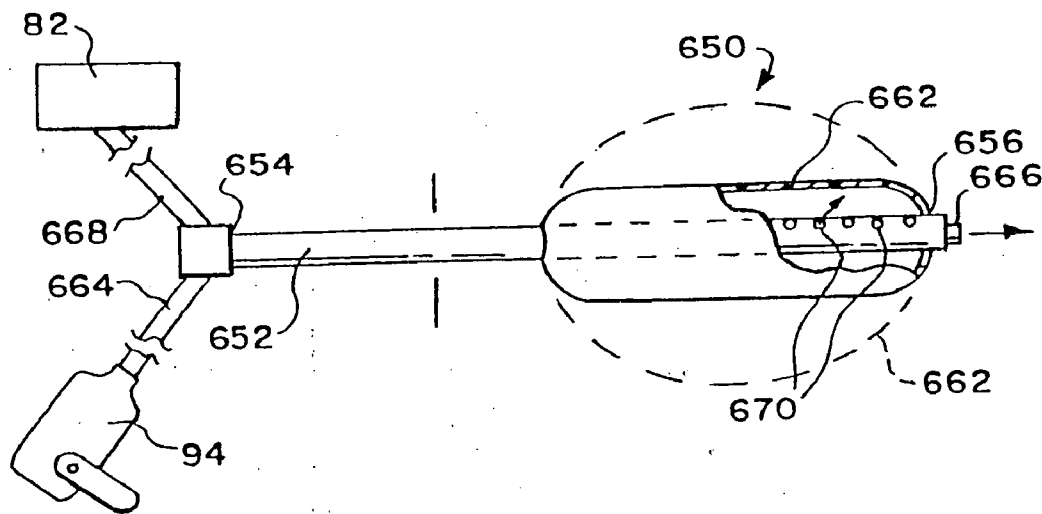


FIG. 1

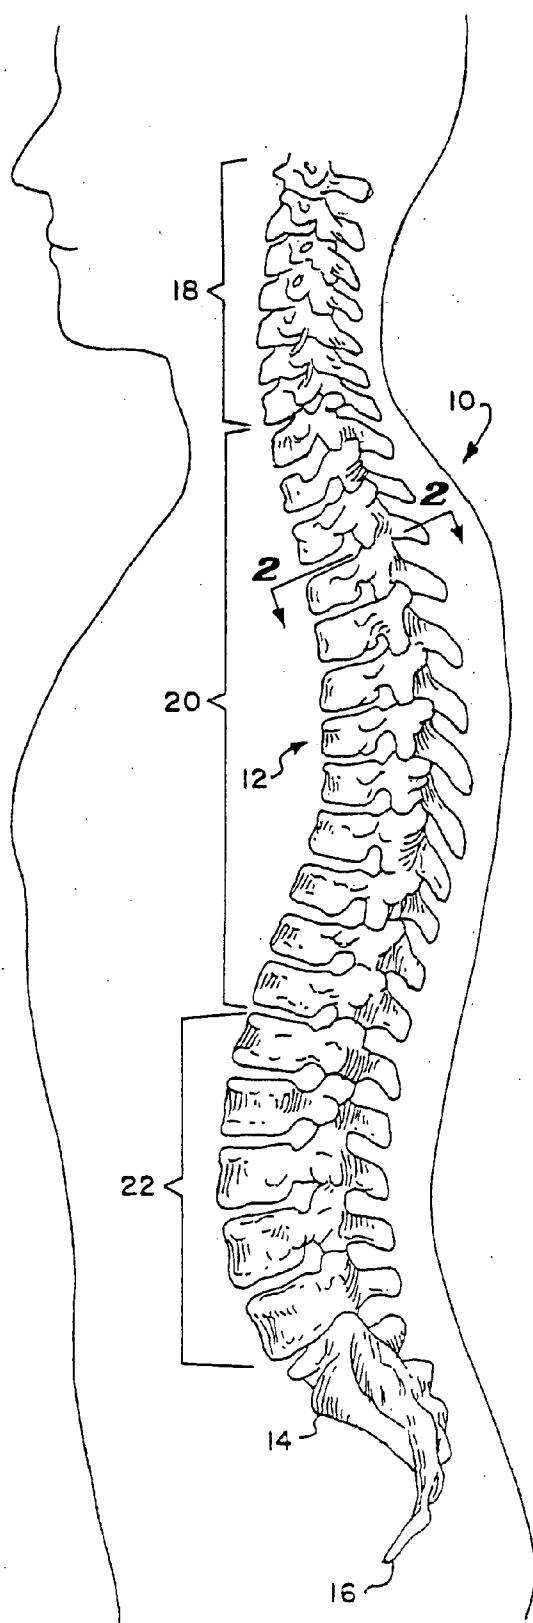


FIG. 2

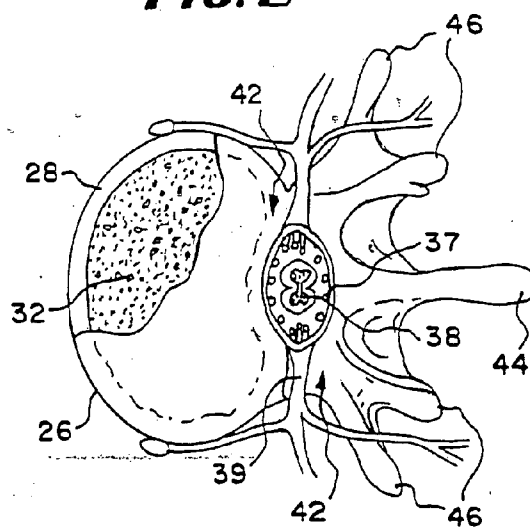
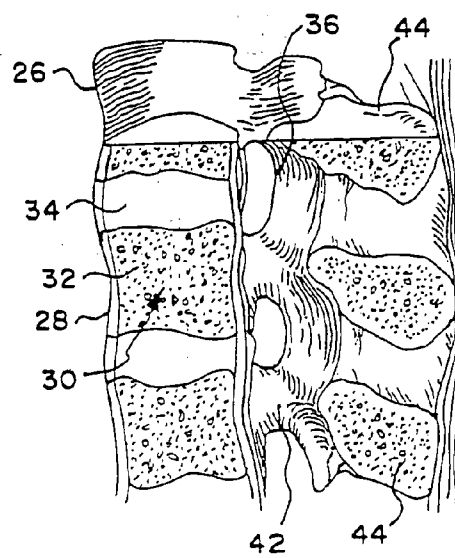


FIG. 3



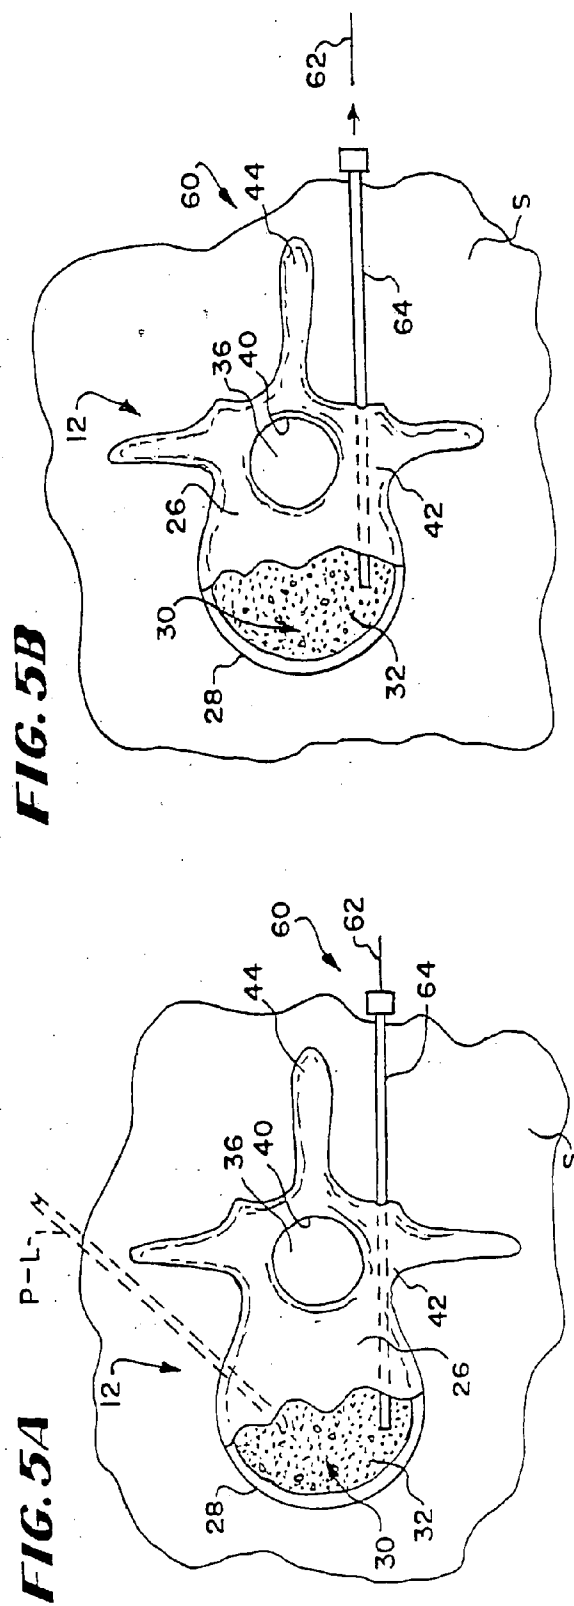
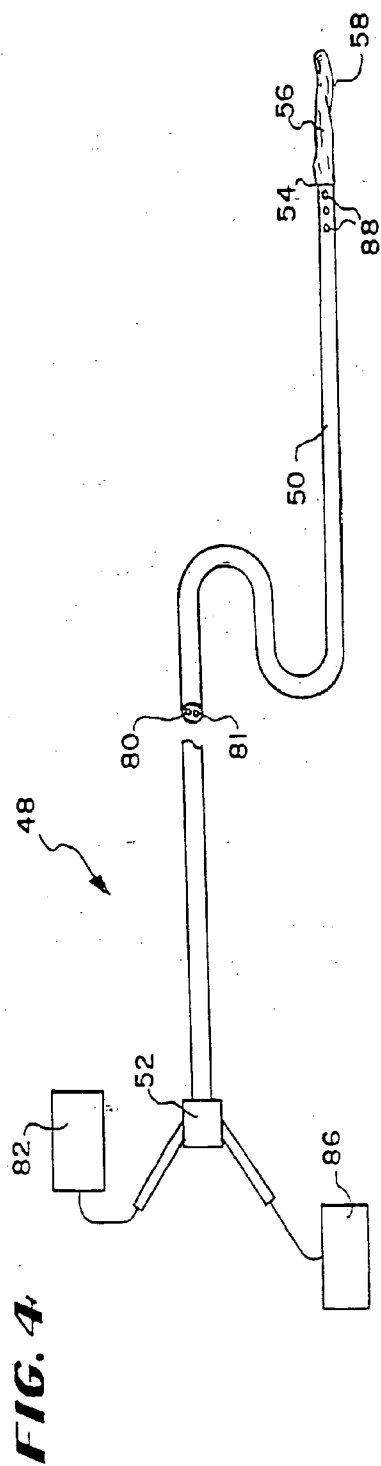
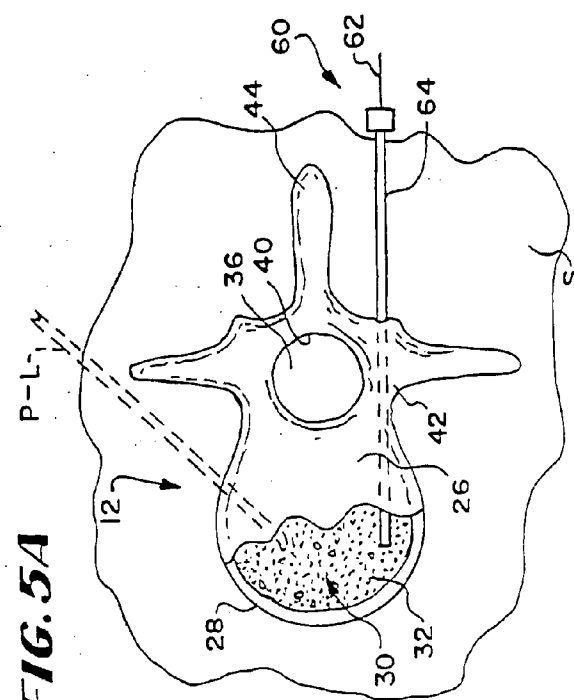


FIG. 5B



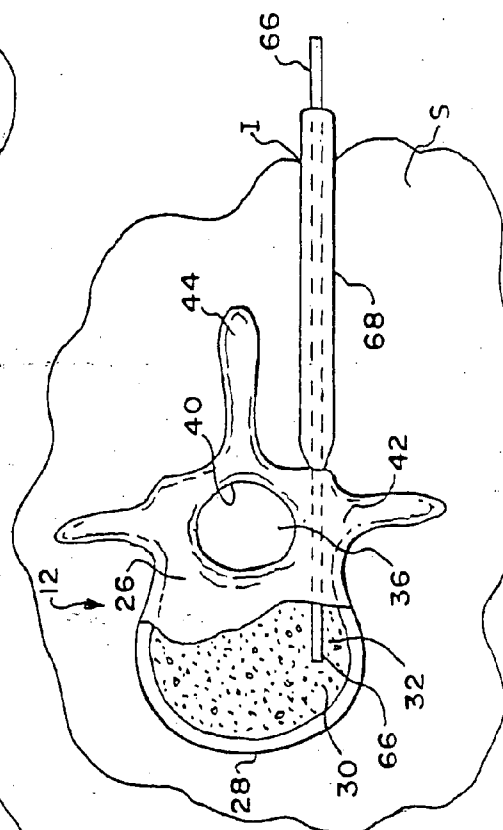
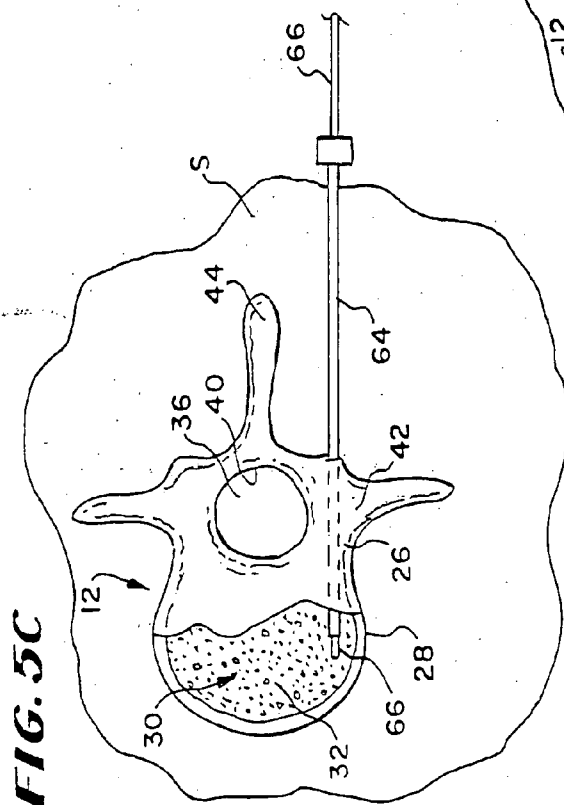
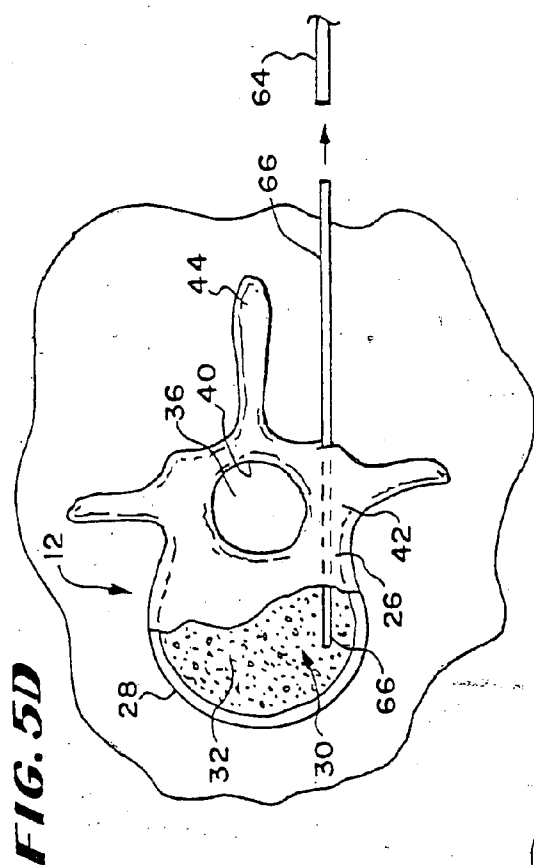


FIG. 5F

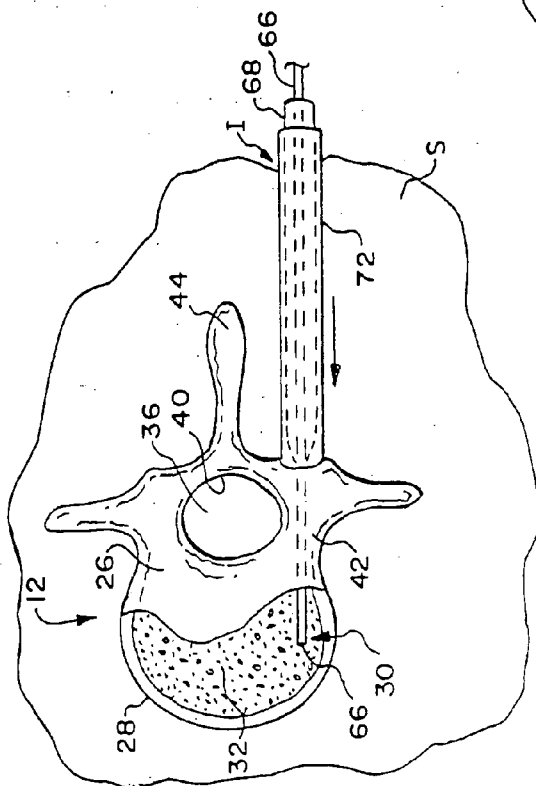


FIG. 5G

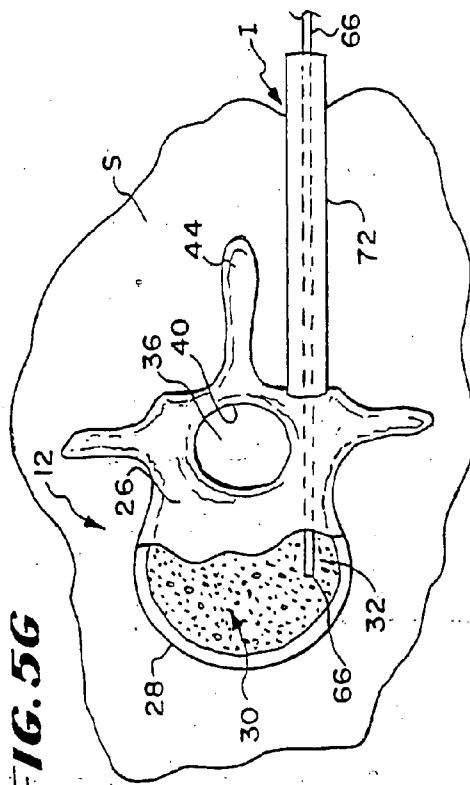


FIG. 5H

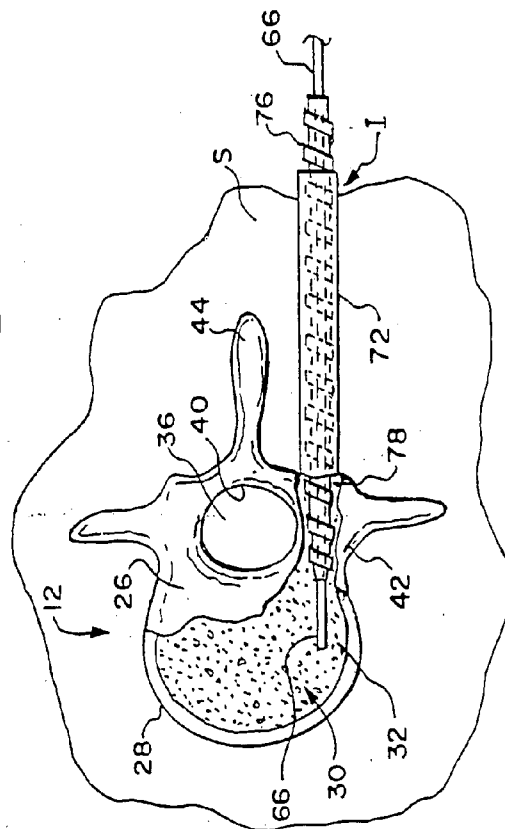


FIG. 5I

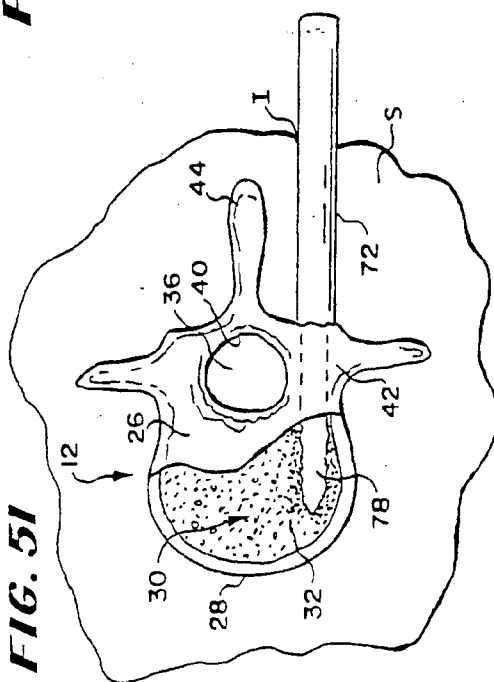


FIG. 5J(1)

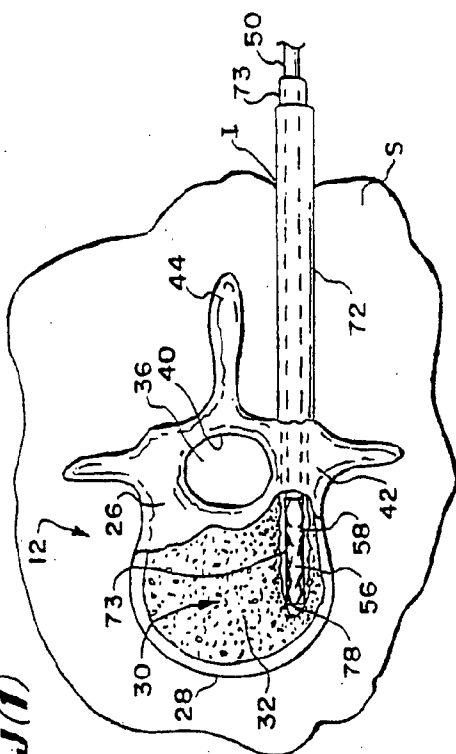


FIG. 5J(2)

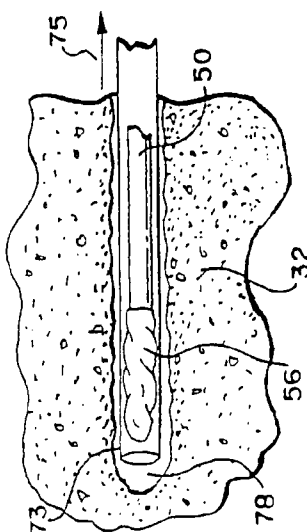


FIG. 5K(1)

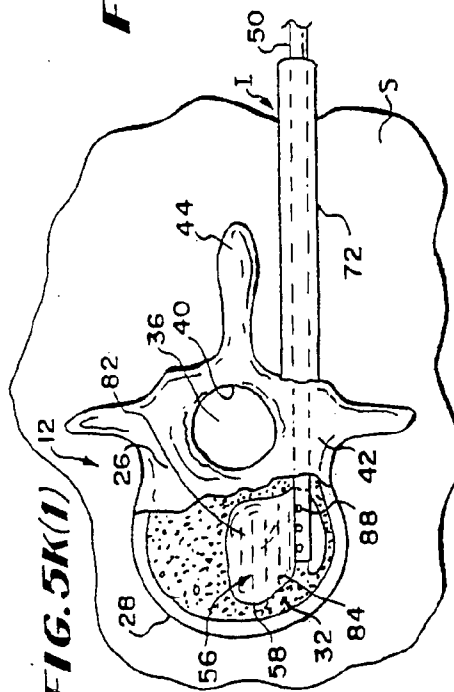
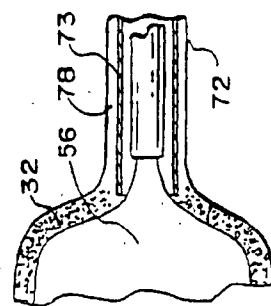


FIG. 5K(2)



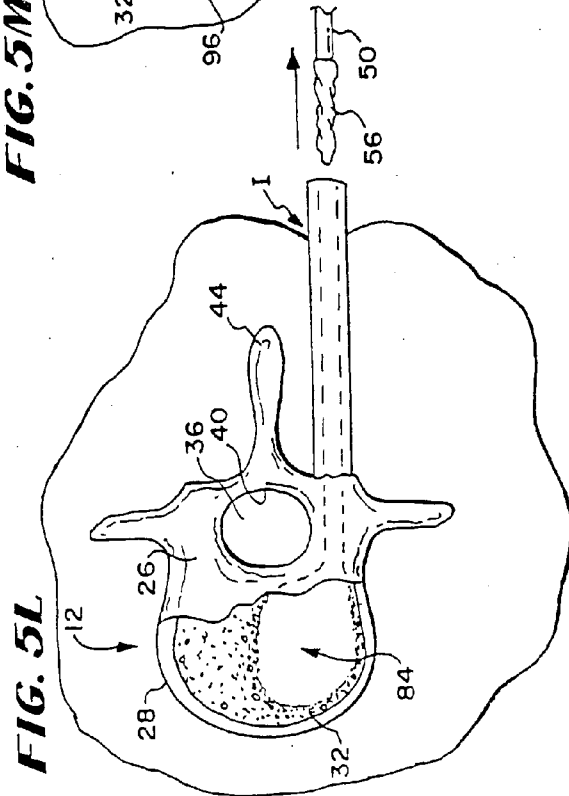
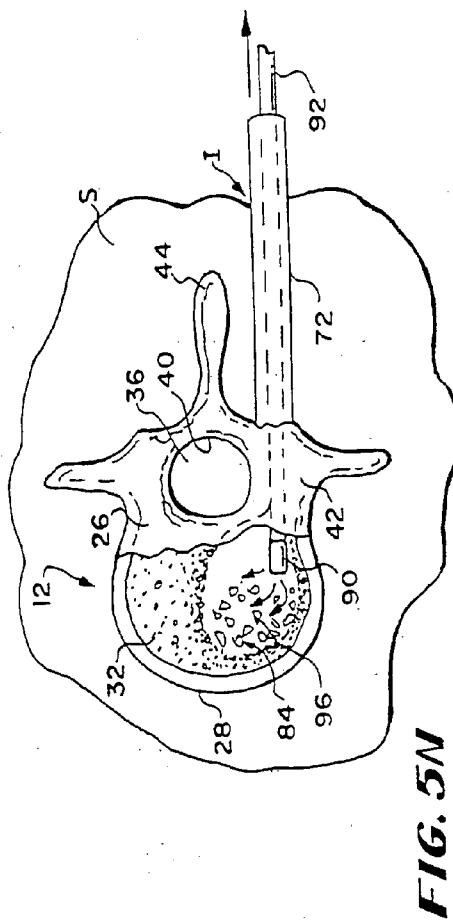
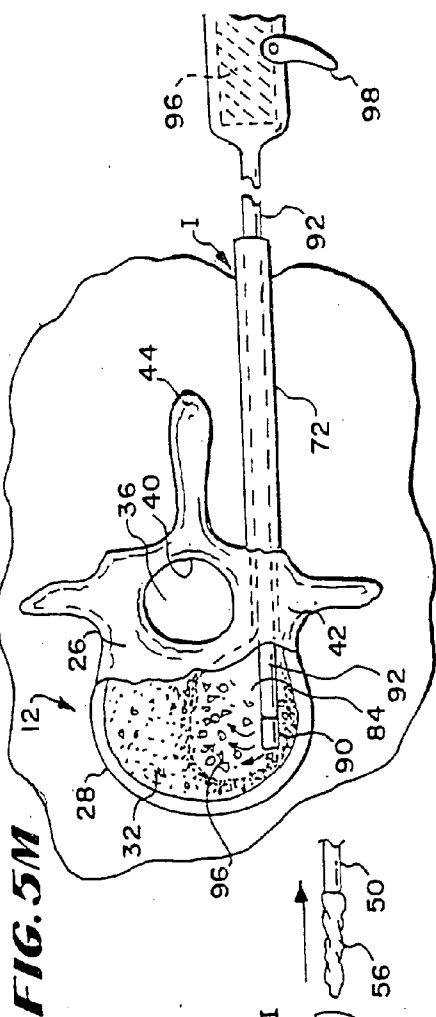


FIG. 5P

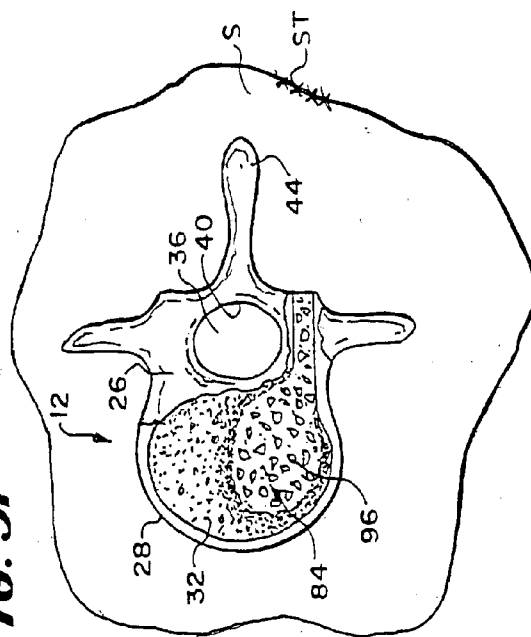


FIG. 5Q

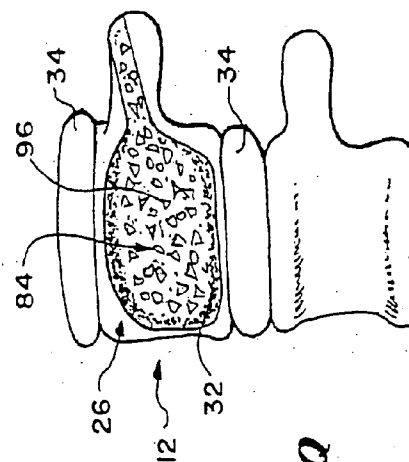
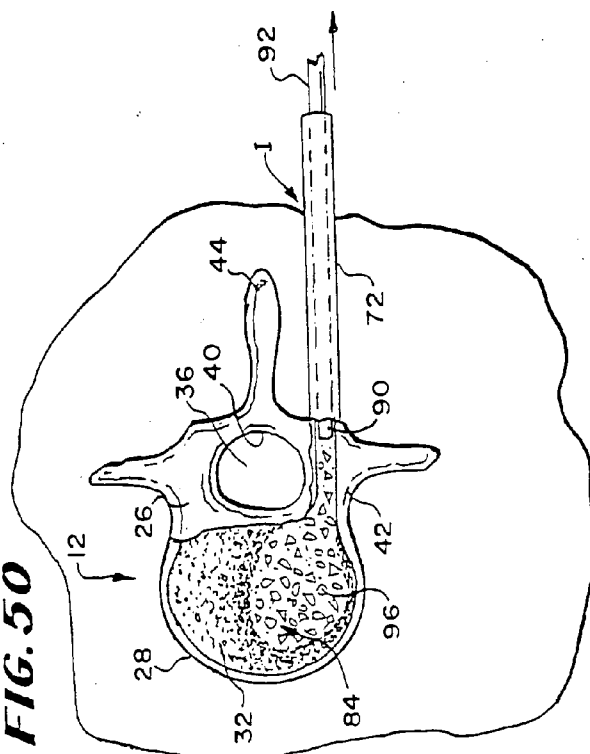


FIG. 5Q

FIG. 7

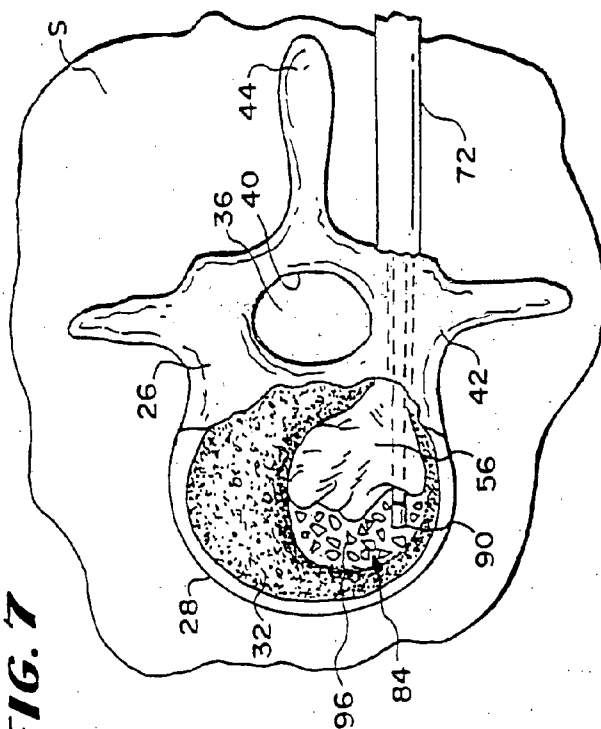
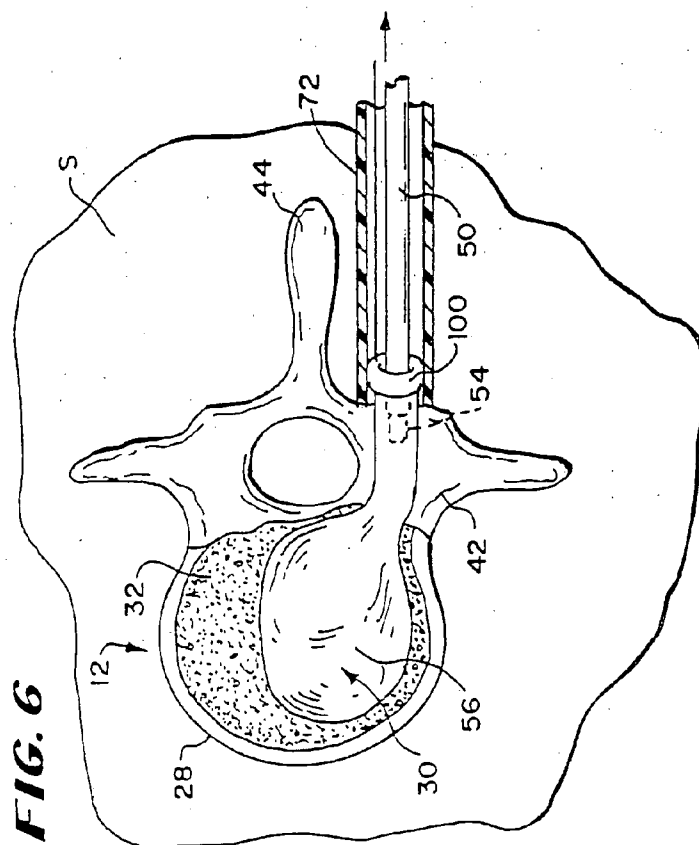
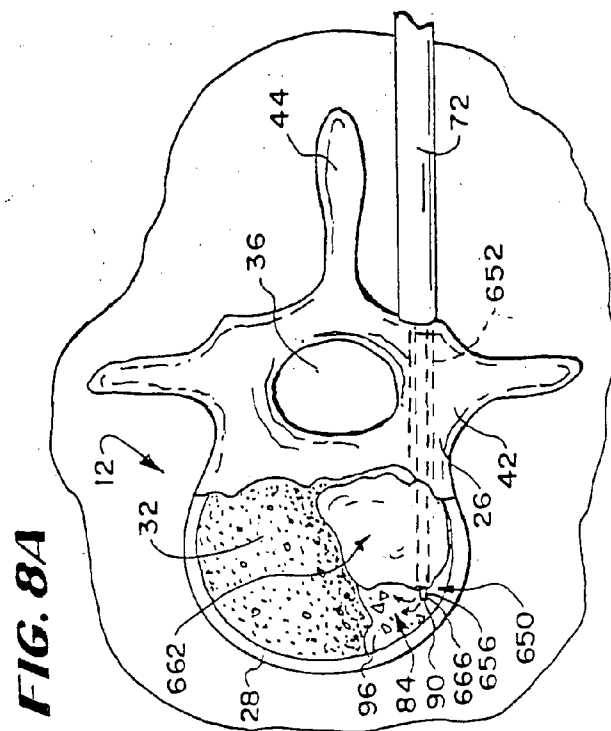
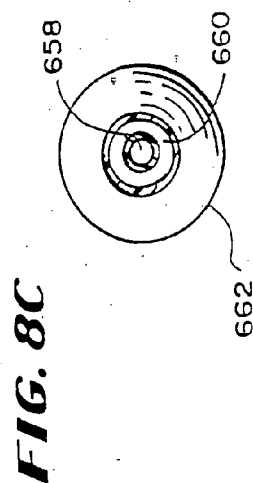
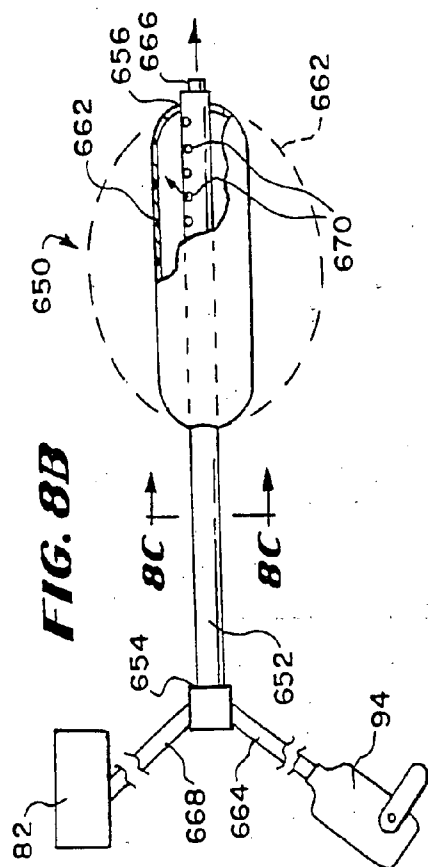


FIG. 6





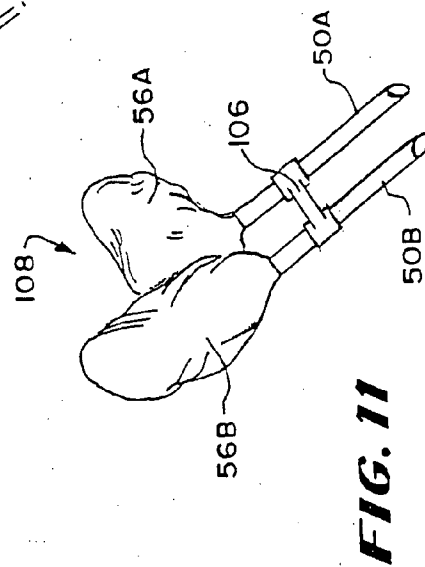
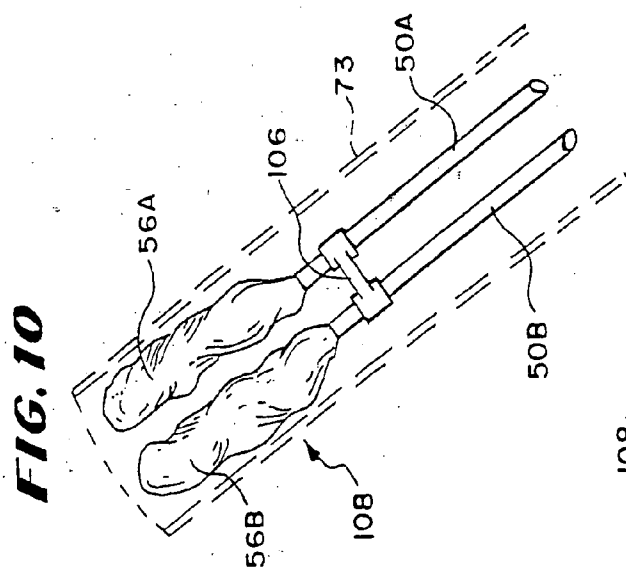
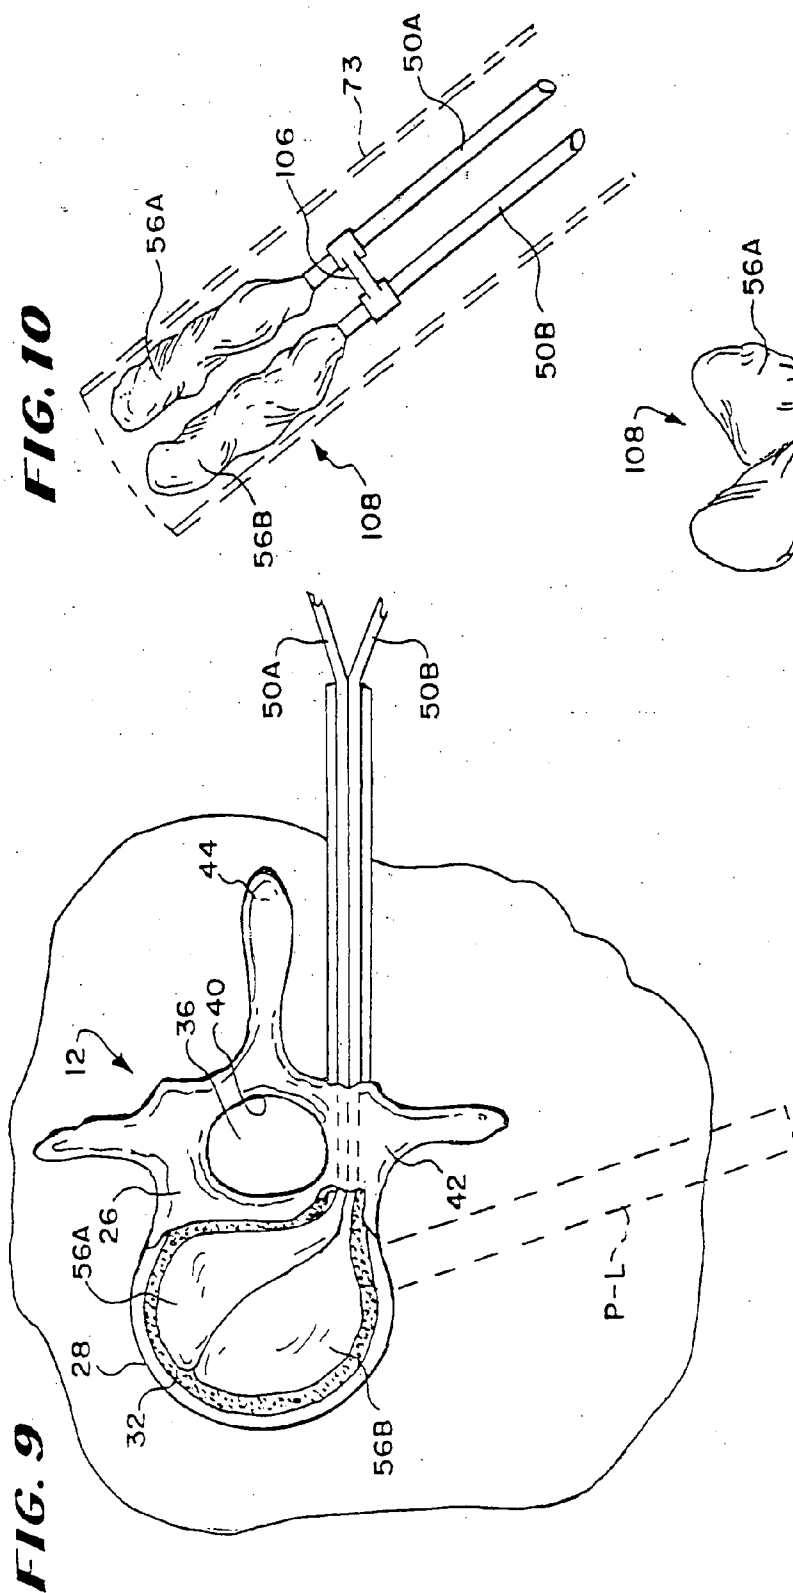


FIG. 12

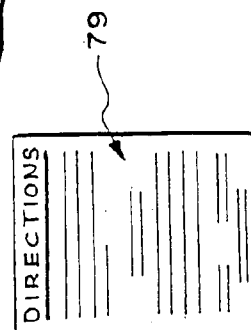
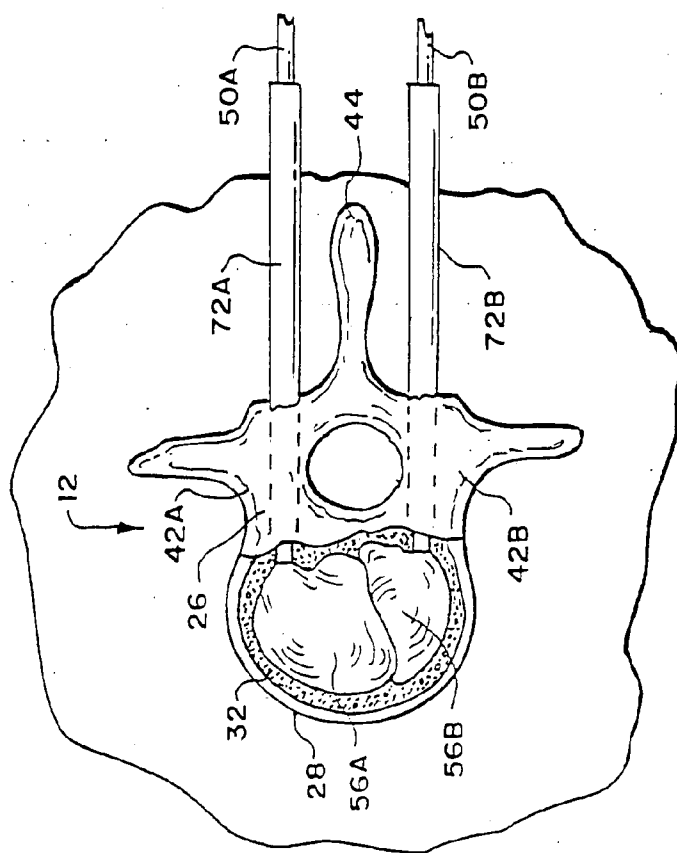


FIG. 13

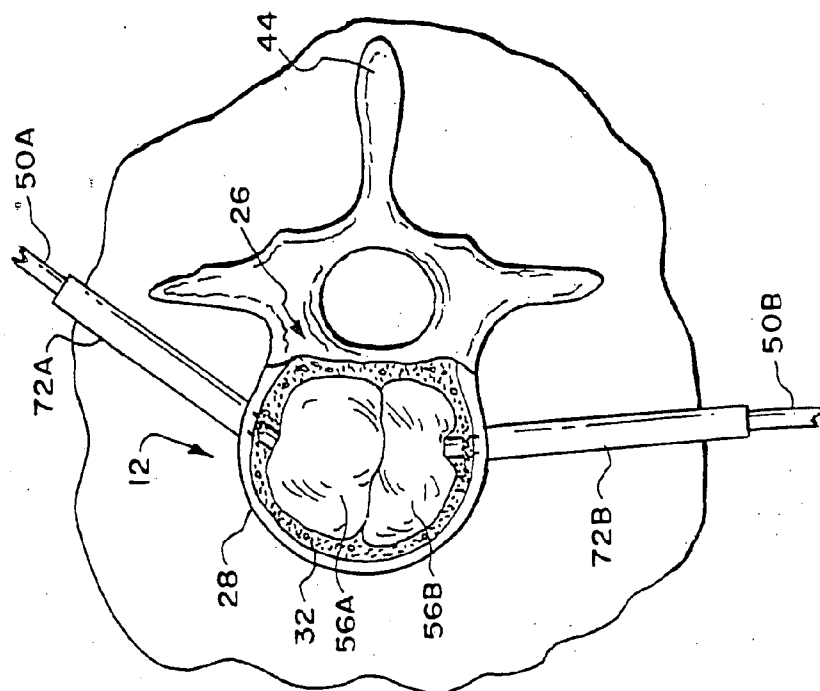


FIG. 15

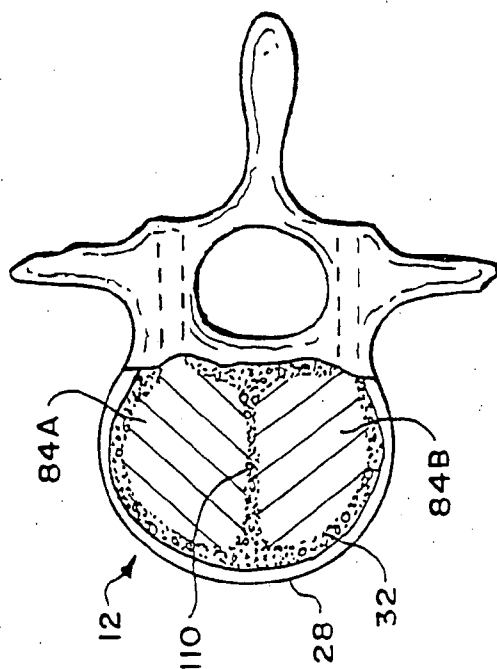


FIG. 14

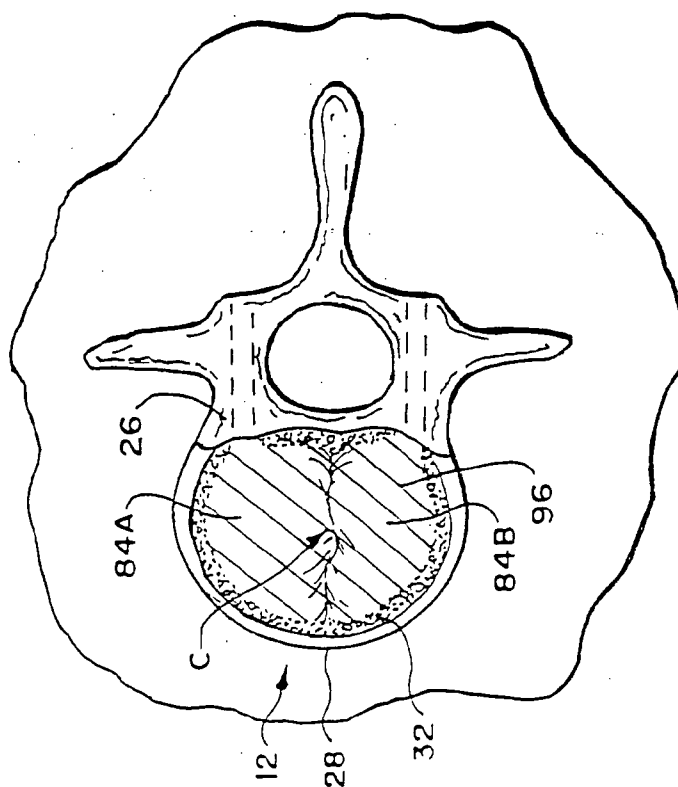


FIG. 17

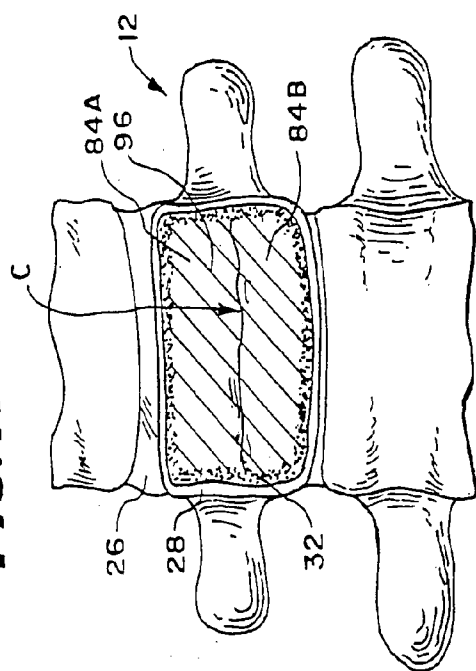


FIG. 18

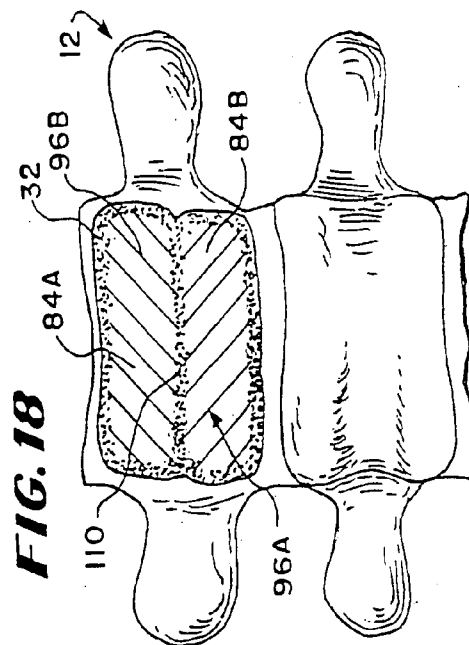


FIG. 16

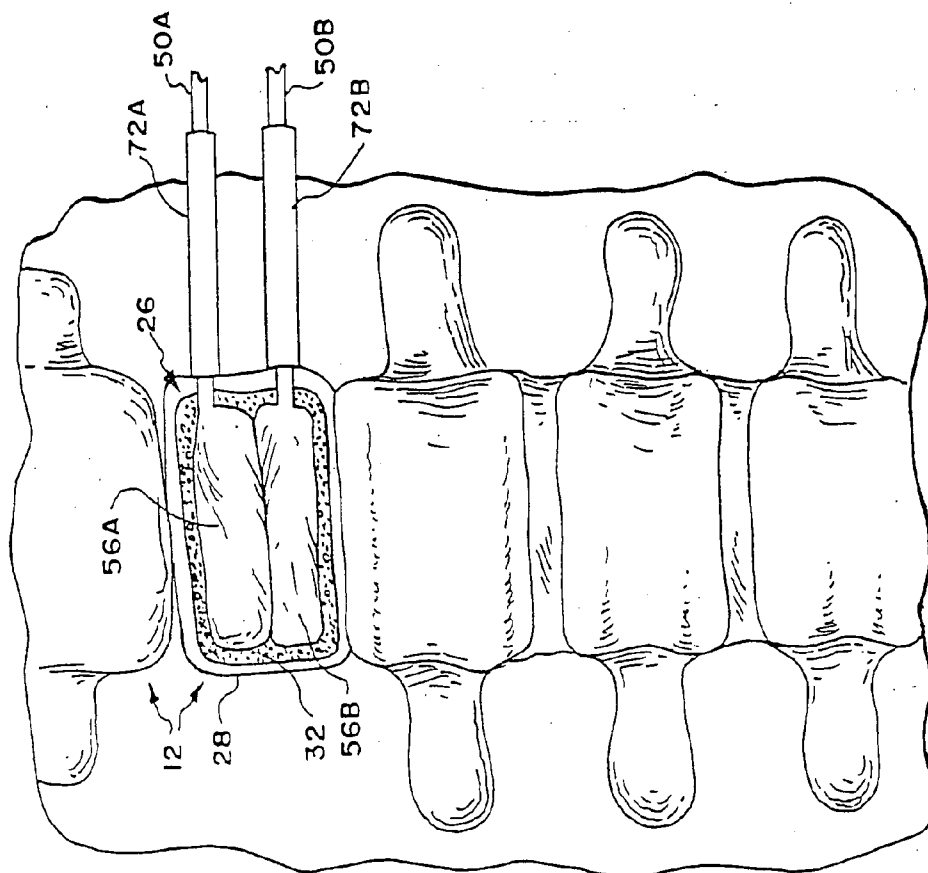


FIG. 19

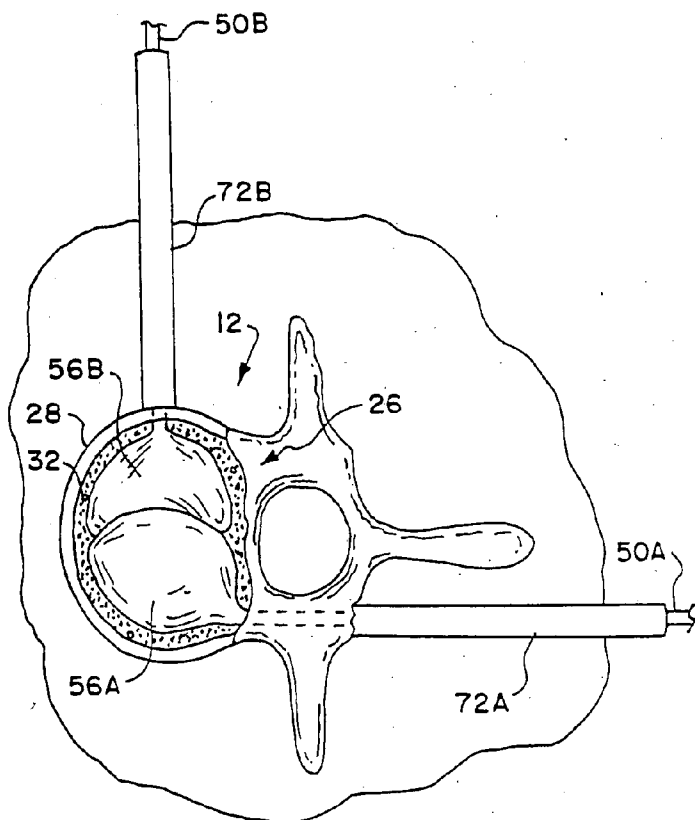


FIG. 21

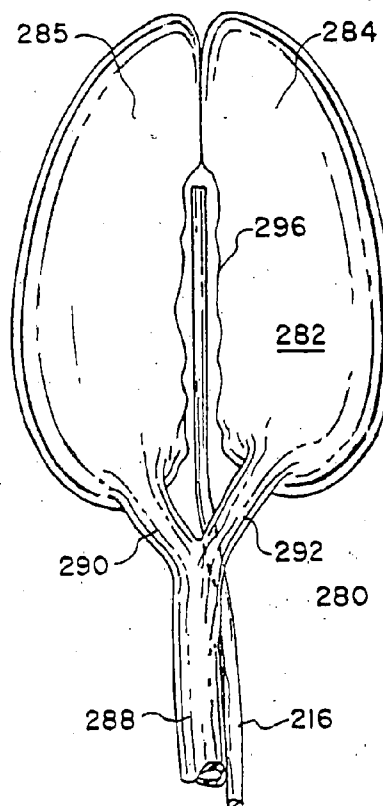


FIG. 20

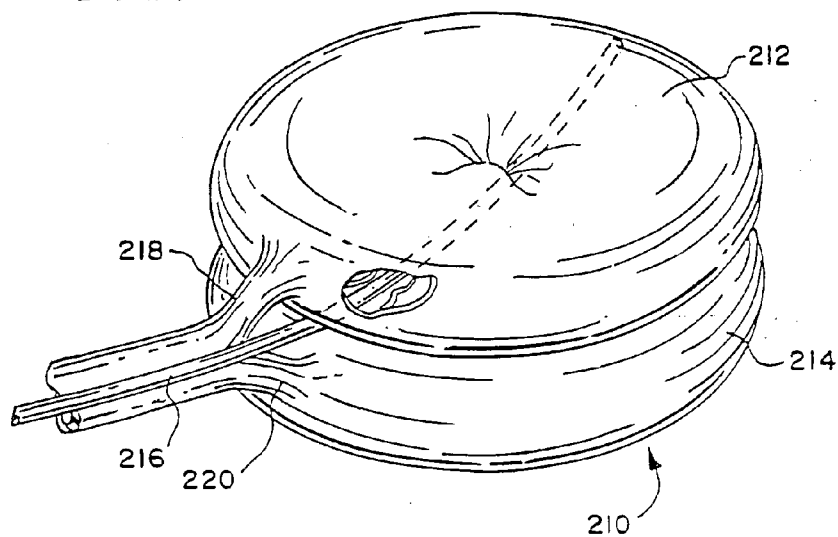


FIG. 22

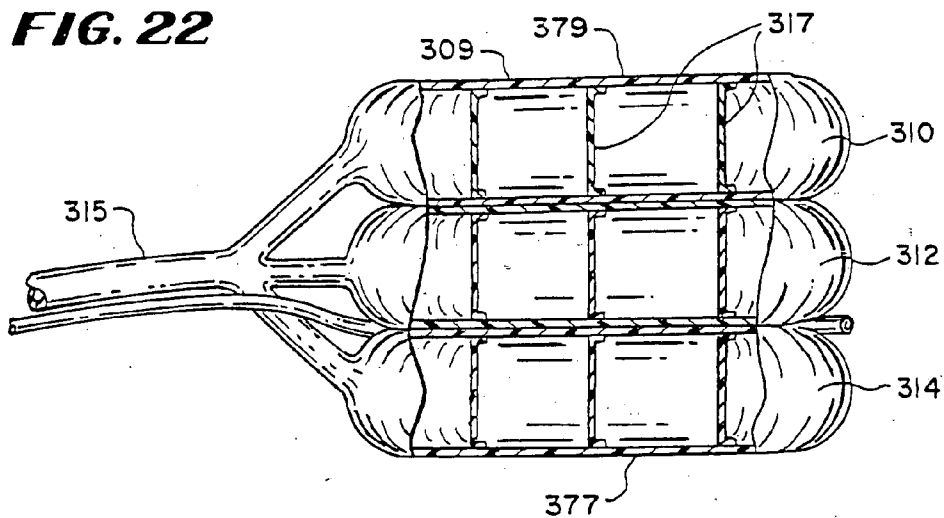


FIG. 23

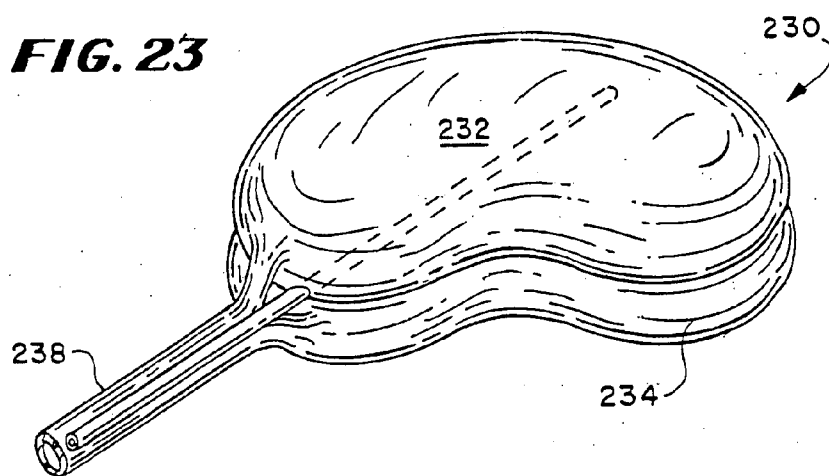


FIG. 24

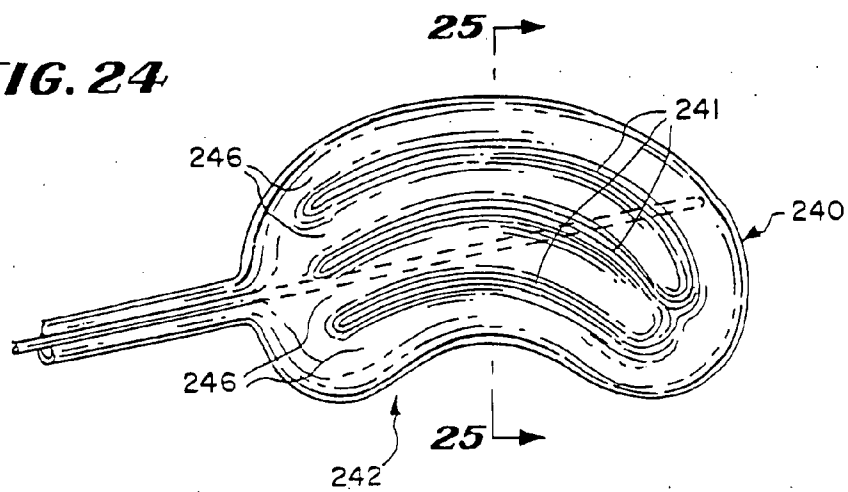


FIG. 25

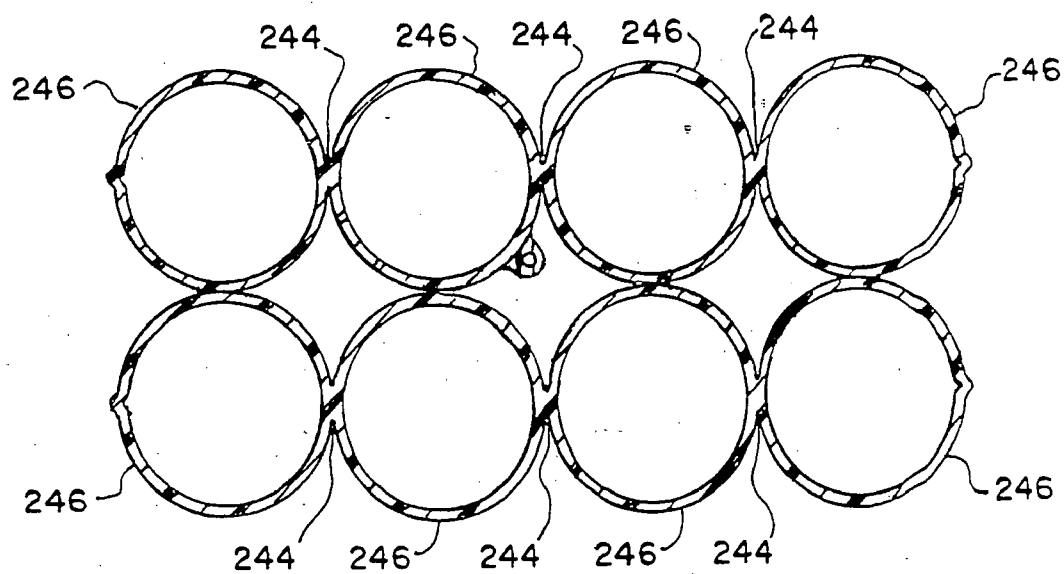


FIG. 26

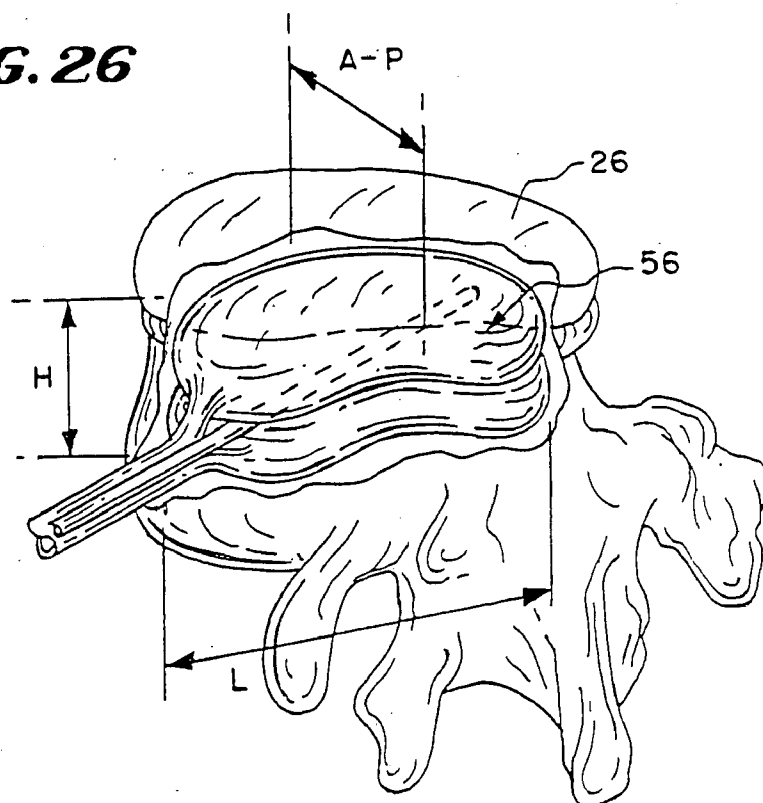


FIG. 27

FIG. 28

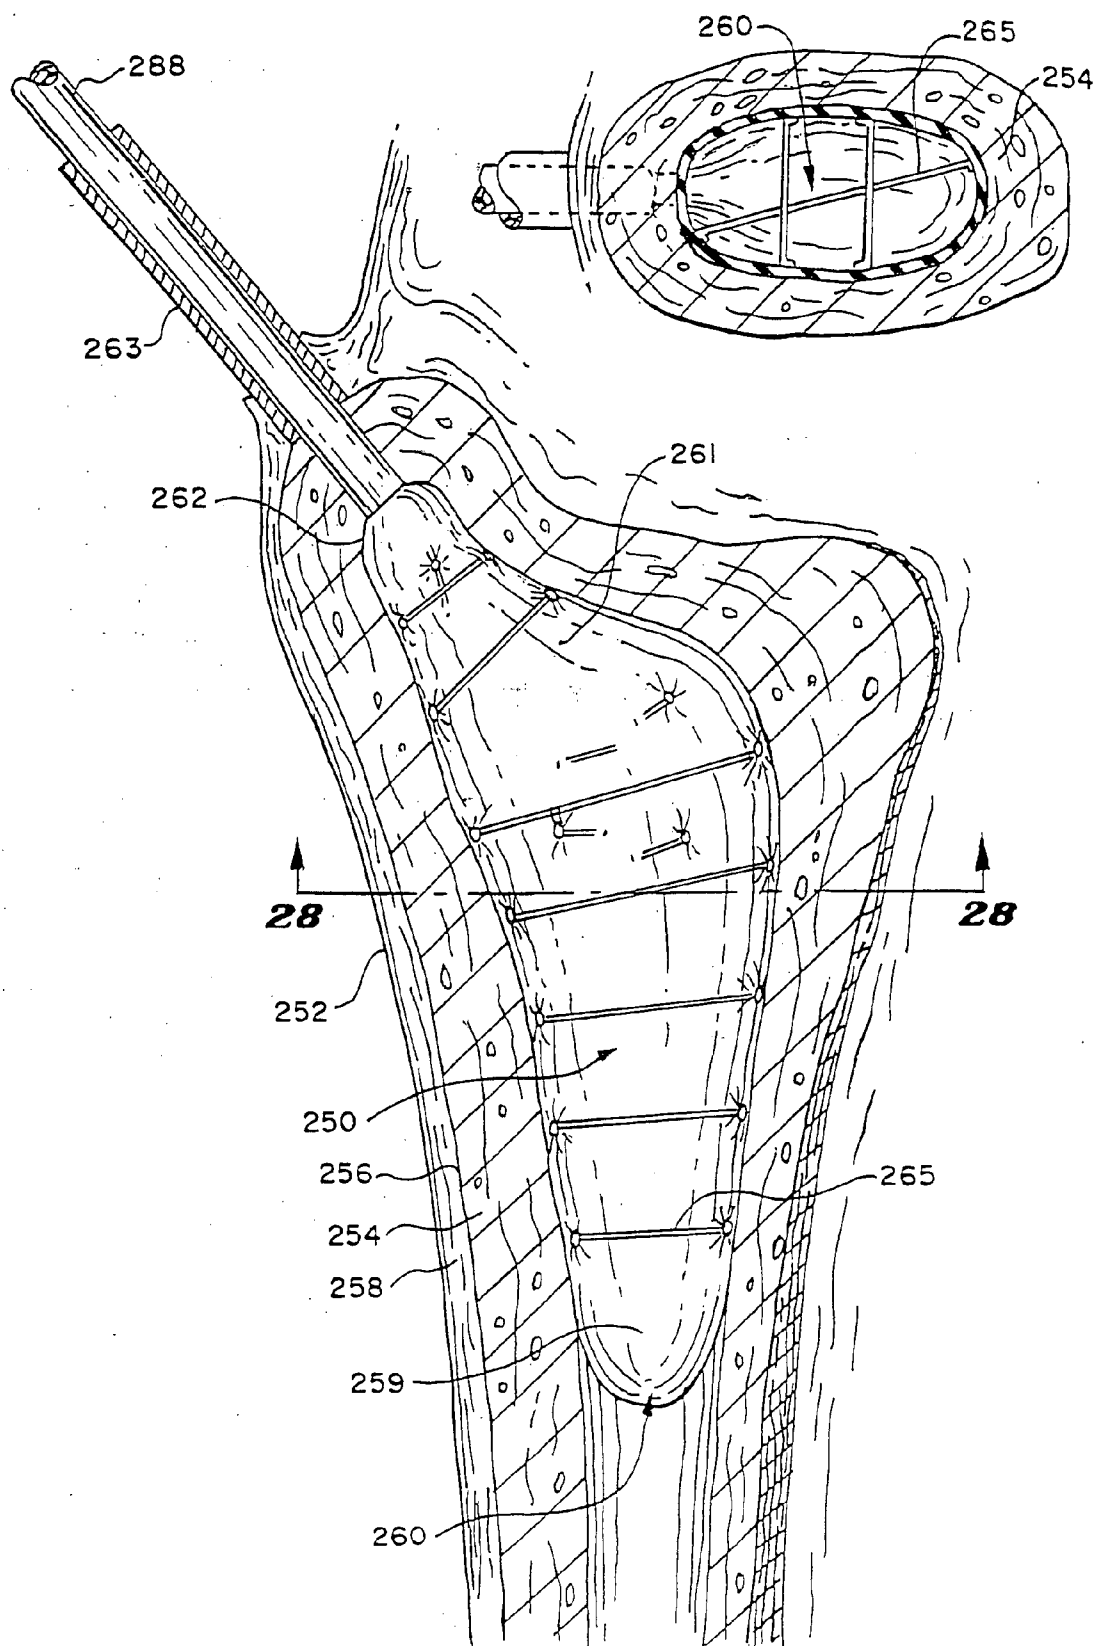


FIG. 29A

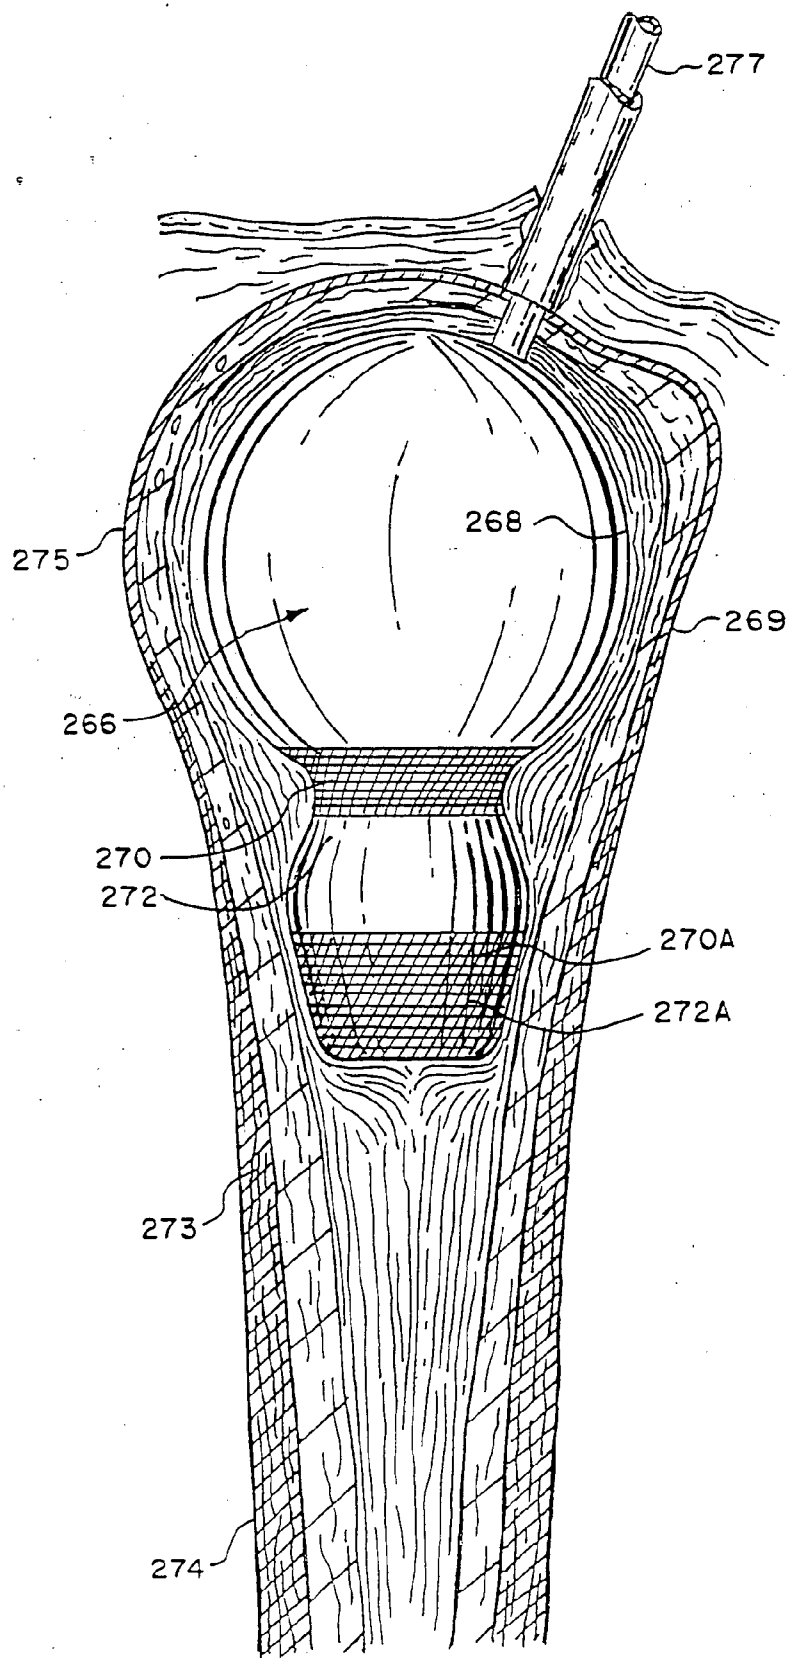


FIG. 29B

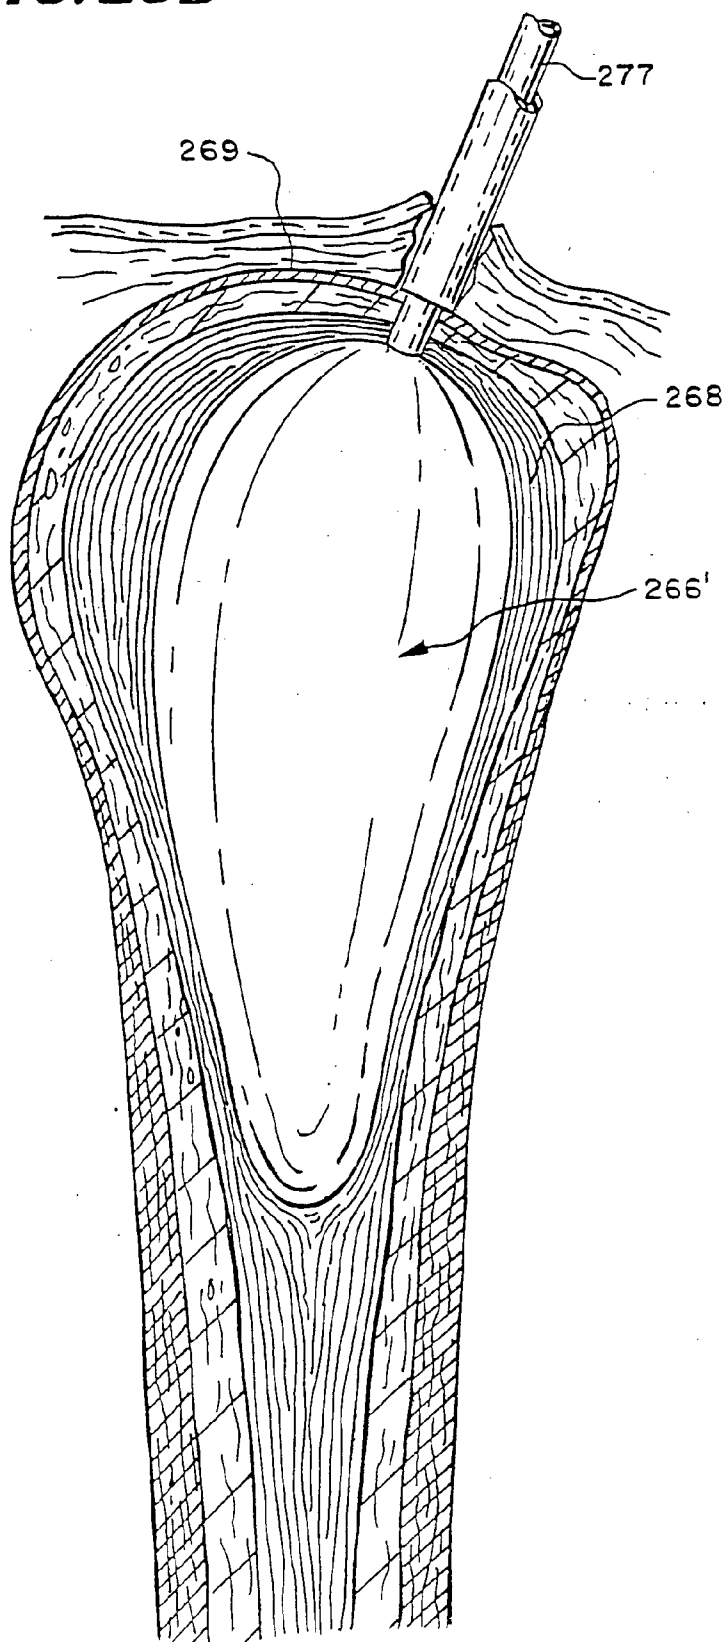


FIG. 30A

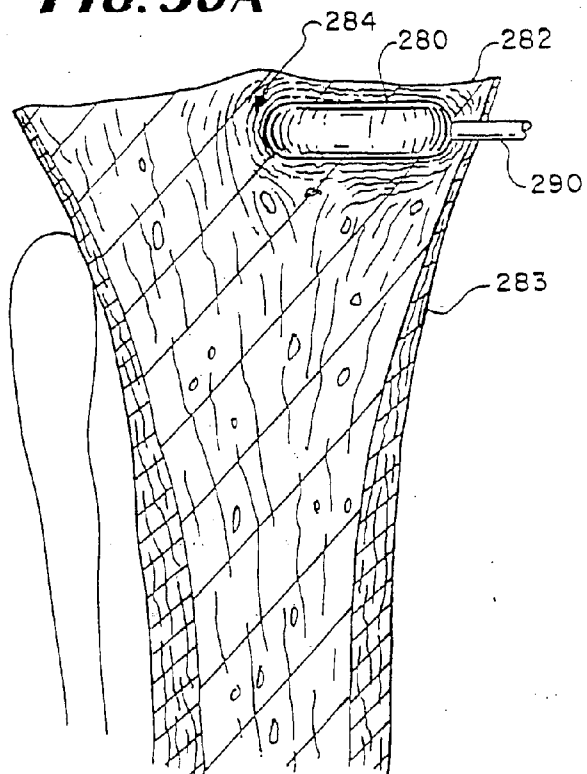


FIG. 30B

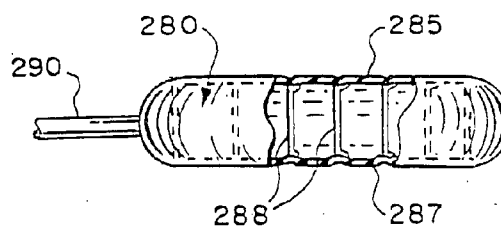


FIG. 31

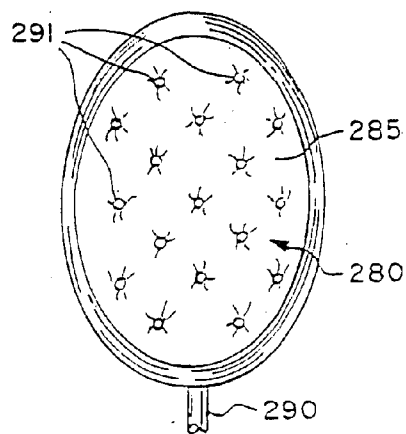


FIG. 30C

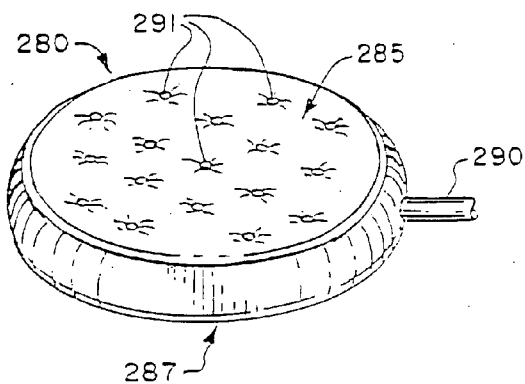


FIG. 32

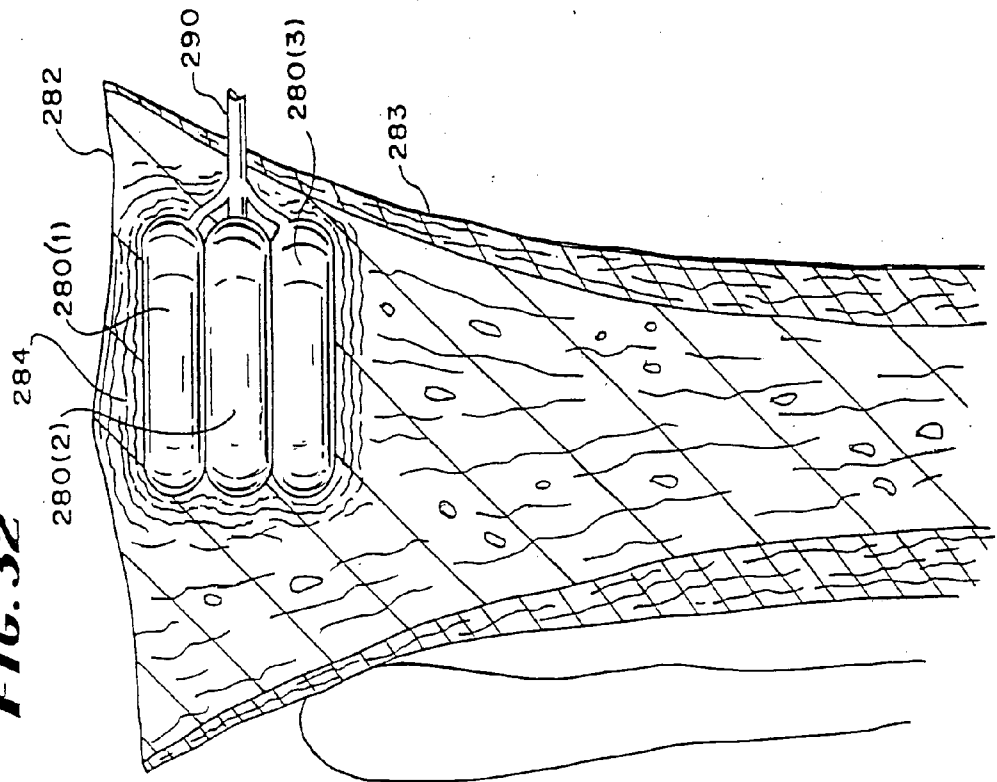


FIG. 33

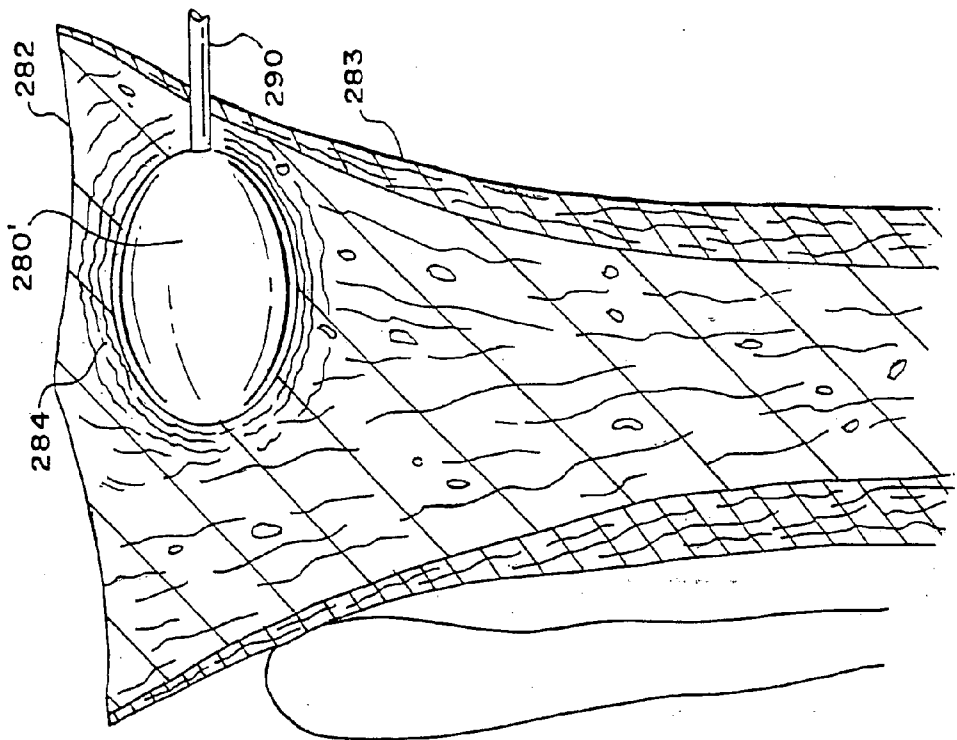


FIG. 34

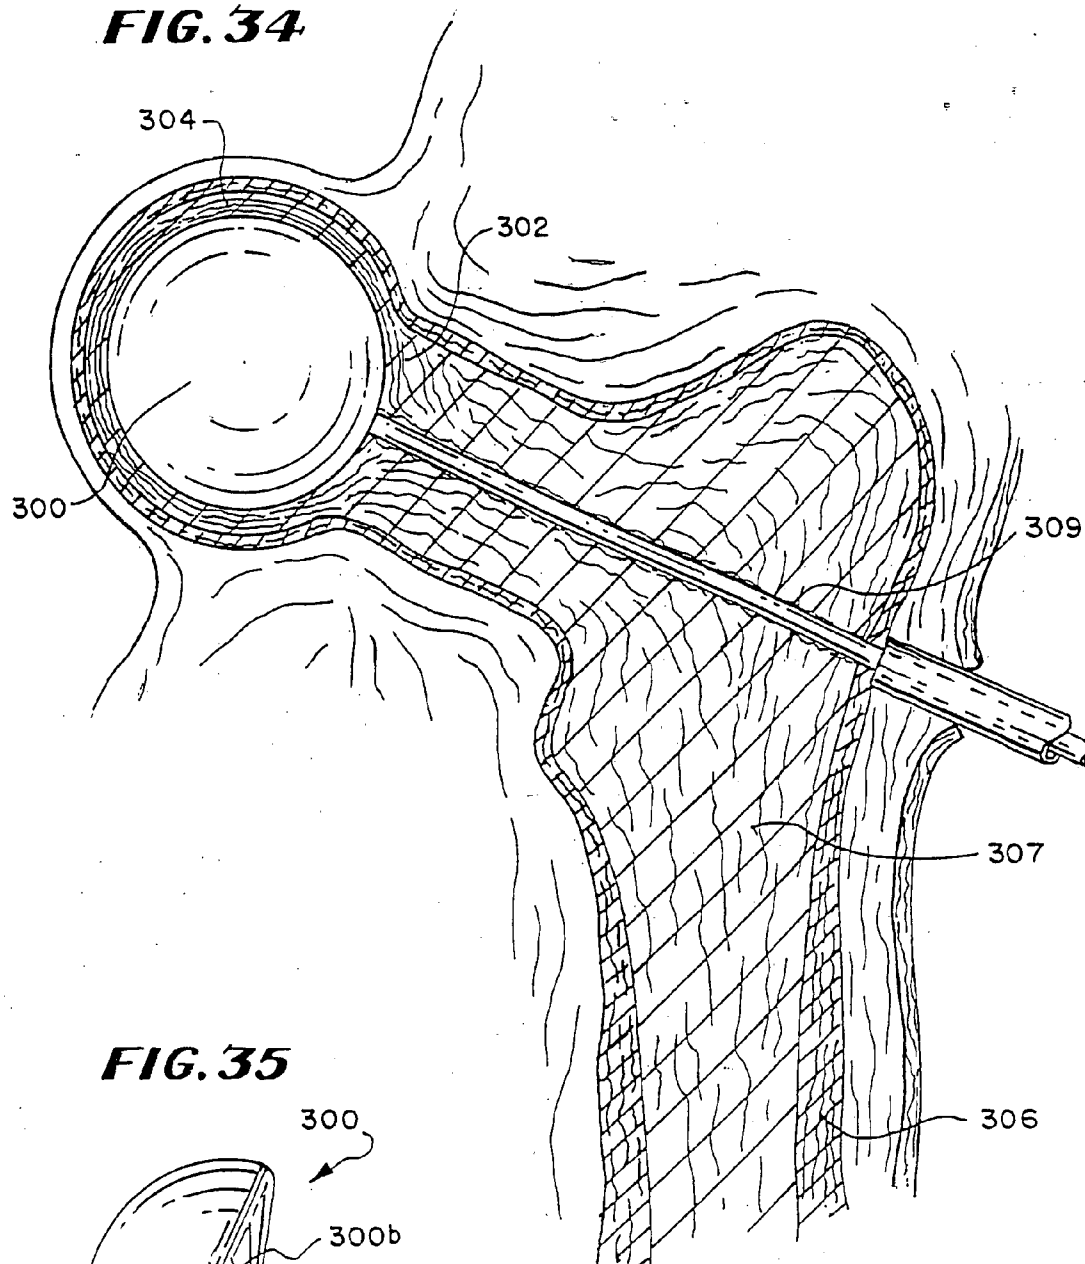


FIG. 35

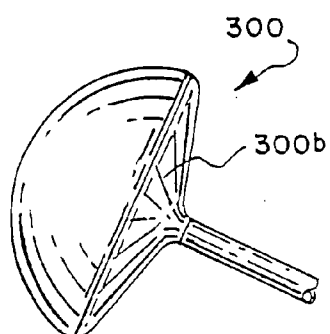


FIG. 36A

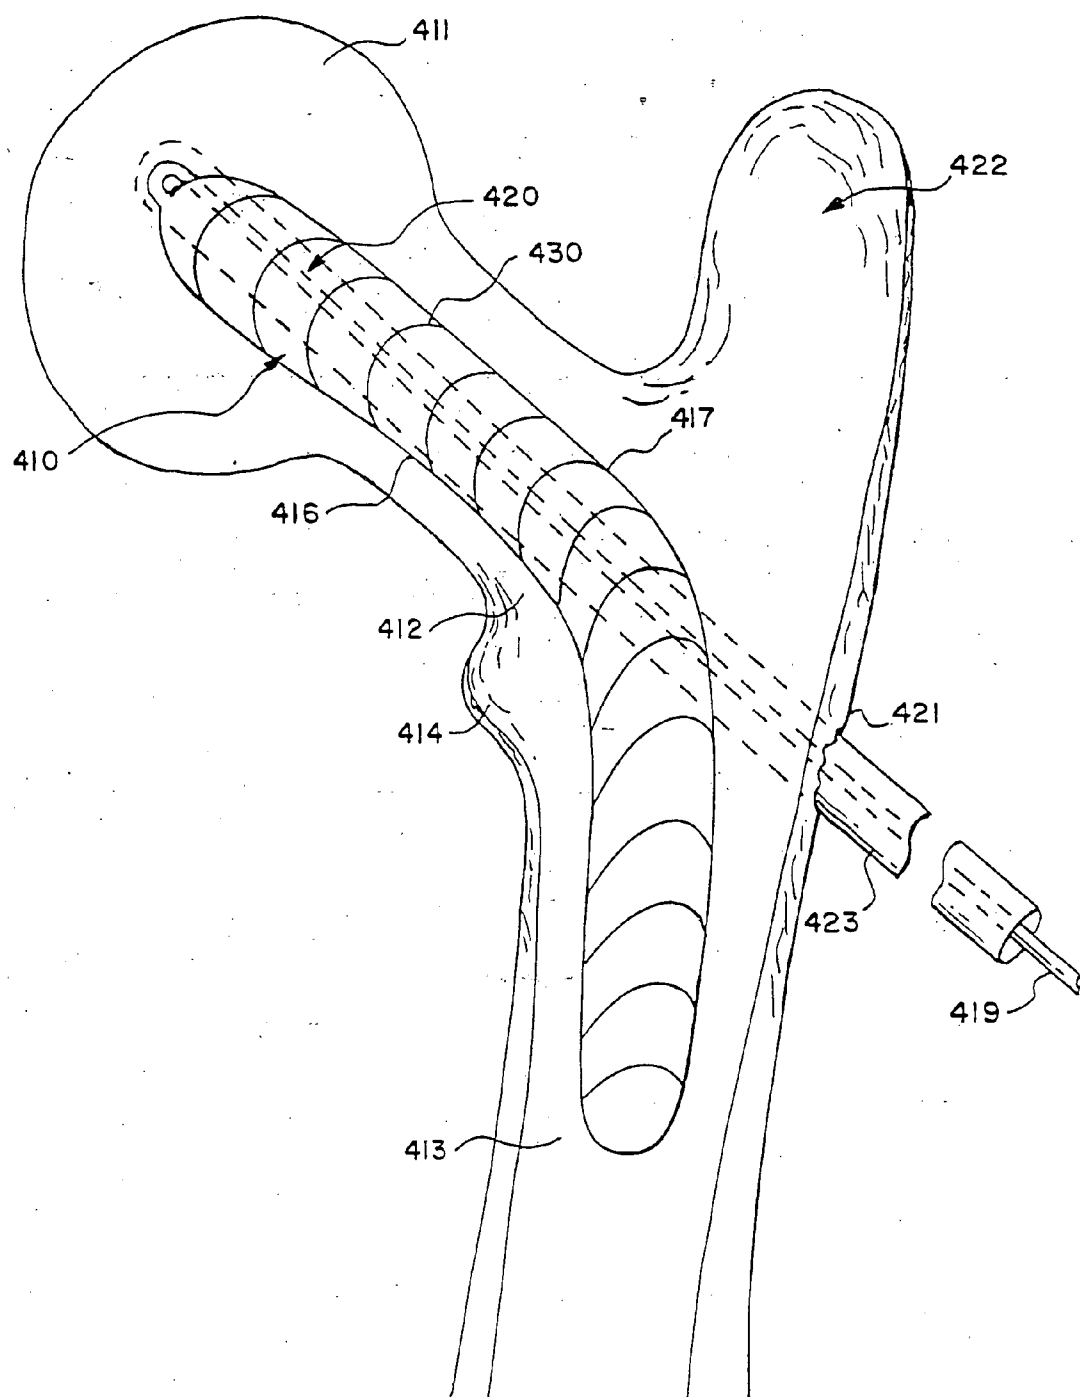


FIG. 36B

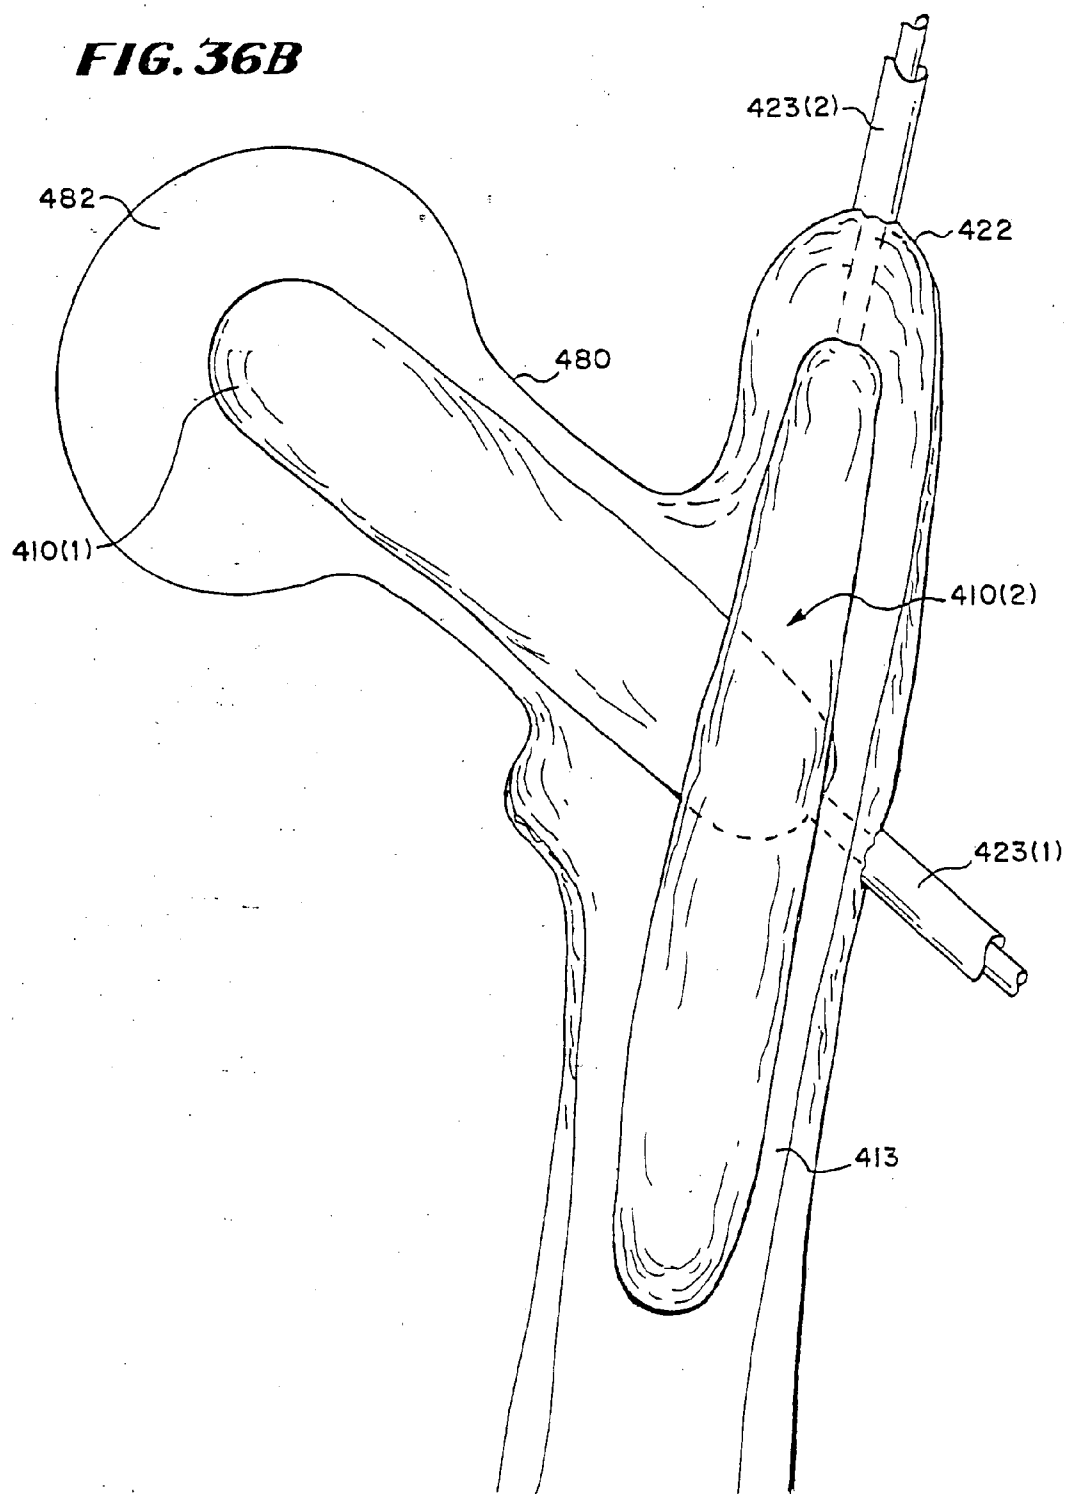


FIG. 37A

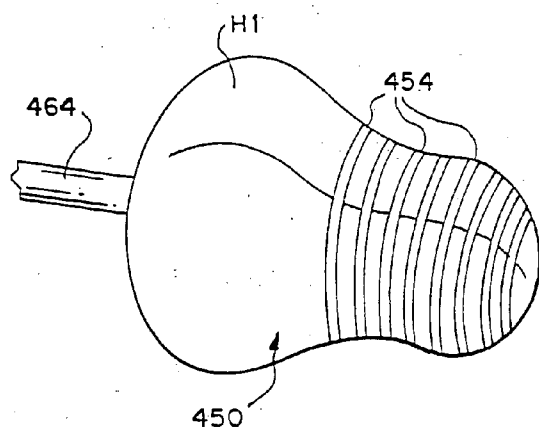
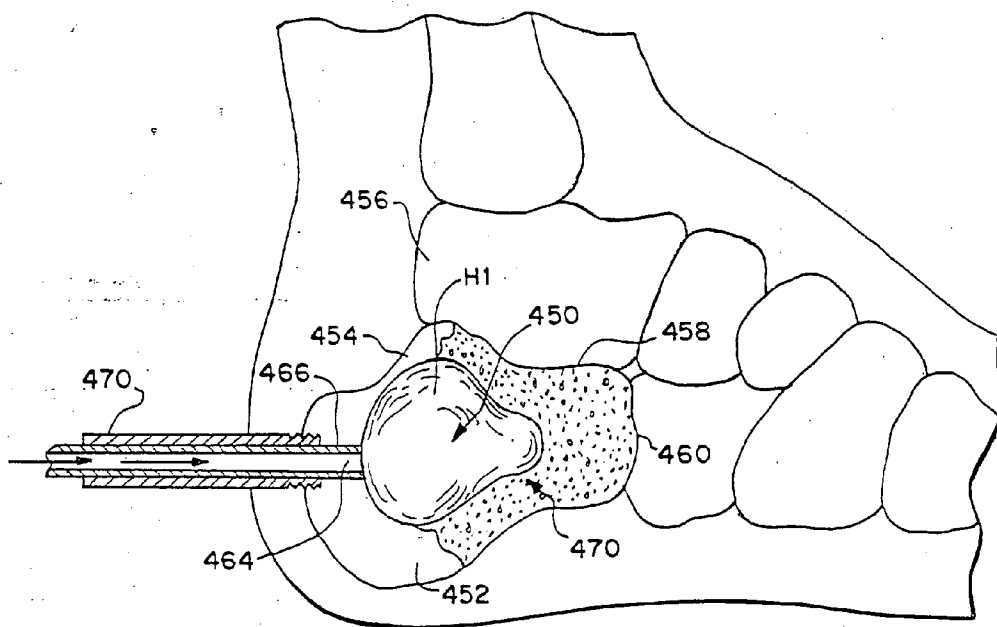


FIG. 37B

FIG. 38

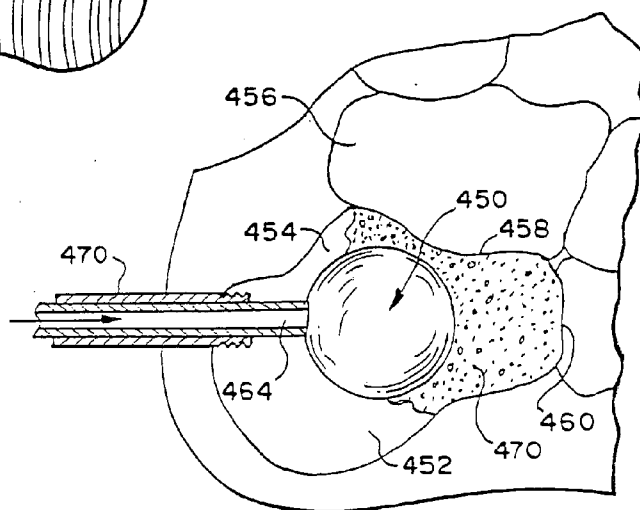


FIG. 39A

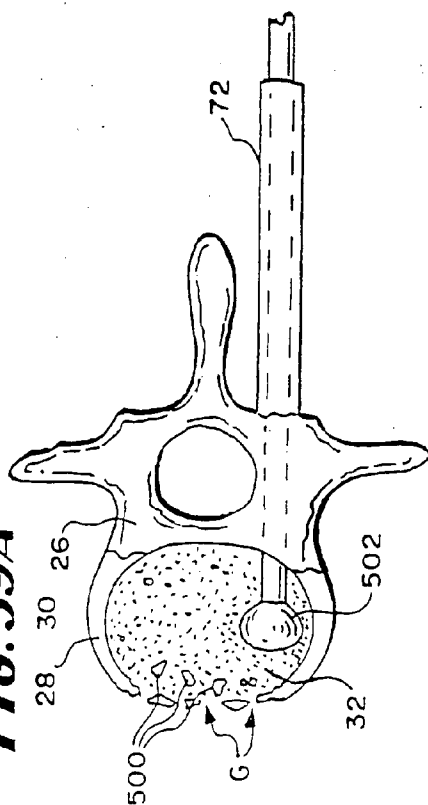


FIG. 39B

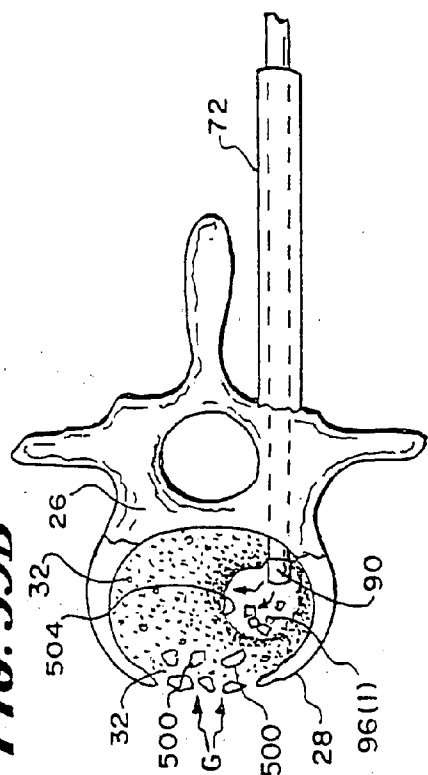


FIG. 39C

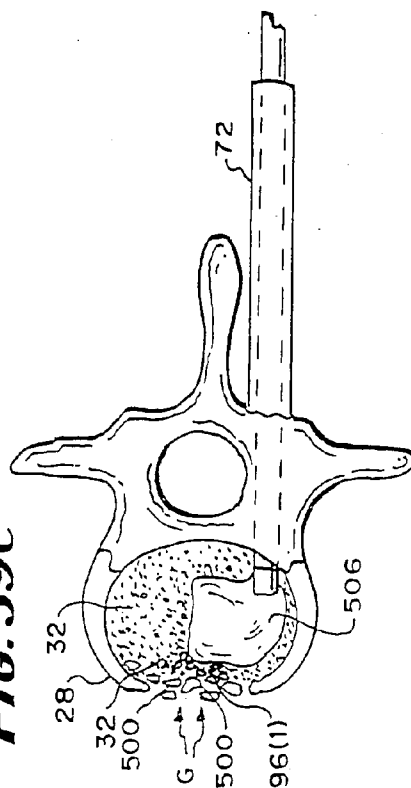


FIG. 39D

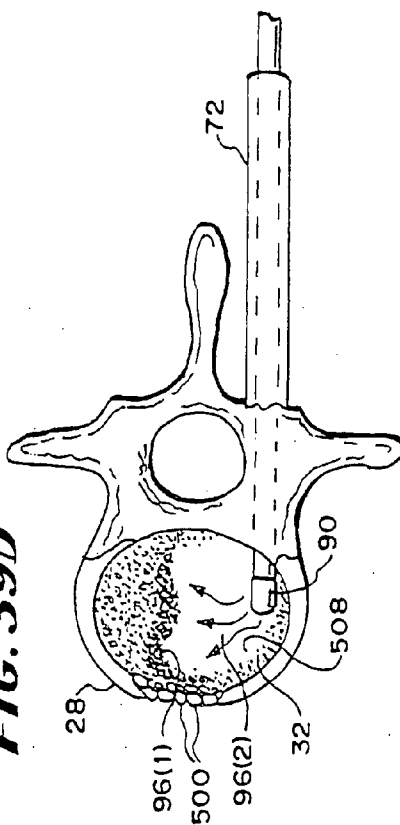


FIG. 41

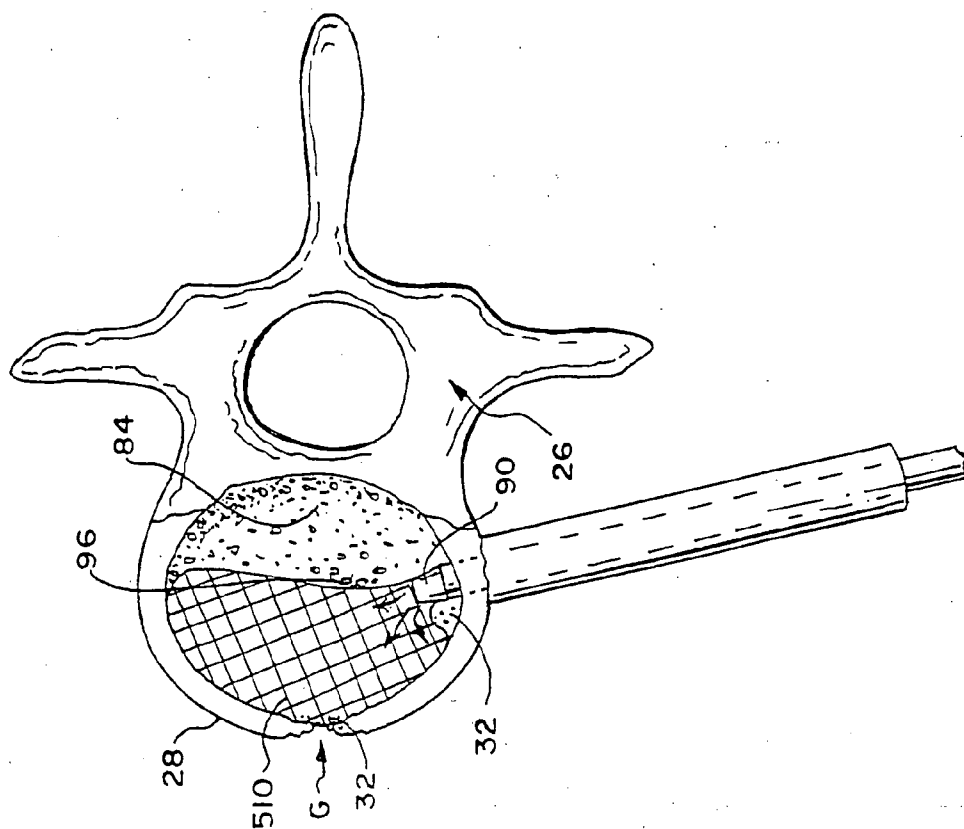


FIG. 40

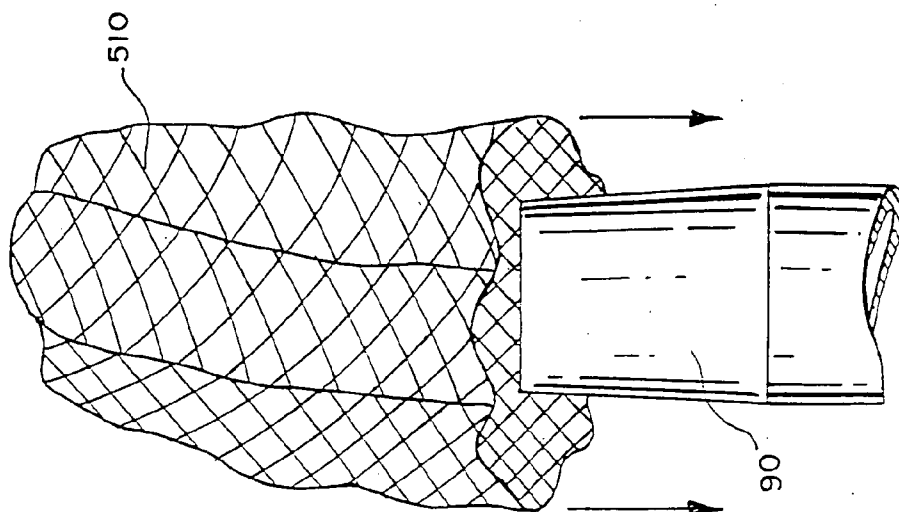


FIG. 42A

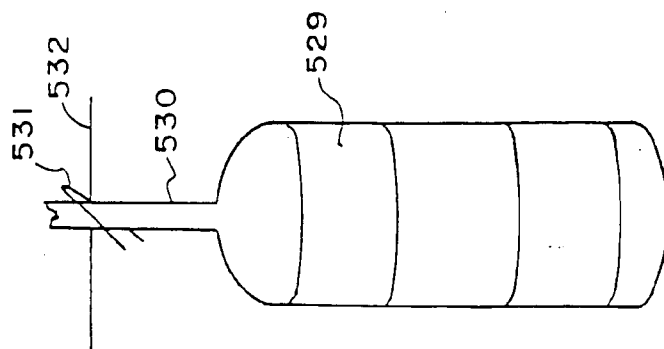


FIG. 42B

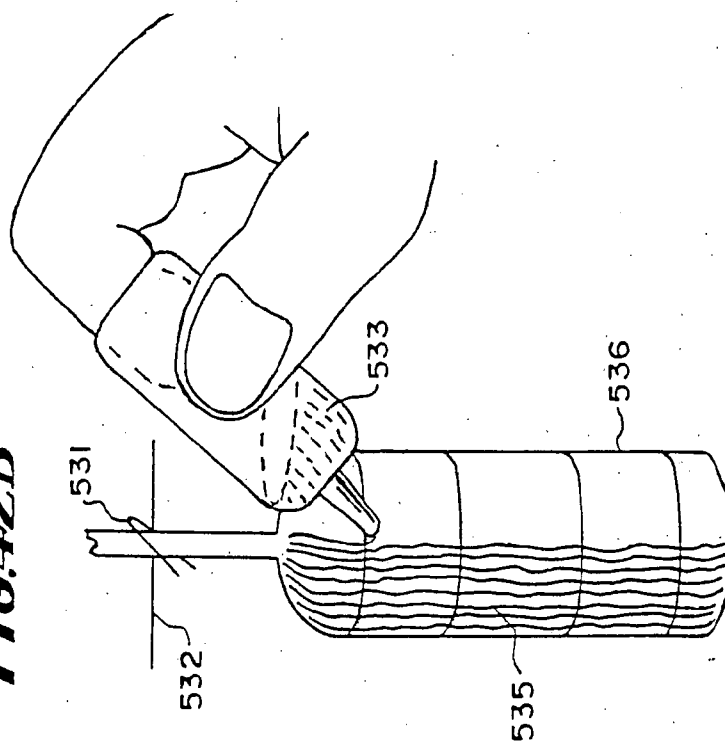


FIG. 42C

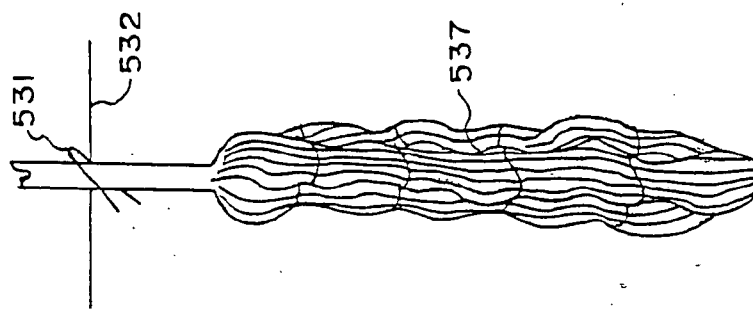


FIG. 43

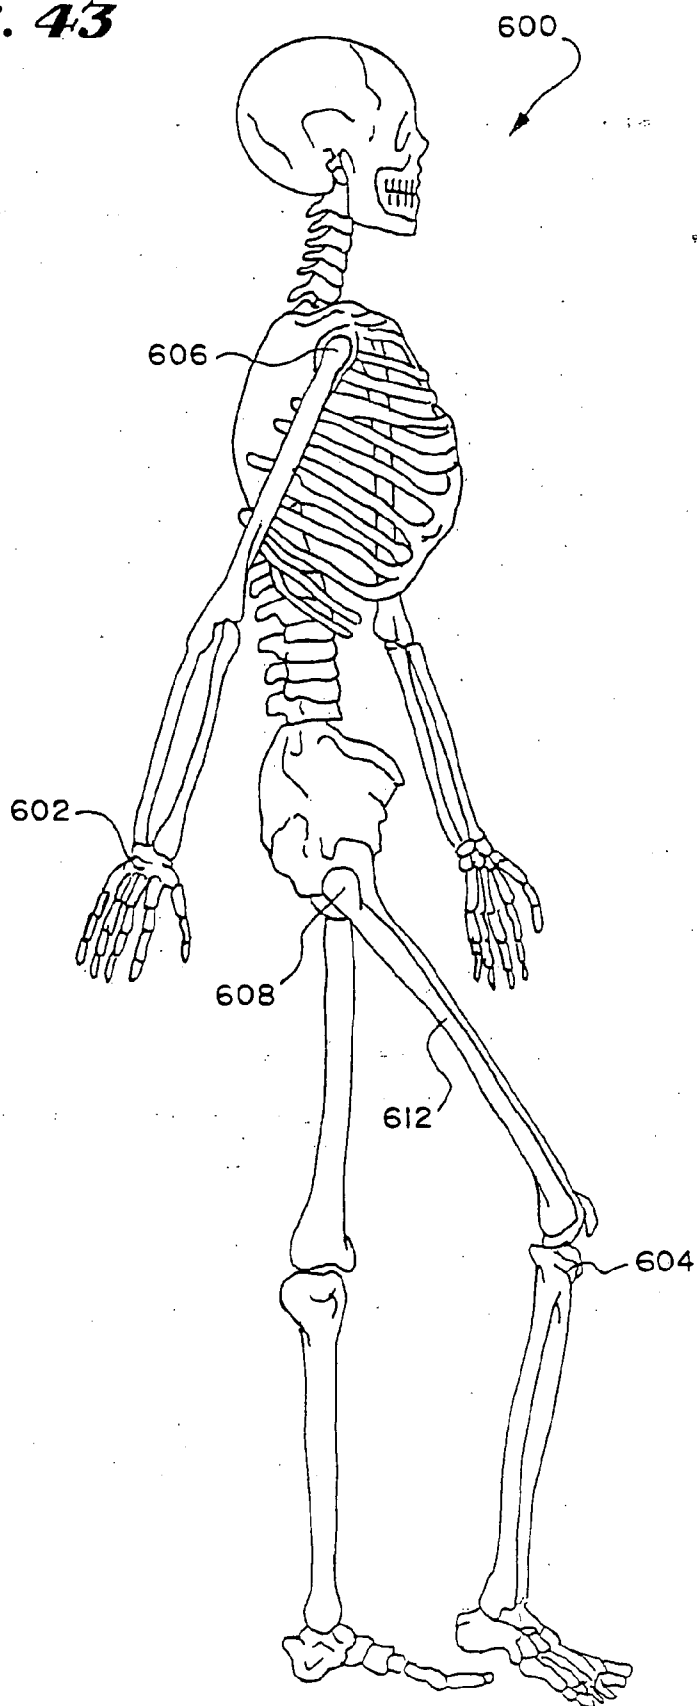


FIG. 44

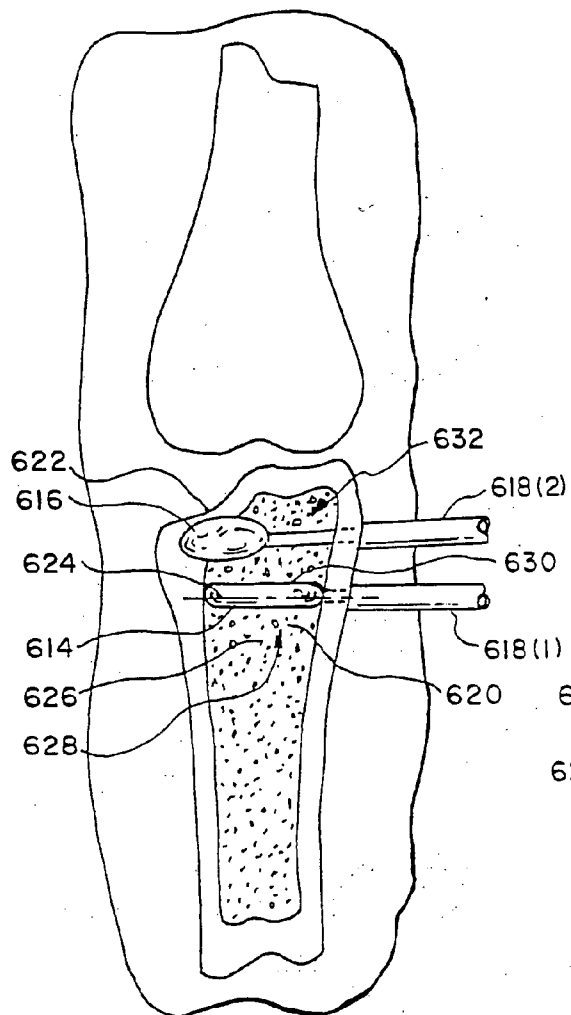


FIG. 45

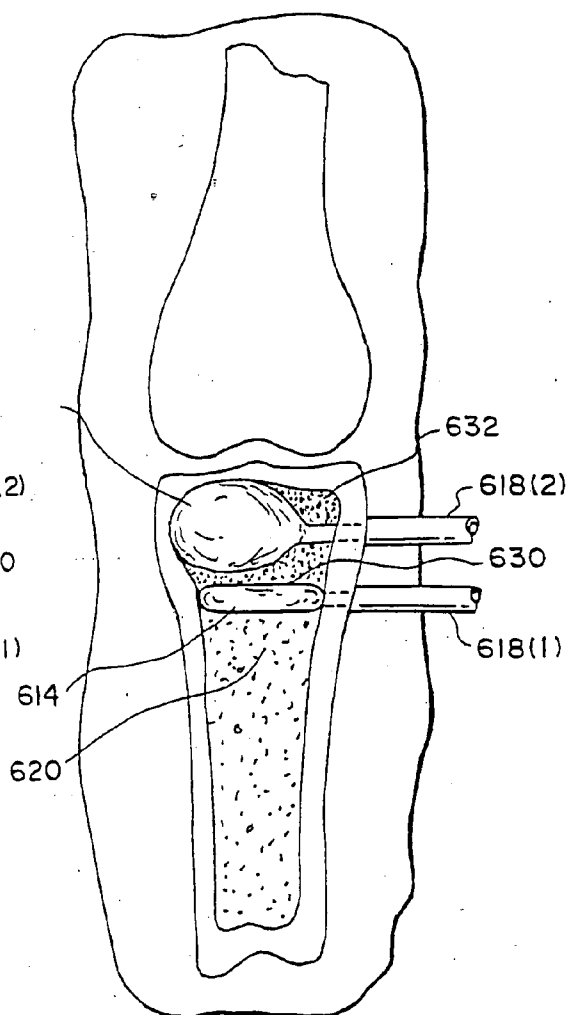


FIG. 46

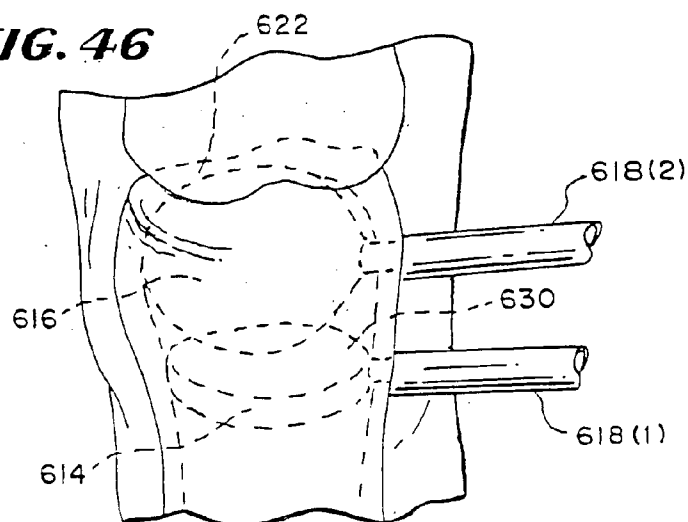


FIG. 47

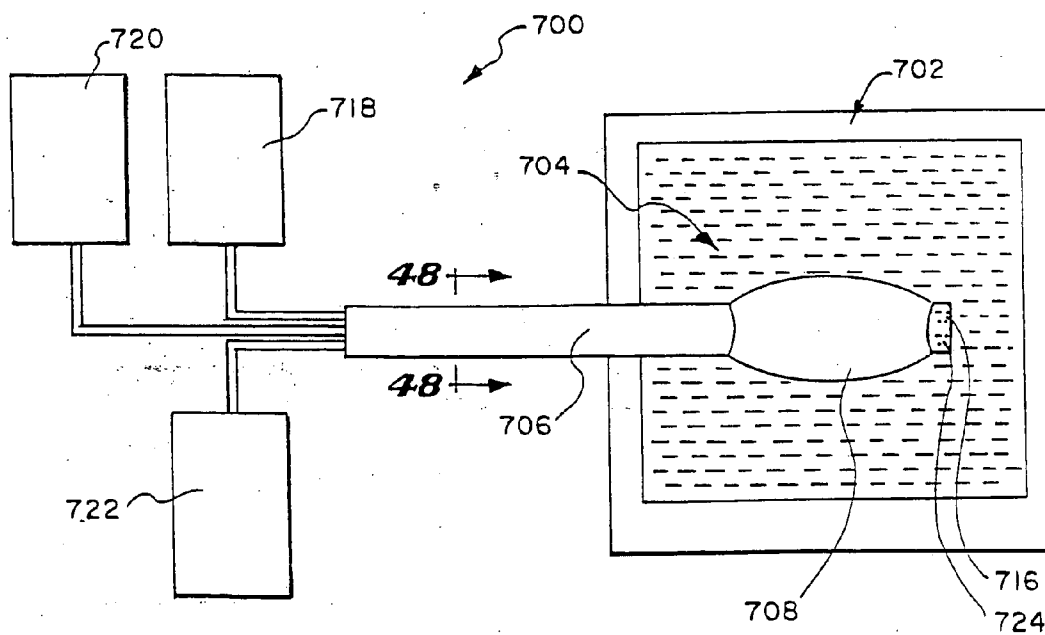


FIG. 48





FIG. 49

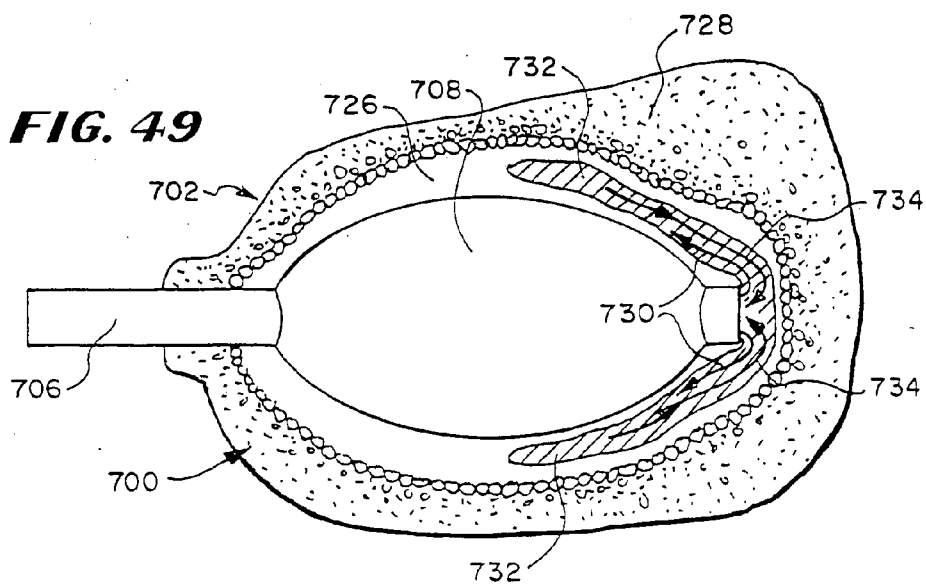

SYSTEMS AND METHODS FOR TREATING BONE USING EXPANDABLE BODIES

RELATED APPLICATIONS

[0001] This application is a divisional of co-pending U.S. patent application Ser. No. 11/528,163, filed 27 Sep. 2006, and entitled "Systems and Methods for Removing Tissue from a Cancellous Bone Volume," which is a divisional of U.S. patent application Ser. No. 10/958,600, filed 5 Oct. 2004, and entitled "Systems and Methods for Treating Fractured or Diseased Bone Using Expandable Bodies," which is a divisional of U.S. patent application Ser. No. 09/754,451, filed 4 Jan. 2001 (now U.S. Pat. No. 6,899,719), which is a continuation of U.S. patent application Ser. No. 08/871,114, filed 9 Jun. 1997 (now U.S. Pat. No. 6,248,110), which is a continuation-in-part of U.S. patent application Ser. No. 08/659,678, filed Jun. 5, 1996 (now U.S. Pat. No. 5,827,289), which is a continuation-in-part of U.S. patent application Ser. No. 08/485,394, filed Jun. 7, 1995 (now abandoned), which is a continuation-in-part of U.S. patent application Ser. No. 08/188,224, filed Jan. 26, 1994 (now abandoned), each of which is incorporated herein by reference.

FIELD OF THE INVENTION

[0002] The invention relates to the treatment of bone conditions in humans and other animals.

BACKGROUND OF THE INVENTION

[0003] When cancellous bone becomes diseased, for example, because of osteoporosis, avascular necrosis, or cancer, the surrounding cortical bone becomes more prone to compression fracture or collapse. This is because the cancellous bone no longer provides interior support for the surrounding cortical bone.

[0004] There are 2 million fractures each year in the United States, of which about 1.3 million are caused by osteoporosis alone. There are also other bone disease involving infected bone, poorly healing bone, or bone fractured by severe trauma. These conditions, if not successfully treated, can result in deformities, chronic complications, and an overall adverse impact upon the quality of life.

[0005] U.S. Pat. Nos. 4,969,888 and 5,108,404 disclose apparatus and methods for the fixation of fractures or other conditions of human and other animal bone systems, both osteoporotic and non-osteoporotic. The apparatus and methods employ an expandable body to compress cancellous bone and provide an interior cavity. The cavity receives a filling material, which hardens and provides renewed interior structural support for cortical bone.

[0006] The better and more efficacious treatment of bone disease that these Patents promise can be more fully realized with improved systems and methods for making and deploying expandable bodies in bone.

SUMMARY OF THE INVENTION

[0007] The invention provides improved systems and methods for treating bone, including vertebral bodies, as well as in other bone types, using one or more expandable bodies.

[0008] One aspect of the invention provides systems and methods that create a cavity in a cancellous bone volume within a vertebral body using an expandable device. The systems and methods place a filling material including a biomaterial within the cavity.

[0009] The filling material can also comprise bone cement.

[0010] The expandable device can expand by inflation and comprise, e.g., a balloon.

[0011] Features and advantages of the inventions are set forth in the following Description and Drawings, as well as in the appended Claims.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] FIG. 1 is a side view of the spinal column of a human;

[0013] FIG. 2 is coronal view of a lumbar vertebra, partially cut away and in section, taken generally along line 2-2 in FIG. 1;

[0014] FIG. 3 is a vertical section of lumbar vertebrae;

[0015] FIG. 4 is a plan view of a probe including a catheter tube carrying an expandable body intended to treat bone;

[0016] FIGS. 5A to 5P are a series of coronal views of a vertebra, partially cut away and in section, showing the steps of introducing, via transpedicular access, an expandable body to compress cancellous bone and create a cavity within a vertebral body, and of then conveying a filling material into the cavity to restore interior integrity to cortical bone;

[0017] FIG. 5Q is a lateral view, with parts broken away, of the vertebra shown in coronal view in FIG. 5P;

[0018] FIG. 6 is a coronal view of a vertebral body in which an expandable body, restrained by an external sealing element, compresses cancellous bone to form a cavity;

[0019] FIG. 7 is a coronal view, partially broken away and in section, of a vertebral body in which an expandable body is being collapsed after having formed a cavity, while an injector tip, also within the vertebral body, is simultaneously injecting filling material into the cavity;

[0020] FIG. 8A is a coronal view of a vertebral body, partially broken away and in section, showing a tool that integrates an injector tube and an integral expandable body to create a cavity in cancellous bone, and also showing the injection of filling material simultaneous with collapse of the expandable body;

[0021] FIG. 8B is a side view of the tool shown in FIG. 8A, located outside bone;

[0022] FIG. 8C is sectional view of the tool shown in FIG. 8B, taken generally along line 8C-8C in FIG. 8B;

[0023] FIG. 9 is a coronal view of a vertebral body showing multiple expandable bodies separately introduced by transpedicular approach;

[0024] FIG. 10 is a view of the distal end of a probe in which two catheter tubes, each carrying an expandable body, are joined to form a symmetric array, when substantially expanded outside a bone;

[0025] FIG. 11 is a view of the distal end of a probe in which two catheter tubes, each carrying an expandable body, are joined to form an asymmetric array, when substantially expanded outside a bone;

[0026] FIG. 12 is a coronal view, partially broken away and in section, of a vertebral body into which multiple expandable bodies have been deployed by dual transpedicular access;

[0027] FIG. 13 is a coronal view of a vertebral body, partially broken away and in section, into which multiple expandable bodies have been deployed by contralateral posterolateral access;

[0028] FIG. 14 is a coronal view of a vertebral body, partially broken away and in section, in which multiple expandable bodies have formed multiple cavities which join to form a single cavity to receive filling material;

[0029] FIG. 15 is a coronal view of a vertebral body, partially broken away and in section, in which multiple expandable bodies have formed multiple separate cavities to receive filling material;

[0030] FIG. 16 is an anterior-posterior view of a region of the spine, showing multiple expandable bodies present within a targeted vertebral body using ipsilateral posterolateral access;

[0031] FIG. 17 is an anterior-posterior view of a vertebral body, partially broken away and in section, in which multiple expandable bodies, introduced using ipsilateral posterolateral access, have formed multiple cavities which are joined to form a single cavity to receive filling material;

[0032] FIG. 18 is an anterior-posterior view of a vertebral body, partially broken away and in section, in which multiple expandable bodies, introduced using an ipsilateral posterolateral access, have formed multiple separate cavities to receive filling material;

[0033] FIG. 19 is a coronal view of a vertebral body, partially broken away and in section, in which multiple expandable bodies have been introduced by both transpedicular and posterolateral access;

[0034] FIG. 20 is a perspective view of one representative embodiment of an expandable body having a stacked doughnut-shaped geometry;

[0035] FIG. 21 is a view of another representative embodiment of an expandable body having an oblong-shaped geometry;

[0036] FIG. 22 is an elevation view of another representative embodiment of an expandable body showing three stacked bodies and string-like restraints for limiting the expansion of the bodies during inflation;

[0037] FIG. 23 is a perspective view of another representative embodiment of an expandable body having a kidney bean-shaped geometry;

[0038] FIG. 24 is a top view of another representative embodiment of an expandable body having a kidney bean-shaped geometry with several compartments by a heating element or branding tool;

[0039] FIG. 25 is a cross-sectional view taken along line 25-25 of FIG. 24;

[0040] FIG. 26 is a perspective, lateral view of a vertebral body, partially broken away to show the presence of an expandable body, and also showing the major reference dimensions for the expandable body;

[0041] FIG. 27 is a dorsal view of a representative expandable body having a humpback banana-shaped geometry in use in a right distal radius;

[0042] FIGS. 28 is a cross sectional view of the expandable body shown in FIG. 27, taken generally along line 28-28 of FIG. 27;

[0043] FIG. 29A is a representative expandable body having a spherical shape with a base, located in a proximal humerus and viewed from the front (anterior) of the left proximal humerus;

[0044] FIG. 29B is a representative expandable body having a cylindrical shape, located in a proximal humerus and viewed from the front (anterior) of the left proximal humerus;

[0045] FIG. 30A is a representative embodiment of an expandable body located, as shown in a front (anterior) view of the proximal tibia, introduced beneath the medial tibial plateau;

[0046] FIG. 30B is a side elevation view of the expandable body shown in FIG. 30A;

[0047] FIG. 30C is a top perspective view of the expandable body shown in FIG. 30A, showing its generally cylindrical geometry;

[0048] FIG. 31 is a top plan view of another representative embodiment of an expandable body for use in treating tibial plateau fractures, having a generally elliptical geometry;

[0049] FIG. 32 is a side view of multiple expandable bodies stacked on atop another for use, for example, in treating tibial plateau fractures;

[0050] FIG. 33 is another representative embodiment of an expandable body having an egg-shaped geometry located, as shown in a front (anterior) view of the proximal tibia, introduced beneath the medial tibial plateau;

[0051] FIG. 34 is a representative embodiment of an expandable body having a spherical-shaped geometry for treating avascular necrosis of the head of the femur (or humerus), which is shown from the front (anterior) of the left hip;

[0052] FIG. 35 is a side view of another representative embodiment of an expandable body having a hemispherically-shaped geometry for treating avascular necrosis of the head of the femur (or humerus);

[0053] FIG. 36A is a view of a representative expandable body having a bent-geometry for preventing hip fracture, as seen from the front (anterior) of the left hip;

[0054] FIG. 36B is a view of multiple expandable bodies individually deployed through multiple access points into the left hip for preventing hip fracture;

[0055] FIG. 37A is a view of a representative expandable body having an asymmetric bow tie-shape for use in treating fracture of the calcaneus bone, shown in lateral view within the calcaneus;

[0056] FIG. 37B is a perspective top view of the expandable body shown in FIG. 37A when substantially expanded outside the calcaneus;

[0057] FIG. 38 shows a representative embodiment of an expandable body having a spherical or egg-shaped geometry shown in lateral view deployed within the calcaneus;

[0058] FIGS. 39A to 39D show a multiple stage process of introducing filling material into a cavity formed by an expandable body in cancellous bone, to prevent or impede flow or seepage of filling material from the interior of the bone;

[0059] FIG. 40 is an elevation view of an injector tip for filling material, over which a mesh is draped, which, when deployed in a cavity formed by an expandable body, impedes or prevents seepage of the material from the cavity;

[0060] FIG. 41 is a coronal view of a vertebra, with parts broken away and in section, showing the deployment of the mesh shown in FIG. 40 within the vertebral body;

[0061] FIGS. 42A to 42C are schematic illustrations of a representative method and system for delivering a therapeutic substance to a bone using an expandable body;

[0062] FIG. 43 is an illustration of the human skeleton, showing regions of long bone that can be treated using expandable bodies;

[0063] FIG. 44 is a representative embodiment of multiple expandable bodies located, as shown in a front (anterior) view, within the proximal tibia, both introduced beneath the medial tibial plateau, one of the bodies being substantially expanded to form an interior barrier and serve as a platform for the other body, which is shown substantially collapsed;

[0064] FIG. 45 is a front (anterior) view of the multiple expandable bodies, shown in FIG. 44, with both bodies in substantially expanded conditions to form a cavity within the proximal tibia beneath the medial tibial plateau;

[0065] FIG. 46 is an enlarged front (anterior) perspective view of the multiple expandable bodies shown in FIG. 45, with the lower expandable body serving as a platform for the upper expandable body;

[0066] FIG. 47 is diagrammatic view of a system for harvesting bone marrow in a bone-marrow producing bone using an expandable body;

[0067] FIG. 48 is a section view of the catheter tube associated with the system shown in FIG. 48, taken generally along line 48-48 of FIG. 47; and

[0068] FIG. 49 is an enlarged view of the expandable body associated with the system shown in FIG. 47 inside a bone for the purpose of harvesting bone marrow.

[0069] The invention may be embodied in several forms without departing from its spirit or essential characteristics. The scope of the invention is defined in the appended claims, rather than in the specific description preceding them. All embodiments that fall within the meaning and range of equivalency of the claims are therefore intended to be embraced by the claims.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0070] This Specification describes new systems and methods to treat bones using expandable bodies. The use of

expandable bodies to treat bones is disclosed in U.S. Pat. Nos. 4,969,888 and 5,108,404, which are incorporated herein by reference. Improvements in this regard are disclosed in U.S. patent application, Ser. No. 08/188,224, filed Jan. 26, 1994; U.S. patent application Ser. No. 08/485,394, filed Jun. 7, 1995; and U.S. patent application Ser. No. 08/659,678, filed Jun. 5, 1996, which are each incorporated herein by reference.

[0071] The new systems and methods will be first described with regard to the treatment of vertebra. It should be appreciated, however, the systems and methods so described are not limited in their application to vertebrae. As will be described in greater detail later, the systems and methods are applicable to the treatment of diverse bone types.

[0072] I. Treatment of Vertebral Bodies

[0073] As FIG. 1 shows, the spinal column 10 comprises a number of uniquely shaped bones, called the vertebrae 12, a sacrum 14, and a coccyx 16 (also called the tail bone). The number of vertebrae 12 that make up the spinal column 10 depends upon the species of animal. In a human (which FIG. 1 shows, there are twenty-four vertebrae 12, comprising seven cervical vertebrae 18, twelve thoracic vertebrae 20, and five lumbar vertebrae 22.

[0074] When viewed from the side, as FIG. 1 shows, the spinal column 10 forms an S-shaped curve. The curve serves to support the head, which is heavy. In four-footed animals, the curve of the spine is simpler.

[0075] As FIGS. 1 to 3 show, each vertebra 12 includes a vertebral body 26, which extends on the anterior (i.e., front or chest) side of the vertebra 12. As FIGS. 1 to 3 show, the vertebral body 26 is in the shape of an oval disk. As FIGS. 2 and 3 show, the vertebral body 26 includes an exterior formed from compact cortical bone 28. The cortical bone 28 encloses an interior volume 30 of reticulated cancellous, or spongy, bone 32 (also called medullary bone or trabecular bone). A "cushion," called an intervertebral disk 34, is located between the vertebral bodies 26.

[0076] An opening, called the vertebral foramen 36, is located on the posterior (i.e., back) side of each vertebra 12. The spinal ganglion 39 pass through the foramen 36. The spinal cord 38 passes through the spinal canal 37.

[0077] The vertebral arch 40 surrounds the spinal canal 37. The pedicle 42 of the vertebral arch 40 adjoins the vertebral body 26. The spinous process 44 extends from the posterior of the vertebral arch 40, as do the left and right transverse processes 46.

[0078] A. Deployment of an Expandable Body

[0079] FIG. 4 shows a tool 48 for preventing or treating compression fracture or collapse of a vertebral body using an expandable body.

[0080] The tool 48 includes a catheter tube 50 having a proximal and a distal end, respectively 52 and 54. The distal end 54 carries an expandable body 56.

[0081] The body 56 includes an exterior wall 58, which, in FIG. 4, is shown in a collapsed geometry. The collapsed geometry permits insertion of the body 56 into the interior volume 30 of a targeted vertebral body 26.

[0082] The insertion of the body 56 into the interior volume 30 of a targeted vertebral body 26 can be accomplished in various ways. FIGS. 5A to 5Q show the insertion of the body 56 using a transpedicular approach, which can be performed either with a closed, minimally invasive procedure or with an open procedure.

[0083] In the described procedure, a patient lies on an operating table, while the physician introduces a conventional spinal needle assembly 60 into soft tissue in the patient's back. The patient can lie facedown on the table, or on either side, or at an oblique angle, depending upon the physician's preference. Indeed, the procedure can be performed through an open anterior procedure or an endoscopic anterior procedure, in which case the tool 48 may be introduced from the anterior aspect of the vertebral body.

[0084] The spinal needle assembly 60 comprises a stylet 62 slidable housed within a stylus 64. The assembly 60 typically has, for example, about an 18 gauge diameter. Other gauge diameters can and will be used to accommodate appropriate guide pins, as will be described in greater detail later.

[0085] Under radiologic, CT, or MRI monitoring, the physician advances the assembly 60 through soft tissue (designated S in FIG. 5A) down to and into the targeted vertebra 12, as FIG. 5A shows. The physician will typically administer a local anesthetic, for example, lidocaine, through assembly 60. In some cases, the physician may prefer other forms of anesthesia.

[0086] The physician directs the spinal needle assembly 60 to penetrate the cancellous bone 32 of the targeted vertebra 12. Preferably the depth of penetration is about 60% to 95% of the vertebral body 26.

[0087] FIG. 5A shows gaining access to cancellous bone 32 through the pedicle 42, which is called transpedicular access. However, posterolateral access, through the side of the vertebral body 12 (designated P-L and shown in phantom lines in FIG. 5A), may be indicated, if a compression fracture has collapsed the vertebral body 26 below the plane of the pedicle 42, or for other reasons based upon the preference of the physician.

[0088] After positioning the spinal needle assembly 60 in cancellous bone 32, the physician holds the stylus 64 and withdraws the stylet 62 (see FIG. 5B). Still holding the stylus 64, the physician slides a guide pin 66 through the stylus 64 and into the cancellous bone 32 (see FIG. 5C). The physician now removes the stylus 64, leaving the guide pin 66 deployed within the cancellous bone 32, as FIG. 5D shows.

[0089] As FIG. 5E shows, the physician makes a small incision (designated I in FIG. 5E) in the patient's back to accommodate a trocar 68. The physician inserts the trocar 68 through the soft tissue S along the guide pin 66 down to the pedicle 42. The physician taps the distal end 70 of the trocar 68 into the pedicle 42 to secure its position.

[0090] As FIG. 5P shows, the physician next slides an outer guide sheath 72 over the trocar 68. The distal end 74 of the outer guide sheath 72 is likewise tapped into the pedicle 42. The physician removes the trocar 68, leaving the guide pin 66 and outer guide sheath 72 in place, as FIG. 5G

shows. Alternatively, the trocar 68 and guide sheath 72 can be introduced together in one step.

[0091] As FIG. 5H shows, the physician advances a drill bit 76 (for example, 5 mm in diameter) over the guide pin 66 through the outer guide sheath 72. Under X-ray control (or using another external visualizing system), the physician operates the drill bit 76 to open a passage 78 through the pedicle 42 and into the cancellous bone 32. The drilled passage 78 preferably extends no more than 95% across the vertebral body 26.

[0092] As FIG. 5I shows, the physician removes drill bit 76 and guide pin 66, leaving the outer guide sheath 72. The passage 78 made by the drill bit 76 remains, passing through the pedicle 42 and into the cancellous bone 32.

[0093] As FIG. 5J(1) shows, the physician next advances the catheter tube 50 and expandable body 56 through the outer guide sheath 72 and into the drilled passage 78 in the cancellous bone 32. As best shown in FIG. 5J(2), the body 56 is maintained in a straightened, collapsed condition distally beyond the end of the catheter tube 50 during transport through the guide sheath 72 and into the drilled passage 78 by a generally rigid, external protective sleeve 73, which surrounds the body 56. Alternatively, an internal stiffening member (not shown) can extend within the body 56, to keep the body 56 in the desired distally straightened condition during passage through the guide sheath 72. Once the body 56 is located in the desired location within the passage 78, the physician pulls the sleeve 73 back, to uncover the body 56. The expandable body 56 can be dipped into thrombin prior to its introduction into the vertebral body 26 to facilitate in situ coagulation.

[0094] The materials for the catheter tube 50 are selected to facilitate advancement of the body 56 into cancellous bone through the guide sheath 72. The catheter tube 50 can be constructed, for example, using standard flexible, medical grade plastic materials, like vinyl, nylon, polyethylenes, ionomer, polyurethane, and polyethylene tetraphthalate (PET). The catheter tube 50 can also include more rigid materials to impart greater stiffness and thereby aid in its manipulation. More rigid materials that can be used for this purpose include Kevlar™ material, PEBAX™ material, stainless steel, nickel-titanium alloys (Nitinol™ material), and other metal alloys.

[0095] Once the protective sheath 73 is withdrawn, the wall 58 of the body 56 is capable of assuming an expanded geometry within the interior volume 30 (generally shown in FIG. 5K(1)). To accommodate expansion of the body 56, the catheter tube 50 includes a first interior lumen 80 (see FIG. 4). The lumen 80 is coupled at the proximal end of the catheter tube 50 to a pressurized source of fluid 82. The fluid 82 is preferably radio-opaque to facilitate visualization. For example, Renograffin™ can be used for this purpose.

[0096] The lumen 80 conveys the fluid 82 into the body 56 under pressure. As a result, the wall 58 expands, as FIG. 5K(1) shows. Because the fluid 82 is radio-opaque, body expansion can be monitored fluoroscopically or under CT visualization. Using real time MRI, the body 56 may be filled with sterile water, saline solution, or sugar solution.

[0097] Expansion of the wall 58 enlarges the body 56 and compacts cancellous bone 32 within the interior volume 30. As FIG. 5K(2) shows, the presence of the sheath 73 serves

to keep the proximal end of the body **56** away from edge-contact with the distal end of the catheter tube **50**.

[0098] The compaction of cancellous bone **32** forms a cavity **84** in the interior volume **30** of the vertebral body **26**. The compaction of cancellous bone also exerts interior force upon cortical-bone, making it possible to elevate or push broken and compressed bone back to or near its original prefracture position. Using a single transpedicular access (as FIG. 5K(1) shows), the cavity **84** occupies about one-half of the interior volume **30**. As will be described in greater detail later, using multiple accesses, e.g., one through each pedicle, a cavity **84** occupying substantially all of the interior volume **30** can be created.

[0099] As FIG. 4 shows, the proximal end of the catheter tube **50** is preferably coupled by tubing to a source of negative air pressure **86**. The negative pressure is conveyed through a second interior lumen **81** to one or more suction holes **88** on the distal end of the catheter tube **50**. Prior to and during the expansion of the body **56**, suction is applied to remove fats and other debris through the suction holes **88** for disposal. A separate suction-irrigation tool can be deployed through the guide sheath **72** for this purpose, if desired.

[0100] The body **56** is preferably left inflated for an appropriate waiting period, for example, three to five minutes, to allow coagulation inside the vertebral body **26**. After the appropriate waiting period, the physician collapses the body **56** and removes it through the outer guide sheath **72** (see FIG. 5L). To facilitate removal, the exterior surface of the body **56** can be treated, e.g., by ion beam-based surface treatment, to reduce friction during passage through the outer guide sheath **72**. As FIG. 5L shows, upon removal of the body **56**, the formed cavity **84** remains in the interior-volume **30**.

[0101] A suction-irrigation tool (not shown) can be introduced through the outer guide sheath **72**, to further flush and clear debris from the formed cavity **84** after removal of the body **56**.

[0102] As FIG. 5M shows, an injector nozzle or tip **90**, coupled by an injector tube **92** to an injector gun **94**, is inserted through the outer guide sheath **72** into the formed cavity **84**. The injector gun **94** carries a filling material **96**. The filling material **96** comprises, for example, methyl-methacrylate cement or a synthetic bone substitute.

[0103] The injector gun **94** can comprise a cement gun made, for example, by Stryker Corporation (Kalamazoo, Mich.). This particular injector gun **94** has a manually operated injection grip **98** with a mechanical advantage of about 9 to 1. Other injection guns may be used, having more or less mechanical advantage. Non-manually operated injection guns can also be used.

[0104] The injector tip **90** can be, for example, about 4.9 mm in diameter, to accommodate the flow a relatively viscous material **96** into the cavity **84**.

[0105] As FIG. 5M shows, the injector gun **94** pushes the filling material **96** into the cavity **84**. While injecting the material **96**, the physician preferably begins with the injector tip **90** positioned at the anterior region of the cavity **84** (as FIG. 5M shows). The physician progressively moves the tip **90** toward the posterior region of the cavity **84** (as FIG. 5N shows), away from the flow of the material **96** as it enters

and fills the cavity **84**. The physician observes the progress of the injection fluoroscopically.

[0106] The physician can also check, using, for example, x-ray, for leakage of the material through cortical bone **28**. Systems and methods for impeding or preventing such leakage will be described in greater detail later.

[0107] The physician flows material **96** into the cavity **84**, until the material **96** reaches the distal end **74** of the outer guide sheath **72** (as FIG. 5O shows).

[0108] Upon removing the injector tube **92** from the outer guide sheath **72**, the physician may, if necessary, tamp residual filling material **96** from the distal end **74** of the outer guide sheath **72** into the cavity **84**. If fluoroscopic examination reveals void regions in the cavity **84**, the physician may again insert the injector tube **92** to add more filling material **96** into the cavity **84**.

[0109] FIG. 7 shows an alternative technique for filling the cavity. In this technique, the injector tip **90** occupies the cavity **84** while the expandable body **56** is collapsing within the cavity **84**. As the body **56** collapses, the tip **90** injects material **96** into the part of the cavity **84** that the collapsing body **56** no longer occupies. The increasing volume of the cavity **84** not occupied by the collapsing body **56** is thereby progressively filled by an increasing volume of material **96**. The presence of the body **56**, partially expanded while the tip **90** injects the material **96**, serves to compact and spread the injected material **96** within the cavity **84**.

[0110] As filling of the cavity **84** progresses, preferably under fluoroscopic monitoring, the physician progressively retracts the injector tip **90** from the anterior region of the cavity **84**, toward the outer guide sheath **72** allowing the material **96** to progressively enter and fill the cavity **84** with the collapse of the body **56**.

[0111] FIGS. 8A to 8C show a preferred embodiment of a tool **650** which integrates the injection tube and expandable body in a single structure. As FIG. 8B shows, the tool **650** includes a catheter tube **652** having a proximal end **654** and a distal end **656**. The distal end carries an expandable body **662**.

[0112] As FIG. 8C shows, the catheter tube **652** has concentric inner and outer lumens, respectively **658** and **660**. The inner lumen **658** communicates, by proximal tubing **664**, with an injector gun, **94**, of the type previously described. The inner lumen **658** also communicates with an injector nozzle or tip **666** at the distal catheter tube end **656**. Operation of the gun **94** serves to inject filling material **96** through the nozzle **666** (as FIG. 8A shows).

[0113] The outer lumen **660** communicates, via proximal tubing **668**, with a source **82** of pressurized liquid. The outer lumen **660** also communicates with ports **670** formed on the distal catheter tube end **656** underlying the expandable body **662**. Operation of the source **82** serves to inject pressurized liquid into the body **662** to expand it, in the manner previously described.

[0114] As FIG. 8A shows, the physician introduces the tool **650** into the cancellous bone **32**. The physician expands the body **662** to create the cavity **84**. Once the cavity **84** is formed, the physician begins to collapse the body **662**, while injecting the filling material **96** through the nozzle **666**. The volume of the cavity **84** occupied by the collapsing body **662**

is progressively filled by the increasing volume of filling material **96** injected through the nozzle **666**.

[0115] As earlier described, the collapsing body **662** serves to compact and spread the filling material **96** more uniformly within the cavity **84**. Under fluoroscopic monitoring, the physician progressively retracts the distal end **656** of the tool **650** from the anterior region of the cavity **84** toward the outer guide sheath **72**, allowing the material **96** to enter and fill the cavity **84**.

[0116] Upon filling the cavity **84** with the material **96**, the physician removes the outer guide sheath **72**, as FIGS. **5P** and **5Q** show. The incision site is sutured or otherwise closed (designated by ST in FIG. **5P**).

[0117] In time, the filling material **96** sets to a hardened condition within the cavity **84** (see FIGS. **5P** and **5Q**). The hardened material **96** provides renewed interior structural support for the cortical bone **28**.

[0118] The above described procedure, carried out in a minimally invasive manner, can also be carried out using an open surgical procedure. Using open surgery, the physician can approach the bone to be treated as if the procedure is percutaneous, except that there is no skin and other tissues between the surgeon and the bone being treated. This keeps the cortical bone as intact as possible, and can provide more freedom in accessing the interior volume **30** of the vertebral body.

[0119] B. Material Selection for the Expandable Body

[0120] The material of the body wall **58** can be selected according to the therapeutic objectives surrounding its use. For example, materials including vinyl, nylon, polyethylenes, ionomer, polyurethane, and polyethylene terephthalate (PET) can be used. The thickness of the body wall **58** is typically in the range of $\frac{2}{1000}$ ths to $\frac{25}{1000}$ ths of an inch, or other thicknesses that can withstand pressures of up to, for example, 250-500 psi.

[0121] If desired, the material for the wall **58** can be selected to exhibit generally elastic properties, like latex. Alternatively, the material can be selected to exhibit less elastic properties, like silicone. Using expandable bodies **56** with generally elastic or generally semi-elastic properties, the physician monitors the expansion to assure that over-expansion and wall failure do not occur. Furthermore, expandable bodies **56** with generally elastic or generally semi-elastic properties will require some form of external or internal restraints to assure proper deployment in bone.

[0122] For example, expandable bodies **56** with generally elastic properties will exhibit the tendency to backflow or creep into the outer guide sheath **72** during their expansion. It is therefore necessary to internally or externally restrain a body **56** that is subject to creeping, to keep it confined within the interior bone region. In FIG. **6**, an exterior sealing element **100** is provided for this purpose. In FIG. **6**, the sealing element **100** takes the form of a movable o-ring.

[0123] The physician advances the o-ring **100** along the catheter tube **50** inside the guide sheath **72** using a generally stiff stylet **102** attached to the o-ring **100**. The physician locates the o-ring **100** at or near the distal end **54** of the catheter tube **50** prior to conveying the liquid **82** to expand the body **56**. The o-ring **100** is held in place by the generally stiff stylet **102**, which provides a counter force to prevent

backward movement of the o-ring **100** in the guide sheath **72** as the body **56** expands. The o-ring **100** thereby keeps all or a substantial portion of the generally elastic body **26** confined inside the interior volume **30**. The body **56** thereby serves to compact as much of the cancellous bone **32** as possible.

[0124] The use of an external sealing element **100** to restrain the expandable body **56** may not be necessary when relatively inelastic materials are selected for the body **56**. For example, the material for the body wall **58** can be selected to exhibit more inelastic properties, to limit expansion of the wall **58** prior to wall failure. The body wall **58** can also include one or more restraining materials, particularly when the body wall **58** is, itself made from more elastic materials. The restraints, made from flexible, inelastic high tensile strength materials, limit expansion of the body wall **58** prior to wall failure. Representative examples of generally inelastic wall structures will be described in greater detail later.

[0125] C. Selection of Shape and Size for the Expandable Body

[0126] As will also be demonstrated later, when relatively inelastic materials are used for the body wall **58**, or when the body wall **58** is otherwise externally restrained to limit its expansion prior to failure, a predetermined shape and size can be imparted to the body **56**, when it is substantially expanded. The shape and size can be predetermined according to the shape and size of the surrounding cortical bone **28** and adjacent internal structures, or by the size and shape of the cavity **84** desired to be formed in the cancellous bone **32**.

[0127] In one embodiment, which is generally applicable for treating bones experiencing or prone to fracture, the shape and size of the body **56**, when substantially expanded, can be designed to occupy at least about 30% of the volume of cancellous bone **32** in the interior volume **30**. A body **56** having a substantially expanded size and shape in the range of about 40% to about 99% of the cancellous bone volume is preferred.

[0128] In another embodiment, which is applicable for treating bones having more localized regions of fracture or collapse caused, for example, by avascular necrosis, the shape and size of the body **56** can be designed to occupy as little as about 10% of the cancellous bone volume. In this embodiment, the drilled passage **78** extends directly to the localized site of injury, to enable targeted introduction of the body **26**.

[0129] The shape of the cancellous bone **32** to be compressed, and the presence of surrounding local anatomic structures that could be harmed if cortical bone were moved inappropriately, are generally understood by medical professionals using textbooks of human skeletal anatomy, along with their knowledge of the site and its disease or injury. The physician is also able to select the materials and geometry desired for the body **56** based upon prior analysis of the morphology of the targeted bone using, for example, plain films, spinous process percussion, or MRI or CRT scanning. The materials and geometry of the body **56** are selected to create a cavity **84** of desired size and shape in cancellous bone **32** without applying harmful pressure to the outer cortical bone **28** or surrounding anatomic structures.

[0130] In some instances, it is desirable, when creating the cavity **84**, to move or displace the cortical bone **28** to achieve

the desired therapeutic result. Such movement is not per se harmful, as that term is used in this Specification, because it is indicated to achieve the desired therapeutic result. By definition, harm results when expansion of the body 56 results in a worsening of the overall condition of the bone and surrounding anatomic structures, for example, by injury to surrounding tissue or causing a permanent adverse change in bone biomechanics.

[0131] D. Deployment of Multiple Expandable Bodies

[0132] Formation of a desired cavity geometry in cancellous bone 32 using an expandable body 56 can be accomplished in diverse ways to achieve the desired therapeutic effect. The foregoing disclosure envisions the deployment of a single-expandable body 56 to compact cancellous bone 32 and, by itself, form a cavity 84 having a desired shape and size to receive a filling material 96.

[0133] Alternatively, a cavity 84 having a desired shape and size in cancellous bone 32 can be formed by the deployment of more than one expandable body 56 in a targeted region of cancellous bone 32, either sequentially or simultaneously.

[0134] FIG. 9 shows the representative deployment of multiple expandable bodies 56A and 56B through a single outer guide sheath 72, which is arranged to provide transpedicular access. It should be understood that deployment of multiple expandable bodies can likewise be achieved through an outer guide sheath 72 arranged to provide a posterolateral access, through the side of the vertebral body 26 (as shown as P-L in phantom lines in FIG. 9). In FIG. 9, the expandable bodies 56A and 56B are carried by separate catheter tubes 50A and 50B, which are not joined together.

[0135] In the-alternative embodiment shown in FIG. 10, a tool 109 comprising an array 108 of catheter tubes 50A and 50B is provided. Each catheter tube 50A and 50B each carries an expandable body 56A and 56B, which are shown in FIG. 10 in a collapsed condition. In FIG. 10, the distal ends of the catheter tubes 50A and 50B are joined by a connector 106, for simultaneous deployment through an outer guide sheath 72 into the vertebral body 26, as FIG. 9 shows. As before described, a slidable protective sheath 73 encloses the bodies 56A and 56B during passage through the guide sheath 72. Upon withdrawal of the protective sheath 73, expansion of the bodies 56A and 56B, either simultaneously or sequentially, creates a cavity 84. If desired, the connector 106 can permit relative adjustment of the catheter tubes 50A and 50B, so that, when deployed, one expandable body is located more distal to another expandable body.

[0136] For the sake of illustration, FIGS. 9 and 10 show two catheter tubes 50A and 50B, but more than two catheter tubes can be deployed in the vertebral body 26, either as separate tools (as FIG. 9 shows), or joined to form a composite array 108 (as FIG. 10 shows).

[0137] In FIG. 10, the bodies 56A and 56B of the array 108 have generally the same geometry, when substantially expanded, thereby providing a symmetric arrangement for compacting cancellous bone 32. A generally symmetric cavity 84 results.

[0138] Alternatively, as shown in FIG. 11, the bodies 56A and 56B possess different geometries when substantially expanded, thereby presenting an asymmetric arrangement

for compacting cancellous bone 32. A generally asymmetric cavity 84 results. By mutually adjusting catheter tubes through a connector 106 (as previously described), the distal extensions of expandable bodies relative to each other can be made to differ, thereby also resulting in asymmetric cavity formation.

[0139] The selection of size and shape of the array 108, whether symmetric or asymmetric, depends upon the size and shape of the targeted cortical bone 28 and adjacent internal structures, or by the size and shape of the cavity 84 desired to be formed in the cancellous bone 32. The deployment of multiple expandable bodies 56 makes it possible to form cavities 84 having diverse and complex geometries within bones of all types. Multiple expandable bodies having generally the same geometry can be deployed in different ways to create cavities of different geometries.

[0140] It should be appreciated that the various styles of multiple expandable bodies 56 shown in FIGS. 9 to 11 are deployed in a distally straightened condition (as FIGS. 10 and 11 show) by using, e.g., a relatively stiff, surrounding sheath 73 (shown in phantom lines in FIG. 10), which is manipulated in the same as previously described in connection with FIGS. 5J(1) and 5J(2). There are, of course, other ways to straighten the bodies 56 for deployment into bone, such as through the use of internal stiffening elements.

[0141] Access for expandable bodies 56 can be achieved through multiple access sites and in many different ways. For example, multiple expandable bodies can access the vertebral body from different regions of a targeted vertebra.

[0142] FIG. 12 shows a representative dual transpedicular access, in which two outer guide sheaths 72A and 72B are used to provide separate access for two or more expandable bodies 56A and 56B through different sides of the pedicle 42A and 42B of the vertebral body 26.

[0143] FIG. 13 shows a representative dual contra lateral posterolateral access, in which two outer guide sheaths 72A and 72B are used to provide separate access for multiple expandable bodies 56A and 56B from different lateral sides of the vertebral body 26.

[0144] Deployed from dual access sites as shown in FIGS. 12 and 13, the multiple expandable bodies 56A and 56B each forms a cavity 84A and 84B (shown in FIG. 14). The cavities 84A and 84B are transversely spaced within the cancellous bone 32. The transversely spaced cavities 84A and 84B may adjoin to form a single combined cavity (designated C in FIG. 14), into which the filling material 96 is injected. Alternatively, as FIG. 15 shows, the transversely spaced cavities 84A and 84B may remain separated by a region of cancellous bone (designated by numeral 110 in FIG. 13). In this arrangement, the filling material 96 is injected into multiple, individual cavities 84A and 84B within the interior volume.

[0145] As another example, multiple expandable bodies 56A and 56B can access the vertebral body 26 from the same general region of the vertebra. FIG. 16 shows a representative dual ipsilateral posterolateral access, in which two outer guide sheaths 72A and 72B are used to provide separate access from the same lateral sides of the vertebral body 26.

[0146] Deployed from these access sites (see FIG. 17), the multiple expandable bodies 56A and 56B form vertically

spaced, or stacked, cavities **84A** and **84B**. The vertically spaced cavities **84A** and **84B** may adjoin to form a single combined cavity (designated **C** in FIG. 17), into which the filling material **96** is injected. Alternatively (see FIG. 18), the vertically spaced cavities **84A** and **84B** may be separated by a region of cancellous bone (designated by numeral **110** in FIG. 18), forming multiple individual cavities **84A** and **84B** within the interior volume, each of which is individually filled with a filling material **96A** and **96B**.

[0147] By way of another example, FIG. 19 shows a first outer guide sheath **72A** arranged to provide a transpedicular access and a second outer guide sheath **72B** to provide a posterolateral access.

[0148] Systems for treating bone using multiple expandable bodies can include directions **79** (see FIG. 12) for deploying the first and second expandable bodies. For example, the directions **79** can instruct the physician to insert a first expandable body into the interior volume through a first access path through cortical bone, while inserting a second expandable body into the interior volume through a second access path through cortical bone different than the first access path.

[0149] In any of the above-described examples, each guide sheath **72A** or **72B** can itself accommodate a single expandable body or multiple expandable bodies. The size and shape of the bodies may be the same, or they may vary, according to the desired objectives of the physician for the targeted vertebral body.

[0150] E. Representative Embodiments of Expandable Bodies to Treat Vertebrae

[0151] i. Constrained Donut-Shaped Geometries

[0152] FIG. 20 shows a representative embodiment of an expandable body, which is broadly denoted by the numeral **210**. The body **210** comprises a pair of hollow, inflatable, non-expandable parts **212** and **214** of flexible material, such as PET or Kevlar. Parts **12** and **14** have a suction tube **216** therebetween for drawing fats and other debris by suction into tube **216** for transfer to a remote disposal location. The catheter tube **216** has one or more suction holes so that suction may be applied to the open end of tube **216** from a suction source (not shown).

[0153] The parts **212** and **214** are connected together by an adhesive which can be of any suitable type. Parts **212** and **214** are doughnut-shaped, as shown in FIG. 20 and have tubes **218** and **220** which communicate with and extend away from the parts **212** and **214**, respectively, to a source of inflating liquid under pressure (not shown). The liquid expands the body **210** as already described.

[0154] FIG. 21 shows a modified doughnut shape body **280** of the type shown in FIG. 20, except the doughnut shapes of body **280** are not stitched onto one another. In FIG. 21, body **280** has a pear-shaped outer convex surface **282** which is made up of a first hollow part **284** and a second hollow part **285**. A tube **288** is provided for directing liquid into the two parts along branches **290** and **292** to inflate the parts after the parts have been inserted into the interior volume of a bone. A catheter tube **216** may or may not be inserted into the space **296** between two parts of the balloon **280** to provide irrigation or suction. An adhesive bonds the two parts **284** and **285** together.

[0155] FIG. 22 shows another representative embodiment of an expandable body, designated **309**. The body **309** has a generally round geometry and three expandable body units **310**, **312** and **314**. The body units **310**, **312**, and **314** include string-like external restraints **317**, which limit the expansion of the body units **310**, **312**, and **314** in a direction transverse to the longitudinal axes of the body units **310**, **312**, and **314**. The restraints **317** are made of the same or similar material as that of the body units **310**, **312**, and **314**, so that they have some resilience but substantially no expansion capability.

[0156] A tubes **315** direct liquid under pressure into the body units **310**, **312** and **314** to expand the units and cause compaction of cancellous bone. The restraints **317** limit expansion of the body units prior to failure, keeping the opposed sides **377** and **379** substantially flat and parallel with each other.

[0157] ii. Constrained Kidney-Shaped Geometries

[0158] FIG. 23 shows another representative embodiment of an expandable body **230**, which has a kidney-shaped geometry. The body **230** has a pair of opposed kidney-shaped side walls **232** and a continuous end wall **234**. A tube **238** directs liquid into the body to expand it within the vertebral body.

[0159] FIG. 24 shows another representative embodiment of an expandable body **242**, which also has a kidney-shaped geometry. The body **242** is initially a single chamber bladder, but the bladder is branded along curved lines or strips **241** to form attachment lines **244** which take the shape of side-by-side compartments **246** which are kidney shaped as shown in FIG. 25. A similar pattern of strips as in **240** but in straight lines would be applied to a body that is square or rectangular. The branding causes a welding of the two sides of the bladder to occur.

[0160] The details of these and other expandable bodies usable to treat vertebral bodies are described in U.S. patent application, Ser. No. 08/188,224, filed Jan. 26, 1994, which is incorporated herein by reference.

[0161] F. Selection of Desired Geometry

[0162] The eventual selection of the size and shape of a particular expandable body or bodies to treat a targeted vertebral body **26** is based upon several factors. When multiple expandable bodies are used, the total combined dimensions of all expandable bodies deployed, when substantially expanded, should be taken into account.

[0163] The anterior-posterior (A-P) dimension (see FIG. 26) for the expandable body or bodies is selected from the CT scan or plain film or x-ray views of the targeted vertebral body **26**. The A-P dimension is measured from the internal cortical wall of the anterior cortex to the internal cortical wall of the posterior cortex of the vertebral body. In general, the appropriate A-P dimension for the expandable body or bodies is less than this anatomic measurement.

[0164] The appropriate side to side dimension **L** (see FIG. 26) for an expandable body or bodies is also selected from the CT scan, or from a plain film or x-ray view of the targeted vertebral body. The side to side distance is measured between the internal cortical walls laterally across the targeted vertebral body. In general, the appropriate side to side dimension **L** for the expandable body is less than this anatomic measurement.

[0165] The lumbar vertebral body tends to be much wider in side to side dimension L then in A-P dimension. In thoracic vertebral bodies, the side to side dimension and the A-P dimensions are almost equal.

[0166] The height dimensions H of the expandable body or bodies (see FIG. 26) is chosen by the CT scan or x-ray views of the vertebral bodies above and below the vertebral body to be treated. The height of the vertebral bodies above and below the vertebral body to be treated are measured and averaged. This average is used to determine the appropriate height dimension of the chosen expandable body.

[0167] The dimensions of expandable body or bodies for use in vertebrae are patient specific and will vary across a broad range, as summarized in the following table:

Vertebra Type	Height (H) Dimension of Typical Expandable Body or Bodies	Posterior(A-P) Dimension of Typical Expandable Body or Bodies	Side to Side Dimension (L) of Typical Expandable Body or Bodies
Lumbar	0.5 cm to 4.0 cm	0.5 cm to 4.0 cm	0.5 cm to 5.0 cm
Thoracic	0.5 cm to 3.5 cm	0.5 cm to 3.5 cm	0.5 cm to 4.0 cm

[0168] A preferred expandable body 56 for use in a vertebral body is stacked with two or more expandable members of unequal height (see FIG. 26), where each member can be separately inflated through independent tube systems. The total height of the stack when fully inflated should be within the height ranges specified above. Such a design allows the fractured vertebral body to be returned to its original height in steps, which can be easier on the surrounding tissue, and it also allows the same balloon to be used in a wider range of vertebral body sizes.

[0169] II. Treatment of Long Bones

[0170] Like vertebrae, the interior regions of long bones substantially occupied by cancellous bone can be treated with the use of one or more expandable bodies. FIG. 43 shows representative regions of the human skeleton 600, where cancellous bone regions of long bones can be treated using expandable bodies. The regions include the distal radius (Region 602); the proximal tibial plateau (Region 604); the proximal humerus (Region 606); the proximal femoral head (Region 608); and the calcaneus (Region 610).

[0171] As for vertebral bodies, expandable bodies possess the important attribute of being able, in the course of forming cavities by compressing cancellous bone, to also elevate or push broken or compressed cortical bone back to or near its normal anatomic position. This is a particularly important attribute for the successful treatment of compression fractures or cancellous bone fractures in the appendicular skeleton, such as the distal radius, the proximal humerus, the tibial plateau, the femoral head, hip, and calcaneus.

[0172] Representative examples of expandable bodies for the treatment of cancellous bone regions of long bones will be next described.

[0173] A. Expandable Body for the Distal Radius

[0174] The selection of an appropriate expandable to treat a fracture of the distal radius (Region 602 in FIG. 43) will depend on the radiological size of the distal radius and the location of the fracture.

[0175] FIGS. 27 and 28 show a representative expandable body 260 for use in the distal radius. The body 260, which is shown deployed in the distal radius 252, has a shape which approximates a pyramid but more closely can be considered the shape of a humpbacked banana. The geometry of the body 260 substantially fills the interior of the space of the distal radius to compact cancellous bone 254 against the inner surface 256 of cortical bone 258.

[0176] The body 260 has a lower, conical portion 259 which extends downwardly into the hollow space of the distal radius 252. This conical portion 259 increases in cross section as a central distal portion 261 is approached. The cross section of the body 260 is shown at a central location (FIG. 27), which is near the widest location of the body 260. The upper end of the body 260, denoted by the numeral 262, converges to the catheter tube 288 for directing a liquid into the body 260 to expand it and force the cancellous bone against the inner surface of the cortical bone.

[0177] The shape of the body 260 is determined and restrained by tufts formed by string restraints 265. These restraints are optional and provide additional strength to the body 260, but are not required to achieve the desired configuration.

[0178] The body 260 is placed into and taken out of the distal radius in the same manner as that described above with respect to the vertebral bone.

[0179] Typical dimensions of the distal radius body vary as follows:

[0180] The proximal end of the body 260 (i.e. the part nearest the elbow) is cylindrical in shape and will vary from 0.4x0.4 cm to 1.8x1.8 cm.

[0181] The length of the distal radius body will vary from 1.0 cm to 12.0 cm.

[0182] The widest medial to lateral dimension of the distal radius body, which occurs at or near the distal radio-ulnar joint, will measure from 0.5 cm to 2.5 cm.

[0183] The distal anterior-posterior dimension of the distal radius body will vary from 0.4 to 3.0 cm.

[0184] B. Expandable Body for Proximal Humerus Fracture

[0185] The selection of an appropriate expandable body 266 to treat a given proximal humeral fracture (Region 606 in FIG. 43) depends on the radiologic size of the proximal humerus and the location of the fracture.

[0186] FIG. 29A shows a representative embodiment of an expandable body 266 for use in the proximal humerus 269. The body 266 is spherical for compacting the cancellous bone 268 in a proximal humerus 269. If surrounding cortical bone has experienced depression fracture, expansion of the body 266 also serves to elevate or move the fractured cortical bone back to or near its anatomic position before fracture.

[0187] A mesh 270, embedded or laminated and/or winding, may be used to form a neck 272 on the body 266. A second mesh 270a may be used to conform the bottom of the base 272a to the shape of the inner cortical wall at the start of the shaft. These mesh restraints provide additional strength to the body 266, but the configuration can be achieved through molding of the body.

[0188] The body 266 has a catheter tube 277 into which liquid under pressure is forced into the body to expand it to compact the cancellous bone in the proximal humerus. The body 266 is inserted into and taken out of the proximal humerus in the same manner as that described above with respect to the vertebral bone.

[0189] Typical dimensions of the expandable body 266 shown in FIG. 29A for proximal humerus fracture vary as follows:

[0190] The spherical end of the body will vary from 0.6×0.6 cm to 3.0×3.0 cm.

[0191] The neck of the proximal humeral fracture body will vary from 0.5×0.5 cm to 3.0×3.0 cm.

[0192] The width of the base portion or distal portion of the proximal humeral fracture body will vary from 0.5×0.5 cm to 2.5×2.5 cm.

[0193] The length of the body will vary from 3.0 cm to 14.0 cm.

[0194] FIG. 29B shows another representative embodiment of an expandable body 266' for use in the proximal humerus 269. Instead of being spherical, the body 266' shown in FIG. 29B has a generally cylindrical geometry for compacting the cancellous bone 268 in a proximal humerus 269. Alternatively, the cylindrical body 266' can be elongated to form an elliptical or football-shaped geometry. Typical dimensions for a cylindrical or elliptical body vary from 0.6 cm to 3.0 cm in diameter to 3.0 cm to 14.0 cm in length.

[0195] C. Expandable Body for Proximal Tibial Plateau Fracture

[0196] The selection of an expandable body to treat a given tibial plateau fracture (Region 604 in FIG. 43) will depend on the radiological size of the proximal tibial and the location of the fracture.

[0197] FIG. 30A shows a representative expandable body 280 for treating a tibial plateau fracture. The body 280 may be introduced into the tibia from any direction, as desired by the physician, for example, from the top, or medial, lateral, anterior, posterior, or oblique approach. In FIG. 30A, the body 280 has been introduced into cancellous bone 284 from the anterior side of the tibia 283 and is shown position in one side 282 of the tibia 283.

[0198] The body 280, when substantially inflated (as FIG. 30A shows), compacts the cancellous bone in the layer 284 surrounding the body 280. If the tibia plateau has experienced depression fracture, expansion of the body 280 also serves to move the tibia plateau back to or near its anatomic elevation before fracture, as FIG. 30A shows. Fractures on both the medial and lateral sides of the tibia can be treated in this manner.

[0199] As FIG. 30B shows, the body 280 has a pair of opposed sides 285 and 287. The sides 285 and 287 are interconnected by restraints 288, which pass through the body 280. FIG. 30C shows the tied-off ends 291 of the restraints 288.

[0200] The restraints 288 can be in the form of strings or flexible members of any suitable construction. The restraints 288 limit expansion of the body 280 prior to failure. The restraints 288 make the sides 285 and 287, when the body 280 is substantially expanded, substantially parallel with each other and, thereby, non-spherical.

[0201] A tube 290 is coupled to the body 280 to direct liquid into and out of the body to expand it. The body is inserted into and taken out of the tibia in the same manner as that described above with respect to the vertebral bone. FIG. 30C shows a substantially circular configuration for the body 280, although the body 280 can also be substantially elliptical, as FIG. 31 shows.

[0202] Other geometries and configurations can also be used. For example, as FIG. 32 shows, two or more expandable bodies 280(1), 280(2), and 280(3) can be stacked one atop another to produce a different cavity geometry and to enhance plateau fracture displacement. The multiple bodies 280(1), 280(2), and 280(3) can comprise separate units or be joined together for common deployment. When deployed as separate units, the bodies 280(1), 280(2), and 280(3) can enter through the same access point or from different access points.

[0203] As another example, as FIG. 33 shows, the body 280' can assume an egg shape when substantially inflated, to form a cavity and reshape broken bones. Other geometries, such as cylindrical or spherical, can also be used for the same purpose. Typical dimensions of the body 280 for treating proximal tibial plateau fracture vary as follows:

[0204] The thickness or height of the body will vary from 0.3 cm to 5.0 cm.

[0205] The anterior-posterior (front to back) dimension will vary from 1.0 cm to 6.0 cm.

[0206] The medial to lateral (side-to-side) dimension will vary from 1.0 cm to 6.0 cm.

[0207] FIGS. 44 and 45 show multiple expandable zones 614 and 616 deployed in cancellous bone 620. One zone 614 serves as a platform to confine and direct the expansion of the other zone 616. For the purpose of illustration, FIGS. 44 and 45 show the multiple zones 614 and 616 used for this purpose to treat a tibial plateau fracture 622.

[0208] In the embodiment shown in FIGS. 44 and 45, the zones 614 and 616 comprise separate expandable bodies. It should be appreciated, however, that the zone 614 and 616 can comprise parts of a single expandable body.

[0209] In the illustrated embodiment (as FIG. 44 shows), the first expandable body 614 is deployed through a first outer guide sheath 618(1) into cancellous bone 620 below the fracture 622. As FIG. 44 shows, when substantially expanded, the first body 614 expands more along its horizontal axis 624 (i.e., in a side-to-side direction) than along its vertical axis 626 (i.e., in a top-to-bottom direction). The greater expanded side-to-side geometry of the first body 614 compacts cancellous bone in a relatively thin region, which

extends substantially across the interior volume **628** occupied by the first body **614**. The geometric limits of the body **614** will typically fall just inside the inner cortical walls of the proximal tibia, or whatever bone in which the first body **614** is deployed.

[0210] The expanded first body **614** creates a barrier **630** within the interior region **628**. Due to the less expanded top-to-bottom geometry of the first body **614**, a substantially uncompacted region **632** of cancellous bone is left above the body **614**, which extends from the formed barrier **630** upward to the fracture **622**. In a representative deployment, the uncompacted region **632** extends about 2 cm below the tibial plateau fracture **622**.

[0211] As FIG. **44** shows, a second expandable body **616** is deployed through a second outer guide sheath **618(2)** into the uncompacted region **632** left between the first body **614**, when substantially expanded, and the targeted tibial plateau fracture **622**.

[0212] As FIG. **45** shows, the second expandable body **616** has a geometry, substantially like that shown in FIGS. **30A** to **30C**. When substantially inflated, the second body **616** compacts a large percentage of the cancellous bone in the region **632** above the first expandable body **614**. The presence of the barrier **630**, which the expanded first body **614** creates (see FIG. **46** also), prevents expansion of the second body **616** in a direction away from the tibial platform fracture **622**. Instead, the barrier **630** directs expansion of the second body **616** toward the fracture **622**. Buttressed by the barrier **630**, the expansion of the body **616** is directed against the fractured plateau **622**, restoring it to its normal anatomic position, as FIGS. **45** and **46** show.

[0213] It should be appreciated that one or more expandable bodies can be used as platforms or barriers to direct the expansion of one or more other expandable bodies in other localized interior bone regions. The barrier makes possible localized cavity formation in interior bone regions. Use of the barrier preserves healthy regions of cancerous bone, while directing the main compacting body toward localized fractures or localized regions of diseased cancellous bone.

[0214] D. Expandable Body for Femoral Head

[0215] The size of an expandable body for use in the femoral head (Region **608** in FIG. **43**) is chosen based upon the radiological or CT scan size of the head of the femur and the location and size of the avascular necrotic bone.

[0216] FIG. **34** shows a representative embodiment of an expandable body **300** introduced inside the cortical bone **302** of the femoral head. As FIG. **34** shows, the femoral head is thin at the outer end **304** of the femur and increases in thickness at the lower end **306** of the femur. A tube **309** directs liquid to expand the body **300**. The tube **309** extends along the femoral neck and into the femoral head. The expandable body **300** compacts the cancellous bone **307** in this bone region, while also moving fractured cortical bone back to or near its normal anatomic position.

[0217] The femoral head is generally spherical in configuration, and the body **300** can have either a hemispherical (see FIG. **35**) as well as spherical geometry (as FIG. **34** shows). The hemispherical shape is maintained in FIG. **34** by bonding overlapping portions of the body **300**, creating pleats **300b**.

[0218] The body **300** is inserted into and taken out of the femoral head in the same manner as that described with respect to the vertebral bone.

[0219] Typical dimensions of an expandable body for use in treating the femoral head vary as follows:

[0220] The diameter of the expandable body will vary from 0.5 cm to up to 4.5 cm. The dimensions of the hemispherical body (FIG. **35**) are the same as the those of the spherical body (FIG. **34**), except that approximately one half is provided.

[0221] E. Expandable Body for Prevention of Hip Fracture

[0222] Patients with bone density in the hip (Region **612** in FIG. **43**) below a threshold value are at increased risk of hip fracture, and lower densities create greater risk. Patient selection is done through a bone density scan.

[0223] FIG. **36A** shows a representative embodiment of an expandable body **410** having a “boomerang” geometry for use in preventing hip fracture. When substantially expanded (as FIG. **36A** shows), the body **410** forms a cylinder, which gradually bends in the middle, like a boomerang, and extends from about 0.5 cm from the end of the femoral head **411** through the femoral neck **412** and down into the proximal femoral diaphysis **413** about 5 to 7 cm past the lesser trochanter **414**.

[0224] Expansion of the body **410** is limited to achieve the described geometry by rings **430** of inelastic material. The rings **430** are held in a spaced apart relationship along one side of the body **410** by attachment to an inelastic band **416**, which runs the length of that side of body **410**. The rings **430** are held in a farther spaced apart relationship along the opposite side of the body **410** by attachment to another, longer inelastic band **417**, which runs the length of the opposite side of the body **410**. A tube **419** conveys liquid to inflate the body **410**.

[0225] Prior to deployment within the body, the body **410** is collapsed and rolled up and held against the inflation tube **419** using, for example, with frangible connectors that will break as the body is subject to expansion. To deploy the body **410** into the hip, the surgeon uses a power drill under radiographic guidance to create a cavity **420**, which is, for example, about 4 to 6 mm wide starting at the lateral femoral cortex **421** and proceeding into the femoral head **411**. The body **410** is deployed through a guide sheath **423**, following the cavity **420**. The body **410** is deployed, prior to expansion, facing the lesser trochanter **414**, so that expansion occurs toward the femoral diaphysis **413**, and not toward the greater trochanteric region **422**.

[0226] The expansion of the body **410** is guided by the rings **430** and bands **416** and **417**, which cause bending of the body **410** downward into the lesser trochanter **414**. Optionally, a second cavity can be drilled down into the diaphysis **413**, starting from the same entry point or from the other side.

[0227] The body length is chosen by the physician to extend about 0.5 cm from the end of the femoral head, through the femoral neck and into the proximal femoral diaphysis, usually about 4 to 8 cm below the lesser trochanter. The body diameter is chosen by measuring the inner cortical diameter of the femoral neck (the most narrow area)

and subtracting 0.5 cm. The preferred dimensions of the body **410** are a total length of 10-20 cm and a diameter of about 1.0-2.5 cm.

[0228] Patients having the lowest bone densities in the femoral head may require greater compacting in the femoral head, which may, for example, be provided by using two bodies, one after the other: the bent body **410** followed by the femoral head body (inserted at the same point and expanded prior to inserting any supporting material). Alternatively, the bent body **410** may be adapted to have a distal portion that approximates the shape of the femoral-head body.

[0229] The geometry of the single, restrained body **410** can be approximated by multiple expandable bodies deployed separately, or coupled together, or stacked together. FIG. 36B shows a representative embodiment of the use of multiple expandable bodies in the hip region.

[0230] As FIG. 36B shows, a first expandable body **410**(1) is introduced through a first outer guide sheath **423**(1) in the proximal lateral cortex of the femoral shaft. The first body **419**(1) is deployed across the femoral neck **480** into the femoral head **482**.

[0231] A second expandable body **410**(2) is introduced through a second outer guide sheath **423**(2) in the greater trochanter **422** of the femur. The first body **419**(1) is deployed in the direction of the femoral diaphysis **413**.

[0232] Other approaches can be used. For example, one body can be introduced through the femoral neck **480**, and the other body can be introduced along the shaft of the femur.

[0233] One or both of the bodies **410**(1) and **410**(2) can include external restraints to limit expansion, in the manner described with regard to the body **410**. Expansion of the bodies **410**(1) and **410**(2) compacts cancellous bone to form a cavity having a geometry approximating that formed by the single body **410**.

[0234] F. Expandable Body for Calcaneus Fracture

[0235] The size of an expandable body for use in treating fracture of the calcaneus (heel bone) (Region **610** in FIG. 43) is chosen based upon the radiological or CT scan size of the calcaneus and the location and size of the fracture.

[0236] FIGS. 37A and 37B show a representative expandable body **450** for treating fracture of the calcaneus **452**. A tube **464** conveys liquid into the body **450** to expand it.

[0237] In FIG. 37A, the body **450** is deployed into the calcaneus **452** by a posterior approach, through the tuberosity. Other approaches can be used, as desired by the physician. A power drill opens a passage **466** through the tuberosity into the calcaneus. An outer guide sheath **470** is positioned within the passage **466**, abutting the posterior of the calcaneus, in the manner previously described in obtaining access to a vertebral body. The body **450** is introduced through the guide sheath **470** and formed passage **466** into the calcaneus.

[0238] Expansion of the body **450** is limited within the confines of the calcaneus by inelastic peripheral bands **454** (see FIG. 37B). The bands **454** constrain expansion of the body **450** to an asymmetric, pear-shaped geometry, best shown in FIG. 37B. The pear-shaped geometry has a major

dimension **H1** occupying the region of the posterior facet **454**. The major dimension **H1** is located here, because the part of the calcaneus most likely to require elevation and realignment during expansion of the body **450** is the depressed part of the posterior facet **454** of the calcaneus, where the posterior facet **454** abuts the talus **456**.

[0239] The pear-shaped geometry has a smaller, minor dimension occupying the region of the anterior facet **458** of the calcaneus, near the calcaneal-cuboid joint **460**, between the calcaneus and cuboid bone **462**.

[0240] Expansion of the body **410** compacts cancellous bone **470** within the calcaneus **452**. The expansion also lifts a depression fracture of the posterior facet **454** back to or near its original anatomic elevation adjacent the talus **456**. When collapsed and removed, the body **410** leaves a cavity in cancellous bone into which filling material can be introduced in the manner previously described.

[0241] FIG. 38 shows another representative embodiment of an expandable body **450'** for use in treating fractures in the calcaneus. The body **450'** in FIG. 38 has a more spherical or egg-shaped geometry than the pear-shaped body **450** shown in FIG. 37B. Like the pear-shaped body **450**, the body **450'**, when expanded within the calcaneus, forms a cavity within cancellous bone and realigns fractured cortical bone at or near its normal anatomic position.

[0242] III. Selection of Other Expandable Bodies (Further Overview)

[0243] Different sizes and/or shapes of expandable bodies may be used at sites not specified above, such as the jaw bones, the midshaft of the arm and leg bones, the cervical vertebral bodies, the foot and ankle bones, the pelvis, the ribs, and the like.

[0244] The choice of the shape and size of an expandable body takes into account the morphology and geometry of the site to be treated. As before stated, the shape of the cancellous bone to be compressed, and the local structures that could be harmed if bone were moved inappropriately, are generally understood by medical professionals using textbooks of human skeletal anatomy along with their knowledge of the site and its disease or injury. Precise dimensions for a given patient can be further determined by X-ray of the site to be treated.

[0245] As one general guideline, the selection of the geometry of the expandable body should take into account that at least 40% of the cancellous bone volume needs to be compacted in cases where the bone disease causing fracture (or the risk of fracture) is the loss of cancellous bone mass (as in osteoporosis). The preferred range is about 30% to 90% of the cancellous bone volume. Compacting less of the cancellous bone volume can leave too much of the diseased cancellous bone at the treated site. The diseased cancellous bone remains weak and can later collapse, causing fracture, despite treatment.

[0246] Another general guideline for the selection of the geometry of the expandable body is the amount that the targeted fractured bone region has been displaced or depressed. The expansion of the body within the cancellous bone region inside a bone can elevate or push the fractured cortical wall back to or near its anatomic position occupied before fracture occurred.

[0247] However, there are times when a lesser amount of cancellous bone compaction is indicated. For example, when the bone disease being treated is localized, such as in avascular necrosis, or where local loss of blood supply is killing bone in a limited area, the expandable body can compact a smaller volume. This is because the diseased area requiring treatment is smaller.

[0248] Another exception lies in the use of an expandable body to improve insertion of solid materials in defined shapes, like hydroxyapatite and components in total joint replacement. In these cases, the body shape and size is defined by the shape and size of the material being inserted.

[0249] Yet another exception is the delivery of therapeutic substances, which will be described in greater detail later. In this case, the cancellous bone may or may not be diseased or adversely affected. Healthy cancellous bone can be sacrificed by significant compaction to improve the delivery of a drug or growth factor which has an important therapeutic purpose. In this application, the size of the expandable body is chosen by the desired amount of therapeutic substance sought to be delivered. In this case, the bone with the drug inside is supported while the drug works, and the bone heals through exterior casting or current interior or exterior fixation devices.

[0250] Generally speaking, providing relatively inelastic properties for the expandable body, while not always required, is nevertheless preferred when maintaining a desired shape and size within the bone is important, for example, in bone graft placement or in a vertebral body, where the spinal cord is nearby. Using relatively inelastic bodies, the shape and size can be better predefined, taking into account the normal dimensions of the outside edge of the cancellous bone. Use of relatively inelastic materials also more readily permits the application of pressures equally in all directions to compress cancellous bone. Still, substantially equivalent results can usually be achieved by the use of multiple expandable bodies having highly elastic properties, if expansion is controlled by either internal or external restraints, as previously disclosed.

[0251] IV. Confinement of Filling Material

[0252] A. Dual Stage Filling

[0253] FIGS. 39A to 39D show a multiple stage process for introducing filling material into a cavity formed by an expandable body in cancellous bone. The process is shown in association with treating a vertebral body. This is for the purpose of illustration. It should be appreciated that the process can be used in the treatment of all bone types.

[0254] Use of the multi-stage process is indicated when pre-examination of the targeted bone reveals that a portion of the cortical wall 28 has fractured or failed (as FIG. 39A shows at the anterior region of the vertebral body 26). The failed cortical wall 28 creates gaps and cracks (designated G in FIG. 39A). Typically, remnant chips 500 of the failed cortical bone 28 may lay in the cancellous bone 32 in the region where cortical wall failure has occurred. Filling material can flow or seep through these gaps or cracks C outside of the interior volume of the bone.

[0255] The process begins at the point where the outer guide sheath 72 has been positioned and the guide pin removed in the manner previously described. The physician

introduces a first expandable body 502 into the cancellous bone 32 near the failed cortical bone region, as FIG. 39A shows. The first expandable body 502 is sized, when substantially expanded, to occupy a relatively small volume (i.e., less than about 20%) of the volume of cancellous bone 32 in interior volume 30.

[0256] The physician expands the first expandable body 502, compacting a relatively small region of cancellous bone. Upon collapse and removal of the first body 502, a small cavity 504, caused by the compaction, remains (as FIG. 39B shows).

[0257] The physician introduces the injector tip 90 and injects an aliquot of filling material 96(1) (for example, about 1 cc to about 9 cc) into the formed small cavity 504 (as FIG. 39B shows).

[0258] In a short time interval (before the filling material 96(1) is allowed to substantially set and harden), the physician withdraws the injector tip 90 and introduces a second expandable body 506 into the cancellous bone 32 (see FIG. 39C). The second expandable body 506 is larger than the first body 502. The second body 506 is sized to create the desired geometry for the therapeutic main cavity 508 in cancellous bone 32.

[0259] As FIG. 39C shows, expansion of the second body 506 displaces the earlier injected aliquot of filling material 96(1) in the cavity 504 toward the failed cortical wall region. The aliquot of filling material 96(1) will envelop remnant chips 500 of cortical bone lying in its path. The material 96(1) and enveloped chips 500 are pressed against the failed cortical bone region as expansion of the second body 506 progresses. The first aliquot of filling material 96(1) will begin to set and harden as the main therapeutic cavity 508 is being formed by the expansion of the second body 506. The second body 506 is collapsed and removed, leaving the main cavity 508.

[0260] As FIG. 39D shows, the first aliquot of filling material 96(1) provides a viscous or (in time) hardened boarder region along the anterior edge of the cavity 508. As subsequent injection of additional filling material 96(2) into the main cavity 508 proceeds, as FIG. 39D shows, the viscous or hardened boarder region 96(1) impedes passage of the additional filling material 96(2) as it fills the main cavity 508. The viscous or hardened boarder region 96(1) serves as a dam, keeping the additional filling material 96(2) entering the main cavity 508 from seeping from the vertebral body 26.

[0261] B. Interior Mesh

[0262] FIGS. 40 and 41 show the use of an interior mesh 510 in association with the introduction of filling material into a cavity formed by an expandable body in cancellous bone. The mesh 510 is shown in association with treating a vertebral body, but it should be appreciated that the process can be used in the treatment of all bone types.

[0263] Use of the mesh 510 is indicated when pre-examination of the targeted bone reveals a failed cortical bone region (as FIG. 41 shows at the anterior region of the vertebral body 26), coupled with the lack of enough bone matter, due to advanced disease or a complex fracture, to adequately fill the failed cortical bone region by compacting using an expandable body. Flowable cement material can

flow or seep through the unfilled gaps or cracks (designated G in FIG. 41) present in the failed cortical bone region.

[0264] The mesh 510 comprises a woven structure made from biocompatible material like Goretex™ material, Nitinol™ material, or Dacron™ material. The mesh presents a surface area, which is about 1/3rd to 1/2 of the interior area of the main therapeutic cavity 84 formed by the selected expandable body.

[0265] Before deploying the injector tip 90 into the formed cavity 84 (which is deployed in FIG. 41 by posterolateral access), the physician drapes the mesh 510 over the tip 90, as FIG. 40 shows. As FIG. 41 shows, the viscous flow of filling material 96 injected from the tip 90 carries the mesh 510 into the cavity 84 in advance of the filling material 96. The mesh 510 is urged by the filling material 96 into contact with the anterior region of the bone, including the failed cortical bone region. The mesh 510, permeated with viscous material 96 and resting over the failed cortical bone region, impedes passage of filling material, until hardening occurs.

[0266] V. Delivery of Therapeutic Materials

[0267] A cavity created in cancellous bone by any of the expandable bodies described above can be filled with a medically-appropriate formulation of a drug or a growth factor.

[0268] An expandable body can compact infected cancellous bone to create a space which can be filled with the antibiotic gel in an open or minimally invasive procedure. The cavity places and holds the required amount of drug right at the site needing treatment, and protects the drug from being washed away by blood or other fluids.

[0269] Not only can the dose be optimized, but additional doses can be applied at later times without open surgery, enhancing the therapeutic outcome. If the required cavity for the optimal drug dose weakens the bone, the bone can be protected from future fracture with a cast or with current internal or external metal or plastic fixation devices.

[0270] The therapeutic substance put into bone may act outside the bone as well. A formulation containing chemotherapeutic agent could be used to treat local solid tumors, localized multiple myeloma or even a nearby osteosarcoma or other tumor near that bone.

[0271] The cavity formed by an expandable body can be filled with an appropriate supporting material, like acrylic bone cement or biocompatible bone substitute, which carries a therapeutic substance. Alternatively, the therapeutic substance can be separately delivered before injection of the filling material. Thus, using an expandable body, the physician is able to treat a fracture while also delivering a desired therapeutic substance (like an antibiotic, bone growth factor or osteoporosis drug) to the site.

[0272] As an alternative, to deliver therapeutic substances, bodies can be dipped in a medical formulation (often a dry powder, liquid or gel) containing a medically-effective amount of any desired antibiotic, bone growth factor or other therapeutic agent to coat the body with the above-mentioned substance before it is inserted into a bone being treated. Optionally, the body can be wholly or partially expanded before the coating is performed. Optionally, the coated body can be dried with air or by other means when the applied formulation is wet, such as a liquid or a gel. The body is

refolded as required and either used immediately or stored, if appropriate and desired. Coated on the body, therapeutic substances can be delivered while cancellous bone is being compressed, or with an additional body once the cavity is made.

[0273] The methods described above can also be used to coat Gelfoam or other agents onto the body before use. Inflating the Gelfoam-coated body inside bone will further fill any cracks in fractured bone not already filled by the compressed cancellous bone.

[0274] FIGS. 42A to 42C schematically illustrate one system and method for delivering a therapeutic substance to the bone using an expandable body 529. The body 529 is carried at the end of the catheter tube 530, which conveys liquid to expand the body 529, as previously described.

[0275] As shown in FIG. 42A, the expandable body 529, in a substantially expanded condition, is stabilized with a clip 531 that couples the catheter tube 530 to a wire 532. As shown in FIG. 42B, a measured amount of gel formulation containing the desired amount of substance 533 is uniformly dispensed from a container 534, preferably in thin lines 535, onto the outer surface of the body 536. The coating substance can be the desired compound alone in its natural state (solid, liquid or gas) or in an appropriate formulation, including a dry powder, an aerosol or a solution. As shown in FIG. 42C, the coated body 537 is collapsed and allowed to dry until the gel sets. Alternatively, the body 536 can also be coated without prior expansion. The optional drying time will, of course, depend on the nature of the compound and its formulation. The coated body 237 is suitable for packaging for use by a surgeon.

[0276] Delivering a therapeutic substance on the outside of expandable body used to compact the bone, or with an expandable body introduced after the bone is compacted, is qualitatively different than putting formulated drug into the cavity. When delivered while the bone is compressed, the therapeutic substance becomes incorporated into the compacted bone. This can serve as a way to instantly formulate a slow release version of the substance. The cavity formed by the expandable body can be filled with an appropriate supporting material, like acrylic bone cement or biocompatible bone substitute, as before described.

[0277] Medically-effective amounts of therapeutic substances are defined by their manufacturers or sponsors and are generally in the range of 10 nanograms to 50 milligrams per site, although more or less may be required in a specific case.

[0278] For example, the cavity can accommodate a typical dose of the antibiotic, gentamicin, to treat a local osteomyelitis (bone infection). A typical dose is about 1 gram, although the therapeutic range for gentamicin is far greater, from 1 nanogram to 100 grams, depending on the condition being treated and the size of the area to be covered. A medically-suitable gel formulated with appropriate gel materials, such as Polyethylene glycol, can contain 1 gram of gentamicin in a set volume of gel, such as 10 cc.

[0279] Other antibiotics that can be used to treat bone infection include, for example, ancef, nafcillin, erythromycin, tobramycin, and gentamicin. Typical bone growth factors are members of the Bone Morphogenetic Factor, Osteogenic Protein, Fibroblast Growth Factor, Insulin-Like

Growth Factor and Transforming Growth Factor alpha and beta families. Chemotherapeutic and related agents include compounds such as cisolatin, doxorubicin, daunorubicin, methotrexate, taxol and tamoxifen. Osteoporosis drugs include estrogen, calcitonin, diphosphonates, and parathyroid hormone antagonists.

[0280] VI. Delivery of Biomaterials

[0281] A cavity created in cancellous bone by any of the expandable bodies described above can also be filled with biomaterials.

[0282] Biomaterials which do not flow into the formed cavity, like hydroxyapatite granules or bone mineral matrix, can be pushed down a tube with a long pin whose diameter is slightly more narrow than the inner-diameter of the outer guide sheath, using the minimally-invasive procedure. During open surgery, the physician can approach the bone in the same way.

[0283] If the biomaterial to be inserted does not flow and should not be pushed into the cavity through the guide sheath (as in the case of the hydroxyapatite block, because that can cause damage), the physician can form the cavity using a minimally invasive approach, then punch a hole using standard tools (such as a punch, gouge or rasp) into one side of the cortical bone to allow insertion of the block.

[0284] VII. Bone Marrow Harvesting

[0285] Any of the expandable bodies described above can also be used in the harvesting of bone marrow for diagnostic or therapeutic purposes, for example, in the diagnosis of multiple myeloma or in the treatment of advanced cancers with bone marrow transplants.

[0286] FIG. 47 shows a system 700 for harvesting bone marrow in a bone-marrow producing bone 702. The bone 702, which is shown diagrammatically in FIG. 47, can comprise, for example, the pelvis, or a vertebral body, or a distal radius.

[0287] The system 700 employs a bone marrow harvesting tool 704. The tool 704 includes a catheter tube 706, which carries an expandable body 708 at its distal end. The tool 704 can be deployed into the bone 702 using a minimally invasive approach, as previously described.

[0288] The catheter tube 706 has three concentric and independent lumens 710, 712, and 714 (see FIG. 48). The outer lumen 710 communicates with the interior of the body 78 and is coupled to a source 718 of an inflation liquid. The middle lumen 712 communicates with a source 720 of rinse liquid and a distal opening 716 on the catheter tube 706. The center lumen 714 communicates with a collection container 722 and a second distal opening 724 on the catheter tube 706.

[0289] The body 708 is deployed in a substantially collapsed condition, as already described. Inflation liquid, which is preferably radiopaque, is convey from the source 718 into the body 708 to expand it. As FIG. 48 shows, the body 708 is constrained by selection of relatively inelastic materials or by exterior restraints (as previously described) to assume an elongated shape. Expansion of the body 708 creates a relatively shallow area of compaction 726 in cancellous bone 728 along a relatively long length. The size and shape of the body 708 will depend upon the geometry

of the harvest site and the amount of bone marrow required. In long bones, like the distal radius, and in bones with narrow width but large area, such as the ribs or pelvis, the body 728 is shaped to compress a large area but not a great depth of cancellous bone 728.

[0290] As FIG. 48 also shows, as the body 708 expands, rinse liquid, which can be saline or another suitable bio-compatible liquid, is conveyed from the source 720 into the area 726 (shown by arrows 730 in FIG. 48). The rinse liquid loosens up biological components (such as red blood cells, bone cells, and immune- β cells) within the defined area 726, forming component-rich suspension 732.

[0291] The body 708 is collapsed, and suction is applied through the lumen 714. The suction draws the component-rich suspension 732 from the area 726 into the collection container 722.

[0292] The above sequence of expansion, rinsing, collapse, and aspiration can be repeated to collect additional component-rich suspension 732 in the container 722. The position of the expandable body 708 in the bone 702 can be changed, if desired, to maintain a component-rich suspension 732 for harvesting.

[0293] Use of the expandable body 708 to form the long but shallow compaction area 726 permits the harvest of a significant concentration of therapeutic biological components with less damage to bone than conventional harvesting methods. If desired, standard casts or other fixation devices can be applied to the bone 702 after bone marrow harvesting until the bone 702 heals.

[0294] The features of the invention are set forth in the following claims.

We claim:

1. A method comprising:

selecting a vertebral body for treatment, the vertebral body having a cortical wall enclosing a cancellous bone volume,

providing an expandable device including an expanded configuration and an unexpanded configuration,

introducing the expandable device into the vertebral body through a percutaneous access path while in the unexpanded condition,

expanding the expandable device while disposed within the cancellous bone volume from the unexpanded configuration toward the expanded configuration to create a cavity in the cancellous bone volume, and

placing a filling material including a biomaterial within the cavity.

2. A method according to claim 1

further including controlling the expansion so that the expandable device expands more in an inferior-to-superior direction than in a lateral direction.

3. A method according to claim 1

wherein the expansion is capable of moving fractured cortical bone toward a desired anatomic position.

4. A method according to claim 1

wherein the filling material hardens within the vertebral body.

5. A method according to claim 1

wherein the filling material comprises bone cement.

6. A method according to claim 1

wherein the expandable device expands by inflation.

7. A method according to claim 1

wherein the expandable device comprises a balloon.

8. A method according to claim 1

further including removing the expandable device from the vertebral body.

9. A method according to claim 2

wherein expansion is controlled by restraining expansion of the expandable device in the lateral direction.

10. A method according to claim 9

wherein expansion is restrained by providing restraints external to the expandable device.

11. A method according to claim 9

wherein expansion is restrained by providing restraints internal to the expandable device.

12. A method according to claim 9

wherein expansion is restrained by providing a wall on the expandable device that varies in wall thickness.

13. A method according to claim 1

wherein the biomaterial comprises hydroxyapatite or bone mineral matrix.

14. A system comprising:

an expandable device including an expanded configuration and an unexpanded configuration sized and configured for introduction into a vertebral body through a percutaneous access path while in the unexpanded condition, the vertebral body having a cortical wall enclosing a cancellous bone volume, the expandable device also being sized and configured for expansion while disposed within the cancellous bone volume to create a cavity in the cancellous bone volume,

a filling material including a biomaterial, and

a tool for placing the filling material within the cavity.

15. A system according to claim 14

wherein the expandable device is sized and configured to expand more in an inferior-to-superior direction than in a lateral direction.

16. A system according to claim 14

wherein the expandable device is sized and configured, when expanding, to move fractured cortical bone toward a desired anatomic position.

17. A system according to claim 14

wherein the filling material also comprises bone cement.

18. A system according to claim 14

wherein the expandable device expands by inflation.

19. A system according to claim 14

wherein the expandable device comprises a balloon.

20. A system according to claim 14

wherein the expandable device includes material restraining expansion of the expandable device in the lateral direction.

21. A system according to claim 14

wherein the expandable device includes restraints external to the expandable device.

22. A system according to claim 14

wherein the expandable device includes restraints internal to the expandable device.

23. A system according to claim 14

wherein the expandable device includes a wall that varies in wall thickness.

24. A system according to claim 14

wherein the biomaterial comprises hydroxyapatite or bone mineral matrix.

* * * * *