

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
21 October 2004 (21.10.2004)

PCT


(10) International Publication Number  
**WO 2004/089188 A2**

- (51) International Patent Classification<sup>7</sup>: **A61B**
- (21) International Application Number:  
PCT/US2004/010253
- (22) International Filing Date: 31 March 2004 (31.03.2004)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
60/459,355 31 March 2003 (31.03.2003) US  
60/483,317 26 June 2003 (26.06.2003) US
- (71) Applicant (for all designated States except US): **LI-  
POSONIX, INC.** [US/US]; P.O. BOX 1676, Bothell, WA  
98041-1676 (US).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): **DESILETS,  
Charles, S.** [US/US]; 23616 Edmonds Way, #G, Ed-  
monds, WA 98026 (US). **QUISTGAARD, Jens, U.**  
[US/US]; 4716 NE 187th Place, Seattle, WA 98155 (US).
- (74) Agents: **HESLIN, James, M.** et al.; Townsend and  
Townsend and Crew Llp, Two Embarcadero Center, 8th  
Floor, San Francisco, CA 94111-3834 (US).
- (81) Designated States (unless otherwise indicated, for every  
kind of national protection available): AE, AG, AL, AM,  
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,  
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,  
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,  
KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD,  
MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG,  
PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM,  
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM,  
ZW.
- (84) Designated States (unless otherwise indicated, for every  
kind of regional protection available): ARIPO (BW, GH,  
GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),  
Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), Euro-  
pean (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR,  
GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK,  
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,  
ML, MR, NE, SN, TD, TG).
- Published:**  
— without international search report and to be republished  
upon receipt of that report
- For two-letter codes and other abbreviations, refer to the "Guid-  
ance Notes on Codes and Abbreviations" appearing at the begin-  
ning of each regular issue of the PCT Gazette.*



WO 2004/089188 A2

(54) Title: VORTEX TRANSDUCER

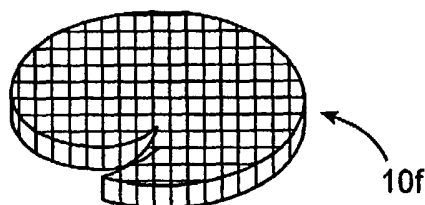

(57) Abstract: A mechanically formed vortex transducer is described. The transducer has a plurality of piezoelectric elements suspended in an epoxy and heat molded into a desired shape. An irregularity in the transducer shape provides for a mechanically induced vortex focal field without the need for electronic steering or lens focusing. A system and methods of making the same are also described.

## VORTEX TRANSDUCER

### BACKGROUND OF THE INVENTION

[0001] 1. Field of the Invention. The present invention relates to an ultrasound transducer for the use in high intensity focused ultrasound (HIFU) applications for medical applications.

[0002] 2. Description of the Background Art. Lysis (the process of disintegration or dissolution) of human tissue using high intensity focused ultrasound (HIFU) is a technique that has been studied for over 50 years. Research into applications of HIFU have revolved mostly around treating malignant tumors in the body either untreatable by other means, or promising a more efficacious treatment modality. HIFU commercialization has been very slow to develop, however, despite some of its early promise. Reasons for this include the inability to visualize the lesions being formed, the necessity of having to lyse an entire malignant tumor to be considered effective, and especially the extended period of time required to lyse a significant volume of tissue. In the last 10 years or so, some companies have been formed to commercialize HIFU for non-cancerous treatment applications. The best-known example is the treatment of enlarged prostate or BPH. Here, it is not necessary to lyse all the tissue to be effective. Advances in the treatment of BPH with drugs, however, has seriously shrunk the commercial prospects for this case. Advances in MRI and diagnostic ultrasound in the last 20 years have aided visualization of HIFU lesions, alleviating a main obstacle to the commercial advancement of the field. Additionally, where small volumes of tissue can be treated, as in hemostasis and blood clot breakup, HIFU is likely to prove to be viable commercially. Lysing large volumes of tissue, as in the case of removing significant amounts of adipose tissue, requires additional technical strategies.

[0003] Cross-sectional histological views of a HIFU lesion formed in vivo in porcine adipose tissue are shown at 40X (Fig. 1) and at 200X (Fig. 2). Tri-chrome staining is employed. Lysed tissue shows blood perfusion around individual fat cells and incursion of phagocytes and red blood cells into the HIFU-treated volume. Lesions formed with HIFU are typically cigar-shaped, with lesions lengths being 5-8 times the diameters. HIFU lesions are typically formed by spherically focusing an ultrasonic beam created by driving electrically a piezoelectric material, causing it to vibrate. These lesions can be as little as 1-2 mm in diameter, and 6-10 mm in length. It would take many lesions to necrose a large volume of

tissue. Preferred thermal processes are generally slow, so that it may take up to 30 seconds to generate enough absorption of the ultrasonic energy to raise the temperature high enough to necrose tissue, and additional time to allow the temperature of tissue between the skin and treated volume to cool sufficiently before the next lesion is created. A simple calculation shows that it could take hours to ablate a volume of tissue on the order of 250cc with a single transducer making individual lesions. Diminishing the time required to ablate a large volume of tissue, as in adipose tissue reduction, could mean the difference between a successful commercial product and an unsuccessful one.

**[0004]** Several strategies can be employed to reduce the time between making individual lesions, such as using multiple, mechanically scanned HIFU transducers, scanning the transducer(s) continuously, and/or using some kind of linear or 2D transducer array or structure to generate multiple focal spots. While some combination of these strategies could be employed, a major physical limitation of reducing scanning time remains the small diameter of the focused ultrasound beam. A defocusing strategy holds some promise of increasing the effective spot size by spreading the energy more laterally than lengthwise, creating a more spherical-shaped lesion. "Wobbling" the HIFU transducer mechanically about its axis could serve to do this, and such ideas have been reported in the literature. However, it would be certainly less complicated and expensive to build the defocusing into the HIFU transducer itself.

**[0005]** A method of creating an annular focal zone where the diameter of the annulus is adjustable has been reported by Cain and Umemura (Cain, Charles A. and Shin-Ichiro Umemura, "Concentric-Ring and Sector-Vortex Phased-Array Applicators for Ultrasound Hyperthermia", *IEEE Trans. on Microwave Theory and Techniques*, Vol MTT-34, No. 5, May 1986, pp. 542-551.) and (Umemura, Shin-Ichiro and C.A. Cain, "The Sector-Vortex Phased Array: Acoustic Field Synthesis for Hyperthermia", *IEEE Trans. on Ultrasonics, Ferroelectrics, and Frequency Control*, Vo. 36, No. 2, March 1989, pp. 249-257.) and Hynynen *et. al.* (Fjield, T., V. Sorrentino, H. Cline, and K. Hynynen, "Design and experimental verification of thin acoustic lenses for the coagulation of large tissue volumes", *Phys. Med. Biol.*, Vol 42, 1997, pp. 2341-2354.) and (Fjield, T. and K. Hynynen, "Experimental Verification of the Sectored Annular Phased Array for MRI Guided Ultrasound Surgery", Proc 1996 IEEE Ultrasonics Symposium, pp. 1273-1276.) and (Fjield, T. and K. Hynynen, "The Combined Concentric-Ring and Sector-Vortex Array for MRI Guided Ultrasound Surgery", *IEEE Trans. on Ultrasonics, Ferroelectrics, and Frequency*

*Control*, Vo. 44, No. 5, September 1997, pp. 1157-1167.) and (Fjield, T., N. McDannold, C. Silcox, and K. Hynynen, "In Vivo Verification of the Acoustic Model Used to Predict Temperature Elevations for MRI Guided Ultrasound Surgery", Proc 1998 IEEE Ultrasonics Symposium, pp. 1415-1418.). This concept, dubbed the sector-vortex array, has been  
5 implemented using electronic array techniques or simply adding a mechanical sector-vortex lens onto the front of a planar transducer. The effect of this lens is to create a double-cone field pattern that yields an annular ring in cross-section.

[0006] Extensive research with mechanically scanned, spherically focused transducers has been conducted in HIFU fat-tissue mimicking gel phantoms and *in vivo* porcine adipose  
10 tissue. The purpose of this research is to determine basic design parameters for optimizing the lysing of subcutaneous adipose tissue and develop candidate lysing and scanning protocols for inclusion into a product development specification and initial human safety trials. This research has shown that challenges remain in reducing the overall treatment time to the desired values. While various scanning strategies have proven fruitful in reducing the  
15 heat build-up tissue in the zone between the skin and HIFU-created focal volume, and thus reducing scanning time, even greater efficacy can be shown if the focal zone overall diameter is increased significantly. Transducers with built-in vortex capability could prove to be a relatively simple, cost-effective means to achieve this capability.

[0007] Spherical focusing is typically achieved by bonding a plano-concave lens on to the  
20 front of a planar piezoelectric material, or shaping the piezoelectric material into a spherical bowl. High ultrasonic intensities ( $1-4 \text{ kW/cm}^2$ ) are created driving the piezoelectric material at very high power levels, and focusing the beam very tightly. Absorption of this energy by tissue elevates its temperature. Raising this temperature in excess of  $60^\circ\text{C}$  in the focal zone coagulates cell proteins, thereby ablating the tissue. There is a very sharp line between  
25 ablated and unablated tissue, as seen in Fig. 1. If the intensity is high enough, the temperature rise is sufficient to cause boiling and the production of small bubbles, producing a lesion with the elongated shape of a weather balloon at high altitudes ("tadpole" shape to others). At an even higher threshold, inertial cavitation (bubble creation) may occur, which can lyse tissue through thermo-mechanical means.

[0008] Lesions made *in vivo* in porcine tissue with spherically focused transducers show  
30 remarkably similar characteristics to those made in adipose tissue. Cigar-shaped lesions are made at relatively low power levels at longer insonification times, following the 6 dB contour

of a classically spherically focused lens, and elongated weather balloon-shaped lesions are made at relatively high power levels where suspected boiling creates bubbles which reflect acoustic power back to the skin surface. At very high power levels, or too long insonification times, excessive heat can be generated above the focal zone which will lyse tissue up to and including the skin surface. While large volumes of tissue can be lysed in this manner, controlling this type of lesion growth can be problematic when considering patient and environmental variability.

[0009] Reducing the focal intensity at the center of the lesion and spreading the energy out over a larger volume should help alleviate the creation of a boiling hot spot while allowing more energy to be deposited during an insonification period, ultimately reducing the scanning time.

[0010] Composite piezoelectric materials have been a subject of research and development for nearly 25 years. Ultrasonic transducers and arrays for diagnostic imaging purposes have been manufactured since the late 1980's, and have application in such diverse areas as sonar and non-destructive testing. One manufacturer (Imasonic, Besançon, FR) builds custom composite HIFU applicators which are used by several research and commercial organizations. Popularly known as piezocomposites, these materials are made by taking solid blocks of piezoelectric ceramic, dicing the block into a forest of tall, thin pillars of ceramic, and backfilling the dicing kerfs with a polymer. This composite ceramic/polymer material is then processed like a normal solid transducer ceramic into thin plates. The volume fraction of the composite is controlled by the dicing kerf width and spacing, and the composite material properties can thereby be tailored to specific applications.

[0011] While many superior properties of composites are exploited in diagnostic imaging, the chief interest for HIFU is the ability to form composites into arbitrary shapes. In diagnostic imaging, the superior piezoelectric and acoustic properties of composites are exploited to produce wideband frequency responses, which are of little interest in HIFU at this time. Flexible polymer materials are often used as composite fillers which allow the material to be easily manipulated into cylindrical or spherical shapes. However, flexible composites are inherently high loss materials and unsuitable to the high power levels used in HIFU. Flexible materials would distort and ultimately disintegrate due to the heat build-up inside the material itself under high drive levels. Using less flexible polymers as composite filler materials would increase the composites' power handling capabilities due to lower

intrinsic loss mechanisms, but would then make forming the composite into a curved shape seemingly impossible. '

[0012] The answer to this dilemma is to make use of an interesting property of many hardset epoxies: these materials can be heated at a relatively low temperature into a partially  
5 cured state (namely, a B-stage cure) that is quite hard, but fairly brittle. In this state, the material can be processed, that is diced, filled, ground, lapped, and electroded into the thin sheets needed for HIFU applicators, and then reheated to a temperature somewhat above the original B-stage cure temperature. At this point, the polymer softens considerably and can be  
10 clamped into a mold shaped to the configuration desired (for instance, a spherically shaped bowl or vortex shape) and reheated to a much higher temperature. The epoxy filler then will fully cure, and further heat treatment can elevate the epoxy glass transition temperature, the temperature at which the polymer suddenly will soften, to levels between 120° and 200°C. The material thus formed is relatively low loss and capable of handling HIFU power levels, albeit with less efficiency than solid, high power, piezoelectric ceramics.

[0013] While requiring custom molds and clamping equipment, ultimately it is easier and  
15 cheaper to produce ceramic elements this way than to grind them directly using expensive equipment or hand labor; the elements are more rugged as well, which is a very important consideration. The lower efficiency is not expected to be a limitation in fat lysis since higher frequencies can be used for the small treatment depths, and thus high intensities can be  
20 achieved with relatively low drive levels. This is easily demonstrated by considering the fact that the intensity antenna gain for a focused radiator increases as the square of the frequency. An optimum frequency for HIFU at a given depth of focus can be obtained from the following equation:

$$f_{opt} = 1/(2\alpha z),$$

25 where  $f_{opt}$  is the optimum frequency,  $\alpha$  is the ultrasonic absorption of fat, and  $z$  is the tissue depth to be treated. For fat treated at 2 cm of depth, the optimum frequency for maximum heat deposition is 4.2 MHz. Other considerations may change the actual operating frequency, of course.

[0014] Clearly the marriage of a technique of increasing the focal area of a HIFU applicator  
30 like the vortex concept and a means of easily and cheaply implementing this interesting structure like piezocomposites can reduce the overall treatment time for lysing large volumes

of adipose tissue. Reducing treatment time and cost are key areas which will determine the fate of lysis commercialization efforts.

[0015] Sector-vortex array design has been extensively described and simulated by Cain and Umemura, Umemura and Cain, and numerous papers from Hynynen and co-workers at Brigham's and Women's Hospital at Harvard. They describe an implementation whereby the driving electrode of a spherical radiator is divided into N number of equal sized, pie-shaped sectors. Following Cain, driving signals are applied to the N sectors with a phase distribution over the N sectors determined by:

$$\phi = m(\theta_l),$$

for  $l = 1, 2, \dots, N$  where  $m$  is the vortex mode number, and  $\theta_l = i2\pi/N$ . The phase distribution over the N sectors is such that that the excitation field rotates around the radiator at a phase velocity  $\omega_0/m$ . When N is large, an approximate analytic expression for the acoustic field in the focal plane can be derived; this field has a shape determined by the  $m$ th order Bessel function. The vortex-shaped field is zero along the central axis for  $m \neq 0$ , and has a diameter proportional to the vortex mode  $m$ . The field in cross-section resembles an annulus with side lobes at radii greater than the annulus.

[0016] However sector-vortex designs require complex electronics to drive the transducers in order to produce the vortex focal field. The electronics are required to drive either sector transducers or phased arrays in sequence. Some prior teachings rely on ancillary technologies such as the use of MRI machines to detect hotspots, and provide for additional electronic to provide real time corrections in the electronic firing of the various transducer elements to eliminate or reduce the occurrence of out-of-field ultrasound excitation. Complex lenses have also been described to facilitate the steering of the ultrasound energy into the body.

[0017] Thus there remains a need in the art for a robust vortex transducer, having a simplified design that can operate without the requirement of complex and expensive electronics.

[0018] There is further a need for a vortex transducer that can be aimed without the use of a lens.

[0019] There is still further a need for a vortex transducer having a fast activation and treatment time for reliably depositing a fixed amount of energy into a focal zone.

## BRIEF SUMMARY OF THE INVENTION

[0020] Some of the needs of the art are addressed by the present disclosure. In accordance with the needs of the art, it is an objective of the present invention to provide a transducer capable of producing a vortex focal zone.

5 [0021] It is further an objective to provide a transducer able to create a vortex focal zone without the use of complex electronics.

[0022] It is still further an objective of the present invention to be able to reliably aim a vortex transducer without using a lens or electronic steering.

10 [0023] Yet another objective is to provide for a vortex transducer with a cheap and cost effective manufacturing process.

[0024] One or more of the above objectives is met utilizing a mechanically formed vortex ultrasound transducer capable of producing at least one, substantially annular focal region when the transducer is excited.

15 [0025] In a second embodiment there is a mechanically formed ultrasound transducer comprising a plurality of piezoelectric elements suspended in a polymer, and having an irregular shape in order to produce a vortex focal field.

[0026] The polymer used in the creation of a heat set transducer shape has a liquid state when introduced into a diced piezoelectric ceramic, a semi solid state during processing and a fixed solid state upon completion of a heat treatment step.

20 [0027] A method of manufacturing is disclosed comprising the steps of first shaping a piezoelectric ceramic into a desired form, the form having a front end and a back end. Second dicing the front end to create a plurality of elements, the elements being attached to the back end and separated by dicing channels. Third, filling the dicing channels with a polymer material and allowing the polymer to gel. Fourth, creating a transducer form by removing the  
25 back end such that the elements are separated from one another. Fifth, pressing the transducer form into a mold and heating the transducer form such that the resin is heated above the B-stage and allowing the resin to cross-link and cool in a set shape. Sixth, treating at least one surface of the transducer form with a conductive material such that all elements are in contact with the conductive material. An additional step involves the formation of a shaped  
30 irregularity to produce the vortex effect. This step can be inserted into the steps above where ever desired and there is no best order for the introduction of this step. The shaped



irregularity can be part of the original forming of the transducer form, or it can be created later by cutting or grinding the transducer form such that the desired irregularity is introduced.

#### BRIEF DESCRIPTION OF THE DRAWINGS

- 5 [0028] Fig. 1 is a histological view of a HIFU lesion in porcine adipose tissue at 40X magnification.
- [0029] Fig 2 is a histological view of a HIFU lesion in porcine adipose tissue at 200X magnification.
- [0030] Fig. 3 is a schematic illustration of a vortex ultrasound transducer/applicator design  
10 in accordance with the present invention.
- [0031] Figs. 4a-4d show a cross-sectional focal zone intensity distributions for a series of sector-vortex applicators, modes 0 through 3, demonstrating the annular structure of the field patterns and the widening of the annulus as a function of mode number.
- [0032] Figs. 5a and 5b is a further illustration of an embodiment of the present invention.
- 15 [0033] Figs. 6a-6g illustrate a process for making transducers in accordance with the present invention.

#### DETAILED DESCRIPTION OF THE INVENTION

- [0034] Described herein is an implementation of a version of the sector-vortex concept. While this concept is known, this disclosure implements the design in a novel manner. In  
20 order to avoid the complexities and cost of an electronic beamformer, or the use of a sector-vortex lens with its attendant issues in reliability, acoustic losses and reverberations, and cooling, a continuous vortex lens can be incorporated into the piezoelectric transducer material itself. This can be done by building the transducer out of piezoelectric composite material which can be molded into a vortex lens. This eliminates the need for complex  
25 driving electronics and all the issues of an external lens. This design could be instrumental in building cheap, reliable devices that can potentially reduce treatment time by factors of two to eight.
- [0035] The present invention implements an applicator design that incorporates the phase shifts mechanically, not electronically. This is mathematically equivalent to letting  $N \rightarrow \infty$ ,  
30 that is letting the number of sectors become infinite, or making a continuously curving shape,

as shown in Fig. 3, that yields a  $2\pi m$  phase shift after one revolution. The applicator would also be preset with spherical focus. As one can see, this shape would be difficult to machine in a solid piezoelectric ceramic material. But one can easily imagine molding a piezocomposite into this shape using steel molds manufactured with a ball end mill or EDM (electric discharge machining) machine. Fig. 3 also illustrates the generic shape of a continuously variable sector-vortex applicator made by splitting a spherical bowl along a radius and translating one split edge axially in relationship to the other edge.

[0036] A  $2\pi$  phase shift (mode number = 1) corresponds to one wavelength of the driving frequency; at 4 MHz in water, this is 380  $\mu\text{m}$ . Thus, for mode 1, the discontinuity at the split on the edge of the spherical bowl would then be 380  $\mu\text{m}$ , mode 2, 760  $\mu\text{m}$ , and so on. Splitting a spherical bowl made of piezocomposite along one radial line, and forming it with a discontinuity on the order of 1 mm is possible, but represents the major technical challenge in the proposed project.

[0037] Fig. 4a-4d show the cross-sectional focal patterns for modes 0, 1, 2, and 3, respectively. Mode 0 reduces just to the simple spherical radiator, and serves as the standard by which to judge the increase in focal zone area in other designs.

[0038] Theoretically, the field along the central axis of the sector-vortex applicator is zero and would not contribute to tissue lysis. However, heat generated in the annulus will flow into this region and will not have ready access to a heat sink. It is expected, if the annulus is not too large, that the temperature will rise to therapeutic levels under interesting drive conditions, forming a large solid lesion.

[0039] Based on the proceeding description, it is possible to produce a vortex transducer. The present invention comprises a mechanically formed vortex ultrasound transducer capable of producing at least one, substantially annular focal region(s) when said transducer is excited. The transducer may incorporate a solid piezoelectric material or a composite piezoelectric material. Furthermore the transducer may incorporate one or more matching layers. The transducer may incorporate a filler material in front of the transducer or backing material in back of the transducer. The transducer may also be formed from a single contiguous piezoelectric element. See Figs. 5a & 5b, where the reference numbers are as follows:

1. Back electrode connection and wire
2. Electrical connector

3. Transducer housing
4. Backing material
5. Piezoelectric element
- 5a. Matching layer(s) on front of piezoelectric element
- 5 6a.-6b. Fluid inlet and outlet for cooling
7. Front electrode connection and wire
8. Filler material
9. Face material
10. Piezoelectric material

10 [0040] A method of making the transducer of the present invention is also provided. The method comprises the steps of: first shaping a piezoelectric ceramic into a desired form, the form having a front end and a back end. Second dicing the front end create a plurality of elements, the elements being attached to the back end and separated by dicing channels. Third filling the dicing channels with a resin material and allowing the resin to gel. Fourth, creating a  
15 transducer form by removing the back end such that the elements are separated from one another. Fifth, pressing the transducer form into a mold and heating the transducer form such that the resin is heated above the B-state and allowing the resin to cross link and cool in a set shape. Sixth, treating at least one surface of the transducer form with a conductive material such that all elements are in contact with the conductive material. An additional step involves  
20 the formation of a shaped irregularity to produce the vortex effect. This step can be inserted into the steps above where ever desired and there is no best order for the introduction of this step. The shaped irregularity can be part of the original forming of the transducer form, or it can be created later by cutting or grinding the transducer form such that the desired irregularity is introduced.

25 [0041] The manner of producing the transducer is detailed below. First, the piezoelectric material is formed into a desired form (Fig. 6a). The form may include the irregularity used to mechanically create the vortex transducer effect, or the irregularity can be introduced into the finished transducer form. The shaping of the piezoelectric ceramic into a desired form follows procedures well established in the art of making ultrasound transducers. The principal  
30 embodiment calls for a flat shape having sufficient size to be later molded into the desired three dimensional form. Otherwise there is no restriction or requirement on the formation process. Similarly the dicing of the ceramic is also well known. In the second step the

ceramic is diced such that there is sufficient depth in the dicing channels to allow a resin like material to fill the channels (Fig. 6b). The filling of the channels with a polymer ( e.g. epoxy or urethane) provides a solid material to support and maintain the elements in a fixed position relative to one another (Fig. 6c). Once the polymer is set sufficiently to hold the elements in place without the structural support of the ceramic back plate, the back plate is removed (Fig. 6d). Now the transducer form comprises the individual elements and the polymer used to suspend the elements and hold them in place.

**[0042]** The resulting two-phase composite material can be tailored to have a number of interesting electro-mechanical and purely mechanical properties by the choice of parameters like ceramic volume fraction and polymer filler material. Of particular interest in permanently forming piezocomposites into interesting shapes is the use of hardset (high durometer) thermoset resin systems such as epoxy as the polymer filler. The set epoxy in the composite can be partially cured at a relatively low temperature where it “gels,” or turns substantially solid from a liquid state. At a slightly higher temperature, the epoxy can then progress into a B-stage partially cross-linked cure which is quite hard, but very brittle. At this level the piezocomposite can be processed easily by grinding to a thickness as a flat plate and applying electrodes. As a final step, the piezocomposite can then be reheated slightly past the B-stage temperature where it softens considerably and can be formed into shapes.

Commonly, the piezocomposite is placed in a warm bottom half of a mold that allows the plate to take the shape of the mold, a top half of the mold is then clamped to the bottom half, and then the mold is heated to a high final curing temperature. At this point, the epoxy filler cures to a fully cross-linked, tempered, stage over a period of time determined by the resin system. The resulting molded piezocomposite now has a shape that takes on the shape of a lens. In this manner, a piezoelectrically active lens can be made that is quite rugged, eliminating the need for separate focusing lenses.

**[0043]** The next step provides an essential process step of the present invention. That is the molding of the transducer form to shape the elements and polymer (epoxy) combination into a shaped transducer (Fig. 6e). The form selected will dictate the focal range, depth and shape of the ultrasound focal zone. Thus the mold must be carefully determined and created since it is not possible to electronically steer the transducer when it is completed. When the transducer form is in the mold, the mold and transducer form are heated until the resin/epoxy is heated past the B-stage of the filler material. This makes the epoxy/resin softer so the transducer form can be properly shaped. The final shaped transducer (Fig. 6f) is then coated

with a conductive material and electronically connected (Fig. 6g) to an activation device such as a high voltage supply (not shown).

[0044] The reference numbers used in Figs. 6a-6g are as follows:

- 10a Piezoelectric ceramic
- 5 10b Dized ceramic
- 10c Filled w/epoxy 13
- 10d Back removed
- 10e Heat molding
- 10f planar transducer w/irregularity
- 10 10g Heat molded w/irregularity and conductive layer 12 and electrical connection. 14

[0045] The transducer can be made to operate either narrowband (roughly at one frequency) or broadband (over a range of frequencies). The decision on narrow or broadband will be left to the designer to choose based on the specific application. The designer should consider the beam pattern the vortex transducer will produce before finalizing the design. The  
15 beam shape will produce a double funnel focus field similar to that described in the prior art; however, with the simplified transducer of the present invention, there will be no need for complex electronics to steer or focus the beam, or run a complex pattern of individual element activations.

[0046] Additional modifications and variations of the present invention are possible in light  
20 of the above teachings and the description provided herein is not to be meant as limiting the invention to the descriptions provided. It is understood those skilled in the art will be able to utilize the present teaching without substantial variation, and such practices are within the intended scope of the present invention and the appended claims.

WHAT IS CLAIMED IS:

- 1           1.     A mechanically formed vortex ultrasound transducer capable of  
2 producing at least one, substantially annular focal region(s) when said transducer is excited.
- 1           2.     The transducer of claim 1 where the transducer incorporates a solid  
2 piezoelectric material.
- 1           3.     The transducer of claim 1 where the transducer incorporates a  
2 composite piezoelectric material.
- 1           4.     The transducer of claim 1 where the transducer incorporates one or  
2 more matching layers.
- 1           5.     The transducer of claim 1 where the transducer incorporates a filler  
2 material in front of the transducer or backing material in back of the transducer.
- 1           6.     The transducer of claim 1, being formed of a single contiguous  
2 piezoelectric element.
- 1           7.     A mechanically formed ultrasound transducer comprising a plurality of  
2 piezoelectric elements suspended in a polymer and having an irregular shape such that a  
3 vortex focal field is produced when the transducer is excited.
- 1           8.     A polymer for use in the creation of a heat set transducer shape having  
2 a liquid state when introduced into a diced piezoelectric ceramic, a semi solid state during  
3 processing and a fixed solid state upon completion of a heat treatment step.
- 1           9.     The polymer of claim 8, wherein the polymer is an epoxy.
- 1           10.    A system for producing a vortex ultrasound focal field comprising:  
2 a mechanically formed ultrasound transducer having an irregular shape for  
3 creating said vortex; and  
4 an activation switch.
- 1           11.    A method of creating a vortex transducer comprising the steps of:  
2 (a) shaping a piezoelectric ceramic into a desired form, the form having a  
3 front end and a back end;

4                   (b)     dicing said front end create a plurality of elements, said elements being  
5 attached to said back end and separated by dicing channels;

6                   (c)     filling said dicing channels with an epoxy material and allowing said  
7 epoxy to gel;

8                   (d)     creating a transducer form by removing said back end such that said  
9 elements are separated from one another;

10                  (e)     pressing said transducer form into a mold and heating said transducer  
11 form such that the epoxy is heated above the B-stage and allowing the resin to cross link and  
12 cool in a set shape;

13                  (f)     treating at least one surface of the transducer form with a conductive  
14 material such that all elements are in contact with said conductive material; and

15                  (g)     making a shape irregularity in the transducer form such that the  
16 transducer will produce a vortex effect.

1                   12.     The method of claim 11, wherein step (g) may be performed before  
2 performing any one of steps (a)-(f).

+

1 / 4

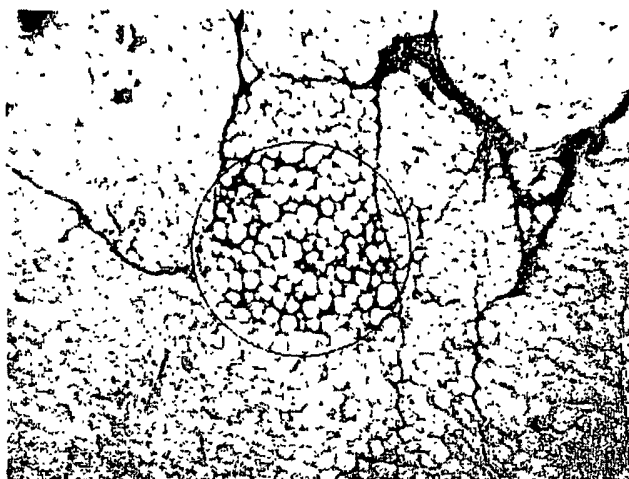


FIG.

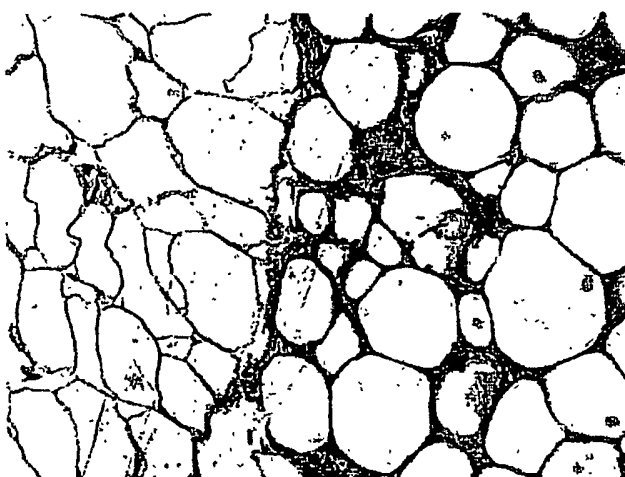


FIG. 2

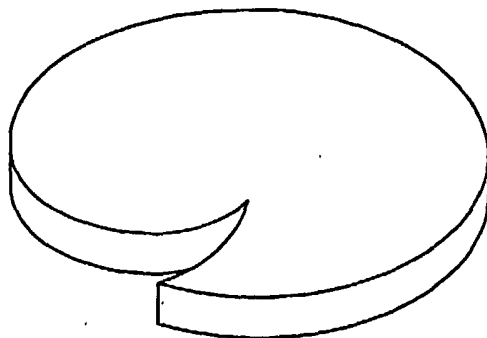


FIG. 3

+



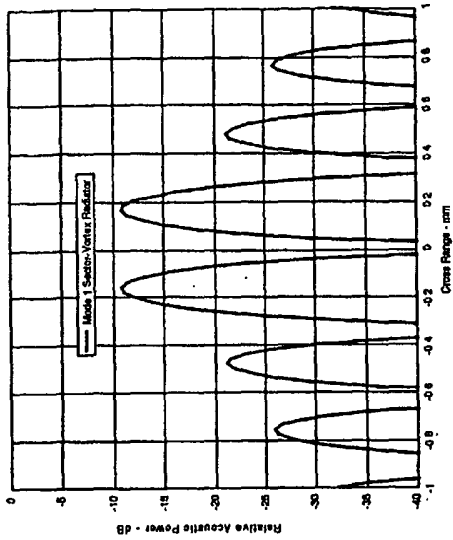


FIG. 4b

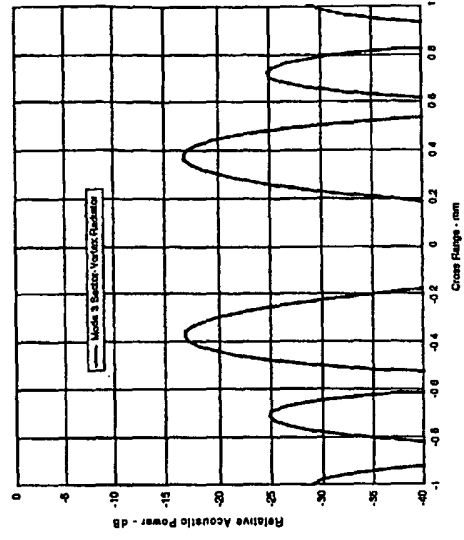


FIG. 4d

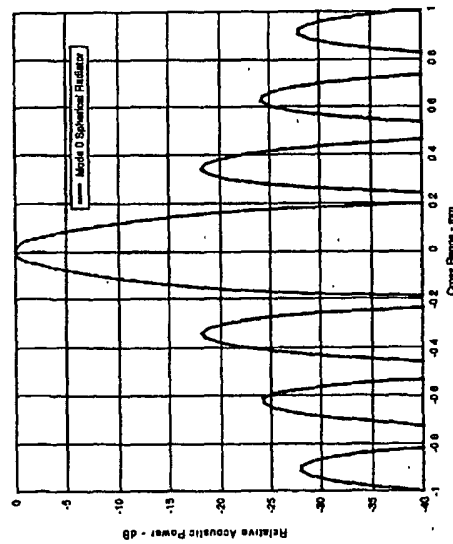


FIG. 4a

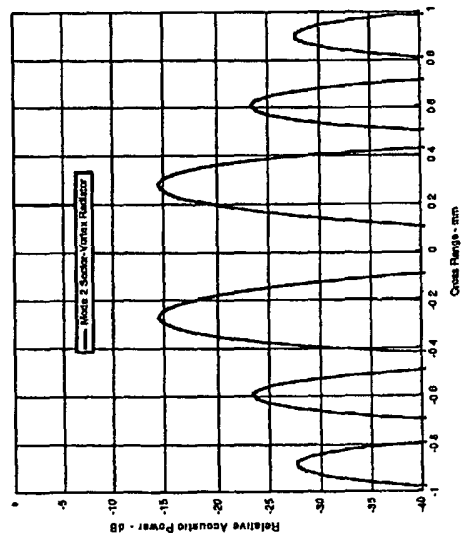


FIG. 4c

+

3 / 4

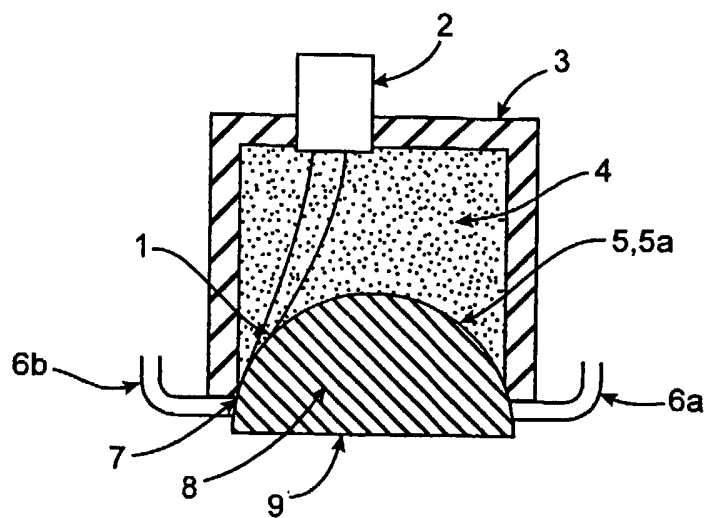


FIG. 5a

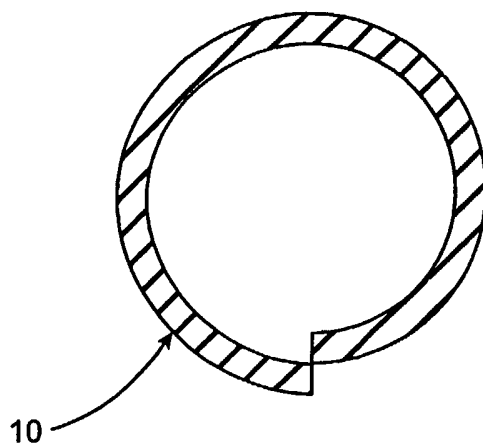


FIG. 5b

+

+







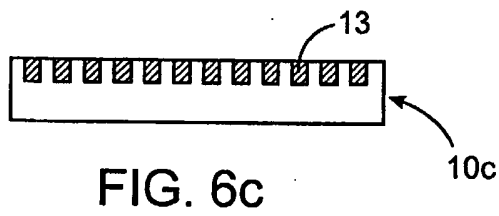


FIG. 6f

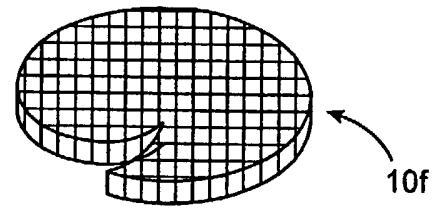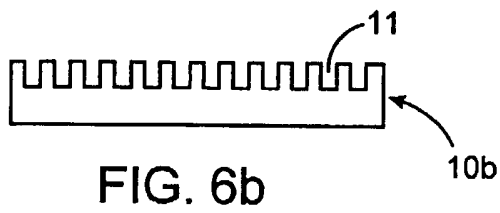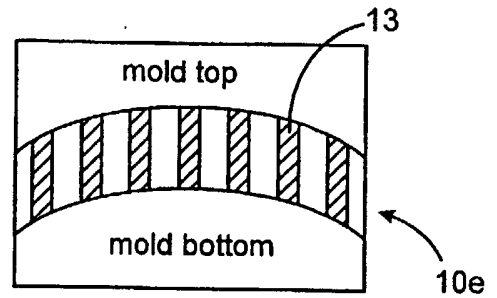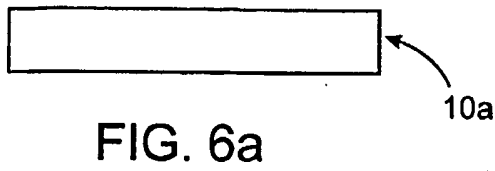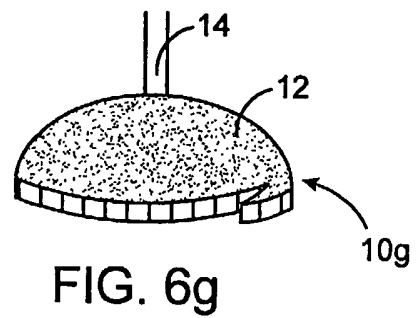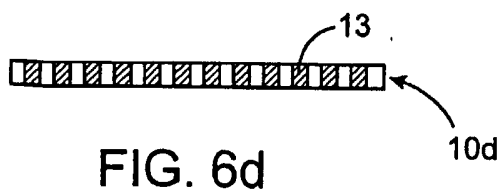

+