



(51) International Patent Classification:

A61G 13/12 (2006.01) A61F 5/37 (2006.01)
A61F 5/01 (2006.01) A61G 13/00 (2006.01)
A61B 46/27 (2016.01)

(21) International Application Number:

PCT/US2018/059190

(22) International Filing Date:

05 November 2018 (05.11.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/582,989 08 November 2017 (08.11.2017) US
62/703,126 25 July 2018 (25.07.2018) US

(71) Applicant: SMITH & NEPHEW, INC. [US/US]; 1450
Brooks Road, Memphis, Tennessee 38116 (US).

(72) Inventors: ZAHYNACZ, Daniel; c/o Smith & Nephew,
Inc., 1450 Brooks Road, Memphis, Tennessee 38116 (US).
OBENDORF, William D.; c/o Smith & Nephew, Inc.,
1450 Brooks Road, Memphis, Tennessee 38116 (US).
SMITH, Graham; c/o Smith & Nephew, Inc., 1450 Brooks
Road, Memphis, Tennessee 38116 (US). TRENHAILE,
Scott; c/o Smith & Nephew, Inc., 1450 Brooks Road, Mem-
phis, Tennessee 38116 (US).

(74) Agent: MARAIA, Joseph M. et al.; BURNS & LEV-
INSON, LLP, 125 Summer Street, Boston, Massachusetts
02110 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,
KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

(54) Title: SURGICAL HAND WRAP AND STERILE CONNECTOR

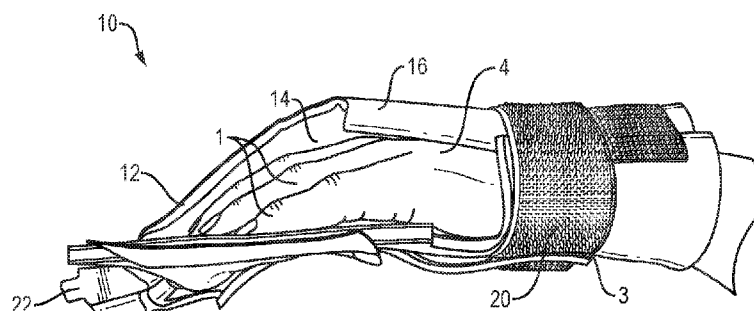


FIG. 2

(57) Abstract: Devices to secure the hand of a patient to a limb positioning device while evenly distributing the applied traction load across the patient's hand and wrist are disclosed. The hand is placed in the open position into a soft mitten, while an anatomically-shaped plate is attached to the mitten for supporting the palm of the hand in the open position. Straps are then secured around the patient's wrist and hand. Finally, the entire device is overwrapped an elastic bandage and secured to the limb positioning device. When traction is applied, the shape of the plate, the construction of the mitten, and the straps combine to allow low-contact pressure across the patient's hand and wrist.

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*

SURGICAL HAND WRAP AND STERILE CONNECTOR

FIELD

This disclosure relates generally to devices which are used to position a limb of a patient during a medical procedure and, more particularly, to devices which are used to position the shoulder and arm of a patient during shoulder surgery.

BACKGROUND

Orthopedic shoulder surgery involves complexities not encountered in other surgeries, such as knee surgery. For example, during shoulder surgery, ports or incisions are placed through a patient's shoulder joint in order to provide access for instruments such as light sources, visual scopes, and surgical tools. However, it is sometimes desirable for a surgeon to gain access to a different area of the joint, without creating new ports, by rotating the operative limb and holding it in a new position. This distraction is achieved by applying traction to the arm via the hand and/or the forearm while it is secured to a limb positioning device.

Traction loads of up to 30lbs generally require that the hand be tightly secured to the limb positioning device. To accomplish this, the hand may be attached to a handle or bar and secured over the bar into a balled fist. The arm and hand are typically draped or covered in a sleeve and the entire arm is wrapped with an elasticated bandage. The distal end of the sleeve is then attached to the limb positioning device. However, this method of securing the hand can lead to numbness in the patient's hand and fingers, and furthermore reduces control of the rotation of the hand and wrist.

Another problem inherent to the use of limb positioning devices is that the non-sterile limb positioning device is usually clamped to the operating room table. A sterile connection is typically made to the patient by passing a sterile rope with a hook attached to its distal end through the limb positioning device, while the sleeve covering the patient's arm and hand is attached to the hook. However, this procedure requires a non-sterile operating assistant outside of the sterile field to pass the rope to a sterile operating assistant inside the sterile field, which leads to the possibility of cross-contamination.

BRIEF SUMMARY

Described herein is a device to secure the hand of a patient to a limb positioning device while evenly distributing the applied traction load across the patient's hand and wrist. The hand is placed in the open position into a soft mitten, while an anatomically-shaped plate is attached to the mitten, supporting the palm of the hand. Straps are then secured around the patient's wrist and hand. Finally, the entire device is overwrapped an elastic bandage and secured to the limb positioning device. When traction is applied, the shape of the plate, the construction of the mitten, and the straps advantageously combine to allow low-contact pressure across the patient's hand and wrist. Further described herein is a sterile drape with a sterile connector and its distal end, which advantageously allows a sterile operating assistant to connect and disconnect the surgical hand wrap of this disclosure from the limb positioning device. This in turn allows for faster turnover between procedures by eliminating the need for re-usable (i.e., autoclaveable) interfaces.

Further examples of the surgical hand wrap and sterile connector of this disclosure may include one or more of the following, in any suitable combination.

In examples, the surgical hand wrap of this disclosure includes a flexible mitten portion having an interior side and an exterior side. The mitten portion is configured to enclose at least a hand of the patient in an open position. The hand wrap also includes an anatomically-shaped plate for supporting a palm of the hand in the open position and at least one closeable strap for wrapping around the exterior side of the mitten portion. When traction is applied to the patient's arm, the plate, the mitten portion, and the at least one strap combine to allow low-contact pressure across the hand of the patient.

In further examples, the mitten portion is comprised of at least one of urethane foam and polyester fabric. In examples, the interior side of the mitten portion includes an anti-slip material, which may be one of SBR bonded foam, rubber, and urethane foam. In examples, an end of the at least one strap is attached to the mitten portion. In other examples, the at least one strap is free-floating. In further examples, the at least one strap is secured to the plate and the hand wrap is enclosed within a bandage. In examples, the plate is made of polycarbonate plate. In examples, the plate has a distal portion configured to attach to the limb positioning device and a curved center portion for supporting the palm of the hand in the open position. In examples, the plate includes at least one slot configured for the passage of the at least one

strap. In further examples, a padding is disposed within the mitten portion for securing about a wrist of the patient. A thickness of the padding is selected to be greater than a thickness of the mitten portion.

In examples, the sterile connector of this disclosure includes a T-fitting at a distal end configured to couple to a support member of a sterile hand wrap and a shaft at a proximal end configured to mate with a receiver of the limb positioning device. The connector is attached to a flexible dam portion at a distal end of a sterile covering, the covering configured to cover at least a portion of the limb positioning device. In examples, the connector is made of polymers or metals. In examples, the covering is made of a clear, polyethylene plastic. In examples, the flexible dam portion is made of rubber. In examples, a proximal end of the covering is open to cover at least a portion of the limb positioning device. In examples, the covering is configured to fold in a telescopic fashion. In examples, the connector is attached to the flexible dam portion in an interference fit. In other examples, the connector is attached to the distal end of the covering.

These and other features and advantages will be apparent from a reading of the following detailed description and a review of the associated drawings. It is to be understood that both the foregoing general description and the following detailed description are explanatory only and are not restrictive of aspects as claimed.

BRIEF DESCRIPTION OF THE DRAWINGS

The disclosure will be more fully understood by reference to the detailed description, in conjunction with the following figures, wherein:

FIGS. 1A and 1B illustrate a prior art surgical hand wrap;

FIG. 1C shows the pressure distribution across the hand and wrist under a typical traction load;

FIG. 2 is a cut-away view of an exemplary mitten portion of the hand wrap of this disclosure;

FIG. 3A illustrates an exemplary palm support plate of the hand wrap of this disclosure;

FIG. 3B illustrates an exemplary wrist support of the hand wrap of this disclosure;

FIG. 4 shows an exemplary overwrapping of the hand wrap of this disclosure;

FIG. 5A is a schematic illustration of a limb positioning device for applying traction to the hand wrap of this disclosure; and

FIGS. 5B-E show an exemplary sterile connector and drape for connecting the hand wrap of this disclosure to the limb positioning device of FIG. 5A.

5

DETAILED DESCRIPTION

In the description that follows, like components have been given the same reference numerals, regardless of whether they are shown in different examples. To illustrate example(s) in a clear and concise manner, the drawings may not necessarily be to scale and certain features may be shown in somewhat schematic form. Features that are described and/or illustrated with respect to one example may be used in the same way or in a similar way in one or more other examples and/or in combination with or instead of the features of the other examples.

As used in the specification and claims, for the purposes of describing and defining the invention, the terms “about” and “substantially” are used to represent the inherent degree of uncertainty that may be attributed to any quantitative comparison, value, measurement, or other representation. The terms “about” and “substantially” are also used herein to represent the degree by which a quantitative representation may vary from a stated reference without resulting in a change in the basic function of the subject matter at issue. “Comprise,” “include,” and/or plural forms of each are open ended and include the listed parts and can include additional parts that are not listed. “And/or” is open-ended and includes one or more of the listed parts and combinations of the listed parts.

FIGS. 1A and 1B illustrate a prior art surgical hand wrap for attaching a patient's arm 2 and hand 4 to a limb positioning device. Typically, before being secured to the limb positioning device, the patient's hand 4 is attached to a handle or bar 6 and secured into a balled fist, as shown in FIG. 1A. Portions of the arm 2 and the hand 4 are draped or covered in a flexible sleeve 8 and secured in place with straps 5. The entire arm 2 is then wrapped with an elasticated bandage 9, as shown in FIG. 1B. The distal end of the bandage 9 is attached to weights via a rope 7 and a series of pulleys on a limb positioning device, such as the limb positioning device illustrated in FIG. 5A. However, this method of securing the hand 4 can lead to numbness in the patient's hand 4 and fingers 1. FIG. 1C shows the high-contact

pressure points across the fingers 1 and wrist 3 of the patient under traction load when the hand 4 and arm 2 are attached to the limb positioning device in this manner. Such high-contact pressure points can lead to the numbing effect of the hand 4 and fingers 1.

Turning now to FIG. 2, a cut-away view of an exemplary surgical hand wrap 10 of this disclosure is shown. As illustrated in FIG. 2, the hand wrap 10 may include a flexible mitten portion 12 having an interior side 14 and an exterior side 16. The mitten portion 12 may be made of a variety of flexible plastic or fabric materials, including, but not limited to, urethane foam and polyester fabric. The mitten portion 12 is configured to enclose at least the hand 4 of a patient in an open position, which advantageously reduces the possibility of numbness developing in the patient's hand 4 and fingers 1 during the surgical procedure. In examples, the interior side 14 of the mitten portion 12 adjacent to the palm of the hand 4 comprises an anti-slip material, such as styrene-butadiene rubber (SBR) bonded foam, rubber, or urethane foam. The hand 4 is secured within the mitten portion 12 by at least one closeable strap 20 (such as Velcro® straps) wrapped around the exterior side 16 of the mitten portion 12. For example, the straps 20 may be wrapped around the mitten portion 12 adjacent the patient's hand 4 and wrist 3. The straps 20 may be secured to the mitten portion 12 at one end or they may be free floating. The straps 20 are used to hold the hand 4 and wrist 3 firmly but not tightly within the mitten portion 12 to prevent any substantial movement of the hand 4 and wrist 3 in either rotation or translation.

Once the hand 4 is secured within the mitten portion 12, the mitten portion 12 may be attached to an anatomically-shaped plate 22, shown in more detail to FIG. 3A. The plate 22 is configured to support the palm of the hand 4 in the open position. In examples, the plate 22 is comprised of a material which has adequate strength and resistance to sterilization using radiation, such as polycarbonate plate. Notably, the plate 22 can take a variety of sizes and shapes as long as it is configured to support the palm in the open position. In the example of FIG. 3A, the plate has a distal portion 23 configured to attach to a limb positioning device. The plate 22 also includes a center portion 24 which is curve-shaped to support the fingers 1 of the hand 4. Finally, the plate 22 includes a proximal portion 25. The proximal portion 25 may include one or more slots 27 through which the straps 20 may be passed to attach the mitten portion 12 to the plate 22 near the patient's wrist 3. In order to reduce slippage and pressure on the ulnar and radial sides of the wrist, which may lead to nerve injury, the hand

wrap 10 may be provided with additional padding 29 within the mitten portion 12 for wrapping around the wrist of the patient, as shown in FIG. 3B. In examples, the padding may be a foam padding, and may be secured to the wrist by a strap 31 wrapped around the wrist. A thickness of the padding 29 is selected to be greater than a thickness of the mitten portion 12. Finally, the hand wrap 10 is overwrapped with an elastic bandage 26, as shown in FIG. 4. It is also contemplated by this disclosure that the hand 4 of the patient could be secured to the plate 22 without the use of the mitten portion 12.

Turning now to FIG. 5A, a limb positioning device 28 is illustrated, the component parts of which are described in more detail below. In FIG. 5A, a patient 30 is shown lying on a standard operating table 32 and prepared for a surgical operation. The forearm of the arm 2 to be operated upon is encased within the hand wrap 10 of this disclosure. The distal end of the hand wrap 10 is then attached to weights 40 via a series of ropes 42 and pulleys 44 on the limb positioning device 28. Advantageously, when traction is applied to the hand wrap 10 by the limb positioning device 28, the shape of the plate 22, the construction of the mitten portion 12, and the straps 20 combine to allow low-contact pressure across the hand 4 and the wrist 3 of the patient 30. In examples, various components of the limb positioning device may contain telescoping or other features for lengthening or shortening the components, and/or height adjusting features for raising or lowering the components.

As shown in FIG. 5B, once the hand wrap 10 has been secured to the plate 22, the distal portion 23 of the plate 22 is connected to the limb positioning device 28 by means of an exemplary sterile connector 34 of this disclosure, shown in more detail in FIG. 5C. The sterile connector 34 may be made of polymers, metals or other suitable materials and is intended to be disposed of after use. As shown in FIG. 5C, the sterile connector 34 has a T-fitting 36 at its distal end and a keyed shaft 38 at its proximal end. The T-fitting 36 is configured to couple to the distal portion 23 of the plate 22 of the limb positioning device 28. The shaft 38 is configured to mate with a receiver 40 permanently attached to the distal end of the limb positioning device 28, as shown in FIG. 5D.

Also shown in FIG. 5D, attached to the sterile connector 34 is a flexible dam portion 42 of a sterile drape or covering 44. In examples, the proximal end of the covering 44 is open such that the covering 44 is configured to cover at least a portion of the limb positioning device 28. The covering 44 may be fabricated from a variety of different materials that may

be sterilized and which are preferably latex-free, such as polyethylene plastics. In examples, the covering 44 may be formed from a pre-formed tubular sheet of the plastic material or from plural sheets of plastic material formed into a tube with longitudinal seams. It will be appreciated that the dimensions and configuration of the covering 44 will vary depending upon the type and structure of the limb positioning device or other equipment that the covering 44 is designed to cover. The dam portion 42 is attached to the covering 44 in an appropriate manner such as sonic welding or adhesives. The dam portion 42 may be fabricated from any number of flexible, non-slip materials, such as rubber. In examples, the sterile connector 34 is held in the dam portion 42 in an interference fit due to the elastic nature of the rubber. As shown in FIG. 5E, in use, the covering 44 may be folded in telescopic fashion to allow for visualization of the shaft 38 of the sterile connector 34 for easing insertion into the receiver 40 of the limb positioning device 28.

In other examples, not shown, the shape of the T-fitting 36 and the shaft 38 could be changed to suit different applications. For example, the shaft 38 could be reconfigured to make it symmetrical to the T-fitting 36. In other examples, the sterile connector 34 could be clamped or glued in place, or held by a fastening ring. In addition, the dam portion 42 could be eliminated, allowing the covering 44 to be directly attached to the sterile connector 34. Advantageously, the sterile connector 34 of this disclosure allows for a sterile operator to attach the sterile hand wrap 10 to the limb positioning device 28 in the sterile field without the need for a non-sterile operator. This in turn allows for faster turnover between procedures by eliminating the need for re-usable (i.e., autoclaveable) interfaces.

While this disclosure has been particularly shown and described with references to preferred embodiments thereof, it will be understood by those skilled in the art that various changes in form and details may be made therein without departing from the spirit and scope of the present application as defined by the appended claims. Such variations are intended to be covered by the scope of this present application. As such, the foregoing description of embodiments of the present application is not intended to be limiting, the full scope rather being conveyed by the appended claims.

CLAIMS

What is claimed is:

1. A surgical hand wrap for attaching a patient's arm to a limb positioning device, the
5 hand wrap comprising:

a flexible mitten portion having an interior side and an exterior side, the mitten portion
configured to enclose at least a hand of the patient in an open position;

an anatomically-shaped plate for supporting a palm of the hand in the open position;
and

10 at least one closeable strap for wrapping around the exterior side of the mitten portion;
wherein, when traction is applied to the patient's arm, the plate, the mitten portion,
and the at least one strap combine to allow low-contact pressure across the hand of the patient.

2. The surgical hand wrap of claim 1, wherein the mitten portion is comprised of at least
15 one of urethane foam and polyester fabric.

3. The surgical hand wrap of claim 1, wherein the interior side of the mitten portion
comprises an anti-slip material.

20 4. The surgical hand wrap of claim 3, wherein the anti-slip material is one of SBR
bonded foam, rubber, and urethane foam.

5. The surgical hand wrap of claim 1, wherein an end of the at least one strap is attached
to the mitten portion.

25 6. The surgical hand wrap of claim 1, wherein the at least one strap is free-floating.

7. The surgical hand wrap of claim 1, wherein the at least one strap is secured to the
plate.

30

8. The surgical hand wrap of claim 1, wherein the hand wrap is enclosed within a bandage.

9. The surgical hand wrap of claim 1, wherein the plate is comprised of polycarbonate.

5

10. The surgical hand wrap of claim 1, wherein the plate comprises a distal portion configured to attach to the limb positioning device.

11. The surgical hand wrap of claim 1, wherein the plate comprises a curved center portion for supporting the palm of the hand in the open position.

10

12. The surgical hand wrap of claim 1, wherein the plate comprises at least one slot configured for the passage of the at least one strap.

13. The surgical hand wrap of claim 1, further comprising a padding disposed within the mitten portion for securing about a wrist of the patient, a thickness of the padding selected to be greater than a thickness of the mitten portion.

15

14. A sterile connector for attaching a surgical hand wrap to a limb positioning device, the connector comprising:

20

a T-fitting at a distal end configured to couple to a support member of a sterile hand wrap; and

a shaft at a proximal end configured to mate with a receiver of the limb positioning device;

25

wherein the connector is attached to a flexible dam portion at a distal end of a sterile covering, the covering configured to cover at least a portion of the limb positioning device.

15. The connector of claim 14, wherein the connector is comprised of polymers or metals.

16. The connector of claim 14, wherein the covering is comprised of a clear, polyethylene plastic.

30

17. The connector of claim 14, wherein the flexible dam portion is comprised of rubber.

18. The connector of claim 14, wherein a proximal end of the covering is open to cover at least a portion of the limb positioning device.

5

19. The connector of claim 14, wherein the covering is configured to fold in a telescopic fashion.

20. The connector of claim 14, wherein the connector is attached to the flexible dam
10 portion in an interference fit.

1/7

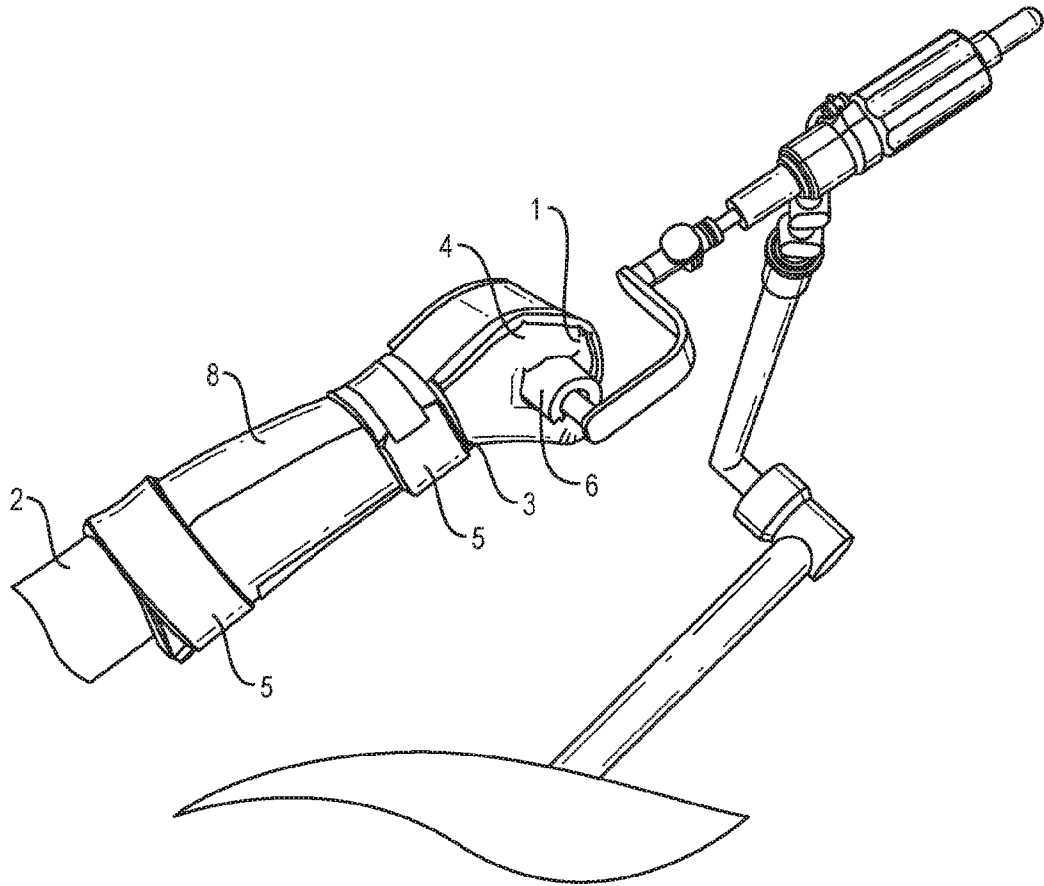


FIG. 1A
(PRIOR ART)

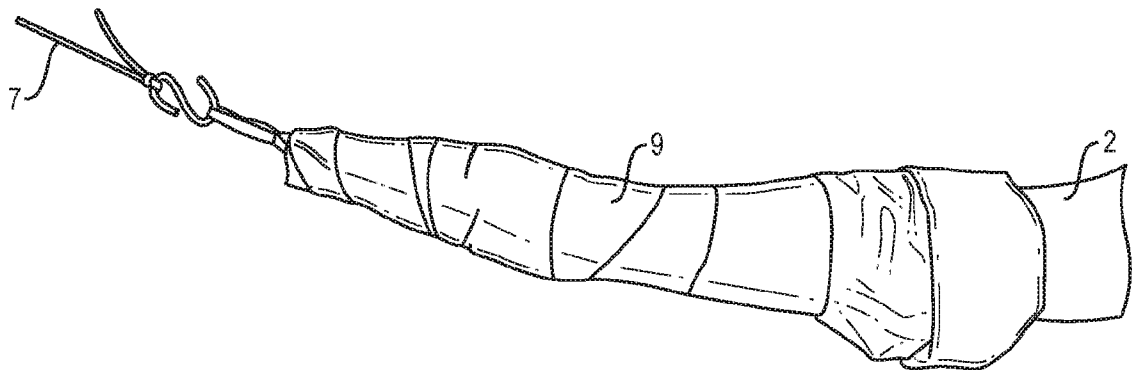


FIG. 1B
(PRIOR ART)

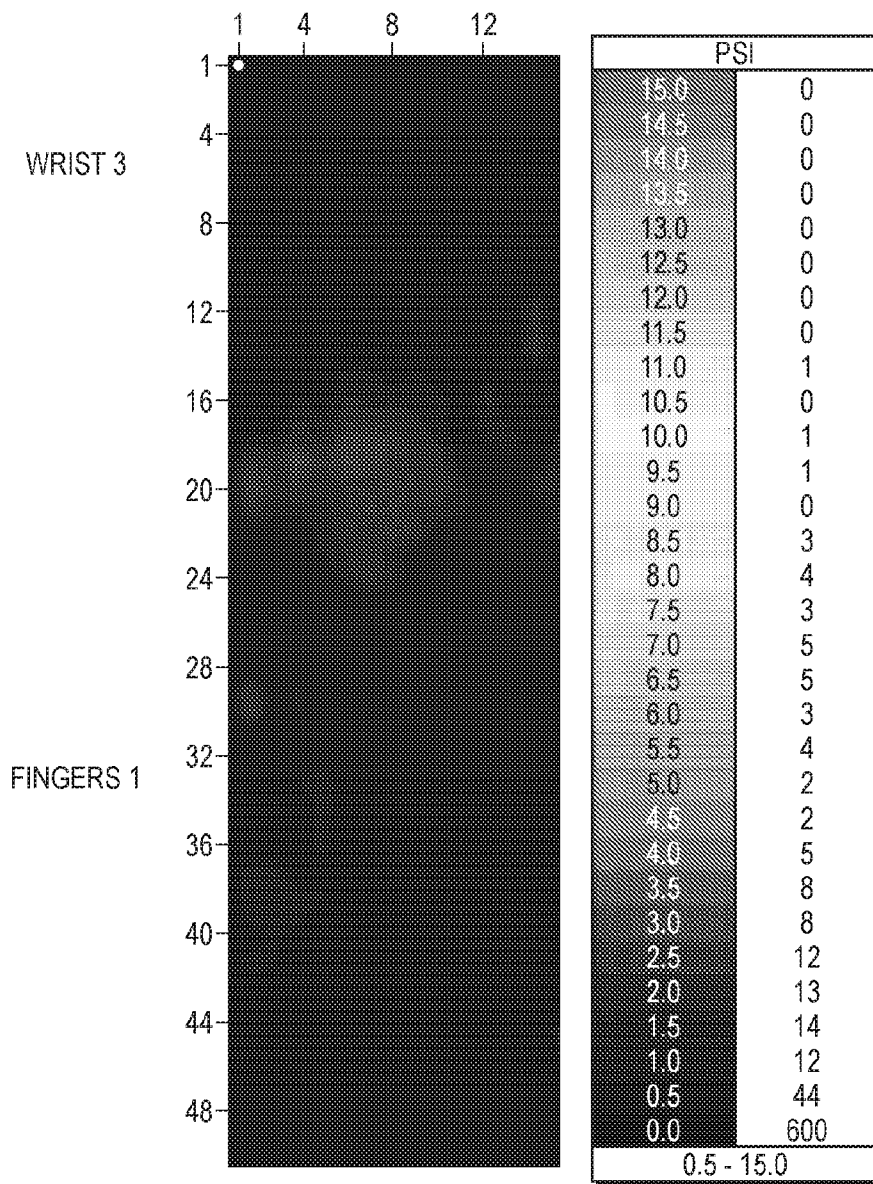


FIG. 1C

3/7

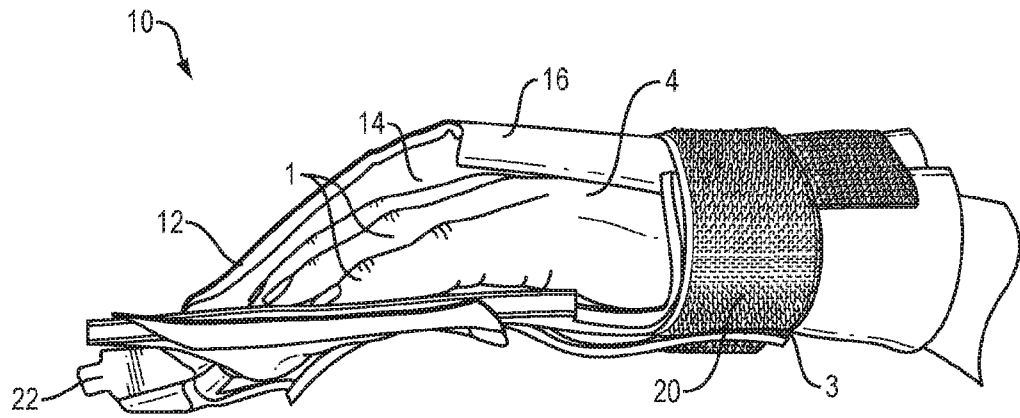


FIG. 2

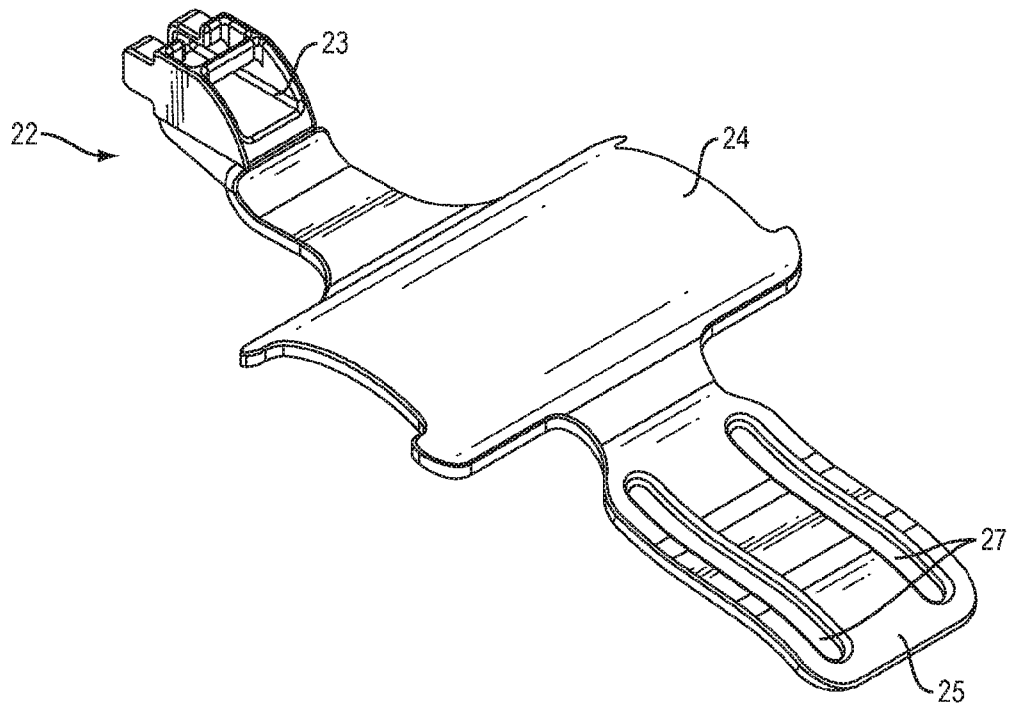


FIG. 3A

4/7

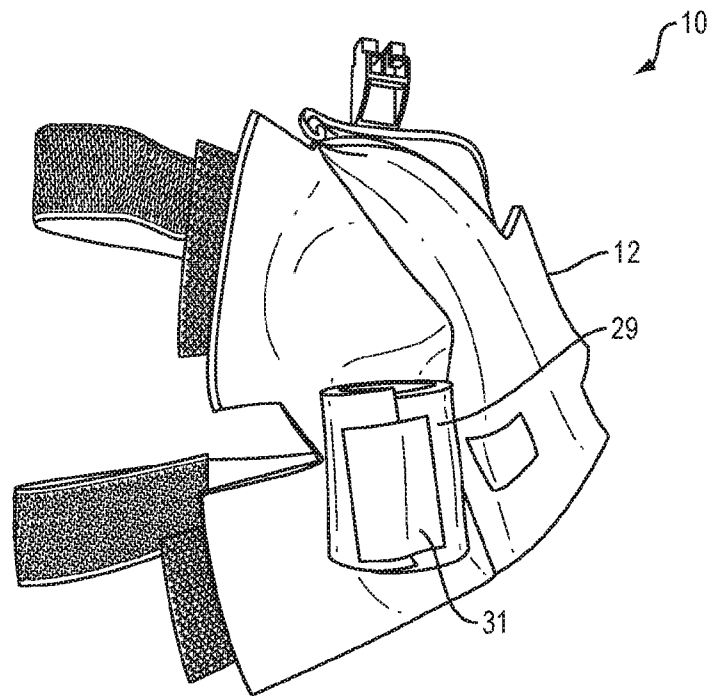


FIG. 3B

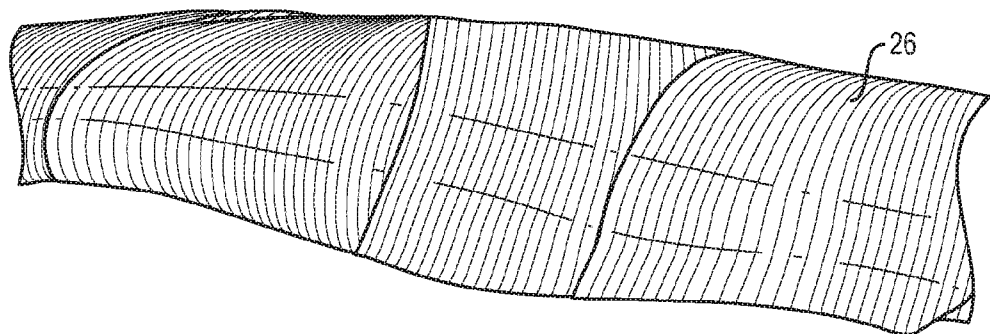


FIG. 4

5/7

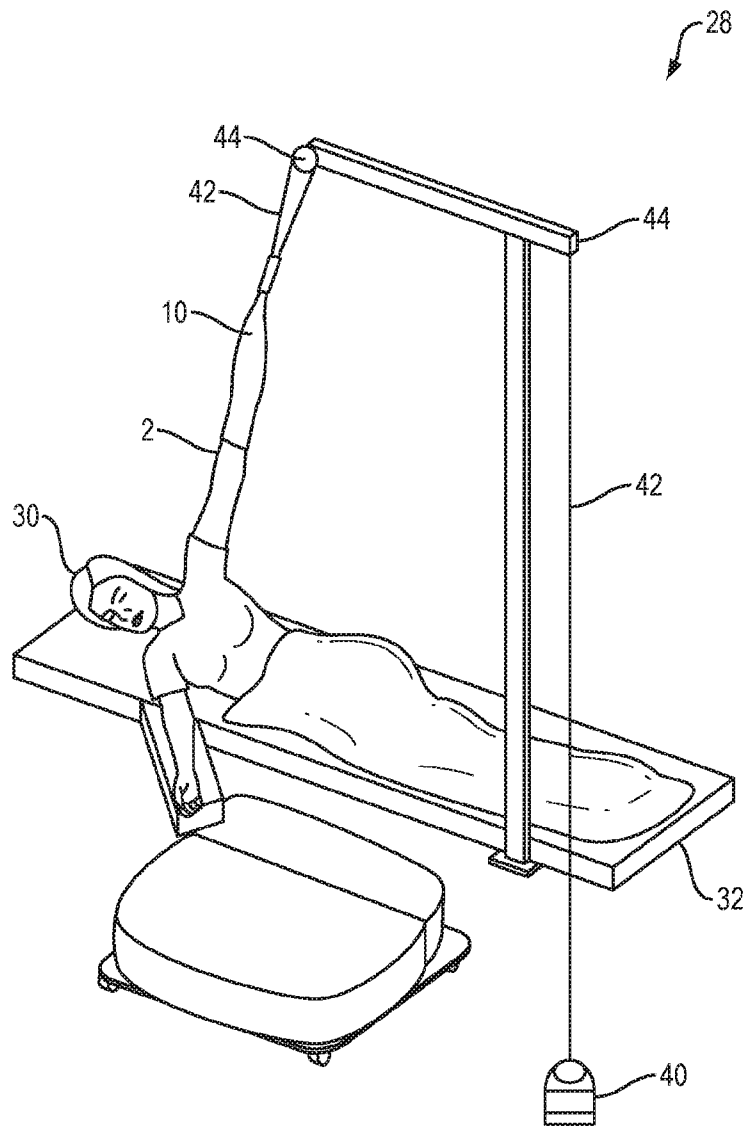


FIG. 5A

6/7

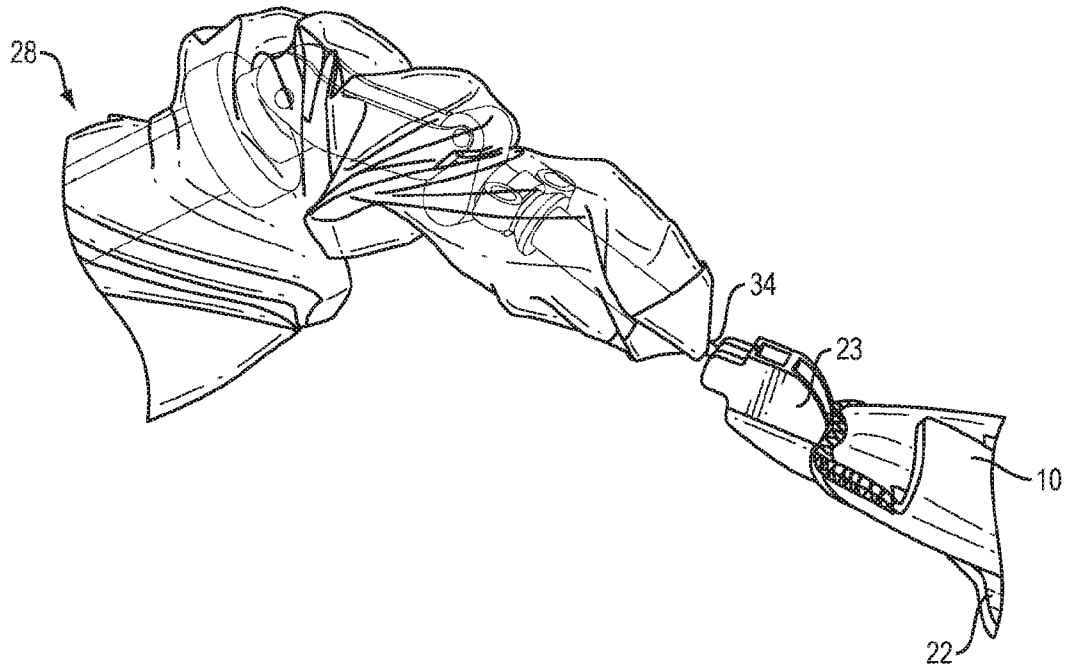


FIG. 5B

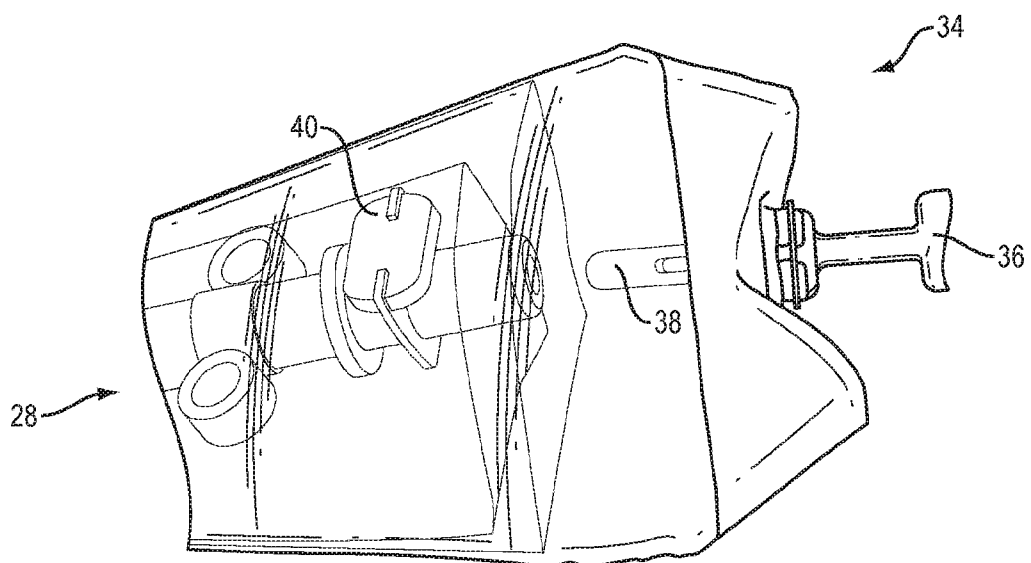


FIG. 5C

7/7

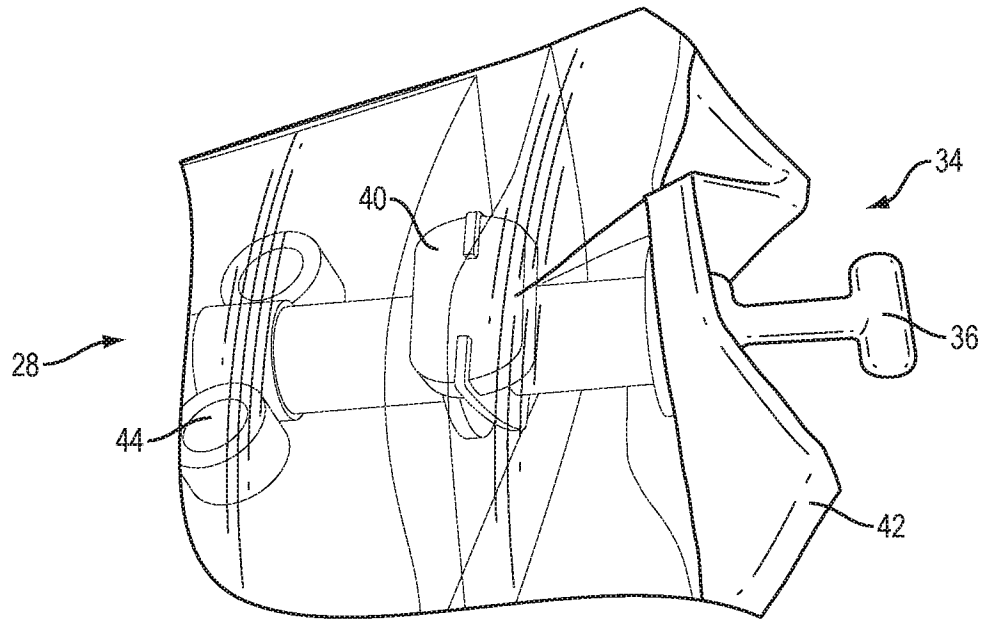


FIG. 5D

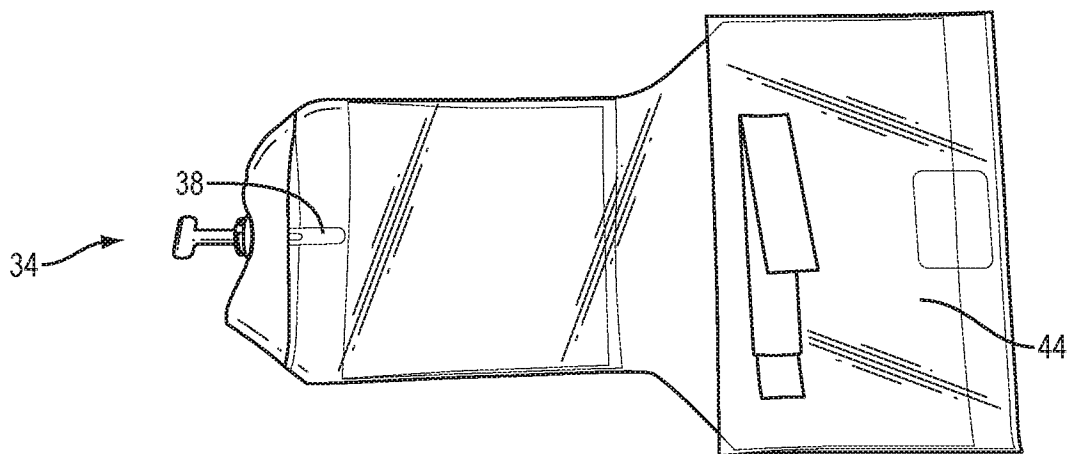


FIG. 5E

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2018/059190

A. CLASSIFICATION OF SUBJECT MATTER INV. A61G13/12 A61F5/01 A61B46/27 A61F5/37 A61G13/00 ADD.		
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) A61G A61F A61B		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) EPO-Internal, WPI Data		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2015/150717 A1 (LOWE MARK H [US] ET AL) 4 June 2015 (2015-06-04) figures 2C, 2D, 4A, 4b paragraphs [0066], [0074] - [0078] -----	1-9, 11-13
X	US 2001/039680 A1 (BOUCHER MICHAEL [US] ET AL) 15 November 2001 (2001-11-15) figure 11 paragraphs [0036], [0037] -----	1-13
A	US 2009/293884 A1 (DASILVA MANUEL F [US]) 3 December 2009 (2009-12-03) figures 6a, 6b paragraphs [0040], [0041] ----- -/-	1-13
☒ Further documents are listed in the continuation of Box C. ☒ See patent family annex.		
* Special categories of cited documents : "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier application or patent but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "&" document member of the same patent family		
Date of the actual completion of the international search	Date of mailing of the international search report	
12 February 2019	26/04/2019	
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Barnas, Christoph	

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2018/059190

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☒ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

1-13

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2018/059190

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 419 756 A (MCCONNELL BERNARD E [US]) 30 May 1995 (1995-05-30) figures 19-21 column 7, line 18 - column 8, line 19 -----	1-13
A	US 5 003 967 A (MCCONNELL BERNARD E [US]) 2 April 1991 (1991-04-02) figures 1, 11, 13, 23 column 5, lines 41-61 -----	1-13

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2018/059190

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2015150717 A1	04-06-2015	US 2015150717 A1 WO 2015050870 A1	04-06-2015 09-04-2015
US 2001039680 A1	15-11-2001	US 2001039680 A1 US 2004123389 A1	15-11-2001 01-07-2004
US 2009293884 A1	03-12-2009	NONE	
US 5419756 A	30-05-1995	NONE	
US 5003967 A	02-04-1991	US 5003967 A US 5127898 A	02-04-1991 07-07-1992

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-13

A surgical hand wrap for attaching a patient's arm to a limb positioning device comprising a flexible mitten portion, an anatomically-shaped plate for supporting a palm of the hand in the open position; and at least one closeable strap for wrapping around the exterior side of the mitten portion.

2. claims: 14-20

A sterile connector for attaching a surgical hand wrap to a limb positioning device comprising a T-fitting at a distal end configured to couple to a support member of a sterile hand wrap; and a shaft at a proximal end configured to mate with a receiver of the limb positioning device.
