



(51) International Patent Classification:

G01N 1/14 (2006.01) C12N 15/10 (2006.01)
C12Q 1/68 (2006.01) G01N 33/02 (2006.01)

(21) International Application Number:

PCT/US2017/027651

(22) International Filing Date:

14 April 2017 (14.04.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/322,840 15 April 2016 (15.04.2016) US

(71) Applicant: INTEGRATED NANO-TECHNOLOGIES, INC [US/US]; 999 Lehigh Station Road, Henrietta, NY 14467 (US).

(72) Inventors: CONNOLLY, Dennis, M.; 289 Hollywood Avenue, Rochester, NY 14618 (US). MURANTE, Richard, S.; 1 Chancery Lane, Rochester, NY 14625 (US). WESTCOTT, Nathaniel, E.; 39 Egret Drive, West Henrietta, NY 14586 (US).

(74) Agents: COLLINS, Brian, A. et al.; Barclay Damon Tower, 125 East Jefferson Street, Syracuse, NY 13202 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: DEVICE SYSTEM AND METHOD FOR FLUID SAMPLE COLLECTION

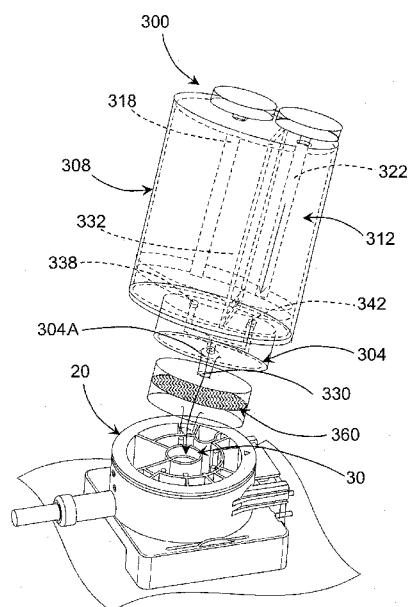


FIG. 19

(57) Abstract: A system and method for preparing a diagnostic fluid sample for use with a fluid assay system. The method comprises the steps of: amplifying the fluid sample to increase the number of cells subject to being tested; drawing a first volume of the fluid sample into a first syringe of a dual-barrel syringe and dispensing the first volume of the fluid sample through a media filter. The method further comprises the steps of placing the bacteria-laced filter into a lysis module; dispensing a first portion of a lysis buffer into the lysis module from the second syringe of the dual-barrel syringe; and dispensing a second portion of the lysis buffer through the media filter into a disposable cartridge of a fluid assay system.



Published:

— *with international search report (Art. 21(3))*

DEVICE SYSTEM AND METHOD FOR FLUID SAMPLE COLLECTION

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a Non-Provisional Utility Patent application which claims priority from a first U.S. Provisional Patent Application Ser. No. 62/322,840, filed April 15, 2016 entitled "Blood Sample Device" and U.S. Provisional Patent Application Ser. No. 62/322,843, filed April 15, 2016 entitled "Food Sample Device." The contents of the aforementioned applications are hereby incorporated by reference in their entirety.

[0002] This application relates to U.S. Patent Application Ser. No. 15/157,584 filed May 18, 2016 entitled "Method and System for Sample Preparation" which is a continuation of U.S. Non-Provisional Patent Application Ser. No. 14/056,603, filed October 17, 2013, now U.S. Patent No. 9,347,086, which claims priority to U.S. Provisional Patent Application Ser. No. 61/715,003, filed October 17, 2012, which is a continuation-in-part of U.S. Patent Application Ser. No. 12/785,864, filed May 23, 2010, now U.S. Patent No. 8,663,918, which claims priority to U.S. Provisional Patent Application Ser. No. 61/180,494, filed May 22, 2009, and which is also a continuation-in-part of U.S. Patent Application Ser. No. 12/754,205, filed April 5, 2010, now U.S. Patent No. 8,716,006, which claims priority to U.S. Provisional Patent Application Ser. No. 61/166,519, filed April 3, 2009. The contents of the aforementioned applications are hereby incorporated by reference in their entirety.

TECHNICAL FIELD

[0003] This invention relates to a device, system, and method for analyzing biological samples. In one embodiment, a device, system and method for collecting samples is disclosed for

use in combination with multi-chambered disposable cartridges for use in assaying blood samples. In another embodiment, a system and method is disclosed for use in combination with multi-chambered disposable cartridges for use in assaying food samples.

BACKGROUND

[0004] There is continuing interest to improve testing methodologies, facilitate collection and decrease the time associated with clinical laboratories. Particular testing requires that a sample be disrupted to extract nucleic acid molecules such as DNA or RNA.

[0005] The number of diagnostic tests performed annually has increased exponentially in the past decade. The use of molecular diagnostics and gene sequencing in research and medical diagnostics is also rapidly growing. For example, DNA testing has also exploded in view of the growing interest in establishing and tracking the medical history and/or ancestry of a family. Many, if not all of these assays, could benefit from a rapid sample preparation process that is easy to use, requires no operator intervention, is cost effective and is sensitive to a small sample size.

[0006] Sample collection and preparation is a major cost component of conducting real-time Polymerase Chain Reaction (PCR), gene sequencing and hybridization testing. In addition to cost, delays can lead to the spread of infectious diseases, where time is a critical component to its containment/abatement. In addition to delaying the test results, such activities divert much-needed skilled resources from the laboratory to the lower-skilled activities associated with proper collection, storage and delivery.

[0007] For example, a portable molecular diagnostic system could be operated by minimally trained personnel (such as described in US 2014/0099646 A1) and have value with

regard to disease surveillance. However, the adoption of such portable systems can be limited/constrained by current methods of sample collection, which require trained personnel to permit safe and effective handling of blood samples for analysis.

[0008] A need, therefore, exists for an improved device, system and method for collection, preparation and testing of fluid samples, facilitates the use of minimally-trained personnel, facilitates the testing of both blood and food samples, and may be used in combination with a portable molecular diagnostic system.

SUMMARY

[0009] The present disclosure relates to a sample collection/carrier device and method for using the same when assaying fluid samples, such as blood and food samples.

[00010] In one embodiment, a blood collection assembly is provided to facilitate the assay of a blood sample, comprising: (i) an absorptive media configured to collect and release the blood sample, (ii) a cartridge defining a cavity and a blood-sampling end configured to hold the absorptive media against a dermal membrane containing the blood sample, (iii) a lancet disposed within the cavity and having a lance at one end thereof, and (iv) a plunger configured to extend and retract the lancet through the absorptive media to lance the dermal membrane and collect the blood sample within the absorptive media. The cartridge containing the blood-filled, absorptive media is configured to be placed into a blood assay device for extraction or elution of the blood sample from the absorptive filter.

[00011] In another embodiment, a device is provided to facilitate the assay of a fluid sample, comprising: (i) an absorptive media configured to collect and release the fluid sample, and (ii) a carrier configured to: (a) hold the absorptive media in contact with the fluid sample

during collection, (b) carry the absorptive media into an apparatus for assaying the fluid sample, and (c) produce a fluid-retaining barrier with the apparatus while assaying the fluid sample.

[00012] In another embodiment, a dual-barrel syringe is provided to facilitate the preparation of a diagnostic fluid sample, comprising: (i) a first syringe operative to draw a quantity of the fluid sample, (ii) a second syringe containing a lysis buffer, the first and second syringes defining first and second barrels, respectively, which are juxtaposed and share a common wall, and (iii) a valve mechanism containing a nozzle which may be rotated into in fluid communication with an opening in each of the first and second barrels.

[00013] In yet another embodiment, a food assay system is provided to facilitate the assay of a fluid sample, comprising: an absorptive media configured to collect and release the fluid sample, and a disposable assay cartridge configured to assay the fluid sample for detecting the presence of a select attribute. The disposable cartridge has least one sample chamber disposed in fluid communication with at least one assay chamber containing at least one assay chemical facilitating the detection of the select attribute. The food assay system comprises, a fluid collection carrier configured to: (i) hold the absorptive media in contact with the fluid sample during collection, (ii) carry the absorptive media into the disposable assay cartridge for assaying the fluid sample, and (iii) produce a fluid-retaining barrier with the disposable assay cartridge while assaying the fluid sample. The fluid collection carrier is configured to be placed into the at least one sample chamber such that the at least one assay chemical is disposed in combination with the fluid sample to determine whether the select attribute is present.

[00014] In yet another embodiment, a method for collecting a blood sample is provided comprising the steps of: providing a cartridge having a filter-retaining end and a plunger/lancet assembly, loading the filter-retaining end with an absorptive media capable of absorbing a fixed-

quantity of blood and placing the absorptive media of the assembly into contact with the skin of a patient. The method further comprises the steps of: activating the plunger/lancet assembly to cause a lancet thereof to penetrate the skin to effect collection of the fixed-quantity of blood into the absorptive media, and placing the assembly and the blood-filled, absorptive media into a blood assaying device.

[00015] In yet another embodiment, a method is provided for preparing a diagnostic fluid sample for use with a fluid assay system. The method comprises the steps of: amplifying the fluid sample to increase the number of cells subject to being tested, drawing a first volume of the fluid sample into a first syringe of a dual-barrel syringe and dispensing the first volume of the fluid sample through a media filter. The method further comprises the steps of: placing the bacteria-laced filter into a lysis module, dispensing a first portion of a lysis buffer into the lysis module from the second syringe of the dual-barrel syringe, and dispensing a second portion of the lysis buffer through the media filter into a disposable cartridge of a fluid assay system.

BRIEF DESCRIPTION OF THE DRAWINGS

[00016] The present invention is disclosed with reference to the accompanying drawings, wherein:

[00017] FIG. 1 is a perspective view of a portable diagnostic assay system operative to accept one of a plurality of disposable cartridges configured to test fluid samples of collected blood or food samples.

[00018] Fig. 2 is an exploded perspective view of one of the disposable cartridges configured to test the biological samples.

[00019] Fig. 3 is a top view of the one of the disposable cartridges illustrating a variety of

assay chambers including a central assay chamber, one of which contains an assay chemical suitable to breakdown the fluid sample to detect a particular blood attribute.

[00020] Fig. 4 is a bottom view of the disposable cartridge shown in Fig. 3 illustrating a variety of channels operative to move at least a portion of the fluid sample from one chamber to another the purpose of performing multiple operations on the fluid sample.

[00021] Figs. 5 and 6 are perspective and profile views, respectively, of a novel blood collection assembly according to one embodiment of the disclosure including: a cartridge body, a blood-collection end configured to secure an absorptive media, and a trigger operative to activate the extension and retraction of a lancet disposed within a cavity of the assembly body and projecting through an aperture in the absorptive media to effect the collection of a blood sample.

[00022] Fig. 7 is an exploded view of the blood collection assembly including an upper body including a pair of laterally projecting finger flanges, a lower body including a blood-retention end, a trigger portion, a piston portion, an absorptive media and a coil spring.

[00023] Fig. 8 depicts the blood collection assembly being placed into a disposable cartridge of a portable diagnostic assay system.

[00024] Fig. 9 depicts the blood collection assembly seated in the disposable cartridge of the portable diagnostic assay system.

[00025] Fig. 10 depicts an isolated perspective view of the trigger and piston portions of the plunger each having a plurality of mating teeth and a telescopic mounting surface for permitting relative motion between the trigger and piston portions.

[00026] Fig. 11 depicts the cavity of the upper and lower body portions for mounting the plunger and absorptive media of the blood collection assembly.

[00027] Fig. 12 depicts an enlarged internal view of the cavity depicting guide and

retention surfaces for axial translation of the plunger, auto-retraction of the piston portion, and a locking feature of the trigger portion in a depressed or retracted position.

[00028] Fig. 13 depicts a novel fluid collection device including an absorptive media disposed at the tip end of a carrier configured to: (i) hold the absorptive media in contact with the fluid sample during collection, (ii) carry the absorptive media into a portable fluid assaying system, and (iii) produce a fluid-tight or fluid-retaining seal/barrier with the portable fluid assaying system while performing an analysis of the fluid sample.

[00029] Fig. 13a depicts an alternate embodiment of the carrier including a plug functionally replacing a cap to produce the fluid-tight or fluid-retaining seal barrier with the portable fluid assaying system.

[00030] Fig. 14 depicts the fluid collection device being placed into, and seated within, a disposable cartridge of a portable diagnostic assay system.

[00031] Fig. 15 depicts a perspective view of a dual-barrel syringe facilitating the preparation of a diagnostic fluid sample, including a first syringe operative to draw a quantity of the fluid sample, a second syringe juxtaposed with and sharing a common wall with the first syringe, the second syringe containing a lysis buffer, and a valve mechanism containing a nozzle which may be rotated into fluid communication with an opening in each barrel of the first and second syringe.

[00032] Figs. 16-19 depict the dual-barrel syringe in various operating positions including drawing, dispensing, exposing and rinsing/flushing the fluid sample in preparation for assay testing within a portable biological assay system.

[00033] Corresponding reference characters indicate corresponding parts throughout the several views. The examples set out herein illustrate several embodiments of the invention but

should not be construed as limiting the scope of the invention in any manner.

DETAILED DESCRIPTION

[00034] A blood collection assembly is described for use in combination with a portable/automated assay system such as that described in commonly-owned, co-pending U.S. Patent Application Ser. No. 15/157,584 filed May 18, 2016 entitled "Method and System for Sample Preparation" which is hereby included by reference in its entirety. The blood collection assembly may be used in combination with a variety of blood diagnostic cartridges which may be used to detect any of a variety of diseases which may be found in a blood specimen. For example, such blood diagnostic cartridges may be dedicated cartridges useful for detecting Hepatitis, Autoimmune Deficiency Syndrome (AIDS/HIV), Diabetes, Leukemia, Graves, Lupus, Multiple Myeloma, etc., just naming a small fraction of the various blood borne diseases that the portable/automated assay system may be configured to detect.

[00035] More specifically, and referring to Figs. 1 and 2, the system employs the use of a portable assay system 10 which receives any one of a variety of disposable assay cartridges 20, each selectively configured for detecting a particular attribute of a fluid sample. The portable assay system 10 includes one or more linear and rotary actuators operative to move fluids into, and out of, various compartments or chambers of the disposable assay cartridge 20 for the purpose of identifying or detecting a fluid attribute. More specifically, a signal processor 14, i.e., a PC board, controls a rotary actuator (not shown) of the portable assay system 10 so as to align one of a variety of ports 16, disposed about a cylindrical rotor 18, with a syringe barrel 22 of the assay cartridge 20. Furthermore, the processor 14 controls a Linear Variable Displacement Transducer (LVDT) 24, to displace a shaft 26 for the purpose of developing pressure i.e.,

positive or negative (vacuum) in the syringe barrel 22. That is, the shaft 26 displaces a plunger 28 within the syringe 22 to move and or admix fluids contained in one or more of the chambers 30, 32.

[00036] The disposable cartridge 20 provides an automated process for preparing the fluid sample for analysis and/or performing the fluid sample analysis. The sample preparation process allows for disruption of cells, sizing of DNA and RNA, and concentration/clean-up of the material for analysis. More specifically, the sample preparation process of the instant disclosure prepares fragments of DNA and RNA in a size range of between about 100 and 10,000 base pairs. The chambers can be used to deliver the reagents necessary for end-repair and kinase treatment. Enzymes may be stored dry and rehydrated in the disposable cartridge, or added to the disposable cartridge, just prior to use. The use of a rotary design allows for a single plunger to draw and dispense fluid samples without the need for a complex system of valves to open and close at various times. This greatly reduces potential for leaks and failure of the device compared to conventional systems. It will also be appreciated that the system greatly diminishes the potential for human error.

[00037] In Figs. 3 and 4, the cylindrical rotor 18 includes a central chamber 30 and a plurality of assay chambers 32, 34 surrounded, and separated by, one or more radial or circumferential walls 36. In the described embodiment, the central chamber 30 receives the fluid sample while the surrounding chambers 32, 34 may contain a premeasured assay chemical or reagent for the purpose of detecting an attribute of the fluid sample. The chemical or reagents may be initially dry and rehydrated immediately prior to conducting a test. Some of the chambers 32, 34 may be open to allow the introduction of an assay chemical while an assay procedure is underway or in process. The chambers 30, 32, 34 are disposed in fluid

communication, e.g., from one of the ports 16 to one of the chambers 30, 32, 34, by channels 40, 42 molded in an underside surface 42 of the rotor 18. For example, a port 16, corresponding to aperture 42, may be in fluid communication with the central chamber 30, via aperture 50.

Blood Collection Assembly

[00038] In Figs. 5 - 8, an embodiment of a novel blood collection assembly 100 comprises: (i) a body 104 having a blood-sampling end 106 configured to hold an absorptive media or filter 108, (ii) a lancet 112 disposed within a cavity 116 (See Fig. 7) of the body 104 and having a lance 118 at one end thereof, and (iii) a plunger or plunger assembly 120 configured to extend and retract the lancet 112 through the absorptive media or filter 108 to lance a dermal membrane, (i.e., the skin of a patient), and collect a blood sample within the absorptive media or filter 108. Once a blood sample has been collected, the assembly body 104 containing the blood-filled, absorptive media or filter 108 is configured to be placed into a blood assay device 10, i.e., the fluid sample chamber 30 of the disposable cartridge 20. This step may be performed immediately, or involve the sterile packaging/storing and/or transport of the blood sample, for subsequent analysis. Notwithstanding the time between collection and analysis, the blood collection assembly 100 is configured to be placed into a blood assay device 10 to elute the blood from the absorptive media 108. Furthermore, the blood collection assembly closes the sample chamber, i.e., produces a fluid-tight seal or fluid barrier, such that fluids may flow between ports 16 as pressure is developed in the various chambers 30, 32, 34 and channels 40, 42 of the disposable cartridge 20.

[00039] In the described embodiment, the assembly body 104 includes an upper body

portion 104a and a lower body portion 104b which collectively define the cavity 116. The body 104 is split to allow assembly of the plunger or plunger assembly 120 for insertion into the cavity 116, or to facilitate the replacement/removal of the absorptive media 108. While the absorptive media 108 may be replaced following use, the blood collection assembly of the present disclosure is intended to be disposable, similar to the disposable cartridge that it supplies.

[00040] The upper body portion 104a includes a pair of finger-receiving flanges 136, 138 projecting laterally from the assembly body 104 to facilitate handling of the assembly 100 while placing the absorptive media 108 against the dermal membrane or skin. The lower body portion 104b is configured to secure the absorptive media 108 within an annular groove or recess formed at the tip-end of the lower body portion 104b, i.e., at the tip of the blood-sampling end 106 of the assembly body 104.

[00041] The lancet 112 comprises a conventional tubular shaft having an end which is cut at a shallow angle, i.e., inclined, to produce a pointed tip end 118. The tip may be machined at an angle to produce a piercing tip, or sharpened to produce a razor-sharp lance 118. One end of the lancet 112 is embedded within a piston portion of the plunger or plunger assembly 120, discussed in greater detail below, while the other end of the lancet 112 faces the absorptive media 108 while disposed within the cavity 116 of the blood collection assembly 100.

[00042] The absorptive media 108 may be any material that absorbs and retains a liquid sample (paper, cellulose matrix, etc.) The material can be cut, pleated or woven in any manner to adjust the collected volume. In one embodiment, the absorptive media 108 includes a cellulose fiber filter having cotton linters treated to achieve an alpha cellulose content greater than about ninety-eight percent (98%). Filter materials suitable for use include Whatman Brand filters such as the Whatman FTA Elute series of paper products which facilitates: (i) long-term room

temperature DNA preservation, (ii) multiple amplifications from a single sample, and (iii) ease of elution.

[00043] In the described embodiment, the absorptive media 108 is an annular ring having an aperture 142 for receiving the lancet 112 upon activation of the plunger 120. While an annular ring is described, the absorptive media may have any shape provided it allows the lancet to penetrate or pass through a portion of the media material.

[00044] In one embodiment, the plunger 120 is spring-biased within the cavity 116 of the assembly body 104 to be retracted and extended relative to the assembly body 104. Furthermore, since the lancet 112 is connected to the plunger 120, the lancet 112 may also extend and retract within the cavity 116 to urge the lance 118 through the opening or aperture 142 in the absorptive media 108. In the described embodiment, a coil spring 160 abuts a raised ring-shaped shoulder 162 formed along the outer circumference of the trigger 120, allowing the trigger 120 to be depressed from, and returned to, an extended position. As mentioned in the preceding sentence, inasmuch as the lancet 112 is mounted to the trigger 120, the lancing end 118 may also extend and retract through the opening 142 in the absorptive media 108.

[00045] In Figs. 10-12, the plunger or plunger assembly 120 includes a piston portion 122 and a trigger portion 124. The piston portion 122 (i) defines a first cylindrical surface 126 slidably guided along an internal cylindrical bore or surface 144 of the cavity 116, (ii) defines a second cylindrical surface 128 telescopically mounting within a bore 134 of the trigger portion 124, and (iii) includes a pair of arrow-shaped radial protrusions 154 (Fig. 10) to axially guide the piston portion 122 within axial channels 156, while preventing rotation of the piston portion 122 about an elongate axis 100A (Fig. 11) of the assembly 100. The trigger portion 124 is: (i) disposed between the finger-receiving flanges 136, 138 of the upper body portion 104a of

the assembly 100, (ii) slideably guided within a bore 135 in the upper body portion 104a, and (iii) axially guided within the bore 142 (see Fig. 12) by the raised linear guide 156 within the cavity 116.

[00046] The piston and trigger portions 122, 124 include first and second crown-shaped teeth 164, 166, respectively, which facilitate the transfer of axial motion between the piston and trigger portions 122, 124 while imparting rotational motion as a consequence of engagement between the inclined surfaces of the crown-shaped teeth 164, 166. Inasmuch as the piston portion 122 employs anti-rotation protrusions 154, the piston portion travels axially within the guide 156 while the trigger portion 124 rotates into a shoulder notch 170. The trigger portion 124 only moves into the notch 170 as the trigger portion 124 moves axially past notch 170 or as the trigger portion 124 moves past a threshold axial location.

[00047] The relative rotation between the piston and trigger portions 122, 124 causes the piston portion 122 to recede into the trigger portion 124 as a consequence of the telescopic mount between the piston and trigger portions 122, 124. Furthermore, inasmuch as the lancet 112 is seated within the piston portion 124, the lancet 112 "auto-retracts" when the trigger portion 124 rotates under the notch 170. Furthermore, when the trigger portion 124 rotates beneath the notch 170, it is no longer capable of retraction and extension. Accordingly, the trigger piston 124 is "locked" and incapable of a second use. This feature may be desirable to prevent cross-contamination of the blood sample. Alternatively, the lancet 122 may move into a position where it is locked by a housing shoulder to prevent the lancet 112 and the blood collection assembly 100 from being used a second time.

[00048] Once a blood sample has been taken, the blood collection assembly 100 is placed within the sample chamber 30 of the disposable cartridge 20. The blood collection assembly 100

may include a sealing ring (not shown) at the tip end of the assembly to facilitate the formation of a fluid-tight seal. Additionally, to augment release and elution of the blood from the absorptive media 108, one or more apertures 172 (see Fig. 6) may be formed in the body 104 to facilitate fluid flow through the absorptive media 108.

Fluid Sample Carrier

[00049] In Figs. 13, 13a, and 14, a novel food assay system and fluid sample carrier 200 includes an absorptive media 208 configured to collect and release or elute a fluid sample when disposed in combination with a disposable cartridge 20 of a food assay system 10. The disposable assay cartridge 20 is essentially the same as was previously described, i.e., the arrangement of chambers, channels, ports, and plungers etc. The principal difference between the disposable assay cartridges 20 relates to the types of biological agents or attributes being assayed. For example, a cartridge 20 may be configured to assay for salmonella, E.coli, mad-cows disease, and other food borne pathogens. Additionally, the assembly can be configured to assay West Nile Virus or Lime Disease.

[00050] The fluid collection carrier 200 of this embodiment includes a sample collection end 202, a protective handle 204, and a connecting shaft 206 disposed therebetween. The sample collection end 202 includes a media or media filter 220 suitable for absorbing and carrying fluids which are suspected of containing a hazardous or dangerous pathogen.

[00051] The absorptive media 208 may be any material that absorbs and retains a liquid sample (paper, cellulose matrix, etc.). In one embodiment, the absorptive media 208 includes a cellulose fiber having cotton linters treated to achieve an alpha cellulose content greater than about ninety-eight percent (98%). Fiber media materials suitable for use include Whatman

Brand filters such as the Whatman FTA Elute series of paper products which facilitates long-term room temperature preservation and ease of elution.

[00052] In the described embodiment, the absorptive media 208 will have an elliptical shape and be sized to collect a select volume of fluid. While an ellipse is depicted, the absorptive media 208 may have any shape suitable for swabbing a surface or absorbing a standing fluid.

[00053] In one embodiment, the carrier 200 comprises a sealing member or cap 210 disposed between the shaft 206 and the protective handle 204. The cap 210 is configured to be disposed over a rim 216 (Fig. 14) of the sample chamber 30 of the disposable cartridge 20 and form a fluid-tight or fluid-retaining seal or barrier between it and the disposable cartridge 20. In the described embodiment, the cap 210 defines a cavity 218 to accept the rim 216 of the disposable cartridge 20. Similar to the previously-described blood collection assembly 100, the carrier 200 forms a seal or barrier with the sample chamber 30 such that the absorptive media 208 may elute the fluid to assay for food-borne diseases, hazardous biological agents, and/or dangerous pathogens.

[00054] In another embodiment depicted in Fig. 13a, an elastomer plug 220 functionally replaces the cap 210 to produce the seal or barrier with the sample chamber 30. In this embodiment, the plug 220 is received within the sample chamber 30 and forms a seal with the internal periphery of the sample chamber 30.

[00055] In another embodiment, the sealing member 210, 220 forms a fluid-tight seal with a vial 230 configured to maintain the purity or sterility of the fluid sample, both before and after collection. Furthermore, the vial 230 may be filled with a sterile fluid before and/or after sample collection.

[00056] The fluid collection carrier 200 is configured to: (i) hold the absorptive media 208

in contact with the fluid sample so as to cause the absorptive media 208 to collect a quantity of the fluid sample; (ii) carry the absorptive media 208 into the disposable assay cartridge 20, and (iii) close an end of the sample chamber 30 to prevent the egress of assay fluids and/or assay chemicals during assay testing.

[00057] In the described embodiment, the protective handle 204 includes a flange 212 projecting laterally outboard from an axis 206A defined by the shaft 206. The flange 212 is disposed axially aft, or rearward of, the sealing member 210 and functions to protect a handler from exposure to the food-borne diseases, hazardous biological agents, and/or dangerous pathogens carried within the absorptive media 208.

Dual-barrel Syringe for Preparation of a Food Sample

[00058] Many diagnostic tests, particularly food safety testing, require bacterial growth or amplification of the sample, prior to testing. This is due to the fact that certain agents, particularly those in food, often present very low levels of the biological attribute sought to be tested or detected in a sample. To enhance the probability of detecting the biological attribute, i.e., a test sample with a low Colony Forming Unit (CFU) count, a large sample size, i.e., typically more than ten milliliters (10 ml) can be required. This requirement, however, runs counter to many diagnostic assay systems which are designed for much smaller sample inputs, i.e., typically less than about fifty micro-liters (50 μ l.)

[00059] To integrate these competing requirements, a multi-barrel syringe 300 in combination with a selector valve 304 may be employed to draw, dispense, expose, and rinse/flush the fluid sample from an initial quantity of a food sample which has been amplified immediately prior to conducting an assay test.

[00060] More specifically, and referring to Figs. 15 and 16, the syringe 300 comprises first and second barrels 308, 312 having first and second syringe plungers 318, 322, and a selector valve 326 rotatably mounted to an end of the syringe 300 about an axis of rotation 304A and having a syringe nozzle 330. The first and second barrels 308, 312 are juxtaposed, share a common wall 332, and define first and second apertures 338, 342 at an end of each of the first and second barrels 308, 312, respectively.

[00061] The first barrel 308 of the dual-barrel syringe 300 is larger than the second barrel 312, and in the described embodiment, the volume of the first barrel 308 is between about five (5) to one-hundred (100) times larger than the volume of the second barrel 312. Furthermore, the first barrel 308 of the dual-barrel syringe 300 is initially empty to allow the first barrel 308 to draw a fluid sample from a biological sample 350 (Fig. 16) which has been amplified/colonized to increase the CFU concentration. The second barrel 312 of the dual-barrel syringe 300 is initially filled with a lysis buffer which is useful for breaking-down the assay sample. In the described embodiment, the second barrel 312 may contain approximately three hundred micro-liters (300 μ l) of a lysis buffer.

[00062] The method for preparing the fluid sample for subsequent use in a portable assay sample system will be described in greater detail herein below. Suffice to say at this juncture that, of the various components provided as part of an aggregate kit, i.e., a kit for identifying a particular attribute of a fluid/food sample, a dual-barrel syringe 300 will be provided wherein: (i) the first barrel 308 is significantly larger in volume than the second barrel 312, (ii) the first barrel 308 is initially empty to allow it to be used for drawing and dispensing an assay sample through a lysis filter, and (iii) the second barrel 312 is completely filled with a lysis buffer and dispensed in stages to properly prepare the assay sample.

[00063] Returning to Fig. 16, a first step of the preparation method involves preparing the biological food sample 350 in a conventional manner such that the biological food sample 350 is amplified/colonized to increase its Colony Forming Unit (CFU) count or concentration. In a second step, the plunger 318 of the first barrel is depressed to its bottom position and the selection valve 304 is rotated to align the aperture 338 of the first barrel 308 with the nozzle passageway of the selector valve 304. The nozzle 330 of the selector valve 304 is then placed in the prepared/pre-treated food sample 350, and the plunger 318 is raised to draw the fluid/food sample into the first barrel 308.

[00064] In Fig. 17, a third, or subsequent step, involves depressing the plunger 318 of the first barrel 308 to dispense the entire contents/volume of the first barrel 308 through a lysis filter 354 within a lysis module 360. The filter media 354 contains a filter material of appropriate porosity to extract the bacterial content of the fluid/food sample with high efficiency. Once all of the assay sample has been captured by the lysis filter 354, the selector valve 304 is rotated from the aperture 338 associated with the first barrel 308 to the aperture 342 associated with the second barrel 312.

[00065] In Fig. 18, a fourth step involves dispensing a portion of the lysis buffer from second barrel 312 into the lysis module 360. In the described embodiment, about one-half of the lysis buffer is dispensed in the lysis module 360. Further, the lysis module 360 is closed in this step to allow the module 360 to hold the contents of the syringe 300, i.e., the lysis buffer, for a predetermined minimum period of time. In the described embodiment, the filtered contents of the lysis filter 354 are exposed into the lysis buffer for a period of at least five minutes (5 mins.), and preferably for as much as fifteen minutes (15 mins.) The lysis buffer breaks-down and liberates the nucleic acids within the lysed material for subsequent analysis. In certain

embodiments, the time period of exposure may be automated such that the timing is controlled by computer software. In yet other embodiments, the lysis module 360 may be heated to facilitate and accelerate the lysis reactions.

[00066] In Fig. 19, a fifth, and final, step involves flushing/rinsing the remaining portion of the lysis buffer, i.e., the remaining one-hundred and fifty micro-liters (150 μ l,) through the lysis module 360 into the sample chamber 30 of the disposable cartridge 20. In other embodiments, the fluid/food sample could be purged into any suitable sample container based on the subsequent analysis to be provided/envisioned.

[00067] As mentioned above, this method allows for the detection of samples having a low CFU concentration in a sample by providing higher concentrations depending on the relative size of the syringe 300 and the lysis module 360. This method has the added benefit of extracting the relevant sample from the high salt broths often used in cultured food samples which have, in the past, been problematic for DNA purification and subsequent Polymerase Chain Reactions (PCRs.)

Example

[00068] In one example, a particular attribute of a food/fluid sample was to be detected based on a desired Colony Forming Unit (CFU)/ml. A ten milliliter (10 ml) sample was extracted from a broth produced by growing bacteria from a twenty-five gram (25 g) sample of ground beef. The selector valve 304 is switched to flow the 10 ml sample through a one hundred and fifty micro-liter (150 μ l) lysis module 360 containing a filter medium 354 to extract the bacterial content in the sample. After extraction, one hundred and fifty micro-liters (150 μ l) of a lysis buffer was injected into the to the lysis module 360 and allowed to react for

approximately 5 minutes. After the prescribed time period, another one hundred and fifty micro-liters (150 μ l) of the lysis buffer is dispensed through the filter medium 354 to cause the entire 300 micro-liters (300 μ l) to be flushed into the sample chamber 30 of the disposable cartridge 20. The lysed DNA material is then flushed through into an assay cartridge

[00069] While the invention has been described with reference to particular embodiments, it will be understood by those skilled in the art that various changes may be made and equivalents may be substituted for elements thereof without departing from the scope of the invention. In addition, many modifications may be made to adapt a particular situation or material to the teachings of the invention without departing from the scope of the invention.

[00070] Therefore, it is intended that the invention not be limited to the particular embodiments disclosed as the best mode contemplated for carrying out this invention, but that the invention will include all embodiments falling within the scope and spirit of the appended claims.

What is claimed is:

1. A system for preparing a fluid sample for assay testing of a fluid attribute, comprising:

a dual plunger syringe having first and second barrels sharing a common wall, and a rotating valve mechanism containing a nozzle in fluid communication with each of the barrels, the first barrel being empty and configured to receive a quantity of the sample fluid, the second barrel being filled with a lysis buffer;

a filter configured to receive the sample fluid by rotating the valve mechanism to the first barrel and dispensing the sample fluid through the filter, the filter capturing the fluid attribute so as to produce a sample-containing filter,

a lysis module defining a container for receiving the sample-containing filter and having a valve for opening and closing the container, the valve being initially closed to fill the lysis module with the lysis buffer by rotating the valve mechanism the second barrel to receive a first portion of the lysis buffer through the nozzle of the valve mechanism, and,

a disposable cartridge operative to receive the fluid sample to assay the fluid attribute, the fluid sample being received within an assay cavity upon opening the lysis module and dispensing a second portion of the lysis buffer from the second barrel through the nozzle of the valve mechanism to flush the sample containing filter with the second portion of the lysis buffer as the fluid sample is received within the assay cavity.

2. The system of claim 1 wherein the first and second barrels define first and second volumes, respectively, the first volume being larger than the second volume.

3. The system of claim 1 wherein the first and second barrels define first and second volumes, respectively, the first volume being five to one-hundred times larger than the second volume.
4. The system of claim 1 wherein about one-half of the lysis buffer from the second barrel fills the lysis module and about one-half of the lysis buffer from the second barrel flushes the sample containing filter within the lysis module.
5. The system of claim 1 further comprising a heater operative to heat the lysis module while the lysis buffer breaks down the material of the fluid sample.
6. A dual-barrel syringe facilitating the preparation of a diagnostic fluid sample, comprising:
 - a first syringe operative to draw a quantity of the diagnostic fluid sample;
 - a second syringe containing a lysis buffer,
 - the first and second syringes defining first and second barrels, respectively, which are juxtaposed and share a common wall; and
 - a valve mechanism containing a nozzle which may be rotated into in fluid communication with an opening in each of the first and second barrels.
7. The dual-barrel syringe of claim 6,

wherein the valve mechanism is rotated to draw a quantity of the fluid sample into the first barrel of the first syringe and dispense the fluid sample through a filter to capture a quantity of the fluid attribute from the fluid sample.

8. The dual-barrel syringe of claim 6

wherein the valve mechanism is rotated to fill a lysis module containing the media filter with a first portion of the lysis buffer from the second barrel of the second syringe; and

wherein a second portion of the lysis buffer rinses the media filter into an disposable assay cartridge from the second barrel of the second syringe.

9. The dual-barrel syringe of claim 6 wherein the first and second barrels define unequal volumes.

10. The dual-barrel syringe of claim 6 wherein the first and second barrels define first and second volumes, respectively, the first volume being at least twice the second volume.

11. A method of preparing a diagnostic fluid sample for use with a fluid assay system, comprising the steps of:

drawing a first volume of the fluid sample into a first syringe of a dual-barrel syringe;

dispensing the first volume of the fluid sample through a media filter;

placing the media filter into a lysis module;

dispensing a first portion of a lysis buffer into the lysis module from the second syringe of the dual-barrel syringe; and

dispensing a second portion of the lysis buffer through the media filter into a disposable cartridge of a fluid assay system.

12. The method of preparing a diagnostic fluid sample of claim 11 further comprising the comprising the step of:

amplifying the fluid sample prior to drawing the first volume into to the first syringe to increase the number of fluid assay cells for testing.

13. The method of preparing a diagnostic fluid sample of claim 11 further comprising the comprising the step of:

heating the lysis module to accelerate the reaction of the first portion of the lysis buffer with the fluid assay sample in the lysis module.

14. A food assay system facilitating the assay of a fluid sample, comprising:

an absorptive media configured to collect and release the fluid sample;

a disposable assay cartridge configured to assay the fluid sample for detecting the presence of a select attribute, the disposable cartridge having at least one sample chamber disposed in fluid communication with at least one assay chamber containing at least one assay chemical facilitating the detection of the select attribute;

a fluid collection carrier configured to:

(i) hold the absorptive media in contact with the fluid sample during collection,

(ii) carry the absorptive media into the disposable assay cartridge for assaying the fluid sample, and

(iii) produce a fluid-retaining barrier with the disposable assay cartridge while assaying the fluid sample;

wherein the fluid collection carrier is configured to be placed into the at least one sample chamber such that the at least one assay chemical is disposed in combination with the fluid sample to determine whether the select attribute is present.

15. The food assay system of claim 14

wherein the carrier includes a cap disposed over the rim of the assay chamber of the disposable assay cartridge to produce the fluid-tight seal.

16. The food assay system of claim 14

wherein the carrier includes a plug configured to seal the assay chamber of the disposable assay cartridge.

17. The food assay system of claim 15

wherein the carrier further comprises a flange disposed about the cap to prevent exposure to the fluid sample.

18. The food assay system of claim 15


wherein the carrier includes an elongate member projecting axially from the cap, and wherein the absorptive media mounts to a tip end of the elongate member to distally separate the absorptive media from the cap.

19. A device facilitating the assay of a fluid sample, comprising:
an absorptive media configured to collect and release the fluid sample; and
a carrier configured to:
(i) hold the absorptive media in contact with the fluid sample during collection,
(ii) carry the absorptive media into an apparatus for assaying the fluid sample, and
(iii) produce a fluid-retaining barrier with the apparatus while assaying the fluid sample.
20. The device of claim 19
wherein the carrier includes a sealing member to produce the fluid-tight seal with an assay chamber of the apparatus.
21. The device of claim 19
wherein the sealing member is a cap producing a fluid-tight seal with the rim of a sample chamber.
22. The device of claim 19
wherein the sealing member is a plug producing a fluid-tight seal with an internal surface of the sample chamber.
23. The device of claim 19

wherein the carrier includes a removable vial disposed in sealing combination with the sealing member for encapsulating the absorptive media containing a fluid sample.

24. The device of claim 19

wherein the carrier includes an elongate member projecting axially from the sealing member, and wherein the absorptive media mounts to a tip end of the elongate member to distally separate the absorptive media from the cap.

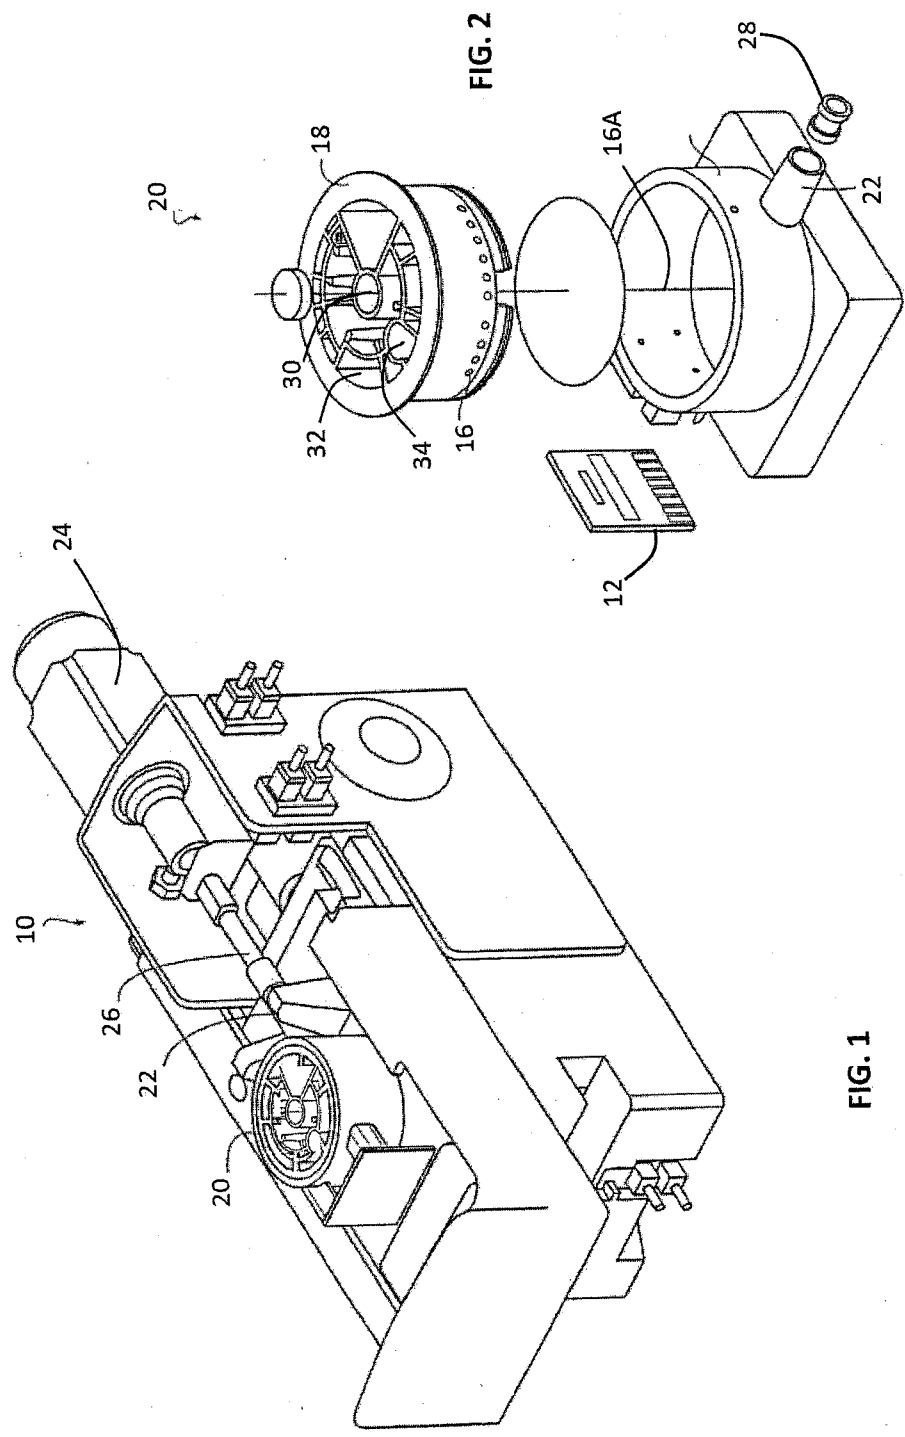

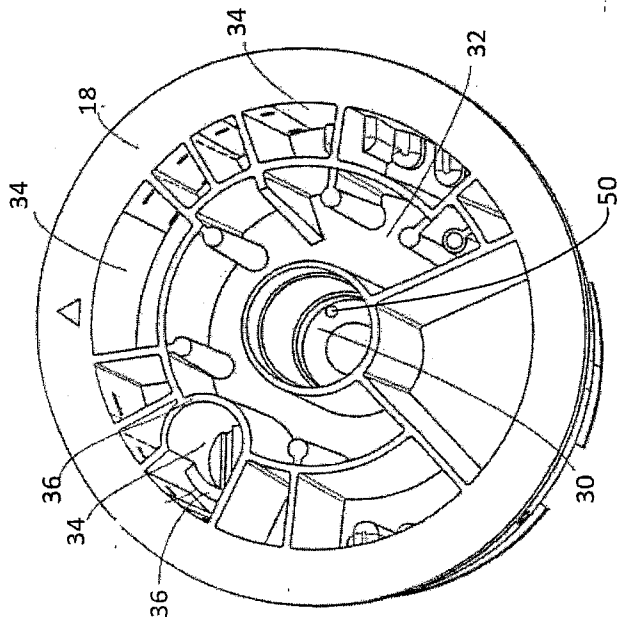


FIG. 3

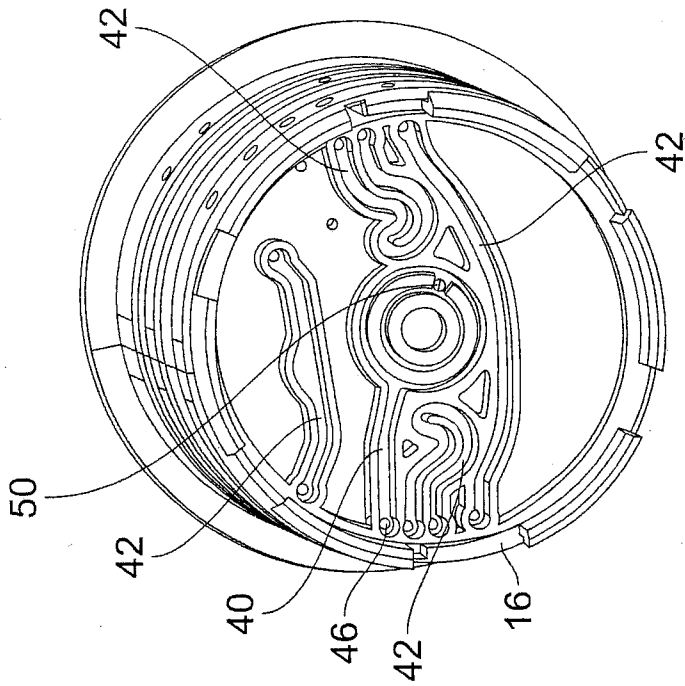


FIG. 4

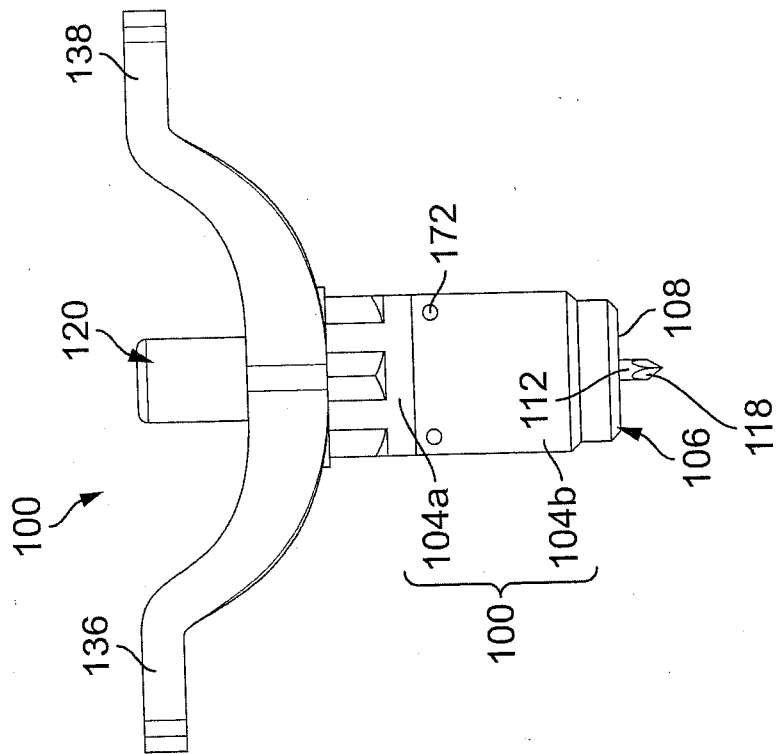


FIG. 6

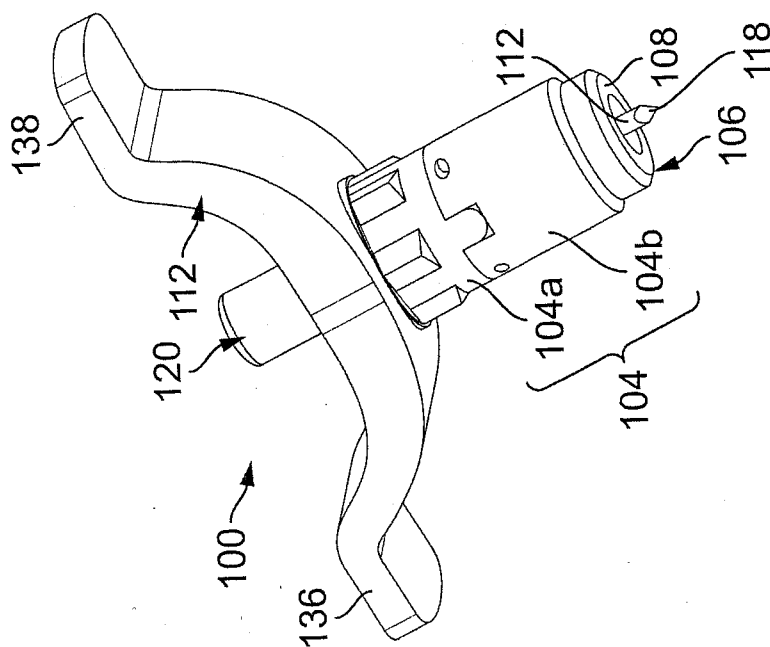


FIG. 5

4/13



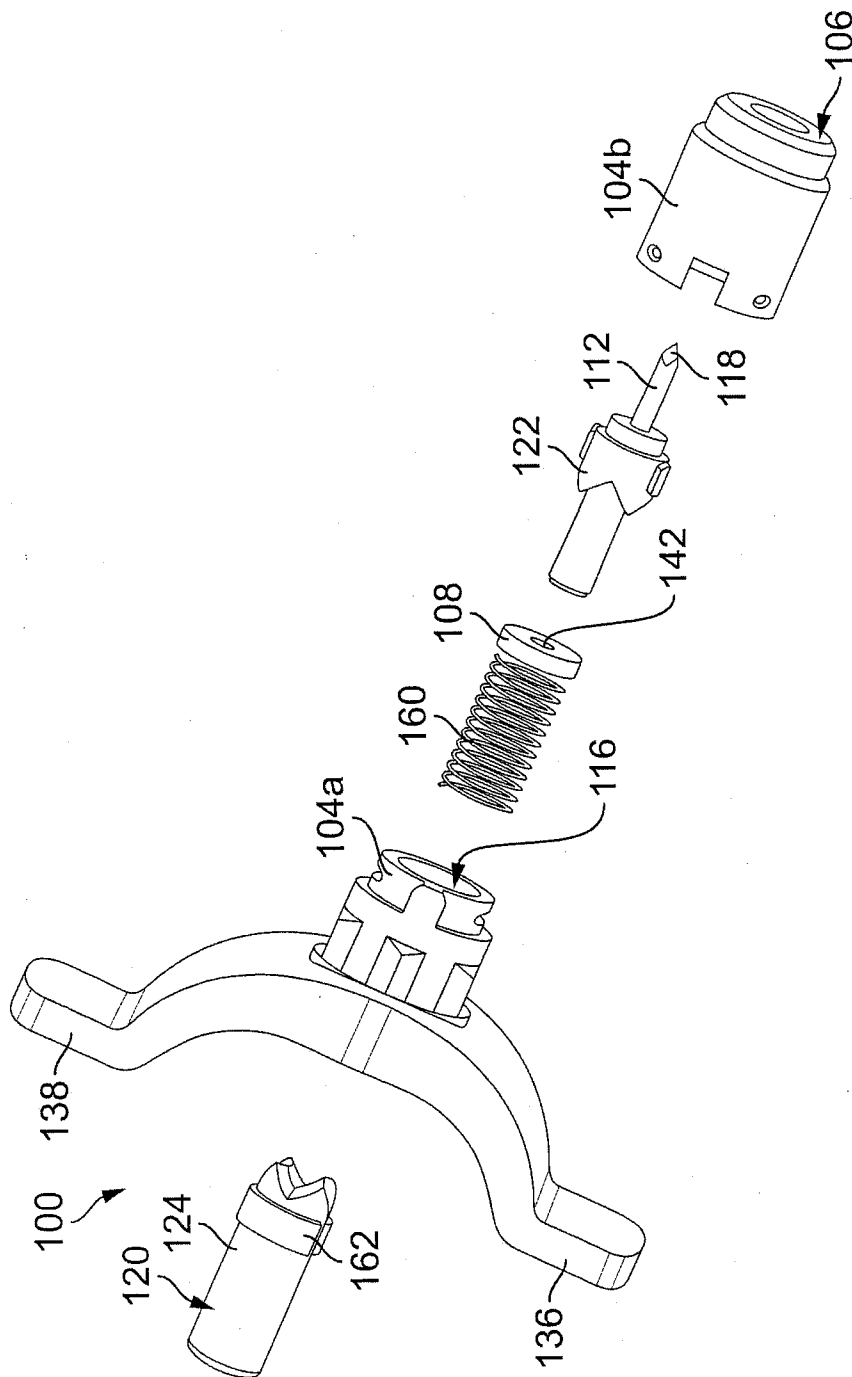


FIG. 7

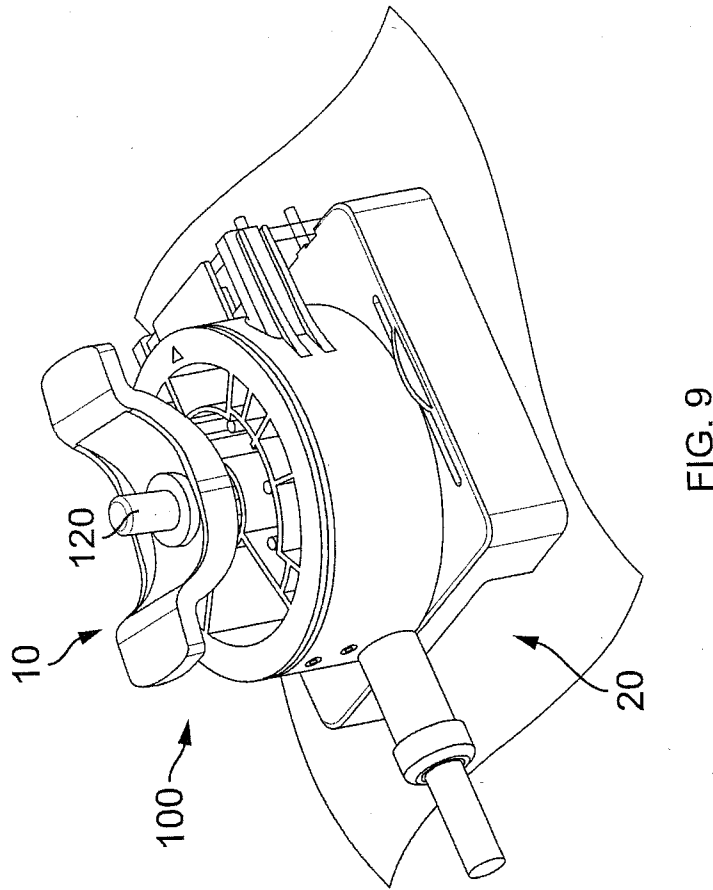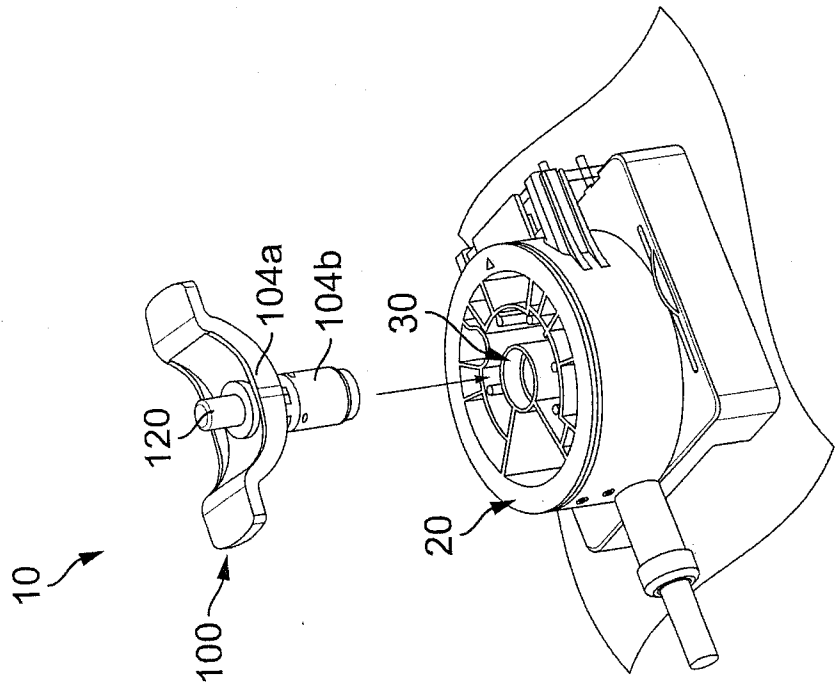

6/13

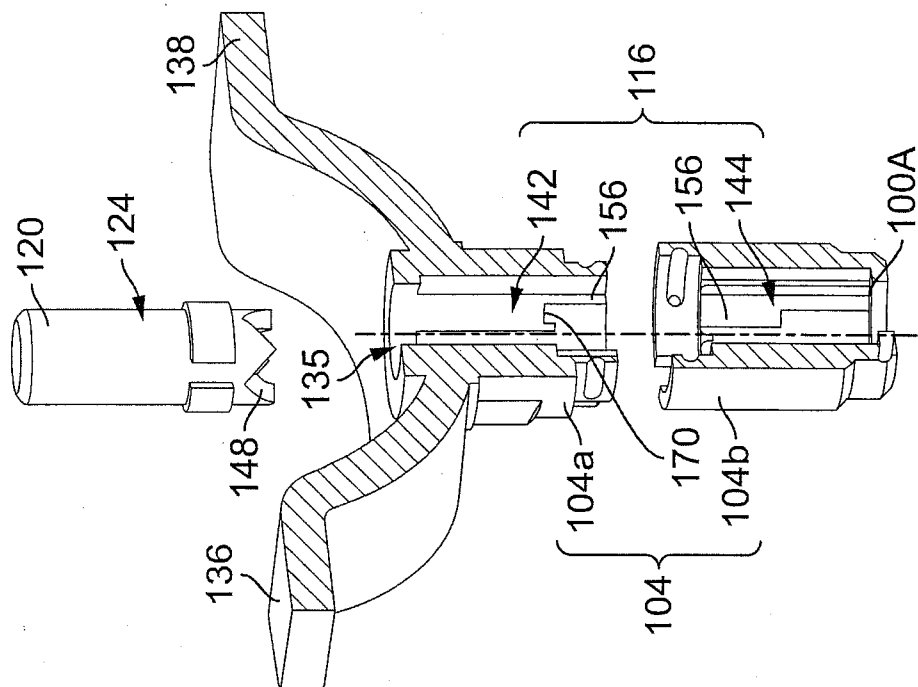


FIG. 11

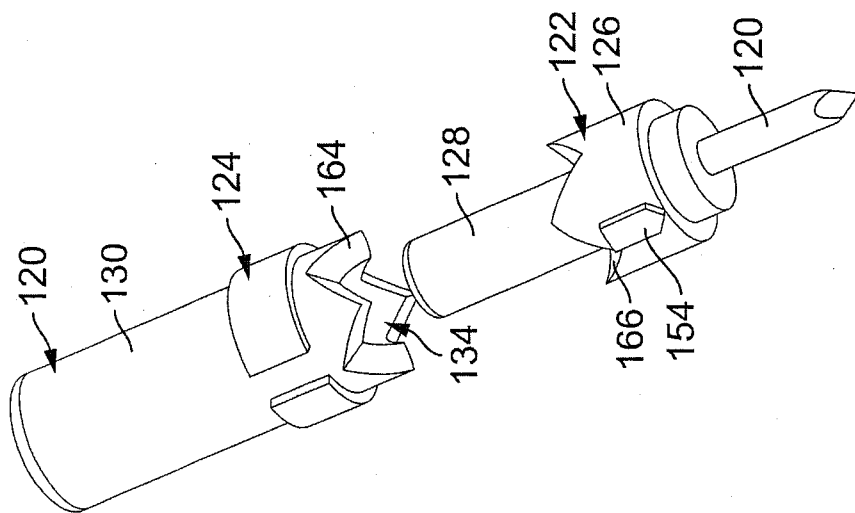


FIG. 10


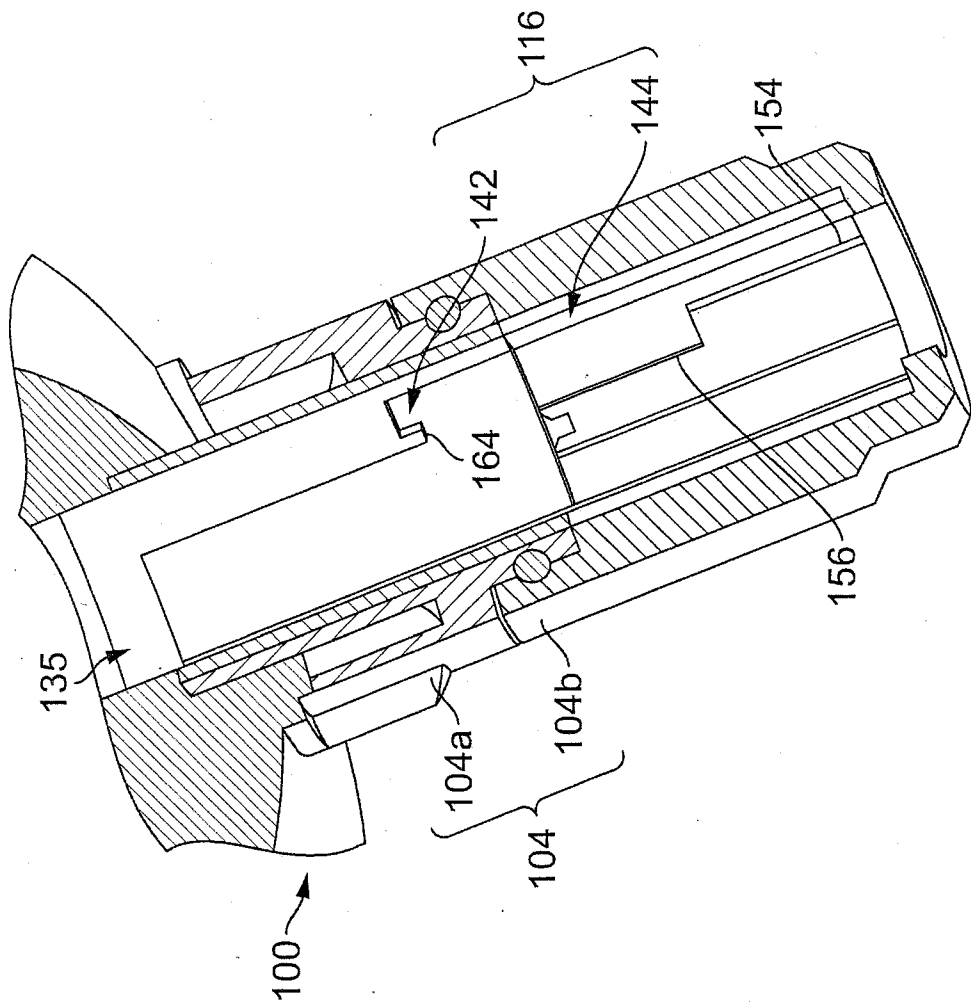


FIG. 12

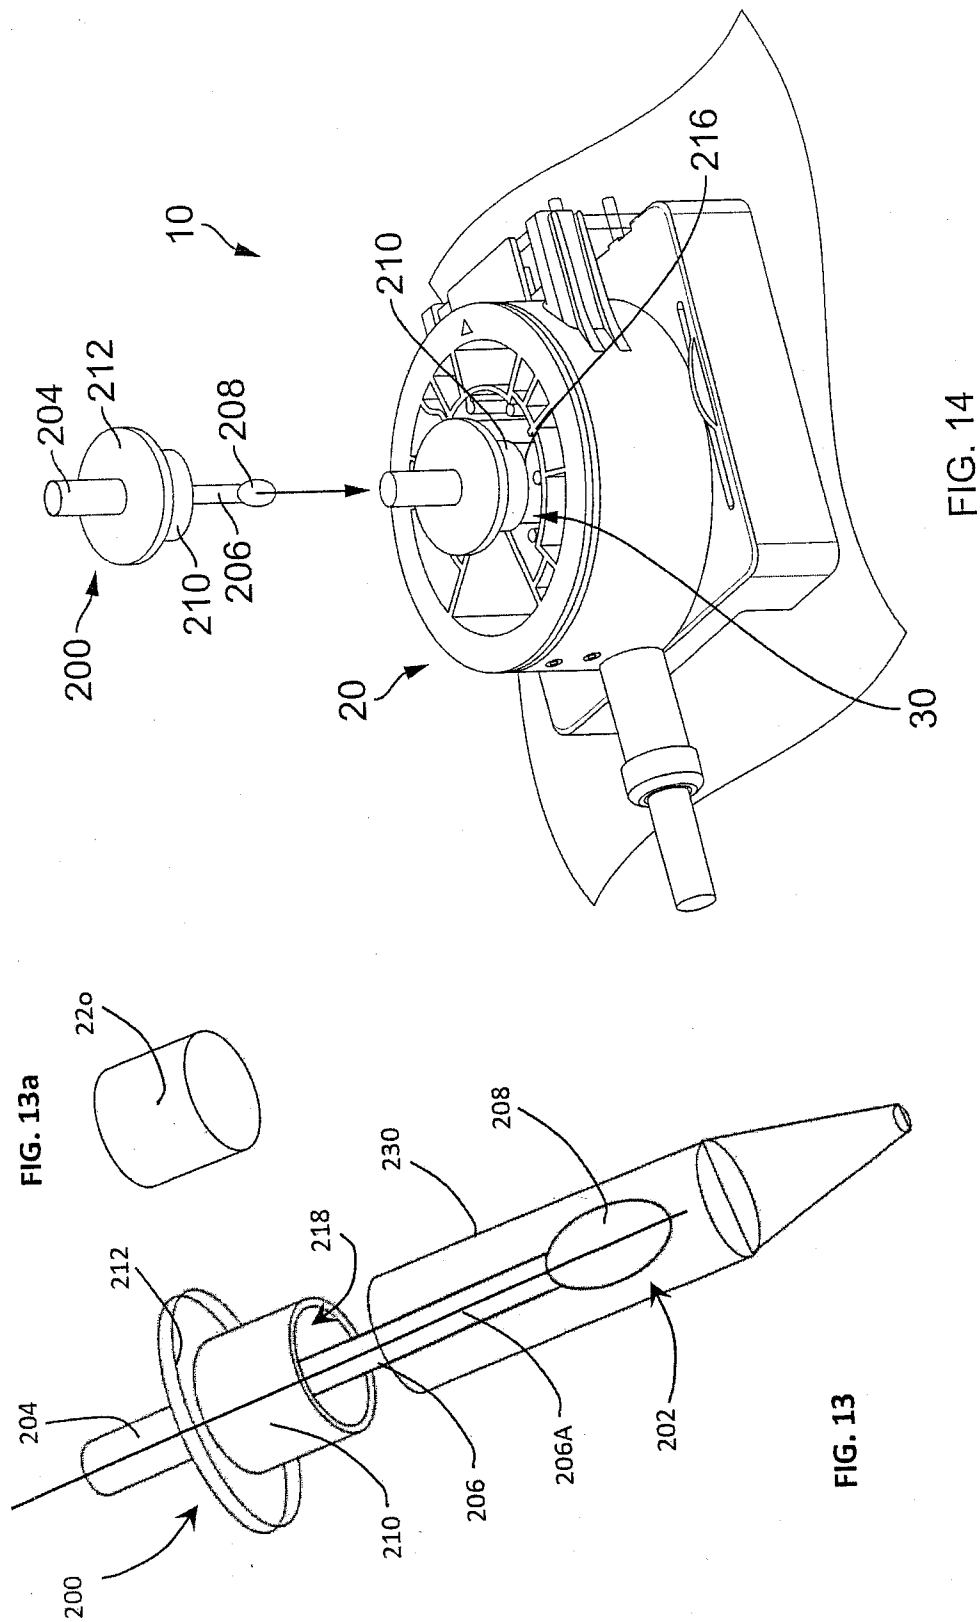

9/13


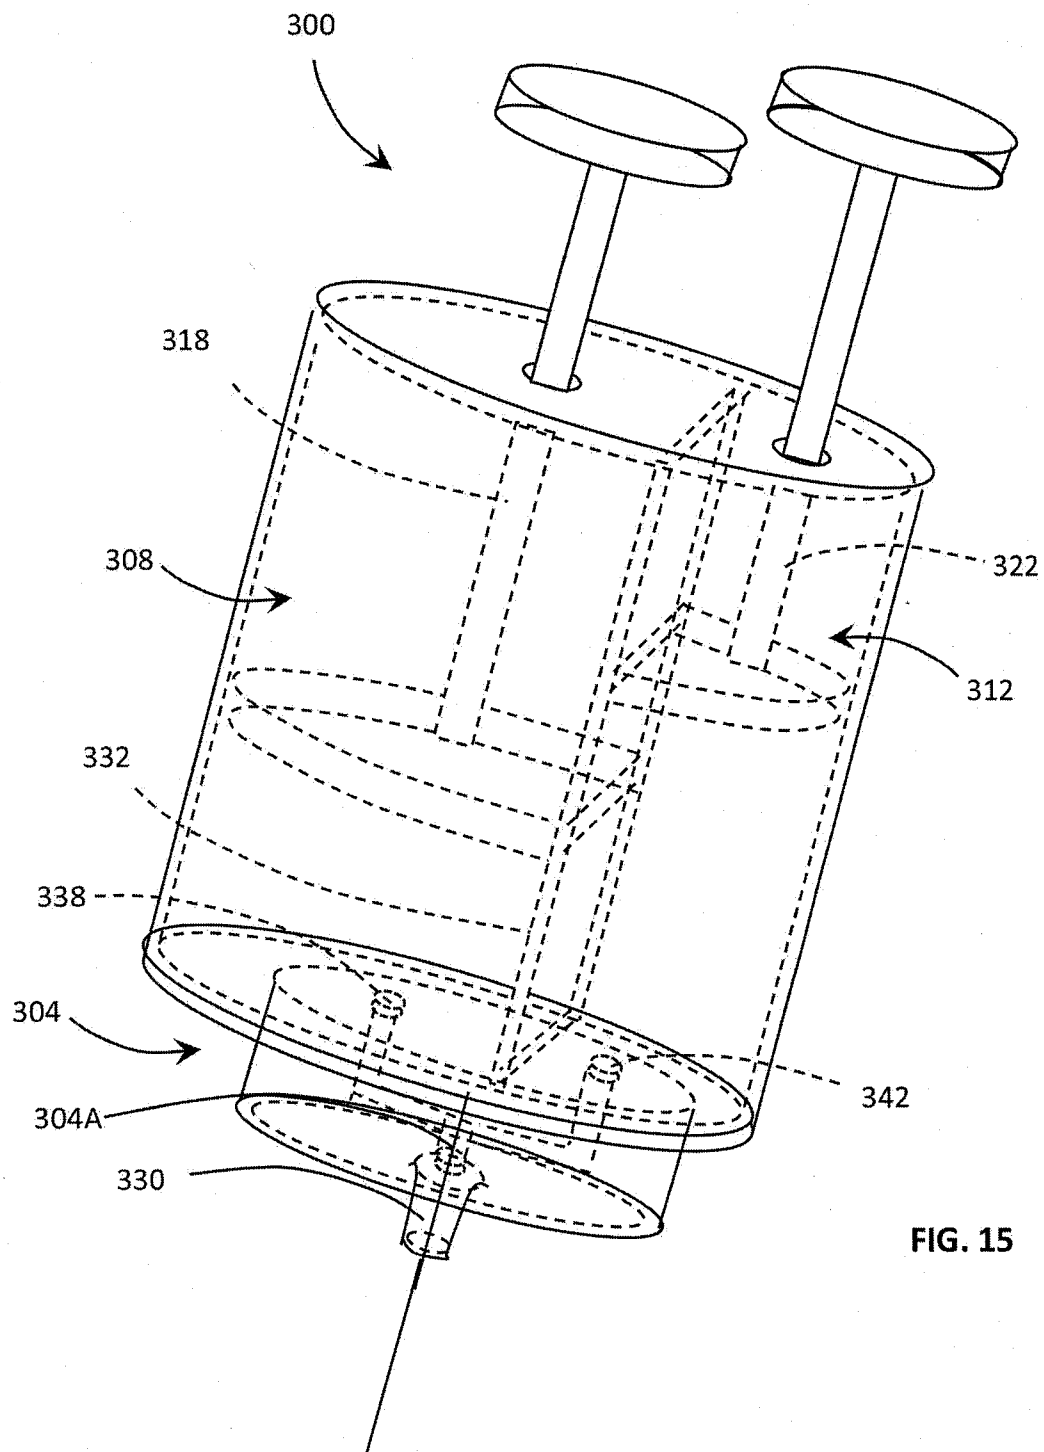


FIG. 15

10/13

FIG. 16

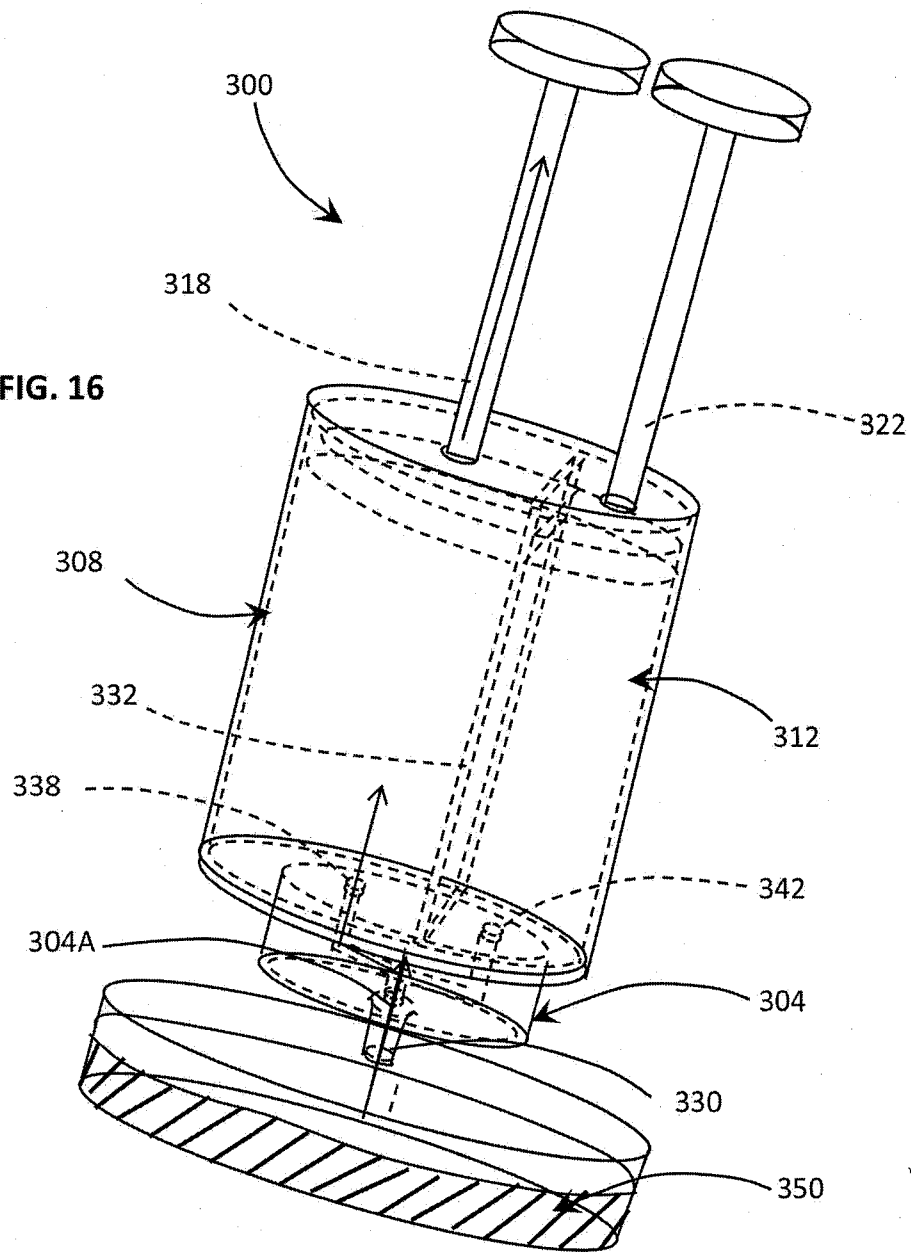

11/13

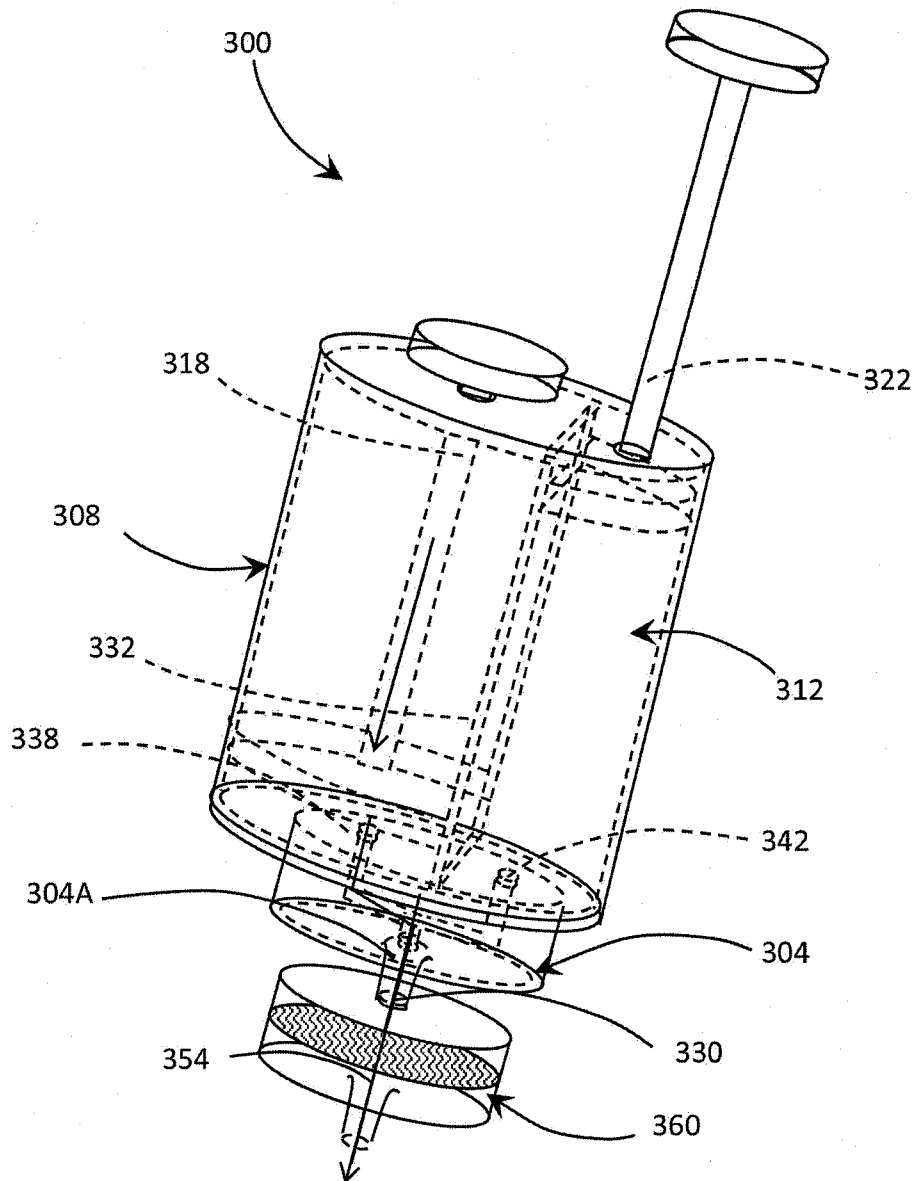


FIG. 17

12/13

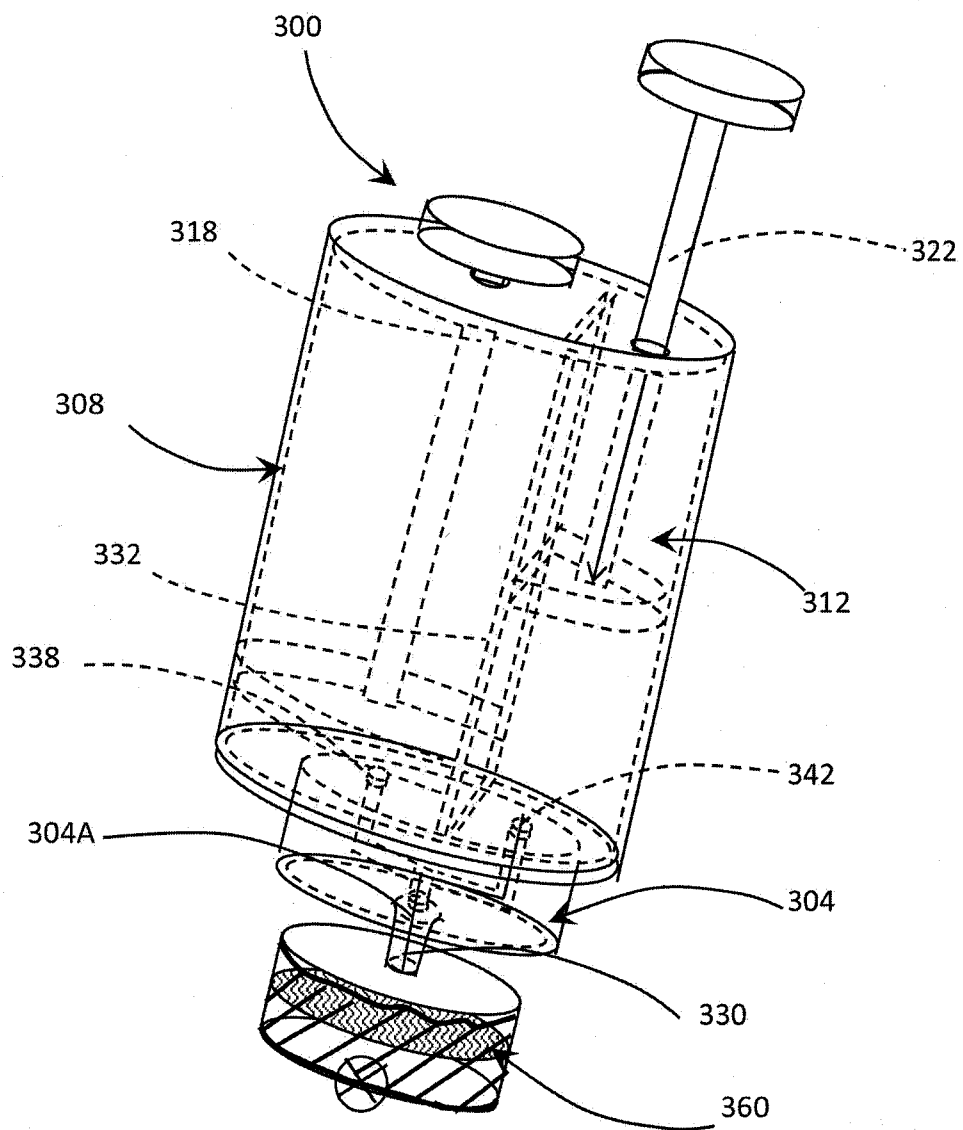


FIG. 18

13/13

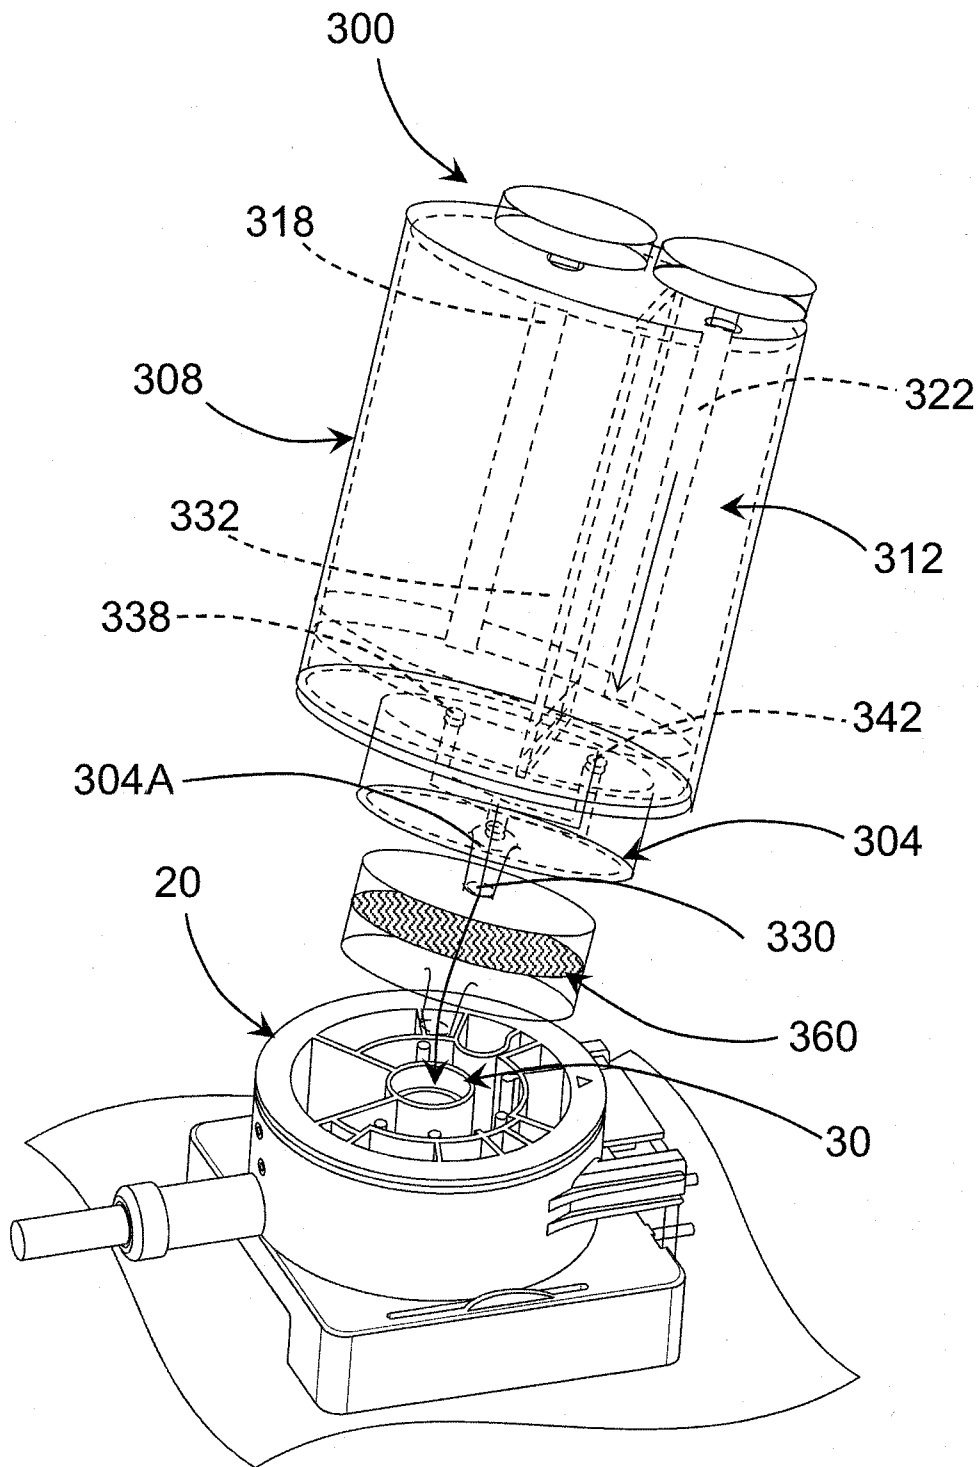


FIG. 19

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2017/027651**A. CLASSIFICATION OF SUBJECT MATTER****G01N 1/14(2006.01)i, C12Q 1/68(2006.01)i, C12N 15/10(2006.01)i, G01N 33/02(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G01N 1/14; G01N 21/76; G01N 33/558; B01L 3/00; G01N 35/00; C12M 1/30; A61M 5/08; C12Q 1/68; C12Q 1/66; C12N 15/10; G01N 33/02

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: dual plunger syringe, valve, filter, lysis module, disposable cartridge

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2003-0109057 A1 (DICESARE et al.) 12 June 2003 See paragraphs [0002], [0056]-[0081] and figures 1-10.	14-24
Y		1-13
Y	US 4609371 A (PIZZINO, JOANNE L.) 02 September 1986 See column 2, line 54 - column 5, line 18 and figures 1, 2A-2B, 3-6.	1-13
Y	EP 0693560 A2 (BECTON DICKINSON AND COMPANY) 24 January 1996 See column 3, line 27 - column 17, line 27 and figures 3-4.	5, 12-13
A	US 5965453 A (SKIFFINGTON et al.) 12 October 1999 See column 9, line 66 - column 10, line 58 and figures 1-4, 5A-5G.	1-24
A	US 2004-0152206 A1 (DAVIS et al.) 05 August 2004 See paragraphs [0037]-[0054] and figures 1-4.	1-24



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

12 July 2017 (12.07.2017)

Date of mailing of the international search report

12 July 2017 (12.07.2017)

Name and mailing address of the ISA/KR

International Application Division

Korean Intellectual Property Office


189 Cheongsa-ro, Seo-gu, Daejeon, 35208, Republic of Korea

Facsimile No. +82-42-481-8578

Authorized officer

LEE, Hun Gil

Telephone No. +82-42-481-8525



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2017/027651

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2003-0109057 A1	12/06/2003	US 2002-0001539 A1 US 2003-0129765 A1 US 2003-0186458 A1 US 6548018 B2 US 6881554 B2 US 6887681 B2 US 7485262 B2	03/01/2002 10/07/2003 02/10/2003 15/04/2003 19/04/2005 03/05/2005 03/02/2009
US 4609371 A	02/09/1986	EP 0212798 A1 EP 0217546 A1 US 4610666 A	04/03/1987 08/04/1987 09/09/1986
EP 0693560 A2	24/01/1996	AU 2331095 A BR 9503364 A CA 2152307 A1 EP 0693560 A3 JP 08-062225 A US 5639428 A	01/02/1996 27/02/1996 20/01/1996 22/01/1997 08/03/1996 17/06/1997
US 5965453 A	12/10/1999	US 6180395 B1	30/01/2001
US 2004-0152206 A1	05/08/2004	US 2005-0059165 A9 WO 03-064046 A1	17/03/2005 07/08/2003