




(86) Date de dépôt PCT/PCT Filing Date: 2007/01/26
 (87) Date publication PCT/PCT Publication Date: 2007/08/09
 (45) Date de délivrance/Issue Date: 2015/05/05
 (85) Entrée phase nationale/National Entry: 2008/07/14
 (86) N° demande PCT/PCT Application No.: US 2007/061118
 (87) N° publication PCT/PCT Publication No.: 2007/090050
 (30) Priorité/Priority: 2006/01/27 (US60/743,183)

(51) Cl.Int./Int.Cl. *A61N 1/362* (2006.01)
 (72) Inventeurs/Inventors:
 MARSEILLE, OLIVER, DE;
 KERKHOFFS, WOLFGANG, DE;
 SCHUMACHER, OLIVER, DE
 (73) Propriétaire/Owner:
 CIRCULITE, INC, US
 (74) Agent: MACRAE & CO.

(54) Titre : **SYSTEME D'ASSISTANCE CARDIAQUE**
 (54) Title: **HEART ASSIST SYSTEM**

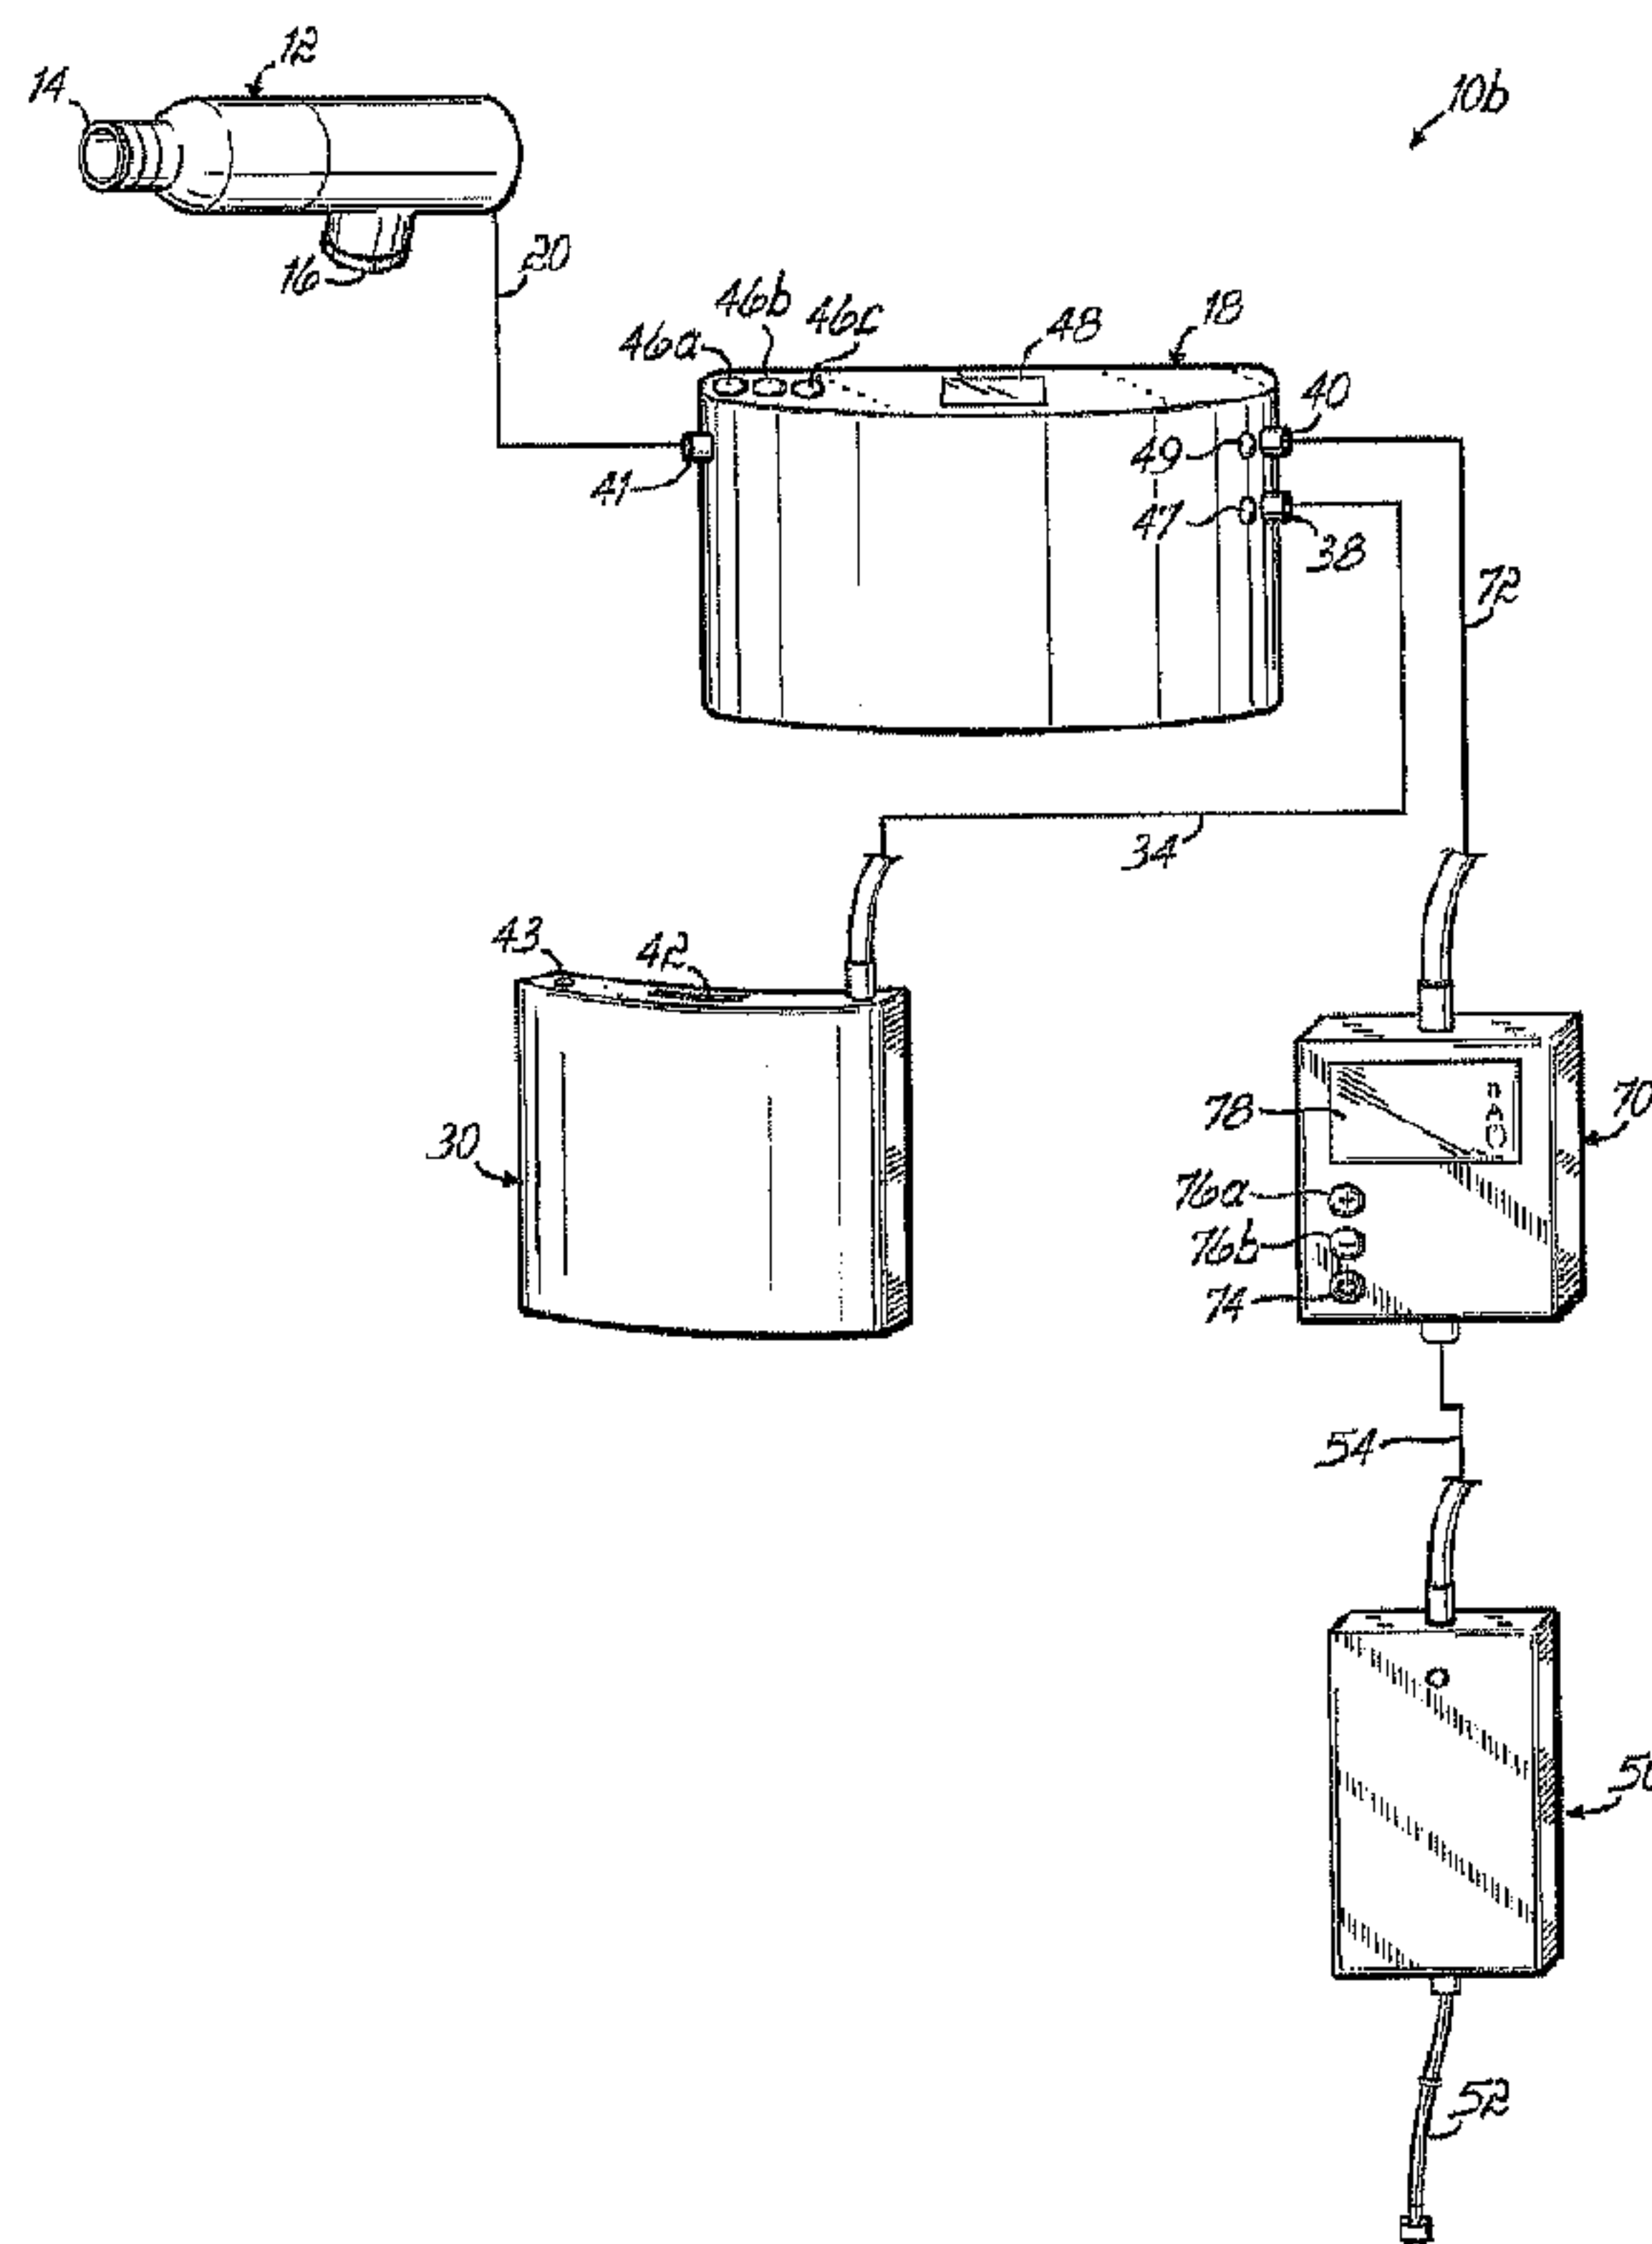

(57) **Abrégé/Abstract:**

A supplemental blood flow system (10, 10a-e) for assisting with blood circulation in a patient. The system includes a supplemental blood flow device (12) implantable in the patient and a controller (18) for directing electrical power to the supplemental blood flow device (12) and controlling the flow rate of blood through the device (12). The controller (18) includes first and second power inlets (38, 40) and a power outlet (41). The power outlet (41) is adapted to be coupled to an electrical line (20) leading to the supplemental blood flow device (12). A portable programming module (70) may be coupled to at least one of the first and second power inlets (38, 40) and operable to adjust pump operating parameters stored in the controller (18) to be changed according to the needs of the patient.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
9 August 2007 (09.08.2007)

PCT

(10) International Publication Number
WO 2007/090050 A3(51) International Patent Classification:
A61N 1/362 (2006.01)Berg 9, 52078 Aachen (DE). SCHUMACHER, Oliver
[DE/DE]; Heinrichsallee 60, Aachen (DE).(21) International Application Number:
PCT/US2007/061118(74) Agents: ROONEY, Kevin, G. et al.; WOOD, HERRON
& EVANS, L.L.P., 441 VINE STREET, 2700 Carew Tower,
Cincinnati, OH 45202 (US).

(22) International Filing Date: 26 January 2007 (26.01.2007)

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS,
JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS,
LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MY,
MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS,
RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(25) Filing Language: English

(26) Publication Language: English


(30) Priority Data:
60/743,183 27 January 2006 (27.01.2006) US(71) Applicant (for all designated States except US): CIR-
CULITE, INC. [US/US]; 401 Hackensack Avenue,
Hackensack, NJ 07601 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): MARSEILLE,
Oliver [DE/DE]; Karl-marx-allee 154, 52074 Aachen
(DE). KERKHOFFS, Wolfgang [NL/DE]; Am Rollefer(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,

[Continued on next page]

(54) Title: HEART ASSIST SYSTEM

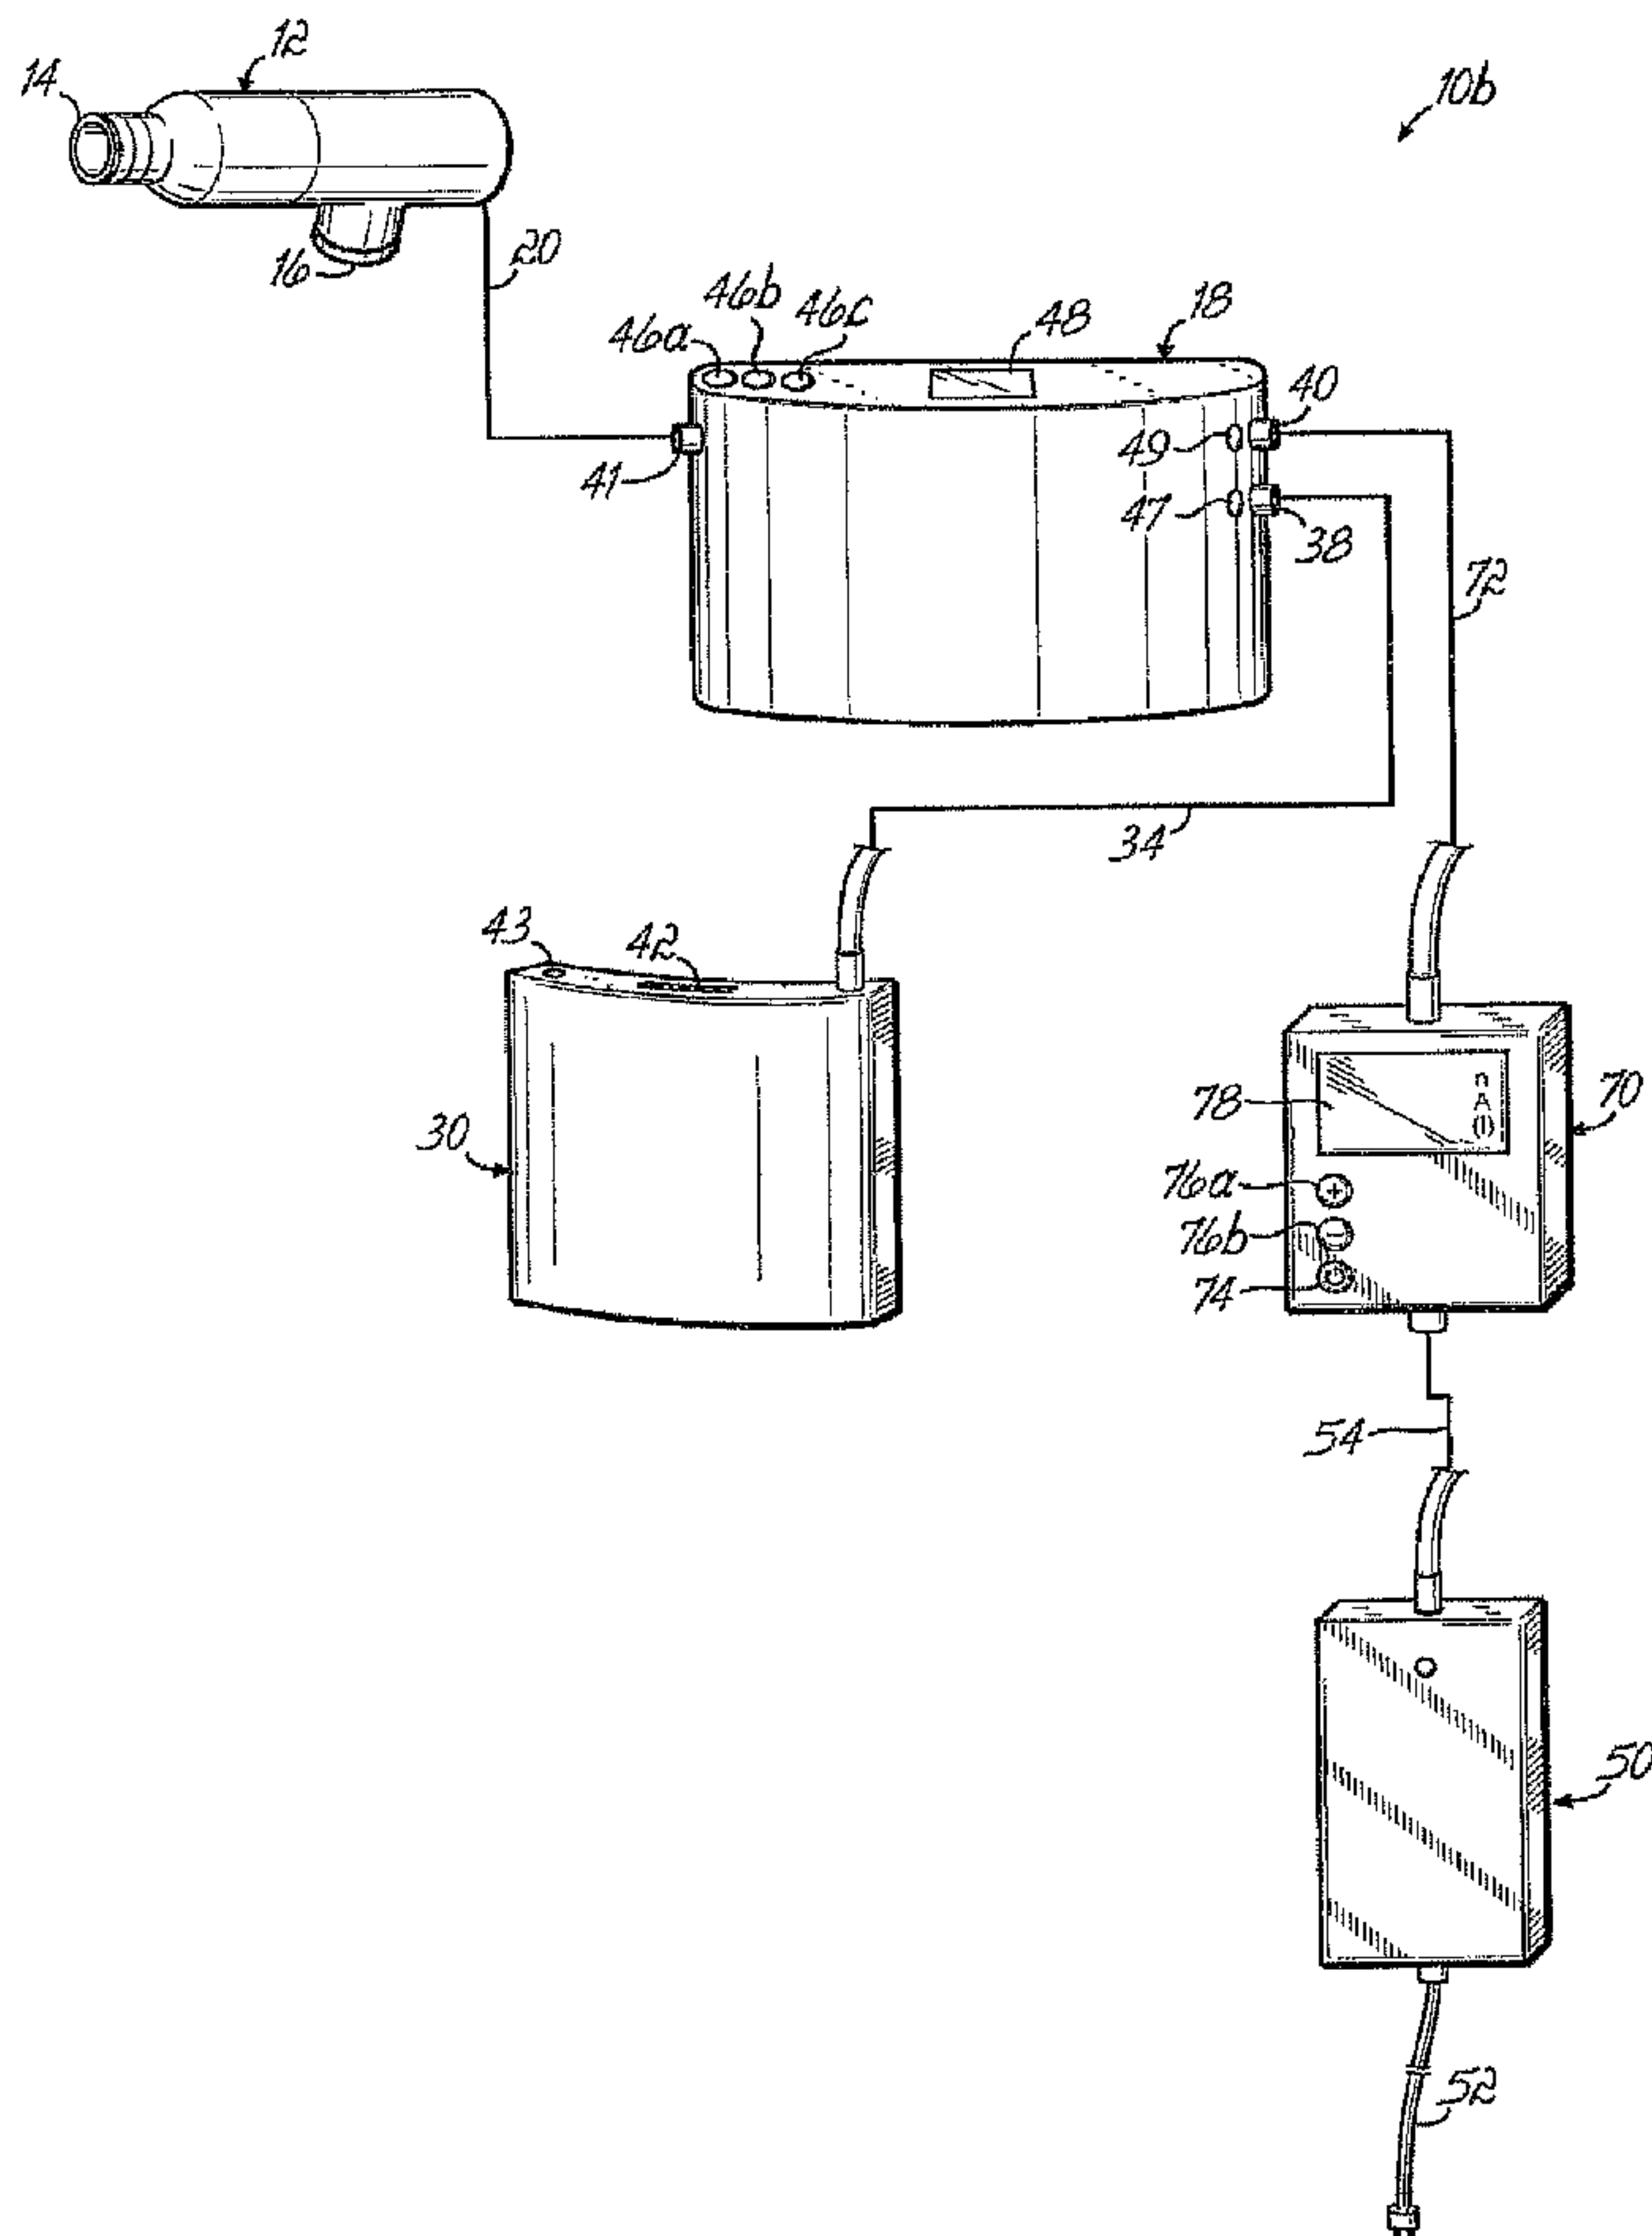

(57) Abstract: A supplemental blood flow system (10, 10a-e) for assisting with blood circulation in a patient. The system includes a supplemental blood flow device (12) implantable in the patient and a controller (18) for directing electrical power to the supplemental blood flow device (12) and controlling the flow rate of blood through the device (12). The controller (18) includes first and second power inlets (38, 40) and a power outlet (41). The power outlet (41) is adapted to be coupled to an electrical line (20) leading to the supplemental blood flow device (12). A portable programming module (70) may be coupled to at least one of the first and second power inlets (38, 40) and operable to adjust pump operating parameters stored in the controller (18) to be changed according to the needs of the patient.

WO 2007/090050 A3

WO 2007/090050 A3



FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT,
RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA,
GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(88) Date of publication of the international search report:
31 January 2008

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

HEART ASSIST SYSTEM

[0001]

TECHNICAL FIELD

[0002] The present invention generally relates to systems for assisting with blood circulation in a patient and, in particular, ventricular assist devices and control systems.

BACKGROUND

[0003] A ventricular assist device (VAD) typically involves the use of a heart pump connected with various control and power source components. VAD systems are desirably portable so that a patient may move around during normal daily activities. Various devices are used to control and monitor the implantable blood pump associated with the system and the patient is permanently linked to the pump controller. Therefore, VAD systems should be as lightweight, small and convenient to wear as possible. A controller that is connected to the pump is adjusted by authorized personnel from time to time. This has generally been accomplished at specified locations such as in hospitals and doctors' offices. In addition, the controller should not be adjusted by unauthorized personnel. Some known manners of addressing these issues have involved the use of a control panel or programming module that is built into the controller worn by the patient and that is locked to prevent misuse or unauthorized use. Alternatively, the controller is linked to a complex and immobile base station control unit for programming purposes (e.g., pump speed adjustment). Unfortunately, incorporating the control panel or programming module into the portable unit worn by the patient increases the complexity, size and weight of the control unit. On the other hand, the use of an immobile base station forces the patient to go to a doctor's office or hospital for any required adjustment of pump speed.

SUMMARY

[0004] Generally, in a first aspect, a supplemental blood flow system for assisting with blood circulation in a patient is provided and comprises a

supplemental blood flow device, a controller and a portable programming module. In this aspect, the controller directs electrical power to the supplemental blood flow device and controls the flow rate of blood through the device. The controller includes first and second power inlets and a power outlet with the power outlet adapted to be coupled to an electrical line leading to the supplemental blood flow device. The portable programming module is configured such that it can be coupled to at least one of the first and second power inlets of the controller and operable to allow pump operating parameters stored in the controller to be changed according to the needs of the patient. The supplemental blood flow device is configured such that it is implantable in the patient.

[0005] In other aspects, first and second power supply units may be connected to the first and second power inlets. At least one of the first and second power supply units may be electrically connected to the programming module. The power supply units may take various forms, such as batteries, AC to DC adaptors, DC to DC adaptors and combinations of these or other types of power supply units. The controller may be configured such that it may transmit data to a computer, such as through a wireless transmitter.

[0006] In another aspect, a supplemental blood flow system for assisting with blood circulation in a patient may comprise the supplemental blood flow device and controller as described above in combination with first and second power supply units capable of being electrically connected to the first and second power inlets of the controller. Other combinations of the various features described herein also fall within the scope of the present invention.

[0007] Various additional combinations, features and advantages of the invention will become more readily apparent to those of ordinary skill in the art upon review of the following detailed description of illustrative embodiments taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] Fig. 1 is a schematic diagram of a system constructed in accordance with a first illustrative embodiment.

[0009] Fig. 2 is a schematic diagram of a system constructed in accordance with a second illustrative embodiment.

[0010] Fig. 3A is a schematic diagram of a system constructed in accordance with a third illustrative embodiment.

[0011] Fig. 3B is a schematic diagram of a system constructed in accordance with a fourth illustrative embodiment.

[0012] Fig. 3C is a schematic diagram of a system constructed in accordance with a fifth illustrative embodiment.

[0013] Fig. 3D is a schematic diagram of a system constructed in accordance with a sixth illustrative embodiment.

[0014] Fig. 4 is a perspective view of a battery recharge unit with two batteries connected thereto.

DETAILED DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

[0015] Fig. 1 illustrates a system 10 constructed in accordance with an illustrative embodiment of the invention. Specifically, system 10 includes a supplemental heart or blood pump 12 having an inlet 14 and an outlet 16. Supplemental heart pump 12 is adapted to be implanted within a patient and, for example, receives blood through the inlet 14 from the left side of the patient's heart (e.g., the left ventricle) and expels the blood into the patient's circulatory system through the outlet 16 and an attached conduit or catheter (not shown). Heart pump 12 is merely illustrative in nature and may be substituted with any appropriate heart pump or supplemental blood flow device. One example is disclosed in U.S. Patent No 6,116,862. Heart pump 12 is connected to a controller 18 via an electrical line 20. Controller 18 supplies power to the heart pump 12 and controls the speed of the pump 12 in accordance with the medical needs of the patient. A primary battery 30 and a backup or secondary battery 32 are respectively coupled to the controller 18 by power lines 34, 36 connected to power inlet connectors 38, 40 on the controller 18. A power outlet connector 41 couples to electrical line 20. The controller 18 and batteries 30, 32 may be carried by a suitable belt or strap arrangement (not shown) to allow the patient to comfortably carry the components during his or her daily activities. All data may be stored in the controller by, for example, a flash memory device or other suitable memory component.

[0016] The batteries 30, 32, respectively, include charge indicator lights 42, 44. These indicator lights may, for example, comprise different colored

LED's (light emitting diodes) such as red, yellow and green lights for indicating battery strength or charge to the user. Separate indicator lights 43, 45 may also be provided on the respective batteries 30, 32. For example, these indicator lights 43, 45 may comprise red LED's which, when lit, will indicate to the user that the associated battery 30 or 32 is not operating or is in need of recharging and/or replacement. The use of two separate batteries 30, 32 in this configuration allows the user a longer period of time away from a stationary power source, such as AC or other main power supplied in their home or other location. When the charge in the primary battery 30 falls below a predetermined level as, for example, sensed by the controller 18, the controller 18 will cause the secondary battery 32 to supply power to the controller 18 and to the pump 12. The controller 18 includes indicator lights 46a, 46b, 46c which may, for example, be red, yellow and green lights, respectively. The red light 46a can indicate that the pump 12 is stopped and/or indicate the need for some immediate repair or diagnostic action to address a problem with the system 10. This may be accompanied by an acoustic alarm. The yellow light 46b may indicate that inspection and/or routine maintenance is required, and the green light 46c may indicate normal operating mode. The display 48 indicates estimated remaining battery life in hours and minutes. Respective indicator lights 47, 49 associated with connectors 38, 40 may also be provided and, when lit, these red indicator lights 47, 49 can indicate the need to change the battery 30 or 32 coupled with the associated connector 38 or 40.

[0017] Fig. 2 illustrates an alternative system 10a. In each of the alternative systems to be described herein, like reference numerals indicate like elements in the various figures and therefore these elements do not require further duplicative description. Fig. 2 illustrates the fact that one of the batteries may be replaced by an adaptor unit 50 which may be plugged into an AC power supply via a plug 52 and thereby supply electrical power to the controller 18 and pump 12 in a manner similar to the battery 32 shown in Fig. 1, and via connector 40. As needed by the user, the adaptor 50 may be an AC to DC adaptor or a DC to DC adaptor. At the same time that adaptor 50 is supplying electrical power to controller 18 and pump 12, it may also be recharging battery 30. As another aspect shown in Fig. 2, a computer 60 may receive data from the controller for review by a physician. This data may be transferred in a wireless manner, or an optional hard cable (not shown) may be connected

between controller 18 and computer 60. The data could be encoded so that the computer can detect and reject any false data. Such data may, for example, include pump speed, motor current, pump serial number, alarm status, or any data obtained by additional sensors or components associated with the system such as pressures, flow, temperature, heart rate, etc. and/or parameters obtained by any combination of the obtained data. The computer 60 may be limited, for example, to use for data acquisition and not used for changing any settings in the controller 18 associated with operating the pump, such as changing the pump speed. Such additional control and adjustment features may be reserved for other dedicated computers, controllers, etc., at a hospital and/or doctor's office and/or through the use of passcodes known only by authorized personnel.

[0018] Fig. 3A illustrates another alternative system 10b in which a programming module 70 is connected between adaptor 50 and connector 40 and pump 12. Electrical power is therefore supplied through programming module 70 to controller 18 via connector 40. In addition, programming module 70 will allow control parameters, such as pump speed, to be changed in the controller 18. Programming module 70 may more specifically include an on/off control element such as a button 74, an adjustment element such as a button 76a for increasing the pump speed, an adjustment element such as a button 76b for decreasing the pump speed, and a display 78 for displaying parameters such as motor current, alarm status and pump speed. Adaptor 50 not only supplies electrical power for operating the programming module 70, but as mentioned above, may also supply power through to the controller 18 and/or to the pump 12, and/or for simultaneously recharging battery 30.

[0019] Fig. 3B illustrates another alternative system 10c which is similar to system 10b shown in Fig. 3A, except that the adaptor 50 and programming module 70 are respectively coupled to connector 38, as opposed to connector 40. In this example, battery 32 has been connected to connector 40 via power line 36. Thus, connectors 38, 40 may be interchangeably used when connecting any types of power supplies and the programming module 70. In this example, line 72 can carry relatively low current electronic data transmissions between module 70 and controller 18 and also carry higher current electronic power necessary for operating the pump 12.

[0020] Fig. 3C illustrates another alternative system 10d which is similar to that shown in Fig. 3A, except that adaptor 50 has been replaced by battery 32 for powering programming module 70 and supplying power through to controller 18 and pump 12.

[0021] Fig. 3D illustrates another alternative system 10e which is similar to that shown in Fig. 3B except that adaptor 50 has been replaced by battery 30 for powering both the programming module 70 and also supplying power to the controller 18 and pump 12.

[0022] It will be appreciated that other configurations of the various components are also possible, as well as the addition of other suitable and useful components such as power supply components, control components or adaptors. One alternative, for example, is a 12 volt or 24 volt adaptor suitable for use in an automobile having a plug that may be inserted into a power receptacle in the automobile. The controller 18 may be designed to recognize when either an automotive adaptor or AC adaptor 50 is connected. Controller 18 can then use power from the connected adaptor as opposed to a connected battery so as to preserve battery life.

[0023] Fig. 4 illustrates a battery recharge unit 80 that may be plugged into a wall receptacle, for example, and may be used to recharge multiple batteries, such as batteries 30, 32 as shown. Recharge unit 80 may have a display 82 for indicating the remaining charging time, and may have various status indicator lights 84 for indicating charge status. For example, a red light may indicate that the battery is non-operative, a yellow light may indicate that the battery is charging, and a green light may indicate that the battery is fully charged. A number of connectors 86 may be provided for coupling several batteries to the charging unit 80.

[0024] While the present invention has been illustrated by a description of various preferred embodiments and while these embodiments have been described in some detail, it is not the intention of the Applicants to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications will readily appear to those skilled in the art. The various features of the invention may be used alone or in any combination depending on the needs and preferences of the user. This has been a description of the present invention, along with the preferred methods of

practicing the present invention as currently known. However, the invention itself should only be defined by the appended claims. What is claimed is:

Claims:

1. A supplemental blood flow system for assisting with blood circulation in a patient, the system comprising:

a supplemental blood flow device implantable in the patient;

a controller configured to direct electrical power to the supplemental blood flow device and controlling the flow rate of blood through the device, the controller having first and second power inlets and a power outlet, the power outlet adapted to be coupled to an electrical line leading to the supplemental blood flow device;

a portable programming module coupled to the first power inlet and configured to allow pump operating parameters stored in the controller to be changed according to the needs of the patient; and

at least one power supply unit configured to be coupled to the first and second power inlets, the at least one power supply unit including a power adaptor coupled to the portable programming module and a battery coupled to the second power inlet;

wherein the power adaptor supplies power to the portable programming module, through the portable programming module and the first power inlet to the controller, and through the controller and the second power inlet to the battery, to thereby charge the battery with power supplied through the controller.

2. The system of claim 1, wherein the at least one power supply unit comprises first and second power supply units capable of being electrically connected to the first and second power inlets.

3. The system of claim 2, wherein at least one of the first and second power supply units may be electrically connected to the programming module.

4. The system of claim 2, wherein the first and second power supply units respectively comprise first and second batteries.

5. The system of claim 2, wherein one of the first and second power supply units comprises an AC to DC adaptor.

6. The system of claim 2, wherein one of the first and second power supply units comprises a DC to DC adaptor.

7. The system of claim 1, wherein the controller is capable of one way data transmission to a computer.

8. The system of claim 7, wherein the controller includes a wireless transmitter for effecting the data transmission.

9. The system of claim 4, wherein the controller is operative to sense when the first battery is not supplying adequate electrical power and, as a result, direct electrical power from the second battery to the supplemental blood flow device.

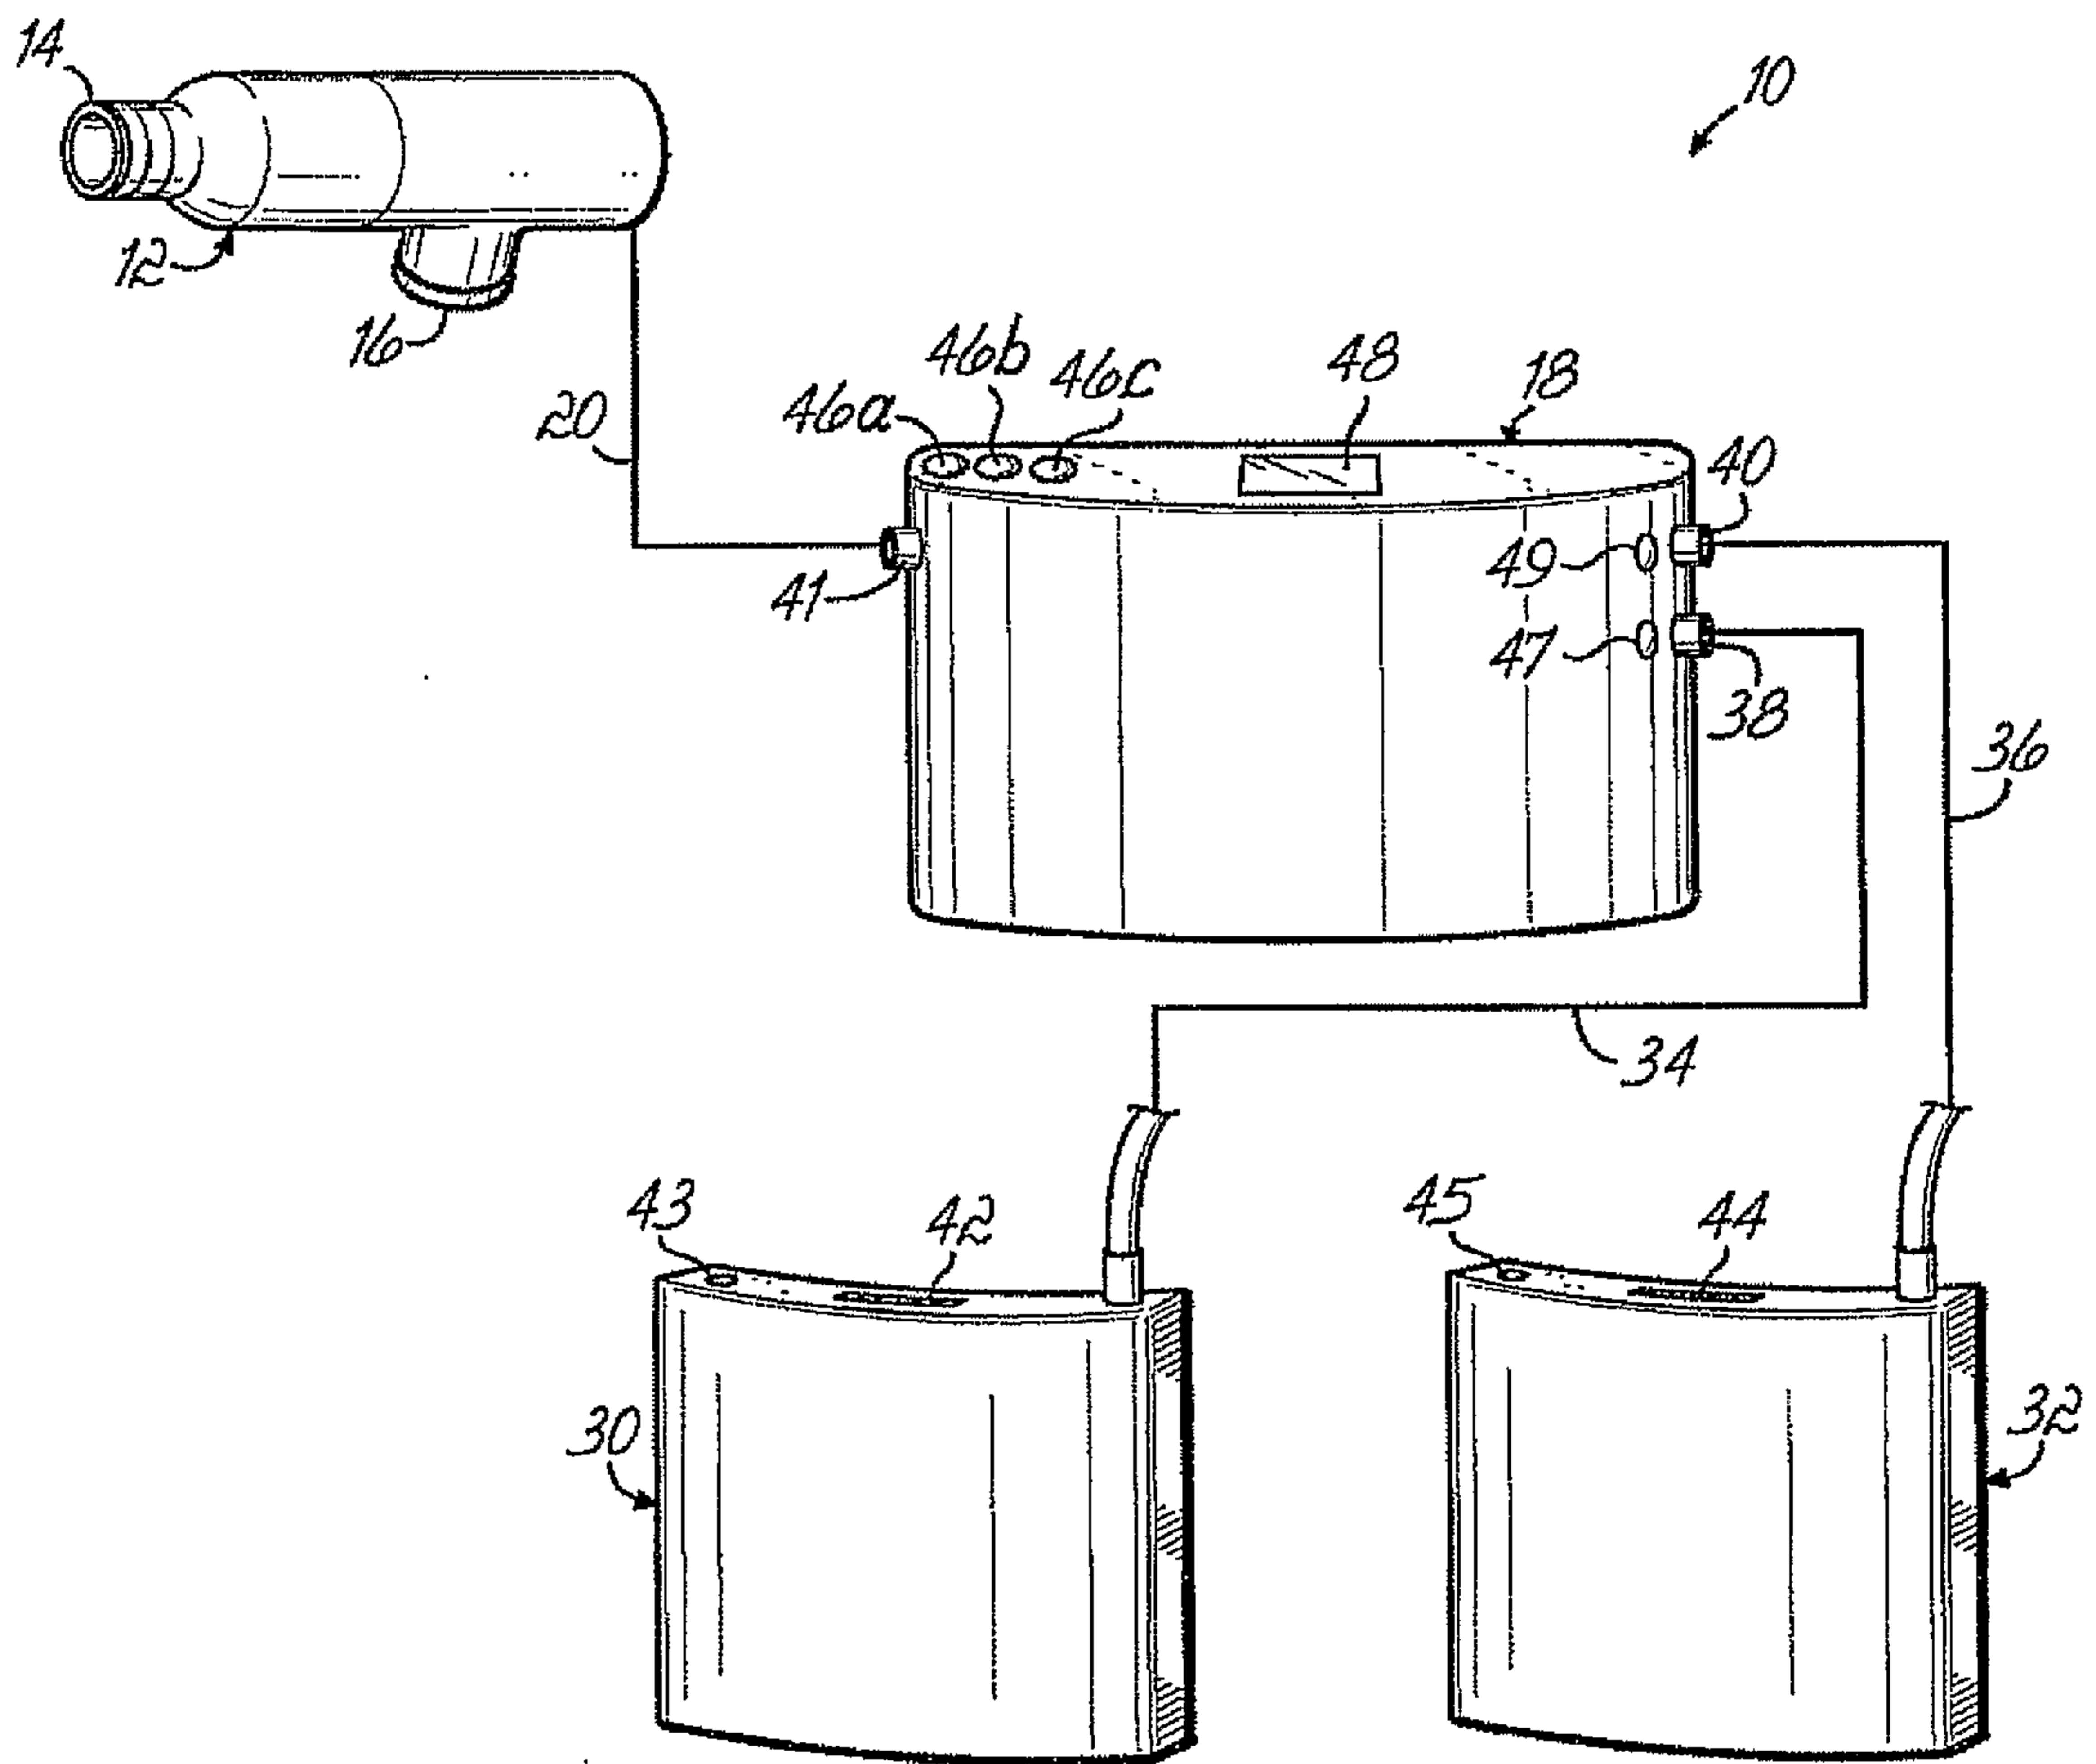


FIG. 1

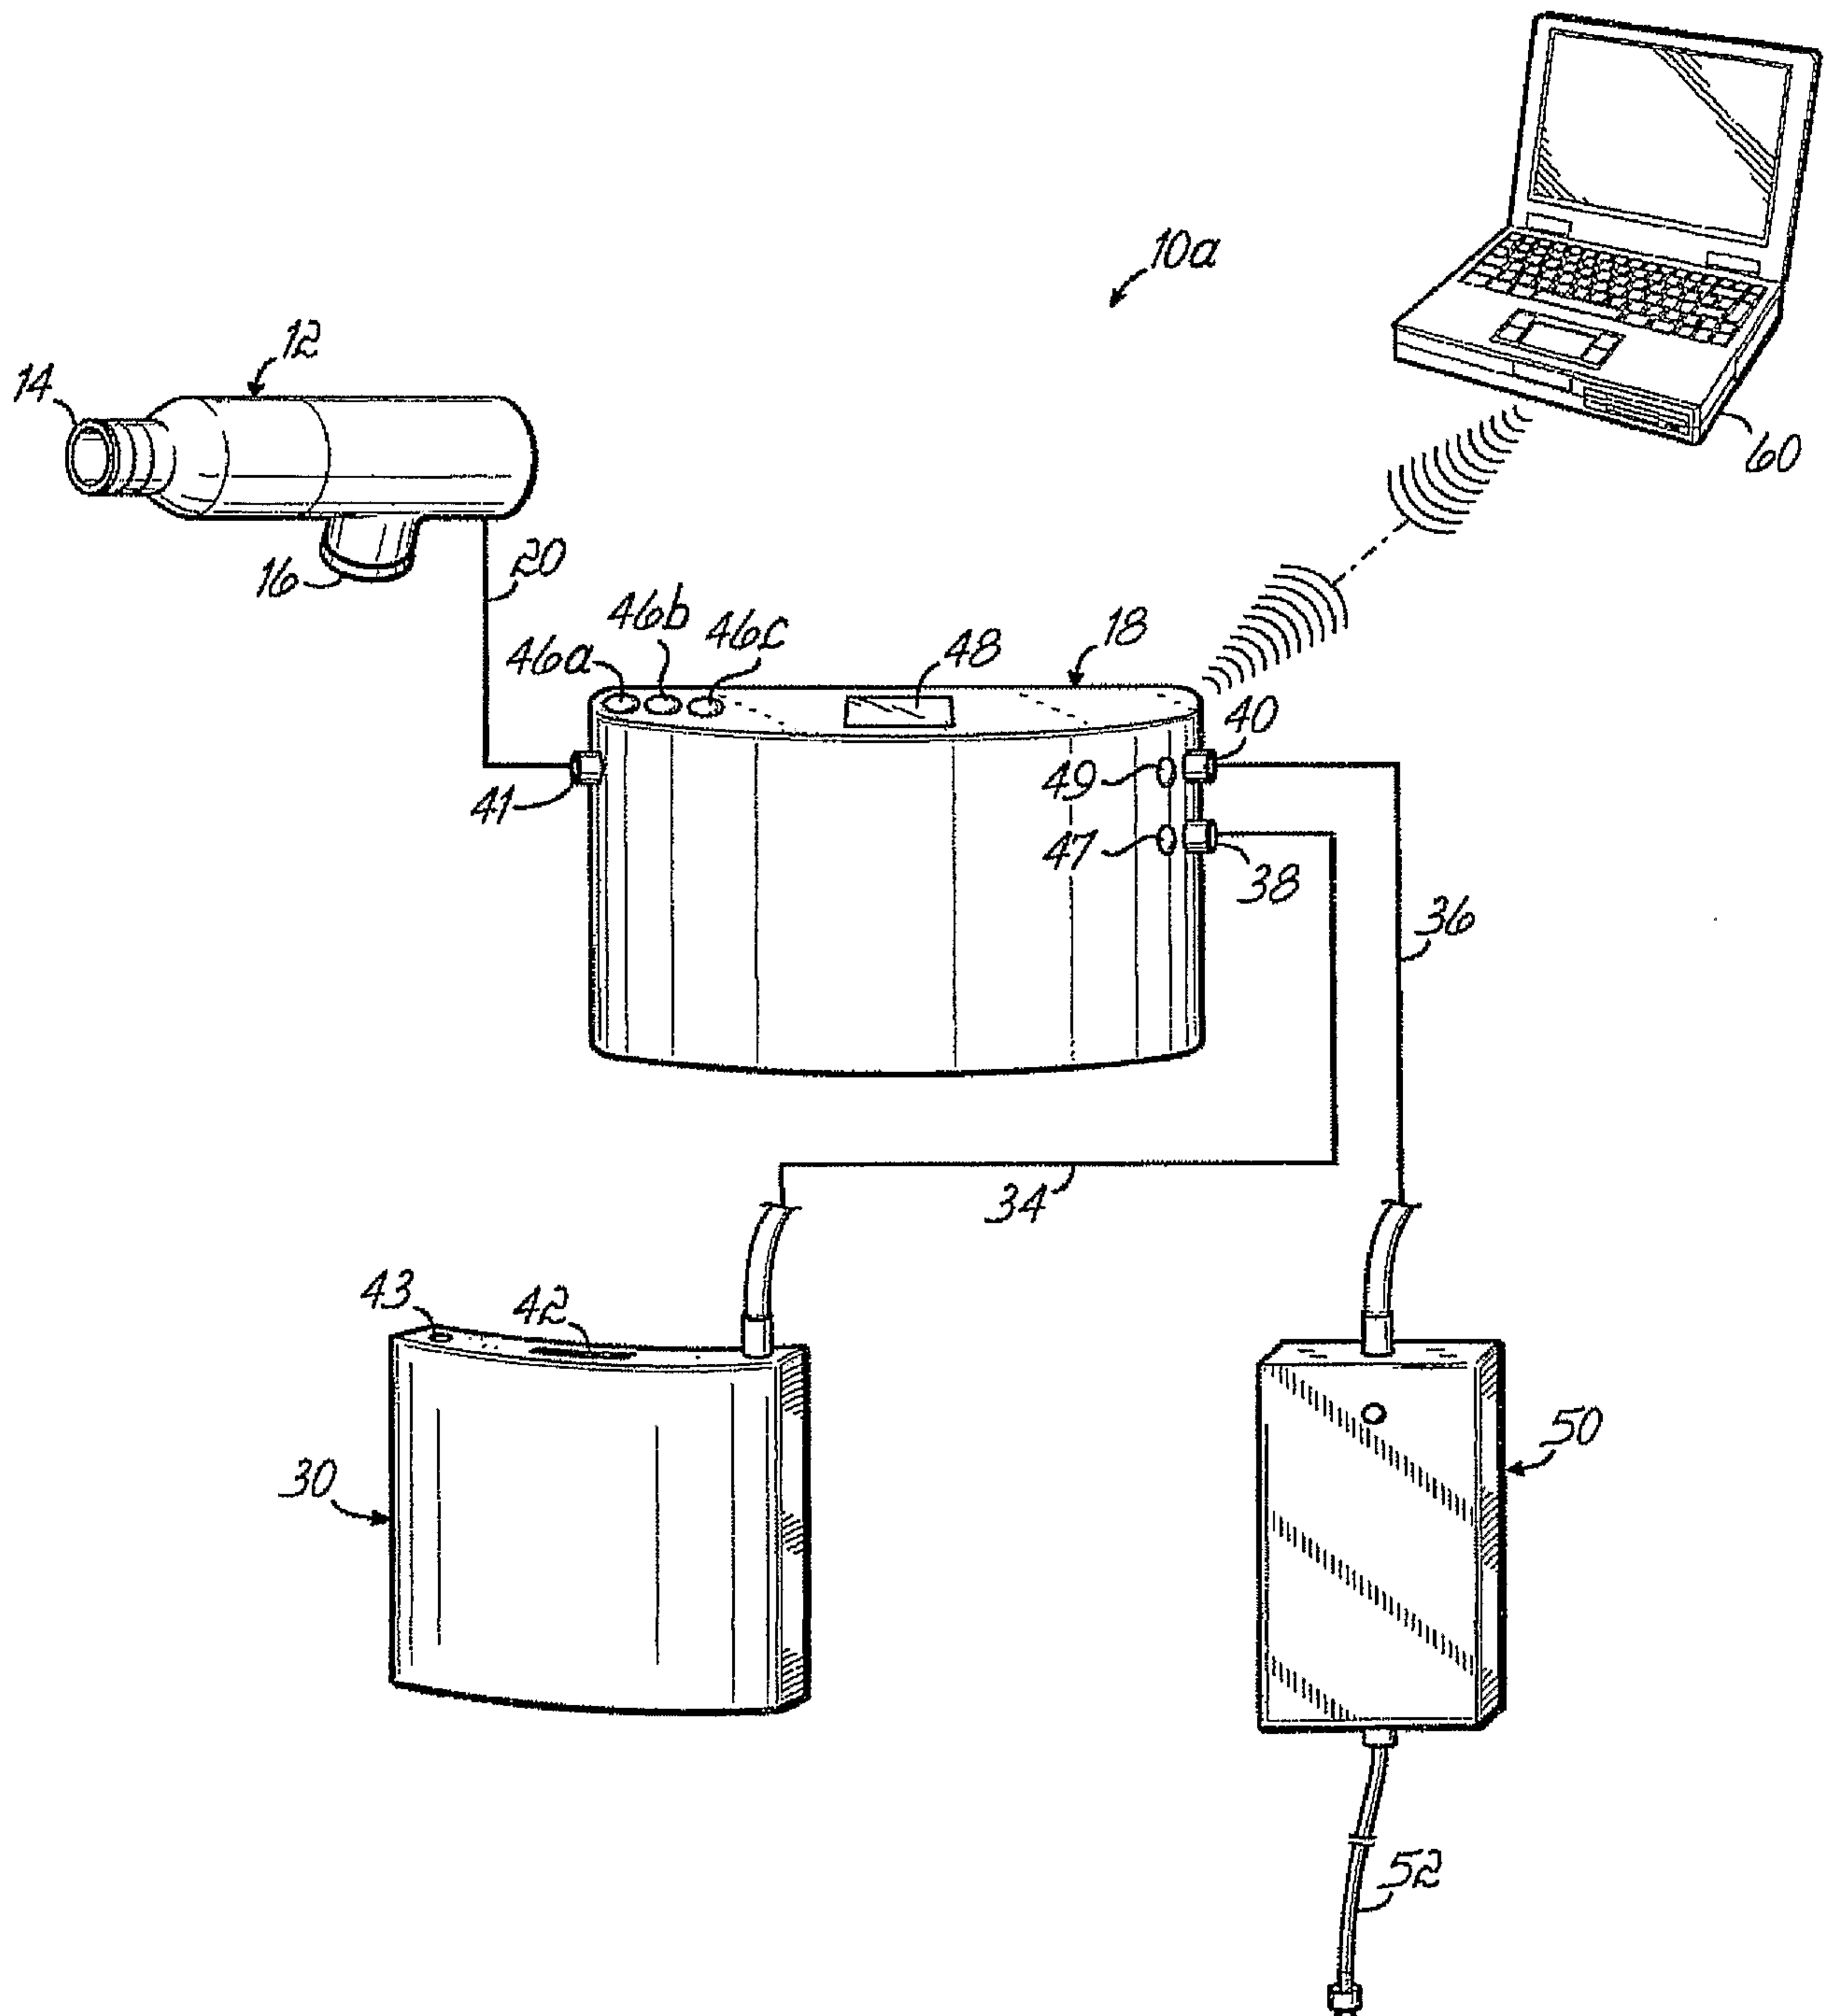


FIG. 2

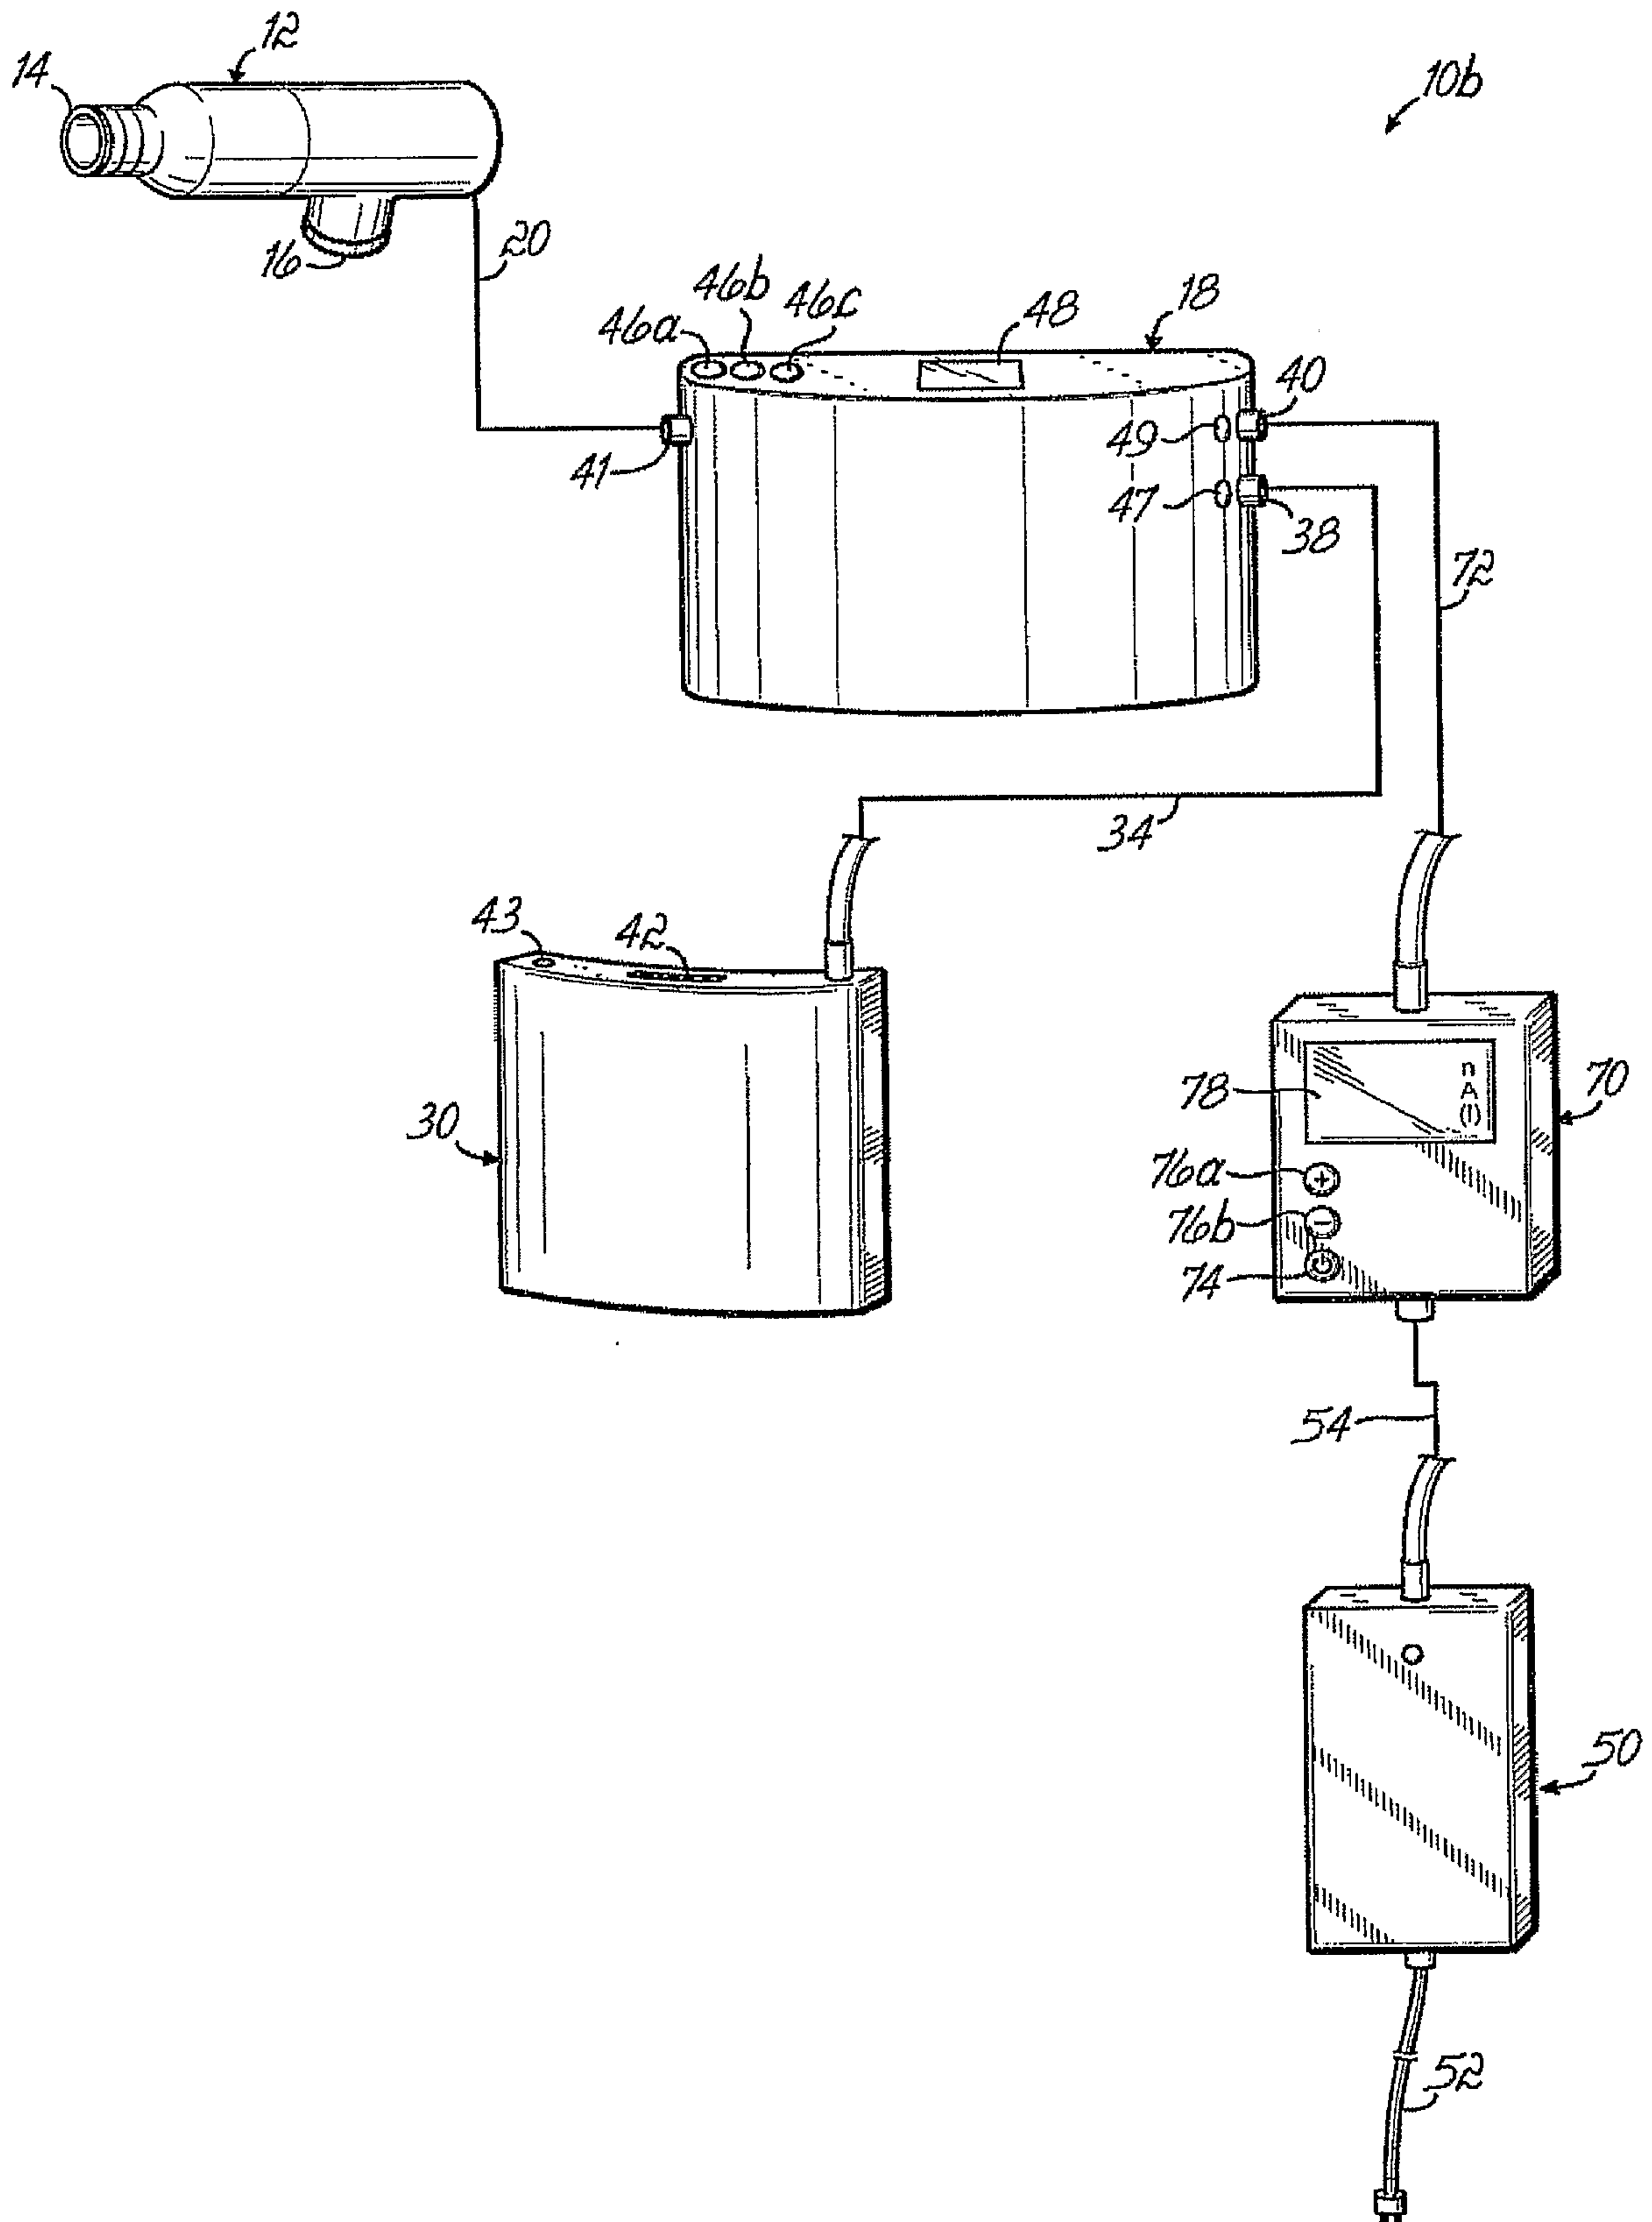


FIG. 3A

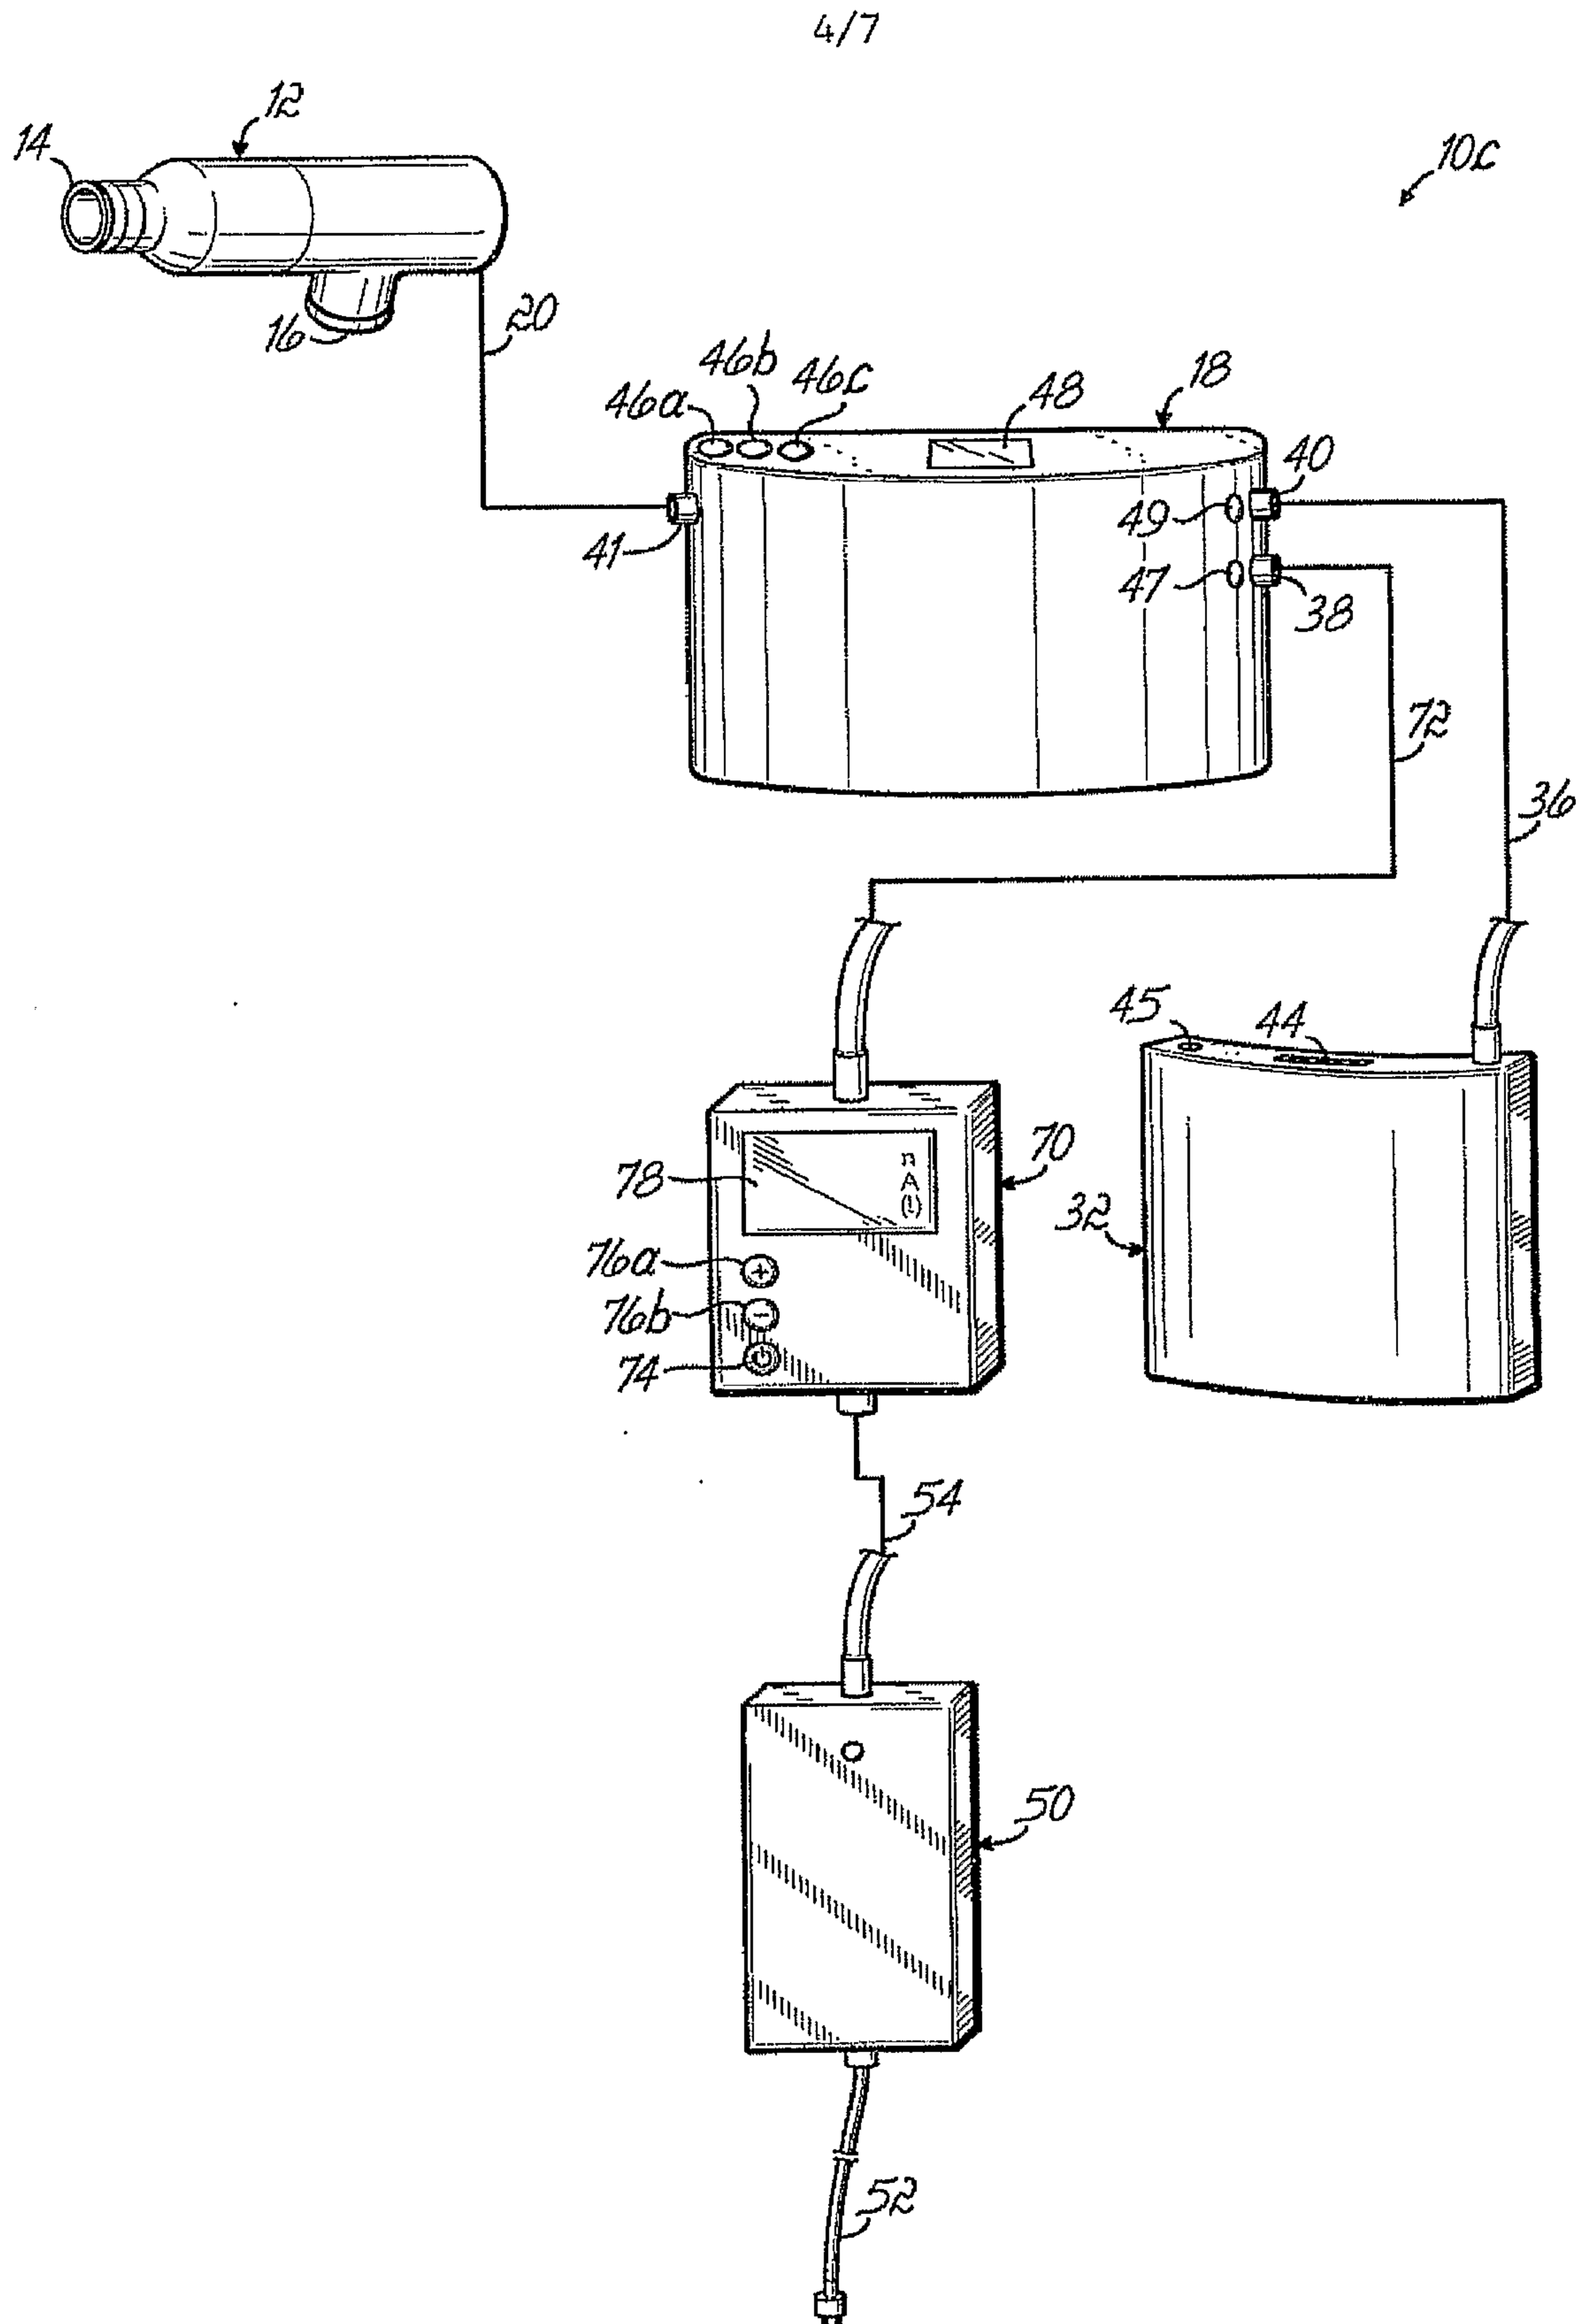


FIG. 3B

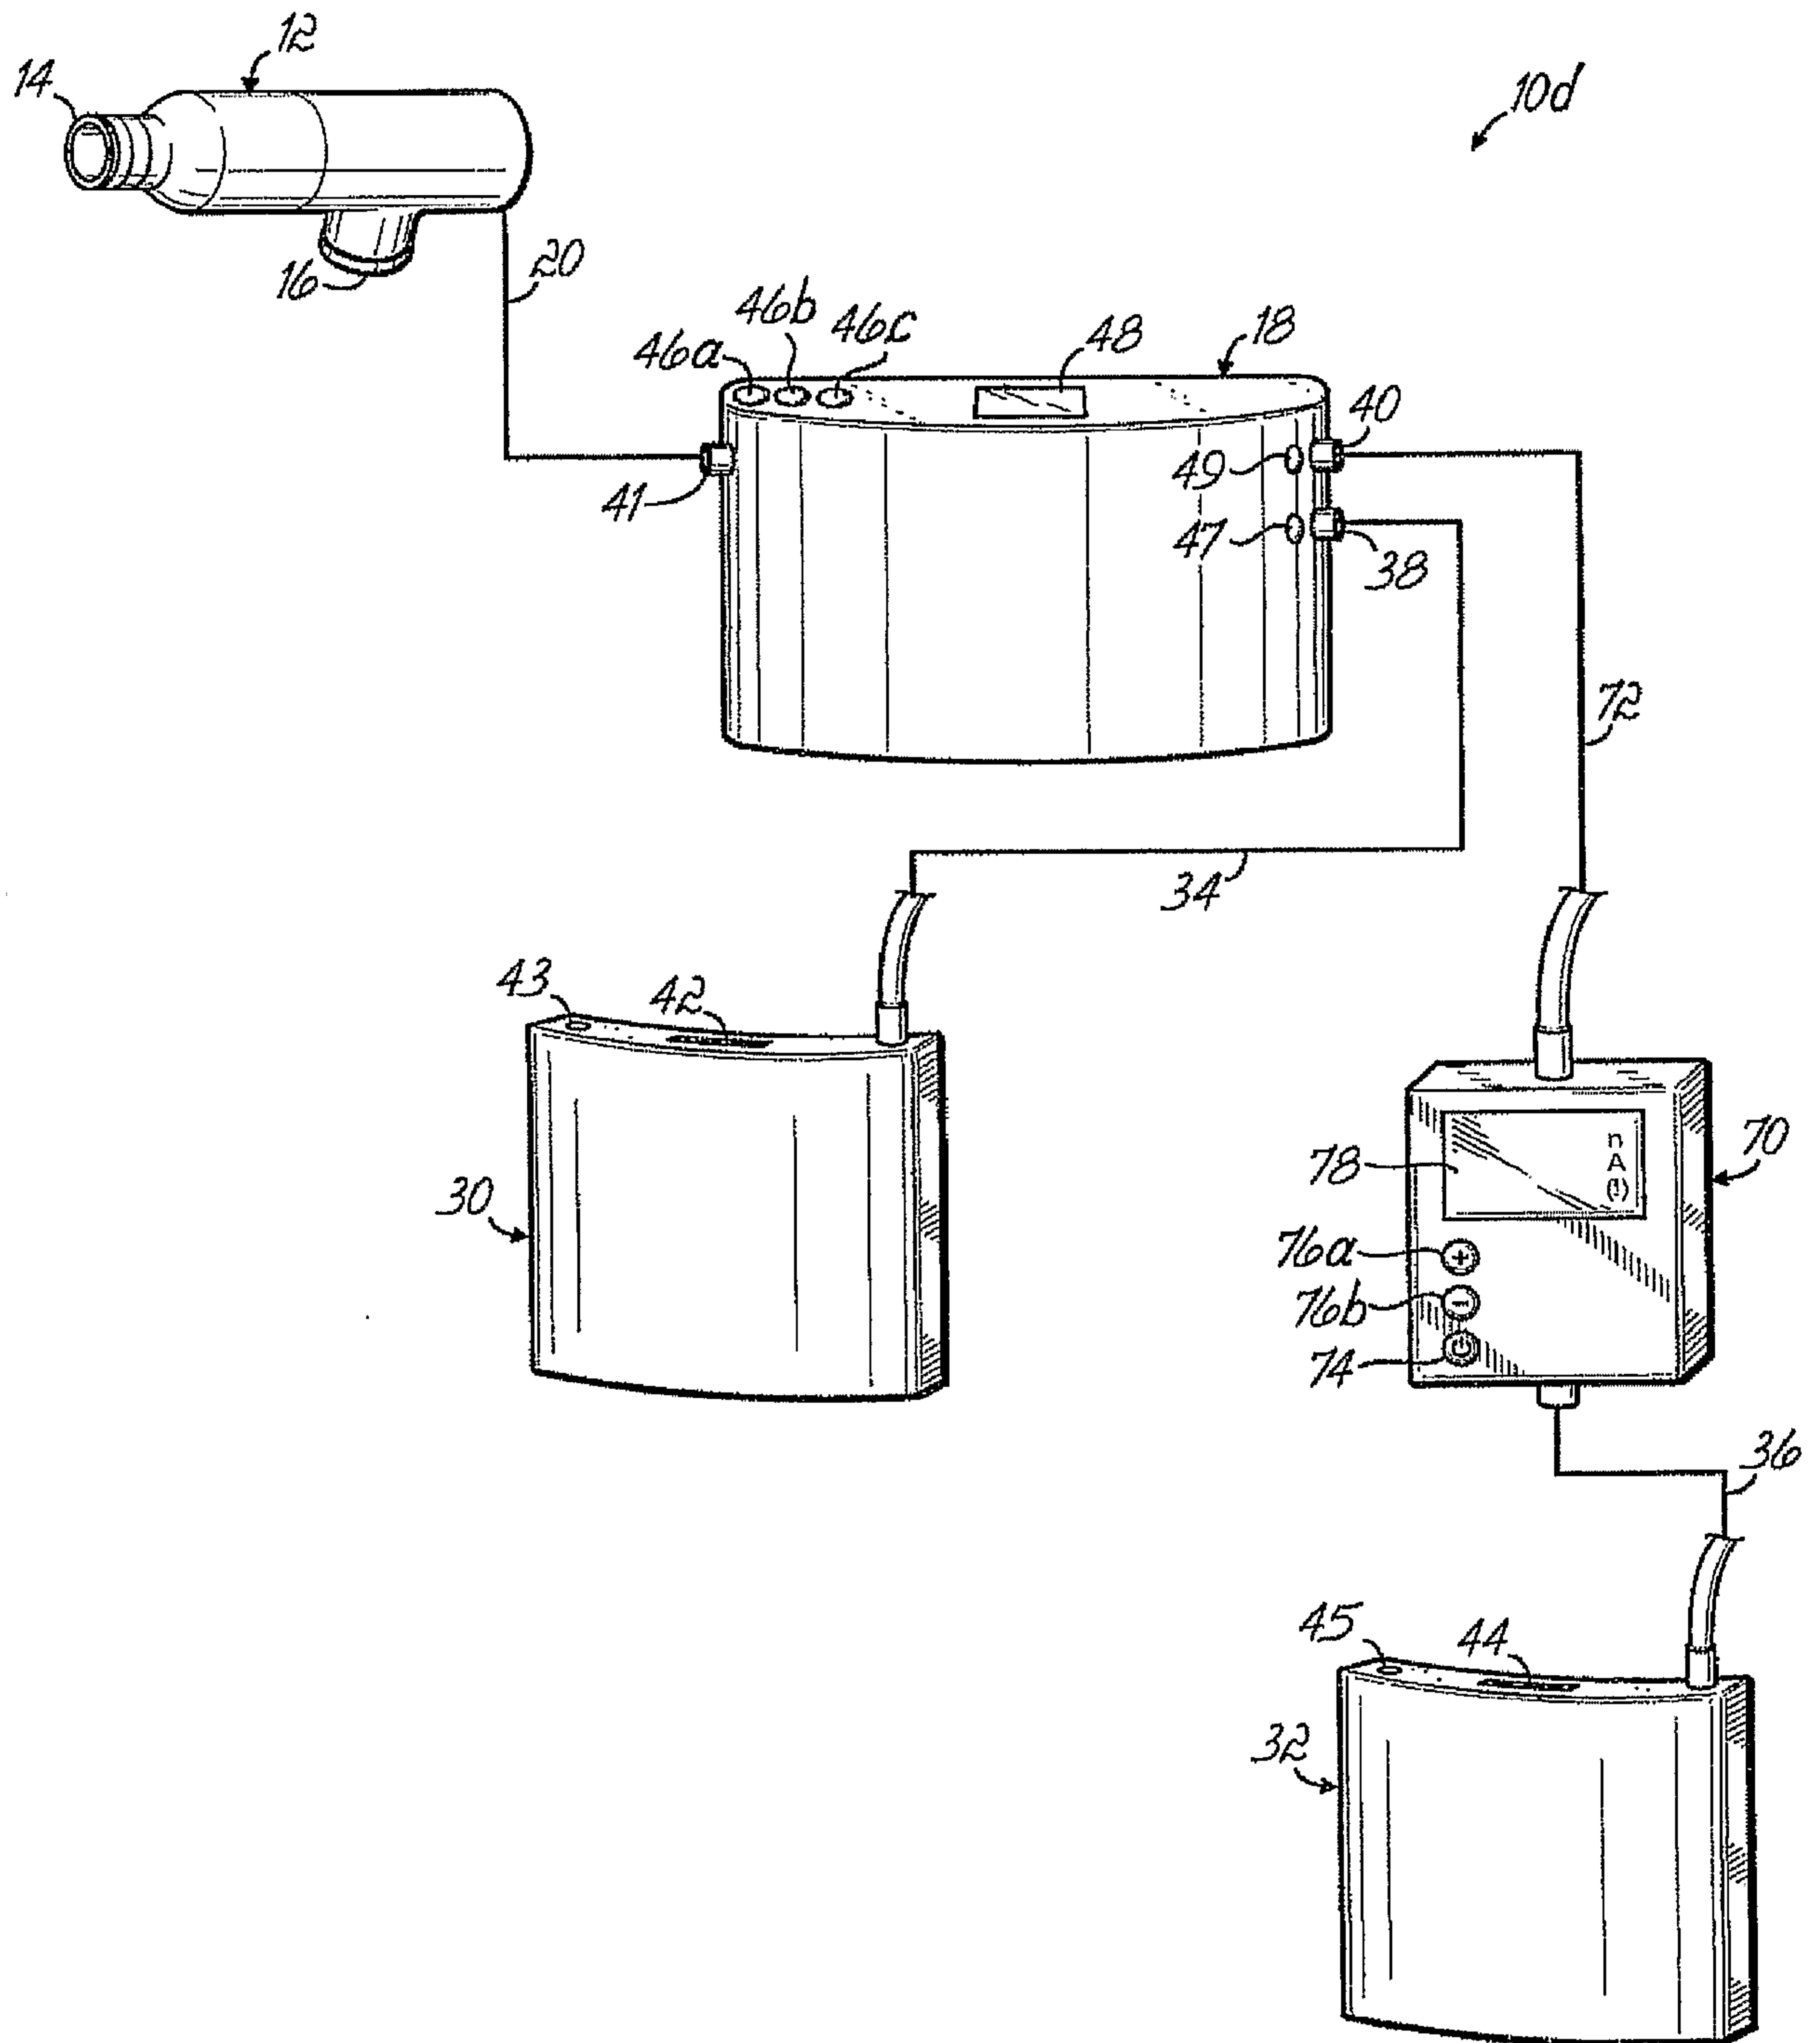


FIG. 3C

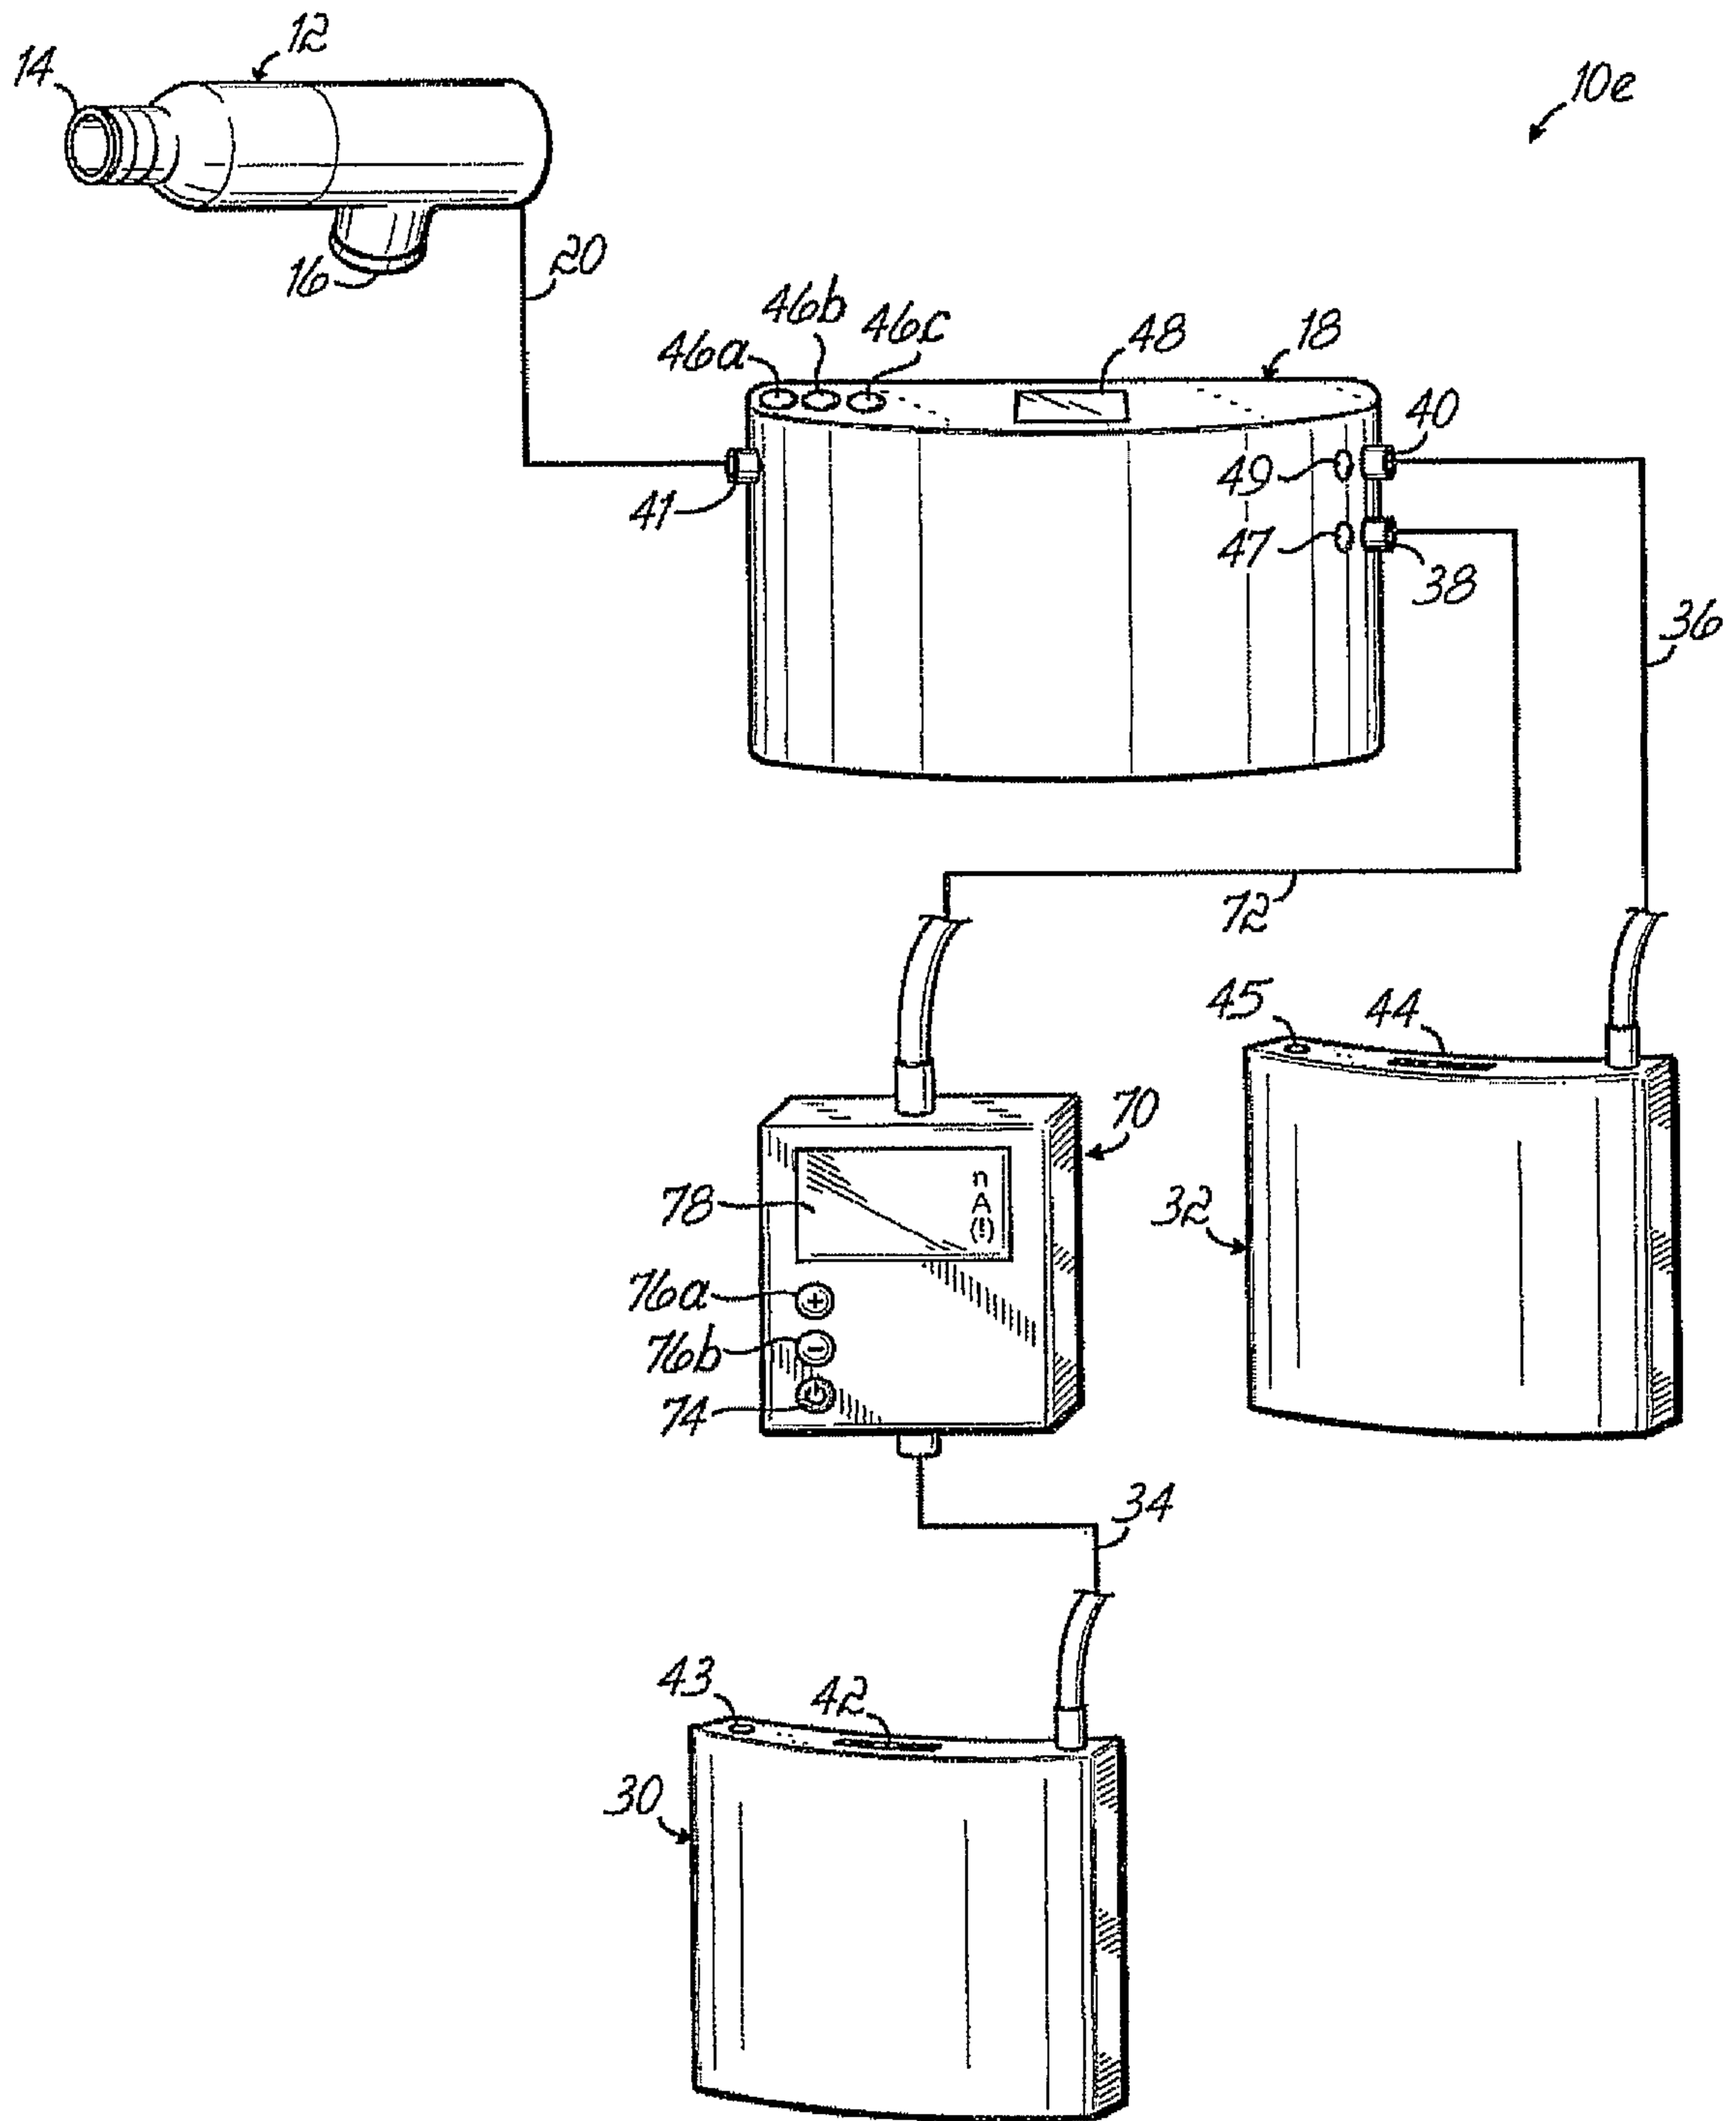


FIG. 3D

7/7

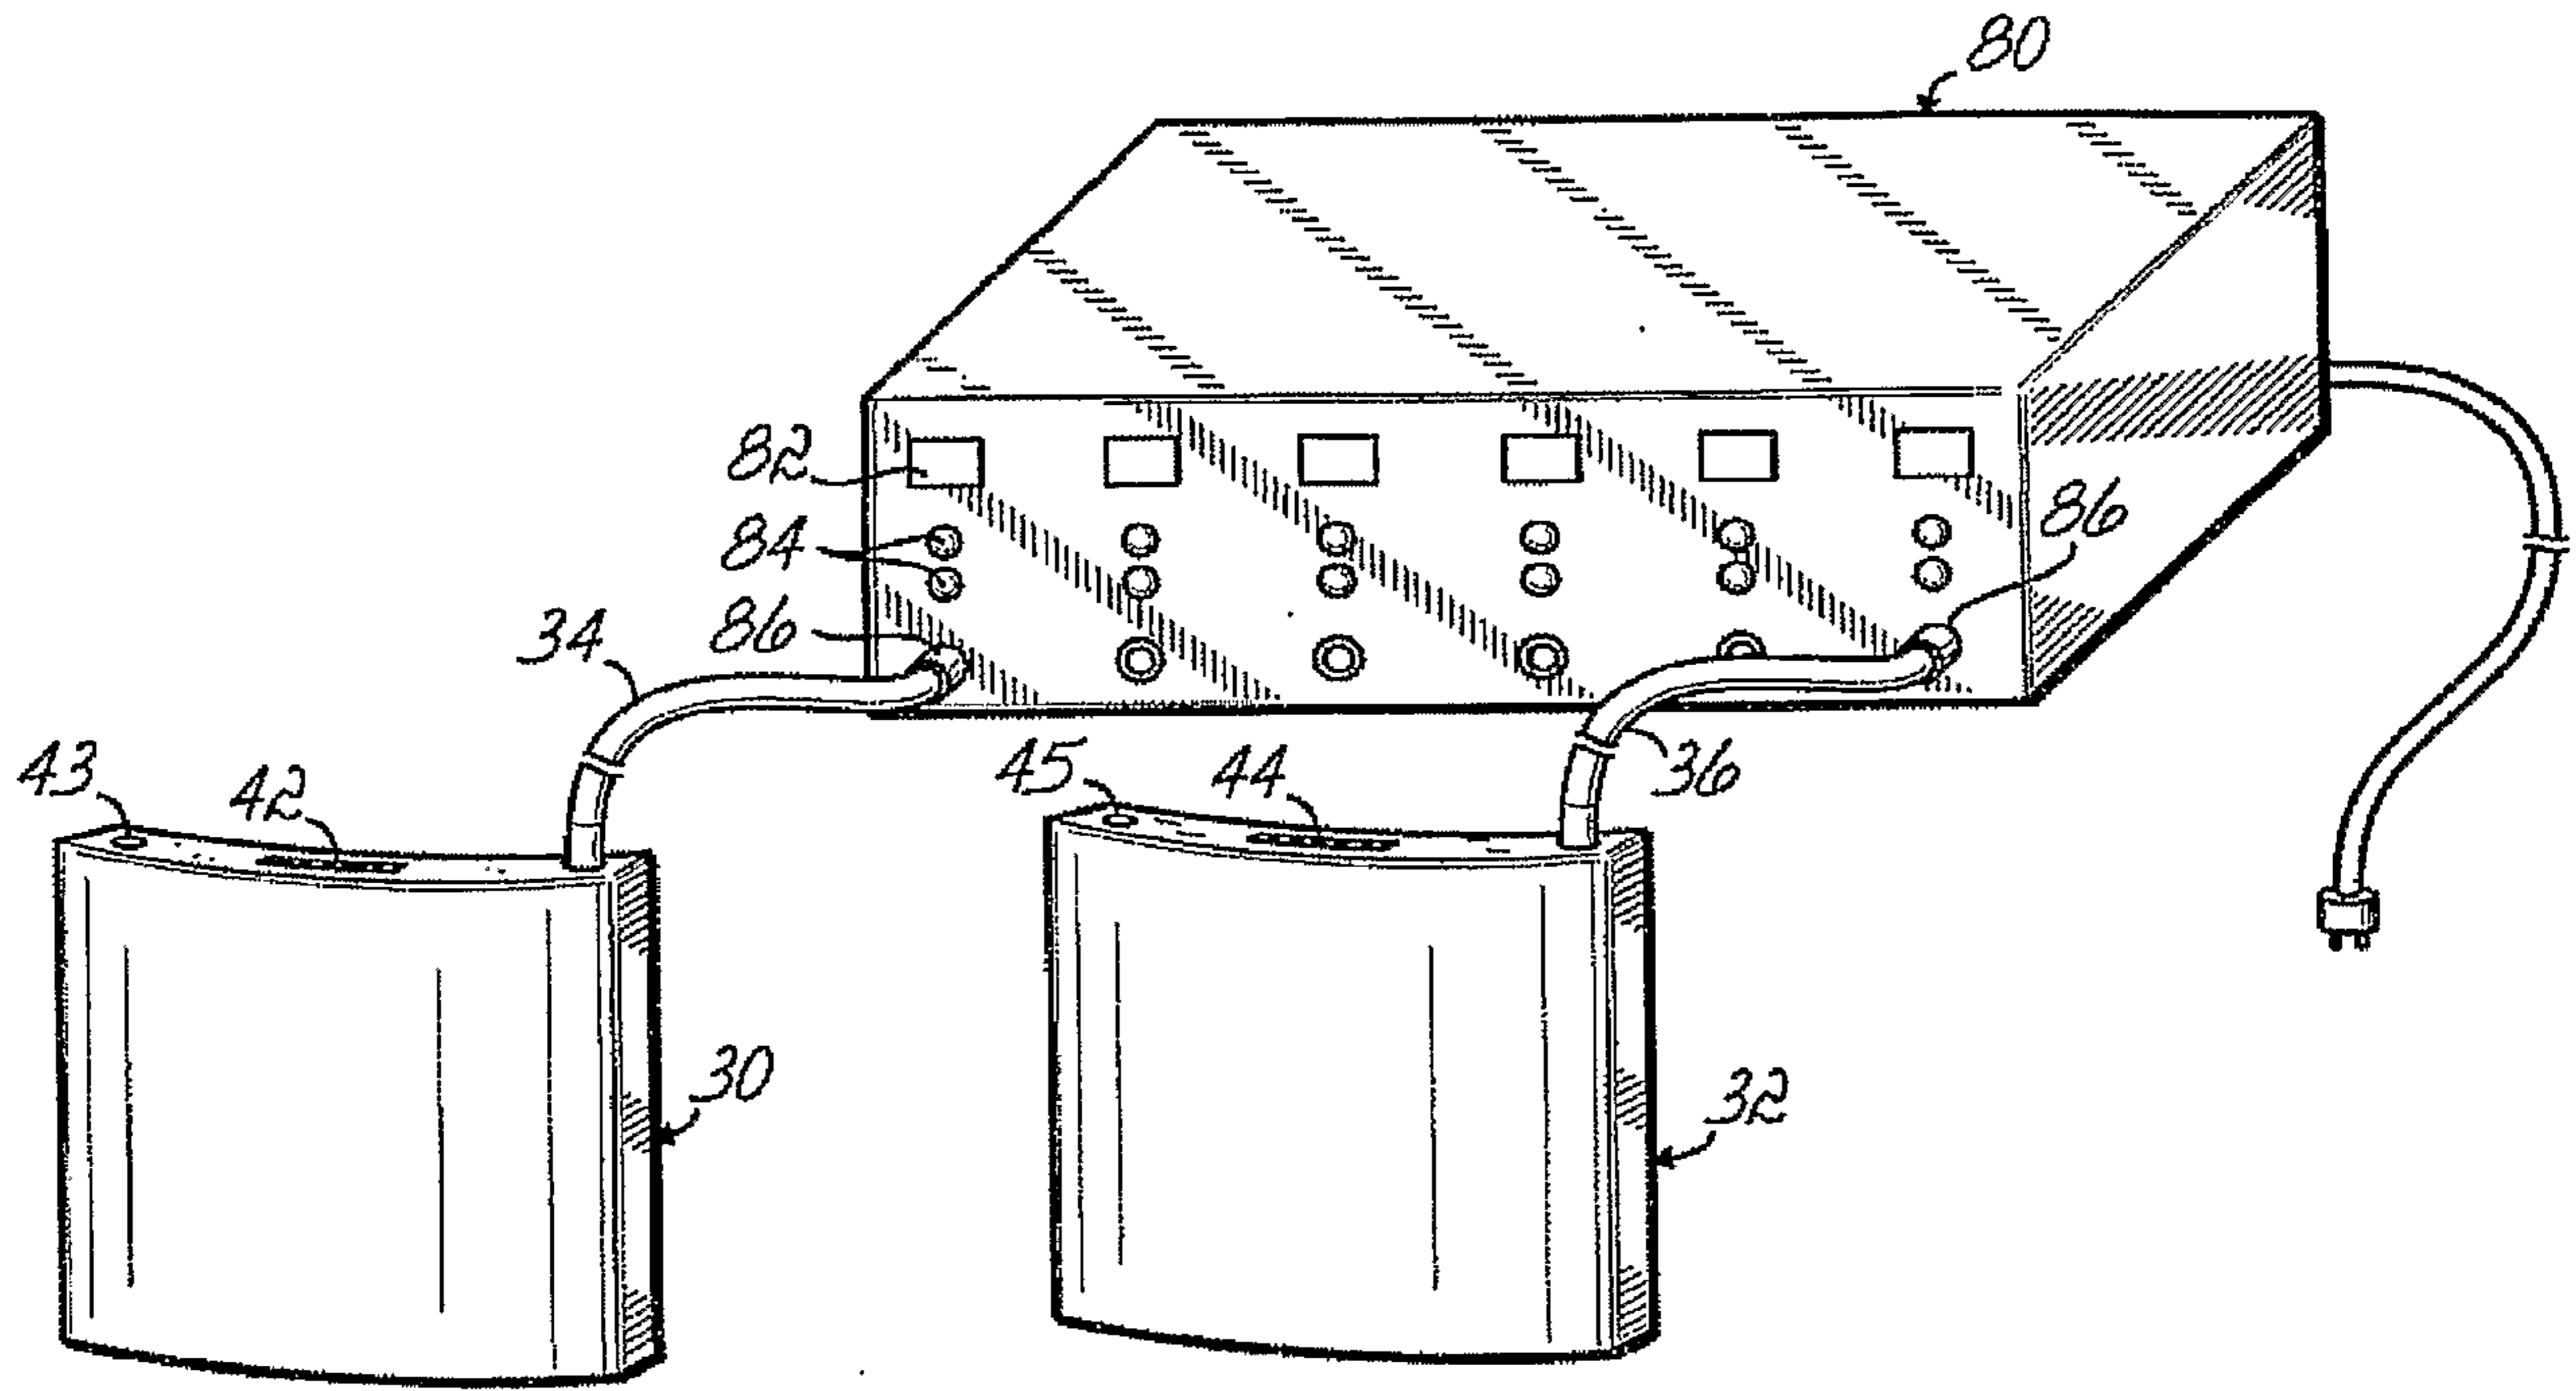


FIG. 4

