

(12) UK Patent Application (19) GB (11) 2 117 233 A

(21) Application No 8232103
(22) Date of filing 10 Nov 1982

(30) Priority data

(31) 8208815
8208848

(32) 25 Mar 1982
25 Mar 1982

(33) United Kingdom (GB)

(43) Application published
12 Oct 1983

(51) INT CL³
A61G 13/00

(52) Domestic classification
A4L 101 ACA
U1S 1738 A4L

(56) Documents cited
GBA 2025764
GB 1579226

GB 1531457

GB 1302229

GB 0620365

GB 1576238

GB 1484637

(58) Field of search
A4L
A4J
A5R

(71) Applicant
Howorth Air Engineering
Limited
(Great Britain),
Lorne Street, Farnworth,
Bolton BL4 7LZ


(72) Inventor
Frederick Hugh Howorth
(74) Agent and/or Address for
Service
Barlow Gillett and
Percival,
94 Market Street,
Manchester M1 1PJ

(54) Autopsy table

(57) Table top 11 is provided, at least along one side, with a number of sockets 15 connecting to a passageway 21 and into which entry spigots 16 are designed to fit. When a body 41 is being examined, extractor fan 30 can be switched on to draw air transversely across the table top 11, into the spigots 16 and the passageway 21 and through filters 28, 29 for exhaustion via a duct (31). This

pattern of air flow has been found to minimise the likelihood of an operator inhaling noxious substances or gases from the body, and spigots 16 do not impede access to the body by the operator.

Spigots 16 may be slideably adjustable in sockets 15 or provided in a range of lengths and/or curvatures and be interchangeable so that they can be arranged at optimal levels above the table top 11. Blanking units or covers 19 may block off sockets 15 where spigots 16 are not required.

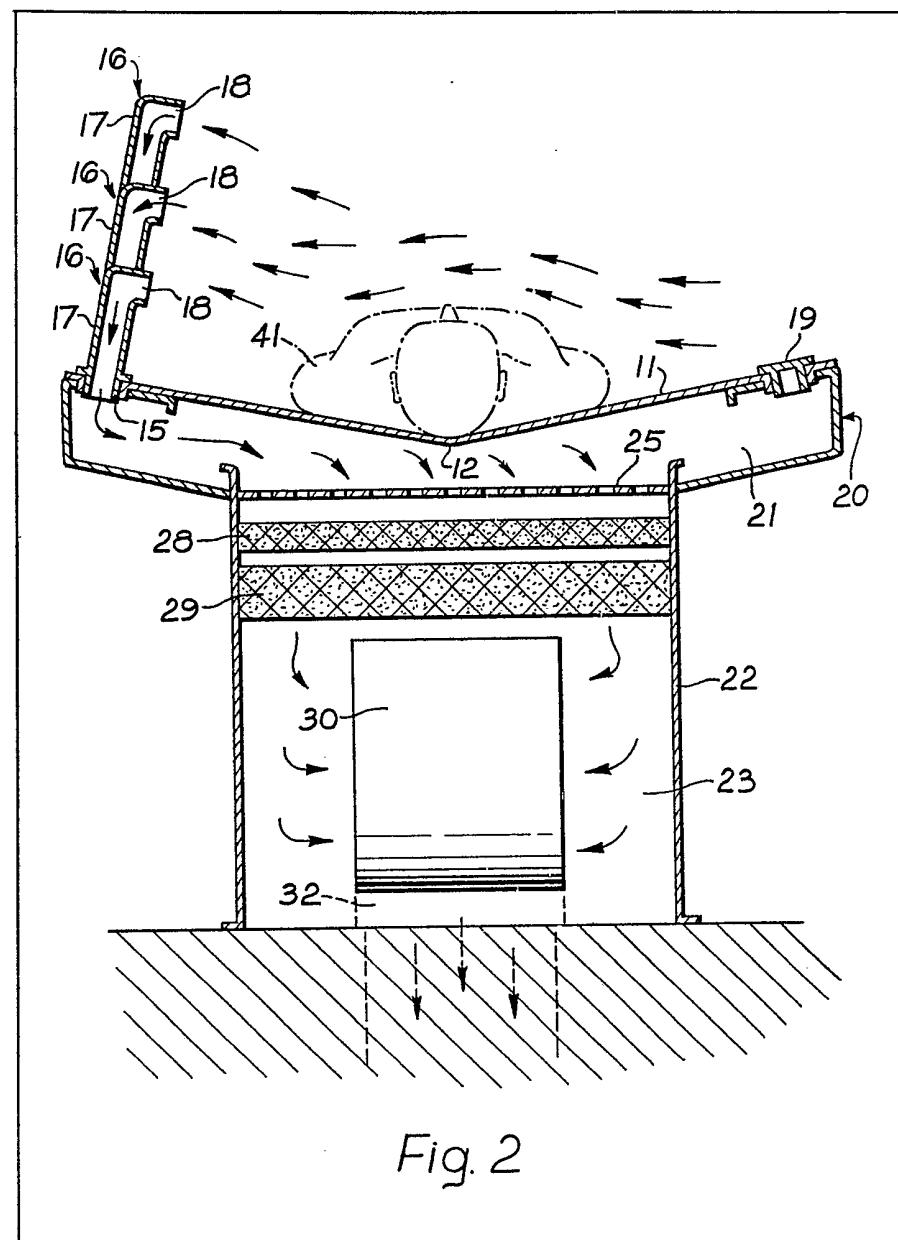

GB 2 117 233 A

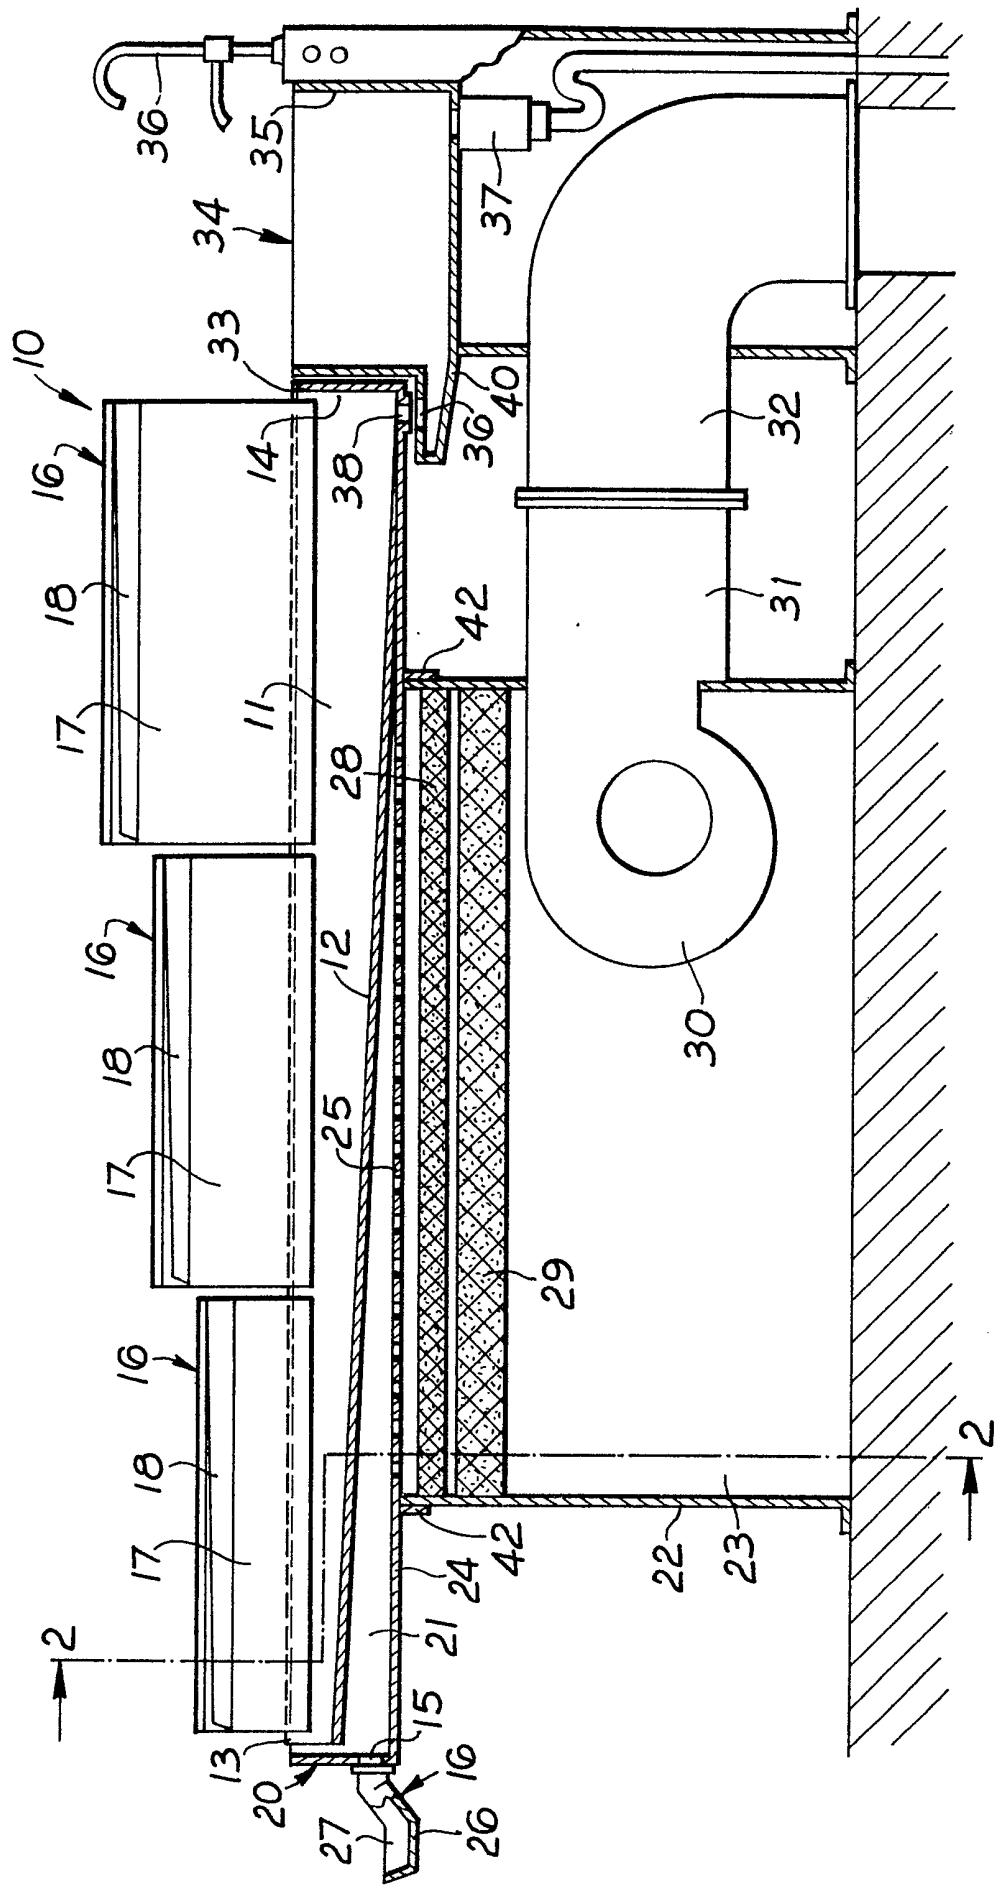


Fig. 1

2/5

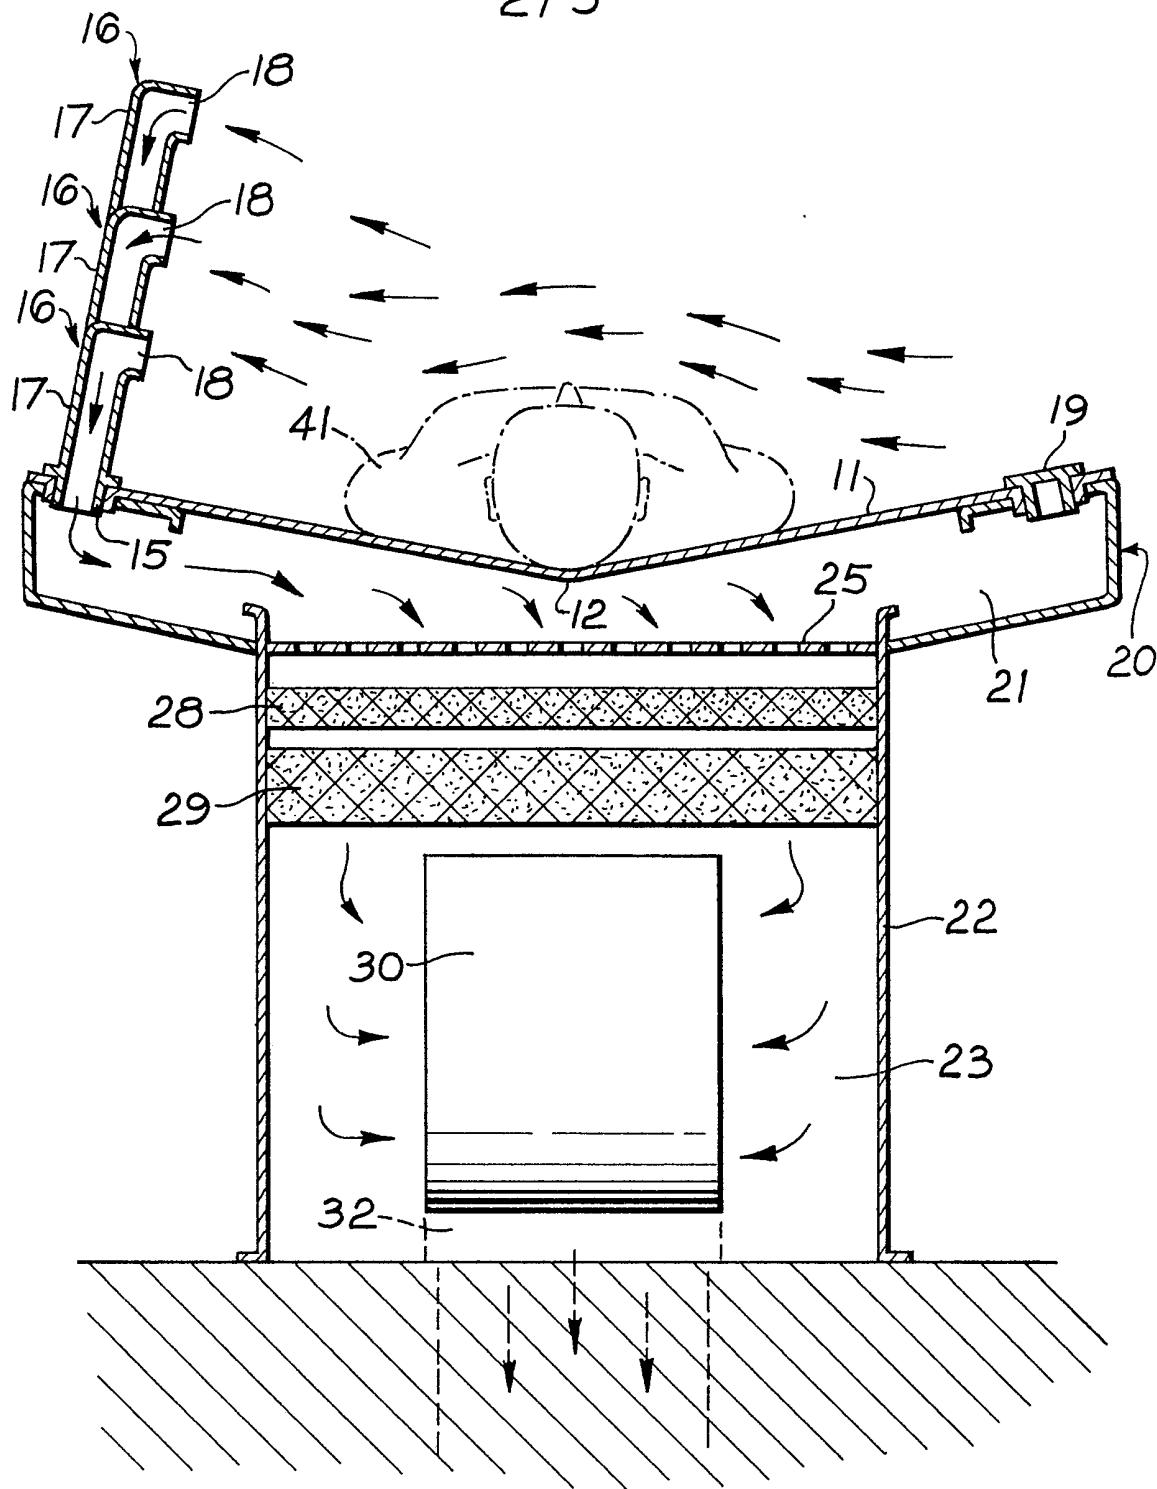


Fig. 2

3/5

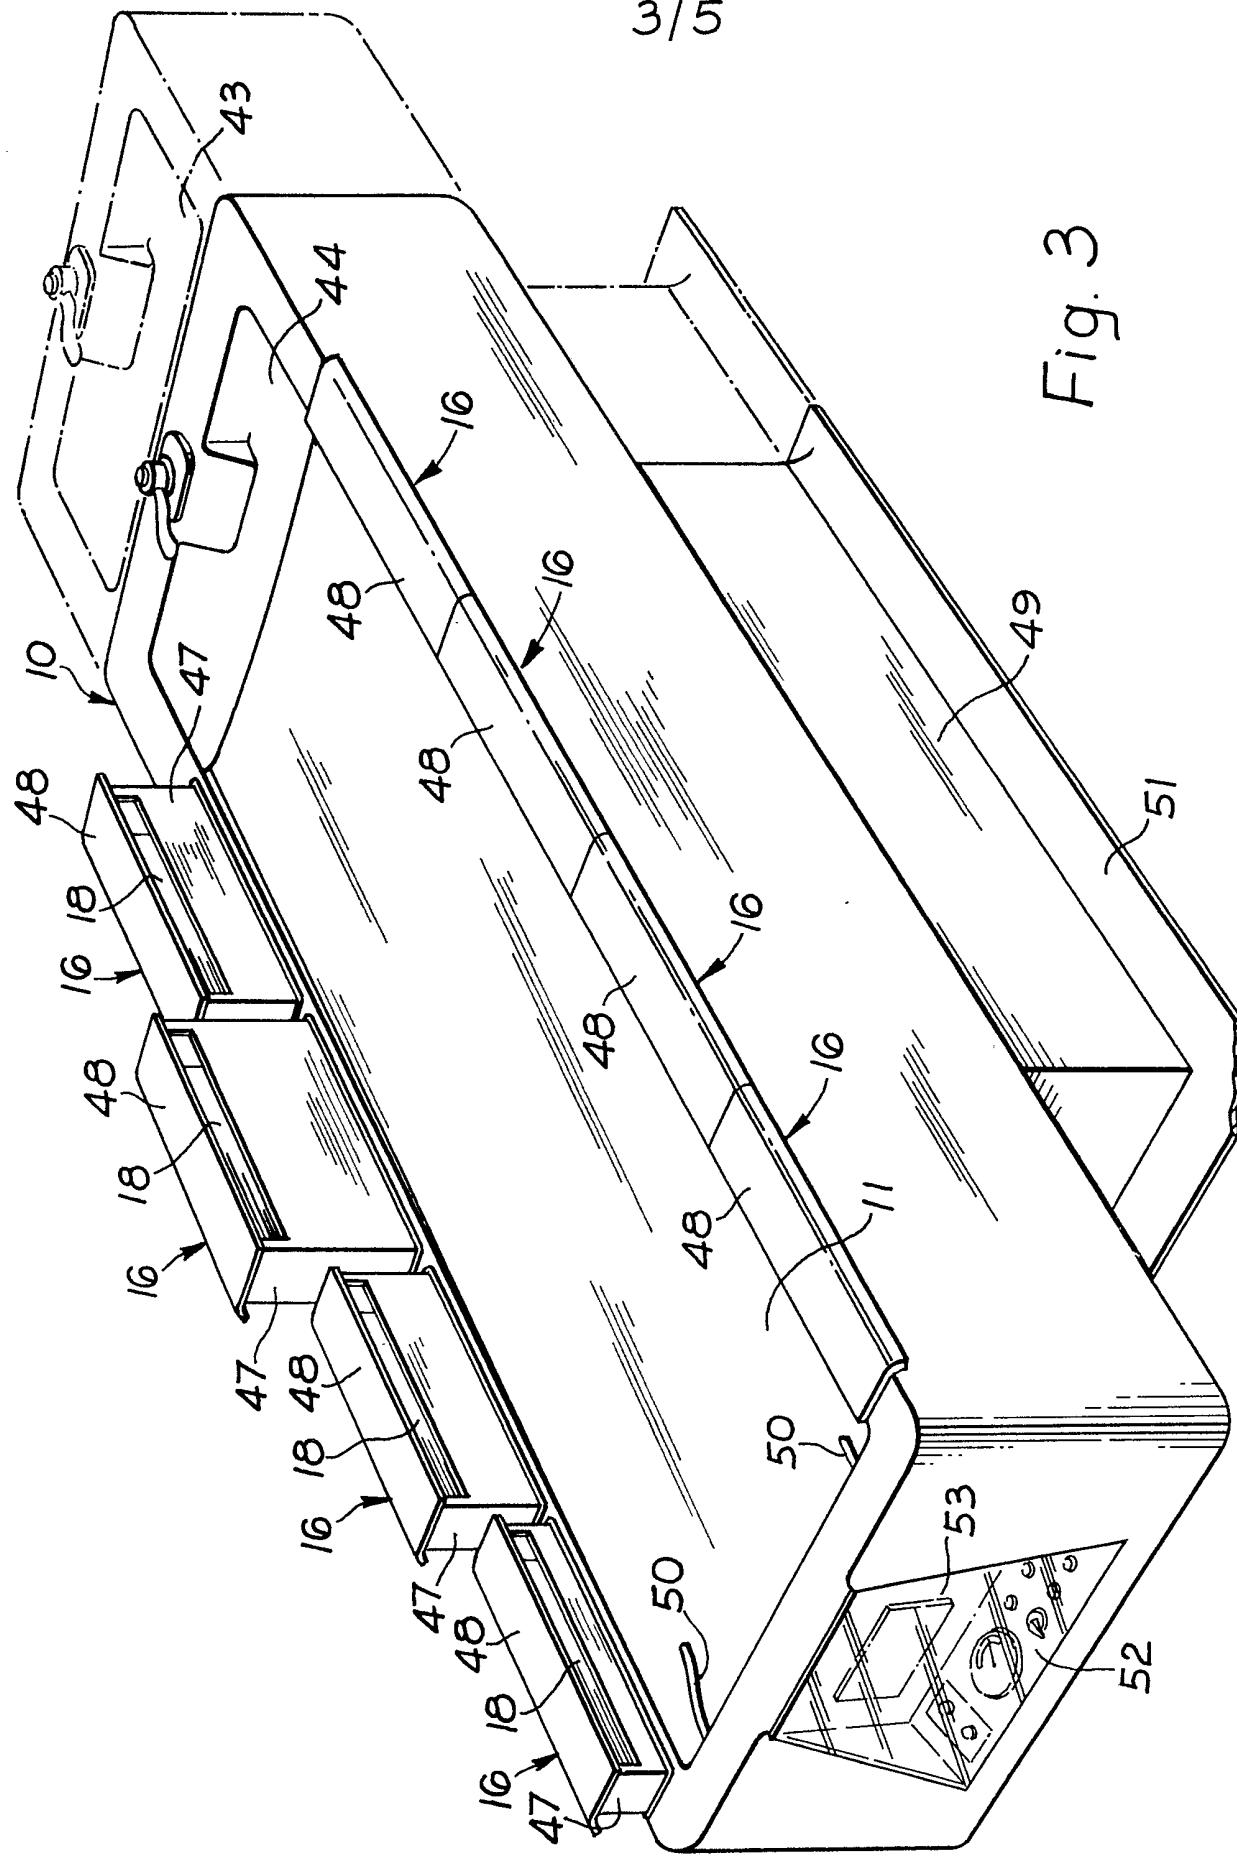


Fig. 3

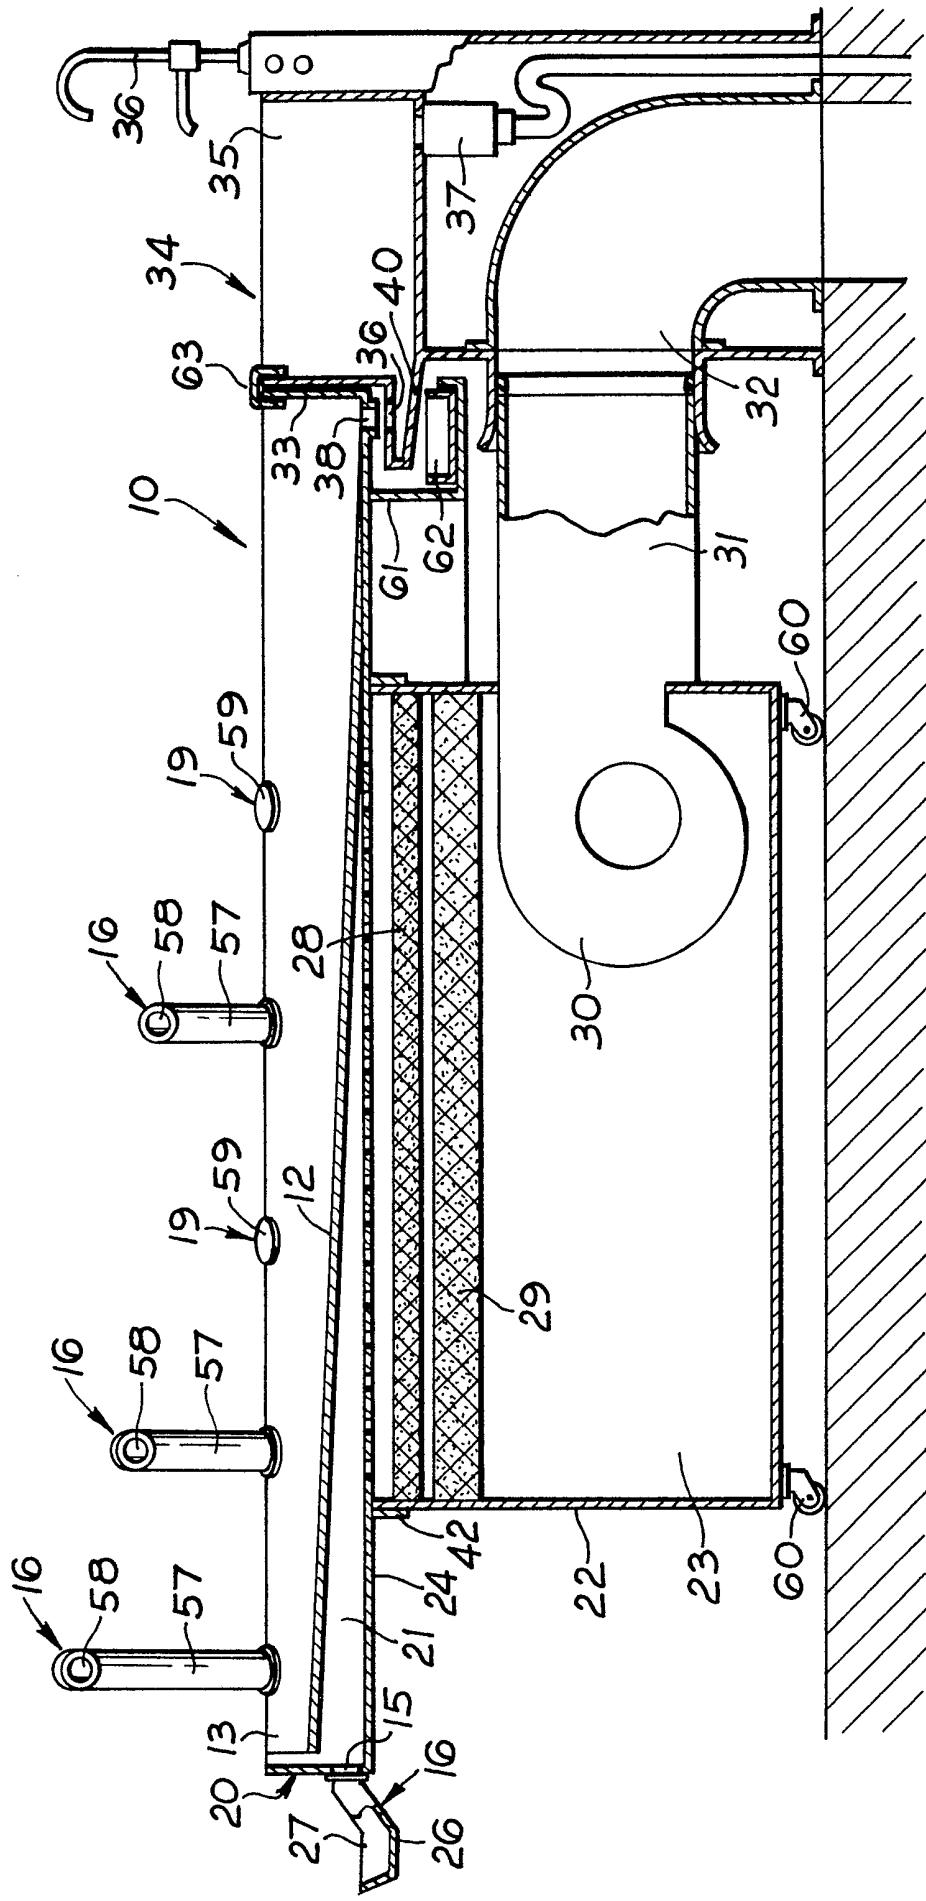


Fig. 4

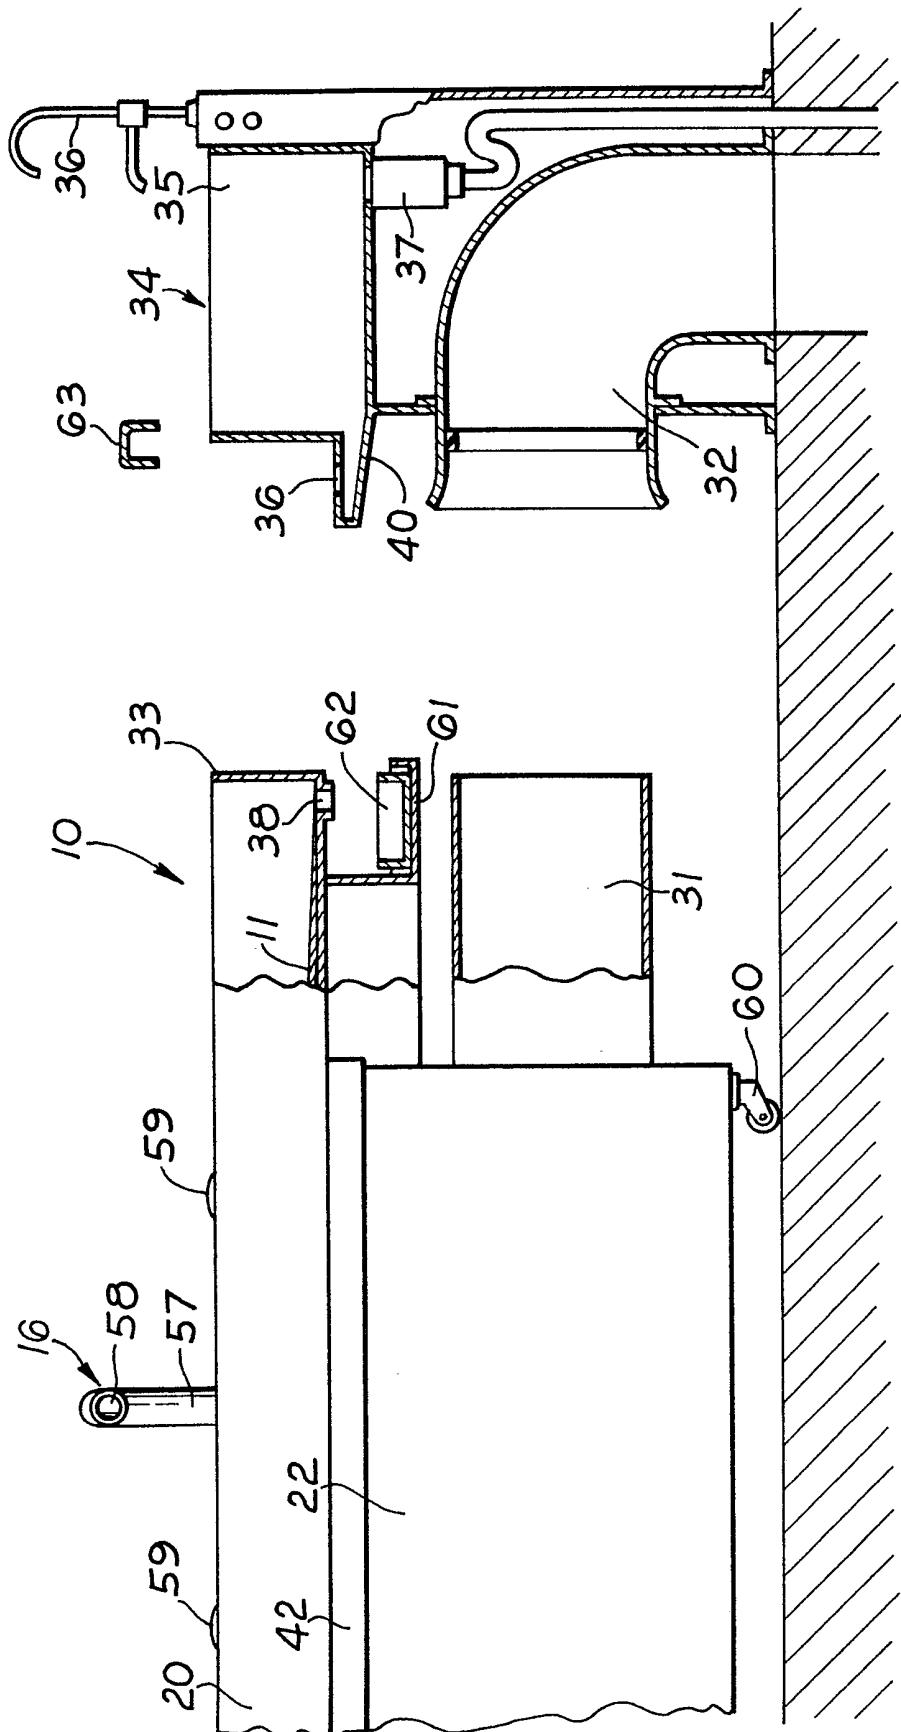


Fig. 5

SPECIFICATION
Autopsy table

This invention relates to an autopsy table, that is to say a table specifically adapted to

5 accommodate a body, or a tray on which a body is disposed, while a post-mortem examination is being carried out.

It is nowadays generally accepted that it is desirable to provide some form of air exhaust 10 system in conjunction with an autopsy table to entrain any noxious substances, including gases, emitted from the body away from an operator and thereby minimize his/her chances of infection and contamination.

15 Probably the most well known and long-established type of autopsy table hitherto used is a simple ceramic slab with no air exhaust system at all. However, more recently, a stainless steel table with a discontinuous or perforated surface has

20 been introduced. This table usually has air exhausted vertically downwards through the surface to a duct in the floor and subsequently via an exhaust fan and a filter out of the building to the external atmosphere.

25 Either of the aforesaid tables may be used in conjunction with an overhead air inlet canopy which supplies sterile or conditioned air in a downward direction to the table. However, after careful research it has been shown that such an air

30 flow arrangement causes undesirable turbulence around the face of an operator carrying out an examination on the table. This turbulence may, of course, have the deleterious effect of increasing the chance of the operator inhaling dangerous

35 bacteria or gases which are often emitted from the body during an autopsy.

Also, both the aforesaid types of autopsy table have generally been fixed in position in a post-mortem room. Although tables which include an 40 exhaust duct beneath the table top may be swung about a vertical axis provided by said duct, they cannot be removed from the duct because the duct is always internally contaminated with, for example, bacteria.

45 There is a need for an autopsy table which can be moved from one location to another, e.g. from one part of the post-mortem room to another to permit flexibility in the use of the table, especially, for example, when the table is to be used for the

50 examination of a body for teaching purposes. It would also be advantageous to be able to move an autopsy table away from associated components such as an exhaust duct and/or a sink for maintenance and repair of these components.

55 However, as mentioned, it would only be safe to remove a table from an associated exhaust duct if the duct was not internally contaminated.

The primary object of the present invention is to provide an autopsy table having an air exhaust 60 system which reduces to a minimum the likelihood of an operator inhaling noxious substances and gases emitted from a body being examined but which at the same time allows easy access to said body. Other aims are to provide a

65 table with a surface which is easier to clean than known perforated or discontinuous surfaces and a table which may safely be removed from its associated exhaust duct.

Pursuant hereto, the present invention provides

70 an autopsy table comprising a table top having a number of sockets adjacent at least one side, which sockets connect to a passageway, a number of entry spigots, at least one of which is fitted into a socket and an extractor operative to 75 draw air transversely across the surface of the table and through the entry spigot or spigots for exhaustion via the passageway.

The table top is preferably continuous and sloping to facilitate cleaning and drainage

80 respectively.

In a preferred practical embodiment of the autopsy table of the invention a number of elongate sockets are located adjacent each opposing longitudinal edge of the table top.

85 Optionally, there may also be a socket or a row of sockets at one or both ends of the table top.

It is envisaged that, within the scope of the invention, a plurality of entry spigots of differing heights and/or curvatures may be provided, which 90 spigots may be removed from the sockets and interchanged as desired. A plurality of removable caps, covers or blanking units should then be provided to block off any socket in which a spigot is not required to be fitted.

95 However, most advantageously a number of slidable entry spigots are provided such that the height of each extending above the relevant socket is adjustable and an overhanging top thereof blocks off the socket when the spigot is 100 withdrawn as far as possible into the passageway beneath the socket.

105 Filter means, preferably comprising a pre-filter and a HEPA (high frequency particulate air) filter, are advantageously located between the entry spigot or spigots and the extractor.

The extractor is conveniently an electrical fan which is preferably located in the exhaust passage of the table.

110 The table may optionally be movable by means of castors fitted adjacent each lower corner of the table structure.

Finally, the table may be connected to the sink of a service unit by an inverted channel section linking one end of the table to one side of the sink.

115 The invention will be described further, by way of example, with reference to the accompanying drawings in which:

120 Fig. 1 is a longitudinal cross-section of a first practical embodiment of the autopsy table of the invention together with a service unit;

Fig. 2 is a section along the line 2—2 shown in Fig. 1 to a larger scale and the position of a body to be examined is additionally indicated in broken lines;

125 Fig. 3 is a perspective view of a second practical embodiment of the autopsy table of the invention;

Fig. 4 is a longitudinal cross-section of a third practical embodiment of the autopsy table of the

invention together with a service unit; and

Fig. 5 is a partial cross-section of the embodiment of Fig. 4 showing the table removed from the service unit.

- 5 As shown in Figs. 1 and 2, a first embodiment of the autopsy table 10 of the invention comprises a substantially rectangular stainless steel table top 11 which is angled along its longitudinal axis 12 and which also slopes downwards along said axis 12 from one end 13 to the opposing end 14. A row of three elongate sockets 15 are located adjacent each longitudinal side of the table top 11. As shown in Fig. 1, a main entry spigots 16 comprising an angled duct 17 of substantially rectangular cross-section extends upwardly from each of the sockets 15 at one side of the table top 11. Angled ducts 17 of different heights are provided and are positioned as required, as will be explained later. Each duct 17 has an upper opening 18 which faces inwardly of the table 10. A respective cover or blanking unit 19 in the form of an inverted channel section is fitted into each of the three sockets 15 at the other side of the table 11 where entry spigots 16 are not required.
- 20 The sloping table top 11 is superimposed upon a tray 20 thus forming an intervening passageway 21 which tapers along its central axis from the end 13 to the end 14 of the table top 11. The tray 20 is supported upon a housing 22 enclosing a cavity 23, a rim 42 projecting downwardly from the base 24 of the tray 20 fitting neatly around the upper margins of the walls of the housing 22. The base 24 of the tray 20 is perforated in the region 25 which is bounded by the rim 42 and directly 30 overlies the cavity 23. The table top 11 and the tray 20 may be removed from the housing 22 to allow access to filters 28, 29 located in the cavity 23, e.g. for removal and replacement of said filters.
- 35 An additional entry spigot 16 in the form of an angled duct 26 having an upwardly facing opening 27 is located in and extends substantially laterally from a socket 15 in the side of the tray 20 adjacent the upper end 13 of the plate 11, as 40 shown in Fig. 1.
- 45 Filter means in the form of a prefilter 28 arranged above a HEPA filter 29 are located within the cavity 23. Both these filters 28 and 29 extend the full length and breadth of the cavity 23 a short 50 distance beneath and substantially parallel to the base 24 of the tray 20. An extractor fan 30 is located beneath the filters 28 and 29 towards one end of the cavity 23. A duct 31 leads from the fan 30, through a wall of the housing 22 to an exhaust 55 duct 32, terminal flanges of ducts 31, 32 being clamped together.
- 60 As shown in Fig. 1, the end 33 of the tray 20 abuts a service unit 34 including a sink 35, provided with hot and cold taps 36 and a drain 37.
- 65 Beneath the sink 35 is located the aforementioned exhaust duct 32, which is firmly attached to the duct 31. At the central, lower extremity of the end 14 of the table top 11, the table top 11 adjoins the base 24 of the tray 20 and an outlet aperture 38 is provided. A corresponding aperture 39 is located

in a sink extension 40 so that any substance e.g. waste fluids draining through the aperture 38 will pass into the sink 35 and thus to the drain 37.

- 70 When an autopsy or post-mortem examination of a body 41 is to be carried out upon the autopsy table 10, the body 41 is firstly placed centrally upon the table top 11, as indicated in Fig. 2 with the head at the upper end 13. Alternatively, a tray accommodating the body, on which the body may 75 have been kept in refrigerated storage, may be placed on the table top 11. The ducts 17, preferably of three different heights and the covers or blanking units 19 are fitted into or rearranged from one to the other of sockets 15 to give the 80 desired arrangement of entry spigots 16 at the most advantageous levels above the table top 11. In the majority of instances it will probably be most convenient to have only covers or blanking units 19 located in the sockets 15 along one side 85 of the table top 11 so as to allow an operator complete access to the body 41 from that side. Location of the ducts 17 will depend on which part of the body 41 is to be examined and how high this part is above the table top 11. For 90 example, if a thoracic examination is to be carried out, covers or blanking units 19 will probably be fitted into the sockets 15 along one side of the table top 11 as already mentioned and also into one socket 15 along the other side of the table top 95 11 adjacent the legs of the body 41. Respective ducts 17 will be fitted into the remaining two sockets 15 adjacent the thorax and adjoining regions, the height of the ducts 17 being selected so that their openings 18 are approximately level 100 with, or slightly above the upper surface of the thorax.
- The aforesaid arrangement of entry spigots 16 has been found to be the most favourable to achieve, when the fan is switched on, a transverse 105 flow of air across the part of the body being examined, and away from the operator so that the risk of the latter breathing-in noxious substances such as bacteria or gases is minimised.
- 110 The angled duct 26 as shown in Fig. 1 is attached at the end of the table 10 adjacent the head of the body 41 whenever the skull is to be sawn so that bone dust may be exhausted.
- 115 Before the examination of the body 41 commences, the fan 30 is switched on and it should remain on throughout the course of the examination. The action of the fan 30 is to draw air transversely across the body 41 into the openings 18 of the ducts 17 and thus into the passageway 21, through the perforations in the 120 base 24 of the tray 20 and through the prefilter 28 and HEPA filter 29. After passing through the fan 30, the air is forced into the duct 31 and, via exhaust duct 32, to the outside atmosphere. The filters 28, 29 retain any particulate matter, such as 125 bacteria, so that the ducts 31, 32 remain uncontaminated.
- 130 Any waste fluids released from the body 41 during the examination together with any irrigating fluids applied will drain down towards the end 14 of the table top 11 and flow through

the apertures 38 and 39 into the sink 35 and thus out of drain 37.

The volume of air exhausted via the spigots 16 is adjustable by closing off exhaust ports, i.e.

5 sockets 15, when they are not required and/or by adjusting the speed of the fan 30. Extensive smoke and air pattern texts indicate that autopsy tables of the above-described type are microbiologically safer and also more economical

10 in terms of heat energy lost in air exhaustion than any table hitherto known.

After purging with formaldehyde, the above-described table may be disconnected from its service unit 34 for repair or replacement of the 15 filters 28, 29 or the fan 30 by unclamping the duct 31 from the duct 32 and pushing the table 10 away from said unit 34. However, the aforesaid embodiment of the autopsy table of the invention is not especially adapted for movement away from

20 its service unit 34.

Fig. 3 illustrates a second somewhat modified embodiment of the autopsy table of the invention in which there are four sockets 15 disposed along each side of the table 10 and an exhaust spigot 16 25 fitted in each socket 15. In this case, each spigot 16 comprises a substantially upright fitment 47 of rectangular cross-section having an overhanging top 48 and an elongate air entry aperture 18 extending along one side immediately beneath

30 said top 48. The fitments 47 are all of equal height and are fitted into respective sockets 15 such that the apertures 18 face towards the table top 11. Also, the fitments 47 are slidably adjustable up and down relative to the sockets 15 with a

35 number of click stops so that the height of the apertures 18 above the table top can be varied as required. As shown at one side of the table 10 in Fig. 3, when the fitments 47 are fully pushed down, their tops 48 serve to completely block off 40 the sockets 15 so that separate blanking units or covers are not required. However, they may still be used, when convenient, in certain circumstances e.g. if the same sockets rarely require spigots with entry apertures.

45 In this embodiment, the table top 11 is not angled at its mid-line and there is an integral sink 44 at the foot end of the table. Optionally, there may be a second sink 43 and this possibility is indicated in dot-dash lines in Fig. 3.

50 At the head end of the table 10 there are two small flexible pipes 50 which are used to trickle water along the sides of the table top 11 or another tray placed thereon to wash the work surface both during the autopsy and at other times

55 as required.

The support housing 49 for the table 10 is firmly affixed to the floor by a waterproof covering 51 and exhaust air and other gases are vented downwardly from the table 10 via ducts within the

60 housing 49. A control panel 52 covered by a rigid transparent hinged lid 53 is located at the head end of the table 10 and may include a control knob for adjustment of fan speed, and also a gauge indicating when the filters require to be

65 changed. In other embodiments, such a control

panel may, of course, be located at some other position on the table, or remote from the table, e.g. on an adjacent wall.

Apart from the foregoing, this embodiment of 70 the autopsy table of the invention is of similar construction to the first embodiment and it is used in a similar manner.

A third practical embodiment of the autopsy table of the invention is illustrated in Figs. 4 and 5.

75 In this case, five sockets 15 are arranged at equidistant spacings along each longitudinal side of the table 10. The spigots 16 are in the form of interchangeable angled tubes 57 having openings 58 and covers or blanking units 19 in the form of 80 disc-like caps 59, are provided.

The remaining construction of the autopsy table 10 and the adjoining service unit 34 and the use of the table are very similar to the description given for the first embodiment hereinbefore

85 described and the same reference numerals as Figs. 1 and 2 have been used for corresponding parts. However, this third embodiment is specifically adapted for mobility by provision of castors 60 on the base of the housing 22. Also, an

90 L-profiled bracket 61 is suspended from the tray 20 beneath the lower end 14 of the table top 11 and a drip bucket 62 is located on said bracket 61 directly beneath the aperture 38 to catch any fluid draining from the table 10 whenever said table is

95 moved away from the service unit 34. A channel section 63 is additionally provided to link the end 33 of the tray 20 to the side of the sink 35 as and when required and the exhaust ducts 31, 32 are formed so that one can easily slot into the other or 100 be disengaged therefrom.

It is feasible to construct the autopsy table of the invention so as to be removable from an adjacent service unit and disconnectable from the exhaust duct because the provision of filters 105 integral with the table itself means that the disconnected ends of the exhaust duct are substantially clean. In earlier tables where filters were not integral, the exhaust ducts were contaminated.

110 Although in further embodiments of the autopsy table of the invention exhaust ports permanently fixed along one or both sides of the table top may be provided, removable entry spigots, as described, are preferable firstly for

115 reasons of access as the operator can decide which side to work from and secondly because only the area of the body being examined needs be exhausted so that volume of air to be exhausted and the energy required to do so may

120 be minimized. This latter point is relevant even when the entire body or trunk is being examined due to the large variation in size of bodies.

Furthermore, in certain embodiments non-adjustable entry spigots of only one length may be 125 provided, so that air is exhausted at an average or compromise height for all bodies. Again, this is not as favourable as providing adjustable spigots or two, three or more different lengths of removable, interchangeable entry spigots so that differences 130 in the size of bodies may be taken into account

and exhaustion at an optimal level achieved.

It should be understood that the foregoing description is illustrative and not limitative of the scope of the invention and variations may be made thereto. In particular a sub-table may be affixed at any point on the autopsy table of the invention, for example for accommodating pieces of equipment, and entry spigots may be appropriately provided in the sub-table or adjacent thereto. Also the table top, the sockets and the entry spigots may be of different shapes and sizes to those described above and a water eliminator may be provided beneath the table top, e.g. adjacent the filters. Furthermore an autopsy table comprising simply a ceramic slab, as described at the beginning of the specification, may be adapted according to the invention by the installation of one or more entry spigots adjacent the slab and an extractor to draw air transversely of said slab into said spigot or spigots.

CLAIMS

1. An autopsy table comprising a table top having a number of sockets adjacent at least one side, which sockets connect to a passageway, a number of entry spigots, at least one of which is fitted into a socket and an extractor operative to draw air transversely across the surface of the table top and through the entry spigot or spigots for exhaustion via the passageway.
2. An autopsy table as claimed in claim 1 wherein the table top is continuous and sloping.
3. An autopsy table as claimed in claim 1 or 2

wherein the table top is substantially rectangular and a number of elongate sockets are located adjacent each opposing longitudinal edge thereof.

4. An autopsy table as claimed in claim 1, 2 or 3 wherein the entry spigots are slidably adjustable relative to the sockets.
5. An autopsy table as claimed in claim 5
- 40 wherein each entry spigot is provided with an overhanging top which serves to block off the relevant socket when the spigot is retracted as far as possible through the socket.
6. An autopsy table as claimed in claim 1, 2 or 45 3 wherein a plurality of entry spigots of differing heights and/or curvatures are provided, which spigots may be removed from the sockets and interchanged as desired.
7. An autopsy table as claimed in any preceding 50 claim wherein a plurality of caps, covers or blanking units are provided to block off any socket in which a spigot is not required to be fitted.
8. An autopsy table as claimed in any preceding 55 claim wherein filter means are located between the entry spigot or spigots and the extractor.
9. An autopsy table as claimed in any preceding claim wherein the extractor is located in the exhaust passageway of the table.
10. An autopsy table as claimed in any 60 preceding claim wherein the table is movable by means of castors fitted to the base of the table structure.
11. An autopsy table substantially as 65 hereinbefore described with reference to and as illustrated in Figs. 1 and 2, or Fig. 3, or Figs. 4 and 5 of the accompanying drawings.