



US0D1079005S

(12) **United States Design Patent**  
**Kersen et al.**

(10) **Patent No.:** **US D1,079,005 S**

(45) **Date of Patent:** **\*\* Jun. 10, 2025**

- (54) **DENTAL X-RAY SENSOR COVER**
- (71) Applicants: **Lawrence Kersen**, Boonton, NJ (US);  
**Marty Vogel**, Flushing, NY (US)
- (72) Inventors: **Lawrence Kersen**, Boonton, NJ (US);  
**Marty Vogel**, Flushing, NY (US)
- (73) Assignee: **Poly-Gel L.L.C.**, Easton, PA (US)
- (\*\*) Term: **15 Years**
- (21) Appl. No.: **29/814,946**
- (22) Filed: **Nov. 10, 2021**
- (51) **LOC (15) Cl.** ..... **24-01**
- (52) **U.S. Cl.**  
USPC ..... **D24/158**
- (58) **Field of Classification Search**  
USPC ..... D24/186, 187, 165, 166, 167, 168, 200,  
D24/231, 185, 170, 160, 209, 210, 161,  
D24/158, 224  
CPC ..... G03B 42/042; A61B 6/14; A61B 6/145  
See application file for complete search history.

- 6,190,042 B1 \* 2/2001 Dove ..... A61B 6/4435  
378/170
  - 6,343,875 B1 \* 2/2002 Eppinger ..... A61B 6/4435  
378/170
  - D579,572 S \* 10/2008 Wittenbrock ..... D24/209
  - D601,444 S \* 10/2009 Jones ..... D24/231
  - D608,900 S \* 1/2010 Giraud ..... D24/231
- (Continued)

**OTHER PUBLICATIONS**

Valtech Silicon Covers, [site visited Jan. 31, 2025]. Available from Internet. URL: [https://midwestdental.com/categories/supplies/x-ray-products/digital-sensor-accessories/\\_item/vatech-silicon-covers-size-15](https://midwestdental.com/categories/supplies/x-ray-products/digital-sensor-accessories/_item/vatech-silicon-covers-size-15) (Year: 2025).\*

*Primary Examiner* — T Chase Nelson  
*Assistant Examiner* — Kelly L Gross  
(74) *Attorney, Agent, or Firm* — Edwin D. Schindler

(57) **CLAIM**

The ornamental design for a dental X-ray sensor cover, as shown and described.

**DESCRIPTION**


FIG. 1 is a front top isometric prospective view of the present design for a dental X-ray sensor cover; FIG. 2 is a front back view of the dental X-ray sensor cover of the design of FIG. 1; FIG. 3 is a cross-sectional view of the dental X-ray sensor cover of the design of FIG. 1 taken along the 3-3 line of FIG. 2; FIG. 4 is a right bottom view of the dental X-ray sensor cover of the design of FIG. 1; and, FIG. 5 is a perspective view showing the dental X-ray sensor cover in a state of use enclosing a dental X-ray sensor. The even length broken lines illustrate environment and form no part of the claimed design. The dot-dash broken lines illustrate the direction of the cross-sectional view and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 1,608,269 A \* 11/1926 Freund ..... G03B 42/042  
378/170
- 3,092,721 A \* 6/1963 Medwedeff ..... A61B 6/4435  
378/170
- 3,831,034 A \* 8/1974 Ota ..... A61B 6/51  
378/197
- 4,166,220 A \* 8/1979 Stutts ..... A61B 6/51  
976/DIG. 428
- 4,554,676 A \* 11/1985 Maldonado ..... G03B 42/042  
378/170
- D295,784 S \* 5/1988 Inoue ..... D24/168
- 4,815,117 A \* 3/1989 Waldo ..... G03B 42/042  
378/170
- 6,033,111 A \* 3/2000 Winters ..... G03B 42/042  
378/170

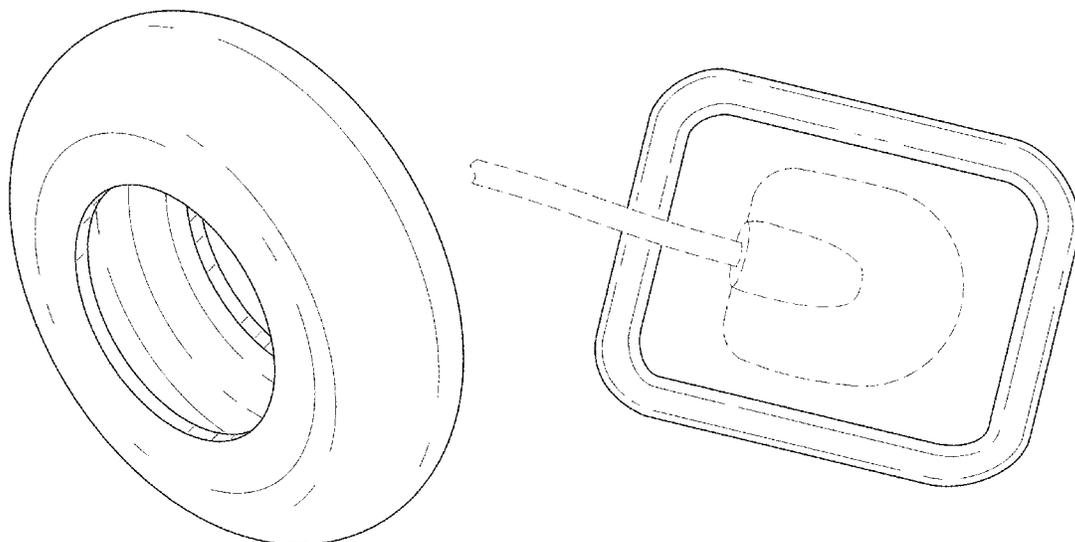



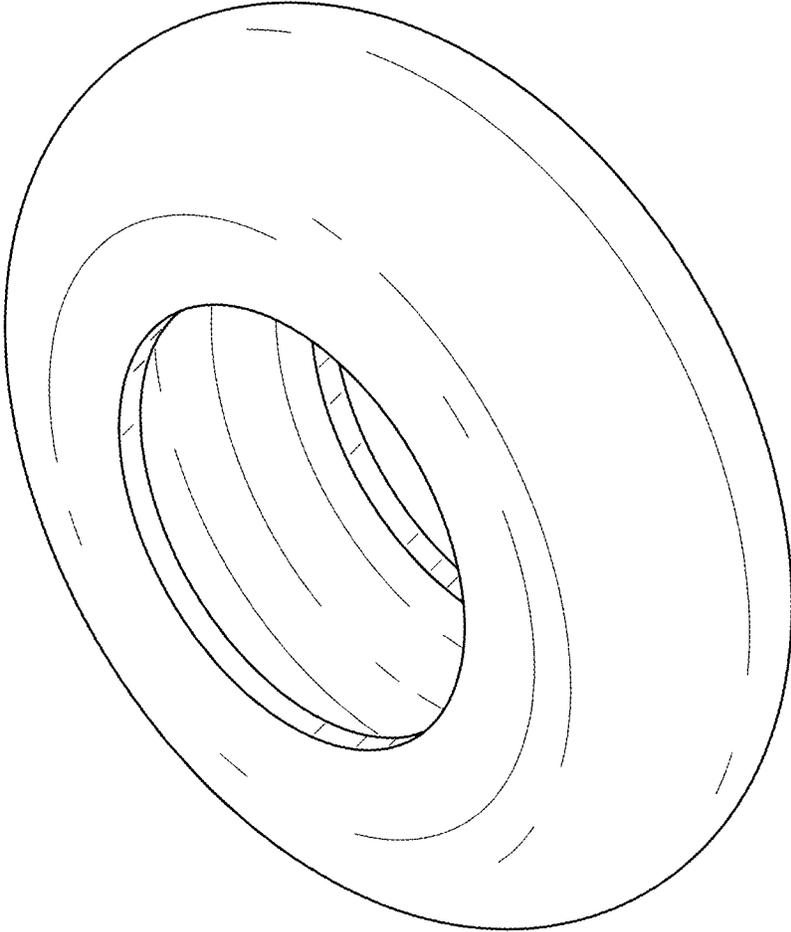


FIG. 1

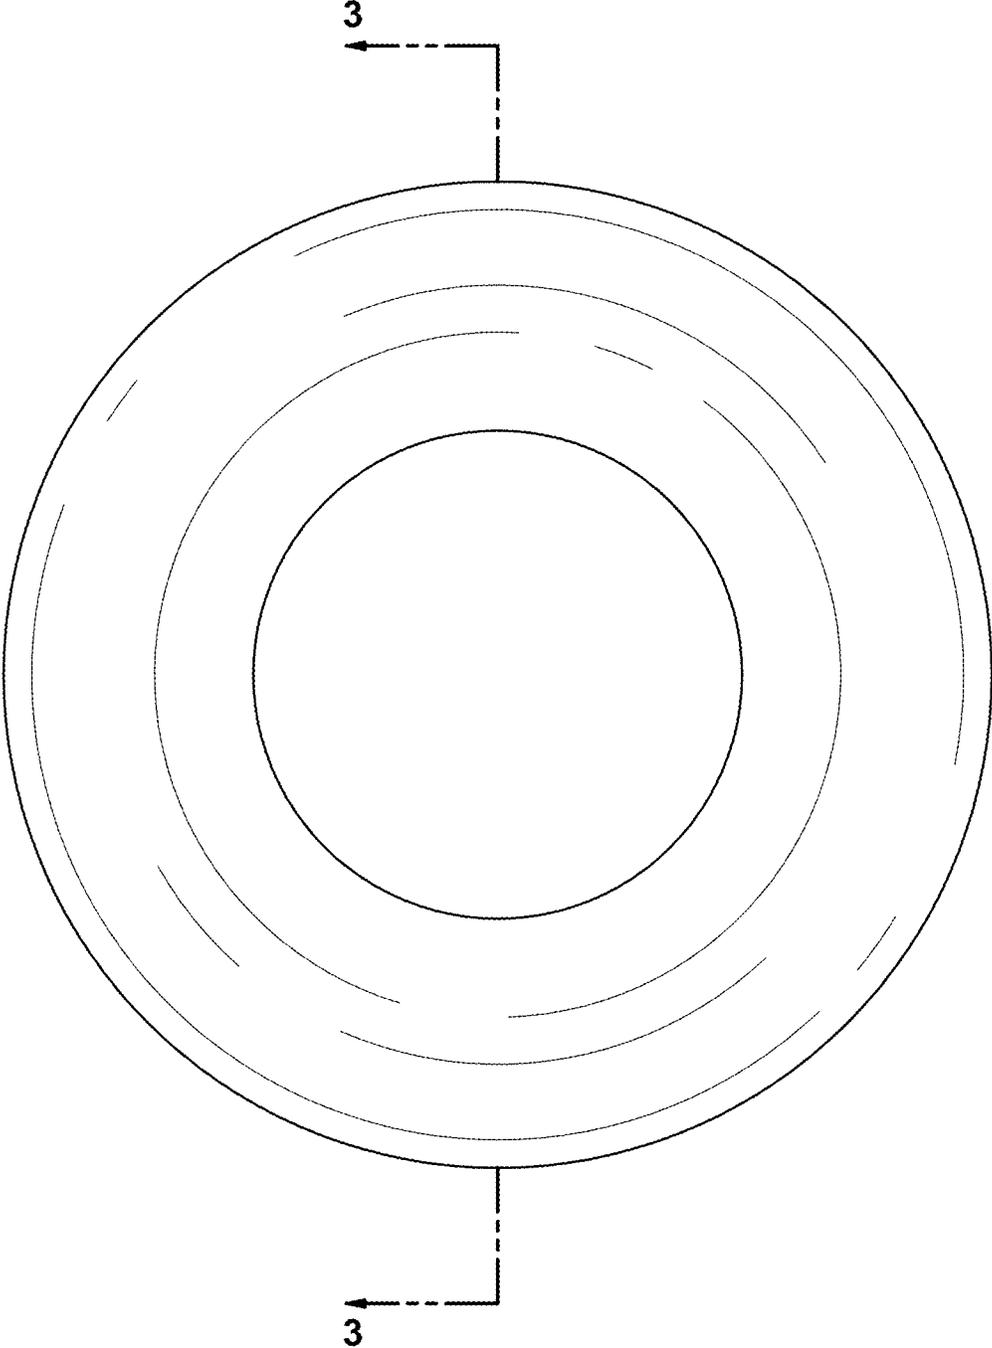


FIG. 2

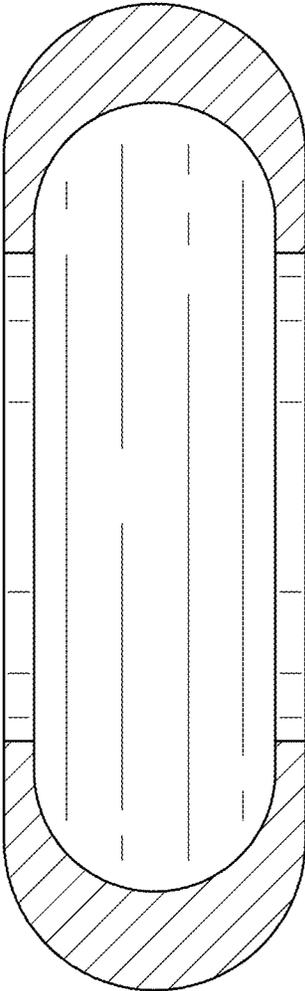


FIG. 3

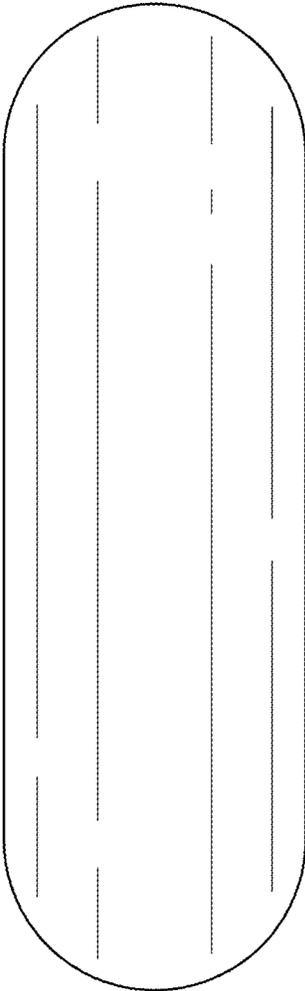


FIG. 4

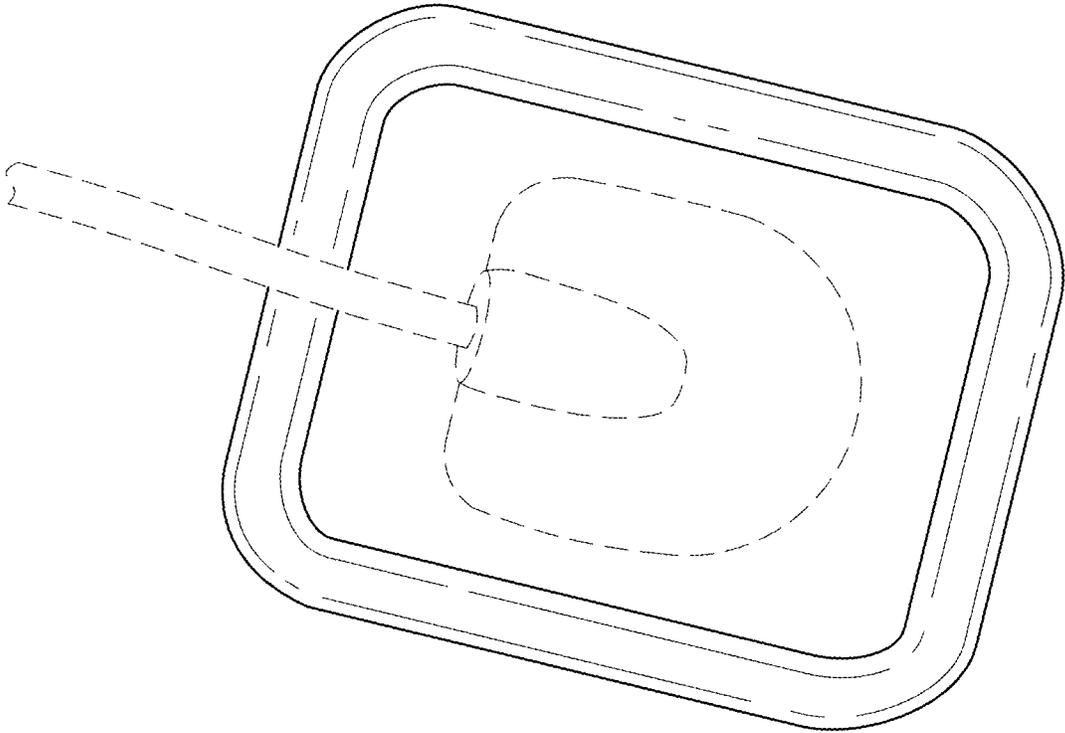


FIG. 5