



US00D760903S

(12) **United States Design Patent**  
**Lin et al.**

(10) **Patent No.:** **US D760,903 S**

(45) **Date of Patent:** **\*\* Jul. 5, 2016**

(54) **APPARATUS FOR MEASURING  
PHYSIOLOGICAL SIGNAL**

(71) Applicants: **Kinpo Electronics, Inc.**, New Taipei  
(TW); **Cal-Comp Electronics &  
Communications Company Limited**,  
New Taipei (TW)

(72) Inventors: **Chi-Hsueh Lin**, New Taipei (TW);  
**Wei-Jen Lo**, New Taipei (TW); **Chih-Ta  
Huang**, New Taipei (TW)

(73) Assignees: **Kinpo Electronics, Inc.**, New Taipei  
(TW); **Cal-Comp Electronics &  
Communications Company Limited**,  
New Taipei (TW)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/516,184**

(22) Filed: **Jan. 30, 2015**

(30) **Foreign Application Priority Data**

Nov. 11, 2014 (EP) ..... 002575415

(51) **LOC (10) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/165**

(58) **Field of Classification Search**  
USPC ..... D24/164-168, 186, 187; D10/75, 70,  
D10/78

CPC .... A61B 5/0402; A61B 5/0404; A61B 5/021;  
A61B 5/024; A61B 5/02438; A61B 5/681;  
A61B 2560/0205; A61B 2560/0462

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D582,043	S	*	12/2008	Koike	.....	D24/165
D634,430	S	*	3/2011	Osiecki	.....	D24/165
D712,541	S	*	9/2014	Brigham	.....	D24/167
D726,680	S	*	4/2015	Kim	.....	D10/37
D744,656	S	*	12/2015	Schempp	.....	D24/165
2011/0237924	A1	*	9/2011	McGusty	.....	A61B 5/0006 600/391
2013/0281868	A1	*	10/2013	Kawachi	.....	A61B 5/02141 600/485

\* cited by examiner

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Jianq Chyun IP Office

(57) **CLAIM**

The ornamental design for an apparatus for measuring physiological signal, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an apparatus for measuring physiological signal showing our new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a left side view thereof;


FIG. 5 is a right side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The broken line showing of portions of the apparatus for measuring physiological signal is for the purpose of illustrating unclaimed portions of the apparatus for measuring physiological signal and forms no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

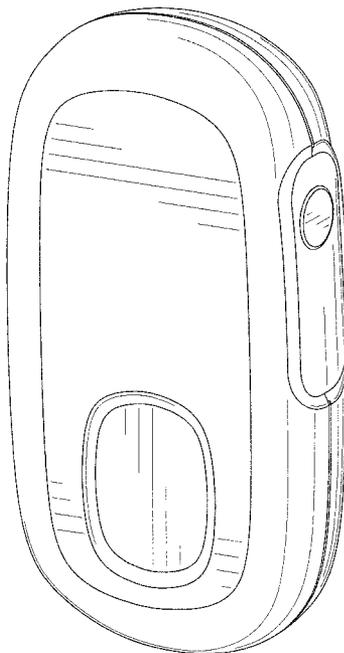

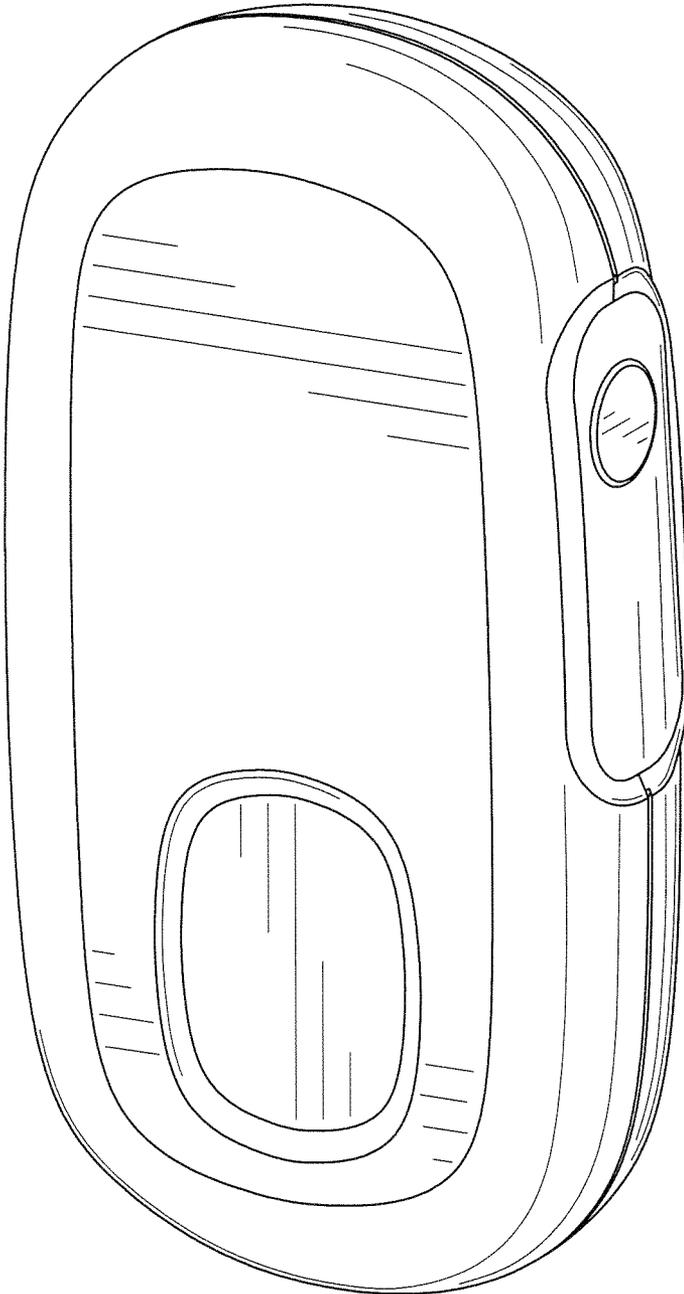


FIG. 1

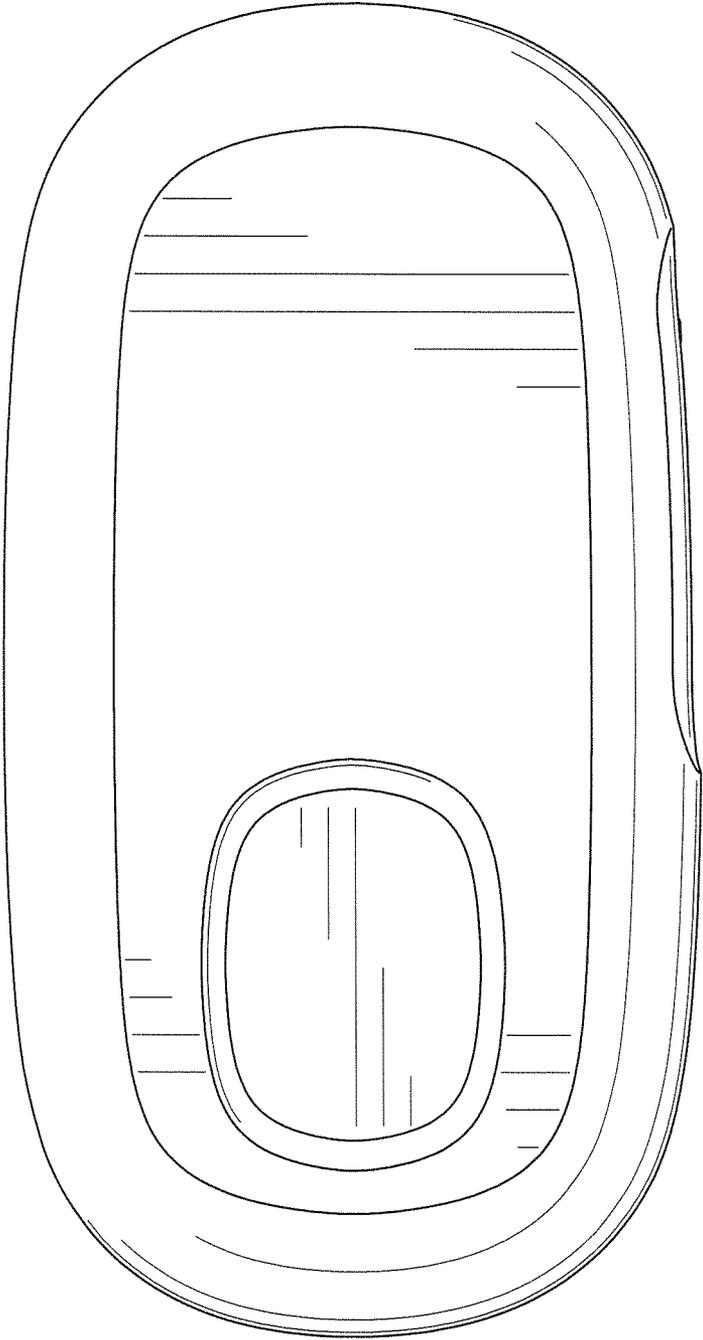


FIG. 2

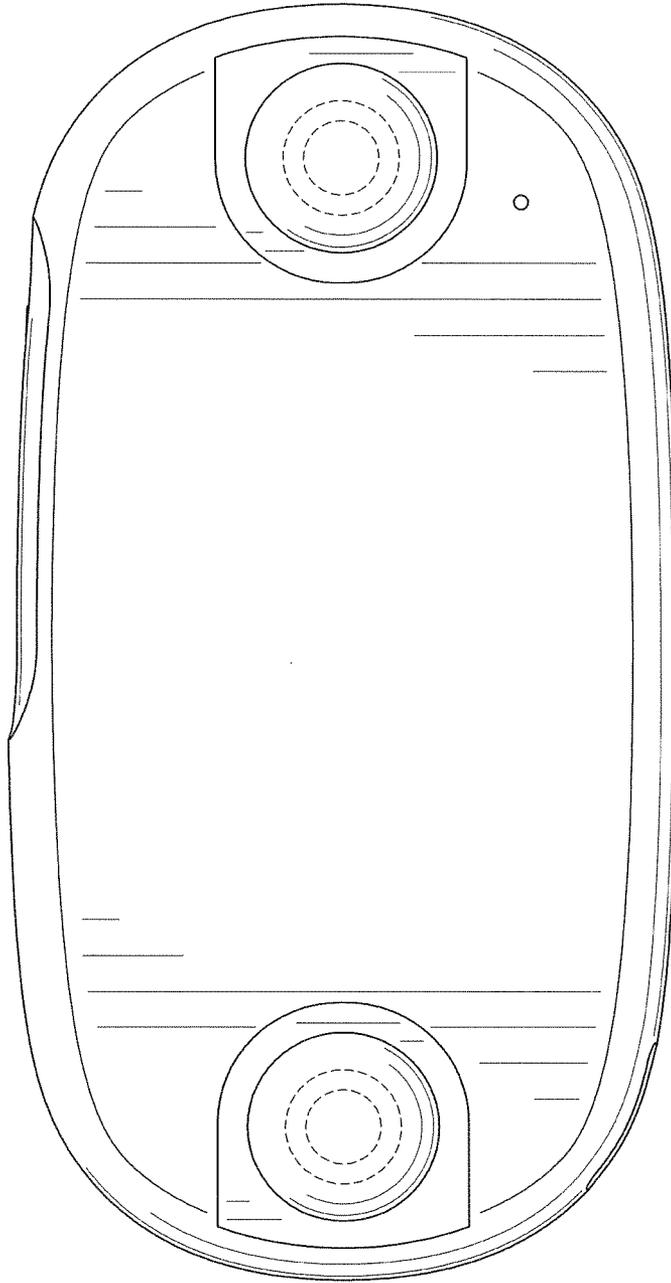


FIG. 3

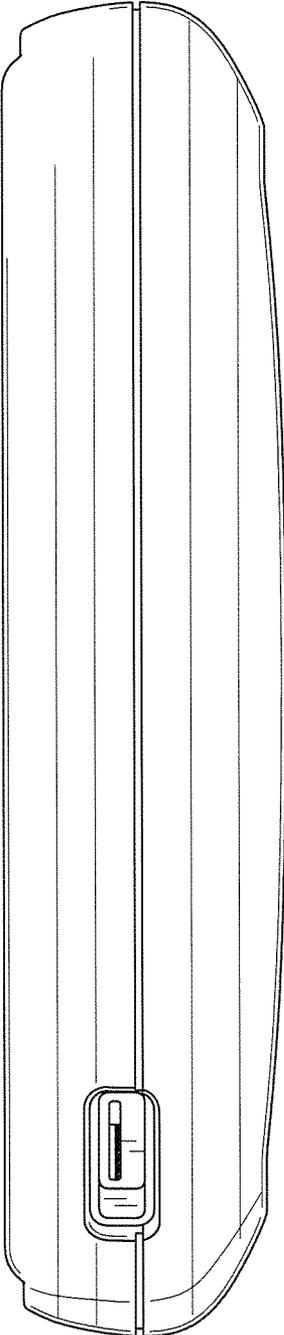


FIG. 4

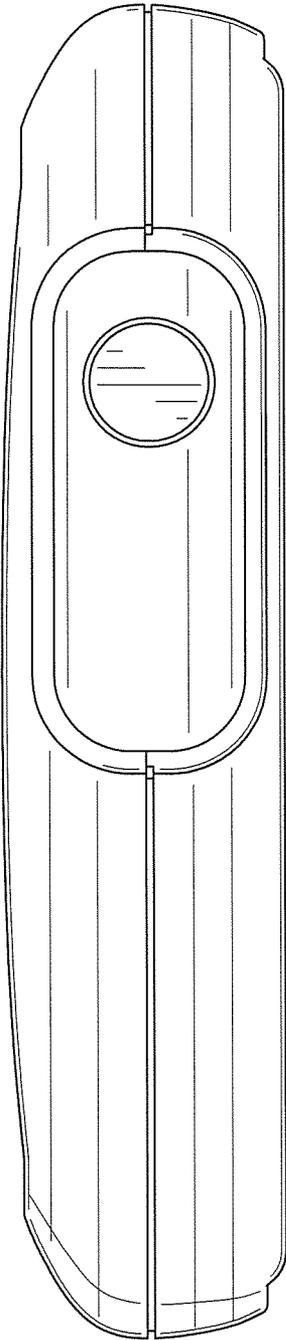


FIG. 5

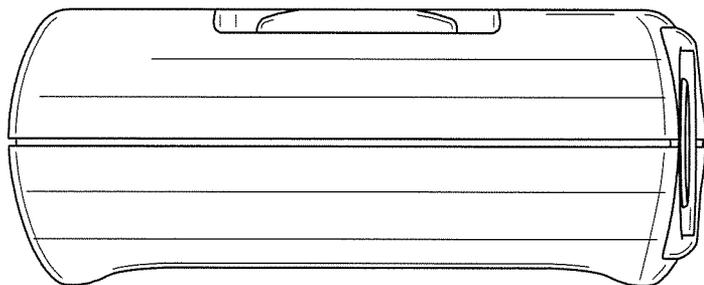


FIG. 6

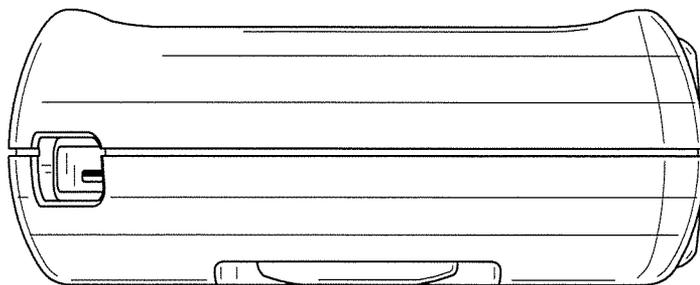


FIG. 7