



(43) International Publication Date
27 February 2014 (27.02.2014)

- (51) International Patent Classification:
A61B 8/00 (2006.01) *A61B 8/08* (2006.01)
A61B 8/14 (2006.01)
- (21) International Application Number:
PCT/US2013/056218
- (22) International Filing Date:
22 August 2013 (22.08.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
13/593,804 24 August 2012 (24.08.2012) US
13/593,789 24 August 2012 (24.08.2012) US
- (71) Applicant: ELWHA LLC [US/US]; 11235 SE 6th Street,
Suite 200, Bellevue, Washington 98004 (US).
- (72) Inventors: BAYM, Michael H.; 12 Remington St., Apt.
206, Cambridge, Massachusetts 02138 (US). HYDE, Rod-

erick A.; 9915 - 161st Avenue N.E., Redmond, Wash-
ington 98052 (US). KARE, Jordin T.; 908 15th Ave. East,
Seattle, Washington 98112 (US). WOOD, Lowell L., Jr.;
989 112th Avenue NE #2310, Bellevue, Washington
98004 (US).

(74) Agents: STEWART, John C. et al.; 11235 SE 6th Street,
Suite 200, Bellevue, Washington 98004 (US).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.

[Continued on next page]

(54) Title: ADAPTIVE ULTRASONIC ARRAY

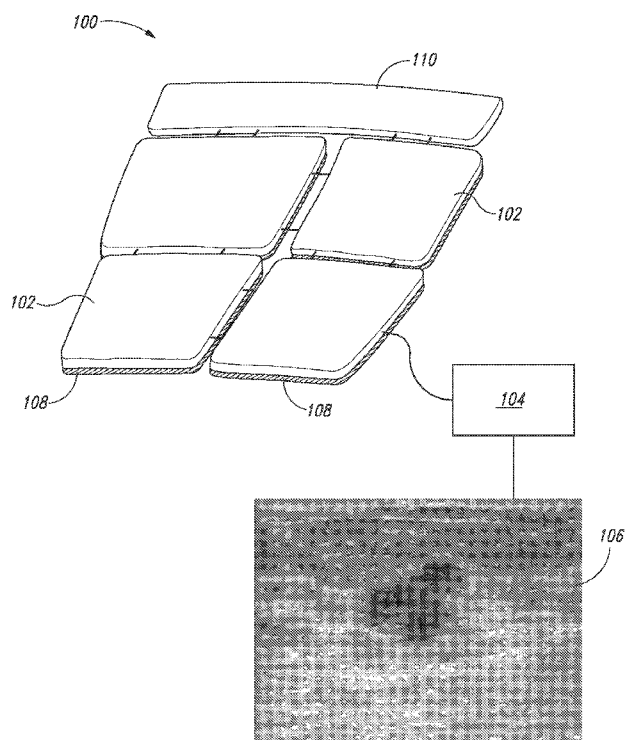


Fig. 1

(57) Abstract: An ultrasound array uses information
about contact quality with the body to weight produced
ultrasound data.



(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,

SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *without international search report and to be republished upon receipt of that report (Rule 48.2(g))*

Adaptive Ultrasonic Array

**Inventor(s): Michael H. Baym, Roderick A. Hyde,
Jordin T. Kare, Lowell L. Wood, Jr.**

CROSS-REFERENCE TO RELATED APPLICATIONS

5 The present application is related to and claims the benefit of the earliest available effective filing date(s) from the following listed application(s) (the “Related Applications”) (e.g., claims earliest available priority dates for other than provisional patent applications or claims benefits under 35 USC § 119(e) for provisional patent applications, for any and all parent, grandparent, great-grandparent, etc. applications of the Related Application(s)). All subject matter of the Related Applications and of any and all parent, grandparent, great-grandparent, etc. applications of the Related Applications, including any priority claims, is incorporated herein by reference to the extent such subject matter is not inconsistent herewith.

Related Applications:

15 For purposes of the USPTO extra-statutory requirements, the present application constitutes a continuation-in-part of United States Patent Application No. **13/593,789**, entitled **ADAPTIVE ULTRASONIC ARRAY**, naming **Michael H. Baym, Roderick A. Hyde, Jordin T. Kare, and Lowell L. Wood, Jr.** as inventors, filed **24 AUGUST 2012**, which is currently co-pending or is an application of which a currently co-pending application is entitled to the benefit of the filing date.

25 The United States Patent Office (USPTO) has published a notice to the effect that the USPTO’s computer programs require that patent applicants reference both a serial number and indicate whether an application is a continuation, continuation-in-part, or divisional of a parent application. Stephen G. Kunin, *Benefit of Prior-Filed Application*, USPTO Official Gazette March 18, 2003. The present Applicant Entity (hereinafter “Applicant”) has provided above a specific reference to the application(s)

from which priority is being claimed as recited by statute. Applicant understands that the statute is unambiguous in its specific reference language and does not require either a serial number or any characterization, such as “continuation” or “continuation-in-part,” for claiming priority to U.S. patent applications.

- 5 Notwithstanding the foregoing, Applicant understands that the USPTO’s computer programs have certain data entry requirements, and hence Applicant has provided designation(s) of a relationship between the present application and its parent application(s) as set forth above, but expressly points out that such designation(s) are not to be construed in any way as any type of commentary and/or admission as to
10 whether or not the present application contains any new matter in addition to the matter of its parent application(s).

SUMMARY

- In one aspect, an ultrasound array includes a plurality of transducer elements
15 configured for contact with a body, and a controller configured to determine a quality of acoustic coupling with the body at each transducer element and to use the determined coupling qualities to apply a weighting to ultrasonic data received from the plurality of transducer elements. The array may further include one or more ultrasound source(s), which may be associated with particular transducer elements.
- 20 The transducer elements may be configured for contact with a living body or a human body, or they may be incorporated into a garment. Determining coupling quality may include determining magnitude of an echo or reflection from an exterior surface of the body or determining magnitude of a signal passing through the body, and may include determining coupling quality at a different frequency from ultrasound
25 imaging. The array may further include a display configured to display an ultrasound image. Applying a weighting may include using ultrasonic data from a subset of the transducers, for example discarding null signals from transducers having a relatively poor contact quality, and may include using contact information from other transducers to determine the weight given to a signal from one or more transducers.
- 30 Applying a weighting may include determining whether an image of a given quality

can be produced, and may further include communicating the fact to a user if it cannot or producing an image only after determining that it can. The transducer elements may be configured to measure a Doppler shift frequency. The array may be configured to respond to determined quality of acoustic coupling by adjusting a quantity of coupling fluid or by adjusting a contact force of a transducer.

Determining quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may further include applying the weighting at the succession of points in time.

In another aspect, an ultrasound array includes a plurality of ultrasound sources configured for contact with a body, a plurality of ultrasound receivers configured to receive ultrasound from the plurality of sources, and a controller configured to determine a quality of acoustic coupling with the body at each ultrasound source and to use the determined qualities to apply a weighting to a power level of each of the plurality of ultrasound sources. Applying a weighting may include determining an in-contact array pattern for the ultrasound sources, and using the determined pattern to calculate a phase-intensity distribution profile selected to deliver a selected irradiation distribution in the body. Applying a weighting may include adjusting a power level of at least some of the ultrasound sources, for example by increasing power to a source having better coupling with the body, increasing power to a source having worse coupling with the body, deactivating a source having inferior coupling, or maintaining a constant total energy of ultrasound coupled into the body by some or all of the ultrasound sources. The ultrasound sources may be configured for contact with a living body or a human body, or they may be incorporated into a garment. Determining coupling quality may include determining magnitude of an echo or reflection from an exterior surface of the body or determining magnitude of a signal passing through the body, and may include determining coupling quality at a different frequency from ultrasound imaging. The array may further include a display configured to display an ultrasound image.

Applying a weighting may include using ultrasonic data from a subset of the receivers, for example discarding null signals from receivers having a relatively poor contact quality. Applying a weighting may include determining whether an image of

a given quality can be produced, and may further include communicating the fact to a user if it cannot or producing an image only after determining that it can. The ultrasound receivers may be configured to measure a Doppler shift frequency. The array may be configured to respond to determined quality of acoustic coupling by
5 adjusting a quantity of coupling fluid or by adjusting a contact force of a receiver or source. Determining quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may further include applying the weighting at a succession of points in time.

In another aspect, an ultrasound method includes applying a plurality of
10 ultrasonic transducer elements to a body, determining a quality of acoustic coupling with the body at each transducer element, and using the determined qualities to apply a weighting to ultrasonic data generated by each transducer element. The method may further include applying one or more ultrasound source(s) to the body, which may be a living body or a human body. The method may further include adjusting a
15 power level of a transducer in response to acoustic coupling quality, for example by turning off the transducer, or by increasing power to a transducer having superior (or inferior) coupling quality. Applying a weighting to the ultrasonic data may include defining an in-contact array pattern, and using the defined pattern to calculate a phase-intensity distribution profile in order to achieve a selected irradiation
20 distribution in the body, and may further include applying the phase-intensity distribution profile. Applying a weighting may include ignoring null signals from out-of-contact transducer elements. Determining a quality of acoustic coupling may include measuring acoustic coupling at a first frequency, and gathering ultrasonic data at a second different frequency. The method may further include displaying an
25 ultrasound image. Applying a weighting may include using data only from a subset of transducer elements, and may include adjusting power level(s) of only a subset of transducer elements, for example by increasing power to an element having a high quality of acoustic coupling with the body, removing power to an element having a low coupling quality, or maintaining a constant total power of ultrasound. Applying a
30 weighting may include discarding null signals from transducers having a relatively poor quality of acoustic coupling with the body. Applying a weighting may include

determining whether a sufficient number of transducers having a sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality, and may further include signaling that the selected quality cannot be achieved, adjusting a quantity of coupling fluid, or adjusting a contact force. Determining a quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may include applying the weighting to ultrasonic data captured in the vicinity of each of these points in time.

In another aspect, an ultrasound method includes applying a plurality of ultrasound sources to a body (*e.g.*, a living body or a human body), applying a plurality of ultrasound receivers to the body, the receivers being configured to receive ultrasound from at least one of the sources, determining a quality of acoustic coupling with the body at each ultrasound source, and using the determined qualities of acoustic coupling to apply a weighting to a power level of each of the ultrasound sources. Applying a weighting to the ultrasonic data may include defining an in-contact array pattern, and using the defined pattern to calculate a phase-intensity distribution profile in order to achieve a selected irradiation distribution in the body, and may further include applying the phase-intensity distribution profile. Applying a weighting may include deactivating at least one ultrasound source, and may include adjusting power level(s) of only a subset of ultrasound sources, for example by increasing power to a source having a high (or low) quality of acoustic coupling with the body, removing power to a source having a low coupling quality, or maintaining a constant total power of ultrasound. Determining a quality of acoustic coupling may include measuring acoustic coupling at a first frequency, and gathering ultrasonic data at a second different frequency. The method may further include displaying an ultrasound image. Applying a weighting may include determining whether a sufficient number of transducers having a sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality, and may further include signaling that the selected quality cannot be achieved. Determining a quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may include applying the weighting to ultrasonic data captured in the vicinity of each of these points in time.

In another aspect, an ultrasound array includes a plurality of transducer elements configured for contact with a body, and a controller configured to determine a quality of acoustic coupling with the body at each transducer element and to use the determined qualities to deactivate transducer elements not meeting a threshold quality of acoustic coupling. The array may further include one or more ultrasound source(s), which may be associated with particular transducer elements. The transducer elements may be configured for contact with a living body or a human body, or they may be incorporated into a garment. Determining coupling quality may include determining magnitude of an echo or reflection from an exterior surface of the body, or determining magnitude of a signal passing through the body. The array may further include a display configured to display an ultrasound image. The transducers may be configured to measure a Doppler shift frequency. Determining quality of acoustic coupling may include determining the quality at a succession of points in type, and applying a weighting may further include applying the weighting at a succession of points in time.

In another aspect, an ultrasound array includes a plurality of transducer elements configured for contact with a body, a plurality of contact sensors, each configured to determine a quality of acoustic coupling with the body at a selected transducer element, and a controller configured to accept quality determinations from the plurality of sensors and use the accepted quality determinations to apply a weighting to ultrasonic data received from the plurality of transducer elements. The contact sensors may be configured to measure contact force with the body, or an electrical property (*e.g.*, resistance or capacitance). The array may further include one or more ultrasound source(s), which may be associated with particular transducer elements. The transducer elements or the contact sensors may be configured for contact with a living body or a human body, or they may be incorporated into a garment. The array may further include a display configured to display an ultrasound image. Applying a weighting may include using ultrasonic data from a subset of the transducers, for example discarding null signals from transducers having a relatively poor contact quality, and may include using contact information from other transducers to determine the weight given to a signal from one or more transducers.

Applying a weighting may include determining whether an image of a given quality can be produced, and may further include communicating the fact to a user if it cannot or producing an image only after determining that it can. The transducer elements may be configured to measure a Doppler shift frequency. The array may be
5 configured to respond to determined quality of acoustic coupling by adjusting a quantity of coupling fluid or by adjusting a contact force of a transducer. Determining quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may further include applying the weighting at the succession of points in time.

10 In another aspect, an ultrasound array includes a plurality of ultrasound sources configured for contact with a body, a plurality of ultrasound receivers configured to receive ultrasound from the plurality of sources, a plurality of contact sensors, each configured to determine a quality of acoustic coupling with the body at a selected ultrasound source, and a controller configured to accept quality
15 determinations from the contact sensors and to use the accepted quality determinations to apply a weighting to ultrasonic data received by the ultrasound receivers. The contact sensors may be configured to measure contact force with the body, or an electrical property (*e.g.*, resistance or capacitance). Applying a weighting may include determining an in-contact array pattern for the ultrasound sources, and
20 using the determined pattern to calculate a phase-intensity distribution profile selected to deliver a selected irradiation distribution in the body. Applying a weighting may include adjusting a power level of at least some of the ultrasound sources, for example by increasing power to a source having better (or worse) coupling with the body, deactivating a source having inferior coupling, or maintaining a constant total
25 energy of ultrasound coupled into the body by some or all of the ultrasound sources. The ultrasound sources or contact sensors may be configured for contact with a living body or a human body, or they may be incorporated into a garment. Determining coupling quality may include determining magnitude of an echo or reflection from an exterior surface of the body, and may include determining coupling quality at a
30 different frequency from ultrasound imaging. The array may further include a display configured to display an ultrasound image. Applying a weighting may include using

ultrasonic data from a subset of the receivers, for example discarding null signals from receivers having a relatively poor contact quality. Applying a weighting may include determining whether an image of a given quality can be produced, and may further include communicating the fact to a user if it cannot or producing an image only after determining that it can. The transducer elements may be configured to measure a Doppler shift frequency. The array may be configured to respond to determined quality of acoustic coupling by adjusting a quantity of coupling fluid or by adjusting a contact force of a receiver or source. Determining quality of acoustic coupling may include determining the quality at a succession of points in type, and applying a weighting may further include applying the weighting at a succession of points in time.

In another aspect, an ultrasound method includes applying a plurality of ultrasonic transducer elements to a body, applying a plurality of contact sensors to the body, each configured to determine a quality of acoustic coupling with the body at a selected transducer element, determining a quality of acoustic coupling with the body at each transducer element, and using the determined qualities to apply a weighting to ultrasonic data generated by each transducer element. Determining a quality of acoustic coupling may include determining contact force with the body, or an electrical property (*e.g.*, resistance or capacitance). The method may further include applying one or more ultrasound source(s) to the body, which may be a living body or a human body. The method may further include adjusting a power level of a transducer in response to acoustic coupling quality, for example by turning off the transducer. Applying a weighting to the ultrasonic data may include defining an in-contact array pattern, and using the defined pattern to calculate a phase-intensity distribution profile in order to achieve a selected irradiation distribution in the body, and may further include applying the phase-intensity distribution profile. Applying a weighting may include ignoring null signals from out-of-contact transducer elements. The method may further include displaying an ultrasound image. Applying a weighting may include using data only from a subset of transducer elements, and may include adjusting power level(s) of only a subset of transducer elements, for example by increasing power to an element having a high (or low) quality of acoustic coupling

with the body, removing power to an element having a low coupling quality, or maintaining a constant total power of ultrasound. Applying a weighting may include discarding null signals from transducers having a relatively poor quality of acoustic coupling with the body. Applying a weighting may include determining whether a
5 sufficient number of transducers having a sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality, and may further include signaling that the selected quality cannot be achieved, adjusting a quantity of coupling fluid, or adjusting a contact force. Determining a quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting
10 may include applying the weighting to ultrasonic data captured in the vicinity of each of these points in time.

In another aspect, an ultrasound method includes applying a plurality of ultrasound sources to a body (*e.g.*, a living body or a human body), applying a plurality of ultrasound receivers to the body, the receivers configured to receive
15 ultrasound from at least one of the sources, applying a plurality of contact sensors to the body, each configured to determine a quality of acoustic coupling with the body at an ultrasound source, determining a quality of acoustic coupling with the body at each ultrasound source, and using the determined qualities of acoustic coupling to apply a weighting to ultrasonic data generated by each ultrasonic receiver. Determining a
20 quality of acoustic coupling may include determining contact force with the body, or an electrical property (*e.g.*, resistance or capacitance). Applying a weighting to the ultrasonic data may include defining an in-contact array pattern, and using the defined pattern to calculate a phase-intensity distribution profile in order to achieve a selected irradiation distribution in the body, and may further include applying the phase-
25 intensity distribution profile. Applying a weighting may include deactivating at least one ultrasound source, and may include adjusting power level(s) of only a subset of ultrasound sources, for example by increasing power to a source having a high (or low) quality of acoustic coupling with the body, removing power to a source having a low coupling quality, or maintaining a constant total power of ultrasound. The
30 method may further include displaying an ultrasound image. Applying a weighting may include determining whether a sufficient number of transducers having a

sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality, and may further include communicating an achievable image quality.

Determining a quality of acoustic coupling may include determining the quality at a succession of points in time, and applying a weighting may include applying the

5 weighting to ultrasonic data captured in the vicinity of each of these points in time.

The foregoing summary is illustrative only and is not intended to be in any way limiting. In addition to the illustrative aspects, embodiments, and features described above, further aspects, embodiments, and features will become apparent by reference to the drawings and the following detailed description.

10 BRIEF DESCRIPTION OF THE FIGURES

Fig. 1 is a schematic of an ultrasound array.

Fig. 2 is a schematic of another ultrasound array.

Fig. 3 is a flow chart illustrating operation of an ultrasound array.

Fig. 4 is a flow chart illustrating weighting of ultrasonic data.

15 Fig. 5 is a schematic of another method of weighting ultrasonic data.

DETAILED DESCRIPTION

In the following detailed description, reference is made to the accompanying drawings, which form a part hereof. In the drawings, similar symbols typically identify similar components, unless context dictates otherwise. The illustrative
20 embodiments described in the detailed description, drawings, and claims are not meant to be limiting. Other embodiments may be utilized, and other changes may be made, without departing from the spirit or scope of the subject matter presented here.

Fig. 1 is a schematic of an ultrasound array **100** configured for producing an ultrasound image. The array includes transducer elements **102** configured for contact
25 with a body. Controller **104** monitors signals from transducer elements **102** indicating the quality of their acoustic coupling with the body, and applies a weighting to data received from the transducers **102** to produce an ultrasound image **106**. In some embodiments, the quality of acoustic coupling at each transducer is determined by using the ultrasound transducer itself, either at the imaging frequency

or at another frequency. Alternatively (or, in some embodiments, in addition), the quality of acoustic coupling may be determined by use of a separate contact sensor **108**. For example, contact sensors **108** may be force measurement transducers, or they may be capacitive or resistive sensors. Ultrasound may enter the body from a source **110** (or plurality of sources) colocated with the transducer elements **102**, or from a remote source or sources. In some embodiments including a plurality of sources, each source **110** is associated with a particular transducer element **102**. In some embodiments, different transducer elements **102** may use different sound frequencies in order to differentiate between sources **110**.

In a very simple embodiment, controller **104** may monitor coupling of transducer elements **102**, and may simply omit imaging data received from a transducer not meeting a contact quality threshold from appearing in the ultrasound image. In other embodiments, there may be a more complicated relationship between contact quality and imaging data. For example, data may be “downgraded” and used only if there is no data available from a nearby transducer element **102** in better contact with the body. In one embodiment, only the best 90% (or 70% or 50% or 30%) transducer elements **102** (that is, the 90% of transducers **102** having the best acoustic contact with the body) are used in the image. The image may also include false color to identify more or less “reliable” areas. For example, all measured image data may be used to generate an ultrasound image, but pixels may be shaded in red in areas where contact with the body is poor, and in green in areas where it is good. In some cases, an ultrasonic image may have “holes” indicating that there was insufficient contact with the body in those areas, or the system may simply indicate that no image can be produced at all because of poor contact quality.

Monitoring of contact with the body may be static or dynamic in nature. For a single image of a non-moving body, it may be sufficient to determine quality of acoustic contact for each transducer once. For a longer imaging process and/or a body in motion, it may be preferable to dynamically monitor the contact with various transducers and to continuously adjust the resultant image, either by weighting the data and using “better” data more heavily, or by applying false color or similar cues to the image to alert the user to areas of better or worse image quality. Data

weighting may be computational in nature (where pixels “count” more heavily when they are considered to be more reliable), or it may be accomplished by providing more power to ultrasound sources (*e.g.*, transducers) that appear to have a better quality of contact with the underlying body.

5 In some embodiments, once the quality of acoustic coupling is measured, the system may attempt to remediate transducers having poor acoustic coupling. For example, the system may dispense additional ultrasound gel (or another acoustic coupling agent) to try to improve the quality of coupling at a transducer element **102** having a poor image quality rating, or it may adjust a contact force in the area having
10 a poor contact rating.

Fig. 2 is a schematic of another ultrasound array **200**. As in **Fig. 1**, array **200** includes a plurality of ultrasound transducers **202**, and controller **204** monitors the quality of acoustic coupling of transducers **202** with a body under examination **206**. However, array **200** is not configured to produce a human-readable image such as that
15 shown in **Fig. 1**. The array illustrated in **Fig. 2** is configured for monitoring the condition of a human heart using a continuously-worn monitoring vest **208**. Since the vest **208** is worn continuously during normal day-to-day activities (or possibly during a testing situation such as, for example, a cardiac stress test), transducers **202** are expected to vary their position and the quality of their acoustic contact with the body
20 substantially over time.

Cardiac monitors such as the one illustrated in **Fig. 2** typically use the Doppler effect to measure the velocity of blood through the aortic arch, using the relationship

$$f = \frac{2v f_0 \cos \theta}{c}$$

where v represents the blood speed, f_0 represents the ultrasound beam frequency, c represents the speed of ultrasound in blood (about 1.6×10^3 m/s), and f represents the
25 Doppler shift frequency. Since θ is relatively difficult to estimate, especially for a wearable ultrasound system like that illustrated in **Fig. 2**, it is preferable (but not required, as long as the angle of insonation is at least approximately known) to orient the beam to be as close as possible to parallel to the flow of blood. Since there are

multiple transducers **202**, controller **204** may also use their relative measurements to estimate the value of θ .

In use, controller **204** monitors the quality of acoustic coupling of transducers **202** with the body, and continuously calculates a best estimate for blood velocity. In some embodiments, data from all transducers **202** is used, but the transducers having the best acoustic contact with the body are weighted more heavily. In other embodiments, data from transducers **202** having poorer contact with the body is discarded. Blood velocity data may be recorded, *e.g.*, for later review by a physician.

The transducer arrays described above may be used to obtain ultrasound data regarding a variety of different objects. In some embodiments, the array may be used to probe a living body or a human body, while in other embodiments, the array may be used to probe an article of manufacture (*e.g.*, checking a casting for cracks before it is deployed). The transducer elements may be, for example, incorporated into a garment, which may be worn by a user in a testing situation and/or during daily activities.

Fig. 3 is a flow chart illustrating use of an ultrasound array like the ones illustrated in **Fig. 1** and **Fig. 2**. The method includes applying ultrasonic transducer elements to a body **300**, determining a quality of acoustic coupling with the body at each transducer element **302**, and using the determined qualities of acoustic coupling to apply a weighting to ultrasonic data generated by each transducer element **304**.

Determining a quality of acoustic coupling at (or in the immediate proximity of) each transducer element may include, for example, determining the magnitude of an echo or reflection from an exterior surface of the body, either at the imaging frequency or at a different frequency. A strong echo is typically associated with good coupling with the body. Alternatively, determining a coupling may include measuring contact with the body by measuring force, resistance, capacitance, or some other property. For example, a strain gage may be placed at the contact surface of a transducer element to measure the force between that element and the body, where a larger contact force is typically indicative of a better quality of acoustic coupling.

Once an array of acoustic coupling data has been determined, it is used to apply a weighting. A simple method of weighting the data is illustrated in **Fig. 4**. The

measured qualities (e.g., the contact forces) are sorted **402**, and the bottom 30% are discarded **404**. (Those of skill in the art will of course recognize that 30% is an arbitrary value, and that another threshold may equally well be substituted, either as a different percentage or as a different absolute value of the quality measure.) In some
5 embodiments, explicitly discarding measurements from sites in poor contact will improve image reconstruction compared to the alternative of receiving a low or null signal due to poor coupling quality and assuming that this value represents an actual trough in the arriving ultrasonic wave. The remaining sensor data is used to generate an ultrasound image **406**. In some embodiments, the 30% of transducers that are
10 removed from the data create “holes” in the ultrasound image, while in other embodiments, data is interpolated **408** from neighboring transducers to show a complete image. In embodiments where the data is interpolated to produce a complete image, false color may be used to identify interpolated regions.

A slightly more complex method of data weighting is illustrated in **Fig. 5**. In
15 this method, the quality of acoustic coupling at each transducer is used to determine a “spot size” for data from that transducer. **Fig. 5** shows spot sizes **500** for a plurality of transducers. Those with relatively good coupling have large spots **502**, while those with relatively poor coupling have smaller spots **504**. In some embodiments of this type, spot sizes may go to zero for sufficiently poor acoustic coupling. When
20 displaying an image, any given pixel is displayed using the ultrasonic measurement generated by the transducer having that pixel in its “spot.” If a pixel appears in multiple spots (as at point **506**), it either uses an average of the values of the spots overlapping the pixel, or it uses the largest spot that overlaps it. No data is generated for pixels falling outside the spots (such as at point **508**).

25 In some embodiments, determination of the acoustic coupling quality may be used to adjust one or more power levels for ultrasound source(s). This may include, for example, increasing power to sources having good contact, or decreasing (or turning off entirely) sources having poor contact. This may include increasing power to sources having poor contact so as to maintain or equalize a desired level of
30 ultrasonic coupling into the body. In some embodiments, the determined quality of acoustic coupling for an ultrasonic source may be used to determine a measure of

how much of its output actually couples into the body; this can then be used within data analysis algorithms by replacing source distributions based on emitted power by ones based on coupled power.

In some embodiments, knowledge of the spatial profile of coupling quality for an array of ultrasonic transducers can be used in operation of a phased array. The activation of individual sources can be based upon the spatial pattern of those having sufficient coupling quality, and the power delivered to each source can depend upon its coupling quality in order to achieve a desired spatial pattern of body-coupled ultrasonic power. Similarly, the spatial pattern of the coupling quality can also be used in determining the reception properties of a phased array. Array elements having poor coupling quality can be deleted from the antenna pattern, and received ultrasonic signals at a location can be divided by the coupling quality to provide a better measure of the ultrasonic signal arriving at the surface of the body.

In a general sense, those skilled in the art will recognize that the various aspects described herein which can be implemented, individually or collectively, by a wide range of hardware, software, firmware, or any combination thereof can be viewed as being composed of various types of “electrical circuitry.” Consequently, as used herein “electrical circuitry” includes, but is not limited to, electrical circuitry having at least one discrete electrical circuit, electrical circuitry having at least one integrated circuit, electrical circuitry having at least one application specific integrated circuit, electrical circuitry forming a general purpose computing device configured by a computer program (*e.g.*, a general purpose computer configured by a computer program which at least partially carries out processes or devices described herein, or a microprocessor configured by a computer program which at least partially carries out processes or devices described herein), electrical circuitry forming a memory device (*e.g.*, forms of random access memory), or electrical circuitry forming a communications device (*e.g.*, a modem, communications switch, or optical-electrical equipment). Those having skill in the art will recognize that the subject matter described herein may be implemented in an analog or digital fashion or some combination thereof.

Those having skill in the art will recognize that the state of the art of circuit design has progressed to the point where there is typically little distinction left between hardware and software implementations of aspects of systems. The use of hardware or software is generally a design choice representing tradeoffs between cost, efficiency, flexibility, and other implementation considerations. Those having skill in the art will appreciate that there are various vehicles by which processes, systems or other technologies involving the use of logic or circuits can be effected (*e.g.*, hardware, software, or firmware), and that the preferred vehicle will vary with the context in which the processes, systems or other technologies are deployed. For example, if an implementer determines that speed is paramount, the implementer may opt for a mainly hardware or firmware vehicle. Alternatively, if flexibility is paramount, the implementer may opt for a mainly software implementation. In these or other situations, the implementer may also opt for some combination of hardware, software, or firmware. Hence, there are several possible vehicles by which the processes, devices or other technologies involving logic or circuits described herein may be effected, none of which is inherently superior to the other. Those skilled in the art will recognize that optical aspects of implementations may require optically-oriented hardware, software, and or firmware.

It will be understood by those within the art that, in general, terms used herein, and especially in the appended claims are generally intended as “open” terms (*e.g.*, the term “including” should be interpreted as “including but not limited to,” the term “having” should be interpreted as “having at least,” the term “includes” should be interpreted as “includes but is not limited to,” etc.). It will be further understood by those within the art that if a specific number of an introduced claim recitation is intended, such an intent will be explicitly recited in the claim, and in the absence of such recitation no such intent is present. For example, as an aid to understanding, the following appended claims may contain usage of introductory phrases such as “at least one” or “one or more” to introduce claim recitations. However, the use of such phrases should not be construed to imply that the introduction of a claim recitation by the indefinite articles “a” or “an” limits any particular claim containing such introduced claim recitation to inventions containing only one such recitation, even

when the same claim includes the introductory phrases “one or more” or “at least one” and indefinite articles such as “a” or “an” (*e.g.*, “a transducer” should typically be interpreted to mean “at least one transducer”); the same holds true for the use of definite articles used to introduce claim recitations. In addition, even if a specific
5 number of an introduced claim recitation *is* explicitly recited, those skilled in the art will recognize that such recitation should typically be interpreted to mean *at least* the recited number (*e.g.*, the bare recitation of “two transducers,” or “a plurality of transducers,” without other modifiers, typically means *at least* two transducers). Furthermore, in those instances where a phrase such as “at least one of A, B, and C,”
10 “at least one of A, B, or C,” or “an [item] selected from the group consisting of A, B, and C,” is used, in general such a construction is intended in the sense one having skill in the art would understand the convention (*e.g.*, any of these phrases would include but not be limited to systems that have A alone, B alone, C alone, A and B together, A and C together, B and C together, or A, B, and C together). It will be
15 further understood by those within the art that virtually any disjunctive word or phrase presenting two or more alternative terms, whether in the description, claims, or drawings, should be understood to contemplate the possibilities of including one of the terms, either of the terms, or both terms. For example, the phrase “A or B” will be understood to include the possibilities of “A” or “B” or “A and B.”

20 While various aspects and embodiments have been disclosed herein, other aspects and embodiments will be apparent to those skilled in the art. The various aspects and embodiments disclosed herein are for purposes of illustration and are not intended to be limiting, with the true scope and spirit being indicated by the following claims.

25 What is claimed is:

CLAIMS

1. An ultrasound array, comprising:
a plurality of transducer elements configured for contact with a body;
a plurality of contact sensors, each contact sensor configured to determine a quality of acoustic coupling with the body at a selected transducer element; and
a controller configured to accept quality determinations from the plurality of sensors and to use the accepted quality determinations to apply a weighting to ultrasonic data received from the plurality of transducer elements.
2. The ultrasound array of claim 1, wherein the plurality of contact sensors are configured to measure contact force with the body.
3. The ultrasound array of claim 1, wherein the plurality of contact sensors are configured to measure an electrical property to determine quality of contact with the body.
4. The ultrasound array of claim 3, wherein the electrical property is selected from the group consisting of resistance and capacitance.
5. The ultrasound array of claim 1, further comprising an ultrasound source.
6. The ultrasound array of claim 1, further comprising a plurality of ultrasound sources.
7. The ultrasound array of claim 6, wherein each ultrasound source is associated with a corresponding member of the plurality of transducer elements.
8. The ultrasound array of claim 1, wherein the plurality of transducer elements are configured for contact with a living body.

9. The ultrasound array of claim 1, wherein the plurality of transducer elements are configured for contact with a human body.
10. The ultrasound array of claim 1, wherein the plurality of transducer elements are incorporated into a garment.
11. The ultrasound array of claim 1, wherein the plurality of contact sensors are configured for contact with a living body.
12. The ultrasound array of claim 1, wherein the plurality of contact sensors are configured for contact with a human body.
13. The ultrasound array of claim 1, wherein the plurality of contact sensors are incorporated into a garment.
14. The ultrasound array of claim 1, further comprising a display configured to display an ultrasound image using the weighted ultrasonic data.
15. The ultrasound array of claim 1, wherein applying a weighting includes using ultrasonic data from a selected subset of the plurality of transducer elements.
16. The ultrasound array of claim 15, wherein applying a weighting includes applying a weighting to one element of the selected subset using contact quality data from a contact sensor associated with a different element of the selected subset.
17. The ultrasound array of claim 1, wherein applying a weighting includes discarding null signals from transducers having a relatively poor quality of acoustic coupling with the body.
18. The ultrasound array of claim 1, wherein applying a weighting includes determining whether a sufficient number of transducers have a sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality.

19. The ultrasound array of claim 18, wherein determining whether a sufficient number of transducers have a sufficient quality of acoustic coupling includes signaling that the ultrasound image of the selected quality cannot be produced.
20. The ultrasound array of claim 18, wherein determining whether a sufficient number of transducers have a sufficient quality of acoustic coupling includes producing an ultrasound image only after determining that the selected quality of ultrasound image can be achieved.
21. The ultrasound array of claim 1, wherein the transducers are configured to measure a Doppler shift frequency.
22. The ultrasound array of claim 1, further comprising responding to a quality determination by adjusting a quantity of coupling fluid between a transducer and the body.
23. The ultrasound array of claim 1, further comprising responding to a quality determination by adjusting a contact force of the transducer.
24. The ultrasound array of claim 1, wherein accepting a quality determination from a contact sensor includes accepting the quality determination at a succession of points in time.
25. The ultrasound array of claim 24, wherein applying a weighting includes applying the weighting to ultrasonic data captured in the vicinity of each point in time.
26. An ultrasound array, comprising:
 - a plurality of ultrasound sources configured for contact with a body;
 - a plurality of ultrasound receivers configured to receive ultrasound from the plurality of ultrasound sources;
 - a plurality of contact sensors, each contact sensor configured to determine a quality of acoustic coupling with the body at a selected ultrasound source;
 - and

a controller configured to accept quality determinations from the plurality of contact sensors and to use the accepted quality determinations to apply a weighting to ultrasonic data received by the ultrasound receivers.

27. The ultrasound array of claim 26, wherein the plurality of contact sensors are configured to measure contact force with the body.
28. The ultrasound array of claim 26, wherein the plurality of contact sensors are configured to measure an electrical property to determine quality of contact with the body.
29. The ultrasound array of claim 28, wherein the electrical property is selected from the group consisting of resistance and capacitance.
30. The ultrasound array of claim 26, wherein applying a weighting includes determining an in-contact array pattern for the ultrasound sources, and further includes using the determined in-contact array pattern to calculate a phase-intensity distribution profile selected to deliver a selected irradiation distribution in the body.
31. The ultrasound array of claim 26, wherein applying a weighting includes adjusting a power level of a selected subset of the plurality of ultrasound sources.
32. The ultrasound array of claim 31, wherein adjusting a power level includes increasing power to an ultrasound source having a superior quality of acoustic coupling with the body compared to another ultrasound source.
33. The ultrasound array of claim 31, wherein adjusting a power level includes increasing power to an ultrasound source having an inferior quality of acoustic coupling with the body compared to another ultrasound source.
34. The ultrasound array of claim 31, wherein adjusting a power level includes removing power to an ultrasound source having an inferior quality of acoustic coupling with the body compared to another ultrasound source.

35. The ultrasound array of claim 31, wherein adjusting a power level includes maintaining a constant total energy of ultrasound coupled into the object by the plurality of ultrasound sources.
36. The ultrasound array of claim 31, wherein adjusting a power level includes maintaining a constant total energy of ultrasound coupled into the object by a member of the plurality of ultrasound sources.
37. The ultrasound array of claim 26, wherein the plurality of ultrasound receivers are configured for contact with a living body.
38. The ultrasound array of claim 26, wherein the plurality of ultrasound receivers are configured for contact with a human body.
39. The ultrasound array of claim 26, wherein the plurality of ultrasound receivers are incorporated into a garment.
40. The ultrasound array of claim 26, wherein the plurality of ultrasound sources are configured for contact with a living body.
41. The ultrasound array of claim 26, wherein the plurality of ultrasound sources are configured for contact with a human body.
42. The ultrasound array of claim 26, wherein the plurality of ultrasound sources are incorporated into a garment.
43. The ultrasound array of claim 26, further comprising a display configured to display an ultrasound image after applying a weighting to a power level of the plurality of ultrasound sources.
44. The ultrasound array of claim 26, wherein applying a weighting to a power level of each of the plurality of ultrasound sources includes deactivating at least one ultrasound source.

45. The ultrasound array of claim 26, wherein applying a weighting to a power level of each of the plurality of ultrasound sources includes adjusting a total power to a level that provides a selected image quality.
46. The ultrasound array of claim 26, wherein applying a weighting to a power level of each of the plurality of ultrasound sources includes determining that an image of a selected quality cannot be produced.
47. The ultrasound array of claim 26, wherein the ultrasound receivers are configured to measure a Doppler shift frequency.
48. The ultrasound array of claim 26, wherein the array is configured to respond to the determined quality of acoustic coupling by adjusting a quantity of coupling fluid between an ultrasound source and the body.
49. The ultrasound array of claim 26, wherein the array is configured to respond to the determined quality of acoustic coupling by adjusting a contact force between an ultrasound source and the body.
50. The ultrasound array of claim 26, wherein the controller is configured to accept quality determinations at a succession of points in time.
51. The ultrasound array of claim 50, wherein the controller is configured to apply a weighting at a succession of points in time.
52. An ultrasound method, comprising:
 - applying a plurality of ultrasonic transducer elements to a body;
 - applying a plurality of contact sensors to the body, each contact sensor configured to determine a quality of acoustic coupling with the body at a selected transducer element;
 - determining a quality of acoustic coupling with the body at each transducer element; and
 - using the determined qualities of acoustic coupling to apply a weighting to ultrasonic data generated by each transducer element.

53. The method of claim 52, wherein determining a quality of acoustic coupling with the body includes determining a contact force.
54. The method of claim 52, wherein determining a quality of acoustic coupling with the body includes determining an electrical property.
55. The method of claim 54, wherein the electrical property is selected from the group consisting of resistance and capacitance.
56. The method of claim 52, further comprising applying an ultrasound source to the body.
57. The method of claim 52, further comprising applying a plurality of ultrasound sources to the body.
58. The method of claim 52, wherein the body is a living body.
59. The method of claim 52, wherein the body is a human body.
60. The method of claim 52, further comprising adjusting a power level of at least one transducer element in response to its determined quality of acoustic coupling.
61. The method of claim 60, wherein adjusting a power level of at least one transducer element includes turning off the transducer element.
62. The method of claim 52, wherein applying a weighting to the ultrasonic data includes defining an in-contact array pattern, and using the defined pattern to calculate a phase-intensity distribution profile in order to achieve a selected irradiation distribution in the body.
63. The method of claim 62, further comprising applying the phase-intensity distribution profile to the plurality of transducer elements.
64. The method of claim 52, wherein applying a weighting to the ultrasonic data includes ignoring null signals from out-of-contact transducer elements.

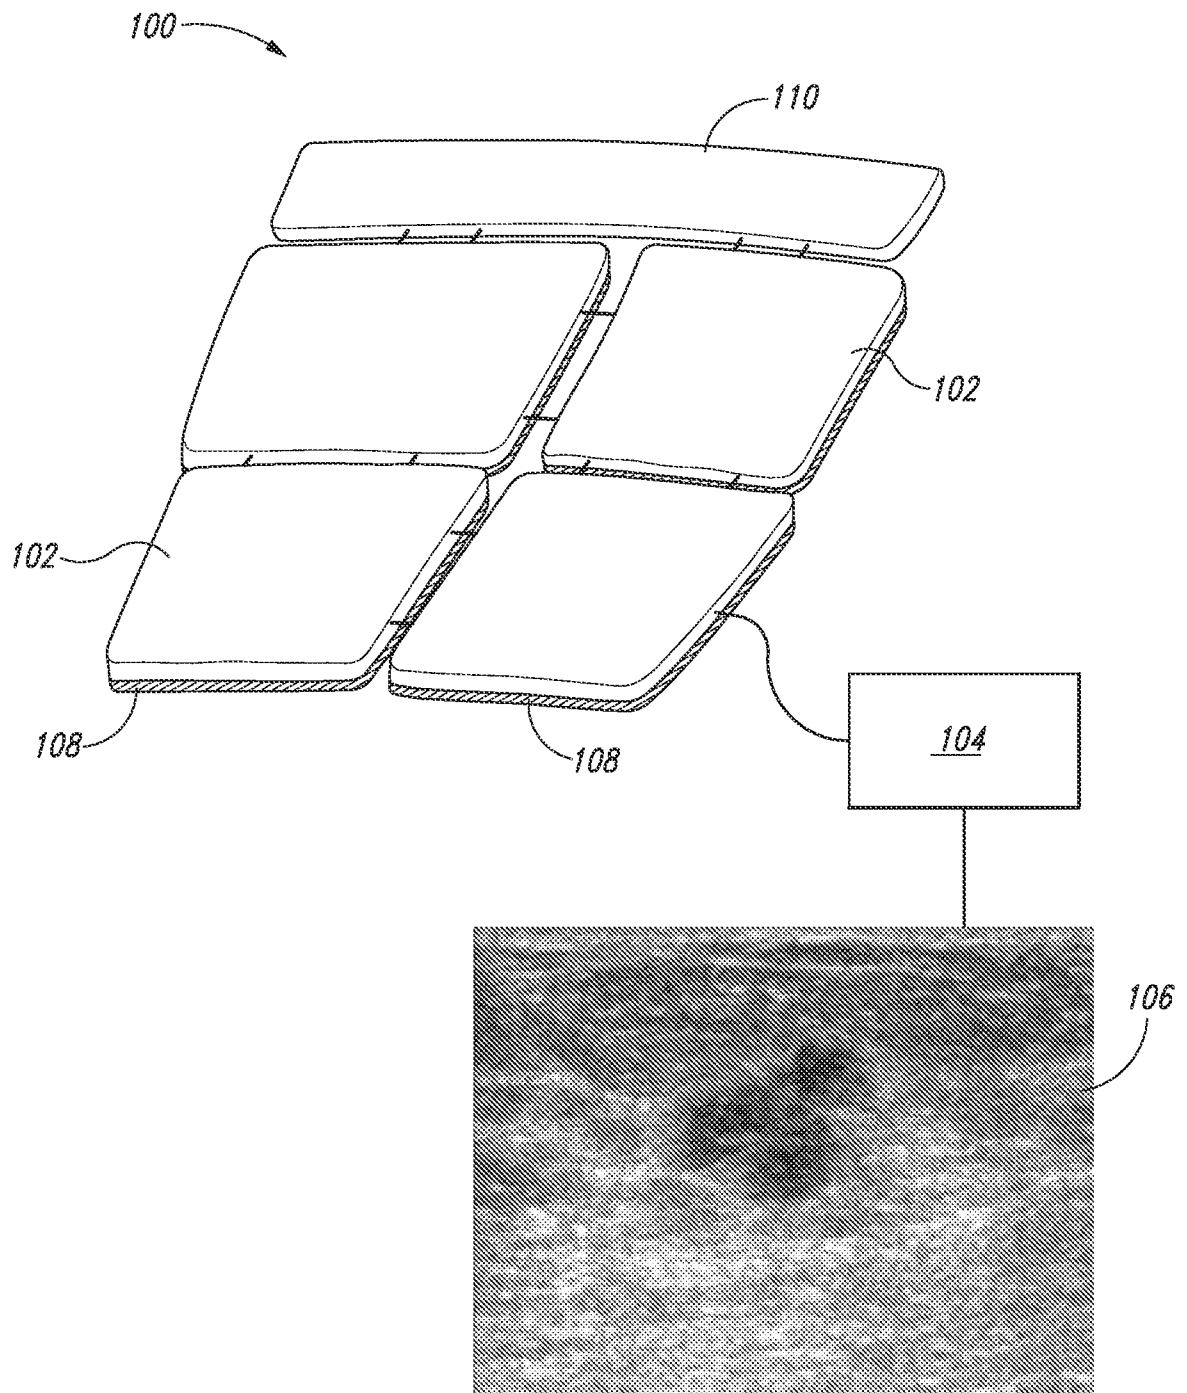
65. The method of claim 52, further comprising displaying an ultrasound image using the weighted ultrasonic data.
66. The method of claim 52, wherein applying a weighting includes using ultrasonic data from a selected subset of the plurality of transducer elements.
67. The method of claim 52, wherein applying a weighting includes adjusting a power level of a selected subset of the plurality of transducer elements.
68. The method of claim 67, wherein adjusting a power level includes increasing power to a transducer element having a superior quality of acoustic coupling with the body compared to another transducer element.
69. The method of claim 67, wherein adjusting a power level includes increasing power to a transducer element having an inferior quality of acoustic coupling with the body compared to another transducer element.
70. The method of claim 67, wherein adjusting a power level includes removing power to a transducer element having an inferior quality of acoustic coupling with the body compared to another transducer element.
71. The method of claim 67, wherein adjusting a power level includes maintaining a constant total power of delivered ultrasound.
72. The method of claim 52, wherein applying a weighting includes discarding null signals from transducers having a relatively poor quality of acoustic coupling with the body.
73. The method of claim 52, wherein applying a weighting includes determining whether a sufficient number of transducers have a sufficient quality of acoustic coupling to generate an ultrasound image of a selected quality.
74. The method of claim 73, wherein determining whether a sufficient number of transducers have a sufficient quality of acoustic coupling includes signaling that the ultrasound image of the selected quality cannot be produced.

75. The method of claim 73, further comprising responding to the determined quality by adjusting a quantity of coupling fluid.
76. The method of claim 73, further comprising responding to the determined quality by adjusting a contact force.
77. The method of claim 52, wherein determining a quality of acoustic coupling with the body at each transducer element includes determining the quality at a succession of points in time.
78. The method of claim 77, wherein applying a weighting includes applying the weighting to ultrasonic data captured in the vicinity of each point in time.
79. An ultrasound method, comprising:
applying a plurality of ultrasound sources to a body;
applying a plurality of ultrasound receivers to the body, the ultrasound receivers being configured to receive ultrasound from at least one of the ultrasound sources;
applying a plurality of contact sensors to the body, each contact sensor configured to determine a quality of acoustic coupling with the body at a selected ultrasound source;
determining a quality of acoustic coupling with the body at each ultrasound source; and
using the determined qualities of acoustic coupling to apply a weighting to ultrasonic data generated by each ultrasonic receiver.
80. The method of claim 79, wherein determining a quality of acoustic coupling with the body includes determining a contact force.
81. The method of claim 79, wherein determining a quality of acoustic coupling with the body includes determining an electrical property.
82. The method of claim 81, wherein the electrical property is selected from the group consisting of resistance and capacitance.

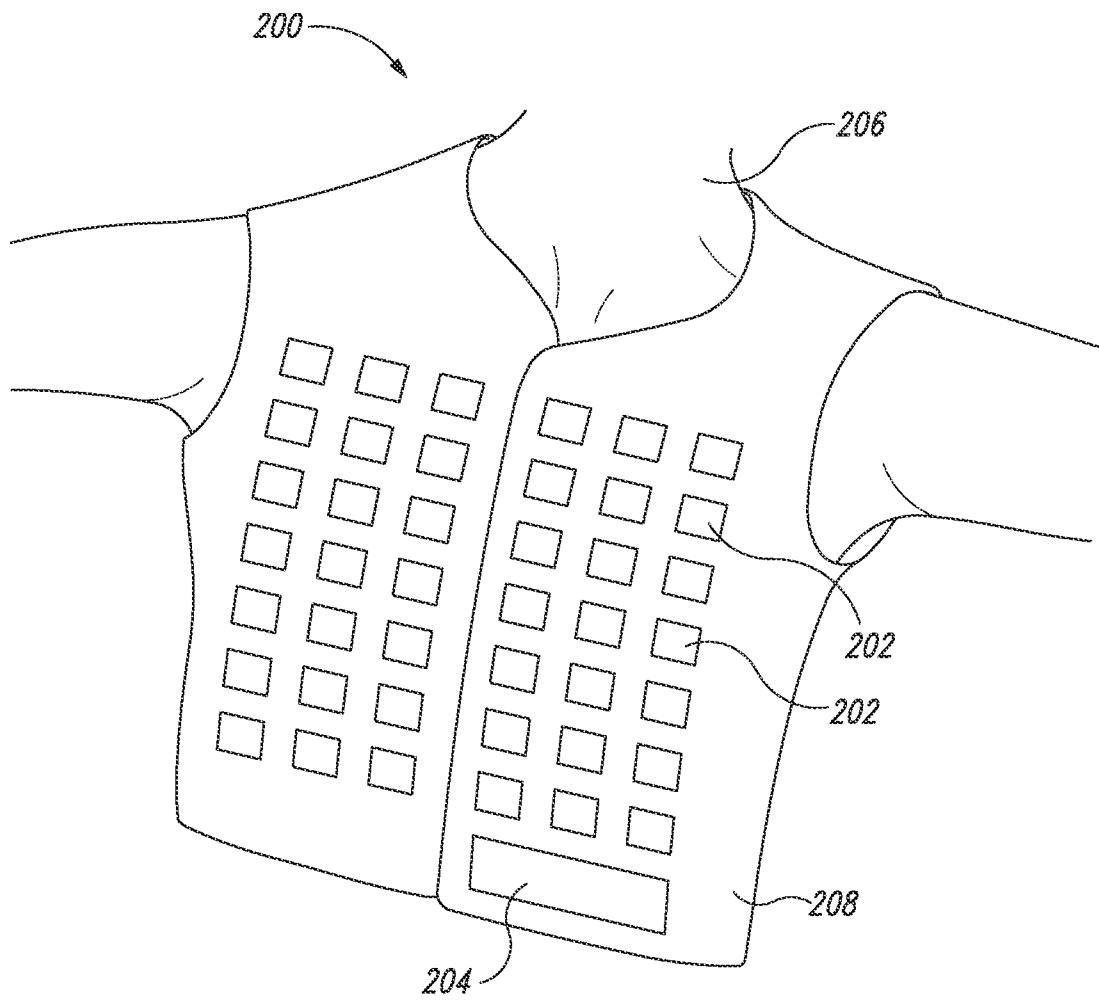
83. The method of claim 79, wherein applying a weighting includes determining an in-contact array pattern for the ultrasound sources, and the method further comprises using the determined in-contact array pattern to calculate a phase-intensity distribution profile selected to deliver a selected irradiation distribution in the body.
84. The method of claim 79, wherein applying a weighting includes adjusting a power level of a selected subset of the plurality of ultrasound sources.
85. The method of claim 84, wherein adjusting a power level includes increasing power to an ultrasound source having a superior quality of acoustic coupling with the body compared to another ultrasound source.
86. The method of claim 84, wherein adjusting a power level includes increasing power to an ultrasound source having an inferior quality of acoustic coupling with the body compared to another ultrasound source.
87. The method of claim 84, wherein adjusting a power level includes removing power to an ultrasound source having an inferior quality of acoustic coupling with the body compared to another ultrasound source.
88. The method of claim 84, wherein adjusting a power level includes maintaining a constant total energy of delivered ultrasound.
89. The method of claim 79, wherein the body is a living body.
90. The method of claim 79, wherein the body is a human body.
91. The method of claim 79, wherein applying a weighting includes deactivating at least one ultrasound source.
92. The method of claim 79, further comprising displaying an ultrasound image.
93. The method of claim 92, wherein applying a weighting includes determining whether an ultrasound image of a selected quality can be produced.

94. The method of claim 92, wherein applying a weighting includes communicating information about a quality of the displayed image.
95. The method of claim 79, wherein determining a quality of acoustic coupling with the body at each ultrasound source includes determining a quality at a succession of points in time.
96. The method of claim 95, wherein applying a weighting includes updating the weighting at a succession of points in time.

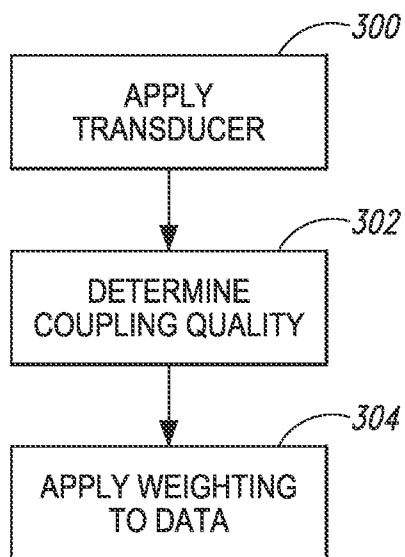
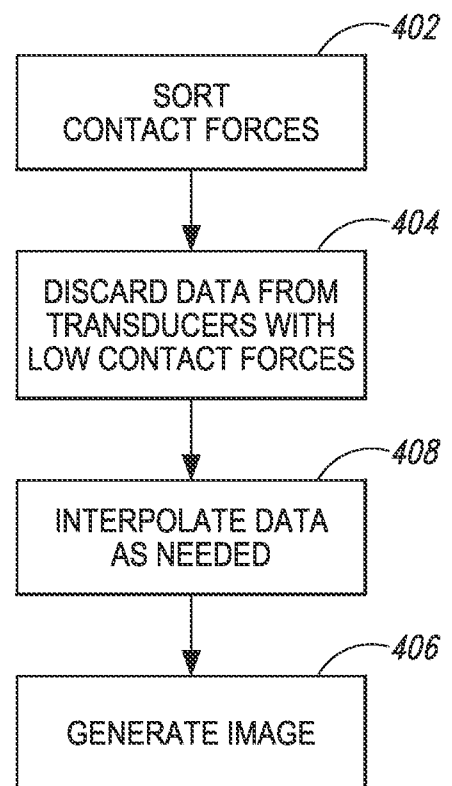
1/4

*Fig. 1*

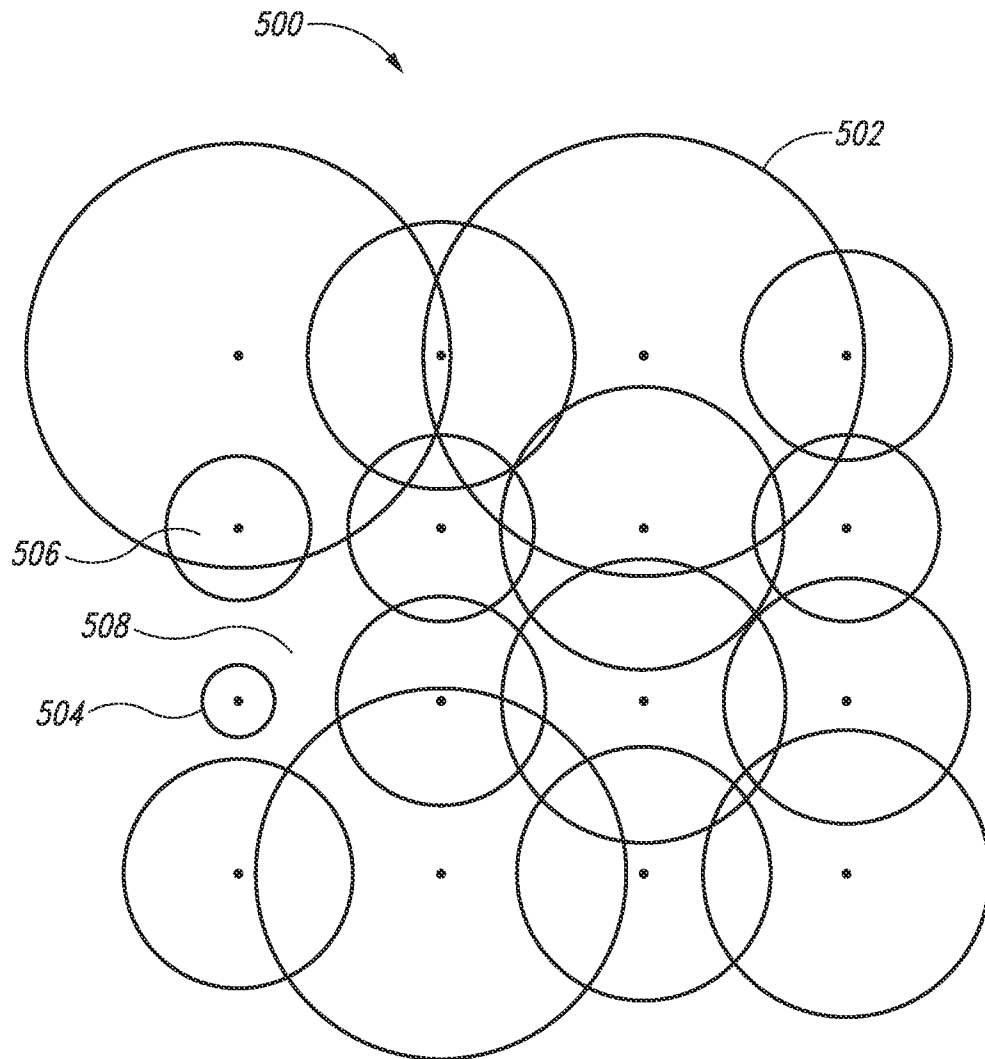
2/4

*Fig. 2*

3/4

*Fig. 3**Fig. 4*

4/4

*Fig. 5*