



US0D1069121S

(12) **United States Design Patent**
Linder et al.

(10) **Patent No.:** **US D1,069,121 S**

(45) **Date of Patent:** **** Apr. 1, 2025**

- (54) **PEDICLE SCREW**
- (71) Applicant: **Curiteva, Inc.**, Tanner, AL (US)
- (72) Inventors: **Eric Linder**, Dublin, OH (US); **Ryan Heskett**, Wellington, FL (US)

2012/0245640 A1* 9/2012 Auerbach A61B 17/7035
606/264
2015/0250512 A1* 9/2015 Poker A61B 17/7037
606/305
2015/0282843 A1* 10/2015 Spitler A61B 17/7037
606/279

(Continued)

- (73) Assignee: **Curiteva, Inc.**, Tanner, AL (US)
- (**) Term: **15 Years**

FOREIGN PATENT DOCUMENTS

KR 300710517.0000 * 10/2013

- (21) Appl. No.: **29/840,847**

OTHER PUBLICATIONS

- (22) Filed: **Jun. 1, 2022**
- (51) **LOC (15) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/171; D8/387**
- (58) **Field of Classification Search**
USPC D24/110, 143-149, 155-157, 170, 171;
D8/387
CPC A61B 17/7071; A61B 17/7073; A61B
17/7074; A61B 17/7076; A61B 17/7082
See application file for complete search history.

Prodigy Pedicle Screw System. 2024. Site visited Mar. 13, 2024.
[https://curiteva.com/products/#thoracolumbar] (Year: 2024).*

(Continued)

Primary Examiner — Wendy L Arminio
Assistant Examiner — Maheen Khurshid
 (74) *Attorney, Agent, or Firm* — Bookoff McAndrews,
 PLLC

- (56) **References Cited**

(57) **CLAIM**

The ornamental design for a pedicle screw, as shown and described.

U.S. PATENT DOCUMENTS

DESCRIPTION

- D574,958 S * 8/2008 Schendel D8/387
- D819,432 S * 6/2018 Bennett D8/387
- D856,509 S * 8/2019 Lange D24/110
- D868,967 S * 12/2019 Sauer D24/145
- D879,965 S * 3/2020 Su D24/171
- D927,295 S * 8/2021 Lanois D8/387
- 11,369,417 B1 * 6/2022 Linder A61B 17/7032
- 11,925,393 B2 * 3/2024 Giannotti A61B 17/7082
- 2005/0234451 A1* 10/2005 Markworth A61B 17/7005
606/301
- 2006/0276789 A1* 12/2006 Jackson A61B 17/7032
606/301
- 2008/0234757 A1* 9/2008 Jacofsky A61B 17/7037
606/301
- 2008/0262556 A1* 10/2008 Jacofsky A61B 17/7032
606/301
- 2011/0257690 A1* 10/2011 Rezach A61B 17/7037
606/302

FIG. 1 is a top perspective view of a pedicle screw showing our new design;
 FIG. 2 is a bottom perspective view thereof;
 FIG. 3 is a front view thereof;
 FIG. 4 is a right view thereof;
 FIG. 5 is a rear view thereof;
 FIG. 6 is a left side view thereof;
 FIG. 7 is a top view thereof; and,
 FIG. 8 is a bottom view thereof.
 The broken lines indicate portions of the pedicle screw that form no part of the claimed design.

1 Claim, 7 Drawing Sheets



(56)

References Cited

U.S. PATENT DOCUMENTS

2015/0289905 A1* 10/2015 Biedermann A61B 17/7059
606/270
2017/0049481 A1* 2/2017 Faulhaber A61B 17/1671
2018/0344357 A1* 12/2018 Berry A61B 17/7035
2019/0274738 A1* 9/2019 Heuer A61B 17/7076
2019/0290341 A1* 9/2019 Loftus A61B 17/8877
2021/0052305 A1* 2/2021 Dong A61B 17/7005
2021/0169530 A1* 6/2021 Ceravolo A61B 17/7034
2022/0280202 A1* 9/2022 Mickiewicz A61B 17/7076
2023/0293207 A1* 9/2023 Theofilos A61B 17/7049
606/270
2023/0404638 A1* 12/2023 Leff A61B 17/7032

OTHER PUBLICATIONS

Curiteva® Announces FDA Clearance of Pedicle & SI Navigation Instrument System. 2023. Site visited Mar. 13, 2024. [<https://curiteva.com/curiteva-announces-fda-clearance-of-pedicle-si-navigation-instrument-system/>] (Year: 2023).*

VTI: InterLink™ Pedicle Screw Surgical Technique. Dec. 14, 2016. Site visited Mar. 13, 2024. [<https://www.youtube.com/watch?v=i08VY5H6T8w>] (Year: 2016).*

Everest® Minimally Invasive Surgical Technique Animation. Oct. 29, 2014. Site visited Mar. 13, 2024. [<https://www.youtube.com/watch?v=vk7velTYRQw>] (Year: 2014).*

Mas Fixation Patient Education Animation. Jan. 10, 2019. Site visited Mar. 13, 2024. [<https://www.youtube.com/watch?v=LC2Y5jt9RQU>] (Year: 2019).*

* cited by examiner

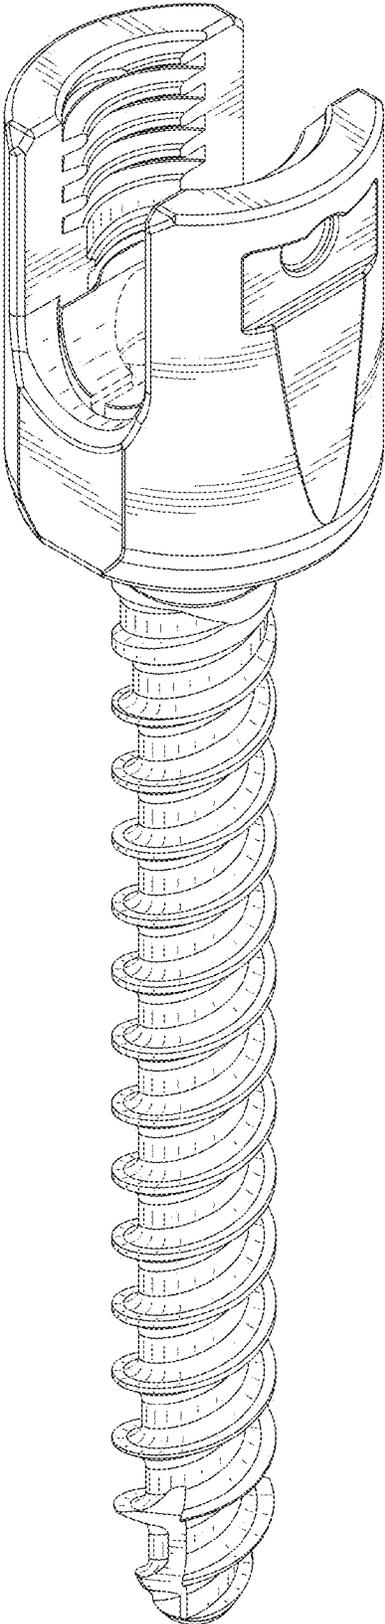


FIG. 1

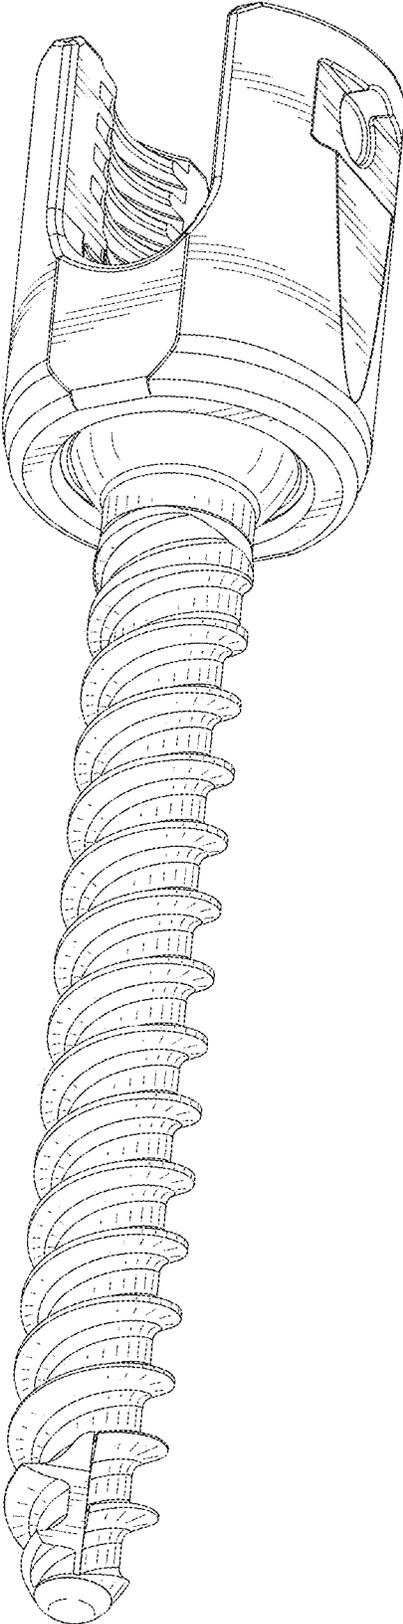


FIG. 2

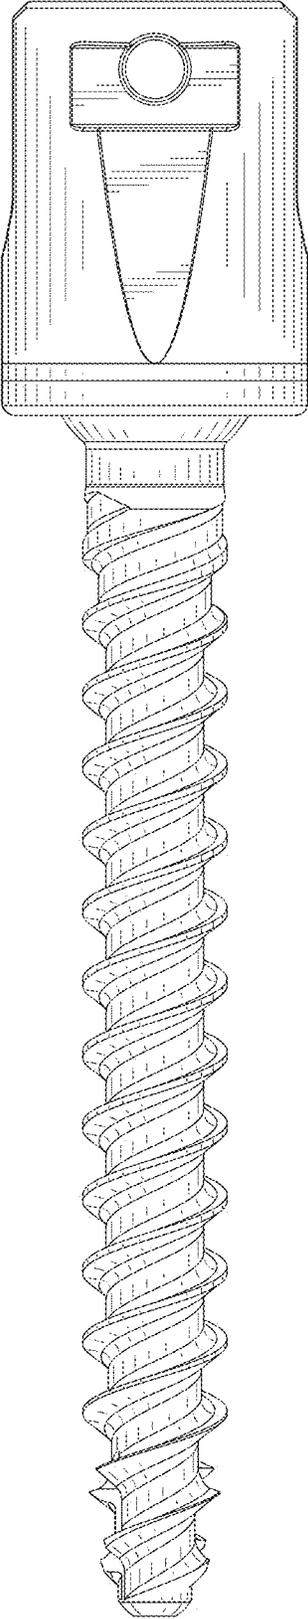


FIG. 3

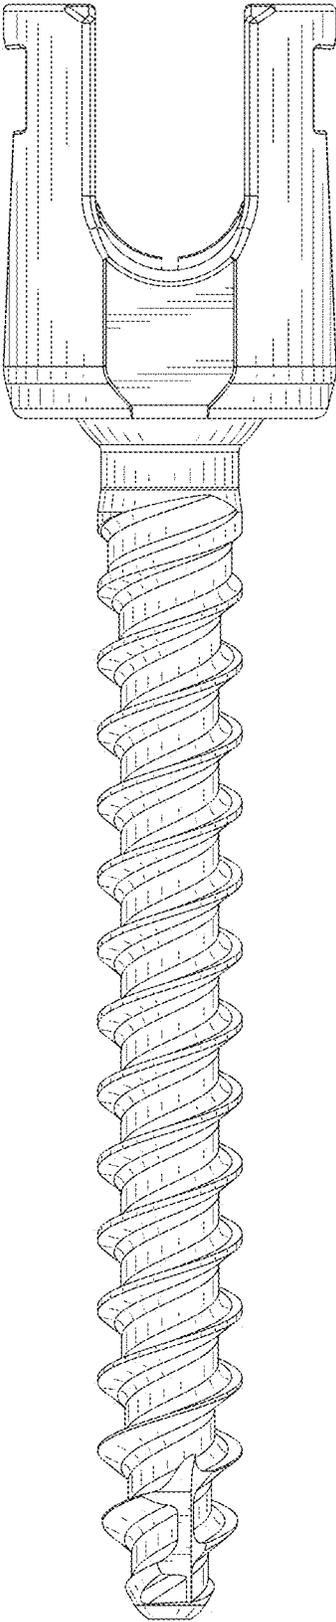


FIG. 4

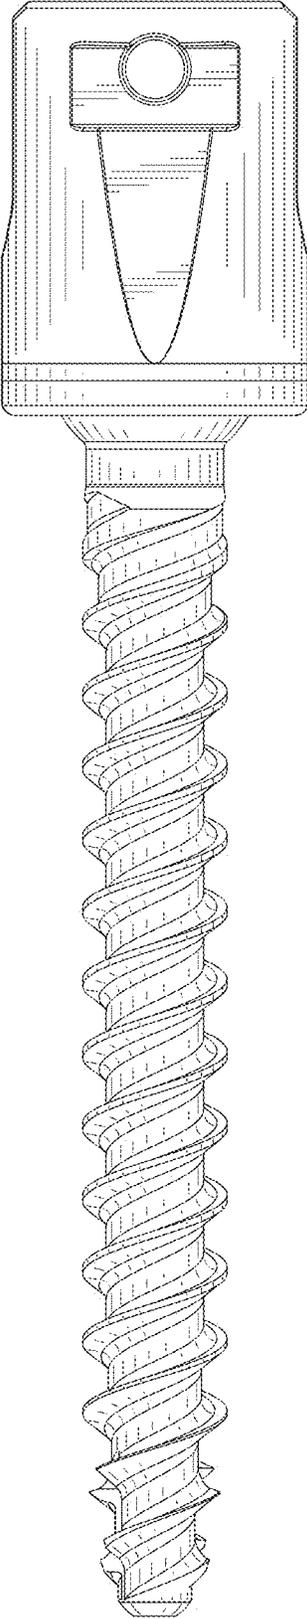


FIG. 5

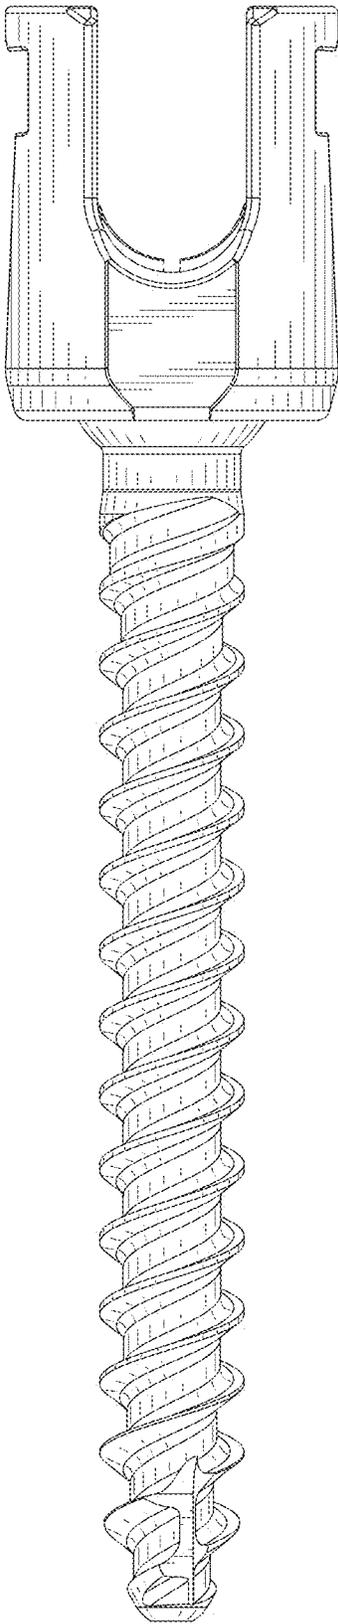


FIG. 6

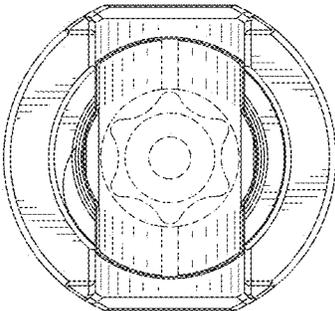


FIG. 7

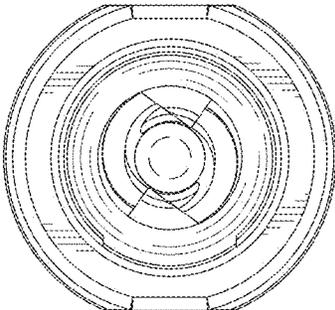


FIG. 8