


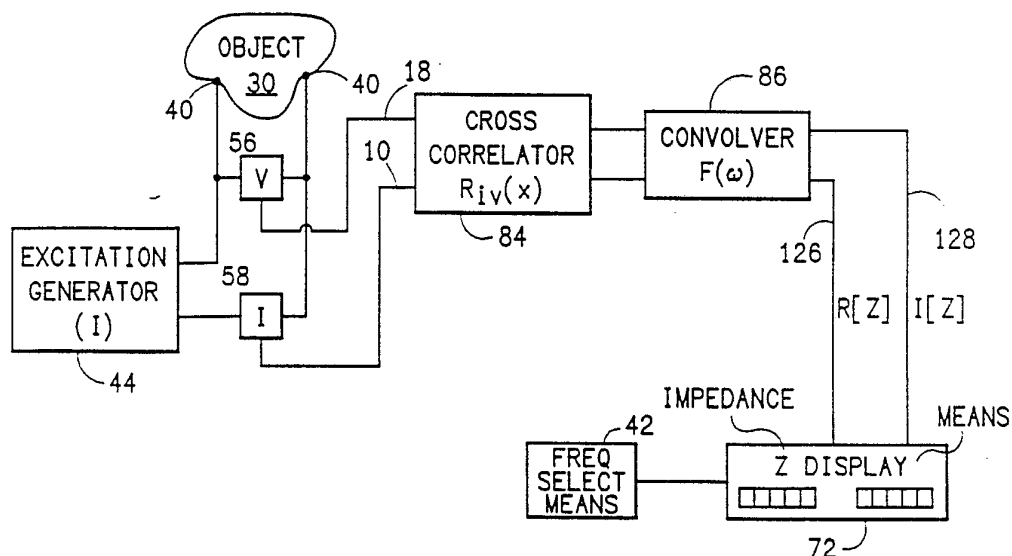

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 5 : A61B 5/04	A1	(11) International Publication Number: WO 92/19153 (43) International Publication Date: 12 November 1992 (12.11.92)
(21) International Application Number: PCT/US92/03458 (22) International Filing Date: 27 April 1992 (27.04.92) (30) Priority data: 693,364 30 April 1991 (30.04.91) US (71) Applicant: XITRON TECHNOLOGIES [US/US]; 10225 Barnes Canyon Road, Suite A102, San Diego, CA 92121 (US). (72) Inventor: WITHERS, Paul, Owen ; 5198 Alejo Street, San Diego, CA 92124 (US). (74) Agent: MARTIN, Neil, F.; Brown, Martin, Haller & McClain, 110 West "C" Street, 13th Floor, San Diego, CA 92101 (US).	(81) Designated States: AT (European patent), BE (European patent), CA, CH (European patent), DE (European patent), DK (European patent), ES (European patent), FR (European patent), GB (European patent), GR (European patent), IT (European patent), JP, LU (European patent), MC (European patent), NL (European patent), SE (European patent). Published <i>With international search report.</i>	

(54) Title: METHOD AND APPARATUS FOR DISPLAYING MULTI-FREQUENCY BIO-IMPEDANCE

**(57) Abstract**

A method and apparatus for displaying complex impedance and related physical characteristics of an object (30) at a plurality of sinusoidal frequencies over a wide frequency range. Excitation signal waveforms (10, 14, 18) are stored in digital form. Digital sampling and processing circuitry (84, 86) provide high form. Digital sampling and processing circuitry (84, 86) provide high noise immunity and accurate measurement at all impedance phase angles. The technique is particularly well-suited to the measurement of complex impedances in living biological tissue because the digital implementation results in highly accurate measurement values over a plurality of selectable frequencies within a wide sinusoidal frequency region. A novel adaptation of digital cross-correlation (84) and convolution (86) techniques is used to simultaneously display (72) real and imaginary electrical impedance of living biological tissue at several selectable sinusoidal frequencies.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCI on the front pages of pamphlets publishing international applications under the PCI.

AI	Austria	FI	Finland	MI	Mali
AL	Albania	FR	France	MN	Mongolia
BB	Barbados	GA	Gabon	MR	Mauritania
BE	Belgium	GB	United Kingdom	MW	Malawi
BF	Burkina Faso	GN	Guinea	NI	Netherlands
BG	Bulgaria	GR	Greece	NO	Norway
BJ	Benin	HU	Hungary	PL	Poland
BR	Brazil	IE	Ireland	RO	Romania
CA	Canada	IT	Italy	RU	Russian Federation
CF	Central African Republic	JP	Japan	SD	Sudan
CG	Congo	KP	Democratic People's Republic of Korea	SE	Sweden
CH	Switzerland	KR	Republic of Korea	SN	Senegal
CI	Côte d'Ivoire	LI	Liechtenstein	SU	Soviet Union
CM	Cameroon	LK	Sri Lanka	TD	Chad
CS	Czechoslovakia	LU	Luxembourg	TG	Togo
DE	Germany	MC	Monaco	US	United States of America
DK	Denmark	MG	Madagascar		
ES	Spain				

-1-

METHOD AND APPARATUS FOR DISPLAYING
MULTI-FREQUENCY BIO-IMPEDANCE

5 BACKGROUND OF THE INVENTION

1. Field of the Invention

My invention relates generally to methods for measurement
10 and display of complex sinusoidal impedance and, more
specifically, to the display of complex sinusoidal electrical
impedance in biological tissues at many frequencies.

2. Background of the Invention

15

The concept of a complex impedance for an object is well-
known in the acoustical, electrical, and mechanical arts. An
object impedance is usually defined as the ratio of a
motivating excitation divided by a resulting object response
20 at a single sinusoidal frequency, ω . For example, the complex
mechanical impedance, Z , of a structure can be expressed as
the ratio of a sinusoidal excitation force, F , to the
resulting sinusoidal velocity, V , of the structure at the
point of application of the excitation force, that is:

25
$$Z(\omega) = F(\omega, t) / V(\omega, t)$$

The complex nature of such a driving point impedance
arises from the time delay, d , of the peak sinusoidal
velocity, V , with respect to the peak sinusoidal excitation
force, F . This is commonly expressed in the following form:

-2-

$$Z = R - iX = \frac{F(e^{i\omega t})}{V(e^{i\omega t})(e^{-i\omega d})} = \frac{F}{V} e^{i\omega d}$$

or

$$Z = \frac{F}{V} (\cos \omega d + i \sin \omega d) = \frac{F}{V} \angle \omega d$$

5

Where:

ω = angular sinusoidal frequency in radians/second, and
 ωd = phase delay of V with respect to F in radians.

10 This concept of complex object impedance at a single sinusoidal frequency can be used to express a mechanical ratio of force to velocity, an acoustic ratio of pressure to displacement, an electrical ratio of voltage to current, a thermal ratio of temperature differential to heat flow, an
 15 electromagnetic ratio of electric field to magnetic field, and so forth as is well-known in the art.

The classical method known in the art for measuring and displaying values of complex object impedance requires the measurement of the response of the object to an applied
 20 excitation at a single sinusoidal frequency. For instance, the complex electrical impedance of an object can be determined by applying a sinusoidal voltage to the object and measuring the resultant sinusoidal current flow through the object. The electrical object impedance magnitude may then be
 25 determined as the ratio of the root-mean-square (RMS) voltage and current values and the object impedance phase angle may be determined as the delay in radians of the peak sinusoidal current with respect to the peak sinusoidal voltage. The real and imaginary components of the complex object impedance may
 30 be determined from impedance magnitude and phase angle according to:

-3-

Resistance = $\text{Re}[Z] = R = |Z| \cos \theta$, where $\theta = \omega d$,

Reactance = $\text{Im}[Z] = X = |Z| \sin \theta$, and

Impedance = $Z = R + iX$

A number of problems are known in the impedance measurement art that lead to errors and ambiguities when the values of complex object impedance are measured and displayed. The most significant problem arises from the requirement that the complex impedance be determined at a single sinusoidal frequency. The presence of other frequency components in the excitation and response signals lead to errors in the displayed complex impedance. Practitioners in the art have proposed analog filtering techniques and special excitation signal generation methods for minimizing the errors arising from such unwanted signal components. However, analog filter devices are subject to calibration errors, thermal drift and other problems, which introduce amplitude and phase errors in the excitation and response signals. These phase errors often become severe at high values of reactance (imaginary impedance) and can completely overwhelm the character of the complex impedance under measurement.

Other serious limitations to accurate complex impedance display are well-known in the art. High impedance magnitudes require the determination of a ratio between a large excitation signal and a very small response signal, leading to errors arising from the presence of noise in the small response signal. Practitioners propose the use of very high excitation signal amplitudes to overcome the effects of such noise, but high levels of excitation signal may damage or destroy the object to which the excitation signal is applied. This is especially problematic in cases where the object under measurement is living biological tissue.

-4-

Another problem arising from the single frequency nature of complex object impedance is the difficulty in measuring complex object impedance at several frequencies over a wide frequency range. Because signal filters are necessary to ensure sinusoidal purity, these filters must be retuned to permit impedance display at other sinusoidal frequencies. The range of frequencies over which analog filters can be retuned is very limited, often to a few octaves. Alternatively, individual signal filters can be provided for each measurement frequency, but this approach seriously limits the number of frequencies for which complex object impedance can be displayed in any particular situation.

The analog signal filtering and display components used in the art are subject to calibration drift resulting from thermal changes and variations in operating region. This problem leads to a requirement for frequent recalibration to minimize complex impedance display errors, thereby preventing the rapid and effective measurement of complex object impedance at several frequencies.

The use of balanced bridge impedance measurement techniques known in the art can overcome many of the deficiencies of the signal ratio measurement methods mentioned above. However, balanced bridge techniques require a well calibrated impedance standard and are limited in practical application to the determination and display of electrical impedances. Moreover, the standard analog bridge components are presumed to be linear with respect to signal amplitude, which is an inaccurate presumption in most applications. This presumption leads to errors in display of complex object impedance that arise with changes in excitation signal level. Finally, balanced bridge techniques are unsuitable for

-5-

accurate complex impedance determination over a wide frequency range and, in fact, are often limited to a single sinusoidal calibration frequency at a single excitation signal amplitude.

Another problem well-known in the art arises from the effects of small errors in impedance phase angle at angle values approaching $\pi/2$ radians (90°). At these phase angles, the tangent function approaches infinity and extremely small errors in phase angle cause extremely high errors in one or both of the complex impedance components. A number of clever techniques have been proposed by practitioners in the art to overcome this problem, but most rely on the thermal discrimination between real and imaginary electrical power flow in a circuit and are unsuitable for use over a range of frequencies or with nonelectrical impedance measurement.

Yet another problem with classical impedance measurement and display techniques is the difficulty in simultaneously determining impedance at widely separated frequencies. This problem arises when the object under measurement experiences changes in impedance properties as a result of the application of the excitation signal. An example of this is the well-known tendency of an object to increase in temperature in response to the application of an electrical voltage. When the complex object impedance is a function of object temperature, then the measurement of complex impedance at one frequency will heat the object and create errors in the measurement of complex impedance at another frequency because of the difficulty in measuring such impedances simultaneously. One solution is to use a plurality of impedance measurement and display devices to simultaneously measure complex object impedance at a plurality of sinusoidal frequencies, but this

-6-

method is cumbersome and not practical for large numbers of measurement frequencies.

These and other related difficulties with accurate display of complex object impedance are exacerbated in the situation where the object of interest is living biological tissue. The measurement and display of complex electrical impedance in biological tissue has been of interest since the late 1800's. By 1921 it had been well-supported that the living cell had a well-conducting interior surrounded by a relatively impermeable, poorly conducting membrane. In 1925, Fricke reported (Fricke, H., Mathematical Treatment of the Electrical Conductivity and Capacity of Disperse Systems, Phys. Rev. 26:678-681, 1925) that at low frequency (LF) currents, there was little conduction through the cell because of high membrane capacitance. Thus, Fricke argued that conduction occurs primarily in the extracellular fluid (ECF) compartment and, at a sufficiently high frequency (HF), the current is shunted through the cell membrane and conducts through both the ECF and intracellular fluid (ICF).

Knowledge of biological material properties has been obtained through complex impedance measurements across various cells, suspensions, fibers, eggs and tissues. Of primary significance were the discoveries of cell membrane capacitance, the beta dispersion region, the additional regions of dispersions for cell suspensions, and Maxwell's mixture theory for analyzing the impedance measurement data.

In general, all cells and tissues may be expected to show three major dispersion regions in relation to frequencies (α , β and γ). Of particular interest is the central β -dispersion region, which is explained by the dielectric capacity of the cell membranes. The α and γ regions are attributed to a

-7-

surface conductance and to intracellular components. The β region can be expressed in either a simple or complex equivalent circuit orientation form, where parallel resistance (R_p) reflects extracellular fluid (R_{ecw}) and the series orientation corresponds to intracellular fluid resistance (R_{icw}) and cell membrane capacitance (C_M). The equivalent circuit used in the Maxwell analysis must give the semi-circular relation (impedance and admittance loci) between the real and imaginary components of the impedance as applied frequency is varied, according to Cole (Cole, K.S., Membrane, Ions and Impulses, University Press, Berkeley, 1968).

An early attempt to apply this concept was made by Thomasset (Thomasset, A., Bio-electrical Properties of Tissues, Lyon Med. 209:1325-1352, 1963), who measured simple impedance at high (100kHz) and low (1kHz) frequency currents using a two-wire technique. The high correlations of high frequency impedance to total body water (TBW) and low frequency impedance to extracellular fluid gave further support to the membrane and dispersion theories. However, Thomasset's approach did not develop into a practical clinical method.

Using a four-wire configuration, Hoffer, et al. (Hoffer, E., Meador, C., Simpson, C., Correlation of Whole-Body Impedance with Total Body Water Volume, J. Appl. Physio. 17, 4:531-534, 1969) reported a high correlation between measured TBW and TBW estimated by $Ht^2/Resistance$ at 100kHz. However, Hoffer, et al. reported that their high standard deviations implied that further development was necessary to make the technique a practical clinical method.

A decade later, Nyboer, et al. (Nyboer, J., Liedtke, Reid, K., Gesert, W., Nontraumatic Electrical Detection of

-8-

Total Body Water and Density in Man, Proceedings of the VI ICEBI, 381-384, 1983) found that measurements of electrical resistance at 50KHz, combined with subject weight, height and age, could accurately determine body density (fat and lean) in human subjects. These relationships were based on the assumption that a strong relationship must exist between Fat-Free Mass (FFM) and TBW estimated by impedance because FFM tissue is consistently hydrated. Following the Nyboer, et al. work, a tremendous amount of interest arose for the impedance method.

Since the Nyboer, et al. presentation, many practitioners have sought to validate the single frequency impedance method of estimating human body composition in various populations (Lukaski, H.C., Johnson, P.E., Bolonchuk, W.W., Lykken, G.I., Assessment of Fat-Free Mass Using Bioelectrical Impedance Measurements of the Human Body, Am. J. Clin. Nutr., 41:810-817, 1985; Segal, K., Van Loan, M., Fitzgerald, P., Hodgdon, J.A., Van Itallie, T.B., Lean Body Mass Estimation by Bioelectrical Impedance Analysis: a Four Site Cross-Validation Study, Am. J. Clin. Nutr. 47:7-14, 1988; and Kushner, R., Kunigk, A., Alspaugh, M., Andronis, P., Leitch, C., Schoeller, D., Validation of Bioelectrical-Impedance Analysis as a Measurement of Change in Body Composition in Obesity, Am. J. Clin. Nutr. 52:219-23, 1990). Results have been mostly positive for normal subjects but the predictions of FFM have been far less precise in the clinical and abnormal population groups. Although impedance data continued to correlate highly to TBW, the underlying assumption that FFM is consistently hydrated has recently been found to be incorrect (Deurenberg, P., Weststrate, J.A., Hautvast, J., Changes in Fat-Free Mass During Weight Loss Measured by Bioelectrical

-9-

Impedance and by Densitometry, Am. J. Clin. Nutr. 49:33-6, 1989). Furthermore, increased awareness of the usefulness of the multi-frequency measurements has led to a general belief that the single frequency method is too simplistic and limiting (Cohn, S., How Valid are Bioelectrical Impedance Measurements in Body Composition Studies?, Am. J. Clin. Nutr. 42:889-890, 1985). Criticism was also raised over the clinical usefulness of TBW in view of frequently encountered fluid shifts between the ICW and ECW. Van Itallie, et al. (Van Itallie, T., Segal, K., Nutritional Assessment of Hospital Patients: New Methods and New Opportunities, Am. J. Hum. Bio 1:205-8, 1989) assert that a practical method of discerning the ICW from the extracellular fluid would offer much greater utility and could profoundly influence hospital patient care and diagnosis.

Recently, several practitioners (Lukaski, H.C., Bolonchuck, W.W., Estimation of Body Fluid Volumes Using Tetrapolar Bioelectrical Impedance Measurements, Aviat. Space Environ. Med. Dec., 1163-69, 1988 and McDougall, D., Shizgal, H., Body Composition Measurements from Whole Body Resistance and Reactance, Surgical Forum, 36:43-44, 1986) have proposed using the reactive element in a complex single frequency (50kHz) impedance measurement to accurately discriminate the extracellular from the cellular mass. However, the use of multi-frequency measurements of impedance remains the technique of choice (Boulier, A., Fricker, J., Thomasset, A.L., Apfelbaum, M., Fat-Free Mass Estimation by Two-Electrode Impedance Method, Am. J. Clin. Nutr. 52:581-5, 1990).

Several practitioners have continued to test the Thomasset technique (Jenin, P., Lenoir, J., Roullet, C., Thomasset, A., Ducrot, H., Determination of Body Fluid

-10-

Compartments by Electrical Impedance Measurements, Aviat. Space Environ. Med. 46:152-5, 1975; Settle, R.G., Foster, K.R., Epstein, B.R., Mullen, J.L., Nutritional Assessment: Whole Body Impedance and Body Fluid Compartments, Nutr. Cancer, 2:72-80, 1980; and Tedner, B.T., Equipment Using an Impedance Technique for Automatic Recording of Fluid-Volume Changes During Hemodialysis, Med. & Biol. Eng. & Comput. 21:285-290, 1983). These practitioners use the ratio of high to low frequency simple impedance to reflect fluid compartment volume, the normal and abnormal fluid ratio, and fluid compartment change. The major problem reported for this technique is that the simple HF/LF ratio is too simplistic because volume is not determined and the compartment actually affected is not identified, although a change in ratio does reflect a change in compartmental volume. Furthermore, practitioners note that the lack of two-frequency simple impedance instrumentation prevents further exploration of this approach.

Because living tissue is mainly affected by ECF at frequencies below the β -dispersion region, and ECF, C_M and ICF at frequencies above this region, Kanai, et al. (Kanai, H., Haeno, M., Sakamoto, K., Electrical Measurements of Fluid Distribution of Legs and Arms, Med. Prog. Tech. 12:159-170, 1987) computed the component values of the human muscle tissue equivalent circuit model (R_{ccw} , R_{icw} , and C_M) known in the art. By mathematically analyzing the complex impedance measurements at multiple frequencies, Kanai, et al. obtained information specific to the ECW and ICW. However, others have been unable to replicate this advanced approach because of the lack of necessary and appropriate complex impedance instrumentation.

-11-

Expanding the prior art human body composition model from a simple two-compartment (lean/fat) model to a more complex model including ICF and ECF, protein, mineral and fat, creates a clearly-felt need for new and improved assessment techniques. This need has been unmet, until now because of the lack of appropriate complex impedance instrumentation and the lack of the necessary degree of sophistication in the associated measurement and analysis methods. This situation has inhibited the progress of this promising technology.

Increased use of diuretic drugs, fluid monitoring difficulties in intensive care, and the shrinking cell mass and expanding ECF that accompany most systemic wasting diseases and malnutrition has led to a well-recognized need for effective multi-frequency bioimpedance instrumentation in support of the compartmental approach to body fluid assessment. These unresolved problems and deficiencies are clearly felt in the art and are solved by my invention in the manner described below.

SUMMARY OF THE INVENTION

My invention is a method and apparatus for the simultaneous determination and display of complex electrical bio-impedance at several frequencies. Although I teach primarily the application of my invention to the display of multi-frequency electrical bio-impedance, my invention is also readily applicable to the determination and display of complex impedances for many other types of objects, including other impedances such as mechanical, acoustic and the like. This can be appreciated by recognizing that my invention determines and displays complex object impedance by treating an

-12-

excitation signal and a response signal as two independent functions in the time domain. Because of this view, I can apply certain signal processing techniques to the two independent time domain signals to obtain results in a manner previously unsuspected in the art.

The first such signal processing concept that I use is the creation of a complex cross-correlation signal as a function of time delay, τ , between the excitation, e , and response, r , signals. My complex cross-correlation function, $R_{er}(\tau)$, can be developed from the integral over time of the product of the two excitation and response signals where the response signal is delayed by time τ with respect to the excitation signal.

The second signal processing concept that I use is the complex Fourier transform, F , of the cross-correlation signal, $R_{er}(\tau)$. The Fourier transform of $R_{er}(\tau)$ is $F(R_{er})$, which is a signal in the frequency domain having a complex value at each angular frequency ω that is proportional to the complex object impedance.

Following the conversion of the two excitation and response signals to an intermediate cross-correlation signal and a final Fourier transform signal, I display the complex object impedance as a function of frequency over a predetermined range. My cross-correlation signal and Fourier transform signals are both complex because they exhibit amplitude and phase information at each point in the time delay and frequency domains, respectively.

My application of these simple signal processing techniques for the conversion of time domain signals to frequency domain signals can be embodied in an apparatus using either analog or digital electronic components. An

-13-

advantage of my preferred embodiment is that my use of digital components leads to improved storage and processing accuracy and minimizes the effects of analog component calibration drift. I have also discovered that the development of a
5 complete cross-correlation signal, $R(\tau)$, over a large time-delay region and the subsequent development of a Fourier transform signal, $F(\omega)$, over a broad frequency region, while possible, is not the most useful embodiment of my invention. Accordingly, I have refined this elementary convolution
10 approach by adding the following improvements.

First, I use an electrical current for the excitation signal instead of the electrical voltage normally used in the art. The constant current excitation signal prevents unsuspected hazards to living biological tissues because the
15 biological hazards are more closely related to current levels than to voltage levels as is known in the medical art. Secondly, I make use of a series of stored digital data to define the excitation current waveform precisely. By precisely defining the excitation current waveform, I can
20 create and apply a single-frequency excitation current to the living biological object under measurement. Conversion of two such single-frequency excitation and response signals to a cross-correlation signal results in a sinusoidal cross-correlation signal having an amplitude and phase
25 representative of the complex cross-correlation between the excitation and response signal. Moreover, the Fourier transform of such a sinusoidal cross-correlation signal is a single impulse function at the point in the frequency domain equivalent to the single frequency of the initial excitation
30 and response signal.

-14-

These observations are particularly useful because they result in simplification of my signal and convolution conversion process to a simple signal multiplication procedure in quadrature. That is, the complex object impedance at a single frequency can be developed from the excitation and response signals in the time domain by a multiplication and integration process in quadrature. This quadrature signal conversion method is the preferred embodiment of my invention because of the relatively simple apparatus necessary.

A potential problem with my quadrature technique is that a different excitation waveform is required for each sinusoidal frequency value at which complex object impedance must be displayed. I have resolved this problem by providing for the storage of a plurality of excitation waveforms in a signal generator digital memory means so that the excitation signal can be quickly stepped through a variety of sinusoidal frequencies merely by selecting the necessary waveform data from the memory device in the desired sequence. The excitation current is then produced from the stored digital data and the analog response voltage developed across the object under measurement is sensed. Moreover, network analyzer means may be added to compute and display a plurality of equivalent circuit elements from a similar plurality of complex impedance data obtained at the different sinusoidal frequencies stored in my digital signal generator memory means.

For ease of implementation and minimization of measurement and display errors, I prefer to perform all signal conversions using digital means. Accordingly, in my preferred embodiment, the response and excitation signals are converted to digital form by sampling means and the multiplication of

-15-

the two excitation response signals in the time domain is performed using digital multiplication means. The real or resistive component of the complex object impedance is related to a first impedance signal expressed as the arithmetic
5 average of the products of a series of simultaneous samples of the excitation signal and response signal. The imaginary or reactive component of the complex object impedance is related to a second impedance signal, expressed as the arithmetic average of a series of products of simultaneous samples of the
10 response signal and a delayed excitation signal, where the delay is precisely equal to $\pi/2$ radians or one-fourth cycle of the sinusoidal waveform representing the frequency at which the complex object impedance is determined.

By using digital sampling techniques and synchronizing
15 the sampling windows of the excitation and response signals, the implementation of my preferred embodiment is simplified and the signal conversion process made more robust (resistant to noise and calibration errors). It is not necessary to independently sample the excitation current waveform because
20 this waveform is developed from digital samples stored in a digital memory device and these samples can be used directly in the quadrature multiplication process. However, I prefer to independently sample the analog excitation current waveform at the point where it is applied to the biological object for
25 two reasons. First, this simplifies the synchronization of the sampling windows for the two excitation and response signals. Secondly, this avoids errors arising from unexpected changes in the excitation signal between the memory storage means and the point of application to the object under
30 measurement.

-16-

One of the advantages of my invention is that complex bio-impedance can be measured almost simultaneously at a plurality of frequencies in a wide frequency region. Another advantage of my invention is that a change in the sinusoidal
5 excitation signal frequency can be achieved without changing analog circuit paths or component values. This minimizes the errors arising from component calibration errors. An objective of my invention is to avoid complex impedance errors arising from nonlinearities in the object under measurement.

10 Yet another advantage of my invention is the rejection of noise effects over a broad frequency range without the use of analog filter techniques. It is another object of my invention to accurately display the complex object impedance phase at all phase values from -90° to $+90^\circ$. Another
15 advantage of my invention is that a variety of calibration factors may be readily applied to the displayed results by using digital techniques known in the art.

An important objective of my invention is to permit the measurement of bio-impedance at a plurality of frequencies in
20 as little as two cycles of the primary frequency waveform. Another important advantage of my invention is that my time series convolution process eliminates most errors that otherwise arise from the undesired presence of random noise in the relevant signals.

25 The foregoing, together with other features and advantages of my invention will become more apparent when referring to the following specifications, claims and the accompanying drawings.

-17-

BRIEF DESCRIPTION OF THE DRAWINGS

For a more complete understanding of my invention, reference is now made to the following detailed description of the embodiments illustrated in the accompanying drawings wherein:

Figure 1, comprising Figures 1(a) through 1(h), shows a series of waveforms in the time domain exemplifying the excitation signal, delayed excitation signal, response signal, first and second impedance signals and the related series of digital samples;

Figure 2, comprising Figures 2A and 2B, illustrates a method for applying an excitation signal to an object and detecting a resulting response signal and shows a typical equivalent circuit representation of a living cell;

Figure 3 is an illustrated embodiment of an apparatus for measuring and displaying the complex impedance of an object;

Figure 4 is an illustrated embodiment of the signal generating means from Figure 3; and

Figure 5 is an illustrated embodiment of an apparatus that uses my more general convolution method to display the complex impedance of an object over a region in the frequency domain.

DESCRIPTION OF THE PREFERRED EMBODIMENT

Figure 1 illustrates the typical waveform characteristics for the excitation and response signals used in my invention for displaying complex object impedance. Figure 1A shows an excitation signal current that varies in amplitude sinusoidally with time in the manner shown. Figure 1B shows

-18-

the resulting series of excitation pulses or samples 12 that represent current 10 samples made at a predetermined sampling rate. This predetermined sampling rate should be high enough (as seen from the Nyquist criteria, known in the art) to avoid losing significant phase and amplitude information contained in current 10. Figure 1C illustrates a delayed excitation signal current 14 that is identical to current 10 except for a time delay of $\pi/2$ radians or one-quarter cycle of the sinusoidal waveform. Figure 1D illustrates a series of delayed excitation pulses or samples 16 that represent current waveform 14 samples taken in synchronism with excitation current samples 12.

In operation, my invention uses excitation signal current 10 to excite a living biological tissue sample and I then monitor the sample for a response signal voltage waveform 18 shown in Figure 1E. Response signal voltage 18 may contain several sinusoidal frequency components, but the fundamental sinusoidal frequency of signal current 10 will predominate. Figure 1F illustrates a series of response voltage samples 20 that are taken in synchronism with samples 12 and 16.

Figures 1G and 1H illustrate the first impedance samples 22 and second impedance samples 24, respectively. Sample 22 is obtained by multiplying the concurrent values of sample 12 and sample 16 ($I_n V_n$), either by analog or digital means. Sample 24 is obtained by multiplying concurrent values of delayed excitation sample 16 and response voltage sample 20 ($I_{90n} V_n$). Figure 1G shows a first mean impedance signal 26 representing the long term arithmetic average of impedance samples 22. Similarly, Figure 1H shows a second mean impedance signal 28 representing the long term arithmetic average of samples 24.

-19-

While I believe that my invention is useful for determining many different types of impedances, including thermal, mechanical, acoustical and so forth, I limit my discussion herein to my preferred application, which is the measuring of complex electrical impedances of living biological tissues. Figure 2A illustrates the fundamental arrangement required to measure and display complex electrical impedance of an object 30. Excitation signal current 10 is applied to object 30 and response signal voltage 18 is monitored.

Figure 2B illustrates a useful equivalent circuit model for the living human cell 32 proposed by Kanai, et al., cited above. Cell model 32 comprises three lumped constant RC circuits 34, 36 and 38. RC circuit 34 represents the cell membrane capacitance and cell membrane resistance. RC circuit 36 represents the intracellular fluid capacitance and resistance. RC circuit 38 represents the extracellular fluid capacitance and resistance.

Human cell equivalent circuit 32 presents a single complex impedance to the pair of terminals 40 at any single sinusoidal frequency. Accordingly, the six lumped-constant model elements can be determined only from impedance data at six (or more) different sinusoidal frequencies by means of a critically-or over-determined system of linear equations as known in the art.

As discussed above, I prefer to use a simplified signal multiplication procedure in quadrature to determine complex object impedance. This signal multiplication procedure was introduced and described in connection with Figure 1, wherein first and second mean impedance signals 26 and 28 represent real and imaginary components ($\text{Re}[Z]$, $\text{Im}[Z]$). Figure 3 shows

-20-

a functional implementation of my invention, including the necessary means for determining a plurality of equivalent circuit element values such as described in Figure 2B for human cell 32. These equivalent circuit analyzer elements are
5 shown connected by dotted lines in Figure 3, and are further described below.

A frequency selection means 42 may comprise front panel switch controls, digital memory means or other related devices suitable for selecting one or more sinusoidal operating
10 frequencies. Each selected frequency is passed to a signal generator means 44 and also to an impedance analyzer memory means 46. Impedance analyzer memory means 46 merely receives the frequency selection and stores it in memory for later use with concurrent complex body impedance data. Signal generator
15 means 44 preferably comprises a frequency sequencing means 48, a frequency memory means 50 and a generator memory means 52 as shown in Figure 4. Frequency sequencing means 48 selects from among a plurality of operating frequencies stored in memory means 50 and 52. Frequency memory means 50 provides the
20 necessary clocking pulses to generator memory means 52, which then provides a train of excitation current pulses making up a sinusoidal excitation current in response to the commands received from frequency sequencing means 48 and frequency memory means 50.

25 Returning to Figure 3, a current limiting means 54 is interposed in series with excitation current samples 12 to prevent the excitation current amplitude from exceeding biologically safe levels. Excitation current samples 12 are then imposed on object 30 at terminals 40 and a response
30 detector means 56 is connected across terminals 40 to measure response signal voltage 18.

-21-

First and second analog-to-digital (A/D) conversion means 58 and 60 serve to convert excitation signal current 10 and response signal voltage 18 from analog form to digital form in a manner known in the art. The operation of A/D means 58 and 60 is synchronized with the operation of signal generator means 44 by clocking means (not shown) to ensure that the leading and lagging edges of the digital pulses created by the three circuits are synchronous in time to within less than one microsecond.

The output of first A/D means 58 presents excitation samples 12 to the input of a quadrature delay means 62 and the first input of a first multiplier means 64. The output of second A/D means 60 presents response samples 20 to the second input of first multiplier means 64 and the first input of a second multiplier means 66. The output of quadrature delay means 62 provides delayed excitation samples 16 that represent a digital embodiment of delayed excitation signal current 14 discussed in connection with Figure 1. Delayed excitation signal current 14 lags excitation signal current 10 by precisely one-fourth of a waveform cycle at the fundamental sinusoidal operating frequency. Delayed excitation samples 16 from quadrature delay means 62 are presented to the second input of second multiplier means 66.

The output of first multiplier means 64 provides a series of pulses equal to the series of products of concurrent excitation samples 12 and response samples 20, which we have named first impedance samples 22 in Figure 1. Similarly, the output of second multiplier means 66 provides a series of pulses named second impedance samples 24, which is the series of products of concurrent delayed excitation samples 16 and response samples 20. First impedance samples 22 are presented

-22-

to a first averaging means 68 and second impedance samples 24 are presented to a second averaging means 70. The outputs from first and second averaging means 68 and 70 comprise first and second mean impedance signals 26 and 28 as discussed above in connection with Figure 1. Signals 26 and 28 are exactly proportional to the real and imaginary components of the complex electrical impedance of object 30. Signals 26 and 28 are presented to impedance display means 72, which is preferably a multi-digit LCD numerical display or other suitable display means known in the art.

The calibration means 74 comprises circuitry that produces a current calibration signal 76 and a voltage calibration signal 78 for use in adjusting impedance display means 72 in response to independent calibration of excitation signal current 10 and response signal voltage 18.

Impedance display means 72 also presents the complex impedance of object 30 to impedance analyzer memory means 36 for storage together with the relevant sinusoidal frequency value presented by signal frequency selection means 42. These data are stored in impedance analyzer memory means 46 for use in computing a plurality of lumped constant equivalent circuit elements as discussed above in connection with Figure 2. These equivalent circuit elements are computed and displayed by means of a network analyzer means 80 and an equivalent circuit display means 82 disposed substantially as shown in Figure 3. Network analyzer means 80 acts to solve a system of linear equations for a plurality of equivalent circuit elements from a plurality of complex impedance and operating frequency data pairs in any suitable digital or analog manner known in the art for solving linear systems of equations. The resulting equivalent circuit element values are then presented

-23-

by network analyzer means 80 to equivalent circuit display means 82 for display in any suitable manner known in the art for displaying data.

Although I prefer the simple digital quadrature
5 multiplication and integration process discussed above, I also show in Figure 5 the use of a cross-correlator means 84 and a convolver means 86 accomplish a similar result in lieu of the apparatus disclosed in Figure 3. The effect of cross-correlation of signals 18 and 10 followed by convolution of
10 the cross-correlation function $R_{vv}(\tau)$ shown in Figure 5 was briefly discussed above and is further treated in detail by K. G. Beauschamp and C. Yuen, Digital Methods for Signal Analysis, George Allen & Unwin, Ltd, London, 1979. The applications of these digital signal processing techniques to
15 the measurement of complex body impedance is suggested herein for the first time. Note that the two outputs 126 and 128 from convolver 86 contain complex impedance data over the entire frequency domain and impedance display means 72 can be configured to display impedance data at a single frequency in
20 response to an input from frequency selection means 42.

Obviously, other embodiments and modifications of my invention will occur readily to those of ordinary skill in the art in view of these teachings. Therefore, my invention is to be limited only by the following claims which include all such
25 obvious embodiments and modifications when viewed in conjunction with the above specification and accompanying drawings.

I CLAIM:

-24-

CLAIMS

1. A method for displaying the complex impedance of an object at a sinusoidal frequency comprising the steps of:
 - selecting a sinusoidal frequency value;
 - selecting a first sampling rate no less than 400% of said sinusoidal frequency;
 - selecting a second sampling rate no less than first said sampling rate;
 - generating a series of excitation pulses at said first sampling rate to form an excitation signal comprising a component at said sinusoidal frequency having a predetermined magnitude;
 - applying said excitation signal to said object;
 - detecting a response signal comprising the response of said object to said applied excitation signal;
 - sampling said excitation signal at said second sampling rate to form a series of excitation samples;
 - sampling said response signal at said second sampling rate in synchronism with said excitational sampling step to form a series of response samples;
 - delaying said excitation samples by a delay time substantially equal to one-fourth cycle of said sinusoidal frequency to form a series of delayed excitation samples;
 - multiplying each said excitation sample by the simultaneous said response sample to form a first impedance sample;
 - multiplying each said delayed excitation sample by the simultaneous said response sample to form a second impedance sample;

-25-

30 averaging said first and second impedance samples over
time to form first and second mean impedance signals,
respectively; and

32 displaying said first and second mean impedance signals
to represent said complex object impedance.

2. The method described in Claim 1 wherein:

2 said complex impedance comprises the electrical impedance
of said object; and

4 said sinusoidal excitation signal comprises an electrical
current of substantially invariant sinusoidal magnitude.

3. The method described in Claim 2 wherein:

2 said first sampling rate is equal to said second sampling
rate and said first and second sampling steps are synchronized
4 with said generating step.

4. The method described in Claim 2 wherein said object

2 comprises living biological tissue.

5. A method for displaying the complex impedance of an
2 object over a range of sinusoidal frequencies comprising the
steps of:

4 selecting a first sampling of no less than 400% of the
maximum said sinusoidal frequency;

6 selecting a second sampling rate no less than said first
sampling rate;

8 generating a series of excitation pulses at said first
sampling rate to form an excitation signal;

10 applying said excitation signal to the object;

-26-

12 detecting a response signal comprising the response of
said object to said applied excitation signal;

14 sampling said excitation signal and said response signal
in synchronism at said second sampling rate to form a series
of synchronous excitation samples and response samples,
16 respectively;

18 computing the complex cross-correlation of said series of
excitation samples and said series of response samples over a
predetermined time delay region;

20 computing the real and imaginary components of the
Fourier transform of said complex cross-correlation over said
22 range of sinusoidal frequencies to form first and second
impedance signals, respectively;

24 computing the square of the magnitude of the Fourier
transform of said excitation signal over said range of
26 sinusoidal frequencies to form a calibration signal;

28 displaying the ratios of said first and second impedance
signals to said calibration signal to represent said complex
object impedance over said range of sinusoidal frequency.

6. The method described in Claim 5 wherein:

2 said first sampling rate is equal to said second sampling
rate and said first and second sampling steps are synchronized
4 with said generating step.

7. The method described in Claim 5 wherein:

2 said object comprises living biological tissue.

8. An apparatus for measuring and displaying the complex

2 impedance of an object comprising:

-27-

frequency selection means for selecting at least one
4 sinusoidal frequency;

signal generating means for creating an excitation signal
6 comprising a sinusoidal component at said selected sinusoidal
frequency;

8 response detection means for detecting a response signal
arising in said object in response to application of said
10 excitation signal;

quadrature delay means for delaying said excitation
12 signal by a predetermined time period to create a delayed
excitation signal;

14 first multiplier means for multiplying said excitation
signal and response signal to form a first impedance signal;

16 second multiplier means for multiplying said delayed
excitation signal and response signal to form a second
18 impedance signal;

first averaging means for averaging said first impedance
20 signal over time to form a first mean impedance signal;

second averaging means for averaging said second
22 impedance signal over time to form a second mean impedance
signal; and

24 display means for displaying said first and second mean
impedance signals to represent said complex object impedance
26 at said selected sinusoidal frequency.

9. The apparatus described in Claim 8 further
2 comprising:

frequency memory means for storing a plurality of
4 selected sinusoidal frequencies; and

frequency sequencing means for stepping through said
6 plurality of sinusoidal frequencies and sequentially

-28-

displaying said complex object impedance for each said
8 sinusoidal frequency in turn.

10. The apparatus described in Claim 9 further
2 comprising:

calibration means for adjusting said first and second
4 mean impedance signals in accordance with variations in
excitation signal magnitude.

11. The apparatus described in Claim 8 wherein:
2 said sinusoidal frequency generating means, said
response detection means, said delay means and said first and
4 second multiplier means comprise digital electronic logic
means.

12. The apparatus described in Claim 11 wherein:
2 said display means comprises digital display means for
displaying numerical values of said complex body impedance.

13. The apparatus described in Claim 11 further
2 comprising:

frequency memory means for storing a plurality of
4 selected sinusoidal frequencies; and

frequency sequencing means for stepping through said
6 plurality of sinusoidal frequencies and sequentially
displaying said complex object impedance for each said
8 sinusoidal frequency in turn.

-29-

14. The apparatus described in Claim 13 further
2 comprising:

generator memory means for storing a plurality of digital
4 words representing said excitation signal; and

digital-to-analog conversion means for converting said
6 digital words to an analog excitation signal.

15. The apparatus described in Claim 14 wherein:

2 said response detection means comprises analog-to-
digital conversion means for sampling said response signal to
4 form a series of response samples.

16. The apparatus described in Claim 15 wherein:

2 said excitation signal comprises a sinusoidal electrical
current and said response signal comprises a sinusoidal
4 electrical voltage.

17. The apparatus described in claim 16 wherein:

2 said object comprises living biological tissue.

18. The apparatus described in Claim 17 further
2 comprising:

current limiting means for limiting said excitation
4 signal current to a value that will cause no harm when applied
to said living biological tissue.

19. An apparatus for measuring and displaying at least
2 one equivalent circuit component arising from a theoretical
model of living biological tissue comprising:

-30-

4 frequency selection means for selecting at least one
sinusoidal frequency;

6 signal generating means for creating an excitation signal
comprising a sinusoidal component at said selected sinusoidal
8 frequency;

response detection means for detecting a response signal
10 arising in said object in response to application of said
excitation signal;

12 quadrature delay means for delaying said excitation
signal by a predetermined time period to create a delayed
14 excitation signal;

first multiplier means for multiplying said excitation
16 signal and response signal to form a first impedance signal;

second multiplier means for multiplying said delayed
18 excitation signal and response signal to form a second
impedance signal;

20 first averaging means for averaging said first impedance
signal over time to form a first mean impedance signal;

22 second averaging means for averaging said second
impedance signal over time to form a second mean impedance
24 signal;

first memory means for storing said first and second mean
26 impedance signals to represent said living biological signal
impedance at said selected sinusoidal frequency;

28 processing means for obtaining a plurality of said first
and second mean impedance signals representing said living
30 biological tissue impedance at a plurality of selected
sinusoidal frequencies;

32 network analyzer means for inverting said plurality of
living biological tissue impedances to a plurality of
34 equivalent circuit element values; and

-31-

display means for displaying said plurality of living
36 biological tissue equivalent circuit value.

1/3

FIG. 1a

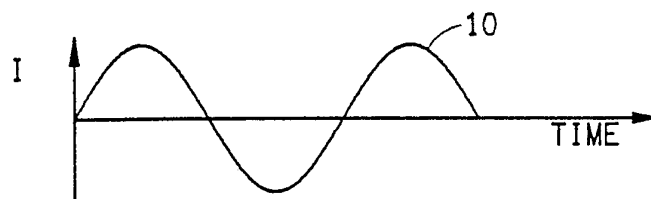


FIG. 1b

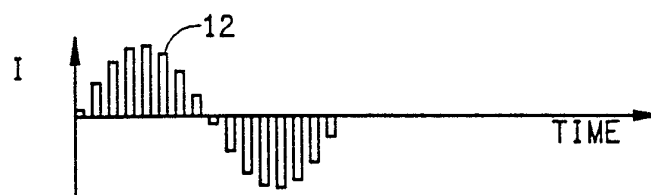


FIG. 1c

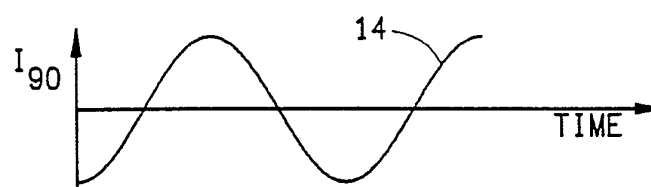


FIG. 1d

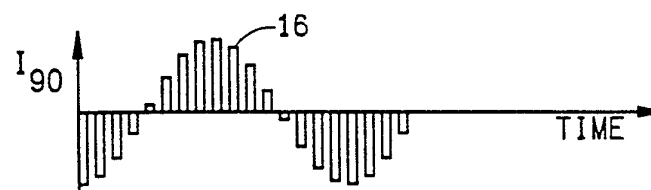


FIG. 1e

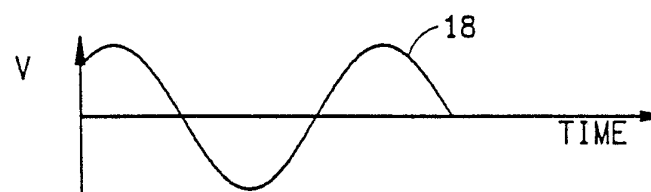


FIG. 1f

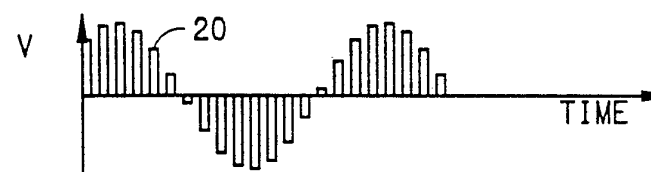


FIG. 1g

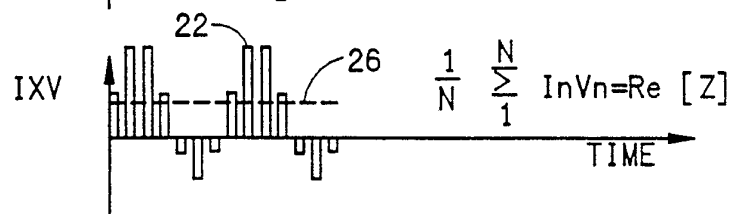


FIG. 1h





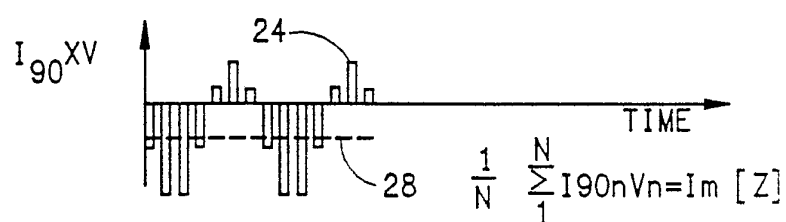


FIG. 2

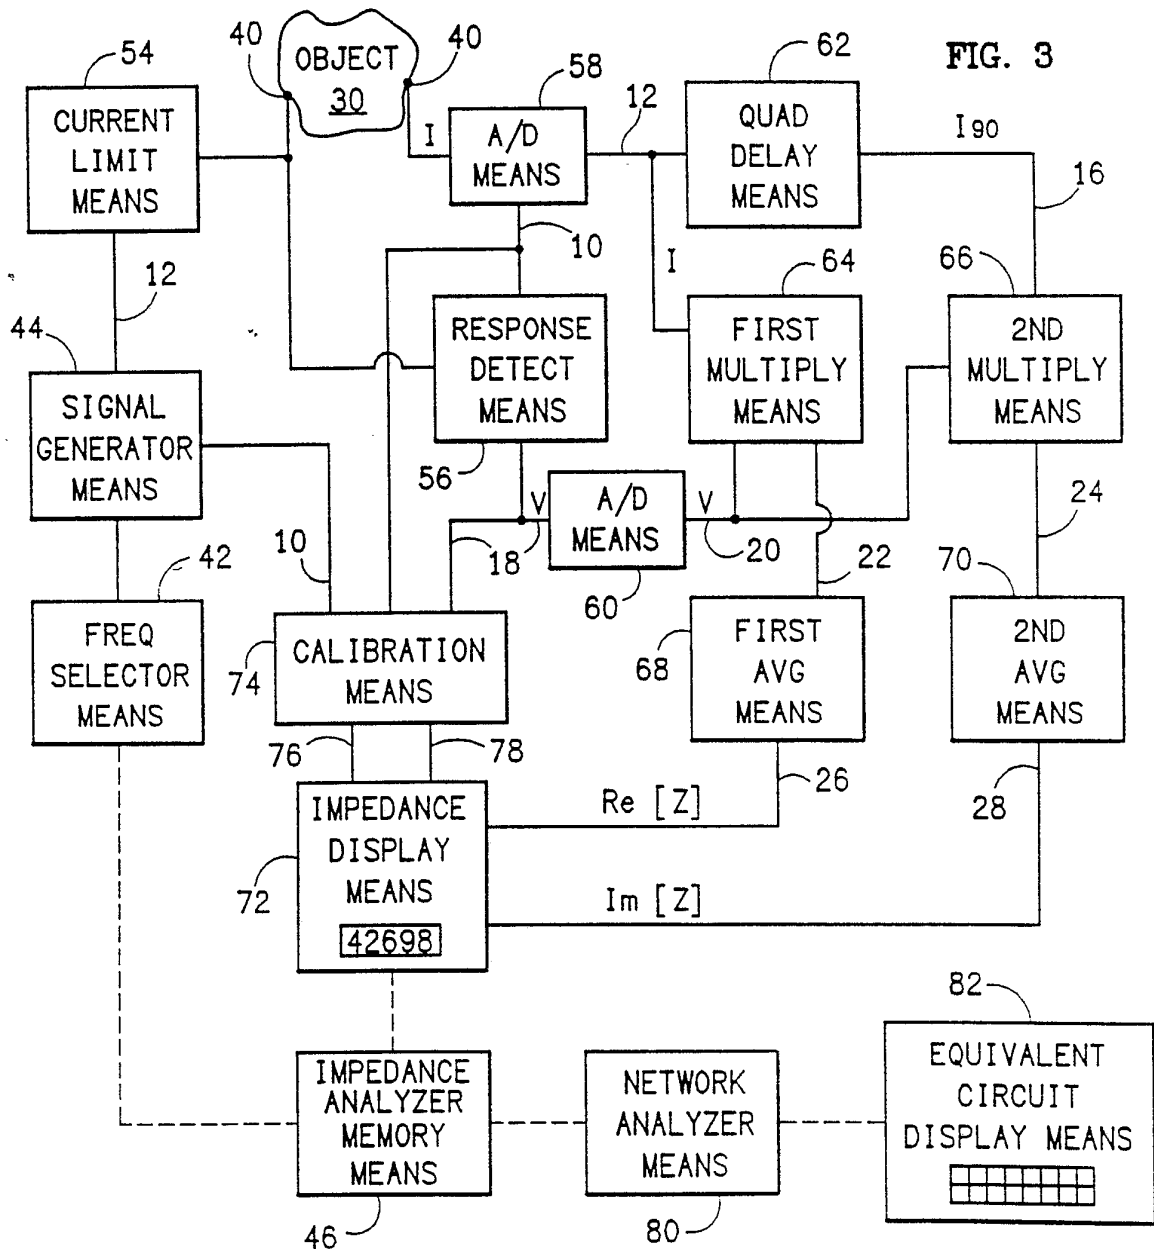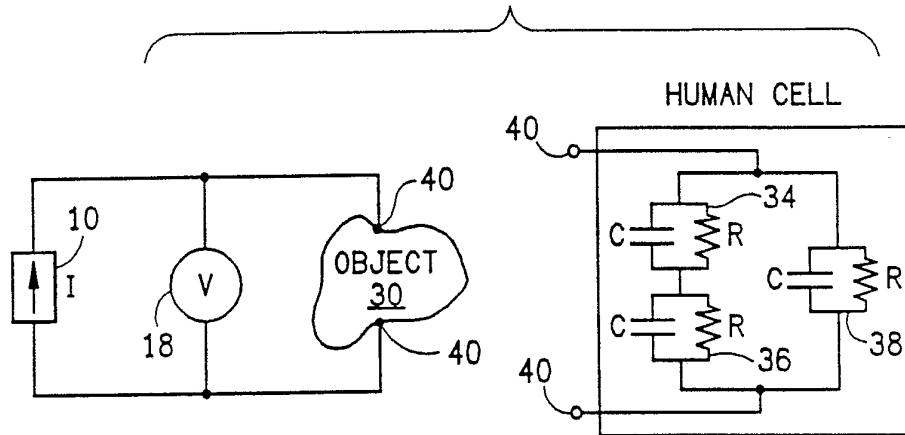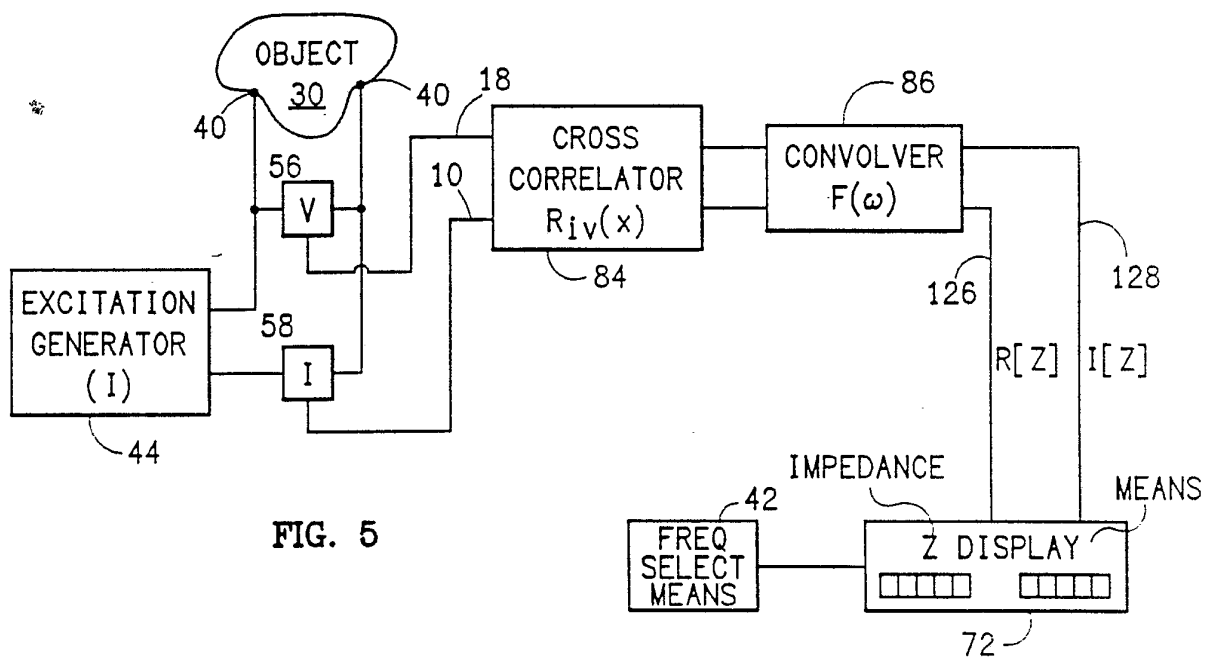

3/3

FIG. 4

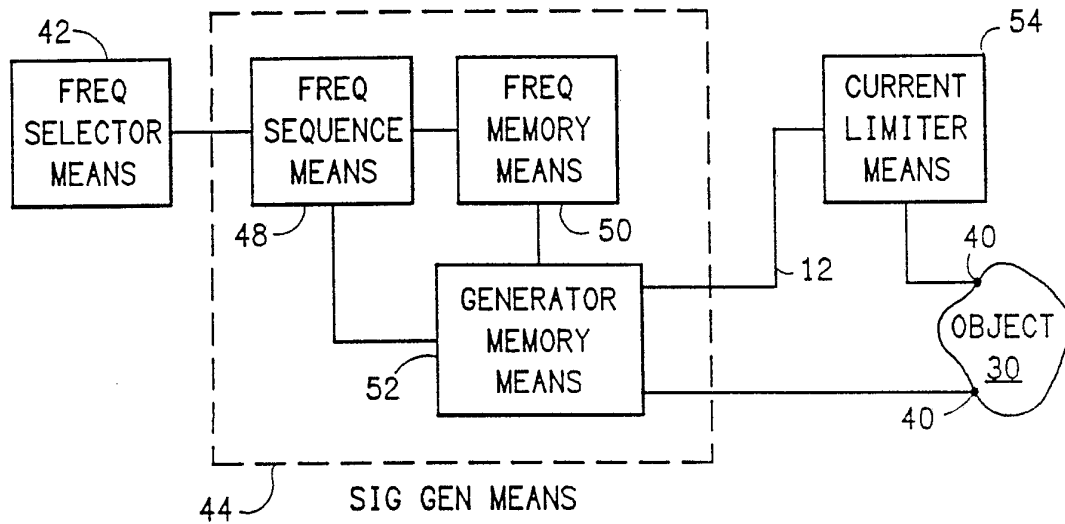

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US92/03458

A. CLASSIFICATION OF SUBJECT MATTER IPC(5) : A61B 5/04 US CL : 364/413.01 According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) U.S. : 128/713, 734 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US, A, 3,316,896 (THOMASSET) 15 October 1963, See col. 1 line 1 - col. 2 line 45.	1-19
A	US, A, 4,008,712 (NYBOER) 22 February 1977, See abstract.	1-19
A	US, A, 4,895,163 (LIBKE ET AL) 23 January 1990, See Summary of Invention.	1-19
A	US, A, 4,942,880 (SLOVAK) 24 June 1990, See Summary of Invention.	1-19
A	US, A, 4,951,682 (PETRE) 28 August 1990, See Summary of Invention.	1-19
A.P	US, A, 5,063,937 (EZENWA ET AL) 12 November 1991, See Abstract.	1-19
A	Medical & Biological Engineering & Computing, May 1983, <u>B. Tedner</u> , "Equipment Using Impedance Technique for Automatic Recording of Fluid-Volume Changes During Haemodialysis" pages 285-290.	1-19
A	Medical Progress through Technology, 1987, <u>Hiroshi Kanai et al.</u> , "Electrical Measurement of Fluid Distribution in Legs and Arms," pages 159-170.	1-19
<input checked="" type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/> See patent family annex.		
* Special categories of cited documents:	*T*	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&"	document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means		
"P" document published prior to the international filing date but later than the priority date claimed		
Date of the actual completion of the international search	Date of mailing of the international search report	
13 JULY 1992	29 JUL 1992	
Name and mailing address of the ISA/ Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231	Authorized officer <i>Andre Robinson</i> GAIL O. HAYES	
Facsimile No. NOT APPLICABLE	Telephone No. (703) 308-1670	

INTERNATIONAL SEARCH REPORT

International application N
PCT/US92/03458

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim N.
A	Aviation, Space, and Environmental Medicine, December 1988 <u>Henry C. Lukaski</u> , PhD et al., "Estimation of Body Fluid Volumes Using Tetrapolar Bioelectrical Impedance Measurements, page 1163-1169.	1-19
A	Third Annual IEEE Symposium on Computer Based Medical System, 3-6 June 3 1990, University of N. C. at Chapel Hill, <u>W.A. Gerth et al.</u> pages 446-453.	1-19
A	US, A, 4,793,362 (TEDNER) 27 December 1988, See Abstract.	1-19
A	US, A, 4,911,175 (SHIZGAL) 27 March 1990, See Abstract.	1-19