



US 20090283670A1

(19) **United States**(12) **Patent Application Publication****Koo et al.**(10) **Pub. No.: US 2009/0283670 A1**(43) **Pub. Date: Nov. 19, 2009**(54) **TECHNIQUE FOR MONITORING AND CONTROLLING A PLASMA PROCESS**

continuation-in-part of application No. 11/371,907, filed on Mar. 10, 2006, now Pat. No. 7,476,849.

(75) Inventors: **Bon-Woong Koo**, Andover, MA (US); **Ludovic Godet**, N. Reading, MA (US); **Vassilis Panayotis Vourloumis**, Peabody, MA (US); **Vikram Singh**, North Andover, MA (US); **Ziwei Fang**, Beverly, MA (US)

Publication Classification

(51) **Int. Cl.**
B01D 59/44 (2006.01)
H01J 49/00 (2006.01)

Correspondence Address:

VARIAN SEMICONDUCTOR EQUIPMENT ASSC., INC.
35 DORY RD.
GLOUCESTER, MA 01930-2297 (US)

(52) **U.S. Cl. 250/282; 250/287**

(73) Assignee: **Varian Semiconductor Equipment Associates, Inc.**, Gloucester, MA (US)

(21) Appl. No.: **12/272,537**(22) Filed: **Nov. 18, 2008****Related U.S. Application Data**

(63) Continuation of application No. 11/678,524, filed on Feb. 23, 2007, now Pat. No. 7,453,059, which is a

(57) **ABSTRACT**

A time-of-flight ion sensor for monitoring ion species in a plasma includes a housing. A drift tube is positioned in the housing. An extractor electrode is positioned at a first end of the drift tube so as to attract ions from the plasma. A plurality of electrodes is positioned at a first end of the drift tube proximate to the extractor electrode. The plurality of electrodes is biased so as to selectively attract ions to enter the drift tube and to drift towards a second end of the drift tube. An ion detector is positioned proximate to the second end of the drift tube. The ion detector detects arrival times associated with the at least the portion of the attracted ions.

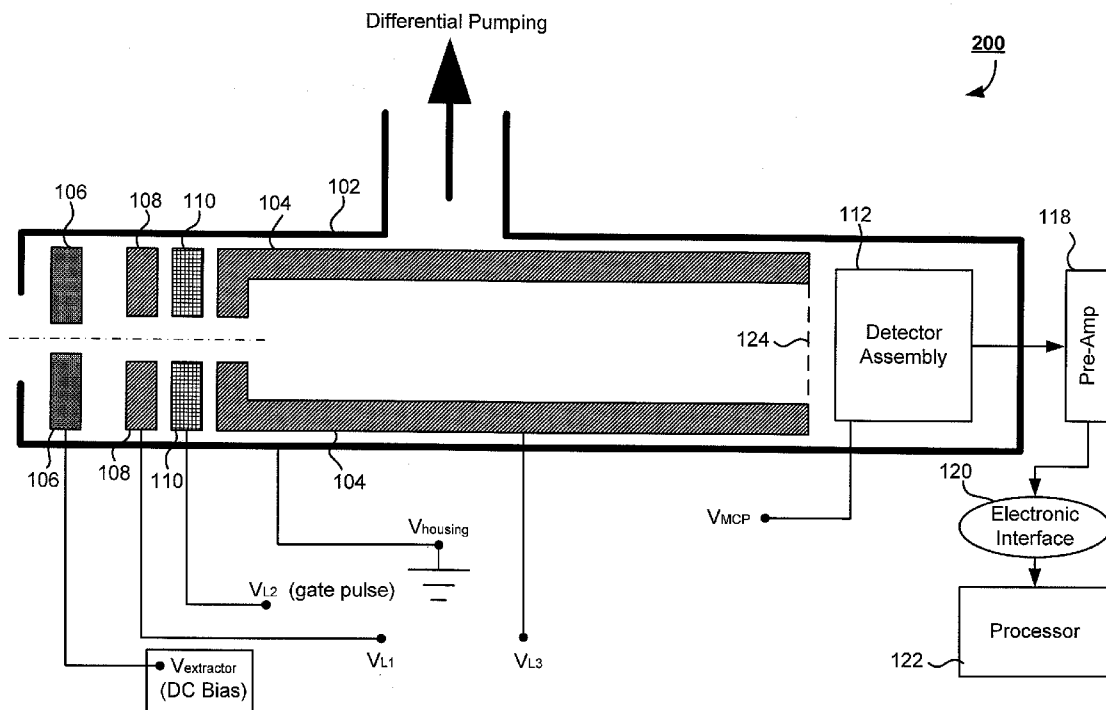


Figure 1

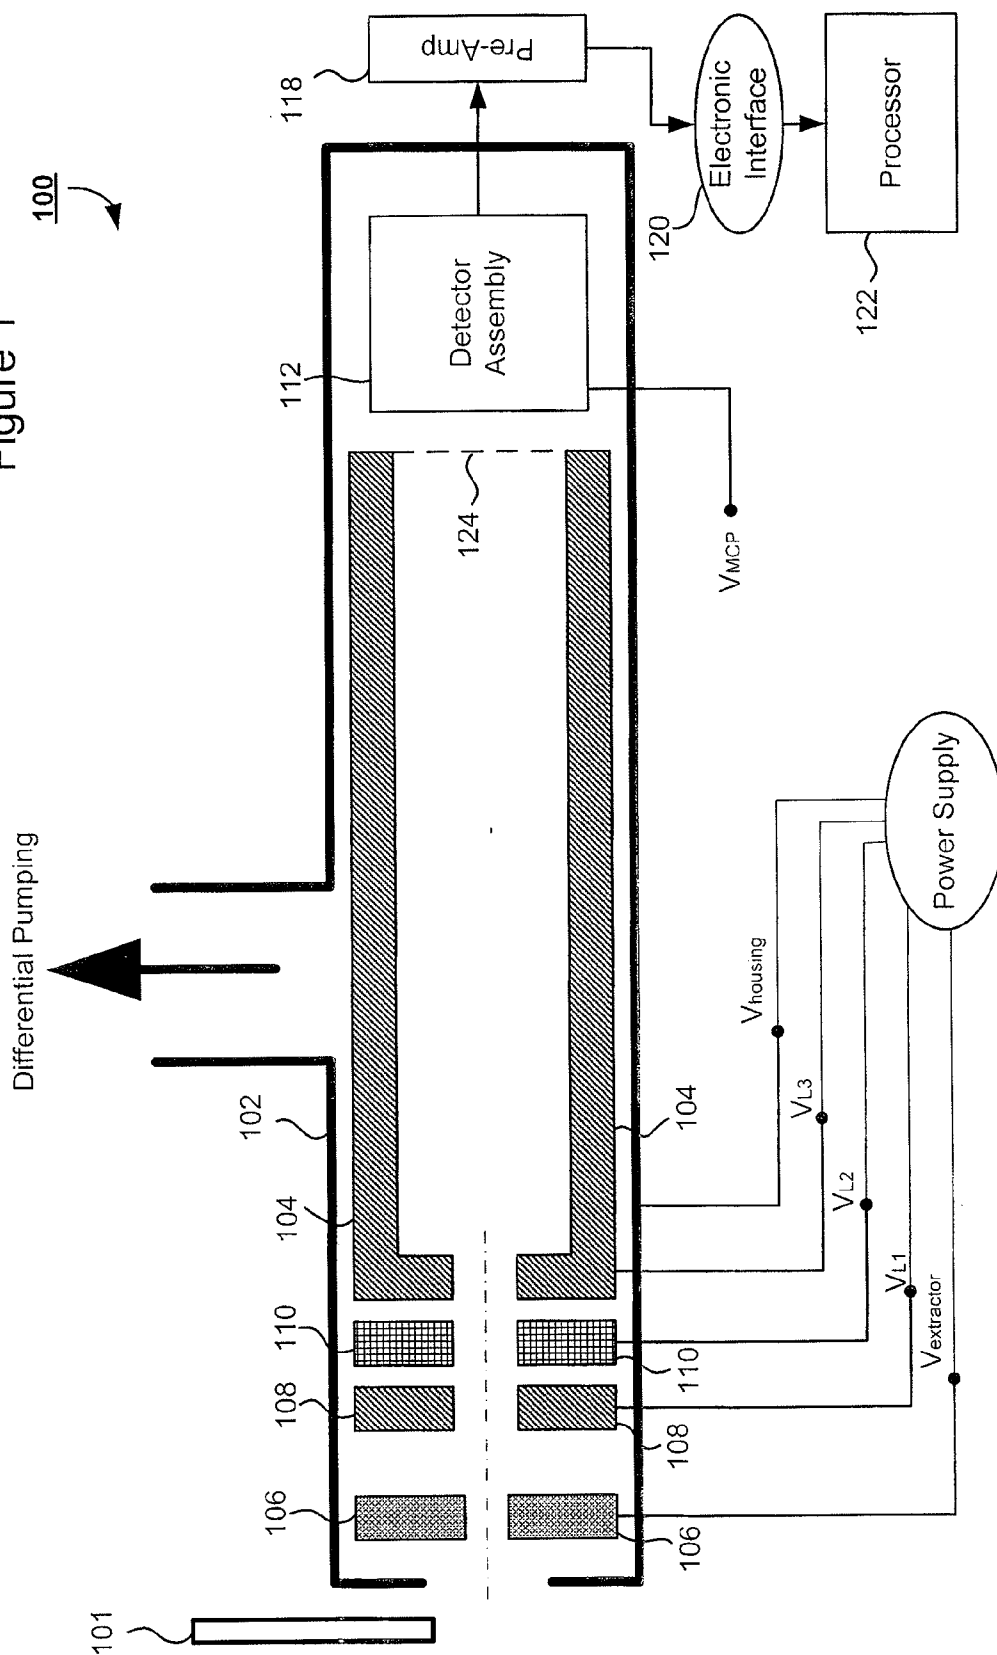
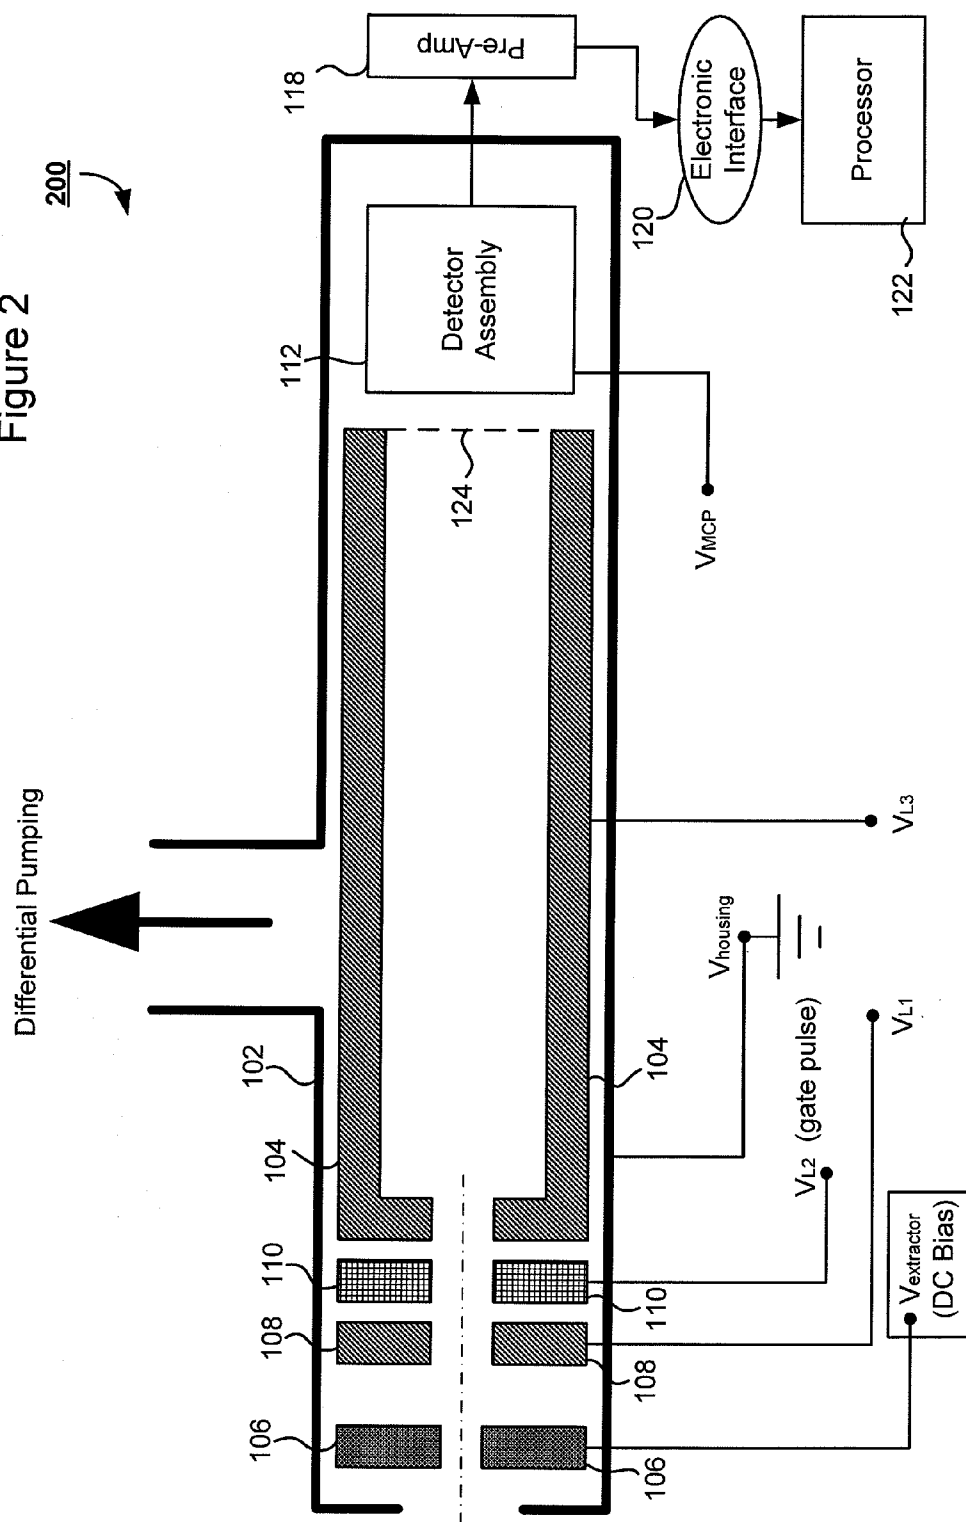


Figure 2



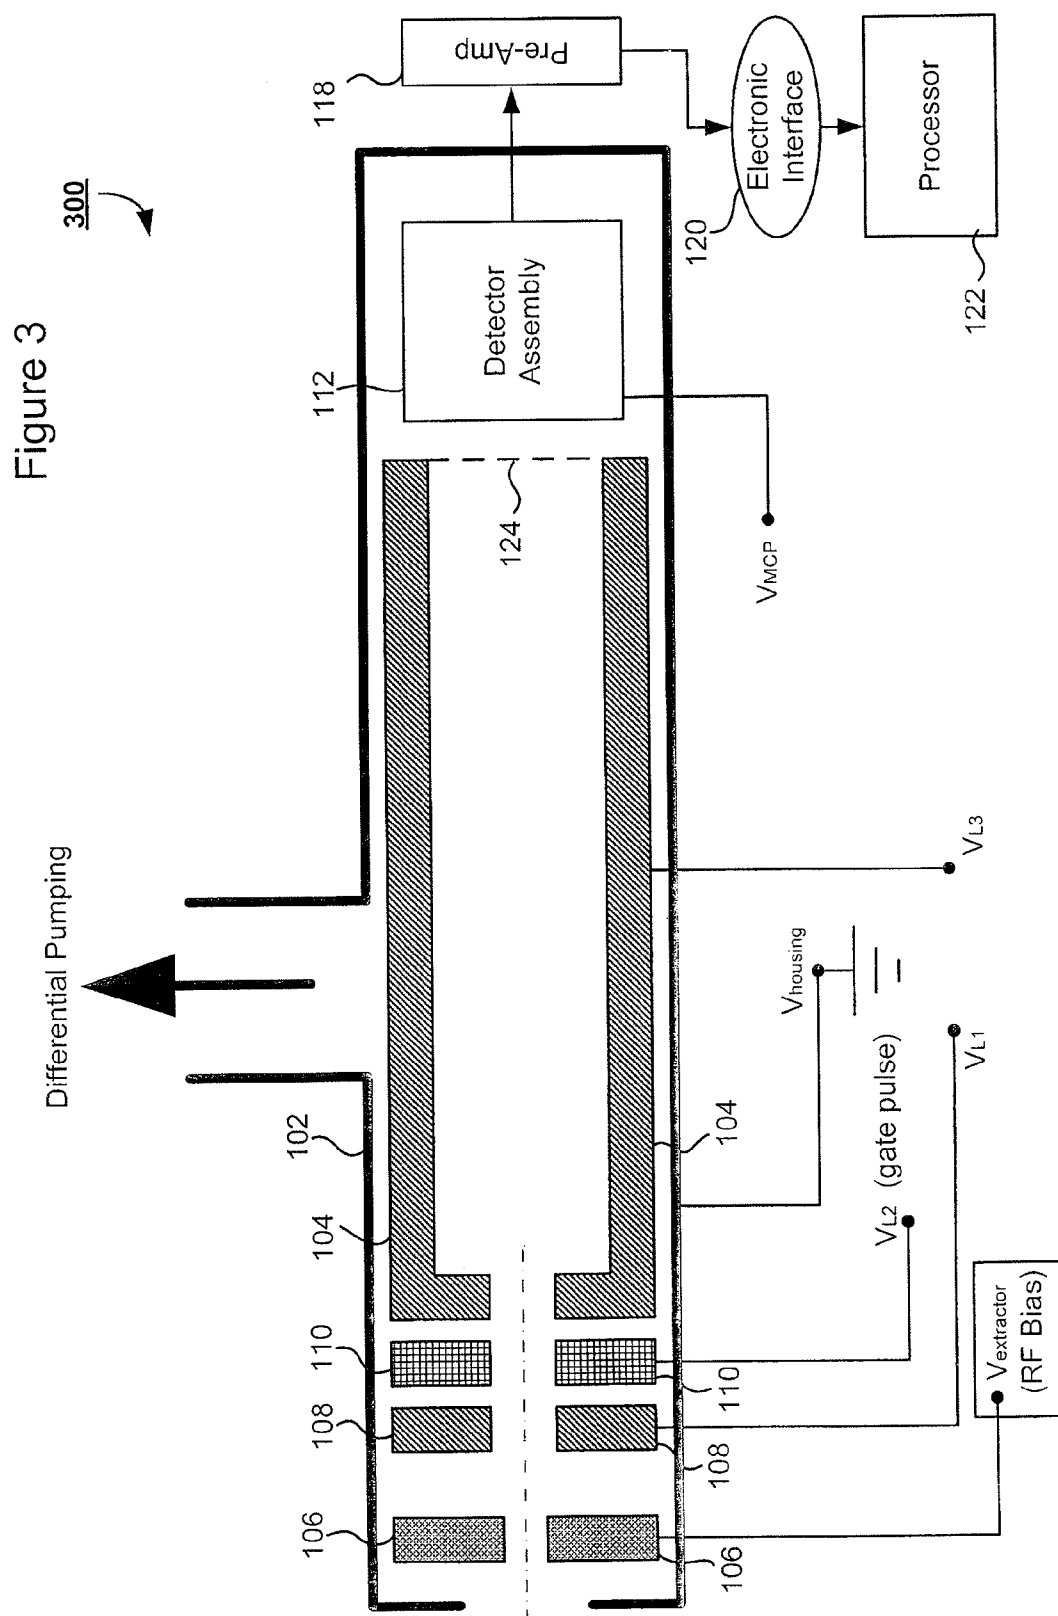


Figure 4

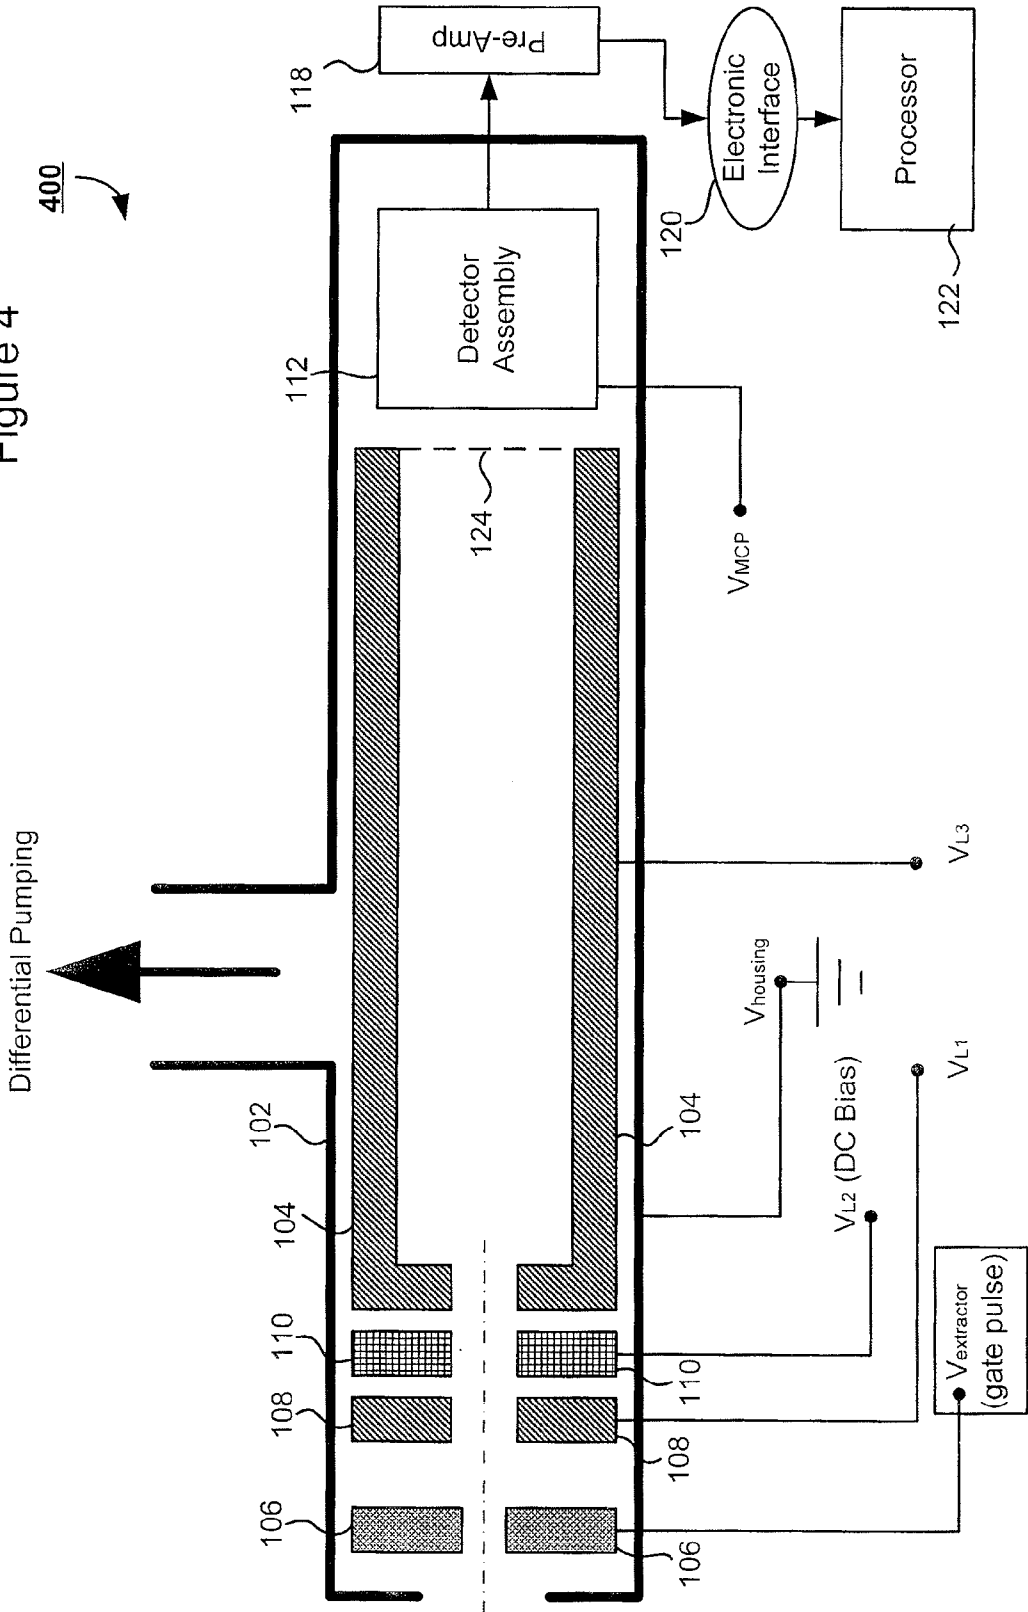
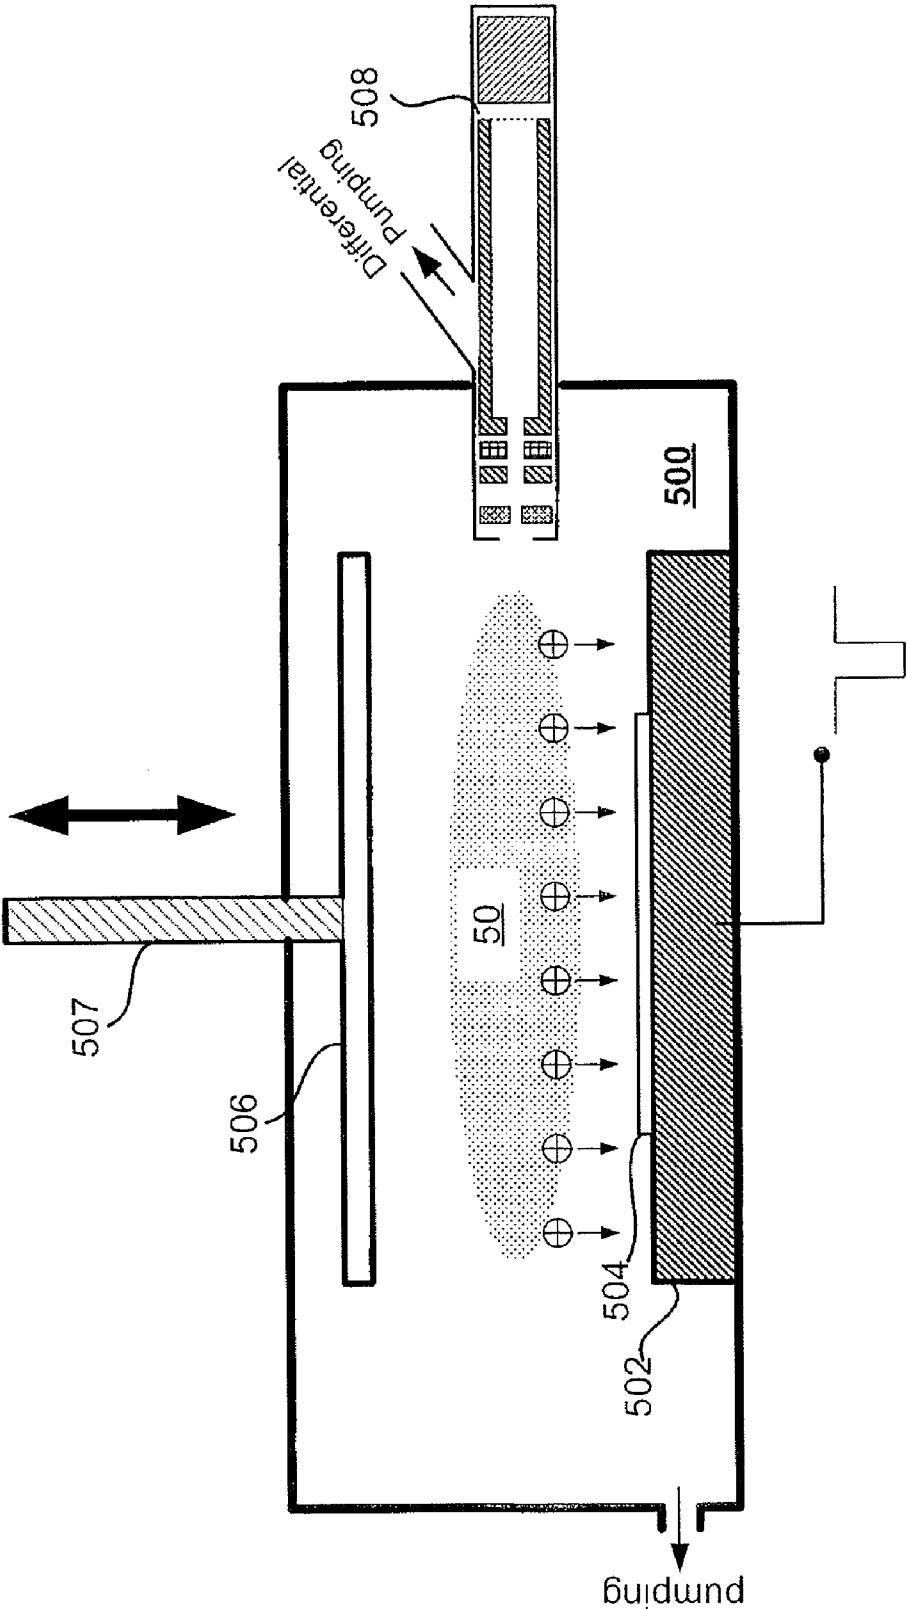


Figure 5



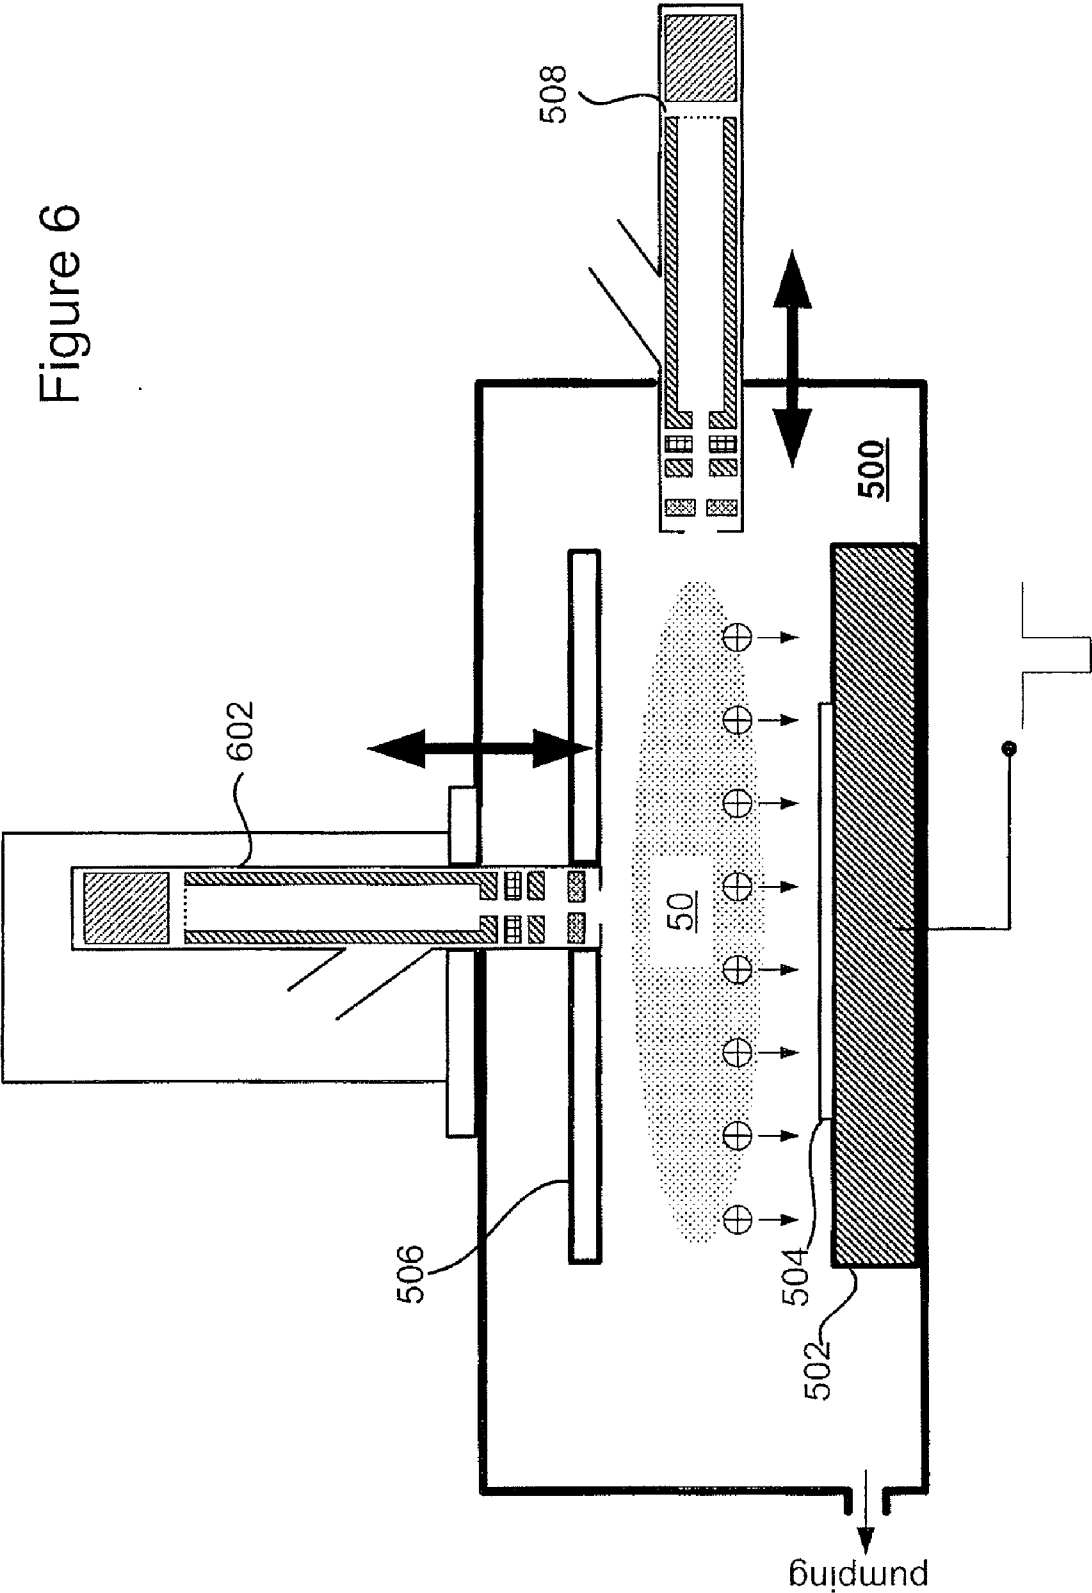


Figure 6

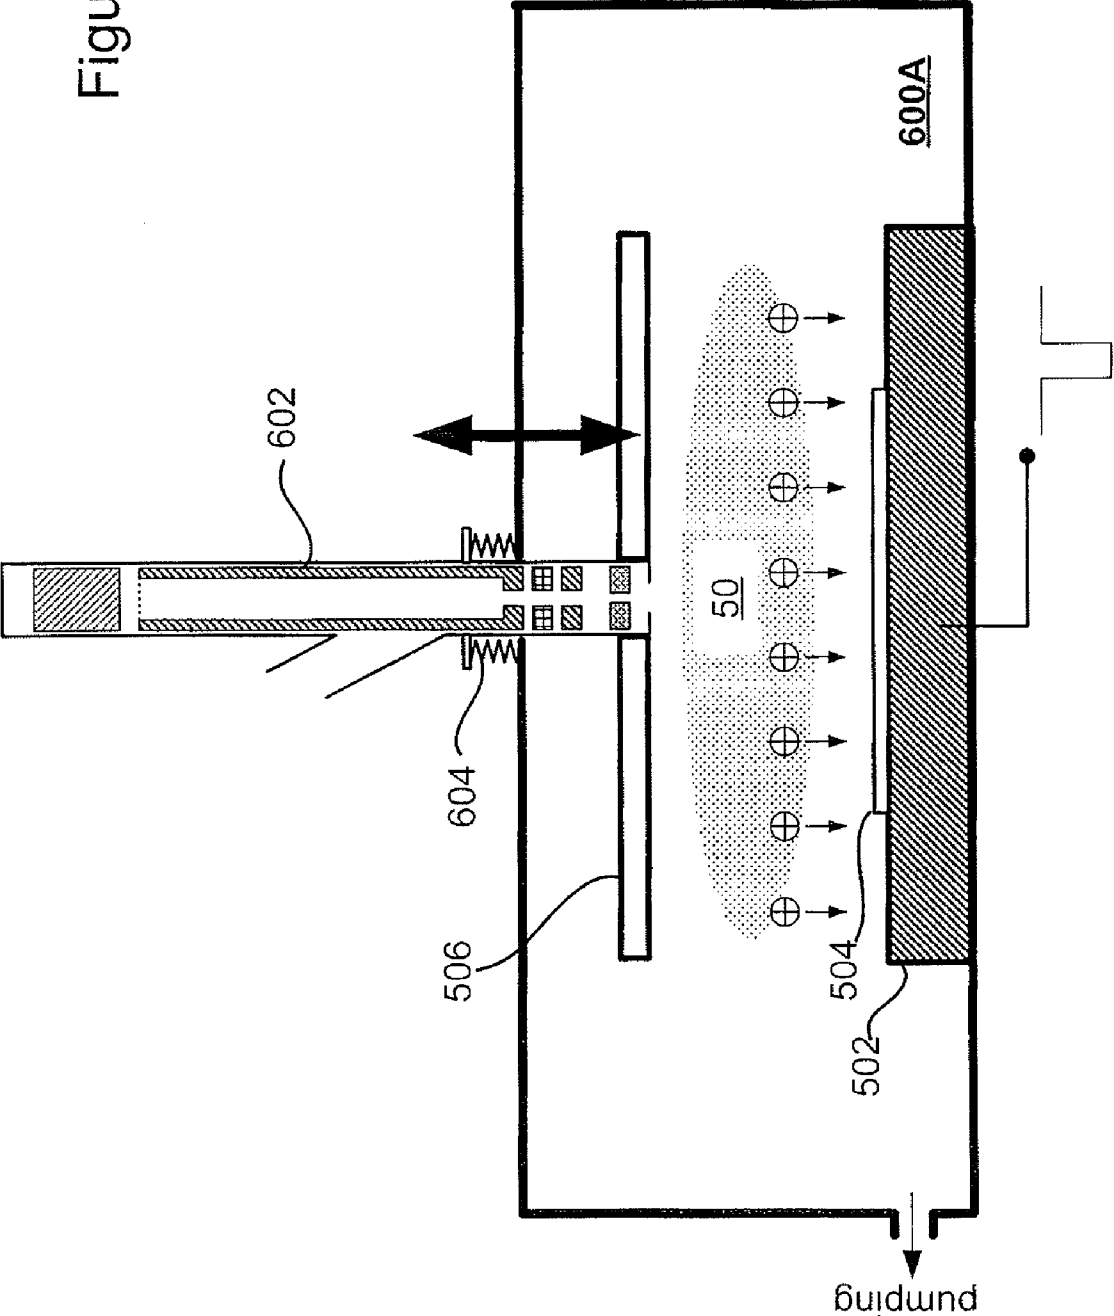
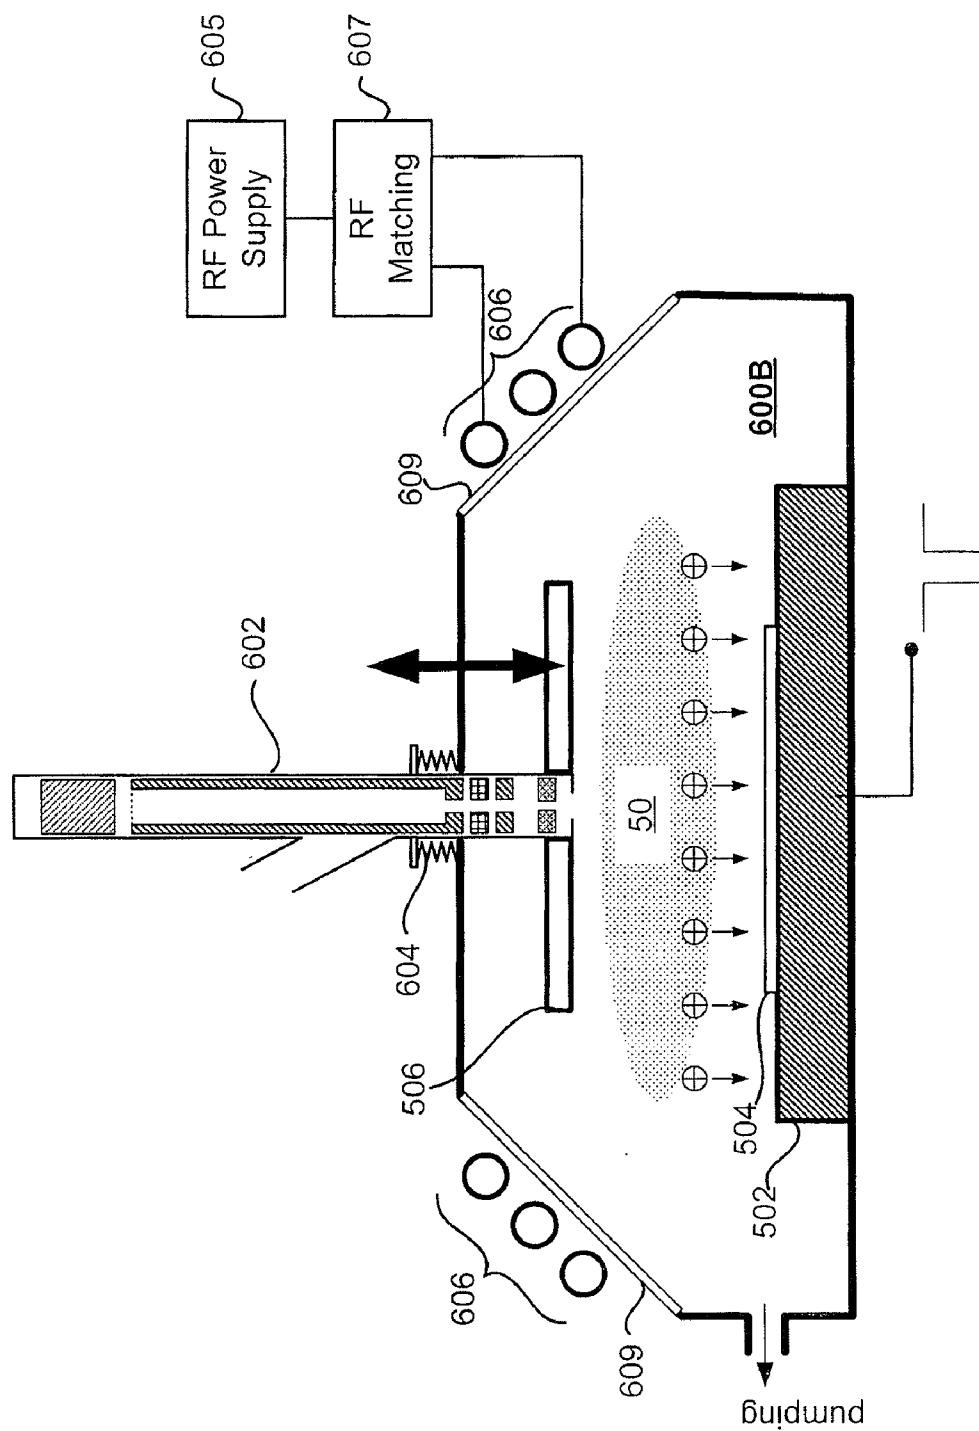


Figure 6a

Figure 6b



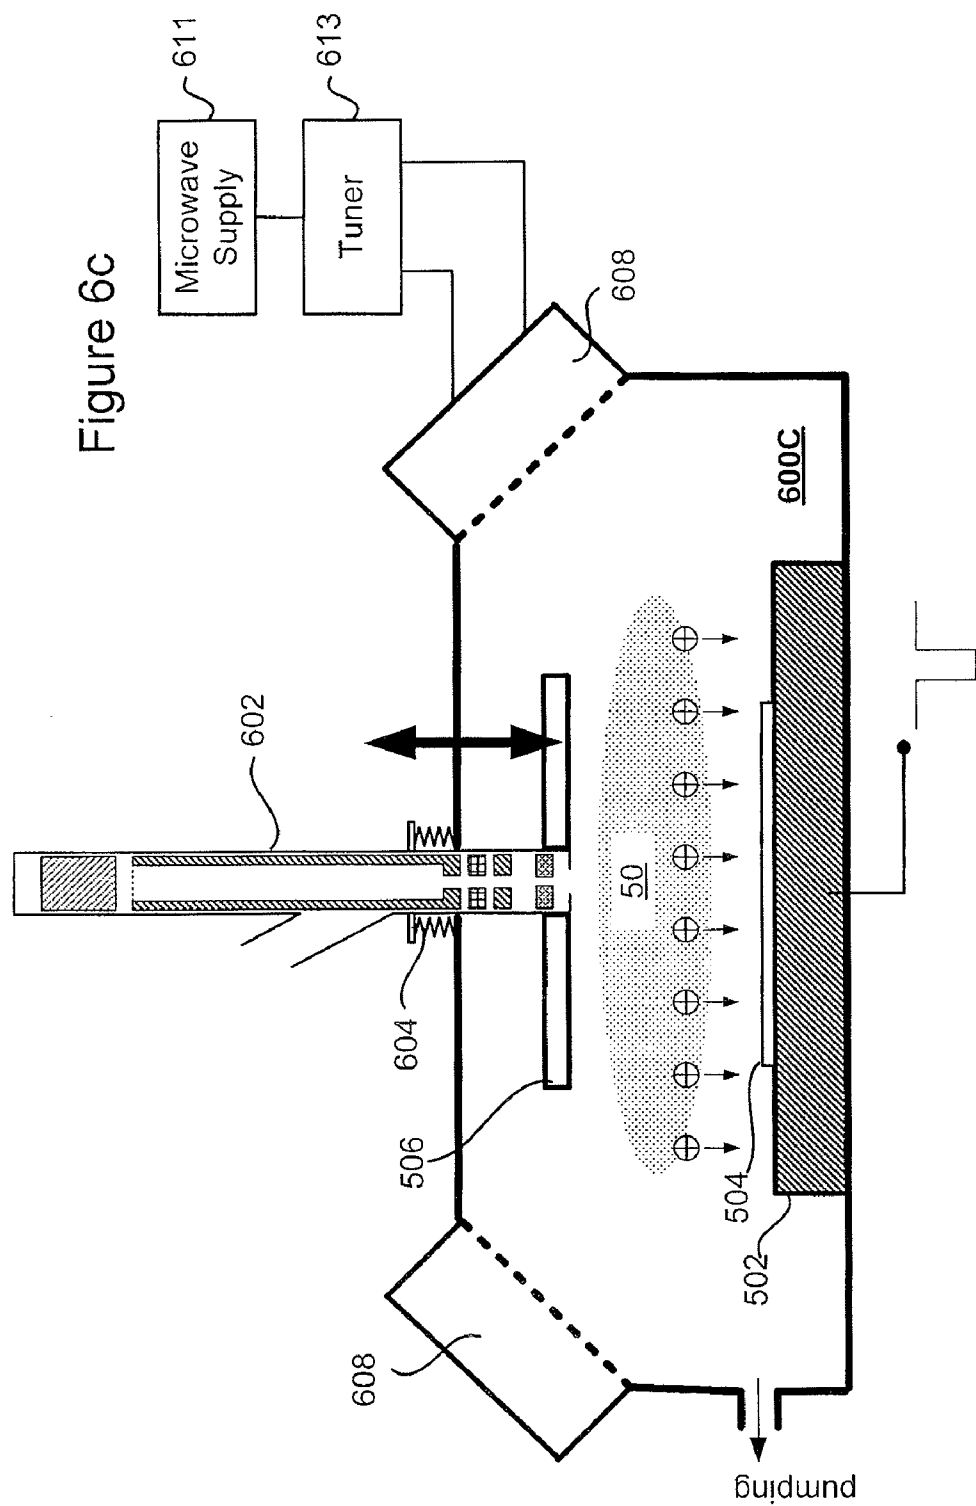


Figure 7

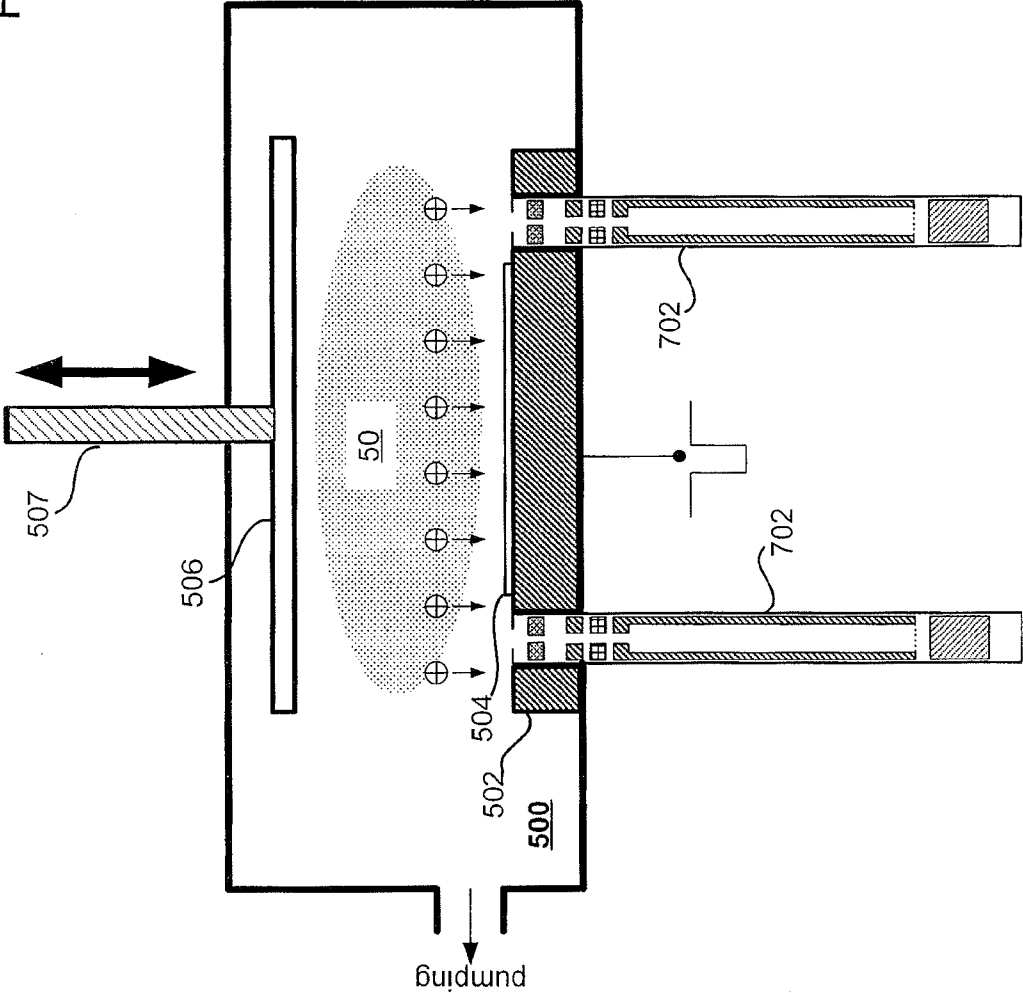
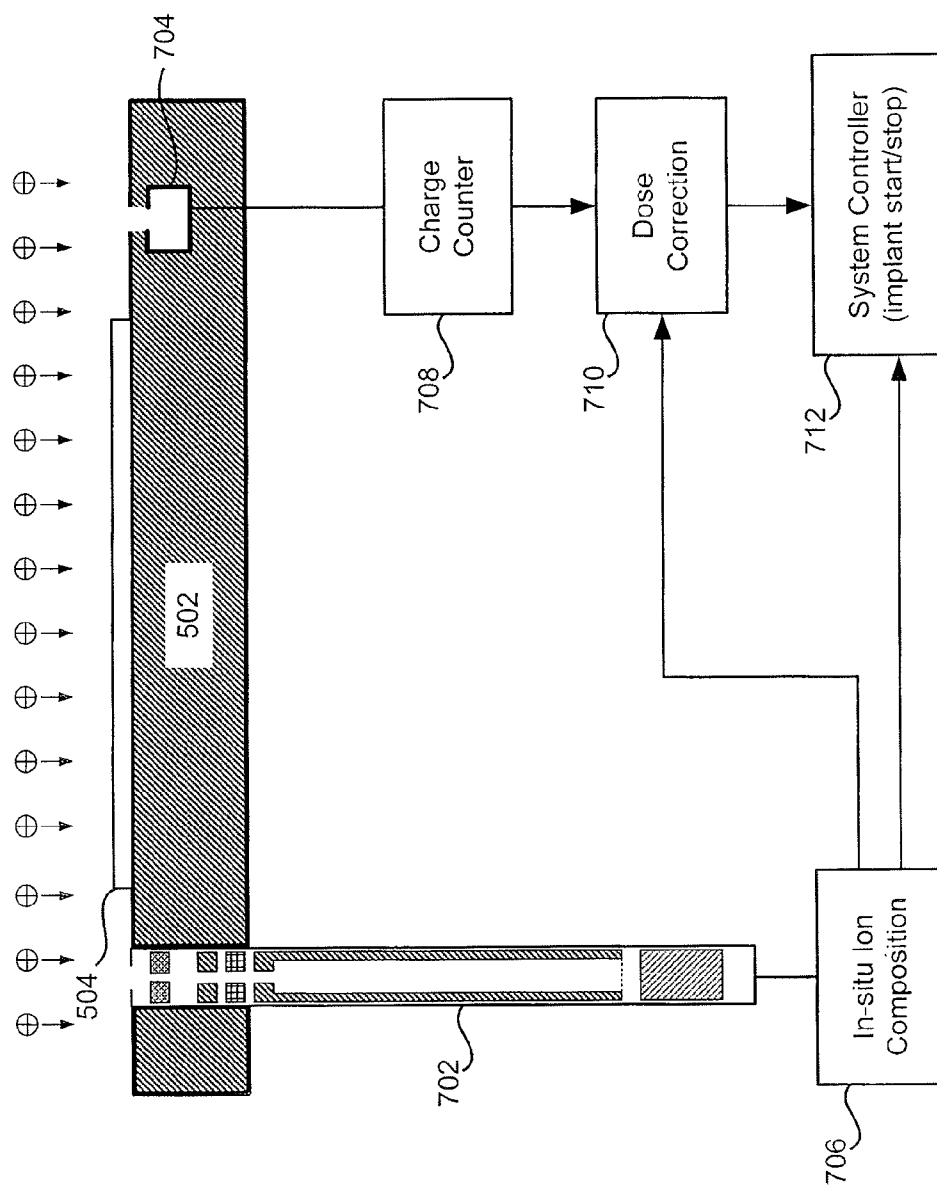


Figure 7a




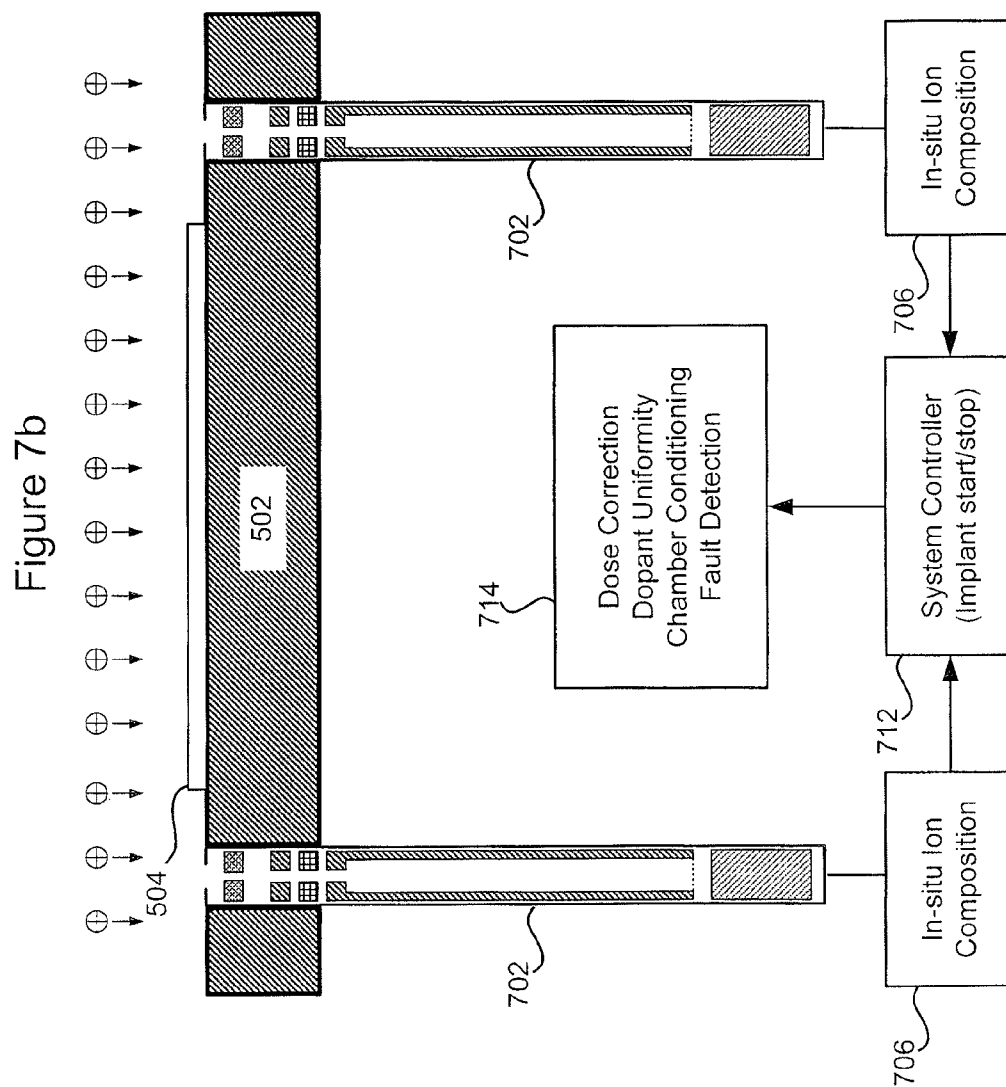


Figure 8

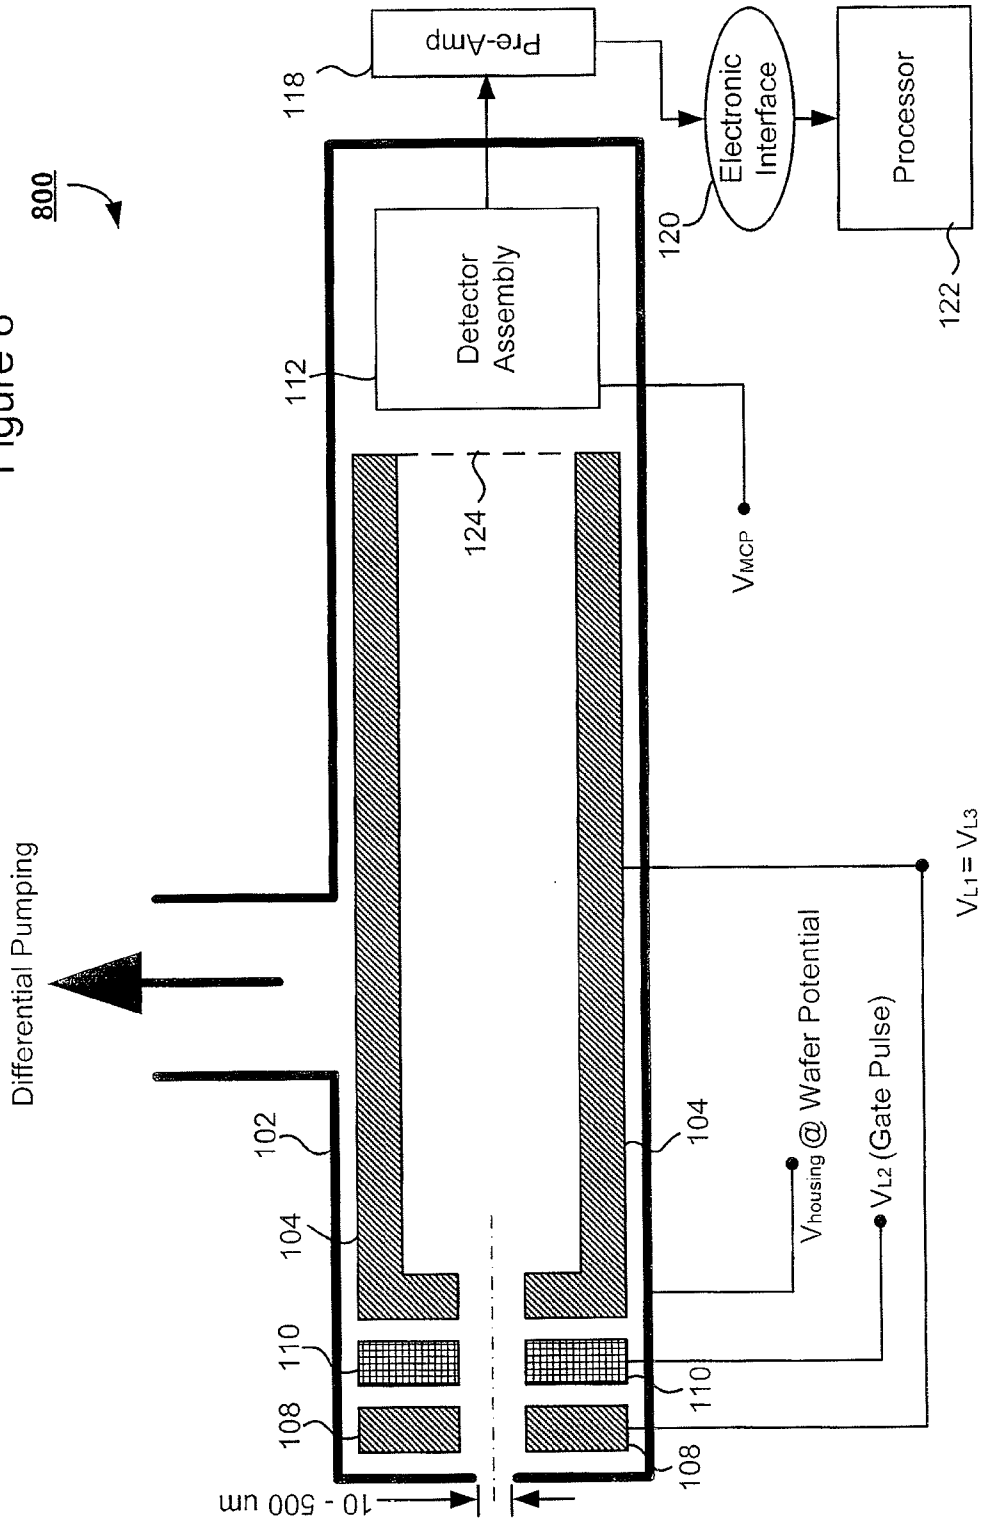

TECHNIQUE FOR MONITORING AND CONTROLLING A PLASMA PROCESS

PRIORITY

[0001] This patent application is a continuation application of and claims priority to U.S. patent application Ser. No. 11/678,524, filed on Feb. 23, 2007, and entitled "Technique for Monitoring and Controlling a Plasma Process," which is a continuation-in-part application of claims priority to U.S. patent application Ser. No. 11/371,907, filed on Mar. 10, 2006 and entitled "Technique for Monitoring and Controlling a Plasma Process." Each of U.S. patent application Ser. Nos. 11/678,524 and 11/371,907 is incorporated in entirety by reference.

BACKGROUND

[0002] Plasma processes are widely used in semiconductor manufacturing, for example, to implant wafers with various dopants, to deposit or to etch thin films. In order to achieve predictable and repeatable process results, it is critical to closely monitor and control the plasma characteristics. For example, studies of plasma doping (PLAD) processes have shown that ion composition of a plasma may be a critical piece of information that determines dopant species, dopant depth profiles, process-related contamination, etc. The ion composition changes with PLAD process parameters such as gas ratio, total gas pressure, and discharge power. The ion composition can also change significantly depending on the conditioning status of a plasma chamber. Therefore, it is important to know the ion composition during a PLAD process, preferably in situ and in real-time, in order to achieve repeatable and predictable process results.

[0003] Existing plasma tools often lack the capability of providing detailed real-time information (e.g., ion composition) of a plasma. In a typical PLAD process, for example, a plasma is controlled by monitoring an implant dose based on a Faraday cup current. However, a Faraday cup is just a total charge counter, which does not distinguish different charged particles or otherwise offer any insight of the plasma properties. Although in-situ mass analysis has been employed in some traditional beam-line ion implantation systems, it has typically been avoided in plasma-based ion implantation systems in order to achieve a high throughput.

[0004] In addition, conventional ion sensors, such as commercial mass/energy analyzers and quadrupole mass spectrometers, are often too bulky and/or too intrusive to implement in production tools. Large ion sensors tend to perturb a plasma under measurement and therefore distort the process results. Furthermore, the size and weight of conventional ion sensors often limit their deployment options in a semiconductor process tool. Furthermore, in pulsed plasma processing wherein a plasma alternates between on and off states, time-resolved measurements of the plasma are often required. However, few existing ion sensors provide the capability of time-resolved measurements.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] In order to facilitate a fuller understanding of the present disclosure, reference is now made to the accompanying drawings, in which like elements are referenced with like numerals. These drawings should not be construed as limiting the present disclosure, but are intended to be exemplary only.

[0006] FIG. 1 shows an exemplary ion sensor in accordance with an embodiment of the present disclosure.

[0007] FIG. 2 shows an ion sensor having one exemplary configuration in accordance with an embodiment of the present disclosure.

[0008] FIG. 2a shows an ion sensor having an energy analyzer in accordance with an embodiment of the present disclosure.

[0009] FIG. 3 shows an ion sensor having another exemplary configuration in accordance with an embodiment of the present disclosure.

[0010] FIG. 4 shows an ion sensor having yet another exemplary configuration in accordance with an embodiment of the present disclosure.

[0011] FIG. 5 shows one installation option for an ion sensor in accordance with an embodiment of the present disclosure.

[0012] FIG. 6 shows another installation option for an ion sensor in accordance with an embodiment of the present disclosure.

[0013] FIGS. 6a-c show different examples of plasma processing chambers in accordance with embodiments of the present disclosure.

[0014] FIG. 7 shows yet another installation option for an ion sensor in accordance with an embodiment of the present disclosure.

[0015] FIGS. 7a-b show exemplary systems for employing ion sensors for process control in accordance with embodiments of the present disclosure.

[0016] FIG. 8 shows an exemplary ion sensor in accordance with an embodiment of the present disclosure.

DETAILED DESCRIPTION

[0017] The present disclosure will now be described in more detail with reference to exemplary embodiments thereof as shown in the accompanying drawings. While the present disclosure is described below with reference to exemplary embodiments, it should be understood that the present disclosure is not limited thereto. Those of ordinary skill in the art having access to the teachings herein will recognize additional implementations, modifications, and embodiments, as well as other fields of use, which are within the scope of the present disclosure as described herein, and with respect to which the present disclosure may be of significant utility.

[0018] Embodiments of the present disclosure provide a number of compact designs of time-of-flight (TOF) ion sensors that are suitable for in-situ monitoring and controlling of a plasma process. These designs may employ flexible ion extraction and ion focusing techniques to measure ion composition in a plasma chamber. Each TOF ion sensor may be installed in a variety of ways in the plasma chamber and may be configured for a number of functions such as, for example, in-situ process control, chamber readiness verification, fault detection, implant dose correction, and implant uniformity measurement. The sensitivity and size of each ion sensor may allow time-resolved measurement and spatial measurement of a plasma.

[0019] Referring to FIG. 1, there is shown an exemplary ion sensor 100 in accordance with an embodiment of the present disclosure. In some embodiments, the ion sensor 100 includes an ionization source 101 that generates ions proximate to the entrance of the ion sensor 100. In one embodiment, the ion source 101 generates an electron cloud using a low energy electron source. The electrons in the electron cloud cause

electron impact that facilitates the ionization of neutral atoms and molecules and the conversion of ions by electron attachment. In various other embodiments, the ion source **101** generates ions proximate to the entrance of the ion sensor **100** by ion-impact and/or by photon-impact ionization. The ion source **101** can be a continuous or a pulsed ion source. The ion source **101** is useful for some applications where it is desirable to provide conventional RGA type measurements of the neutral gas or fast neutral species.

[0020] Ion sensor **100** comprises a housing **102** that may be adapted for installation in a view port of a plasma chamber and that may accommodate differential pumping. The housing **102** may be individually biased at a desired potential $V_{\text{sub.housing}}$. A left hand side of the housing **102** may be referred to as an “extractor side” since ions extracted from a plasma enter the ion sensor **100** via an aperture (“housing aperture”) on the left hand side of the housing **102**. A right hand side of the housing **102** may be referred to as a “detector side” since ion detection takes place on the right hand side of the housing **102**.

[0021] The ion sensor **100** includes a drift tube **104** inside the housing **102** which may also be individually biased, for example, at a desired potential $V_{\text{sub.L3}}$. The drift tube **104** typically has a hollow space with a negligible electromagnetic field. An extractor side of the drift tube **104** may have an aperture (“drift tube aperture”) for admitting ions. A detector side of the drift tube **104** may have a grid **124** that allows ions to exit while shielding out external electric fields. The plasma chamber's pressure is typically 1-3,000 mTorr, while the drift tube pressure is typically at 2.times.10.sup.-6 Torr or less. Differential pumping can be used to maintain the pressure difference.

[0022] Various embodiments include one or more electrodes and/or grids that form lenses or deflectors proximate to the extractor side of the drift tube **104**, between the housing aperture and the drift tube aperture. In some embodiments, there are a series of electrodes for extracting and focusing ions. For example, there may be an extractor electrode **106** proximate to the housing aperture. The extractor electrode **106** may have an aperture that is between 10 and 500 microns in diameter (preferable 50-200 microns for some embodiments), although the actual aperture size may vary, at least in part, on the differential pumping requirements. The extractor electrode **106** may be biased at a suitable potential V_{sub} . extractor in order to attract either positive or negative ions from a plasma. The attracted ions may be traveling at diverse angles.

[0023] To ensure that the attracted ions travel towards the detector side within a finite beam angle (e.g., equal or less than ± 1.5 degrees), two or more electrodes (e.g., electrostatic lenses **108** and **110**) may be arranged in series with their apertures aligned with those of the housing **102**, the extractor **106**, and the drift tube **104**. Each electrostatic lens may be individually biased to create a desired electrostatic field that directs the ions in a focused beam. In various modes of operation, the electrostatic lenses are biased with either a positive or a negative voltage. One of the electrostatic lenses may be provided with a voltage pulse to admit a portion (or packet) of the attracted ions into the drift tube **104**. The voltage pulse may be repeated in a timed manner for a periodical or near-continuous sampling of the ions.

[0024] In various embodiments, a combination of a repeller voltage and an extraction voltage pulse is applied to any pair of electrodes to drive positive ions into the drift tube **104**.

The flight time of the ions is determined relative to the time at which the extraction pulse occurs. For example, in one embodiment, the electrostatic lens **108** is biased with a positive voltage pulse $V_{\text{sub.L1}}$. The positive voltage pulse can be periodic or non-periodic. The electrostatic lens **110** is biased at a positive repelling voltage $V_{\text{sub.L2}}$. In one embodiment, a positive repeller voltage is applied to electrostatic lens **110** and a positive voltage pulse is applied to the nearby electrostatic lens **108** in order to drive positive ions past the repeller electrodes and into the drift tube **104**. The positive repeller voltage may be periodic or not. The drift tube **104**, when biased at $V_{\text{sub.L3}}$, may function as a third electrostatic lens in the series. The bias voltage on the drift tube may be a pulsed voltage. Negative ions may be extracted into the drift tube using a similar arrangement.

[0025] In some embodiments, voltage pulses are applied to more than one of the electrodes. For example voltage pulses can be applied to at least two of the drift tube **104**, the extractor **106**, the electrostatic lens **108**, and the electrostatic lens **110**. The at least two voltage pulses can be applied either simultaneously or delayed by a predetermined time in order to cause ions to enter the drift tube.

[0026] In some embodiments, a blocking voltage is applied to at least one of the extractor **106**, the electrostatic lens **108**, and the electrostatic lens **110** in order to effectively prevent ions from traveling into the drift tube **104**. In some methods of operation, the magnitude of the blocking voltage is periodically varied in order to allow some ions to enter the drift tube. The flight time of the ions through the drift tube **104** is determined relative to the time at which this voltage is changed.

[0027] Once admitted into the drift tube **104**, the ions drift towards the detector end virtually unaffected by any electric field. The ions typically have the same kinetic energy. Heavy ions travel relatively slow and light ions travel relatively fast. Given a sufficient flight time (i.e., sufficient length of the drift tube **104**), the ions become separated into individual packets based on ion mass of their ionic species.

[0028] In some embodiments, the transmission of ions (positive or negative) through the drift tube is modulated using an arrangement of quadrupole elements. In one embodiment, the modulation is periodic. In another embodiment, the modulation is non-periodic. Modulation may be accomplished by varying the RF or DC voltages associated with the individual quadrupole elements. In these embodiments, the flight time of the ions is determined relative to the time at which the modulation occurs.

[0029] In various other embodiments, the transmission of ions (positive or negative) through the drift tube can be modulated by numerous other means. For example, the transmission of ions can be modulated by electrostatic deflection of the ions. The transmission of ions can also be modulated by a mechanical means such as a mechanical gating, multi-stage chopper, or any other type of mechanical interrupter. For example, in one embodiment, the mechanical interrupter is a mechanical shutter. Modulation by mechanical means is sometimes advantageous for low energy applications. In these embodiments, the flight time of the ions is also determined relative to the time at which the modulation occurs.

[0030] On the detector side, a detector assembly **112** may be used to detect the ions. The detector assembly **112** may be any type of commercially available or customized ion detection device (e.g., micro-channel plate (MCP) assembly). Detection and/or collection of the ions may be controlled, for

example, with one or more voltage biases such as $V_{\text{sub.MCP}}$. The detector assembly 112 may be coupled to a pre-amplifier 118 that is in turn coupled to a processor unit 122 via an electronic interface 120. The electronic interface 120 may be, for example, a fast data acquisition card. The processor unit 122 may be, for example, a personal computer (PC) or an industrial type of computing device.

[0031] The individual ion packets having distinct ion mass numbers are detected sequentially by the detector. The detected signals are amplified by the pre-amplifier 118. The amplified signals are then processed by the processor unit 122. Signals corresponding to each individual packet produce a mass peak in a mass spectrum. The mass spectrum accurately reflects an ion composition of the plasma based on one or more samplings of ion species from the plasma.

[0032] In some embodiments, the detector assembly 112 includes position-sensitive particle detectors that are used to detect the ions at certain predetermined positions. These position-sensitive particle detectors provide ion positional information that can be used to determine ion mass or ion energy. In various embodiments, the portion of the detector surface used to detect ions is selected by electrical, magnetic, or mechanical means. For example, an electrically addressable detector array can be used to detect ions as a function of position. A software algorithm can be used to extract the position-sensitive data from the detector signals. Also, mechanical means can be used to control the effective divergence of the ions impacting the detector. For example, a mechanical barrier can be used to shield a portion of the detector. In addition, ion deflectors or ion collimators can be used to deflect or to collimate the ions so that they only impact a desired portion of the detector.

[0033] According to embodiments of the present disclosure, the ion sensor 100 may be flexibly configured by applying different combinations of voltage potentials to the housing 102, the drift tube 104, the extractor electrode 106, the electrostatic lenses 108 and 110, and the detector assembly 112. Exemplary configurations are shown in FIGS. 2-4.

[0034] FIG. 2 shows an ion sensor 200 having one exemplary configuration in accordance with an embodiment of the present disclosure. The ion sensor 200 may comprise substantially the same components as the ion sensor 100 shown in FIG. 1. In this exemplary configuration, the housing 104 may be grounded and/or attached to a plasma chamber wall.

[0035] In some embodiments, the extractor electrode 106 is biased at a DC extractor voltage $V_{\text{sub.extractor.about.}-50V}$ DC for extraction of positive ions or $V_{\text{sub.extractor.about.}0V-50V}$ DC for extraction of negative ions. In other embodiments, a pulsed voltage or RF signal is applied to the extractor electrode 106 to attract or repel ions. In another embodiment, the extractor electrode 106 is electrically floating. In various embodiments, the pulsed voltage is periodic or non-periodic and the RF signal is pulsed or CW. The pulsed and RF voltage signals may be used to enable desorption from or deposition on the electrode surface.

[0036] For illustration purposes, the description below will assume that only positive ions are sampled. It should be noted, however, that embodiments of the present disclosure can be easily adapted or configured for sampling of negative ions. Furthermore, for simplicity, the electrostatic lens 108 is referred to as Lens 1, the electrostatic lens 110 is referred to as Lens 2, and the drift tube 104 is referred to as Lens 3. Lens 1 and Lens 3 may be held at a same or similar potential which may be a fixed value between, for example, $-150V$ and

$-300V$. The desired potential is determined by factors, such as the length of the drift tube 104 and the desired ion mass resolution.

[0037] In some embodiments, Lens 1 and Lens 3 may be biased at different potentials (e.g., $V_{\text{sub.L1}}=-400V$ – $200V$ and $V_{\text{L3}}=-200V$). Lens 2 may be biased at $V_{\text{sub.L232}}=-500V$ – $900V$. Lens 2 may be further configured as a “gate” for the drift tube 104. To open the gate, a short voltage pulse (e.g., 50-500 nanosecond) may be provided to Lens 2 to admit a packet of ions into the drift tube 104. To close the gate, a relatively large positive potential may be imposed on Lens 2 to block positive ions from entering the drift tube 104. According to one embodiment, Lens 2 (i.e., gate electrode) may be normally biased with a positive voltage, e.g. $+30V$ or above, except during the very short gating period. For example, assuming that the gate pulse width is 100 ns, and the wafer’s pulse frequency is 5,000 kHz (period=200 microsecond) and that samples are performed once per wafer pulse, then during 99.95% of the period (199.9 microsecond) the gate electrode is closed and in only 0.05% of the period is the gate electrode open.

[0038] When the gate pulse is synchronized with the wafer pulse, a delay may be introduced to control where the gate pulse is open relative to the wafer pulse. In this way, it is possible to sample the plasma at different points in time space with a high resolution. The collective effect of the biases on Lenses 1-3 may be an electrostatic field that focuses the admitted ions into a beam with a limited divergence angle. On the detector side, the detector assembly 112 may be biased at a high voltage $V_{\text{sub.MCP}}$. The grid 124 may electrostatically shield the drift tube 104 from the high voltage $V_{\text{sub.MCP}}$.

[0039] The ion sensor 200 may also be configured for time-resolved measurements of a plasma. Many semiconductor processing plasmas are “pulsed plasmas” which alternate between on and off (afterglow) states periodically. The plasma-on state may last 1-50% (or higher) of each cycle. The pulsed operation can cause dynamic changes in plasma conditions and process chemistries. The sampling of the ion species may be synchronized with either the plasma pulses or wafer bias pulse, or both if they are synchronized. By changing the gate delay relative to the reference pulse (plasma pulses and/or wafer bias), time-resolved measurement could be carried out over the whole period.

[0040] The flight times of the ions are determined by observing the time difference between a start signal and a stop signal. The ion modulation event (an electrical or mechanical event) is initiated by the start signal. The stop signal is determined by the arrival time of the ions at the ion detector. In some embodiments, start and stop signals are used to gate a pulse train of known frequency to give a count that is proportional to the flight time. In one specific embodiment, the start and stop signals are used to generate a voltage across a capacitor, which is then discharged at a constant rate. The discharge period is used to gate a pulse train to give an count that is proportional to the flight time. In another embodiment, the start and stop signals are used to enable the generation of an analog pulse whose magnitude is proportional to the flight time.

[0041] The ion sensor 200 may also be configured to measure the energy distribution of the ions and/or the plasma potential. In one embodiment, an electrode or grid, such as the extractor electrode 106, the electrostatic lens 108, and the electrostatic lens 110 is biased to be a retarding element. The number of ions transmitted as a function of the electrode

voltage is then measured. Both the energy distribution and the plasma potential can be determined from the measured data.

[0042] In another embodiment, the energy distribution of the ions is determined by observing the spread in the arrival times of the ions at the detector assembly **122**. For example, position-sensitive particle detectors can be used to detect the ions at certain predetermined positions as described in connection with FIG. 1. Also, the energy distribution can be measured directly by methods that are well known in the art. For example, calibrated particle detectors can be used to measure energy or mass by observing the amplitude of signals generated by the detectors.

[0043] In yet other embodiments, the drift tube **104** is configured to perform the function of an energy analyzer. There are numerous ways to configure the drift tube **104** as an energy analyzer. For example, in one embodiment, the drift tube **104** is formed in a curved shape and includes electrostatic or magnetic deflection elements. The shape of the drift tube **104** is chosen so that ions with different energies bend with different angles. In another embodiment, the drift tube **104** includes a parallel-plate energy analyzer as part of the drift path to the detector assembly **112**. For example, the energy analyzer can be a 45 degree type energy analyzer. In another embodiment, the drift tube **104** includes a cylindrical mirror or a spherical energy analyzer as part of the drift path to the detector assembly **112**. In another embodiment, one or more grids are placed in the ion path to configure the drift tube **104** as a retarding potential analyzer. Also, in another embodiment, the drift tube can include a RF quadrupole or one or more permanent or electromagnets with the ability to differentiate between ions of different energies by adjusting the RF or DC voltages. The positions of the permanent magnets can be adjustable.

[0044] FIG. 2a shows an ion sensor **200A** having an energy analyzer **114** in accordance with an embodiment of the present disclosure. The energy analyzer **114** is positioned between the drift tube **104** and the detector assembly **112**. The energy analyzer **114** can be used to select ions within a desired energy range.

[0045] FIG. 3 shows an ion sensor **300** having another exemplary configuration in accordance with an embodiment of the present disclosure. The ion sensor **300** may comprise substantially the same components as the ion sensor **100** shown in FIG. 1. However, in this exemplary configuration, the extractor electrode **106** receives a RF (1-300 MHz, typically 13.56 MHz) bias. The RF biased extractor electrode **106** may serve dual functions. That is, the extractor electrode **106** may extract ions and also may remove deposits from the extractor aperture in a deposition-dominant environment.

[0046] Many semiconductor manufacturing processes are carried out in a deposition-dominant environment wherein thin-film materials are deposited in a plasma chamber. If a thick insulating film blocks the extractor aperture, a DC bias on the extractor electrode **106** may no longer be effective. A RF bias may help sputter clean the extractor aperture to remove the deposited materials. Thus, a RF bias may provide the ion sensor **300** with a "self-cleaning" capability. For ion extraction, the RF bias may have a negative average potential (or RF self-bias) between -50V and 0V, and a peak-to-peak value of 0V-100V. For sputter cleaning purposes, the RF self-bias may be larger than a sputtering threshold and the peak-to-peak value may be 100-1000V or higher.

[0047] FIG. 4 shows an ion sensor **400** having yet another exemplary configuration in accordance with an embodiment

of the present disclosure. The ion sensor **400** may comprise substantially the same components as the ion sensor **100** shown in FIG. 1. However, in this exemplary configuration the extractor electrode **106** also functions as a gate. A gate pulse may be provided to the extractor electrode **106** to pull a packet of ions into the ion sensor **400**. Lens **2** may be provided with a DC bias to focus the ion beam.

[0048] Ion sensors in accordance with embodiments of the present disclosure may be installed in a number of ways for flexible detection of ion species in a plasma chamber. Exemplary installation options are shown in FIGS. 5-7.

[0049] FIG. 5 shows one installation option for an ion sensor **508** in accordance with an embodiment of the present disclosure. An over-simplified plasma chamber **500** is shown with a platen/cathode **502** holding a wafer **504**. An anode **506** is positioned above the platen/cathode **502**. The anode **506** is not necessarily grounded but may be biased at a voltage, for example, that is between -1 kV and +1 kV (other voltages are possible). An anode shaft **507** may enable movement of the anode **506** in the vertical direction. A plasma **50** may be generated between the anode **506** and the platen/cathode **502**, either by cathode bias voltages or by additional plasma sources.

[0050] For ion implantation applications, negative voltage pulses may be applied to the platen **502** to draw positive ions towards the wafer **504**. For negative ions, positive voltage pulses may be used. The ion sensor **508** may be installed in a sidewall of the plasma chamber **500**. The installation may be through a view port or similar mechanism. The ion sensor **508** may have its extractor tip extended sideways into or near an edge of the plasma **50**. The extractor tip may be positioned on a movable mount. Due to the small size of the extractor tip, it may be inserted deep into the plasma **50** without significantly disturbing the plasma **50**.

[0051] FIG. 6 shows another installation option for an ion sensor in accordance with an embodiment of the present disclosure. In this installation option, instead of or in addition to the ion sensor **508** installed in the sidewall, an ion sensor **602** may be installed on the anode side. That is, the ion sensor **602** may be positioned through the anode **506** and may be vertically oriented with its extractor tip pointing downwards at or into the plasma **50**. The ion sensor **602** may be electrically connected with the anode **506**. The ion sensor **602** or its extractor tip may move up and down independent from the anode **506** to sample ions at different spatial points in the plasma chamber **500**. Alternatively, the ion sensor **602** or its extractor tip may move up and down together with the anode **506** for in-situ diagnostic of different process conditions. The horizontally positioned ion sensor **508** may be similarly actuated for a spatial measurement of the plasma **50**.

[0052] FIGS. 6a-c show different examples of plasma processing chambers in accordance with embodiments of the present disclosure.

[0053] In FIG. 6a, there is shown a plasma chamber **600A**. An ion sensor **602** may be installed through an anode **506**. A bellows seal **604** may accommodate installation and movement of the ion sensor **602** through the chamber wall. The plasma **50** may be generated by negatively pulsed voltages applied on the wafer **504** or the platen **502**. According to one embodiment, extraction of ions from the plasma **50** into the ion sensor **602** may be synchronized with the plasma generation, and therefore the voltage pulses on the wafer **504**.

[0054] In FIG. 6b, there is shown a plasma chamber **600B**. The plasma generation technique shown in FIG. 6b is differ-

ent from the plasma generation technique shown in FIG. 6a. The plasma chamber 600B may have one or more external plasma sources, such as, for example, ICP or Helicon plasma sources. For example, in one embodiment, a RF power supply 605 and a RF matching unit 607 is coupled to RF coils 606. Through dielectric interfaces 609, the RF coils 606 may supply RF electrical power into the plasma chamber 600B. The platen 502 may be biased to control the energy of ions that impact the wafer 504.

[0055] In FIG. 6c, there is shown a plasma chamber 600C, wherein another plasma generation technique is employed. One or more microwave sources may be coupled to the plasma chamber 600C to supply the power to generate and sustain the plasma 50. For example, a microwave supply 611 may be coupled to a microwave cavity 608 via a tuner 613 and a waveguide or cable. The microwave power supplied to the microwave cavity 608 may generate a "source plasma" therein, whereupon the source plasma may diffuse into the plasma chamber 600C to produce the plasma 50. Alternatively, the plasma 50 may be generated directly inside the plasma chamber 600C by coupling microwave power via the cavity 608 and into the plasma chamber 600C.

[0056] FIG. 7 shows yet another installation option for an ion sensor in accordance with an embodiment of the present disclosure. In this installation option, one or more ion sensors 702 may be installed on the cathode side. That is, an ion sensor 702 may be positioned vertically through the platen/cathode 502 with the extractor tip positioned next to the wafer 504. The installation location for the ion sensor 702 may be (or near) where a Faraday cup would be typically located. Since the extractor tip is pointing up at the plasma 50, the ion sensor 702 and the wafer 504 may share a same or similar vantage point with respect to the plasma 50. As a result, the ion sensor 702 may "see" the same composition and dose of ions as what the wafer 504 sees, which may facilitate a more accurate control of plasma processing of the wafer 504. In a plasma doping (PLAD) system, for example, the ion sensor 702 may be able to directly detect what ions are implanted into the wafer 504. If desired, the ion sensor 702 may also be moved up and down for a spatial measurement.

[0057] FIGS. 7a-b show exemplary systems for employing ion sensors for process control in accordance with embodiments of the present disclosure.

[0058] FIG. 7a shows an ion sensor 702 being installed next to the wafer 504. A Faraday cup 704 may be installed on the other side of the wafer 504 or the Faraday cup 704 may partially surround the wafer 504. Both the ion sensor 702 and the Faraday cup 704 face up to a plasma (not shown) as the wafer 504. The ion sensor 702 may be coupled to a unit 706 that calculates an in-situ ion composition based on detection data received from the ion sensor 702. The Faraday cup 704 may be coupled to a charge counter 708 that calculates a total ion dose based on the Faraday cup current. The ion composition information and the ion dose data may be input to a dose correction module 710. In addition, the ion composition data may be input to a system controller 712 for further process control.

[0059] FIG. 7b shows two or more ion sensors 702 being installed around the wafer 504. The in-situ ion composition data from these ion sensors 702 may be input to the system controller 712. Output functions 714 of the system controller 712 may include, but are not limited to, ion dose correction, dose uniformity control, plasma chamber conditioning, and/or process fault detection. In embodiments where the sensor

is installed in a platen around the wafer 504, the drift tube 104 (FIG. 1) may either be isolated from the platen or be at the platen potential.

[0060] For the cathode-side (or wafer-side) measurement of the plasma 50, the ion sensor 702 may be configured differently from those shown in FIGS. 2-4. One example is shown in FIG. 8.

[0061] FIG. 8 shows an exemplary ion sensor 800 in accordance with an embodiment of the present disclosure. The ion sensor 800 may comprise substantially the same components as the ion sensor 200 shown in FIG. 2, except that the extractor electrode 106 is removed. The housing aperture at the extractor side may be shrunk to approximately 10-500 microns (preferably 50-200 microns). The housing 102 may be biased at a same or similar potential (e.g., 0V--0 kV) as the wafer 504. Lens 1, Lens 3 (drift tube 104), and detector assembly 112 may also be biased at a same or similar potential. Lens 2 may function as a gate to pulse ion packets into the drift tube 104.

[0062] At this point it should be noted that the ion sensors in accordance with the present disclosure as described above typically involves the processing of input data and the generation of output data to some extent. In various embodiments, this input data processing and output data generation may be implemented in hardware or software. For example, specific electronic components may be employed in a plasma processing tool or similar or related circuitry for implementing the functions associated with in-situ monitoring of ion species in accordance with the present disclosure as described above. Alternatively, one or more processors operating in accordance with stored instructions may implement the functions associated with in-situ monitoring of ion species in accordance with the present disclosure as described above. If such is the case, it is within the scope of the present disclosure that such instructions may be stored on one or more processor readable carriers (e.g., a magnetic disk), or transmitted to one or more processors via one or more signals.

[0063] In one embodiment, the dose or plasma conditions may be changed as part of an automated or semi-automated closed control loop that includes a controller or computer and electronic instrumentation that is responsive to data obtained from TOF sensor according to the present invention. The data obtained from the detector assembly 112 can include the absolute or relative magnitudes of various portions of the measured TOF spectra. The data from the detector assembly 112 can also include the shape of the time-of-flight peaks, such as changes in FWHM. The data from the detector assembly 112 can also include the presence or absence of minor (contaminant) peaks, the energy distribution, and the mass distribution.

[0064] The data from the TOF sensor can be used to detect fault conditions, such as gas impurities, residual contaminants, and malfunctions of equipment used to control the plasma. The plasma conditions can be changed in response to the data by adjusting the TOF sensor's operating parameters, such as gas flow, gas mixture, pressure, RF power, RF frequency, implant voltage, duty cycle, or other plasma related parameter.

[0065] The present disclosure is not to be limited in scope by the specific embodiments described herein. Indeed, other various embodiments of and modifications to the present disclosure, in addition to those described herein, will be apparent to those of ordinary skill in the art from the foregoing description and accompanying drawings. Thus, such

other embodiments and modifications are intended to fall within the scope of the present disclosure. Further, although the particular implementation in a particular environment for a particular purpose, those of ordinary skill in the art will recognize that its usefulness is not limited thereto and that the present disclosure may be beneficially implemented in any number of environments for any number of purposes. Accordingly, the claims set forth below should be construed in view of the full breadth and spirit of the present disclosure as described herein.

What is claimed is:

1. A time-of-flight ion sensor for monitoring ion species in a plasma, comprising:

a drift tube disposed near an edge of the plasma;

an extractor electrode and a plurality of electrostatic lenses disposed at a first end of the drift tube, wherein the extractor electrode is biased to attract ions from a plasma in the plasma chamber, and wherein the plurality of electrostatic lenses cause at least one portion of the attracted ions to enter the drift tube and drift towards a second end of the drift tube within a limited divergence angle;

an ion detector disposed at the second end of the drift tube, wherein the ion detector detects arrival times associated with the at least one portion of the attracted ions; and

a housing for the extractor, the plurality of electrostatic lenses, the drift tube, and the ion detector, wherein the housing accommodates differential pumping between the ion sensor and the plasma chamber.

2. The ion sensor according to claim 1, wherein the extractor electrode is biased at a plurality of potentials that perform attraction and repulsion of ions from the plasma.

3. The ion sensor according to claim 1, wherein the extractor electrode is floating.

4. The ion sensor according to claim 1, wherein the extractor electrode is RF biased.

5. The ion sensor according to claim 4, wherein the extractor electrode is RF biased to cause one or more deposited materials on the extractor electrode to be sputtered.

6. A time-of-flight ion sensor for monitoring ion species in a plasma, the time-of-flight ion sensor comprising:

a housing;

a drift tube that is positioned in the housing;

an extractor electrode positioned in the housing at a first end of the drift tube, the extractor electrode being biased at a first potential to attract ions from the plasma and a second potential to repel ions from the extractor electrode;

a plurality of electrodes that are positioned at a first end of the drift tube proximate to the extractor electrode, the plurality of electrodes being biased so as to cause at least a portion of the attracted ions to enter the drift tube and to drift towards a second end of the drift tube; and

an ion detector that is positioned proximate to the second end of the drift tube, the ion detector detecting arrival times associated with the at least a portion of the attracted ions.

7. A method for monitoring ion species in a plasma, the method comprising:

applying a first bias voltage and a second bias voltage to an extractor electrode, the first and second bias voltage performing at least one of attraction and repulsion of ions;

applying a voltage signal to at least one of a plurality of electrodes that are positioned proximate to the extractor electrode, the voltage signal causing at least a portion of the attracted ions to drift through a drift tube;

detecting arrival times at an end of the drift tube, the arrival times being associated with the at least a portion of attracted ions; and

determining information about the plasma from the arrival times.

* * * * *