



(86) Date de dépôt PCT/PCT Filing Date: 1994/04/15

(87) Date publication PCT/PCT Publication Date: 1994/11/10

(45) Date de délivrance/Issue Date: 2005/09/13

(85) Entrée phase nationale/National Entry: 1995/10/24

(86) N° demande PCT/PCT Application No.: US 1994/004175

(87) N° publication PCT/PCT Publication No.: 1994/025110

(30) Priorité/Priority: 1993/04/30 (08/055,826) US

(51) Cl.Int.⁶/Int.Cl.⁶ A61B 17/36, A61B 17/34


(72) Inventeurs/Inventors:
NARDELLA, PAUL C., US;
YATES, DAVID CARLYLE, US

(73) Propriétaires/Owners:
ETHICON ENDO-SURGERY, US;
MEDICAL SCIENTIFIC, INC., US

(74) Agent: RICHES, MCKENZIE & HERBERT LLP


(54) Titre : TROCART ELECTROCHIRURGICAL BIPOLAIRE

(54) Title: BIPOLAR ELECTROSURGICAL TROCAR

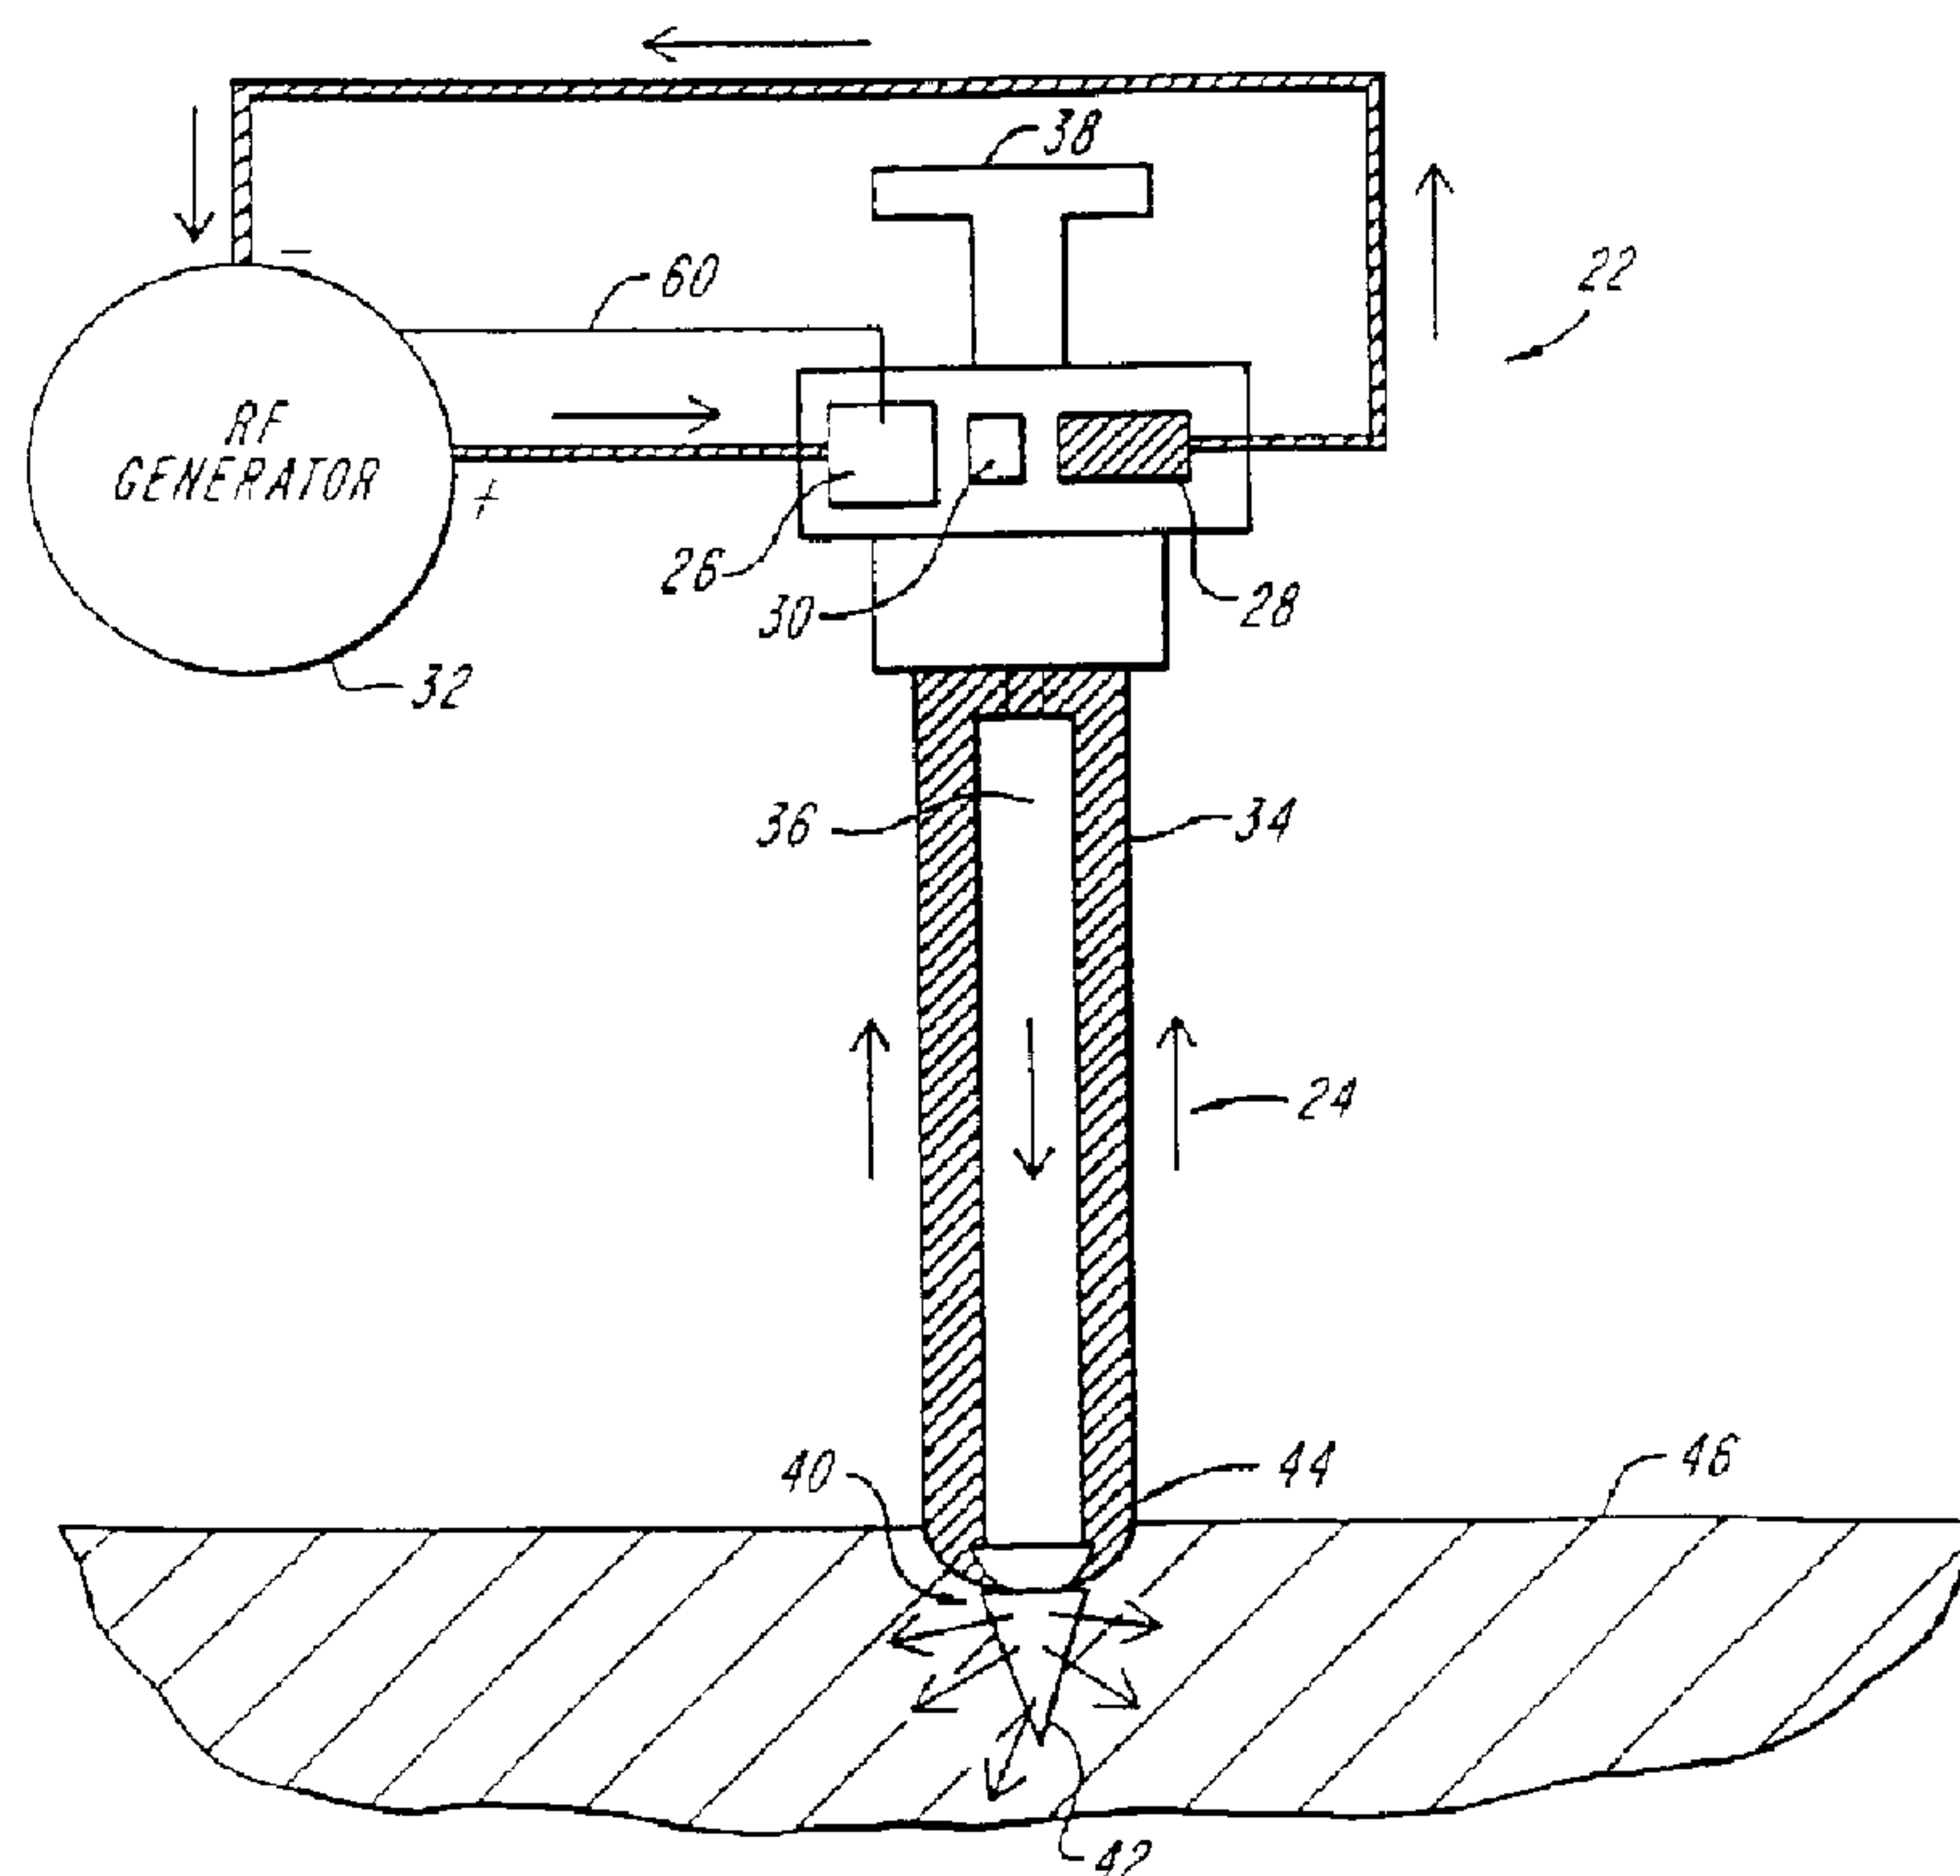

(57) Abrégé/Abstract:

The invention provides an electrosurgical tissue penetrating probe (e.g., a trocar) (24) for use with surgical procedures such as a laparoscopy. The trocar (24) has a stylet (36) disposed within the housing member (34), having an active electrode (42) disposed on a distal end thereof to deliver electrosurgical energy to the target tissue in contact with the stylet (36). A return electrode (48) is disposed on the housing member to form part of a return electrical path to the delivery electrosurgical energy. The invention also provides an electrosurgical trocar system having an impedance monitor and associated power regulating circuitry to control the amount of electrosurgical energy delivered to tissue so that the measured tissue impedance is maintained within a preselected range.

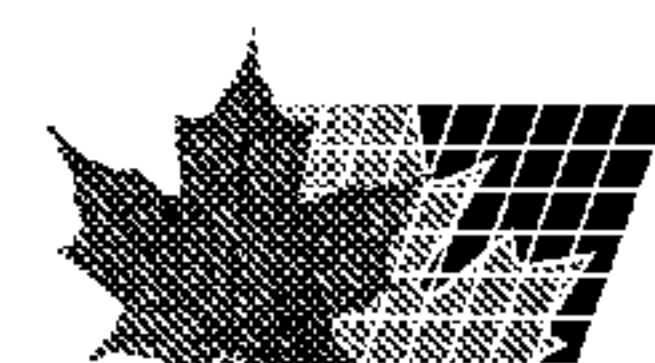



PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁵ : A61N 5/06	A1	(11) International Publication Number: WO 94/25110 (43) International Publication Date: 10 November 1994 (10.11.94)
(21) International Application Number: PCT/US94/04175 (22) International Filing Date: 15 April 1994 (15.04.94) (30) Priority Data: 08/055,826 30 April 1993 (30.04.93) US (71) Applicants: MEDICAL SCIENTIFIC, INC. [US/US]; 125 John Hancock Road, Taunton, MA 02780 (US). ETHICON, INC. [US/US]; 4545 Creek Road, Cincinnati, OH 45242-2839 (US). (72) Inventors: NARDELLA, Paul, C.; 140 Rockland Street, North Eaton, MA 02356 (US). YATES, David, Carlyle; 7434 Galway Court, West Chester, OH 45069 (US). (74) Agents: GEARY, William, C., III et al.; Lahive & Cockfield, 60 State Street, Boston, MA 02109 (US).		(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE). Published With international search report. With amended claims.

(54) Title: BIPOLAR ELECTROSURGICAL TROCAR

(57) Abstract

The invention provides an electrosurgical tissue penetrating probe (e.g., a trocar) (24) for use with surgical procedures such as a laparoscopy. The trocar (24) has a stylet (36) disposed within the housing member (34), having an active electrode (42) disposed on a distal end thereof to deliver electrosurgical energy to the target tissue in contact with the stylet (36). A return electrode (48) is disposed on the housing member to form part of a return electrical path to the delivery electrosurgical energy. The invention also provides an electrosurgical trocar system having an impedance monitor and associated power regulating circuitry to control the amount of electrosurgical energy delivered to tissue so that the measured tissue impedance is maintained within a preselected range.

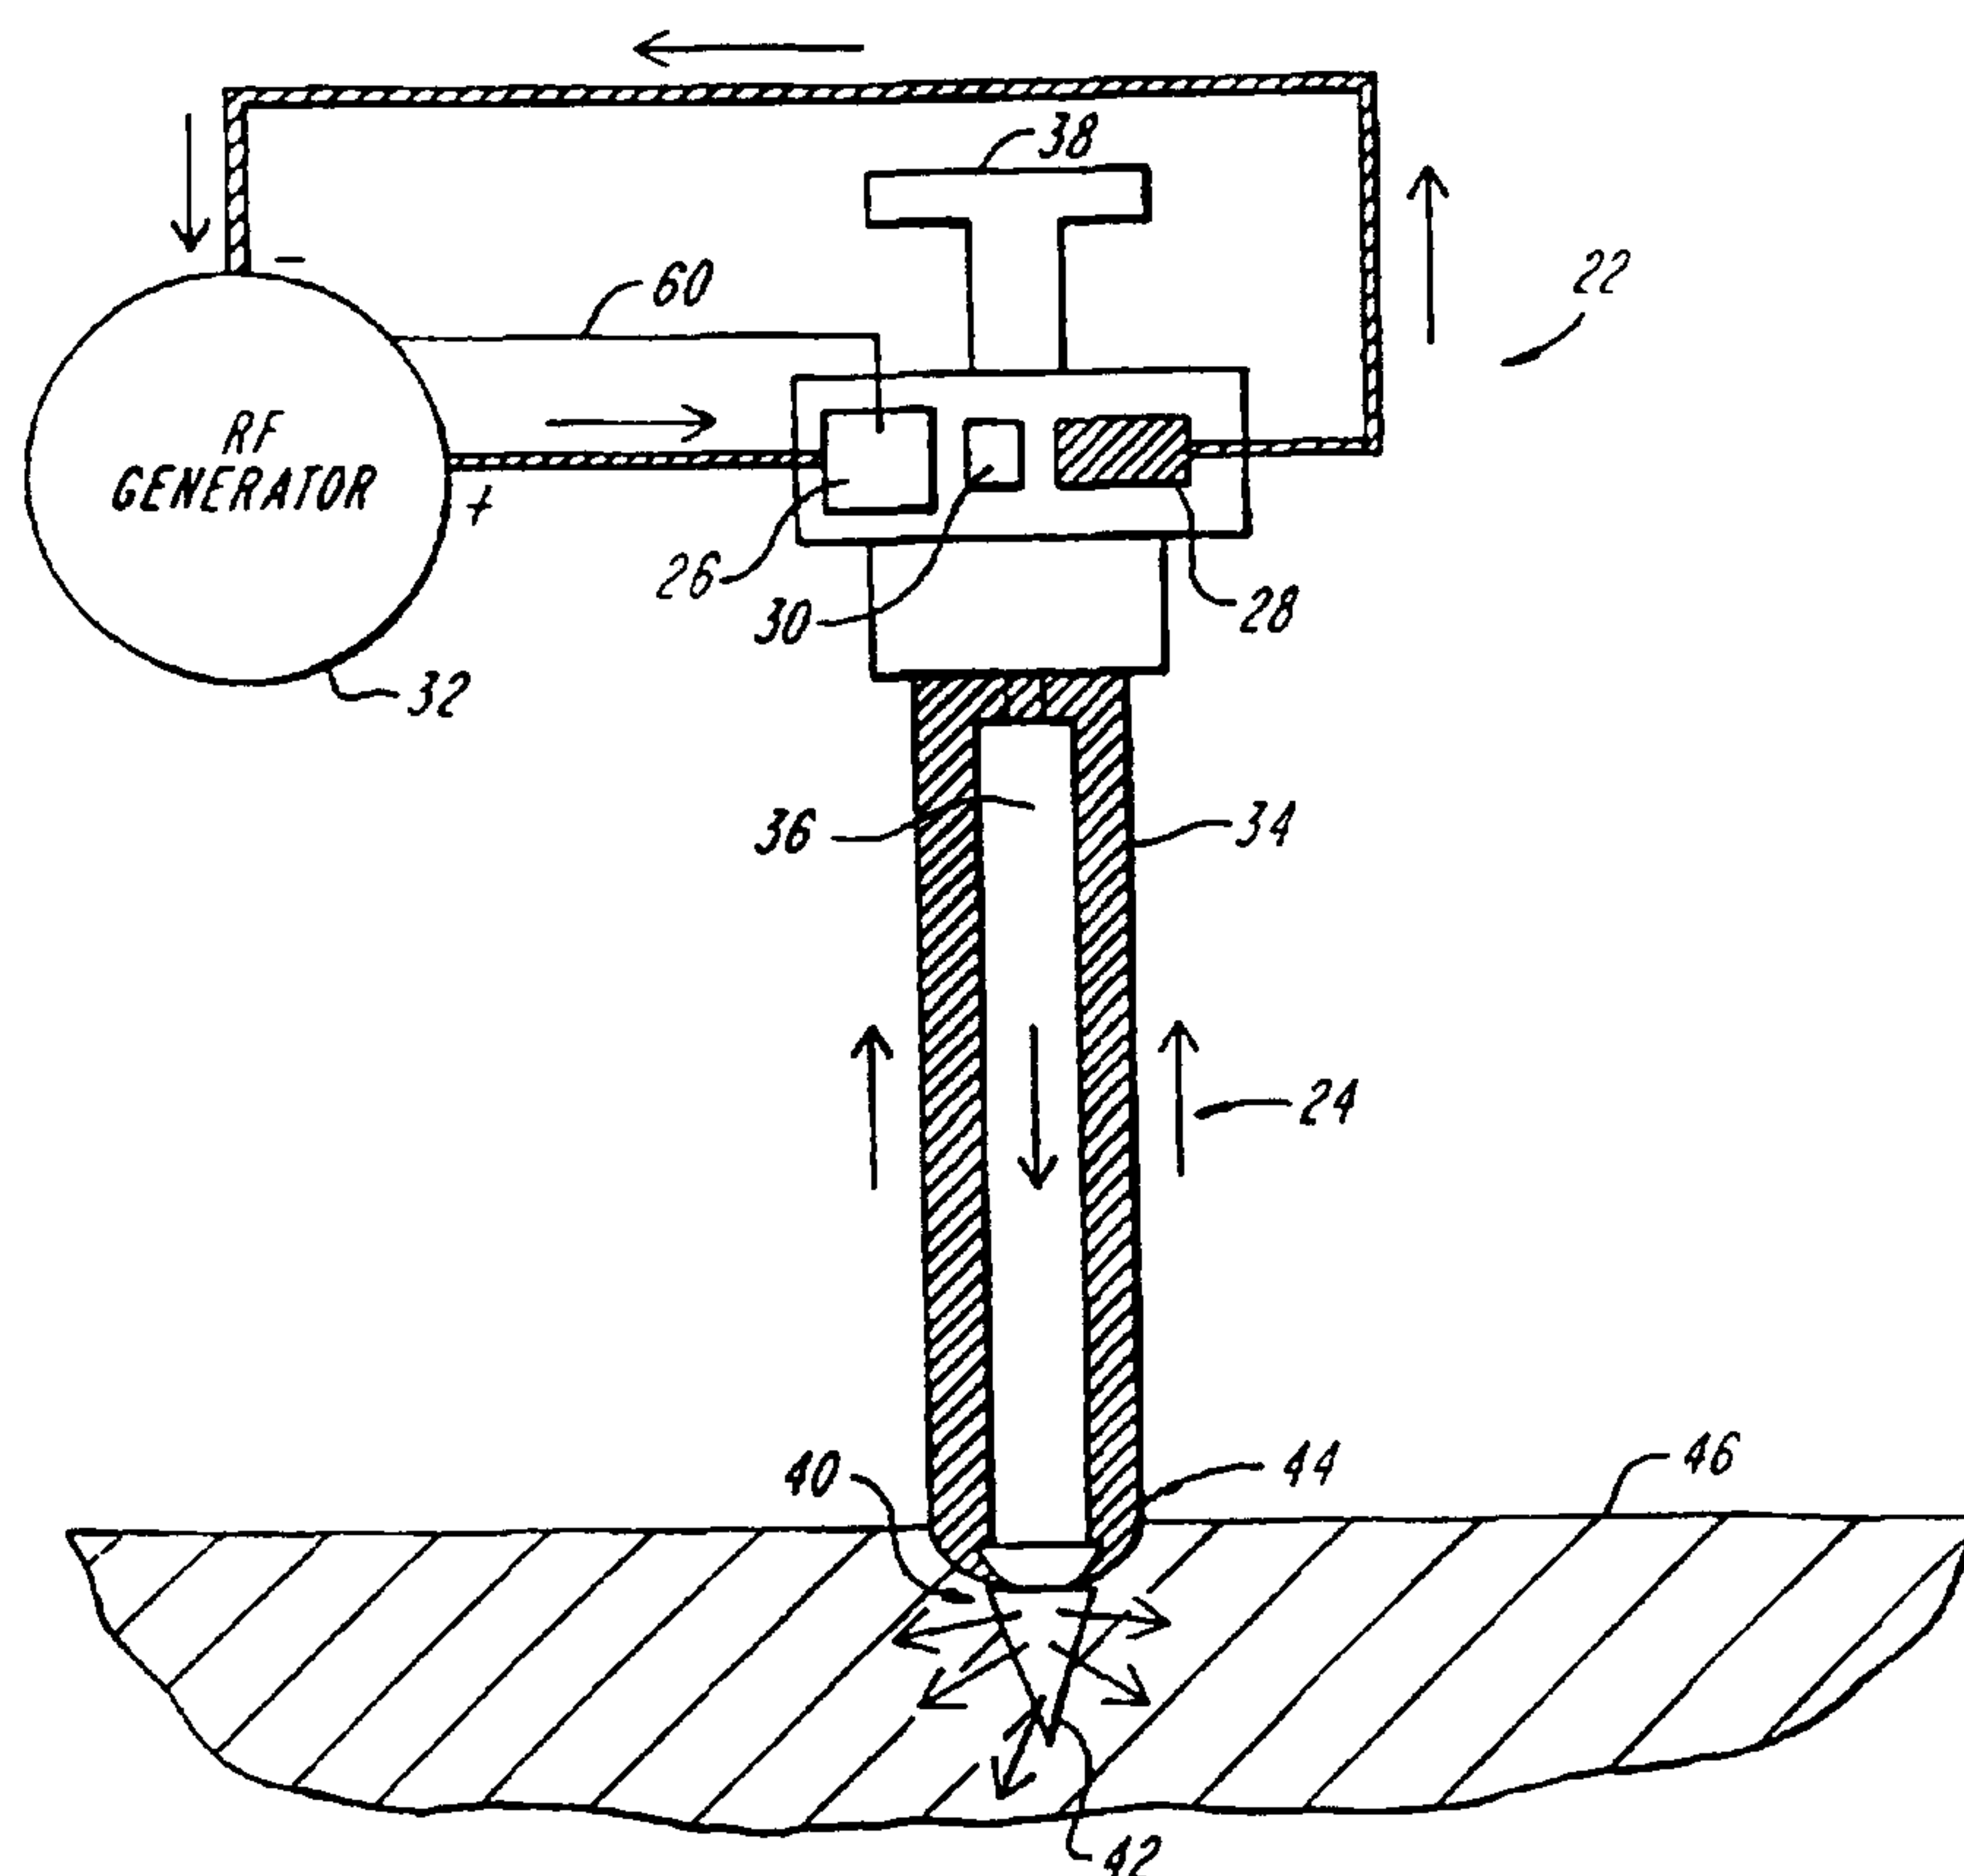

BIPOLAR ELECTROSURGICAL TROCAR

Background of the Invention

5 This invention relates generally to a bipolar electrosurgical device, such as a trocar, for penetrating tissue.

 Tissue penetrating probes, such as trocars and insufflation needles, are well known. A trocar typically includes an elongate stylet having a sharp, pointed obturator tip, disposed within a sheath or sleeve, and a handle portion that controls reciprocation of the stylet. A user of the trocar grips the handle and applies force such that the sharp tip of stylet penetrates tissue to a desired depth. A common use of the trocar is to gain access to the abdominal cavity for subsequent surgical purposes. This is typically accomplished by penetrating the abdomen with the tip of the stylet, removing the stylet from the sheath, and leaving the sheath within the abdominal wall to serve as a conduit to facilitate surgical procedures or inspections.

 Insufflation needles are known devices, smaller in diameter than trocars, that also enable penetration of the abdominal wall. These often are used to insufflate the abdominal cavity before a larger opening is made with a trocar.

 Electrosurgical energy, typically in the radio frequency range, has been used to enhance surgical procedures.

25 Various monopolar electrosurgical devices also are known. However, monopolar devices are not believed to be the most effective means for applying electrosurgical energy in surgical techniques. Typically, a remote ground pad is placed on the patient to form the negative pole in the electrosurgical circuit. The energy applied through the electrosurgical instrument must often traverse significant distances through the patient's body before reaching the return electrode. This can lead to ineffective control in applying the optimal amount of energy. In some instances patient burning can also result due to poor contact of the ground pad or ineffective control of energy delivery.

35 A trocar that uses electrosurgical energy is described in International Application No. WO/92/14514. The trocar can be monopolar or bipolar. In the monopolar mode the obturator tip of the trocar serves as the active electrode while a remote ground pad

serves as the return electrode. In the bipolar mode the obturator tip has two separate, insulated elements (forming a "duckbill" shape), each of which serves as one of the poles. Although this form of the trocar is bipolar in the sense that it forms both poles in circuit, it does so on the single cutting element and does not simultaneously function as a traditional trocar.

5

Despite existing technology applied to electrosurgical trocars, there remains a need for an effective bipolar trocar able to safely utilize electrosurgical energy to assist in penetrating and cauterizing tissue.

10

Accordingly, an object of the invention is to provide a bipolar tissue penetrating probe that uses electrosurgical energy to enhance tissue penetration and to cauterize tissue simultaneous with tissue penetration. Another object is to provide a bipolar trocar device able to penetrate and to cauterize tissue simultaneously. A further object of the invention is to provide such a device that enables more effective use of electrosurgical energy to penetrate and cauterize tissue. These and other objects of the invention will be evident from the disclosure that follows.

15

Summary of the Invention

20

The invention comprises a bipolar electrosurgical probe that simultaneously penetrates and cauterizes tissue. The probe preferably is a trocar, but can also take the form of other probes such as insufflation needles.

25

The electrosurgical trocar of the invention comprises a stylet disposed within a hollow housing or sheath member. The stylet includes a sharpened tissue penetrating obturator tip at its distal end and a handle, for manipulating the trocar, at its proximal end. The trocar further includes an active electrode formed by or on the tissue-penetrating obturator tip, and a return electrode formed by or disposed on a tissue contacting portion of the sheath member. Separate current communication lines connect between an external power source and the active and return electrodes.

30

35

The stylet further is adapted to reciprocate within the housing member, such that it can protrude from the open distal end of the housing member and retract within the housing. The trocar handle, mounted adjacent the proximal end of the housing member, is used both to manipulate the trocar and to control any axial displacement of the stylet.

In operation, the trocar is placed in contact with tissue and electrosurgical energy is delivered from an external source generator to the active electrode formed by the tissue penetrating distal tip of the stylet as tissue penetration is effected. The tissue

penetrating tip of the stylet, which serves as the active electrode, is electrically isolated from the return electrode mounted on the housing member. The active electrode (i.e. the edge) utilizes electrosurgical energy to assist in cutting and cauterizing tissue. The return electrode as noted above, serves as a ground.

5

In another aspect, the electrosurgical energy applied to the tissue can be regulated by monitoring tissue impedance. Once the tissue impedance is known, the generated electrosurgical energy can be regulated so that the current and voltage will change within the electrosurgical circuit to maintain a tissue impedance to within a
10 preselected range. The energy delivered to the active electrode can be shutdown, in another aspect, if the measured impedance is outside a preselected range or exceeds a preselected value.

Accordingly, in one of its broad aspects, the invention resides in providing
15 A bipolar electrosurgical trocar system, comprising: a trocar having an elongate hollow housing member having an open distal end and a return electrode associated with a tissue contacting portion at the distal end thereof; an elongate stylet, having, at a distal end thereof, an electronically conductive tissue-penetrating edge electrically isolated from the return electrode, the stylet being adapted for axial movement within the housing member
20 between an extended position in which the edge protrudes from the open distal end of the housing member, and a retracted position in which the edge is disposed within the housing member; handle means, adjacent a proximal end of the housing member, for manipulating the trocar and for controlling axial displacement of the stylet; active current communication means associated with the trocar for communicating electrical
25 energy through the trocar from a power source to the edge of the stylet for discharge through the edge to the tissue to be penetrated by the edge; return current communication means associated with the trocar for communicating the electrical energy delivered to the tissue by the edge from the return electrode to the power source; characterized in that the stylet has, at a distal end thereof, an electrically conductive spring electrode assembly
30 having said edge; and wherein the assembly, when confined within the housing member,

-3a-

is in a compressed condition; and when the assembly is in the extended position, is in an expanded condition and thereby providing a greater surface area.

In another of its broad aspects, the invention resides in providing An
5 electrosurgical tissue penetrating trocar device, comprising: a trocar having an elongate, hollow housing member having an open distal end; an elongate stylet having, at a distal end thereof, an electrically conductive tissue penetrating edge, the stylet being adapted for axial movement within the housing member between an extended position in which the edge protrudes from the open distal end of the housing member and a retracted position in
10 which the edge is disposed within the housing member; a handle element adjacent a proximal end of the housing member, the handle element being adapted to manipulate the trocar and to control axial displacement of the stylet; active current communication means associated with the trocar for communicating between a power source and the edge, the active current communication means being adapted to communicate electrical
15 current from the power source to the edge; characterised in that there is further provided a radially expendable element having said edge, the radially expendable element being capable of increasing the diameter of the edge in contact with tissue when the tissue penetrating edge is in the extended position and protrudes from the housing member.

20 Although the invention is primarily disclosed with respect to a bipolar trocar, the invention also relates to other bipolar tissue penetrating probes such as insufflation needles.

These and other aspects will be apparent from the following description,
25 were the invention is described and illustrated in connection with certain preferred embodiments. However, it should be clear that various additions, subtractions, and modifications can be made by those skilled in the art without departing from the scope of the invention.

-3b-

Brief Description of the Drawings

FIGURE 1 schematically illustrates a prior art trocar before and after tissue
5 penetration.

FIGURE 2 schematically illustrates an electrosurgical trocar system
constructed according to the present invention.

10 FIGURE 3 schematically illustrates a distal end of a trocar of the type
illustrated in Figure 2.

FIGURE 4A schematically illustrates an alternative embodiment of a trocar
device having a tissue penetrating electrode in a retracted position.

15

FIGURE 4B schematically illustrates the trocar of Figure 4A with the
tissue penetrating electrode in an extended position.

Detailed Description of the Invention

FIGURE 1 illustrates a prior art trocar 10 prior to (A) and after (B) penetrating tissue 12. In configuration A, the trocar 10 is simply in contact with the tissue 12 at a surface location 13. In configuration B, the trocar 10 has penetrated tissue 12 to a depth 15 by extending the distal, pointed end 17 of the stylet from within the housing member into the tissue 12.

The prior art trocar 10 as illustrated has an outer housing member 14 and an inner stylet 16 which can be axially displaced within the housing 14. A handle 18 is disposed at proximal end 20 of the trocar and is used to both control the trocar and to axially drive the stylet 16 out of the distal end of the housing member 14.

FIGURE 2 illustrates a bipolar electrosurgical trocar system 22 constructed according to the invention. As illustrated, system 22 comprises an electrosurgical trocar 24 which preferably includes a power control module 26, an impedance monitor 28 and an activation switch 30. The power control module 26 and impedance monitor 28 are in communication with a source of electrosurgical energy such as RF generator 32.

The trocar 24 includes an elongate, hollow housing or sheath 34 within which is disposed an elongate stylet 36. Preferably a handle 38 is mounted at a proximal portion of the trocar and is secured to a proximal end of the stylet 36 to facilitate axial movement of the stylet such that its distal tip 40 may be retracted within the sheath 34 and extended beyond sheath 34. The distal end 40 of the stylet comprises a sharp obturator tip 42 that is adapted to penetrate tissue when extended from the distal end of sheath 34. Preferably, the distal end of sheath 34 includes an opening that enables at least a portion of the obturator tip 42 to extend therefrom, but which prevents the entire stylet 36 from passing through the opening.

It should be clear to those skilled in the art that the system 22 is illustrative rather than limiting. For example, the power control module 26, impedance monitor 28, and activation switch 30 can be configured external to the remainder of the trocar 24, for example at the RF generator 32. Accordingly, a trocar constructed in accordance with the invention can comprise an electrosurgical trocar which is adaptable to external electronics, for example one with current communication lines disposed with the trocar to electrically connect the electrodes and to one or more electronic devices. Alternatively, one of ordinary skill in the art will appreciate that the trocar 24 can be constructed to have a generator unit and the associated electronics mounted upon the trocar itself.

FIGURE 3 illustrates a distal portion 44 of a trocar device constructed in accordance with the invention, for example for use with the trocar 24 illustrated in FIGURE 2. As illustrated, the distal portion 44 of trocar 24 is configured as a bipolar electrosurgical instrument adapted to apply electrosurgical energy to tissue 46. Obturator tip 42 preferably serves as an active, energy delivering electrode such that tissue penetration is enhanced and cauterization is achieved by the delivery of electrosurgical energy from obturator tip 42 to tissue 46. Preferably, one or more electrodes 48 disposed at a lower, tissue contacting portion 49 of sheath 34 serve as return or ground electrodes. The tissue penetrating obturator tip 42 preferably is in electrical contact with a first communication line 50 that communicates with an external power source such as generator 32 to enable the tip 42 to serve as an electrosurgical energy delivering electrode. Similarly, second communication line 52 is in circuit with the return electrodes 48 to provide communication with the ground or negative pole of a power source such as RF generator 32.

The tip 42 can also include a penetrating wire (not shown) extending from the distal end of the device 44. Such a wire preferably is connected electrically to the active electrode at the tissue-penetrating edge 42 and functions to reduce the force of entry required to penetrate tissue. Preferably, in this configuration, only the extreme distal end of the tip 42 would serve as a conductive electrode to deliver energy to tissue. This increases the current density at the distal tip 42 (and extended wire), thus heating only a small portion of a wound. The distance by which penetrating wire extends from tip 42 may vary, but typically is on the order of about 0.5 cm.

During use, the distal tip 44 of the bipolar trocar 24 shown in FIGURE 3 forms a part of the circuit used to apply electrosurgical energy to tissue. The tissue-penetrating obturator tip 42 functions as the positive pole of the circuit and the return electrodes 48 function as the negative pole. Thus an external power source, e.g., illustrated as the generator and monitor 32, can be connected to the obturator tip 42 and to the return electrodes 48 to complete the circuit with the tissue 46, thereby forming the bipolar electrosurgical trocar of the invention.

As further shown in FIGURE 3, the first communication line 50 may extend from generator 32 through the interior of sheath 34, and terminate at a point on the obturator tip 42. In another embodiment (not illustrated) stylet 36 may be made entirely of a conductive material and line 50 may simply extend from generator 32 and terminate at a proximal portion of the stylet. Stylet 36, as noted above, preferably is made entirely of a conductive material such as surgical grade stainless steel. Alternatively, the stylet can be made of stainless steel, and have a highly conductive material (e.g., gold, silver, or platinum) coated upon the obturator tip 42. In this embodiment it is preferred to have the

communication line 50 extend from the generator 32 to the conductive coating of the obturator tip 42.

5 Sheath 34 preferably is manufactured from a surgically compatible polymeric material of the type known in the art. A distal, tissue contacting portion 49 of sheath 34 preferably includes one or more electrodes 48 positioned so as to contact tissue when obturator tip 42 is in contact with tissue. Electrodes 48 can be point electrodes disposed at a bottom tissue contacting portion 49 of sheath 34 as illustrated in FIGURE 3. Alternatively, the electrodes may comprise one or more ring electrodes (not shown) that extend about the
10 outer circumference of the bottom portion 49 of sheath 34. Similarly, the tissue-penetrating obturator tip 42 can form an annulus or cone shaped (not shown) active electrode that extends about the circumference of the tip.

In another embodiment, sheath 34 may be manufactured from or coated with a
15 conductive material. For example, sheath 34 may be made entirely of a conductive material, as long as it is electrically isolated from stylet 36. When the entire sheath is made of a conductive material, it is preferred to apply an insulating material over at least a portion of the outer surface of the sheath 34. Electrodes 48 may also be formed from a conductive coating applied to a distal, tissue contacting surface of sheath 34.

20

The electrodes 48 communicate with generator 32 through second communication line 52. Communication line 52 preferably extends through the interior of sheath 34, terminating at electrodes 48. If sheath 34 is made entirely of a conductive material communication line 52 need only connect to a proximal portion of sheath 34.

25

Electrodes 48 are, of course, manufactured from a conductive material suitable for use in surgical applications. Suitable materials include gold, silver, and platinum.

As noted, FIGURE 2 illustrates an electrosurgical trocar system 22 constructed
30 in accordance with the invention. The electrosurgical trocar system 22 has a stylet 36 disposed within a sheath member 34. The stylet 36 and sheath 34 together function as the two poles of the system 22 when connected to an RF generator 32. The stylet 36 has a tissue penetrating obturator tip 42 at its distal end which forms the active electrode at the positive pole, while a distal, tissue contacting portion 49 of the sheath member 34 functions as the
35 return electrode or negative pole of the system. In order for the trocar 24 to effectively function as a bipolar surgical instrument it is necessary that the obturator tip 42, serving as the active electrode, be electrically isolated from the return electrode(s) 48.

-7-

As further illustrated in FIGURE 2, system 22 may also include power control module 26, impedance monitor 28, and activation switch 30. The impedance monitor 28 preferably determines the impedance of tissue 46 by quantifying the applied electrosurgical voltage and current within the circuit of the system 22 when in contact with the tissue 46.

5 The impedance monitor 28 then transmits a signal representative of tissue impedance to the power control module 26 via internal circuitry (not shown). The power control module 26 responds to this signal and further communicates with the RF generator 32 via signal line 60 to regulate the flow of electrosurgical energy to the tissue 46. Preferably, the electrosurgical energy is regulated such that the tissue impedance as measured by impedance monitor 28

10 remains within a preselected range, such as about 20-500 Ohms. Preferably, the power control module is further arranged to cease the flow of electrosurgical energy to the tip 42 when the measured impedance changes significantly or is outside the preselected range.

As further shown in FIGURE 2, the activation switch 30 allows an operator to

15 halt the flow of energy at any time, and thus functions as an electrical switch for the entire system. Although switch 30 is illustrated as mounted on trocar 24, it is understood that the switch may alternatively be located remote from the trocar, such as on a foot pedal (not shown).

20 In operation, the active electrode-obturator tip 42 delivers electrosurgical energy to the tissue 46 while the return electrode(s) 48 mounted on outer sheath member 34 receives the energy within the tissue by completing the circuit. This enhances the performance of the trocar as both the obturator tip 42 and the applied electrosurgical energy cooperate to penetrate and cauterize tissue simultaneously. The application of energy to tissue enhances

25 the cutting performance of the obturator tip and also acts to cauterize tissue. This eliminates or reduces any bleeding associated with trocar use and accordingly reduces trauma.

The trocar construction of the present invention is also advantageous as it operates as a bipolar surgical instrument and requires no ground pad. This enables more

30 effective and controlled application of electrosurgical energy with reduced risk of patient burning.

Virtually any generator able to provide electrosurgical energy for medical applications may be used with the present invention. Preferably, the generator 32 is a voltage

35 determinative, low source impedance generator that provides radio frequency energy. A preferred generator is able to supply up to 3 amps of current and has an impedance value of less than 10 ohms.

WO 94/25110

PCT/US94/04175

-8-

The energy supplied by the generator 32 to the trocar 24 preferably is in the radio frequency (RF) range. Although virtually any frequency in the RF range may be supplied to trocar 24, the preferred range is about 500 to 700 KHz, and most preferably about 550 KHz.

5

FIGURES 4A and 4B illustrate a distal portion of an alternative embodiment of a trocar-like device 70. As illustrated, the device 70 includes a stylet 71 enclosed within an elongate hollow housing member 74. A distal portion of stylet 71 includes a spring electrode assembly 78 having a tissue penetrating edge 72 at its distal end. Block 76 simply illustrates that the device 70 is preferably connected to a handle and other selective operable features, as described above.

The tissue penetrating edge 72 and spring electrode assembly or radially-expandable element 78 form the active electrode used to deliver electrosurgical energy to the tissue. In this embodiment the active electrode may, for example, take the form of tip 42 as shown in FIGURE 3. Similarly, the housing member 74 includes a return electrode (not shown) to form the inventive bipolar device described herein. The active electrode at the tissue penetrating edge 72 is electrically isolated from the return electrode disposed on the housing by any suitable arrangement, for example, as described above with respect to FIGURES 2 and 3. Moreover, the active electrode can comprise the entire surface area of the spring electrode assembly 78, or just a portion thereof.

FIGURE 4A illustrates device 70 having spring electrode assembly 78 disposed within housing 74 in a retracted position. Spring electrode assembly 78 preferably is formed of or is coated with a medically compatible conductive material. Moreover, the assembly 78 is made of a pliable material or is otherwise biased to an expanded position. When retracted within housing 74, as shown in FIGURE 4A, the assembly 78 is compressed. When the spring electrode assembly 78 is extended from housing 74, such as by actuation of stylet 71, the assembly 78 is free to expand to its natural configuration. As illustrated in FIGURE 4B, the natural configuration of assembly 78 preferably is one where the diameter of spring electrode assembly 78 is greater than when it is compressed within housing 74.

This embodiment is advantageous because in the extended position the spring electrode assembly 78 has a greater surface area. Thus, the tissue penetrating edge 72 is able to contact more tissue and deliver more electrosurgical energy to the tissue than could safely be delivered with a more conventional tissue penetrating edge.

FIGURES 4A and 4B further illustrate that housing 74 can have a safety switch or shield 80. As illustrated the shield 80 is spring loaded and is biased to an extended

position, as in FIGURE 4A, in which it extends beyond the distal end of housing 74. The application of a compressive force to the distal end of shield 80 will cause the shield to slide rearwardly (as shown in FIGURE 4B) to expose the distal end of housing 74 to tissue. When the force is removed from the distal end of shield 80, e.g., when the device 70 penetrates an
5 internal barrier such as the abdomen, shield 80 returns to its extended position.

Preferably, shield 80 acts as a switch and is connected in circuit with the electrosurgical delivery electronics. When the shield 80 is in the extended position the flow of energy to tissue is prevented. However, when the shield 80 is in the retracted position
10 energy is free to flow to tissue.

Thus, device 70 as described above is suitable for delivering electrosurgical energy to tissue in a trocar-like fashion. The device 70 can be further arranged to include impedance monitoring and power control electronics, as described with respect to
15 FIGURES 2 and 3, to measure and control the flow of energy to the tissue based upon tissue impedance. The device 70 has the additional advantage of expanding the surface area contact of the active electrode to the target tissue during operation. This improves the delivery and flexibility of electrosurgery because tissue impedance is a function of the electrode's surface area, the distance between the electrodes, and the conductivity of the tissue, as well as the
20 changes in tissue that result from heating.

It is understood that various modifications may be made to the invention described and claimed herein without departing from its intended scope. For example, the trocar-like devices described herein can also be constructed in a monopolar configuration,
25 where the return electrode to an external generator is arranged externally to the device, such as through a ground pad. Furthermore, an activation switch, such as illustrated by item 30 in FIGURE 2, is preferably arranged with each device constructed in accordance with the invention to improve patient safety while operating the device. A switch so constructed would enable the user to quickly and easily inhibit the power delivered to the patient. Also,
30 the configuration of the electrodes formed at the tissue-penetrating edge and on the housing member can form a variety of shapes, including, for example, the conical tip shape illustrated in FIGURE 2, or a pyramid shape, or a blunt tip, or as an annulus.

It is accordingly intended that all matters contained in the above description or
35 shown in the accompanying drawings be interpreted as illustrative rather than in a limiting way.

What is claimed is:

1. A bipolar electrosurgical trocar system, comprising:
 - a trocar having an elongate hollow housing member having an open distal end and a return electrode associated with a tissue contacting portion at the distal end thereof;
 - an elongate stylet, having, at a distal end thereof, an electronically conductive tissue-penetrating edge electrically isolated from the return electrode, the stylet being adapted for axial movement within the housing member between an extended position in which the edge protrudes from the open distal end of the housing member, and a retracted position in which the edge is disposed within the housing member;
 - handle means, adjacent a proximal end of the housing member, for manipulating the trocar and for controlling axial displacement of the stylet;
 - active current communication means associated with the trocar for communicating electrical energy through the trocar from a power source to the edge of the stylet for discharge through the edge to the tissue to be penetrated by the edge;
 - return current communication means associated with the trocar for communicating the electrical energy delivered to the tissue by the edge from the return electrode to the power source; characterized in that the stylet has, at a distal end thereof, an electrically conductive spring electrode assembly having said edge; and wherein the assembly, when confined within the housing member, is in a compressed condition; and when the assembly is in the extended position, is in an expanded condition and thereby providing a greater surface area.
2. A system as claimed in claim 1 wherein the assembly when in the extended position, has a diameter greater than that of the assembly when in the compressed condition.
3. A system as claimed in claim 1 or claim 2, further comprising a shield means for controlling the level of electrical energy from the spring electrode assembly to

adjacent tissue, the shield means comprising an annular member slideably mounted upon a distal end of the housing and moveable between an extended position in which energy delivery is prevented and a retracted position in which energy delivery is permitted.

4. A system as claimed in claim 3 wherein the annular member is biased to the extended position.
5. A system as claimed in any of claims 1 to 4 further comprising impedance measurement means, in circuit with the active current communication means and return current communication means, for measuring the electrical impedance of the tissue based upon the current within the tissue and generating a signal representative of tissue impedance; and
a power control means, in circuit with the impedance measurement means and the remote power source, for regulating the electrosurgical energy delivered to the tissue from the edge in response to a signal from the impedance measurement means to maintain a measured tissue impedance to within a preselected range.
6. A system as claimed in claim 5, wherein the preselected range of the tissue impedance is between 20-500 Ohms.
7. An electrosurgical tissue penetrating trocar device, comprising:
a trocar having an elongate, hollow housing member having an open distal end;
an elongate stylet having, at a distal end thereof, an electrically conductive tissue penetrating edge, the stylet being adapted for axial movement within the housing member between an extended position in which the edge protrudes from the open distal end of the housing member and a retracted position in which the edge is disposed within the housing member;

a handle element adjacent a proximal end of the housing member, the handle element being adapted to manipulate the trocar and to control axial displacement of the stylet;

active current communication means associated with the trocar for communicating between a power source and the edge, the active current communication means being adapted to communicate electrical current from the power source to the edge;

characterised in that there is further provided a radially expendable element having said edge, the radially expendable element being capable of increasing the diameter of the edge in contact with tissue when the tissue penetrating edge is in the extended position and protrudes from the housing member.

8. A device according as claimed in claim 7, further comprising return current communication means, associated with the trocar and electrically isolated from the active current communication means, for communicating the electrical energy from a return electrode to a power source.
9. A device as claimed in claim 7 or claim 8 wherein the radially expendable element is a spring.
10. A device as claimed in any one of claims 8 to 10 wherein the stylet is removeably disposed within the housing such that the stylet can be removed from the housing following penetration of tissue.
11. A device as claimed in any one of claims 7 to 10 wherein the return current communication means is comprised of a tissue contacting return electrode mounted on a distal portion of the housing member, the return electrode being electrically isolated from the electrically conductive tissue penetrating edge.
12. A device as claimed in any one of claims 7 to 11, further comprising a controller element adapted to selectively activate and regulate the electrosurgical

energy delivered though the active current communication means to the edge of the stylet.

13. A device as claimed in any one of claims 7 to 12, wherein the edge further comprises an energy delivering wire extending from the distal end of the stylet, the wire serving to reduce the force required to penetrate tissue.
14. A device as claimed in any one of claims 8 to 13, further comprising an impedance measurement element in circuit with the active and return current communication means, the impedance measurement element providing to the controller element a signal indicative of measured tissue impedance.
15. A device as claimed in claim 14 wherein the controller element inhibits the flow of energy to the edge in response to the signal from the impedance measurement element when the measured tissue impedance exceeds a preselected value.
16. A device as claimed in any one of claims 7 to 15, further comprising a shield element having an annular member slideably mounted upon a distal end of the housing and movable between an extended position in which energy delivery is prevented and a retracted position in which energy delivery is permitted.
17. A device as claimed in claim 16, wherein the annular member is biased to the extended position.

2/2

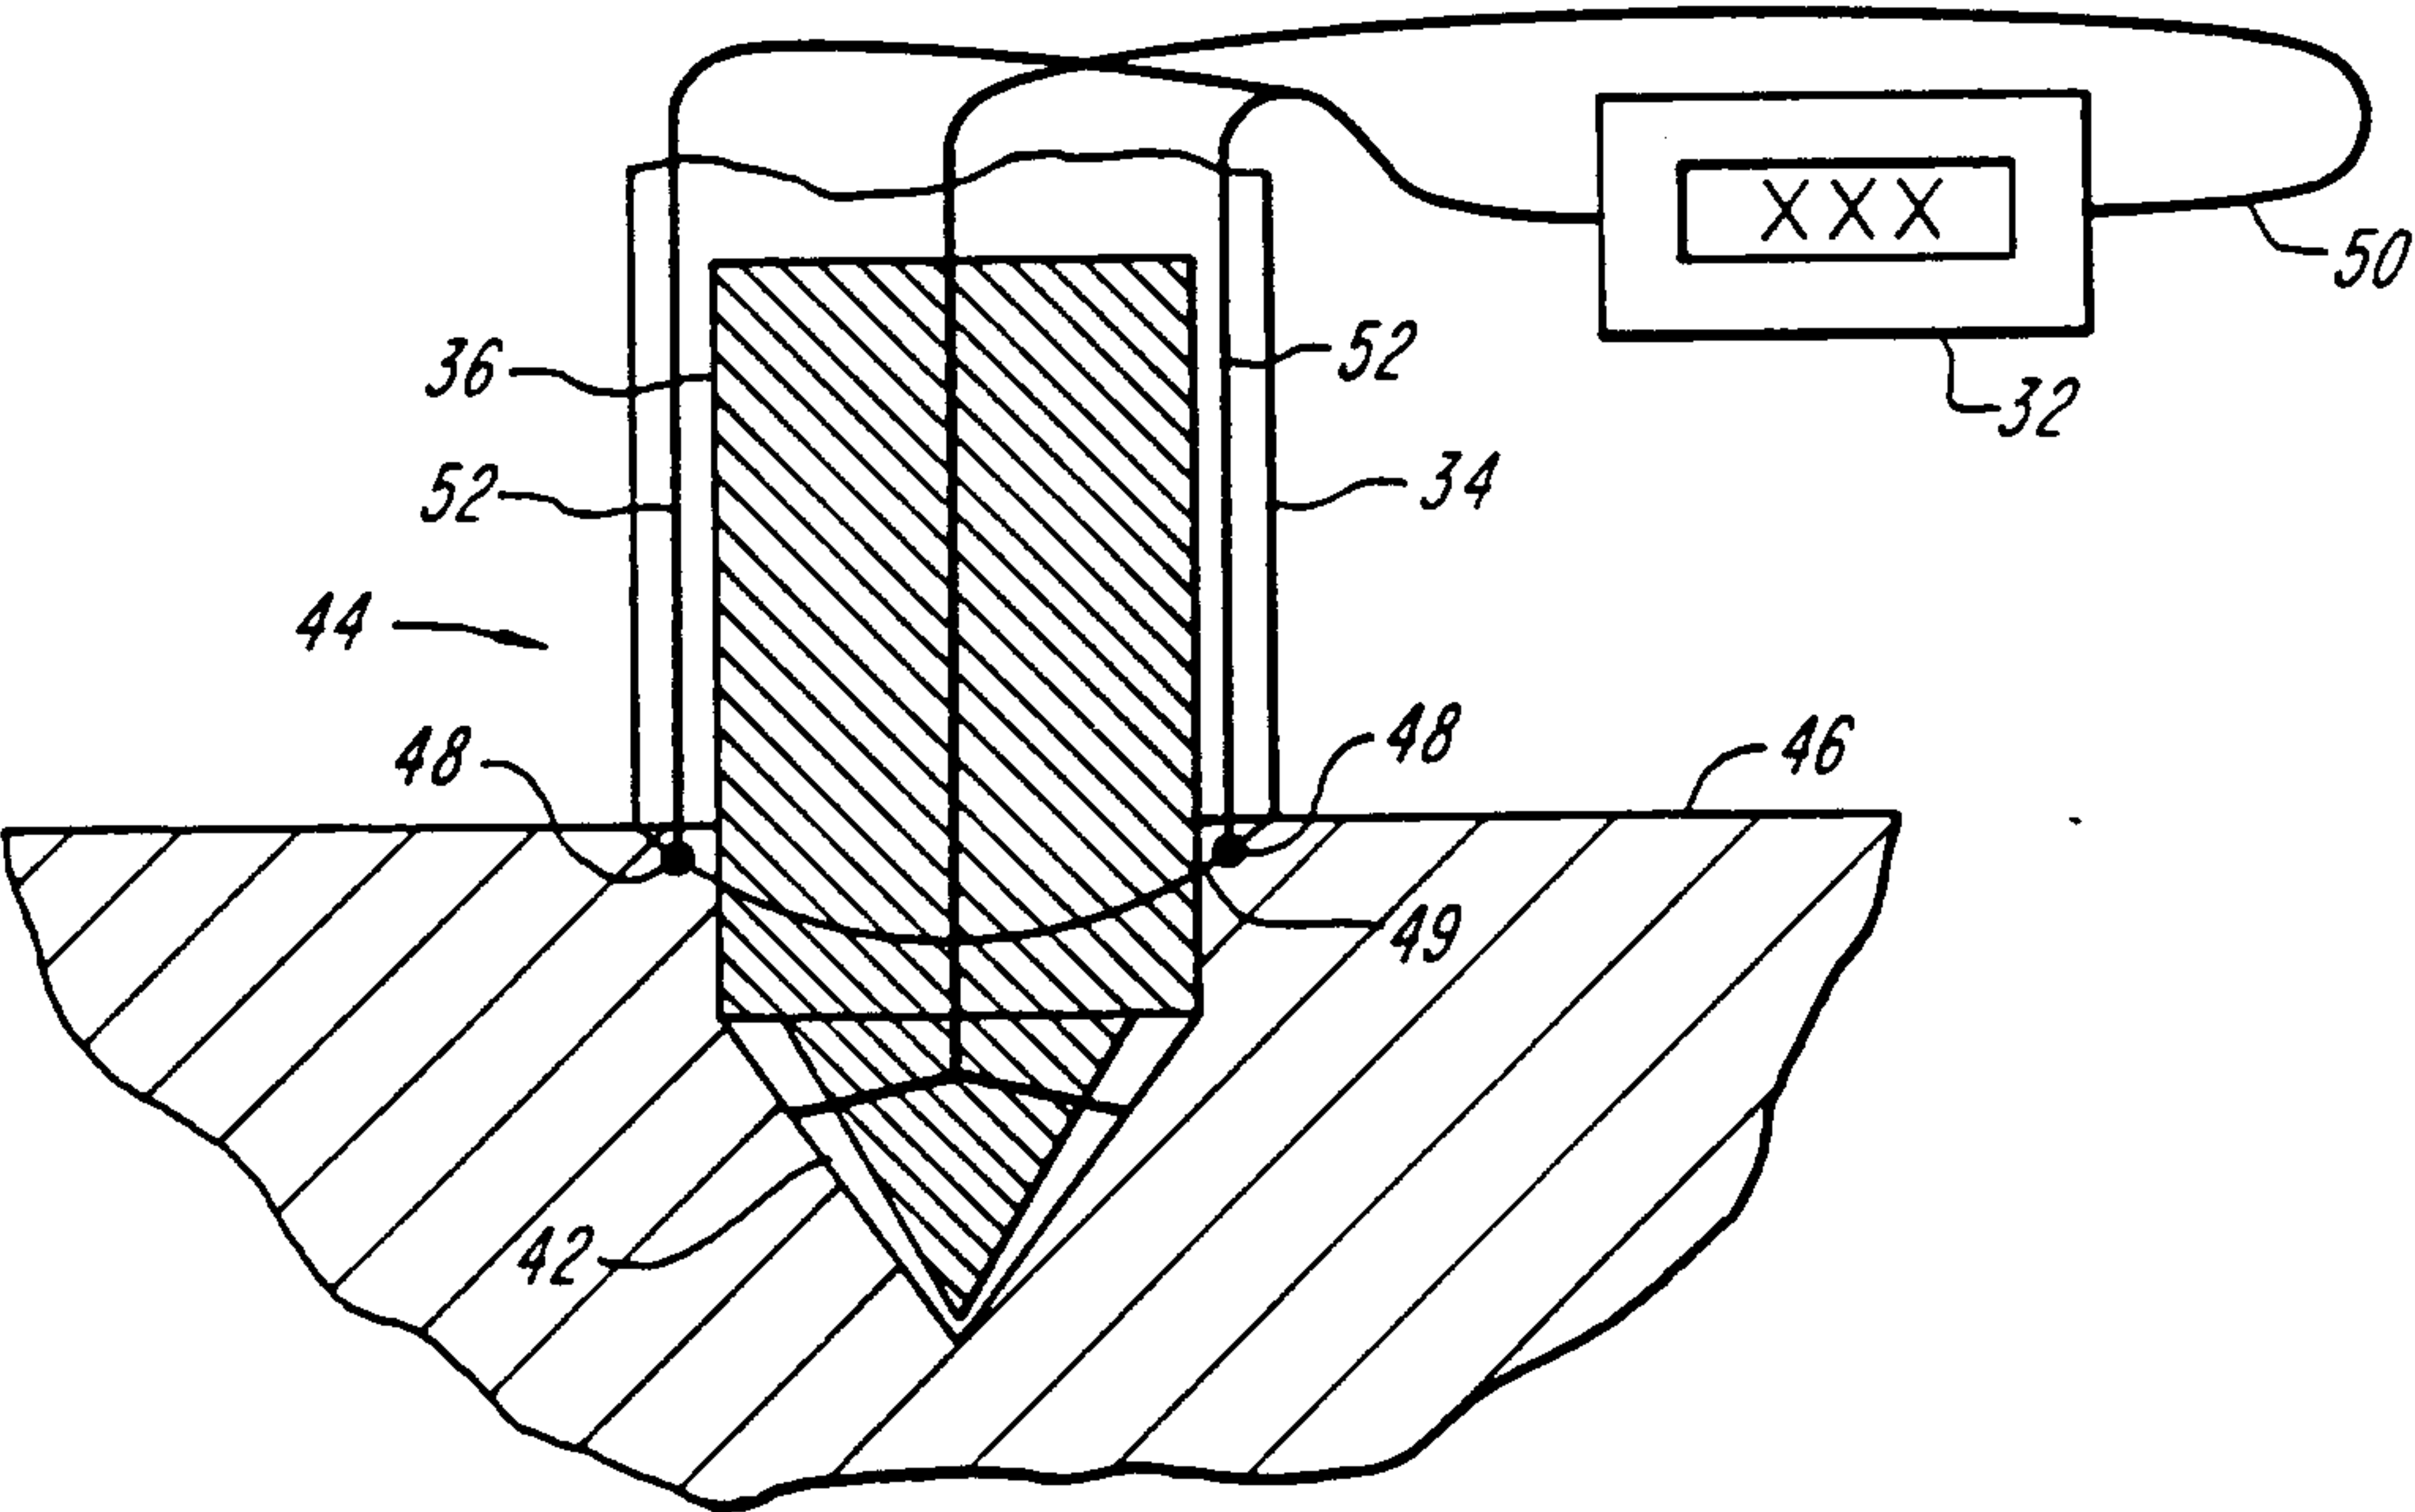


FIG. 3

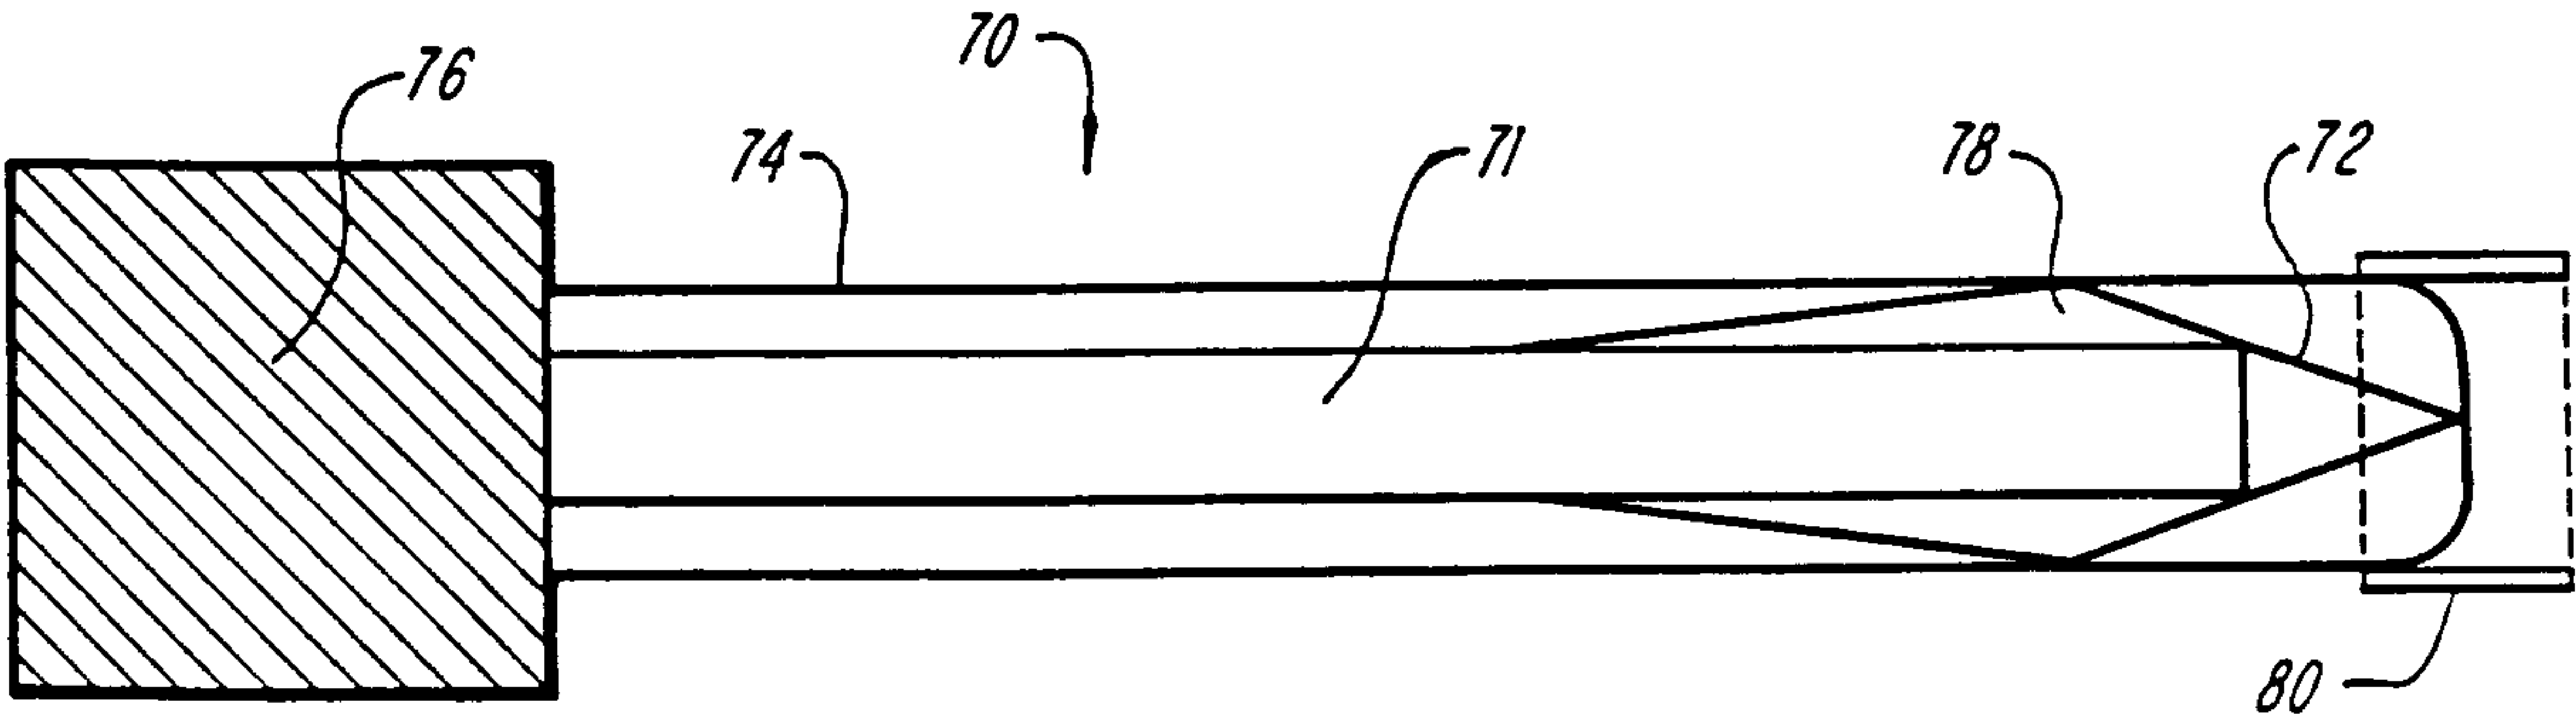


FIG. 4A

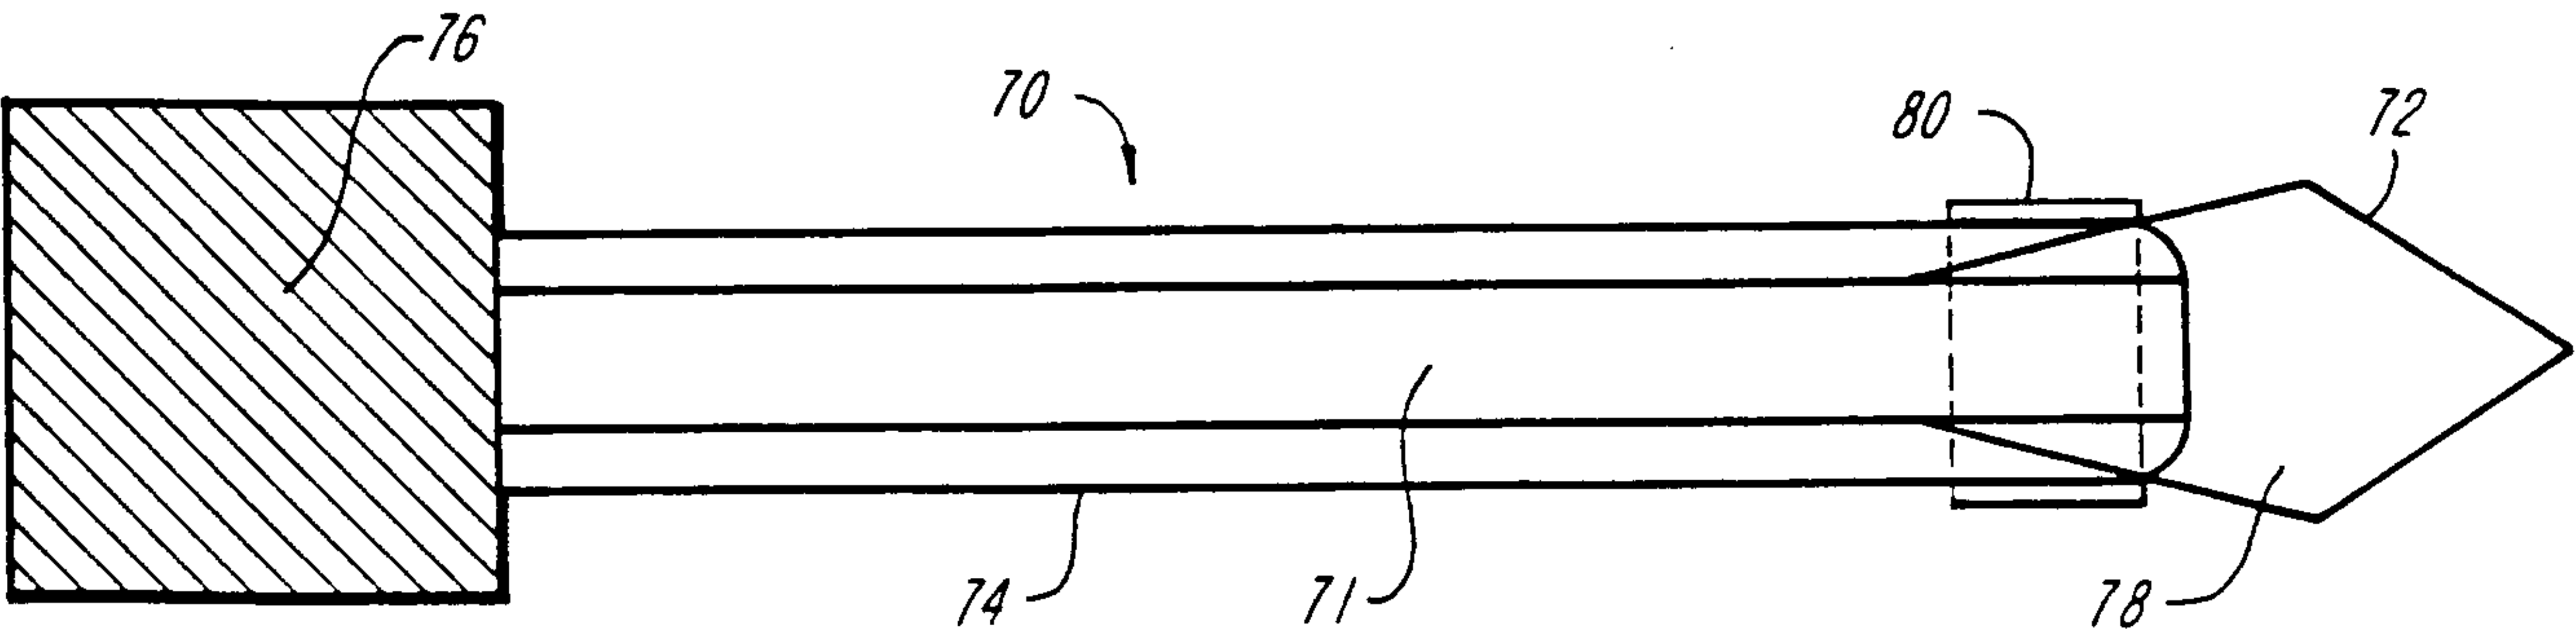


FIG. 4B

