

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
25 January 2007 (25.01.2007)

PCT

(10) International Publication Number
WO 2007/011383 A2

(51) International Patent Classification:
G01L 1/04 (2006.01)

(74) Agents: **DIXON, Michael, K.** et al.; AKERMAN SEN-
TERFITT, P.O. Box 3188, West Palm Beach, FL 33402-
3188 (US).

(21) International Application Number:
PCT/US2005/033968

(22) International Filing Date:
22 September 2005 (22.09.2005)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
10/947,799 23 September 2004 (23.09.2004) US

(71) Applicant (for all designated States except US): **UT-BAT-
TELLE, LLC** [US/US]; P.O. Box 2008, Oak Ridge, TN
37831-6258 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **DOKTYCZ,
Mitchel, J.** [US/US]; 1405 Rush Limbaugh Lane,
Knoxville, TN 37932 (US). **ALLISON, David, P.**
[US/US]; 146 Copenhaver Road, Lenoir Icty, TN 37771
(US).


(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KM, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, LY,
MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO,
NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK,
SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ,
VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT,
RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA,
GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:
— without international search report and to be republished
upon receipt of that report

[Continued on next page]

(54) Title: COUPLED SPRING SYSTEM FOR MEASURING MOLECULAR FORCES

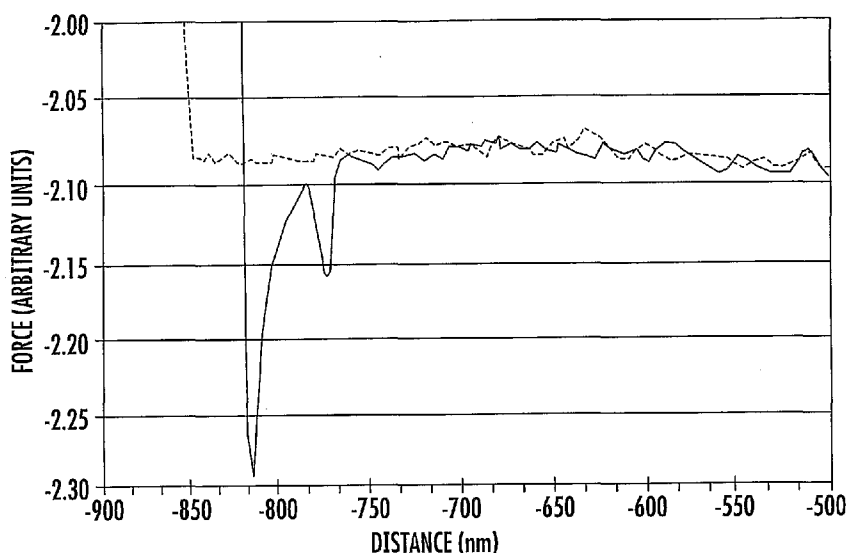

(57) Abstract: A coupled spring system is applied to dynamic force spectroscopy measurements. A microcantilever-mounted probe (19) acts as a first spring, and a supported micromachined membrane (15) acts as a second spring. The coupled spring system provides a system spring constant that is lower than either spring individually. By probing different regions of the membrane (15), the spring constant of the system can be varied.

WO 2007/011383 A2



For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

COUPLED SPRING SYSTEM FOR MEASURING MOLECULAR FORCES

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0001] The United States Government has rights in this invention pursuant to Contract No. DE-AC05-00OR22725 between the United States Department of Energy and UT-Battelle, LLC.

BACKGROUND OF THE INVENTION

FIELD OF THE INVENTION

[0002] The invention relates to force measurement systems, and more particularly to a coupled spring system comprising a microcantilever and a flexible thin film membrane. The combination enables a very soft and variable system spring constant for molecular force measurements.

DESCRIPTION OF PRIOR ART

[0003] One valuable attribute of the scanning probe microscope is its ability to assess and/or measure forces. These forces can be between the scanning probe and a surface, or between molecules that are specifically tethered or otherwise disposed on these surfaces. The force sensitivity is due to the weak spring of the microcantilever arm upon which the probe is mounted. It is also due to the ability to sensitively measure sub-Angstrom deflections of the spring. The combination can quantify molecular scale forces such as those involved in chemical recognition.. Measurements of the energetics between ligands and receptors, the energetics of intramolecular folds in a single protein molecule, and

the structural changes within a single enzyme molecule during catalysis have all been demonstrated (Willemsen 2000)¹. The technique is often referred to as dynamic force spectroscopy (DFS) and is proving invaluable for characterizing interactions between molecules and/or surfaces.

[0004] Typically, a force-distance curve is collected under a range of force loading rates (Willemsen 2000)¹. FIG. 1 shows a typical force-distance curve, collected in our laboratory, where biotin is tethered to the probe and avidin is bound to the surface. The dashed line is the approach curve. The horizontal portion of the approach curve occurs before the probe makes contact with the surface. Upon contact, the microcantilever arm deflects, and the slope of the force-distance curve in this region depends on the microcantilever spring constant. Upon retraction (solid line), the probe may show adhesion at the point of lift-off. The point of lift-off depends on interaction forces between the probe and the surface. With a suitable length tether or linker molecule, the specific interaction occurring between the tethered biotin and surface bound avidin can be separated from the probe adhesion and observed as a deflection in the horizontal region of the withdrawal curve. The microcantilever spring constant can be measured by a variety of techniques including those of Hutter (1993)², Cleveland (1993)³, and D'Costa (1995)⁴. Knowledge of the microcantilever spring constant and the deflection measurement can be used to estimate the binding force.

[0005] Typically, hundreds to thousands of force-distance curves are collected under various loading rates for an evaluation of binding energetics. Varying the retraction speed, combined with different microcantilever spring constants (i.e., different microcantilevers), results in different loading rates. The need to collect a large number of curves per loading rate is a result of the stochastic or random binding event. The fraction of curves showing a binding event is dependent on numerous factors, including interaction strength and molecular orientation. Examination of various loading rates allows for effective interpretation of the interaction energy. In general, slow loading rates result in lower force measurements than higher loading rates. This is due to thermal

energy that can lead to bond disruption. Evans (1997)⁵, based on a model by Bell (1978)⁶, has provided a theoretical interpretation of force measurements by dynamic force spectroscopy and related techniques. Further, these measurements can be related to reaction energies and kinetics carried out in bulk.

[0006] Several obstacles stand in the way of maturing dynamic force spectroscopy into a robust technique for routine measurement of molecular interactions. A key obstacle is the coupling chemistry (Willemsen 2000)¹. The orientation of the molecules and the degrees of freedom available are extremely important for producing a binding event. Chemical coupling to the probe must be sufficiently robust to withstand repeated unbinding events. The tether must be stronger than the forces being evaluated. Further, the tether must be sufficiently flexible to provide sampling of a sufficient number of molecular orientations and sufficiently long to separate probe adhesion forces from specific molecular events. A second obstacle is rapidly performing force measurements under a variety of loading rates. Extending the dynamic range of these measurements is critical for identifying weak interactions and for characterizing the activation energy barriers. Our invention directly addresses this shortcoming.

References

- [0007]** 1. Willemsen, O. H., Snel, M. M. E., Cambi, A., Greve, J., De Grooth, B. G., and Figdor, C. G., "Biomolecular Interactions Measured by Atomic Force Microscopy", *Biophysical Journal* 79, 3267 (2000).
- [0008]** 2. Hutter, J. L. and Bechhoefer, J., "Calibration of Atomic-Force Microscope Tips", *Rev. Sci. Instrum.* 64, 1868 (1993).
- [0009]** 3. Cleveland, J. P., Manne, S., Bocek, D., Hansma, P.K., "A Nondestructive Method for Determining the Spring Constant of Cantilevers for Scanning Force Microscopy", *Rev. Sci. Instrum.* 64, 403 (1993).

- [0010] 4. D'Costa, N. P. and Hoh, J. H., "Calibration of Optical Lever Sensitivity for Atomic Force Microscopy", Rev. Sci. Instrum. 66, 5096 (1995).
- [0011] 5. Evans, E. and Ritchie, K. "Dynamic Strength of Molecular Adhesion Bonds", Biophysical Journal 72, 1541, (1997).
- [0012] 6. Bell, G. I., "Models for the Specific Adhesion of Cells to Cells", Science 200, 618 (1978).
- [0013] 7. Ciarlo, D. R., "Silicon Nitride Thin Windows for Biomedical Microdevices", Biomedical Microdevices 4, 63 (2002).
- [0014] 8. Griffel, W., "Handbook of Formulas for Stress and Strain", Chapter V, Sections 50-51, Frederick Ungar Publishing Co., New York (1966).
- [0015] 9. Allen, M. G., Mehregany, M., Howe, R. T., and Senturia, S. D., "Microfabricated Structures for the In Situ Measurement of Residual Stress, Young's Modulus, and Ultimate Strain of Thin Films", Appl. Phys. Lett. 51, 241 (1987).

SUMMARY OF THE INVENTION

[0016] It is an object of the invention to provide a coupled spring system for dynamic force measurements.

[0017] It is another object of the invention to provide a molecular force measurement system having a system spring constant that can be varied by positioning a microcantilever probe at different locations on a suspended thin film membrane.

[0018] A further object of the invention is to provide a molecular force measurement system having a system spring constant that can be softened without changing to a different microcantilever.

[0019] In a preferred embodiment, the invention is a coupled spring system for assessing interaction forces. It comprises a cantilever selected for the spring constant of its projecting arm, a probe located at the distal end of the projecting arm, and a supported membrane selected for its spring constant. The probe and supported membrane are positioned for measurement of the force between at least one molecule disposed on the probe and at least one molecule disposed on the supported membrane.

BRIEF DESCRIPTION OF THE DRAWINGS

[0020] FIG. 1 shows a force-distance measurement typical of the prior art where biotin is tethered to a microcantilever probe and avidin is bound to a surface.

[0021] FIG. 2 shows the coupled spring system of the invention.

[0022] FIG. 3 shows examples of force-distance measurements using a suspended silicon nitride membrane and a microcantilever-mounted probe according to the invention. The figure illustrates that by positioning the microcantilever probe at different locations on the membrane surface, different effective spring constants (k_{eff}) can be obtained.

[0023] FIG. 4 illustrates an array of membrane structures fabricated on a single substrate, and their use with a plurality of microcantilevers.

DETAILED DESCRIPTION OF THE INVENTION

[0024] Attractive forces between molecules are important to all chemical, physical, and biological processes and to materials as well. Techniques for assessing and/or measuring these forces are essential. The weak spring used in atomic force microscopy can be used for measuring forces between surfaces or between individual molecular pairs in virtually any environment (i.e., liquid, gas, vacuum). However, the technique is compromised by the need to evaluate microcantilevers possessing different spring constants. Ideally, the microcantilever spring constant should correlate with the forces being evaluated. For evaluating the weakest coupling forces, such as those commonly seen in biological systems, an extremely low or soft spring constant is needed.

[0025] We provide a coupled spring system useful for evaluating force measurements under a variety of load rates. The coupled spring system shown in FIG. 2 allows for the utilization of various spring constants without changing microcantilevers. This alleviates time-consuming alignment of the optical system and extends the dynamic range of the force measurements.

[0026] In FIG. 2, the arm **14** of a microcantilever **13** provides the first spring. This is well known in the field. The second spring is a flexible thin film membrane **15** supported from a suitable base **16**. In one embodiment, the membrane **15** would support a single target molecule **17** tethered to the membrane **15** by a tether **21**. In this example, the target molecule **17** is one molecule of a molecular pair. The other molecule is the probe molecule of interest **18** tethered to the microcantilever probe **19** by a tether **20**. The probe **19** could be any commonly used probe device such as an integrated or attached tip or tip structure, glass, latex, gold or silver bead, or just the distal end of the arm **14**, for example. The tethers **20** and **21** could be linker molecules, for example.

[0027] The first spring of the coupled spring system can be provided by any microcantilever such as is commonly employed for atomic force microscopy.

Microcantilevers are produced in a variety of shapes and possess spring constants in the range of 0.01 – 10 N/m. The probe **19** at the distal end of the arm **14** may have a radius of curvature on the order of 10 nm, and is used to probe a surface. This probe can be physically or chemically functionalized.

[0028] The second spring in the coupled spring system, the thin film membrane, may be such as has been used in a variety of sensor applications. Thin film membranes have been used, for example, as pressure sensors, infrared sensors, vacuum windows, acoustic devices and as microscopy substrates (Ciarlo, 2002)⁷. Membranes can be prepared from a variety of materials, including polymers, gold, silicon, silicon oxide and silicon nitride, for example. Silicon nitride membranes are commercially available from Structure Probe Inc. (West Chester, PA). Standard coating and etching processes, available from a number of MEMS foundries, can also be used to fabricate these membranes.

[0029] Since standard micromachining techniques are employed, the membrane **15** can be constructed of varying thicknesses and sizes. The spring constant of the membrane can be estimated from the elastic modulus (E) of the material, the thickness of the membrane (t) and size of the membrane (side length, a). For a square membrane, the spring constant (k) can be estimated from:

$$k = \frac{Et^3}{Ka^2}$$

where K is a dimensionless constant that depends on the geometry of the membrane (Griffel, 1966)⁸. More refined calculations that take into account the residual stress of the membrane can also be used to characterize the load-deflection behavior of the membrane (Allen 1987)⁹. Clearly, thinner and larger membranes will have lower spring constants. Square silicon nitride membranes on the order of 30 nm thick and 460 μ m on a side are commercially available.

The estimated spring constant for this membrane would be 0.012 N/m, not including estimated surface stresses.

[0030] In FIG. 2, an attachment layer **22** may be applied to the flexible membrane **15**. This attachment layer serves to couple a target species to the surface. The target species could be one of a pair of reagents to be tested for an interaction, for example. The other member of the pair is tethered to the microcantilever probe. The attachment layer may serve further to reduce non-specific interactions (i.e., probe adhesion forces), control the density of target molecules on the surface, space the target species away from the surface, and facilitate the interaction between the pair of reagents.

[0031] FIG. 3 shows an example of force-distance measurements using a suspended silicon nitride membrane and a microcantilever-mounted probe according to the invention. The membrane used for this demonstration was not optimized for measuring weak forces. Nevertheless, the effect of a coupled spring system on the force-distance curves is clearly seen. By positioning the microcantilever probe **19** at different locations or regions on the membrane **15** surface, different effective spring constants (k_{eff}) can be obtained. This result is observed as a change in slope of the force-distance curve in the region where contact is made with the surface. The softest effective spring constant is normally located at the center of the membrane. The effective spring constant can be determined directly from the force-distance curve. If the membrane spring constant (k_1) and the microcantilever spring constant (k_2) are known, then k_{eff} can be determined by the following relationship:

$$k_{eff} = \frac{k_1 k_2}{k_1 + k_2}.$$

[0032] The principal benefit of coupling the two springs in the described manner is that the effective spring constant of the device will be lower than either spring alone. This is significant as the smallest force that can be measured

depends on the spring constant of the system. The ability to change the system spring constant by using different positioning of the probe on the membrane surface enables evaluation of different loading rates without changing the microcantilever. This enables rapid collection of dynamic force measurements. Different membrane and microcantilever designs can be considered.

[0033] While the above discussion describes movement of the probe relative to the membrane, the membrane could be moved relative to a stationary probe just as well. It will also be appreciated that positioning of the probe on the membrane includes not only static placement of the probe relative to a membrane or target molecule, but also includes arranging for movement of the probe relative to the membrane or to the target molecule. Movement of a probe molecule relative to a target molecule is already done in some measurements in the field.

[0034] One or both of the above described springs can be fabricated in an array format for higher experimental throughput. FIG. 4, for example, shows an array of membrane structures **25, 26, 27** can be fabricated onto a single substrate **28**. Individual membranes may be of different dimensions to produce different effective spring constants in combination with particular microcantilever springs **29, 30, 31** used with the membranes. Alternatively, the different membrane structures could also be coupled with different reagents for examination of an array of target reagents with a single microcantilever-mounted probe molecule. An array of microcantilever springs could also be fabricated to match the spatial separation of the different membrane structures. This could lead to the parallel evaluation of multiple probe molecules against an array of target reagents.

[0035] While the invention has been described with reference to a microcantilever device and a thin film membrane, it will be apparent that the invention is equally applicable to any size cantilever device and membrane structure. In like manner, while the invention has been described for the

assessment and/or measurement of molecular forces, it is just as applicable to the measurement of forces between large numbers of molecules and to the measurement of forces between surfaces.

[0036] The ability to better measure adhesion forces afforded by our invention will improve biophysical studies of biomolecular interactions, including protein-protein, protein-DNA, and DNA-DNA interactions. Binding of potential pharmaceutical reagents to protein targets, as in drug discovery applications, is also likely. The technique can be used for both qualitative and quantitative evaluations.

[0037] While there has been shown and described what are at present considered the preferred embodiments of the invention, it will be obvious to those skilled in the art that various changes and modifications can be prepared therein without departing from the scope of the inventions defined by the appended claims.

CLAIMS

We claim:

1. A coupled spring system for assessing interaction forces, characterized in that:

a cantilever (13) formed from a projecting arm, wherein the cantilever (13) is selected for the spring constant of the projecting arm (14);

a probe (19) located at the distal end of said projecting arm (14); and

a supported membrane (15) selected based upon a spring constant of the supported membrane (15), wherein said probe (19) and said supported membrane (15) are positioned for measurement of the force between at least one molecule (18) disposed on said probe (19) and at least one molecule (17) disposed on said supported membrane (15).

2. The system of claim 1, characterized in that said cantilever (13) is a microcantilever (13).

3. The system of claim 1, characterized in that said membrane (15) is a thin film membrane.

4. The system of claim 1, characterized in that said at least one molecule (18) disposed on said probe (19) is tethered by a linker molecule (20).

5. The system of claim 1, characterized in that said at least one molecule (17) disposed on the surface of said supported thin film membrane (15) is tethered by a linker molecule (21).

6. The system of claim 1, characterized in that said at least one molecule (18) disposed on said probe (19) is a biomolecule.

7. The system of claim 1, characterized in that said at least one molecule (17) disposed on the surface of said supported membrane (15) is a biomolecule.

8. The system of claim 6, characterized in that said at least one biomolecule disposed on said probe (19) is tethered by a linker molecule (20).

9. The system of claim 7, characterized in that said at least one biomolecule disposed on the surface of said supported membrane (15) is tethered by a linker molecule (21).

10. The system of claim 1, characterized in that said thin film membrane (15) is a micromachined thin film membrane.

11. The system of claim 1, further characterized in that a molecule attachment layer (22) on said thin film membrane (15).

12. The system of claim 1, characterized in that said thin film membrane (15) is a polymer.

13. The system of claim 1, characterized in that said thin film membrane (15) is gold.

14. The system of claim 1, characterized in that said thin film membrane (15) is silicon.

15. The system of claim 1, characterized in that said thin film membrane (15) is silicon oxide.

16. The system of claim 1, characterized in that said thin film membrane (15) is silicon nitride.

17. The system of claim 1, characterized in that said probe (19) is physically functionalized.

18. The system of claim 1, characterized in that said probe (19) is chemically functionalized.

19. The system of claim 1, characterized in that said thin film membrane (15) further includes a probe (19) structure on a surface of the thin film membrane (15) for supporting said at least one molecule (17) tethered to the surface of said supported thin film membrane (15).

20. The system of claim 1, further characterized in that a plurality of cantilevers (13) selected for the spring constants of their projecting arms (14), said plurality of cantilevers (13) having probes (19) located at the distal ends of said projecting arms (14); and

a plurality of supported membranes (15), said membranes (15) selected for their spring constants, wherein said probes (19) are positioned for measurement of the forces between at least one molecule (18) disposed on each of said probes (19) and at least one molecule (17) disposed on each of said supported membranes (15).

21. The system of claim 1, characterized in that said at least one molecule (18) disposed on said probe (19) is a plurality of molecules (18).

22. The system of claim 1, characterized in that said at least one molecule (17) disposed on the surface of said supported thin film membrane (15) is a plurality of molecules (17).

23. The system of claim 21, characterized in that said plurality of molecules (18) is the surface of a material.

24. The system of claim 22, characterized in that said plurality of molecules (17) is the surface of a material.

1/4

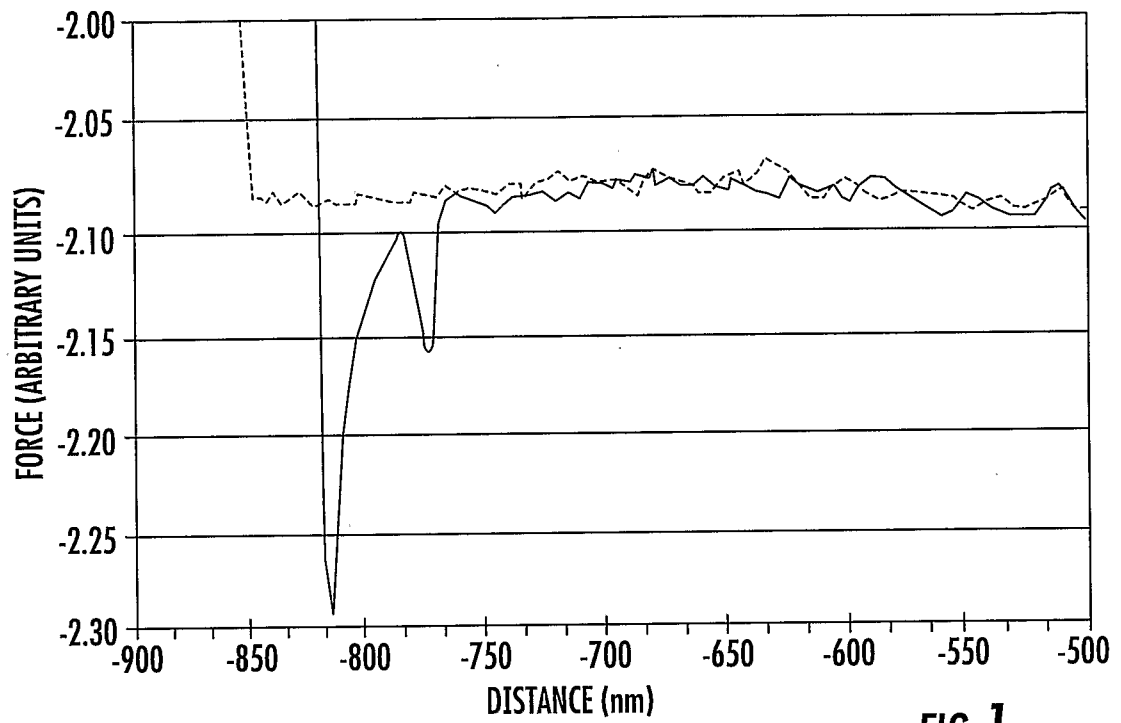


FIG. 1
(PRIOR ART)

2/4

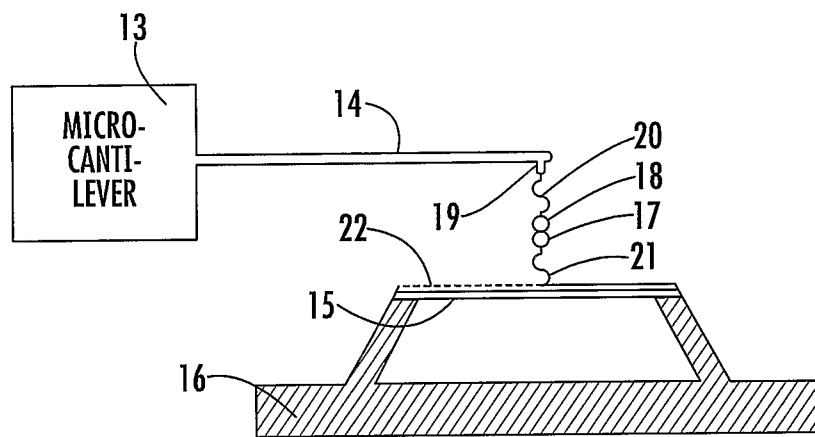
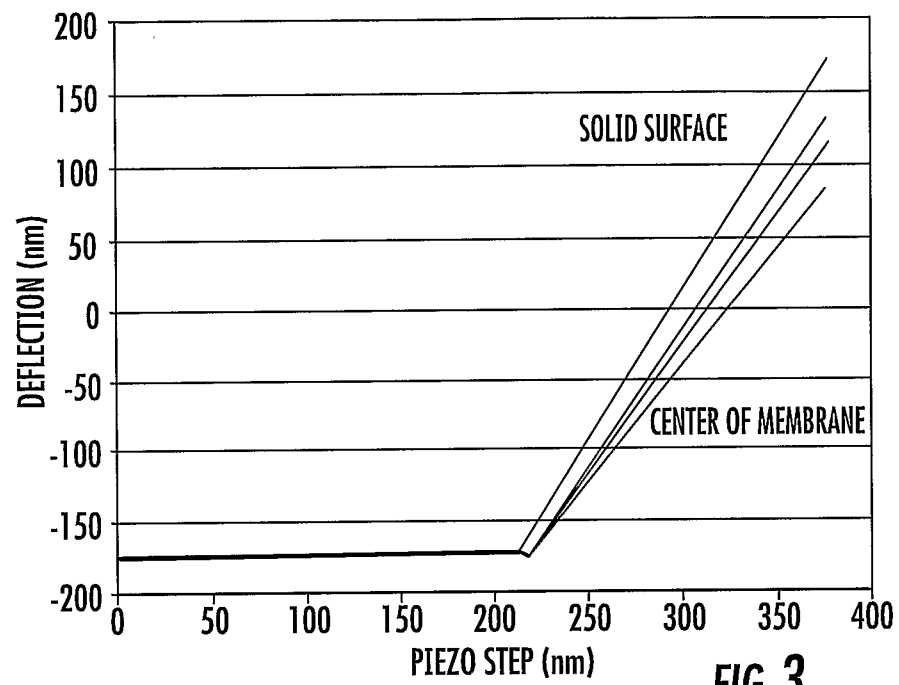
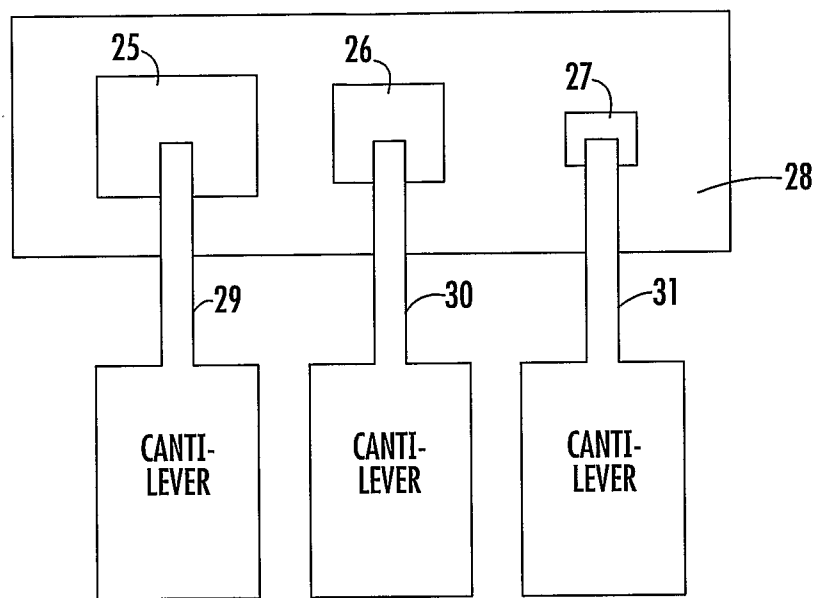


FIG. 2

3/4

**FIG. 3**

4/4

**FIG. 4**