



US 20060121415A1

(19) **United States**(12) **Patent Application Publication****Anitua Aldecoa**(10) **Pub. No.: US 2006/0121415 A1**(43) **Pub. Date: Jun. 8, 2006**(54) **SET OF MOTOR-DRIVEN INSTRUMENTS
TO AID THE FIXING OF DENTAL
IMPLANTS**(30) **Foreign Application Priority Data**

Sep. 2, 2002 (ES) P200202006

Nov. 18, 2002 (ES) P200202646

(76) Inventor: **Eduardo Anitua Aldecoa, Vitoria (ES)****Publication Classification**


Correspondence Address:

BROWDY AND NEIMARK, P.L.L.C.**624 NINTH STREET, NW****SUITE 300****WASHINGTON, DC 20001-5303 (US)**(51) **Int. Cl.****A61C 3/02** (2006.01)(52) **U.S. Cl.** **433/165**

(57)

ABSTRACT

Set of motor-driven instruments to aid the fixing of dental implants that combines drills (1, 2) and motor-driven osteotomes (4A, 4B, 4C, 4D) of progressive diameters. These have a threaded conical section (9), followed by a threaded cylindrical section (8) and another area (7) to fit the connectors (14, 17) to the surgical motor or a manual extractor.

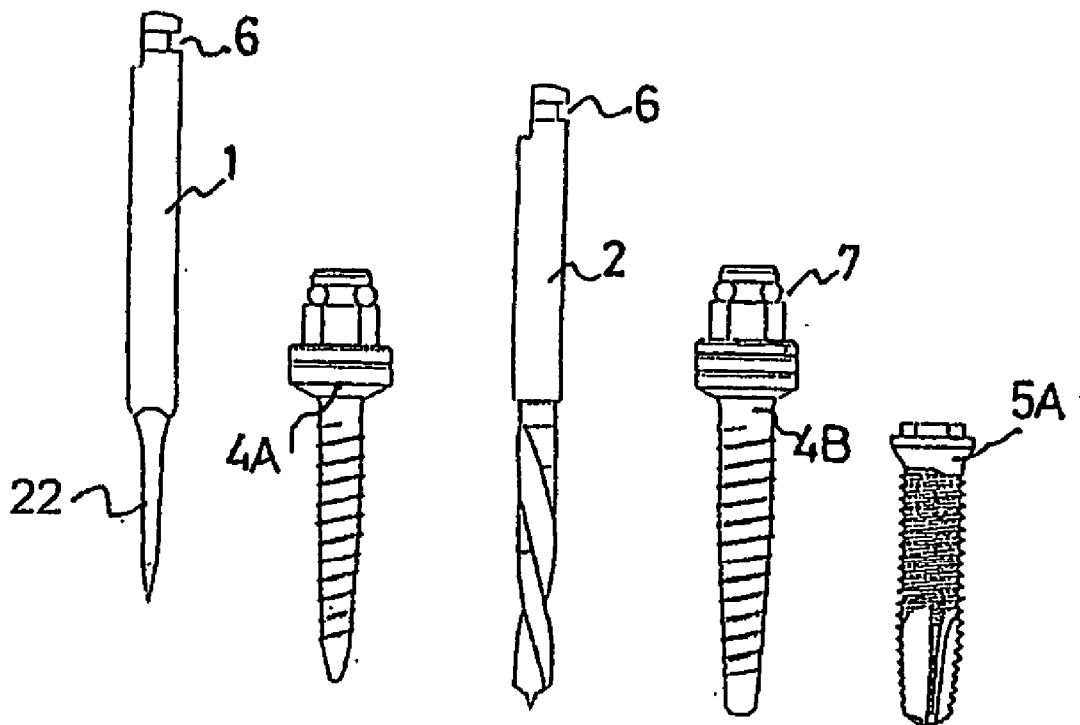(21) Appl. No.: **10/526,187**(22) PCT Filed: **Sep. 2, 2003**(86) PCT No.: **PCT/ES03/00443**

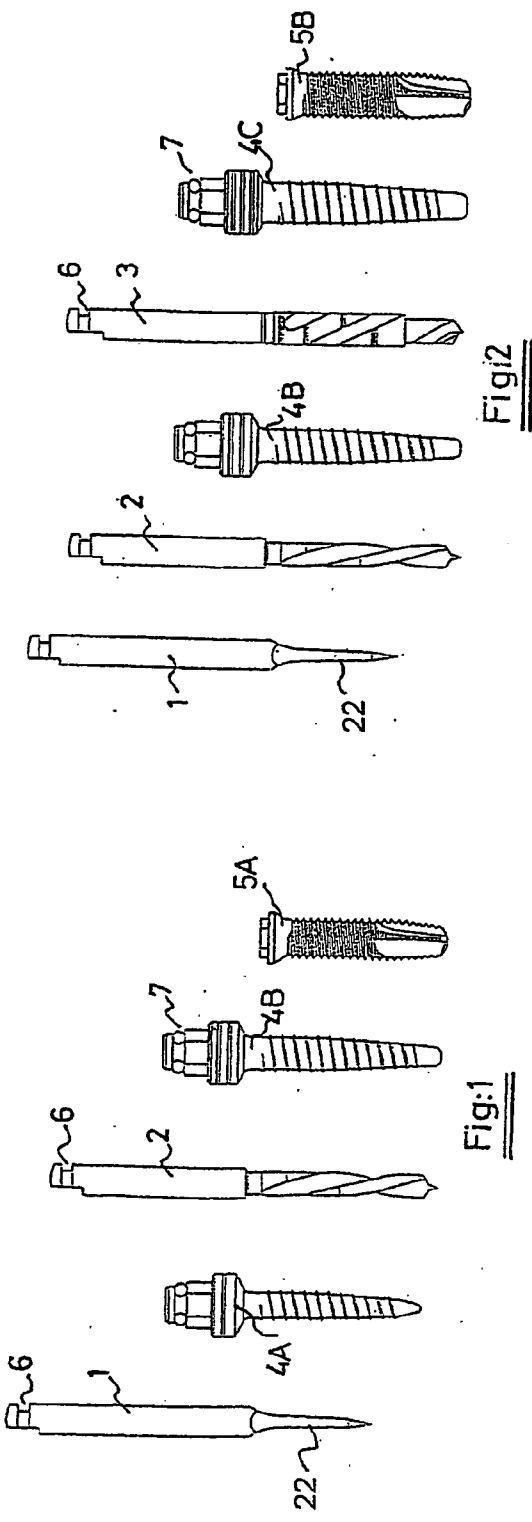


Fig:1

Fig:2

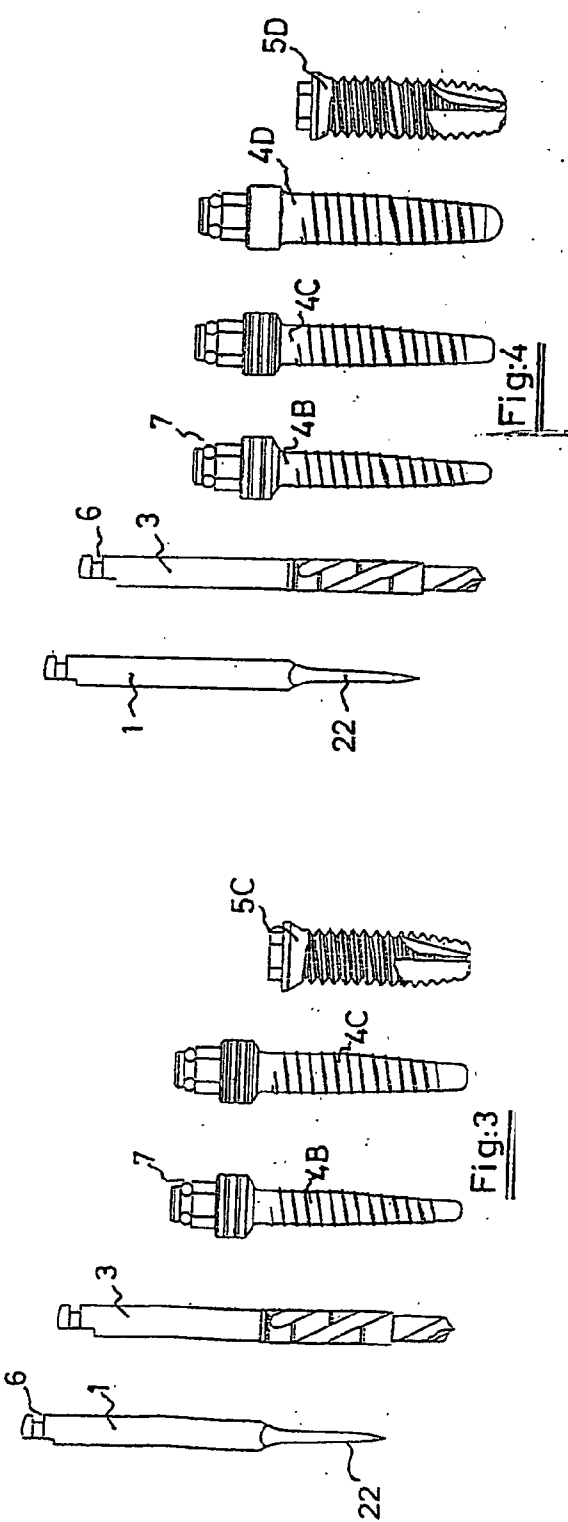


Fig:3

Fig:4

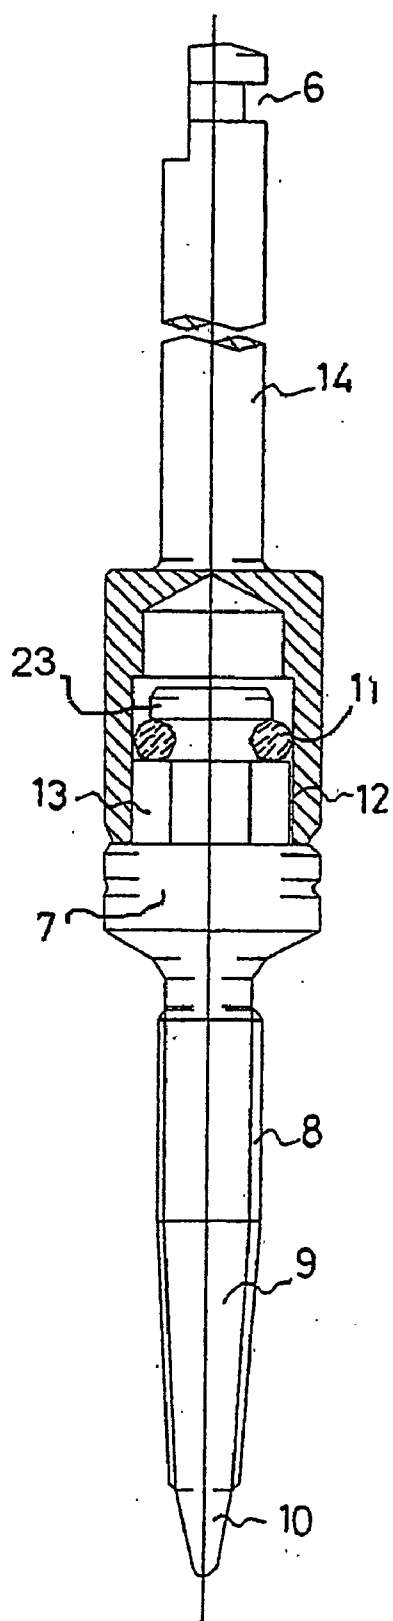


Fig:5

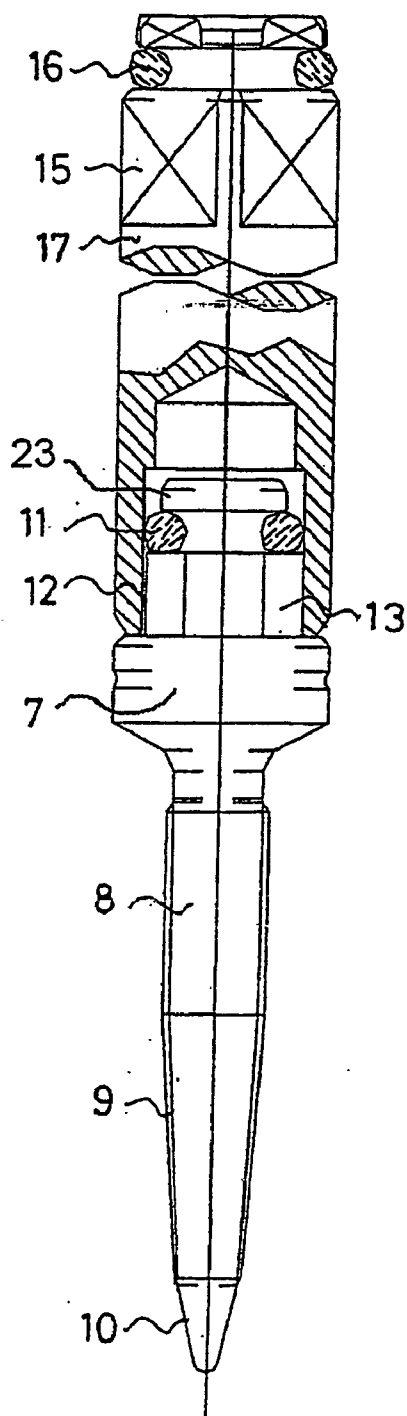


Fig:6

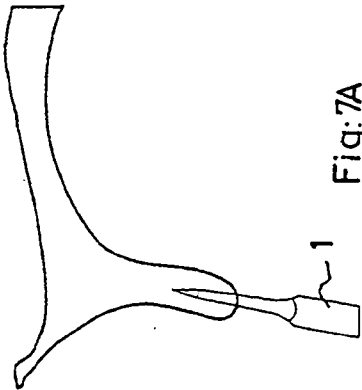


Fig:7A

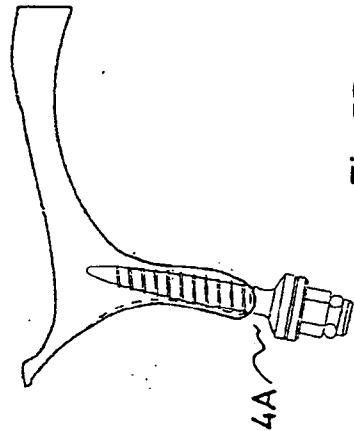


Fig:7B

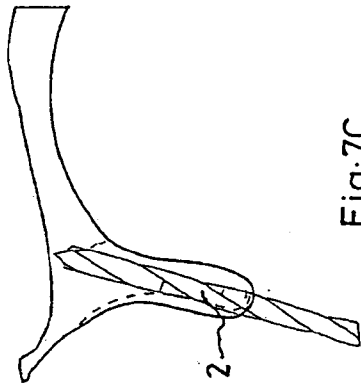


Fig:7C

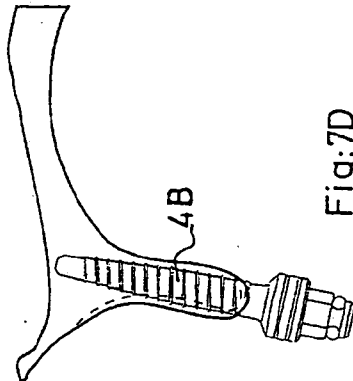


Fig:7D

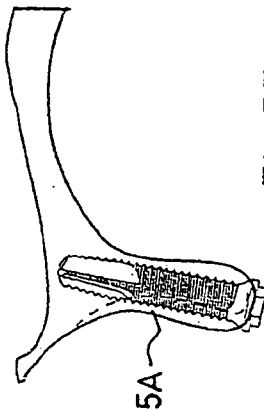


Fig:7E

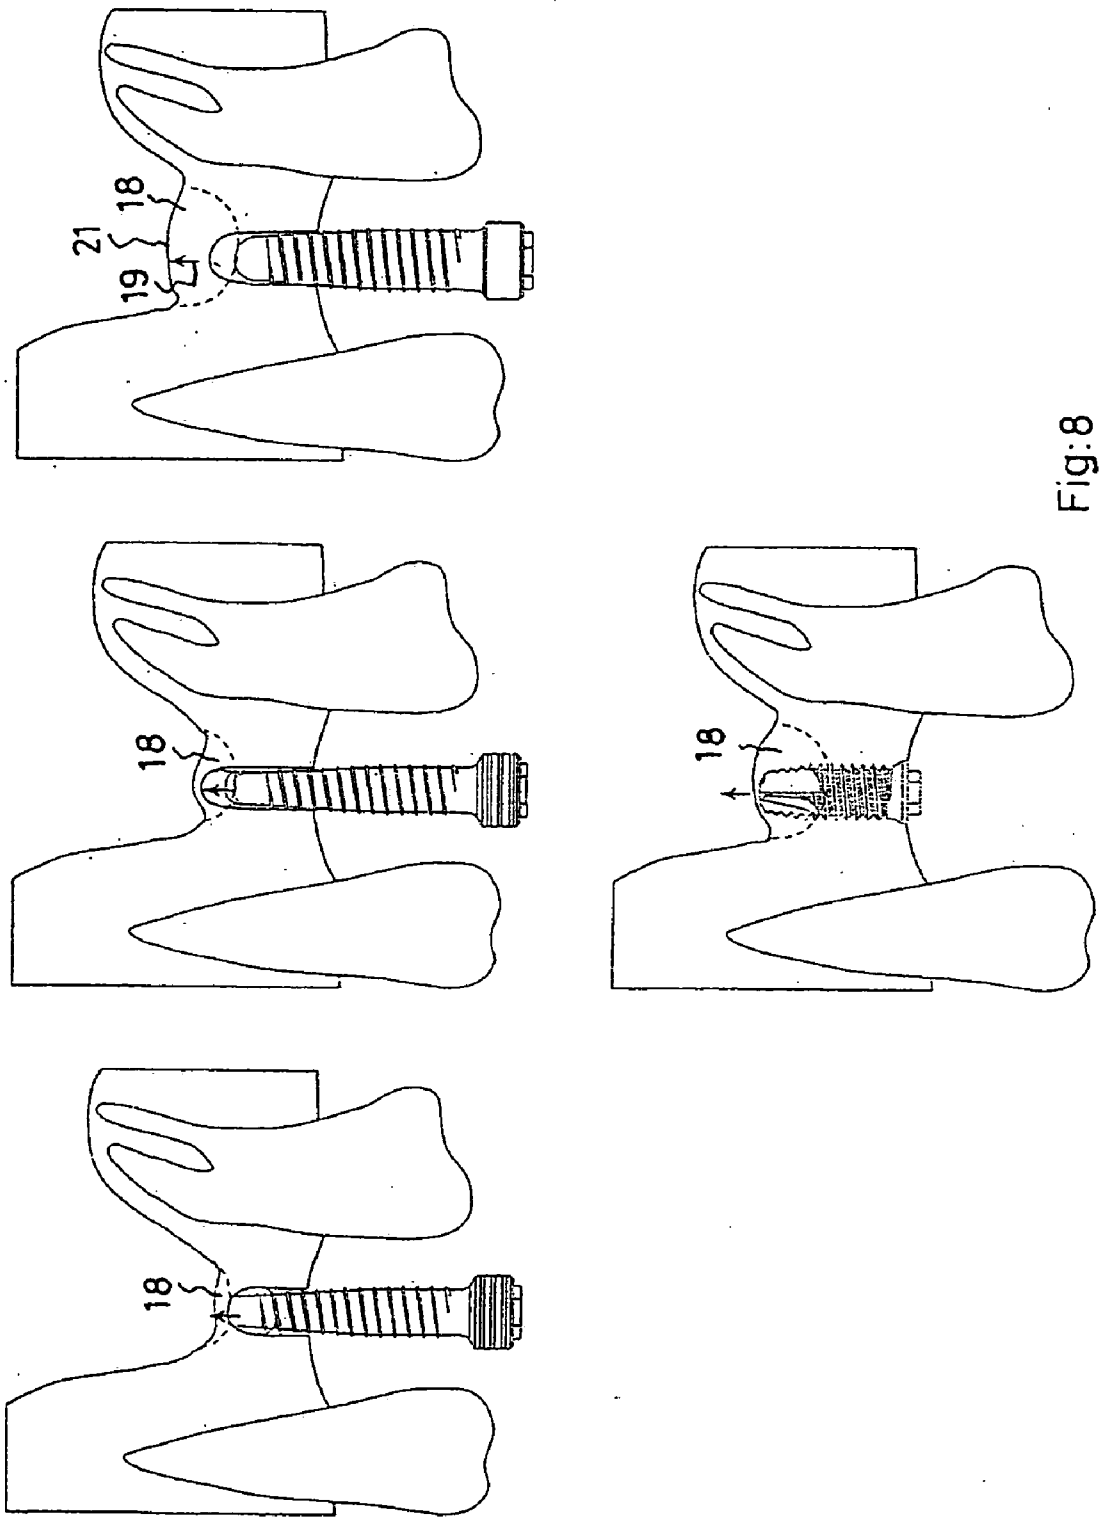


Fig: 8

SET OF MOTOR-DRIVEN INSTRUMENTS TO AID THE FIXING OF DENTAL IMPLANTS

[0001] The invention relates to a set of motor-driven instruments to aid the fixing of dental implants, in particular to those instruments used in bone expansion, bone compaction or sinus elevation techniques; techniques designed to modify in a suitable way the bone structure that receives the implant before it is finally fixed in position. This set of instruments includes atraumatic bone osteotomes consisting of a series of members with a conical apical zone and with progressive diameters, which are individually and successively introduced into the bone and then extracted using suitable manual means.

[0002] Some traditional osteotomes known in the prior art are described in the publication, "A New Approach to Surgery and Prosthesis on Implants" (Dr. Eduardo Anitua, 1996), in the cases that describe the fixing of implants in the area at the front of the upper maxillary bone in cases of bone type 3 or 4, i.e. spongy or cancellous bone, with the conducting beforehand of a phase of expansion of the bone crest that will house the implant. The process to expand the crest and fix the implant is based on the alternate use of osteotomes or instruments in the following way: the process begins with the use of an instrument whose function it is to mark the start point or insertion point where an implant is to be fitted; the crest of the bone is then expanded by pressing in the appropriate instrument, always by hand, with it even being necessary to use a hammer if the bone is compact.

[0003] Then, with other osteotomes of a greater diameter the aim is to expand the crest until a suitable floor is created to allow the implant to be inserted, for example an implant of 3.3 mm, as suggested in WO 0224102 awarded in favour of this applicant.

[0004] In short, in this way an implant can be inserted using only manual osteotomes successively.

[0005] The instruments or manual osteotomes used in techniques to expand narrow bone crests can also be used to impact against and compact the bone, a technique that is necessary when the bone onto which the implant is to be fixed is cancellous, for example, an area at the rear of the upper maxillary of bone type 4. The process for conducting this technique is generally similar to the expansion technique, with the exception that at a specific moment the surrounding bone is compacted or condensed as a result of the application of osteotomes of a larger diameter.

[0006] As regards the atraumatic elevation of the sinus, the procedure usually commences with an initial phase in which incisions are made with the first two osteotomes down to the floor of the sinus, and then proceeding with the elevation of the sinus by using successive osteotomes and also introducing bone graft material into the base.

[0007] The formal characteristic of these instruments known and used in the aforementioned techniques is that they usually have a cylindrical or conical form similar to that of the cores of the implants used, in order to obtain good stability that ensures that the implants are inserted with excellent results.

[0008] As mentioned above these traditional techniques were published by Dr. Eduardo Anitua in 1996 under the title, "A New Approach to Surgery and Prosthesis on

Implants". The disadvantage of these techniques, all of them manual, is that they cannot be used on the lower jawbone or in areas at the rear of the maxillary bone, and furthermore if the bone is very compact (types 1 or 2), tapping must be carried out with a hammer, which is very painful for patients.

[0009] In addition ES 2127116 B relates to a set of expanders that, it is claimed, prevent problems deriving from osteotomes, (with osteotomes being understood in this document as punches that are tapped on the dental base by a small hammer in an erroneous interpretation of the prior art from 1996. However, the disadvantage of these expanders is that they do not meet the objectives they were designed to achieve and they do not give rise to properly stabilised fixing of the implants, as bone-implant inconsistencies are created that derive from their specific form not being adapted to that of the final implant to be inserted. Furthermore they are introduced by manual means, keys etc; and their combined use with drills is not intended.

[0010] For the purposes of overcoming the drawbacks of the instruments and known manual techniques, it is an object of this invention to provide a set of osteotomes and drills of a new design that can be used alternately, with all of them motorised and driven by a surgical motor.

[0011] By using motor-driven instruments, and applying a known and controlled torque, crests can be expanded in areas at the rear of the maxillary bone or in areas at the front and rear of the lower jawbone and in any type of bone.

[0012] It is another object of this invention to provide a set of instruments that allow better directional and torque control than common techniques.

[0013] It is another object of this invention to provide a set of instruments that allows crests to be expanded, creating a greenstick fracture in extreme cases, preventing total fracture and the loss of the vestibular plate, which is the case in the aforementioned ES 2127116 B.

[0014] In order to reach these objectives and with a view to their correct interpretation, five sheets of drawings are attached in which the following is represented:

[0015] **FIGS. 1 and 2** show two examples of implant-fixing procedures with prior bone expansion using the inventive motor-driven instruments.

[0016] **FIGS. 3 and 4** show two examples of implant-fixing procedures with prior bone compaction using the inventive motor-driven instruments.

[0017] **FIG. 5** shows an elevation in cross section of an osteotome assembled to a connector connected to the surgical motor, according to the invention.

[0018] **FIG. 6** shows an elevation in cross section of an osteotome assembled to a safety connector connected to the ratchet wrench, according to the invention.

[0019] **FIGS. 7A to 7E** show the sequence of application of the procedure in **FIG. 1**.

[0020] **FIG. 8** shows an example of an implant-fixing procedure with prior elevation of the sinus using the inventive motor-driven instruments.

[0021] **FIGS. 1 to 4** show that, according to the invention, the implant-fixing procedures both with prior bone expansion (**FIGS. 1 and 2**) and prior bone compaction (**FIGS. 3**

and 4 begin always with the use of a starter drill (**1**). One end (**22**) of this starter drill (**1**) acts on the patient's bone whereas its other end (**6**) receives a surgical motor to drive it. The end (**22**) is narrow and short and has a quadrangular section, characteristics that endow the starter drill with optimal qualities for piercing the hardest outer layer of the bone.

[0022] Other drills (**2**, **3**) of different sections can also be fitted to the surgical motor, and are used to define the directional depth and other parameters of the cavity housing the implant. The use of the drills (**2**, **3**) is alternated with the use of the osteotomes (**4A**, **4B**, **4C** and **4D**) with different-sized cross sections, which are applied gradually depending on the type of bone in question, the purpose of the action (expansion or compaction) and the size of the final implant.

[0023] The ends of the inventive osteotomes adopt similar geometries to those of the different implants (**5A**, **5B**, **5C**, **5D**), with a threaded conical area followed by another cylindrical area, as can be seen in greater detail in **FIGS. 5 and 6** below.

[0024] With regard to the coronal ends or adjustment areas (**7**) of the osteotomes, these are partly designed in order to receive connectors to the surgical drive motor or to a manual extractor (for example a ratchet wrench), all of which is also defined in **FIGS. 5 and 6**.

[0025] In these units in **FIGS. 1 to 4**, the final implants are of different dimensions. Thus, the implant (**5A**) measures 3.3×15, the implant (**5B**) 3.75×15, the implant (**5C**) 4.5×15 and the implant (**5D**) 5×15.

[0026] **FIG. 5** shows the design of an osteotome and a connector (**14**) according to the invention, as well as the assembly between both. With regard to the design of the osteotome, this presents an apical end (**10**) from which extends a threaded conical section (**9**) followed by a threaded cylindrical section (**8**).

[0027] Next, the coronal end or adjustment area (**7**) is capped by a polygonal projection (**13**) in its cross section upon which rests an O-ring seal (**11**) held in position by a rivet (**23**).

[0028] Upon the adjustment area (**7**) is assembled the connector (**14**), which has an end (**6**) that can be connected to the surgical motor, as is the case with the aforementioned drills. The connector comprises, on its opposite end, a blind axial recess (**12**) with a polygonal cross section that coincides with that of the polygonal projection (**13**) of the osteotome, so that the connector fits around the osteotome.

[0029] In order to keep this assembly between parts stable, the O-ring seal (**11**) comes into contact with the inside of the connector (**12**) so that when the connector fits around the polygonal projection (**13**) of the osteotome, the seal acts as a member maintaining and retaining the assembly so that the two elements cannot be inadvertently detached while they are being handled.

[0030] In the event that it is necessary, for whatever reason, to remove an osteotome that has become stuck inside the bone in which it has been disposed, reference shall be made to the arrangement described in **FIG. 6**. In this arrangement it can be seen that the connector (**17**) is provided with a free end in which an O-ring seal (**16**) can be

seen disposed in proximity to a coupling area (**15**) in which the hand ratchet wrench is fitted to allow the osteotome to be extracted without difficulty.

[0031] The O-ring seal (**16**) has the same function as the O-ring seal (**11**), i.e.—to prevent the ratchet wrench from separating from the connector.

[0032] The inventive osteotomes present a conical/cylindrical geometry with a progressive cross section, and as a result they act as wedges that gradually cause the crest to expand. Because of this progressive form, an excellent location is also created for the implants that have a very similar form to that given to the osteotomes.

[0033] The drills, used in combination and alternately with the osteotomes, enable the crest to be expanded, for example, in a lower maxillary or upper maxillary bone comprising very compact bone, for example, in bone types 1, 2 or 3.

[0034] In addition, the use of the surgical motor implies greater control of the torque, considerably more control of the direction in addition to better control of the force to be applied.

[0035] **FIGS. 7A to 7E** show a typical example of the working method with the inventive set, specifically with the set represented in **FIG. 1**, based on the starter drill (**1**), the osteotome (**4A**), the drill (**2**), the osteotome (**4B**) and finally the implant (**5A**), measuring 3.3×15 in this proposal. In this typical example the hardest outer layer of the bone is pierced by the starter drill (**1**), to be followed by a process to expand the bone and define the cavity housing the implant carried out as a result of the combined use of the tools (**4A**, **2**, **4B**), and to be completed with the fitting of the implant (**5A**).

[0036] The representations in **FIG. 8** show how the atraumatic elevation of the maxillary sinus is conducted, protecting the sinus membrane (**21**) or Schneiderian membrane in the process. The procedure is based on the gradual elevation of the sinus (**18**) in conjunction with the gradual insertion of autograft bone, preferably a coagulum of plasma rich in growth factors, either comprising bone graft material or not. The drills and osteotomes start cutting at a distance (**19**) from the base of the sinus of, for example, 1.5 mm.

[0037] In this way, as can be deduced from **FIG. 8**, suitable blunt osteotomes, are used to introduce the bone graft by raising the floor of the sinus (**18**) and maintaining the integrity of the sinus membrane (**21**).

1. Set of motor-driven instruments to aid the fixing of dental implants that comprise a series of atraumatic bone osteotomes of progressive diameters, with these motor-driven osteotomes designed for their assembly to motor-driven or manual-drive connectors, characterised in that:

the osteotomes (**4A**, **4B**, **4C**, **4D**) have an apical end (**10**) followed by a threaded conical section (**9**) and a threaded cylindrical section (**8**), with the threaded cylindrical section capped by an adjustment area (**7**) in which the connectors are assembled (**14**, **17**),

the set of instruments comprises starter drill (**1**), comprising a quadrangular-section end (**22**) that is smaller in section than the osteotomes, comprising an end (**6**) for its connection to a surgical motor,

the set of instruments comprises at least two drills (2, 3) of different diameters that comprise ends for connection to a surgical motor, and which is used alternately with the osteotomes

the set of instruments includes connectors (14, 16) for the motor-driven or manual-drive operation of the osteotomes.

2. Set of motor-driven instruments to aid the fixing of dental implants according to claim 1, wherein the adjustment area (7) of the osteotomes comprises a polygonal-section projection (13), preferably hexagonal, which is capped by a cylindrical projecting section that creates a circular recess in which an O-ring seal (11) is housed.

3. Set of motor-driven instruments to aid the fixing of dental implants according to claim 1, wherein the connectors (14, 17) present an end comprising a blind axial recess (12) with a polygonal section, preferably hexagonal, in which is housed the polygonal section (13) of the osteotomes incorporating the O-ring seal (11) that retains the connectors.

4. Set of motor-driven instruments to aid the fixing of dental implants according to claim 1, wherein the connector (14) possesses motor functions and comprises an extension (6) for its connection to a surgical motor.

5. Set of motor-driven instruments to aid the fixing of dental implants according to claim 1, wherein the connector (17) possesses extractor functions and comprises a coupling area (15) for connection to a ratchet wrench.

6. Procedure to facilitate the fixing of dental implants wherein during said fixing process the set of motor-driven instruments according to claim 5 is used.

7. Set of motor-driven instruments to aid the fixing of dental implants according to claim 3, wherein the connector (14) possesses motor functions and comprises an extension (6) for its connection to a surgical motor.

8. Set of motor-driven instruments to aid the fixing of dental implants according to claim 3, wherein the connector (17) possesses extractor functions and comprises a coupling area (15) for connection to a ratchet wrench.

9. Procedure to facilitate the fixing of dental implants wherein during said fixing process the set of motor-driven instruments according to claim 1 is used.

10. Osteotome (4A, 4B, 4C, 4D) applicable in techniques that modify the bone structure in a suitable way before receiving a dental implant, wherein the osteotome comprises an apical end (10) followed by a threaded conical section (9) and a threaded cylindrical section (8), said threaded conical section being finished by an adjustment area (7) to which a manually-driven or motor-driven connector (14, 17) can be connected.

11. Osteotome (4A, 4B, 4C, 4D), according to claim 10, wherein the adjustment area (7) comprises a polygonal projection (13) which is capped by a cylindrical projection that creates a circular recess in which an O-ring seal (11) is housed.

12. Osteotome (4A, 4B, 4C, 4D), according to claim 11, wherein the polygonal projection (13) is hexagonal.

13. Connector (14, 17), to be connected to an osteotome (4A, 4B, 4C, 4D) according to claim 10, so to allow the manual or motorised driving of said osteotome (4A, 4B, 4C, 4D), wherein the connector (14, 17) comprises one end provided with a blind axial recess (12) with a polygonal section to receive the polygonal projection (13) of the osteotome (4A, 4B, 4C, 4D).

14. Connector (14, 17), according to claim 13, wherein the blind axial recess (12) has a hexagonal section.

15. Connector (14, 17), according to claim 13, comprising an end (6) for its connection to a surgical motor.

16. Connector (14, 17), according to claim 13, comprising a coupling area (15) for connection to a ratchet wrench.

17. Starter drill (1), provided with an end (22) to act on a patient's bone and another end (6) to be driven by a surgical motor, where end (22) is narrow and has a quadrangular section, to allow the starter drill (1) to pierce the hardest outer layer of the bone.

* * * * *