




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 5 : A61M 1/00, A61B 5/0215 G01L 9/00	A1	(11) International Publication Number: WO 91/05575 (43) International Publication Date: 2 May 1991 (02.05.91)
(21) International Application Number: PCT/US90/05804 (22) International Filing Date: 10 October 1990 (10.10.90) (30) Priority data: 419,938 11 October 1989 (11.10.89) US (71) Applicant: BAXTER INTERNATIONAL INC. [US/US]; One Baxter Parkway, Deerfield, IL 60015 (US). (72) Inventors: HALL, John, P. ; 1212 Hyde Park, Santa Ana, CA 92705 (US). BECKMAN, Ronald, B. ; 28785 El Mio Lane, Mission Viejo, CA 92692 (US). (74) Agents: BOSTICH, June, M. et al. ; 2132 Michelson Drive, Irvine, CA 92715 (US).		(81) Designated States: AT (European patent), BE (European patent), CA, CH (European patent), DE (European patent), DK (European patent), ES (European patent), FR (European patent), GB (European patent), GR (European patent), IT (European patent), JP, LU (European patent), NL (European patent), SE (European patent). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>
(54) Title: INTEGRAL INTRACRANIAL PRESSURE MONITOR AND DRAINAGE CATHETER ASSEMBLY (57) Abstract A monitor-driven intracranial catheter assembly including a dual lumen catheter (70, 72) for monitoring intracranial pressure via a pressure sensor (76) located in one lumen while simultaneously draining cerebrospinal fluid through the other lumen (72, 66). The pressure sensor (76) is preferably a spectral modulation sensor that communicates with a photodetector apparatus by means of a single optical fiber (98), thus minimizing the diameter of the catheter. The photodetector is self-correcting for signal errors caused by temperature change, changes in intensity of the input light, and transmission losses within the optical apparatus. Moreover, the photodetector operates off the output voltage of the standard hospital monitor by "scaling" the signal from the monitor to provide a pressure measurement signal that emulates the output of a piezoresistive strain gauge sensor or Wheatstone bridge. Therefore, the entire catheter assembly is designed to be used with any of the common types of hospital monitors. The pressure monitoring catheter assembly can be used in any situation requiring very sensitive pressure measurements and can be zeroed and calibrated in situ.		

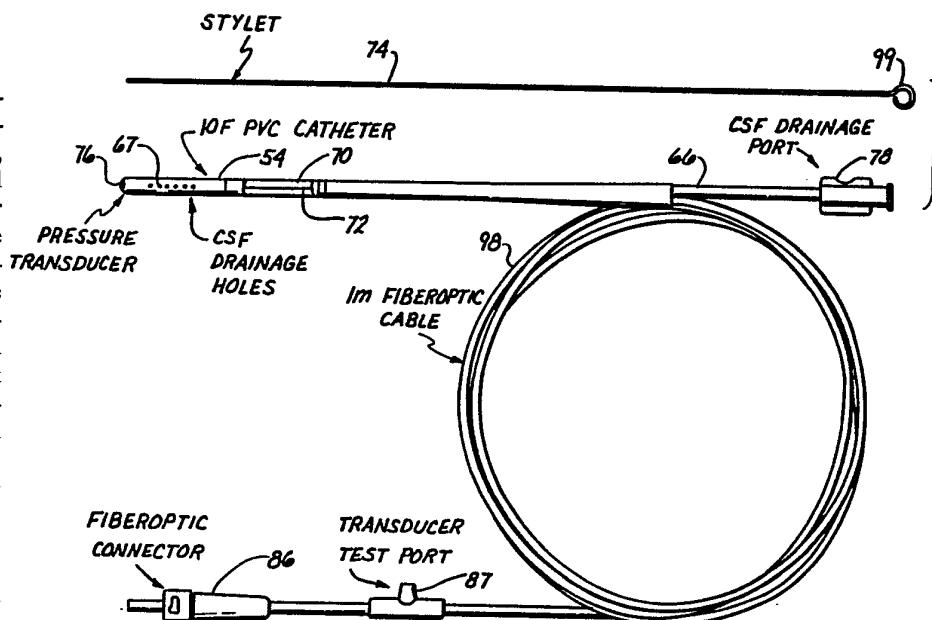

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	ES	Spain	MG	Madagascar
AU	Australia	FI	Finland	ML	Mali
BB	Barbados	FR	France	MR	Mauritania
BE	Belgium	GA	Gabon	MW	Malawi
BF	Burkina Faso	GB	United Kingdom	NL	Netherlands
BG	Bulgaria	GR	Greece	NO	Norway
BJ	Benin	HU	Hungary	PL	Poland
BR	Brazil	IT	Italy	RO	Romania
CA	Canada	JP	Japan	SD	Sudan
CF	Central African Republic	KP	Democratic People's Republic of Korea	SE	Sweden
CG	Congo	KR	Republic of Korea	SN	Senegal
CH	Switzerland	LI	Liechtenstein	SU	Soviet Union
CI	Côte d'Ivoire	LK	Sri Lanka	TD	Chad
CM	Cameroon	LU	Luxembourg	TG	Togo
DE	Germany	MC	Monaco	US	United States of America
DK	Denmark				

INTEGRAL INTRACRANIAL PRESSURE MONITOR
AND DRAINAGE CATHETER ASSEMBLY

BACKGROUND OF THE INVENTION

5 1. Field of the Invention

The present invention relates to a catheter assembly for monitoring fluid pressure while simultaneously removing a part of the fluid or infusing therein to a second fluid. More particularly, the invention relates to a
10 monitor-driven intracranial catheter assembly including a dual lumen catheter having an in situ pressure monitoring device at the distal tip for continuously monitoring intracranial pressure via one lumen while optionally conducting simultaneous drainage or sampling of
15 cerebrospinal fluid through the other lumen.

2. Description of the Prior Art

The skull is a bony housing of fixed volume containing three types of matter--blood, brain and cerebrospinal fluid--each of which occupies a portion of that volume. If
20 the portion of the volume of one of the three increases without a concomitant fall in the portions of the other two, the intracranial pressure increases. Because the brain has a limited capacity to adapt to increases in intracranial volume, once the limit has been met, small
25 increases in volume cause significant increases in intracranial pressure.

Maintaining cerebral blood flow to provide adequate oxygen and glucose to the brain is critical. However, an increase in the volume of the brain or of cerebral spinal
30 fluid as the result of trauma, and the like, correspondingly constricts the flow of blood and can stop it completely if the increase in fluid is large enough to herniate the brain at the base of the skull. In such cases, death results.

35 Because it is not practical to monitor cerebral blood flow at the bedside, an algorithm based upon the relationship between mean arterial pressure, intracranial

pressure and the cerebral perfusion pressure is used to calculate blood flow in the brain ($CPP = MAP - ICP$). Thus, a satisfactory means for monitoring intracranial pressure by placement of a pressure transducer into the
5 intraventricular, subarachnoid or intraparentchymal spaces is of utmost importance to the management of head injury cases and has long been sought.

Assemblies for monitoring pressure at various locations within the body are known. The earliest pressure
10 monitoring devices utilize a pressure sensitive diaphragm in contact with a column of sterile fluid contained within a catheter inserted into the blood vessel, the brain, or other area containing a fluid pressure of interest. Pressure exerted by the fluid, for instance the
15 cerebrospinal or cephalorachitic liquid, is transmitted through the fluid column within the catheter to an external pressure transducer that transforms the pressure signal into an analog or digital form suitable for readout on a monitoring device. such as that commonly used to monitor
20 blood pressure. However, pressure monitoring devices that utilize a column of fluid are easily contaminated with bacteria or air bubbles. Air bubbles in the line distort the pressure readings and bacterial contamination of the fluid may inadvertently expose the patient to sepsis. The
25 fluid coupled systems used to monitor intracranial pressure access the compartments of the brain by means of a ventricular catheter or bolts placed through the skull. Since the pressures to be monitored are relatively low (0 - 50 mm Hg), the hydrostatic effects of the fluid column
30 can compromise the readings. Additionally, the fluid column can affect the frequency response of the system.

To eliminate the risks and disadvantages inherent in catheters employing a fluid column for transmitting the pressure reading, improved pressure monitoring devices have
35 been developed that couple the pressure sensitive diaphragm located at the distal end of the catheter with an

electrical or optical means for generating a pressure signal and transmitting it to the proximal end of the catheter, and thence to the pressure transducer and monitor. The electrical pressure monitoring diaphragms are typically fitted with a miniaturized Wheatstone bridge strain gauge comprising a series of resistors whose resistance is modified in proportion to the distance from the zero position the diaphragm of the pressure sensor is displaced by the applied pressure. Electrical pressure sensors are commonly employed in hospital for continuous monitoring of blood pressure and the like. For this reason hospitals employ monitors adapted to receiving an electrical output from the Wheatstone bridge pressure sensor and transforming it into a pressure reading using well known technology. Thus an intracranial pressure monitoring catheter employing an electrical pressure sensor could be plugged directly into the pressure monitor found in most hospital rooms without the need for an expensive intervening transducer to modify the signal into a format compatible with the monitor.

However, in designing a pressure monitoring assembly for monitoring intracranial pressure special considerations are required. Inherent in all electrical pressure monitoring sensors is a risk of electrical shock that may render them unsuitable for insertion into the interior of the brain. Introducing electrical currents into the brain risks permanent damage.

Optical pressure monitoring transducers avoid this risk. Optical pressure sensors generally employ a light reflective diaphragm placed at the distal tip of an optical fiber. Displacement of the reflective diaphragm by applied pressure changes the intensity and/or other spectral characteristics of the reflected light signal, depending upon the type of reflective sensor used. For instance, European Patent Application 0 127 476 owned by Camino Laboratories, Inc., which is hereby incorporated by

reference in its entirety, discloses an optical pressure catheter having a set of optical fibers for transmitting a light beam to and from a transducer which modulates the intensity of the reflected light in accordance with the sensed pressure. A photosensor comprising a bellows compressible by pressure is located at the distal end of the catheter and a photodetector located at the proximal end of the catheter measures the modulated intensity of the returned beam and produces a corresponding measurement signal. However, optical transducers operating upon the principles of intensity modulation suffer from the drawback that any curvature of the fiber optic extraneously reduces the intensity of the reflected light.

To overcome this source of error the Camino catheter preferably also contains a second set of optical fibers for transmitting a reference light beam to and from the location of the sensor. The reference light beam is sent to a second photosensor that measures the intensity of the returned reference light beam and produces a correction signal that compensates for variations in transmittance caused by bending of the catheter.

One of the disadvantages of the Camino system for monitoring intracranial pressure is that a dedicated stand alone interface module, such as that manufactured by Camino Laboratories, is required to display the pressure and communicate with various commercial patient monitors. Zeroing is also dependent upon the interface module, which "reads" the characteristics of the individual sensor and provides for zeroing by means of a screw type adjustment. Additionally, to reduce the error caused by bending the optical fibers, intracranial pressure catheters that rely upon modulated intensity of the reflected beam must be very rigid in construction and are therefore inserted into the skull via a bolt. And the most reliable intensity modulation catheters, since they require four optical

fibers, are larger, more invasive, and therefore inherently more dangerous, than is desirable.

Optical pressure transducers that modulate the wavelength of the reflected light in accordance with the variable to be measured are also known. For instance, U. S. Patents 4,329,058 and 4,678,904, which are hereby incorporated by reference in their entirety, describe an optical transducer having an optically resonant sensor by which the wavelength of the reflected light is modified if the reflective diaphragm is deflected by applied pressure from its zero position. This kind of pressure transducer incorporates a Fabry-Perot interferometer in the reflective sensor.

The Fabry-Perot interferometer operates according to well-known principles whereby the gap between two reflective surfaces causes a plurality of reflections and splittings of a single beam of incident light, such that constructive and destructive interference of the components of the incident light beam may occur numerous times. Inasmuch as an inherent phase reversal occurs when light is reflected from a more dense medium to a less dense medium (for example, when it passes through the diaphragm of the optical sensor to the air or other medium in the Fabry-Perot gap), it is possible for the main reflected light beams to cancel in a gap having a width equal to a multiple of half wavelengths of the incident light. Light beams transmitted through the Fabry-Perot gap and the surface of the sensor (those not having half wavelengths in multiples of the gap width) undergo an even number of reflections, so that, in the event of the phase reversal above described, the even number of phase reversals produces no net phase reversal. These light beams transmitted through the gap are in constructive interference with each other and are therefore transmitted through the gap and returned to the photosensor assembly for processing. Under conditions of high reflectivity,

even a small variation in the frequency of light caused by passage through the Fabry-Perot interferometer dramatically reduces transmission of the frequency-altered light beams.

Based upon these principles (See Handbook of Physics, 5 2d, published by Mc Graw-Hill Section 7, Chapter 5, Part 6 for further information), a Fabry-Perot sensor having a displaceable diaphragm can be used to monitor a physical variable such as applied pressure, temperature, gas density or pH value. In operation, the gap width varies as a 10 function of the physical parameter to be measured. Therefore, the width in the gap corresponding to an applied pressure can be used to measure the pressure. As is described in full detail in U. S. Patent 4,908,474, photodetector circuits can readily compare the incident and 15 reflected light beams to determine the width of the Fabry-Perot gap and compute the magnitude of the sensed variable therefrom. For example, the Model 1400 multisensor system manufactured by Metricor (Woodenville, Washington) can be used with a Fabry-Perot sensor to detect 20 pressure readings generated by as little as a single Angstrom of change in the gap width.

The changes in intensity or in wavelength in reflected light beams can be converted to a signal compatible with conventional monitors for display as a digital readout or 25 printout by a suitable pressure transducer. However, known pressure transducers having this capability, such as those useful for monitoring intracranial pressure are expensive and cumbersome. For instance, U. S. Patents 4,611,600, 4,703,174, and 4,705,047 disclose various types of 30 transducer circuits suitable for receiving reflected light beams and processing them to yield signals to the monitor that indicate the value of the parameter of interest. However, there is great need for an inexpensive optical pressure transducer, preferably one that employing modern 35 techniques of microcircuitry, that operates off the output voltage of the common hospital pressure monitor and

produces a modified electrical signal (such as that supplied by the output from a Wheatstone bridge electrical strain gauge) suitable for input to the same bedside monitor.

5 Intracranial pressure monitoring devices are needed to monitor dangerously high intracranial pressures. One means of reducing elevated intracranial pressure is to drain off cerebrospinal fluid. Thus, a need exists, not only for intracranial pressure monitors, but also for devices for
10 draining fluid from the brain, without inflicting unnecessary damage.

 The pressure monitoring device must be inserted into the interior of the skull through a drillhole. If a second hole is drilled to insert a drain, the risk of trauma is
15 obviously doubled. Thus, the need exists for a single device capable of simultaneously monitoring intracranial pressure and draining cerebrospinal fluid.

 Simultaneous optical pressure monitoring and drainage assemblies are known. For instance, the Camino intensity
20 modulation sensor can be used with an auxillary drain inserted into the skull through a bolt. However, the assembly is subject to breakage, requires a large drillhole to accommodate the bolt, and is assembled out of standard connectors that are subject to leakage and, therefore,
25 provide sources of infection. However, an optical pressure monitoring and drainage assembly is highly desirable because the accuracy of fluid column intracranial sensors is destroyed by simultaneous drainage of cerebrospinal fluids. What is needed is an integral fiber optic pressure
30 transducer and simultaneous drainage system that interfaces with conventional monitors via a low cost processor.

 All pressure monitoring systems require calibration. In pressure monitoring systems utilizing two fluid reservoirs separated by a diaphragm, such as the fluid
35 column pressure sensor, one reservoir is usually in pressure communication with the local atmosphere, while the

other, the applied pressure, is connected to the pressure source to be measured. If the atmospheric pressure is also placed momentarily on the applied pressure input, then the diaphragm moves to the zero point location, and the zero pressure offset error can be measured. However, an implanted catheter, such as an intracranial catheter, cannot be removed for calibration and replaced without introducing the risk of infection. Thus, calibration must be accomplished in situ within the brain.

One means of calibrating a pressure sensor is to provide a substitute pressure transducer system for generating a known test pressure that is displayed on the monitoring device as a calibrated output indicating the level of the known pressure. Another method is that employed by the Model CT/6FB catheter tip pressure transducer manufactured by Medical Measurements Incorporated. In this system the sensor, which includes a mechanical stop to indicate the zero pressure location of the transducer, is depressurized in vivo and calibrated using a micromanometer to provide known test pressures. Thus the zero pressure error and calibration error can be determined. For pressure sensors used in monitoring intracranial pressure, it is particularly desirable to calibrate the sensor in situ so that the sensor can be left in place for up to five days, thereby minimizing the risks of infection and the like. Therefore, the need exists for new and improved pressure monitoring systems such as a dual lumen catheter for monitoring fluid pressure via a first lumen while simultaneously withdrawing an amount of the fluid being measured or infusing a second fluid through a second lumen. And for monitoring intracranial pressure, what is particularly needed is an integrated intracranial pressure monitor and drain assembly, preferably one employing a Fabry-Perot sensor and providing an output signal to standard hospital monitors that "looks like" the signal generated by Wheatstone bridge strain gauge sensors.

SUMMARY

The catheter of this invention is used in a pressure monitoring assembly that comprises, in basic form, a catheter housing at least one lumen containing a pressure sensor means for generating a pressure signal, which sensor is in communication with a transducer means for converting the output pressure signal from the sensor into electrical signals. Optionally, the sensor has a vent to provide fluid communication with a reference pressure via the first lumen. The catheter usually contains a second lumen that serves as a fluid conduit for infusing or draining fluids through the catheter while monitoring pressure. In addition, the second lumen is adapted to receive a stylet, which is inserted therein as a stiffening agent while the catheter is placed into the brain or other location of operation.

Preferably the above-described catheter is an integral intracranial pressure monitoring and drainage catheter used in a pressure monitoring assembly that comprises, in basic form, a light source, one or more light transmission means, one or more spectral modulation sensors having optically resonant structures, a photodetector means for converting the output light from the spectral modulation sensor(s) into electrical signals of the type generated by a Wheatstone bridge piezoresistive strain gauge, and a monitor means for receiving the signals and displaying the pressure measurement(s). The catheter allows for simultaneous intracranial pressure monitoring and drainage of cerebrospinal fluids.

It is a feature of the preferred embodiment that the monitor provides the excitation voltage to the photodetector and that the photodetector scales the excitation voltage to create the measurement signal(s), which are returned to the monitor to be displayed as the pressure measurement(s).

BRIEF DESCRIPTION OF THE FIGURES

FIG. 1 is an illustration of one preferred embodiment of the catheter and stylet of the present invention.

FIG. 2 is a cross-sectional view of the preferred dual
5 lumen catheter housing.

FIG. 3 is a schematic illustration of the catheter assembly employing a spectral modulation sensor.

FIG. 4 is an illustration of a spectral modulation sensor.

10 FIG. 5 is a graphic representation of a reflectivity curve for an optically resonant structure.

FIG. 6 shows a portion of the curve of FIG. 5 during operation of the spectral modulation sensor.

FIG. 7 is a schematic illustration of the catheter
15 assembly employing the spectral modulation sensor with a ratiometric photodetector.

FIG. 8 is a schematic illustration of the catheter assembly employing two spectral modulation sensors with a ratiometric photodetector.

20 FIG. 9 is a graphic representation of the spectrally modulated output light from a spectral modulation sensor having multiwavelength input light.

FIG. 10 is a cross-sectional view of a spectral modulation sensor having a zero stop.

25 FIG. 11 is an illustration of the sensor of Fig. 10 under applied pressure.

FIG. 12 is an illustration with partial cut-away view of the catheter assembly employing an intensity modulation sensor.

30 DESCRIPTION OF THE PREFERRED EMBODIMENT

In a preferred embodiment, the catheter is a dual lumen catheter adapted for insertion into the ventricular and/or parenchymal spaces of the brain of humans and other mammals for measuring intracranial pressure and for
35 simultaneously draining cerebrospinal fluids. As shown in

Figure 1, the catheter comprises catheter housing 54, which encloses first lumen 70 and optional second lumen 72.

Catheter housing 54 is an elongate flexible tube closed at the distal end, except for sensor aperture 76, to facilitate insertion of the catheter into the environment whose pressure is to be monitored. Sensor aperture 76 opens into the distal end of first lumen 70 and provides external fluid access to the pressure sensor.

Usually catheter housing 54 is extruded from a biocompatible plastic material, preferably silicone rubber. Catheter housing 54 is elongate, flexible and sized to be passed through a borehole in the skull and received within the brain.

First lumen 70 extends continuously from the proximal end to sensor aperture 76 at the distal tip of the catheter housing and has a diameter of between about .005 and .050 square inch for containing a pressure sensor and a means for transmitting to the proximal end of catheter housing 54 a signal containing information regarding the pressure measurement sensed by the sensor.

The pressure sensor can be any known pressure sensor device suitable for insertion into a catheter. However, catheters are primarily useful for operations that require the least intrusive means of measuring pressure. Therefore, pressure sensor is usually selected to minimize the diameter of first lumen 70.

Non-limiting examples of the types of pressure sensors that can be housed within the first lumen fall into four types. The first are fluid column sensors wherein the pressure measurement is transmitted from the distal to the proximal end of the catheter housing via a column of liquid being in fluid or, at the least, pressure communication with the fluid whose pressure is being monitored. Usually, a transducer located externally to the catheter housing generates an electrical signal from the measurement signal provided by the fluid column. A second type of sensor

employs piezo-resistive strain gauge pressure sensors wherein the change in resistance of small resistors located in the sensor upon a pressure sensitive diaphragm at the distal end of the catheter generates the pressure measurement signal. The electrical pressure measurement signal is transmitted via electrical wires located within the first lumen to a transducer located at the proximal end thereof, usually completely externally to the catheter housing. A third type of pressure sensor employs optical means for generating the pressure measurement signal at the distal end of the catheter housing and for transmitting the signal to the proximal end thereof. Optical pressure sensors usually transmit the pressure signal by means of at least one optical fiber located within the first lumen of the catheter housing.

There are two known basic types of optical pressure transducer, those that generate a pressure signal by detecting the degree to which the intensity of a source light beam is modulated when it is reflected from a moveable pressure sensitive diaphragm, and those that generate a pressure signal by detecting the constructive and destructive interference in a source light beam when it is reflected from a moveable pressure sensitive diaphragm. The later type of sensor, which employs an optically resonant structure, is preferred herein because such sensors can be made to yield a pressure signal that is linear with pressure over the desired pressure range and because such sensors require a single optical fiber, yet yield measurements of high accuracy.

When an optical pressure sensor is housed within the first lumen, as shown in Fig. 1, the sensor transmits the optical measurement signal via an optical fiber means extending from the first lumen and having located thereon a test port 97 and an optical fiber connector 96 for providing optical communication to a photodetector means (not shown) with which it is in optical communication.

As shown in Fig. 1, catheter housing 54 optionally contains a second lumen 72 for transporting fluids between the distal and proximal ends of catheter housing 54. Second lumen 72 can have any cross-sectional area appropriate to the application for which it is intended. When used as a drain for draining cerebrospinal fluid, for example, lumen 72 has a diameter of between about .025 and .100 square inch and extends continuously from the proximal to the distal end of the catheter housing, opening at the distal end exterior to catheter housing 54 through aperture 67. At the proximal end optional lumen 72 is fluidtightly attached to drain conduit 66 by any suitable means of attachment 78, preferably one containing a drainage port such as a luer lock fitting. Drain conduit 66 can be provided by any flexible tubing material, such as common hospital polyvinylchloride tubing.

Preferably, catheter housing 54 is about six inches in length, and a plurality of apertures 67 opening into second lumen 72 are spaced along the distal end, preferably along about the extreme half inch of the catheter housing. Most preferably, aperture 67 are bore holes having a diameter of from about .005 to .050 inch, and the bore holes are arranged in three rows along the length of the catheter housing 54, most preferably at .100 inch intervals for allowing an unobstructed flow of cerebrospinal or other fluid therethrough.

Optionally, first lumen 70 is in fluid communication with the sensor 22 contained in first lumen 70 via vent 62 (shown in Figs. 10 and 11) and is used to vent the sensor to the atmosphere or to apply a reference pressure, such as atmospheric pressure, to the sensor for in situ calibration, as is explained in full hereinafter.

In addition, second lumen 72 is optionally adapted to receive therein stylet 74, which is a slim, stiff rod made of any non-brittle material, such as plastic or metal, and has a handle means, such as a loop 99, at one end for

inserting and removing the stylet. When inserted into second lumen 72, stylet 74 provides stiffness to the catheter housing while it is being inserted into the brain and can be removed thereafter so that second lumen 72 can
5 be used as a fluid conduit.

In one embodiment shown in Figure 2 in cross section, first lumen 70 and second lumen 72 have the general arrangement of a tube within a tube. The first lumen is adapted for housing one or more fiber optics and is
10 comprised of a tube 75 having a relatively smaller diameter, for example 0.016 inch, than the diameter of the housing 54, which is, for example 0.100 inch. As is also shown in Figure 2, first lumen 70 is fixedly attached along one interior side of the larger second lumen 72 such that
15 the remaining open space within the housing forms a second irregularly shaped conduit 66, the exterior of the first lumen having a single cross-sectional point of tangency with the interior circumference of second lumen 72. The catheter housing containing the first and second lumens can
20 optionally be coextruded from silicone rubber. In this embodiment of the invention, apertures 67 are preferably arranged in rows, preferably three rows along the length of second lumen 72, which itself forms the catheter housing, and are preferably located at angles of 90, 180 and 360
25 degrees around the cross-sectional circumference of second lumen 72 as measured from said point of tangency.

When conduit 66 is used for draining or infusing fluids, it is in fluid communication with the exterior of the catheter housing via at least one of apertures 67.

30 The preferred pressure sensor housed within the first lumen of the catheter is a spectral modulation sensor located at the distal end thereof. The light transmission means comprises an input optical fiber, an optical beam splitter, an optical fiber connector, a sensor optical
35 fiber, and an output optical fiber. The optical beam splitter and optical fiber connector optically connect the

sensor optical fiber with the input and output optical fibers.

5 A single optical fiber namely the sensor optical fiber, acts to both convey input light to the spectral modulation sensor and to convey output light reflected therefrom. This simplifies the optical measuring device, reduces its size and cost, and increases its reliability as compared to a system employing two or more optical fibers for conveying light to and from the sensor. Moreover, the
10 use of a single optical fiber reduces the external diameter of the catheter to a minimum and leaves open space surrounding the optical fiber within the first lumen proximal to the sensor, which open space can be used to vent the sensor to a reference pressure via a vent in the
15 sensor substrate, the first lumen and the vent serving as a conduit to the cavity between the reflective surfaces of the sensor.

The spectral modulation sensor has as its active element an optically resonant structure, comprising a pair
20 of separated reflective surfaces, with the reflectivity and transmission of the resonant structure being a function of the distance between its reflective surfaces. In spectral modulation sensors, the optical characteristics of its reflecting surfaces, and the index of refraction of the
25 medium between its reflective surfaces will also affect the reflectivity and transmission of the sensor; therefore, in this invention the said medium is held constant so as to have no effect upon the measurement signal.

Thus, if the distance between the reflective surfaces
30 of the spectral modulation sensor's optically resonant structure is altered by the pressure being measured, then the light reflected and/or transmitted by the spectral modulation sensor will change as a function of the measured pressure. Accordingly, the output light from the spectral
35 modulation sensor will be spectrally modulated by its optically resonant structure as a function of the pressure

measured and carries information regarding the physical parameter being measured.

The spectrally modulated output light from the spectral modulation sensor is converted into an output
5 electrical signal by the photodetector means which comprises photodetector and amplifier means. The output electrical signal provides an accurate determination of the physical parameter being measured, within a certain range of values for the pressure being measured once the optical
10 measuring device has been calibrated.

However, the basic form of the invention may be susceptible to measurement inaccuracies due to two causes. The first cause is changes in the light source intensity or in light transmission intensity due to bending of the
15 optical fibers or due to optical connector light loss. These inaccuracies can be eliminated if the light source is selected to emit light over at least two wavelengths such as is provided by a light emitting diode (LED), for example. A second cause of inaccuracy is spectral
20 modulations in light from light emitting diodes caused by a change in temperature of the diode.

The inaccuracies caused by transmission loss and variations in the light source can be corrected automatically by the detection means if the spectrally
25 modulated output light wavelength(s) from the spectral modulation sensor are separated into two spectral components, each of which is separately converted into an electrical signal by photo detector means and then amplified. The two amplified signals are sent to a divider
30 circuit that takes the ratio of the two electrical signals to provide an output signal that is accurate within a certain range of values for the physical parameter being measured, once the optical measuring device has been calibrated.

35 Because changes in the light source intensity or in light transmission intensity due to bending of optical

fibers normally effect the two spectral components of the spectral modulation sensor equally, when the two electrical signals corresponding to the two spectral components are divided in the divider circuit, such changes cancel each other out and have no effect on the output signal from the divider circuit.

To self correct for temperature caused inaccuracies in the apparatus, the optical fiber beam splitter contains a filter that separates the spectrally modulated output light wavelengths from the spectral modulation sensor into two spectral components. This filter is selected to incorporate a temperature effect upon the spectrum of light emitted from it that matches or "tracks" the spectral temperature effect of the light emitting diode with which it is in optical communication. By this matching of the spectral shift in the LED with that in the filter, the detection means provides a self-correcting device for removing any spectral modification in the output light caused by a change in temperature of the diode during operation of the apparatus.

Thus, the invention features a self correcting detection means requiring no adjustment by the operator during operation.

Turning now to Fig. 3, the first embodiment of the integral pressure sensor and fluid transport catheter assembly is schematically illustrated. Light source 10 is for providing suitable measuring input light, which may be monochromatic or which may be dispersed over two or more adjacent or non adjacent wavelengths bands. Light source 10 can comprise a single source of monochromatic light, such as a laser or a lasing diode, a source of two or more wavelengths such as a light emitting diode, and/or suitable optical filters to provide the desired input light. Power for light source 10 is provided by any suitable source of electrical power through conventional electrical connection means 11.

Input light from light source 10 is coupled into sensor optical fiber 14 via input optical fiber 12 optical beam splitter 18 and optical fiber connector 20.

Optically connected to the end of optical sensor fiber 14, and receiving input light therefrom, is a spectral modulation sensor 22 having an optional substrate 9 supporting an optically resonant structure 21. If used, substrate 9 preferably has a thickness about equal to the diameter of sensor optical fiber 14. Improved sensitivity of optically resonant structure 21 results if substrate 9 is used because light entering optically resonant structure 21 from sensor optical fiber 14 is relatively more collimated than if substrate 9 were omitted and sensor 22 were secured directly to the end of sensor optical fiber 14. If substrate 9 is omitted, optically resonant structure 21 is secured directly to the end of sensor optical fiber 14. Substrate 9 serves as an aid in the manufacture of sensor 22 and in the assembly of optically resonant structure 21 to the end of sensor optical fiber 14, since as well known, optically resonant structure 21 can be less than 1 micron thick. Preferably, substrate 9 does not play a part in spectrally modulating the measuring input light to optically resonant structure 21, but it could do so.

Optically resonant structure 21 comprises, in general, a pair of separated reflective surfaces 13 and 15 with the reflectivity and transmission of the optically resonant structure being a function of its optically physical sensitive characteristics, such as the distance between reflective surfaces 13 and 15, the optical characteristics of reflective surfaces 13 and 15, and the index of refraction of any medium located within cavity 17 between reflective surfaces 13 and 15. In this invention, the output light from sensor 22 is spectrally modulated by optically resonant structure 21 as a function of the distance between reflective surfaces 13 and 15. For

measuring fluid pressure, it is further preferred that the medium in cavity 17 be either a vacuum or air, both of which have an index of refraction of one and therefor have no effect upon the reflectivity and transmission of the optically resonant structure.

Spectrally modulated output light from sensor 22 travels sequentially through sensor optical fiber 14, optical fiber connector 20, optical beam splitter 18 and output optical fiber 16 where it is optically coupled to photodetector 30 in photodetector assembly 50. Photodetector assembly 50 comprises photodetector 30, and amplifier 34, which receives an output signal from photodetector 30 via electrical connection means 32. The amplified output signal from amplifier 34 is delivered to output terminal 36, and provides a measurement of the sensed pressure.

Power is provided from any suitable source to photodetector 30 and amplifier 34 through electrical connection means 31 and 33, respectively.

Spectral modulation sensor 22 is shown in Fig. 4 in greater detail. Sensor 22 preferably comprises a cylindrical substrate 24 defining a cylindrical cavity 26 and has a cover 28 which covers cavity 26. Cavity 26 has a reflective bottom surface 27 while cover 28 has a reflective inner surface 29 and an outer surface 25, surfaces 27 and 29 being parallel. It is preferred, but not required, that the thickness of substrate 24 between bottom 27 and the end of sensor optical fiber 14 be as was discussed regarding substrate 9 of sensor 22 with regard to Fig. 3.

If an absolute pressure sensor is desired, then cavity 26 is preferably evacuated, cover 28 providing it with a fluidtight seal. Alternatively, if a differential pressure sensor 22 is desired, cavity 26 is in fluid communication via optional conduit 41 and the first lumen (not shown) with a source of pressure, such as atmospheric pressure,

while a source of applied pressure bears against outside surface 25 of cover 28. Naturally, optional conduit 41 is omitted if sensor 22 is to be an absolute pressure sensor.

5 Reflective surfaces 27 and 29 are preferably coated with about 100 to 200 Angstroms of high refractive index transparent media, for reasons explained hereinafter.

Cavity 26, its reflective bottom 27, and reflective intersurface 29 of cover 28 form optically resonant structure 21. Alternatively, cavity 26 can be formed in
10 cover 28 rather than in substrate 24. As alternative constructions for sensor 22, it is of course possible to form cavity 26 in cover 28 rather than in substrate 24; or even to form the cavity partially in substrate 24 and partially in cover 28, without departing from the scope of
15 the invention.

The method of making sensor 22 and its optically resonant structure is described in detail in U.S. Patent 4,678,904, which is incorporated herein by reference in its entirety. It should be noted here, however, that when
20 cavity 26 is evacuated, a getter structure (not shown) in the form of a ring of deposited layers of chrome and iron is optionally deposited in the bottom of each cavity 26 to absorb residual gases or subsequent outgassing in cavity 26 after the initial evacuation thereof is performed. The
25 optional getter structure comprises a donut shaped ring of the deposited chrome and iron layers with an inner diameter of about 140 microns and an outer diameter of about 190 microns centered in bottom 27 of cavity 26. Thus, getter rings leave a clear central portion of about 140 microns in
30 diameter in the bottom of each cavity 26 through which light can pass. After cover 28 is bonded to cavity 26, the getter ring removes gases from cavity 26.

When in operation as an absolute pressure sensor, sensor 22 is subjected to an external pressure such that
35 cover 28 over evacuated cavity 26 is bowed inwardly toward the reflective bottom 27 of cavity 26 to a greater or

lesser degree depending upon the amount of external pressure. As the external pressure on cover 28 increases, such bowing increases; and as the external pressure decreases, the bowing decreases and becomes zero when the
5 external pressure is zero.

Thus, as the external pressure on cover 28 increases and decreases the distance between reflective surfaces 27 and 29 of optically resonant structure 21 alters. Changes in the said distance of as little as one Angstrom in length
10 can be detected by the catheter assembly of this invention.

When sensor 22 is operated as a differential pressure sensor, one source of pressure is fluidly communicated to cavity 26, such as through conduit 41 and the first lumen, while surface 25 of cover 28 is exposed to a second source
15 of pressure. Cover 28 will bow inwardly towards reflective bottom 27 of cavity 26 when pressure on surface 25 of cover 28 exceeds that within cavity 26, the amount of bowing depending upon the pressure differential, and will not bow at all when the pressure differential is zero. However,
20 when the pressure within cavity 26 is greater than that on surface 25 of cover 26, cover 28 will bow outwardly, the amount of bowing again depending on the pressure differential.

Whether sensor 22, is used as an absolute or
25 differential pressure sensor, bowing of cover 28 in response to applied pressure alters the distance between reflective surfaces 27 and 29, which in turn produces corresponding microshifts in the reflectivity curve and operating segment(s) of optically resonant structure 21 as
30 a function of the pressure to which sensor 22 is subjected, as will be described in greater detail hereinafter. As a result, output light from sensor 22 is spectrally modulated as a function of the pressure to which sensor 22 is subjected and carries accurate information regarding such
35 pressure.

To make and use sensor 22, a brief summary of its theory of reflectivity is required. The reflectivity R of parallel plane optically resonant structure 21 is well known to be a periodic function of the wavelength of its input light--a common characteristic of optically resonant structures. Figure 5 shows a typical reflectivity curve 40 of parallel plane optically resonant structure 21 having a given set of physical characteristics. It should be particularly noted that reflectivity curve 40 also represents the reflectivity curve of optically resonant structure 21 when the reflective surfaces are not parallel (i.e., when the moveable diaphragm is not in the zero position). Reflectivity R of parallel plane optically resonant structure 21 is known to be given by the equation:

$$R = 1 - s^2 / ((1-r)^2 + 4r^2 \sin^2 (\theta))$$

$$\text{Where } s = (s_1, s_2)^{0.5} \text{ and } r = (r_1, r_2)^{0.5}$$

The quantities s_1, s_2 are, respectively, the transmittances of reflective surfaces 13 and 15 while r_1, r_2 are, respectively, the reflectances of reflected surfaces 13 and 15 (or 27 and 29) as seen from within parallel plane optically resonant structure 21. The angle θ in the sine term of the above equation is known to be given by:

$$\theta = 2(\pi)nt \cos (\phi) / \lambda + e$$

Where:

n = the refractive index of medium 17 between reflective surfaces 13 and 15;

t = the distance between reflective surfaces 13 and 15;

35

-23-

phi = the angle of light reflection between reflective surfaces 13 and 15;

5 lambda = the wave length of input light impinging on optically resonant structure 21;

e = any phase shift caused by reflection from either reflective surface 13 or 15.

10 Parallel plane optically resonant structure 21 is designed so that parameter group $nt \cos(\phi)/\lambda$ changes in response to applied pressure as distance t changes. Thus, for any selected wavelength of input light, parallel plane optically resonant structure 21 will exhibit
15 varying reflectivity as a function of pressure.

Figure 6, which shows an enlarged portion of reflectivity curve 40, illustrates the effect on reflectivity curve 40 when distance t between the reflective surfaces of its particular corresponding
20 optically resonant structure 21 is altered.

As is also seen in Figure 6, reflectivity curve 40 of optically resonant structure 21 is shifted to the left, with respect to any particular selected wavelength L_1 of input light from light source 10, to become reflectivity
25 curve 40' when the distance between its reflective surfaces 13 and 15 is reduced; and it is shifted to the right with respect to L_1 to become reflectivity curve 40" when the distance between its reflective surfaces 13 and 15 is increased.

30 By way of nonlimiting example, a resonance cycle on reflectivity curve 40 of any optically resonant structure 21 is ΔB , as seen in Figure 3.

In general the reflectivity curve of any optically resonant structure 21 shifts left and/or right with respect
35 to wavelength L_1 as a function of any change in the distance between its reflective surfaces, and hence as a function of

any change in the measured pressure, such shifts being termed herein microshifts. The resonant cycle of the reflectivity curve of any optically resonant structure 21 is defined as one complete cycle on its reflectivity curve.

5 There are, of course, a plurality of such resonance cycles on its reflectivity curve since a resonance cycle may start anywhere on its reflectivity curve.

It is known that accurate measurements of pressure can be made using operating segments of the reflectivity
10 curve of the particular optical resonant structure 21 that are less than about one resonant cycle in length and by using operating segment microshifts which are also less than about one resonance cycle in length at the measuring input light wavelength(s). As the reflectivity curve is
15 cyclic, there are a plurality of such operating segments on it.

By way of nonlimiting example, if the operating segment of reflectivity curve 40 of Figure 3 were A"B" it is of course, one resonance cycle in length. Further, if
20 in response to sensed pressure operating segment A"B" were microshifted to the left until point B" intersected wavelength L_3 , then the microshift of operating segment A"B" would be one resonance cycle in length.

With regard to the embodiment of the invention wherein
25 light source 10 delivers monochromatic input light of a wavelength, such as L_1 , wavelength L_1 does not change in response to sensed pressure. However, from an inspection of Figure 6 it is seen that for any given intensity of any input light of wavelength L_1 to sensor 22, the output
30 intensity at wavelength L_1 will be different when distance t is altered in response to sensed pressure, as compared to distance t when sensed pressure is zero. Thus, operating segment AC of optically resonant structure 21 undergoes a microshift to the left and/or right of operating segment AC
35 (to become A'C' and A"C") in response to the pressure being measured.

Thus, sensor 22 is a spectral modulation sensor whose optically resonant structure 21 modulates input light of wavelength L_1 as a function of the pressure being measured and produces modulated output light of light wavelength L_1 that carries information regarding the pressure being measured. This information is converted by photodetector 30 and amplifier 34, as has been described, into an electrical output measuring signal carrying the same information.

10 Naturally, the wavelength(s) of input light from light source 10 and the distance between reflective surfaces 13 and 15 of optically resonant structure 21 are selected such that the wavelength(s) of input measuring light fall at least substantially within the desired operating segment of its reflectivity curve, such as AC for example, over the
15 desired operating range of values for pressure being measured. Thus, as seen in Figure 6, wavelength L_1 remained within operating segment AC, despite operating segment AC being microshifted by optically resonant structure 21 in response to sensed pressure to become A'C' and/or A"C".

20 Preferably, the operating segment, the wavelength(s) and/or amplitude(s) of the input measuring light are selected to obtain an operating segment of greatest length which will yield unambiguous spectrally modulated output
25 light over the range of values of the interest of for the pressure being measured.

For example, for a monochromatic input light of wavelength L_1 , changes in the output light of optically resonant structure 21 are maximized when operating segment
30 AC extends, as illustrated in Figure 6, between any maxima and adjacent minima (or vice versa) on its reflectivity curve 40, and when the pressure being measured alters optically resonant structure 21 such that its operating segment AC intersects the input measuring light wavelength
35 L_1 , i.e., is microshifted a full half resonance cycle. Most preferably, only the linear portion of the operating

segment is used. So that the spectrally modulated output light bears a unique one to one relationship to the pressure being measured over the range of values of interest.

5 To maximize sensitivity, it is desirable to increase the maximum to minimum reflectivity difference of optically resonant structure 21, such as between AC in Figure 3. This is done by coating at least one of reflectivity surfaces 13 and 15 with an appropriate thickness, say 100
10 to 200 Angstroms, for example, of a high refractive index transparent media that increases surface reflectivity, such as rutile, titanium dioxide, cubic zirconia or silicon.

An alternative and preferred embodiment of the invention is illustrated in Figure 7. In this embodiment,
15 light source 48 is chosen to produce at least two light wavelengths and may be, by way of example, a light emitting diode (LED) which emits a band of light wavelength(s) centered at approximately 810 nm, such as part #MFOE1202, made by the Motorola Company. Power for light source 48 is
20 provided by any suitable source of electrical power through electrical connection means 49.

Spectrally modulated output light from output optical fiber 16 is directed onto a beam splitter 51 which divides it into two output light beams. The first output light
25 beam from beam splitter 51 passes through short pass optical filter 52, which transmits to an appreciable degree only light having a wavelength shorter than a given, preselected wavelength. The short wavelength output light band from filter 52 is converted to a first electrical
30 signal by photodetector 154 and then conveyed to amplifier 156 by electrical connection means 158 to be amplified by amplifier 156. Said preselected wavelengths may be, by way of example, the wavelength of light from light source 48 of highest intensity, such as the wavelength of 810 nm, for
35 the particular LED mentioned above.

The second output light beam from beam splitter 51 passes through long pass optical filter 160, which transmits to an appreciable degree only light having a wavelength longer than said given, preselected wavelength.

5 The long wavelength output light band from filter 160 is converted to a second electrical signal by photodetector 162 and then conveyed by electrical connection means 164 to amplifier 166 to be amplified by amplifier 166. Amplifiers 156, 166 preferably amplify their respective signals to the

10 same degree.

The amplified first and second electrical signals from amplifiers 156, 166 are conveyed to a divider circuit 168 by electrical connection means 170 and 172. Divider circuit 168 takes a ratio thereof and provides an output measuring

15 signal to electrical connection means 174. The output measuring signal carries information regarding the physical parameter being measured.

Power for photodetectors 154, 162, amplifiers 156, 166 and divider circuit 168 are provided by any suitable source

20 of electrical power through electrical connections means 176, 178, 180, 182, 184, respectively. Preferably, however, power to the photodetector assembly is provided by a hospital bedside monitor such that the excitation voltage to the photodetector assembly is scaled by amplifiers

25 156, 166 and divider circuit 168 to provide an output signal to the monitor.

In the most preferred embodiment of the invention the pressure monitoring apparatus employs a multiwavelength light source providing at least two wavelengths of light

30 and a second, reference sensor having a second photodetector for producing a reference signal by operations that repeat the operations described above with reference to the photodetector means depicted in Fig. 7. The photodetector assembly compares the reference signal

35 with the measurement signal to produce an absolute

measurement signal that is free from transmission, barometric pressure, and temperature errors.

Most preferably, as shown schematically in Fig. 8, the photodetector assembly means 100 splits light received from a single multiwavelength source 48 by means of beamsplitter 102 and steers split beams 114 and 116, each containing at least two light wavelengths, to spectral modulation sensors 22A and 22B by means of optical fibers 16A and 16B (not shown), respectively.

Sensor 22A is located at the distal tip of the catheter assembly (not shown) and sensor 22B is a reference transducer located elsewhere. Each of the sensors contains an optically resonant structure 21A and 21B consisting of two parallel reflecting surfaces 27A, 29A and 27B, 29B separated by a hollow cavity 26A and 26B to form a Fabry-Perot gap. The cavities of sensors 22A and 22B are maintained at a vacuum, while a pressure to be measured is applied to the pressure sensitive surface 25A of sensor 22A.

The reflected light beams from sensors 22A and 22B are transmitted via fiber optics 16A and 16B and beamsplitters 106, 108, 110 and 112 to separate photodetectors 30A and 30B as described above. Each photodetector comprises means 52A and 52B and 60A and 60B for integrating the intensity of the reflected light beam directed thereto over a first and a second different wavelength bands. Preferably, means 52A and 60A are a first pair of short pass and long pass optical filters centered on a preselected wavelength from the first wavelength band of beam 114 from light source 48, and means 52B and 60B are a second pair of optical filters centered on a different preselected wavelength selected from the second wavelength band of beam 116.

The integrated signals are sent via connector means 94A, 96A, 94B, 96B to means 90A and 90B respectively for taking the ratio of the two integrated signals to produce from each reflected light beam a normalized signal output

at connectors 92A and 92B. The normalized signals are independent of the absolute intensity of the reflected light beam. (For example photodetector 30A takes the ratio of the integrated signals from short pass and long pass filters 52A and 60A.) The resulting signal from each photodetector represents a measure only of the distance between the reflecting surfaces of the sensor from which it emanates. The normalized signals output at terminals 92A and 92B are then transmitted via connectors 93A and 93B to means for subtracting the signal transmitted via connector 93A from the signal transmitted via connector 93B to yield a signal representing the difference between the applied pressure and the reference pressure output at terminal 118.

It is especially preferred that photodetectors 52A 60A, 52B, 60B, divider means 90A, 90B and means 116 for subtracting the signals output from the divider means be such that when the input voltage received at input terminal 120 is the output voltage provided by any of the common types of hospital monitor devices, which can be either direct, alternating, or pulsed, the said photodetector assembly "scales" the input voltage by the above described operations thereon to generate an electrical signal at output terminal 118 that can be returned to the monitor for display as a pressure measurement reading. In other words, the preferred photodetector assembly produces an output signal that "looks" like one produced by a Wheatstone bridge piezoresistive electrical pressure sensor.

When the pressure applied to reference sensor 22B is atmospheric and sensor 22A is vented to atmospheric pressure via conduit 41 and first lumen 70, the resultant measurement signal represents the gauge pressure at surface 25A of sensor 22A.

Any commercial photodetector device capable of performing the above operations can be used as photodetectors 30A and 30B, for example, the Model 1400

Multisensor System manufactured by Metricor Corporation (Woodenville, Washington).

This technique of spectroscopic normalization is sensitive only to variations in the source light beam, with spectral microshifts appearing as pressure changes for an individual sensor. By using the same light source for both sensors and computing the difference as described above to find the pressure, any microshifts in the spectrum that might occur in the source beam during the course of the monitoring period will affect both reflected beams equally and thus cancel at the ratio taking step.

As has been mentioned, the catheter assembly employing a multiwavelength light source 48 is self correcting for changes in the intensity of light source 48 and changes in light transmission intensity due to bending of optical fibers and due to light loss in optical connectors. Both short and long wavelength output light band from optical filters 52 and 60 are effected equally by intensity changes. Accordingly, when their respective amplified first and second electrical signals are divided in divider circuit 68 or divider means 92A and 92B, such changes cancel each other out and have no effect on the output measuring light signal therefrom. Such dividing of two signals is known as radiometric signal processing.

Moreover, to self correct for signal errors resulting from temperature effects upon the LED's, optical filters 52 and 60 are selected such that temperature changes produce a microshift in the respective output light band equal to and in the same direction as is produced by temperature change in the output light from the LED. Similarly, beamsplitters 108 and 112 optionally can contain filters selected to accomplish the same goal with regard to source 48, when it is an LED. Therefore, the microshift in the operating signal produced by temperature effect in the LED is canceled by the corresponding microshift produced in the operating segment by selection of the filter. Thus,

photodetector assembly means 50 and 100 are self correcting for any microshift in output signal caused by effects other than those caused by changes in the measured pressure.

It is within the scope of the present invention to
5 eliminate the inaccuracies in the output measuring signal discussed above by having photodetector assembly means 100 take the ratio of the electrical signals corresponding to any two different portions of the output light from the sensors, even wherein one portion may be the entire output
10 light from the sensor.

Light source 48 can comprise at least two sources of monochromatic light such as lasers or laser diodes, if a minimum of two wavelengths are required. Alternatively, it could comprise one or more sources of a plurality of
15 wavelengths, such as LED's or white light sources, along with suitable optical filters, as needed, to provide the at least two input measuring light wavelengths and/or wavelength bands.

However, it is preferred for simplicity that light
20 source 48 be a single LED whose band width is substantially less than the resonant cycle length of the reflectivity curve of optically resonant structure 21.

The theoretical constraints on operation of the ratiometric preferred embodiments of the spectral
25 modulation sensor require different operational parameters to avoid ambiguity in the output signal than are required with monochromatic light. The ratiometric embodiments, it will be remembered, require at least two different input measuring light wavelengths to the photodetector assembly.

30 It is known that when multiwavelength source light is used, the output light signal from spectral modulation sensor 22 contains a minimum of ambiguity when the maximum length and the maximum microshifting of the operating segment on its reflectivity curve both approach but do not
35 exceed about one full resonance cycle. This criteria is different than that for the embodiment of the invention

employing monochromatic input measuring light. In that case the maximum length and maximum microshifting of the operating segment of the reflectivity curve should not exceed one-half of a resonance cycle. Of course, the length and microshifting of the operating segment may be selected to be considerably less than the maximum allowable so as to improve linearity in the output light signal of optical resonance structure 21.

The intensity curve of the output light of multiwavelength light source 48 is shown in Fig 9 by curve 86, wherein light source 48 is a single LED. Wavelength L_2 is, by way of example, selected to be at or near the most intense output wavelength of light from said light source. Also schematically shown in Figure 9 is an enlarged portion of reflectivity curve 40 taken from Figure 5, which illustrates by way of example, operating segment DE on reflectivity curve 40 on optically resonant structure 21 and corresponding reflectivity curve 45 and operating segments D'E' which result from a shift of reflectivity curve 40 to the left due to the influence of sensed pressure on the distance between the reflective surfaces of optically resonant structure 21. Reflectivity curve 40 and its operating segment DE could also be shifted to the right in the same manner, but this is not illustrated in Figure 5 for clarity.

The optically resonant structures used in this preferred embodiment of the invention and described in U. S. Patent 4,678,904 are fabricated from a silicon wafer using photolithography and micromachining processes. These sensors are remarkably free from the phenomenon commonly known as "drift" wherein the "zero" reading of the transducer varies over time. When the spectral modulation sensors are employed in an intracranial pressure monitoring assembly the reliability and constancy of the pressure reading is of utmost importance. Dangerously elevated pressures in the brain are usually on the order of only

about 50 mm Hg so that small inaccuracies in pressure readings may have dangerous consequences.

However, all pressure sensors are subject in some degree to inaccuracies wherein the monitor reads some pressure other than zero in the absence of any applied pressure and to calibration error, wherein the transducer reading is larger or smaller over the range of measured pressure than it should be. But an intracranial catheter cannot be removed to check the accuracy of the reading without subjecting the patient to increased risks of trauma and infection.

Therefore, in one embodiment of the invention, the pressure monitoring assembly is designed to allow correction of the offset error and any calibration error without removing the applied pressure and venting the transducer to atmospheric pressure (ie. without removing the catheter from the patient's brain). The problem is eliminated by providing a means for positioning the pressure sensitive diaphragm of the sensor in the same position as it would occupy under the condition of equal pressures so as to allow for in situ calibration testing.

As is shown in Fig. 10, to provide for in situ calibration of the sensor, during fabrication of circular pressure sensitive diaphragm 28, a ground and polished glass wafer 56, between about 0.005 and 0.025 inch thick, preferably about 0.011 inch thick, is bonded concentrically thereto. Glass wafer 56 is chemically etched using known methods to form a circular channel 58 concentric to the center point of the wafer, the width of the channel usually being between about ____ and ____ inch. Etching of the channel leaves an outer concentric raised ring and an inner raised concentric circular plateau, or "stop" 56A on the surface of the glass wafer. Glass wafer 58 and substrate 24 are chemically bonded concentrically to surface 25 of circular diaphragm 28 such that the centers of the circular substrate, diaphragm, and glass wafer are

coaxially aligned. When so aligned, the surface of "stop" 56A formed by etching the channel into the glass wafer rests against surface 25 of diaphragm 28, but is not bonded thereto. The outer radius of channel 58 has a diameter
5 equal to or greater than that of circular cavity 26 etched into substrate 24.

Thus, as is shown in Fig. 10, under zero pressure surface 25 of diaphragm 28 is flush against the surface of the stop 56A. But, as is shown in Fig. No. 11, under
10 applied pressure surface 25 of diaphragm 28 is deflected from the stop a distance proportional to or at least functionally related to the amount of applied pressure.

Wafer 56 contains aperture 60 therethrough opening into channel 58, through which aperture an applied pressure
15 impinges upon and deflects diaphragm 28. Substrate 24 contains aperture 62, in fluid communication with the first lumen, which houses the sensor, aperture 62 preferably having a cross-sectional area equal to that of aperture 60, whereby a selected reference pressure, such as atmospheric
20 pressure, impinges upon surface 29 of diaphragm 28. so as to exert a force opposite to that of the applied pressure. When the reference pressure exerted against surface 29 is equal to or greater than that of the applied pressure, as shown in Fig. 9, surface 25 of diaphragm 28 is restored to
25 zero pressure position and rests flush against stop 56A.

An in vivo calibration reading indicating the offset error contained in the reading on the monitor can be obtained by slowly increasing the amount of back pressure applied to surface 29 of diaphragm 28 via vent 62 and the
30 first lumen until the reading on the monitor ceases to fall and attains a constant low value. This constant low value represents the zero error of the system and should be subtracted from all pressure readings in obtaining a true pressure reading. In addition, the calibration accuracy of
35 the transducer system can be obtained without the need to remove it from its location of operation if a manometer or

other means of applying a known back pressure is used to measure the amount of pressure applied through aperture 62 against surface 29. The difference between the known back pressure and the constant pressure reading on the monitor
5 generated when the diaphragm is restored to its zero position can be used to obtain the calibration error of the system.

Alternatively, the calibration error can be found by applying a known vacuum to surface 29 of diaphragm 25,
10 which technique is equivalent to applying a positive pressure to the opposite side of the diaphragm. The displacement caused by the vacuum will result in a pressure being displayed on the monitor that can be evaluated using known methods against the known negative pressure to
15 determine the calibration error. Once known, the operator can use the zero error and the calibration error to obtain the true pressure reading at any time without withdrawing the catheter from its location of operation.

The ability to calibrate and zero the instrument in
20 situ offers a great advantage for any application requiring uninterrupted monitoring of the variable of interest, such as the pressure of a fluid stream in a chemical plant, and the like. This ability also has important clinical significance for monitoring intracranial pressure because
25 the intracranial pressure catheter can be left in place for up to about five days according to current clinical practice while periodic checks are made to determine the integrity and accuracy of the system.

As shown in Figs. 10 and 11, aperture 62 and the first
30 lumen can also be used to vent the system to the atmospheric pressure to obtain a gauge pressure measurement without contaminating the fluid system because diaphragm 28 serves as a protective barrier between the atmosphere and the fluid system under observation. Atmospheric gauge
35 pressure readings are commonly preferred for monitoring pressure of bodily fluids, such as blood pressure, since

the body is at atmospheric pressure. When the fluid system is the bloodstream or the intracranial cavity, and the like, this safety feature is highly desirable. It is also of great importance when monitoring any fluid stream that might be compromised by contact with the constituents of air.

A less preferred type of fiber optic pressure sensor adapted for use in the present invention is described in European patent 0127476, which is hereby incorporated by reference in its entirety, and is schematically illustrated in Figure 12. The apparatus includes catheter housing 111 comprised of a first lumen 116 having a first set of optical fibers and a second fluid transport lumen 129. The first set of fibers includes emitter fiber 115 and return fiber 117 for transmitting a first light beam to and from the remote end of the catheter. In this type of pressure transducer, the removable reflective surface is mounted on bellows 119 located at the distal end of the catheter. Reflective surface 121 moves in accordance with pressure and thereby modulates the intensity of the first light beam, not by microshifts in the operating segment of the reflectivity curve of an optically resonant structure, but by scattering of the source light beam caused by movement of the reflective bellows, as is described in detail in European patent application 0127476. This type of optical sensor can be used with monochromatic light or with the multiwavelength light produced by LED 123 and transmitted by the first set of optical fibers to a first photodetector means 125, for detecting the modulated intensity of the reflected beam caused by movement of bellows 119. Since bending of the catheter 111 effects the light transmittance of both the emitter fiber 115 and return fiber 117, the pressure monitoring apparatus optionally includes a reference channel comprised of a second set of optical fibers located within first lumen 116 and extending substantially along its entire length. This reference

channel is used to determine the effects of bending on transmittance and to determine the effects of temperature and aging on the efficiency of LED 123 and photodetector 125. Since the first and second set of optical fibers are substantially coextensive and experience substantially the same degree of bending within catheter 111, the effect of that bending on their respective transmittances is presumed to be substantially equivalent. A second light beam produced by LED 123 is transmitted by the second set of optical fibers so that variation in transmittance of the fibers and variations in light from the LED can be determined and a corresponding correction made to the intensity signal. The second set of optical fibers includes an emitter fiber 137 for transmitting the second light beam from LED 123 to a location near the distal end of catheter 111 and a return fiber 139 for transmitting the light beam back from that location. A second photodetector means 141 for detecting the intensity of this reflected light beam, and for producing a correction signal on line 143 having an electrical current whose magnitude is proportional to intensity. Preferably the correction signal is sent to control means 145 for generating a feedback control signal to be sent to light source 123 via power box 145 to compensate for any variation in light intensity caused by transmission losses such as those resulting from bending of the optical fibers and thereby to correct the measurement signal issuing from photodetector 125 at output terminal 146.

To standardize the intensity of the reflectivity of the reference sensor, a translucent droplet 145 of an epoxy containing a white pigment bonds together the remote ends of the second set of fibers and thereby reflects a predetermined fixed proportion of a light beam from the emitter fiber to the return fiber. The epoxy droplet is preferably coated with an opaque silver paint, the opacity preventing movement of adjacent reflective bellows 119 from

effecting the reflected beam and the silver color maximizing the intensity of the reflected beam.

The above described photodetector assembly can be fashioned by one skilled in the art from commercially available elements. A type of photodetector apparatus
5 suitable for use in this invention is Model manufactured by Camino Laboratories, which interfaces with standard patient monitors.

This type of intensity modulation sensor requires that
10 the first lumen be large enough to enclose at least two optical fibers, and four optical fibers are required if the reference channel is used. Therefore, the catheter housing is larger than that required for the spectral modulation sensor, which preferably uses a single optical fiber. For
15 this reason intensity modulation sensors are for favored for use in intracranial pressure monitoring catheters.

From the foregoing various further applications, modifications, and adaptations of the invention within the scope of the claims appended hereto will be apparent to
20 those skilled in the art to which it pertains. All embodiments, examples and alternatives, and the like, set forth herein are strictly intended as non-limiting examples.

WE CLAIM:

1. An integral pressure sensor and fluid transport catheter apparatus for simultaneously measuring fluid pressure while injecting or withdrawing fluids comprising:
 - 5 a catheter housing comprising a first lumen containing at least one sensor means for sensing pressure of fluids at the distal end of the catheter and means for transmitting to the proximal end thereof a pressure measurement signal received from the means for sensing
 - 10 pressure; and a second lumen in fluid communication with the exterior of the catheter housing for transporting a fluid between the distal and proximal ends thereof.
2. The apparatus of claim 1 wherein the sensor means comprises a fluid column means having a pressure transducer
- 15 located at the proximal end of the catheter.
3. The apparatus of claim 1 wherein the sensor means comprises an electrical strain gauge sensor located at the distal end of the catheter and a electrical pressure transducer located at the proximal end of the catheter in
- 20 electrical communication with the sensor.
4. The apparatus of claim 1 wherein the sensor means is for measurably modulating a physical parameter of light reflected therefrom in accordance with the magnitude of the fluid pressure, said sensor means comprising a
- 25 light-reflective diaphragm located at the distal end of the catheter, said diaphragm being movable in accordance with the pressure of the fluid and wherein a first optical fiber means is for directing an input light beam from the light source at the diaphragm and for receiving a reflected light
- 30 beam therefrom, said apparatus further comprising:
 - a source of an input light beam,
 - photodetector means for producing a measurement signal indicative of the magnitude of the pressure measured in accordance with the modulation of the physical
 - 35 parameter,

transmission means for conveying the reflected light beam from said first optical fiber means to said photodetector means, and

5 a monitor means for displaying the pressure measurement signal.

5. The apparatus of claim 4 wherein an excitation voltage from the monitor means is scaled by the photodetector means to produce the measurement signal input to the monitor means.

10 6. The apparatus of claim 4 wherein the physical parameter is the intensity of a light beam reflected from the diaphragm, and wherein the apparatus further comprises correction means for adjusting the measurement signal to correct for inaccuracies caused by transmission losses in
15 the first optical fiber means.

7. The apparatus of claim 6 wherein the first optical fiber means includes an emitter fiber for directing the input light beam at the light-reflective diaphragm of the sensor means and a return fiber for receiving the reflected
20 light beam from the diaphragm, the proportion of the input light beam that is reflected by the diaphragm and received by the return fiber varying in accordance with movement of the diaphragm.

8. The apparatus of claim 6 wherein the correction
25 means comprises:

a second optical fiber means including a correction emitter fiber for transmitting a reference light beam to a reflector means and a correction return fiber for returning the reflected light beam from the reflector means to a
30 remote location, wherein the reflector means is located at the distal end of the correction and emitter fibers for directing a predetermined proportion of the light supplied by the correction emitter fiber to the correction return fiber; and

35 means for measuring transmission losses in the reference light beam transmitted by the return fiber of the

second optical fiber means and for adjusting the intensity of the input light beam accordingly.

9. The apparatus of claim 7 or 8 wherein an excitation voltage from the monitor means is scaled by the photodetector means to produce the measurement signal input to the monitor means.

10. The apparatus of claim 4 wherein the physical parameter is the spectral characteristics of light, the input light beam contains at least two wavelengths of light, and the first optical fiber means contains only one optical fiber.

11. The apparatus of claim 10 wherein the sensor means is a spectral modulation sensor comprising a body defining a cavity having a pair of opposed reflective surfaces with a distance between and forming an optically resonant structure with the distance between said surfaces changing as a function of sensed pressure over a range of pressure values so as to alter the spectral characteristics of the reflected light beam, and wherein one of the surfaces comprises a light-reflective pressure sensitive diaphragm and the said change in distance is caused by movement of the diaphragm in response to sensed pressure.

12. The apparatus of claim 11 wherein the sensor is located at the distal end of the catheter housing.

13. The apparatus of claim 12 wherein the sensor has a reflectivity curve and a transmission curve with at least one operating segment on at least one of said reflectivity curve and said transmission curve, the change in the distance between the reflective surfaces inducing a corresponding microshift greater than one half of a resonance cycle over the said range of values in the said operating segment.

14. The apparatus of claim 13 wherein at least one of said operating segments is less than about one resonance cycle in length for said range of values of the sensed pressure and the operating segment is correspondingly

microshifted less than about one resonance cycle over the said range,

and wherein the wavelengths of the source light beam are selected to fall at least substantially within the operating segment over the said range of values so that over the said range the reflected light is spectrally modulated so as to bear a unique one-to-one relationship to the sensed pressure, and

further wherein the photodetector means is for deriving two electrical signals corresponding to any two different wavelength portions of said spectrally modulated light, and for taking the ratio of the two said signals to provide an output measuring signal which is a function of the sensed pressure.

15 15. The apparatus of claim 12, 13, or 14 wherein an excitation voltage from the monitor means is scaled by the photodetector means to produce the measurement signal input to the monitor means.

16. The apparatus of claim 15 wherein the photodetector means automatically adjusts the microshift in the said operating segment to correct for variations in the output signal caused by changes in temperature of the apparatus.

17. The apparatus of claim 15 wherein the source of the input light beam is a light emitting diode, a change in the temperature of the diode causing a microshift in the said operating segment, and further wherein the photodetector means comprises a filter, said filter being selected such that a change in the temperature of the filter causes an automatic adjustment in the microshift of said operating segment such that the temperature change caused by the filter corrects for the temperature change caused by the diode.

18. The apparatus of claim 13 wherein the catheter assembly comprises at least two said spectral modulation sensors, the first sensor being located at the distal tip

of the catheter housing and the second sensor being located elsewhere and being subjected to a reference pressure,

and wherein the light source emits light of at least two wavelengths and the photodetector means is a photodetector assembly means comprising a beamsplitter means for splitting the source light beam into two beams containing at least two wavelengths of light, a first split beam being sent to the first sensor and being reflected therefrom to a first photodetector means for integrating the reflected first split beam over two non-identical wavelength bands to produce two integrated first sensor signals and for taking the ratio of the two said first sensor signals to produce a first normalized signal, and a second split beam being sent to the second sensor, and being reflected therefrom to a second photodetector means for integrating the reflected second split beam over two non-identical wavelength bands to produce two integrated second sensor signals and for taking the ratio of the two said second sensor signals to produce a second normalized signal,

and further wherein the photodetector assembly means is for subtracting the first normalized signal from the second normalized signal to produce the pressure measurement signal.

19. The apparatus of claim 14 wherein the cavity in the sensor means has a vent for providing fluid communication with the first lumen and the first lumen is in fluid communication with a reference pressure.

20. An optical pressure sensing catheter assembly for measuring pressure in a fluid comprising:

a source of an input light beam of at least two wavelengths;

a catheter housing containing therein:

a) a single optical fiber means for transmitting the input light beam from the light source to a spectral modulation sensor means located at the distal end of the

catheter housing and for transmitting a reflected light beam therefrom, and

b) a spectral modulation sensor means located at the distal end of the catheter and in optical communication
5 with the optical fiber means for measurably modulating in accordance with the magnitude of the pressure of a fluid in contact therewith at least one spectral characteristic of light received from the optical fiber means and reflected thereunto, wherein the sensor means comprises a body
10 defining a cavity having a pair of opposed reflective surfaces with a distance between and forming an optically resonant structure with the distance between said surfaces changing as a function of sensed pressure so as to alter the spectral characteristics of the reflected light beam,
15 and wherein one of the surfaces comprises the light-reflective pressure sensitive diaphragm and the said change in distance is caused by movement of the diaphragm in response to the sensed pressure;

c) photodetector means in optical communication
20 with the fiber optic means for receiving the reflected light beam and for producing therefrom an output pressure measurement signal as a linear function of the magnitude of pressure while automatically correcting the output signal therefrom for changes caused by variations in temperature
25 and in intensity of the light beam; and

d) a monitor means for displaying the output pressure measurement signal.

21. The apparatus of claim 20 wherein the optical sensor has a reflectivity curve and a transmission curve
30 with at least one operating segment on at least one of said reflectivity curve and said selectivity curve, the change in the distance between the reflective surfaces inducing a corresponding microshift greater than one half of a resonance cycle over the said range of values in the said
35 operating segment.

22. The apparatus of claim 21 wherein at least one of said operating segments is less than about one resonance cycle in length for said range of values of the sensed pressure and the operating segment is correspondingly
5 microshifted less than about one resonance cycle over the said range,

and wherein the wavelengths of the source light beam are selected to fall at least substantially within the operating segment over the said range of values so that
10 over the said range the spectrally modified light bears a unique one-to-one relationship to the sensed pressure, and

further wherein the photodetector means is for deriving two electrical signals corresponding to any two different wavelength portions of said spectrally modulated
15 output beam, and for taking the ratio of the two said signals to provide an output measuring signal which is a function of the sensed pressure.

23. The catheter assembly of claim 20, 21 or 22 wherein the catheter is for monitoring intracranial pressure and
20 wherein the monitor supplies electrical power to drive the assembly and wherein the photodetector means scales the excitation voltage provided by the monitor to produce the output pressure measurement signal to the monitor.

24. The apparatus of claim 23 wherein the photodetector
25 means automatically adjusts the microshift in the said operating segment to correct for variations in the output signal caused by changes in temperature of the apparatus.

25. The apparatus of claim 24 wherein the light source contains a light emitting diode for providing the input
30 light beam, a change in the temperature of the diode causing a microshift in the said operating segment, and further wherein the photodetector means comprises a filter, said filter being selected such that a change in the temperature of the filter causes an automatic adjustment in
35 the microshift of said operating segment such that the

temperature change caused by the filter corrects for the temperature change caused by the diode.

26. The apparatus of claim 25 wherein the photodetector means automatically corrects for variations in the measurement signal caused by variations in intensity of the source light beam and by transmission losses in the source light beam.

27. The apparatus of claim 26 wherein the catheter assembly comprises at least two said spectral modulation sensors, the first sensor being located at the distal tip of the catheter housing and the second sensor being located elsewhere and being subjected to a reference pressure,

and wherein the light source emits an input light beam of at least two wavelengths and the photodetector means comprises a photodetector assembly means comprising a beamsplitter means for splitting the source light beam into two beams containing at least two wavelengths of light, a first split beam being sent to the first sensor and being reflected therefrom to a first photodetector means for integrating the reflected first split beam over two non-identical wavelength bands to produce two integrated first sensor signals and for taking the ratio of the two said first sensor signals to produce a first normalized signal, and a second split beam being sent to the second sensor, and being reflected therefrom to a second photodetector means for integrating the reflected second split beam over two non-identical wavelength bands to produce two integrated second sensor signals and for taking the ratio of the two said second sensor signals to produce a second normalized signal,

and further wherein the photodetector assembly means is for subtracting the first normalized signal from the second normalized signal to produce the pressure measurement signal.

28. The apparatus of claim 27 wherein the cavity in the sensor means has a vent for providing fluid communication

with the first lumen and the first lumen is in fluid communication with a atmospheric pressure.

1/7

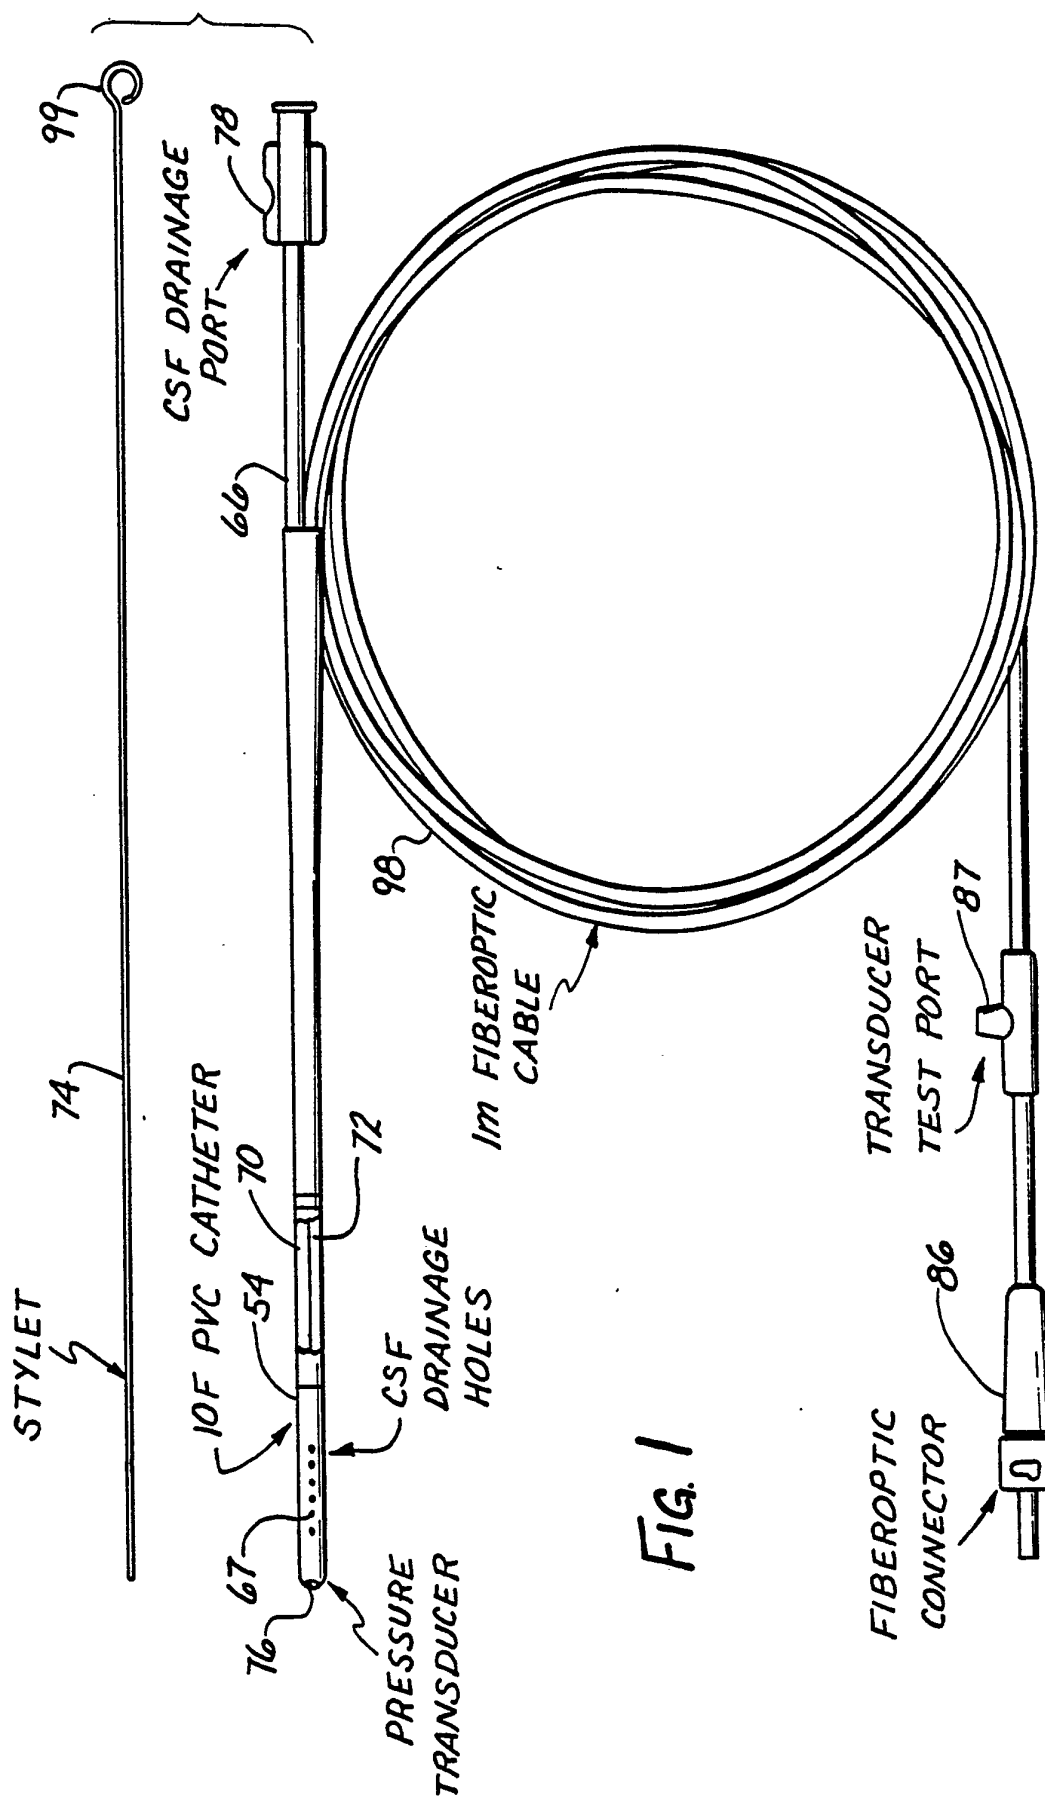


FIG. 1

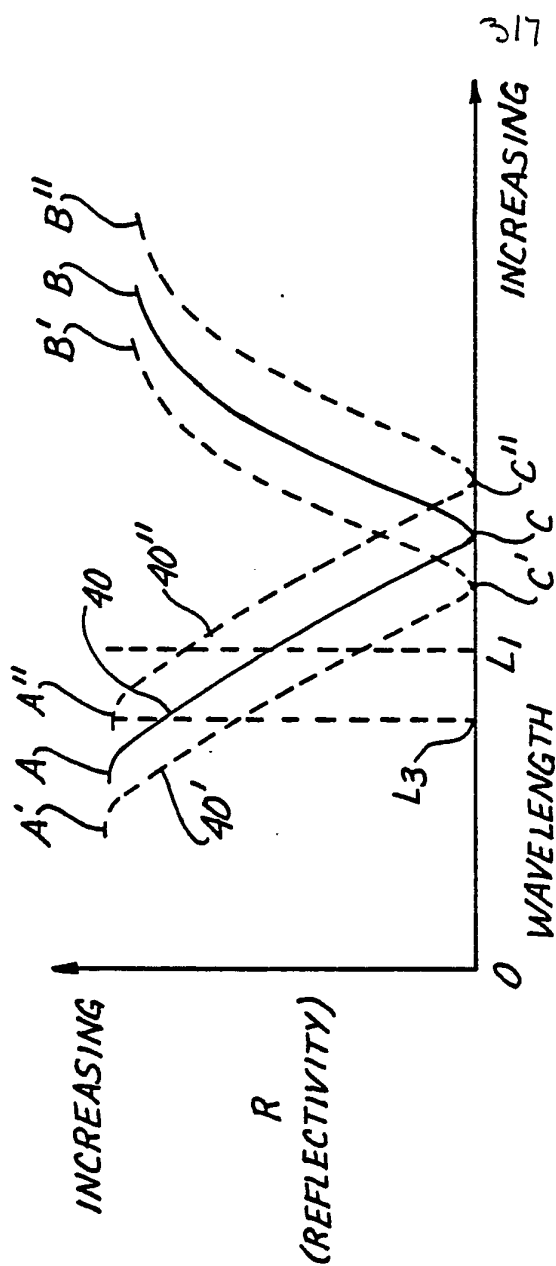


FIG. 6

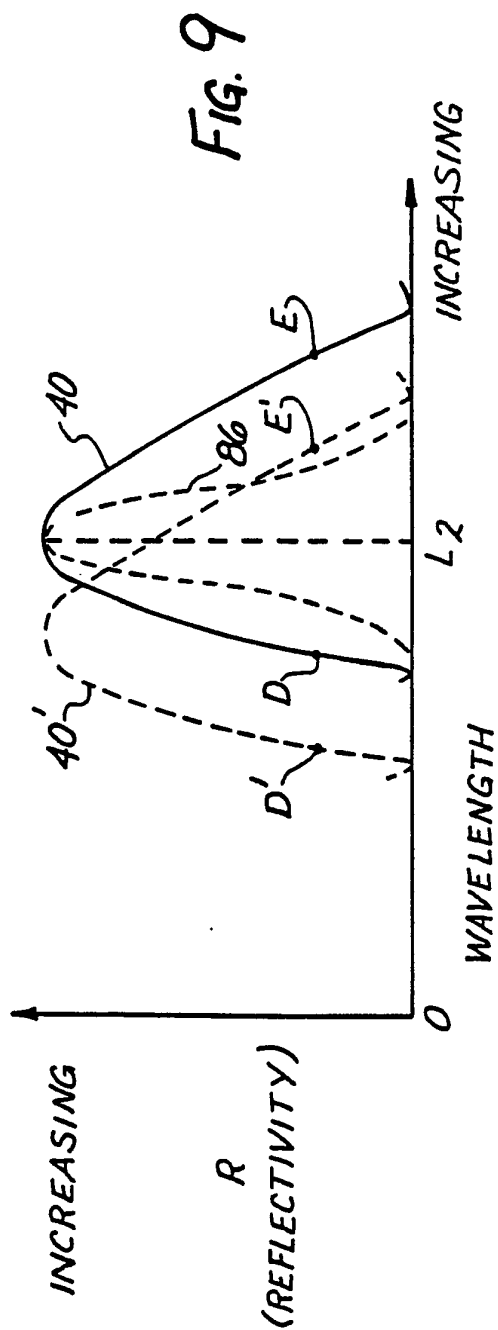
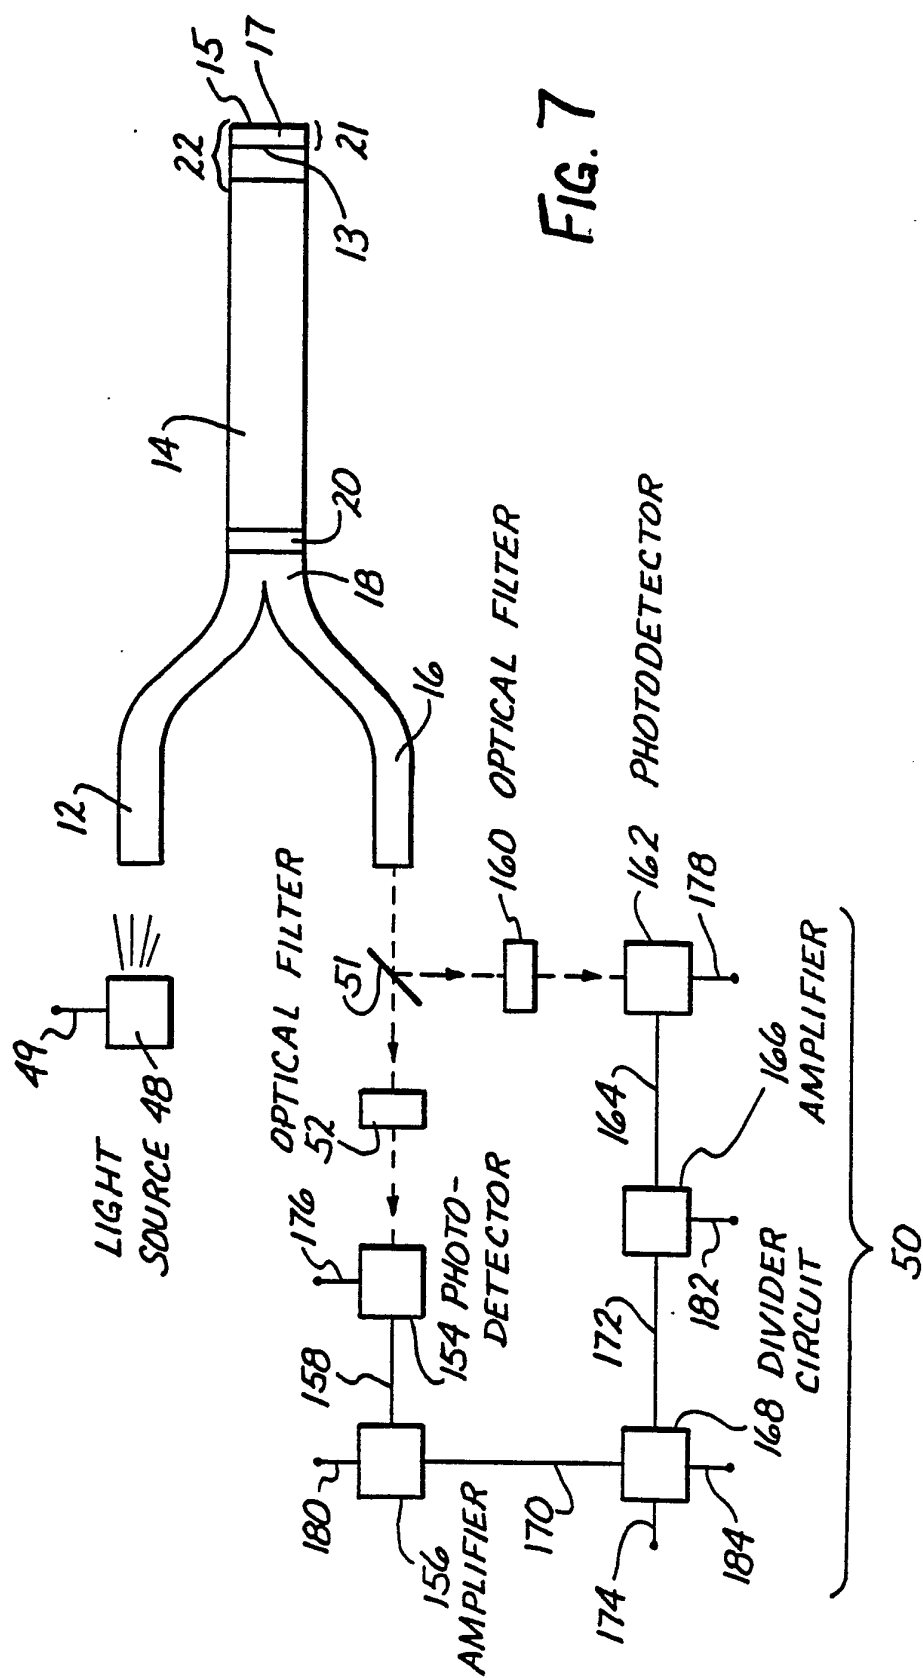


FIG. 9



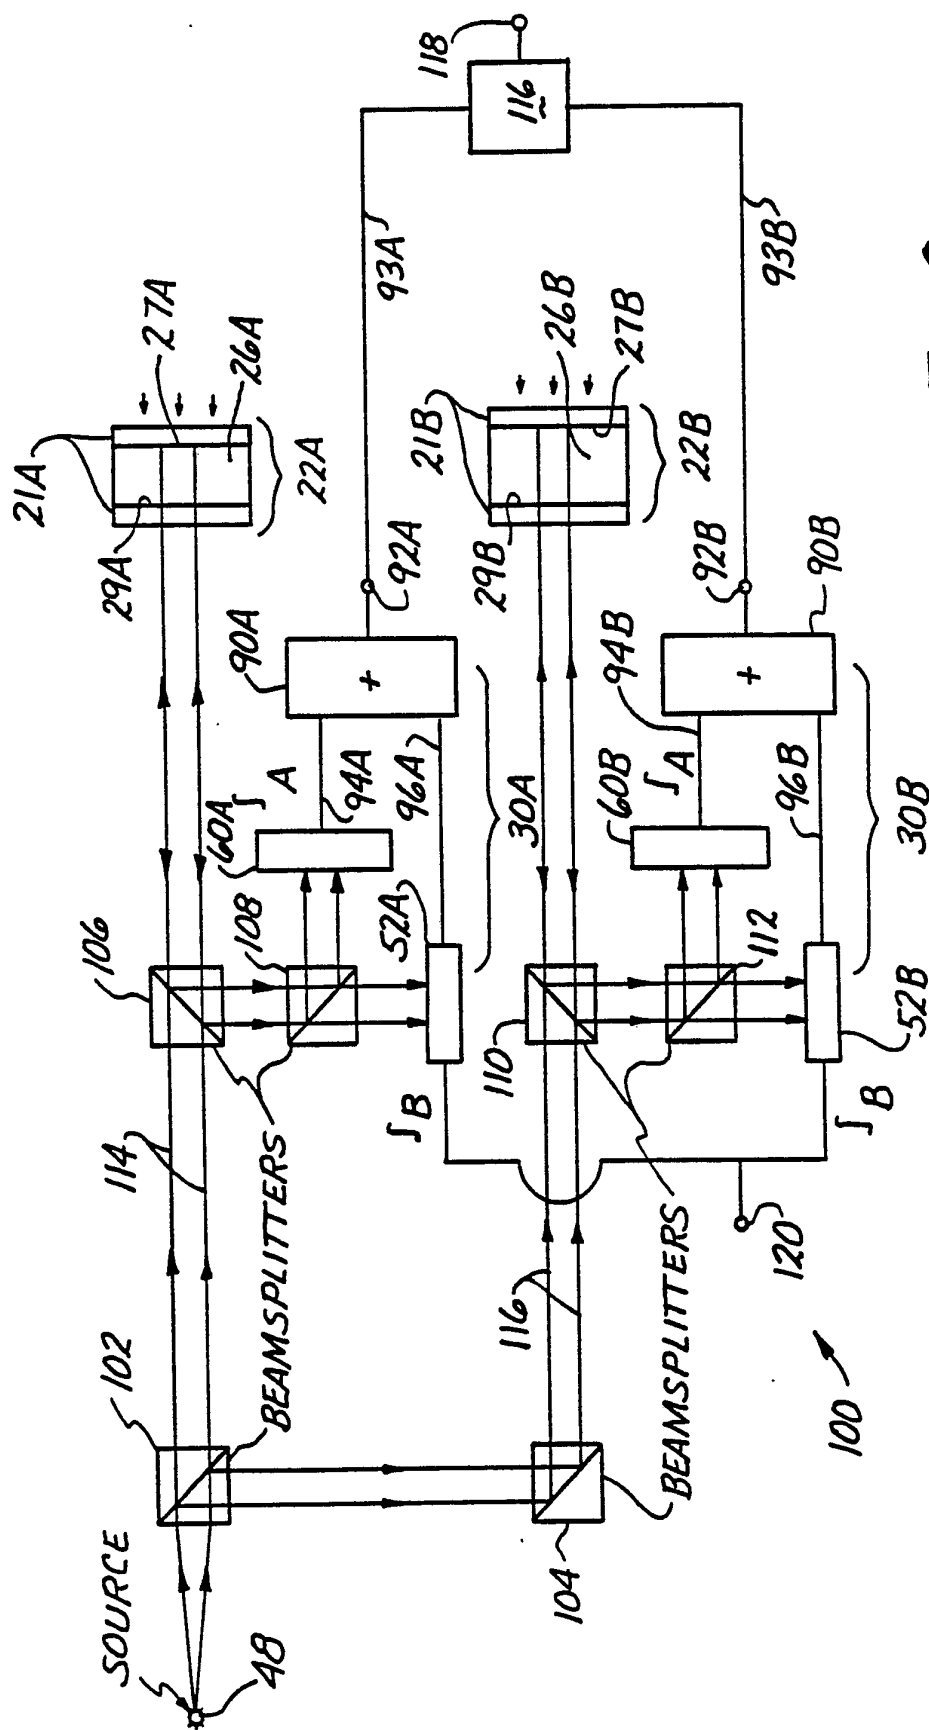


FIG. 8

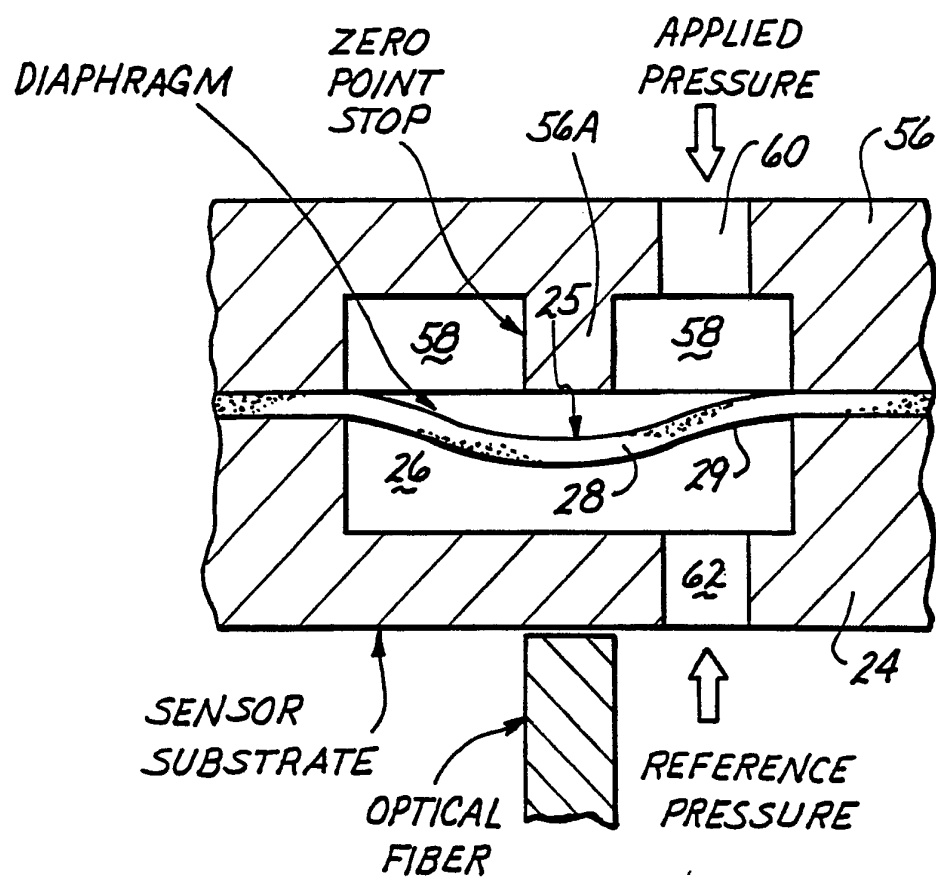
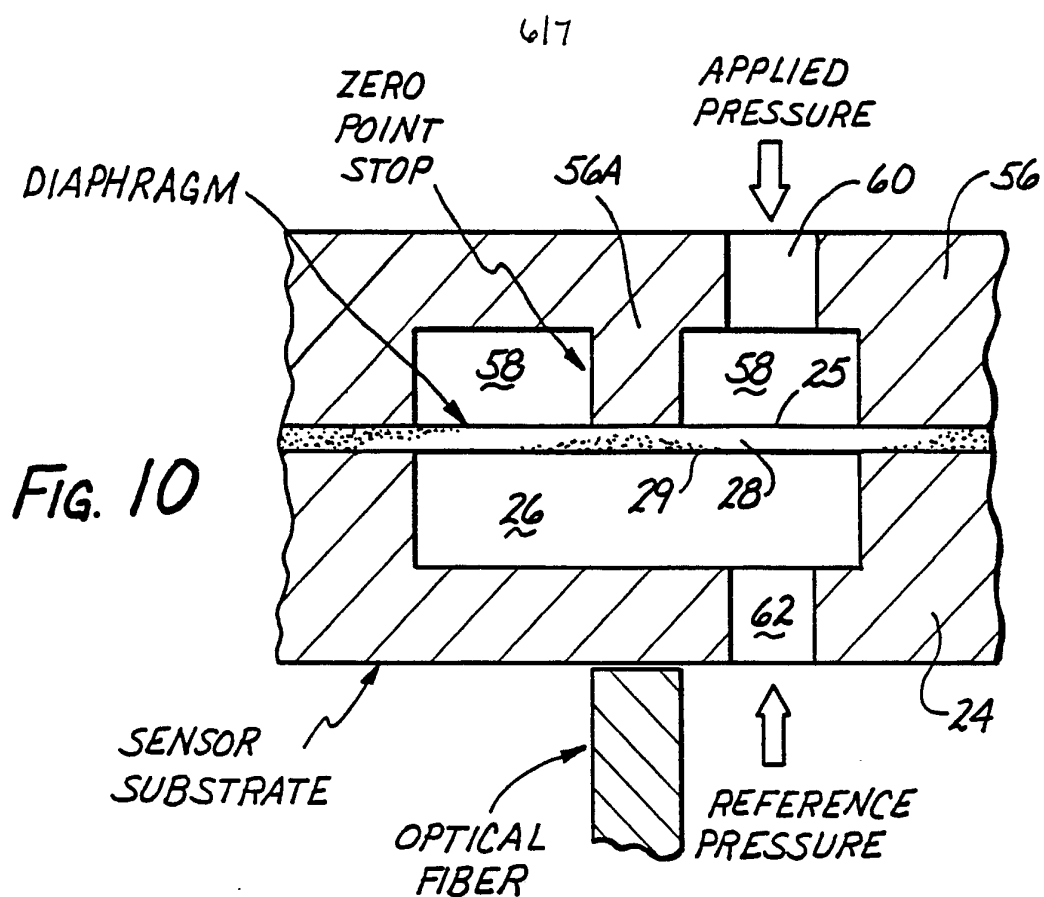


FIG. 11

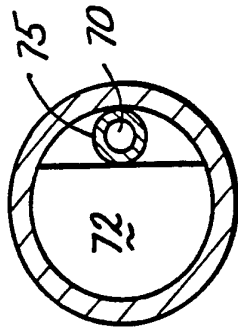
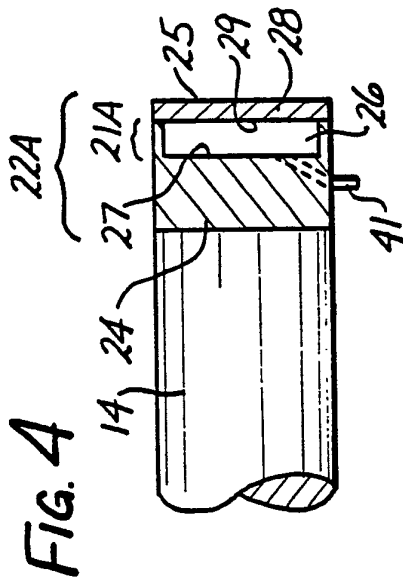


FIG. 2

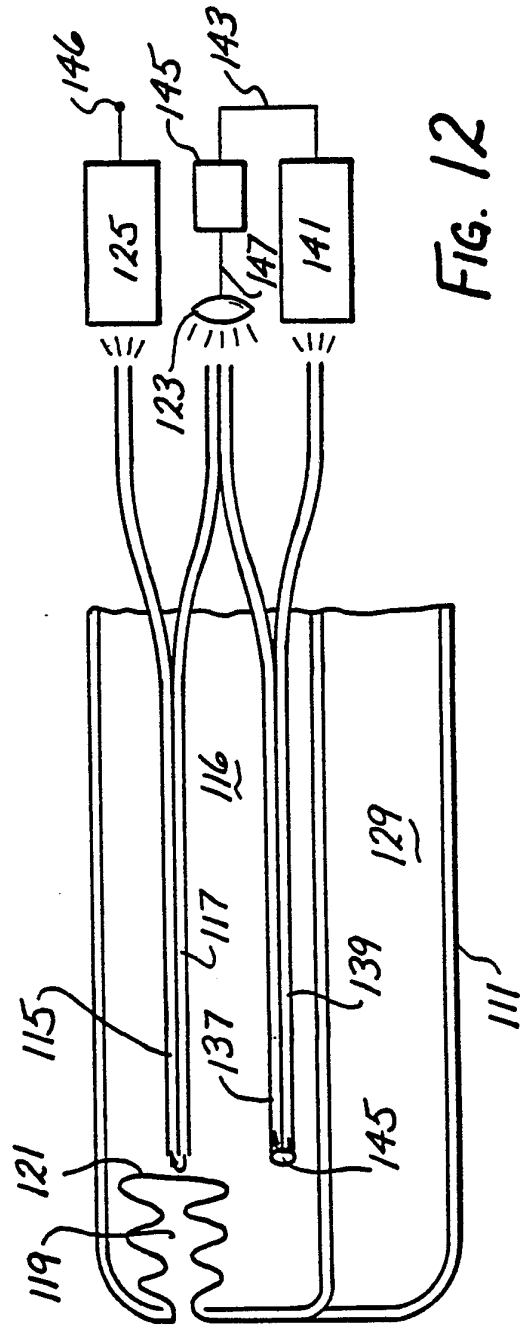


FIG. 12

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 90/05804

I. CLASSIFICATION OF SUBJECT MATTER (if several classification symbols apply, indicate all) ⁶		
According to International Patent Classification (IPC) or to both National Classification and IPC Int.Cl. 5 A61M1/00 ; A61B5/0215 ; G01L9/00		
II. FIELDS SEARCHED		
Minimum Documentation Searched ⁷		
Classification System	Classification Symbols	
Int.Cl. 5	A61M ; A61B	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched ⁸		
III. DOCUMENTS CONSIDERED TO BE RELEVANT ⁹		
Category ¹⁰	Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²	Relevant to Claim No. ¹³
X	EP,A,251512 (THE REGENTS OF THE UNIVERSITY OF CALIFORNIA) 07 January 1988 see abstract see column 5, lines 7 - 18 see column 8, line 30 - page 9, line 6; figures 1-4	1
Y	---	2, 4, 12, 20
X	GB,A,2205244 (BLAGOVESCHENSKY GOSUDARSTVENNY MEDITSINKY INSTITUT) 07 December 1988 see abstract see page 7, lines 8 - 28; figures 1, 2	1
X	FR,A,2378494 (RICHARD WOLF GMBH) 25 August 1978 see page 3, lines 7 - 26 see page 4, lines 1 - 11; figure 2	1

	-/--	
¹⁰ Special categories of cited documents : "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier document but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art. "&" document member of the same patent family		
IV. CERTIFICATION		
Date of the Actual Completion of the International Search	Date of Mailing of this International Search Report	
31 JANUARY 1991	18. 02. 91	
International Searching Authority	Signature of Authorized Officer	
EUROPEAN PATENT OFFICE	miss T. MORTENSEN 	

III. DOCUMENTS CONSIDERED TO BE RELEVANT (CONTINUED FROM THE SECOND SHEET)		
Category °	Citation of Document, with indication, where appropriate, of the relevant passages	Relevant to Claim No.
Y	US,A,2603210 (MILLET) 15 July 1952 see column 1, lines 1 - 18; figures 1, 2, 8 ---	2
Y	WO,A,8503855 (OPTICAL TECHNOLOGIES INC.) 12 September 1985 see abstract see page 16, lines 15 - 21 see page 21, line 6 - page 22, line 4; figures 6, 23 ---	4, 12, 20
A	US,A,4678904 (SAASKI ET AL.) 07 July 1987 see abstract; figure 1 (cited in the application) ---	4, 20
A	DE,A,3127882 (MORINGLANE) 03 February 1983 see abstract; figures 1-3 ---	1, 23

**ANNEX TO THE INTERNATIONAL SEARCH REPORT
ON INTERNATIONAL PATENT APPLICATION NO.**

US9005804

SA 41992

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

13/02/91

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A-251512	07-01-88	AU-A- 7386287	10-12-87
		JP-A- 63040541	20-02-88
		US-A- 4902276	20-02-90
GB-A-2205244	07-12-88	DE-A- 3720553	05-01-89
		FR-A- 2616332	16-12-88
		SE-A- 8702418	11-12-88
		US-A- 4893634	16-01-90
FR-A-2378494	25-08-78	DE-A, B, C 2703274	03-08-78
US-A-2603210		None	
WO-A-8503855	12-09-85	AU-A- 4064085	24-09-85
		US-A- 4873989	17-10-89
US-A-4678904	07-07-87	CA-A, C 1246354	13-12-88
		EP-A- 0172623	26-02-86
		JP-A- 61035334	19-02-86
		US-A- 4945230	31-07-90
		US-A- 4778987	18-10-88
DE-A-3127882	03-02-83	None	