



US00D717459S

(12) **United States Design Patent**
Lin et al.

(10) **Patent No.:** **US D717,459 S**

(45) **Date of Patent:** **** Nov. 11, 2014**

- (54) **DIAGNOSTIC DEVICE**
- (71) Applicant: **Edan Diagnostics**, San Diego, CA (US)
- (72) Inventors: **Chao Lin**, San Diego, CA (US); **Paul David Swanson**, Santee, CA (US); **Zhixiang Jason Zhao**, Plainsboro, NJ (US)
- (73) Assignee: **Edan Diagnostics**, San Diego, CA (US)

D694,422 S *	11/2013	Cook et al.	D24/216
D705,943 S	5/2014	Chang et al.		
8,741,234 B2	6/2014	Wang et al.		
8,741,235 B2	6/2014	Janisch et al.		
2007/0172388 A1	7/2007	Padmanabhan et al.		
2009/0065368 A1	3/2009	Davis et al.		
2010/0273248 A1*	10/2010	Ha et al.	435/287.3
2010/0328405 A1	12/2010	Ness et al.		
2011/0086378 A1	4/2011	Shany et al.		
2011/0198241 A1	8/2011	Murakami		
2011/0229373 A1	9/2011	Asakura		
2011/0287447 A1	11/2011	Norderhaug et al.		

(Continued)

(**) Term: **14 Years**

OTHER PUBLICATIONS

(21) Appl. No.: **29/437,044**

U.S. Appl. No. 29/437,042, filed Nov. 12, 2012, Lin et al.

(22) Filed: **Nov. 12, 2012**

(Continued)

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/216, 107, 169, 186, 232; D10/81;
422/62, 68.1, 69, 70, 72, 500;
435/287.1; 436/43, 45, 47; 204/403.1
See application file for complete search history.

Primary Examiner — Anhdao Doan
(74) *Attorney, Agent, or Firm* — Foley & Lardner LLP;
Gilberto M. Villacorta; Karl F. Reichenberger

(57) **CLAIM**
We claim the ornamental design for a diagnostic device, as shown and described.

(56) **References Cited**


DESCRIPTION

U.S. PATENT DOCUMENTS

D288,478 S *	2/1987	Carlson et al.	D24/216
5,042,691 A	8/1991	Maldonado		
D336,514 S	6/1993	Valerio et al.		
D390,661 S *	2/1998	Foggia	D24/169
D445,509 S	7/2001	Berndt et al.		
D447,569 S *	9/2001	Baily et al.	D24/186
D489,816 S *	5/2004	Ross	D24/107
D597,216 S *	7/2009	McGuigan et al.	D24/216
D634,442 S	3/2011	Tajima et al.		
D638,545 S *	5/2011	Okawa et al.	D24/186
D647,209 S *	10/2011	Muller et al.	D24/216
D657,067 S	4/2012	Shibata		
D675,335 S *	1/2013	Feuerabend et al.	D24/216
D681,231 S *	4/2013	Steinhauer et al.	D24/232

FIG. 1 is a top, front, right perspective view of an embodiment of the claimed design;
FIG. 2 is a top, front, left perspective view thereof;
FIG. 3 is a front elevation view thereof;
FIG. 4 is a rear elevation view thereof;
FIG. 5 is a right elevation view thereof;
FIG. 6 is a left elevation view thereof;
FIG. 7 is a top plan view thereof; and,
FIG. 8 is a bottom plan view thereof.
The broken lines in the drawings are for purposes of illustrating unclaimed portions of the diagnostic device and form no part of the claimed design.

1 Claim, 8 Drawing Sheets

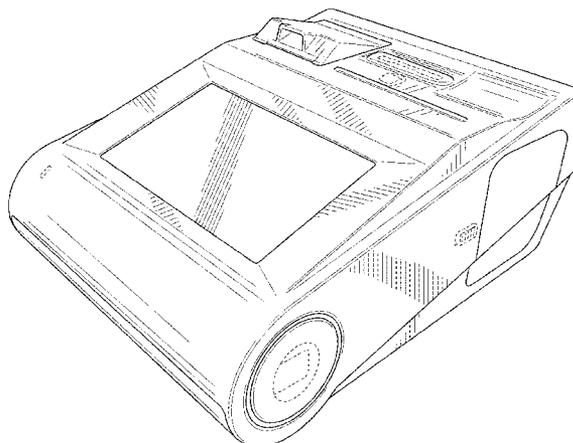

(56)

References Cited

U.S. PATENT DOCUMENTS

2012/0179101	A1	7/2012	Briones et al.
2012/0193376	A1	8/2012	Evans et al.
2012/0218740	A1	8/2012	Estes et al.
2013/0140177	A1	6/2013	Lin et al.
2013/0140179	A1	6/2013	Lin et al.
2013/0142709	A1	6/2013	Lin et al.

OTHER PUBLICATIONS

U.S. Appl. No. 29/437,043, filed Nov. 12, 2012, Lin et al.
Search Report and Written Opinion for Int'l Appln No. PCT/
US2012/068299, mailed Apr. 1, 2013.

US Office Action on 104218-0200 mailed Jun. 5, 2013.
US Office Action on 104218-0300 mailed Jun. 5, 2013.
Non-Final Office Action mailed Jan. 14, 2014, as received in co-
pending Design U.S. Appl. No. 29/437,043.
Notice of Allowance mailed Jan. 17, 2014, as received in co-pending
Design U.S. Appl. No. 29/437,042.
Notice of Allowance issued in related U.S. Appl. No. 29/437,043,
dated Jul. 2, 2014.
International Preliminary Report on Patentability issued in related
International Patent Application No. PCT/US2012/068299, dated
Jun. 10, 2014.

* cited by examiner

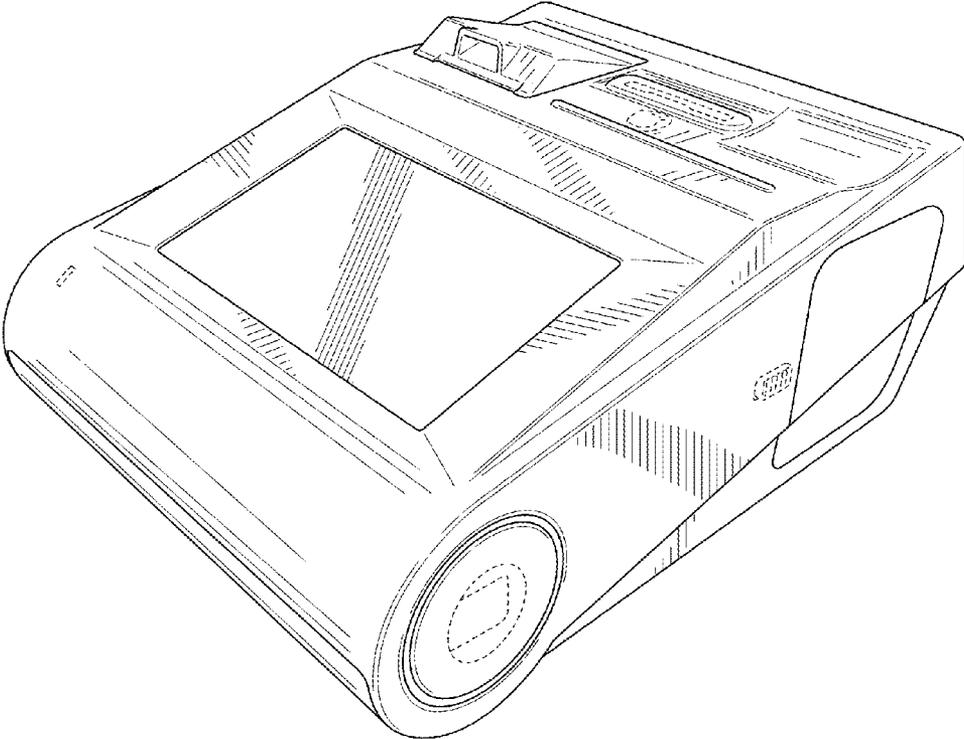


FIG. 1

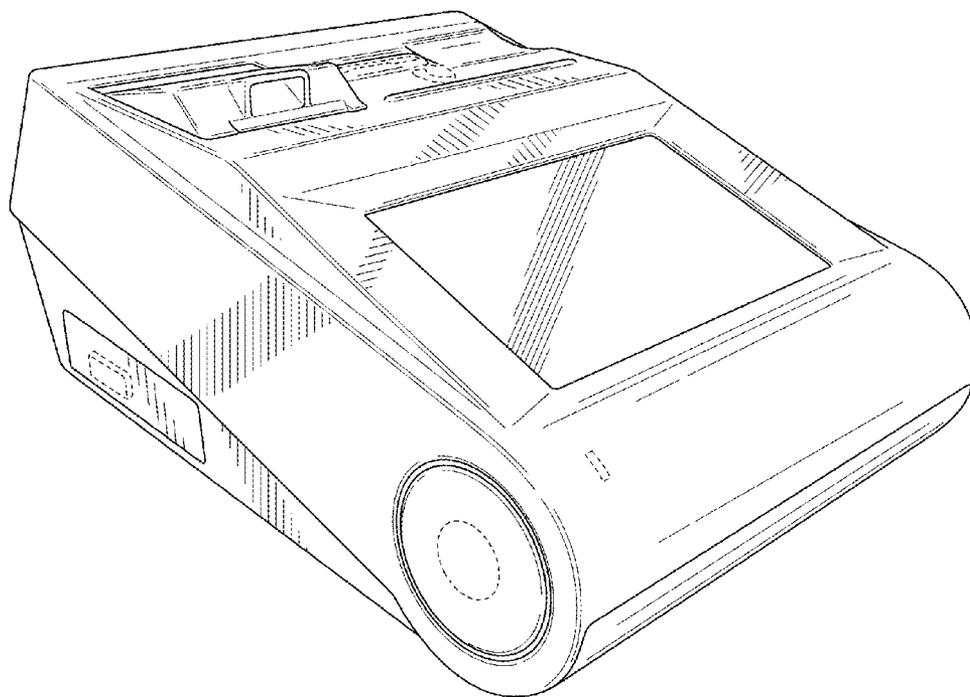


FIG. 2

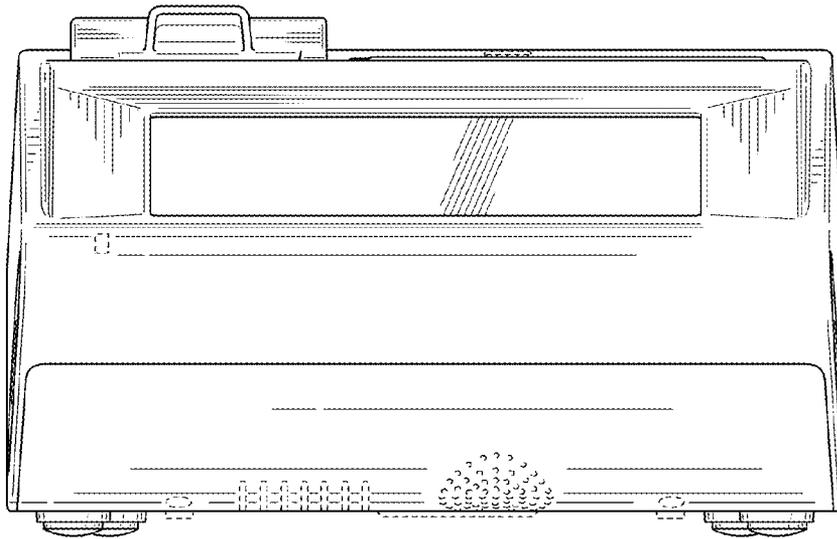


FIG. 3

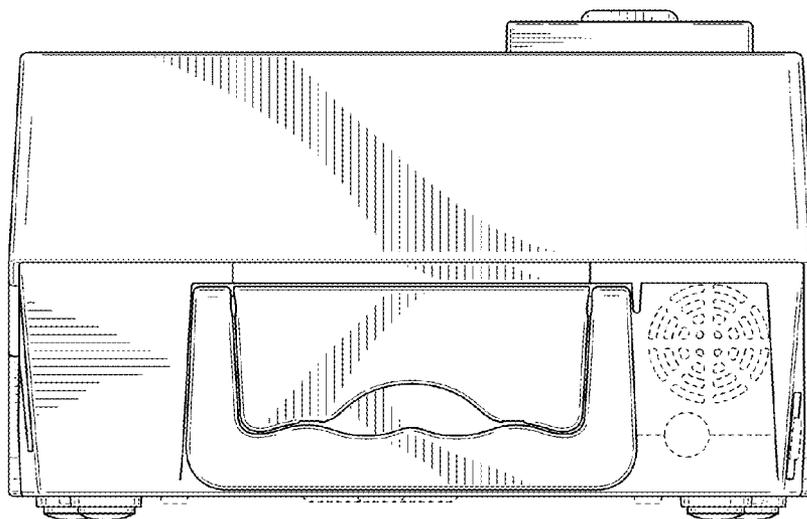


FIG. 4

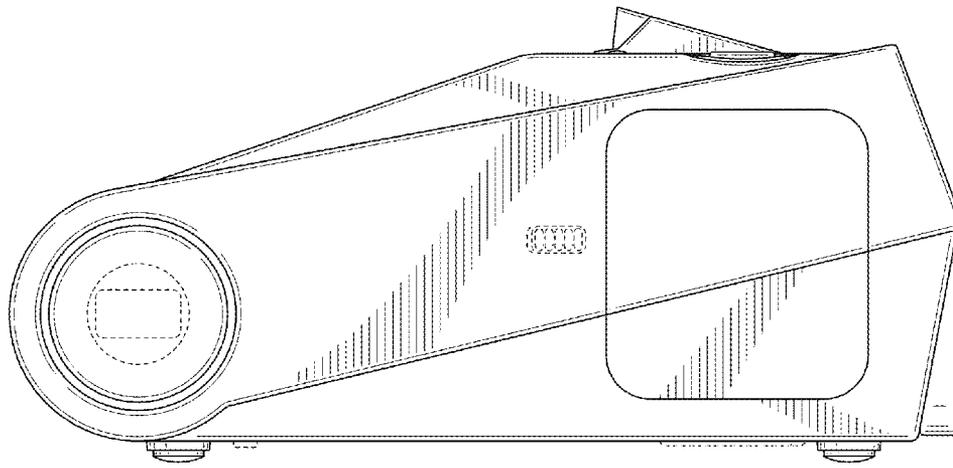


FIG. 5

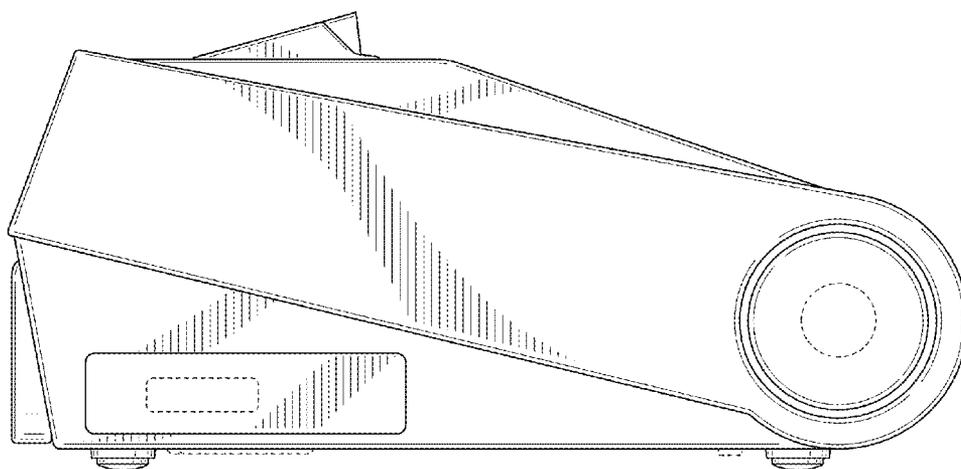


FIG. 6

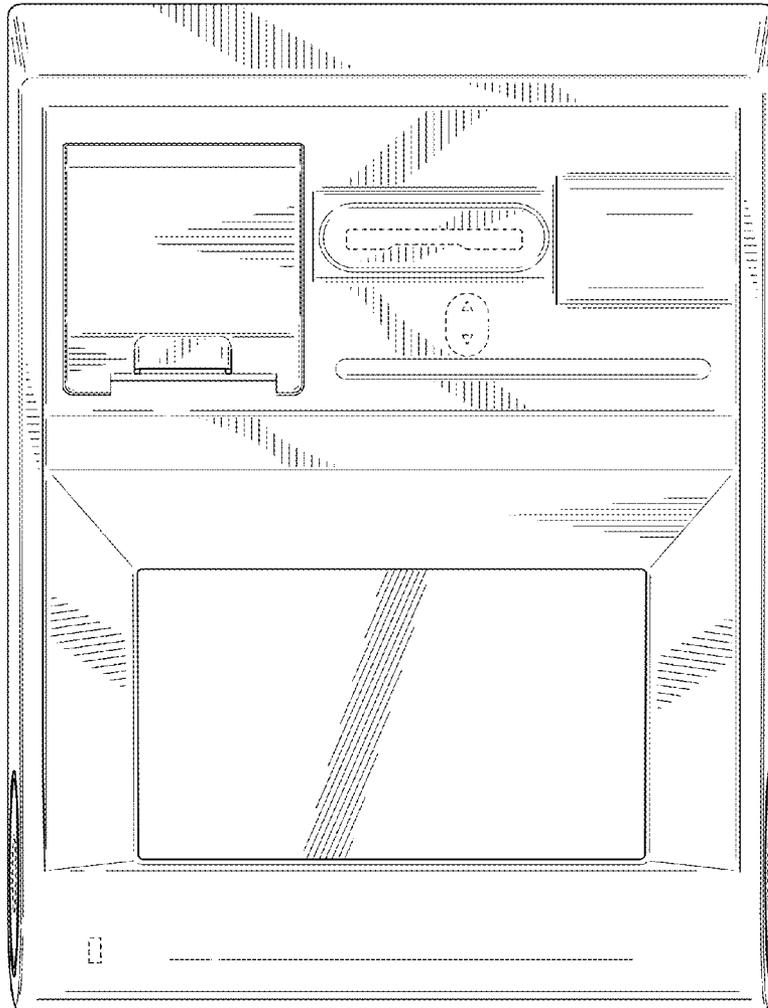


FIG. 7

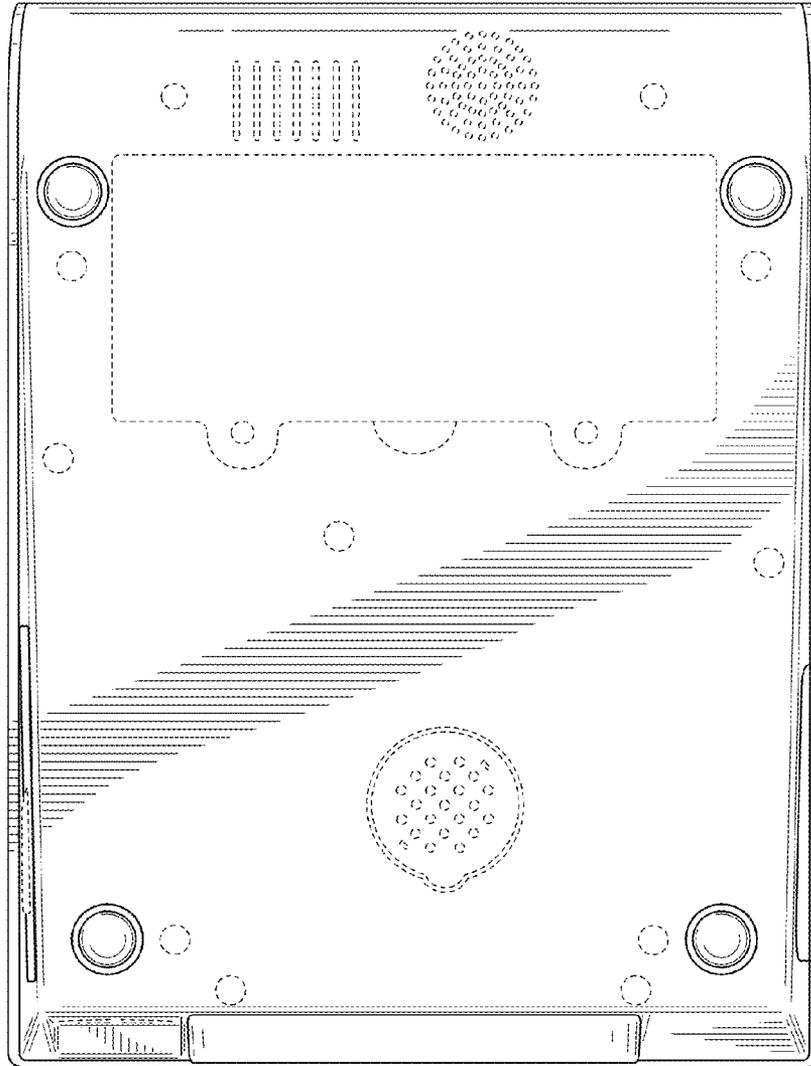


FIG. 8