

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
26 October 2006 (26.10.2006)

PCT

(10) International Publication Number
WO 2006/113763 A2

(51) International Patent Classification:
A61F 2/06 (2006.01)

(74) Agents: HESLIN, James, M. et al.; TOWNSEND AND TOWNSEND AND CREW LLP, Two Embarcadero Center, 8th Floor, San Francisco, California 94111-3834 (US).

(21) International Application Number:
PCT/US2006/014653

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(22) International Filing Date: 18 April 2006 (18.04.2006)

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/672,735 18 April 2005 (18.04.2005) US
60/758,726 12 January 2006 (12.01.2006) US


(71) Applicant (for all designated States except US):
TRIREME MEDICAL, INC. [US/US]; 7060 Koll Center Parkway, Suite 300, Pleasanton, California 94566 (US).

Published:

— without international search report and to be republished upon receipt of that report

[Continued on next page]

(54) Title: APPARATUS AND METHODS FOR DELIVERING PROSTHESES TO LUMINAL BIFURCATIONS

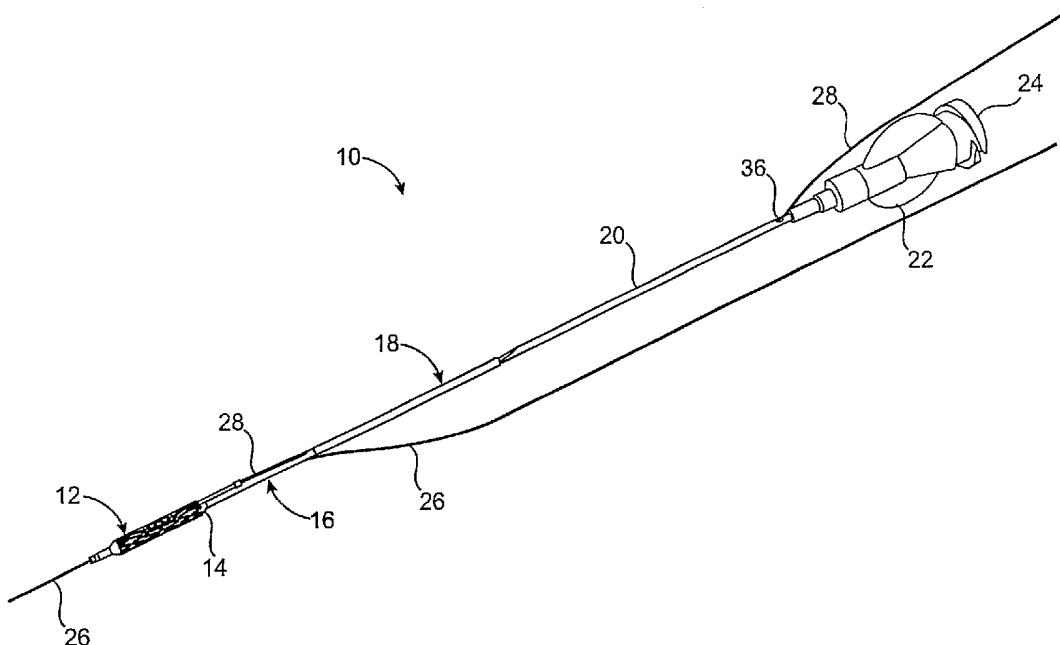

WO 2006/113763 A2

(57) Abstract: A catheter for delivering luminal prostheses comprises a catheter body having an expandable member near a distal end. The prosthesis has a side hole, and a guidewire extends beneath a proximal portion of the prosthesis and over the exterior of the expandable member. A distal end of the guidewire is retracted proximally from the closest point on the side opening to reduce possible interference with catheter advancement.



For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

APPARATUS AND METHODS FOR DELIVERING PROSTHESES TO LUMINAL BIFURCATIONS

BACKGROUND OF THE INVENTION

5 [0001] 1. Field of the Invention. The present invention relates generally to medical devices and methods. More particularly, the present invention relates to apparatus and methods for delivering stents and other luminal prostheses to bifurcations in the vasculature and other body lumens.

10 [0002] Stenting is a common medical procedure used in the vasculature and other body lumens. Over the last decade, the use of stents and other vascular prostheses has become wide spread in the revascularization of stenotic blood vessels where the blood vessel is first dilated and a stent placed to maintain vessel patency following the procedure. The stents are typically small, mesh-like tubular devices which are expanded *in situ*. They are typically formed from a metal and can be coated with drugs or other active agents.

15 [0003] The use of stents, and in particular drug-coated stents, has been very successful in the treatment of many forms for coronary artery disease. The success of stents, however, has been more limited for the treatment of lesions occurring at vessel bifurcations. While the disease in the main vessel is generally treated successfully, the outcome in the smaller or "side branch" vessel is often less successful. The lack of success is believed to result from a 20 lack of coverage by the stent at the ostium (opening) of a lesion and the resulting lack of drug delivery to that area.

25 [0004] To overcome at least some of these shortcomings, the inventors herein have developed a stent having a self-opening side portion which covers the side branch ostium when the stent is opened in the main blood vessel or other body lumen. This stent is described in co-pending application no. 11/330,382 (Attorney Docket No. 022246-000240US), filed on January 10, 2006, the full disclosure of which is incorporated herein by reference.

30 [0005] Stents having side holes or openings for alignment with side branch lumens are generally known in the art, and a variety of protocols and systems for delivering such stents to vascular and other luminal bifurcations are known. Of particular interest of the present

invention, several guidewire systems have been proposed for delivering such stents to a luminal bifurcation and for aligning the side hole with a side branch ostium prior to expansion of the stent. For example, U.S. Patent No. 5,749,825 to Fischell et al. describes introducing a balloon catheter carrying the stent over a main vessel guidewire. A side branch tube is positioned beneath a proximal portion of the stent and over the exterior of the balloon. A distal portion of the side branch tube extends through a side hole in the stent and permits advancement of a side branch guidewire into the side branch vessel. While generally effective for aligning the side hole of the stent with the side branch, the unconstrained distal portion of the side branch tube which extends from the side hole can interfere with advancement of the catheter through the vasculature. The presence of the side branch tube can increase the profile of the catheter, thus making it more difficult to introduce to smaller blood vessels and body lumens. Finally, Fischell suggests no specific approach for assuring that the two guidewires have not become crossed at the bifurcation so that the side hole is misaligned with the side branch ostium.

[0006] A similar stent and catheter structure is described in U.S. Patent No. 6,048,361, to Von Oepen. The guidewire tube of the '361 patent (referred to as a "hollow chamber"), however, is shown to extend to the center of the side opening in the stent. While this reduces the likelihood that the guidewire tube will interfere with catheter advancement, the chance of such interference is not completely eliminated. The distal tip of the guidewire tube (hollow chamber) remains exposed through the side hole and can potentially impede advancement of the catheter.

[0007] Other patents showing the use of side tubes for delivering stents having side holes to bifurcated body lumens include U.S. Patent No. 6,099,497; U.S. 6,165,195; and U.S. 6,596,020, and various related patents and publications.

[0008] For these reasons, it would be desirable to provide improved apparatus, systems, and methods for delivering stents and other prostheses to bifurcated vasculature and other body lumens. In particular, it would be desirable to provide for the delivery of stents having a side opening such that the side opening is properly aligned with the ostium of a side branch lumen prior to expansion of the stent or other prostheses. It would be still more desirable if the delivery systems were compatible with stents having self-opening side structures in which to find the side opening in the stent. Such devices, systems, and methods should be compatible with small diameter (low profile) catheter structures, should reduce or eliminate

any structure which exposed at or through the side openings in the stent or prostheses, and should allow for conformation of proper positioning of the side hole prior to expansion of the stent or other prostheses. At least some of these objectives will be met by the inventions described herein below.

5 [0009] 2. Description of the Background Art. Patents and published applications describing bifurcated stents and delivery systems include U.S. Patent Nos. 4,994,071; 5,609,627; 5,749,825; 5,755,735; 5,928,248; 6,048,361; 6,099,497; 6,165,195; 6,221,098; 6,210,429; 6,325,826; 6,596,020; 6,599,316; 6,676,691; 6,682,536; 6,689,156; 6,692,483; 6,709,440; 6,706,062; 6,835,203; 6,884,258; U.S. Publication Nos. 2002/0042650; 10 2002/0156516; 2002/0173835; 2003/0187494; 2003/0195606; 2004/0015227; 2004/0019302; 2004/0133268; 2004/0138737; 2005/0010278; 2005/0015108; 2005/0060027; 2005/0102,019; 2006/0036315; EP 1 2554 506 B1; and German Patents DE 297 08 803 U1; and DE 29 701 758 U1.

BRIEF SUMMARY OF THE INVENTION

15 [0010] The present invention provides apparatus and systems for the delivery of vascular and other luminal prostheses having side openings at bifurcations in the vasculature or other body lumens. Bifurcations will usually include a main branch vessel and a side branch vessel, where the cylindrical body of the prosthesis will be positioned within the main branch with the side opening aligned with an ostium or opening into the side branch. While the 20 apparatus and systems will be particularly useful for delivering prostheses having self-opening side structures, as taught in co-pending U.S. Patent Application No. 11/330,382, the full disclosure of which has previously been incorporated herein by reference, it should be appreciated that they are also useful for delivering any stent or prosthesis having a side hole or other opening and/or side structure which is to be aligned with the ostium of a side branch.

25 [0011] In a first specific aspect of the present invention, a delivery catheter comprises a catheter shaft having a proximal end and a distal end. An expansion member, such as an inflatable balloon, is disposed near the distal end of the shaft, and an expandable prosthesis is mounted over the expansion member. The expandable prosthesis will typically be formed from a deformable metal so that expansion of the expansion member will enlarge the 30 prosthesis from a small diameter configuration to a large diameter configuration which is anchored within the main vessel of the vasculature or other body lumen being treated. The prosthesis will further have a side hole, optionally in the form of a self-opening side structure,

which is to be aligned with an ostium of the side branch lumen after the prosthesis has been expanded. The phrase "side hole" includes any opening or structure which is to be aligned with an ostium of a side branch lumen or vessel. The side hole may simply be a cell or a slit in the prosthesis structure which is preselected to be aligned with a side branch vessel but

5 which is otherwise similar to other cells, slits, or the like in the prosthesis. More usually, however, the side hole will be an enlarged or enlargeable cell which is distinguishable from the adjacent or remaining structure of the prosthesis. In other embodiments, the "hole" comprises a self-opening or balloon openable peripheral structure which is intended to bridge the circumference of the side branch ostium after the prosthesis is opened in the main branch.

10 Such alignment is achieved with a guidewire structure which is disposed over the expansion member (optionally over or within the folds of an inflatable balloon) and beneath a proximal portion of the prosthesis. In an initial configuration of the catheter, the guidewire structure will extend to a holding location which is spaced proximally from the side hole of the prosthesis, usually by a distance of at least 1 mm, preferably at least 2 mm, and more

15 preferably at least 3 mm.

[0012] The guidewire structure may have a variety of configurations. In one specific embodiment, the guidewire structure comprises a guidewire tube which carries the guidewire in a lumen thereof. The guidewire tube will be positioned between the prostheses and the expandable member, as just described, and the guidewire will remain in the guidewire tube

20 with a distal end retracted fully within the tube during advancement of the catheter to a position near the bifurcation. In an alternative embodiment, the guidewire structure may comprise an elongate slide having a channel which slidably receives the guidewire. The channel can be formed, for example, as a "half tube" with an open top which can be oriented either toward the balloon or toward an inner surface of the prosthesis. The use of a slide may

25 be preferred over the use of a full guidewire tube since it can reduce the resulting profile or diameter of the catheter. As a second alternative, the guidewire structure may consist essentially or only of the guidewire itself. That is, the guidewire may be directly placed between the inner surface of the prosthesis and the outer surface of the expandable member without any further structure surrounding it. In all cases, however, the guidewire and any

30 other structure associated with the guidewire will be withdrawn proximally of the side hole by the requisite distances described above.

[0013] The delivery catheters of the present invention will preferably further comprise a central guidewire extending distally from the catheter shaft. In some instances, the central

guidewire could be fixed to (combined and immobilized with) the catheter shaft, but more often the central guidewire will be a conventional moveable guidewire, either in a over-the-wire design (which extends fully or almost fully through the entire catheter shaft), in a rapid exchange design where the guidewire extends only through a distal portion of the catheter shaft, or in other conventional simplified exchange designs.

[0014] In a second aspect of the present invention, a delivery catheter comprises a catheter shaft, an expansion member, and an expandable prosthesis having a side hole, generally as described above. The guidewire is disposed over the expansion member and beneath at least a proximal portion of the prosthesis so that the guidewire is advanceable through the side hole. In this particular embodiment, the guidewire may extend partially or fully to side hole and in some instances through the side hole of the prosthesis even while the catheter is being advanced through the vasculature toward the bifurcation. In this aspect of the invention, the catheter shaft includes a split lumen along at least a portion of its length for removably receiving a proximal portion of the side guidewire. The split lumen is particularly useful for constraining the side guidewire in embodiments where a main guidewire is received only in a distal portion of the catheter shaft (typically to facilitate rapid exchange). In such instances, the side guidewire could become entangled or twisted with the main guidewire if both guidewires were free of the catheter shaft structure. The split lumen would preferably be used to constrain the side guidewire, but could be used for the main or the side guidewires. In other embodiments, it would be possible to enlarge the split lumen to receive both wires or to provide two split lumens for receiving both the main guidewire and the side guidewire.

[0015] Other features of the delivery catheter having the split guidewire lumen are generally the same as those described in connection with the first aspect of the present invention. The delivery catheter will usually comprise a central guidewire, either a fixed central guidewire or moveable central guidewire. The side guidewire may be received in a guidewire tube, in a guidewire slide, or maybe disposed directly between the expandable member and an inner surface of the prosthesis. In this aspect of the invention, the guidewire and any other guidewire structure may also extend through the side hole in the prosthesis even when the catheter is in its delivery configuration for advancement through the main vessel.

[0016] In a third aspect of the present invention, methods are provided for delivering a prosthesis having a side hole (as defined above) to a luminal location. The methods comprise

advancing a catheter over a central guidewire through a main lumen, such as an artery or other blood vessel, to position the prosthesis near the bifurcation. A side guidewire is then advanced through the side hole into a branch lumen of the bifurcation, and the prosthesis is eventually expanded at the bifurcation with the side hole aligned with the side branch. In 5 order to assure that the side hole is properly aligned with the ostium or opening of the side branch, radiopaque markers are provided on the prosthesis and/or on the guidewire so that the positions may be observed under fluoroscopy. If it is observed that the catheter is rotated so that the guidewire crosses the prosthesis to reach the side branch, or the side hole is directed away from the ostium, then it is clear that the side hole is not properly aligned with the side 10 branch ostium. Thus, the catheter may be rotated until it is apparent under the fluoroscopic imaging that the guidewire is no longer crossing the prosthesis and the side hole is therefore rotationally aligned with the side branch ostium.

[0017] This method for rotationally aligning the prosthesis is compatible with any of the catheter systems described previously where the side guidewire extends through the side hole 15 of the prosthesis to aid in alignment of the side hole with the side branch ostium, including systems which require a separate balloon to deploy a side structure on the prosthesis into the ostium of the side branch.

BRIEF DESCRIPTION OF THE DRAWINGS

[0018] Fig. 1 is an isometric view of a delivery catheter constructed in accordance with the 20 principles of the present invention.

[0019] Fig. 2 is an enlarged view of a distal portion of the catheter of Fig. 1, shown with an expanded prosthesis in broken line.

[0020] Fig. 3 is an enlarged view of a proximal portion of the delivery catheter of Fig. 1.

[0021] Fig. 4 is a cross-sectional symmetric view taken along line 4-4 of Fig. 3.

25 [0022] Fig. 5 illustrates a side guidewire which is useful in the apparatus and methods of the present invention.

[0023] Figs. 6A and 6B illustrate positioning of a guidewire tube beneath a prosthesis mounted on an expandable member in accordance with the principles of the present invention.

[0024] Figs. 7A and 7B illustrate positioning of a guidewire slide positioned beneath the prosthesis and over an expandable member in accordance with the principles of the present invention.

[0025] Figs. 8A and 8B illustrate a guidewire which is positioned without additional

5 supporting structure beneath a prosthesis and over and expandable member in accordance with the principles of the present invention.

[0026] Figs. 9A through 9E illustrate use of the delivery catheters of the present invention for implanting a prosthesis having a side hole at an ostium of a side branch in the vasculature of a patient in accordance with the principles of the present invention.

10 **[0027]** Figs. 10A and 10B illustrate an optional aspect of the method of the present invention for assuring that the side guidewire does not cross the prosthesis as the prosthesis is expanded.

DETAILED DESCRIPTION OF THE INVENTION

[0028] Referring now to Fig. 1, a delivery catheter 10 carries a prosthesis 12 having a side hole 15 (Fig. 2) on an expandable member 14, such as an inflatable balloon of the type normally employed in stent delivery. The delivery catheter 10 further comprises a distal section 16, an intermediate section 18, and a proximal section 20, where the sections are arranged to provide an elongate catheter body to support the expandable member 14 so that it may be delivered intraluminally or intravascularly to a target site in a generally conventional manner. Typically, the distal and intermediate sections 18 will be relatively more flexible than the proximal section 20. A proximal hub 22 having a connector 24 for connection to a balloon inflater is attached to a proximal end of the proximal section 20. The hub can have any design including a y-shaped hub, a hub with flexible connector, and the like. A central guidewire 26 is received through the balloon and exits from a port near the proximal end of distal section 16 of the catheter body. Although illustrated as a "rapid exchange" design, it will be appreciated that the shaft of the delivery catheter 10 could also be adapted for over-the-wire introduction over the central guidewire 26, or any other known or future design.

[0029] Of particular interest to the present invention, a side guidewire 28 is disposed

beneath a proximal portion of the prosthesis 12 and over the expandable member 14. As

30 described in more detail in connection with Figs. 6-8, the side guidewire may be disposed in a guidewire tube, guidewire slide, or without further supporting structure. As shown in Fig. 2,

the side guidewire 28 is disposed in a guidewire tube 30 which extends beneath the prosthesis 12. The side guidewire 28 passes into a lumen within the catheter shaft through a port 34 and passes back out of the shaft through a proximal port 36 (Fig. 1). The prosthesis 12 will have a side hole 15, preferably in the form of a self-opening or other side structure, as shown in broken line in Fig. 2. Details of a self-opening side structure are provided in copending application no. 11/330,382, the full disclosure of which has previously been incorporated herein by reference.

[0030] Referring now to Figs. 3 and 4, the proximal section 20 of the delivery catheter may optionally be formed with a split side lumen 34 for removably receiving the side guidewire 28, as best seen in Fig. 4. This section can be formed over a hypotube 36 with a polymeric extrusion 38 over the hypotube forming the split guidewire lumen 34. Open lumen 40 through the hypotube will serve as the inflation lumen for the catheter. The split side guidewire lumen is particularly advantageous since it allows the guidewire to be constrained during advancement of the catheter. By constraining the side guidewire, the chance of crossing or otherwise entangling the side guidewire 28 with the main guidewire 26 is greatly reduced. It would be possible, of course, to provide a second split guidewire for the main guidewire, or in other instances deeming guidewire could be received within a central lumen of the catheter shaft in a conventional over-the-wire configuration. In alternative embodiments, the polymeric tube may be extended separately and may be separate from the hypotube.

[0031] Referring now to Fig. 5, an exemplary side guidewire 40 comprises a round proximal section 42, a reduced diameter round transition section 44, and a flat distal section 42. A radiopaque coil 46 joins the distal end of the flat section 42 optionally with an atraumatic distal sphere 48. The guidewire can be formed from stainless steel, shape memory materials, or other conventional guidewire materials, and will have dimensions normally associated with guidewires for intravascular or other luminal uses. The delivery catheters of the present invention can be used with a variety of other guidewires, including very low profile guidewires which can further reduce the diameter of the catheter system.

[0032] Referring now to Figs. 6 through 8, positioning of the side guidewire 28 beneath a proximal portion of prosthesis 12 and over the expandable member 14 will be described for several embodiments of the present invention. In the embodiment of Fig. 6A and 6B, guidewire 28 is disposed in a guidewire tube 50 which is located beneath a proximal portion

of the prosthesis 12 and over an outer surface of the expandable member 14. A distal tip 52 of the guidewire tube is located by a minimum distance ℓ from the closest point of the side hole 15. The distance ℓ will generally be at least 1 mm, preferably being at least 2 mm, and often being 3 mm or more. In the catheter introduction configuration, the guidewire 28 will 5 be fully retracted within the guidewire tube 50, as shown in Fig. 6A. Once the catheter has been advanced to the bifurcation, the guidewire 28 may be advanced distally and through the opening 15 so that it may be guided to the side branch, as shown in Fig. 6B.

10 [0033] In a first alternative embodiment as shown in Figs. 7A and 7B, the side guidewire 28 may be disposed in a guidewire slide 60 having a region 62 which is open on the side adjacent the prosthesis 12. Thus, the guidewire 28 may be received in a channel formed by the open region of the slide 60 which provides a guide to help advance the guidewire through the opening 15, as shown in Fig. 7B. As with the previous embodiment, the distal most end of the guidewire 28 and guidewire slide 60 will be maintained by the minimum distance ℓ from the closest portion of the opening 15.

15 [0034] In a second alternative embodiment, guidewire 28 may be disposed directly between the inner surface of the prosthesis 12 and the outer surface of the expandable member 14, as shown in Figs. 8A and 8B. Again, the distal tip of the guidewire 28 will be maintained at a minimum distance ℓ from the closest portion of the opening 15 in the prosthesis. Once the catheter has been advanced to a location near the bifurcation, the side guidewire may be 20 advanced through the opening, as shown in Fig. 8B.

25 [0035] Referring now to Figs. 9A through 9E, an example of the delivery of prosthesis 12 using the delivery catheter 10 to a branch lumen comprising a main vessel MV and a side vessel SV will be described. First, the central guidewire 26 is advanced through the main vessel to a point beyond the ostium O of the side vessel SV, as shown in Fig. 9A. The catheter 10 may be advanced over the central guidewire 26 in the conventional manner until the prosthesis 12 approaches the ostium O of the side vessel SV. In Fig. 9B, the side guidewire 28 is shown in the guidewire tube 50, but it will be appreciated that any of the guidewire structures of Fig. 6-8 could be employed.

30 [0036] The side guidewire 28 is next distally advanced through the opening 15 of prosthesis 12, as shown in Fig. 9C, and the guidewire is then advanced through the ostium O and into the side vessel SV, as shown in Fig. 9D. At that point, the catheter may be advanced so that the opening 15 in the prosthesis 12 approaches and eventually aligns with the

ostium O. The balloon or other expandable member 14 may then be inflated so that the prosthesis 12 expands within the main vessel MV and the side opening (shown as a self-opening side structure) aligns with the ostium O, as shown in Fig. 9D. In one embodiment, the side guidewire will have a stiffer section near its distal end to improve system alignment.

5 [0037] In a preferred aspect of the present invention, the side guidewire 28 may be radiopaque (or include radiopaque markers) and/or radiopaque markers may be provided on a side of the prosthesis 12 aligned with the side opening 15. The use of such radiopaque structures allows the physician to easily determine whether the prosthesis is rotationally misaligned with the ostium O of the side vessel SV. As shown in Fig. 10A, when the 10 prosthesis is rotationally misaligned, the side guidewire will extend across the prosthesis 12. Expansion of the prosthesis 12 in this position will of course not result in alignment of the side opening 15 with the ostium O. In cases where a separate balloon is used to deploy a side structure, such misalignment can dissect or perforate the artery or other treated lumen. The catheter can then be torqued to rotate the prosthesis 12 so that the opening 15 is adjacent the 15 ostium O with the side guidewire 28 positioned as shown in Fig. 10B. This configuration is readily observed under fluoroscopic imaging since the radiopaque markers 70 on the prosthesis 12 (generally adjacent to the opening 15) will be adjacent to the ostium O. Additionally, the radiopaque side guidewire 28 can be observed going directly from the opening into the side branch vessel SV. In this configuration, the prosthesis may be 20 deployed by expanding the expandable member 14.

[0038] While the above is a complete description of the preferred embodiments of the invention, various alternatives, modifications, and equivalents may be used. Therefore, the above description should not be taken as limiting the scope of the invention which is defined by the appended claims.

WHAT IS CLAIMED IS:

- 1 1. A delivery catheter comprising:
2 a catheter shaft having a proximal end and a distal end;
3 an expansion member disposed near the distal end of the shaft;
4 an expandable prosthesis mounted over the expansion member; and
5 a guidewire structure disposed over the expansion member, beneath a
6 proximal portion of the prosthesis, and extending to a holding location spaced proximally of a
7 side hole of the prosthesis by a distance of at least 1 mm.
- 1 2. A delivery catheter as in claim 1, wherein the guidewire structure
2 comprises a side guidewire slidably received in a passage of a guidewire tube.
- 1 3. A delivery catheter as in claim 1 wherein the guidewire structure
2 comprises a side guidewire slidably received in a channel of an elongate slide.
- 1 4. A delivery catheter as in claim 1, wherein the guidewire structure
2 consists essentially of a guidewire which directly contacts an inner wall of the prosthesis and
3 an outer surface of the expansion member.
- 1 5. A delivery catheter as in claim 1, further comprising a central
2 guidewire extending distally from the distal end of the catheter shaft.
- 1 6. A delivery catheter as in claim 5, wherein the central guidewire is
2 fixed.
- 1 7. A delivery catheter as in claim 5, wherein the central guidewire is
2 moveable.
- 1 8. A delivery catheter as in claim 1, wherein the holding location is
2 spaced at least 2 mm proximally of the side hole.
- 1 9. A delivery catheter as in claim 1, wherein the holding location is
2 spaced at least 3 mm proximally of the side hole.
- 1 10. A delivery catheter comprising:
2 a catheter shaft having a proximal end and a distal end;
3 an expansion member disposed near the distal end of the shaft;

4 an expandable prosthesis having a side mounted over the expansion member;
5 and

6 a guidewire disposed over the expansion member and beneath at least a
7 proximal portion of the prosthesis, said guidewire being advanceable through a side hole of
8 the prosthesis, wherein a proximal portion of the shaft includes a split lumen for removably
9 receiving a proximal portion of the guidewire.

1 11. A delivery catheter as in claim 10, further comprising a guidewire tube
2 having a passage for slidably receiving a side guidewire.

1 12. A delivery catheter as in claim 10, further comprising an elongate slide
2 having a channel for slidably receiving the guidewire.

1 13. A delivery catheter as in claim 10, wherein the guidewire is received
2 directly between the inner wall of the prosthesis and an outer surface of the expansion
3 member.

1 14. A delivery catheter as in claim 10, further comprising a central
2 guidewire extending distally from the distal end of the catheter shaft.

1 15. A delivery catheter as in claim 14, wherein the central guidewire is
2 fixed.

1 16. A delivery catheter as in claim 14, wherein the central guidewire is
2 moveable.

1 17. A method for delivering a prosthesis having a side hole to a luminal
2 bifurcation, said method comprising:

3 advancing a catheter over a central guidewire through a main lumen to
4 position the prosthesis near the bifurcation:

advancing a side guidewire through the side hole into a branch lumen at the bifurcation;

7 observing radiopaque markers on the prosthesis and/or the guidewire to
8 determine if the side guidewire is crossing the prosthesis to reach the side branch:

9 if the guidewire is crossing the prosthesis, rotating the catheter until the
0 guidewire no longer crosses the prosthesis: and

11 expanding the prosthesis at the bifurcation with the side hole aligned with the
12 side branch.

1 18. A method as in claim 17, wherein the guidewire had been fully
2 retracted beneath the prosthesis while the catheter had been initially advanced over the
3 central guidewire.


1 19. A method as in claim 17, wherein the side guidewire is advanced
2 through a guidewire tube which passes over an expansion member and beneath a proximal
3 portion of the prosthesis.

1 20. A method as in claim 17, wherein the side guidewire is advanced
2 through a channel in an elongate slide which passes over an expansion member and beneath a
3 proximal portion of the prosthesis.


1 21. A method as in claim 17, wherein the side guidewire is positioned
2 directly between an expansion member and an inner surface of the prosthesis prior to
3 advancing.

1 22. A method as in claim 17, wherein expanding the prosthesis comprises
2 expanding an expansion member within the prosthesis.

1 23. A method as in claim 22, further comprising deflating the expansion
2 member, wherein deflating the expansion member releases the side guidewire from the side
3 hole.

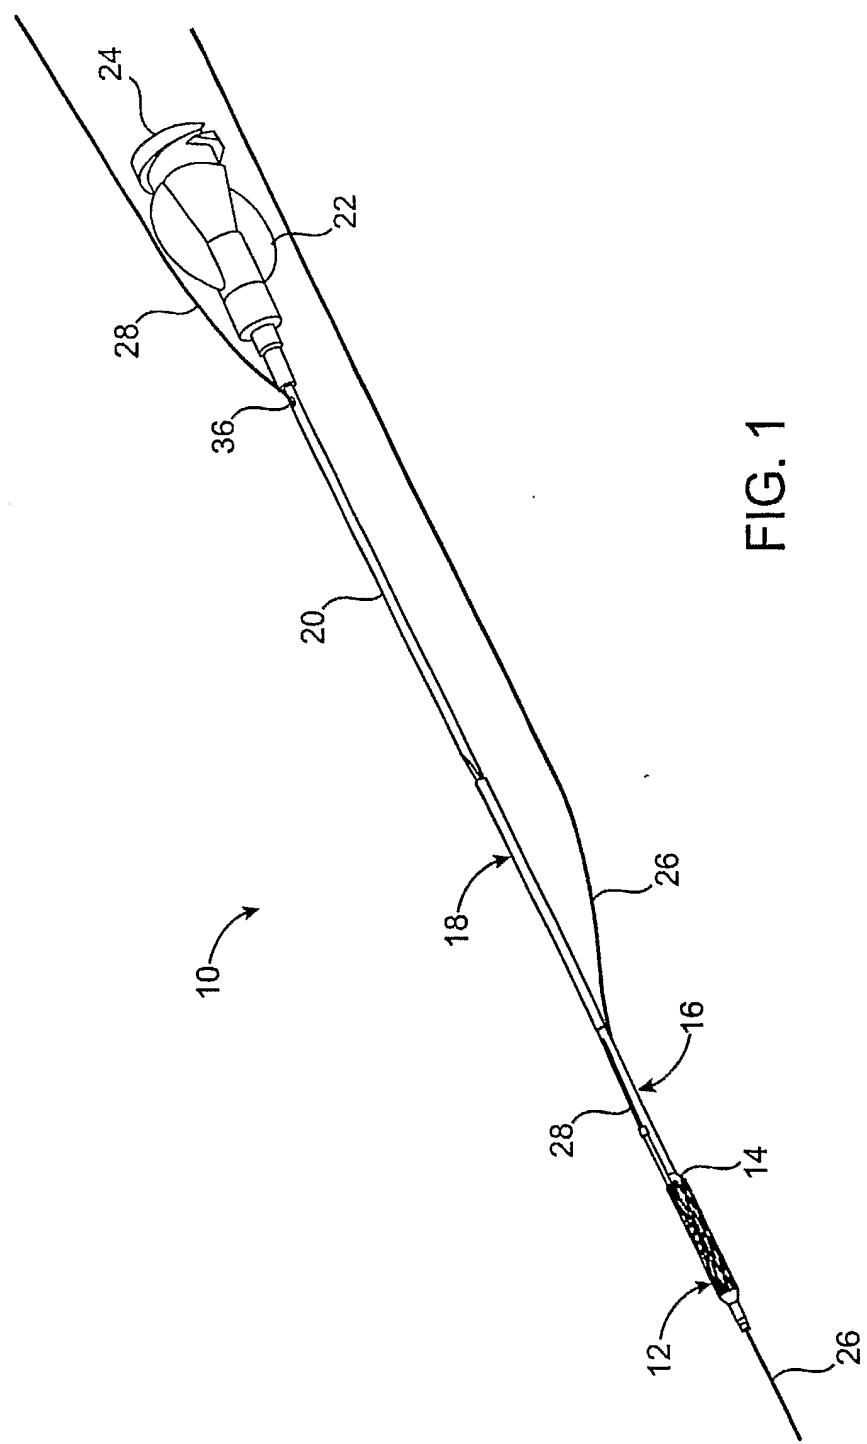


2 / 13

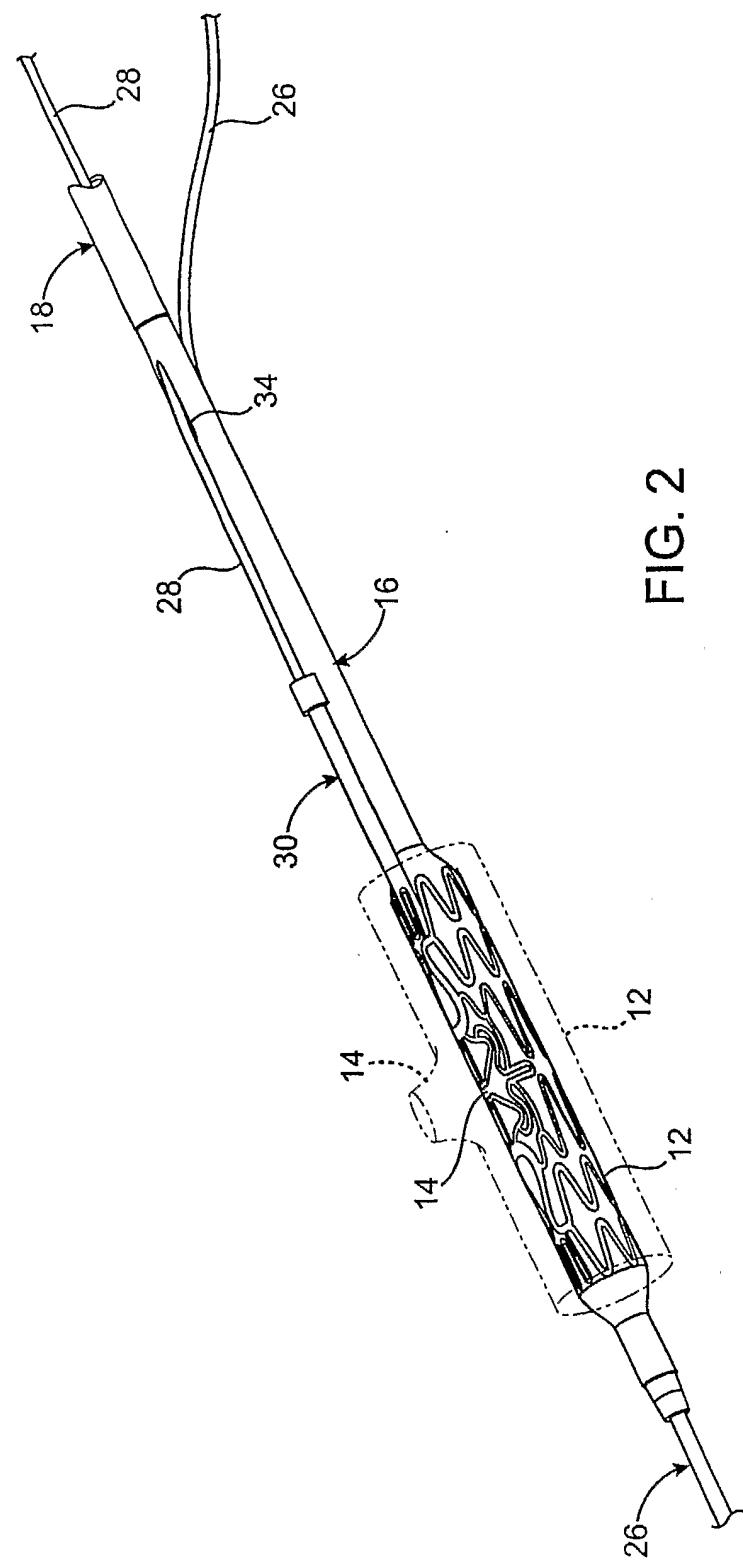

SUBSTITUTE SHEET (RULE 26)


3 / 13

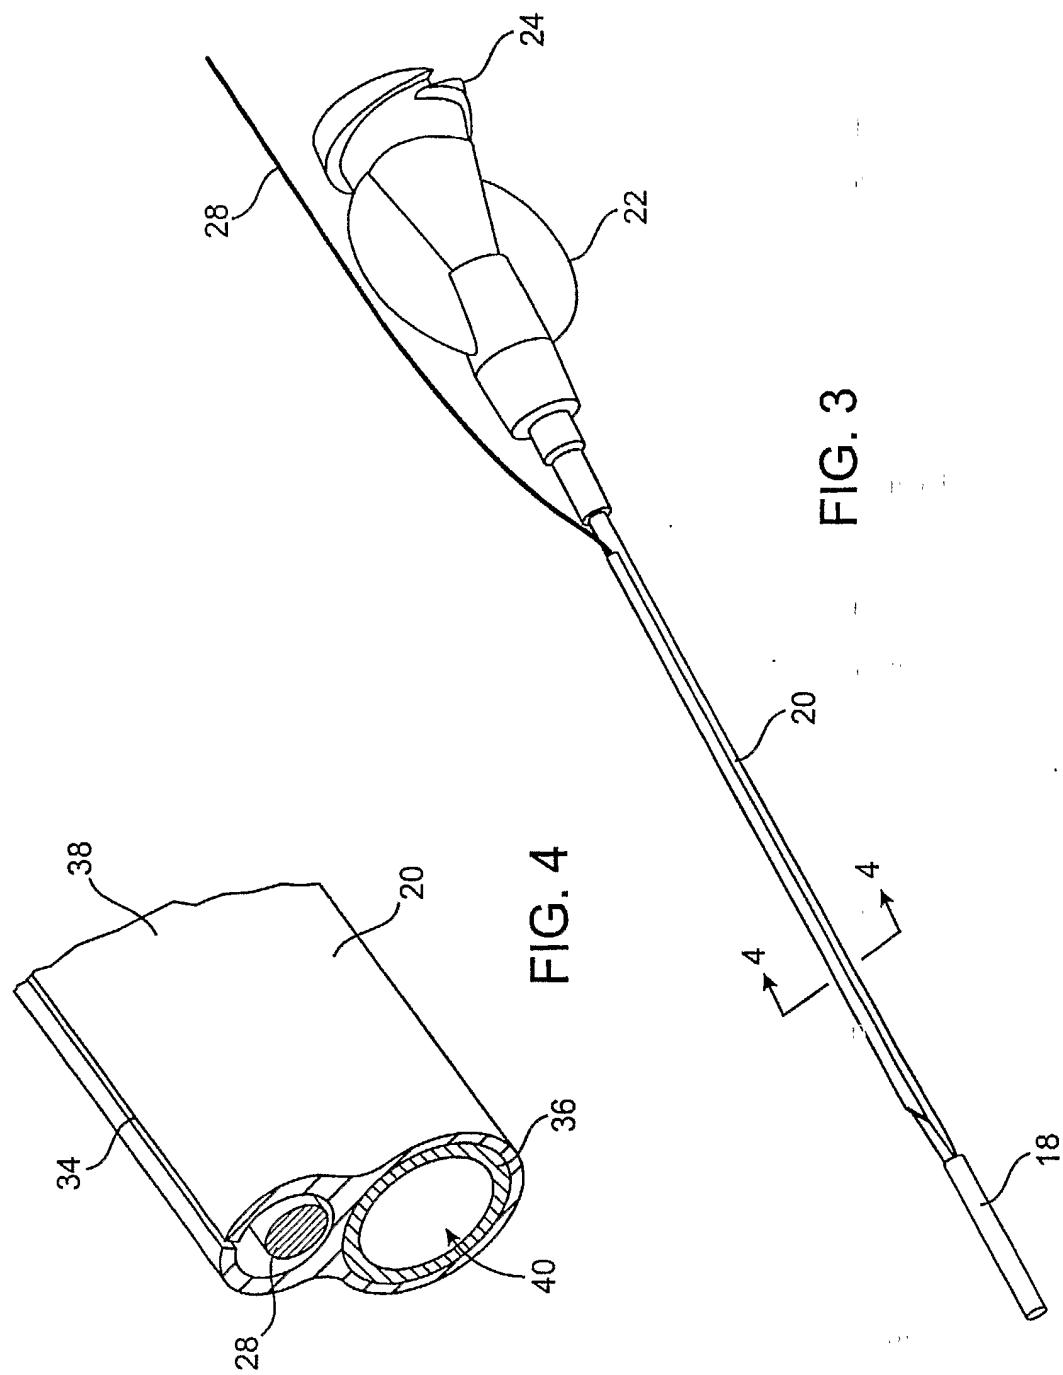

SUBSTITUTE SHEET (RULE 26)

4 / 13

FIG. 5

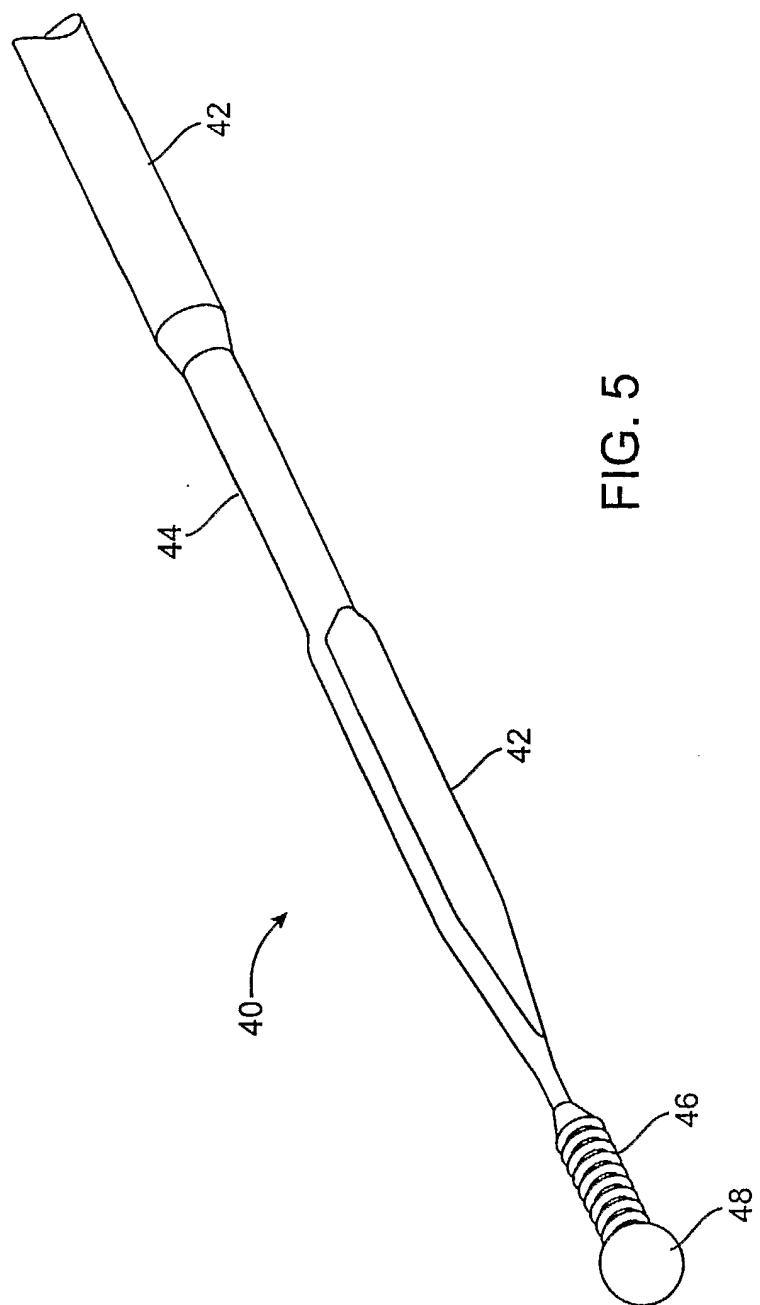

SUBSTITUTE SHEET (RULE 26)

5 / 13

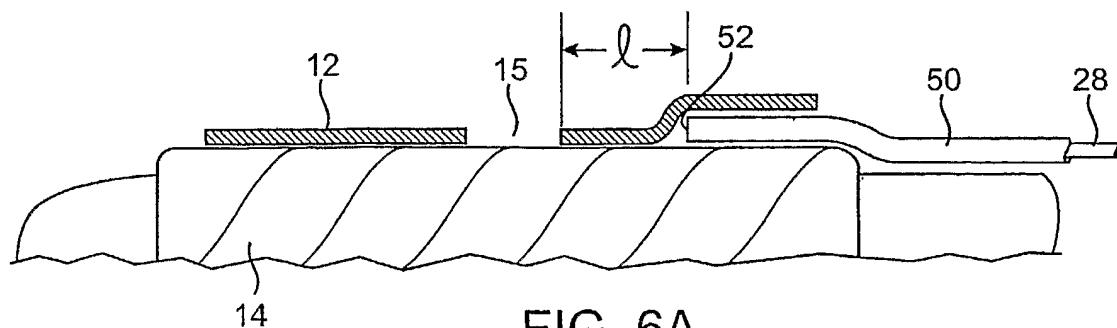


FIG. 6A

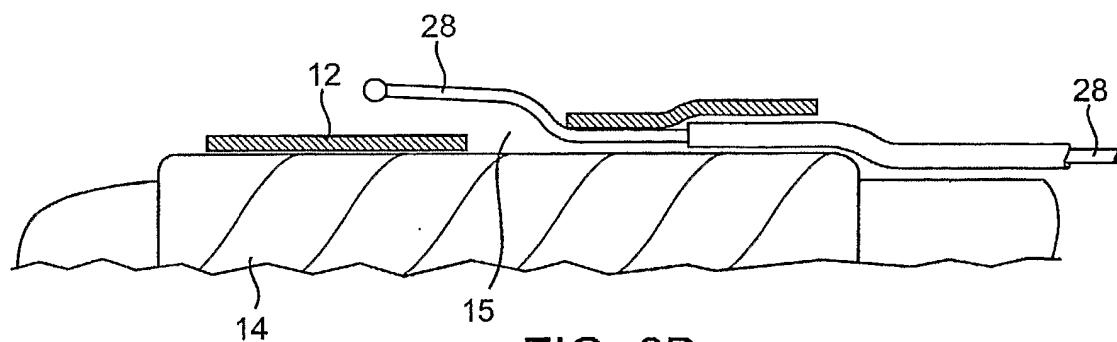


FIG. 6B

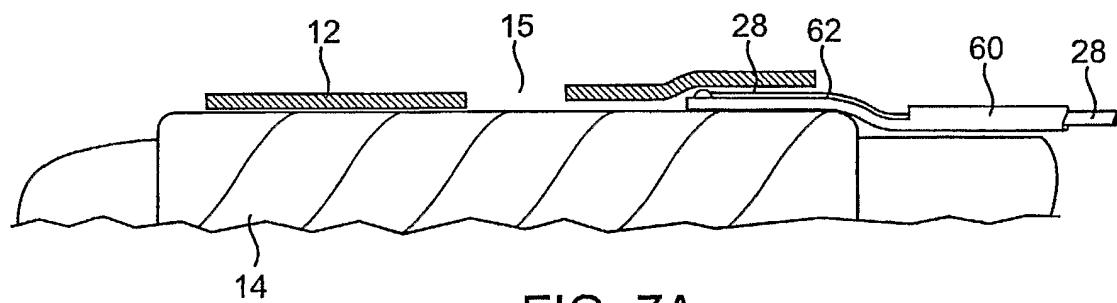


FIG. 7A

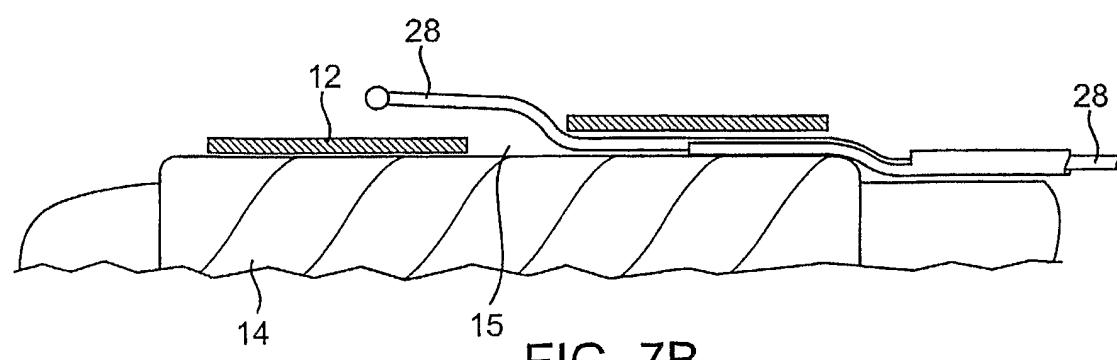


FIG. 7B

6 / 13

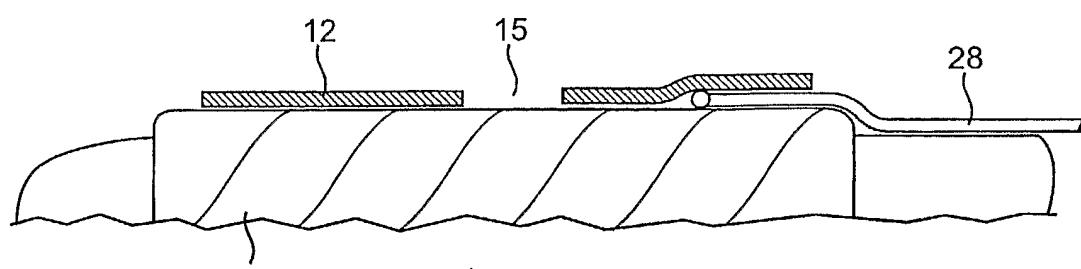


FIG. 8A

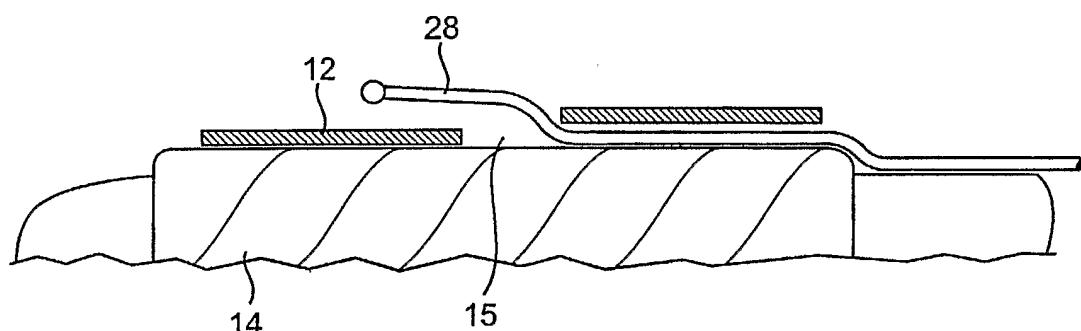


FIG. 8B

7 / 13

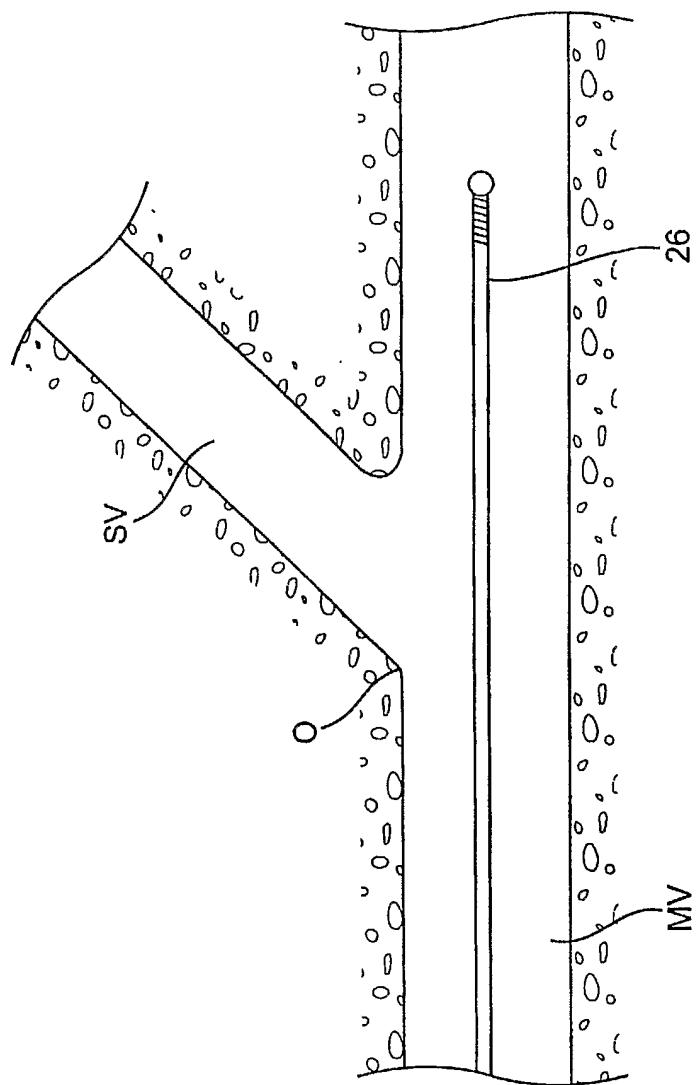


FIG. 9A

SUBSTITUTE SHEET (RULE 26)

8 / 13

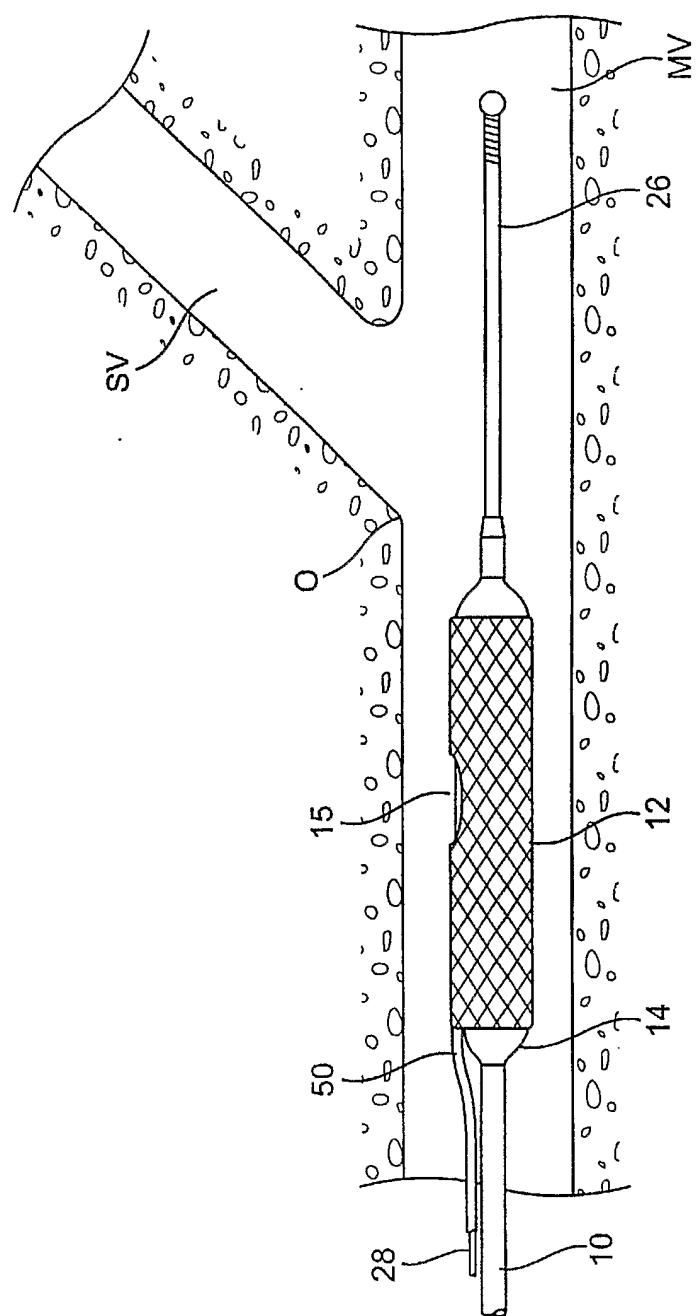


FIG. 9B

SUBSTITUTE SHEET (RULE 26)

9 / 13

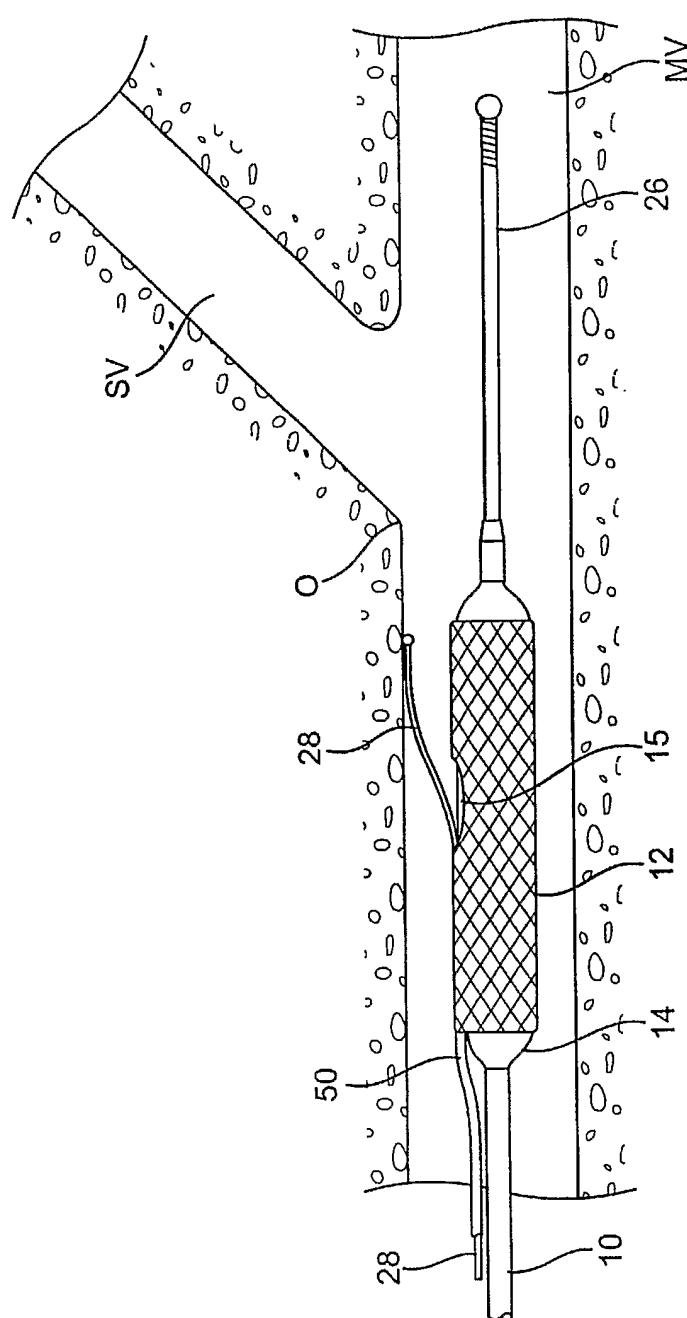


FIG. 9C

SUBSTITUTE SHEET (RULE 26)

10 / 13

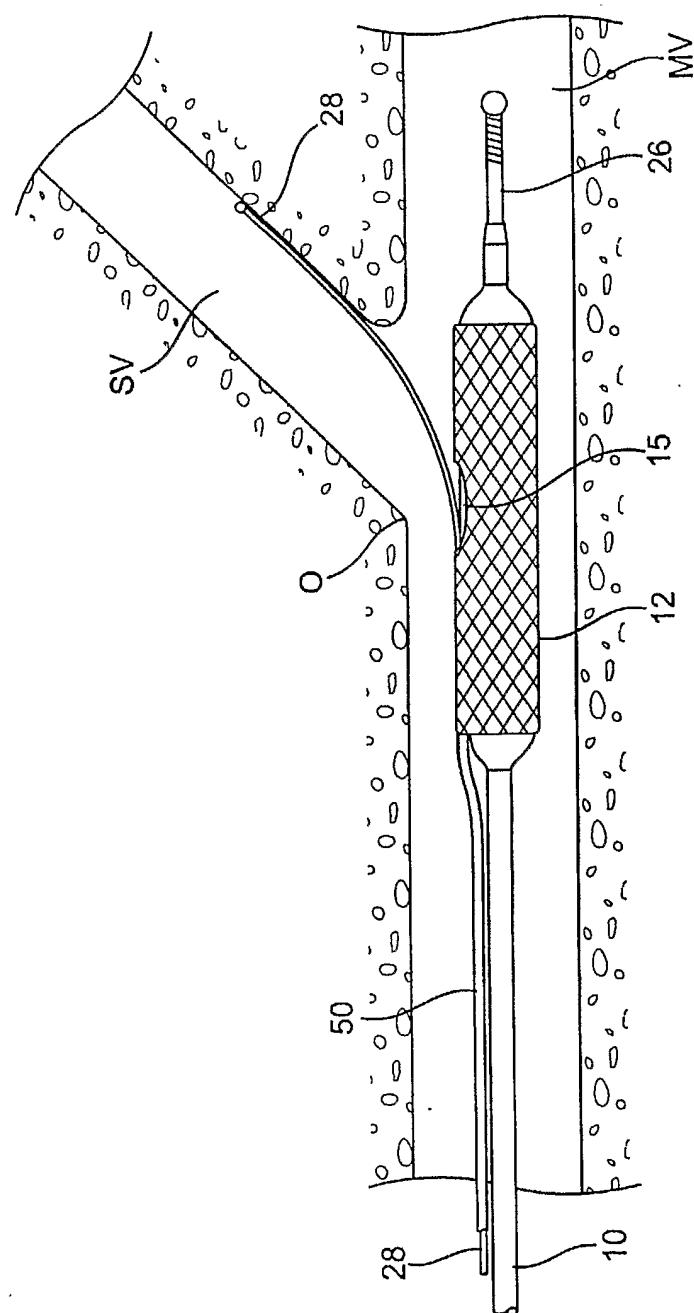


FIG. 9D

SUBSTITUTE SHEET (RULE 26)

11 / 13

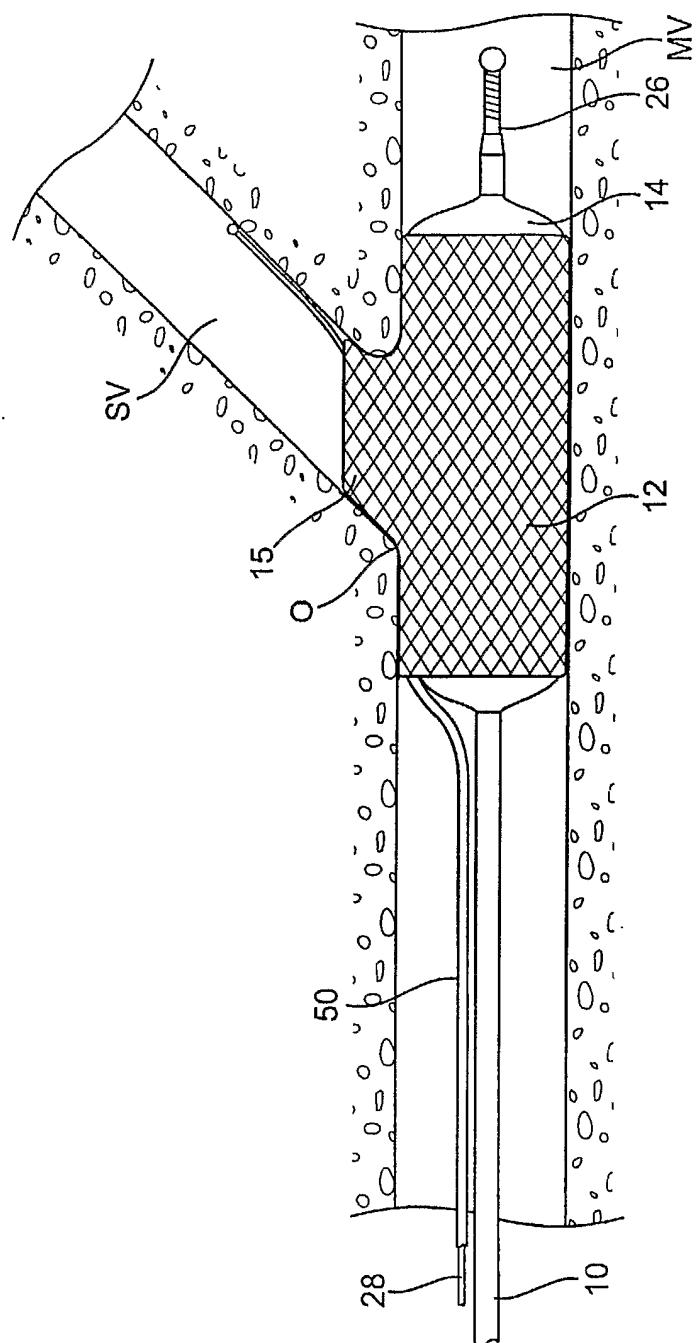


FIG. 9E

SUBSTITUTE SHEET (RULE 26)

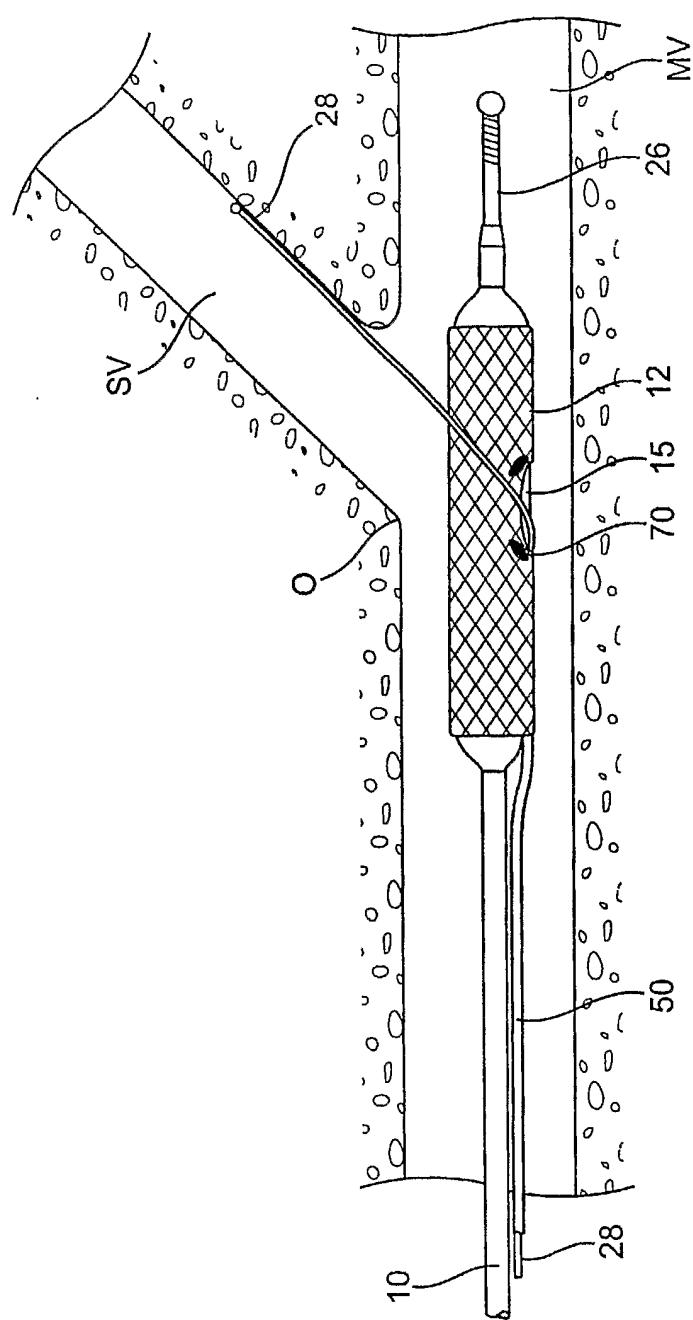


FIG. 10A

13 / 13

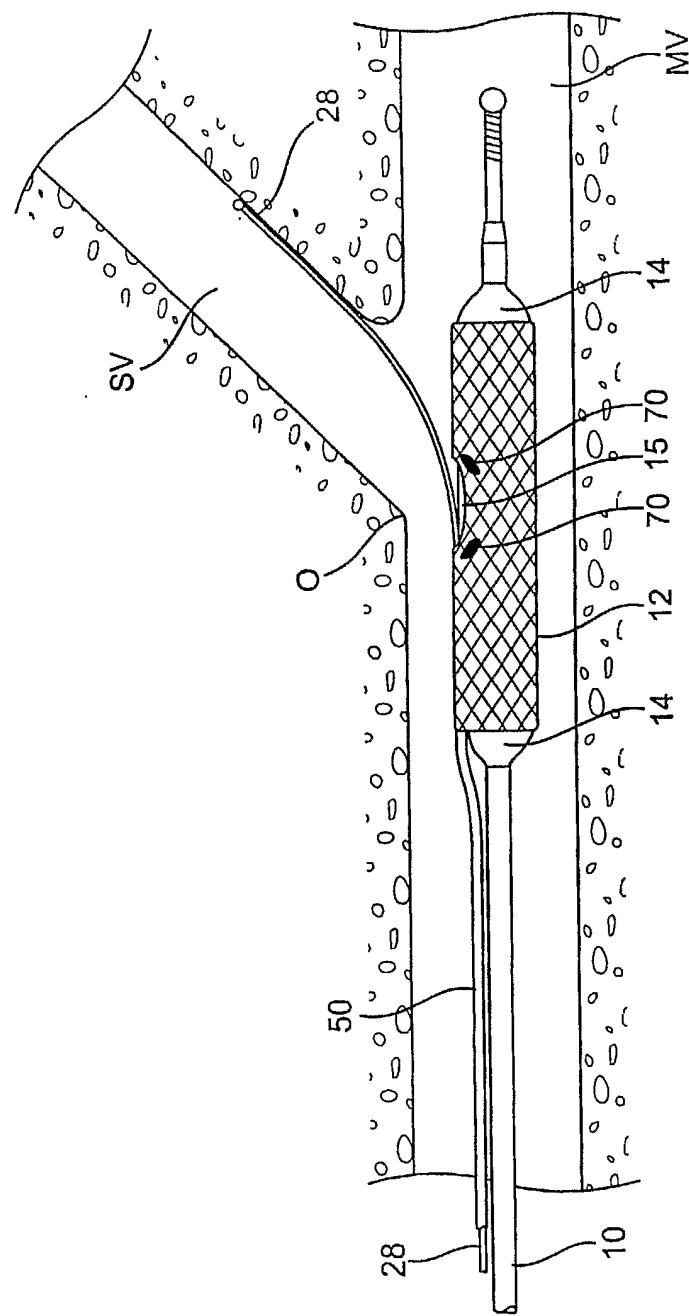


FIG. 10B

SUBSTITUTE SHEET (RULE 26)