



US00D717968S

(12) **United States Design Patent**  
**Klein et al.**

(10) **Patent No.:** **US D717,968 S**

(45) **Date of Patent:** **\*\* Nov. 18, 2014**

(54) **MULTI-BLOCK PCR THERMAL CYCLER DEVICE**

(71) Applicant: **Life Technologies Corporation,**  
Carlsbad, CA (US)

(72) Inventors: **Sandro David Klein,** Irvine, CA (US);  
**Joseph Lee,** San Diego, CA (US);  
**Byron Lee,** Thousand Oaks, CA (US);  
**Shushuo Wu,** Thousand Oaks, CA (US);  
**Lance Hussey,** Thousand Oaks, CA (US)

(73) Assignee: **Life Technologies Corporation,**  
Carlsbad, CA (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/438,754**

(22) Filed: **Dec. 3, 2012**

(51) **LOC (10) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/232**

(58) **Field of Classification Search**  
USPC ..... D24/230-233, 216-220, 221, 225-227,  
D24/229; D10/81; 422/50-53, 62-63, 68.1,  
422/500, 565; 435/285.1, 287.1, 288.4,  
435/287.2, 288.7, 303.1, 809  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D256,726	S	*	9/1980	Meuli et al.	.....	D24/232
5,525,300	A	*	6/1996	Danssaert et al.	.....	435/285.1
D467,349	S	*	12/2002	Niedbala et al.	.....	D24/232
D537,951	S	*	3/2007	Okamoto et al.	.....	D24/233
D556,914	S	*	12/2007	Okamoto et al.	.....	D24/233
D571,480	S	*	6/2008	Beck et al.	.....	D24/232
D607,569	S	*	1/2010	Yukikado et al.	.....	D24/186
D647,209	S	*	10/2011	Muller et al.	.....	D24/216
8,046,175	B2	*	10/2011	Kuo et al.	.....	422/63



\* cited by examiner

*Primary Examiner* — Wan Laymon  
(74) *Attorney, Agent, or Firm* — Life Technologies Corporation

(57) **CLAIM**  
The ornamental design for a multi-block PCR thermal cyclers device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top and side perspective view of an multi-block PCR thermal cyclers device, according to a first exemplary embodiment;  
FIG. 2 is a front view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 3 is a back view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 4 is a right side view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 5 is a left side view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 6 is a top view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 7 is a bottom view of the multi-block PCR thermal cyclers device of FIG. 1;  
FIG. 8 is a front, top and side perspective view of an multi-block PCR thermal cyclers device, according to a second exemplary embodiment;  
FIG. 9 is a front view of the multi-block PCR thermal cyclers device of FIG. 8;  
FIG. 10 is a back view of the multi-block PCR thermal cyclers device of FIG. 8;  
FIG. 11 is a right side view of the multi-block PCR thermal cyclers device of FIG. 8;  
FIG. 12 is a left side view of the multi-block PCR thermal cyclers device of FIG. 8;  
FIG. 13 is a top view of the multi-block PCR thermal cyclers device of FIG. 8; and,  
FIG. 14 is a bottom view of the multi-block PCR thermal cyclers device of FIG. 8.  
The broken lines shown in the figures are included for the purpose of illustrating portions of the multi-block PCR thermal cyclers device and form no part of the claimed design.

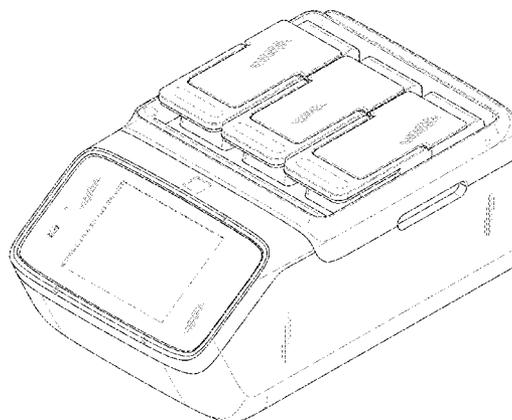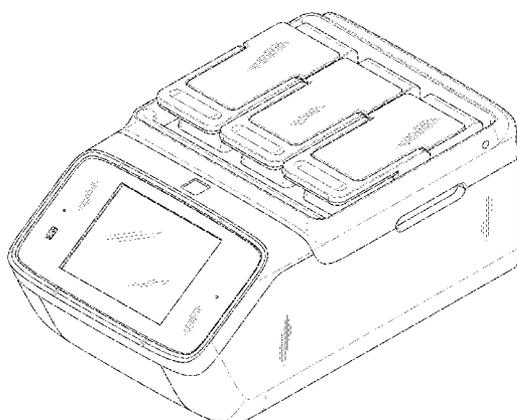

**1 Claim, 14 Drawing Sheets**

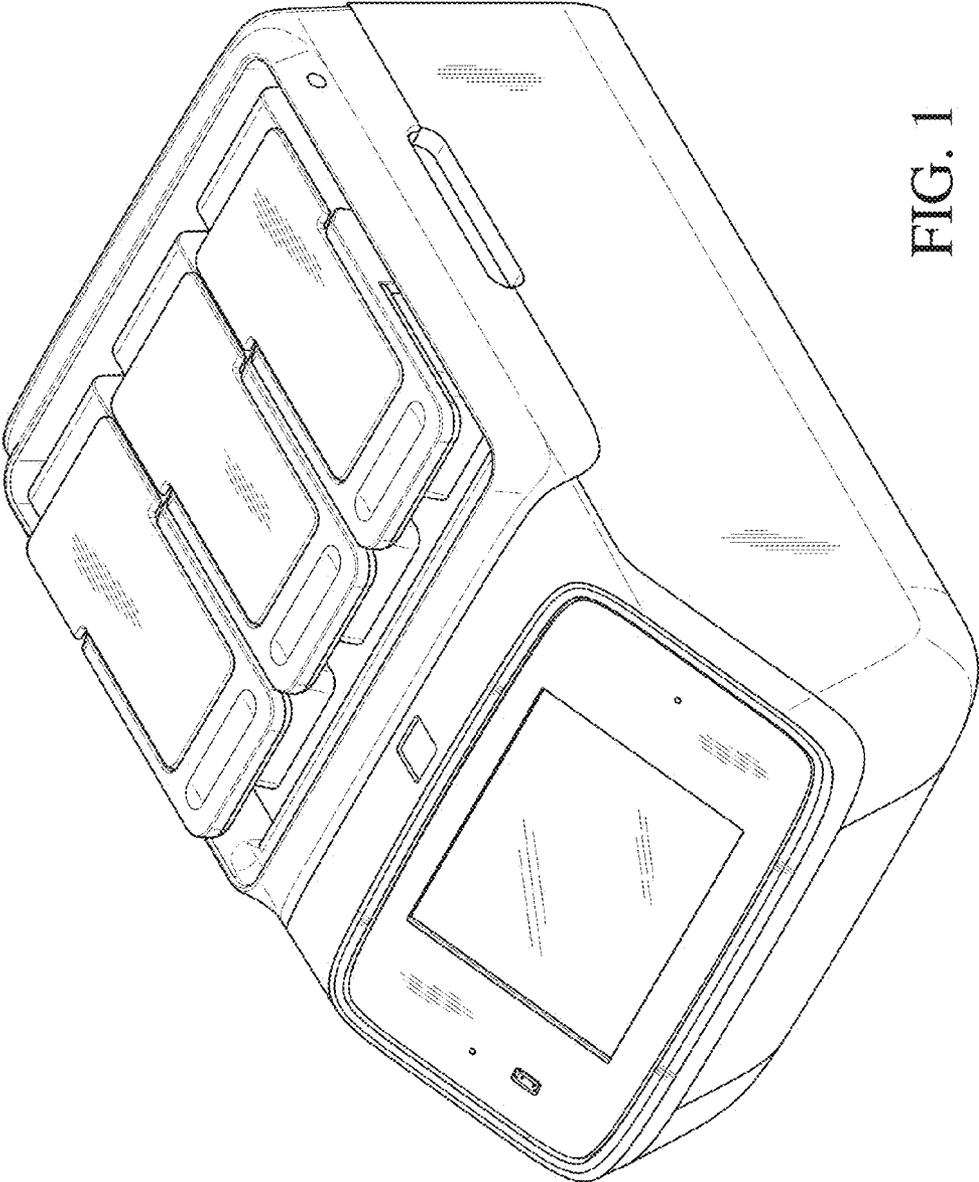


FIG. 1

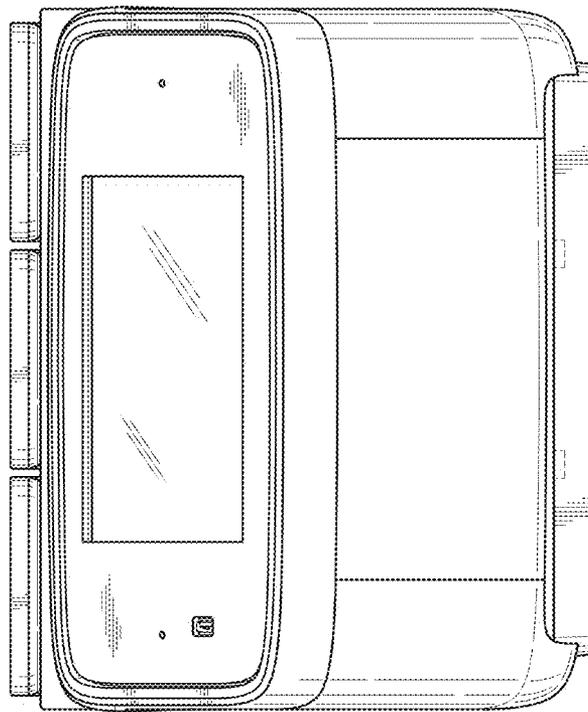


FIG. 2



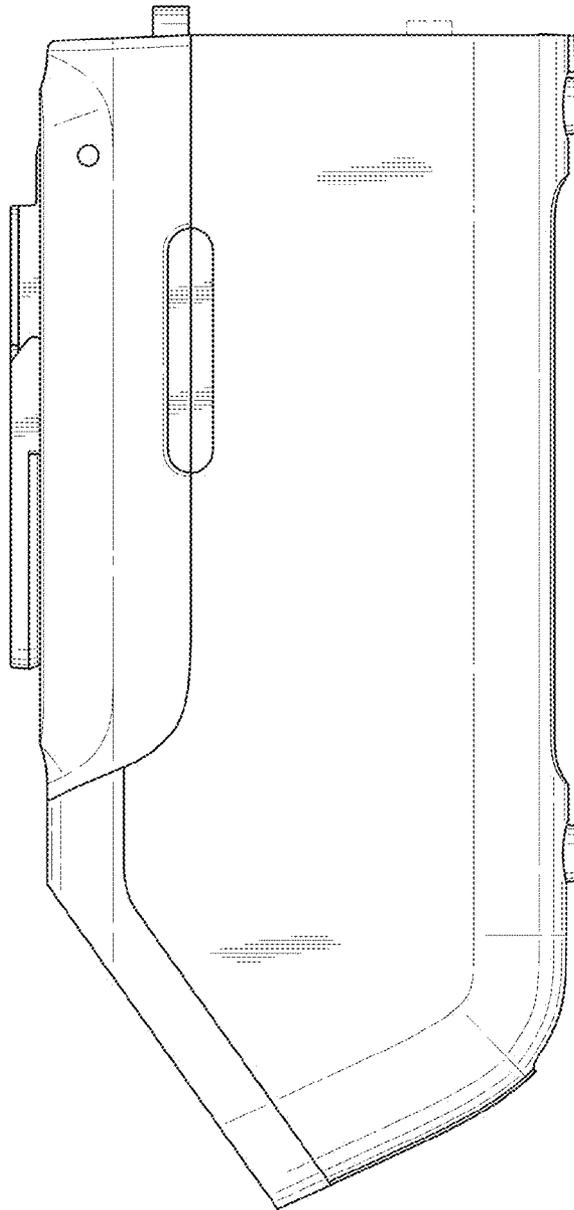


FIG. 4

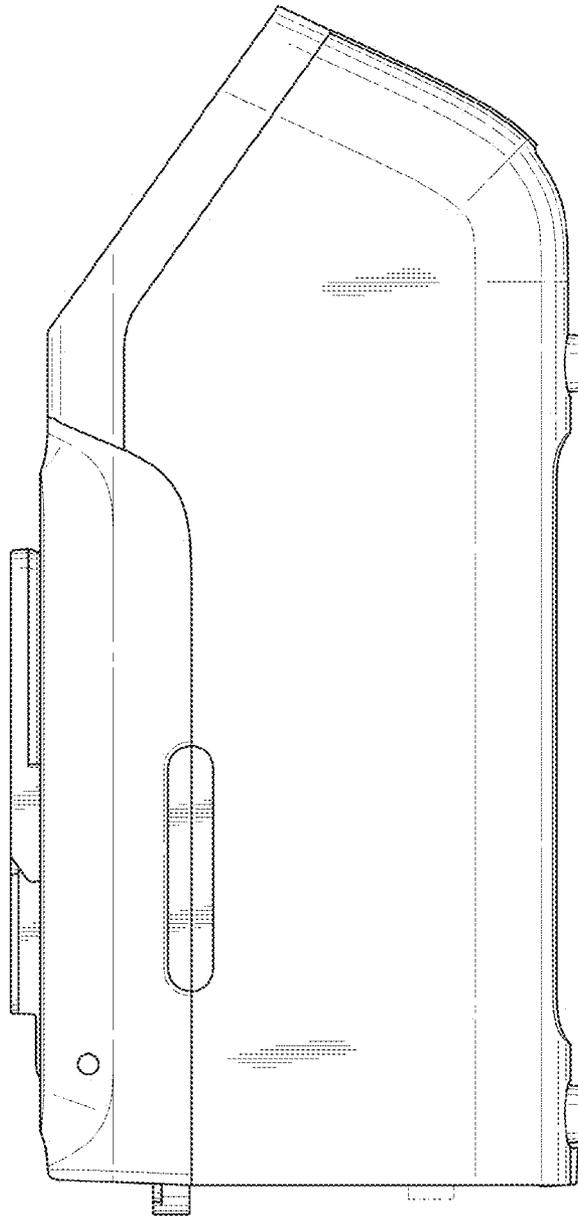


FIG. 5

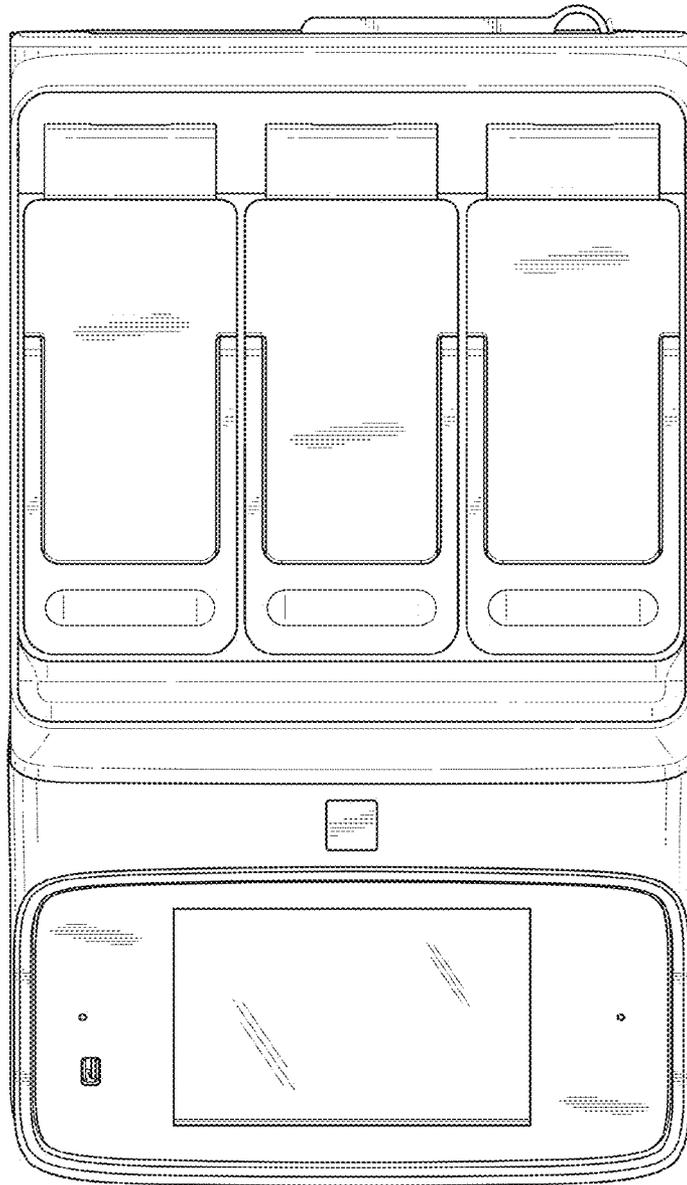


FIG. 6

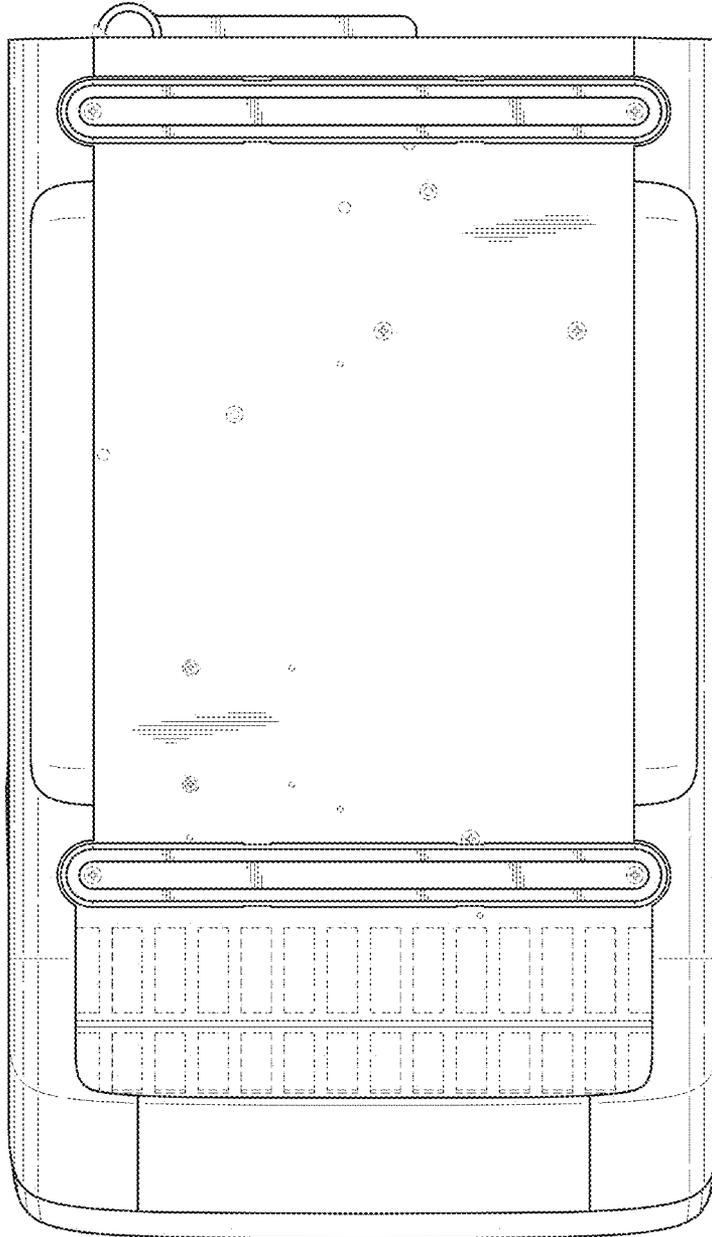


FIG. 7

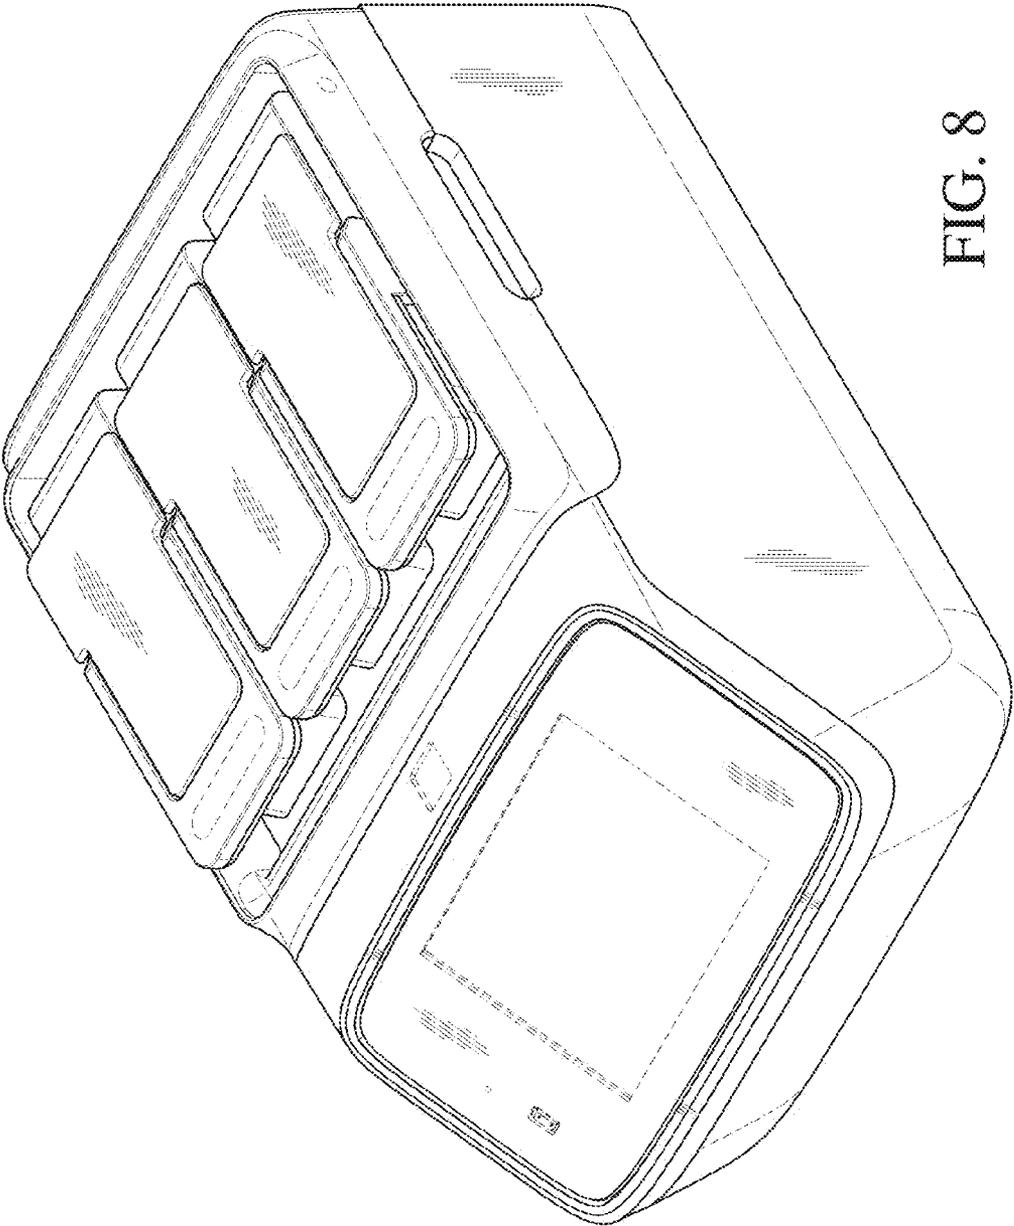


FIG. 8

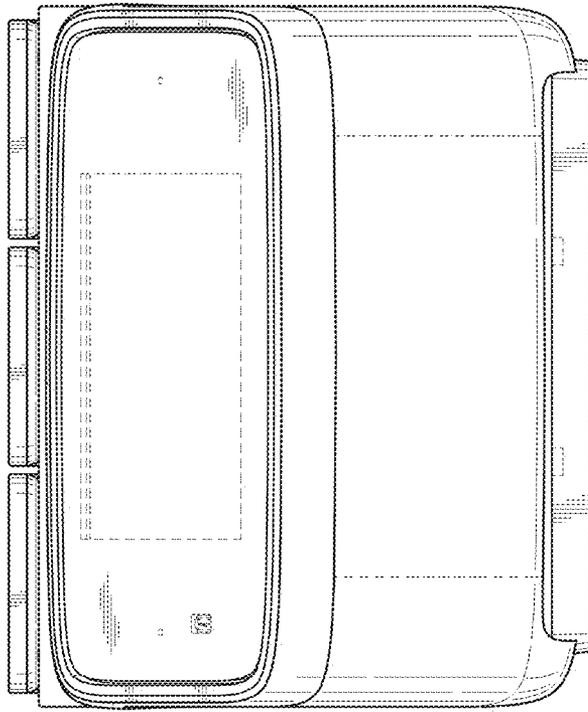


FIG. 9

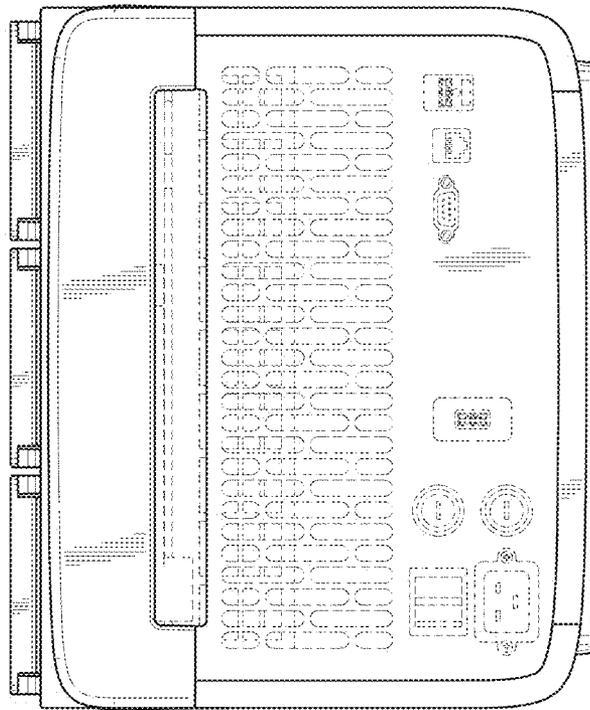


FIG. 10

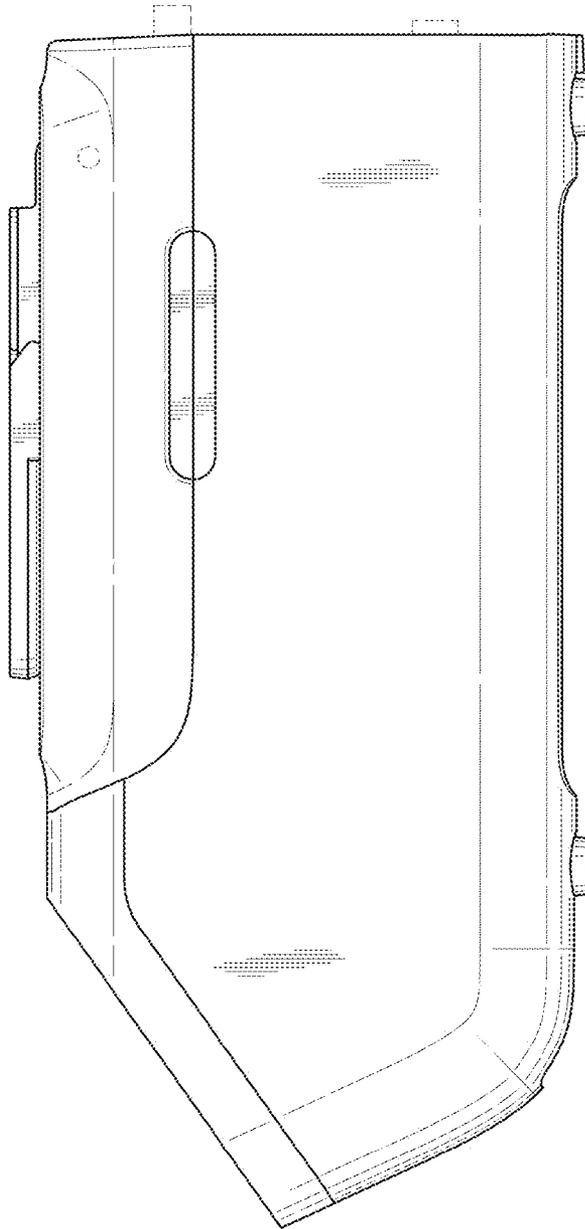


FIG. 11

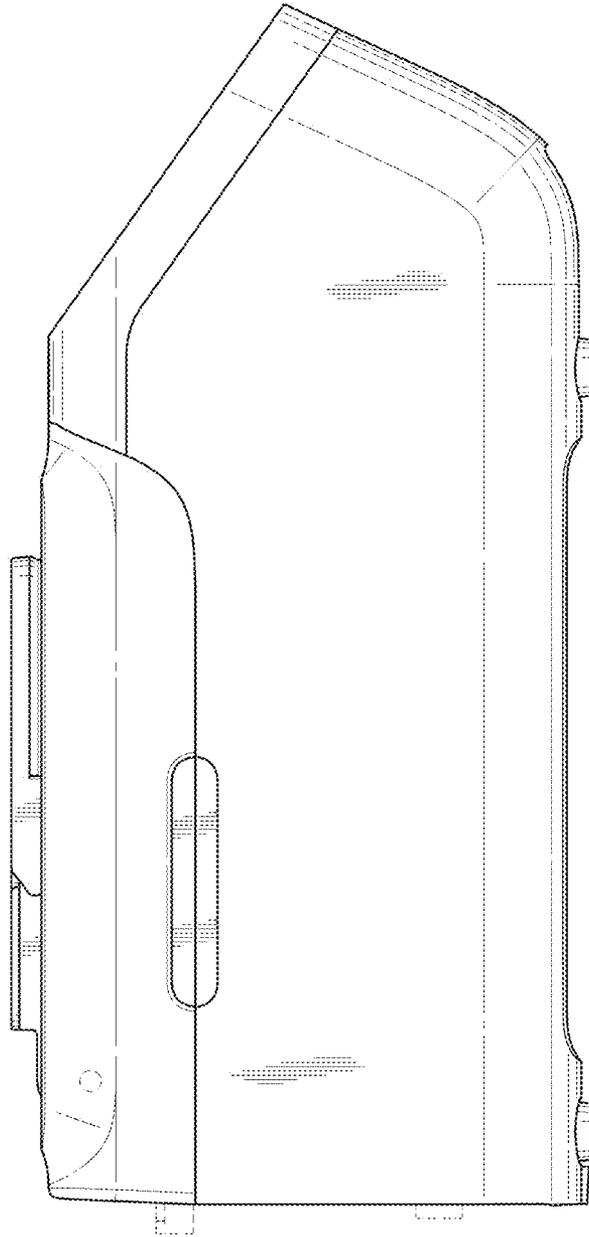


FIG. 12

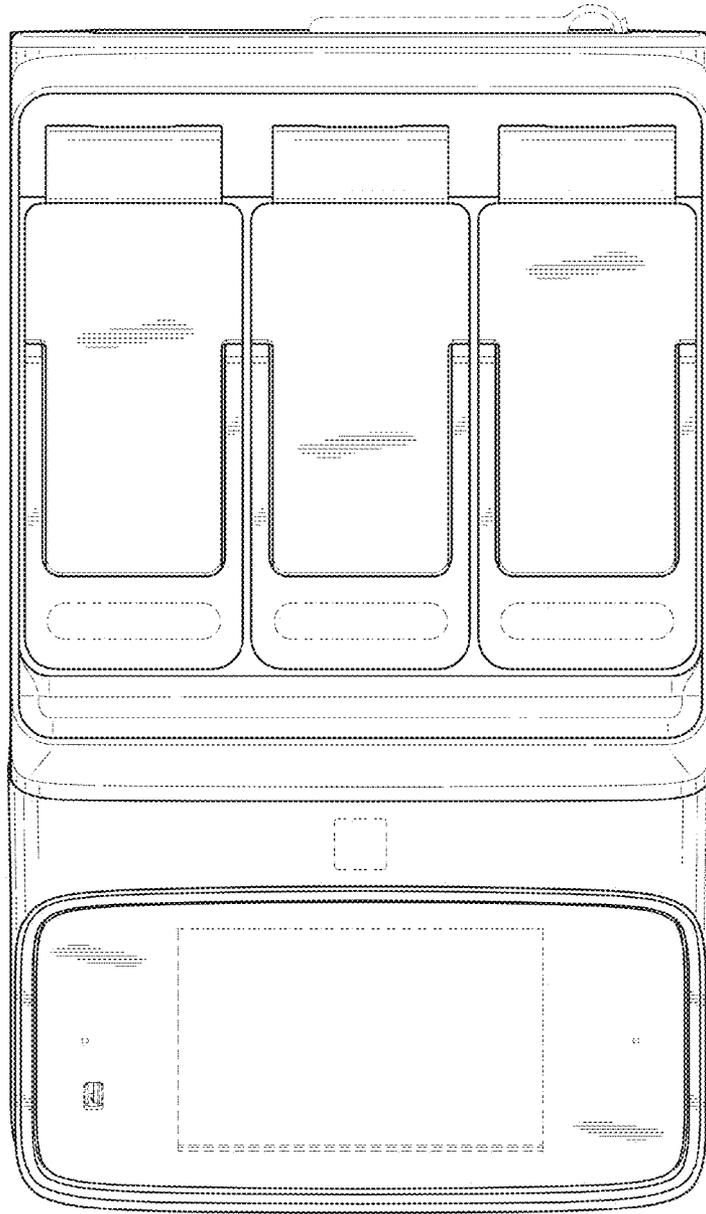


FIG. 13

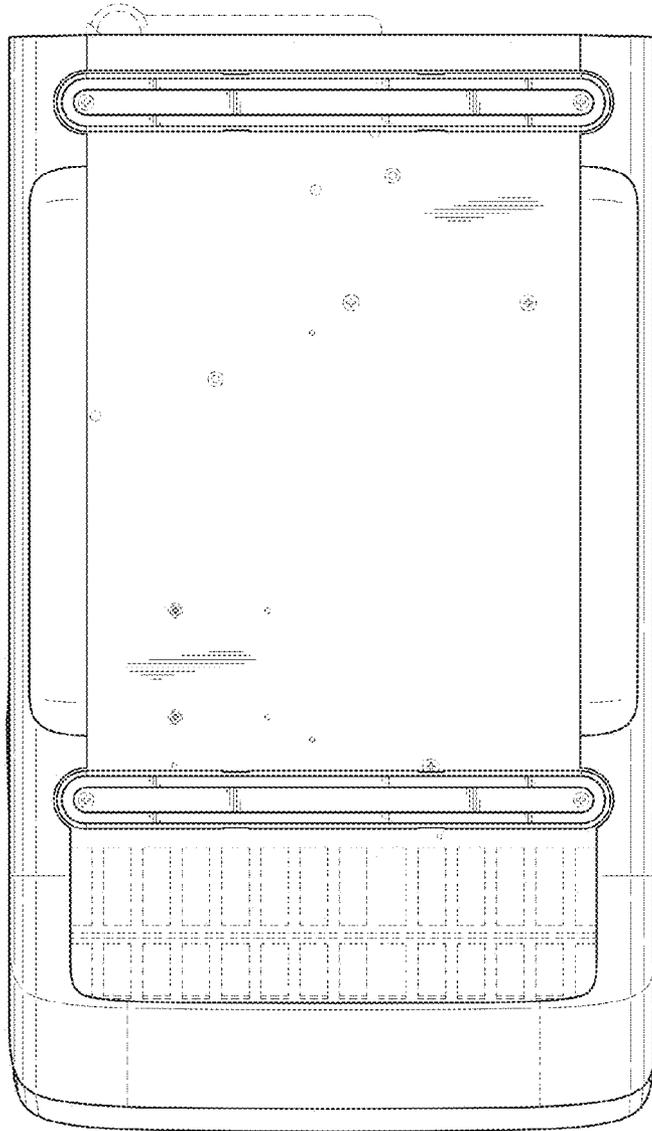


FIG. 14