



US0D1036655S

(12) **United States Design Patent**
Petersen et al.

(10) **Patent No.:** **US D1,036,655 S**
(45) **Date of Patent:** **** Jul. 23, 2024**

(54) **AUTOINJECTOR**

(71) Applicant: **Phillips-Medisize A/S**, Struer (DK)

(72) Inventors: **Carsten Petersen**, Højbjerg (DK); **Emil Wegger Jensen**, Viby J (DK); **Troels Rask Pedersen**, Egå (DK)

(73) Assignee: **Phillips-Medisize A/S**, Struer (DK)

(**) Term: **15 Years**

(21) Appl. No.: **29/840,212**

(22) Filed: **May 26, 2022**

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/113**

(58) **Field of Classification Search**
USPC D24/112–114, 133, 186, 127–131, 144;
D19/115–123, 177, 193
CPC A61M 5/3156; A61M 5/31591; A61M
5/3155; A61M 5/3157; A61M 5/24;
A61M 5/31501; A61M 5/31551; A61M
5/31585

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D696,774	S	*	12/2013	Guarraia	D24/113
D757,255	S	*	5/2016	Wohlfahrt	D24/113
D773,648	S	*	12/2016	Wohlfahrt	D24/113
D773,649	S	*	12/2016	Wohlfahrt	D24/113
D893,021	S	*	8/2020	Dyer	D24/113
D956,212	S	*	6/2022	Petersen	D24/113
D956,214	S	*	6/2022	Petersen	D24/113
D956,960	S	*	7/2022	Petersen	D24/113
D958,972	S	*	7/2022	Neby	D24/113
D965,140	S	*	9/2022	Petersen	D24/113
D1,016,276	S	*	2/2024	Petersen	D24/113

D1,017,028	S	*	3/2024	Petersen	D24/113
2023/0131522	A1	*	4/2023	Lebau	A61M 5/31568 385/123
2023/0132062	A1	*	4/2023	Marsh	A61M 5/3157 604/187

FOREIGN PATENT DOCUMENTS

CN	306812626	*	9/2021
IN	341806-001-0001	*	4/2022
WO	D215207-008	*	10/2021

OTHER PUBLICATIONS

SmartPilot, YpsoMate, [Post date: Oct. 30, 2020], [Site seen Sep. 22, 2023], Seen at URL: <https://yds.ypsomed.com/en/injection-systems/smart-devices/smartpilot-for-ypsomate.html> (Year: 2020).*

(Continued)

Primary Examiner — Natasha Vujcic
Assistant Examiner — Gilbert B Ford


(57) **CLAIM**

The ornamental design for an autoinjector, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an autoinjector showing our new design;
FIG. 2 is a rear perspective view thereof;
FIG. 3 is a front view thereof;
FIG. 4 is a rear view thereof;
FIG. 5 is a left side view thereof;
FIG. 6 is a right side view thereof;
FIG. 7 is a top view thereof; and,
FIG. 8 is a bottom view thereof.
The broken lines depicting the remainder of the autoinjector form no part of the claimed design.

1 Claim, 7 Drawing Sheets

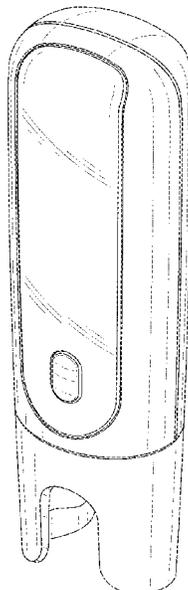

(56)

References Cited

OTHER PUBLICATIONS

UniSafe® 1mL Auto-injector, Owen Mumford, [Post date: Jan. 21, 2022], [Site seen Sep. 22, 2023], Seen at URL: <https://www.ompharmaservices.com/products/unisafe-platform/unisafe-auto-injector/> (Year: 2022).*

“Phillips-Medisize launches smart autoinjector for improve sustainability”, MEDtech news, [Post date: May 26, 2021], [Site seen Sep. 22, 2023], Seen at URL: <https://www.med-technews.com/news/sustainability-in-medtech/phillips-medisize-launches-smart-autoinjector-for-improved-s/> (Year: 2021).*

Aria Smart Injector, Phillips-Medisize, a Molex company, youtube.com, [Post date: Dec. 1, 2022], [Site seen Sep. 22, 2023], Seen at URL: https://www.youtube.com/watch?v=-5_jTv6EUJo (Year: 2022).*

* cited by examiner

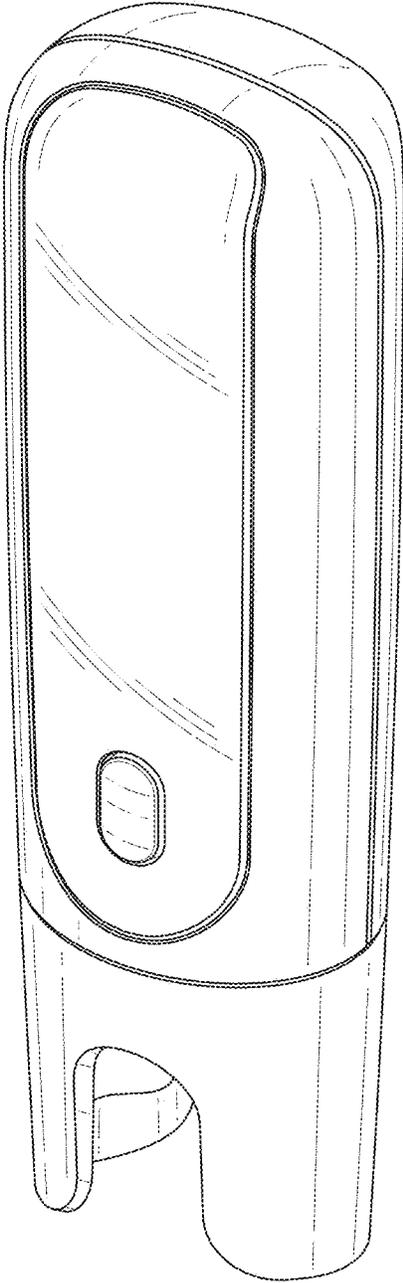


FIG. 1

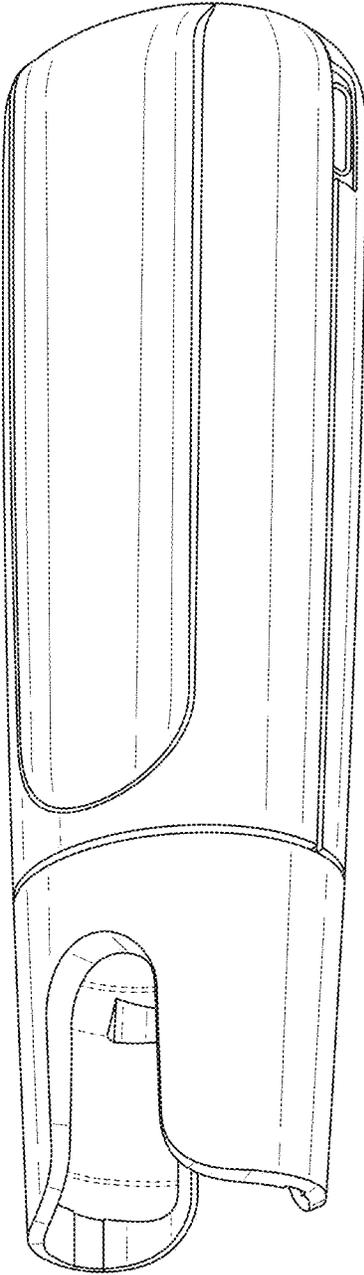


FIG. 2

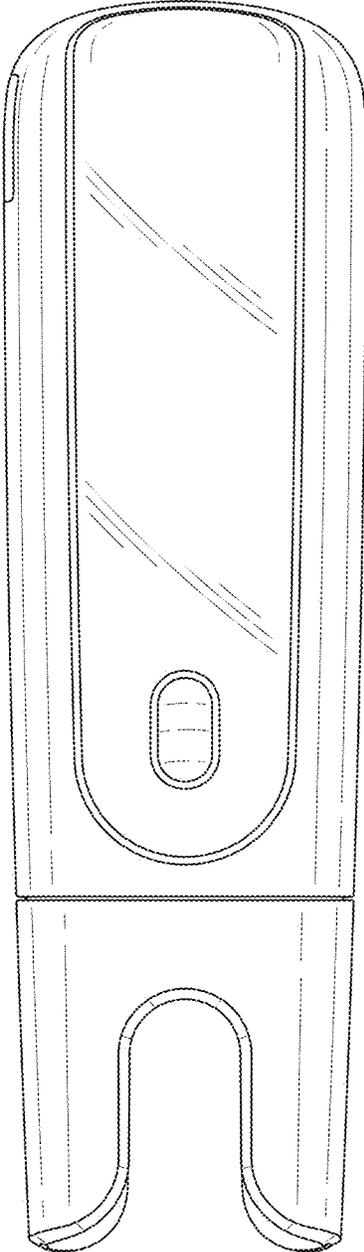


FIG. 3

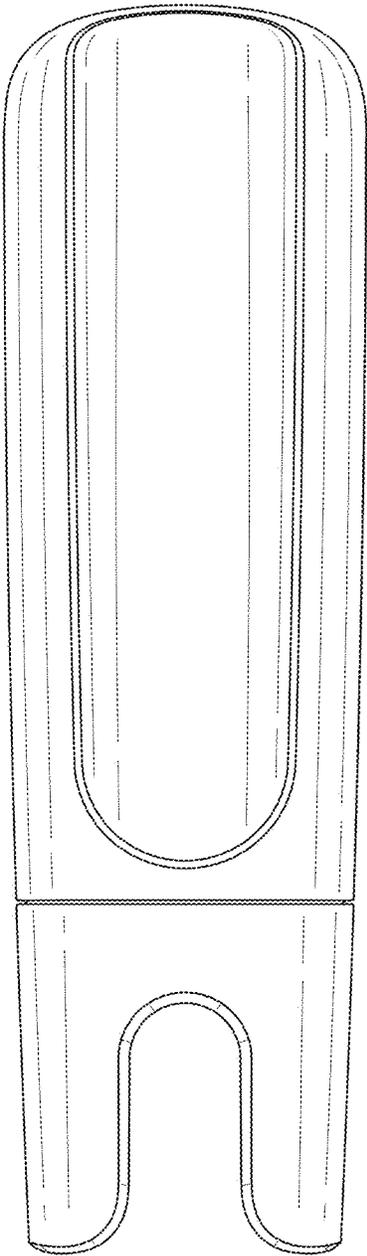


FIG. 4

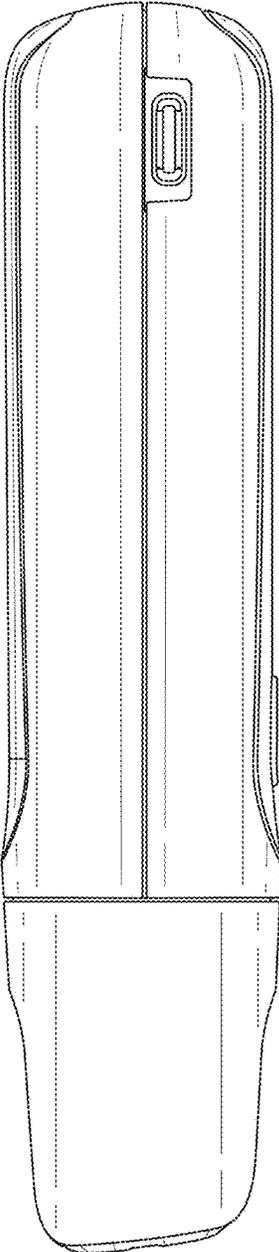


FIG. 5

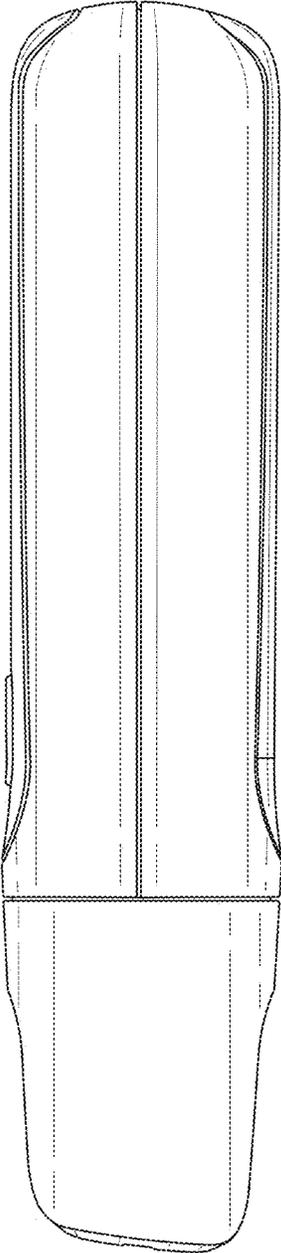


FIG. 6

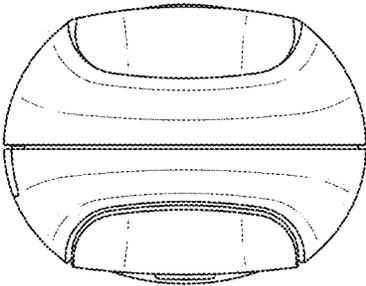


FIG. 7

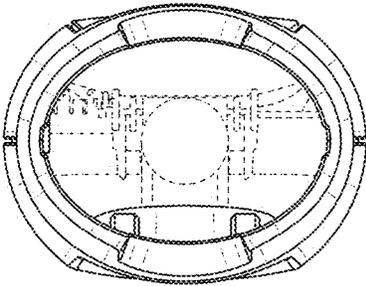


FIG. 8