



US00D920522S

(12) **United States Design Patent**
Funakoshi

(10) **Patent No.:** **US D920,522 S**

(45) **Date of Patent:** **** May 25, 2021**

(54) **TRANSDUCER FOR TREATMENT TOOL
USED IN SURGERY**

(71) Applicant: **OLYMPUS CORPORATION,**
Hachioji (JP)

(72) Inventor: **Yasuo Funakoshi,** Hachioji (JP)

(73) Assignee: **OLYMPUS CORPORATION,** Tokyo
(JP)

(**) Term: **15 Years**

(21) Appl. No.: **29/709,805**

(22) Filed: **Oct. 17, 2019**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/133, 137, 138, 141, 158, 160, 164,
D24/165, 167, 170, 186, 187, 200;
D10/57, 60, 78; D8/82, 83, 107;
D16/243, 245

CPC . A61B 5/0095; A61B 8/4444; A61B 5/02055;
A61B 5/0404; G01S 7/5208

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D160,160 S *	9/1950	Friedman	D24/152
D239,027 S *	3/1976	Knox	D24/129
D256,882 S *	9/1980	Jansson	D8/83
D404,464 S *	1/1999	Niemczyk	D23/233
D429,526 S *	8/2000	Sullivan	D24/133
D467,340 S *	12/2002	Mayer	D24/133
D600,525 S *	9/2009	Meng	D8/86
D641,088 S *	7/2011	Giraud	D24/224
D650,067 S *	12/2011	Py	D24/112

D655,002 S *	2/2012	Bast	D24/133
D655,413 S *	3/2012	Nino	D24/133
D770,609 S *	11/2016	Adams	D24/112
D781,419 S *	3/2017	Bojanowski	D24/144
D782,034 S *	3/2017	Adams	D24/112
D830,538 S *	10/2018	Guillermo	D24/112
D831,834 S *	10/2018	Bader	D24/187
D865,212 S *	10/2019	Kakuda	D24/224
D866,766 S *	11/2019	Cahill	B25B 15/02 D24/171
D912,254 S *	3/2021	Roy	D24/186

FOREIGN PATENT DOCUMENTS

JP	D2017-15789	*	7/2017
JP	D2020-17078	*	8/2020

* cited by examiner

Primary Examiner — Susan Bennett Hattan

Assistant Examiner — Omeed Agilee

(74) *Attorney, Agent, or Firm* — Oliff PLC

(57) **CLAIM**

The ornamental design for a transducer for treatment tool used in surgery, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, right-side perspective view of the transducer for treatment tool used in surgery;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left-side elevational view thereof;

FIG. 5 is a right-side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines depict parts of the transducer for treatment tool used in surgery that form no part of the claimed design.

1 Claim, 3 Drawing Sheets

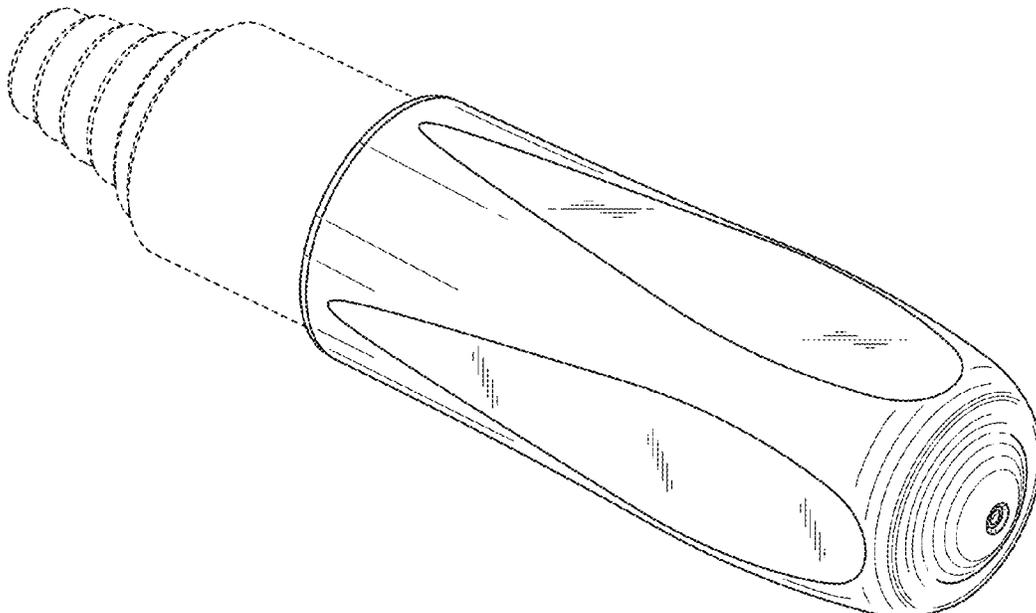


FIG. 1

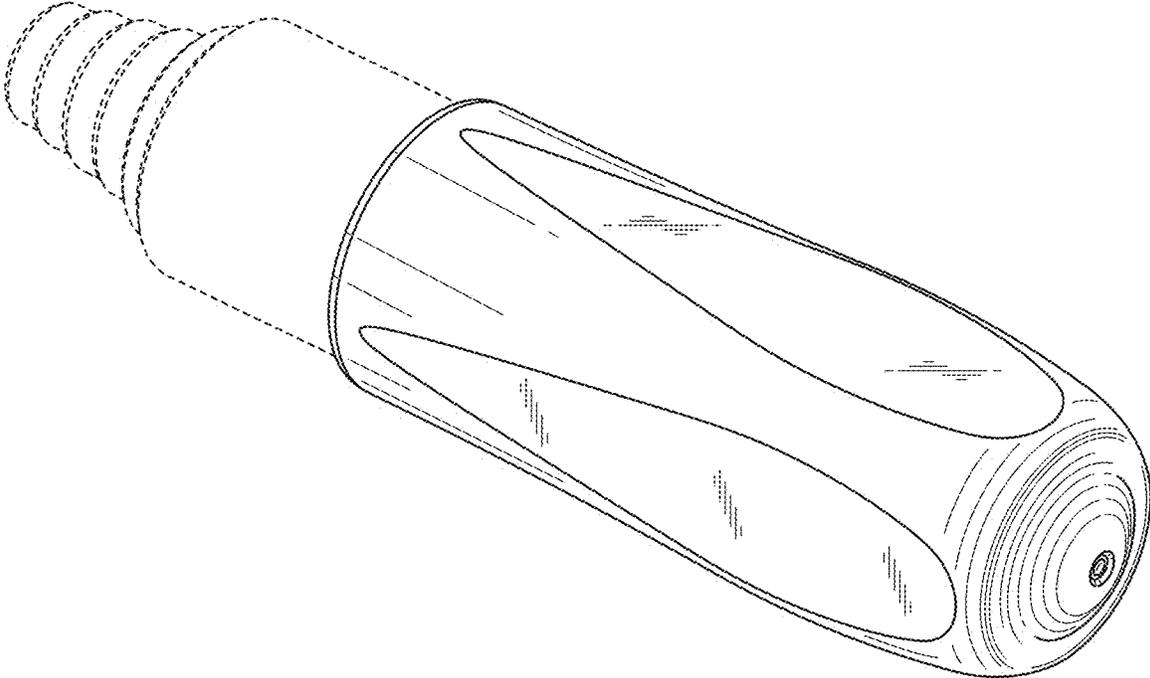


FIG. 2

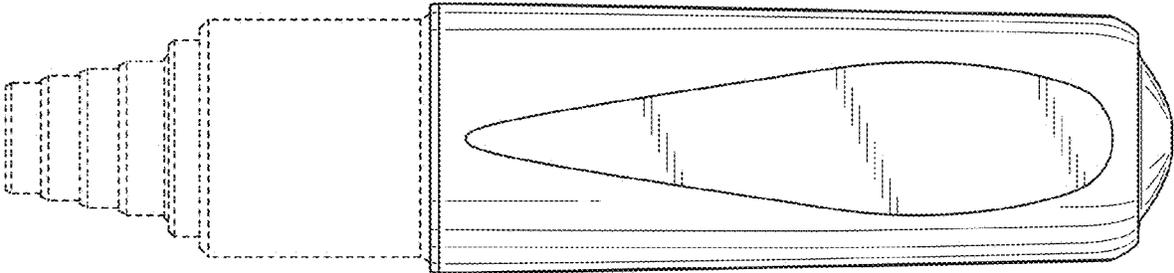


FIG. 3

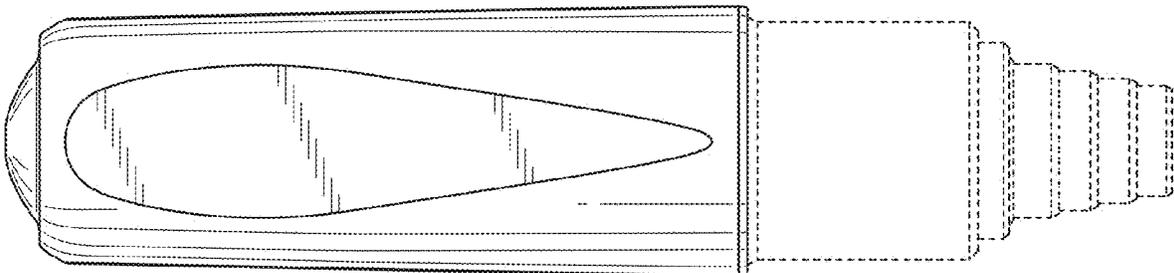


FIG. 4




FIG. 5




FIG. 6

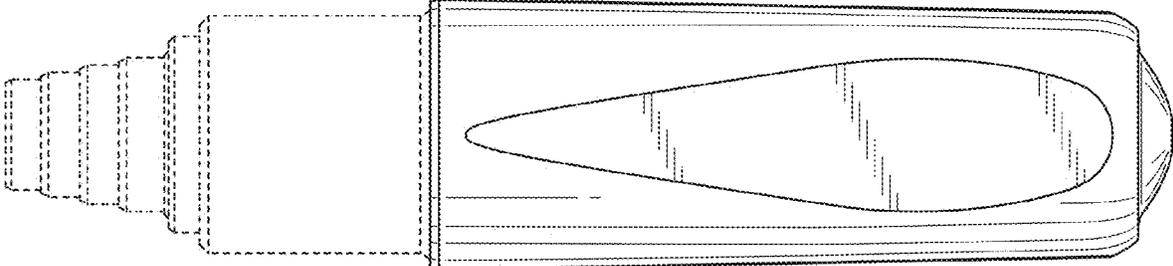


FIG. 7

