



- (51) International Patent Classification:
A61B 17/00 (2006.01) *A61B 1/00* (2006.01)
A61F 2/95 (2013.01)
- (21) International Application Number:
PCT/US2014/017179
- (22) International Filing Date:
19 February 2014 (19.02.2014)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/766,527 19 February 2013 (19.02.2013) US
- (71) Applicant: **BETH ISRAEL DEACONESS MEDICAL CENTER** [US/US]; 330 Brookline Avenue, Boston, MA 02215 (US).
- (72) Inventors: **TSAI, Leo, Lee**; 55 Epping Street, Arlington, MA 02474 (US). **CHEN, Yuyin**; 54 Bishop Allen Drive #2, Cambridge, MA 02139 (US). **RAMANAN, Vyas**; 6 Marie Avenue, Apt 2, Cambridge, MA 02139 (US).
- (74) Agents: **HOOVER, Thomas, O.** et al.; McCarter & English, LLP, 265 Franklin Street, Boston, MA 02110 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,

[Continued on next page]

(54) Title: ADJUSTABLE STIFFNESS CATHETER

(57) Abstract: The application relates to a catheter (10) that has adjustable stiffness that enables a user to select the stiffness of at least one region of the catheter during insertion and navigation through a body lumen. A preferred embodiment of the application works in combination with a guidewire to enable placement of the catheter at a position within the vascular system, for example, to enable treatment of a variety of medical conditions. The catheter can include segments (12, 14, 16, 18) that undergo relative movement in response to actuation by the user to adjust the flexibility of the at least one region, preferably located at or near the distal end of the catheter.

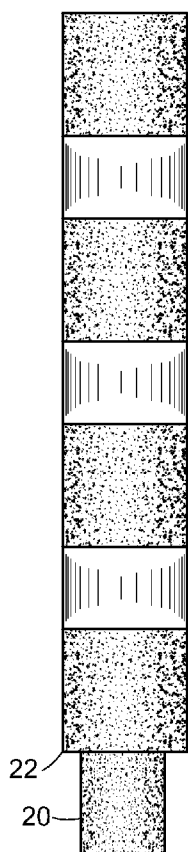


FIG. 1C



HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,

Published:

— *with international search report (Art. 21(3))*

TITLE OF INVENTION
ADJUSTABLE STIFFNESS CATHETER

CROSS REFERENCE TO RELATED APPLICATION

5 This application claims priority to U.S. Provisional Application No. 61/766,527 filed February 19, 2013 entitled ADJUSTABLE STIFFNESS CATHETER, the entire contents of the above application being incorporated herein by reference.

BACKGROUND OF THE INVENTION

10 The present invention relates to variable stiffness catheters and more specifically relates to devices and methods for accessing tubular structures in the body. Existing catheters commonly use a guidewire to aid in the positioning thereof within body lumens for the purpose of delivering medical devices or therapeutic agents to treat a variety of medical conditions. Often, the delivery path within the lumens or vessels of a mammalian body can
15 include regions under 2 mm in diameter and may require the distal end of the device to undergo turns of 90 degrees or more to reach the region requiring treatment. Many vascular applications involving the treatment of strokes, aneurysms, or embolizations, for example, involve navigation through the turns that are required, while catheters that are too flexible may kink and thereby complicate proper placement within the body. There are also risks of
20 vessel perforation or vasospasm in procedures that are frequently time sensitive.

 Many available catheters have fixed variable stiffness in which the proximal end is stiffer than the distal end. This improves the pushability of the device and also allows the distal end to bend at the required angles. Some devices are made with materials that are preshaped, or alternatively, permit steam shaping of the distal end to improve navigational
25 performance. However, existing devices continue to be limited in the capabilities needed to access small remote locations requiring treatment. Thus, a continuing need exists for improvements in catheter design that enable fast and safe delivery of various treatment options within the mammalian body.

SUMMARY OF THE INVENTION

The invention generally relates to a catheter having adjustable stiffness in which the user can select a level of stiffness to enable navigation within lumens of a mammalian body. A preferred embodiment can include a tubular body with at least two portions or layers that are able to move relative to each other. Relative motion of the two portions of the tubular body changes the stiffness of at least one region of the catheter such that the at least one region can bend at an angle relative to the longitudinal axis of the catheter. In a preferred embodiment, each of the plurality of layers can include segments of different lengths, materials, and/or durometer rating.

The catheter can include an inner tube and an outer tube that slide relative to each other by manual actuation. The inner tube has a distal portion with a first plurality of spaced regions having a first stiffness. The spaced regions can be separated by a corresponding plurality of spaced segments having a greater stiffness than the spaced regions. These alternating stiff and flexible elements of the inner tube can be moved longitudinally relative to an outer tube that has alternating segments and regions of differing stiffness. This operates to alter the overall state of flexibility of a distal portion of the catheter. An important metric that reflects this flexibility is the minimum radius of curvature of the flexible portion of the catheter that is associated with a selected relative position of the adjustable catheter elements. For preferred embodiments, the minimum radius of curvature is in a range of 2-6 mm and preferably in a range of 3-5 mm.

A preferred embodiment includes an actuator or switch to change the position of the layers of the tube relative to each other. The actuator can be mounted on a handle positioned at a proximal end of the catheter, which can also include other operative elements to perform selected modes of treatment within the vascular system, for example.

The catheter can include a central lumen having a diameter such that a guidewire can slide into the proximal or distal opening of the catheter lumen.

Thus, preferred embodiments of the present invention provide access to tubular structures in the body with high tortuosity and can be used for accessing vessels that perfuse the central nervous system, the abdomen, the pelvis, the cardiovascular system, the respiratory system, peripheral vessels, the gastrointestinal system, the genitourinary tract and the neurovascular system. The catheter can be inserted into body lumens, or alternatively, by percutaneous entry with an introducer.

Preferred embodiments of the invention can include a plurality of treatment devices and methods that can be delivered to anatomic sites within the human or animal body. Devices for treatment of the vascular system can include stents, filters and/or balloon devices, for example. Medications can be delivered with the catheter through one or more channels within the catheter or in combination with the above referenced devices. The handle can include one or more side ports to introduce devices and or medications.

Preferred embodiments of the invention also relate to methods of manufacturing adjustable stiffness catheters. The inner and outer tubes can be made with a coiled or braided structure. A preferred embodiment can include steps of forming annular segments of differing stiffness, arranging the segments in a selected order, and heating the segments to thereby form the inner and outer tubes such that the segments are arranged to provide the desired range of flexibility.

Other objects and advantages of the present invention will become apparent to the reader, and it is intended that these objects and advantages are within the scope of the present invention. To the accomplishment of the above and related objects, this invention may be embodied in the form illustrated in the accompanying drawings, attention being called to the fact, however, that the drawings are illustrative only, and that changes may be made in the specific construction illustrated and described within the scope of this application.

BRIEF DESCRIPTION OF THE DRAWINGS

Figs. 1A- 1D are side views of flexible and rigid states, respectively, of preferred embodiments of the present invention;

Figs. 2A-2B are side views of flexible and rigid states of a catheter body in accordance with the present invention;

Figs. 2C-2F illustrate a process of advancing the catheter through a series of branching features of a lumen system to a treatment site;

Figs. 3A-3B are partial cutaway perspective views of an actuator such as a sliding switch to adjust between flexible and stiff states in accordance with the present invention;

Figs. 4A-4I illustrate embodiments of a sliding two-layer system for an adjustable stiffness catheter in accordance with preferred embodiments of the invention;

Figs. 4J-4K illustrate a spring-operated actuator in accordance with certain embodiments of the invention;

Figs. 5-9 illustrate sectional views of methods of forming catheters in accordance with preferred embodiments of the invention;

5 Figs. 10-14 are process sequence diagrams of methods for fabricating adjustable stiffness catheters in accordance with preferred embodiments of the invention;

Figs. 15A-15B illustrate side cutaway views of a catheter according to certain embodiments of the present disclosure;

10 Figs. 16A-16C illustrate side cutaway views of a catheter according to certain embodiments of the present disclosure;

Fig. 17 illustrate a side view of a catheter including a balloon treatment device according to certain embodiments;

Figs. 18A-18C illustrate side cutaway views of a catheter used to deliver a stent to a treatment site according to certain embodiments of the present disclosure;

15 Figs. 19A-19C illustrate a method of positioning a second catheter or treatment device using various embodiments of the present invention;

Fig. 20 illustrates a side cutaway view of a catheter with a handle region according to certain;

20 Figs. 21A-21D illustrate components of an actuator in a handle region of a catheter according to certain embodiments; and

Figs. 22A-22B illustrate side cutaway views of catheters incorporating lubricious coatings, according to various embodiments.

DETAILED DESCRIPTION OF THE INVENTION

25 Turning now to a description of the drawings, in which similar reference characters denote similar elements throughout the several views, Figs. 1A-1D illustrate a tube 10 with at least two layers 20,22 that are able to slide past each other, each of which includes a plurality of segments 12,14 and 16,18 that can have different lengths, materials, and/or durometer rating. The device 10 can further comprise an actuator such
30 as a mechanical switch, to change the relative positioning of the layers of the tube relative to each other.

The outer tube layer 22 can have segments 16,18 of different lengths, materials, and/or durometer ratings. In the preferred embodiment, the outer layer 22 comprises two

alternating segments 16,18, each with its own characteristic length, material(s), and durometer ratings. In some embodiments, the length of the segment with higher durometer rating 18 will be greater than that of the segment with the lower durometer rating 16.

5 Segment materials can comprise (but are not limited to) FEP, PFA, Pebax, polyurethane, nylon, PVC, TPE, polyester. The catheter elements may be formed by methods including, but not limited to, extrusion or casting. Segment or layer reinforcing material may include a metal such as, but not limited to, 304 SS, 316 SS, and/or monofilament materials.

10 The segments may be of appropriate length, be made of appropriate material(s), and have any appropriate durometer rating required for a given application. Catheters having lengths ranging from 10 cm to 2 m, and diameters of less than 1 mm to more than 10 mm, can be made in accordance with preferred embodiments of the invention. Small diameter guide catheters can be less than 2 mm in diameter in the distal region and
15 preferably less than 1 mm.

 The outer layer 22 can comprise two types of segments (each with a characteristic length, material composition, durometer rating) that alternate. It can also comprise selected combinations of different segments. The length of the segment with higher durometer rating (18) can be greater than, equal to, or less than that of the segment with
20 the lower durometer rating (16).

 The inner tube layer 20 has segments of different lengths, materials, and/or durometer ratings. In the preferred embodiment, the outer layer comprises two alternating segments 12 and 14, each with its own characteristic length, material(s), and/or durometer ratings. The length of the segment with higher durometer rating (12) can be greater than
25 that of the segment with the lower durometer rating (14). The length of segment 12 can equal that of 18 and the length of segment 14 can equal that of 16, for example.

 Segment materials can comprise, but are not limited to, FEP, PFA, pebax, polyurethane, nylon, PVC, TPE, polyester. The catheter may be formed by methods including, but not limited to, extrusion or casting. Segment reinforcing material may
30 include a metal, nitinol, or specifically stainless steel, such as, but not limited to: 304 SS, 316 SS, or can comprise one or more monofilaments. Thus, one or more components of the catheter can comprise a shape memory material. The catheter can include a curved distal tip to assist with steering of the device.

The inner layer 20 can comprise two types of segments (each with a characteristic length, material composition, durometer rating) that alternate. It may also comprise a combination of any number of different segments. The length of the segment with higher durometer rating (12) can be greater than, equal to, or less than that of the segment with the lower durometer rating (14).

The inner layer 20 can also take the form of a wire instead of a tube where the application does not require a central lumen for a guidewire or to provide a port for insertion of fluids such as a flushing liquid, or for delivery of medication, or to introduce other tools or devices through, or with, the catheter.

An actuator used for adjusting catheter stiffening can comprise a sliding device that allows the inner and outer layers of the tube to be switched from a position in which segments 12 and 18 are in register and 14 and 16 are in register, to a position in which they are out of register where the segment 12 bridges the gap between adjacent segments 18 (Fig. 1D). In the in-register state (Fig. 1B), the flexibility of the overall tube is dictated by the less stiff segments 14 and 16. In the out of-register state, the flexibility of the overall tube is dictated by the more stiff segments 12 and 18.

As shown in Figs. 2A and 2B, the catheter body 10 can have a flexible region 40 in which segments are registered such that the flexible region 40 can bend along a selected radius of curvature R. The catheter 10 can include a handle 52 mounted at a proximal end that can have a plurality of actuators, buttons, or switches 58 that are operative to change the flexibility of all or a portion of the catheter. A slider element can also be used to advance a guidewire 56 that can be inserted into a central lumen of the catheter. The guidewire 56 can have a distal hook, or “J” shaped distal end, that can allow the user to select one of a plurality of branches of an arterial system. The guidewire can be used with the adjustable catheter to navigate the many branches of the neurovascular system, for example, to deliver treatment or aid in the imaging of a particular treatment site. A fluid source 54 can be used to deliver a fluid such as a contrast agent, a medication, nutrients, electrolytes, blood products, chemotherapy agents or radiotherapy agents, for example. As shown in Fig. 2B, the catheter in its more rigid state has limited flexibility and is generally aligned along its longitudinal axis 50. The catheter 10 can include a device 55, such as a stent or balloon, which can be positioned with the catheter at a treatment site. Fluoroscopic markers 57 can be included to aid in visualization.

However, as illustrated in the sequence of Figs. 2C-2F, the catheter is used to bend in different directions where the more flexible state is used to initiate turns and a more rigid state to advance along more linear regions of a lumen system. Note that the catheter can simply switch back and forth between two states (rigid and flexible) or alternatively, the user can select a level of stiffness from a continuum of available levels depending on the sizes and locations of the second, third, or fourth degree turns that can be encountered, as illustrated in Fig. 2C. The catheter can be initially stiff upon percutaneous introductions, is adjusted to a flexible state at the first turn (Fig. 2D) is made rigid while advancing to the next turn (Fig. 2E) and made flexible to initiate the second turn at Fig. 2F. This process is continued through the third and fourth turns, as needed, to reach the treatment site.

As shown in Figs. 3A-3B, an actuator such as a slider switch device 60 can comprise a base 26 that can slide relative to the outer layer 28 wherein the user can manually engage the slider element 60 that is connected to the outer layer 28 (see Figs. 4J-4K, hereinafter, for example).

The inner and outer layers 20,22 of the tube 10 are concentric and can slide past each other in this embodiment. The switch 60 is connected to the two layers 20,22 of the tube, with the base connected to the inner layer 20 of the tube, and a slider 60 connected to the outer layer of the tube. This switch 60 allows the outer layer to slide longitudinally over the inner layer.

The tube 10 is comprised of inner and outer layers 20,22, each consisting of alternating flexible segments of length x and semi-rigid segments of length y . The inner and outer layers 20,22 of the tube 10 can comprise either two concentric tubes with differing radii, or a combination of a tube and wire. The alternating segments can be made of materials, have a selected thickness, have a selected tensile strength, and have a selected shear modulus to achieve the desired thickness and radius of curvature required for a given application. The inner and outer layers 20,22 will move longitudinally against each other in a controlled manner, via a mechanical switching device. When the alternating stiff and flexible segments of the inner and outer layers of the catheter tube are in register, the catheter tube is in a "relaxed" flexible state. When the segments are out of register, the rigid segments of the inner and outer layers overlap with each other and the catheter tube stiffens to achieve a more rigid state.

In the preferred embodiment, the tube is a diagnostic microcatheter with walls strong enough to handle high pressure injections of intravascular radio-opaque contrast. The lengths x and y are 1-5mm, with $y > x$. The microcatheter is used to navigate second and third order vessels within patients during interventional radiological, cardiac, or surgical procedures. Figs. 4A-4I show different embodiments in which different segments of the two layers comprise different materials, have different lengths, or register in differing combinations to achieve different bending characteristics. As shown in Figs. 4J-4K, the proximal end 100 of the catheter can comprise a handle in which a proximal stop 110 can be used with a thumb knob 104 and one or more spring elements 102 to actuate relative movement between the two layers 20, 22. This can be used with a guidewire positioned within central lumen 120 to manipulate the distal end of the catheter through a sequence of turns in which a physician can navigate through interconnected lumens within the body.

In another preferred embodiment, a catheter layer 200, shown in Fig. 5, can comprise a variable pitch coil 202 mounted on an inner tube or liner 204 and covered with an outer polymer 206 to provide a flexible region 40, surrounded by stiffer regions 208, 210. Thus, the layer 200 can include a plurality of alternating segments of higher and lower stiffness. A second layer having an identical structure, except with a larger diameter, can be paired with layer 200 which is inserted within the second layer as described herein to form a flexible catheter that can be adjusted so that the alternating flexible and stiff regions can either be aligned with each other, or moved out of alignment, to provide a flexible or more rigid structure, respectively. Note that the stiffness of each segment can be selected by adjusting the pitch, or number of windings, within a given segment. Thus, stiff regions have a greater pitch and flexible regions have a smaller pitch.

In a preferred method of making a catheter having adjustable stiffness as shown in Fig. 6, an inner liner 304 can be mounted with a coil braid 302. Grinding wheels 310 can form intervals to form alternating stiff and flexible regions. Another preferred method shown in Fig. 7 first forms a polymer layer 360 around an inner liner 350. Grinding wheels can form spaces and a second polymer layer 362 can be deposited in the spaces to form a composite structure of alternating segments.

In Fig. 8, another preferred method of fabrication selectively deposits a polymer 402 to form segments on liner 400. A third polymer layer 404 can be formed and ground

with grinding element 420 to form alternating stiff 422 and flexible 424 regions. In Fig. 9, stiff 452 and flexible tubes 454 can be positioned along a liner 450 which are then coated with an outer polymer 460 to secure the segments in place.

Shown in Figs. 10-14 are process sequences illustrating steps for fabricating catheters in connection with preferred embodiments of the invention. In Fig. 10, the process 500 includes mounting a liner on a mandrel 502, mounting coil elements with different pitches 504, bonding these the liner 506, overlaying additional polymer layers 508, 510, assembling the different layers 512, and connecting the 514 actuator.

In the method 600 of Fig. 11, a layer is formed on a mandrel 602, form a braid or coil 604 and bonding thereof to a liner 606. A second polymer is overlayed 610, followed by an optional third layer 612. An outer tube is formed 614 and connected to a handle 616. A centerless grinding tool can be used to remove portions 608 of material to form segments. In the method 700 of Fig. 12, grooves formed by centerless grinding 706, for example, can be filled with a polymer of lower durometer 708 to form alternating segments of different durometers in a given layer. This is followed by outer catheter fabrication 712 and connection to a catheter hub or handle 714. In the method 800 of Fig. 13, with steps 802 and 804 followed by an overlying layer formed 806 with a third polymer can be formed over adjacent segments of different durometers along with steps 808, 810 and 812. In the method 900 of Fig. 14, two polymer layers can be formed 902, 904 on the same mandrel and then cut to selected lengths 906 for mounting on a selected liner in alternating fashion 908. These segments can then be secured in place with a third polymer layer or adhesive or a heat shrink material to secure the segments in place 910, 912 and 914.

Current vascular catheters and wires generally employ a different technique to engage second- or third-order vessels. A common problem occurs when small tortuous vessels prevent a catheter from being advanced because of sharp turns. This step is often the most time-intensive and unpredictable component of a procedure. Failure to advance is often due to the catheter being too soft and unable to traverse a sharp bend over a wire, or too stiff, causing the catheter and wire to disengage from the target vessel altogether. Ideally, an advancing catheter needs to be flexible when making initial sharp turns, but stiff enough to allow effective advancement into the vessel to obtain enough purchase for either further advancement or deployment of contrast materials, medication, or therapeutic devices.

The present invention is useful for any application that requires the operator to navigate a tube through a torturous tubular structure in the body. Preferred embodiments comprise vascular microcatheters, which can be used for procedures ranging from thrombolysis of cerebral artery occlusions to the coiling of bleeding mesenteric arteries.

5 However, the invention provides a suitable solution to similar problems found in endoscopic procedures involving the GI and GU tracts as well as solving problems that frequently occur in cardiac procedures involving intravascular ultrasound catheters. Finally, simple and robust variable-stiffness catheters may also be in industrial applications involving drilling and exploration.

10 The catheters of the present disclosure can be used in a variety of different diagnostic and therapeutic procedures. For example, in certain embodiments, the catheters of the present disclosure can be used to sample or delivery fluids to selected anatomic sites. Examples of various diagnostic and therapeutic procedures that may be performed using fluids delivered or obtained through the catheters can include adrenal vein
15 sampling: (e.g., sampling blood from several veins surrounding the adrenal glands in order to determine levels of aldosterone; neurovascular (including carotid, cerebral, and spinal vessels) diagnostic or therapeutic procedures; injection of thrombolytics to break up clots for ischemia treatment; contrast or MR angiography used to identify peripheral vascular disease and plan for future surgical intervention; catheter-based imaging of
20 mesenteric artery to detect or rule out aneurysm, thrombosis, ischemia, or to locate the source of gastrointestinal bleeding; detection of portal hypertension and cirrhosis; imaging of the celiac artery to detect or rule out aneurysm, thrombosis, ischemia, or to locate the source of gastrointestinal bleeding; confirmation or detection of vascular anatomy and patency of hepatic vasculature prior to surgical intervention, for example for
25 liver transplant; catheter-based delivery of contrast for gastric, pancreaticoduodenal, splenic, renal, thoracic, intercostal, coronary, or pulmonary angiography catheter-based delivery of contrast into biliary tree for imaging the biliary network; selective catheter angiography to identify anastomoses for percutaneous transluminal angioplasty (PTA) or surgical repair and/or selective catheter angiography to identify
30 anastomoses for PTA or surgical repair; catheter-based injection of contrast agents for imaging lymph vessels to detect cancer metastasis; and/or injection of radiocontrast agents into the urinary tract for diagnostic imaging

In other embodiments, solids can be delivered using the devices of the present disclosure. As discussed further below, smaller solid agents can be delivered directly by removing the guidewire and then introducing the agents through the microcatheter. For larger agents, however, the inner layer 20 may be removed to increase the inner diameter of the system. The devices of the present disclosure can be used to deliver embospheres (20 μ m to 2000 μ m, or .0008" to .008"), coils (0.01" to 0.4"), gelfoam (variable, typically ~0.25"), or mechanical thrombectomy devices (stentriever). At the 3 French OD scale, agents up to .018" can be delivered without removing the inner catheter, and for larger agents the inner layer may be removed. As examples, the devices of the present disclosure can be used for neurovascular aneurysm coiling, including aneurysms within the circle of Willis, cerebral arteries (posterior, anterior, and middle, up to 2nd order branches), and spinal vessels (aneurysm sizes 2-20 mm); transhepatic arterial chemoembolization (same requirements as hepatic arteries) for tumors; coiling or embolization of hepatic arteries; embolization of gastric artery to prevent aneurysm rupture or to cut off blood supply to a portion of the stomach producing the hormone ghrelin, which can lead to decreased feeding and weight loss in obese individuals; splenic artery coiling/embolization for aneurysms or pseudoaneurysms (aneurysm sizes 5-20 mm); gastroduodenal arterial coiling (aneurysm sizes 3- 15 mm) for pseudoaneurysms; superior mesenteric artery embolization/coiling for aneurysms/pseudoaneurysms; mesenteric artery branch embolization/coiling for small bowel bleeding; colonic (right, middle, left) artery branch embolization or coiling for GI bleeding; rectal artery branch embolization or coiling for bleeding; uterine artery branch embolization or coiling (for uterine fibroids, uterine bleeding); pulmonary arterial embolization for treatment of pulmonary arteriovenous malformations, aneurysm, or bleeds; and lymphatic or thoracic duct coiling to prevent leakage of lymphatic fluids into the thoracic duct by selectively blocking the leaking vessels.

The devices of the present disclosure can further be used to deliver various therapeutic agents or therapies. As examples, the devices can be used for venous sclerosing treatments to selectively deliver sclerosing agents or fiber optic lasers to specific varicose veins in order to target their dissolution. Furthermore, the devices can be used to retrieve objects within a body lumen, include stents, thrombotic filters, unwanted foreign bodies, or instruments accidentally dislodged during surgical or radiological procedures.

In addition, in certain embodiments, the devices of the present disclosure can be fitted with a camera to be placed into a vessel or other cavity in order to image the area in question. Since cameras must fit within the inner diameter of the assembly (or the inner diameter of the outer catheter), these procedures may require slightly larger catheter systems, perhaps up to 5 French. Visualization using optical cameras may be employed in GI/Biliary applications

imaging of the esophagus, stomach, and proximal small bowel; colonoscopy; ERCP (endoscopic retrograde cholangiopancreatography); laparoscopic procedures; mediastinoscopy; rhinoscopy, otoscopy; laryngoscopy; bronchoscopy; neurosurgical scoping; urological procedures; cystoscopy; ureteroscopy; prostatectomies; colposcopy; hysteroscopy; fallopscopy; and arthroscopy or visualization of any joint or musculoskeletal structure. In addition, the devices of the present disclosure may be used to drain or place tubes in various anatomic sites including, urinary catheters; urethral or bladder catheters; percutaneous nephrostomy tubes; abdominal/pelvic cavity tubes; general drains for abscesses or fluid collections; chest tubes; thoracostomy tubes; devices for paracentesis or thoracentesis; neurological devices; and ventriculostomy devices.

The devices of the present disclosure can be used in a variety of angioplasty or stenting procedures, including, but not limited to carotid stenting or angioplasty; vertebral artery stenting or angioplasty; spinal artery angioplasty; peripheral vascular stenting or angioplasty (lower or upper extremity); superior mesenteric artery stenting or angioplasty; celiac stenting or angioplasty; hepatic artery stenting or angioplasty; arteriovenous graft angioplasty; vascular anastomoses stenting or angioplasty (hepatic artery, vein, portal vein, renal artery, mesenteric artery anastomoses for transplants); biliary ballooning or stenting; pancreatic duct ballooning or stenting; esophageal ballooning or stenting; duodenal ballooning or stenting; colonic ballooning or stenting; and urinary tract stenting or ballooning

A variety of different sizes and configurations of devices can be selected depending on the specific clinical application. It should be appreciated that the specific size and configuration may vary based on patient-specific factors, clinical situations, and/or clinician preference. Table 1, however, provides typical specifications for various applications, including an expected radius of curvature that the device should obtain for effective use. The presently disclosed devices provide advantages in that they can be

produced with a range of sizes and shapes to provide systems for treatment of many different anatomic sites and conditions, and can be scaled to allow for a desired radius of curvature, which may be a critical factor in determining whether or not the device can reach a target site.

5 Table 1: Typical device specifications.

Type of vessel/technique	Req. catheter size	Req. tip length	Min. radius of curvature	Vessel diameter
Adrenal vein sampling	2-4 Fr	3-5 cm	3 mm	2-7 mm
Neurovascular	1.5-4 Fr	1-10 cm	5 mm	
Upper and lower extremity	1.5-6 Fr	1-10 cm	5 mm	
Mesenteric artery	2-4 Fr	1-10 cm	5 mm	
Celiac trunk	3-5 Fr	1-10 cm	5 mm	
Hepatic arteries/veins	2-4 Fr	1-10 cm	5 mm	
Gastric arteries	2-4 Fr	1-10 cm	5 mm	
Pancreaticoduodenal arteries	2-4 Fr	1-10 cm	5 mm	
Splenic arteries	2-4 Fr	1-10 cm	5 mm	
Renal arteries or veins	2-4 Fr	1-10 cm	5 mm	
Thoracic or intercostal arteries	2-4 Fr	1-10 cm	5 mm	
Pulmonary arteries and veins	2-6 Fr	1-5 cm	5 mm	
Coronary arteries	1.5-3 Fr	0.5-5 cm	3 mm	
Arterial anastomoses	2-4 Fr	1-10 cm	3 mm	
Bile duct anastomoses	2-10 Fr	1-15 cm	5 mm	
Bile duct cholangiogram	2-8 Fr	1-10 cm	3 mm	
Bowel anastomoses	4-16 Fr	5-20 cm	10 mm	
Lymphangiography	1.8-4 Fr	1-10 cm	5 mm	
Urinary tract imaging	2-10 Fr	1-10 cm	5 mm	

AV graft angioplasty	2-5 Fr	1-10 cm	5 mm	
EGD	4-20 Fr	5-20 cm	5 mm	
Colonoscopy	4-25 Fr	5-20 cm	5 mm	
Bronchoscopy	2-4 Fr			
Cytoscopy/ureteroscopy	4-12 Fr			
Hysteroscopy	2-5 Fr			
Fallopscopy	1.5-4 Fr			
Urethral catheter	8-20 Fr			
Percutaneous nephrostomy	4-15 Fr			
General drains	4-40 Fr	1-10 cm		
Paracentesis	4-8 Fr			

Figs. 15A-22B provide additional details illustrating how the devices of the present disclosure may be used in various clinical situations. Figs. 15A-15B illustrate side cutaway views of a catheter 10 according to certain embodiments of the present disclosure. As shown, the catheter 10, comprises inner layer 20 and outer layer 22. In addition, the catheter 10 can comprise a guidewire 56 disposed within a lumen of inner layer 20. In certain embodiments, to deliver therapeutic or diagnostic agents, the guidewire 56 may be removed, thereby providing sufficient surface area within the catheter for effective flow of the agents. Alternatively, as discussed above, the inner layer 20, may be removed, as illustrated in Figs. 16A-16C. As such, the lumen 150 will have an even greater cross-sectional area, which may be desirable for delivery of solid materials or for insertion of devices such as balloons or stents.

As discussed previously, the devices of the present disclosure can be used for therapeutic interventions, including balloon dilation and/or stenting. Fig. 17 illustrates a side view of a catheter including a balloon treatment device according to certain embodiments; and Figs. 18A-18C illustrate side cutaway views of a catheter used to deliver a stent to a treatment site according to certain embodiments of the present disclosure. As shown, the devices 10 (Fig. 17) can include a balloon dilation device 170 positioned on a portion thereof, or alternatively, a separate balloon catheter may be advanced over a guidewire positioned using the catheters described herein, or may be passed through a lumen of the catheters described herein. Furthermore, a stent or other therapeutic device can be passed through a

lumen of the disclosed catheters after optionally removing the inner layer and/or guidewire and inserting a secondary catheter 184 carrying a stent 180 and deployment device 182, as shown in Figs. 18A-18C.

5 In some embodiments, the devices of the present disclosure can be used to access a desired anatomic site, and then to place a secondary catheter or treatment device. For example, Figs. 19A-19C illustrate a method of positioning a secondary catheter or treatment device using various embodiments of the present invention. As shown in Fig. 19A, a device 10 can be deployed to a desired anatomic site, and may include a guidewire 56. After positioning the device 10 at the desired site, the catheter 10 may be removed, leaving only the
10 guidewire 56 in place. Subsequently, a secondary device configured for a particular therapeutic or diagnostic application, but perhaps unable to be navigated to the desired site on its own, will be passed over the positioned guidewire 56, thereby allowing positioning of the secondary catheter 11 or treatment device.

As noted above, the devices of the present disclosure can include a handle region 57,
15 which can provide a variety of different structures and functional control for a clinician. Fig. 20 illustrates a side cutaway view of a catheter with a handle region 57 according to certain. And Figs. 21A-21D illustrate components of an actuator in a handle region 57 of a catheter according to certain embodiments. As shown, the handle 57 can include a button 210, which can be attached to a cam 220, and cam follower 224. Further, as illustrated in Figs. 21A-21D,
20 the cam follower 224 can move along a path from an extended position Fig. 21B-21D, to a retracted position (Fig. 21A). As such, the cam follower 224, which is operably attached to at least one of the inner and outer layers 20,22 provides longitudinal movement of the layers 20,22 relative to one another. Furthermore, the inner and outer layers are held in either an in register or out of register position relative to one another, similar to the mechanism used to
25 hold a "click pen" in an extended or retracted position.

In addition, Fig. 20 illustrates various other components of the devices of the present disclosure. As noted above, the devices can be used to deliver fluid, e.g., for therapeutic or diagnostic applications, and the handle may include one or more fluid ports 230,232. In addition, the devices can include one or more radiopaque markers 260,270 on either or both
30 of the inner or outer layers 20,22, thereby allowing visualization of the catheters during use, and assisting in determining if the catheter is in a stiffer or flexible state.

Fig. 20 further illustrates a space 240 between the inner and outer layers 20,22. The space 240 may vary based upon the particular clinical use and dimensions of the device.

However, the space 240 should be sized to allow the devices to bend at a high radius of curvature without producing excessive frictional contact between the layers 20,22. In various embodiments, the space is 1-50 microns, or 30-70 microns, on all sides of the inner layer.

In various embodiments, in order to allow ease of movement through lumens, and in order to provide for movement of the inner and out layer 20,22 relative to one another, even during large bends, the surfaces of the layers may be treated to reduce the friction between various components. For example, Figs. 22A-22B illustrate side cutaway views of catheters incorporating lubricious coatings 23, according to various embodiments. When rounding multiple tortuous bends with the catheter assembly, the increased area of direct contact between the two catheter layers 20,22 (due to pressing of the inner catheter against the one side of the outer catheter's inner surface) can generate friction that prevents shifting between the flexible and stiff states by restricting the movement of the inner catheter relative to the outer catheter. Accordingly, lubricious coatings 23 may be used in order to reduce the coefficient of friction between the inner and outer catheter, and between the outer catheter and the anatomic sites such as blood vessel walls. The lubricating coatings 23 will be applied to the outer surface of the inner catheter, the outer surface of the outer catheter, and/or the inner surface of the outer catheter. Generally, the coatings 23 will be applied and cured prior to assembly of the inner catheter, outer catheter, and handle into a finished device.

In various exemplary embodiments, the coatings 23 may be made of the from a variety of materials include a PTFE liner added on top of a mandrel (to coat inner surface of catheter) or on top of the catheter while on a mandrel (to coat outer surface of catheter), a hydrophilic synthetic polymer network that is applied by dip or brush coating and cured to the catheter surface by heat treatment, a hydrophilic synthetic polymer network that is applied by dip or brush coating and cured to the catheter surface by UV treatment, a hydrophilic synthetic polymer network that is applied by gaseous activation of the catheter surface and subsequent grafting onto catheter surface by polymer from aqueous solution, and/or hydrophilic natural polymer network (such as those based on hyaluronic acid) that is bonded to a base coat layer attached to the catheter surface. Further, although the coatings 23 can have a variety of sizes and material properties, exemplary coatings may have a thickness between 1 and 10 micrometers and a coefficient of friction between 0.005 and 0.03, or a reduction of up to 90% compared to uncoated

coefficients of friction. Compatible with pebax base materials, and with common methods of sterilization (EtO, gamma irradiation, etc.).

What has been described and illustrated herein is a preferred embodiment of the invention along with some of its variations. The terms, descriptions and figures used herein are set forth by way of illustration only and are not meant as limitations. Those skilled in the art will recognize that many variations are possible within the spirit and scope of the invention in which all terms are meant in their broadest, reasonable sense unless otherwise indicated. Any headings utilized within the description are for convenience only and have no legal or limiting effect.

CLAIMS

1. An adjustable catheter comprising:

an inner tube having a first plurality of spaced regions having a first stiffness separated by a first plurality of spaced segments having a greater
5 stiffness than the plurality of spaced regions;

an outer tube extending around the inner tube such that the outer tube and the inner tube undergo relative longitudinal translation, the outer tube having a second plurality of spaced regions having a second stiffness separated by a second plurality of spaced segments having a greater
10 stiffness than the second plurality of spaced regions; and

an actuator configured to provide relative longitudinal motion of the inner tube and the outer tube.

2. The catheter of claim 1, wherein the first plurality of spaced segments
15 comprise tubular elements.

3. The catheter of any of claims 1 or 2, further comprising a third tube positioned between the inner tube and the outer tube.

20 4. The catheter of claim 3, wherein the third tube comprises a flexible region having alternating segments of higher and lower stiffness.

5. The catheter of any of claims 1-4, further comprising a handle mounted at a proximal end of the catheter, the handle including a portion of the
25 actuator.

6. The catheter of claim 5, wherein the handle comprises at least one fluid supply port.

30 7. The catheter of claim 5, wherein the handle comprises two fluid supply ports.

8. The catheter of any of claims 1-7, wherein the actuator comprises a cam and cam follower operably attached to one of the inner layer and outer layer.

5 9. The catheter of any of claims 1-8, further comprising at least one lumen extending through the catheter.

10. The catheter of claim 9, further comprising a fluid source coupled to the lumen for delivering a fluid through the lumen.

10

11. The catheter of any of claims 1-10, further comprising a guidewire positioned within a lumen within the inner tube.

12. The catheter of any of claims 1-11, wherein the first plurality of spaced regions and second plurality of spaced regions each comprise polymeric materials.

15

13. The catheter of any of claims 1-2, further comprising a lubricious coating disposed on the surface of at least one of the inner tube and the outer tube.

20

14. The catheter of claim 13, comprising a lubricious coating disposed on an outer surface of the inner tube.

15. The catheter of claim 13, comprising a lubricious coating disposed on an outer surface of the inner tube and a lubricious coating disposed on an outer surface of the outer tube.

25

16. The catheter of any of claims 13-15, wherein the coating comprises polytetrafluoroethylene.

30

17. The catheter of any of claims 13-15, wherein the coating comprises a hydrophilic polymer.

18. The catheter of any of claims 13-15, wherein the coating has a coefficient of friction between about 0.005 and 0.03.

5 19. The catheter of any of claims 13-15, wherein the coating has a coefficient of friction that is at least 90% less than the coefficient of friction of the inner and outer layer without a coating.

10 20. The catheter of any of claims 1-19, wherein the first plurality of spaced regions are disposed at a distal end of the catheter and such that the distal end has a minimum radius of curvature in a range of 2-6 mm, or preferably 3-5 mm.

15 21. The catheter of any of claims 1-20, wherein the second plurality of spaced regions are disposed at a distal end of the catheter.

22. The catheter of any of claims 1-21, further comprising at least one radiopaque marker.

20 23. The catheter of any of claims 1-22, wherein the first plurality of spaced regions comprise tubular polymeric regions.

24. The catheter of any of claims 1-23, wherein the second plurality of spaced regions comprises tubular polymeric regions.

25 25. The catheter of any of claims 23-24, further comprising at least one polymeric coating disposed around the surface of at least one of the inner tube and the outer tube.

30 26. The catheter of any of claims 1-25, wherein the first plurality of spaced regions comprise coiled wire.

27. The catheter of any of claims 1-26, wherein the second plurality of spaced regions comprise coiled wire.

28. The catheter of any of claims 1-27, wherein the actuator is operably coupled to the inner tube to move the inner tube longitudinally within the outer tube.

29. The catheter of any of claims 1-28, further comprising a treatment device for delivery to a treatment site.

30. The catheter of claim 29, wherein the treatment device comprises a stent.

31. The catheter of claim 29, wherein the treatment device comprises a balloon.

32. The catheter of claim 29, wherein the treatment device comprises an embolic device.

33. The catheter of any of claims 1-32, further comprising a medicament.

34. The catheter of any of claims 1-32, further comprising a contrast agent.

35. The catheter of any of claims 1-27, further comprising a guidewire passing through a lumen in the inner layer.

36. The catheter of any of claims 1-35, wherein the catheter comprises a gap between the inner layer and outer layer.

37. The catheter of claim 36, wherein the gap is sized to allow the catheter to bend with a desired radius of curvature.

38. The catheter of claim 36, wherein the gap is between about 30 microns and 70 microns.

39. The catheter of any of claims 1-38, wherein the first plurality of spaced regions have lengths that are larger than lengths of the first plurality of spaced segments.

40. The catheter of any of claims 1-39, wherein the second plurality of spaced regions have lengths that are larger than lengths of the second plurality of spaced segments.

41. The catheter of any of claims 1-40, wherein the lengths of the first plurality of spaced regions are approximately equal to the lengths of the second plurality of spaced regions.

42. The catheter of any of claims 1-41, wherein the lengths of the first plurality of spaced segments are approximately equal to the lengths of the second plurality of spaced segments.

43. A method for guiding a catheter to a treatment site within a body comprising:
inserting a catheter into a body lumen, the catheter having a flexible distal region including a plurality of movable segments;
actuating relative movement between the plurality of movable segments to alter a stiffness of the flexible distal region; and
advancing the catheter within the body lumen.

44. The method of claim 1, wherein the actuating step comprises sliding at least one layer within the catheter to alter the stiffness.

45. The method of any of claims 43-44, further comprising advancing a guidewire through a central lumen of the catheter to select a lumen branch to advance the catheter to a treatment site.

46. The method of any of claims 43-45, wherein the actuating step comprises actuating relative movement of a first layer and a second layer, the first layer comprising alternating first regions of differing stiffnesses, and the second layer comprising alternating second regions of the differing stiffnesses.

5

47. The method of any of claims 43-46, further comprising delivering a fluid to a site within the body.

10

48. The method of any of claims 43-46, further comprising delivering a treatment device to a treatment device.

49. The method of claim 48, wherein the step of delivering a treatment device comprises inserting at least one of a coil, a snare, a balloon, or a stent to a treatment site.

15

50. The method of any of claims 43-49, further comprising removing the catheter and inserting a second catheter to deliver a fluid or treatment device.

51. The method of any of claims 43-50, further comprising delivering a contrast agent or medicament.

20

52. The method of any of claims 43-51, further comprising grasping a handle to move the catheter, the handle including an actuator to adjust a flexibility of the catheter.

25

53. The method of claim 43, further comprising percutaneously introducing the catheter into a body lumen wherein the catheter comprises:

an inner tube having a first plurality of spaced regions having a first stiffness separated by a first plurality of spaced segments having a greater stiffness than the plurality of spaced regions; and

30

an outer tube extending around the inner tube such that the outer tube and the inner tube undergo relative longitudinal translation, the outer tube having a second plurality of spaced regions having a second stiffness separated by a second plurality of spaced segments having a greater stiffness than the second plurality of spaced regions.

54. The method of claim 53, wherein the first plurality of spaced segments comprise tubular elements.

5 55. The method of any of claims 53 or 54, further comprising positioning a third tube between the inner tube and the outer tube.

56. The method of claim 55, wherein the third tube comprises a flexible region having alternating segments of higher and lower stiffness.

10

57. The method of any of claims 53-56, further comprising manually grasping a handle mounted at a proximal end of the catheter.

15 58. The method of claim 57, further comprising inserting a fluid with the handle that comprises at least one fluid supply port.

59. The method of claim 58, further comprising inserting a fluid with the handle that comprises two fluid supply ports.

20 60. The method of any of claims 53-59, wherein the first plurality of spaced regions and second plurality of spaced regions each comprise polymeric materials.

25 61. The method of any of claims 53-60, wherein the catheter further comprises a lubricious coating disposed on the surface of at least one of the inner tube and the outer tube.

62. The method of claim 61, wherein the catheter comprises a lubricious coating disposed on an outer surface of the inner tube.

30

63. The method of claim 61, wherein the catheter comprises a lubricious coating disposed on an outer surface of the inner tube and a lubricious coating disposed on an outer surface of the outer tube.

5 64. The method of any of claims 61-63, wherein the coating comprises polytetrafluoroethylene.

65. The method of any of claims 61-63, wherein the coating comprises a hydrophilic polymer.

10

66. The method of any of claims 61-63, wherein the coating has a coefficient of friction between about 0.005 and 0.03.

15

67. The method of any of claims 61-63, wherein the coating has a coefficient of friction that is at least 90% less than the coefficient of friction of the inner layer and outer layer without a coating.

20

68. The method of any of claims 53-67, wherein the first plurality of spaced regions are disposed at a distal end of the catheter.

69. The method of any of claims 53-68, wherein the second plurality of spaced regions are disposed at a distal end of the catheter.

25

70. The method of any of claims 1-14, wherein the catheter further comprises at least one radiopaque marker.

71. The method of any of claims 53-70, wherein the first plurality of spaced regions comprise tubular polymeric regions.

30

72. The method of any of claims 53-71, wherein the second plurality of spaced regions comprises tubular polymeric regions.

73. The method of any of claims 43-72, wherein the catheter comprises at least one polymeric coating disposed around the surface of at least one of the inner tube and the outer tube.

5 74. The method of any of claims 53-73, wherein the first plurality of spaced regions comprise coiled wire.

75. The method of claim 43 wherein the catheter has a minimum radius of curvature in a range of 2-6 mm.

10

76. The method of any of claims 53-74, wherein the second plurality of spaced regions comprise coiled wire.

15 77. The method of any of claims 43-74, further comprising delivering a treatment device for to a treatment site.

78. The method of claim 77, wherein the treatment device comprises a stent.

20 79. The method of claim 77, wherein the treatment device comprises a balloon.

80. The method of claim 77, wherein the treatment device comprises an embolic device.

25

81. The method of any of claims 43-80, further comprising administering a medicament to a desired treatment site.

30 82. The method of any of claims 43-81, further comprising delivering a contrast agent to a selected anatomic site.

83. The method of any of claims 43-82, further comprising removing a guidewire from a lumen in the inner layer.

84. The method of any of claims 53-83, wherein the catheter comprises a gap between the inner layer and outer layer.

5 85. The method of claim 84, wherein the gap is sized to allow the catheter to bend with a desired radius of curvature.

86. The method of claim 84, wherein the gap is between about 30 microns and 70 microns.

10

87. The method of any of claims 53-86, wherein the first plurality of spaced regions have lengths that are larger than lengths of the first plurality of spaced segments.

15 88. The method of any of claims 53-86, wherein the second plurality of spaced regions have lengths that are larger than lengths of the second plurality of spaced segments.

20 89. The method of any of claims 53-86, wherein the lengths of the first plurality of spaced regions are approximately equal to the lengths of the second plurality of spaced regions.

25 90. The method of any of claims 53-86, wherein the lengths of the first plurality of spaced segments are approximately equal to the lengths of the second plurality of spaced segments.

91. The method of any of claims 43-90 further comprising removing a tubular body from the catheter and delivering an agent to an anatomic site within the body through the catheter.

30

92. A method of manufacturing a catheter, comprising,

forming an inner tube having a first plurality of spaced regions having a first stiffness separated by a first plurality of spaced segments having a greater stiffness than the plurality of spaced regions; and

forming an outer tube extending around the inner tube such that the outer tube and the inner tube undergo relative longitudinal translation, the outer tube having a second plurality of spaced regions having a second stiffness separated by a second plurality of spaced segments having a greater stiffness than the second plurality of spaced regions.

93. The method of claim 92, wherein the first plurality of spaced segments comprise tubular elements.

94. The method of any of claims 92 or 93, further comprising forming a third tube positioned between the inner tube and the outer tube.

95. The method of claim 94, wherein the third tube comprises a flexible region having alternating segments of higher and lower stiffness.

96. The method of any of claims 92-95, further comprising attaching a handle a proximal end of the catheter.

97. The method of claim 96, wherein the handle comprises at least one fluid supply port.

98. The method of claim 97, wherein the handle comprises two fluid supply ports.

99. The method of any of claims 92-98, wherein the first plurality of spaced regions and second plurality of spaced regions each comprise polymeric materials.

100. The method of any of claims 92-98, further comprising forming a lubricious coating on the surface of at least one of the inner tube and the outer tube.

5 101. The method of claim 100, wherein the lubricious coating is disposed on an outer surface of the inner tube.

10 102. The method of claim 100, comprising forming a lubricious coating disposed on an outer surface of the inner tube and a lubricious coating disposed on an outer surface of the outer tube.

103. The method of any of claims 100-102, wherein the coating comprises polytetrafluoroethylene.

15 104. The method of any of claims 100-102, wherein the coating comprises a hydrophilic polymer.

20 105. The method of any of claims 100-102, wherein the coating has a coefficient of friction between about 0.005 and 0.03.

106. The method of any of claims 100-102, wherein the coating has a coefficient of friction that is at least 90% less than the coefficient of friction of the inner and outer layer without a coating.

25 107. The method of any of claims 92-106, wherein the first plurality of spaced regions are disposed at a distal end of the catheter.

108. The method of any of claims 92-107, wherein the second plurality of spaced regions are disposed at a distal end of the catheter.

30 109. The method of any of claims 92-108, wherein the catheter further comprises at least one radiopaque marker.

110. The method of any of claims 92-109, wherein the first plurality of spaced regions comprise tubular polymeric regions.

5 111. The method of any one of claims 91-110, wherein the second plurality of spaced regions comprises tubular polymeric regions.

112. The method of any one of claims 92-111, further comprising forming at least one polymeric coating disposed around the surface of at least one of the inner tube and the outer tube.

10 113. The method of any one of claims 92-112, wherein the first plurality of spaced regions comprise coiled wire.

114. The method of any one of claims 92-113, wherein the second plurality
15 of spaced regions comprise coiled wire.

115. The method of any of claims 96-98, wherein the handle comprises an actuator to control relative longitudinal positioning of the outer tube and the inner tube.





20 116. The method of claim 92 further comprising forming the inner tube by cutting a plurality of annular segments with different flexural stiffness.

25 117. The method of Claim 116 further comprising positioning the annular segments with differing flexural stiffness in a colinear position and heating the annular elements to join the elements together to form the inner tube.

30 118. The method of Claim 116 further comprising applying a layer onto the annular segments and applying heat to the layer to join the annular segments.

119. The method of any of Claims 116-118 further comprising forming the outer tube by heating a second plurality of annular segments to join the segments together.

- 5 120. The method of Claim 119 further comprising forming the inner tube and/or the outer tube with polymers and optionally applying a lubricating layer.

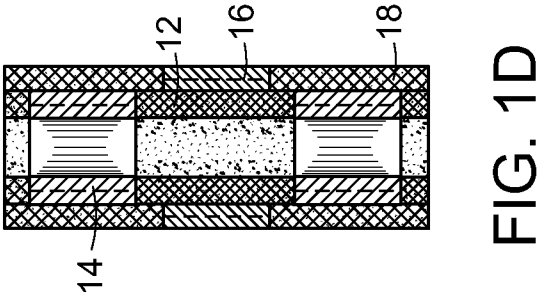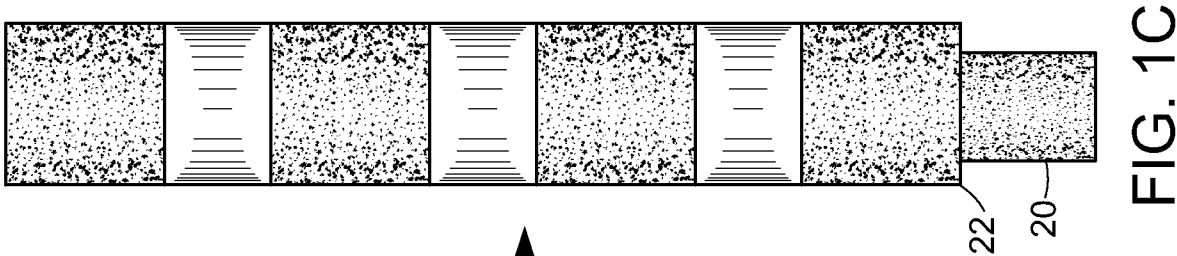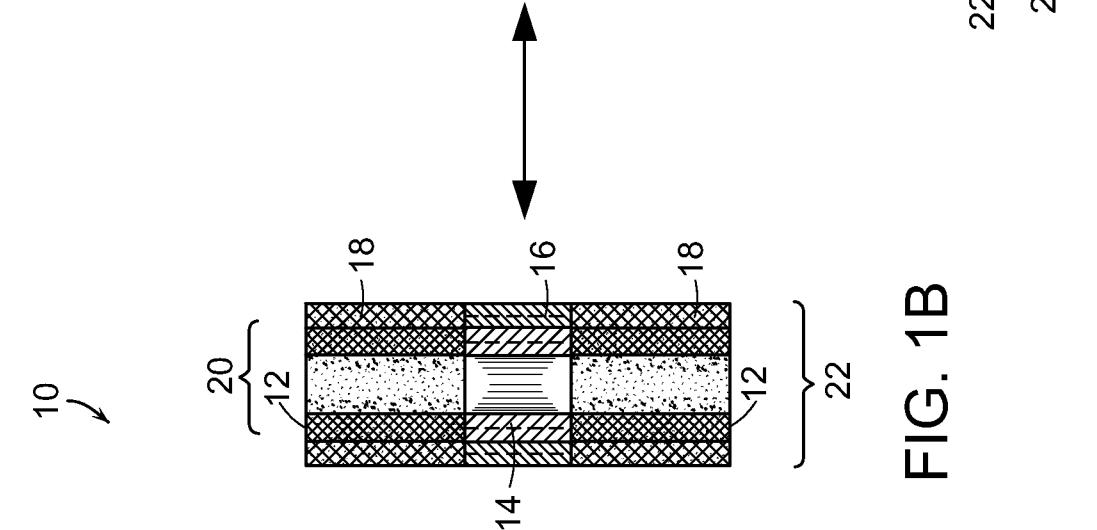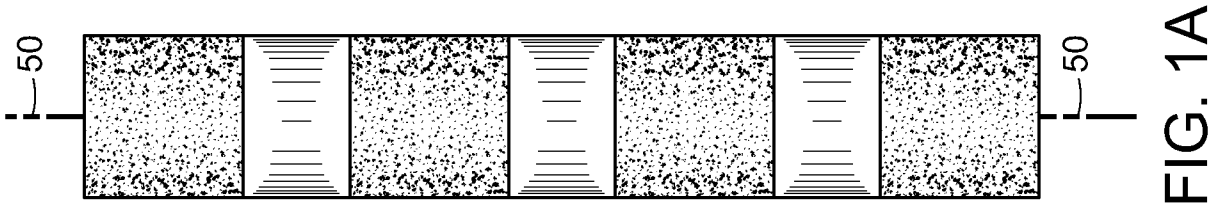

2/23

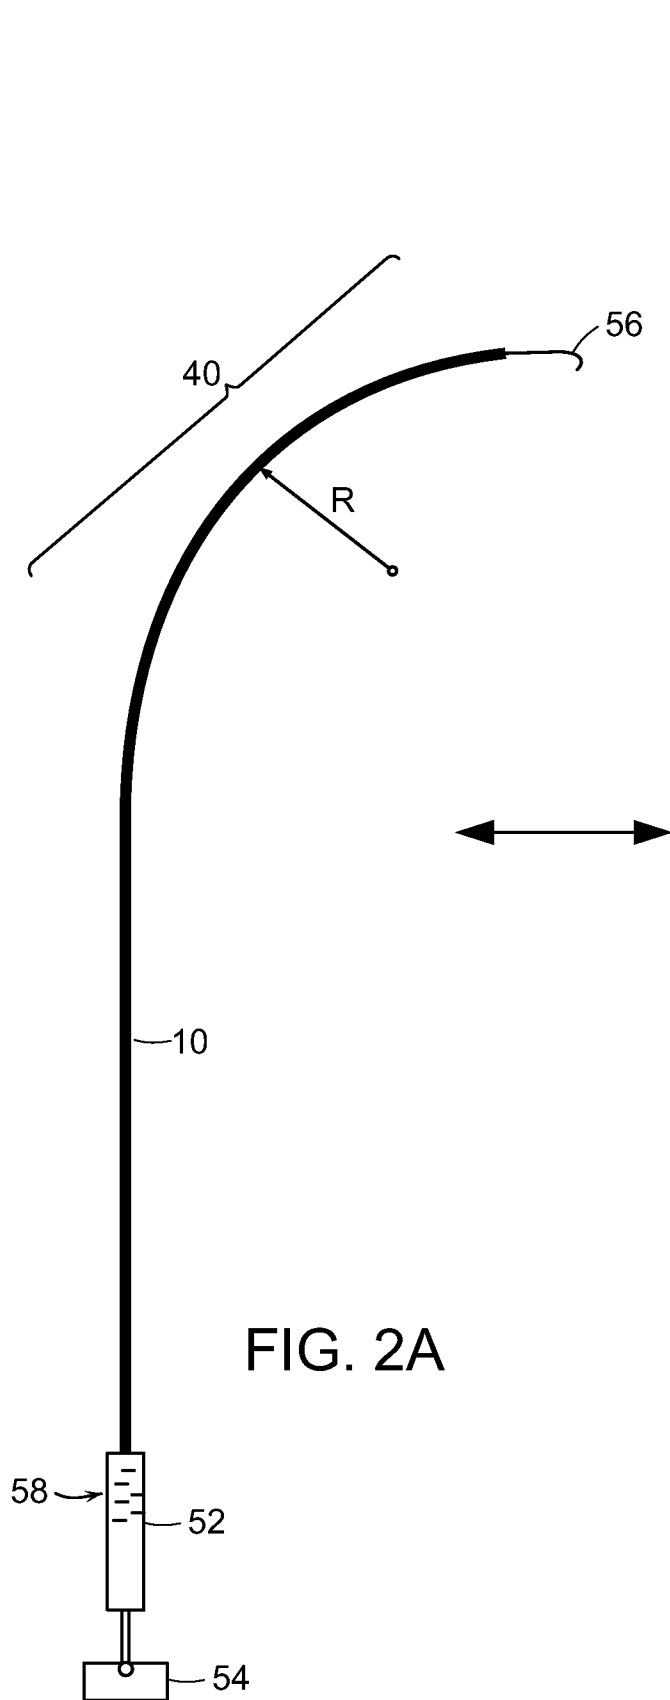


FIG. 2A

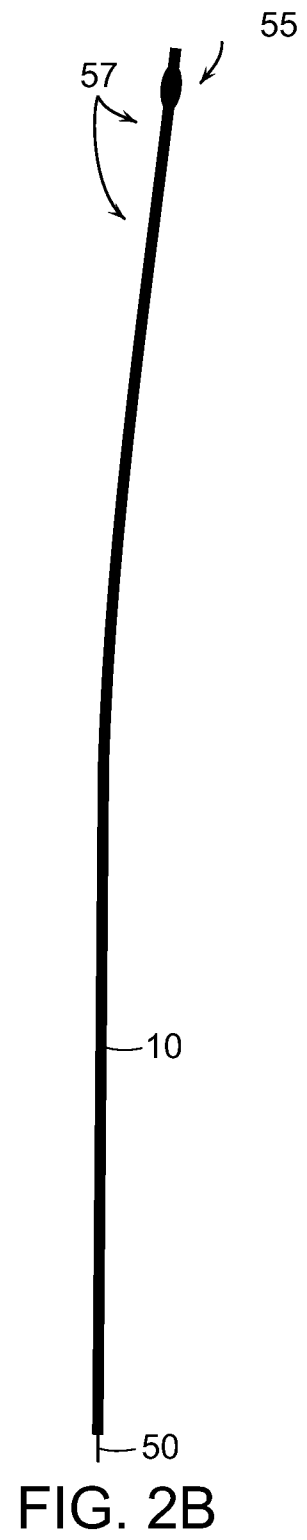


FIG. 2B

FIG. 2C

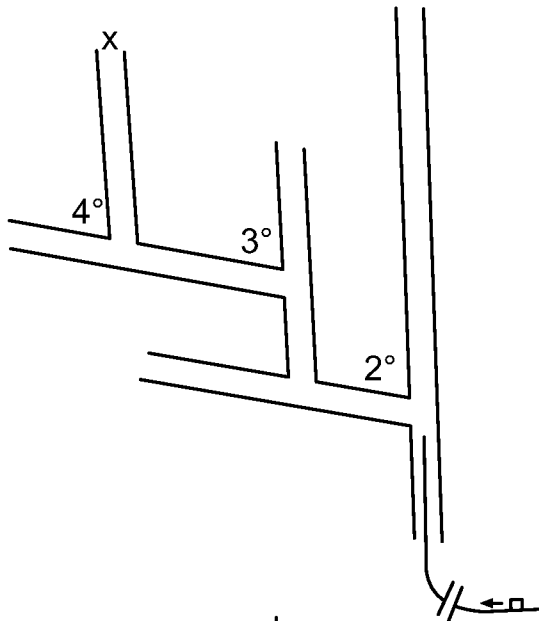


FIG. 2F

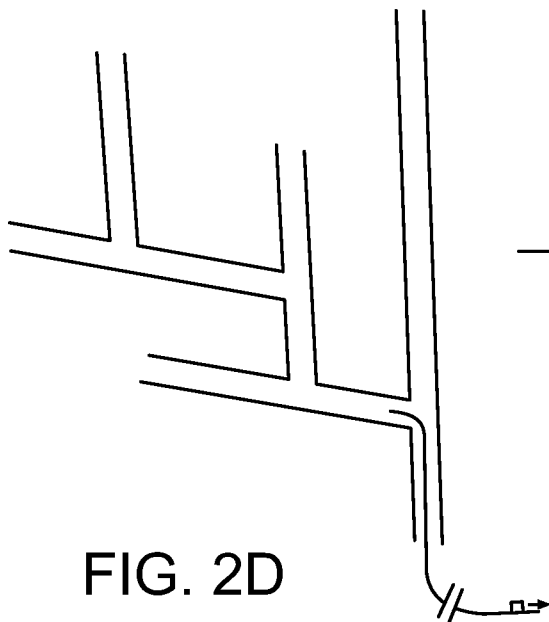
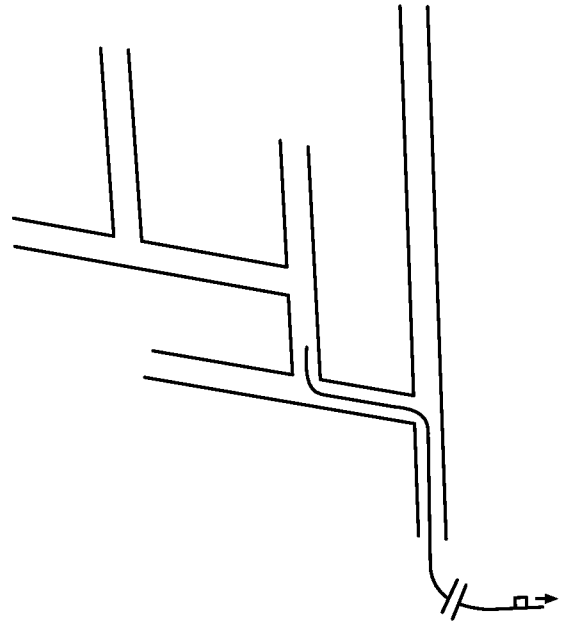


FIG. 2D

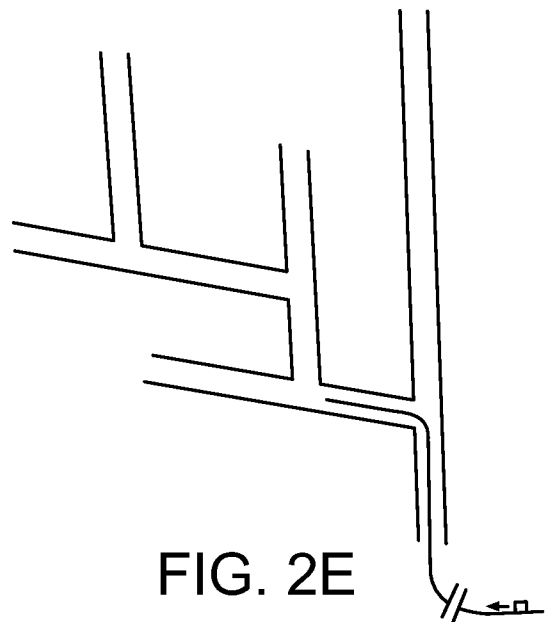



FIG. 2E

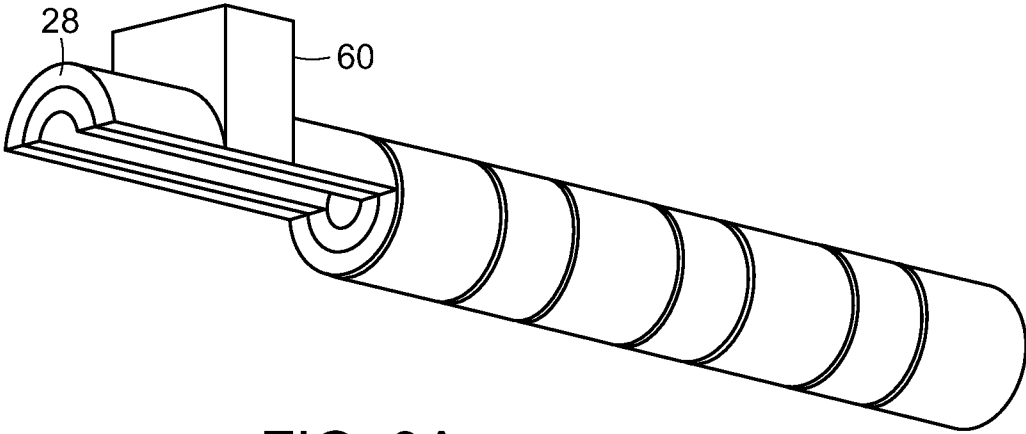


FIG. 3A

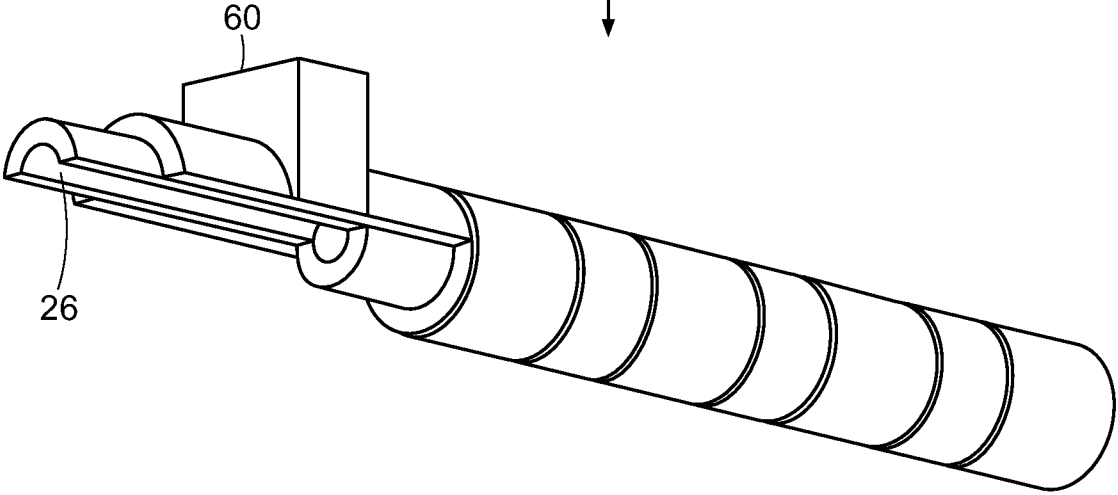


FIG. 3B

5/23

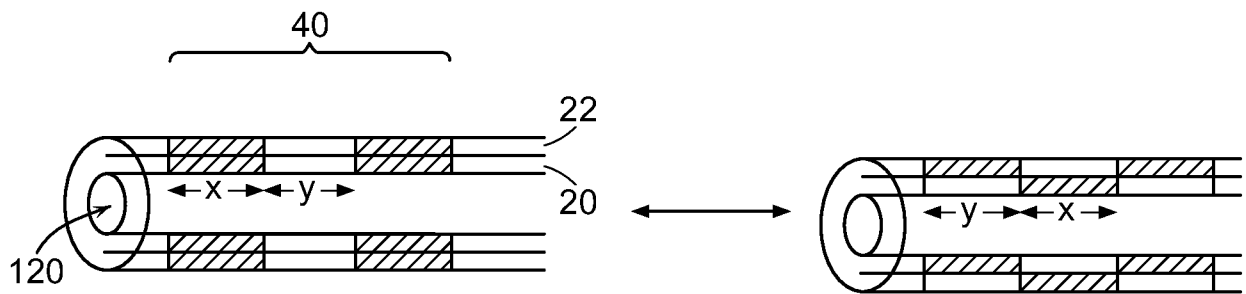


FIG. 4A

FIG. 4B

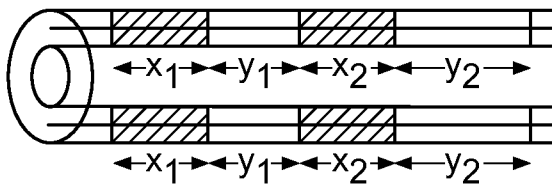


FIG. 4C

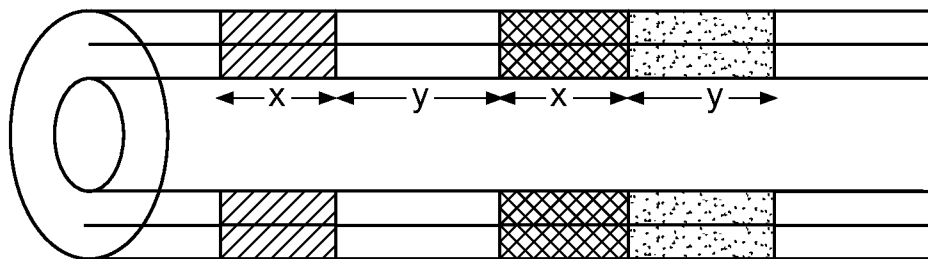


FIG. 4D

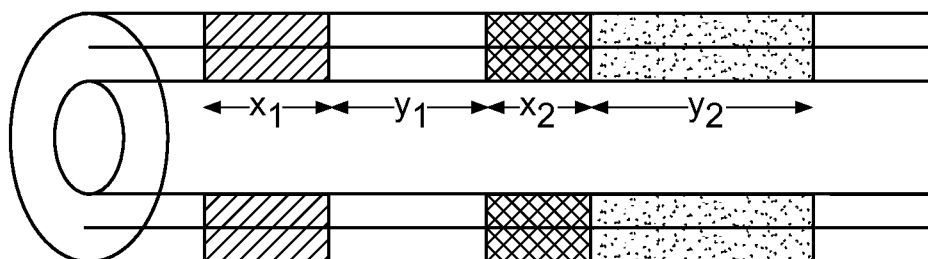


FIG. 4E

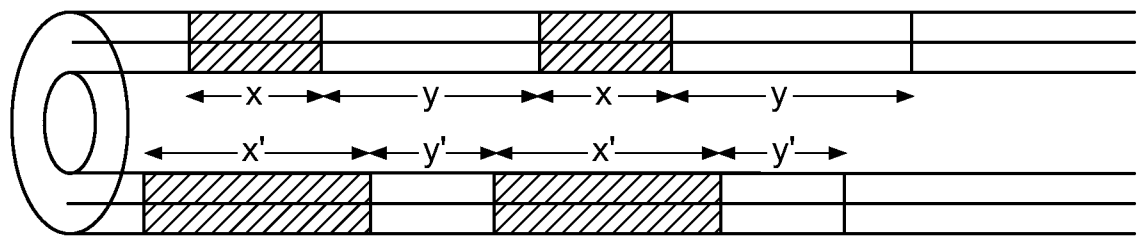


FIG. 4F

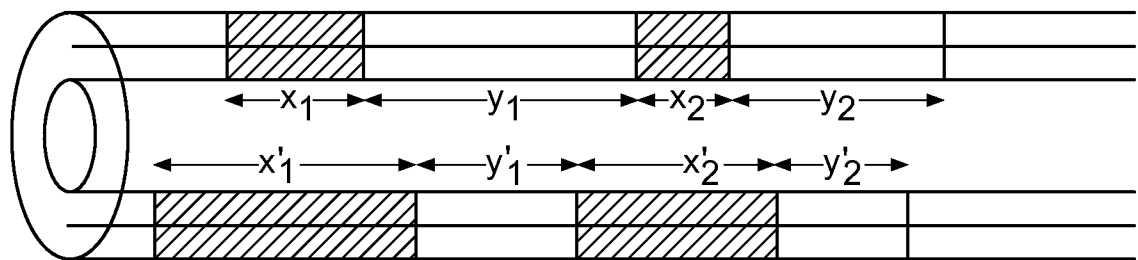


FIG. 4G

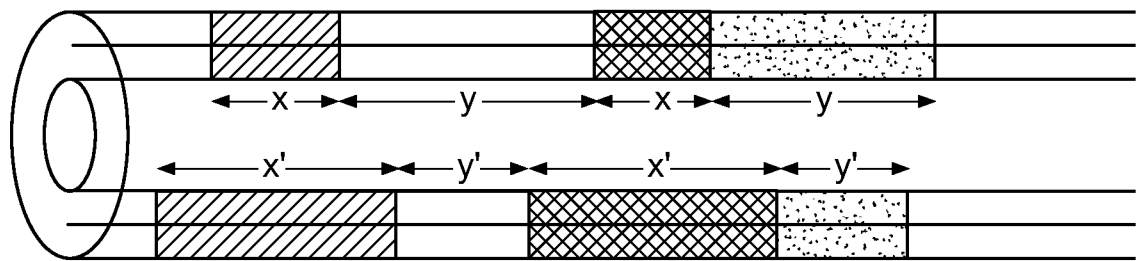


FIG. 4H

7/23

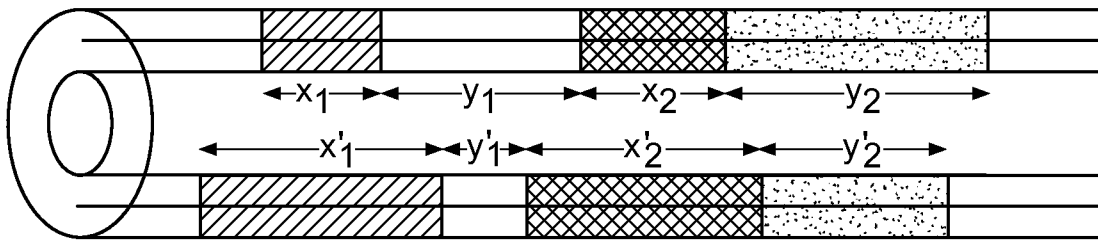


FIG. 4I

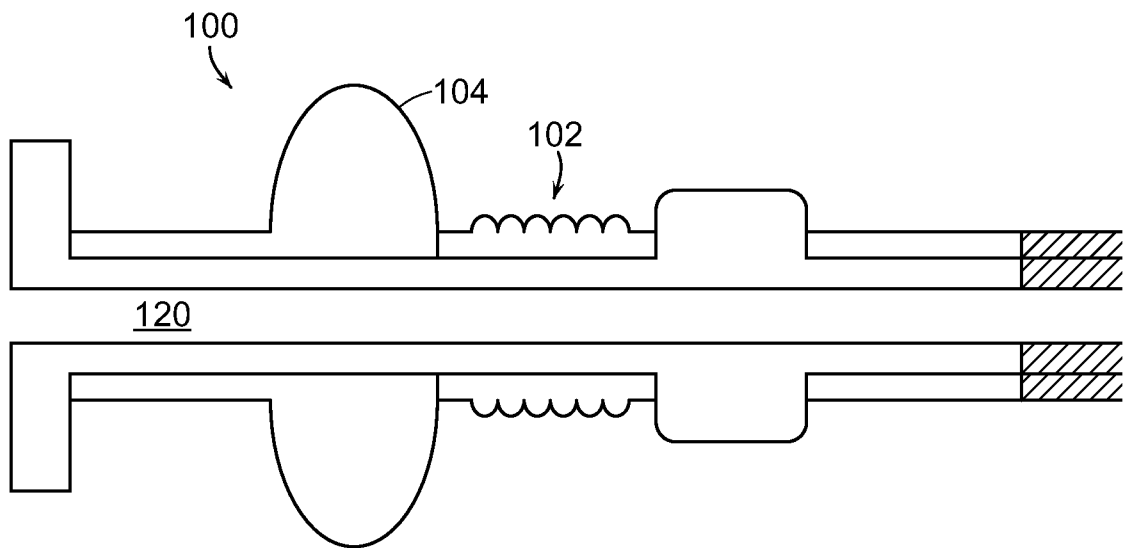


FIG. 4J

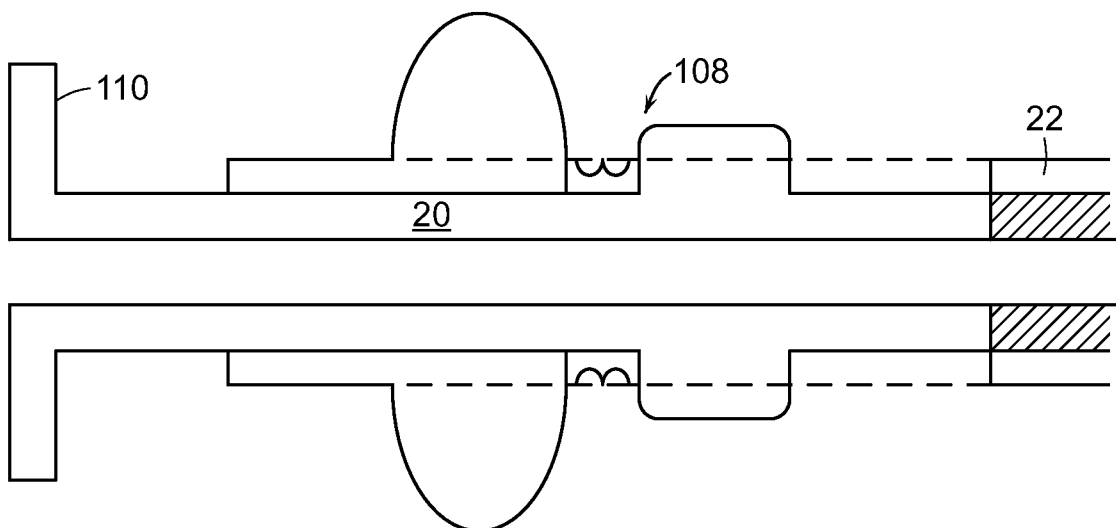


FIG. 4K

8/23

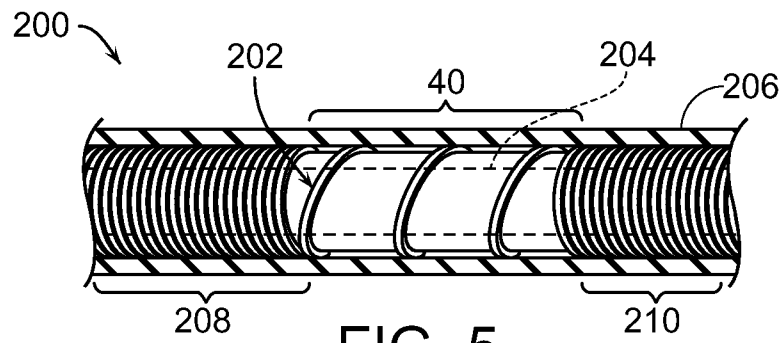


FIG. 5

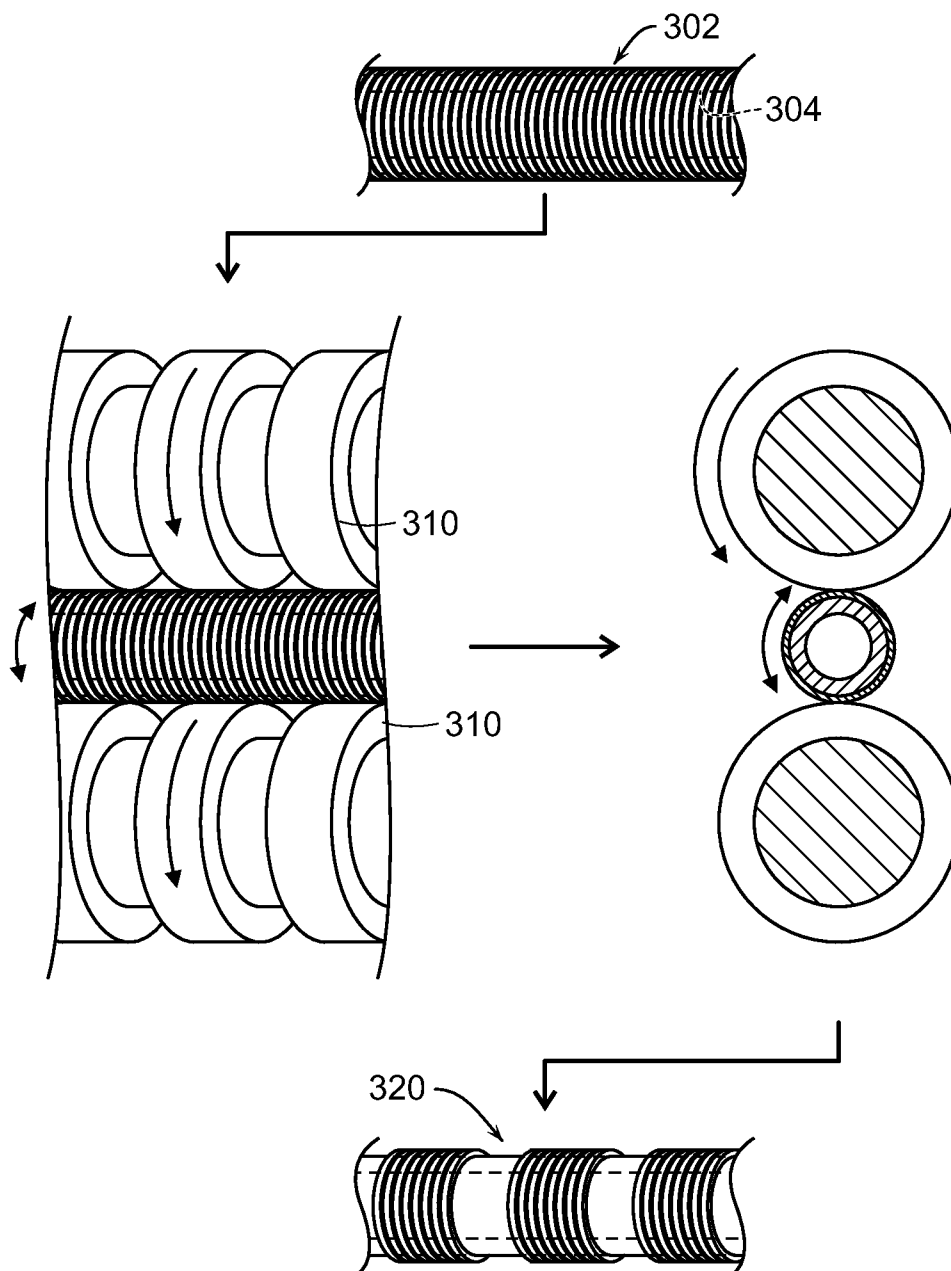


FIG. 6

9/23

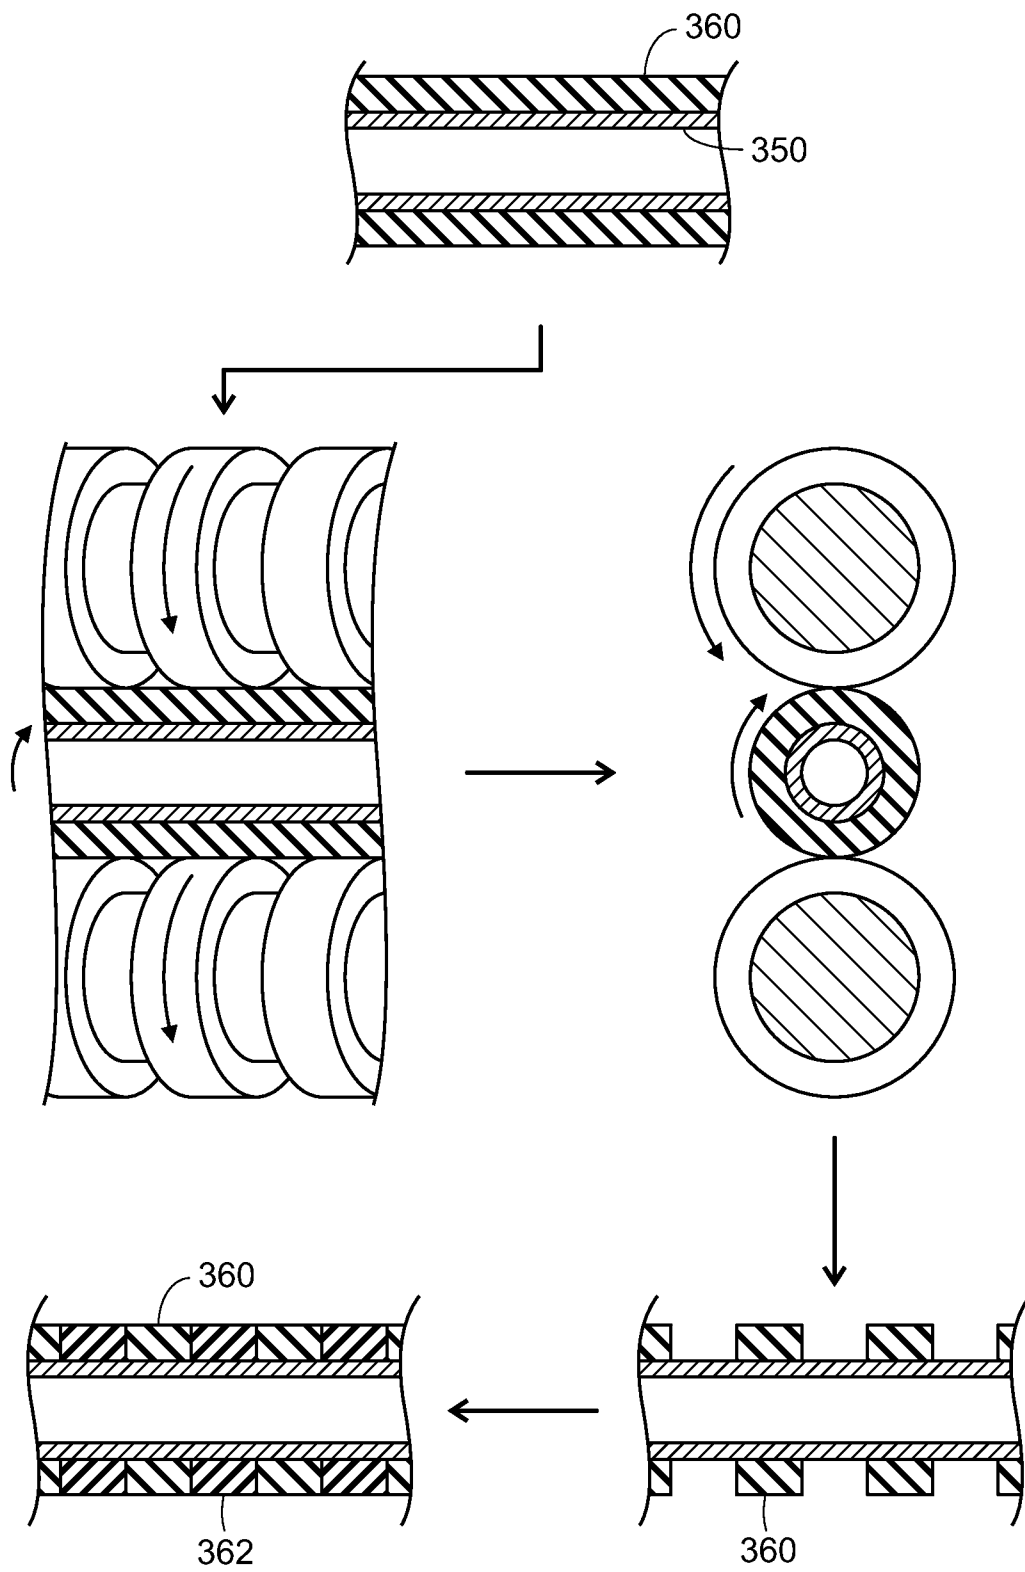


FIG. 7

10/23

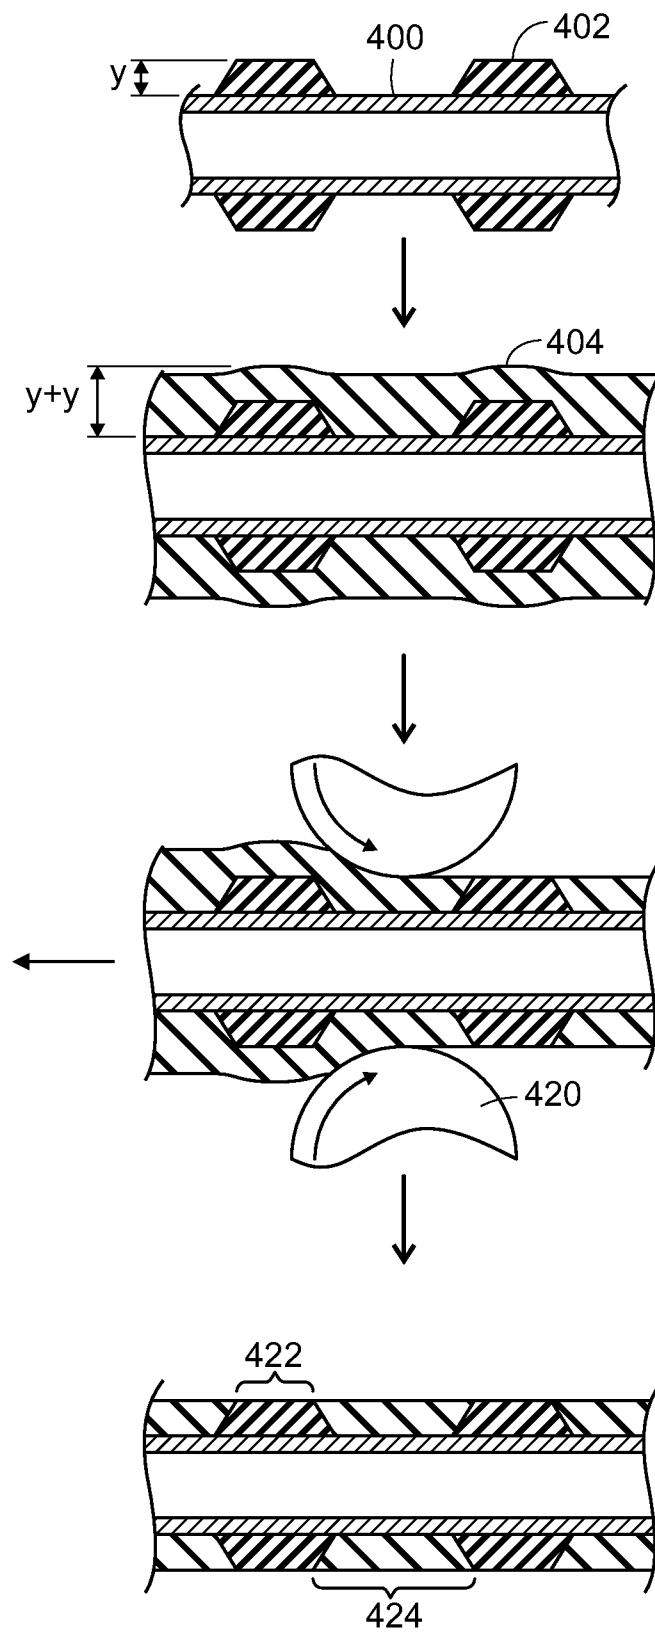


FIG. 8

11/23

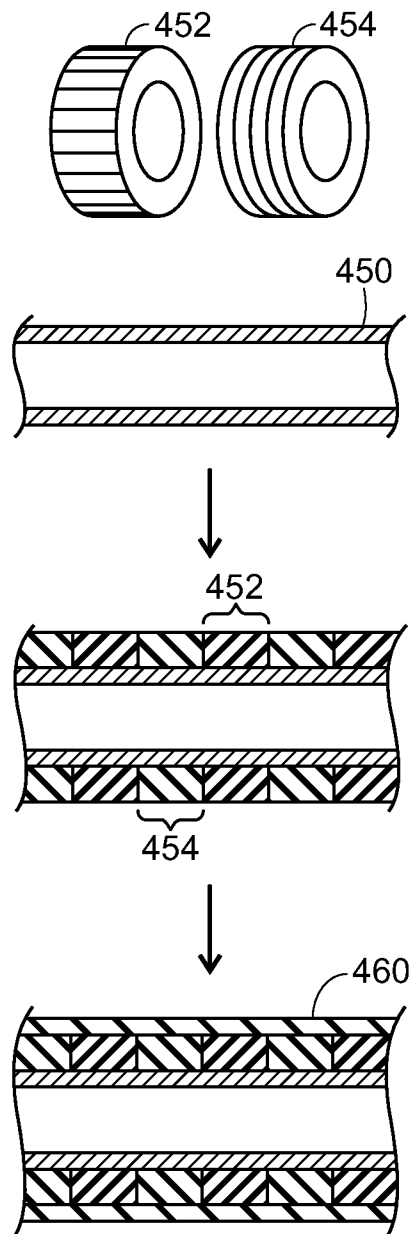


FIG. 9

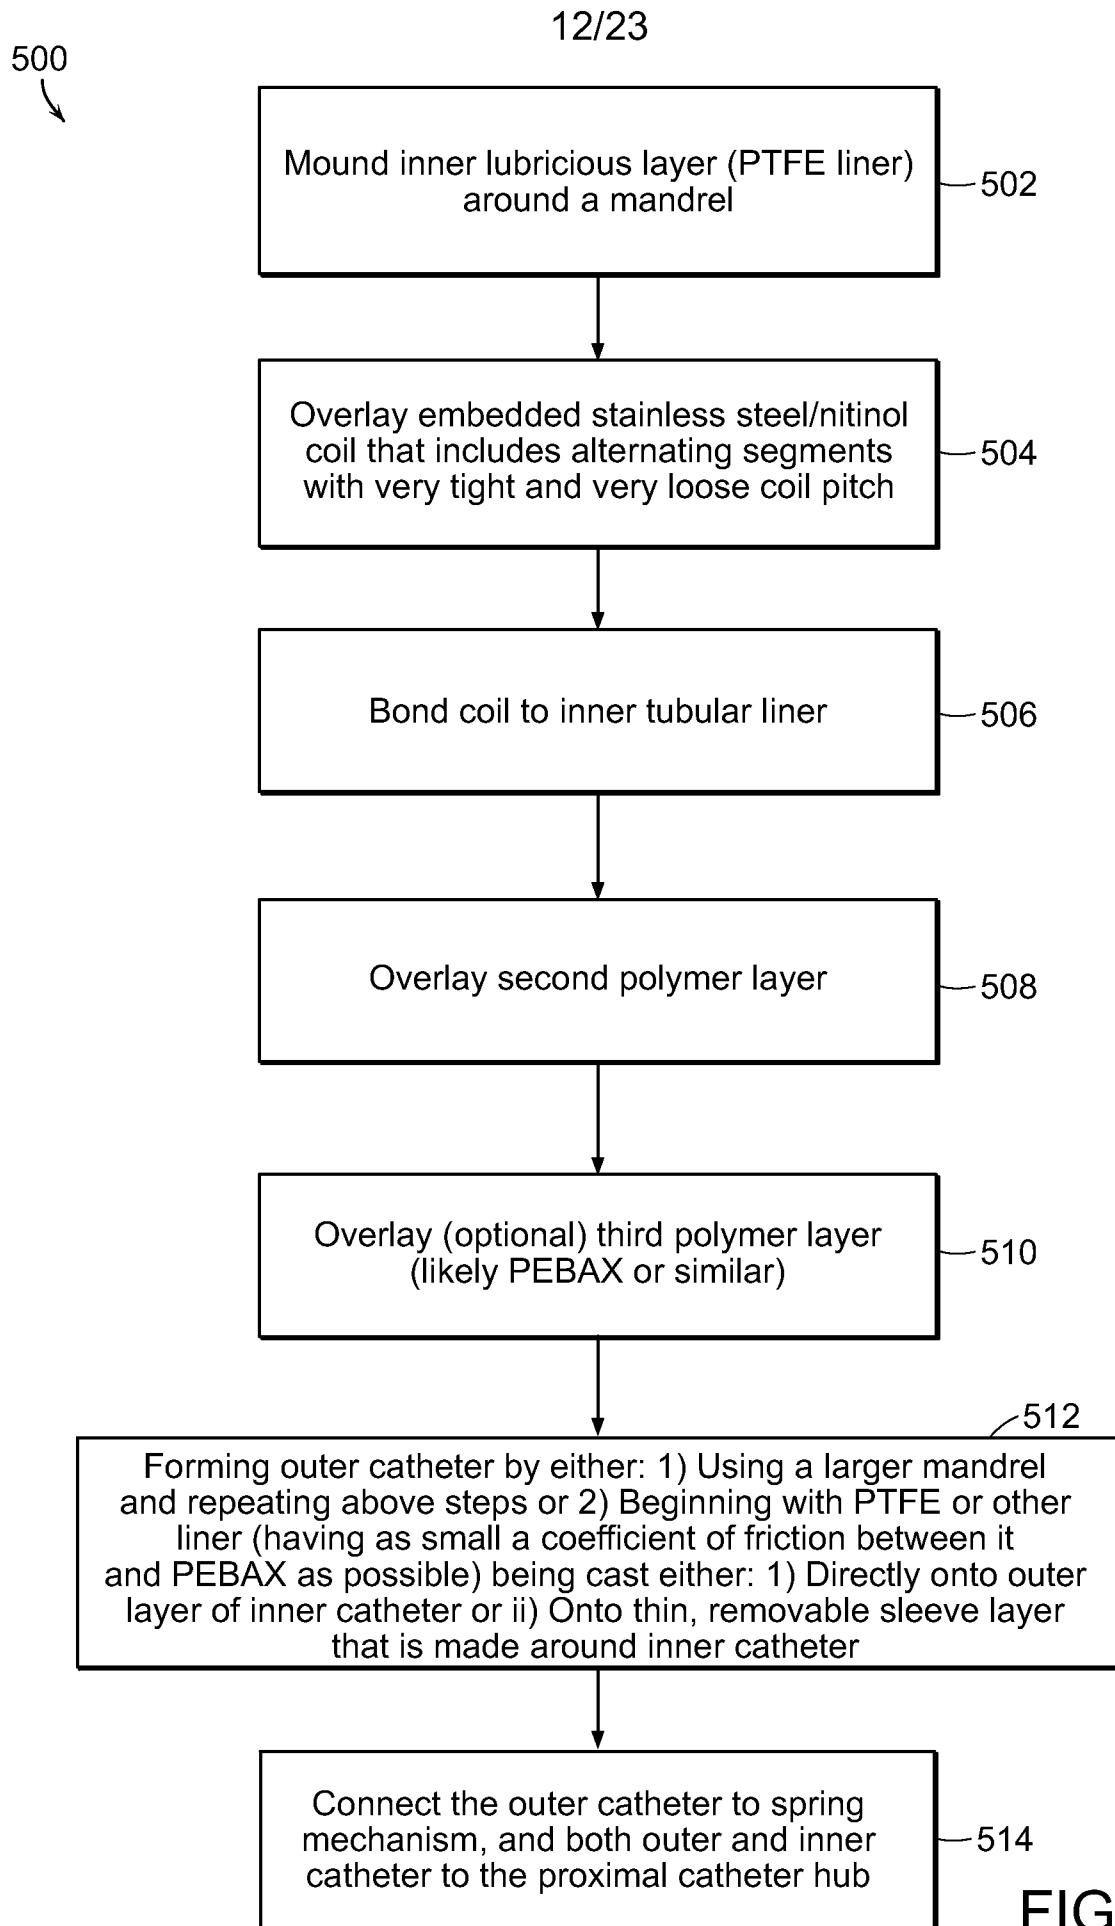
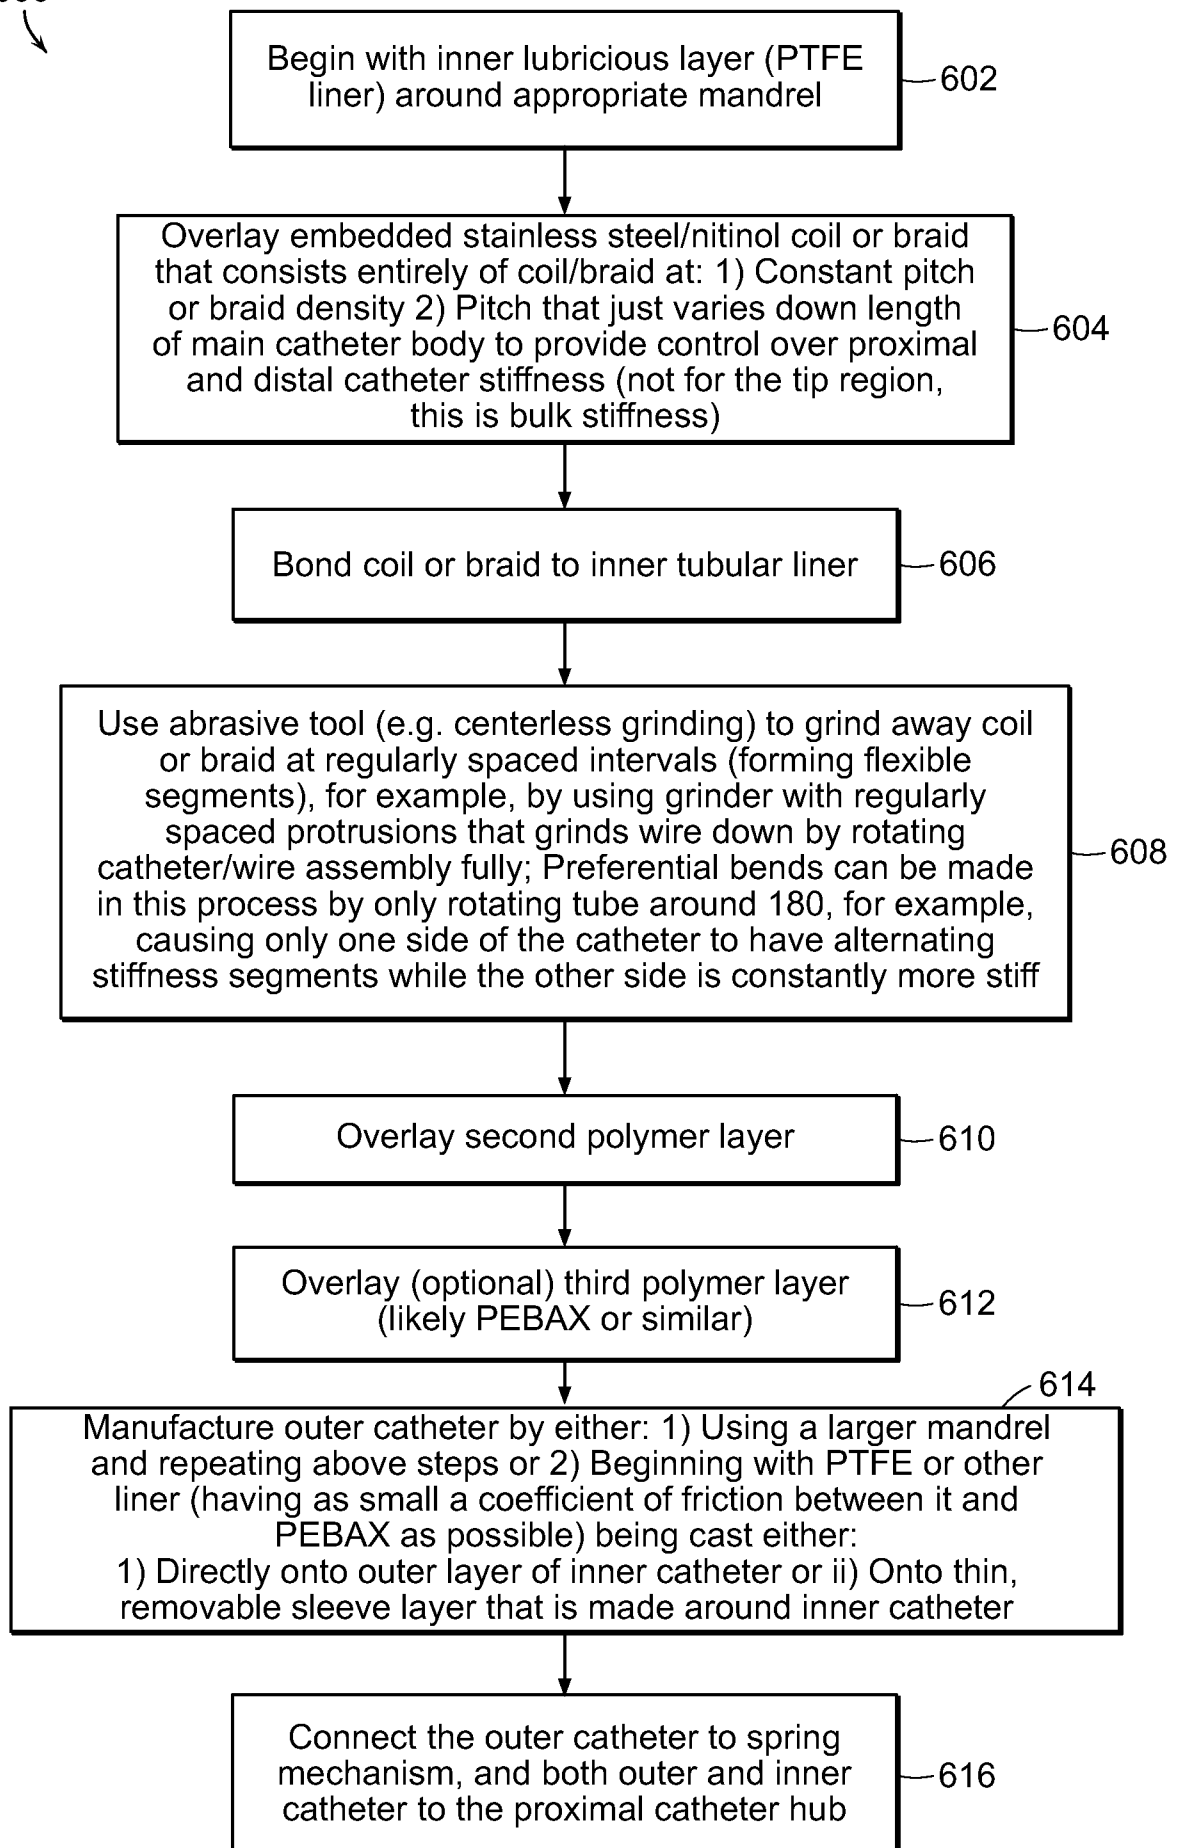



FIG. 10


13/23


600
↓

700
↓

14/23

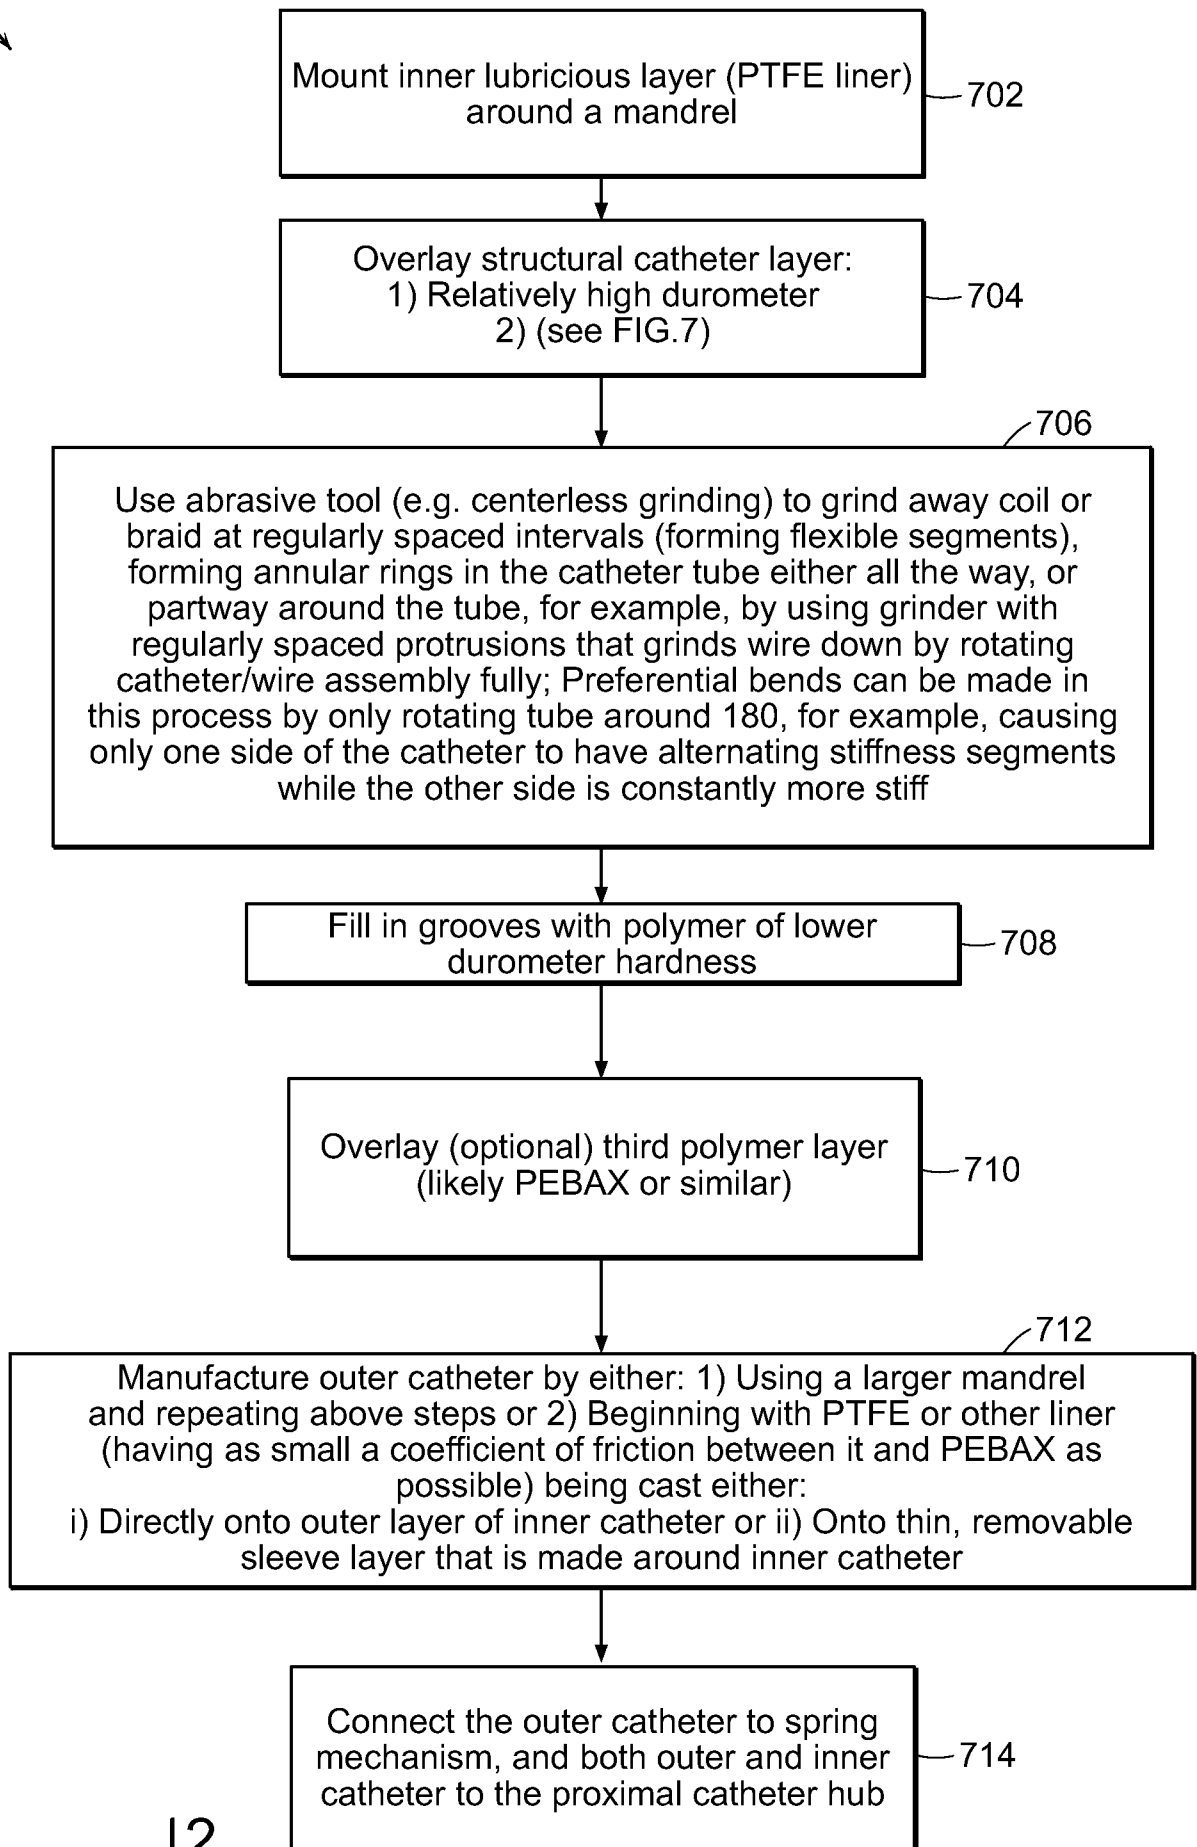

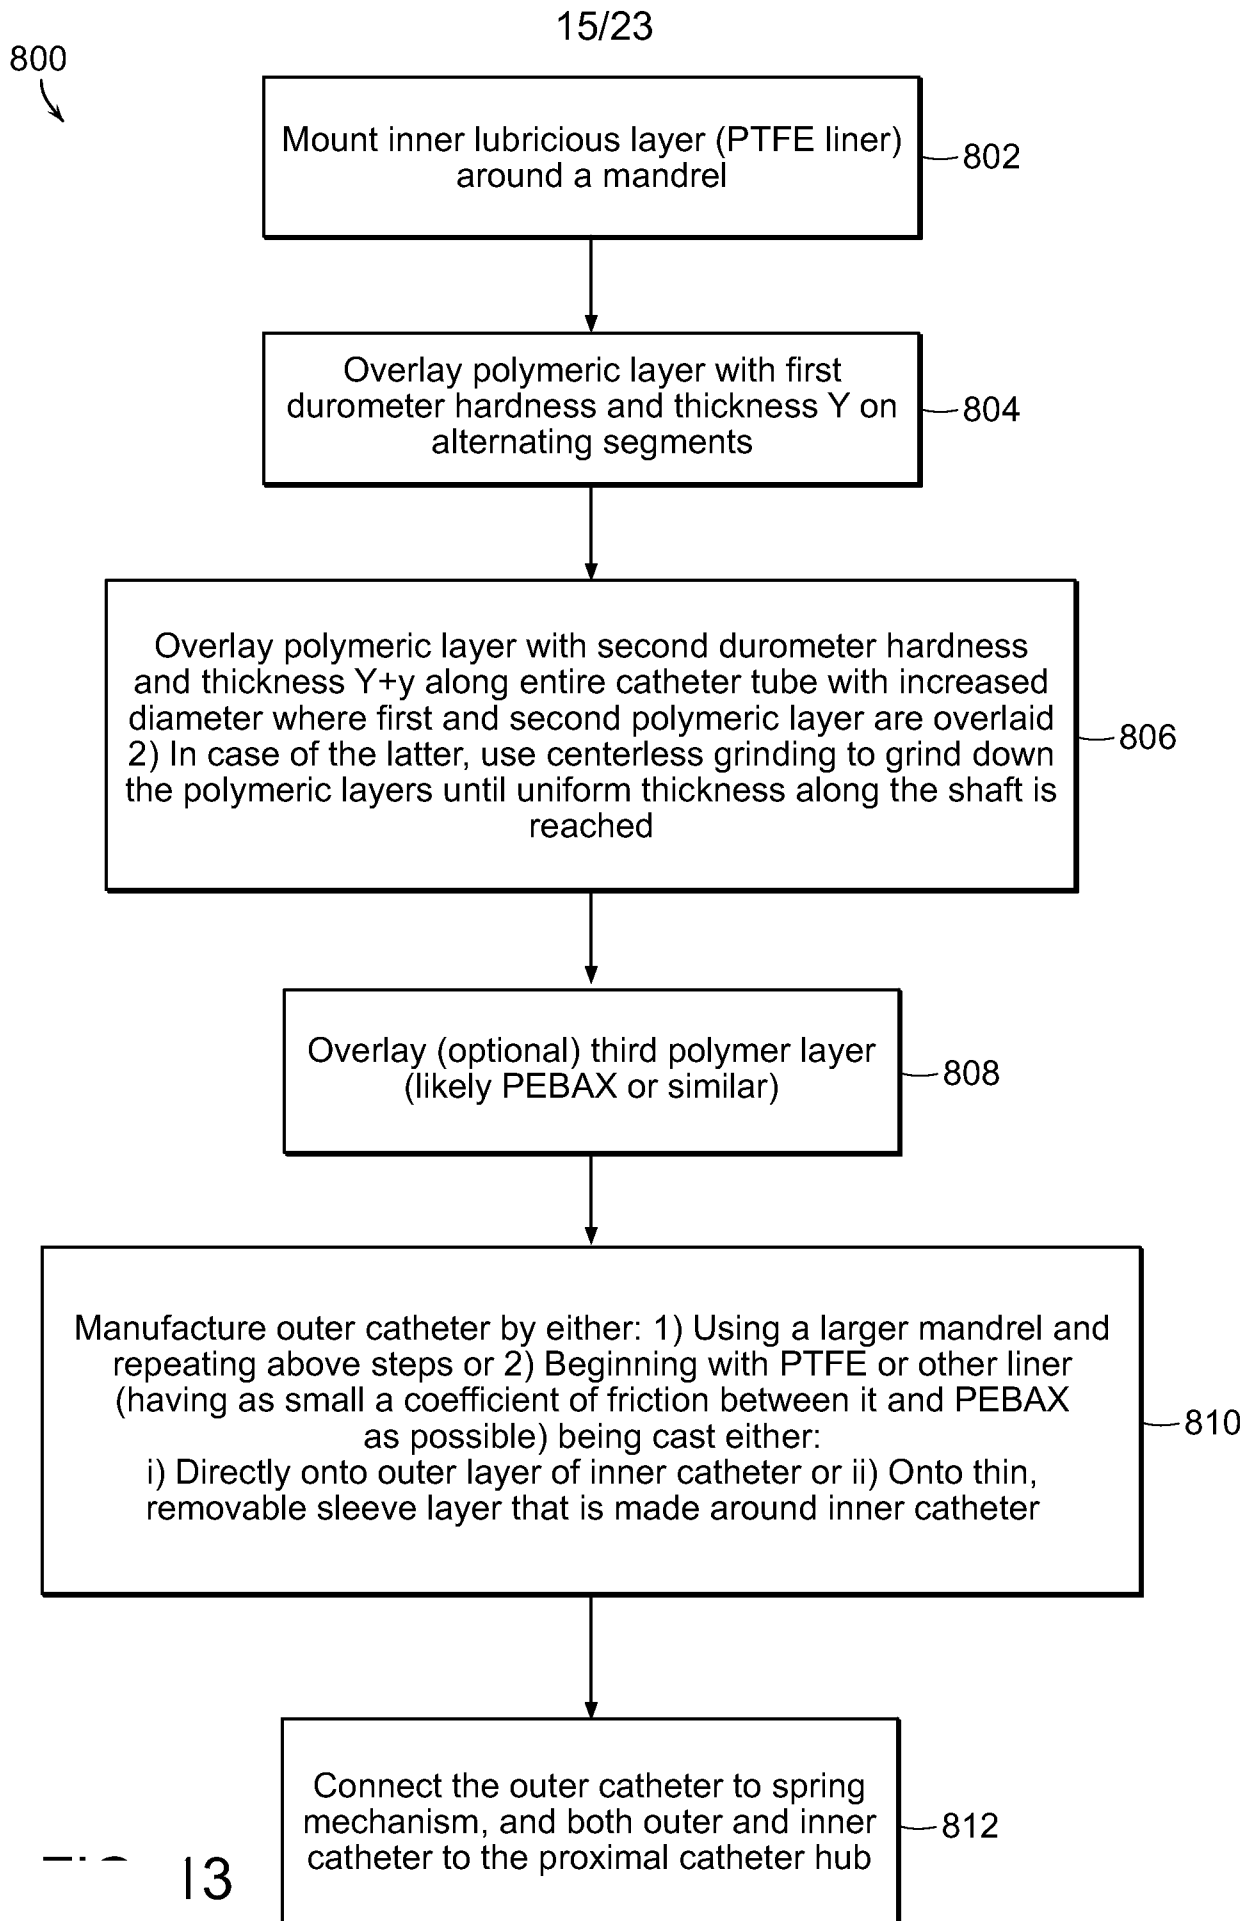

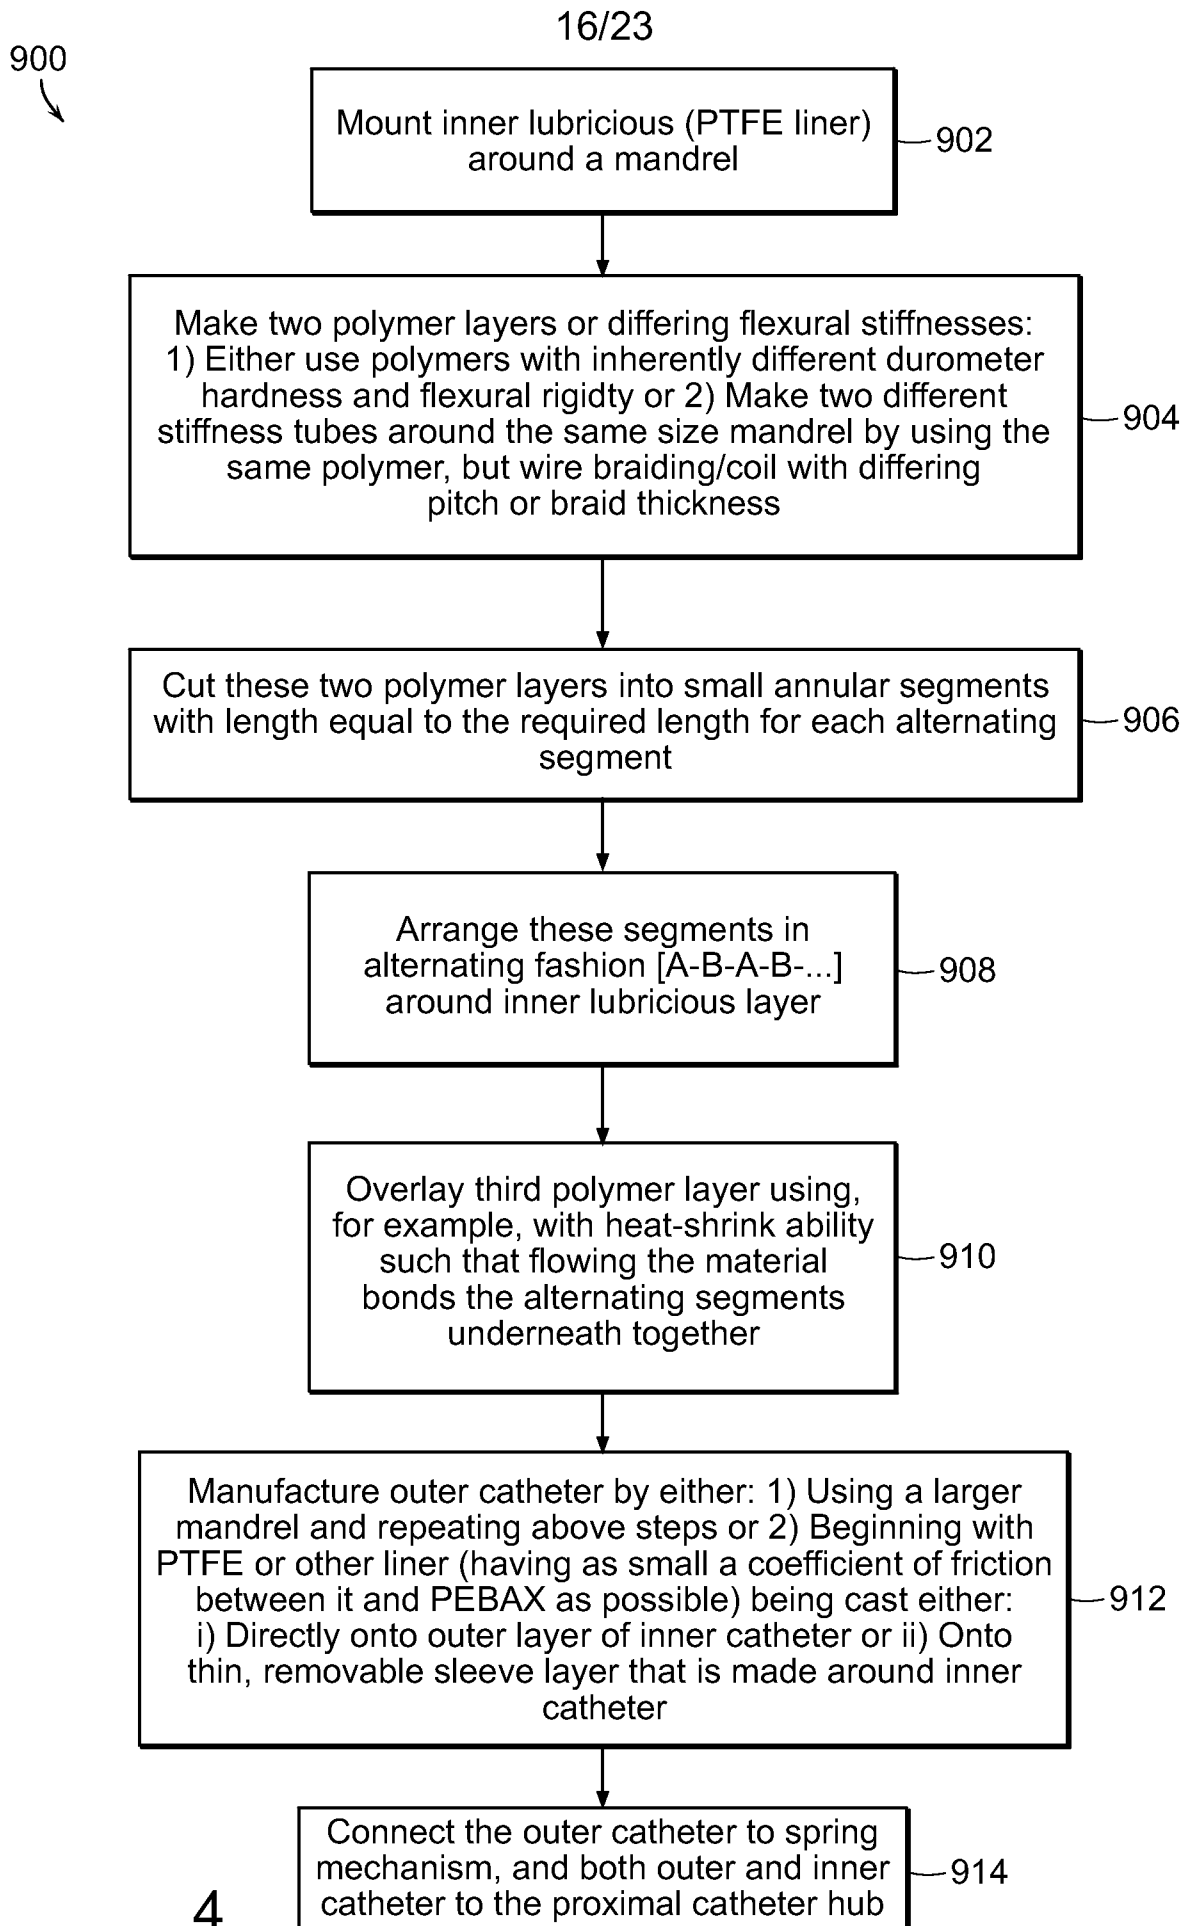

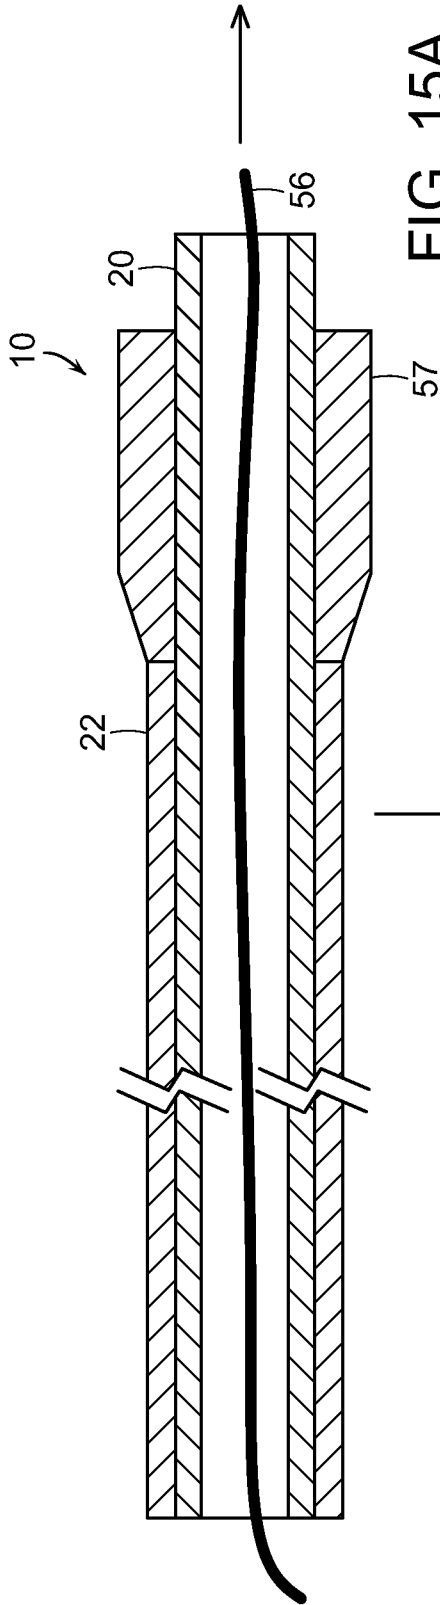


FIG. 15A

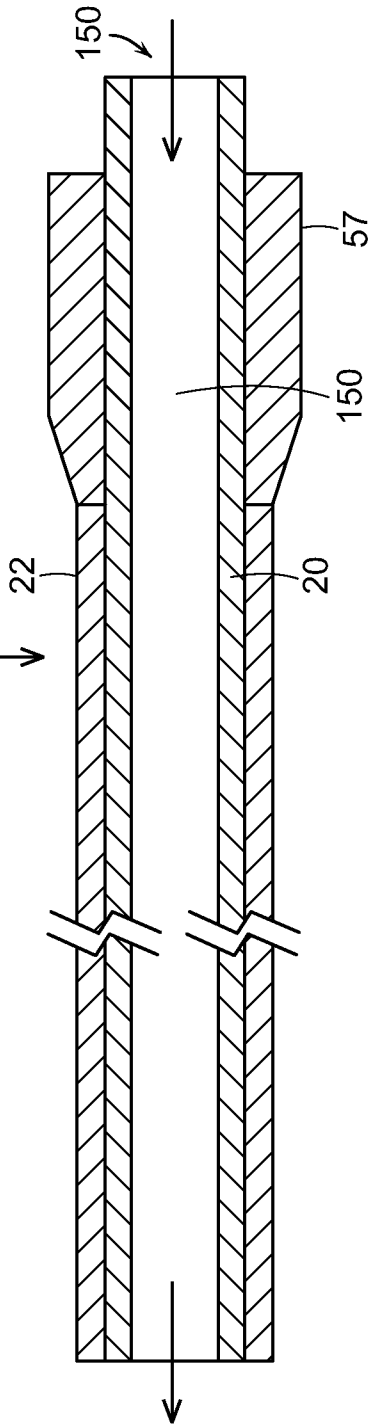


FIG. 15B

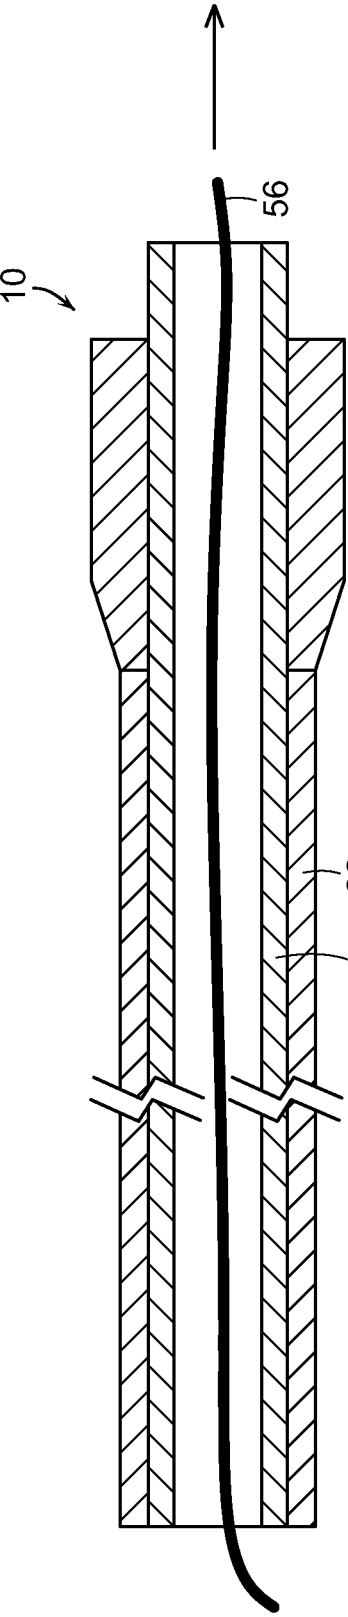


FIG. 16A

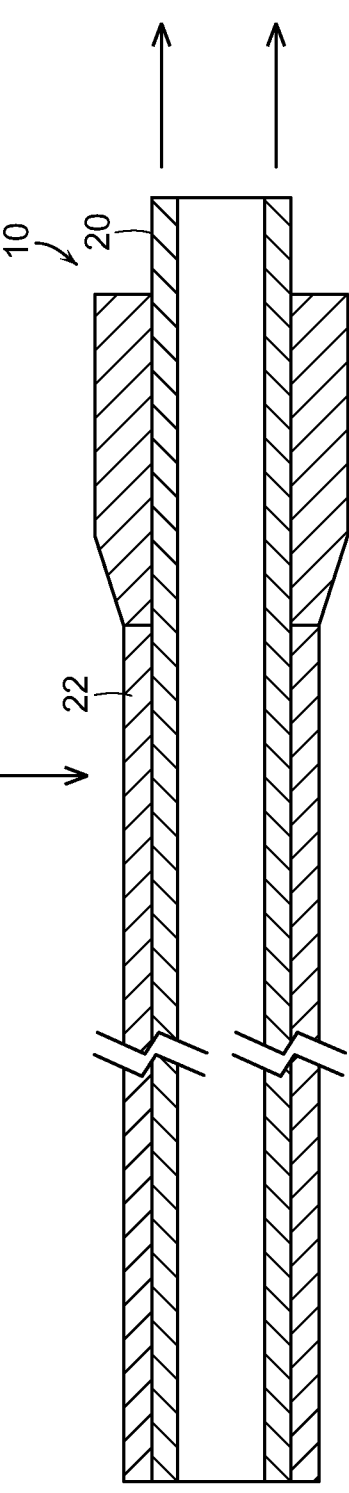


FIG. 16B

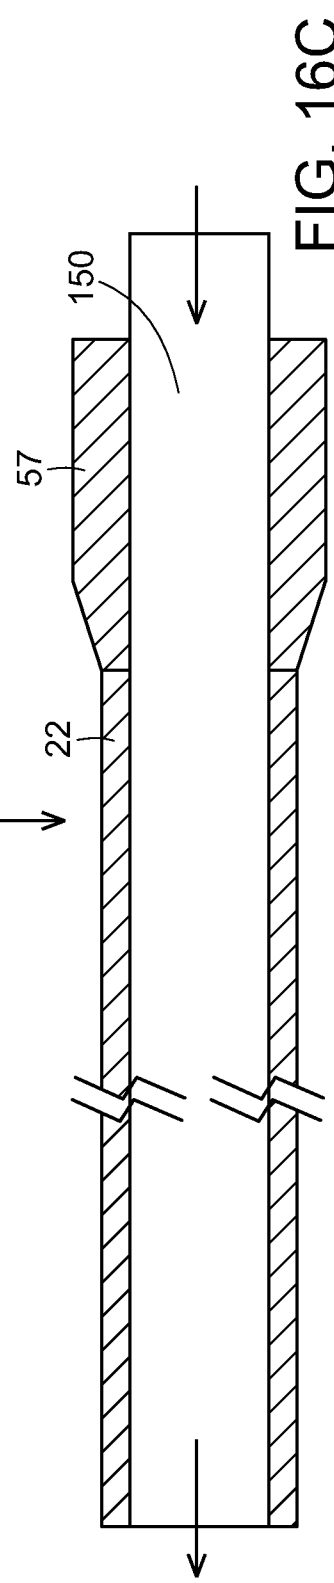


FIG. 16C

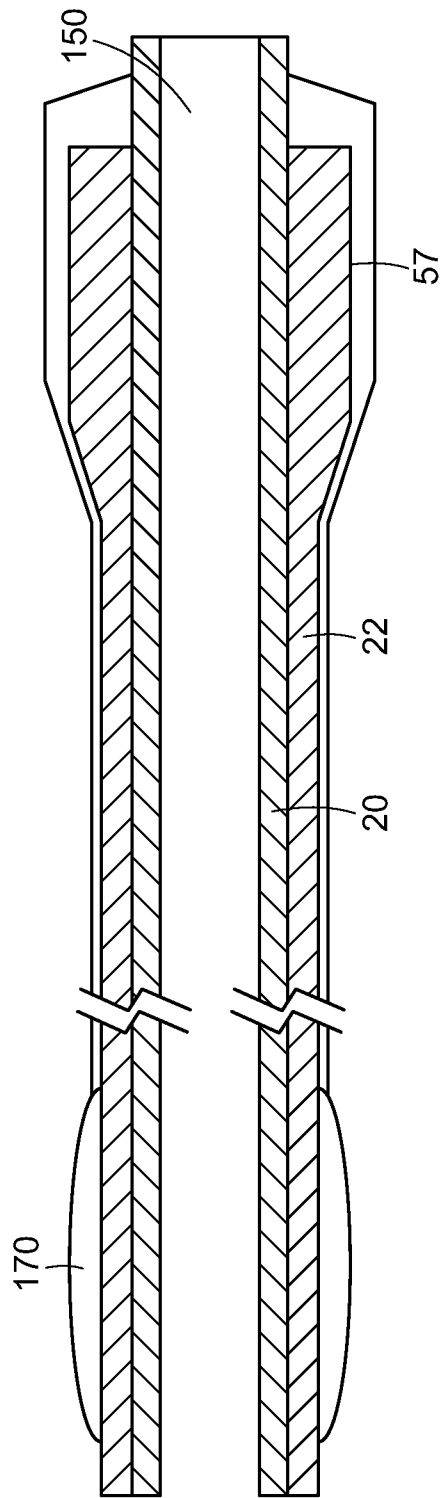


FIG. 17

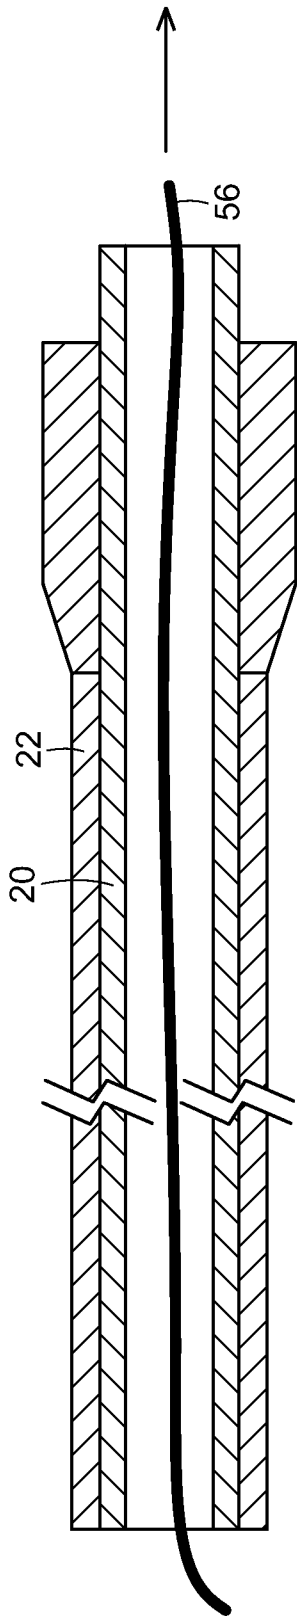


FIG. 18A

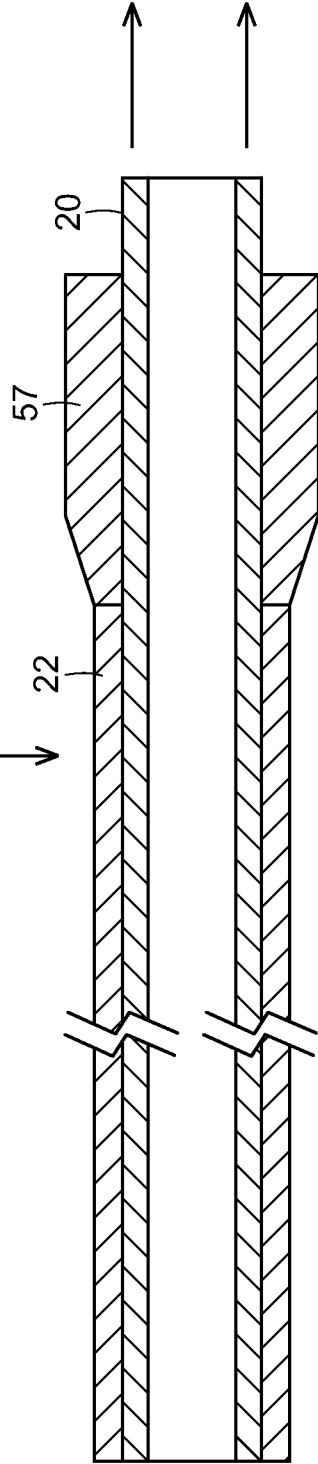


FIG. 18B

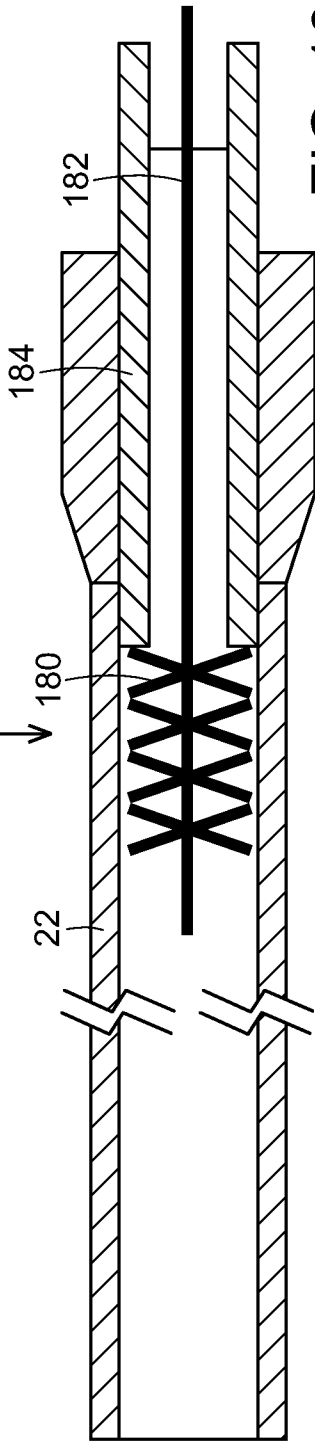


FIG. 18C

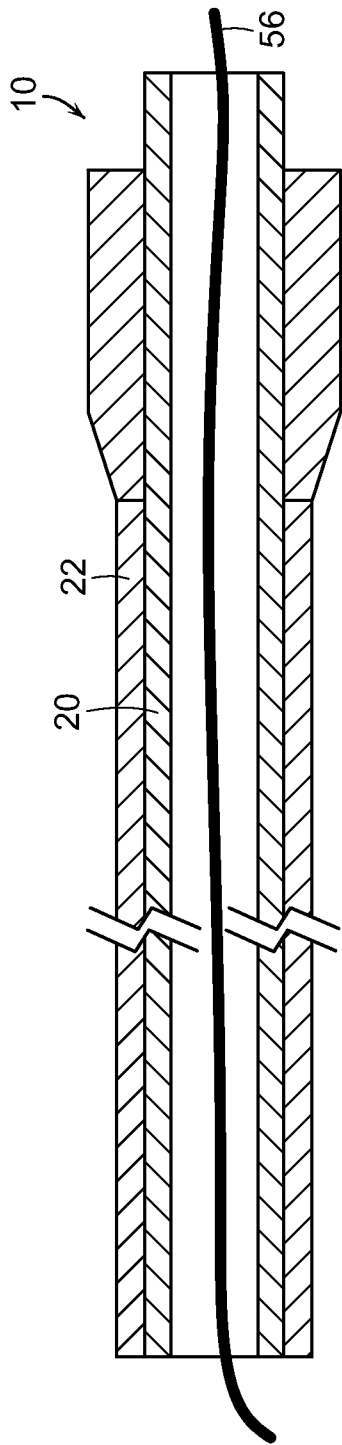


FIG. 19A



FIG. 19B

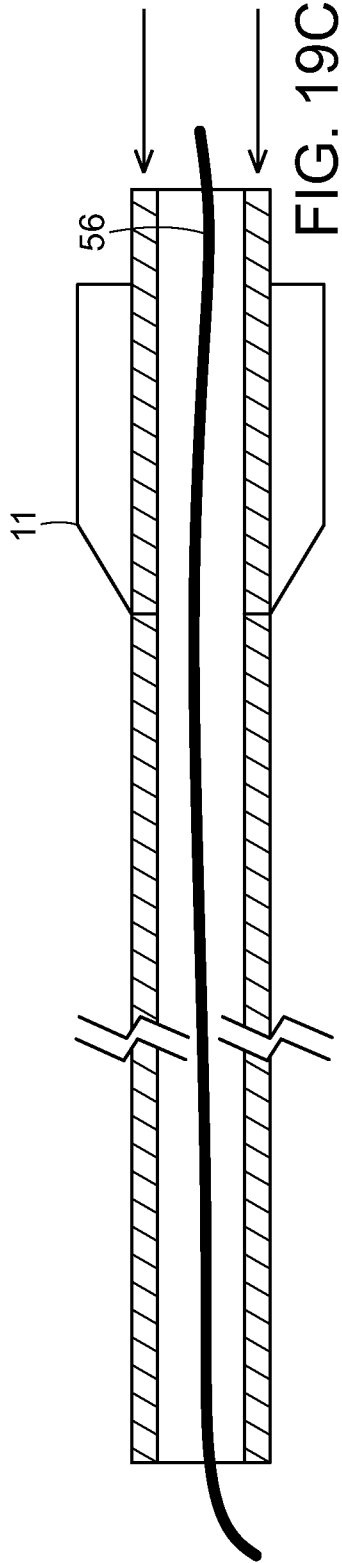


FIG. 19C

22/23

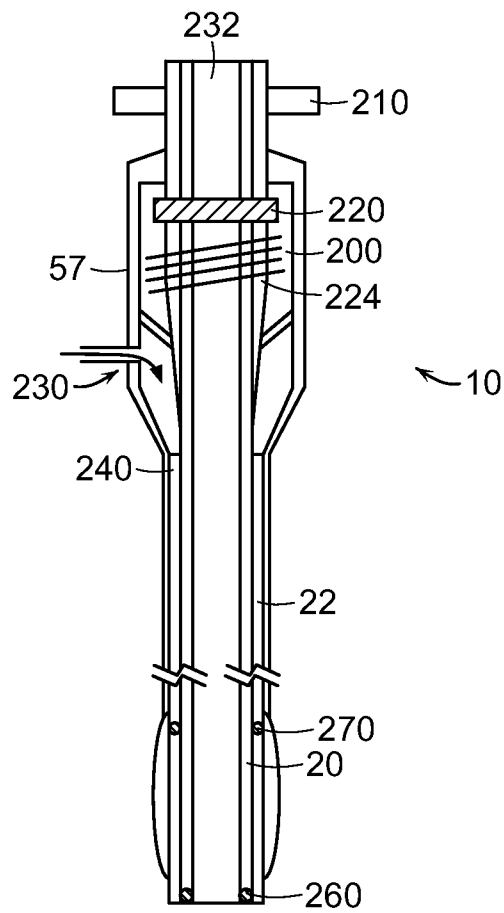
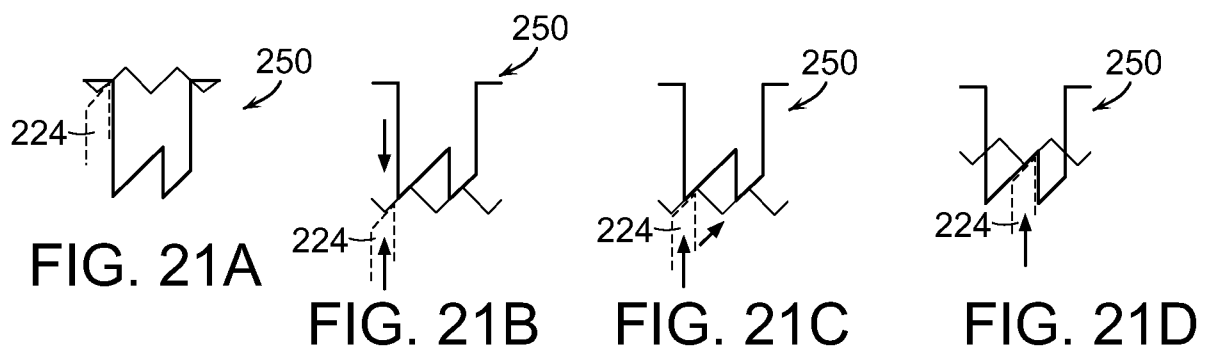


FIG. 20



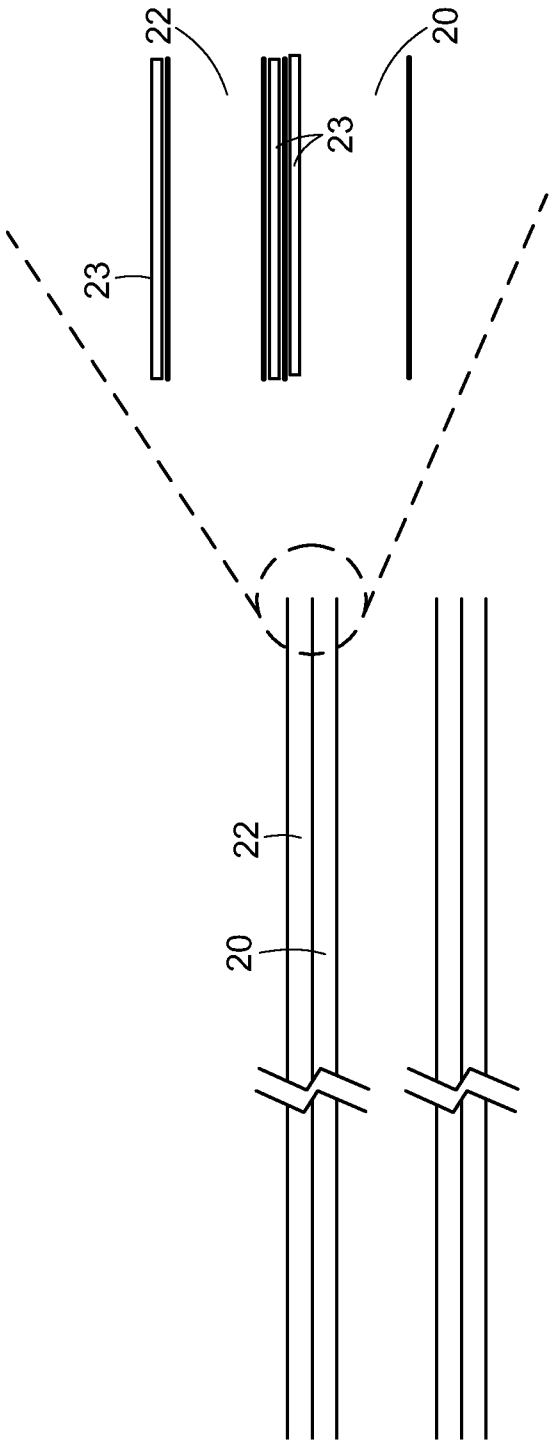


FIG. 22B

FIG. 22A

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2014/017179

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61B17/00 A61F2/95 A61B1/00
ADD. A61M25/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61M A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EP0-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2007/028058 A2 (BOSTON SCIENT SCIMED INC [US]; GREGORICH DANIEL J [US]; YOON SOO-YOUNG) 8 March 2007 (2007-03-08)	1,2,5-7, 9-27, 29-42, 92,93, 96-115
A	figures 1-6 paragraph [0002] paragraph [0049] - paragraph [0050] paragraph [0052] paragraph [0054]	3,4,8, 28,94, 95, 116-120
A	----- WO 2008/057839 A2 (PERCUTANEOUS SYSTEMS INC [US]; HUANG ALEX [US]; DESAI RUPESH [US]) 15 May 2008 (2008-05-15) claims 1-45; figures 1-14 ----- -/--	1-42, 92-120



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

21 March 2014

Date of mailing of the international search report

01/04/2014

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Przykutta, Andreas

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2014/017179

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: **43-91**
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2014/017179

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2010/014882 A1 (PILE-SPELLMAN JOHN [US]; LIN ERWIN [US]) 4 February 2010 (2010-02-04) claims 1-20 -----	1-42, 92-120
A	WO 2007/057132 A1 (MICROMUSCLE AB [SE]; KROGH MAGNUS [SE]; JAGER EDWIN [SE]) 24 May 2007 (2007-05-24) claims 1-57 -----	1-42, 92-120

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2014/017179

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2007028058	A2	08-03-2007	CA 2621220 A1 08-03-2007
		EP 1933918 A2 25-06-2008	
		JP 2009506839 A 19-02-2009	
		US 2007060880 A1 15-03-2007	
		US 2011301574 A1 08-12-2011	
		US 2013096535 A1 18-04-2013	
		WO 2007028058 A2 08-03-2007	
WO 2008057839	A2	15-05-2008	US 2008172037 A1 17-07-2008
			WO 2008057839 A2 15-05-2008
WO 2010014882	A1	04-02-2010	NONE
WO 2007057132	A1	24-05-2007	CA 2630215 A1 24-05-2007
		EP 1957141 A1 20-08-2008	
		JP 2009515617 A 16-04-2009	
		US 2009082723 A1 26-03-2009	
		WO 2007057132 A1 24-05-2007	