



(51) International Patent Classification:
A61B 34/30 (2016.01)

(21) International Application Number:

PCT/US2018/036349

(22) International Filing Date:

06 June 2018 (06.06.2018)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/515,762

06 June 2017 (06.06.2017)

US

(71) Applicant: **THE REGENTS OF THE UNIVERSITY OF CALIFORNIA** [US/US]; 1111 Franklin St., Oakland, CA 94607 (US).

(72) Inventors: **GUNN, Aaron**; c/o UCSD, 9500 Gilman Drive, La Jolla, CA 92093-0448 (US). **WEISSBROD, Philip**; c/o

UCSD, 9500 Gilman Drive, La Jolla, CA 92093-0448 (US).
YIP, Michael; c/o UCSD, 9500 Gilman Drive, La Jolla, CA 92093-0448 (US).

(74) Agent: **MAYER, Stuart, H.** et al.; Mayer & Williams P.C., 55 Madison Avenue, Suite 400, Morristown, NJ 07960 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) Title: MULTI-CATHETER FLEXIBLE ROBOTIC SYSTEM

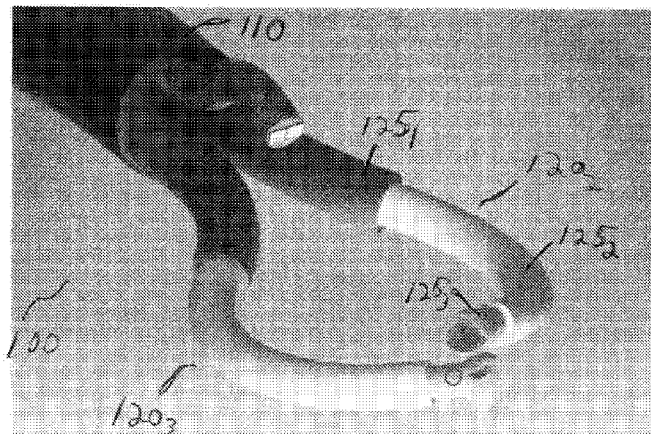


Figure 2

(57) Abstract: A multicatheter subsystem is provided for a steerable catheter robotic system. The subsystem includes a flexible output sheath, a plurality of flexible multi-lumen assemblies and a plurality of robotic instruments for performing a surgical procedure. The plurality of flexible multi-lumen assemblies extends through the outer sheath. Each of the multi-lumen assemblies has a proximal end and a distal end. Each of the robotic instruments is operatively and removably attachable to the distal end of one of the multi-lumen assemblies such that each instrument is teleoperable independently of every other robotic instrument. At least a first of the robotic instruments includes a plurality of interconnected articulating segments. Each of the articulating segments is operatively and removably attachable to a different one of the multi-lumen assemblies.





(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

MULTI-CATHETER FLEXIBLE ROBOTIC SYSTEM

Cross-Reference to Related Applications

[0001] This application claims benefit of priority of US Provisional Patent Application Serial Number 62/515,762, filed June 6, 2017, entitled " MULTI-CATHETER FLEXIBLE ROBOTIC SYSTEM ", owned by the assignee of the present application and herein incorporated by reference in its entirety.

Background

[0002] Remotely-controlled surgical instruments, which can include teleoperated surgical instruments (e.g., surgical instruments operated at least in part with computer assistance, such as instruments operated with robotic technology) as well as manually operated (e.g., laparoscopic, thorascopic) surgical instruments, are often used in minimally invasive medical procedures. During such procedures, a surgical instrument, which may extend through a cannula inserted into a patient's body, can be remotely manipulated to perform a procedure at a surgical site. For example, in a teleoperated surgical system, cannulas and surgical instruments can be mounted at manipulator arms of a patient side cart and be remotely manipulated via teleoperation at a surgeon console.

[0003] In the present landscape of surgical robotics, the field of continuum (or flexible) surgical robotic systems is still very much in development. These biomimetic systems, many modeled after tentacles or trunks, allow for minimally-invasive access to previously unreachable anatomy. By developing these devices with a smaller footprint and more robust laminate manufacturing techniques, lower impact surgery can be portably and efficiently performed in even tighter spaces than traditional rigid surgical robots.

Summary

[0004] In accordance with one aspect of the present disclosure, a multicatheter subsystem is provided for a steerable catheter robotic system. The subsystem includes a flexible output sheath, a plurality of flexible multi-lumen assemblies and a plurality of robotic instruments for

performing a surgical procedure. The plurality of flexible multi-lumen assemblies extends through the outer sheath. Each of the multi-lumen assemblies has a proximal end and a distal end. Each of the robotic instruments is operatively and removably attachable to the distal end of one of the multi-lumen assemblies such that each instrument is teleoperable independently of every other robotic instrument. At least a first of the robotic instruments includes a plurality of interconnected articulating segments. Each of the articulating segments is operatively and removably attachable to a different one of the multi-lumen assemblies.

Brief Description of the Drawings

[0005] FIGs. 1 and 2 show perspective views of a multi-catheter subsystem.

[0006] FIG. 3 shows one example of a multi-lumen assembly that is used to steer a single one of the robotic instruments shown in FIGs. 1 and 2.

[0007] FIG. 4 shows a motor control assembly.

[0008] FIG. 5 shows a pulley housing assembly.

[0009] FIG. 6 shows an example of a steerable catheter robotic system that includes the multi-catheter subsystem shown in FIGs. 1 and 2.

Detailed Description

[00010] As described in more detail below, a steerable catheter robotic system with a significantly reduced size-footprint is provided for deployment in field or outpatient pulmonary surgical procedures. The small size and portability of this system can help overcome a major disadvantage of current surgical robots which take up an immense amount of space in already crowded-operating rooms, while still being able to imitate, copy and improve human capabilities. In some embodiments the dimensions of the robotic instruments or tools may be as small as 1 mm.

[00011] FIGs. 1 and 2 show perspective views of a multi-catheter subsystem 100 that includes a flexible outer guide shaft 110 having a distal end from which one or more robotic instruments extend. Although the embodiment shown in FIGs. 1 and 2 shows three robotic instruments 120₁, 120₂ and 120₃ ("120"), more generally any number of such robotic instruments 120 may be employed. In this particular embodiment the robotic instruments 120 include a camera 120₁ and first and second grasping forceps 120₂ and 120₃. A control assembly (not shown

in FIGs. 1 and 2) is located at the proximal end of the outer sheath 110 controls the operation of the robotic instruments 120.

[00012] In some embodiments each robotic instrument 120 may include two or more articulating segments that provide the instrument with multiple degrees of freedom. For instance, as best seen in FIG. 2, the first grasping forcep 120₂ includes three articulating segments 125₁, 125₂ and 125₃. The second grasping forcep 120₃ may be similarly configured. By employing a suitable number of articulating segments, some instruments may be supplied with 7 degrees of freedom of articulation (i.e. positional control of x, y, z in cartesian space, and roll-pitch-yaw in orientation, and an actuation degree of freedom such as a pinch grip of a forcep), thereby essentially recovering the dexterity of a human hand. In such an embodiment a one-to-one mappings can be advantageously realized of a teleoperating using to the robotic instrument. If more than 7 degrees of freedom are provided to a given instrument, the instrument can have additional degrees of freedom to conform to the environment without affecting the controllability of the 7 degrees of freedom that are controlled by the human operator. Some instruments may have additional elbow deflection locations that allow the shape of the instrument to better conform to the environment.

[00013] When one of the robotic instruments is a camera, it may be operated with only 6 degrees of freedom for full visual control, although the focal depth (if so integrated) may be considered a 7th degree of freedom.

[00014] FIG. 3 shows one example of a multi-lumen assembly 200 that is used to steer a single instrument 120. Each of the lumens is formed from a flexible material such as a flexible polymer. The multi-lumen assembly 200 extends through the outer guide shaft 110 shown in FIG. 1. The multi-lumen assembly 200 includes a center channel 210 that has a liner 212 that serves as an instrument port for one segment of a multi-segment instrument (or a complete instrument of a single-segment instrument). Surrounding the center channel 210 are a series of control lumens 220 through which articulation wires (not shown) extend. In this example 4 control lumens 220₁, 220₂, 220₃ and 220₄ are shown. The control lumens 220 are secured (e.g., fused) to the center channel 210. Articulation of the instrument segment located in the center channel 210 is determined by the coordinated operation of the articulation wires via the control assembly, which will be described below. The center channel 210 and the control lumens 220

may extend through a flexible sheath 230 (which itself extends through the outer guide shaft 110 shown in FIGs. 1 and 2).

[00015] Each articulating segment of a multi-segment instrument includes its own dedicated multi-lumen assembly 200 for controlling that segment. The different multi-lumen assemblies 200 of a single multi-segment instrument may be concentrically arranged with one another.

[00016] As mentioned above, the multi-lumen assembly 200 may be fabricated from flexible polymers. For example, in some embodiments the flexible sheath 230 and center channel 210 may be formed from a varying durometer thermoplastic polymer such as a polyester block amide (available, for instance, under the tradename PEBAX[®]). An optional stainless steel or fiber braid (not shown) may surround the flexible sheath 230. Likewise, in some embodiments the control lumens may be formed polyimide and the liner 212 lining the center channel 210 may be formed from PTFE (i.e., Teflon[®]). The use of flexible polymers for the multi-lumen assembly affords significant flexibility in short segments without deterioration of the assembly and tight radiuses of curvatures can be achieved. Lamination of these polymers, which can become micron-thickness layers, enables these robotically controlled lumens to reach as small as 1 mm in diameter.

[00017] FIG. 4 shows a motor control assembly 400 that can be used in conjunction with a pulley housing assembly 500 (FIG. 5) to control the four pull wires that extend through the control lumens 220. The motor control assembly 400 includes four motors 410₁, 410₂, 410₃ and 410₄ (where motor 410₄ is not visible in FIG. 4). that each respectively control the rotation of a rotatable shaft 415₁, 415₂, 415₃ and 415₄. The pulley housing assembly 500 includes four torque-limiting pulleys 510₁, 510₂, 510₃ and 510₄. When the pulley housing assembly 500 is mated with the motor control assembly 400 each pulley 510₁, 510₂, 510₃ and 510₄ is axially mounted on one of the shafts 415₁, 415₂, 415₃ and 415₄. The pulley housing assembly 500 also includes a shaft mount 520 onto which is mounted the outer guide shaft 110 and the multi-lumen assemblies 200 extending therethrough. Once installed, rotational actuation of the motors 410 located in the motor control assembly 420 is translated to linear actuation, providing four degrees of freedom to each instrument segment.

[00018] The motor control assembly 400 includes an additional motor 410₅ that is used to extend and retract the robotic instrument under its control.

[00019] The control of the robotic instruments is accomplished using inverse kinematics to map Cartesian coordinates into the positions of the four pull wires. Coordinates are first multiplied by a dynamically adjustable rotation matrix, and then by constants derived during a simple calibration process in order to standardize actuation across multiple instruments. A position-based control approach using analog values to scale targets in Cartesian space that are then mapped to R^4 , resulting in high position accuracy along with precise control over actuation velocity. The final result is accurate and intuitive control over two degrees of freedom per instrument, all mapped to a user interface.

[00020] FIG. 6 shows an example of the steerable catheter robotic system that includes the multi-catheter subsystem 110 shown in FIGs. 1 and 2, which includes the three instruments 120₁, 120₂ and 120₃. Like reference numerals shown in FIG. 6 and the remaining figures denote like elements. As shown, the proximal end of the multi-catheter subsystem 110 includes controllers 550₁, 550₂, 550₃ and 550₄ ("550"). Each controller 550 includes one of the motor control assemblies 400 mated with one of the pulley housing assemblies 500. Controller 550₁ is used to control instrument 120₁, controller 550₂ is used to control instrument 120₂ and controller 550₃ is used to control instrument 120₃. The additional controller 550₄ is used control the overall movement of the multi-catheter subsystem 110.

[00021] Control of the steerable catheter robotic system via a user interface (not shown) focuses on two distinct tasks: robot movement and multiple catheter articulation. Both movements can be controlled from a single console. For instance, in one embodiment the operator is able to advance the robot via a haptic joystick. The path of the multi-catheter subsystem can be visualized on a display of the user interface console. The display may include a high-definition or 3-D screen. Additional screens within the console may allow for projection of imaging studies or electromagnetic instrument registration for use during the procedure being performed. The joystick allows forward and backward movement and 180° movement in an x and y plane of the distal tip. To prevent traumatic navigation, haptic feedback may be provided which is associated with the platform movement. Once positioned in the desired location, the platform can be fixed to allow stability during instrument insertion and movement.

[00022] As discussed above, in one embodiment there are two articulating instruments that can be inserted through the length of the multi-catheter subsystem. Movement of each instrument is controlled by independent finger grasping interfaces. The instruments can be advanced or

withdrawn by depression or retraction of a grasping unit. In instances where there are no grasping movements, the instruments may be moved as if grasping a virtual pencil.

[00023] A wide variety of different interchangeable robotic instruments may be used in the multi-catheter subsystem. Examples of such instruments include, without limitation, biopsy cups, grasping forceps, injection needles, biopsy needles, laser introducers, basket retrievers, hot knives, clip applicators, and scissors. The instrument or instruments that are used will be application-dependent. Examples of such applications include laryngeal, pharyngeal, hypopharyngeal, tracheal, bronchial, esophageal, stomach, large and small bowel applications. Additionally, applications include newer advanced endoscopic procedures, including endoluminal tumor ablation in varying anatomic locations, Peroral Endoscopic Myotomy (POEM), and Natural Orifice Transluminal Endoscopic Surgery (NOTES).

[00024] Robotic instruments may be interchangeable so that the multi-catheter subsystem 100 can swap the types and locations of instruments as required to generate different configurations for a user to extend their ability to work with tissues in a narrow space, extend their reach, improve their visual range, or improve the ergonomics of control. The software controlling the multi-catheter sub-system may reposition its coordinate frame to match an intuitive viewpoint of the teleoperator.

[00025] In some cases it is possible that the system can introduce more robotic instruments than a single user can control. In this scenario, both a primary user and an assistant may operate different instruments through the same system, enabling multiple robotic instruments to be controlled simultaneously. This encourages shared tasks, allowing assistants to help with the retraction of objects or environmental roadblocks while the primary user is operating on the exposed area.

[00026] One embodiment of the system may involve the autonomous control of one instrument that follows or performs some assistive task that follows the behavior of a primary user. For example, a continuous ablation using a laser that reaches deeper within a site may be realized by having one of the robotic instruments follow a user-controlled ablation probe as it moves through the environment, i.e., a robotically controlled camera. In this case one instrument would be teleoperated while the other is autonomous and following the teleoperated camera.

[00027] The ability to simultaneously control and steer multiple robotic instruments can provide critical capabilities in manipulating areas of tissues with bimanual manipulation. For

example, controlled stretching of tissue or peeling of tissue can be achieved only with two or more instruments. Likewise, the ability to mount and control a camera independently of the other instruments (and vice-versa) is a significant advantage over current endoscopic approaches where the endoscope is the camera and dictates the controllability of the instruments exiting from its orientation-fixed instrument lumen. Moreover, the multi-catheter system may be mixed with manual instrumentation given that the instrumentation fits within the available lumens for control.

[00028] Another advantage of the steerable catheter robotic system described herein is that one of its intracorporeal instruments can be used to stabilize another when there is a desire for improved stiffness. For example, an outstretched robotic instrument may become too compliant to lift a tissue that is far away. A support provided from a second robotic instrument may be devised to generate mechanical leverage that can amplify the force generation or the reachability of the original, unsupported instrument. In the same way, the robotic instruments may be used to support the sub-system in general and create anchors to provide stabilization against patient or anatomical motions or more generally to combat moment-arm effects.

[00029] Yet another advantage of the steerable catheter robotic system described herein arises in those embodiments that are fabricated exclusively from polymer or other non-metallic materials since these embodiments may be used in conjunction with magnetic resonance imaging (MRI) techniques.

[00030] Reference in the specification to “an embodiment,” “one embodiment,” “some embodiments,” or “other embodiments” means that a particular feature, structure, or characteristic described in connection with the embodiments is included in at least some embodiments, but not necessarily all embodiments. The various appearances of “an embodiment,” “one embodiment,” or “some embodiments” are not necessarily all referring to the same embodiments. If the specification states a component, feature, structure, or characteristic “may,” “might,” or “could” be included, that particular component, feature, structure, or characteristic is not required to be included. If the specification or claim refers to “a” or “an” element, that does not mean there is only one of the element. If the specification or claims refer to “an additional” element, that does not preclude there being more than one of the additional element.

[00031] While certain exemplary embodiments have been described and shown in the accompanying drawings, it is to be understood that such embodiments are merely illustrative of and not restrictive on the broad invention, and that this invention not be limited to the specific constructions and arrangements shown and described, since various other modifications may occur to those ordinarily skilled in the art.

Claims

1. A multicatheter subsystem for a steerable catheter robotic system, comprising:
 - a flexible output sheath having a proximal end and a distal end;
 - a plurality of flexible multi-lumen assemblies extending through the outer sheath, each of the multi-lumen assemblies having a proximal end and a distal end;
 - a plurality of robotic instruments for performing a surgical procedure, each of the robotic instruments being operatively and removably attachable to the distal end of one of the multi-lumen assemblies such that each instrument is teleoperable independently of every other robotic instrument, at least a first of the robotic instruments including a plurality of interconnected articulating segments, each of the articulating segments being operatively and removably attachable to a different one of the multi-lumen assemblies.
2. The multicatheter system of claim 1 wherein the first instrument is configured to have 7 degrees of freedom.
3. The multicatheter system of claim 1 wherein the flexible outer sheath, the plurality of flexible multi-lumen assemblies and the plurality of robotic instruments are formed from polymer materials.
4. The multicatheter system of claim 1 wherein each of the multi-lumen assemblies includes at least one actuating arrangement for steering the instrument attached thereto.
5. The multicatheter system of claim 4 further comprising a control assembly operatively coupled to the proximal end of the multi-lumen assemblies for providing rotational movement that imparts translational movement to the actuating arrangement.
6. The multicatheter system of claim 5 wherein at least one of the actuating arrangements includes:
 - a plurality of control lumens attached to and surrounding a central lumen to which one of the instruments is removably attached; and

a plurality of pull wires each extending through one of the control lumens, a proximal end of each of the pull wires being operatively connected to the control assembly.

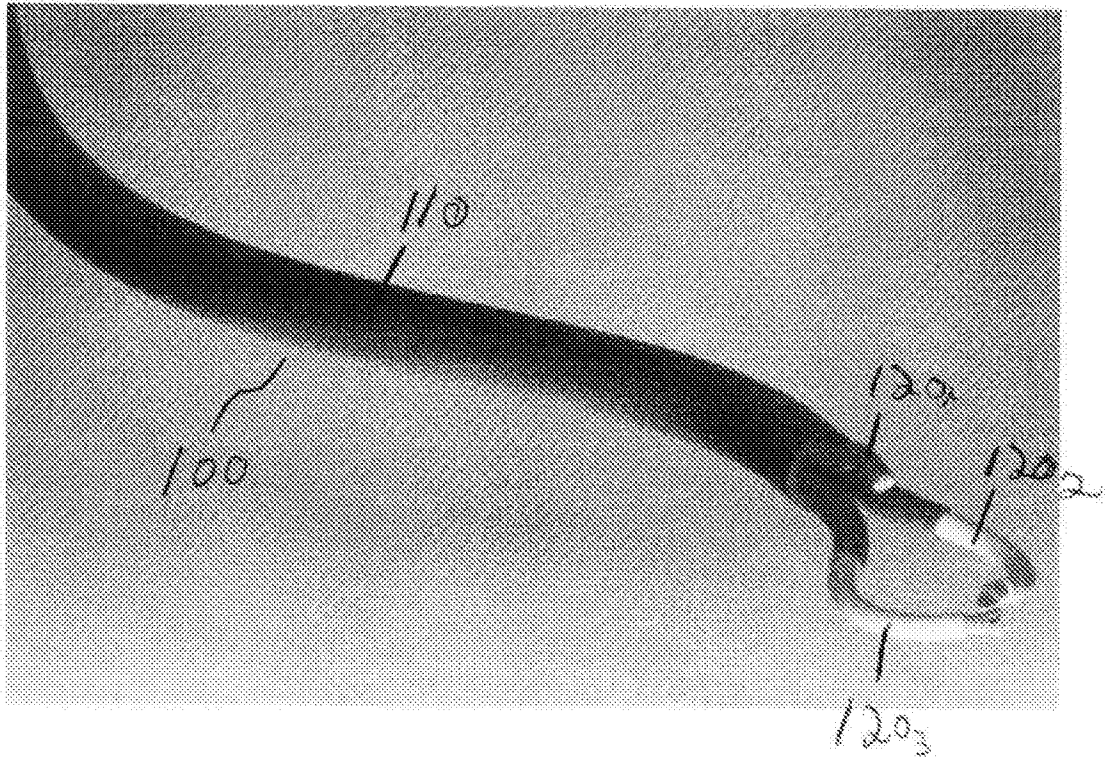


Figure 1

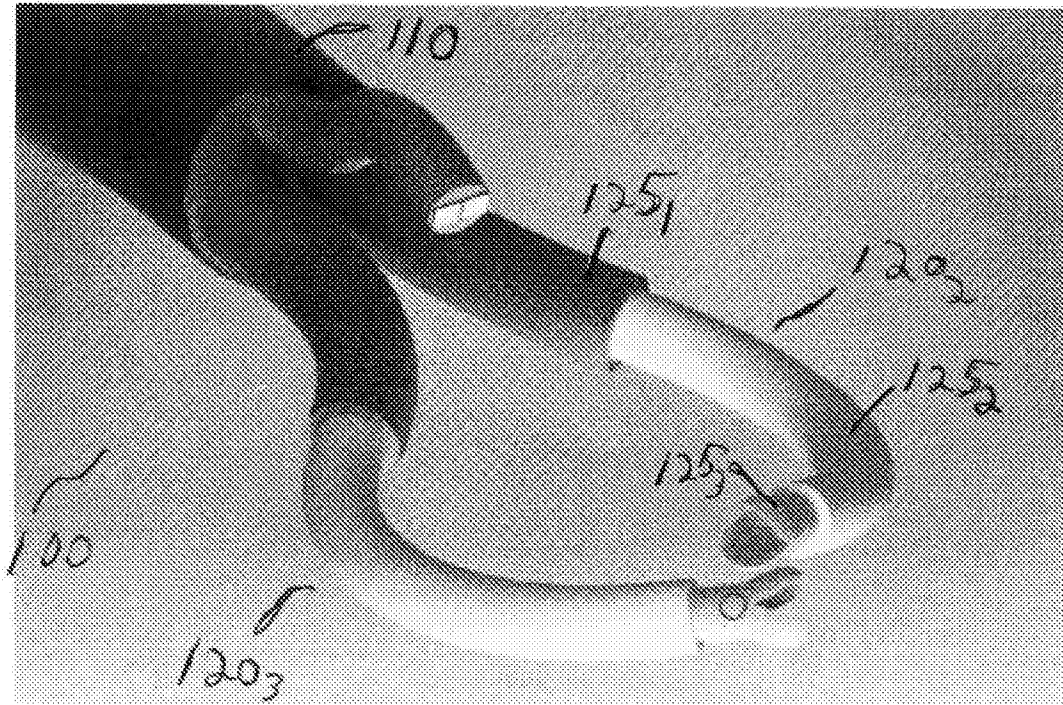


Figure 2

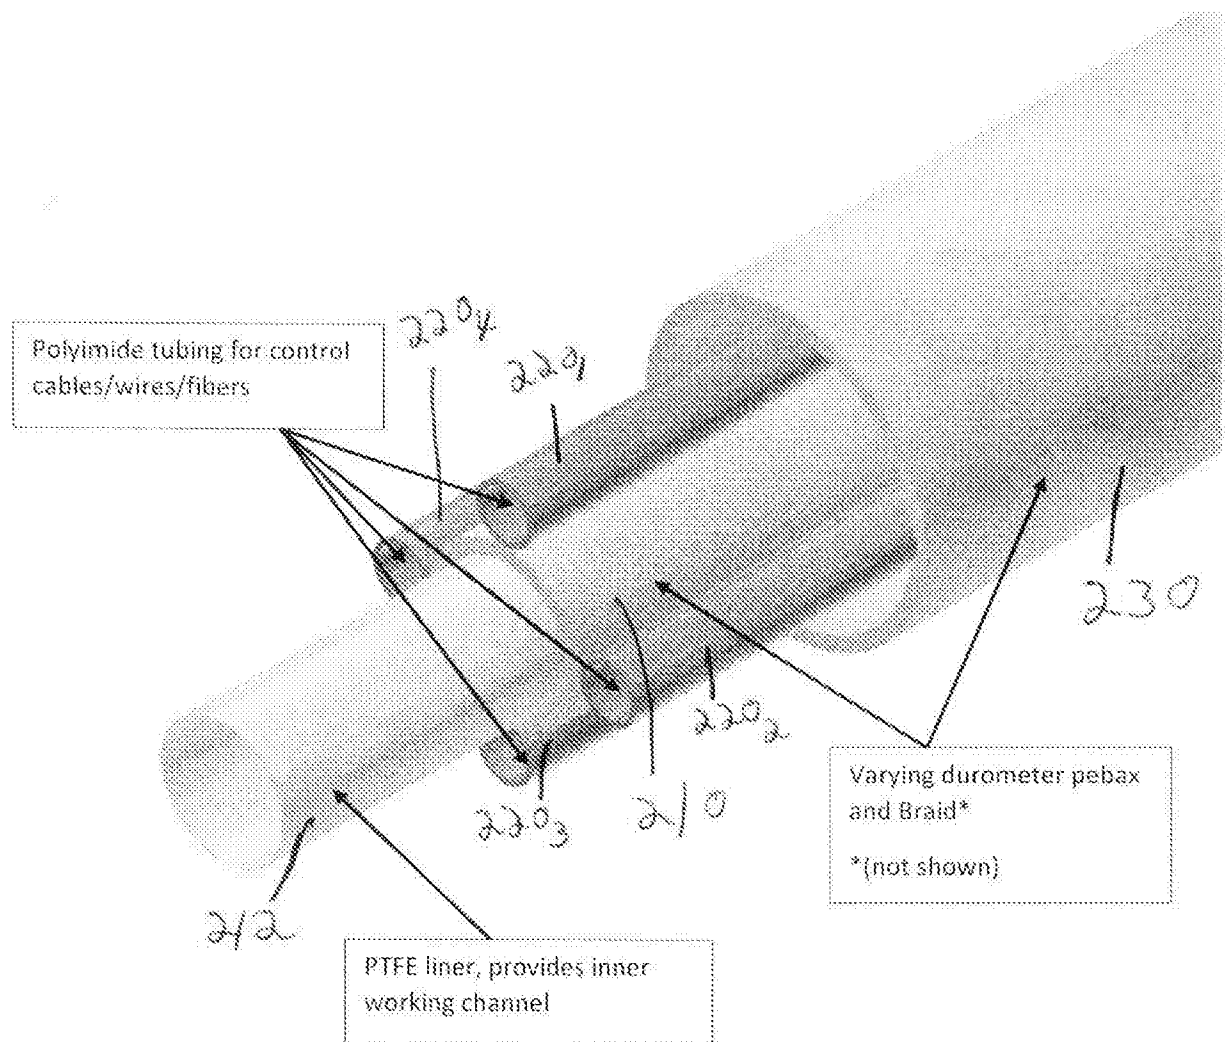


Figure 3

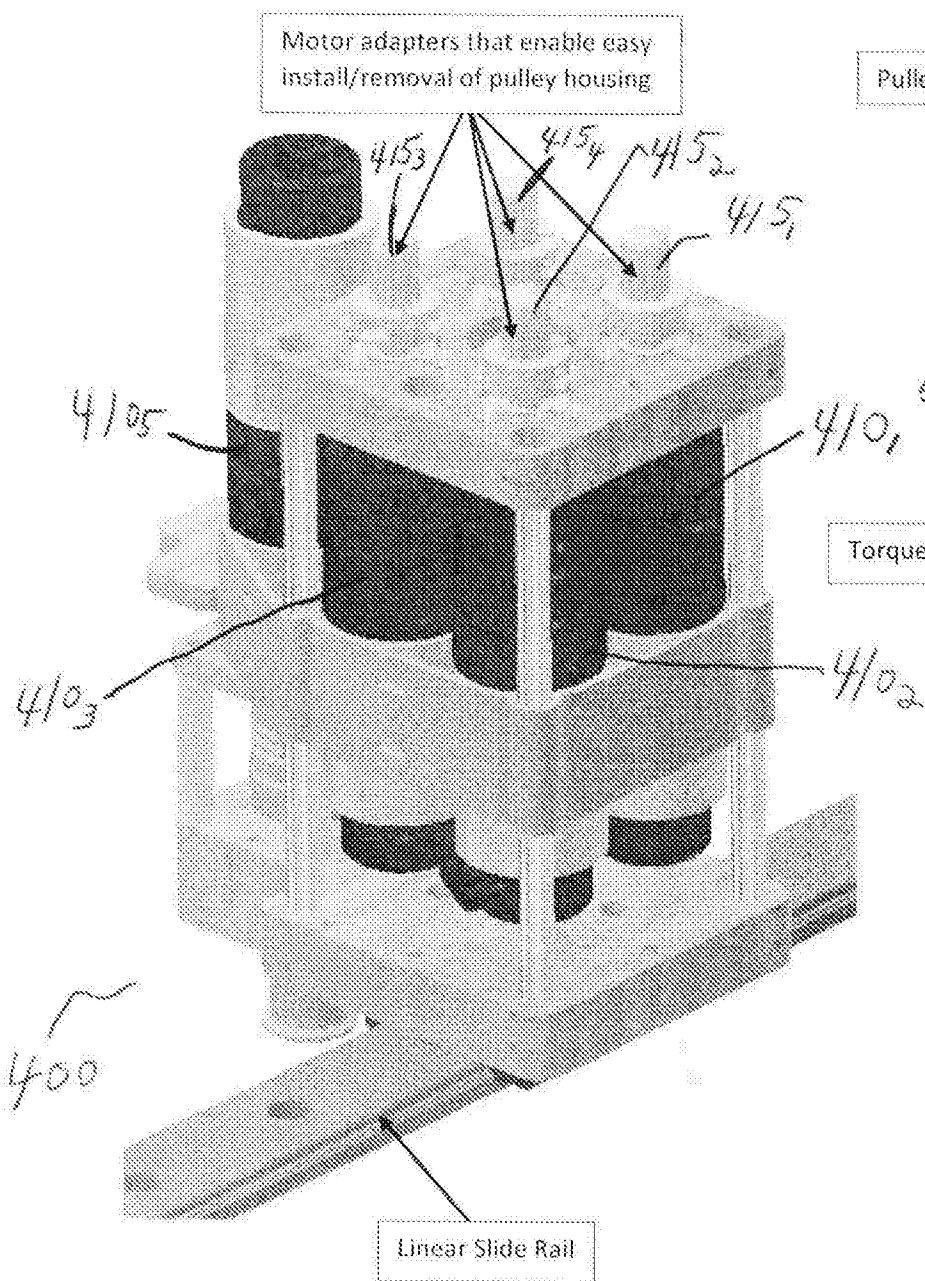


Figure 4

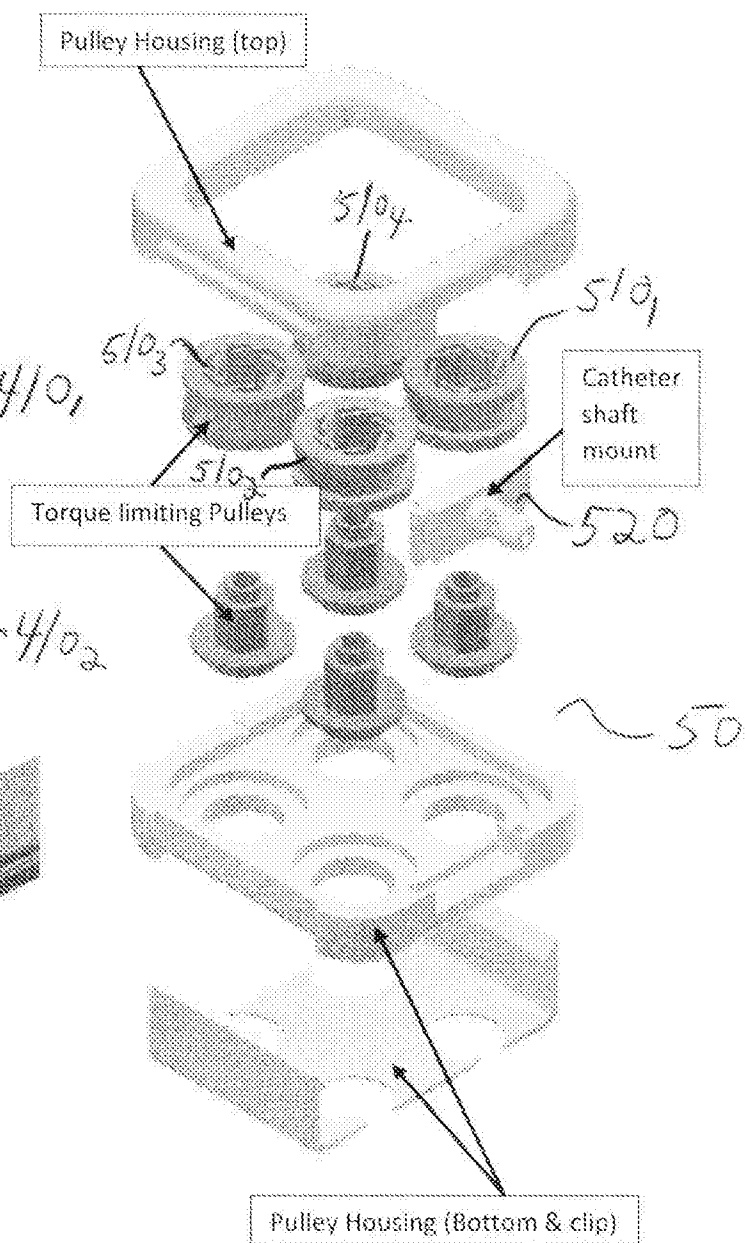


Figure 5

5/5

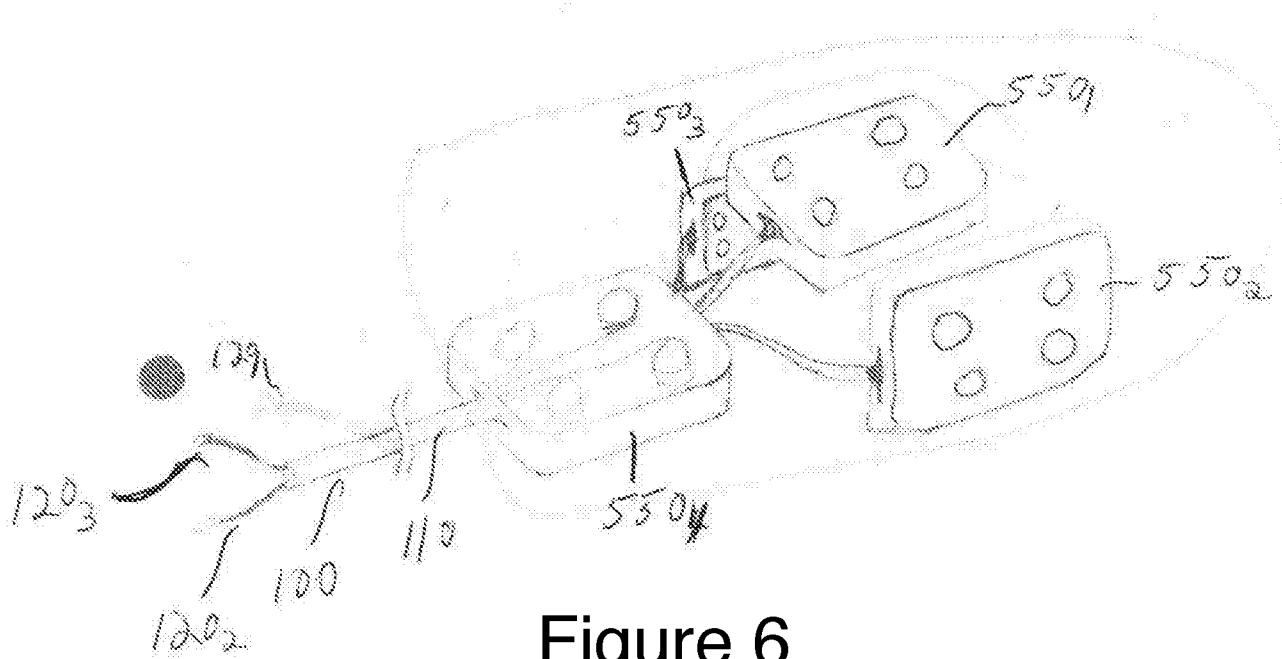


Figure 6

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 18/36349

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 34/30 (2018.01)

CPC - A61B 34/30, A61B 2034/301, A61B 2034/302, A61B 2034/305, A61B 34/71

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History Document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History Document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History Document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2004/0138525 A1 (SAADAT et al.) 15 July 2004 (15.07.2004) Entire document, especially Abstract, para[0012], [0061]-[0065], [0090], [0115] and FIGS. 1-2.	1-2, 4-6 ----- 3
Y	US 2017/0049298 A1 (MASSACHUSETTS INSTITUTE OF TECHNOLOGY) 23 February 2017 (23.02.2017) Entire document, especially Abstract, para[0005], [0030]-[0032] and FIG. 1A.	1-2, 4-6 ----- 3
A	US 9,364,289 B2 (WISCONSIN ALUMNI RESEARCH FOUNDATION) 14 June 2016 (14.06.2016)	1-6
A	US 2014/0330432 A1 (VANDERBILT UNIVERSITY) 06 November 2014 (06.11.2014) Entire document.	1-6
A	US 2015/0045812 A1 (SAMSUNG ELECTRONICS CO., LTD.) 12 February 2015 (12.02.2015) Entire document.	1-6
A	US 2011/0288536 A1 (DEJIMA) 24 November 2011 (24.11.2011) Entire document.	1-6
A	US 2015/0250546 A1 (INTUITIVE SURGICAL OPERATIONS, INC.) 10 September 2015 (10.09.2015)	1-6

☐ Further documents are listed in the continuation of Box C.

☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

10 August 2018

Date of mailing of the international search report

04 SEP 2018

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774