

(43) International Publication Date  
27 August 2015 (27.08.2015)(51) International Patent Classification:  
*A61M 25/00* (2006.01)    *A61M 39/20* (2006.01)  
*A61M 39/16* (2006.01)

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(21) International Application Number:  
PCT/US2015/015482(22) International Filing Date:  
11 February 2015 (11.02.2015)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
14/185,827 20 February 2014 (20.02.2014) US(71) Applicant: **BECTON, DICKINSON AND COMPANY** [US/US]; 1 Becton Drive, Mail Code 110, Franklin Lakes, New Jersey 07417-1880 (US).(72) Inventors: **MA, Yiping**; 2220 North 2300 East, Layton, Utah 84040 (US). **SHEVGOOR, Siddarth**; 9450 South State Street, Sandy, Utah 84070 (US).(74) Agents: **HIGHET, David W.** et al.; Becton, Dickinson And Company, 1 Becton Drive, Mail Code 110, Franklin Lakes, New Jersey 07417-1880 (US).


(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

— as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

*[Continued on next page]*

(54) Title: IV ACCESS PORT CAP FOR PROVIDING ANTIMICROBIAL PROTECTION

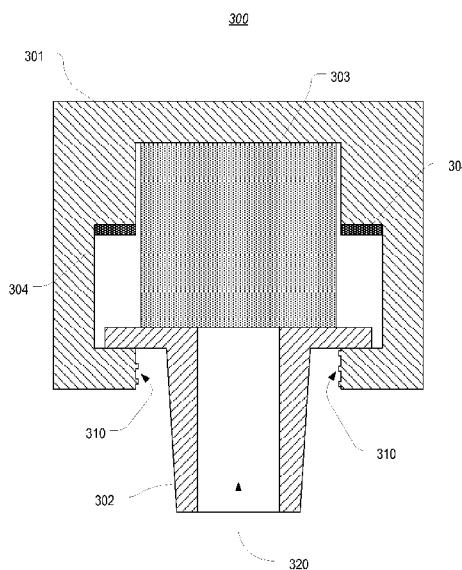**FIG. 4**

(57) Abstract: A cap (300) is configured to provide antimicrobial protection to a female luer port of an intravenous device. The cap distributes an antimicrobial solution within the intraluminal surfaces of the port when the cap is connected to the port. A cap is also designed to distribute an antimicrobial solution around the exterior surfaces of the port. Once connected to a port, the cap can form a seal that minimizes the evaporation of the antimicrobial solution from within the lumen of a port. The cap can therefore provide antimicrobial protection against another device that is connected to the port once the cap is removed.



---

**Published:**

— *with international search report (Art. 21(3))*

## IV ACCESS PORT CAP FOR PROVIDING ANTIMICROBIAL PROTECTION

### CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] Not Applicable.

### BACKGROUND OF THE INVENTION

[0002] The present invention relates generally to caps for providing antimicrobial protection to an IV access port or other type of device having a female luer connection. In particular, the caps of the present invention can be used to distribute an antimicrobial solution within the intraluminal space of a female luer device.

[0003] Currently, there are various products available for capping a port of an intravenous device (e.g. a catheter or other infusion device). In this specification, port will be used generally to describe any type of connector for interconnecting two devices. For example, Figure 1 generally illustrates a port 100 that is configured as a female luer lock connector, while Figure 2 generally illustrates a port 200 that is configured as a needleless female luer connector. Typically, a needleless connector employs a valve that seals the lumen of the device from the exterior environment and which is pierced or otherwise separated by a male connector to obtain access to the lumen.

[0004] In this specification, a female luer connector should be interpreted as any connector having an internal lumen that is tapered to conform to a corresponding male connector having the same or similar degree of tapering. These female luer connectors can include luer lock and luer slip (or non-lock luer) connectors.

[0005] Intravenous devices can employ ports to provide quick access to a patient's vasculature. These ports also enable the device to remain within the patient's vasculature even when no access to the vasculature is needed. When a port of an intravenous device is not in use, it is desirable to maintain the port clean and free from bacteria and other microbes. If the port becomes contaminated with microbes while not in use, it is possible that the microbes will be flushed into the patient's vasculature once the port is again used for accessing the patient's vasculature. Accordingly, maintaining a sterile port is essential to minimize the risk of infection.

[0006] To maintain the sterility of a port, various types of caps have been designed. These caps typically contain an antimicrobial solution that is applied to the exterior surfaces of the port when a cap is attached to the port. For example, some caps employ an alcohol-soaked material that is disposed within the cavity of the cap so that the material scrubs the

exterior surfaces of the port when the cap is screwed on. Once screwed on, these caps can retain an amount of the antimicrobial solution around the exterior surface of the port to ensure that the exterior surface remains sterile until the cap is removed.

**[0007]** These caps have proven to be effective for disinfecting the exterior surfaces of the port. However, current designs only disinfect the exterior surfaces. Any microbes that may exist within the intraluminal space will likely remain even after these current caps are used.

**[0008]** Alternatively, to address this risk of infection, some ports are configured to have antimicrobial coatings on the intraluminal surfaces. With such coatings, the intraluminal surfaces can remain sterile even if microbes come in contact with the surfaces. These coatings can also dissolve into the fluid within the lumen to effectively spread antimicrobial agents throughout the lumen. However, there are various drawbacks to using antimicrobial coatings on the intraluminal surfaces of ports. For example, ports that employ antimicrobial coatings are significantly more expensive to produce. As a result many facilities choose not to use them. Also, for a coating to be effective, it must retain its antimicrobial properties for at least the amount of time that the port could possibly be used (e.g. up to 7 days). To accomplish this, relatively thick coatings or highly concentrated coatings are used. This causes the concentration of antimicrobial agents to be very high during the initial usage time which poses a toxicity risk.

#### **BRIEF SUMMARY OF THE INVENTION**

**[0009]** The present invention extends to caps for providing antimicrobial protection to a female luer port of an intravenous device. The caps of the present invention are designed to distribute an antimicrobial solution within the intraluminal surfaces of the port. Additionally, in some embodiments, the caps are designed to also distribute an antimicrobial solution around the exterior surfaces of the port. Accordingly, the caps of the present invention provide a complete solution for disinfecting a port of an intravenous device.

**[0010]** In one embodiment, the present invention is implemented as a cap for a port of an intravenous device. The cap can comprise a body having a cavity; an actuator positioned within the cavity; and an absorbent material containing an antimicrobial solution. The absorbent material is contained within the cavity between the actuator and an inner surface of the body. When the cap is connected to a port of an intravenous device, the actuator is forced into the cavity and compresses the absorbent material causing the antimicrobial solution to flow onto an intraluminal surface of the port.

**[0011]** In some embodiments, the actuator comprises a lumen through which the antimicrobial solution flows to reach a lumen of the port.

**[0012]** In some embodiments, the actuator comprises a male luer in which the lumen is formed.

**[0013]** In some embodiments, the antimicrobial solution flows through a gap between the body and an exterior surface of the actuator and onto an exterior surface of the port.

**[0014]** In some embodiments, the body includes a seal that the actuator contacts when the cap is connected to the port thereby forming a seal between the actuator and the body.

**[0015]** In some embodiments, the concentration of an antimicrobial agent within the antimicrobial solution is selected such that when the antimicrobial solution mixes with fluid contained within the lumen of the port, the concentration of the antimicrobial agent remains higher than the minimum inhibitory concentration of the antimicrobial agent.

**[0016]** In some embodiments, the port is a female luer into which the actuator inserts.

**[0017]** In some embodiments, the port is a needless connector into which the actuator inserts.

**[0018]** In some embodiments, the actuator includes a protrusion that is positioned within a lumen in the body, the protrusion having a lumen through which the antimicrobial solution flows.

**[0019]** In some embodiments, the actuator includes a plurality of prongs that extend through corresponding openings in the body.

**[0020]** In some embodiments, the antimicrobial solution flows through the openings when the actuator is forced into the cavity.

**[0021]** In some embodiments, the actuator includes a lumen that has an antimicrobial coating.

**[0022]** In another embodiment, the present invention is implemented as a cap for a port of an intravenous device. The cap can comprise a body having a cavity; an actuator positioned within the cavity, the actuator having a lumen; and an absorbent material containing an antimicrobial solution, the absorbent material being contained within the cavity between the actuator and an inner surface of the body. Prior to the cap being connected to a port of an intravenous device, the absorbent material remains uncompressed. Then, when the cap is connected to a port of an intravenous device, the actuator compresses the absorbent material causing the antimicrobial solution to flow through the lumen of the actuator and into a lumen of the port.

**[0023]** In some embodiments, the actuator is sized such that a gap exists between an outer edge of the actuator and a wall of the cavity, the antimicrobial solution also flowing through the gap onto an exterior surface of the port.

**[0024]** In some embodiments, the actuator includes a plurality of prongs which extend through corresponding openings in the body. The antimicrobial solution flows through the openings onto the exterior surface of the port

**[0025]** In some embodiments, the body includes a seal for sealing the lumen of the actuator.

**[0026]** In some embodiments, the actuator comprises a male luer.

**[0027]** In another embodiment, the present invention is implemented as a cap for a needleless connector of an intravenous device. The cap can comprise a body having a cavity; an absorbent material positioned within the cavity, the absorbent material containing an antimicrobial solution; and an actuator positioned within the cavity against the absorbent material. The actuator is moveable within the cavity to compress the absorbent material such that upon the cap being connected to a needleless connector, the needleless connector causes the actuator to compress the absorbent material releasing the antimicrobial solution onto an intraluminal surface of the needleless connector.

**[0028]** In some embodiments, the actuator comprises a lumen. The antimicrobial solution flows through the lumen of the actuator onto the intraluminal surface of the needleless connector.

**[0029]** In some embodiments, the antimicrobial solution also flows around an exterior surface of the actuator onto an exterior surface of the needleless connector.

**[0030]** This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to identify key features or essential features of the claimed subject matter.

**[0031]** Additional features and advantages of the invention will be set forth in the description which follows, and in part will be obvious from the description, or may be learned by the practice of the invention. The features and advantages of the invention may be realized and obtained by means of the instruments and combinations particularly pointed out in the appended claims. These and other features of the present invention will become more fully apparent from the following description and appended claims, or may be learned by the practice of the invention as set forth hereinafter.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

**[0032]** In order to describe the manner in which the above-recited and other advantages and features of the invention can be obtained, a more particular description of the invention briefly described above will be rendered by reference to specific embodiments thereof which are illustrated in the appended drawings. Understanding that these drawings depict only

typical embodiments of the invention and are not therefore to be considered to be limiting of its scope, the invention will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

**[0033]** Figure 1 illustrates a perspective view of an example of a prior art port that is configured as a female luer lock connector.

**[0034]** Figure 2 illustrates a perspective view of an example of a prior art port that is configured as a needleless female luer connector.

**[0035]** Figure 3 illustrates a perspective view of a cap in accordance with one or more embodiments of the invention that may be used to apply an antimicrobial solution to the intraluminal surfaces of a port.

**[0036]** Figure 4 illustrates a cross-sectional view of a cap in accordance with one or more embodiments of the invention in which an actuator is movable within the body of the cap to cause an antimicrobial solution to be squeezed from an absorbent material contained within the body and distributed through the actuator into the intraluminal space of a port.

**[0037]** Figure 5 illustrates a cross-sectional view of a cap having a body that is comprised of two pieces in accordance with one or more embodiments of the invention.

**[0038]** Figure 6 illustrates a cross-sectional view of a cap that is configured to be connected to a port that is configured as a luer slip connector in accordance with one or more embodiments of the invention.

**[0039]** Figures 7A-7C illustrate a sequence of how the cap depicted in Figure 4 is connected to a port of an intravenous device. Figure 7A illustrates the cap prior to contacting the port. Figure 7B illustrates that, as the cap is being forced onto the port, the actuator is forced into the absorbent material causing antimicrobial solution to flow towards the port through the gaps formed by the movement of the actuator and through the lumen of the actuator. Figure 7C illustrates that, once the cap is fully connected to the port, the actuator is forced against a seal to seal the lumen of the port.

**[0040]** Figure 8 illustrates a cross-sectional view of the cap depicted in Figure 4 when connected to a port that does not include a ridge against which the actuator presses.

**[0041]** Figures 9A and 9B illustrate a sequence of how the cap depicted in Figure 4 can be used on a port that employs a septum.

**[0042]** Figure 10A illustrates a cross-sectional view of an alternate embodiment of a cap which employs prongs to facilitate the flow of antimicrobial solution to the exterior surfaces of the port.

**[0043]** Figure 10B illustrates an exploded view of the cap of Figure 10A.

**[0044]** Figures 11A-11C illustrate a sequence of how the cap depicted in Figure 10A is connected to a port of an intravenous device. Figure 11A illustrates the cap upon contacting the port. Figure 11B illustrates that, as the cap is being forced onto the port, the actuator is forced into the absorbent material causing antimicrobial solution to flow towards the port through the gaps formed by the movement of the actuator and through the lumen of the actuator. Figure 11C illustrates that, once the cap is fully connected to the port, the actuator is forced against a seal to cause further flow of the antimicrobial solution to be only through the lumen of the actuator.

#### **DETAILED DESCRIPTION OF THE INVENTION**

**[0045]** The present invention extends to caps for providing antimicrobial protection to a female luer port of an intravenous device. The caps of the present invention are designed to distribute an antimicrobial solution within the intraluminal surfaces of the port. Additionally, in some embodiments, the caps are designed to also distribute an antimicrobial solution around the exterior surfaces of the port. Accordingly, the caps of the present invention provide a complete solution for disinfecting a port of an intravenous device.

**[0046]** In one embodiment, the present invention is implemented as a cap for a port of an intravenous device. The cap can comprise a body having a cavity; an actuator positioned within the cavity; and an absorbent material containing an antimicrobial solution. The absorbent material is contained within the cavity between the actuator and an inner surface of the body. When the cap is connected to a port of an intravenous device, the actuator is forced into the cavity and compresses the absorbent material causing the antimicrobial solution to flow onto an intraluminal surface of the port.

**[0047]** In some embodiments, the actuator comprises a lumen through which the antimicrobial solution flows to reach a lumen of the port.

**[0048]** In some embodiments, the actuator comprises a male luer in which the lumen is formed.

**[0049]** In some embodiments, the antimicrobial solution flows through a gap between the body and an exterior surface of the actuator and onto an exterior surface of the port.

**[0050]** In some embodiments, the body includes a seal that the actuator contacts when the cap is connected to the port thereby forming a seal between the actuator and the body.

**[0051]** In some embodiments, the concentration of an antimicrobial agent within the antimicrobial solution is selected such that when the antimicrobial solution mixes with fluid contained within the lumen of the port, the concentration of the antimicrobial agent remains higher than the minimum inhibitory concentration of the antimicrobial agent.

**[0052]** In some embodiments, the port is a female luer into which the actuator inserts.

**[0053]** In some embodiments, the port is a needleless connector into which the actuator inserts.

**[0054]** In some embodiments, the actuator includes a protrusion that is positioned within a lumen in the body, the protrusion having a lumen through which the antimicrobial solution flows.

**[0055]** In some embodiments, the actuator includes a plurality of prongs that extend through corresponding openings in the body.

**[0056]** In some embodiments, the antimicrobial solution flows through the openings when the actuator is forced into the cavity.

**[0057]** In some embodiments, the actuator includes a lumen that has an antimicrobial coating.

**[0058]** In another embodiment, the present invention is implemented as a cap for a port of an intravenous device. The cap can comprise a body having a cavity; an actuator positioned within the cavity, the actuator having a lumen; and an absorbent material containing an antimicrobial solution, the absorbent material being contained within the cavity between the actuator and an inner surface of the body. Prior to the cap being connected to a port of an intravenous device, the absorbent material remains uncompressed. Then, when the cap is connected to a port of an intravenous device, the actuator compresses the absorbent material causing the antimicrobial solution to flow through the lumen of the actuator and into a lumen of the port.

**[0059]** In some embodiments, the actuator is sized such that a gap exists between an outer edge of the actuator and a wall of the cavity, the antimicrobial solution also flowing through the gap onto an exterior surface of the port.

**[0060]** In some embodiments, the actuator includes a plurality of prongs which extend through corresponding openings in the body. The antimicrobial solution flows through the openings onto the exterior surface of the port

**[0061]** In some embodiments, the body includes a seal for sealing the lumen of the actuator.

**[0062]** In some embodiments, the actuator comprises a male luer.

**[0063]** In another embodiment, the present invention is implemented as a cap for a needleless connector of an intravenous device. The cap can comprise a body having a cavity; an absorbent material positioned within the cavity, the absorbent material containing an antimicrobial solution; and an actuator positioned within the cavity against the absorbent

material. The actuator is moveable within the cavity to compress the absorbent material such that upon the cap being connected to a needleless connector, the needleless connector causes the actuator to compress the absorbent material releasing the antimicrobial solution onto an intraluminal surface of the needleless connector.

**[0064]** In some embodiments, the actuator comprises a lumen. The antimicrobial solution flows through the lumen of the actuator onto the intraluminal surface of the needleless connector.

**[0065]** In some embodiments, the antimicrobial solution also flows around an exterior surface of the actuator onto an exterior surface of the needleless connector.

**[0066]** Figure 3 illustrates a perspective view of a cap 300 in accordance with one or more embodiments of the invention. As shown, cap 300 comprises a body 301 and an actuator 302. Body 301 is generally shaped to allow cap 300 to be connected to a female luer connector such as port 100. If the cap is designed to connect to a female luer lock connector, the inside surface of the body can include threads (e.g. as shown in Figure 4). In contrast, if the cap is designed to connect to a female luer slip connector, the inside surface of the body may or may not include threads. In either case, actuator 302 can be configured as a male luer connector to allow actuator 302 to be inserted into the female luer port 100.

**[0067]** Figure 4 illustrates a cross-section view of cap 300. As shown, cap 300 includes body 301, actuator 302, and absorbent material 303 positioned between body 301 and actuator 302. Cap 300 includes threads 310 and is therefore an example of a cap designed for a female luer lock connector. Actuator 302 has a tip that is designed as a male luer connector to allow the tip to be inserted into the lumen of a female luer connector.

**[0068]** Figure 4 depicts cap 300 prior to being connected to a port. Before connection, actuator 302 is positioned against the interior surface of body 301 and does not compress absorbent material 303. In some embodiments, actuator 302 can be held in this position by an adhesive, welding, or other physical force between body 301 and actuator 302. In other embodiments, actuator 302 can be held in this position by absorbent material 303. In other words, absorbent material 303 may be sufficiently rigid to retain the position of actuator 302 until a substantial force is applied against actuator 302. In any case, actuator 302 is designed to not compress absorbent material 303 until cap 300 is connected to a port. A seal (not shown) can be applied overtop of actuator 302 and possibly the opening of body 301 to seal absorbent material 303 from the exterior environment until cap 300 is to be used.

**[0069]** Figure 5 illustrates a cross-sectional view of an alternate embodiment of cap 300. In this alternate embodiment, body 301 comprises two pieces, a top piece 301a and a bottom

piece 301b. This two piece design can be used to facilitate manufacturing (e.g. to facilitate positioning actuator 302 within body 301). Whether the design of Figure 4 or of Figure 5 is employed, cap 300 will function the same as will be described below.

**[0070]** Figure 6 illustrates a cross-sectional view of another alternate embodiment of cap 300. In this embodiment, body 301 does not include threads but is configured to form a friction fit with the exterior surface of a port. Accordingly, a cap in accordance with this alternate embodiment could be used on a non-lock female luer connector. Regardless of the type of port to which cap 300 will be connected, it is desirable to secure body 301 to the port (e.g. via threads or a friction fit) to allow a seal to be formed between actuator 302 and body 301 once the cap is connected. The role of this seal will be further described below with reference to Figure 7C.

**[0071]** With continued reference to Figures 4-6, absorbent material 303 is saturated with an antimicrobial solution which remains within absorbent material 303 until absorbent material 303 is compressed. Actuator 302 is designed to provide a fluid pathway to distribute the antimicrobial solution to a port when cap 300 is connected to the port. The primary fluid pathway is through lumen 320. However, a secondary fluid pathway is also provided around the exterior of actuator 302. The distribution of the antimicrobial solution is illustrated in Figures 7A-7C.

**[0072]** Figures 7A-7C illustrate a sequence that occurs when cap 300 is connected to a port. Although Figures 7A-7C illustrate the design of cap 300 as shown in Figure 4, the same sequence would occur when a cap designed as shown in Figures 5 or 6 is connected. Also, for simplicity of illustration, cap 300 is shown as being connected to port 100. However, the same sequence would occur when cap 300 is connected to any port that is configured as a female luer connector. Examples of ports on which cap 300 can be used include the BD Q-Syte® (manufactured by Becton, Dickinson and Company), the CareFusion MaxPlus® Clear (manufactured by CareFusion Corp), and the LifeShield MicroClave® (manufactured by Hospira, Inc.) among many others.

**[0073]** Figure 7A shows the state of cap 300 prior to contacting port 100. In this state, cap 300 is as shown in Figure 4. Port 100 is shown as including an internal ridge 111 against which the tip of actuator 302 presses when cap 300 is connected to the port. Port 100 is also shown as including threads 110 and is therefore an example of a luer lock connector. Accordingly, cap 300 is connected to port 100 by threading the cap onto the port.

**[0074]** As shown in Figure 7B, as cap 300 is initially inserted into and advanced onto port 100, the tip of actuator 302 contacts ridge 111 of port 100. This contact forces actuator

upward away from body 301 and into absorbent material 303. The compression of absorbent material 303 causes the antimicrobial solution to flow out of the absorbent material. The arrows in Figure 7B indicate the pathways along which the absorbent material will flow.

**[0075]** The primary pathway along which the antimicrobial solution flows is through lumen 320 of actuator 302. Because lumen 320 aligns with lumen 120 of port 100, the antimicrobial solution flowing through lumen 320 will ultimately be distributed along the surfaces of lumen 120 and into any fluid contained within lumen 120. In this way, the intraluminal surfaces of port 100 can be disinfected.

**[0076]** The secondary pathway is around actuator 302 as depicted by the outer arrows in Figure 7B. The antimicrobial solution will flow along the secondary pathway until the top surface of actuator 302 contacts seal 304 formed along the interior surface of body 301 as is shown in Figure 7C. The contact between actuator 302 and seal 304 limits the antimicrobial solution from flowing around actuator 302 and therefore forces further flow through lumen 320. In this way, an adequate amount of antimicrobial solution will flow into the intraluminal space of port 100.

**[0077]** As shown in Figure 7C, after cap 300 has been connected, antimicrobial solution will be contained within lumen 320 and lumen 120 as well as in the spaces between the outer surface of actuator 302, and the inner surface of body 301. This antimicrobial solution outside of actuator 302 can disinfect the top and outer surfaces of port 100. Because the connection between port 100 and cap 300 may not be fluid tight, the antimicrobial solution may be allowed to seep between threads 110 and 310 and onto the exterior surfaces of port 100. Also, in some embodiments where a tight seal is not formed (or at least not formed initially when the antimicrobial solution flows around actuator 302) this antimicrobial solution can flow into the opening of port 100 between the exterior surface of actuator 302 and the interior surface of port 100. In this way, the intraluminal surfaces that may otherwise not be reached by antimicrobial solution that has flowed through lumen 320 may still be disinfected.

**[0078]** Accordingly, the design of cap 300 allows the intraluminal surfaces of a port to be disinfected. Because the lumen of port 100 may typically contain a fluid (e.g. a saline solution or other solution that was infused into the patient), the antimicrobial solution can mix with the fluid to enhance the distribution of the antimicrobial agents throughout lumen 120.

**[0079]** When cap 300 is fully connected to port 100, a seal can be formed between actuator 302 and seal 304 as shown in Figure 7C. The tight fit between the male luer actuator

302 and the female luer port 100 can also form a seal between these two connectors. Accordingly, lumens 120 and 320 can be substantially sealed from the external environment thereby limiting the amount of antimicrobial solution within lumen 120 that evaporates after cap 300 has been connected. The antimicrobial solution can therefore remain active until the cap is removed for attachment of another device. In this way, when another device is connected to the port, the antimicrobial solution that remains within lumen 120 can disinfect the tip of the device. Accordingly, cap 300 not only disinfects port 100 when not in use, but can also disinfect other devices that are connected to the port after cap 300 has been removed.

**[0080]** Figure 8 illustrates a cross-sectional view of an alternate embodiment in which a port 100a does not include a ledge against which the tip of actuator 302 presses. In such cases, the frictional force created when actuator 302 has been inserted into lumen 120 can be sufficient to force actuator 302 upward into absorbent material 303. This frictional force can also be sufficient to form a seal between actuator 302 and port 100.

**[0081]** Figures 9A and 9B illustrate a cross-sectional view of another alternate embodiment in which cap 300 is connected to a port 200 that is configured as a needleless connector that includes a split septum 230. As shown in Figure 9A, as the tip of actuator 302 initially contacts septum 230 and is forced through septum 230, actuator 302 is forced upwardly to initiate the flow of antimicrobial solution. Actuator 302 will pass through septum 230 and ultimately contact a ledge within lumen 220 of port 200 (or if port 200 does not contain a ledge, may contact the tapered sides of the port). As shown in Figure 9B, when fully connected, cap 300 is positioned in a similar manner on port 200 as cap 300 is positioned on port 100. Accordingly, cap 300 can be used to disinfect the intraluminal surfaces of ports of various designs and configurations.

**[0082]** Figure 10A illustrates a cross-sectional view of another embodiment of a cap 1000. Cap 1000, like cap 300, includes a body 1001, an actuator 1002, and absorbent material 1003. However, actuator 1002 and the bottom surface of body 1001 have a different configuration to enhance the flow of absorbent material to the exterior surfaces of a port.

**[0083]** Figure 10B illustrates a cross-sectional exploded view of cap 1000 in which actuator 1002 is shown removed from body 1001. As shown, actuator 1002 includes a central protrusion 1053 that forms lumen 1020. Actuator 1002 also includes prongs 1052 that extend from the bottom surface of actuator 1002. The bottom of body 1001 is configured to accommodate actuator 1002. For example, body 1001 includes a lumen 1050 within which protrusion 1053 is contained and openings 1051 through which prongs 1052 extend. Figures 11A-11C illustrate how this configuration of cap 1000 enhances the flow of antimicrobial

solution to the exterior surfaces of a port while still distributing sufficient antimicrobial solution to the lumen of the port.

**[0084]** Figure 11A illustrates cap 1000 upon actuator 1002 contacted the top surface of port 1100. As shown, the design of actuator 1002 causes prongs 1052 to first contact port 1100. Then, in Figure 11B, the upward force on prongs 1052 causes actuator 1002 to compress absorbent material 1003 resulting in antimicrobial solution flowing through lumen 1020 and around the exterior of actuator 1002 in much the same manner as described with reference to Figures 7B.

**[0085]** However, because of the positioning of openings 1051 near the edges of port 1100, the antimicrobial solution that flows through openings 1051 will more easily flow onto the exterior surfaces of port 1100. Additionally, as with cap 300, the primary pathway of the flow of the antimicrobial solution is through lumen 1020 and into lumen 1120 of port 1100.

**[0086]** Figure 11C illustrates cap 1000 once fully connected to port 1100. As shown, in this position, port 1100 has forced actuator 1002 upward until it contacts seal 1004. At this point, antimicrobial solution will be forced to flow through lumen 1020. However, the antimicrobial solution that flowed around actuator 1002 and is contained within the internal spaces of body 1001 will be allowed to flow out through openings 1051 onto the exterior surfaces of port 1100.

**[0087]** Although Figure 11C shows that a gap exists between protrusion 1053 and the internal surfaces of lumen 1050 when cap 1000 is fully connected, in some embodiments, the dimensions of protrusion 1053 and lumen 1050 can be configured so that protrusion 1053 forms a tight seal within lumen 1050 when actuator 1002 is in the upward position. Forming a seal between protrusion 1053 and lumen 1050 may be desired when a tight seal is not formed between port 1100 and body 1001.

**[0088]** The caps of the present invention also provide the advantage of minimizing the concentrations of antimicrobial solution that must be used to ensure that the port is adequately disinfected. For example, as stated in the Background, one problem that arises when antimicrobial coatings are used is that the coatings may be too concentrated and may therefore pose toxicity problems. In contrast, because the caps of the present invention are intended for one-time use and are deployed when the port is not in use, the concentrations of antimicrobial solution can be minimized. In other words, in contrast to coatings which must remain active from the time they are applied to the port (e.g. when manufactured) until the port will no longer be used, the caps of the present invention will only remain on the port in between uses. Because the fluid volume in the port is static and fixed, the concentration of

the antimicrobial solution will not change when the cap is in place. Therefore a reduced concentration of antimicrobial solution can be employed in the caps of the present invention while still providing adequate antimicrobial protection. In some embodiments, the concentration of the antimicrobial solution (or the concentration once mixed with fluid already present within the lumen of the port) can be just higher than the minimum inhibitory concentration of the antimicrobial agent in the solution.

**[0089]** Many different types of antimicrobial solutions may be used in caps of the present invention. For example, any antimicrobial agent that is soluble in alcohol, saline, or saline/heparin solutions can be employed. The concentration of the antimicrobial agent within the antimicrobial solution can be selected so that the resulting concentration of the agent once the antimicrobial solution is mixed with the fluid in the lumen of the port is above the minimum inhibitory concentration of the antimicrobial agent. Suitable antimicrobial agents include CHA and CHG among others.

**[0090]** In alternate embodiments, the lumen of the actuator can be coated with an antimicrobial coating. In such embodiments, the cap may or may not also include the absorbent material containing the antimicrobial solution. For example, when the cap does not include the absorbent material, the antimicrobial protection can be provided when the fluid within the lumen of the port contacts the antimicrobial coating within the lumen of the actuator. The dry antimicrobial coating can dissolve into the fluid to thereby disinfect the lumen of the port. Providing an antimicrobial coating on the lumen of the actuator as opposed to on the lumen of the port can allow a lower concentration of antimicrobial agent to be used for the reasons described above.

**[0091]** When the cap does include the absorbent material and an antimicrobial coating, the flow of the antimicrobial solution from the absorbent material may be partially or completely directed around the exterior of the actuator to ensure distribution on the exterior surfaces of the port. Some antimicrobial solution may be designed to flow through the lumen in the actuator to assist in distributing the antimicrobial coating throughout the lumen of the port. In this way, an antimicrobial solution can still be directed to both the intraluminal and the exterior surfaces of the port.

**[0092]** The present invention may be embodied in other specific forms without departing from its spirit or essential characteristics. The described embodiments are to be considered in all respects only as illustrative and not restrictive. The scope of the invention is, therefore, indicated by the appended claims rather than by the foregoing description. All changes

which come within the meaning and range of equivalency of the claims are to be embraced within their scope.

## CLAIMS

1. A cap for a port of an intravenous device, the cap comprising:  
a body having a cavity;  
an actuator positioned in contact with the cavity; and  
an absorbent material containing an antimicrobial solution, the absorbent material being contained within the body such that it is compressible;  
wherein when the cap is connected to a port of an intravenous device, the actuator is advanced into the cavity and compresses the absorbent material causing the antimicrobial solution to flow onto an intraluminal surface of the port.
2. The cap of claim 1, wherein the actuator comprises a lumen, the antimicrobial solution flowing through the lumen into a lumen of the port.
3. The cap of claim 2, wherein the actuator comprises a male luer in which the lumen is formed.
4. The cap of claim 1, wherein the antimicrobial solution flows through a gap between the body and an exterior surface of the actuator and onto an exterior surface of the port.
5. The cap of claim 1, wherein the body includes a seal that the actuator contacts when the cap is connected to the port thereby forming a seal between the actuator and the body.
6. The cap of claim 1, wherein the concentration of an antimicrobial agent within the antimicrobial solution is selected such that when the antimicrobial solution mixes with fluid contained within the lumen of the port, the concentration of the antimicrobial agent remains higher than the minimum inhibitory concentration of the antimicrobial agent.
7. The cap of claim 1, wherein the port is a female luer into which the actuator inserts.
8. The cap of claim 1, wherein the port is a needless connector into which the actuator inserts.
9. The cap of claim 1, wherein the actuator includes a protrusion that is positioned within a lumen in the body, the protrusion having a lumen through which the antimicrobial solution flows.
10. The cap of claim 9, wherein the actuator includes a plurality of prongs that extend through corresponding openings in the body.

11. The cap of claim 10, wherein the antimicrobial solution flows through the openings when the actuator is forced into the cavity.

12. The cap of claim 1, wherein the actuator includes a lumen, the lumen having an antimicrobial coating.

13. A cap for a port of an intravenous device, the cap comprising:

a body having a cavity;

an actuator positioned within the cavity, the actuator having a lumen; and

an absorbent material containing an antimicrobial solution, the absorbent material being contained within the cavity between the actuator and an inner surface of the body;

wherein prior to the cap being connected to a port of an intravenous device, the absorbent material remains uncompressed, and when the cap is connected to a port of an intravenous device, the actuator compresses the absorbent material causing the antimicrobial solution to flow through the lumen of the actuator and into a lumen of the port.

14. The cap of claim 13, wherein the actuator is sized such that a gap exists between an outer edge of the actuator and a wall of the cavity, the antimicrobial solution also flowing through the gap onto an exterior surface of the port.

15. The cap of claim 14, wherein the actuator includes a plurality of prongs which extend through corresponding openings in the body, the antimicrobial solution flowing through the openings onto the exterior surface of the port.

16. The cap of claim 13, wherein the body includes a seal for sealing the lumen of the actuator.

17. The cap of claim 13, wherein the actuator comprises a male luer.

18. A cap for a needleless connector of an intravenous device, the cap comprising:

a body having a cavity;

an absorbent material positioned within the cavity, the absorbent material containing an antimicrobial solution; and


an actuator positioned within the cavity against the absorbent material, the actuator being moveable within the cavity to compress the absorbent material such that upon the cap being connected to a needleless connector, the needleless connector causes the actuator to compress the absorbent material releasing the antimicrobial solution onto an intraluminal surface of the needleless connector.

19. The cap of claim 18, wherein the actuator comprises a lumen, the antimicrobial solution flowing through the lumen of the actuator onto the intraluminal surface of the needleless connector.

20. The cap of claim 19, wherein the antimicrobial solution also flows around an exterior surface of the actuator onto an exterior surface of the needleless connector.

1 / 17


100

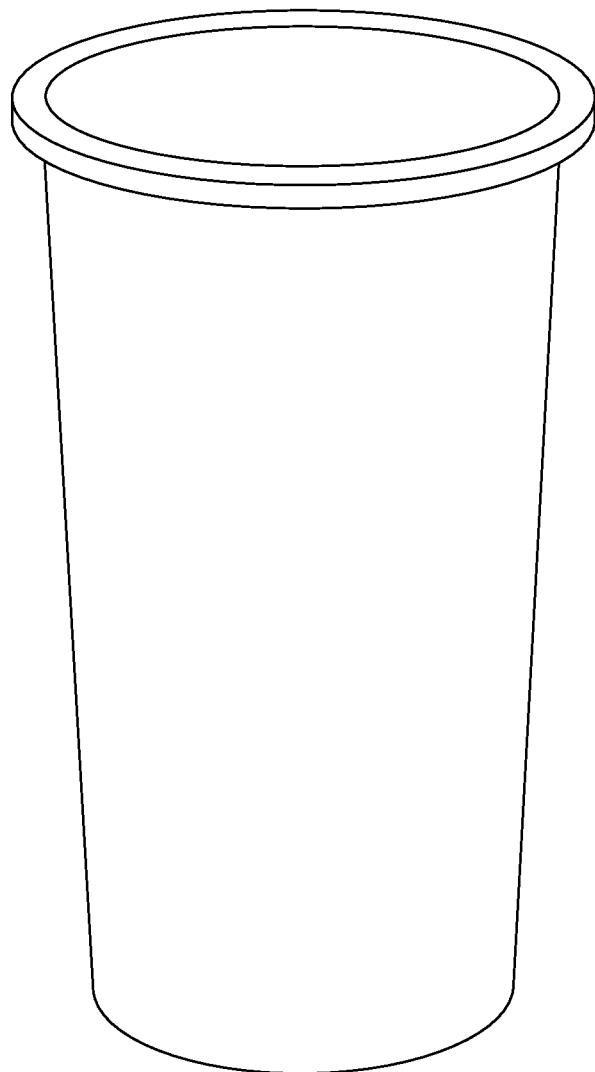

**FIG. 1**  
**(PRIOR ART)**


2 / 17

200

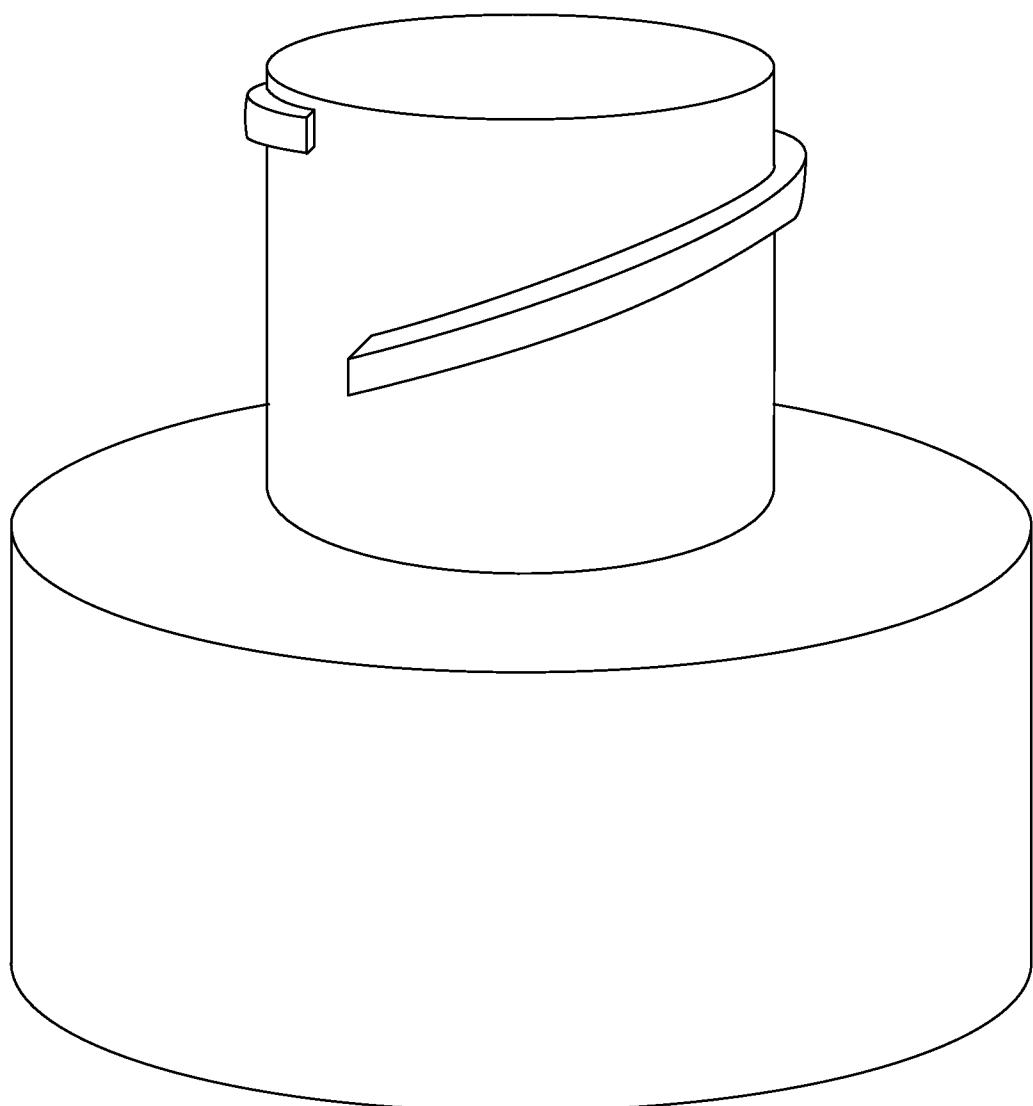


**FIG. 2**  
**(PRIOR ART)**


3 / 17

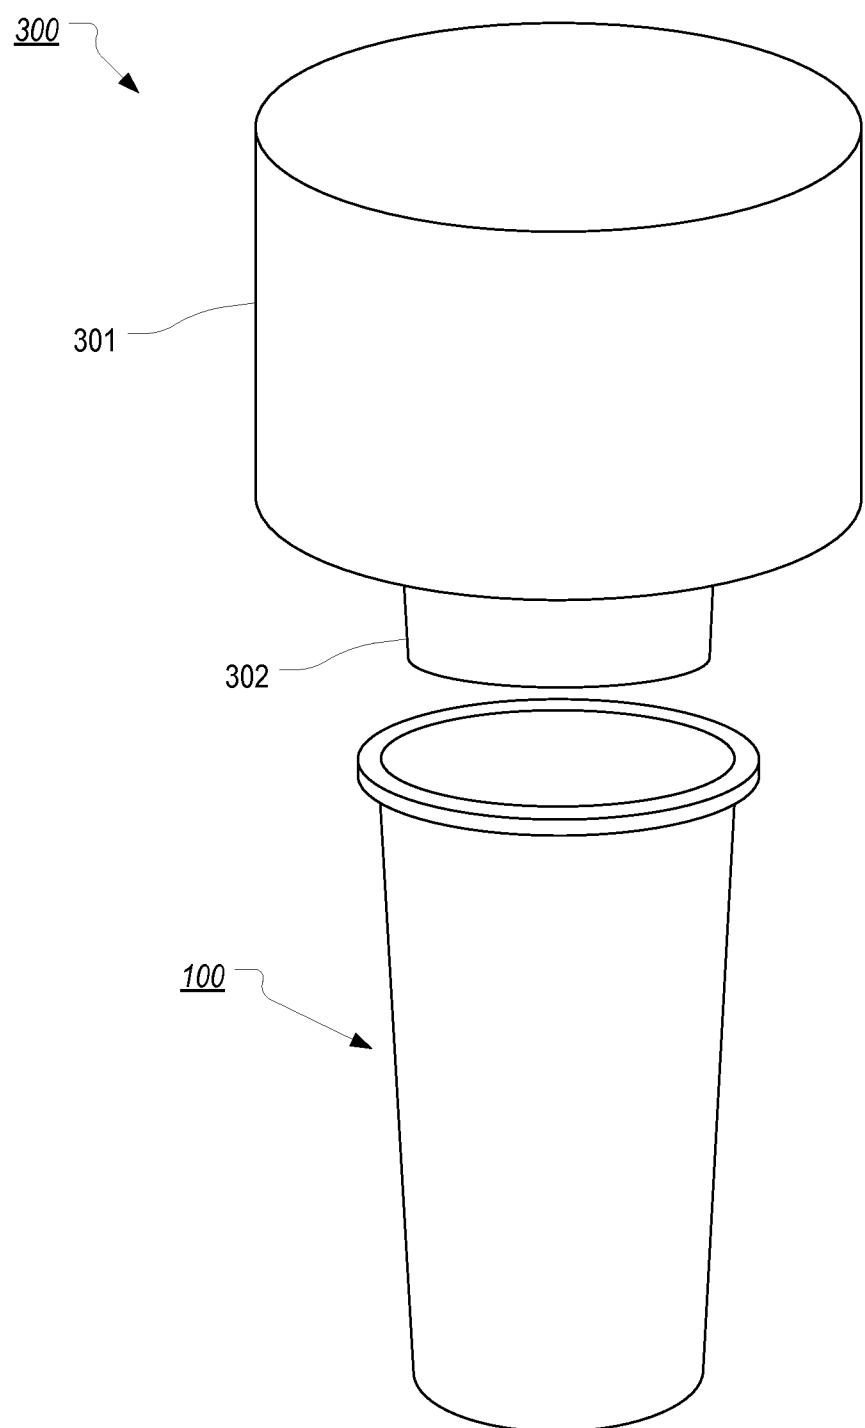***FIG. 3***


4 / 17

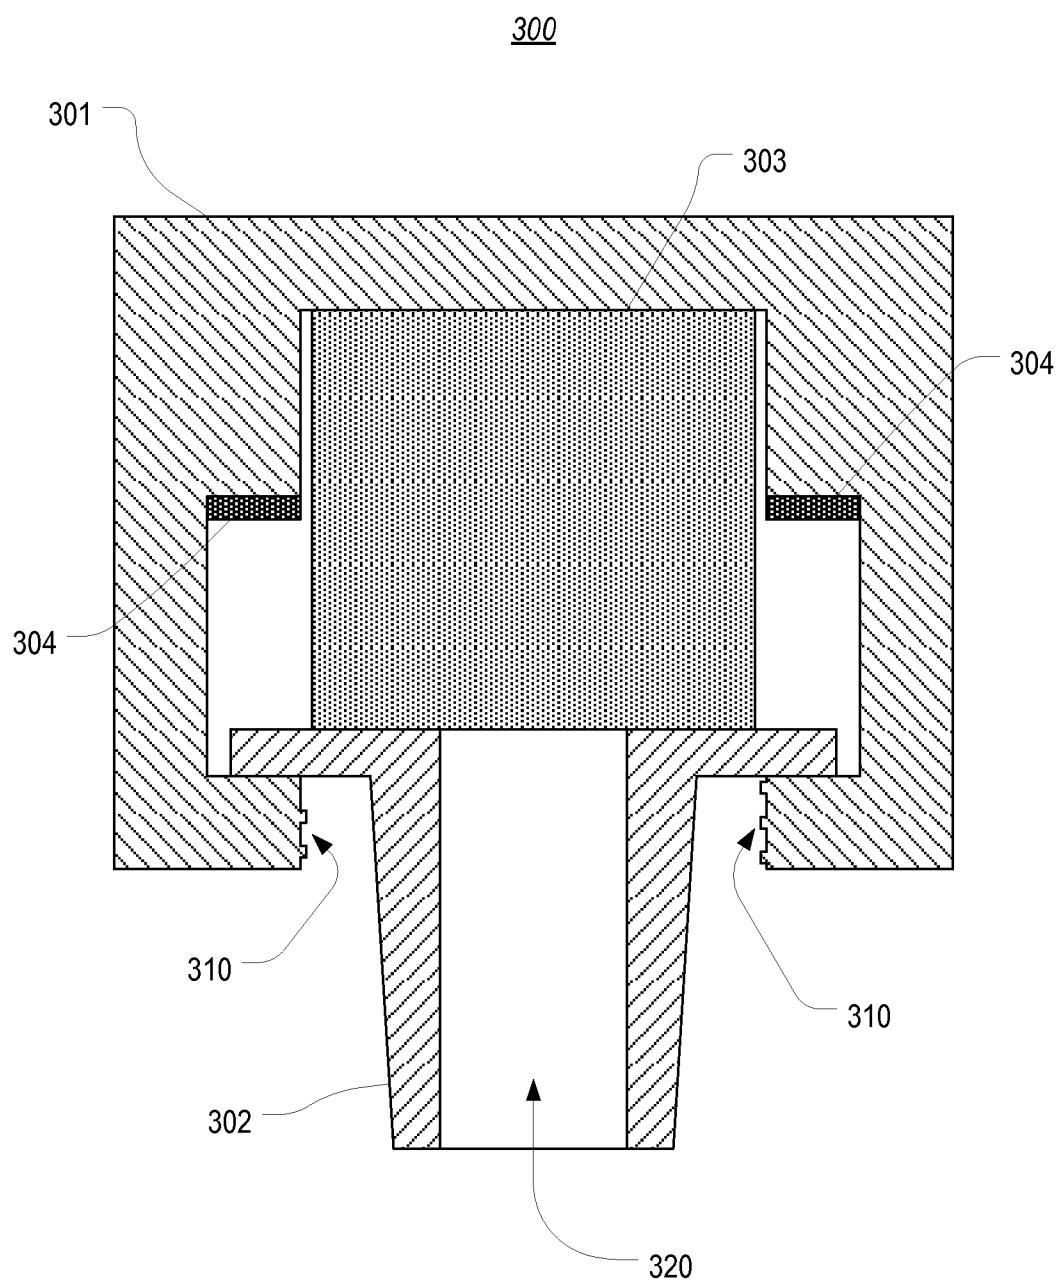**FIG. 4**

5 / 17

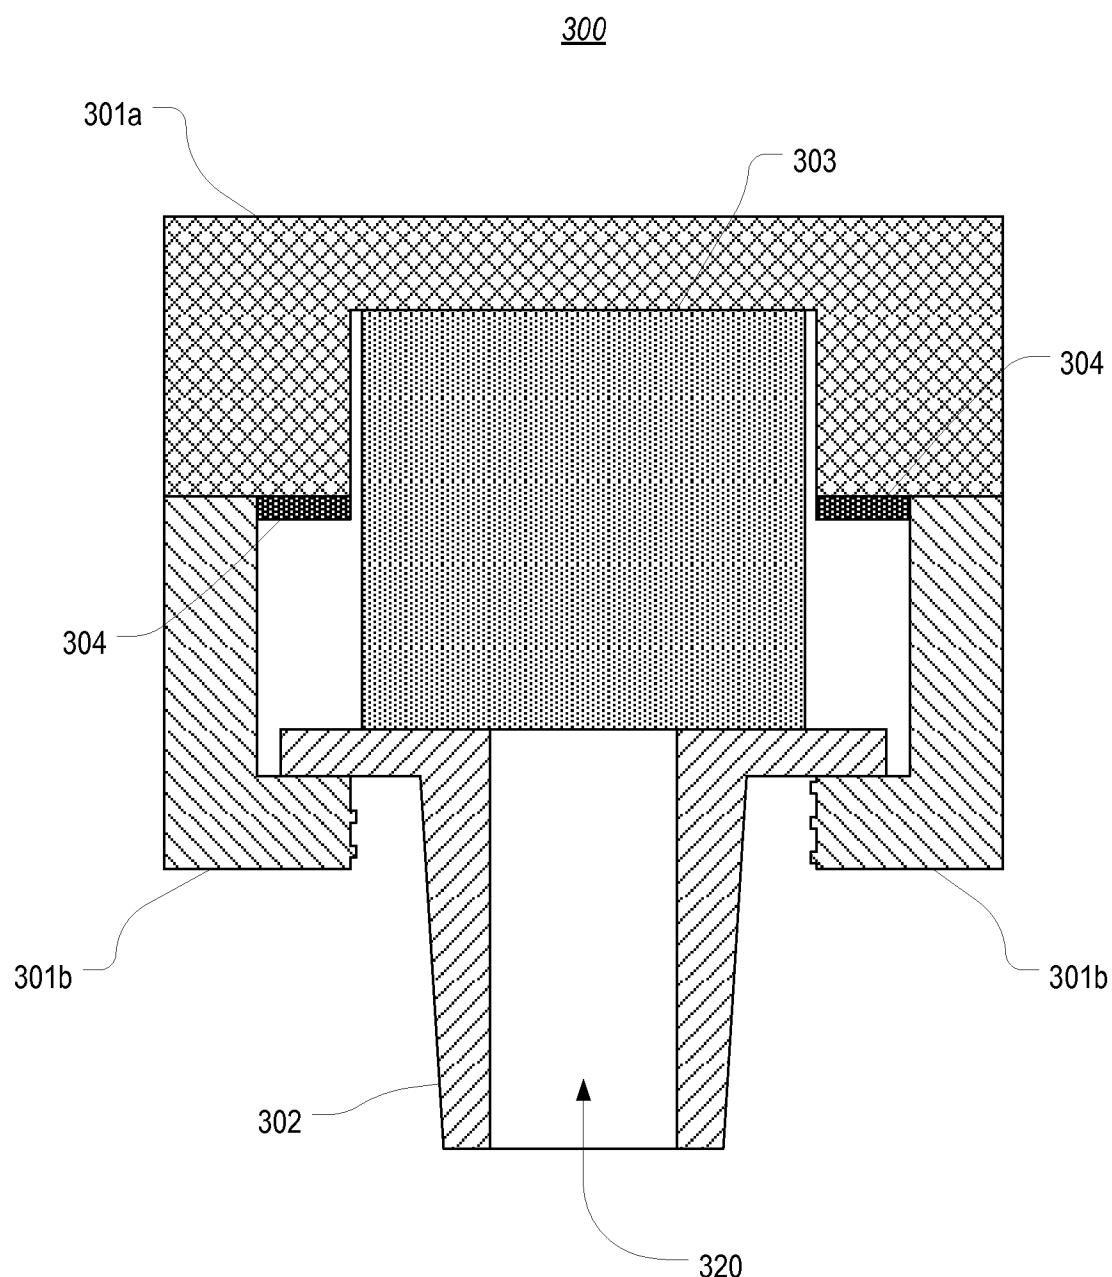**FIG. 5**

6 / 17

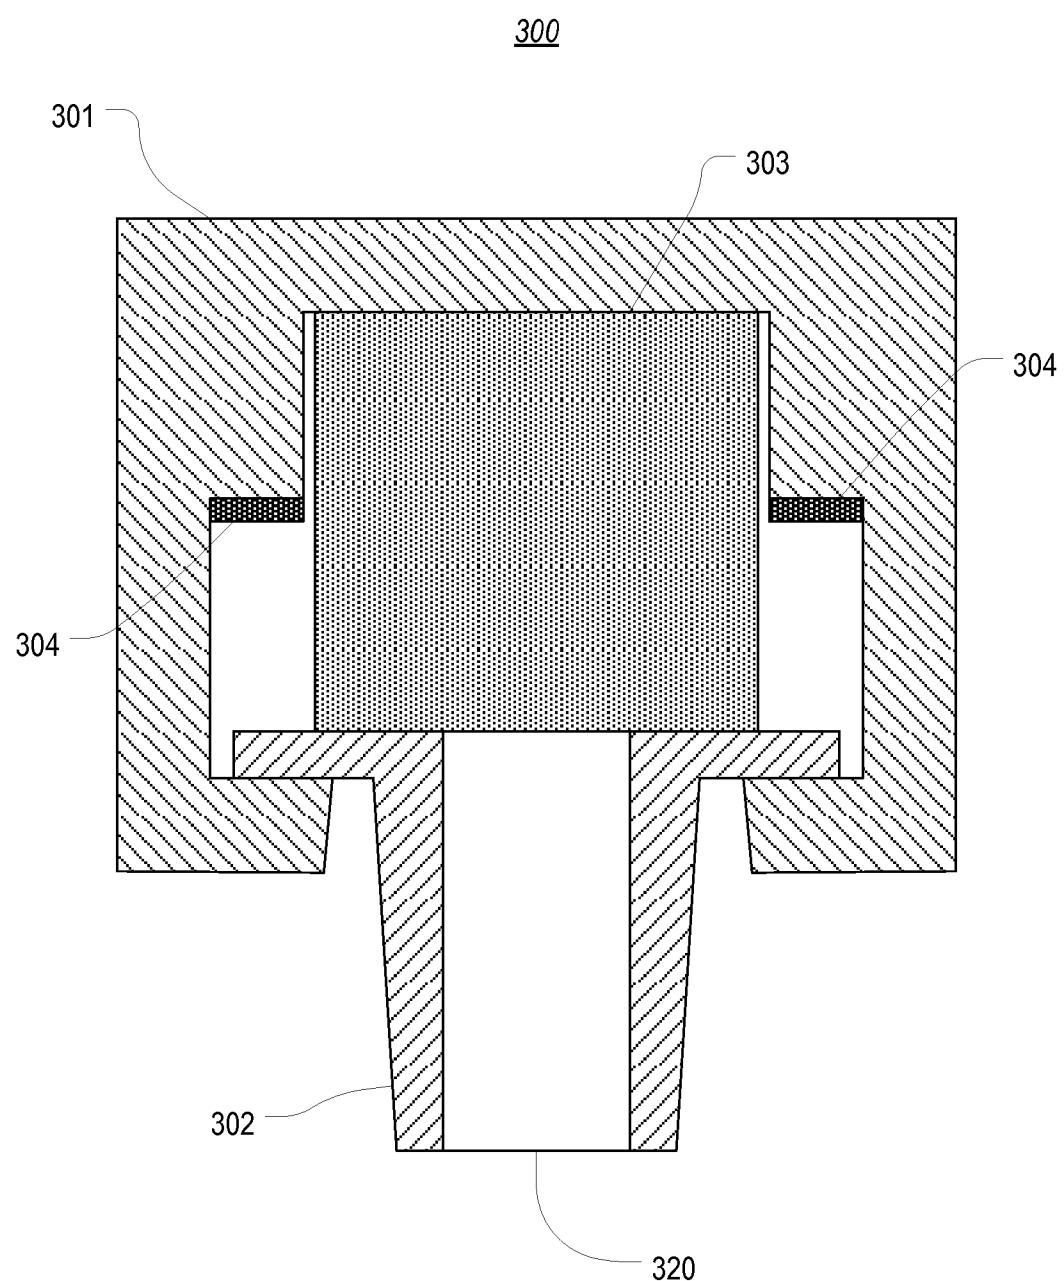**FIG. 6**

7 / 17

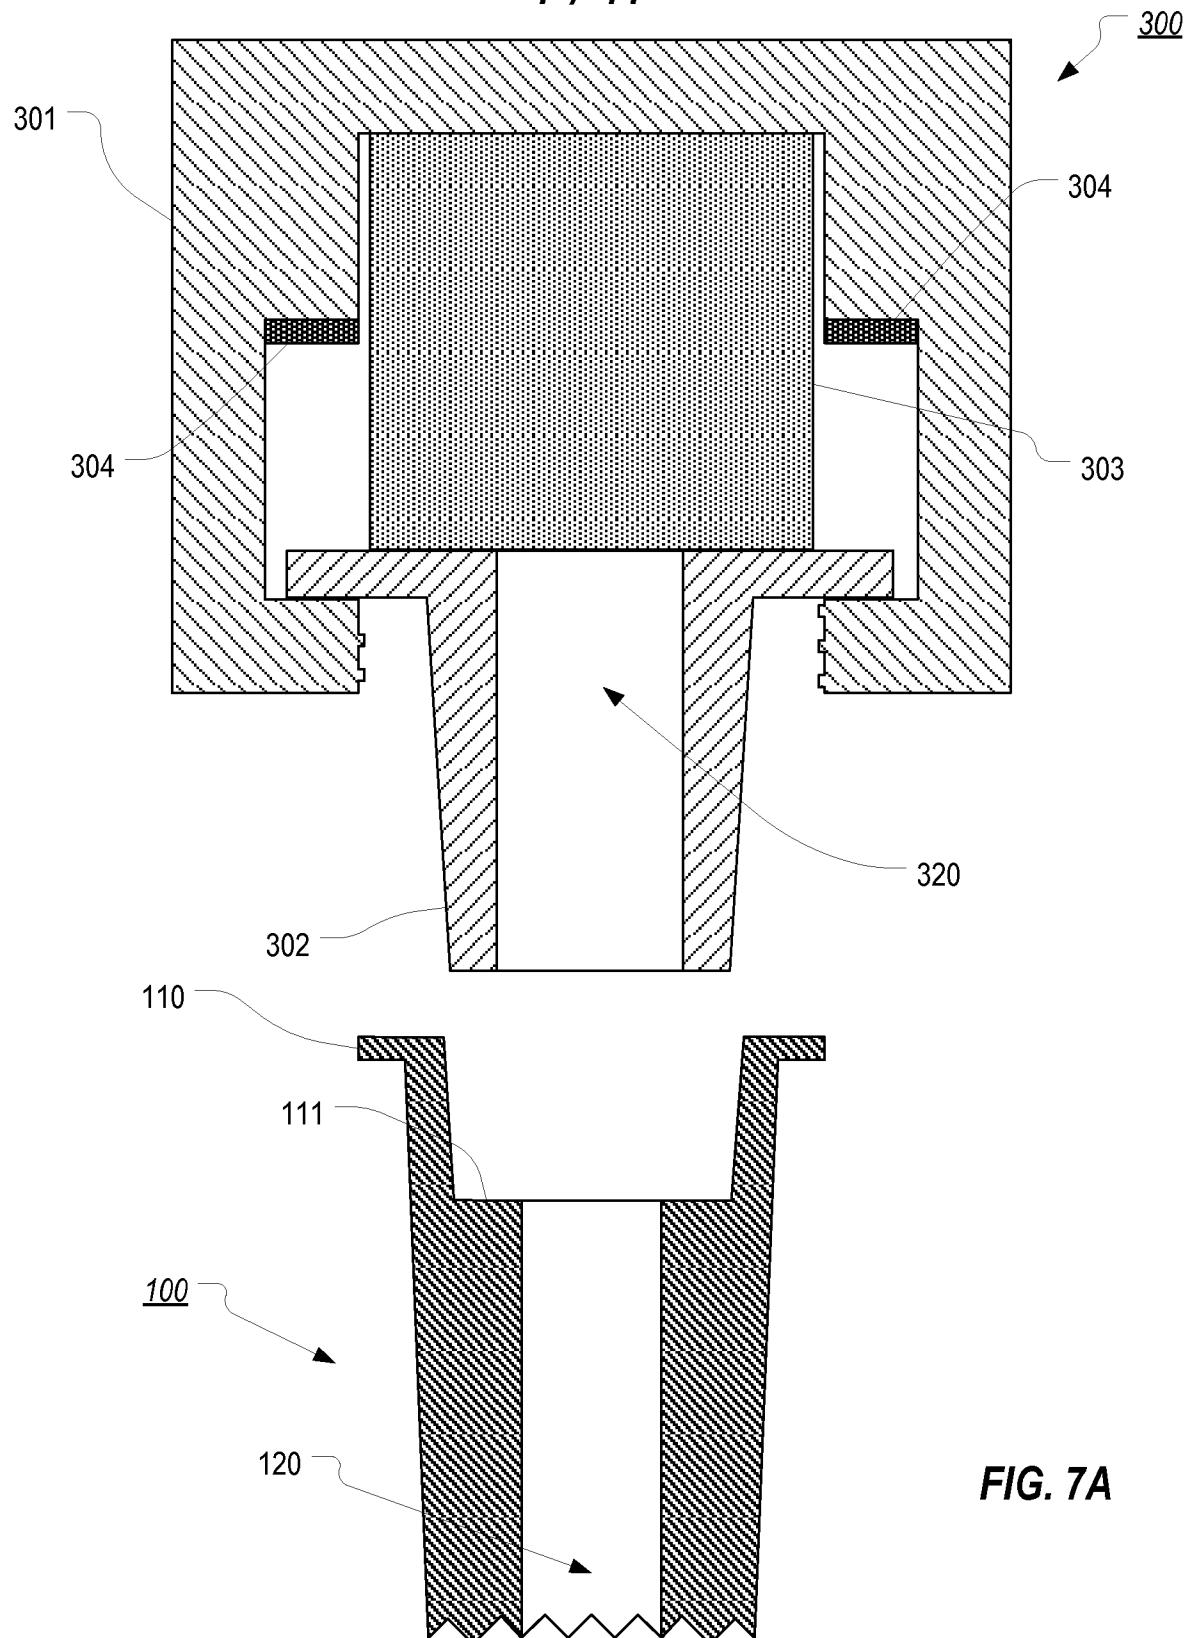


FIG. 7A

8 / 17

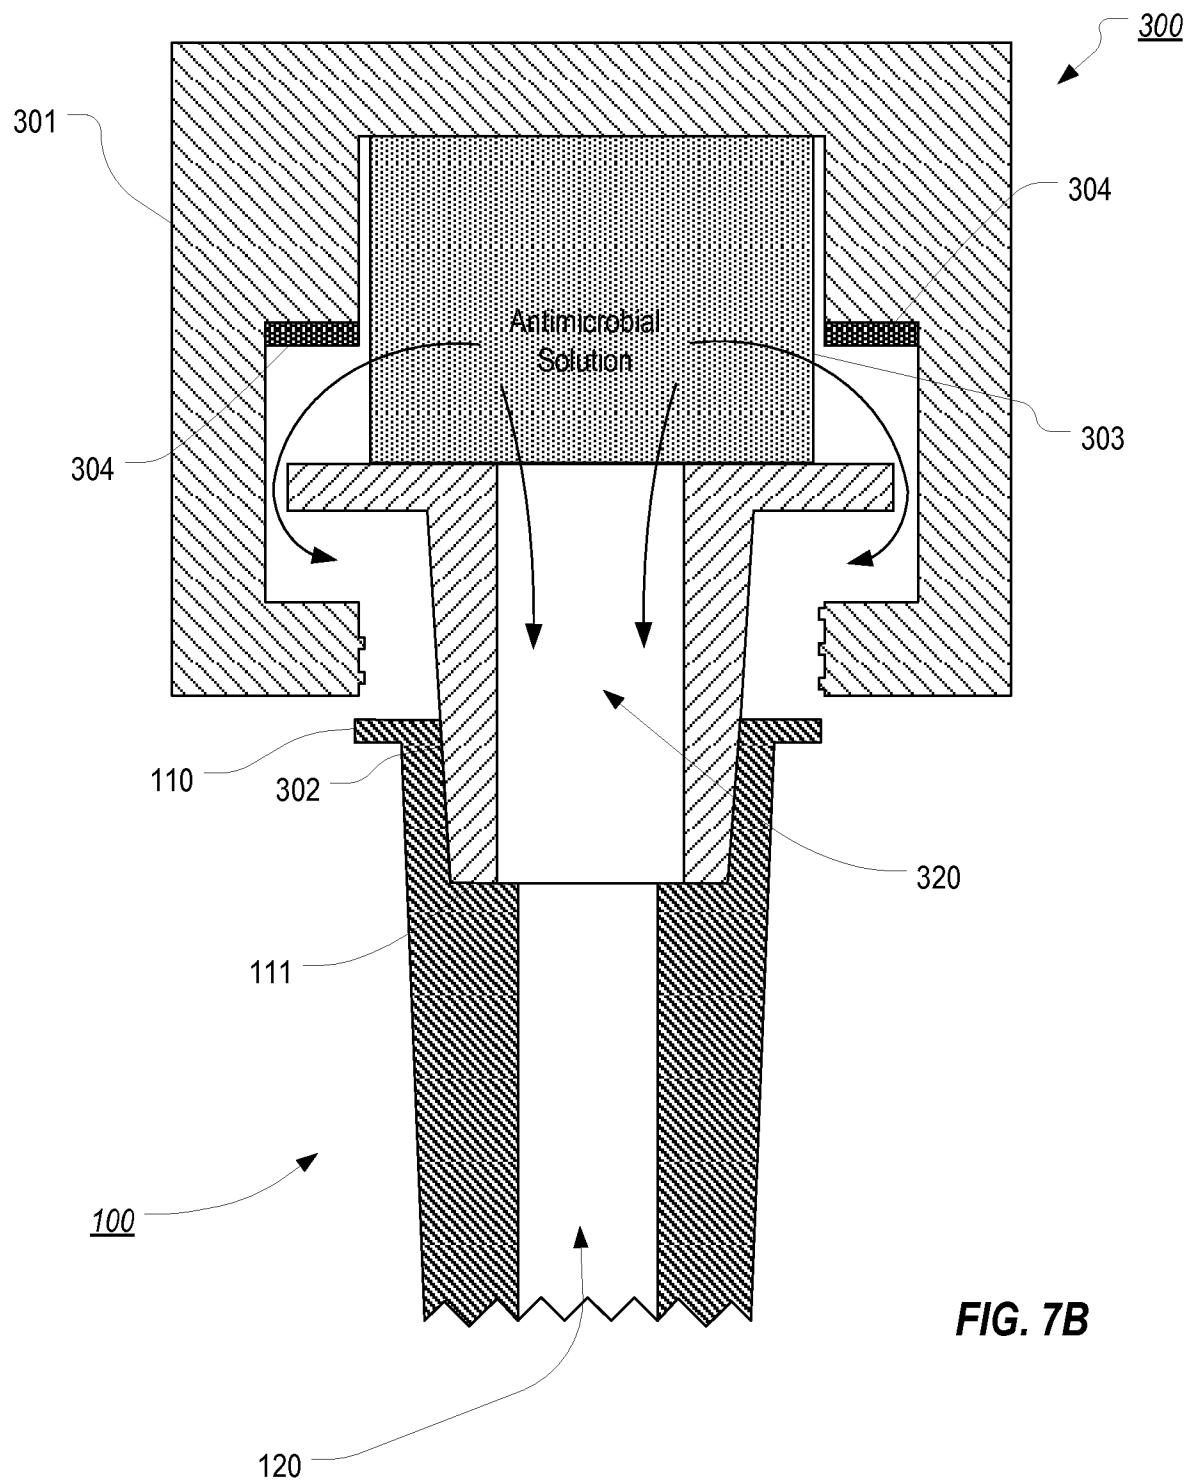


FIG. 7B

9 / 17

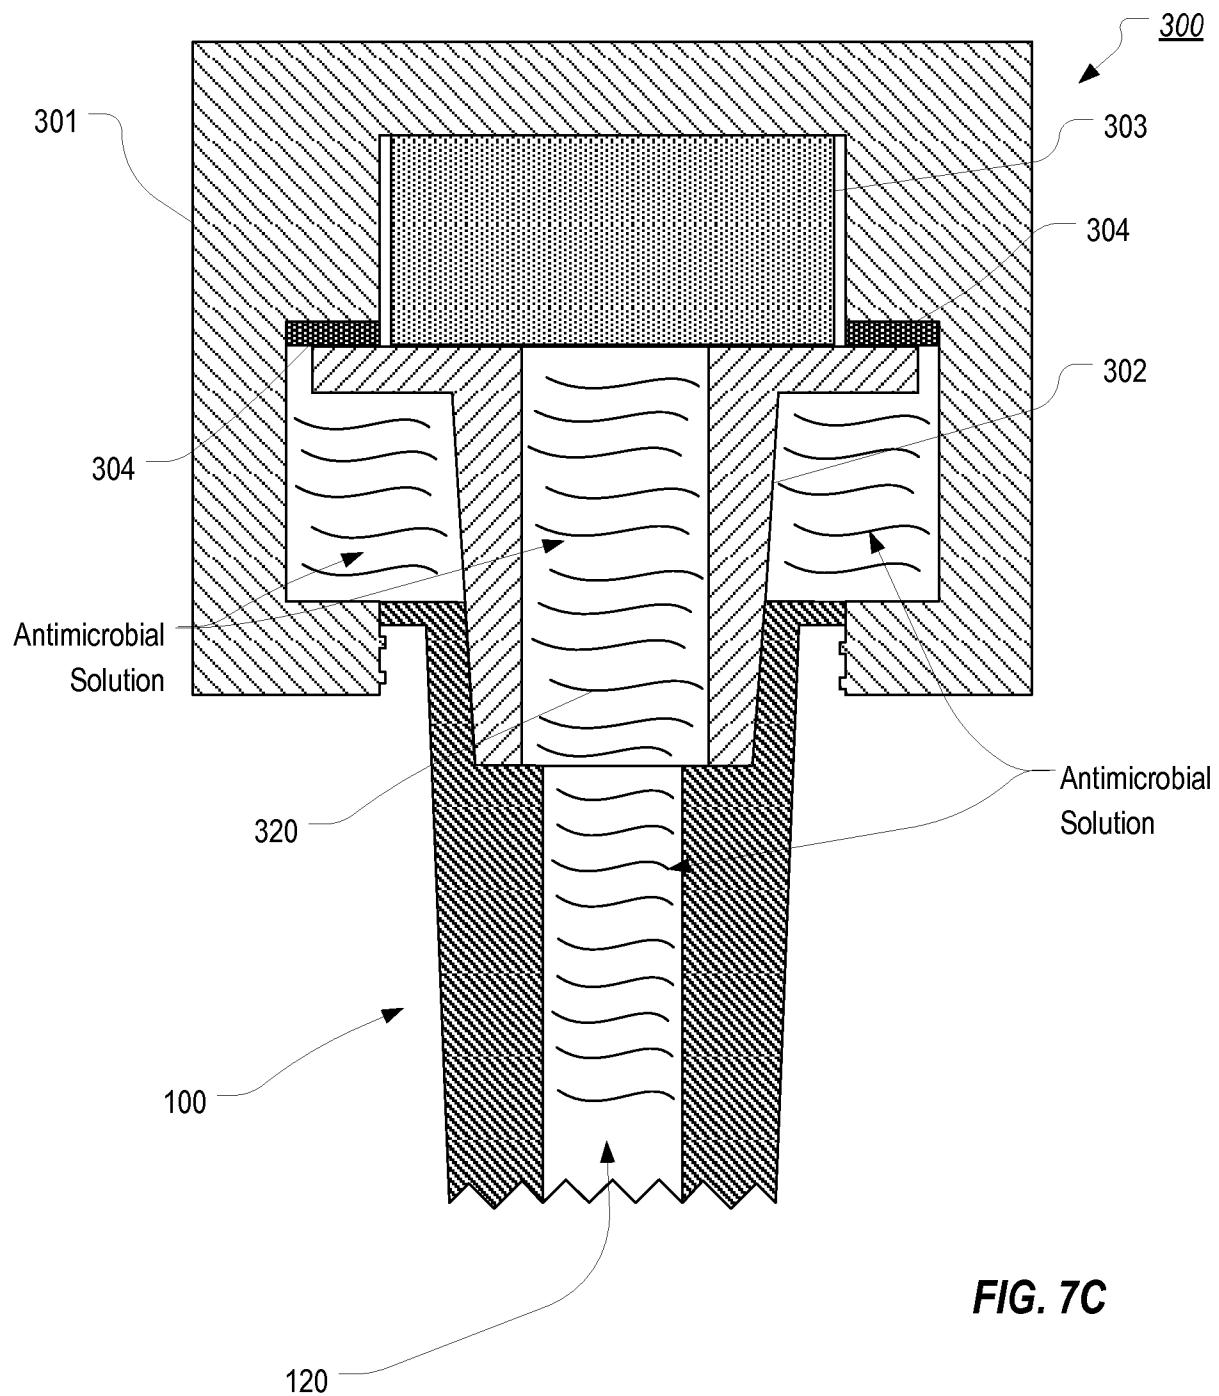


FIG. 7C

10 / 17

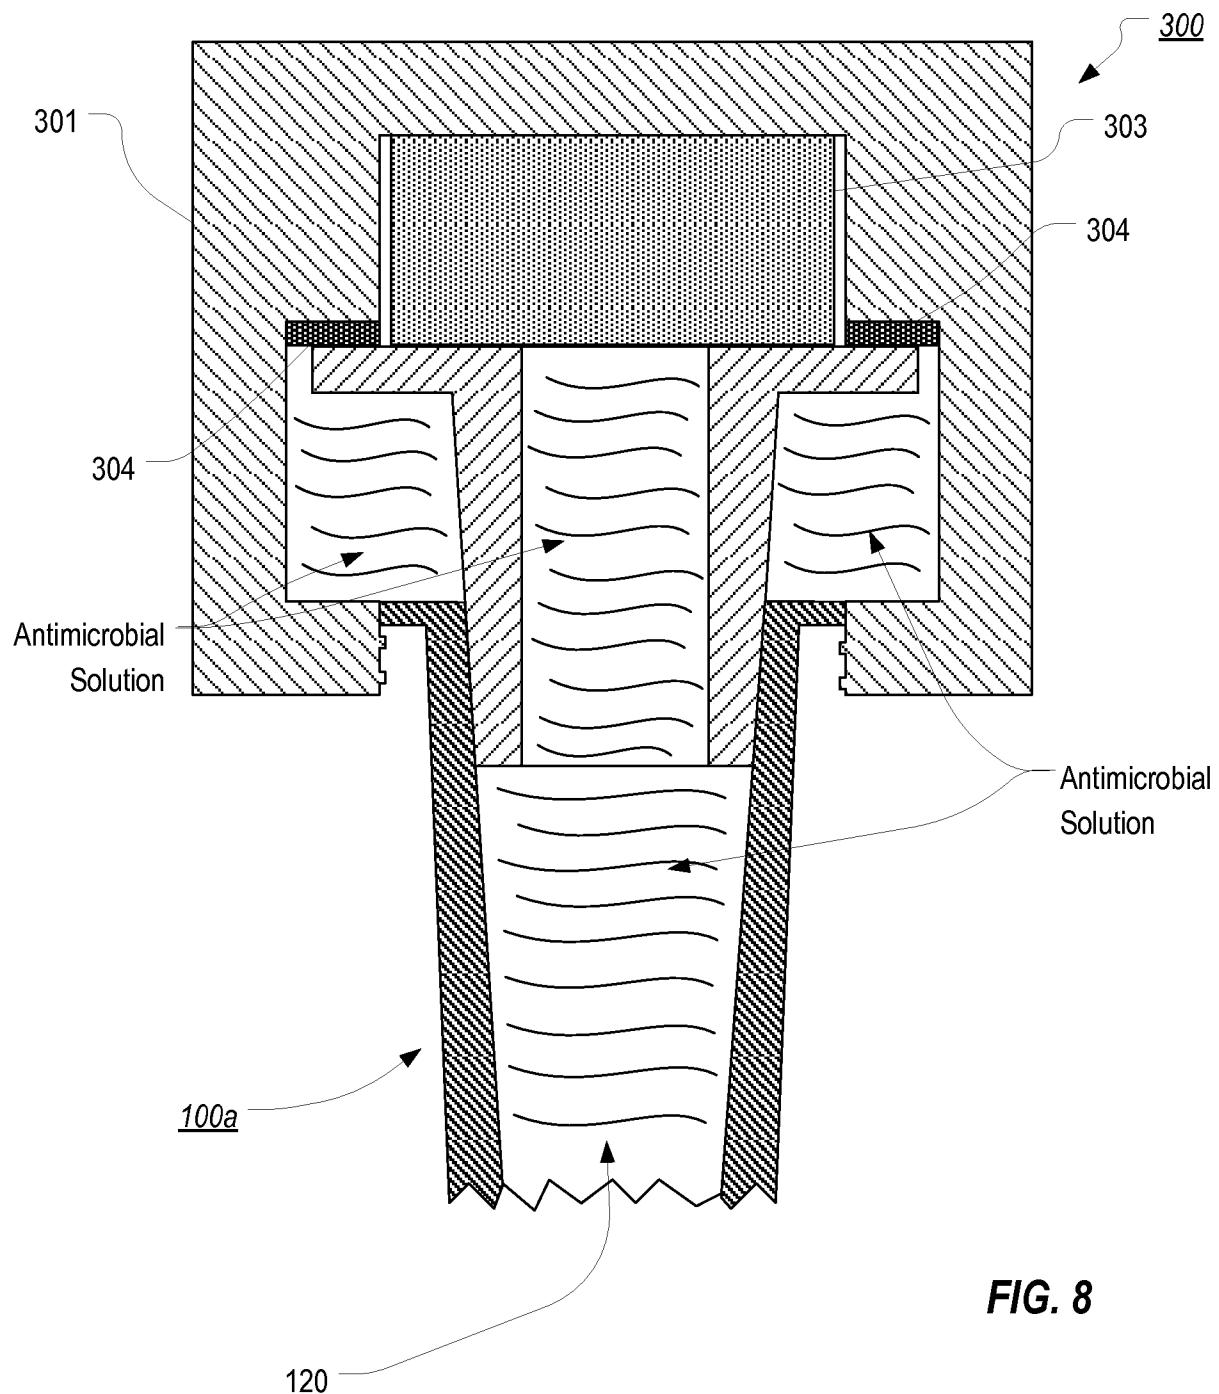


FIG. 8

11 / 17

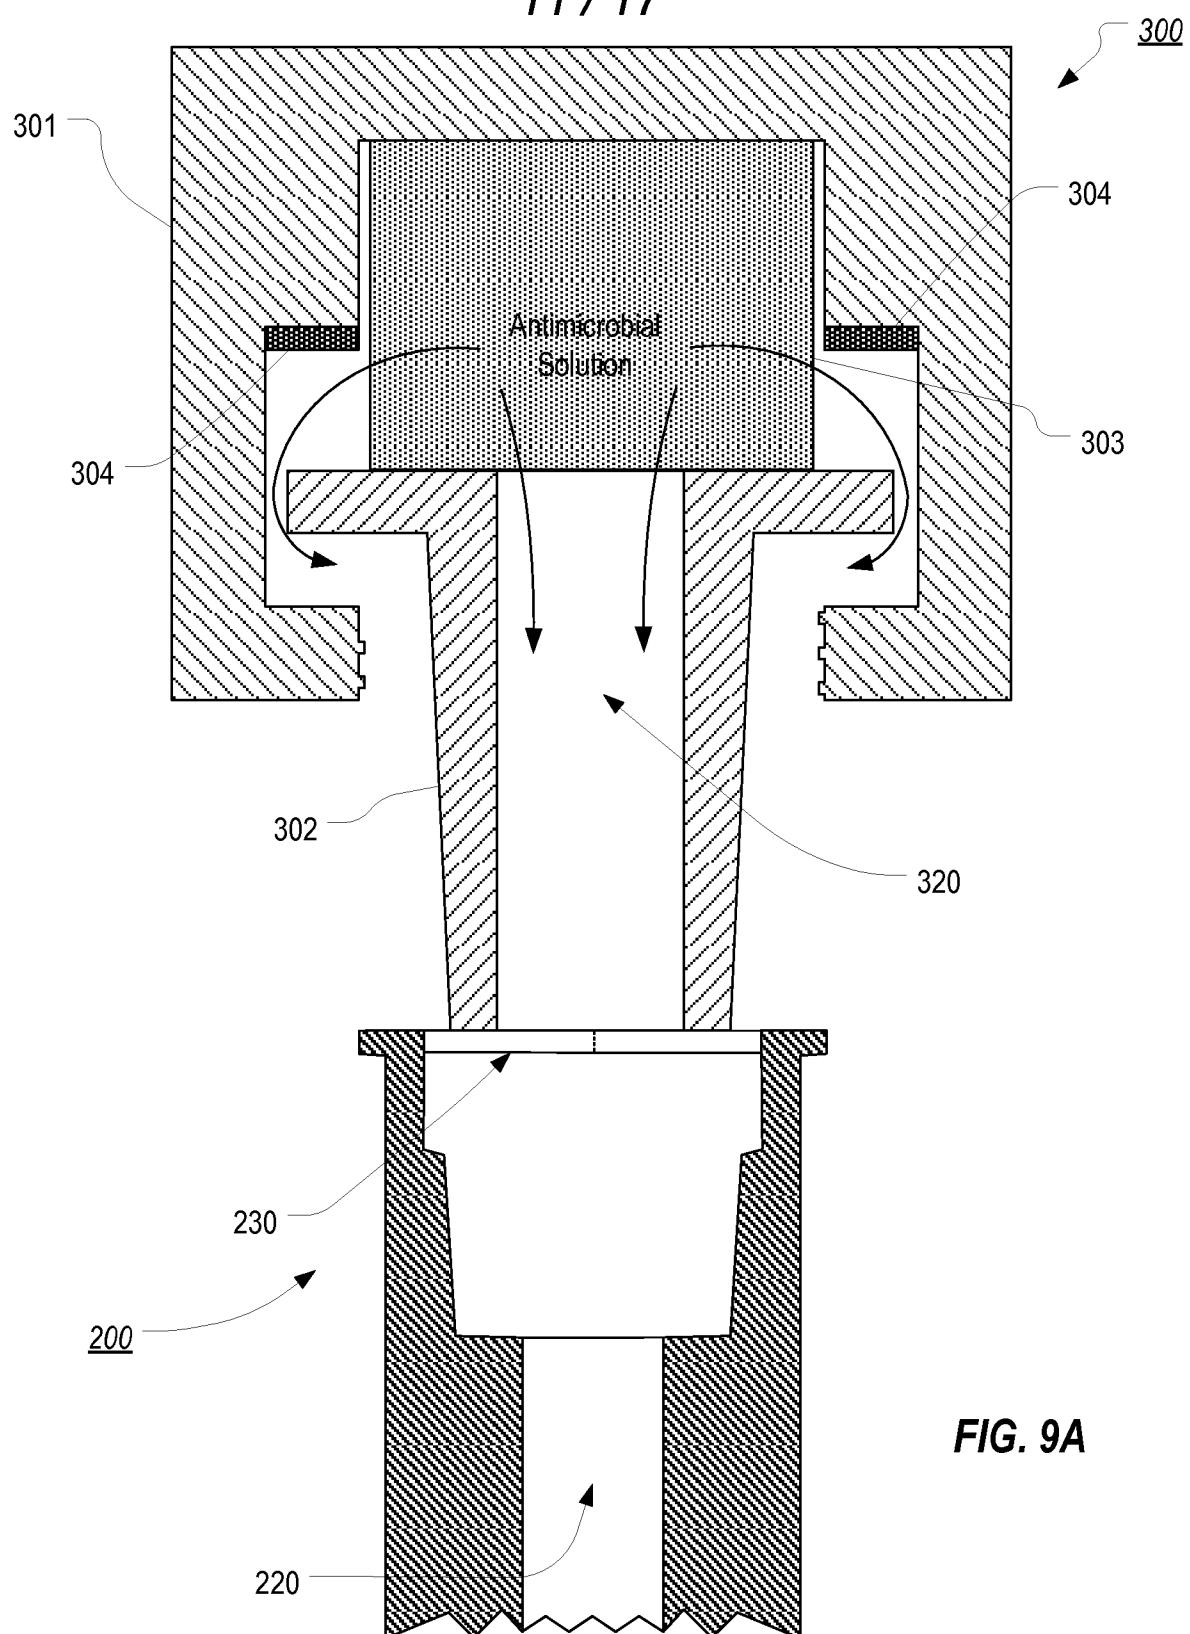
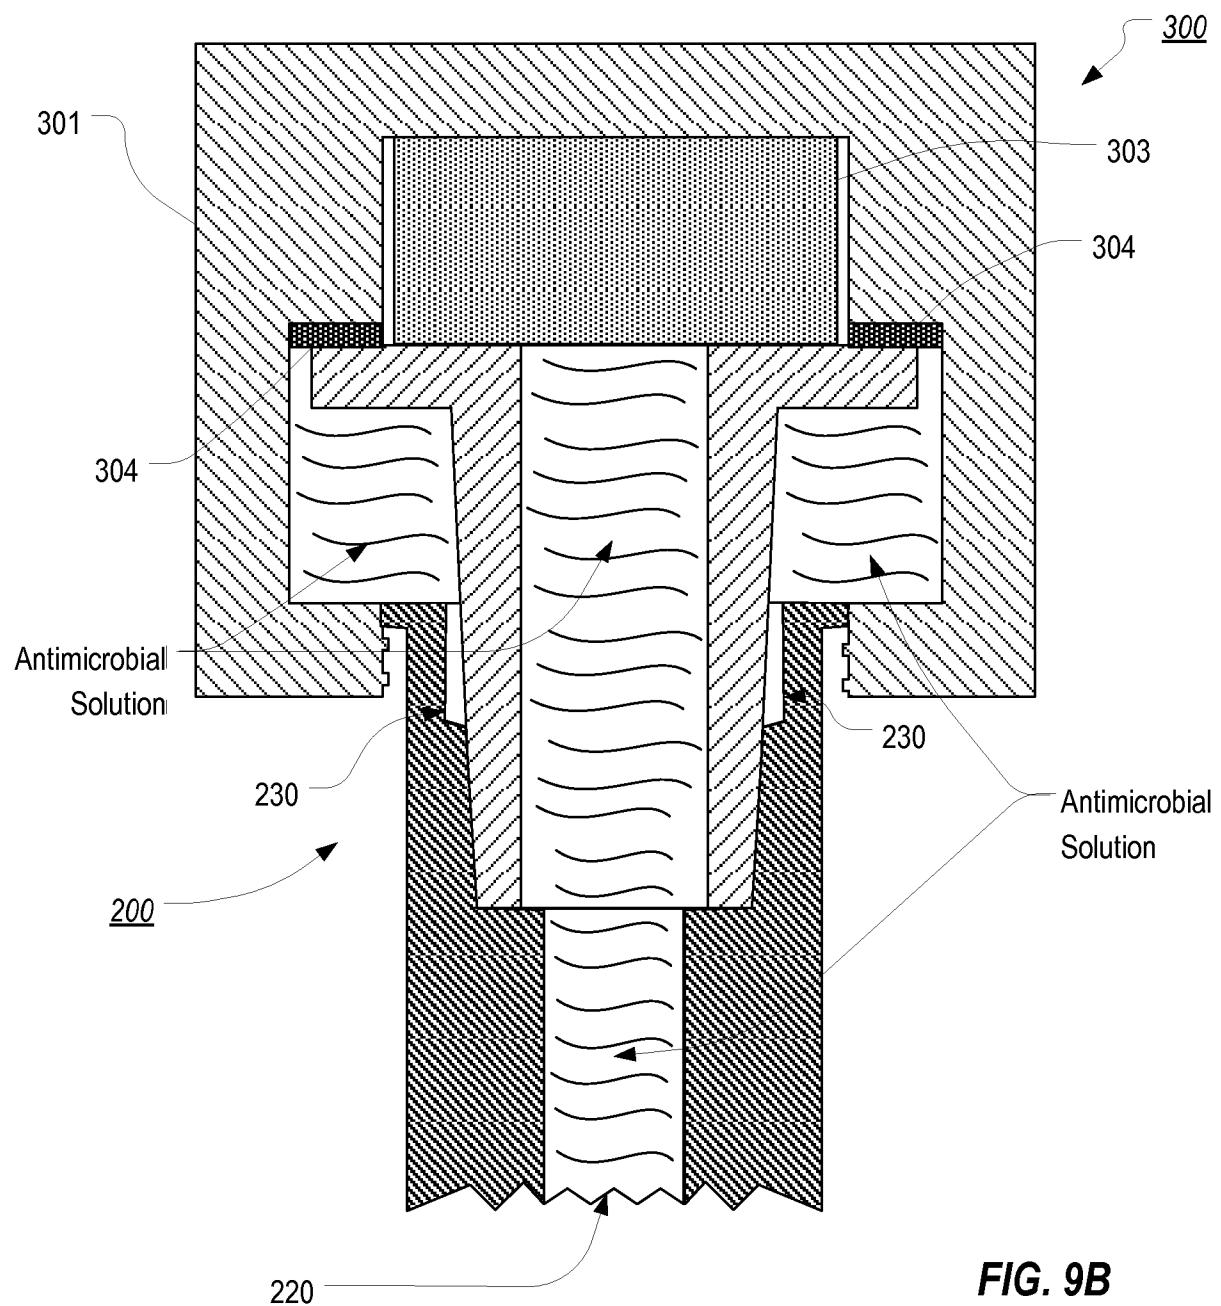
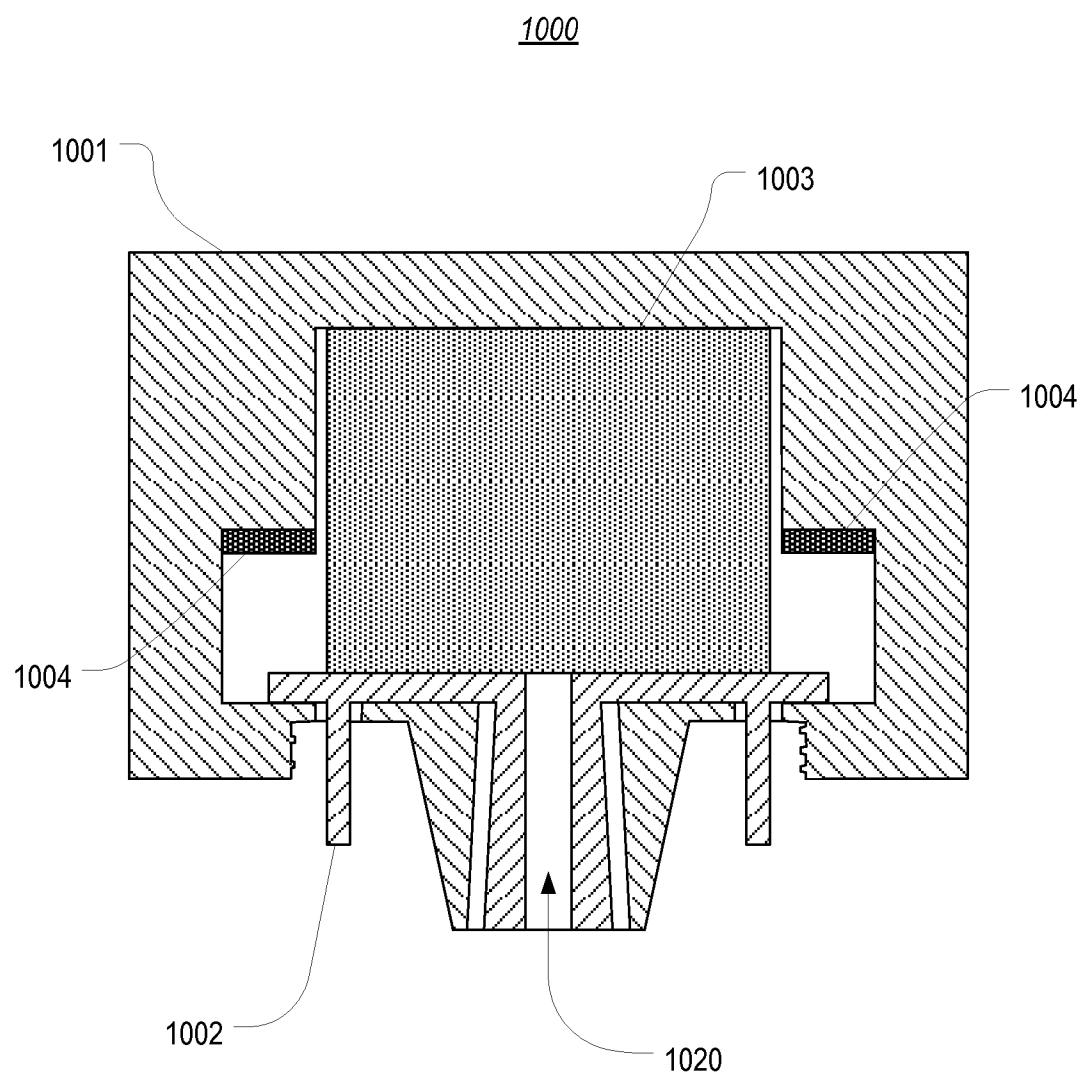


FIG. 9A


12 / 17

**FIG. 9B**

13 / 17

**FIG. 10A**

14 / 17

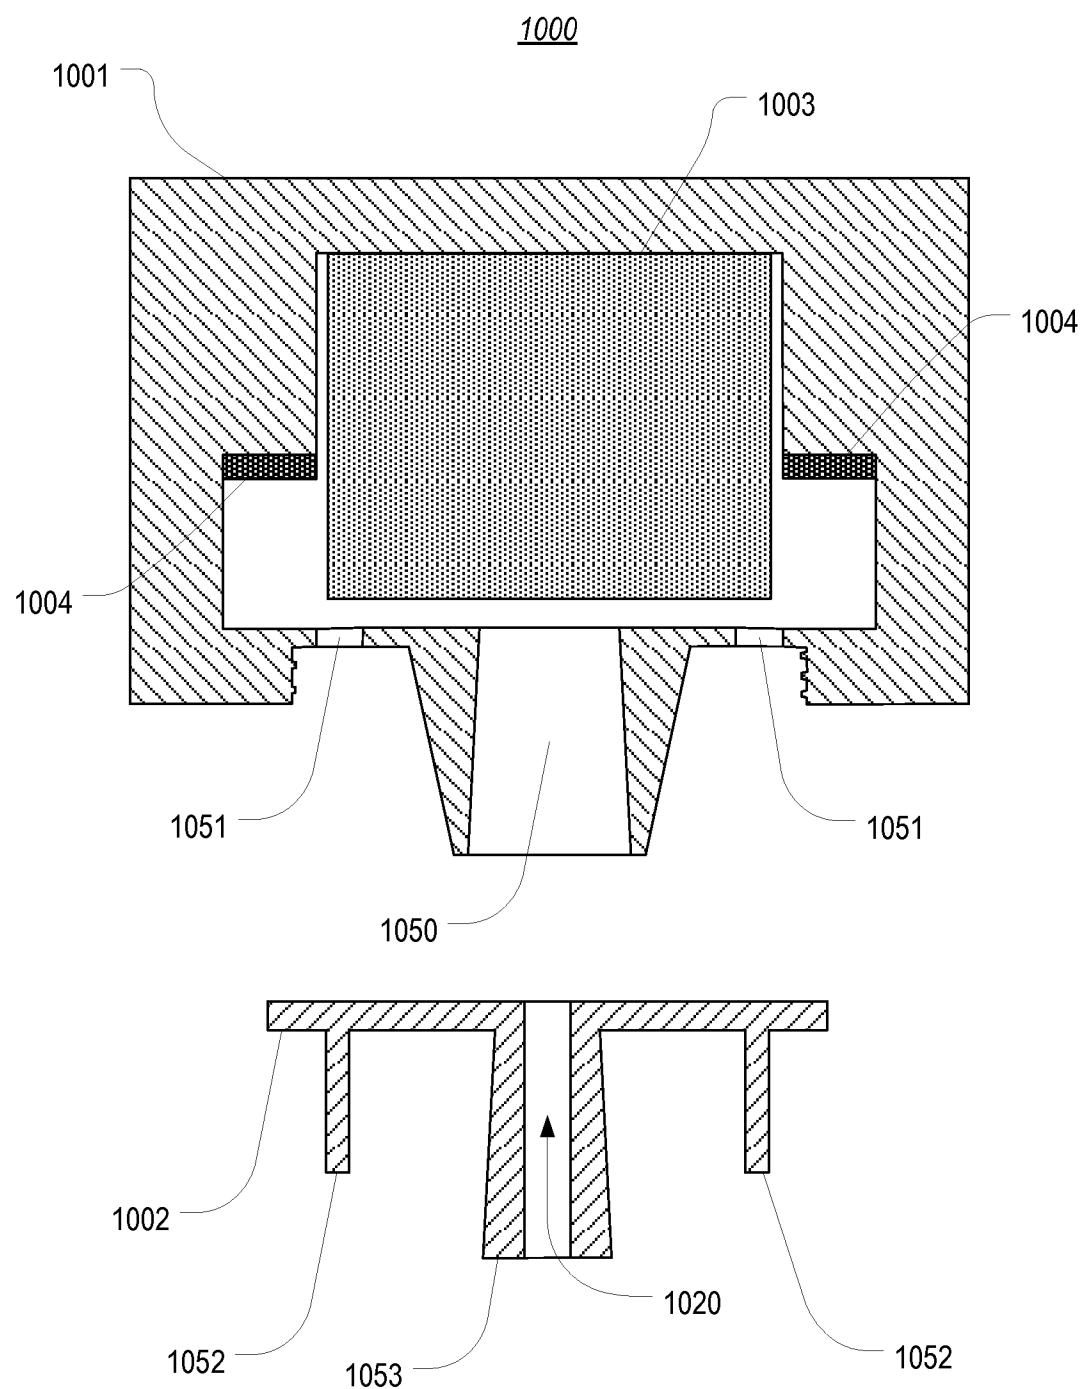**FIG. 10B**

15 / 17

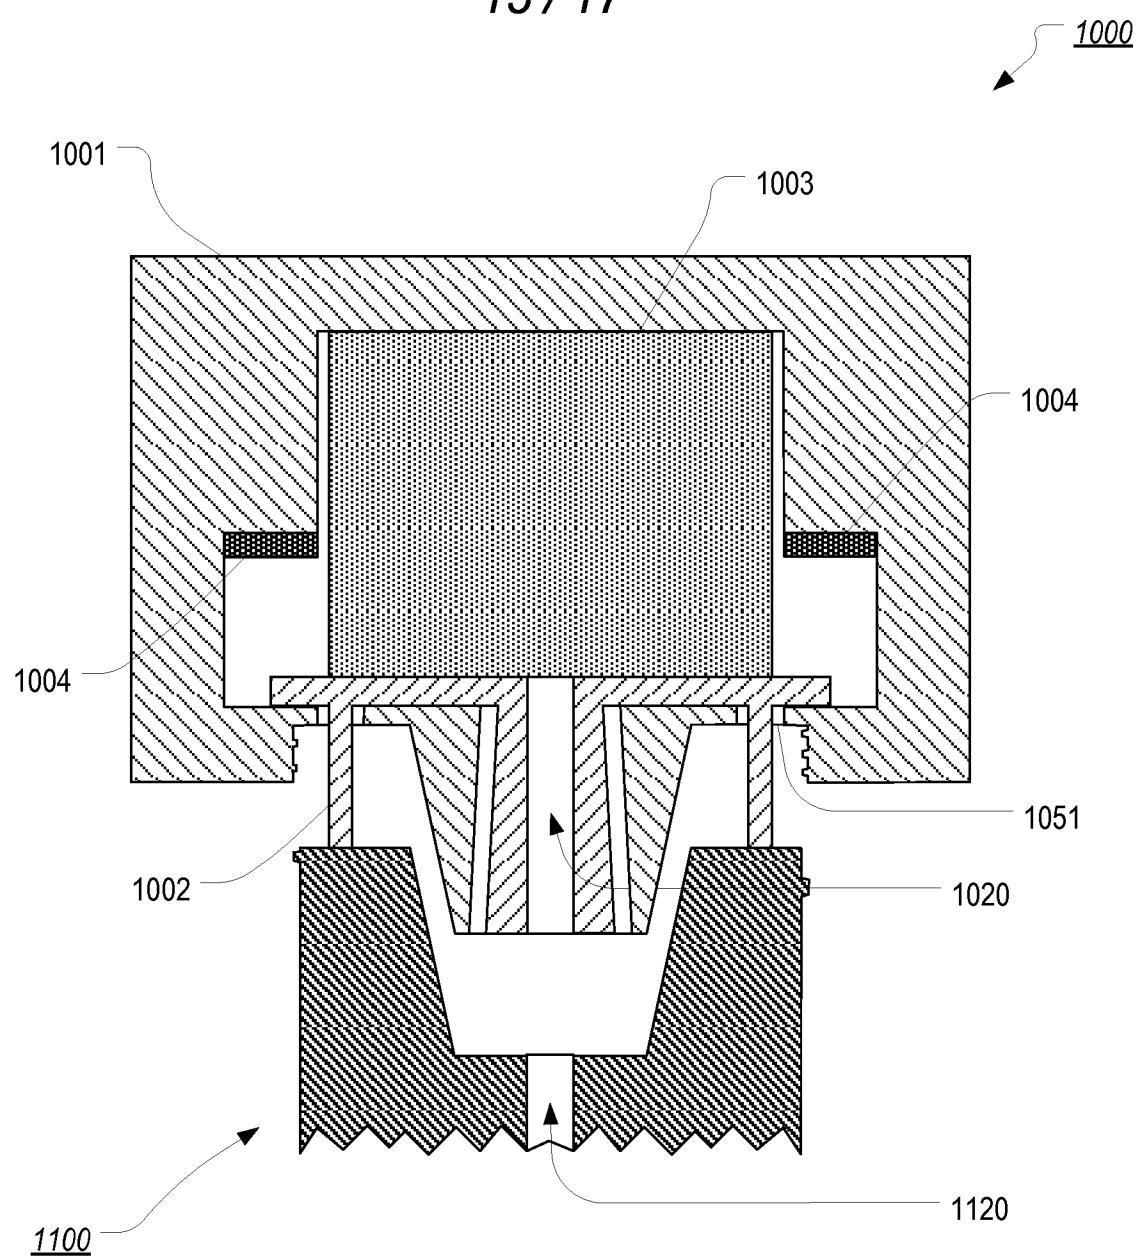


FIG. 11A

16 / 17

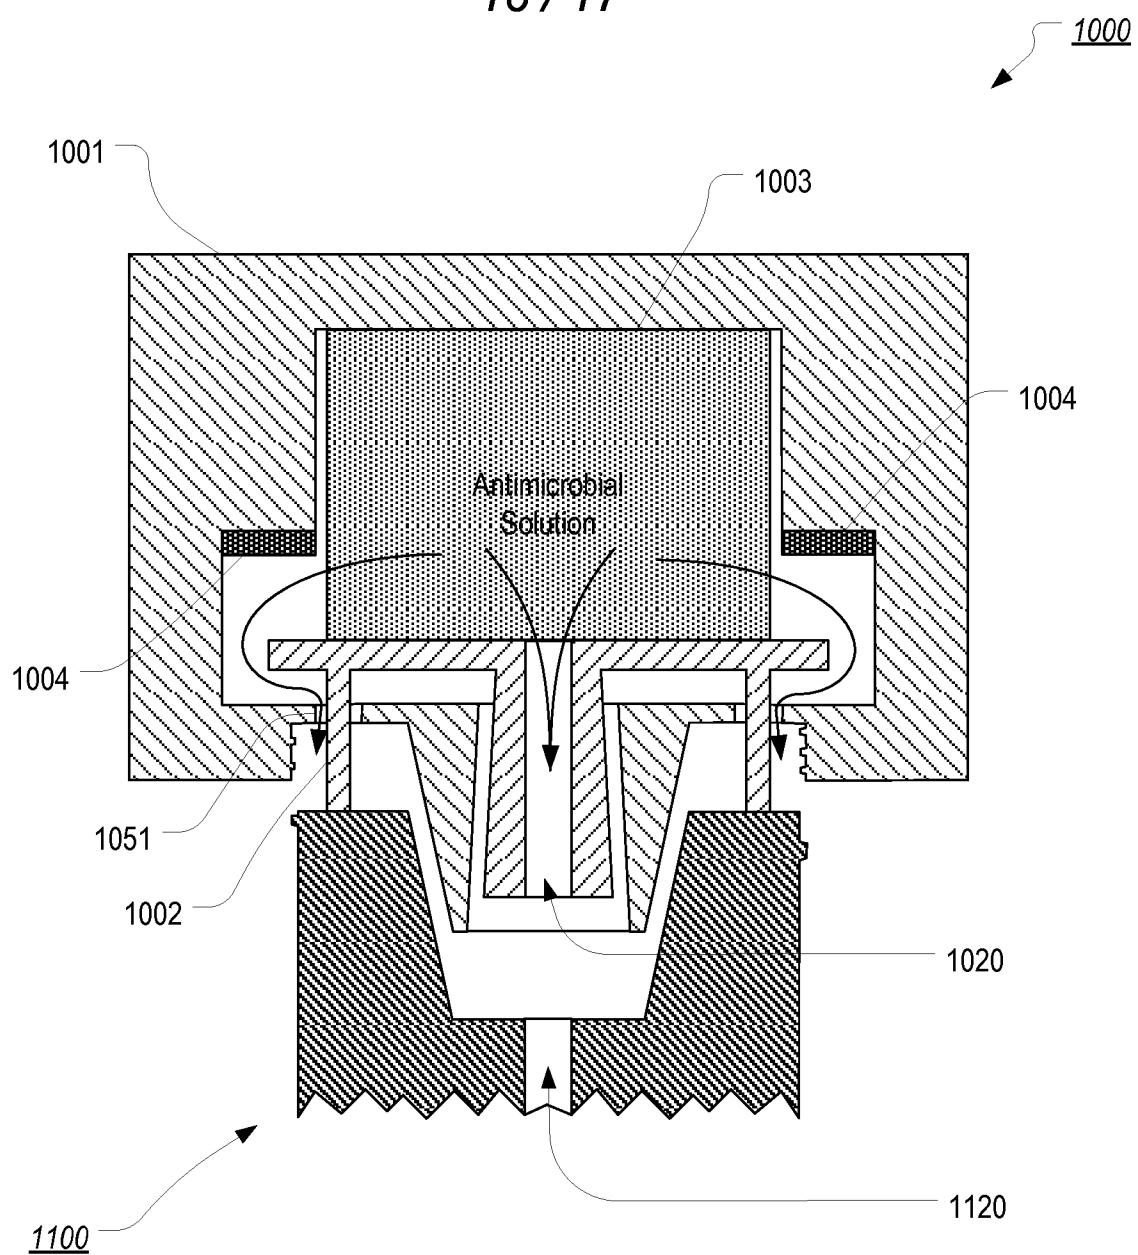


FIG. 11B

17 / 17

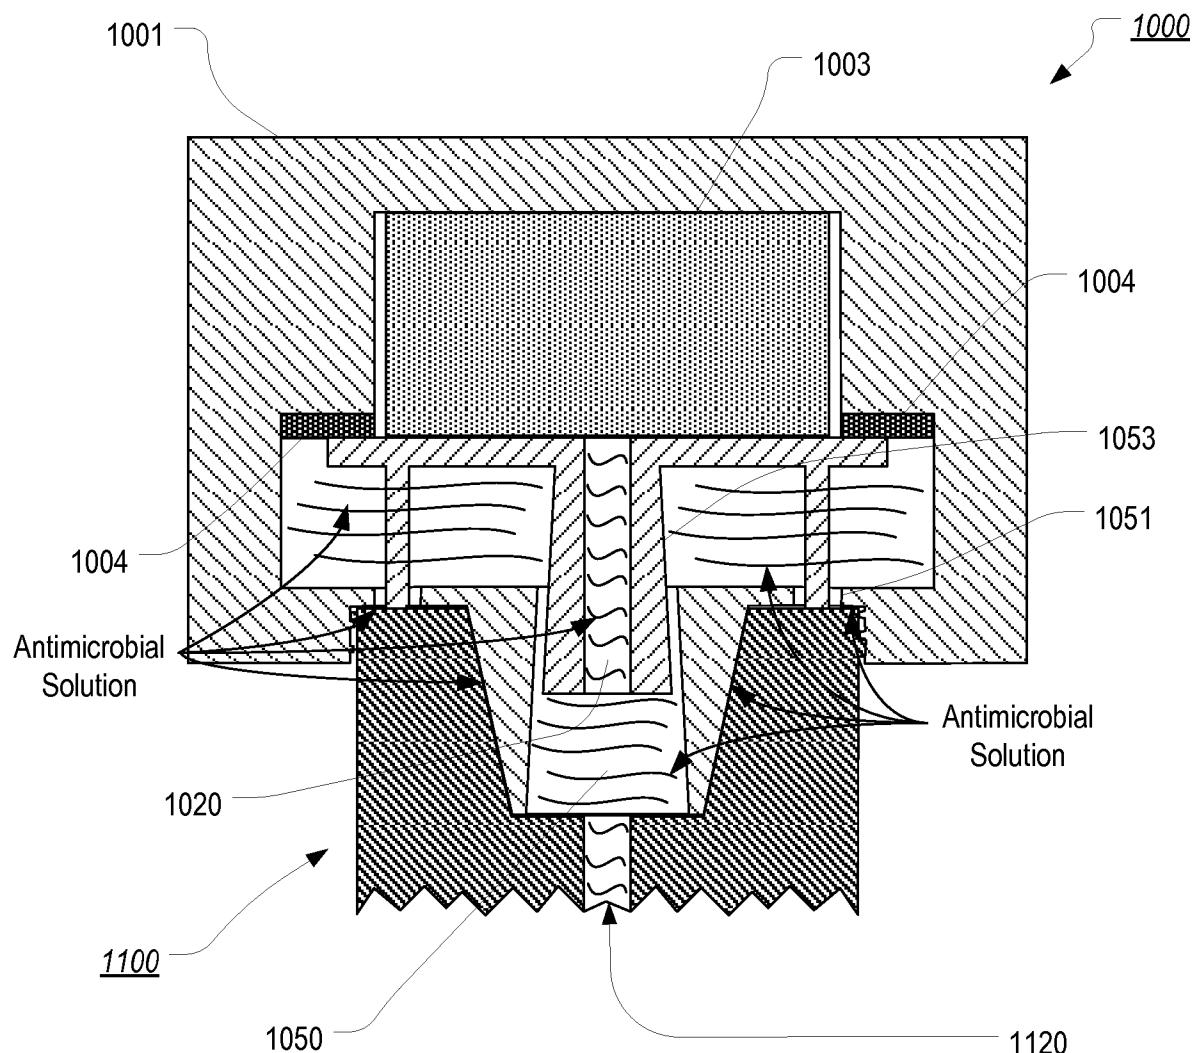


FIG. 11C

# INTERNATIONAL SEARCH REPORT

International application No  
PCT/US2015/015482

**A. CLASSIFICATION OF SUBJECT MATTER**  
INV. A61M25/00 A61M39/16 A61M39/20  
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2011/066586 A1 (CATHETER CONNECTIONS INC [US]; UNIV UTAH RES FOUND [US]; HITCHCOCK ROB) 3 June 2011 (2011-06-03) paragraph [0040] paragraph [0085] - paragraph [0093] figures 8A-8D -----	1-12
A	WO 2011/053924 A1 (CATHETER CONNECTIONS INC [US]; UNIV UTAH RES FOUND [US]; SOLOMON DONAL) 5 May 2011 (2011-05-05) paragraph [0197] figure 33 -----	13,18
X	WO 2008/100950 A2 (122 CORP [US]; ROGERS BOBBY E [US]; DIPERNA PAUL [US] IVERA MEDICAL CO) 21 August 2008 (2008-08-21) paragraph [0043] figure 6 -----	1-12
A	----- -/-	13,18

Further documents are listed in the continuation of Box C.

See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
8 May 2015	20/05/2015
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer  Amaro, Henrique

## INTERNATIONAL SEARCH REPORT

International application No  
PCT/US2015/015482

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 2 606 930 A1 (HADDEN GORDON [US]) 26 June 2013 (2013-06-26) paragraph [0023] figure 11 -----	1-12
A		13,18

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2015/015482

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
WO 2011066586	A1	03-06-2011	US	2011213341 A1		01-09-2011
			US	2013338644 A1		19-12-2013
			WO	2011066586 A1		03-06-2011
<hr/>						
WO 2011053924	A1	05-05-2011	CA	2778635 A1		05-05-2011
			CN	102686253 A		19-09-2012
			EP	2493528 A1		05-09-2012
			JP	2013509274 A		14-03-2013
			WO	2011053924 A1		05-05-2011
<hr/>						
WO 2008100950	A2	21-08-2008	US	2008019889 A1		24-01-2008
			US	2010313366 A1		16-12-2010
			US	2011277788 A1		17-11-2011
			US	2012216360 A1		30-08-2012
			US	2014101876 A1		17-04-2014
			US	2015000062 A1		01-01-2015
			WO	2008100950 A2		21-08-2008
<hr/>						
EP 2606930	A1	26-06-2013	CA	2775213 A1		21-06-2013
			EP	2606930 A1		26-06-2013
			US	2013164189 A1		27-06-2013
<hr/>						