



(51) International Patent Classification:

H01J 49/40 (2006.01)

(21) International Application Number:

PCT/GB2019/051839

(22) International Filing Date:

28 June 2019 (28.06.2019)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

1810573.4

28 June 2018 (28.06.2018)

GB

(71) Applicant: MICROMASS UK LIMITED [GB/GB];

Stamford Avenue, Altrincham Road, Wilmslow Cheshire
SK9 4AX (GB).

(72) Inventor: VERENCHIKOV, Anatoly; 15-Vladimira

Rolovica, City of Bar (ME).

(74) Agent: CHIVA, Andrew Peter; Dehns, St Bride's House,

10 Salisbury Square, London Greater London EC4Y 8JD
(GB).

(81) Designated States (unless otherwise indicated, for every

kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every

kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,

(54) Title: MULTI-PASS MASS SPECTROMETER WITH HIGH DUTY CYCLE

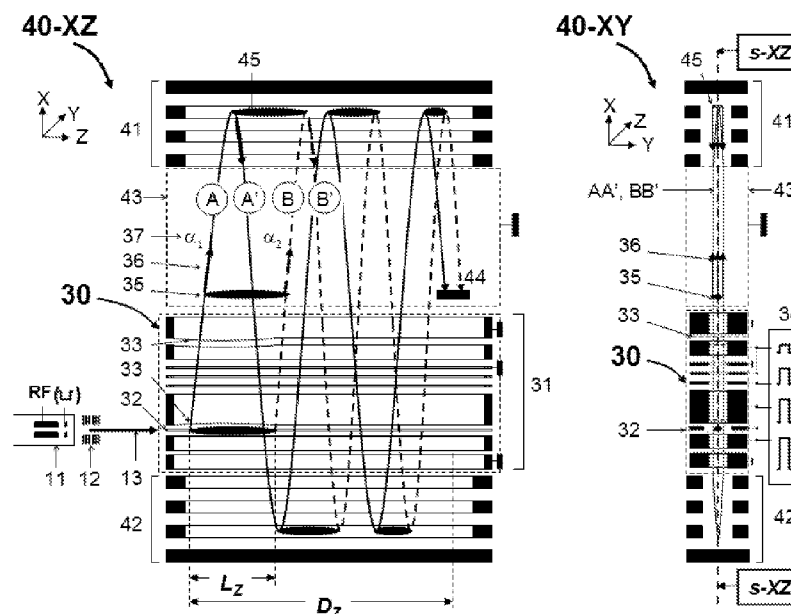


Fig.3

(57) **Abstract:** A multi-pass time-of-flight mass spectrometer is disclosed having an elongated orthogonal accelerator (30). The orthogonal accelerator (30) has electrodes (31) that are transparent to the ions so that ions that are reflected or turned back towards it are able to pass through the orthogonal accelerator (30). The electrodes (31) of the orthogonal accelerator (30) may be pulsed from ground potential in order to avoid the reflected or turned ion packets being defocused. The spectrometer has a high duty cycle and/or space charge capacity of pulsed conversion.



MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

MULTI-PASS MASS SPECTROMETER WITH HIGH DUTY CYCLE

5

CROSS-REFERENCE TO RELATED APPLICATION

This application claims priority from and the benefit of United Kingdom patent application No. 1810573.4 filed on 28 June 2018. The entire content of this application is incorporated herein by reference.

10

FIELD OF THE INVENTION

The invention relates to the area of time of flight mass spectrometers, multi-reflecting and multi-turn mass spectrometers, and is particularly concerned with improved duty cycle of pulsed converters.

15

BACKGROUND

Time-of-flight mass spectrometers (TOF MS) are widely used in combination with continuous ion sources, like Electron Impact (EI) ion sources, Electrospray Ionisation (ESI) ion sources, Inductively Coupled Plasma (ICP) ion sources and gaseous Matrix Assisted Laser Desorption and Ionization (MALDI) ion sources. To convert an ion beam from an intrinsically continuous ion source into pulsed ion packets there are employed orthogonal accelerators (OA), radiofrequency (RF) ion guides with axial ion ejection, and RF ion traps with radial pulsed ejection.

20

25

Initially, the OA method has been introduced by Bendix corporation as described in G.J. O'Halloran et.al, Report ASD-TDR-62-644, The Bendix Corporation, Research Laboratory Division, Southfield, MI, 1964. Dodonov et.al in SU1681340 and WO9103071 reintroduced and improved the OA injection method by using an ion mirror to compensate for multiple inherent OA aberrations. The beam propagates in the drift Z-direction through a storage gap between plate electrodes. Periodically, an electrical pulse is applied between plates. A portion of the continuous ion beam, located in the storage gap, is accelerated in an orthogonal X-direction, thus forming ribbon-shaped ion packets. Due to conservation of initial Z-velocity, the ion packets drift slowly in the Z-direction, thus traveling within the TOF MS along an inclined mean ion trajectory, get reflected by ion mirror, and finally reach a detector.

30

35

For improving duty cycle of pulsed conversion there were proposed various radio-frequency ion traps with either axial ion ejection as in US6020586 and US6872938, or radial ion ejection as in US6545268, US8373120, and US8017909. Ions are admitted into a radio-frequency ion guide for radial confinement with RF fields. Ions are locked axially by various types of DC plugs, get dampened in gas collisions at gas pressures of about 1 to 10mTorr, and are ejected by pulsed electric field, either axially or radially. Radial traps reach nearly 100% duty cycle of pulsed conversion, but they are strongly affected by space charge effects. The space charge capacity of RF traps is limited by the useful trap length, which in turn is limited by the geometrical arrangement within MPTOF analyzers (described below), necessary for the ion packet to bypass the trap after the ion mirror reflection.

40

45

In the last two decades, the resolution of TOF MS has been substantially improved by using multi-pass TOFMS (MPTOF) instruments. These instruments either have ion mirrors for multiple ion reflections (i.e. a multi-reflecting TOF (MRTOF)), such as described in SU1725289, US6107625, US6570152, GB2403063, and US6717132, or have electrostatic sectors for multiple ion turns (i.e. a multi-turn TOF (MTTOF)) such as described in US7504620, US7755036, and M. Toyoda, et.al, J. Mass Spectrom. 38 (2003) 1125, each of which is incorporated herein by reference. The term “pass” is a generalized term covering ion mirror reflections in an MRTOF and ion turns in an MTTOF. In other words, an MP-TOF covers both MRTOF and MTTOF instruments. The resolving power of an MP-TOF instrument grows with increasing numbers of passes N . However, arranging a conventional OA in an MP-TOF instrument, as in US6717132 and US7504620, limits the efficiency of pulsed conversion of the OA, elsewhere called the duty cycle. To avoid spectral overlaps, the duty cycle of an MP-TOF with an OA is limited to being $DC < 1/N$ for heaviest ions, and realistically $DC < 1/2N$, accounting for the rims of the OA and of the detector, and further drops as the square root of the specific ion mass $\mu = m/z$ for lighter ions (see *eq.3* below).

WO2016174462 proposes increasing the OA length and duty cycle by displacing the OA from the central path of the MR-TOF analyser and arranging ion oscillations around the symmetry plane of isochronous trajectory. However, operation off the isochronous plane strongly affects the resolution and the spatial ion focusing of the MRTOF analyzer. Copending application WO2019/030475 proposes shifting the accelerator from the MPTOF symmetry plane and pulsed deflection of ion packets back onto the symmetry plane. However, the solution poses limits onto the admitted mass range.

SUMMARY

The present invention provides a time-of-flight mass analyser comprising: at least one ion mirror or electrostatic sector for reflecting or turning ions, respectively; an orthogonal accelerator having electrodes for receiving ions and orthogonally pulsing packets of the ions into the ion mirror or electrostatic sector such that the ions are reflected or turned, respectively, in a first dimension (x-direction) as they drift in a drift direction (z-direction); and an ion detector; wherein the electrodes of the orthogonal accelerator define slits or comprise meshes for allowing ions that have been reflected by the ion mirror, or turned by the electrostatic sector, to pass back into and through the orthogonal accelerator as they travel towards the detector.

The mass analyser is configured such that after the ions have been reflected or turned they pass back into, through and out of the orthogonal accelerator (e.g. into a first side and out of a second, opposite side of the orthogonal accelerator), without the ions hitting the electrodes of the orthogonal accelerator. As such, the orthogonal accelerator can be relatively long in the drift direction, so as to provide a relatively high duty cycle instrument, without the orthogonal accelerator blocking the path of the ions to the detector (or without having to cause the ions to advance a relatively long distance in the drift direction for each ion reflection or turn such that the ions do not impact on the orthogonal accelerator).

The drift direction (z-direction) is perpendicular to the first dimension (x-direction).

The slits described herein may be gridless slits, i.e. they do not include meshes therein.

In the embodiments in which the ions are reflected by the at least one mirror, the

mean trajectory of the reflected ions may be in a plane defined by the first dimension and the drift direction (z-direction). The orthogonal accelerator and the slits are arranged in this plane such that the ions pass through the slits.

The mass analyser may be either: (i) a multi-reflecting time-of-flight mass analyser
5 having the orthogonal accelerator arranged between two ion mirrors, and arranged and configured so that the ions are reflected multiple times between the ion mirrors and pass through the orthogonal accelerator, via the slits or meshes, multiple times as the ions travel from the orthogonal accelerator to the detector; or (ii) a multi-turn time-of-flight mass
10 analyser having the orthogonal accelerator arranged between electrostatic sectors of a plurality of electrostatic sectors that turn the ions a plurality of times such that the ions pass through the orthogonal accelerator multiple times, via the slits or meshes, as they travel from the orthogonal accelerator to the detector.

In the embodiments in which the mass analyser is a multi-reflecting time-of-flight mass analyser, the ions may pass into a first side of the orthogonal accelerator and out of a
15 second opposite side of the orthogonal accelerator for at least some of the times, or each and every time, that the ions pass from one mirror to another. Similarly, in the embodiments in which the mass analyser is a multi-turn time-of-flight mass analyser, the ions may pass into a first side of the orthogonal accelerator and out of a second opposite side of the orthogonal accelerator for at least some of the times, or each and every time, that the ions complete one
20 complete turn (i.e. are turned 360 degrees by the sectors).

The electrodes of the orthogonal accelerator and their slits or meshes may extend in the drift direction (z-direction) from an upstream end of the orthogonal accelerator to a point proximate or downstream of the detector.

The electrodes of the orthogonal accelerator may define said slits; and at least one
25 slit, or each slit, may be provided as an aperture through an electrode of the orthogonal accelerator that is elongated in the drift direction, such that electrode material completely surrounds the perimeter of the slit; and/or at least one slit, or each slit, may be defined between electrode portions that are elongated in the drift direction and spaced apart in a direction perpendicular to the first dimension and drift direction.

30 The electrode portions may not be joined together at one or both of their longitudinal ends (in the z-direction). For example, the electrode portions may be two spaced apart wires or rods.

The downstream ends of the orthogonal accelerator electrodes may be spaced apart from the detector, in the drift direction (z-direction); and the electrodes of the orthogonal
35 accelerator may define said slits; wherein each slit is defined between elongated electrode portions that are not joined together at their downstream ends.

The downstream ends are downstream in the drift direction (z-direction).

For example, each slit may be defined by a c-shaped electrode that is open at one longitudinal end, or between two separate elongated electrode portions that are not joined
40 together at both of their longitudinal ends (e.g. two spaced apart wires or rods).

Ions may be reflected by a mirror or between ion mirrors, or turned by one or more of the electrostatic sectors, such that the ions pass through the gap one or more times as they pass from the downstream end (in the z-direction) of the orthogonal accelerator to the detector.

45 The mass analyser may comprise: one or more voltage supply for applying one or more voltage pulse to the electrodes of the orthogonal accelerator for performing said step of orthogonally pulsing the packets of the ions; and control circuitry configured to control the one or more voltage supply so as to only apply said one or more voltage pulse to the electrodes for orthogonally pulsing a packet of ions out of the orthogonal accelerator when

ions that have previously been pulsed out of the orthogonal accelerator are not passing back through the orthogonal accelerator.

5 The orthogonal accelerator may comprise an ion guide portion having electrodes arranged to receive ions, and one or more voltage supply configured to apply potentials to these electrodes for confining ions in at least one dimension (X- or Y-dimension) orthogonal to the drift direction.

10 The orthogonal accelerator may comprise: an ion guide portion having electrodes arranged to receive ions travelling along a first axis (Z-direction), including a plurality of DC electrodes spaced along the first axis; and DC voltage supplies configured to apply different DC potentials to different ones of said DC electrodes such that when ions travel through the ion guide portion along the first axis they experience an ion confining force, generated by the DC potentials, in at least one dimension (X- or Y-dimension) orthogonal to the first axis.

15 The mass analyser may comprise focusing electrodes that are arranged and configured to control the motion of ions along the drift direction (z-direction) so as to spatially focus or compress each of the ion packets so that it is smaller, in the drift direction, at the detector than when pulsed out of the orthogonal accelerator.

20 The focusing electrodes may be configured to impart ions located at different positions, in the drift direction, within the ion packet with different velocities in the drift direction so as to perform the spatial focusing or compression.

25 The focusing electrodes may comprise a plurality of electrodes configured to generate an electric field region through which ions travel in use that has equipotential field lines that curve and/or diverge as a function of position along the drift direction so as to focus ions in the drift direction.

30 The focusing electrodes may comprise a plurality of electrodes configured to control the velocities of the ions such that ions within the orthogonal accelerator when it is pulsed have velocities, in the drift direction, that decrease as a function of distance in the drift direction towards the detector.

35 The plurality of electrodes may comprise an ion guide or ion trap upstream of the orthogonal accelerator and one or more electrodes configured to pulse ions out of the ion guide or ion trap such that the ions arrive at the orthogonal accelerator at different times and with velocities in the drift direction that increase as a function of the time at which they arrive at the orthogonal accelerator.

40 The mass analyser may comprise circuitry that synchronises the pulsing of ions out of the ion guide or ion trap with the pulsing of ion packets out of the orthogonal accelerator, wherein the circuitry is configured to provide a time delay between the pulsing of ions out of the ion guide or ion trap and the pulsing of ion packets out of the orthogonal accelerator, wherein the time delay is set based on a predetermined range of mass to charge ratios of interest to be mass analysed.

45 The plurality of electrodes may comprise electrodes arranged within the orthogonal accelerator to generate an axial potential distribution along the drift direction that slows ions by different amounts depending on their location, in the drift direction, within the orthogonal accelerator.

The mass analyser may be configured such that the length of the orthogonal accelerator from which ions are pulsed (L_z) is longer, in the drift direction, than half of the distance (A_z) that the ion packet advances for each mirror reflection or sector turn in the first dimension.

For an MRTOF mass analyser, the distance A_z may be determined along the axis that is half-way between the mirrors (i.e. half way in the x-direction). The distance A_z may

be determined based on the positions of the centre (in the z-direction) of the ion packet before and after each reflection. The distance A_z may be the mean distance A_z for all of the mirror reflections. Similarly, for an MTTOF mass analyser, the distance A_z may be determined along the axis that is half-way between opposing sectors (i.e. half way in the x-direction). The distance A_z may be determined based on the positions of the centre (in the z-direction) of the ion packet before and after each 180 degree turn. The distance A_z may be the mean distance A_z for all of the mirror reflections.

The ratio L_z/A_z may be selected from the group of: (i) $0.5 < L_z/A_z < 1$; (ii) $1 < L_z/A_z < 2$; (iii) $2 < L_z/A_z < 5$; (iv) $5 < L_z/A_z < 10$; (v) $10 < L_z/A_z < 20$; and (vi) $20 < L_z/A_z < 50$; or the length of the region of the orthogonal accelerator from which ions are pulsed (L_z) may be longer, in the drift direction, than x% of the distance, in the drift direction, between the entrance to the orthogonal accelerator and the midpoint of the detector, wherein x is: ≥ 10 , ≥ 15 , ≥ 20 , ≥ 25 , ≥ 30 , ≥ 35 , ≥ 40 , ≥ 45 , or ≥ 50 .

The present invention also provides a mass spectrometer comprising: an ion source; and a mass analyser as described herein.

The present invention also provides a method of mass spectrometry comprising: providing a mass analyser as described herein; receiving ions in said orthogonal accelerator; pulsing ions from said orthogonal accelerator into said ion mirror or sector; reflecting or turning the ions with the ion mirror or electrostatic sector, respectively, so that the ions pass back into and through the orthogonal accelerator via the slits defined by the electrodes or the meshes in the orthogonal accelerator; and receiving ions at said detector.

An improved orthogonal accelerator is proposed for multi-pass time-of-flight mass spectrometers (MPTOF). The orthogonal accelerator is elongated in the drift Z-direction and placed on the MPTOF surface of isochronous ion motion in the orthogonal Y-direction, being a symmetry plane in MRTOF. The electrodes of orthogonal accelerator are made transparent, for example using slits in all electrodes, including the push plate. As described elsewhere herein, each slit may be formed by a slot in an electrode, or between elongated electrode portions (such as between wire or rod electrode portions, or by between the electrodes on different PCBs. Less preferably, the electrodes of the orthogonal accelerator may be made transparent by using mesh electrodes through which the ions can pass. Thus, ions may pass through the switched off accelerator after at least one reflection or turn in the MPTOF analyzer. To ease the detector bypassing and to avoid spectral confusion, ion packets may be isochronously focused in the drift Z-direction onto detector, either by isochronous trans-axial or Fresnel lens and wedge, or by arranging spatial and temporal correlation within a continuous ion beam.

To retain the ion beam within a relatively long orthogonal accelerator before it is pulsed, the ion beam may be confined with an RF quadrupolar field or within a spatially alternated DC quadrupolar field.

A long orthogonal accelerator may improve the duty cycle and space charge capacity of an MPTOF by an order of magnitude, without introducing additional analyzer aberrations and need not set limits onto the admitted mass range.

The approach may be adopted for MPTOF with radially ejecting RF ion traps. RF traps are elongated for larger space charge capacity. The trap is placed on the plane of isochronous ion motion in the MPTOF and is made of electrodes with slits, so that ions may pass through the switched off trap after at least one turn or reflection. Ion packets may be spatially focused by isochronous lens to fit the detector size after multiple passes in MPTOF.

According to the one aspect of the invention, there is provided a multi-pass MPTOF (multi-reflecting or multi-turn) time-of-flight mass spectrometer comprising:

- (a) an ion source, generating an ion beam along a first drift Z-direction;
- (b) an orthogonal accelerator with spatial confinement means and with electrodes connected to pulsed supplies for admitting said ion beam into a storage gap, for retaining ion beam within said confinement means and for pulsed accelerating a portion of said ion beam in the second orthogonal X-direction, thus forming ion packets;
- (c) isochronous means for ion packet focusing in said Z-direction towards a detector, arranged either within or immediately after said orthogonal accelerator;
- (d) an electrostatic multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), built of parallel ion mirrors or electrostatic sectors, separated by a drift space and substantially elongated in the Z-direction to form an electrostatic field in an orthogonal XY-plane; said two-dimensional field provides for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion within an isochronous mean ion trajectory s-surface – either symmetry s-XY plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of said accelerator and of said z-focusing means; and
- (e) wherein electrodes of said orthogonal accelerator comprise slits, transparent for return ion passage after at least one reflection or turn.

Optionally, said means for ion beam spatial confinement may comprise at least one mean of the group: (i) side plates connected to radiofrequency (RF) signal; (ii) side plates connected to an attracting DC potential; (iii) segmented side plates connected to spatially alternated DC potentials; (iv) segmented DC dipoles connected to spatially alternated dipolar DC potentials.

Optionally, said isochronous means for ion packet focusing in the Z-direction may comprise at least one means of the group: (i) a set of trans-axial lens and wedges; (ii) a Fresnel lens and wedge arranged in multi-segmented deflector; and (iii) means for spatial or temporal variations of ion beam energy for arranging negative correlation between energy and position in Z-direction.

Optionally, said spatial-temporal correlation may be arranged with at least one means of the group: (i) pulsed acceleration of continuous ion beam in the Z-direction either within electrostatic channel or within a radio frequency RF ion guide, located upstream of said orthogonal accelerator; (ii) a time-variable floated elevator within an electrostatic channel or an RF ion guide, located upstream of said pulsed converter; (iii) a Z-dependent deceleration of ion beam within said orthogonal accelerator.

Optionally, said drift space of said multi-pass analyzer may be set at ground and wherein electrodes of said orthogonal accelerator may be energized by pulsed voltages to extract said ion packets.

According to the another aspect of the invention, there is provided a method of time-of-flight mass spectrometry comprising the following steps:

- (a) generating an ion beam along a first drift Z-direction in an ion source;
- (b) admitting said ion beam into a storage gap of an orthogonal accelerator, spatially confining said ion beam within said storage gap, and pulsed accelerating a portion of said ion beam in the second orthogonal X-direction, thus forming ion packets;
- (c) ion packet focusing in said Z-direction towards a detector, arranged at or immediately after said orthogonal accelerator step;
- (d) in an orthogonal XY-plane, arranging two dimensional electrostatic fields of multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), substantially elongated in the Z-direction; said two-dimensional fields provide for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion within an isochronous mean ion trajectory s-surface – either symmetry s-XY

plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of electric fields at said acceleration and said z-focusing steps; and

- (e) Wherein said fields of orthogonal accelerator are arranged with transparent electrodes for non destructing and non defocusing return ion passage after at least one reflection or turn.

Optionally, said step of ion beam spatial confinement may comprise at least one step of the group: (i) radial ion confinement by radiofrequency (RF) quadrupolar field; (ii) ion confinement in the X-direction by quadrupolar DC field; (iii) radial ion confinement within periodic DC field of annular ion guide; and (iv) radial ion confinement within quadrupolar and spatially periodic DC field.

Optionally, said step of isochronous ion packet focusing in the Z-direction may comprise at least one step of the group: (i) ion focusing in electrostatic field of trans-axial lens and wedges; (ii) ion focusing by a Fresnel lens and wedge arranged in multi-segmented deflector; and (iii) arranging negative correlation between ion energy and position in Z-direction within said ion storage gap.

Optionally, said spatial-temporal correlation may be arranged with at least one step of the group: (i) pulsed acceleration of continuous ion beam in the Z-direction either within electrostatic channel or within a radio frequency RF ion guide, located upstream of said orthogonal accelerator; (ii) a time-variable floating of an elevator within an electrostatic channel or an RF ion guide, located upstream of said pulsed converter; and (iii) a Z-dependent deceleration of ion beam at said step of ion beam spatial confinement.

Optionally, said drift space of said multi-pass analyzer may be set at ground and wherein electrodes of said orthogonal accelerator may be energized by pulsed voltages to extract said ion packets.

Optionally, the ratio L_z/A_z of said of ion packet length and of an ion advance per single pass (reflection or turn) may be one of the group: (i) $0.5 < L_z/A_z \leq 1$; (ii) $1 < L_z/A_z \leq 2$; (iii) $2 < L_z/A_z \leq 5$; (iv) $5 < L_z/A_z \leq 10$; (v) $10 < L_z/A_z \leq 20$; and (vi) $20 < L_z/A_z \leq 50$.

According to another aspect of the invention, there is provided a multi-pass MPTOF (multi-reflecting or multi-turn) time-of-flight mass spectrometer comprising:

- (a) an ion source, generating an ion beam;
- (b) a radio-frequency ion trap converter, substantially elongated in the first Z-direction and ejecting ion packets substantially along the second orthogonal X-direction;
- (c) means for steering and focusing of ion packets within or immediately past said trap converter;
- (d) an electrostatic multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), built of parallel ion mirrors or electrostatic sectors, separated by a drift space and substantially elongated in the Z-direction to form an electrostatic field in an orthogonal XY-plane; said two-dimensional field provides for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion within an isochronous mean ion trajectory s-surface – either symmetry s-XY plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of said pulsed converter and of said z-focusing means; and
- (e) wherein electrodes of said trap converter comprise slits, transparent for return ion passage after at least one reflection or turn.

Optionally, said pulsed converter may be tilted to the Z-axis for angle $\alpha/2$ and said means for Z-spatial focusing comprise means for ion ray steering, so that steering of ion trajectories at inclination angle α within said analyzer may be arranged isochronously.

BRIEF DESCRIPTION OF DRAWINGS

Various embodiments will now be described, by way of example only, and with reference to the accompanying drawings in which:

Fig.1 shows prior art US6717132 planar multi-reflecting TOF with gridless orthogonal pulsed accelerator OA, illustrating geometrical limits on the OA duty cycle;

Fig.2 shows prior art US7504620 planar multi-turn TOF with OA; both analyzer geometry and laminated sectors do limit the ion packet width and the OA duty cycle;

Fig.3 shows an OA-MRTOF embodiment of the present invention, improving the duty cycle of an elongated OA by ion beam confinement, spatial z-focusing of ion packets and by making the OA transparent to reflected ions;

Fig.4 shows a schematic of the electronic for pulsed ion acceleration and an example of a low capacitance OA built using ceramic printed circuit boards;

Fig.5 shows an OA-MTTOF embodiment of the present invention, improving the duty cycle of an orthogonal pulsed converter;

Fig.6 illustrates various methods of ion beam spatial confinement within the storage gap of the elongated orthogonal accelerator;

Fig.7 illustrates an embodiment of ion packet spatial focusing in the z-direction; and

Fig.8 shows an MRTOF embodiment of the present invention with an RF ion trap OA, improving space charge capacity of the trap by substantial trap elongation, followed by ion packets spatial focusing towards the detector.

DETAILED DESCRIPTION

Fig.1, shows a multi-reflecting TOF with an orthogonal accelerator (OA-MRTOF) according to US6717132. The MRTOF comprises: an ion source with a lens system to form a substantially parallel ion beam 13; an orthogonal accelerator (OA) with a storage gap 14 to admit the ion beam 13; a pair of gridless ion mirrors 18 separated by a field-free drift region, and a detector 19. Both the OA 15 and mirrors 18 are formed with plate electrodes having slit openings, oriented in the Z-direction, thus forming a two dimensional electrostatic field, characterized by symmetry about the XZ-symmetry plane, denoted as s-XZ. All of the storage gap 14, the plates of the OA 15, the ion mirrors 18 and the detector 19 are aligned parallel to the drift axis Z.

In operation, ion source 11 generates ions having a range of specific masses $\mu=m/z$. Gaseous ion sources (like ESI, APCI, APPI, gaseous MALDI or ICP) comprise gas-filled radio-frequency (RF) ion guides (not shown) for dampening of the ion beams, followed by a lens 12 to form a substantially parallel continuous ion beam 13. Typical ion beam parameters are: 1mm diameter, 1 degree angular divergence at a specific ion energy (energy per charge) U_Z of from 10 to 50V at typical axial energy spread of 1eV.

The beam 13 propagates in the Z-direction through storage gap 14, which is a field-free region between plate electrodes. Periodically, an electrical pulse is applied between the plates defining the storage gap 14. A portion of the continuous ion beam 13, in the storage gap 14, is accelerated in the X-direction by a pulsed field and is accelerated to specific energy U_X , thus forming a ribbon-shaped ion packet 16 travelling along the mean ion trajectory 17. Since the ion packets preserve the z-velocity of the continuous ion beam 13, the trajectories 17 are inclined at an angle α to the X-dimension, typically being several degrees, where:

$$\alpha = (U_Z/U_X)^{0.5} \quad (eq.1)$$

Ion packets 16 are reflected by ion mirrors 18 in the X-direction, and continue to slowly drift in the Z-direction, and arrive on detector 19 after multiple N ion mirror reflections during a jigsaw shaped ion trajectory 17. To obtain higher resolving power, MRTOF analyzers are designed for longer flight paths and for larger numbers of reflections $N \gg 1$ (e.g. $N=10$). To avoid spectral overlaps on the detector 19 (i.e. confusion between various numbers of reflections), the useful length of each ion packet L_Z becomes limited to:

$$L_Z < D_Z/N \quad (eq.2)$$

where D_Z is the distance in the Z-dimension from the most upstream point of the OA 15 that ions are ejected from to the mid-point of the detector 19 at which ions are detected.

For the realistic values of $D_Z = 300\text{mm}$ and $N=10$, the ion packet length L_Z is therefore under 30mm. In practice, the packet length is actually about twice as small, accounting for the OA and detector rims. This in turn limits the conversion efficiency of continuous ion beam 13 into pulsed packets 16, denoted as the duty cycle DC of the orthogonal accelerator 15:

$$DC = \sqrt{\mu/\mu^*} L_Z/D_Z, < \sqrt{\mu/\mu^*}/2N \quad (eq.3)$$

Here $\mu = m/z$ denotes the specific mass, i.e. mass to charge ratio, and μ^* defines the heaviest specific mass in the beam 13. Assuming $N=10$ and the smallest $\mu/\mu^* = 0.01$, the duty cycle for heaviest ions is under 10% and for the lightest ions in the beam is under 1% (and realistically under 0.5%). Thus, the OA-MRTOF instrument has a low duty cycle.

The duty cycle limit occurs due to the ion trajectory arrangement within the s-XZ symmetry plane of mirrors 18 and OA 15. The alignment of the ion trajectory within the s-XZ plane is forced to keep the isochronous properties of the ion mirrors and gridless OA, reaching up to third order full isochronicity as described in WO2014142897. The prior art MRTOF 10 has been designed with recognition of the symmetry requirements. The duty cycle is sacrificed in exchange for higher resolving power of OA-MRTOF.

Fig.2 shows a multi-turn TOF analyzer having an orthogonal accelerator (OA-MTTOF) 20 according to US7504620. The MTTOF 20 comprises: an ion source 11 with a lens system 12 to form a substantially parallel ion beam 13; an orthogonal accelerator (OA) 15 with a storage gap 14 to admit the beam 13; four laminated electrostatic sectors 28, separated by field-free drift regions, and a TOF detector 19.

Similarly to the instrument in Fig. 1, the OA 15 in Fig. 2 admits a slow (say, 10eV) ion beam 13 and periodically ejects ion packets 26 along the ion trajectory 27. Electrostatic sectors 28 are arranged isochronously for a spiral ion trajectory 27 with a figure-of-eight shaped ion trajectory in the XY-plane and with a slow advancing in the drift Z-direction due to the fixed inclination angle α at which the sectors 28 are arranged. The energy of ion beam 13 and the OA acceleration voltage are arranged to match the inclination angle α of the laminated sectors.

The laminated sectors 28 provide three dimensional electrostatic fields for ion packet confinement in the drift Z-direction along the mean spiral trajectory 27. The fields of the four electrostatic sectors 28 also provide for isochronous ion oscillations along the figure-of-eight shaped central curved ion trajectory 27 in the XY-plane, also denoted as s . These sector analyzers are known to provide so-called triple focusing, i.e. first-order focusing with respect to energy spread around a mean ion energy and with respect to

angular and spatial spread of ion packets around the mean ion trajectory. The sector MTTOF isochronicity has been recently improved with electrostatic sectors of non-equal radii, as described in WO2017042665.

The ion trajectory in the MTTOF 20 is locked to the fixed spiral trajectory 27 (s), which forces the sequential arrangement of the OA 15, sectors 28 and of the detector 19, thus limiting the duty cycle of the OA to being under $1/N$, where N is the number of full turns. In addition, to arrange the spatial ion confinement within laminated sectors 28 in the Z-direction, the length L_Z of ion packets 26 in the Z-dimension shall be at least twice as small as the width in the Z-dimension of each laminated channel in the sectors, and hence, the duty cycle of the MTTOF 20 is limited as described by *eq.3* above. Embodiments of the present invention provide a method and apparatus for improving the duty cycle of orthogonal accelerators (OA) for multi-pass MPTOF analysers, i.e. for both multi-reflecting OA-MRTOF and multi-turn OA-MTTOF analysers.

Fig.3 shows an embodiment of an OA-MRTOF instrument 40 according to the present invention, in both the XZ plane (40-XZ) and the XY plane (40-XY). The instrument 40 comprises: a continuous ion source 11; a lens system 12 to form a continuous and substantially parallel ion beam 13; an orthogonal accelerator 30, composed of electrodes with elongated slits 31 (elongated in the Z-dimension) the OA 30 having means for ion beam spatial confinement 32 (detailed in **Fig.6**) and an isochronous Z-focusing lens 33 which is exemplified here by a trans-axial lens formed within electrodes 31; two opposite and parallel gridless ion mirrors 41 and 42 that are separated by a grounded field-free drift space 43; and a TOF ion detector 45. The electrodes of the OA 30 and ion mirrors 41 and 42 are substantially elongated in the drift Z-direction to provide a two-dimensional electrostatic field in the X-Y plane, that is symmetric around the s-XZ symmetry plane of isochronous trajectory surface and which has a zero field component in the Z-direction.

Contrary to the prior art, the electrodes 31 of the OA 30 are made transparent for the ions being reflected back from an ion mirror 41,42. The accelerating field of the OA 30 is pulsed during ion extraction from the OA and is switched off afterwards, so that the ions reflected by the mirrors and returning through the OA are not defocussed.

In operation, a continuous or quasi-continuous ion source 11 generates ions. A substantially parallel ion beam 13 passes through ion optics 12 and enters OA 30 substantially along the Z-direction. Optionally, the beam may be spatially confined in at least the X-direction (optionally also the Y-direction) with confinement means 32 within the z-elongated storage gap of OA 30. An L_Z long portion of continuous beam 13 is converted into a pulsed ion packet 35 by an orthogonal pulsed acceleration field of OA 30, energized by pulse generator 34. Ejected ion packets 35 move at some inclination angle α to the X-direction, which is controlled by the U_Z specific energy of the incoming ion beam 13 and acceleration voltage U_X gained at pulsed acceleration in the OA (see *eq.1* above). Each ion packet 35 is reflected between ion mirrors 41 and 42 in the X-direction within the s-XZ symmetry plane for a large number of reflections (say, $N =$ between 6 and 20) and while drifting in the Z-direction towards the detector 44 because the ions retain the K_Z component of ion energy from the ion source 11.

Similarly to **Fig.1**, the embodiment 40 employs two-dimensional Z-extended MR-TOF mirrors and an OA oriented in the Z-direction. Distinctly from **Fig.1**, the duty cycle of the MRTOF 40 according to the embodiment shown is improved by the combination of the following features:

(A) To improve the duty cycle of the OA 30, the length L_Z of the ion packets 35 ejected from the OA 30 may be made longer than half the distance in the Z-direction that the ion packet advances per single mirror reflection $2L_Z > A_Z = D_Z/N$. The distance A_Z in the

z-direction may be determined along the axis that is half-way (in the x-direction) between the mirrors, and based on the positions of the centre (in the z-direction) of the ion packet. Ultimately, the L_z length may be comparable to a notable portion (say, 1/2) of the total drift length D_z (e.g. where D_z is the distance in the Z-dimension from the most upstream point of the OA 30 that ions are ejected from to the mid-point of the detector 44 at which ions are detected), even if using a large number of mirror reflections. Optionally, the ratio L_z/A_z may be one of the group: (i) $0.5 < L_z/A_z \leq 1$; (ii) $1 < L_z/A_z \leq 2$; (iii) $2 < L_z/A_z \leq 5$; (iv) $5 < L_z/A_z \leq 10$; (v) $10 < L_z/A_z \leq 20$; and (vi) $20 < L_z/A_z \leq 50$.

(B) Means 32 may be arranged for spatial confinement of the ion beam so as to prevent the natural expansion of ion beam 13 within the OA 30 and to allow substantial (potentially indefinite) elongation of the OA without ionic losses and without ion beam spread, as detailed below in Fig.6.

(C) To avoid ion losses on the detector 44, so as to avoid spectral overlaps and spectral confusion (contrary to prior art open traps, described in WO2011107836), the ion packets 35 may be spatially focused in the Z-direction by a trans-axial lens 33 that may be within the OA 30 (or immediately downstream of the OA), or by a Fresnel lens, or by spatial space-velocity correlation of the continuous ion beam 13 within the OA, e.g. as described in co-pending application WO2019/030475. The trans-axial lens 33 may comprise focusing electrodes configured to generate an electric field region through which ions travel in use that has equipotential field lines that curve and/or diverge as a function of position along the drift Z-direction so as to focus ions in the drift Z-direction. As the result of ion packet z-focusing, the inclination angle α of ion trajectories with respect to the x-direction become dependent on z-position, as illustrated by ion packet vectors 36 having inclination angles α_1 and α_2 . The spatial focusing (in the z-direction) leads to ion packet confinement towards the detector 44. The Z-focusing may be arranged isochronous, i.e. with compensation of T/Z and T/ZZ time aberrations per Z-width of ion packets, which otherwise would occur if using a conventional Einzel lens.

(D) The ion mirrors 41,42 return the long ion packets 35 towards the OA 30, as shown by trajectories A' and B'. To avoid interferences of ion rays A' and B' with the long OA 30, OA electrodes 31 are made transparent to the reflected ions, say, with elongated slits. In other words, the mass analyser is configured such that the ions pass back through the OA30 between exiting one mirror and entering the other ion mirror (for at least some of the passes between the ion mirrors), and without the ions hitting the electrodes 31 of the OA 30. Although not shown in Fig. 3, it is contemplated that the ions may pass through the OA when travelling from the final mirror reflection to the detector 44. In order to prevent the ions hitting the OA 30, the OA electrodes 31 may comprise slits through which the ions pass as they travel between the mirrors 41,42. Each electrode 31 may comprise a single slit through which the ions pass, and that is elongated in the Z-direction. The slits (and therefore the OA electrodes) may each extend for the entire Z-width of the ion trajectories within the MRTOF analyzer. The slits may extend from the most upstream point of the OA 30 that ions are ejected from (or from further upstream) to a point in the z-direction that is proximate the position of the detector 44 (in the z-direction) such that ions do not hit the electrodes 31 when passing through the OA 30. The slits may extend to a location in the z-direction that is adjacent the upstream or downstream edge of the detector 44. The slits may be substantially coincident, in the Z-direction, with the windows of the ion mirrors 41,42. Examples of the slits are well seen in both the XZ and XY views of Fig. 3. Although Fig. 3 shows each slit as being a slotted aperture within an electrode 31 (i.e. each slit is fully surrounded by the electrode), it is contemplated that each slit may be defined between two separate electrode sections that are elongated in the Z-direction (i.e. the slit may not be

bounded at one or both ends in the Z-direction). For the avoidance of doubt, the OA 30 referred to herein is the device that receives ions and pulses them orthogonally towards an ion mirror. The ion mirrors are not part of the OA 30.

To pulse each ion packet out of the OA 30, high voltage (e.g. 3 to 10kV) pulses, produced by high voltage generators such as those built of Behlke switches, are applied to the OA electrodes 31, as shown in Fig. 3, while drift space 43 between the ion mirrors is grounded. Once the ion packet 35 is ejected from the OA 30, the potentials of the OA 30 are returned to ground (optionally except for small potentials on optional ion guide 32) before the ions are reflected back through the OA 30. The ion packets may therefore pass through the slits of the OA electrodes 31 without being defocused by the OA pulses. Each ion packet 35 may be allowed to reach the detector 44 before the next ion packet is pulsed. Alternatively, one or more further ion packets may be pulsed out of the OA before the ions in the preceding ion packet(s) have reached the detector 44. In the latter embodiment, each of these OA pulses may be times such that ions from the previous pulse(s) are not within the OA 30 at the time it is pulsed.

A numerical example for the preferred embodiment 40 is presented below, where the main parameters are as shown in the Table 1 below.

Table 1:

D_X mm	D_Z mm	U_X V	U_Z V	α mrad	A_Z mm	N refl	L m	L_Z mm	DC %
1000	300	10000	10	30	30	10	10	150	50

20

In this example, the distance between the mirror caps of the mirrors in the x-direction is $D_X=1\text{m}$ and $D_Z=300\text{mm}$ (accounting for the useful Z-width of ion mirrors, which is not affected by 3D fringing fields at the Z-edges). The acceleration voltage for acceleration ions in the x-direction into the ion mirror is $U_X=10\text{kV}$. By setting the ion beam specific energy to $U_Z=10\text{V}$, the average inclination angle α is set to $\alpha\sim 30\text{mrad}$ (by *eq.1*), i.e. the ion packet advance A_Z per ion mirror reflection is $A_Z=30\text{mm}$, and the number of ion mirror reflections is $N=D_Z/A_Z=10$ (the approximate total flight path $L=D_X*N=10\text{m}$). If using a conventional OA-MRTOF 10, and accounting for rims of the OA and detector, the ion packet length L_Z shall be limited under $D_Z/2N=15\text{mm}$ and the duty cycle for the heaviest μ mass component would be limited to under $\text{DC}=1/2N=5\%$, as defined by equation (3). With the improvements of the embodiment 40, the ion packet length can be increased, say, to $L_Z=150\text{mm}$, thus improving the OA duty cycle for the heaviest μ to $\text{DC}=50\%$, i.e. by an order of magnitude.

Accounting for *eq.3*, the duty cycle DC of any OA instrument drops for lighter (smaller $\mu=m/z$) ions. As an example, even if the $\text{DC}=50\%$ for an upper mass (say $\mu=2500$), the duty cycle is still limited to $\text{DC}=10\%$ for $\mu=100$ ions. The duty cycle for lighter ions can be further improved if using an ion guide (e.g. RF ion guide) of the ion source 11 (or between the source and OA 30) in a so-called "Pulsar" mode. Ions may be intermittently stored within the ion guide and released therefrom in a pulsed manner that is synchronized with the OA pulses, e.g. by operating an ion gate between the ion guide and OA (as indicated by pulse symbol at the exit aperture of the ion guide) such that the ions stored in the ion guide are pulsed by the OA 30. The propagation time of light ions within the OA (estimated as $50\mu\text{s}$ for $\mu=100$ at $K_Z=10\text{eV}$ and $L_Z=150\text{mm}$) appears smaller than the time delay for extraction of heavy ions from the "Pulsar" RF ion guide, known to be about 20-30 μs for $\mu=1000$ ions. Thus, using long OA 30 allows analysis of wide mass range at enhanced sensitivity.

45

Using a long OA 30 substantially extends the mass range able to be mass analysed to match M/m (i.e. the ratio of the heaviest mass ion to the lightest mass ion) for ions simultaneously transmitted from the RF ion guide, i.e. the Pulsar mode does not limit the mass range. Contrary to Pulsar OA-TOF instruments, the "Pulsar" gain is substantially
 5 higher for OA-MRTOF at substantially longer flight times and flight paths (say, tens and hundreds of meters). Indeed, ions may be stored in the RF ion guide between rare OA pulses, while ion packets ejected from the ion guide may be admitted into the OA with nearly unity duty cycle and a wide mass range.

Referring to **Fig.4**, an exemplary electronics pulse circuitry 34 is shown for
 10 energizing the multiple electrodes 31 and 32 of OA 30. A positive U_A accelerating voltage may be buffered by a large capacitor C_A (e.g. tens of nF), and may be pulse connected to an RC dividing chain via high voltage switch 38. A Behlke switch may be used, e.g. a HTS-61-05 model operating up to 6kV, 50A peak current and may connect a high voltage at a 40ns rise time at capacitive loads up to a few nF. Capacitors C may be in the order of 10-100pF
 15 to reduce the voltage sagging during the pulse. The resistors R may be in the 0.1-1M Ω range to reduce average current to well under 0.5A, accounting for about 1% time duty cycle of pulses at a few μ s pulse duration and 100-300 μ s pulse period. A clean pulse shape depends on stray capacitances and inductances. To reduce electrode capacitance and to provide short and wide connecting leads, OA 39 may be made as a ceramic PCB board with
 20 conductive strips 31, with a resistive coating in between strips, and with small and precise 10pF size capacitors C constructed across the PCB. The combination of circuit 34 and PCB OA 39 is expected to provide clean fractions of pulse amplitude, here shown as 1, 0.75, 0.5 and 0.25 of pulse amplitude. While most OA electrodes are pulsed from ground, electrodes 32 of the OA ion guide may be pulsed from some small (say, -10 to -30V) negative offset.
 25 The offset pulses may be arranged with a separate RC dividing chain.

Fig.5 shows an OA-MTTOF embodiment 50 of the present invention. This is similar to the previously described embodiments, but has sectors for turning the ions rather than mirrors for reflecting the ions. Fig. 5 shows a view 50-XZ in the XZ plane and a view 50-XY in the XY plane. The analyser comprises: a (e.g. continuous) ion source to form a
 30 substantially parallel ion beam 13; a Z-elongated gridless orthogonal accelerator 30 comprising electrodes 31 with elongated slits means 32 for spatial ion confinement, and means for isochronous Z-focusing(exemplified here by a trans-axial lens 33); a set of electrostatic sectors 51 and 52, separated by drift spaces 53; and a TOF detector 54. Each of the sectors 51 and 52 may be substantially extended in the drift Z-direction (i.e. may not use
 35 lamination). This allows the ions to spiral around the device and through any given sector multiple times as the ions drift in the z-direction, as will be described below. Each sector may extend, in the z-direction, at least from the most upstream point of the OA 15 that ions are ejected from to the detector 54. The beam 13 may initially be oriented along the Z-direction.

40 In operation, orthogonal accelerator 30 receives (e.g. continuous) ion beam 13 within a Z-elongated storage gap, wherein means 32 may be provided to confine the ion beam at least in the X-direction (and optionally the y-direction), as detailed in **Fig.6** below. OA 30 accelerates a portion of ion beam 13 by electrical pulses from generator 34 in the X-direction, thus forming ion packets 35 (denoted 55 within the analyzer). Ion packets 35
 45 move at some mean inclination angle α to the x-direction, controlled by the specific energy of the ion beam 13. Trans-axial lens 33 in the OA 30 (or a Fresnel lens, or some other Z-focusing means described below) may be arranged for spatial focusing of ion packets 35 in the Z-direction as they travel towards the detector 54, so that the inclination angle in the MTTOF analyzer becomes dependent on the initial z-position within ion packets. Due to the

z-energy of the continuous ion beam 13, the ion packets 55 follow the spiral ion trajectory shown by rays A-B as they pass around the sectors 51,52 and within the mean trajectory surface S to provide for at least first order full isochronicity, while slowly converging in the Z-direction towards detector 54.

5 Optionally, sectors 51 and 52 have different radii, as described in WO2017042665 to provide for higher order isochronicity. Contrary to the prior art of Fig. 2, the sectors of the MTTOF in embodiment 50 may not have any electrostatic field component in the Z-direction, which would otherwise affect the spiral motion.

10 The stadium shaped ion trajectory s-surface is arranged between electrostatic sectors 51 and 52, separated by grounded field-free regions 53. The sectors XY-field and ion packet energy in the X-direction may be adjusted for isochronous ion packet motion within the trajectory surface S . The inclination angle α is controlled by the ion beam 13 energy and by Z-focusing means 32 only. The drift length D_z and the injection inclination angle α are chosen to allow for multiple (say $N=10$) full ion turns, before ions hit the detector 54.

15 To improve the duty cycle of OA 30, the length L_z of the ion packets 35 may be made comparable (say $1/2$) of the total drift length D_z . At a large number of ion turns (say $N=10$) the ion packet length L_z appears much longer than the ion packet advance A_z per single turn.

20 Similarly to embodiment 40 in Fig. 3, embodiment 50 of Fig. 5 employs similar ion optical methods for: the OA elongation, ion beam confinement within the OA, Z-focusing of ion packets, making long slits in the OA electrodes, and pulsed switching off the OA potentials for return ion packet passage through the OA.

25 It is desired to prevent the ion beam expanding (before being pulsed) in the field free storage gap of the OA. Even with ion beam dampening in an RF ion guide upstream of the OA, the ion beam emittance is still finite (about $1\text{mm} \cdot \text{deg}$ at 10eV), and the ion beam would naturally diverge by several mm within 100mm along OA. This would compromise the combination of time and energy spreads of ion packets, affecting MPTOF resolution.

30 Referring to **Fig.6**, embodiments 61, 63, 65, and 67 present generalized means 32 for the spatial confinement of ion beam 13 within the gridless orthogonal accelerator OA 30. As described above, slit electrodes 31 of the gridless OA 30 are energized by pulse generator 34 to convert the continuous ion beam 13 into pulsed ion packets 35. The embodiments in Fig. 6 differ from each other by the applied electrical signals and by the shape of ion confining electrodes 62, 64, 66, and 68.

35 Embodiment 61 employs a rectilinear RF ion guide similar to US5763878. RF signals are applied to electrodes 62 so as to generate a quadrupolar RF field, radially confining ion beam 13 as it travels in the z-direction along the OA 30. Embodiment 61 has drawbacks: (i) RF confinement is mass dependent; (ii) the RF field must be turned off before the acceleration pulse within microseconds, where an RF signal decay is incomplete; (iii) pulses applied to electrodes are known to excite a resonant generator of the RF signal; 40 and (iv) the initial ion position and initial velocity are mass and RF-phase dependent, which affect resolution, mass accuracy and angular losses in TOF analyzers.

45 Embodiment 63 employs a rectilinear electrostatic quadrupolar lens, formed by applying negative DC potentials to electrodes 64, as proposed in RU2013149761. A weak electrostatic quadrupolar field focuses and confines the ion beam in the critical TOF X-direction, while defocusing the ion beam in the non-critical transverse Y-direction. The method allows lossless ion beam transfer for up to $L_z \leq 50\text{mm}$.

Embodiment 65 employs the spatially alternated electrostatic DC quadrupolar field along the Z-axis by alternating the polarity on DC electrodes 66, as in co-pending application WO2019/030475. The embodiment provides for indefinite ion beam

confinement in both X and Y directions, although a variable central potential along the Z-axis may have a negative effect on ion beam packet focusing in the Z-direction.

Embodiment 67 provides for ion beam spatial confinement by spatial alternation of electrostatic quadrupolar field, now achieved without spatial modulation of the center-line potential $U(z)$. The field is formed by an array of alternating DC dipoles 68, as described in co-pending application WO2019/030475. Optionally, the average potential $(DC1+DC2)/2$ is slightly negative to form a combination of the alternated quadrupolar field with a weak static quadrupolar field, thus providing somewhat stronger compression of the ion beam 13 in the X-direction Vs Y-direction. Relative to RF confinement 61, the electrostatic confinement 67 provides multiple advantages: (i) it is mass independent; (ii) it does not require resonant RF circuits and can be readily switched off; (iii) the strength and shape of the transverse confining field can be readily varied along the guide length; (iv) it can provide axial gradient of the guide potential without constructing complex RF circuits.

Ion packet Z-focusing may be provided as detailed in co-pending application WO2019/030475, such as by the following means:

(A) A trans-axial (TA) lens may be incorporated into the exit lens of a gridless OA (focusing in the Y-direction). For reaching isochronicity, the TA-lens may be compensated by a slight curvature of the accelerating field around the continuous ion beam. Such compensating curvature of the accelerating field may be achieved for example by TA curvature of the next extracting electrode or by an even yet slighter TA-curvature of the first push electrode. The TA-lens and the TA-compensator may be arranged for at least the Z-length of the extracted ion packet and they may be turned off by removing the pulsed OA voltages during the ion packet return passage through the OA. Optionally, the TA-lens may be combined with a TA-wedge for compensating non-intended misalignments of the OA and of the analyzer;

(B) A Fresnel lens, achieved with a multi-segmented deflector, which is energized with a gradient step voltage between thin deflecting plates may be provided. The Fresnel lens also allows arranging wedge fields with a constant bias applied to all deflecting segments, this way serving as a compensator for mechanical misalignments. The Fresnel lens may be arranged at least for the z-length of extracted ion packets and may be switched off together with the OA to allow a non-distorted return ion passage;

(C) Z-focusing may be provided by spatial-temporal correlations within a continuous ion beam, which is described below. Ion packet auto-focusing may be obtained by controlling and correlating the axial velocity V_z of the continuous ion beam with its z-position within the OA. In this case the OA does not need means for spatial Z-focusing 33. Co-pending application WO2019/030475 describes two general methods of Z-auto-focusing, which may be used in embodiments of the present invention, and which are as follows:

(A) To focus (or compress) a range of $\mu=m/z$ ions in the z-direction by the time they reach the detector, the z-directional speed of the ions may be caused to be different as a function of their z-directional position within the OA. Ions arranged within the OA at locations progressively further away from the detector (in the z-direction) may be given progressively higher z-directional speeds towards the detector such that the ion packet is compressed in the z-direction by the time that it reaches the detector. For example, one may arrange a negative correlation $V_z(z)$ within the storage gap of the OA 30 according to $V_z(z)/V_{z0} = 1-z/D_z$, where D_z is the distance from beginning of the OA to the detector, $V_z(z)$ is the axial velocity for depending on ions' z-position within the OA, $V_{z0} = V_z(z=0)$, where $Z=0$ is the beginning (upstream end) of the OA.

(B) To focus (or compress) ions in a wide mass range (e.g. for all μ), the z-dependent specific energy per charge $U(z)$ may be caused to be different as a function of their z-directional position within the instrument. Ions arranged at locations progressively further away from the detector (in the z-direction) may be given progressively higher specific energy per charge $U(z)$ in a direction towards the detector such that the ion packet is compressed in the z-direction by the time that it reaches the detector. For example, the z-dependent specific energy per charge $U(z)$ may satisfy: $U(z)/U_{z0} = (1-z/D_z)^2$, where $U_{z0}=U(z=0)$.

Referring to **Fig.7**, the embodiment 70 comprises the MRTOF 40 of Fig.3 with an orthogonal accelerator 30, but may not have the TA-lens 33; and may have at least one beam correlating feature of the group: (i) an ion source 73 with a time variable acceleration bias $U_z(t)$; (ii) an RF ion guide 74 with a time variable DC acceleration bias and/or with an electrode structure for switching an axial field gradient within the RF ion guide to different values; (iii) an extraction electrode 75, connected to a pulse supply 76; (iv) an extraction electrode 75, connected to a time variable power supply 77; and (v) a supply 78 for arranging a DC gradient within the ion guide 60 of the OA 30. Those beam correlating features are synchronized with pulse generator 34 of the OA 30.

In operation, substantially elongated ion beam 33 may be retained within long OA 30 by spatial confinement means 60, e.g. as described in relation to Fig. 6. Neither the OA nor MRTOF Z-focus the ions, and the orthogonal ion X-motion in the MRTOF (or MTTOF) does not affect the ion Z-motion, which is instead defined by the axial ion velocity within the OA, and hence by correlations $V(z)$ or $U(z)$ within continuous ion beam would control ion packet Z-auto-focusing.

In one embodiment, an acceleration pulse 76 is applied to RF ion guide 74 (for example, a segmented quadrupole, or quadrupole with auxiliary electrodes, or an ion tunnel ion guide), thus forming a pulsed axial Z-field. Alternatively, a negative pulse 76 may be applied to gate 75, to follow a Pulsar method such as that described herein above. The pulse 76 amplitude and the length of axial Z-field within the guide 74 are arranged for time-of-flight compression of ion packets in the z-direction by the time the ions reach the detector 44 plane, located at distance D_z . Ions located at the entrance of the axial acceleration Z-field when it is pulsed on will arrive at the OA 30 at a later time than ions located towards the exit of the axial acceleration Z-field when it is pulsed on. However, the ions that were initially located at the entrance of the axial acceleration Z-field will have a larger speed in the z-direction V_z by the time they enter the OA, as compared to ions that were initially located further from the entrance of the axial acceleration Z-field. This produces ion packet compression or bunching (in the z-direction) at the detector 44. The desired negative $Z-V_z$ correlation occurs for a mass range only, where μ range is controlled by the time delay between pulse 76 and OA pulse 79. This embodiment is attractive for target analysis, where a narrow mass range is selected intentionally, while TOF data may be acquired at maximal OA frequency and dynamic range of the detector.

In another embodiment, the potential of a field-free elevator is controlled by the time variable floating $U(t)$ 77 of either ion guide 74, or of ion optics downstream of the guide 74. The voltage at which the ion guide 74 or ion optics is floated may be varied with time so as to achieve the above described bunching effect (in the z-direction), though the elevator exit may be set closer to the OA entrance and allows a somewhat wider μ range to be accelerated by the OA.

In yet another embodiment, the beam 33 is slowed down within the confinement means 60 by arranging a Z-dependent axial potential distribution $U(z)$ 78, e.g. by a resistive divider connected to electrodes of the confinement means 60 such that different potentials

are applied at different z-locations in the confinement means 60. Then the desired z-focusing of ion packets may be achieved for the entire ionic mass range, i.e. for ions of all μ . This method is particularly attractive when using the RF ion guide in the Pulsar mode, i.e. accumulating and pulse releasing ion packets from the guide 74 in a manner that is synchronized with pulses 79 of the OA.

The OA may be a pulsed converter based on a radiofrequency (RF) ion trap with radial pulsed ejection. The space charge capacity of the trap and of the MRTOF analyzer are then improved by substantial trap elongation.

Fig.8 shows an OA-MRTOF embodiment 90 of the present invention that is similar to that of Fig. 3 except that the OA is a tilted ion trap 80 and the ions are introduced into the OA along a tilted axis. The embodiment 90 comprises: a continuous ion source 11 generating a continuous ion beam 13; a multi-reflecting TOF 40, similar to one in Fig.3, and a radially ejecting (substantially in the X-direction) ion trap 80 constructed of slit electrodes 81, energized by pulsed voltages from a generator 34, and incorporating an ion guide 82 that is energized with a radio-frequency (RF) field for radial ion confinement. The electrodes of ion mirrors 41 and 42 are substantially elongated in the drift Z-direction. Trap 80 is elongated in the z-direction and is tilted to the Z axis by a small angle $\alpha/2$ (say 1-2 degrees). Trap 80 may comprise a trans-axial wedge and lens 83 and a trans-axial lens 84 for ion z-focusing and for adjusting the ion steering of the mean ion trajectory by an average angle of $\alpha/2$. Trap 80 is made of electrodes with slits, so it is transparent for ions at their return passage, as described above with respect to the OA.

In operation, an ion source 11 generates continuous or quasi-continuous (e.g. time-modulated within RF ion guide of the interface) ion beam 13. Beam 13 enters and get trapped within ion guide 82 by a radial confining RF field and by using electrostatic blocking potentials at one or both z-directional ends of the ion guide 82, for example, produced by a DC or pulsed bias of a segment of the ion guide 82. Ions may be trapped as a ribbon, optionally dampened with a pulsed gas admission. At the ion ejection stage, an ion ribbon is accelerated by pulsed application of voltages by the generator 34 and the ions are urged orthogonally to electrodes 81 so as to travel at an inclination angle $\alpha/2$ relative to the X-axis. To correct for the tilt of the ion packet time front relative to the ion mirrors (that occurs due to the axis of the ion trap being tilted relative to the z-direction), a wedge shaped field of TA-lens 84 steers ions forward for another $\alpha/2$ angle, so that ion packets 85 are parallel to the Z-direction. The wedge 84 may also have a lens component for ion packet z-focusing, whose time aberrations may be compensated for by a weaker TA-wedge 83.

After pulsed ejection and steering in the wedge field 84, ion packets 85 are aligned parallel to the Z-axis and move at an inclination angle α to the z-direction. On their way back, i.e. after the first ion mirror reflection, the ions pass through the slits of the switched off trap 80. Spatially focused (in the z-direction by lens 84) ion packets eventually reach the detector 44 after multiple mirror reflections, thus, improving MRTOF (or MTTOF in embodiments using sectors rather than mirrors) resolution.

Compared to the embodiment of the OA 30 in Fig. 3, trap 80 is capable of nearly 100% duty cycle within a wide mass range, but on the other hand may introduce several parasitic effects, such as RF phase and mass dependent parameters of ion packets, oscillations of trapping RF voltage induced by pulse pick up, and larger time and energy spreads of ion packets relative to the OA-MRT in Fig.3. Substantial elongation of the novel (transparent) trap converter notably improves space charge capacity of the trap and of the MPTOF analyzer.

Although the present invention has been describing with reference to preferred embodiments, it will be apparent to those skilled in the art that various modifications in

form and detail may be made without departing from the scope of the present invention as set forth in the accompanying claims.

5 For example, although embodiments have been described in which the mass analyser is an MRTOF or a MTTOF, it is contemplated that the mass analyser may instead only have a single ion mirror or sector that reflects or turns the ions, respectively, onto the detector.

10 Although the OA electrodes in the specific embodiments have been described as being transparent to the ions by providing them with slits, it is contemplated that the electrodes may instead be provided as mesh electrodes or with mesh portions through which the ions pass.

15 In the depicted embodiments, the OA electrodes and their slits extend in the drift direction (z-direction) from an upstream end of the orthogonal accelerator to a point proximate or downstream of the detector. However, it is contemplated herein that the OA electrodes and their slits (or meshes) may not extend, in the drift direction (z-direction), all of the way to the detector. Rather, there may be a gap, in the drift direction (z-direction), between the downstream end of the OA electrodes and the detector. In such embodiments, it is preferred that each slit is defined between separate elongated electrode portions (separated in the y-direction) rather than a slot in an electrode.

20

14285902v2

CLAIMS:

5

1. A time-of-flight mass analyser comprising:
at least one ion mirror or electrostatic sector for reflecting or turning ions,
respectively;

10

an orthogonal accelerator having electrodes for receiving ions and orthogonally
pulsing packets of the ions into the ion mirror or electrostatic sector such that the ions are
reflected or turned, respectively, in a first dimension (x-direction) as they drift in a drift
direction (z-direction); and

15

an ion detector;

wherein the electrodes of the orthogonal accelerator define slits or comprise meshes
for allowing ions that have been reflected by the ion mirror, or turned by the electrostatic
sector, to pass back into and through the orthogonal accelerator as they travel towards the
detector.

20

2. The mass analyser of claim 1, wherein either:

(i) the mass analyser is a multi-reflecting time-of-flight mass analyser having the
orthogonal accelerator arranged between two ion mirrors, and arranged and configured so
that the ions are reflected multiple times between the ion mirrors and pass through the
orthogonal accelerator, via the slits or meshes, multiple times as the ions travel from the
orthogonal accelerator to the detector; or

25

(ii) wherein the mass analyser is a multi-turn time-of-flight mass analyser having the
orthogonal accelerator arranged between electrostatic sectors of a plurality of electrostatic
sectors that turn the ions a plurality of times such that the ions pass through the orthogonal
accelerator multiple times, via the slits or meshes, as they travel from the orthogonal
accelerator to the detector.

30

3. The mass analyser of claim 1 or 2, wherein the electrodes of the orthogonal
accelerator and their slits or meshes extend in the drift direction (z-direction) from an
upstream end of the orthogonal accelerator to a point proximate or downstream of the
detector.

35

4. The mass analyser of claim 1, 2 or 3, wherein the electrodes of the orthogonal
accelerator define said slits; and wherein at least one slit, or each slit, is provided as an
aperture through an electrode of the orthogonal accelerator that is elongated in the drift
direction, such that electrode material completely surrounds the perimeter of the slit; and/or

40

wherein at least one slit, or each slit, is defined between electrode portions that are
elongated in the drift direction and spaced apart in a direction perpendicular to the first
dimension and drift direction.

45

5. The mass analyser of claim 1 or 2, wherein the downstream ends of the orthogonal
accelerator electrodes are spaced apart from the detector, in the drift direction (z-direction);
wherein the electrodes of the orthogonal accelerator define said slits; and wherein each slit
is defined between elongated electrode portions that are not joined together at their
downstream ends.

6. The mass analyser of any preceding claim, comprising: one or more voltage supply for applying one or more voltage pulse to the electrodes of the orthogonal accelerator for performing said step of orthogonally pulsing the packets of the ions; and control circuitry configured to control the one or more voltage supply so as to only apply said one or more
5 voltage pulse to the electrodes for orthogonally pulsing a packet of ions out of the orthogonal accelerator when ions that have previously been pulsed out of the orthogonal accelerator are not passing back through the orthogonal accelerator.
7. The mass analyser of any preceding claim, wherein the orthogonal accelerator
10 comprises an ion guide portion having electrodes arranged to receive ions, and one or more voltage supply configured to apply potentials to these electrodes for confining ions in at least one dimension (X- or Y-dimension) orthogonal to the drift direction.
8. The mass analyser of any preceding claim, wherein the orthogonal accelerator
15 comprises: an ion guide portion having electrodes arranged to receive ions travelling along a first axis (Z-direction), including a plurality of DC electrodes spaced along the first axis; and DC voltage supplies configured to apply different DC potentials to different ones of said DC electrodes such that when ions travel through the ion guide portion along the first axis they experience an ion confining force, generated by the DC potentials, in at least one
20 dimension (X- or Y-dimension) orthogonal to the first axis.
9. The mass analyser of any preceding claim, comprising focusing electrodes that are arranged and configured to control the motion of ions along the drift direction (z-direction) so as to spatially focus or compress each of the ion packets so that it is smaller, in the drift
25 direction, at the detector than when pulsed out of the orthogonal accelerator.
10. The mass analyser of claim 9, wherein the focusing electrodes are configured to impart ions located at different positions, in the drift direction, within the ion packet with different velocities in the drift direction so as to perform the spatial focusing or
30 compression.
11. The mass analyser of claim 9 or 10, wherein the focusing electrodes comprise a plurality of electrodes configured to generate an electric field region through which ions travel in use that has equipotential field lines that curve and/or diverge as a function of
35 position along the drift direction so as to focus ions in the drift direction.
12. The mass analyser of any one of claims 9-11, wherein the focusing electrodes comprise a plurality of electrodes configured to control the velocities of the ions such that ions within the orthogonal accelerator when it is pulsed have velocities, in the drift
40 direction, that decrease as a function of distance in the drift direction towards the detector.
13. The mass analyser of claim 12, wherein the plurality of electrodes comprise an ion guide or ion trap upstream of the orthogonal accelerator and one or more electrodes configured to pulse ions out of the ion guide or ion trap such that the ions arrive at the
45 orthogonal accelerator at different times and with velocities in the drift direction that increase as a function of the time at which they arrive at the orthogonal accelerator.
14. The mass analyser of claim 13, comprising circuitry that synchronises the pulsing of ions out of the ion guide or ion trap with the pulsing of ion packets out of the orthogonal

accelerator, wherein the circuitry is configured to provide a time delay between the pulsing of ions out of the ion guide or ion trap and the pulsing of ion packets out of the orthogonal accelerator, wherein the time delay is set based on a predetermined range of mass to charge ratios of interest to be mass analysed.

5

15. The mass analyser of claim 12, 13 or 14, wherein the plurality of electrodes comprise electrodes arranged within the orthogonal accelerator to generate an axial potential distribution along the drift direction that slows ions by different amounts depending on their location, in the drift direction, within the orthogonal accelerator.

10

16. The mass analyser of any preceding claim, configured such that the length of the orthogonal accelerator from which ions are pulsed (L_z) is longer, in the drift direction, than half of the distance (A_z) that the ion packet advances for each mirror reflection or sector turn in the first dimension.

15

17. The mass analyser of claim 16, wherein the ratio L_z/A_z is selected from the group of: (i) $0.5 < L_z/A_z < 1$; (ii) $1 < L_z/A_z < 2$; (iii) $2 < L_z/A_z < 5$; (iv) $5 < L_z/A_z < 10$; (v) $10 < L_z/A_z < 20$; and (vi) $20 < L_z/A_z < 50$; or

20

wherein the length of the region of the orthogonal accelerator from which ions are pulsed (L_z) is longer, in the drift direction, than $x\%$ of the distance, in the drift direction, between the entrance to the orthogonal accelerator and the midpoint of the detector, wherein x is: ≥ 10 , ≥ 15 , ≥ 20 , ≥ 25 , ≥ 30 , ≥ 35 , ≥ 40 , ≥ 45 , or ≥ 50 .

25

18. A mass spectrometer comprising:
an ion source; and
a mass analyser as claimed in any preceding claim.

30

19. A method of mass spectrometry comprising:
providing a mass analyser as claimed in any one of claims 1-17;
receiving ions in said orthogonal accelerator;
pulsing ions from said orthogonal accelerator into said ion mirror or sector;
reflecting or turning the ions with the ion mirror or electrostatic sector, respectively,
so that the ions pass back into and through the orthogonal accelerator via the slits defined by the electrodes or the meshes in the orthogonal accelerator; and
receiving ions at said detector.

35

20. A multi-pass time-of-flight mass spectrometer comprising:
(a) an ion source, generating an ion beam along a first drift Z-direction;
(b) an orthogonal accelerator with spatial confinement means and with electrodes connected to pulsed supplies for admitting said ion beam into a storage gap, for retaining ion beam within said confinement means and for pulsed accelerating a portion of said ion beam in the second orthogonal X-direction, thus forming ion packets;
(c) isochronous means for ion packet focusing in said Z-direction towards a detector, arranged either within or immediately after said orthogonal accelerator;
(d) an electrostatic multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), built of parallel ion mirrors or electrostatic sectors, separated by a drift space and substantially elongated in the Z-direction to form an electrostatic field in an orthogonal XY-plane; said two-dimensional field provides for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion

40

45

within an isochronous mean ion trajectory s-surface – either symmetry s-XY plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of said accelerator and of said z-focusing means; and
 5 (e) wherein electrodes of said orthogonal accelerator comprise slits, transparent for return ion passage after at least one reflection or turn.

21. The spectrometer as in claim 20, wherein said means for ion beam spatial confinement comprise at least one mean of the group: (i) side plates connected to radiofrequency (RF) signal; (ii) side plates connected to an attracting DC potential; (iii) segmented side plates
 10 connected to spatially alternated DC potentials; (iv) segmented DC dipoles connected to spatially alternated dipolar DC potentials.

22. The spectrometer as in claims 20 or 21, wherein said isochronous means for ion packet focusing in the Z-direction comprise at least one means of the group: (i) a set of trans-axial
 15 lens and wedges; (ii) a Fresnel lens and wedge arranged in multi-segmented deflector; and (iii) means for spatial or temporal variations of ion beam energy within said storage gap for arranging negative correlation between ion energy and position in Z-direction.

23. The spectrometer as in claim 22, wherein said ion spatial-temporal correlation is arranged with at least one means of the group: (i) pulsed acceleration of continuous ion
 20 beam in the Z-direction either within electrostatic channel or within a radio frequency RF ion guide, located upstream of said orthogonal accelerator; (ii) a time-variable floated elevator within an electrostatic channel or an RF ion guide, located upstream of said pulsed converter; (iii) a Z-dependent deceleration of ion beam within said orthogonal accelerator.

24. The spectrometer as in claims 20 to 23, wherein said drift space of said multi-pass analyzer is set at ground and wherein electrodes of said orthogonal accelerator are energized
 25 by pulsed voltages to extract said ion packets.

30 25. A method of time-of-flight mass spectrometry comprising the following steps:
 (a) generating an ion beam along a first drift Z-direction in an ion source;
 (b) admitting said ion beam into a storage gap of an orthogonal accelerator, spatially confining said ion beam within said storage gap, and pulsed accelerating a portion of
 35 said ion beam in the second orthogonal X-direction, thus forming ion packets;
 (c) ion packet focusing in said Z-direction towards a detector, arranged at or immediately after said orthogonal accelerator step;
 (d) in an orthogonal XY-plane, arranging two dimensional electrostatic fields of multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), substantially
 40 elongated in the Z-direction; said two-dimensional fields provide for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion within an isochronous mean ion trajectory s-surface – either symmetry s-XY plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of electric fields at said acceleration and said z-focusing steps; and
 45 (e) Wherein said fields of orthogonal accelerator are arranged with transparent electrodes for non destructing and non defocusing return ion passage after at least one reflection or turn.

26. The method as in claim 25, wherein said step of ion beam spatial confinement comprise at least one step of the group: (i) radial ion confinement by radiofrequency (RF) quadrupolar field; (ii) ion confinement in the X-direction by quadrupolar DC field; (iii) radial ion confinement within periodic DC field of annular ion guide; and (iv) radial ion confinement within quadrupolar and spatially periodic DC field.
27. The method as in claims 25 or 26, wherein said step of isochronous ion packet focusing in the Z-direction comprise at least one step of the group: (i) ion focusing in electrostatic field of trans-axial lens and wedges; (ii) ion focusing by a Fresnel lens and wedge arranged in multi-segmented deflector; and (iii) arranging negative correlation between energy and position in Z-direction.
28. The spectrometer as in claim 27, wherein said spatial-temporal correlation is arranged with at least one step of the group: (i) pulsed acceleration of continuous ion beam in the Z-direction either within electrostatic channel or within a radio frequency RF ion guide, located upstream of said orthogonal accelerator; (ii) a time-variable floating of an elevator within an electrostatic channel or an RF ion guide, located upstream of said pulsed converter; and (iii) a Z-dependent deceleration of ion beam at said step of ion beam spatial confinement.
29. The spectrometer as in claims 25 to 28, wherein said drift space of said multi-pass analyzer is set at ground and wherein electrodes of said orthogonal accelerator are energized by pulsed voltages to extract said ion packets.
30. The method as in claims 25-29, wherein the ratio L_z/A_z of said of ion packet length and of an ion advance per single pass (reflection or turn) is one of the group: (i) $0.5 < L_z/A_z \leq 1$; (ii) $1 < L_z/A_z \leq 2$; (iii) $2 < L_z/A_z \leq 5$; (iv) $5 < L_z/A_z \leq 10$; (v) $10 < L_z/A_z \leq 20$; and (vi) $20 < L_z/A_z \leq 50$.
31. A multi-pass MPTOF (multi-reflecting or multi-turn) time-of-flight mass spectrometer comprising:
- (a) an ion source, generating an ion beam;
 - (b) a radio-frequency ion trap converter, substantially elongated in the first Z-direction and ejecting ion packets substantially along the second orthogonal X-direction;
 - (c) means for steering and focusing of ion packets within or immediately past said trap converter;
 - (d) an electrostatic multi-pass (multi-reflecting or multi-turn) time-of-flight mass analyzer (MPTOF), built of parallel ion mirrors or electrostatic sectors, separated by a drift space and substantially elongated in the Z-direction to form an electrostatic field in an orthogonal XY-plane; said two-dimensional field provides for a field-free ion drift in the Z-direction towards a detector, and for an isochronous repetitive multi-pass ion motion within an isochronous mean ion trajectory s-surface – either symmetry s-XY plane of said ion mirrors or curved s-surface of electrostatic sectors; wherein said s-surface is aligned with the symmetry plane of said pulsed converter and of said z-focusing means; and
 - (e) wherein electrodes of said trap converter comprise slits, transparent for return ion passage after at least one reflection or turn.
32. A spectrometer as in claim 31, wherein said pulsed converter is tilted to the Z-axis for angle $\alpha/2$ and said means for Z-spatial focusing comprise means for ion ray steering, so that

steering of ion trajectories at inclination angle α within said analyzer is arranged isochronously.

-1/4-

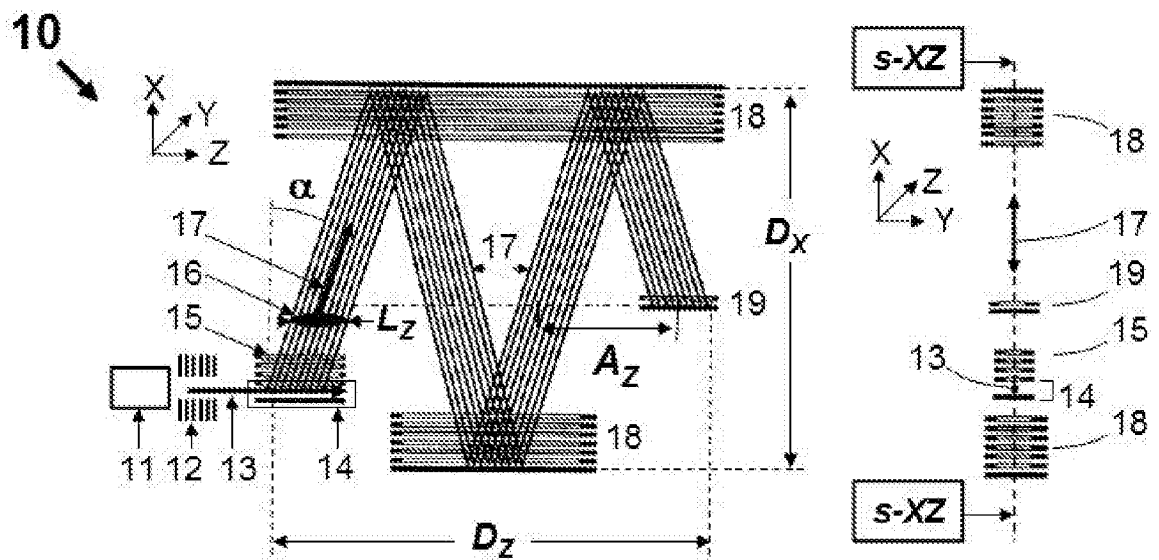


Fig.1 Prior Art

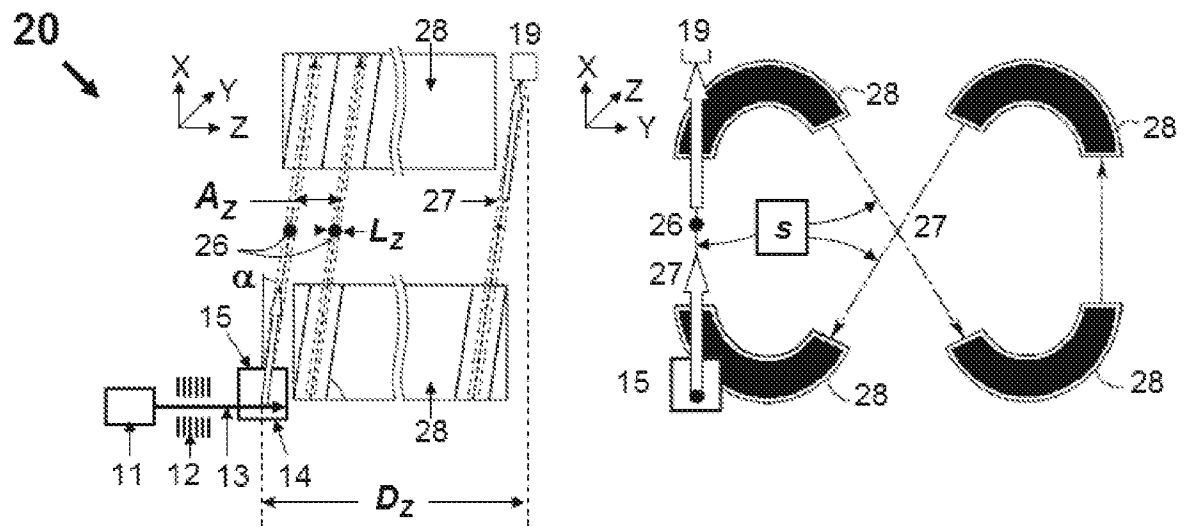


Fig.2 Prior Art

-2/4-

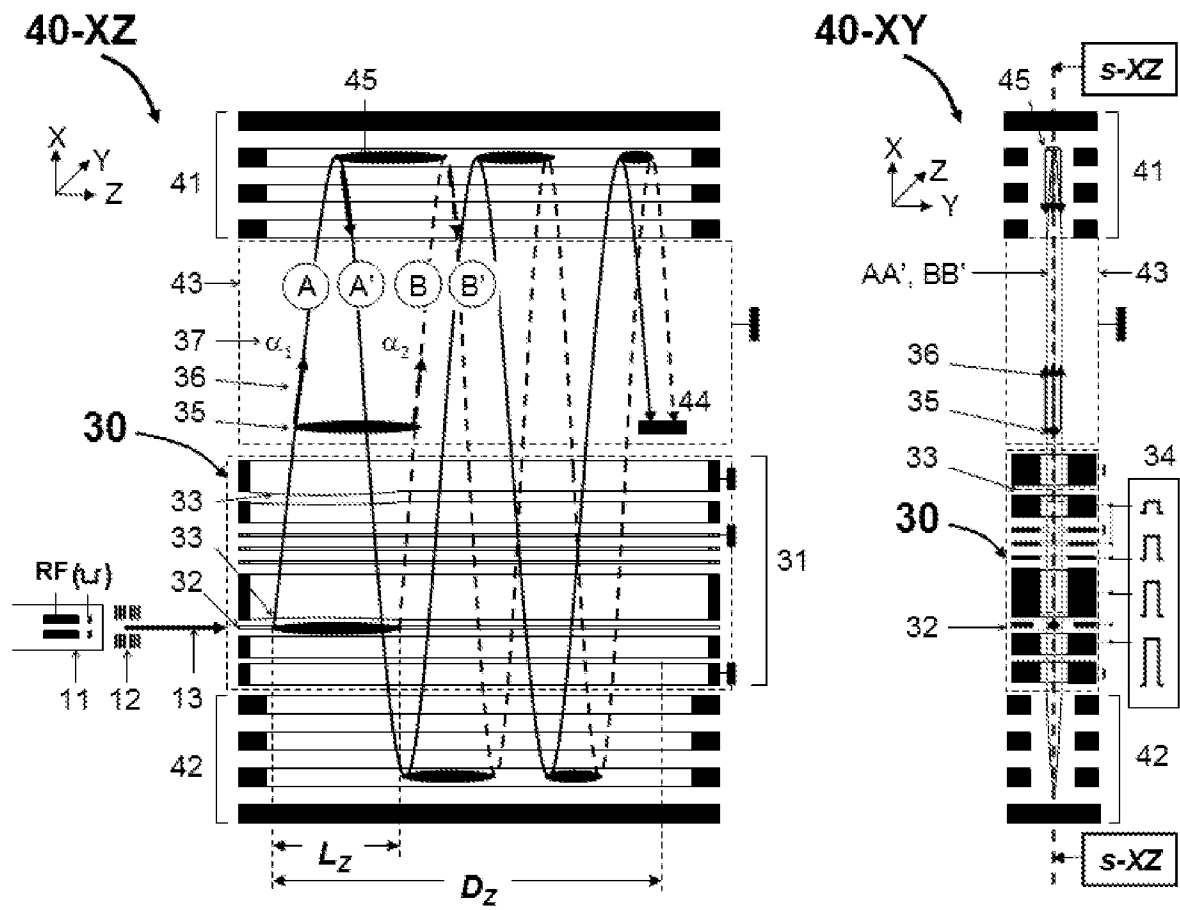


Fig.3

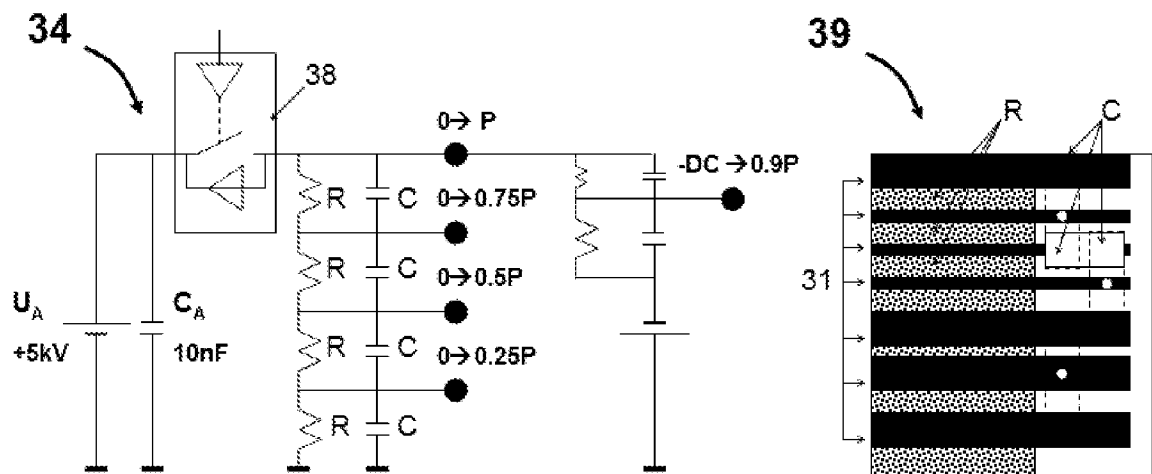


Fig.4

-3/4-

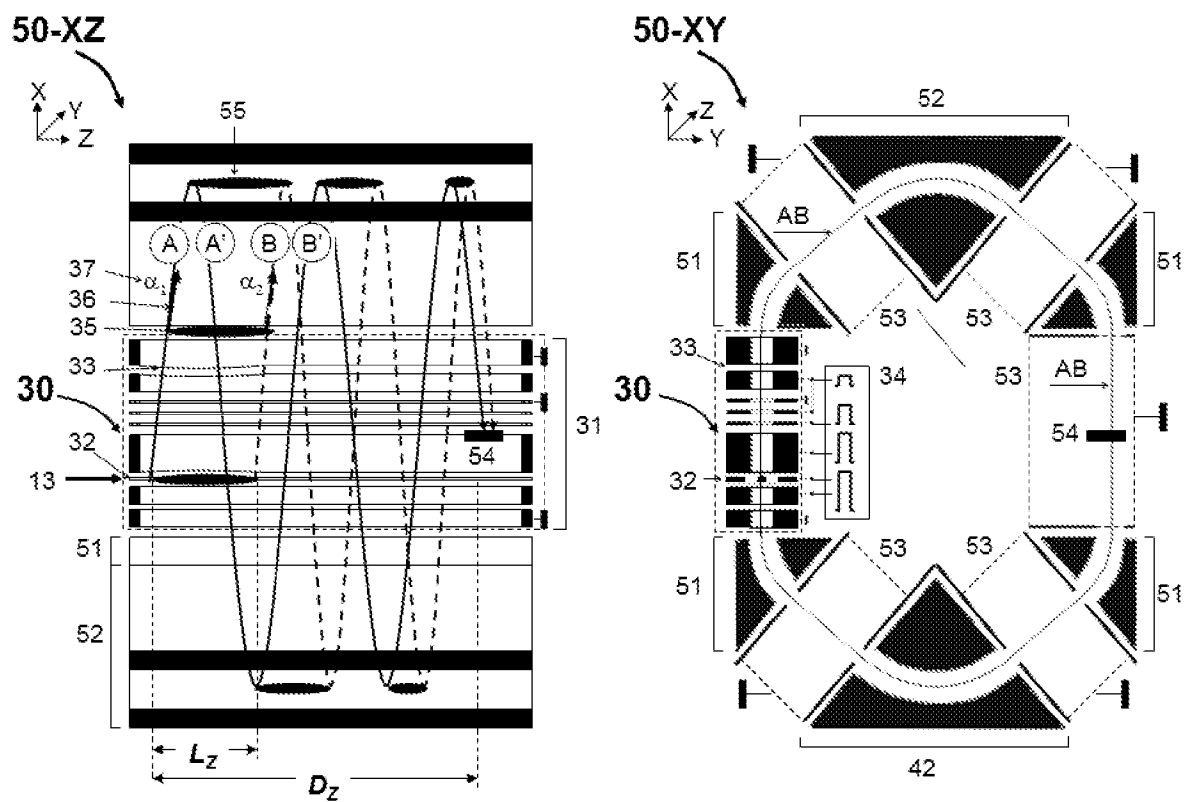


Fig. 5

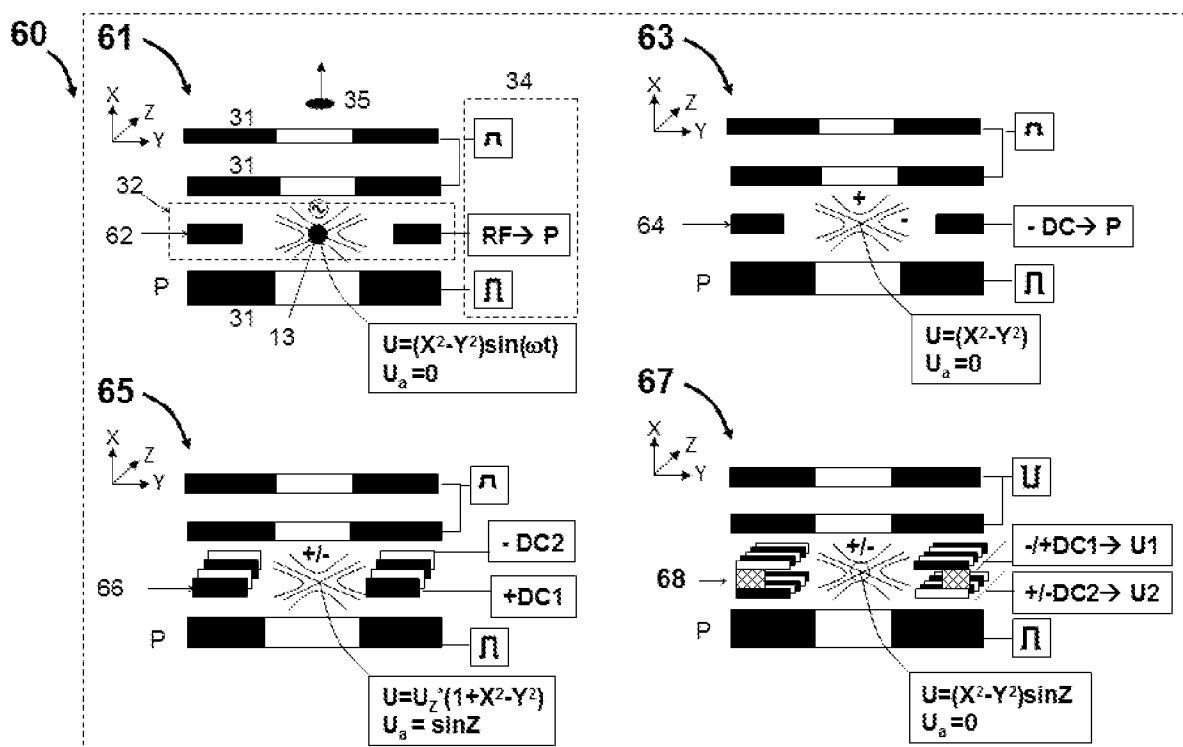


Fig. 6

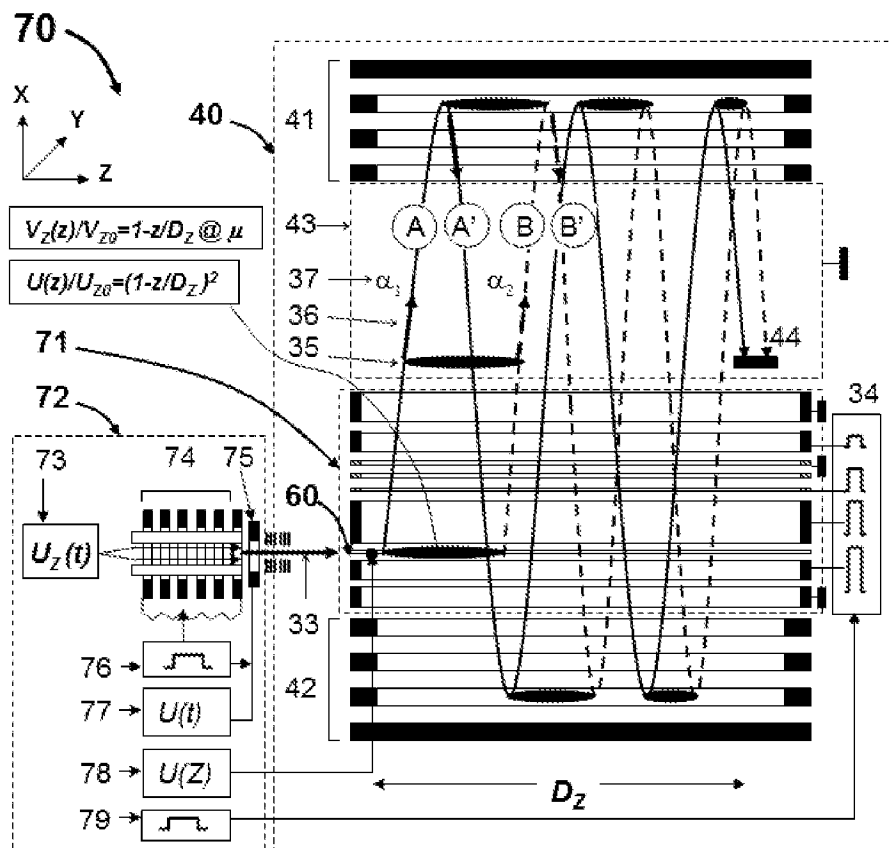


Fig. 7

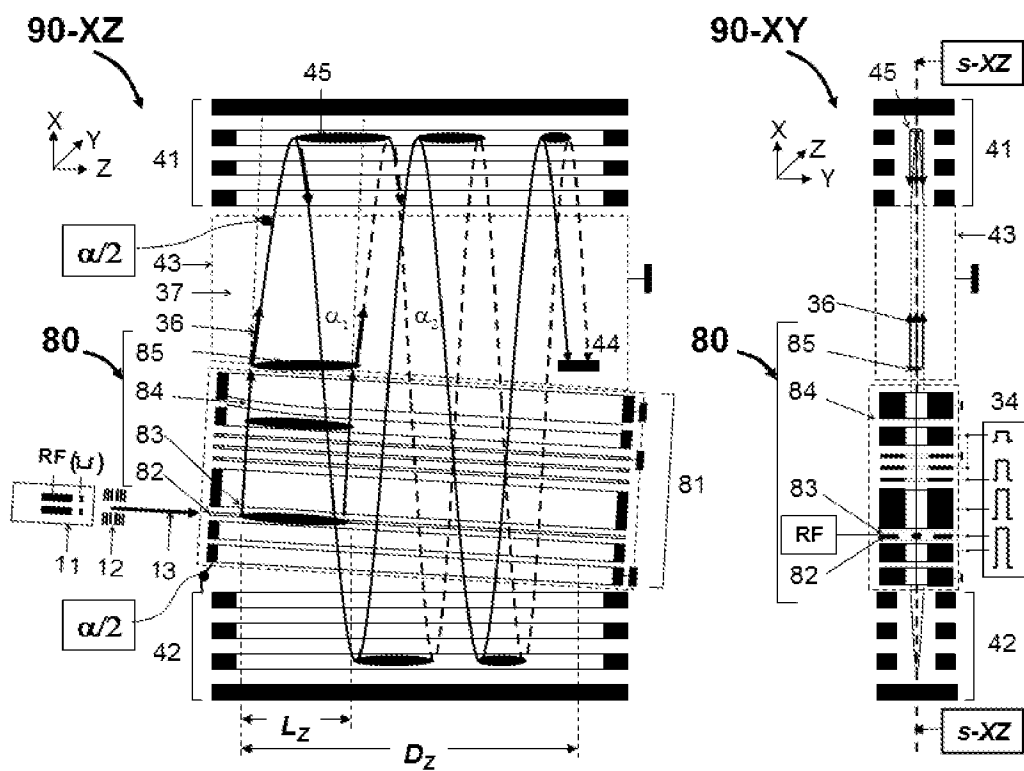


Fig.8

INTERNATIONAL SEARCH REPORT

International application No
PCT/GB2019/051839

A. CLASSIFICATION OF SUBJECT MATTER
INV. H01J49/40
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
H01J

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 2011/086430 A1 (VERENCHIKOV ANATOLY [RU]) 21 July 2011 (2011-07-21) abstract figures 11-A, 14 page 16, lines 8-12 page 48, line 9 - page 56, line 22 -----	1-32
A	WO 2016/174462 A1 (MICROMASS LTD [GB]; LECO CORP [US]) 3 November 2016 (2016-11-03) cited in the application abstract figures 4A-C page 19, lines 4-19 ----- -/-	1-32



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

11 September 2019

Date of mailing of the international search report

18/09/2019

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Dietsche, Rainer

INTERNATIONAL SEARCH REPORT

International application No
PCT/GB2019/051839

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	JP 2006 049273 A (JEOL LTD) 16 February 2006 (2006-02-16) abstract figures 6, 7 paragraphs [0025] - [0031] -----	1-32
X,P	WO 2019/030476 A1 (VERENCHIKOV ANATOLY [ME]; MICROMASS LTD [GB]) 14 February 2019 (2019-02-14) abstract figure 9 page 1, lines 18-22 page 19, lines 5-45 -----	1-32
A	WO 2007/104992 A2 (MICROMASS LTD [GB]; BROWN JEFFERY MARK [GB]) 20 September 2007 (2007-09-20) abstract figure 2 page 28, lines 1-16 -----	1-32
A	US 6 107 625 A (PARK MELVIN [US]) 22 August 2000 (2000-08-22) cited in the application abstract figures 1, 3, 4 column 9, line 20 - column 10, line 47 -----	1-32
A	TOYODA M ET AL: "Multi-turn-time-of-flight mass spectrometers with electrostatic sectors", JOURNAL OF MASS SPECTROMETRY, WILEY, CHICHESTER, GB, vol. 38, 3 November 2003 (2003-11-03), pages 1125-1142, XP002990932, ISSN: 1076-5174, DOI: 10.1002/JMS.546 cited in the application abstract figure 17 Section "Small mass spectrometers for planetary exploration" on page 1140 -----	1-32

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/GB2019/051839

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2011086430	A1	21-07-2011	CN 102884608 A 16-01-2013
		DE 112010005660 T5 18-07-2013	
		GB 2476964 A 20-07-2011	
		GB 2477007 A 20-07-2011	
		JP 5805663 B2 04-11-2015	
		JP 6247261 B2 13-12-2017	
		JP 2013517595 A 16-05-2013	
		JP 2016006788 A 14-01-2016	
		US 2013068942 A1 21-03-2013	
		US 2015380233 A1 31-12-2015	
		US 2016005582 A1 07-01-2016	
		US 2016005584 A1 07-01-2016	
		US 2016005587 A1 07-01-2016	
		US 2016013040 A1 14-01-2016	
		US 2017365456 A1 21-12-2017	
		US 2017365457 A1 21-12-2017	
		US 2017372883 A1 28-12-2017	
		US 2019157062 A1 23-05-2019	
		WO 2011086430 A1 21-07-2011	
WO 2016174462	A1	03-11-2016	CN 107851549 A 27-03-2018
		EP 3289602 A1 07-03-2018	
		GB 2554291 A 28-03-2018	
		JP 2018517244 A 28-06-2018	
		US 2018144921 A1 24-05-2018	
		WO 2016174462 A1 03-11-2016	
JP 2006049273	A	16-02-2006	JP 4649234 B2 09-03-2011
		JP 2006049273 A 16-02-2006	
WO 2019030476	A1	14-02-2019	NONE
WO 2007104992	A2	20-09-2007	CA 2645651 A1 20-09-2007
		CA 2821097 A1 20-09-2007	
		EP 2002461 A2 17-12-2008	
		EP 2688088 A2 22-01-2014	
		GB 2437609 A 31-10-2007	
		GB 2447160 A 03-09-2008	
		GB 2453468 A 08-04-2009	
		GB 2456089 A 08-07-2009	
		JP 5162479 B2 13-03-2013	
		JP 2009530761 A 27-08-2009	
		US 2009314934 A1 24-12-2009	
		WO 2007104992 A2 20-09-2007	
US 6107625	A	22-08-2000	US 6107625 A 22-08-2000
		US 6576895 B1 10-06-2003	