

(12) PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. AU 199963503 B2
(10) Patent No. 768756

(54) Title
Imaging

(51)⁷ International Patent Classification(s)
G06T 005/00

(21) Application No: **199963503**

(22) Application Date: **1999.10.15**

(87) WIPO No: **WO00/22573**

(30) Priority Data

(31) Number	(32) Date	(33) Country
9822397	1998.10.15	GB
9825165	1998.11.18	GB
9902332	1999.02.02	GB

(43) Publication Date : **2000.05.01**

(43) Publication Journal Date : **2000.06.22**

(44) Accepted Journal Date : **2004.01.08**

(71) Applicant(s)
Kui Ming Chui

(72) Inventor(s)
Kui Ming Chui

(74) Agent/Attorney
PHILLIPS ORMONDE and FITZPATRICK,367 Collins Street,MELBOURNE VIC 3000



00000/99


INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification ⁷ : G06T 5/00</p>	<p>A1</p>	<p>(11) International Publication Number: WO 00/22573 (43) International Publication Date: 20 April 2000 (20.04.00)</p>
<p>(21) International Application Number: PCT/GB99/03417 (22) International Filing Date: 15 October 1999 (15.10.99) (30) Priority Data: 9822397.7 15 October 1998 (15.10.98) GB 9825165.5 18 November 1998 (18.11.98) GB 9902332.7 2 February 1999 (02.02.99) GB (71)(72) Applicant and Inventor: CHUI, Kui, Ming [GB/GB]; 8 Gilbey Close, Ickenham, Uxbridge, Middlesex UB10 8TD (GB). (74) Agent: COLES, Graham, Frederick; Graham Coles & Co., 24 Seeleys Road, Beaconsfield, Buckinghamshire HP9 1SZ (GB).</p>	<p>(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, DM, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>	

(54) Title: IMAGING

(57) Abstract

A de-convolution process is applied to an MR, CT or other image (25) of a scanned-object (23) to derive the point-spread function (22') at an object-edge and to pin-point from the mid-point of its full-width-half-maximum FWHM, the location (30) of the true image-edge. With the object-image (25') overlying the PSF function (22') in the de-convolution space, sub-pixels which follow location (30) are transferred to before it to re-construct the image-edge (25') for sharper conformity to the object-edge (23). Sharp definition of image-contour (37) facilitates accurate determination of area and volume of image profiles (35) and their segmentation. The accurate image-edge definition enables viable correction of geometrical distortion in stand-alone MR diagnosis and treatment planning.

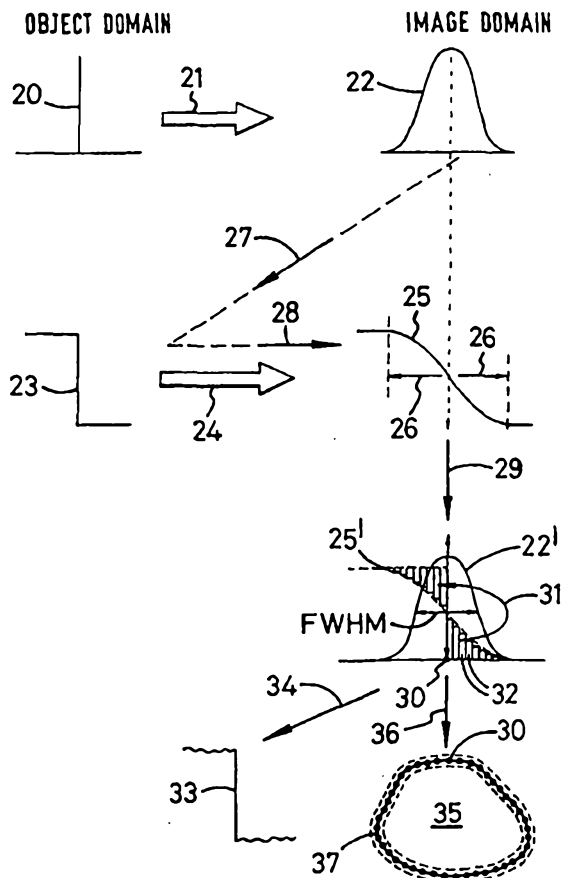

Imaging

5

This invention relates to imaging and in particular to methods and systems for image enhancement.

10

Imaging involves transfer from the object domain into the image domain, but owing to limiting factors such as the finite size of energy source, detector size, sampling frequency, display density, software filter function, and possibly partial-volume effects experienced with some imagers, an infinitely fine delta function in the object domain cannot be faithfully reproduced in the image domain. Instead, a smeared-out image, or point-spread function (PSF), is observed. Similarly, an infinitely sharp edge-response function (ERF) in the object domain becomes a smeared-out ERF in the image domain. The smearing effect becomes more intense as the adjacent ERFs of discontinuities or contrast profiles get closer to each other.

It is an object of the present invention to provide a method and system by which the above problem can be at least partly overcome.

According to one aspect of the present invention there is provided a method of imaging wherein a de-convolution process is carried out with sub-pixel sampling of the image edge-response function in the image domain of each of one or more scanned object-discontinuities to derive the profile of the respective point- or line-spread function, the derived profile is correlated with the image-domain profile of the respective edge-response function, the location in the image domain of the respective discontinuity is determined from the mid-point of the full-width half-maximum of said derived profile, and sub-pixels within the image-domain profile of the edge-response function are transferred from one side to the other of said location for enhancing the spatial resolution of the image-edge at the discontinuity.

According to another aspect of the invention there is provided

an imaging system including means for performing a de-convolution process with sub-pixel sampling of the image edge-response function in the image domain of each of one or more scanned object-discontinuities to derive the profile of the
5 respective point- or line-spread function, means for correlating this derived profile with the image-domain profile of the respective edge-response function and determining the location in the image domain of the respective discontinuity from the mid-point of the full-width half-maximum of said derived
10 profile, and means for transferring sub-pixels within the image-domain profile of the edge-response function from one side to the other of said location for enhancing the spatial resolution of the image-edge at the discontinuity.

15 With the method and system of the invention there is the advantage that the location of the discontinuity in the image domain is derived with the use of sub-pixel sampling, from the image-domain profile of the respective point- or line-spread function, and in this respect has accuracy that takes into
20 account not only the point- or line-spread function of the imaging system itself, but also the contrast-level and partial-volume effects, and random noise as well as overshoots (for example due to filtering) that occur in the image edge-response function.

25 The transfer of sub-pixels from one side to the other of the derived location of the respective discontinuity provides an empirical method of accurately enhancing the spatial resolution of the image-edge at the discontinuity. In this way, the method
30 and system of the invention enable loss of spatial resolution in the imaging to be recovered without the trade-off loss of other properties, and in particular achieves this without increase in noise in the resultant image. The original high-resolution 'step-function' feature at the discontinuity is in effect
35 restored without increase in noise, and the absence of increased noise is of critical importance to the provision of accurate image-definition free of any substantial smearing.

40 The de-convolution process of the method and system of the present invention may be carried out by sub-pixel sampling using least-squares running filtering.

Low-contrast filtering may be used to remove spurious edges in

the image domain.

An edge-contour of the object scanned may be defined in the image domain by enhancing edge-image definitions as aforesaid of
5 the images of a multiplicity of scanned object-discontinuities. The area and/or volume and/or intensity of the object-image within the edge-contour may be determined.

An imaging method and system according to the present invention
10 will now be described, by way of example, with reference to the accompanying drawings, in which:

Figure 1 illustrates schematically the method and system of the invention;





Figure 2 illustrates features of processing performed in the method and system of Figure 1;

5 Figure 3 shows results achieved from use of the method and system of Figure 1;

Figure 4 shows to an enlarged scale a section of the contour of an image profile depicted in Figure 2;

10 Figures 5 and 6 are a plan view and sectional end-elevation of a couch-top used in the method and system of Figure 1; and

15 Figure 7 provides illustrates of a convolution operation, as a basis for a mathematical model of de-convolution processing in accordance with the method and system of Figure 1.



20 The method and system to be described with reference to Figure 1 utilise MR scanning for medical diagnostic and treatment-planning purposes. In principle and in the general techniques described, the method and system of the invention can be used in other applications of MR scanning and also in circumstances where other scanning
25 techniques are utilised. Furthermore, although both structure and function are represented by discrete 'boxes' 1 to 19 in Figure 1, the method and system are to a substantial extent manifest in programmed digital data-processing operations.

30 Referring to Figure 1, data derived in accordance with conventional operation of an MR scanner 1 is processed for imaging purposes within a processor 2. The output of the processor 2 is used to provide a display 3, and from
35 this is subject to post-imaging processing 4. The post-imaging processing 4 includes the facility for selecting

a region of the display 3 for more-detailed and closer
5 inspection.

To the extent the imaging method and system of Figure 1 have so far been described, they are conventional, and it is in further processing 5 of the image data of the selected region of
10 interest obtained by the post-imaging processing 4 that a step forward from what is already known is achieved. More particularly, the further processing 5 is operative to define more clearly the true edges or boundaries of image contour(s) in the selected region of interest, and to enhance the accuracy of
15 the imaging of those contours.

The definition and accuracy of transfer of features from the object domain scanned by the scanner 1, to the image domain manifest in the post-imaging processing 4, is limited by many
20 factors. The limitations arise from within the scanner 1 itself (in particular the finite size of the energy source), within the processing performed by the processor 2, and within the display 3; limitations arise inherently from, for example, the data sampling frequency and display density used, and also from the
25 filter-function of the software involved. More particularly, and referring to Figure 2, an infinitely fine delta function 20 in the object domain is not faithfully reproduced in the image domain. Instead, the transfer as represented by the arrow 21 results in a point-spread function (PSF) or smeared-out image 22 in the image domain. Similarly, an infinitely sharp edge-
30 response function (ERF) or step 23 in the object domain becomes through the transfer represented by arrow 24, a smeared-out transition 25 of spread represented by dimension arrows 26, in the image domain. When two ERF image-profiles are close to one another, the smeared-out effects run into each other. The
35 consequent deterioration of the spatial resolution is often



40

5



monitored by the percentage modulation transfer which is given
by the ratio, expressed as a percentage, of the amplitude of the
10 modulation in the image domain to that in the object domain.

The smearing effect becomes more intense as adjacent ERFs of
discontinuities or contrast profiles get closer to each other
(or as the spatial frequency of the modulation becomes higher);
15 this also causes loss of profile height. The inherent loss of
the spatial resolution (that is, the part that is indicated by
the smeared-out effect on the corner edge of the ERF) cannot be
restored or partially restored even by re-scanning the image
with an ultra high resolution digital scanner system.

20

The further processing 5 is operative in accordance with the
invention to provide accurate edge-image definition and
location, and to improve spatial resolution in the imaging.
More especially, in the context of Figure 2, the edge position
25 corresponding to the discontinuity or step 23 of the object ERF
is pin-pointed in the image domain from the mid-point of the
full-width half-maximum (FWHM) of the image PSF; the
pin-pointing is to sub-pixel accuracy for the ERF image-profile.
Low-contrast and 'area' filtering are used to remove 'spurious'
30 edges, and sub-pixel sampling to detect detail to the resolution
of the single-pixel modulation. The discontinuity or step 23 of
the ERF is then restored within the image domain by removing the
sub-pixel values from outside the optimum edge position to
compensate for those within. It is to be noted that the
35 sub-pixels then become pixels in display, and that the
enhancement is equivalent to the performance of an extra high
resolution image transfer system.

As represented in Figure 2 by the arrows 27 and 28, the ERF
40 image-profile 25 of an infinitely-sharp step 23 can



5

be produced by convolution of the image PSF 22 with the object ERF 23. In accordance with the present invention, de-convolution of the ERF image-profile 25 using sub-pixel sampling represented by the arrow 29, reproduces the image PSF 22 in a de-convolution space as profile PSF 22'. The ERF image-profile 25 is superimposed on the PSF 22' within this space as ERF image-profile 25', and the optimum edge-position 30 is derived from the mid-point of the FWHM of the image PSF 22', and is pin-pointed to sub-pixel accuracy.



For one-dimensional cases, the operation in accordance with the invention is relatively simple, as only either the x- or the y-profile, that is to say a line spread function LSF is involved. But for two-dimensional operations, both the x- and y-profiles, and if necessary, the xy-diagonal profiles to eliminate any possible streakings in the image, may be used; in this case, a proper weighting scheme will be required to re-construct the image.

25

Once the original sharp-edge feature represented by the object ERF 23 is pin-pointed at the position 30 within further processing 5, that feature may be restored by additional re-processing 6 (Figure 1). In re-processing 6, the sub-pixel values occurring 'outside' the optimum edge-position 30 are transferred to compensate those 'within'. This is illustrated in Figure 2 by arrow 31 transferring sub-pixel blocks 32 from after point 30 in the ERF image-profile 25', to before it. The re-construction of the ERF image-profile 25' into ERF image-profile 33 conforming closely in configuration to object ERF 23 is represented by arrow 34. Image-profile 33 is displayed in enlarged form in display 7 (Figure 1).

These techniques enable substantial recovery of the loss of spatial resolution in the imaging, without the

40



5



trade-off loss of other properties such as image noise. Furthermore, the enhancement of spatial resolution in display 7 reproduces the region of interest selected from display 3, without blurring (or step) effects at the profile edge.

Figure 3 is illustrative of some of the low-contrast results provided in practice from MR scanning of a pig's brain in fluid. Curve A is the ERF image-profile produced, whereas curve B is the line spread function (LSF) resulting from de-convolution of curve A carried out in processing 5. The optimum edge-position is established from the mid-point C of the FWHM of curve B, and the additional re-processing 6 is operative by means of sub-pixel transfer, to re-construct curve A to conform substantially to the edge-feature from which it originated in the display 7.

It is to be noted that whereas curve A is stepped, curve B is nonetheless smooth and that mid-point C is located to sub-pixel accuracy. Furthermore curve B indicates a sensitivity of more than 8:1 between the profile-height and background noise.

Referring again to Figure 2, the complete profile 35 of an image within the selected area of interest of display 3, is built up as indicated by arrow 36, from the edge-position data derived within processing 5. This data identifies the location of the point 30, together with the locations of all corresponding points derived from sampling the multiple x- or y-profiles of the selected area of interest. The build up and display of these points from the data takes place in display 8 so that a substantially true contour 37 for the profile 35 is defined. The sharpness of the true contour 37 is in contrast to the smeared contour that in the absence of enhancement, would have been obtained by virtue of the

40



5 spread (represented by the arrows 26) of the relevant ERF image-
profiles 25.

A small portion of the contour 37 is shown enlarged in Figure 4
and is defined as a best-fit line between optimum edge-positions
10 derived respectively from x- and y-profiles; the x-profile
positions are indicated by black dots and the y-profile
positions by white dots. The closeness to one another of
corresponding positions in the x- and y-profiles is indicative
of the accuracy to sub-pixel level achieved. The smear-out that
15 would have been manifest in the image-profile contour if the de-
convolution technique were not used, would have extended
throughout the space bounded by the dashed lines 38 and 39;
these boundaries are indicated in dashed line in the
representation of profile 35 in Figure 2.

20

The accurate definition of the image contour 37 derived in the
display 8 allows correspondingly accurate determination in
calculation 9 of the area within that contour; the volume
involved can also be derived from successive slices scanned.
25 The determination of area and volume is especially useful for
diagnostic and accurate assessment 10 of the size of a tumour or
lesion before and after treatment. It is similarly useful for
assessment of arterial dimensions in angiography.

30

Moreover, the accurate definition of the image contour 37
derived in the display 8, is particularly useful for segmenting
anatomical structures for diagnostic and treatment planning 11.
Furthermore, the ratio of intensities of two scans are derived
by processing 12 to derive values of relaxation times T_1 and T_2 ,
and of proton density. The values are then represented in
35 display 13 within the boundary of the image contour, utilising
standardisation data derived from a couch-top 14 used
within the scanner 1. The couch-top 14, which also

40

provides landmarks for determining position coordinates, has the form shown in Figures 5 and 6, and will now be described.

5 Referring to Figures 5 and 6, the couch-top 40, which is of polystyrene bubble foam, has the form of a flat slab, and is supported on a curved foam base 41 that fits to the scanner table of the MR installation. Two zig-zag runs of tubing 42 are embedded within the top 40 to
10 extend along the length of the couch either side of centrally-embedded straight tubing 43.

The tubing 42 of each zig-zag run is of double-bore rectangular cross-section, whereas the tubing 43 is of
15 single-bore cross-section. The five bores defined by the array of tubing 42 and 43 may be filled respectively with the five MR solutions S_0 to S_4 of Table I, for standardisation and calibration purposes. The four
20 $MnCl_2 \cdot 4H_2O$ solutions, S_1 to S_4 , cover the full range of values of T_1 and T_2 for anatomical tissues, and the fifth solution, S_0 , of $CuSO_4 \cdot 5H_2O$, is nominally equivalent to "loosely bound water".

Table I

25	Solution		T_1 at 0.5T	T_2 at 0.5T
	S_0	1.25 g/l $CuSO_4 \cdot 5H_2O$	200 ms	200 ms
	S_1	3.41×10^{16} Mn^{+2} ions/ml	840 ms	300 ms
	S_2	1.15×10^{17} Mn^{+2} ions/ml	440 ms	120 ms
	S_3	2.30×10^{17} Mn^{+2} ions/ml	250 ms	60 ms
30	S_4	4.37×10^{17} Mn^{+2} ions/ml	150 ms	30 ms

The tissue types revealed by the T_1 , T_2 and proton density values in display 13 are determined by processing 15 from look-up tables, and tissue densities are assigned within the image-contour boundaries in display 16. The images
5 of display 16 are furthermore corrected empirically for geometry distortion in accordance with data supplied from memory 17. The data stored in memory 17 is derived using a set of drum phantoms of the spider-web form, and correction for geometry distortion is realistically
10 effective principally because of the accuracy and spatial resolution with which image-contours are defined.

The tissue types assigned to the corrected images are utilised in display 16 through the Bulk Heterogeneity
15 Correction method described by Richard A, Geise *et al*, Radiology, 124:133-141, July, 1977, to establish for each image a normalised tissue density value; the up-datable look-up table for this is stored in memory 18. Accordingly, the display 16 when used at step 19 in
20 conjunction with the positional datums derived from the couch 14, has all the tissue contours accurately mapped out with their respective tissue densities and locations. This establishes an accurate and readily-usable, stand-alone basis for diagnosis and treatment planning, and
25 enables a true three-dimensional assessment and plan to be made when both orthogonal and oblique MR images are involved.

Although the method and system of the invention have been
30 described above in the medical context they are applicable more widely than this, for example, in engineering, in physical science and in the field of instrumentation generally. Moreover, the method and system is not limited to MR imaging, but may be utilised
35 where other forms of imaging are involved. The steps and structure represented in Figure 1 by 'boxes' 1 to 11 are just as applicable to computer assisted tomography (CT),

as they are to MR imaging. Other forms of imaging to which the invention is applicable include X-ray radiography, film- or print-image transformation to digital form, digital X-ray fluorography, ultra-sound imaging, nuclear medicine, positron emission tomography (PET) and other camera or imaging. The technique is particularly suitable for use in X-ray digital fluorography, in which small structures under study are highlighted by injection of contrast liquids; the small structures may also be isolated from surrounding interfering effects by using an image subtraction technique.

The inherent resolutions of X-ray radiography, ultra-sound imaging, nuclear medicine, and PET scanning are relatively low, and some are used for real-time study. Only the individual still frame or hard-copy images may be re-processed.

In the context of engineering, physical science and the field of instrumentation, the invention is applicable to one-dimensional imaging as used, for example, in regard to bar-code patterns, the spectrum of DNA analysis, iris patterns of eyes (for example, for identification purposes in commercial banking), finger-print identification, and emission spectroscopy. The invention is also applicable to two-dimensional imaging, for example, in relation to images obtained by satellite or pattern recognition, or from a surveillance camera or during laboratory experimentation. As a general matter, the invention is applicable where there needs to be accurate determination of the edge position in an image versus the true object-edge position, for the purpose, for example, of measurement of the positional displacement between object and image, distortion correction and manufacturing control.

As a further example of application of the present invention, a method and system that uses CT and MR imaging in conjunction with one another, will now be described.

5

The major contribution to the magnetic-resonance (MR) signal comes from the abundant protons content of water molecules and protein. It is a quantum process at the Larmor frequency according to the magnetic field in use. The ' T_1 -weighted' and ' T_2 -weighted' MR signals from protons provide contrast numbers that are relative in scale, whereas in CT, the X-ray absorption is a polychromatic attenuation process affected by the electron densities of all the atoms presented within the X-ray beam. There is no equation to correlate the CT number (or the linear attenuation coefficient, electron density, or tissue density) with the MR-contrast numbers; no direct calibration between the two types of signal is possible. This lack of correlation is confirmed by consideration of bone and air which are at opposite ends of the CT contrast (absolute) scale using water as the base-line reference, but which are at the same end of the MR-image contrast (relative) scale owing to their common low proton-population.

20
25

The lack of correlation between the CT and MR signals acts against their use in combination for imaging purposes, but the present invention provides a method and system by which the advantages of each may be utilised to improve image resolution and contrast information.

30

In the latter regard, CT provides a high spatial resolution but only in regard to view normal to the transverse slice. Resolution for all re-constructed non-transverse planes is poor owing to the need to use elongate voxels to improve signal-to-noise ratio. Also, the partial-volume effect of using elongate voxels may

35

give rise to detection errors at the thin edge of a contrast profile of a lesion. MR, on the other hand, can give the same high degree of spatial resolution viewed in the normal direction to any image-slice plane, and can
5 also provide isotropic resolution with cubic-voxel volume imaging.

To this end, multiple-slice transverse CT scans are collected across a section of the volume of interest in a
10 patient or other subject. Corresponding multiple-slice transverse MR scans of the same volume are also collected. The slice thickness of the latter scans may be one half, or smaller, of the thickness of the CT slices, and may be collected two-dimensionally or three-
15 dimensionally. The patient or other object scanned is constrained throughout on a couch that provides landmarks with respect to a coordinate reference arrangement on the couch-top. This is to ensure the reproducibility of, for example, anatomical positions and features to the first
20 order accuracy for the corresponding CT and MR scans, and possibly for radiation treatment to be made.

The respective transverse planes of the CT and MR images are processed individually in the method and are matched
25 with one another in a de-convoluted space for the CT and MR images. The two sets of de-convoluted maps are then merged together to a second order of accuracy in order that the CT numbers may be transferred over to replace the corresponding MR contrast numbers. Once this has
30 been achieved, non-transverse (or oblique) planes can be obtained from the two-dimensional MR images, or from the re-arrangement of the corresponding voxels of the three-dimensional volume images; where two-dimensional MR is used, a further step of contrast transformation may be
35 required.

The respective transverse planes of CT and MR images are processed individually by using 'boundary' or 'finger-print' matching techniques in a de-convolution space for the CT & MR images. In these transverse image planes, in particular when used medically, the skin-contour features along the sides of the patient may be best used for second-order alignment and matching purposes, as they are less affected by patient-movements. Transitional error may be readily corrected with respect to the coordinate positions of a rectangular tubing system embedded in the couch-top (for example that described above with reference to Figures 5 and 6). The processed data may then be used for a 'diagnostic and statistics software package' of CT image versus MR image for their exactly corresponding transverse slice(s), and an associated 'statistical package' for accurate computation of the 'true' area, and then the 'true' volume, of a lesion or tissue profile or contour.

The two sets of de-convoluted maps may also be merged together to a second order of accuracy in order that the CT numbers may be transferred over to replace the corresponding MR contrast numbers. Once this has been done, non-transverse (or oblique) planes are obtained from the two-dimensional image or from the re-arrangement of the corresponding voxels of the three-dimensional volume; in the two-dimensional MR case, a further step of contrast transformation is required. The transferred contrast data may then be used in a three-dimensional radiotherapy treatment planning software package for an in-plane, oblique-image pseudo-three-dimensional approach using MR images.

Software required for de-convolution processing of image data according to the invention may be implemented in conjunction with a least-squares curve-fitting method. A mathematical model of the method, from which the required

software can be readily developed, will now be given in relation to Figure 7 which indicates the convolution of an LSF $L(x)$ with a step function SF having a step-down edge SDE, to produce an ERF image-profile $E(x)$. Considering the values of $E(x)$ resulting from the convolution at points $x=1$ to $x=n$ of SF:

at $x=1$:

$$\sum_0^a L(x) \Delta x = E(x)_1$$

10 at $x=2$:

$$\sum_0^a L(x) \Delta x - \sum_{a-1}^a L(x) \Delta x = E(x)_2$$

at $x=3$:

$$\sum_0^a L(x) \Delta x - \sum_{a-2}^a L(x) \Delta x = E(x)_3$$

until at $x=n$:

$$\sum_0^a L(x) \Delta x - \sum_1^a L(x) \Delta x = E(x)_n$$

15

For de-convolution, that is to say, for the ERF $E(x)$ to manifest the LSF $L(x)$:

$$E(x)_1 - E(x)_2 = \sum_{a-1}^a L(x) \Delta x = L(x)_{(a-1)-a} \Delta x$$

$$\{E(x)_1 - E(x)_2\} / \Delta x = L(x)_{(a-1)-a}$$

thus:

$$\{E(x)_2 - E(x)_3\} / \Delta x = L(x)_{(a-2)-(a-1)}$$

leading to

$$\{E(x)_{(n-1)} - E(x)_n\} / \Delta x = L(x)_{(n-1)-n}$$

20

Thus, the same shape of LSF is recovered by the de-convolution process independently of the sense of the ERF; it does not matter whether a roll-up or a roll-down ERF of a positive or a negative contrast profile, is involved. This is an important property as a positive contrast contour will have roll-up (from low to high) ERFs at both ends whereas a negative contrast contour will have roll-down (from high to low) ERFs at both ends.

In the practical implementation, the LSF is derived from the ERF by de-convolution using a running filter. This enhances the accuracy of the method in overcoming the problem of noise that affects the digitised pixel values of the image. Use is made of a least-squares fitting of a set of data points that advances along the whole length of the function from one point to another.

Assuming that $y = a_0 + a_1x + a_2x^2$ represents the ERF curve a five-point or seven-point fit is used, and the normal equation becomes:

$$\begin{vmatrix} \sum 1 & \sum x_i & \sum x_i^2 \\ \sum x_i & \sum x_i^2 & \sum x_i^3 \\ \sum x_i^2 & \sum x_i^3 & \sum x_i^4 \end{vmatrix} \begin{vmatrix} a_0 \\ a_1 \\ a_2 \end{vmatrix} = \begin{vmatrix} \sum y_i \\ \sum x_i y_i \\ \sum x_i^2 y_i \end{vmatrix}$$

where: i is $1+n, \dots, 5+n; \dots$ until $m-5, \dots, m$
 or
 i is $1+n, \dots, 7+n; \dots$ until $m-7, \dots, m$
 n is $0, 1, 2, \dots$; and
 $1, \dots, m$ is the span of the ERF profile.

The solution may be derived from either:

$$\begin{vmatrix} a_0 \\ a_1 \\ a_2 \end{vmatrix} = \begin{vmatrix} \sum 1 & \sum x & \sum x^2 \\ \sum x & \sum x^2 & \sum x^3 \\ \sum x^2 & \sum x^3 & \sum x^4 \end{vmatrix}^{-1} \begin{vmatrix} \sum y \\ \sum xy \\ \sum x^2 y \end{vmatrix}$$

or:

$$\begin{bmatrix} a_0 \\ \Sigma y & \Sigma x & \Sigma x^2 \\ \Sigma xy & \Sigma x^2 & \Sigma x^3 \\ \Sigma x^2 y & \Sigma x^3 & \Sigma x^4 \end{bmatrix} = \begin{bmatrix} a_1 \\ \Sigma 1 & \Sigma y & \Sigma x^2 \\ \Sigma x & \Sigma xy & \Sigma x^3 \\ \Sigma x^2 & \Sigma x^2 y & \Sigma x^4 \end{bmatrix} = \begin{bmatrix} a_2 \\ \Sigma 1 & \Sigma x & \Sigma y \\ \Sigma x & \Sigma x^2 & \Sigma xy \\ \Sigma x^2 & \Sigma x^3 & \Sigma x^2 y \end{bmatrix} = \begin{bmatrix} 1 \\ \Sigma 1 & \Sigma x & \Sigma x^2 \\ \Sigma x & \Sigma x^2 & \Sigma x^3 \\ \Sigma x^2 & \Sigma x^3 & \Sigma x^4 \end{bmatrix}$$

For both of these equations to be valid:-

$$\begin{bmatrix} \Sigma 1 & \Sigma x & \Sigma x^2 \\ \Sigma x & \Sigma x^2 & \Sigma x^3 \\ \Sigma x^2 & \Sigma x^3 & \Sigma x^4 \end{bmatrix} \neq 0$$

- 5 The gradient at $dy/dx_{(3+n)}$ or $dy/dx_{(4+n)}$ can then be derived and plotted against x for the LSF profile.

The graph of dy/dx against x gives the LSF profile. The peak of this profile is located centrally of the mid-
 10 points of the ascending and descending limbs of the graph. These points define the extremes of the full-width-half-maximum (FWHM) of the profile and the mid-point of this is determined with an accuracy of sub-pixel level owing to the 'average' effect.

15 The point spread function (PSF) is the two dimensional profile which may be derived, in practice, from the two corresponding LSFs orthogonal to one another within an image plane. The peak position of the PSF profile is,
 20 therefore, from the 'mean' or 'cross-over' of the two peaks or the two LSF profiles. The PSF is obtained in practice from two orthogonal axes in a two-dimensional plane.

- 25 The generation of the LSF (or PSF) is, after phase-reversal correction, independent of the roll-up or roll-down nature of ERFs at the edges of the contrast contour. In other words, it is independent of the sense and the absolute value of the contrast numbers within the

contour. The peak position of the LSF (or PSF) is the central half-way (50%) point of the roll-up or roll-down ERF which is the optimum position for true-edge definition.

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

5 1. A method of imaging wherein a de-convolution process is carried out with sub-pixel sampling of the image edge-response function in the image domain of each of one or more scanned object-discontinuities to derive the profile of the respective point- or line-spread function, the derived profile is
10 correlated with the image-domain profile of the respective edge-response function, the location in the image domain of the respective discontinuity is determined from the mid-point of the full-width half-maximum of said derived profile, and sub-pixels within the image-domain profile of the edge-response function
15 are transferred from one side to the other of said location for enhancing the spatial resolution of the image-edge at the discontinuity.

20 2. A method according to Claim 1 wherein the de-convolution process is carried out by sub-pixel sampling using least-squares running filtering.



25 3. A method according to Claim 1 or Claim 2 wherein low-contrast filtering is used to remove spurious edges in the image domain.

30 4. A method according to any one of Claims 1 to 3 wherein an edge-contour of the object scanned is defined in the image domain by enhancing edge-image definitions as aforesaid of the images of a multiplicity of the scanned object-discontinuities.

35 5. A method according to Claim 4 wherein the area and/or volume and/or intensity of the object-image within the edge-contour is determined.

35

40



6. A method according to Claim 4 or Claim 5 wherein the
5 object-scan is a magnetic resonance (MR) scan, values of
relaxation times T_1 and T_2 are derived for the object-image
within said contour, and these values are used to identify from
stored data, types of tissue or other material involved in the
scanned object.

10

7. A method according to Claim 6 wherein density values for
the identified tissue or other material types are derived from
further stored data.

15

8. A method according to Claim 6 or Claim 7 wherein geometric
correction is applied to the imaging derived from the MR scan,
in accordance with stored data.

20

9. A method of imaging according to any one of Claims 1 to 8
applied to edge-response functions in the image domains of
magnetic resonance (MR) and computed tomography (CT) scans of
the same part of an object, and the enhanced image-edges of the
two scans are correlated with one another with respect to said
part, and wherein imaging of said part of the object is provided
25 in accordance with the enhanced MR-scan image as modified in
dependence upon the CT contrast numbers applicable to
corresponding, correlated positions within the CT scan.

30

10. An imaging system including means for performing a de-
convolution process with sub-pixel sampling of the image edge-
response function in the image domain of each of one or more
scanned object-discontinuities to derive the profile of the
respective point- or line-spread function, means for correlating
this derived profile with the image-domain profile of the
35 respective edge-response function and determining the location
in the image domain of the respective discontinuity from the
mid-point of the full-width half-maximum of said derived profile,
and means for transferring sub-pixels within the image-domain

40

profile of the edge-response function from one side to the other
5 of said location for enhancing the spatial resolution of the
image-edge at the discontinuity.

11. A system according to Claim 10 wherein the de-convolution
10 process is carried out by sub-pixel sampling using least-squares
running filtering.

12. A system according to Claim 10 or Claim 11 including means
for defining in the image domain an edge-contour of the object
15 scanned by enhancing edge-image definitions as aforesaid of the
images of a multiplicity of the scanned object-discontinuities.

13. A system according to Claim 12 including means for
determining the area and/or volume and/or intensity of the
20 object-image within the edge-contour.



14. A system according to any one of Claims 10 to 13 wherein
the object-scan is a magnetic resonance (MR) scan.

15. A method of imaging substantially as hereinbefore
25 described with reference to the accompanying drawings.

16. An imaging system substantially as hereinbefore described
with reference to the accompanying drawings.


30

DATED: 20 October 2003
PHILLIPS ORMONDE & FITZPATRICK
Attorneys for:
KUI MING CHUI



1/6

FIG. 1

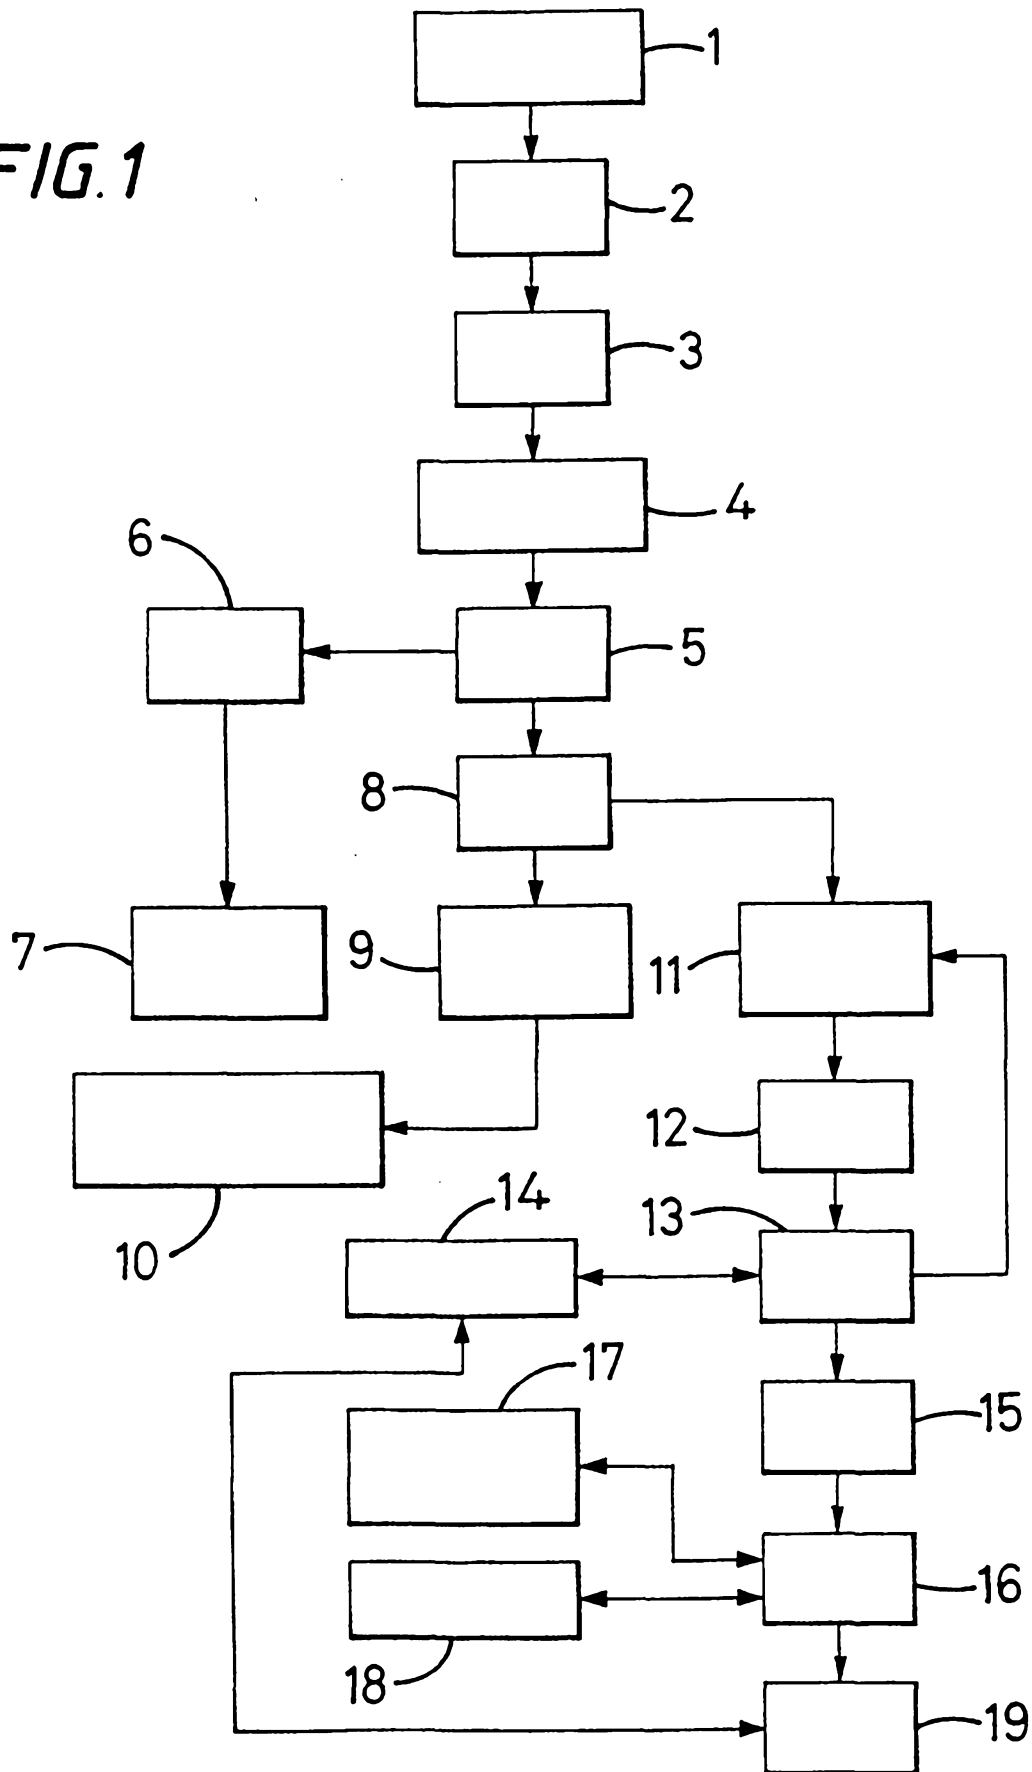

2/6
FIG. 2


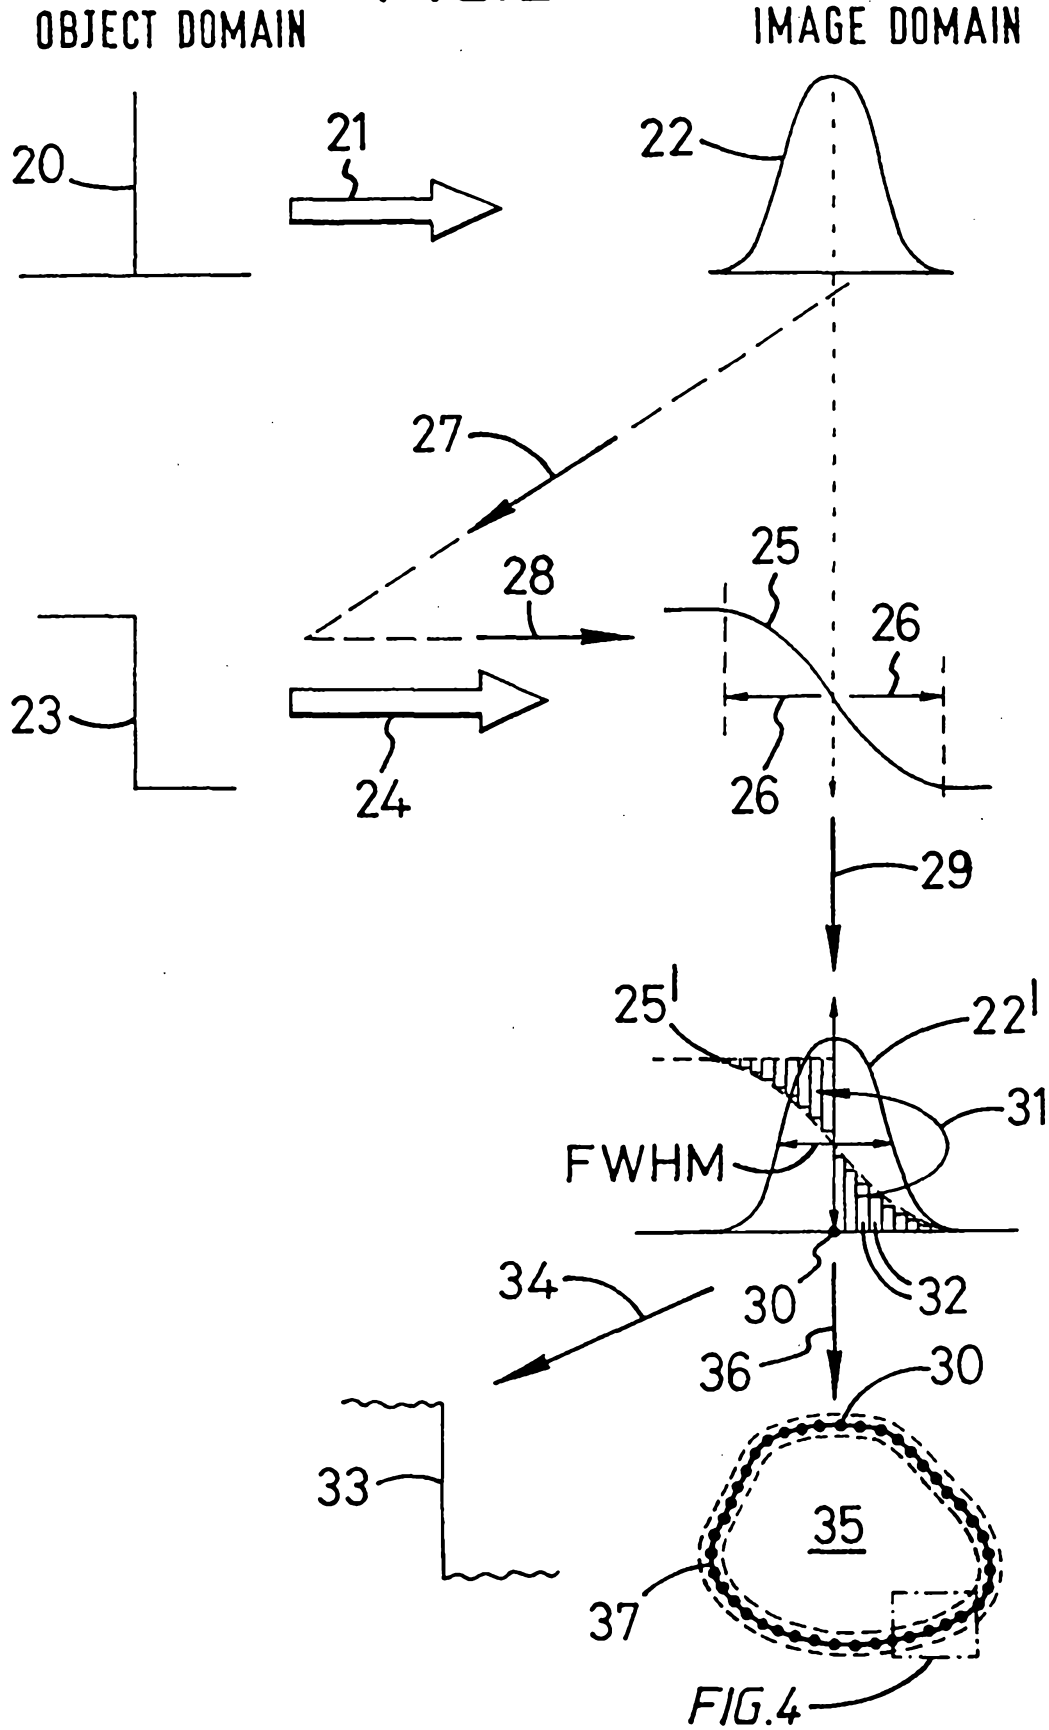


FIG. 4

FIG. 3

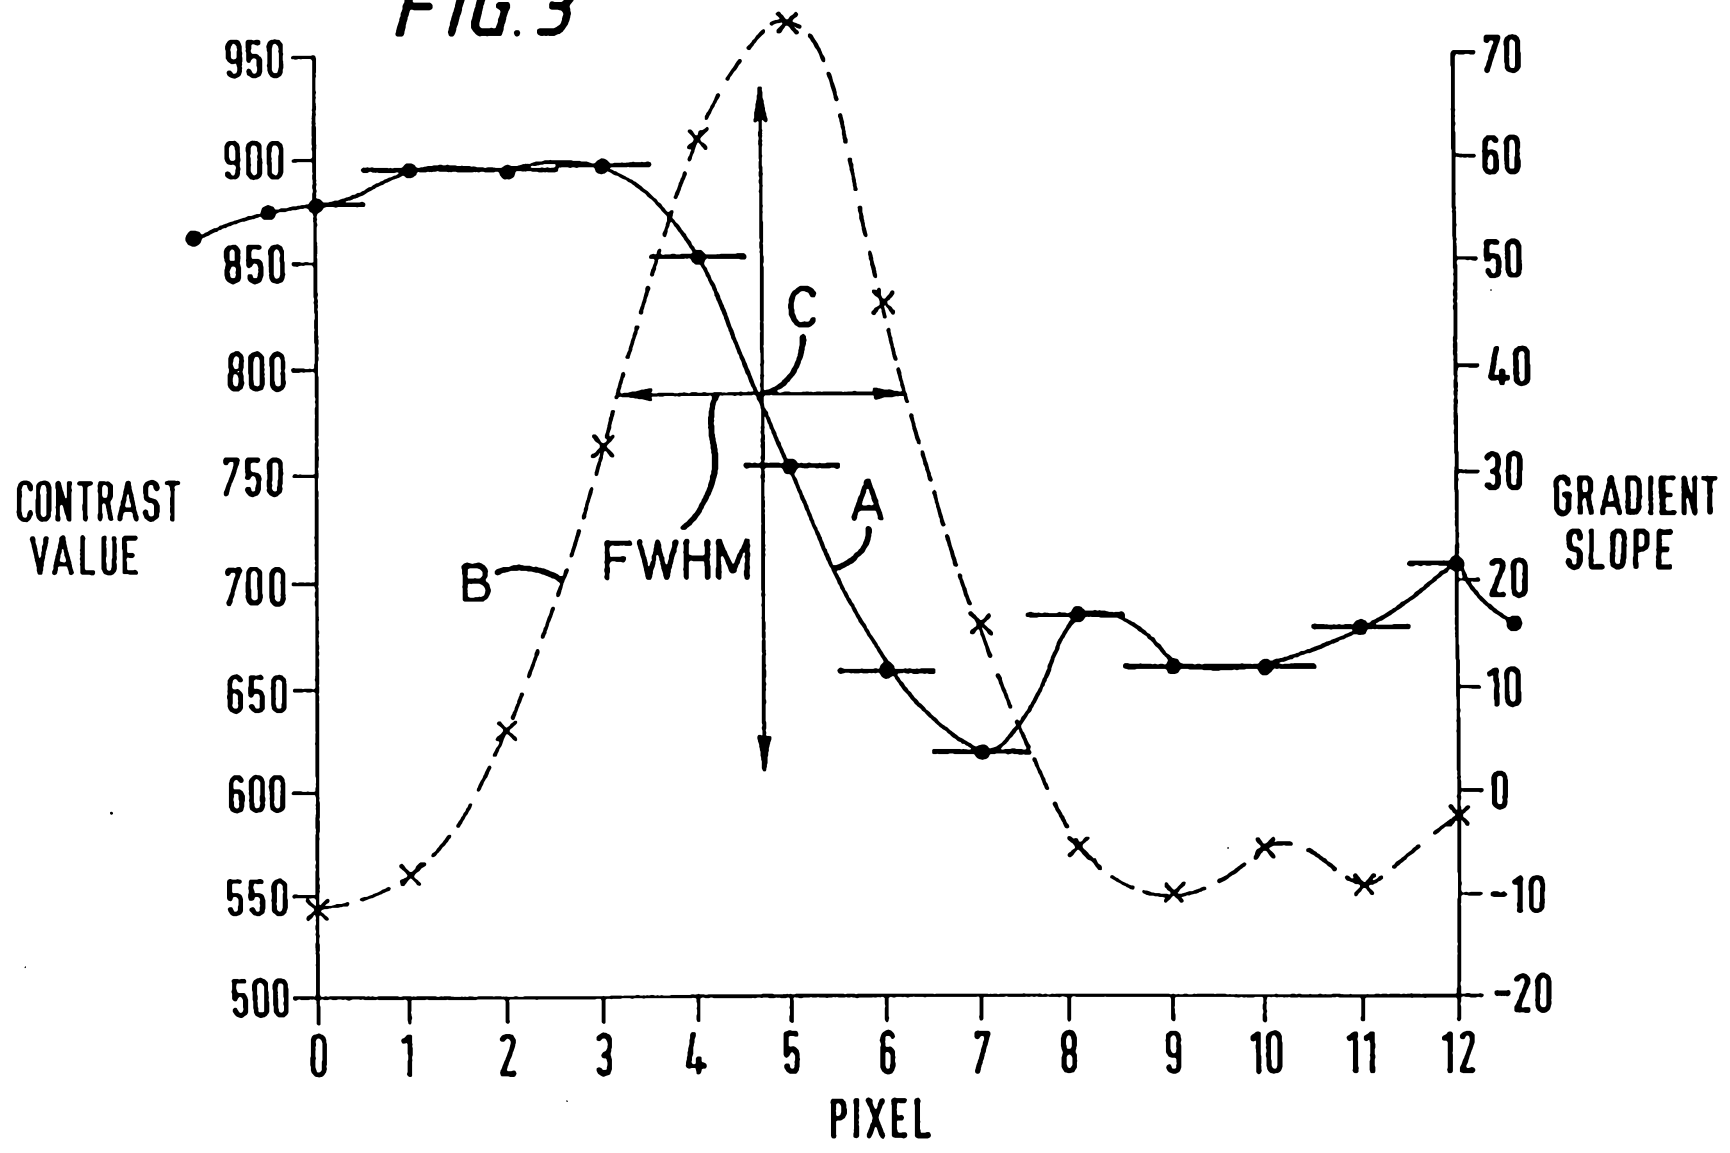

AMENDED SHEET

3/6

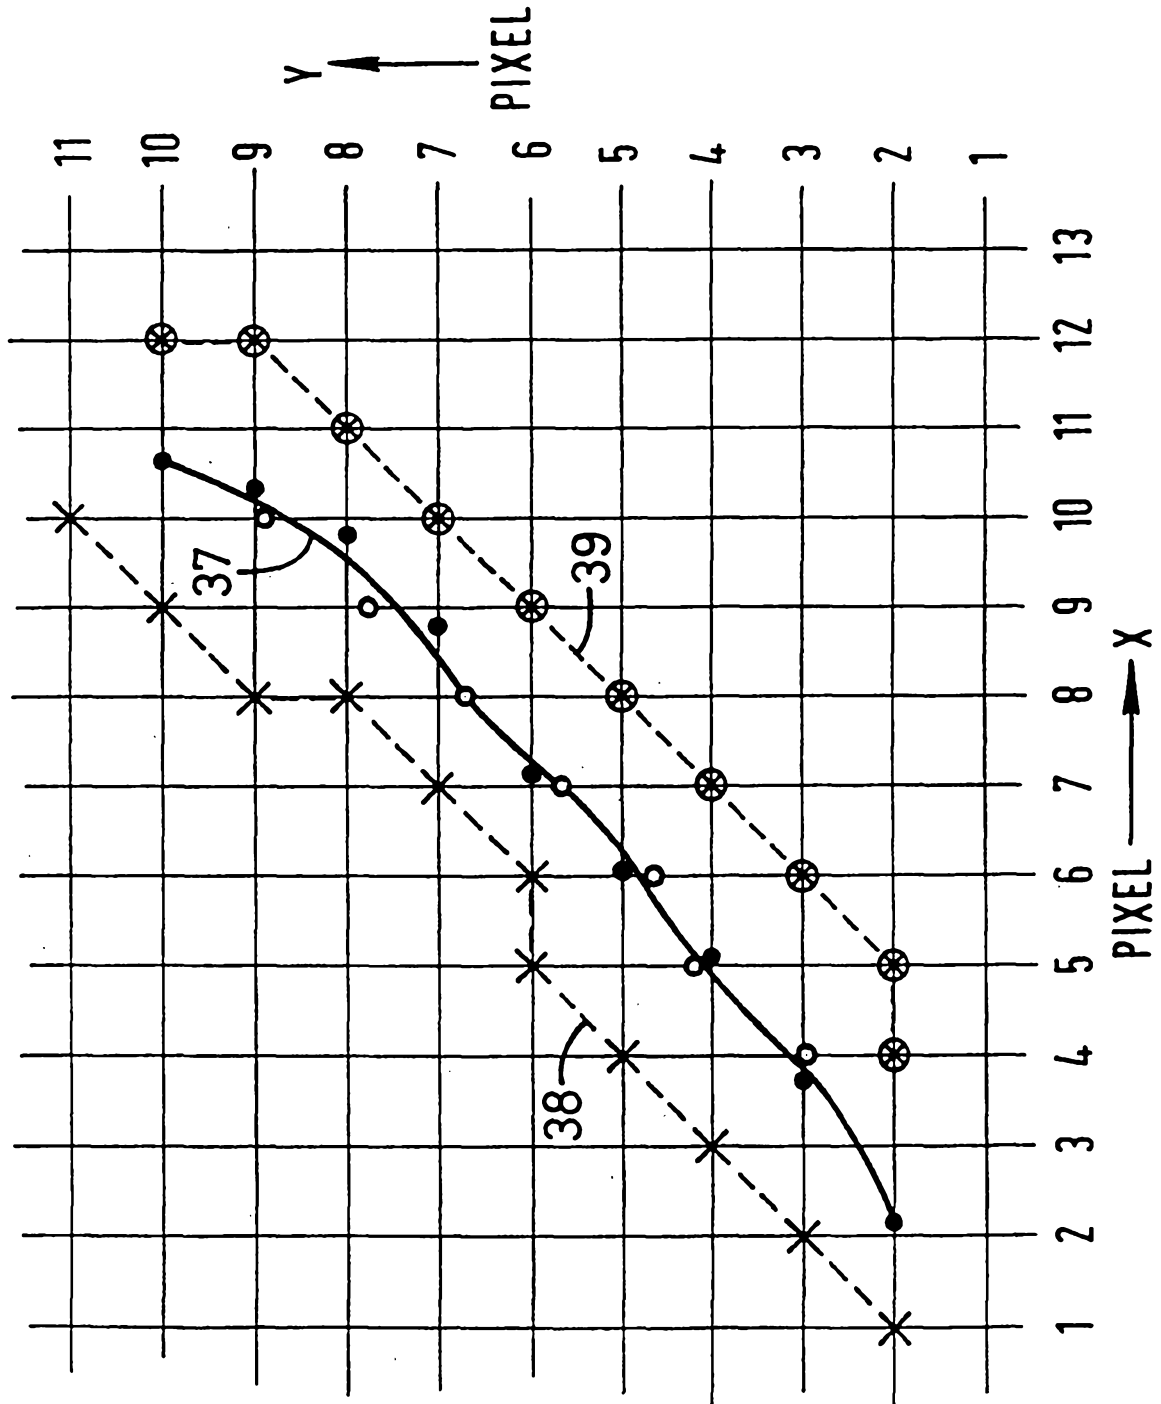


FIG. 4

FIG. 5

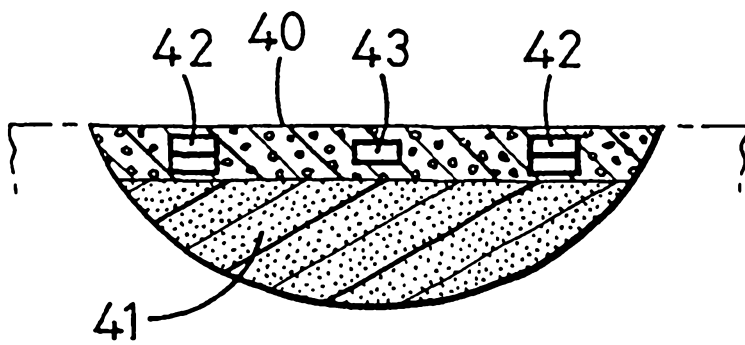
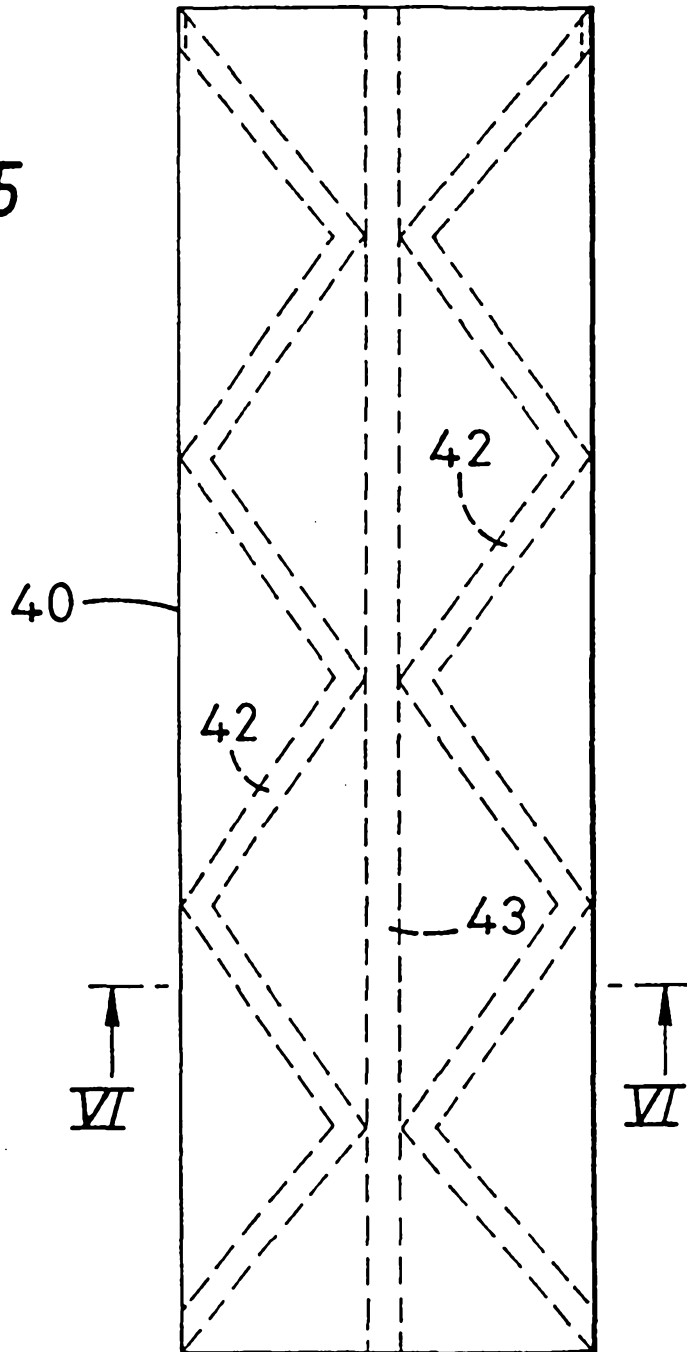


FIG. 6

6/6

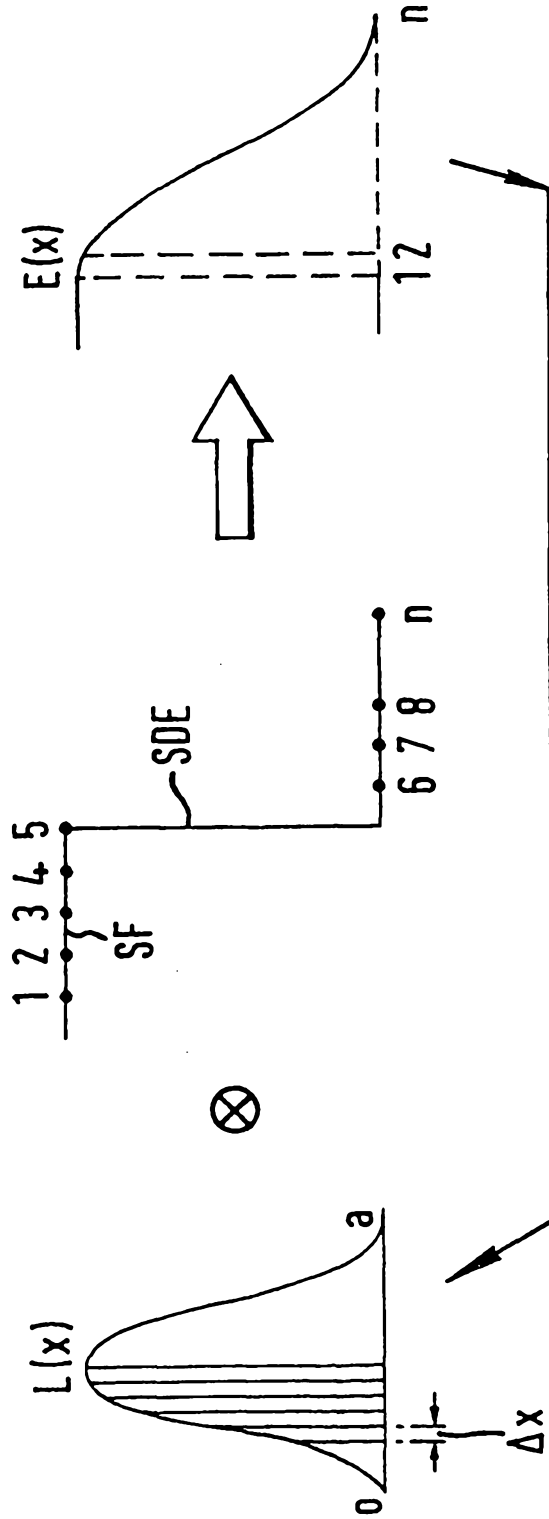


FIG. 7