



(86) Date de dépôt PCT/PCT Filing Date: 2005/03/03

(87) Date publication PCT/PCT Publication Date: 2005/09/15

(45) Date de délivrance/Issue Date: 2013/12/10

(85) Entrée phase nationale/National Entry: 2006/08/31

(86) N° demande PCT/PCT Application No.: CH 2005/000127

(87) N° publication PCT/PCT Publication No.: 2005/084524

(30) Priorité/Priority: 2004/03/04 (FR0402238)

(51) Cl.Int./Int.Cl. *A61B 1/015* (2006.01),
A61B 1/12 (2006.01)


(72) Inventeurs/Inventors:
FRANCISCO, ANDRE, FR;
JANIN, PATRICK, FR;
PASCUAL, THIERRY, FR;
DIAS, ARMANDO, FR

(73) Propriétaire/Owner:
FUTURE MEDICAL SYSTEM S.A., CH

(74) Agent: ROBIC

(54) Titre : CONNECTEUR A DETECTEUR DE PRESSION DESTINE A UN SYSTEME D'ENDOSCOPIE

(54) Title: PRESSURE TRANSMITTING CONNECTOR FOR AN ENDOSCOPY SYSTEM

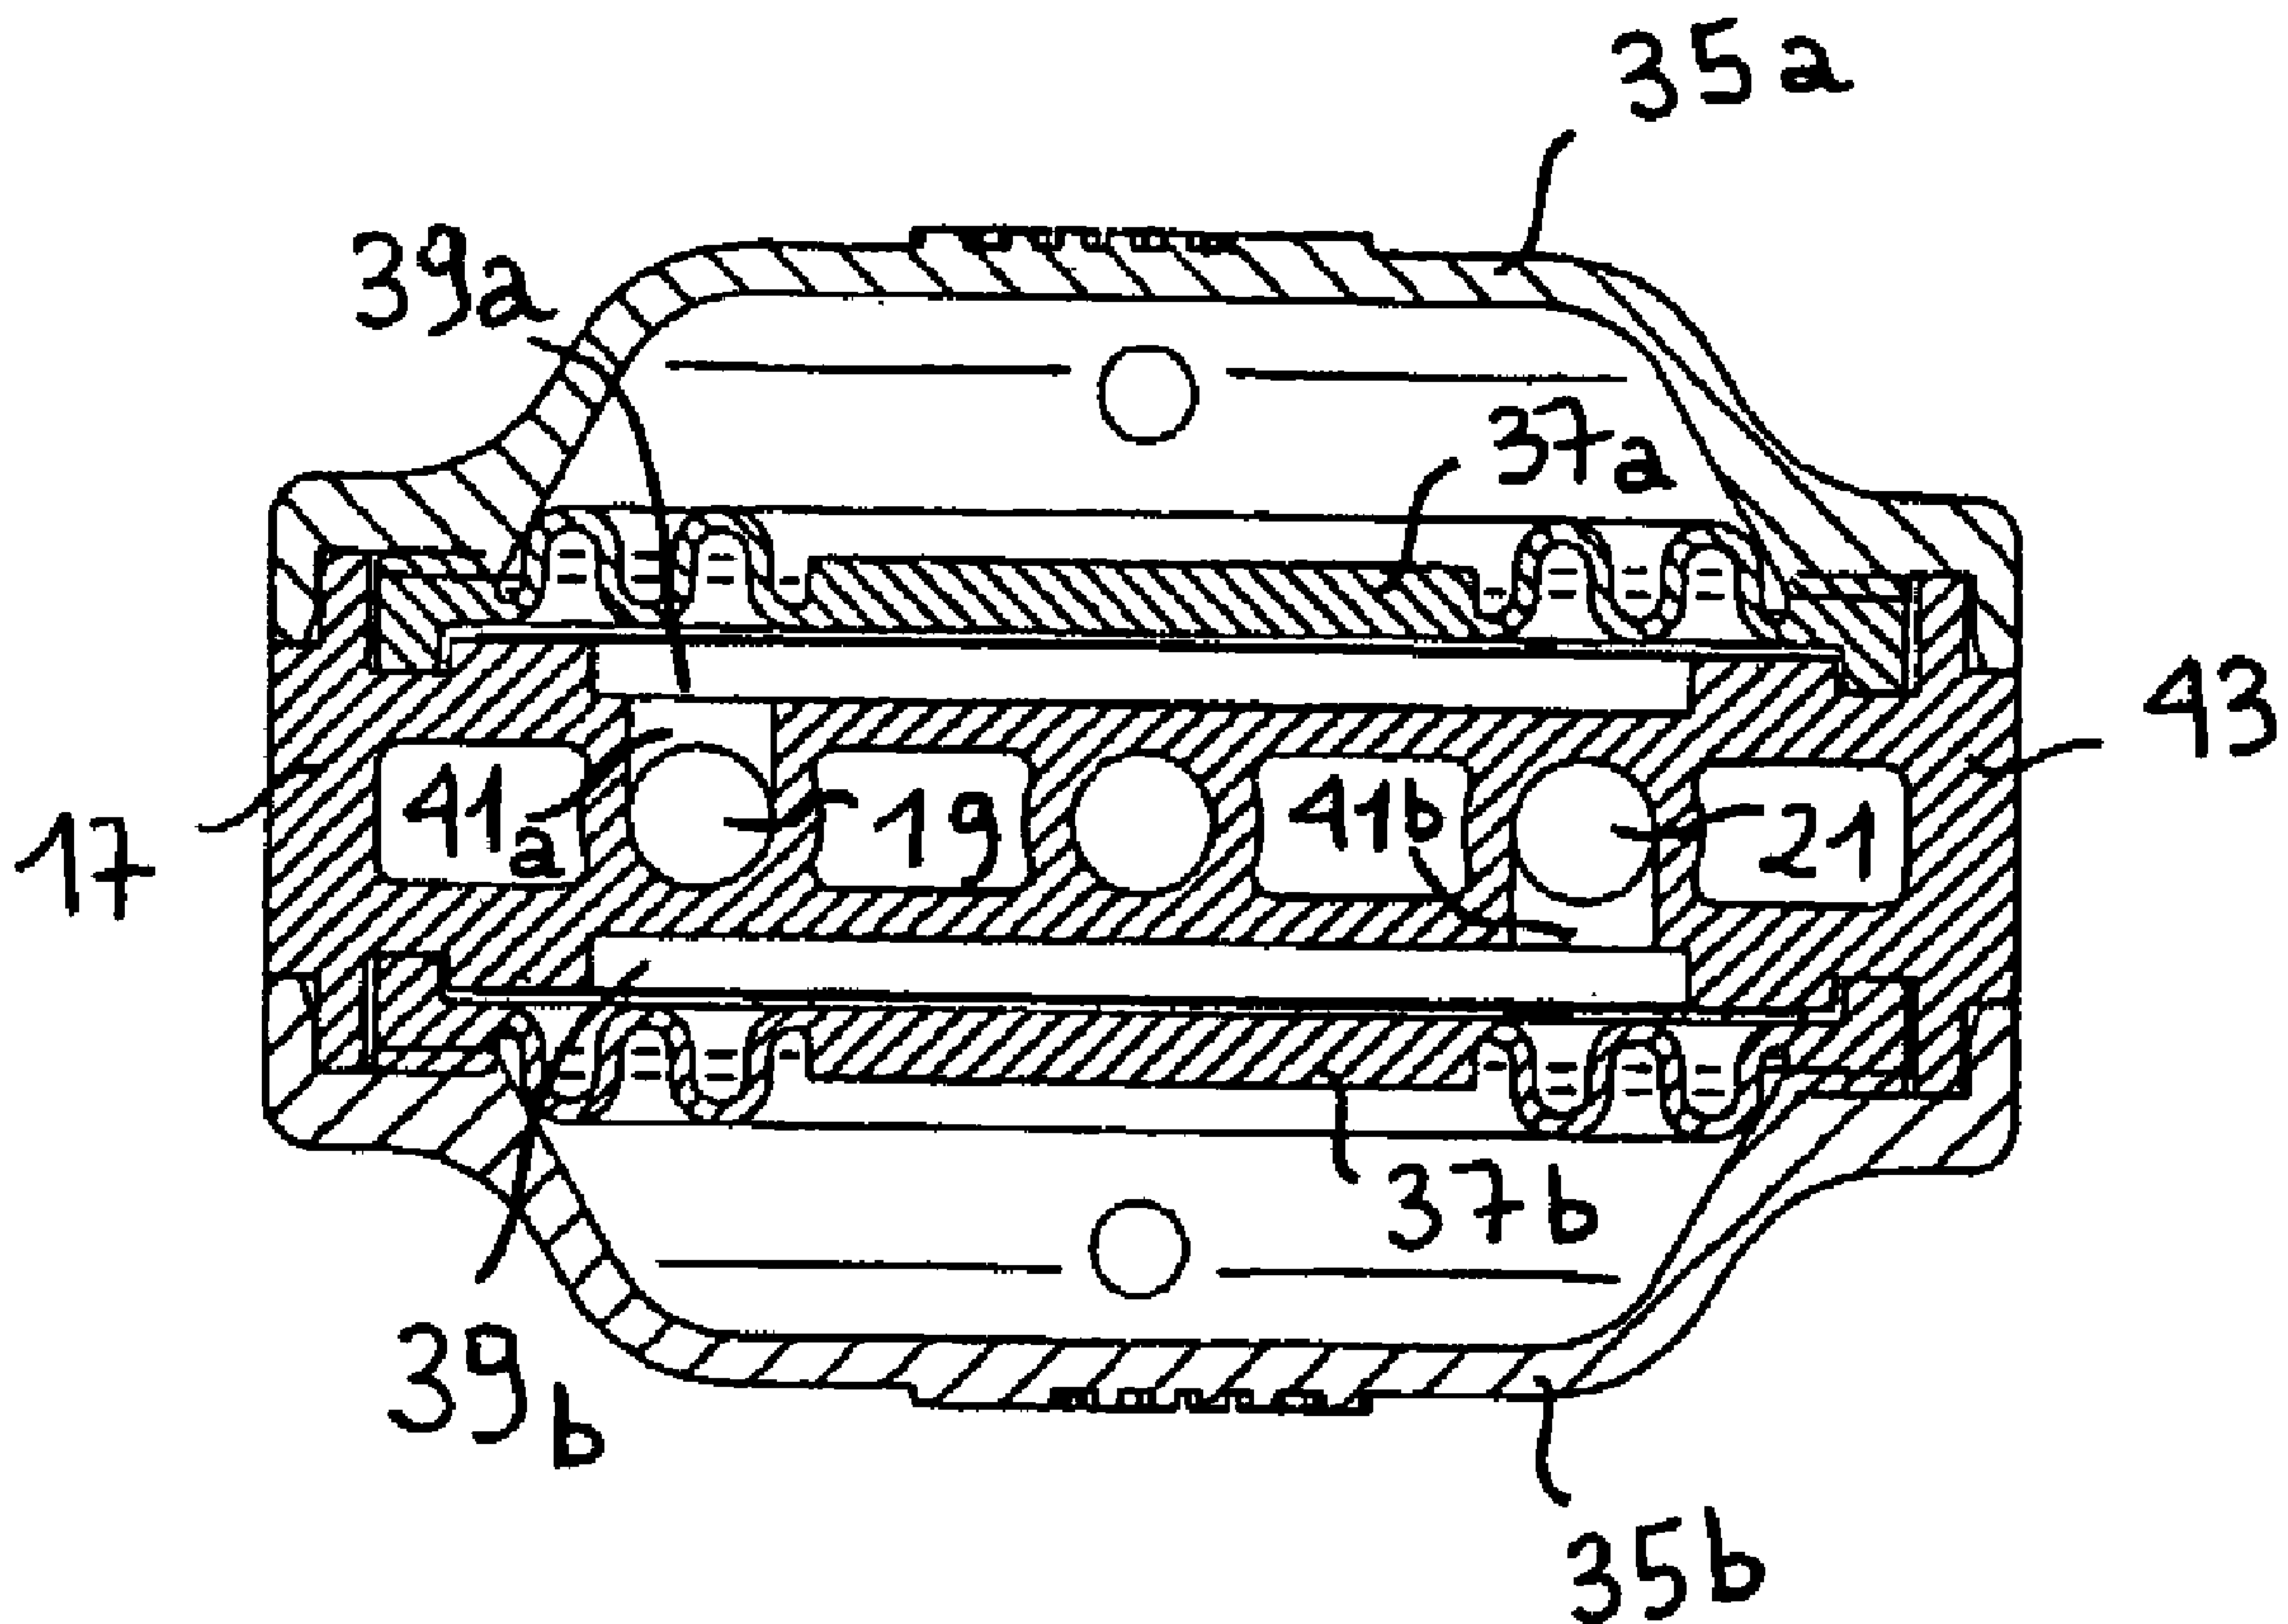

(57) Abrégé/Abstract:

The inventive pressure transmitting connector, in particular for an endoscopy system comprises a fluid transporting channel (19, 21), a blind compartment (39a, 39b) which open (41a, 41b) towards the transport channels (19, 21) by a pipe (41a, 41b) and



(57) Abrégé(suite)/Abstract(continued):

closed by a membrane (37a, 37b) which is deformable according to a pressure in said transport channels (19, 21) and means for transmitting a representative quantity of the pressure in the transport channel according to the membrane deformation. According to said invention, the transport channel (19, 21), the pipe (41a, 41b) and the blind compartment (39a, 39b) are embodied in the same rigid part (43) to which the membrane (37a, 37b) is attached. In a preferred embodiment, the membrane (37a, 37b) simultaneously closes the blind compartment (39a, 39b) and a pressure transmitting chamber (35a, 35b) attached to said rigid part (43).

(12) DEMANDE INTERNATIONALE PUBLIÉE EN VERTU DU TRAITÉ DE COOPÉRATION
EN MATIÈRE DE BREVETS (PCT)(19) Organisation Mondiale de la Propriété
Intellectuelle
Bureau international(43) Date de la publication internationale
15 septembre 2005 (15.09.2005)

PCT

(10) Numéro de publication internationale
WO 2005/084524 A1(51) Classification internationale des brevets⁷ :
A61B 1/015, 1/12(21) Numéro de la demande internationale :
PCT/CH2005/000127

(22) Date de dépôt international : 3 mars 2005 (03.03.2005)

(25) Langue de dépôt : français

(26) Langue de publication : français

(30) Données relatives à la priorité :
0402238 4 mars 2004 (04.03.2004) FR(71) Déposant (pour tous les États désignés sauf US) : **FUTURE MEDICAL SYSTEM S.A.** [CH/CH]; 38, chemin du Grand Puits, CH-1217 Meyrin (CH).

(72) Inventeurs; et

(75) Inventeurs/Déposants (pour US seulement) : **FRANCISCO, André** [FR/FR]; 3, rue Soubeirane, F-06560 Sophia Antipolis (FR). **JANIN, Patrick** [US/FR]; 47, Corniche des Oliviers, F-06000 Nice (FR). **PASCUAL,****Thierry** [FR/FR]; Résidence Méditerranée Bât. B, 4, avenue des Mimosas, F-06800 Cagnes-Sur-Mer (FR). **DIAS, Armando** [FR/FR]; Résidence Bella Vista, 2642, route de Saint-Jeannet, F-06700 Saint Laurent Du Var (FR).(74) Mandataires : **GAGLIONE, Renaud** etc.; Moinas & Savoye SA, 42, rue Plantamour, CH-1201 Genève (CH).


(81) États désignés (sauf indication contraire, pour tout titre de protection nationale disponible) : AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) États désignés (sauf indication contraire, pour tout titre de protection régionale disponible) : ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,

[Suite sur la page suivante]

(54) Title: PRESSURE TRANSMITTING CONNECTOR FOR AN ENDOSCOPY SYSTEM

(54) Titre : CONNECTEUR A DETECTEUR DE PRESSION DESTINE A UN SYSTEME D'ENDOSCOPIE

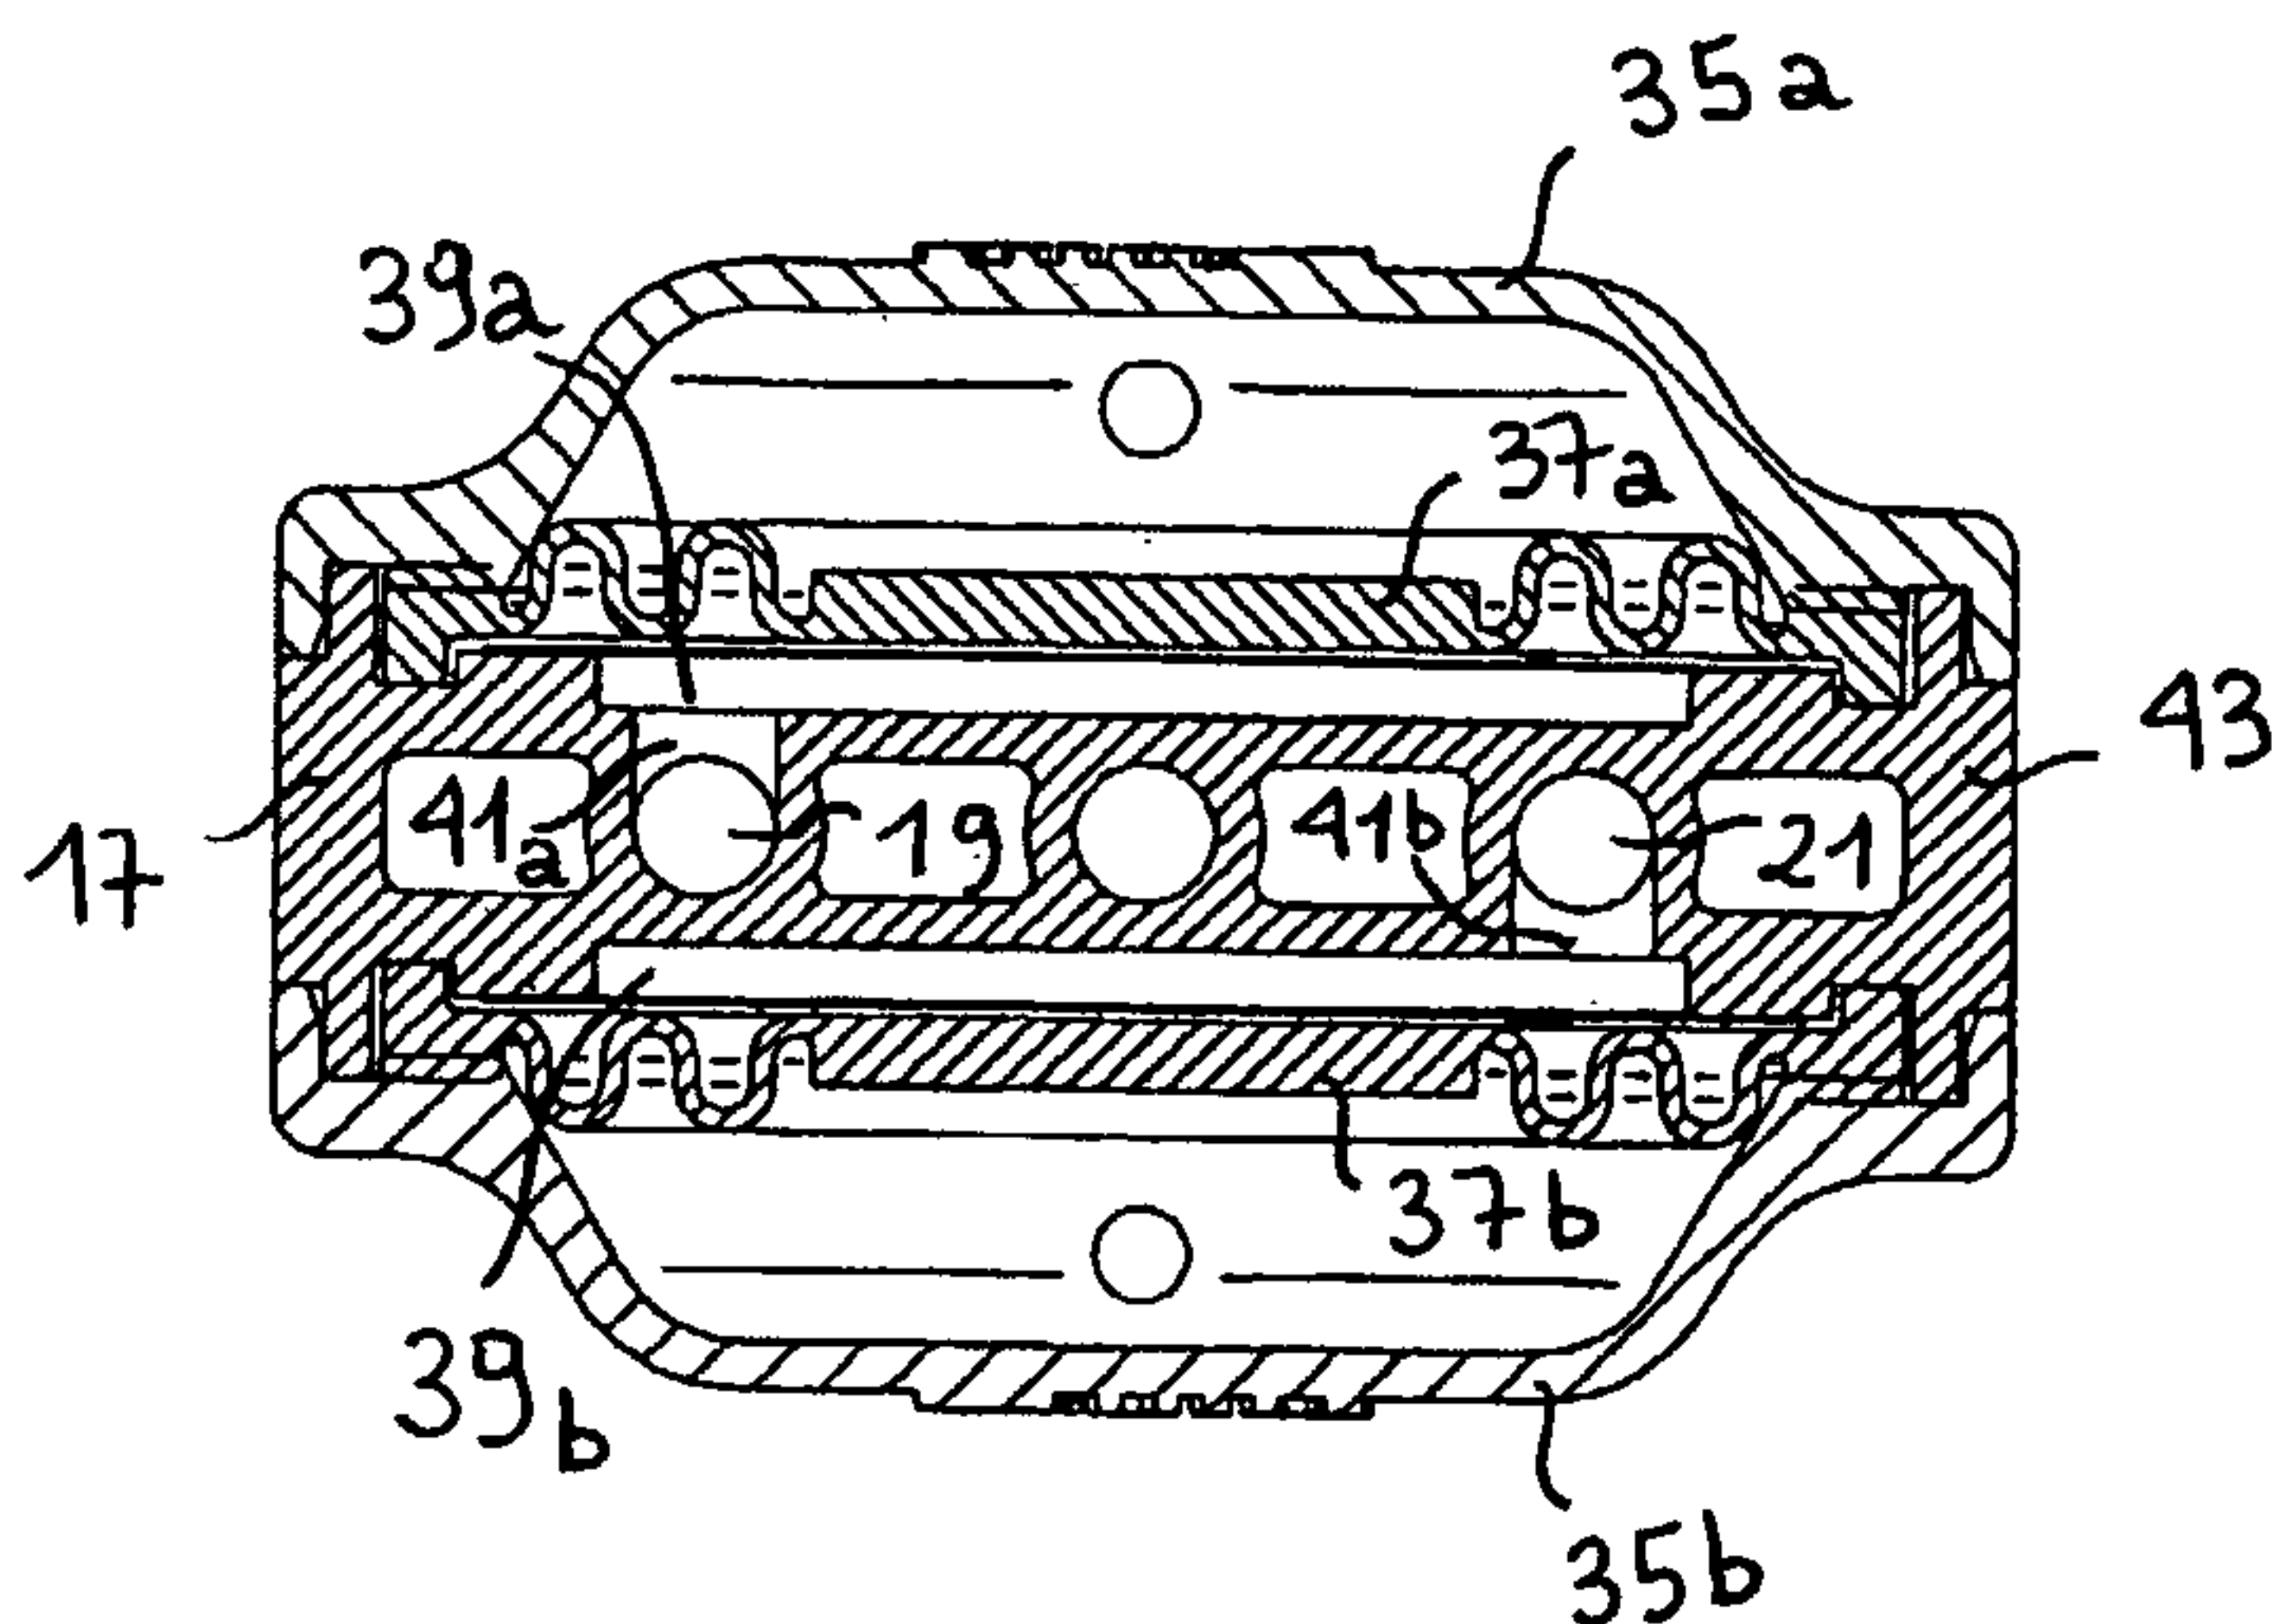

(57) Abstract: The inventive pressure transmitting connector, in particular for an endoscopy system comprises a fluid transporting channel (19, 21), a blind compartment (39a, 39b) which open (41a, 41b) towards the transport channels (19, 21) by a pipe (41a, 41b) and closed by a membrane (37a, 37b) which is deformable according to a pressure in said transport channels (19, 21) and means for transmitting a representative quantity of the pressure in the transport channel according to the membrane deformation. According to said invention, the transport channel (19, 21), the pipe (41a, 41b) and the blind compartment (39a, 39b) are embodied in the same rigid part (43) to which the membrane (37a, 37b) is attached. In a preferred embodiment, the membrane (37a, 37b) simultaneously closes the blind compartment (39a, 39b) and a pressure transmitting chamber (35a, 35b) attached to said rigid part (43).

(57) Abrégé : Connecteur à détection de pression destiné plus particulièrement à un système d'endoscopie, comprenant une voie de communication à fluide (19, 21), un compartiment borgne (39a, 39b) ouvert (41a, 41b) sur la voie de communication (19, 21) par un conduit (41a, 41b) et fermé par une membrane (37a, 37b) se déformant en fonction d'une pression dans la voie de communication (19, 21) et un moyen pour transmettre une grandeur représentative de la pression dans la voie de communication en fonction de la déformation de la membrane. Selon l'invention, la voie de communication (19, 21), le conduit (41a, 41b) et le compartiment borgne (39a, 39b) sont formés dans une même pièce rigide (43) sur laquelle la membrane (37a, 37b) est rapportée. De préférence, la membrane (37a, 37b) ferme à la fois le compartiment borgne (39a, 39b) et une chambre à transmission de pression (35a, 35b) rapportée sur la pièce rigide (43).

WO 2005/084524 A1

WO 2005/084524 A1



ZW), eurasien (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), européen (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

En ce qui concerne les codes à deux lettres et autres abréviations, se référer aux "Notes explicatives relatives aux codes et abréviations" figurant au début de chaque numéro ordinaire de la Gazette du PCT.

Publiée :

— avec rapport de recherche internationale

PRESSURE TRANSMITTING CONNECTOR FOR AN ENDOSCOPY SYSTEM**Technical field**

[0001] The invention relates to a pressure-sensing
5 connector intended more particularly for an endoscopy
system, comprising a fluid communication path, a blind
compartment opening onto the communication path via a
duct and closed off by a membrane that deforms
according to the pressure in the communication path,
10 and a means for transmitting the deformation of the
membrane in the form of a quantity representative of
the pressure in the communication path.

Prior art

15 [0002] An endoscopy system comprising more
particularly a cannula for housing an endoscope and for
forming, between the cannula and the endoscope, an
irrigation or outflow channel, is described for example
by documents US 5 037 386 and US 6 086 542. The system
20 also includes a coupling ring mounted around the
cannula and provided with a coupling path for
communicating with the irrigation or outflow channel.
It is used in joint arthroscopy and more particularly
in knee arthroscopy. The endoscope is connected to a
25 video screen in order to display the joint. The
irrigation or outflow channel makes it possible to
create a circulation of physiological saline in order
to keep the medium in front of the endoscope optically
clear and to bathe the joint. The circulation is
30 provided by a pump connected to a reservoir and
discharging into a tubing connected to the irrigation
or outflow channel via the coupling ring.

[0003] The pressure of the physiological saline in the
35 joint is controlled by a membrane pressure sensor
placed in a tubing connected via the coupling ring to a
channel formed in the cannula and dedicated to pressure

sensing.

[0004] This arrangement has the drawback of resulting in the pressure being erroneously determined under
5 certain operating conditions, for example by accident there is a sharp bend in the tubing between the pressure sensor and the coupling ring.

[0005] Document US 5 044 203 discloses a membrane
10 pressure sensor to be connected to such a tubing. The sensor comprises a rigid communication path provided with an opening for communicating with a blind compartment in the form of a flexible tube connected around the communication path. Two oil-filled chambers
15 are placed around the blind compartment in such a way that two membranes fixed to the transmission chambers are brought into contact with two portions of the blind compartment consisting of two other membranes. A fluid circulating in the communication path enters the blind
20 compartment via the opening and deforms the membranes of the blind compartment and of the two transmission chambers. The oil pressure, which depends on the deformation of the membranes, is transmitted to sensors mounted on each oil pressure chamber in order to
25 determine the pressure in the communication path.

[0006] This arrangement has the drawback in which the blind compartment in the form of a flexible tube may itself be deformed on its walls and thus introduce a
30 source of error in the determination of the pressure compared with what it would be if the deformation of the membranes were to result only from the effect of the pressure in the communication path.

35 [0007] Document US 5 643 203 discloses an endoscopy system of the type mentioned above, in which a connector is mounted on the coupling ring and comprises a communication path for communicating with the

irrigation channel and a pressure sensor for sensing the pressure in the communication path. The pressure of the physiological saline in the joint is extrapolated using a law based on the pressure sensed in the communication path.

[0008] The extrapolation of the pressure in the joint on the basis of the pressure sensed in the communication path of the connector makes it possible to dispense with one channel in the cannula dedicated for pressure sensing. Thus it is possible to decrease the diameter of the cannula, for the purpose of reducing the trauma when it is being introduced into the joint. Compared to a tubing, the connector thus eliminates the risk of a variation in cross section of the communication path and allows reliable sensing of the pressure in this communication path.

[0009] The connector is a rigid part comprising a fluid communication path and a duct perpendicular to the communication path. A pressure sensor is attached to the connector. It comprises a blind compartment designed to be placed facing the duct so as to open into the communication path. A membrane placed in the blind compartment is connected to a piezoelectric transducer in order to convert a deformation due to the pressure in the communication path into an electrical voltage.

[0010] This arrangement has the drawback whereby, during assembly, it is necessary for the duct formed in the connector and the blind compartment formed in the piezoelectric transducer sensor to be positioned precisely.

[0011] The object of the invention is to modify a connector known from the prior art, illustrated above, in order to simplify the assembly.

- 4 -

Disclosure of the invention

According to the present invention, there is provided a pressure-sensing connector for an endoscopy system, comprising:

- 5 two fluid communication paths,
 two blind compartments, each of said blind compartments opening onto one of the communication paths and being closed off by a respective membrane that deforms according to a pressure in the respective communication path, and
10 a means for transmitting quantities representative of the pressure in each of said communication paths according to the deformation of the respective membrane,
 wherein each blind compartment opens onto its respective communication path via a respective duct,
15 wherein the communication paths, the ducts and the blind compartments are formed in the same rigid part to which the membranes are attached, and
 wherein said membranes move independently from one another so that the pressure in each blind compartment can be
20 sensed independently.


- [0012] Preferably, for this purpose, the subject of the invention is a pressure-sensing connector intended more particularly for an endoscopy system, comprising a fluid communication path, a blind compartment that opens onto the
25 communication path via a duct and is closed off by a membrane that deforms according to the pressure in the communication path, and a means for transmitting a quantity representative of the pressure in the communication path according to the deformation of the membrane, characterized in that the
30 communication path, the duct and the blind compartment are

4a

formed in the same rigid part to which the membrane is attached.

5 [0013] Mounting the membrane on the blind compartment, in order for the latter to be closed off, simplifies the assembly of the connector according to the invention. In addition, the rigid part, in which the communication path, the duct and the blind compartment are formed, can be easily cleaned before mounting the membrane. Finally, the fully assembled connector
10 is easily sterilized.

[0014] In a preferred embodiment of the invention, the membrane closes off both the blind compartment and a pressure-transmitting chamber, preferably filled with air and connected
15 to the rigid part, in order to transmit the deformation of the membrane in the form of an air pressure. Compared to a piezoelectric transducer, this arrangement eliminates the risk of any deterioration during an operation to sterilize the connector. Compared to oil transmission, this arrangement also
20 eliminates the risks of contaminating the blind compartment and the communication path of the connector, and also the irrigation or outflow channel.

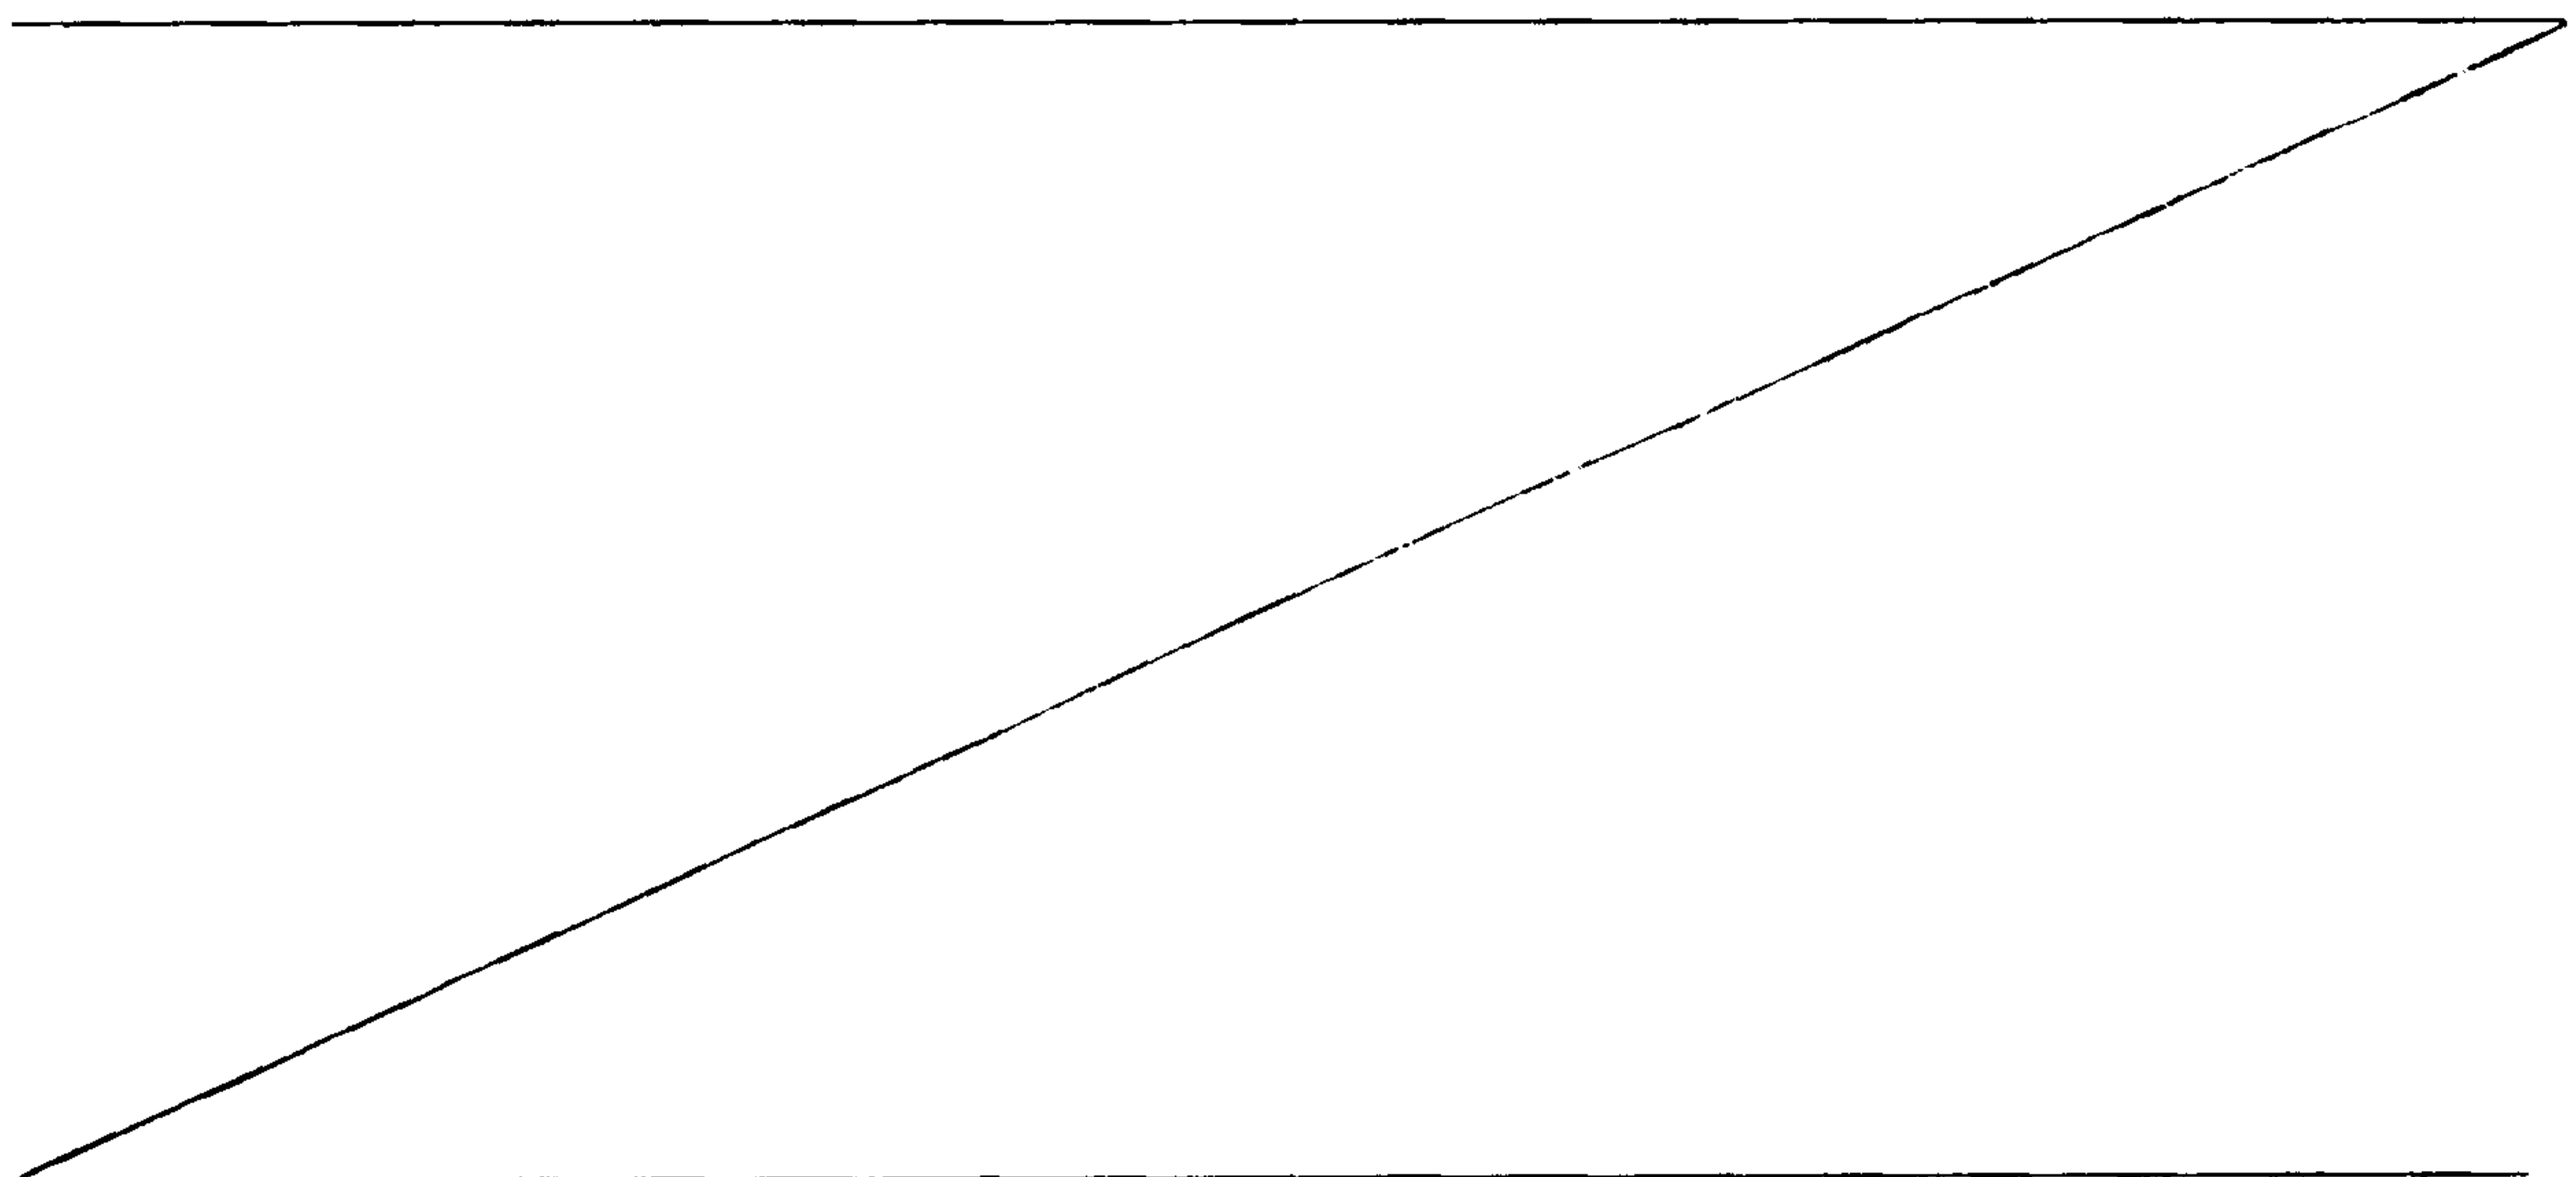

Brief description of the drawings

[0015] The invention will become apparent on reading the description of one embodiment illustrated below by the drawings.

5

[0016]

Figure 1 shows an endoscopy system in front view.

Figure 2 shows the endoscopy system of figure 1 in top view.

10 Figure 3 shows the endoscopy system of figure 1 in longitudinal section.

Figure 4 shows the endoscopy system of figure 1 in cross section.

15 Figure 5 shows, in perspective, a connector according to the invention in the position for being connected to a coupling ring of an endoscopy system according to figures 1 to 4.

20 Figure 6 shows a cross section of a first connector intended for an endoscopy system according to the invention.

Figure 7 shows, in cross section, a second connector intended for an endoscopy system according to the invention.

25

Embodiments of the invention and industrial application

[0017] An endoscopy system comprises (figures 1 to 4) a cannula 1 for housing an endoscope 3 and for forming, between the cannula 1 and the endoscope 3, an
30 irrigation channel 5. In the embodiment illustrated by the figures, the irrigation channel 5 is formed between the endoscope 3 and a tube 7 internal to the cannula 1, and an outflow channel 9 is formed between the internal tube 7 and the cannula 1.

35

[0018] A coupling ring 11 is mounted around the cannula 1 in order to communicate with the irrigation channel 5 and the outflow channel 9. A first coupling

- 6 -

path 13 communicates with the irrigation channel 5. A second coupling path 15 communicates with the outflow channel 9.

5 [0019] A connector 17 is mounted on the coupling ring 11. It comprises a first communication path 19, for communicating with the first coupling path 13 at the irrigation channel 5, and a second communication path 21, for communicating with the second coupling path 15
10 at the outflow channel 9. A blind compartment 39a, 39b opens onto each communication path 19, 21 via a duct 41a, 41b. A transmission chamber 35a, 35b provided with a membrane 37a, 37b is designed so that a pressure in the communication path 19, 21 is transmitted to the
15 transmission chamber 35a, 35b by deformation of the membrane.

[0020] Tubings (not shown) are connected to the communication paths 19 and 21 of the connector 17 and
20 are connected to a pump in order to create a flow of fresh physiological saline in the irrigation channel 5 and of soiled physiological saline in the outflow channel 9. The coupling ring 11 comprises, in a manner known per se, taps 23 and 25 for opening or closing the
25 coupling paths 13 and 15 according to the desired flow in the irrigation channel 5 or in the outflow channel 9.

[0021] The connector 17 is mounted on the coupling
30 ring 11 so as to allow the irrigation channel 5 and the outflow channel 9 to communicate with the communication paths 19 and 21 of the connector via a tubing. With this arrangement, the pressure sensed in one or other communication path of the connector is not subject to
35 an error due to an accidental variation in the cross section of the tubings that would be connected to the coupling paths of the coupling ring.

REPLACEMENT SHEET (RULE 26)

- 7 -

[0022] The communication path 19, 21, the duct 41a, 41b and the blind compartment 39a, 39b are formed in the same rigid part 43 to which the membrane 37a, 37b and the transmission chamber are connected, in order to
5 close off the transmission chamber on the blind compartment 39a, 39b by the membrane 37a, 37b.

[0023] The rigid part 43 is provided with fastening means 31 for reversibly connecting (figure 5) the
10 connector 17 to the coupling ring 11. Preferably, the rigid part 43 is provided with a polarizing feature 45, which polarizes the connection to the coupling ring 11. These arrangements allow a surgeon to connect the connector to the coupling ring in an easy and reliable
15 manner.

[0024] The physiological saline flowing in the communication path 19 with the irrigation channel 5, or in the communication path 21 with the outflow channel
20 9, enters the blind compartment 39a, 39b closed off by the membrane 37a, 37b. The latter 37a, 37b deforms according to the pressure of the physiological saline in the communication path 19 or 21. This deformation causes a variation in the air pressure inside the
25 transmission chamber 35a, 35b. Capillaries (not shown) are connected to connection points 47 of the transmission chambers 35a, 35b in order to transmit the pressure variation to sensors (not shown) and to determine the pressure of the physiological saline in
30 each of the communication paths 19, 21.

[0025] The pressure of the physiological saline in the joint is extrapolated using a law based on the pressure sensed in the communication path. Preferably, a
35 relationship between the fluid flow rate is used, given by the speed of rotation of the irrigation pump, or the outflow pump, and a pressure drop, determined experimentally, between the communication path of the

connector and the mouth of the irrigation or outflow channel.

[0026] In figure 6, each blind compartment 39a, 39b
5 opens onto each respective communication path 19, 21.
This arrangement allows the pressure in each
communication path 19, 21 to be sensed independently.
In this embodiment of the invention, the connector 17
allows, in the endoscopy system described above, two
10 determinations of the pressure of the physiological
saline in the joint, by extrapolation on the basis of
the pressure sensed in the communication path 19 with
the irrigation channel 5 on the one hand, and in the
communication path 21 with the outflow channel 9 on the
15 other. Advantageously, the pressure in the joint may be
extrapolated by means of one 19 of the two
communication paths even when the circulation of the
physiological saline is interrupted in the other 21
communication path by closing the irrigation tap 23, or
20 outflow tap 25 respectively. Also in this arrangement,
the surgeon advantageously connects the coupling ring,
in a single operation, to the communication path for
irrigation and to the communication path for outflow,
while still being able to sense the pressure in each of
25 these two channels.

[0027] The two pressure taps on the two communication
paths of the connector allow the integrity of the
endoscopy system described above to be better checked,
30 by comparing the sensed pressures with expected values
obtained experimentally. Should there be a difference,
a fault in the irrigation tap 23 or the outflow tap 25
may be diagnosed, or else the presence of a foreign
body in the irrigation channel or in the outflow
35 channel may be diagnosed. Advantageously, these checks
will be made by the surgeon at the start of use of the
endoscopy system.

[0028] In figure 7, the two blind compartments 39a, 39b open onto the same communication path, for example 19. This arrangement allows double sensing of the pressure in the communication path 19.

5

[0029] Preferably, the rigid part 43 is manufactured by the injection molding of a plastic. This method of manufacture is advantageous in order to obtain single-use connectors.

10

- 10 -

WHAT IS CLAIMED IS:

1. A pressure-sensing connector for an endoscopy system, comprising:

two fluid communication paths,

two blind compartments, each of said blind compartments opening onto one of the communication paths and being closed off by a respective membrane that deforms according to a pressure in the respective communication path, and

10 a means for transmitting quantities representative of the pressure in each of said communication paths according to the deformation of the respective membrane,

wherein each blind compartment opens onto its respective communication path via a respective duct,

wherein the communication paths, the ducts and the blind compartments are formed in the same rigid part to which the membranes are attached, and

wherein said membranes move independently from one another so that the pressure in each blind compartment can be sensed independently.

20 2. The connector as claimed in claim 1, wherein the two blind compartments open onto the same communication path.

3. The connector as claimed in claim 1, wherein each membrane closes off both said respective blind compartment and a respective pressure-transmitting chamber, connected to the rigid part, in order to convert the deformation of each membrane into a pressure representative of the pressure in the respective communication path.

- 11 -

4. The connector as claimed in claim 3, wherein the pressure-transmitting chambers are totally filled with air in order to convert the deformations of the membranes into air pressures.

5. The connector as claimed in claim 1, wherein the rigid part is provided with a polarizing feature.

6. The connector as claimed in claim 1, wherein the rigid part is made of injection-molded plastic.

7. The connector as claimed in claim 1, wherein said
10 communication paths are located on a same side of the connector so that they can be connected in a single operation to a coupling ring.

1/7

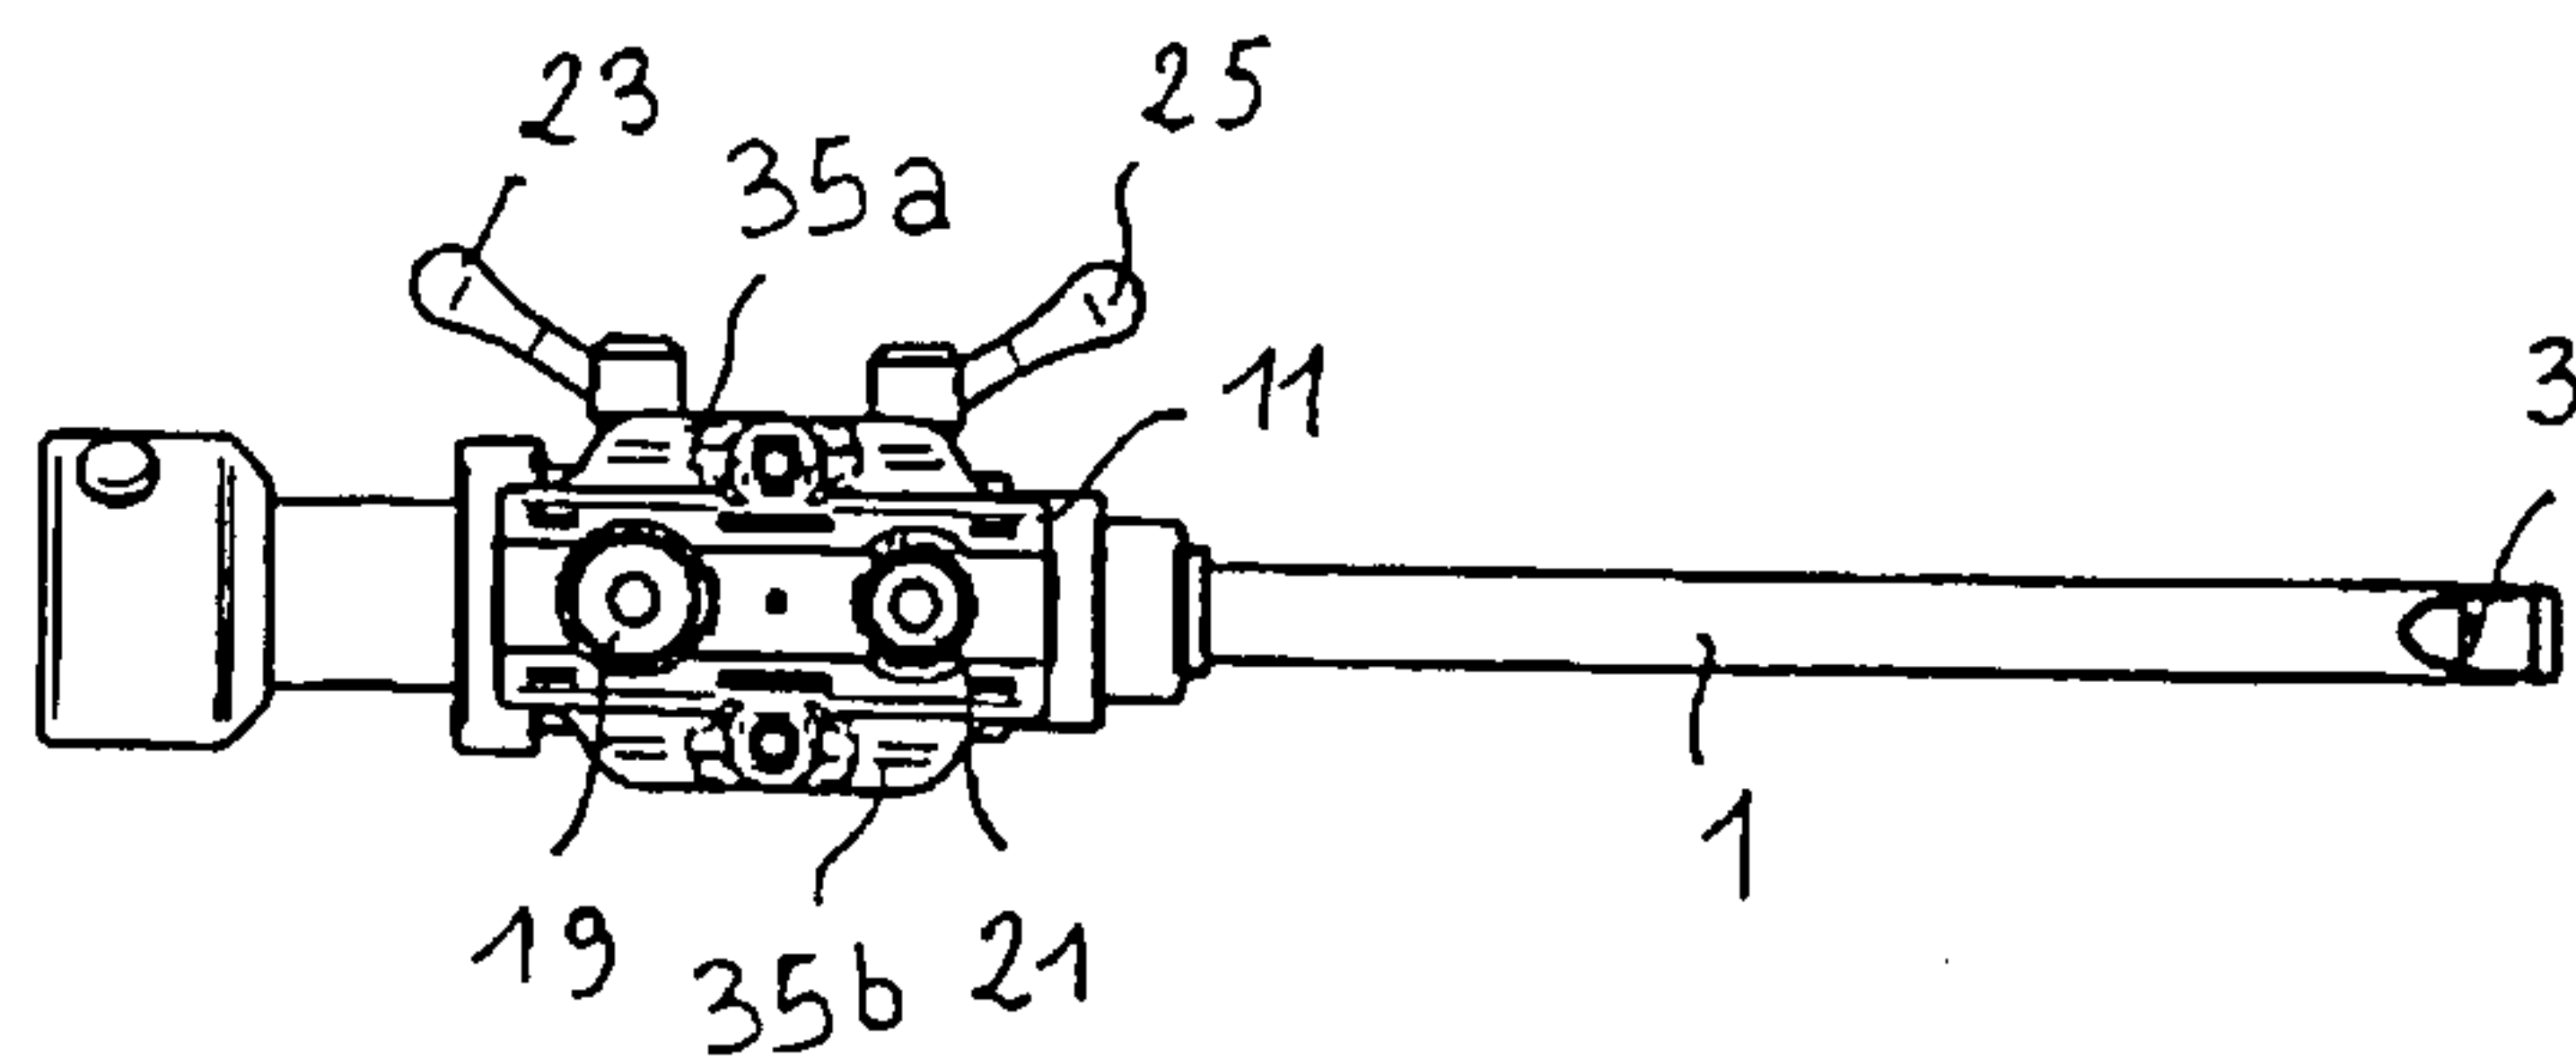


Fig. 1

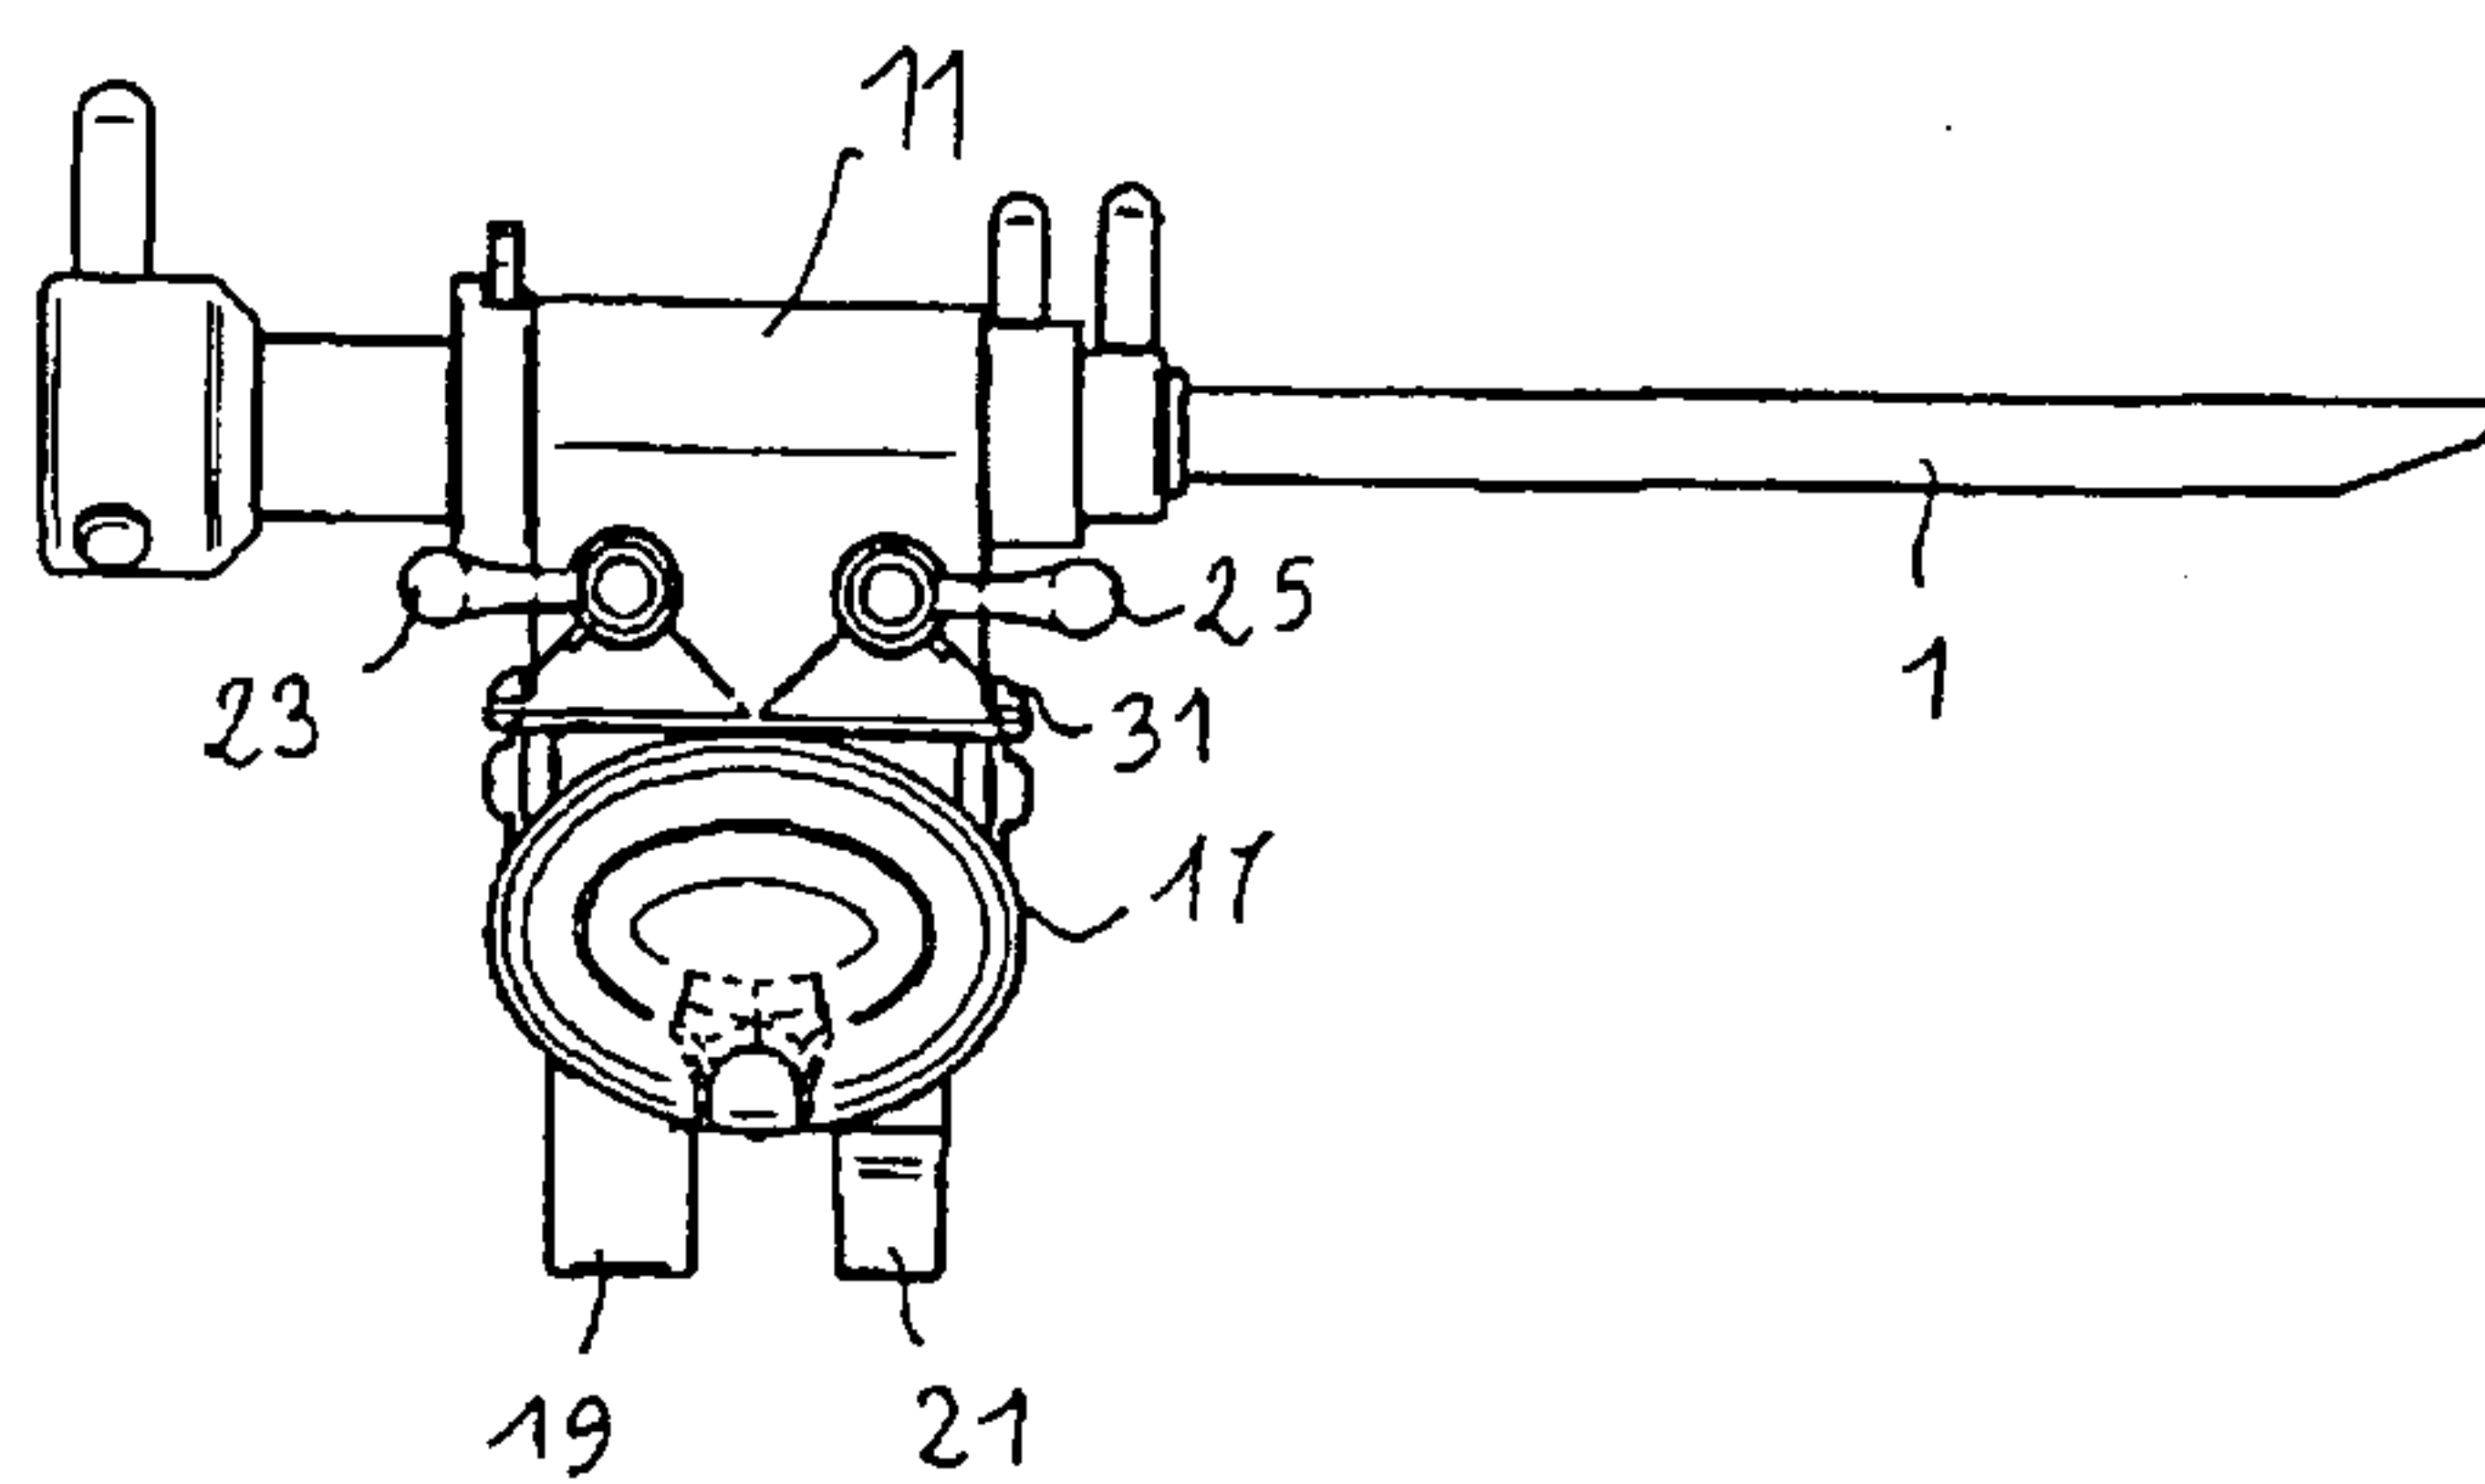


Fig. 2

3/7

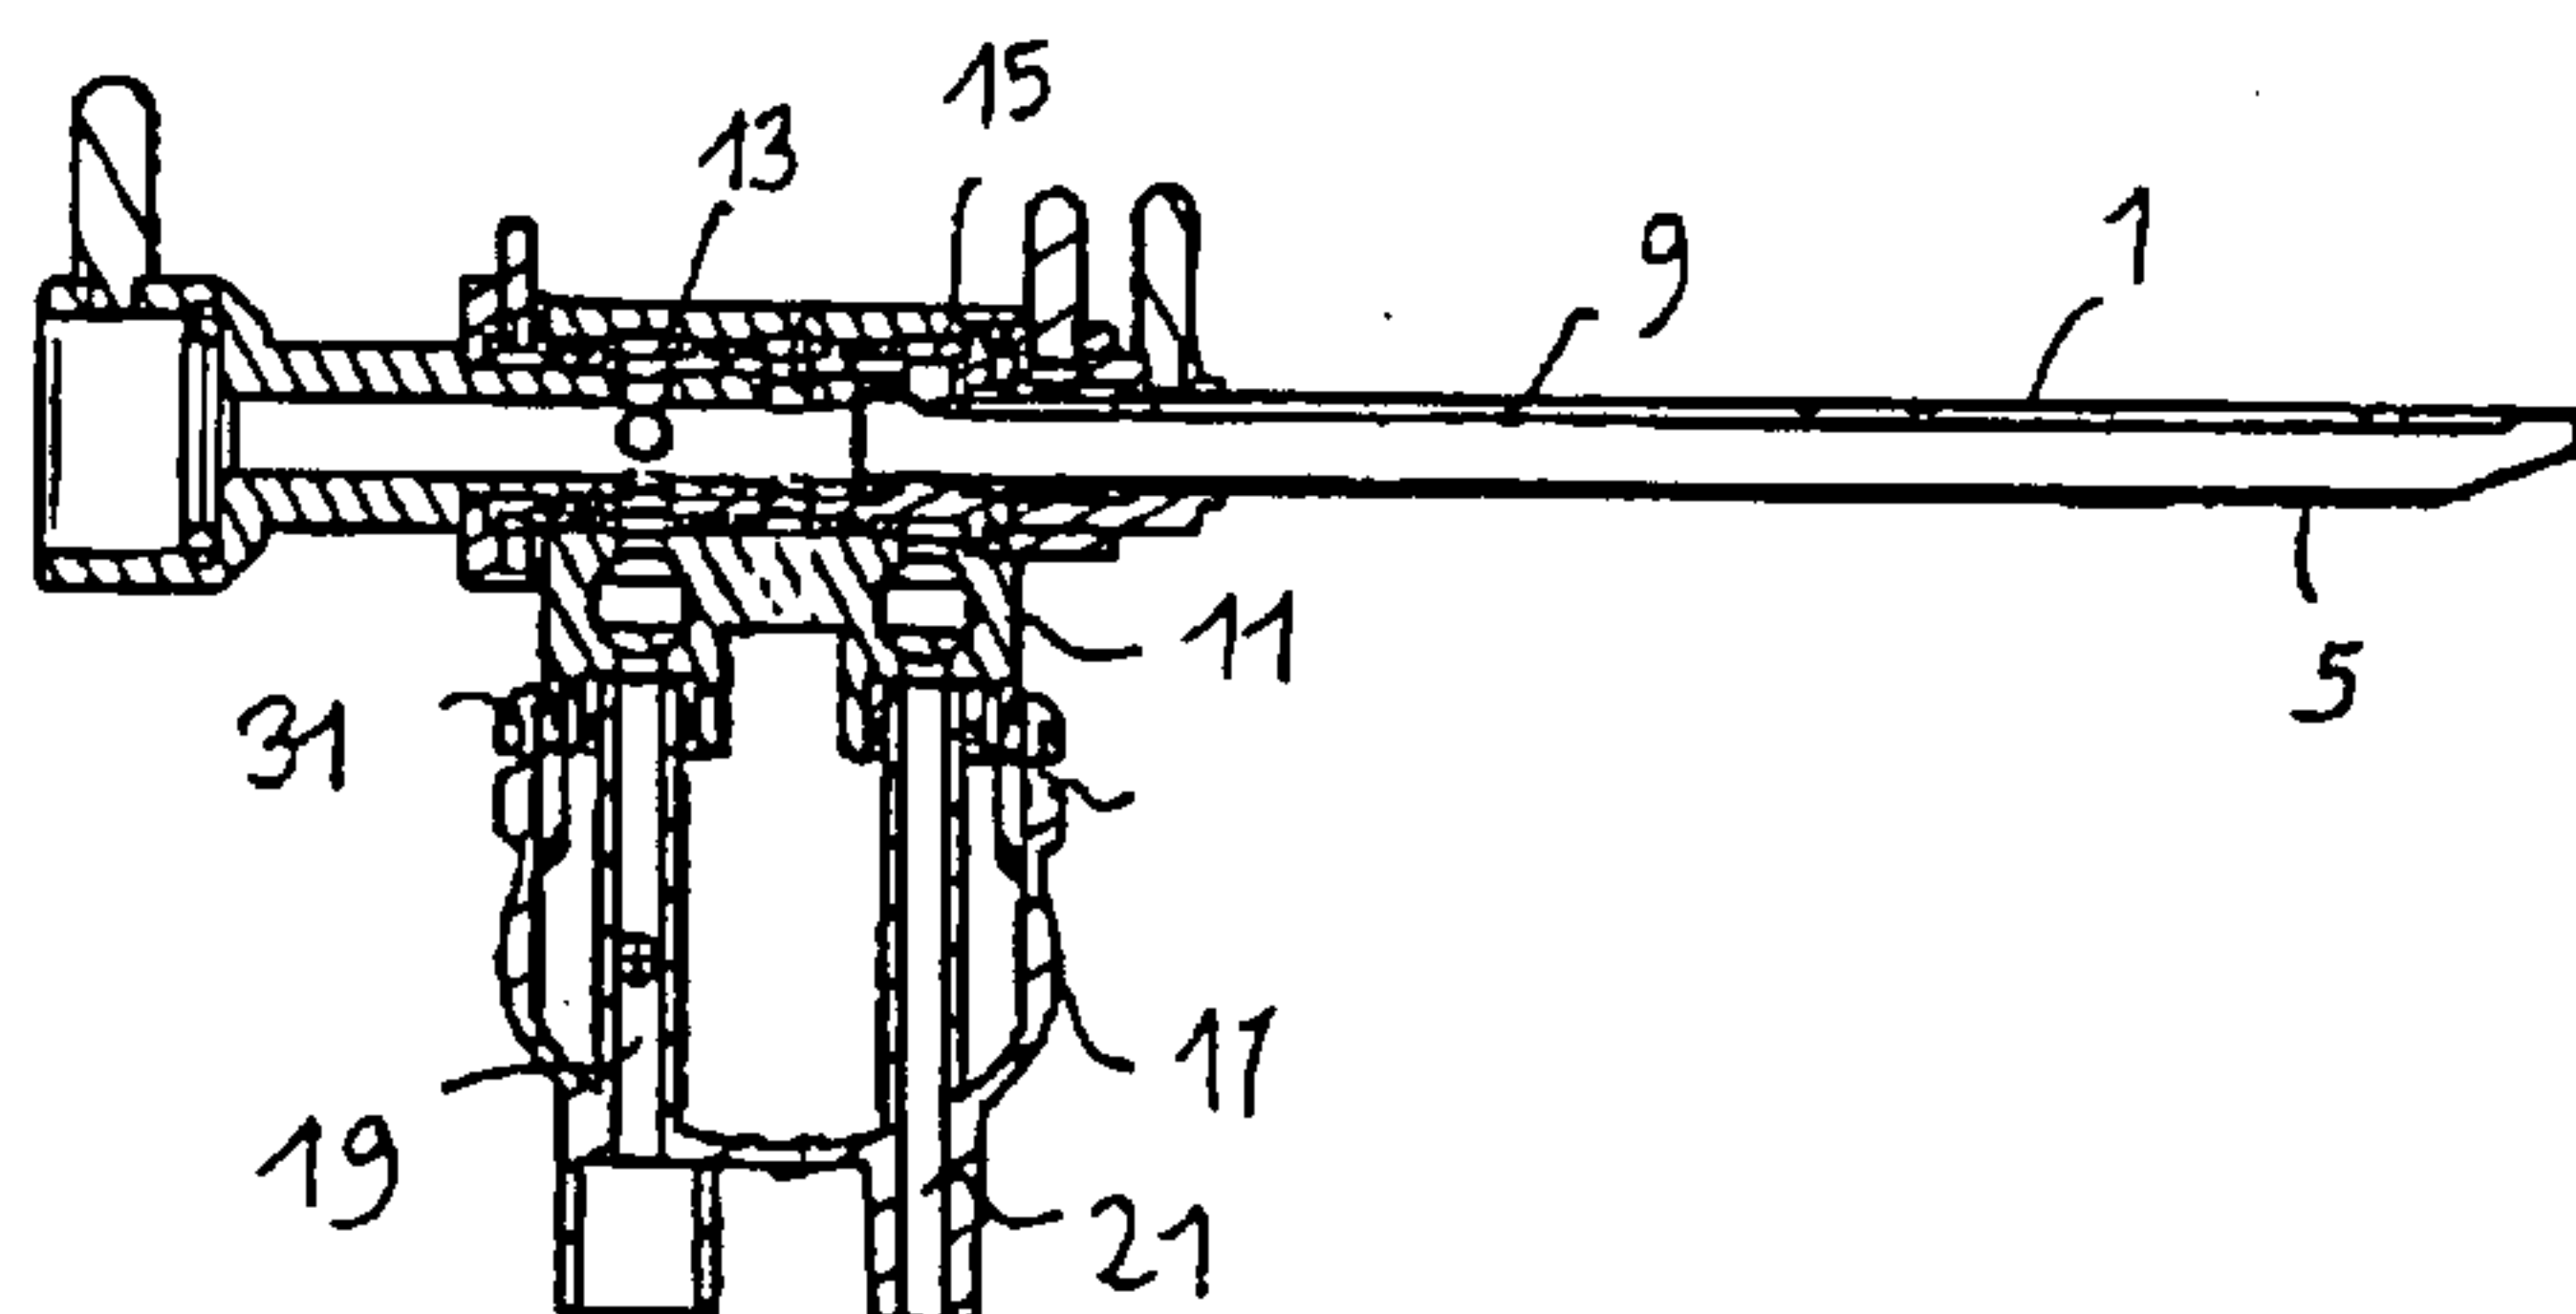


Fig. 3

4/7

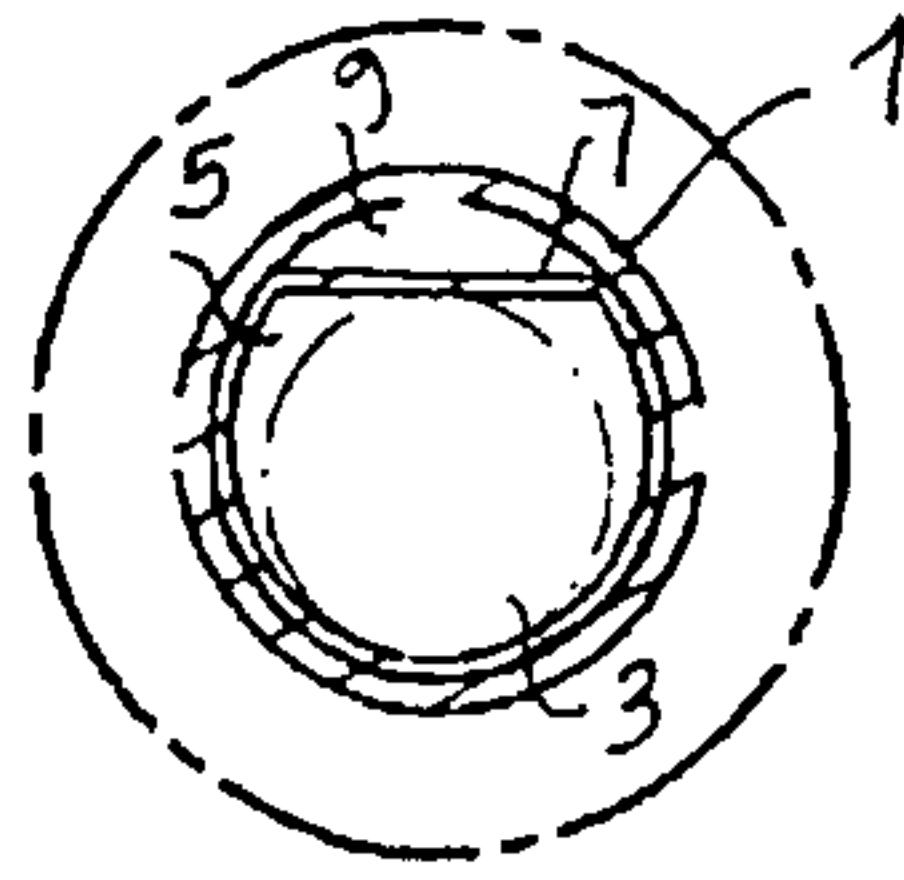


Fig. 4

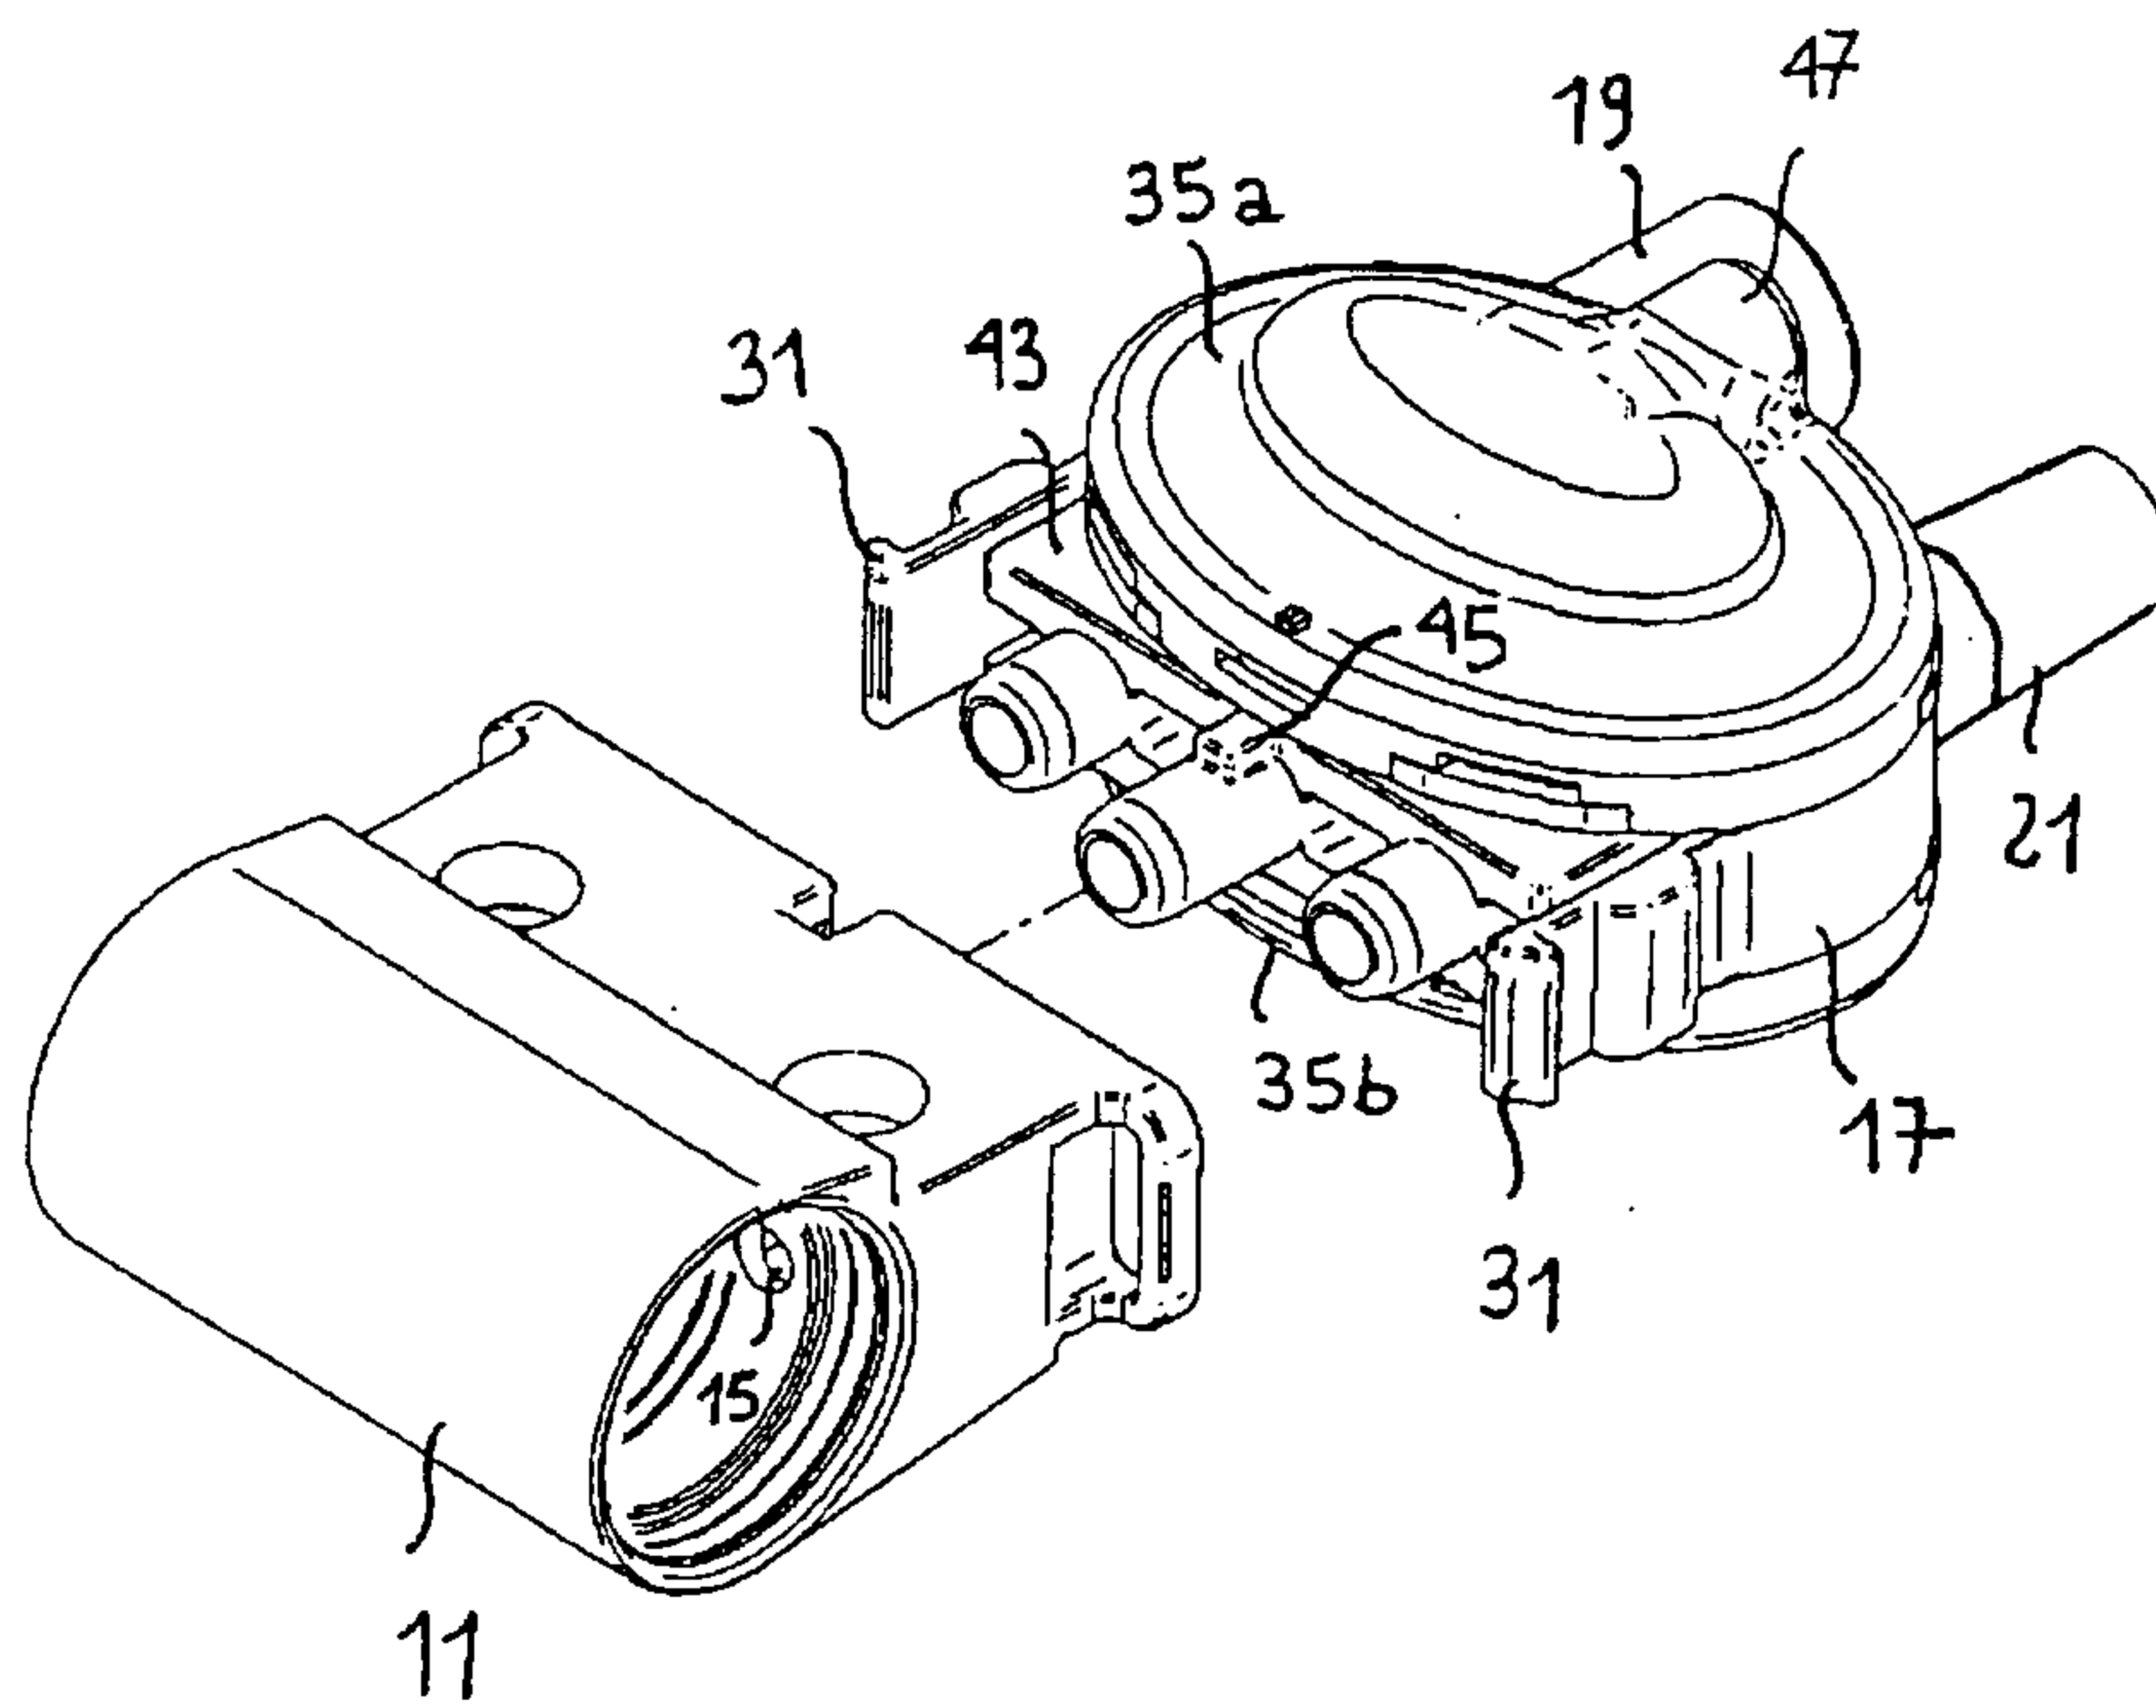


Fig. 5

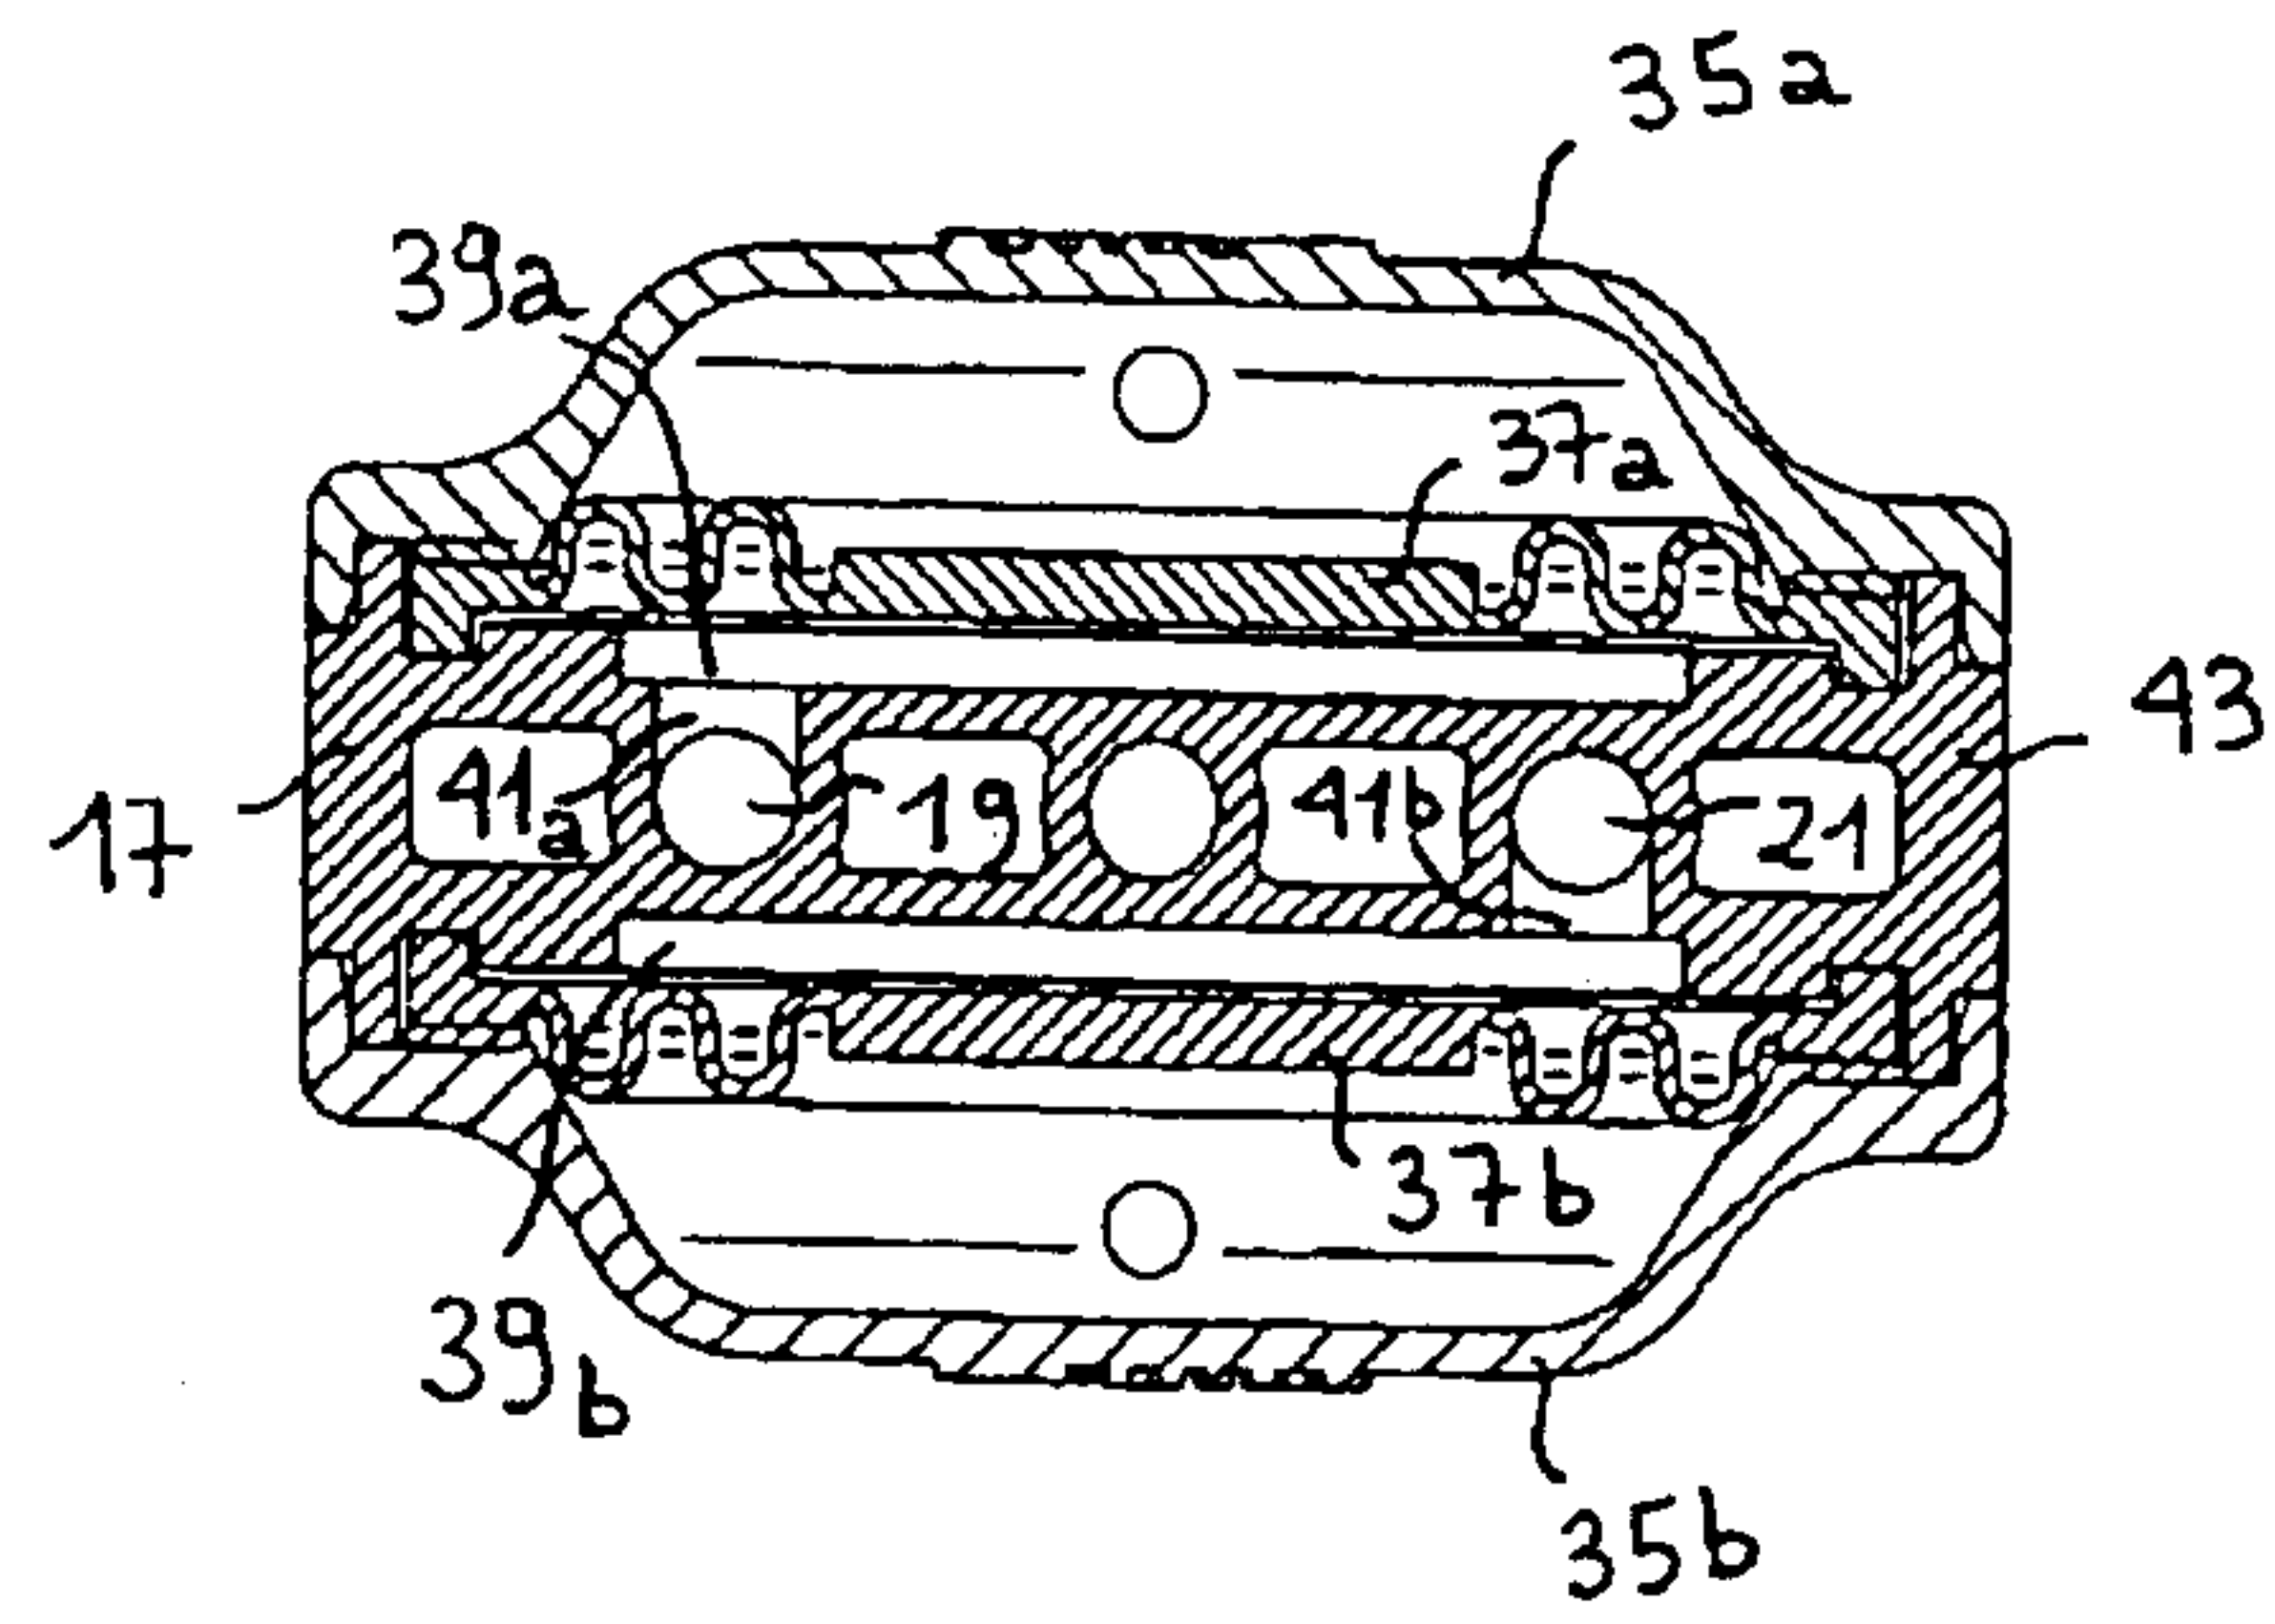


Fig. 6

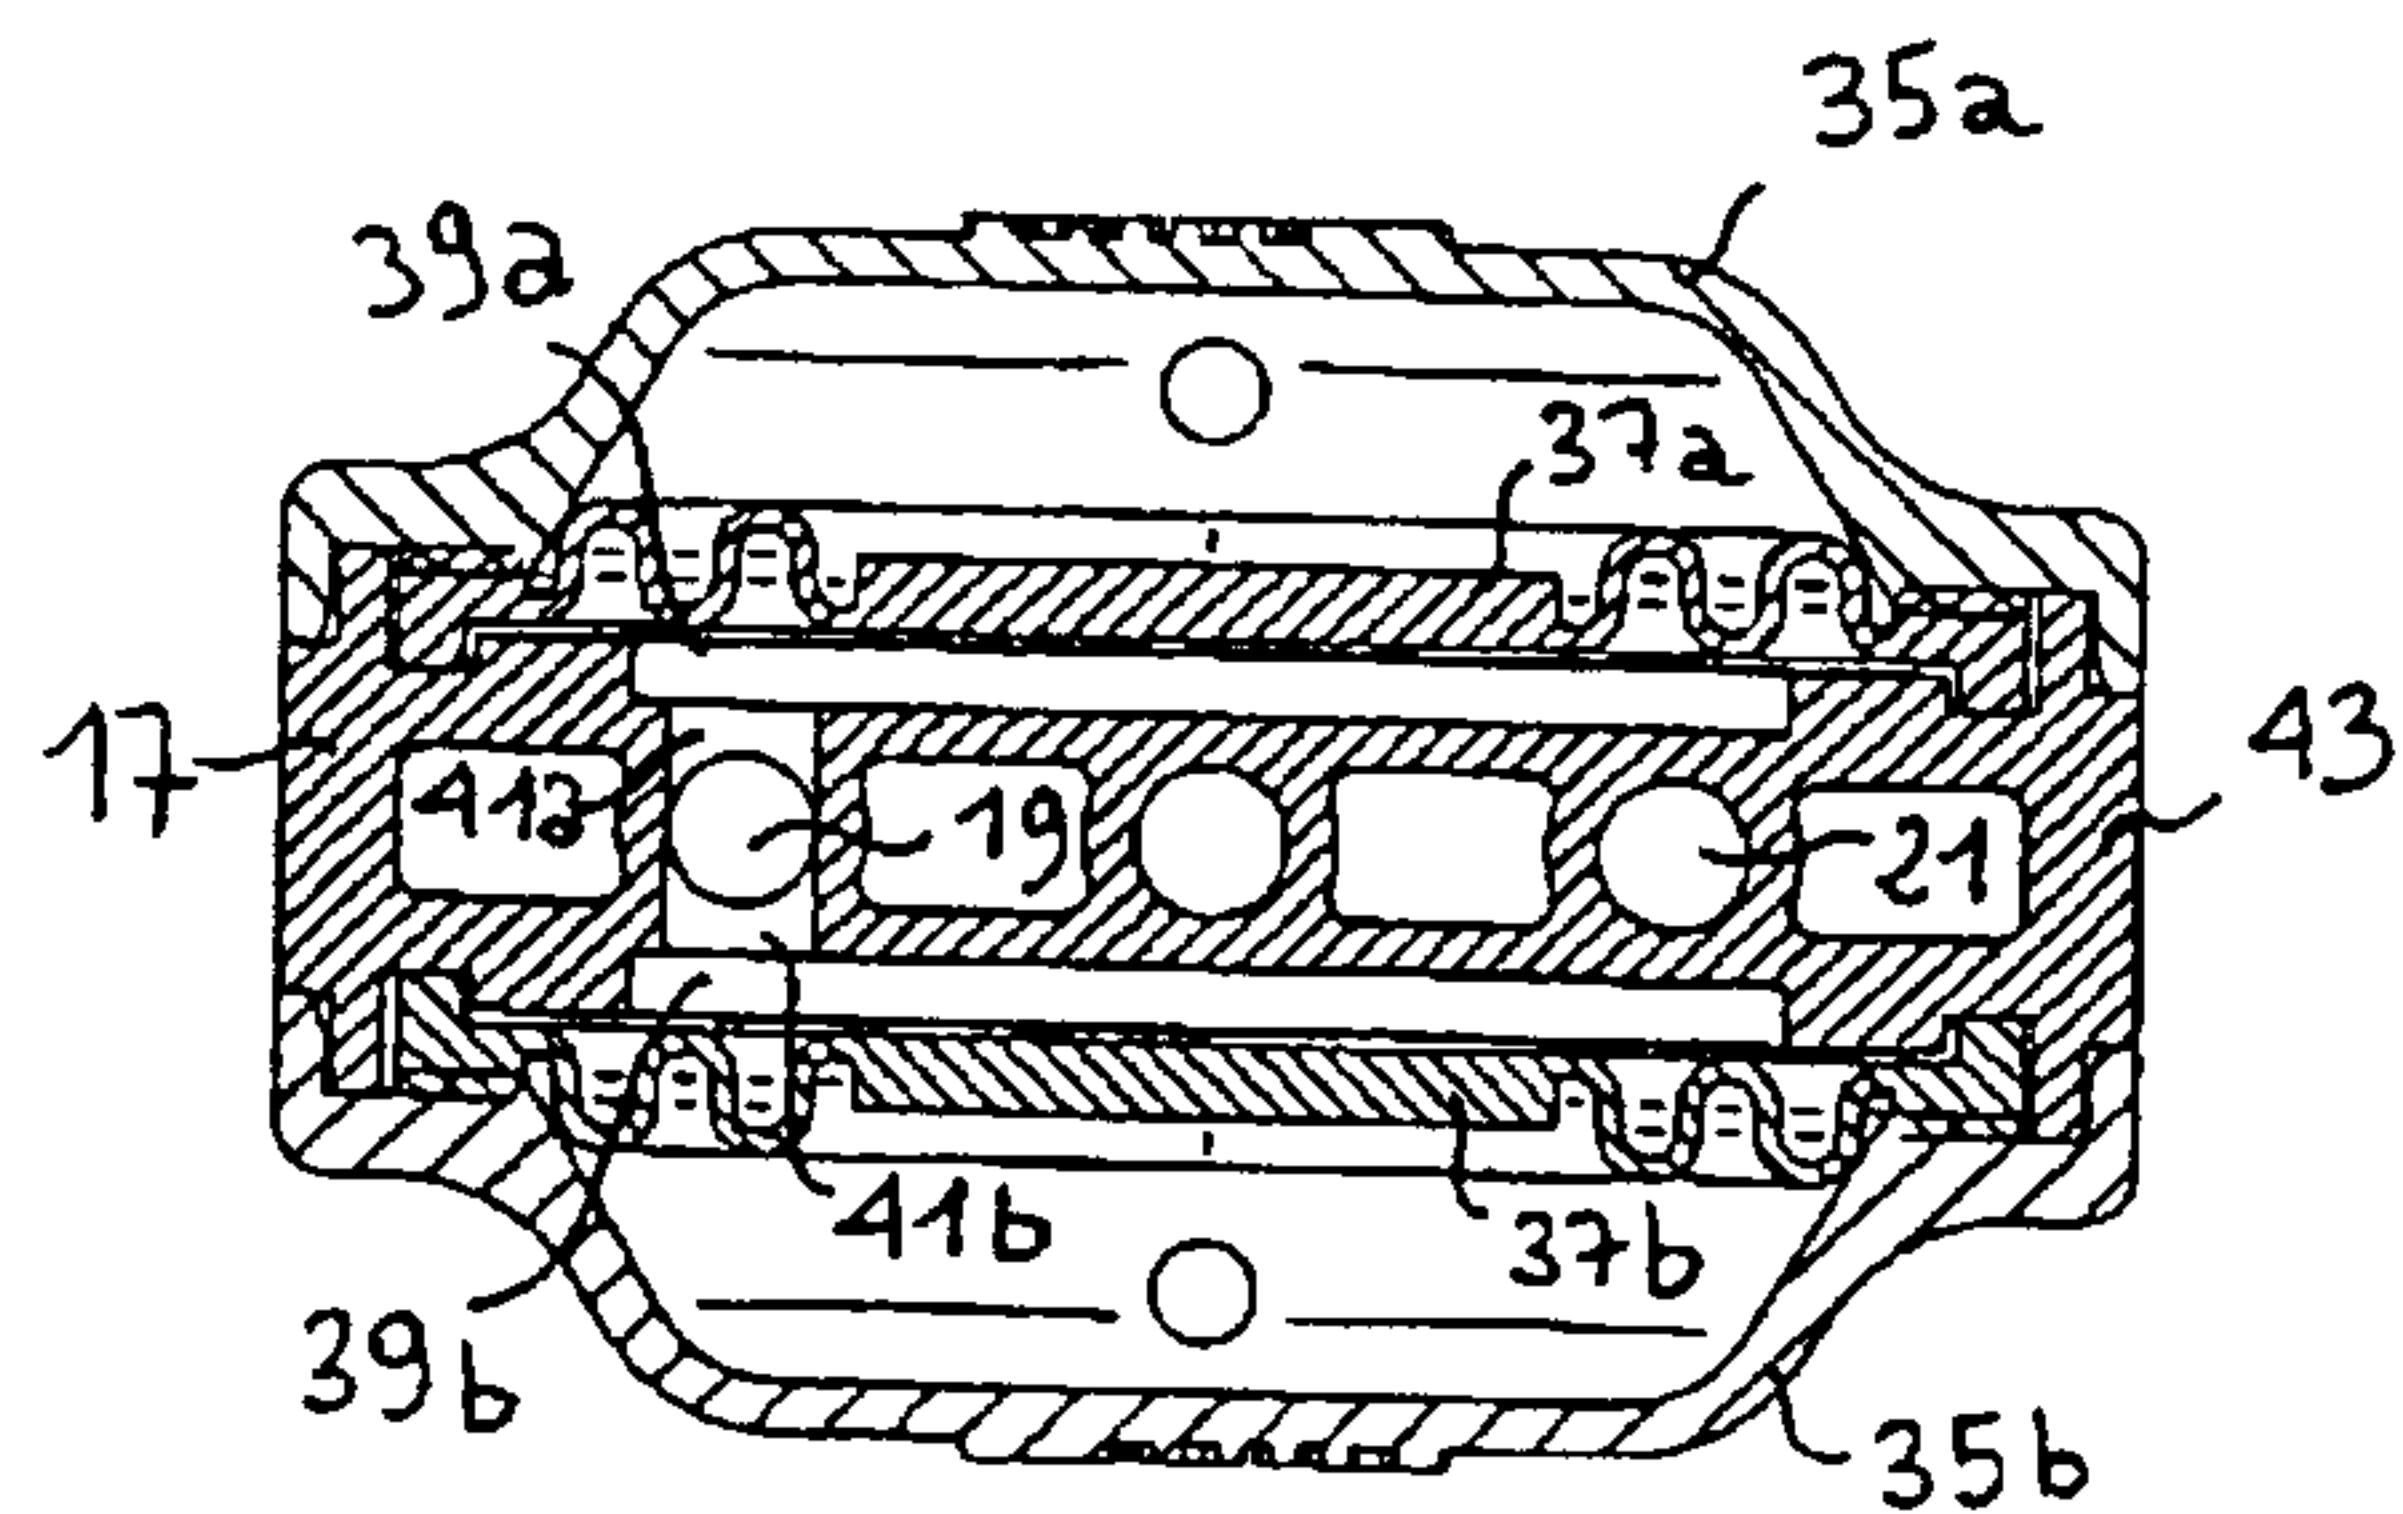


Fig. 7

