

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
28 September 2006 (28.09.2006)

PCT

(10) International Publication Number
WO 2006/102593 A2

(51) International Patent Classification:
G01N 33/00 (2006.01)

(21) International Application Number:
PCT/US2006/010788

(22) International Filing Date: 23 March 2006 (23.03.2006)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/665,726 24 March 2005 (24.03.2005) US

(71) Applicants and

(72) Inventors: **FOLLONIER, Stephane, Andre** [CH/US];
685 A Paso Nogal Road, Pleasant Hill, California 94523
(US). **INDERMUHLE, Pierre, Francois** [CH/US]; 1817
A Oregon Street, Berkeley, California 94703 (US).

(74) Agent: **HEINRICH, Julie, L.**; Finnegan, Henderson,
Farabow, Garrett & Dunner LLP, 901 New York Avenue,
Washington, D.C., District of Columbia 20001-4413 (US).

(81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,

AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN,
CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI,
GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE,
KG, KM, KN, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV,
LY, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI,
NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG,
SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US,
UZ, VC, VN, YU, ZA, ZM, ZW.


(84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM,
ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI,
FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT,
RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA,
GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *without international search report and to be republished
upon receipt of that report*

*For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.*

(54) Title: DEVICE, SYSTEM AND METHOD OF DETECTING TARGETS IN A FLUID SAMPLE

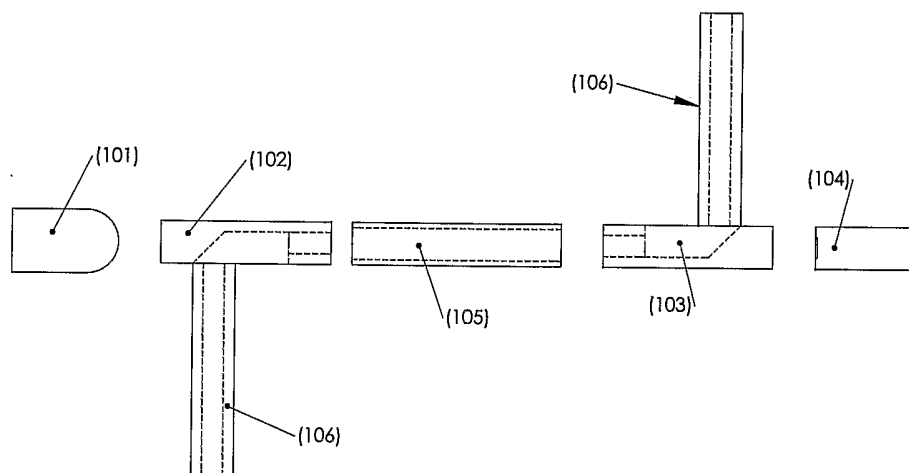

(57) Abstract: The present invention provides a biochemical detection system that comprises an exchangeable cartridge unit with light guiding tubes pre-coated with capture agent(s) and an optical detection unit. Upon flowing the liquid or gaseous sample containing the target(s) through the cartridge unit, the target(s) bind(s) to the capture agent(s) and is (are) detected by the amount of light or the variation of its properties while guided through the tubes. The optical detection unit is comprised of a light emitting element(s), a light connecting element(s) and a light detecting element(s) that delivers the amount of target(s) in the sample under investigation.



WO 2006/102593 A2

DEVICE, SYSTEM AND METHOD OF DETECTING TARGETS IN A FLUID SAMPLE

[0001] This application claims the benefit of U.S. Provisional Application No. 60/665,726, filed March 24, 2005, which is incorporated by reference herein in its entirety for any purpose.

TECHNICAL FIELD

[0002] The present invention is directed to wave-guiding devices that can detect targets in fluid samples. In one embodiment the amount of a target in a sample solution is determined by measuring differences in light transmission through the wave-guiding measuring cell before and after the target is bound by the capture agent on the inner surface of the wave-guiding tube.

BACKGROUND

[0003] Over the past decade, miniaturization and integration have revolutionized the world of biotechnology, allowing the realization of small sample volume, high throughput and multiplexed assays. From DNA micro-arrays to Elisa 1536-well plates, multiplexed systems appear to be the promising approach for biotechnology. These systems are directed towards highly multiplexed assays with multiple capture agents and targets. However, for clinical diagnostic tests, higher specificity (lower false positive data points), lower multiplexing (<10 capture agents), shorter assay time (30 minutes or less) as well as easier handling are required.

[0004] The diagnostic tests available on the market today suffer from one or more of the following disadvantages: long assay time (more than 30 minutes), large sample volume, low throughput, high complexity and especially a lack of modularity. Therefore, there is a strong need for an easy to handle, high sensitivity/selectivity/specificity, lower multiplexing, low cost,

low sample volume and high throughput device, which can perform quantitative measurements of target(s) concentration in samples.

SUMMARY OF INVENTION

[0005] Our approach is based on building a device that comprises an exchangeable cartridge unit coupled with a detection system. The cartridge unit is seen as a bundle of short light guiding tubes with pre-coated highly specific capture agents on their inner walls that can be very easily tailored to the customer request. By inserting the desired cartridge unit as well as the sample in the instrument, the user can determine the concentration of a panel of targets of his choice in this sample. Depending on the application, there are a variety of techniques to make the tubes that compose the cartridge light guiding.

[0006] Thanks to the flexibility of our approach, the use of the cartridge unit can be expanded from pure biotechnological applications (DNA, proteins) to different functionalities such as chemicals, toxins, viruses and/or bacteria or any other targets in liquid samples for which a capture agent can be engineered. Applications such as water quality monitoring, environmental safety monitoring, rapid diagnostic kits, portable field sensors, integrated point of care sensors are among the many possible applications. Potential users include research institutes, pharmaceutical companies, analysis laboratories as well as point of care customers both in military and in civil applications.

[0007] By expanding the exchangeable cartridge unit from a liquid waveguide to a gaseous waveguide (using a photonic bandgap crystal structure), our approach also covers measurements of air born pathogens such as anthrax, SARS or other viruses/bacteria or any target, for which a capture agent can be produced. Applications such as sensor for explosives, environment sensor, air quality sensor or military portable sensors are among many possible applications.

BRIEF DESCRIPTION OF DRAWINGS

[0008] Figure 1: The biochemical detection system comprising an optical detection unit with one light emitting element (101), with one primary light connecting element (102), with one secondary light connecting element (103), and with one light detecting element (104). The system further comprises an exchangeable cartridge unit (105) with light guiding tubes pre-coated with capture agent(s) and one fluid dispensing element (106).

[0009] Figures 2 and 3: The biochemical detection system comprising the measuring cell of the present invention in a 96-well array format.

° DISCLOSURE OF THE INVENTION

[0010] In one aspect, this invention is directed to a measuring cell, which comprises at least one tube capable of both guiding light and capable of binding a target(s) from a liquid or gaseous sample facilitated by at least one capture agent immobilized on its inner surface. The tube(s), comprises an input opening, an output opening and an inner surface coated with a binding agent(s), which is exposed to a sample by flowing, in an optionally regulated manner, the sample into the input opening, through the tube(s) and out from the output opening. The flow of the sample through the tube can be regulated by pressure, gravity, capillary forces or electrophoresis.

[0011] The ability of the tube(s) to guide light is generated either by the properties of its inner surface (which may be made of one or more organic or inorganic layer, e.g. in such a way that this layer or these layers builds an optical coating) or through an inherent property of the material used to construct the tube(s). Alternately, the ability of the tube(s) to guide light is a result of features designed within the material building the tube(s) or is a result of features designed within a material surrounding the tube(s). Examples of such tube(s) are hollow fibers and photonic bandgap crystals. Another alternative to generate the ability of the tube to guide light is a the result of the introduction into the tube of a fluid (e.g. a liquid) with a refractive index high enough to render the tube or the tube with its surrounding material a light guide.

[0012] The capture agent(s) may be bound directly to the inner surface of the tube(s) (or to one of the layers building it) or bound to an interstitial layer comprised of one or more layers. This layer(s) may contain an additional agent(s) that prevents or retards non-specific adsorption and/or non-specific binding of the target(s) and/or other components of the sample. In another embodiment, the inner surface of the tube is coated with an additional layer, which interacts with the bound target in a way that changes the properties of the light guided through the tube.

[0013] In another aspect, this invention is directed to a system that comprises a light emitting element(s), a primary light connecting element(s), a measuring cell as described in the first aspect, a secondary light connecting element(s), a light detecting element(s) and a fluid dispensing element(s). It may also comprise a sample and a disposal reservoir.

[0014] In this system, the fluid dispensing element(s) dispenses in a regulated manner the liquid or gaseous sample from the sample reservoir into the measuring cell and from the measuring cell into the disposal reservoir. The light, emitted by the light emitting element(s), is connected to the measuring cell by the primary light connecting element(s). It is guided through this measuring cell and then connected through the secondary light connecting element(s) to the light detecting element(s). The change in the amount or in the properties of the detected light relates to the amount of the target(s) bound to the capture agent(s) on the inner surface of the tube(s) of the measuring cell, or to a change of at least one of its properties.

[0015] Examples of the light emitting element(s) are a laser, a Light Emitting Diode, a white light source, a Vertical cavity light emitting laser and an array of those elements. Examples of the light detecting element(s) are a photomultiplier tube, a camera, a photodiode and an array of those elements. Examples of light connecting element(s) are a Brewster angle window, a lenslet array, a grating index coupler, a partially reflecting mirror, a spectral or an intensity filter and a combination of two or more of the connecting elements described above. The light connecting element(s) that may be the same or not, may also be a liquid dispensing element(s). In another embodiment, the light connecting element(s) is integrated in the tube(s) of the measuring cell.

[0016] The capture agent(s) may be bound directly to the inner surface of the tube(s) (or to one of the layers building it) or bound to an interstitial layer comprised of one or

more layers. This layer(s) may contain an additional agent(s) that prevents or retards non-specific adsorption and/or non-specific binding of the target(s) and/or other components of the sample. In another embodiment, the inner surface of the tube is coated with an additional layer, which interacts with the bound target in a way that changes the properties of the light guided through the tube.

[0017] In a third aspect, this invention is directed to a method for detecting a target(s) in a liquid or gaseous sample. This method comprises the introduction, using the fluid dispensing element(s), of a sample into the measuring cell(s), which comprises at least one tube capable of both guiding light and binding a target(s) from a sample. This method also comprises the step of connecting the light emitted by the light emitting element(s) into the measuring cell using the primary light connecting element(s), wherein the light is then guided through the measuring cell where it interacts with the bound target(s). In addition, it comprises the step of connecting light, by using the secondary light connecting element(s), from the measuring cell(s) to the light detecting element(s). The detection, with the light detecting element(s), of the amount of light or of the variation of the property(ies) of the light that went through the measuring cell allows the determination or the calculation of the amount of target(s) bound to the capture agent(s) on the inner surface of the measuring cell, or of the properties of this target.

[0018] The mentioned tube(s) comprises an input opening, an output opening and an inner surface coated with binding agent(s). In this method, the fluid dispensing element(s) dispenses the liquid or gaseous sample into the measuring cell from the sample reservoir and from the measuring cell into the disposal reservoir in a regulated manner.

[0019] In another embodiment, the method comprises the introduction, after the sample is introduced to the measuring cell using a fluid dispensing element(s), of one cleaving and/or digesting agent into the at least one measuring cell, using at least one fluid dispensing element, after the at least one target is immobilized on the inner surface of the at least one measuring cell in a first step, and wherein the at least one cleaving and/or digesting agent modifies the structure of the at least one bound target. In yet another embodiment, the method comprises the introduction, after the sample is introduced to the measuring cell using a fluid dispensing element(s), of a second binding agent(s) into the measuring cell that binds to the target(s), which has been captured by the capture agent(s). The second binding agent(s) emits

light or absorbs light or has optical properties that enhance detection. The interaction of the target(s) with any agent and/or any layer bound or immobilized on the inner surface of the tube may change the optical properties of either, the second binding agent(s), the bound target(s) or any agent and/or any layer bound or immobilized on the inner surface of the tube. This interaction or the optical properties of the second binding agent(s) changes the amount of light or the property(ies) of the light that went through the measuring cell allowing the determination or the calculation of the amount of target(s) bound to the capture agent(s) on the inner surface of the measuring cell, or of the properties of this target.

[0020] In a further embodiment, the method comprises the introduction of an amplification agent(s) to the measuring cell(s), where the amplification agent(s) binds to the second binding agent(s). The amplification agent(s) emits light or absorbs light or has optical properties that enhance detection. The interaction of the target(s) with any agent and/or any layer bound or immobilized on the inner surface of the tube may change the optical properties of either the bound target(s) or any agent and/or any layer bound or immobilized on the inner surface of the tube. This interaction or the optical properties of the amplification agent(s) changes the amount of light or the property(ies) of the light that went through the measuring cell allowing the determination or the calculation of the amount of target(s) bound to the capture agent(s) on the inner surface of the measuring cell, or of the properties of this target.

[0021] In another embodiment, the sample undergoes a required number of sample preparation steps before being introduced into the measuring cell.

[0022] In yet another embodiment, the method comprises or not a washing step between any immobilization or detection steps.

[0023] In another embodiment, an optical fluid (e.g. a liquid) is introduced into the at least one tube of the at least one measuring cell, said optical fluid having a refractive index high enough to render the at least one tube or the at least one tube with its surrounding material a light guide.

[0024] In a further embodiment, the optical fluid is introduced at any step of the method or between any step of the method or both.

[0025] In yet another embodiment, the optical fluid is kept in the at least one tube of the at least one measuring cell during the time necessary to perform any desired measurement(s).

[0026] In a further embodiment, the immobilization times are adequately chosen for each step of each embodiment of the method.

MODE FOR CARRYING OUT THE INVENTION

[0027] The following detailed description illustrates the invention by way of example and not by way of limitation. This description will enable one skilled in the art to make and use the invention, and describes several embodiments, adaptations, variations, alternatives and uses of the invention.

[0028] The present invention is directed to a measuring cell which comprises at least one tube capable of guiding light. The interior walls of the tube are coated with at least one specific capture agent to bind at least one specific target from a sample containing known and/or unknown components. The measuring cell may be used as a component of a system used to analyze samples for at least on specific target. The system comprises a measuring cell capable of binding targets from a sample integrated in, for example, an exchangeable cartridge unit, which in turn is coupled to both a light source and a detection system. These elements build an extremely sensitive, inexpensive and compact system for quantitative detection of targets in a sample (liquid or gaseous). In alternative embodiments, more than one measuring cell may be bundled together to measure the same sample multiple times or to measure the same sample for multiple targets.

THE MEASURING CELL

[0029] The tube has one input opening and one output opening such that the fluid sample can be introduced into the tube and removed from the tube. A sample may be introduced to the tube by first flowing an amount of a fluid sample into the tube that is sufficient to fill the tube and then stopping the flow. Alternatively, a predetermined amount of the sample solution may flow through the tube before the flow is stopped. For example from about 1nl to about 1

mL of sample may flow through the tube. In either case, the flow through the tube can be regulated through pressure, through capillary forces, through gravity, through electrophoresis, through pumps (Fluidigm Inc. South San Francisco, CA 94080), through passive or active valves or through an external flow control device. Also contemplated are systems where the sample flows continuously through the tube of the measuring cell. The fluid sample may be liquid or gaseous.

[0030] Analysis of the sample for the desired target occurs once the sample has interacted with the capture agent immobilized on the inner surface of the tube. This interaction may take place immediately following the introduction of the sample to the tube. Alternatively, the sample may flow through the tube for a certain period of time and/or may require an incubation process before the measurement takes place. The incubation time, i.e. the total time during which the sample is in contact with the capture agent, can be set depending on the type of interaction and the desired sensitivity of the assay, typically between 1 minute and 4 days and preferably between 1 and 30 minutes. Also contemplated are continuous flow systems where the sample is continually flowed through the wave-guiding tube, and sample analysis occurs without stopping the flow of the sample. Similarly, continuous real-time monitoring are also possible.

[0031] The diameter and the length of the at least one tube depend on the sensitivity and sample volume requested by the application, typically from 5 microns to 1000 microns, preferably from about 50 to about 400 microns, for the diameter and from 1mm to 1000mm for the length. For liquid samples, e.g., for strong and specific antibody-antigen interactions, a length of 10mm for a diameter of 50 microns to 100 microns is a good fit. Gaseous samples may require a longer tube (100mm to 1000mm) to increase the size of active surface to allow the detection of smaller amounts of targets in the sample.

[0032] The at least one tube has the ability to guide light. Wave-guiding properties are seen in devices where light is being propagated through a first material and that first material is bounded by a second material with a lower refractive index than the refractive index of the first material. When the light propagating through the first material encounters the boundary between the first and second material, the light is reflected instead of transmitted through the boundary. In the present invention, the first material is the gas or liquid within the measuring cell and the second material is the walls of the measuring cell tube.

[0033] The interior wall of the measuring tube may be the same material as the rest of the tube. For example a fused silica tube with a solvent of higher refractive index inside the tube will guide light. Alternatively the interior walls of the tube may have a coating such as Teflon AF, or some other optical coating which becomes and integral part of the interior wall of the tube. Optical coatings for use in waver guides are known in the art.

[0034] In a first example, Teflon AF polymer (Dupont), which has a low refractive index ($n < 1.33$), can be used as a coating material for the inner surface of the tube. Alternatively, Teflon AF can be used as the construction material (Biogeneral, Inc. San Diego, CA 92121), to fabricate the complete tube. In either case the low refractive index of the Teflon AF polymer coupled with a liquid sample that has a refractive index higher than $n < 1.33$ imparts the tube with the desired optical wave guiding characteristics. Because Teflon AF has such a low refractive index, aqueous samples (with no additional "optical fluid") have a refractive index sufficient to create the wave-guiding conditions.

[0035] In another example, a tube made out of glass, fused silica or another material becomes light guiding when filled with a fluid having a higher refractive index (Cargille Laboratories, Inc., Cedar Grove, NY 07009) than the effective refractive index of its own material. As discussed above, when the tube material has a refractive index lower than the refractive index of the sample solution, or of the solution within the tube when the analytical measurement is being made, the tube will act as a waveguide. When the tube is constructed from fused silica, ($n = 1.46$), the sample solution should have an index of refraction higher than 1.46, typically 1.49. This can be accomplished by using a solvent with an inherently high refractive index. Alternatively, additives such as glycerol, sucrose, and the like, can be added to the sample solution. Sample solutions with a lower index of refraction can also be used with a fused silica tube if the index of refraction of the solution in the tube is increased, prior to making the analytical measurement, using additives and/or solvents similar to those discussed above.

[0036] Some materials, guide light due to physical features built into the material bounding the tube causing the light propagating through the tube to be reflected instead of transmitted. For example, photonic bandgap crystals (US 6,571,045 May 27, 2003 Hasegawa et al.) commercially available from BlazePhotonics (Denmark), guide light due to a honeycomb structure that is constructed around the tube. Any type of wave-guiding tube whose interior

surface can be coated with capture agents is useful in the present invention. Photonic bandgap crystals act as an optical waveguide when filled with a gas.

[0037] The capture agents may be bound directly to the inner surface of the tube through, for example, chemical bonding or adsorption. Alternatively, the capture agent may be bonded indirectly to the interior surface of the tube through at least one interstitial layer. Examples of such interstitial layers are polymers (PLL-PEG, silanes, Self-Assembled Monolayers (alkanethiols)). The capture agents can be chemically bonded or adsorbed to the interstitial layer. Specifically, for tubes made from Teflon AF (i.e. for liquid samples), the inner surface of the tubes may be modified by oxygen plasma so that the capture agent(s) is(are) directly bonded to the inner surface; The inner surface of the tube may also be coated with an interstitial layer of nitrocellulose or of e.g. Optodex (Arrayon Biotechnology SA, Neuchatel, 2007, Switzerland). For tubes made from or coated with glass (filled with a fluid with a refractive index high enough to render the tube or the tube with its surrounding material a light guide) or silicon for photonic bandgap crystal, the capture agent may be bound to the tube inner surface by, for example, well known silane surface chemistry. For tubes made out of or coated with other materials, e.g. plastics, polymers, any of or a combination of the above surface chemistries may be used to bind the capture agents to the tube's inner surface.

[0038] If desired, the inner surface of the at least one tube may also be provided with additional agents that prevent or retard non-specific adsorption and/or non-specific binding of the target and/or of other components of the sample. These additional agents ensure that only the desired target in the sample binds to the inner surface of the tube and will therefore ensure the specificity of the assay. Examples of those additional agents are PEG chains.

[0039] The measuring cell is an assembly of one or more tubes that are pre-loaded with similar or different capture agents to allow for duplicates or to detect several targets in the same sample or to serve as calibration. Several of such tubes can be held together by integration (Schott Glas, 55122 Mainz, Germany), before or after loading the capture agents. For ease in production, the capture agent loading can be achieved in longer tubes that are cut to size in a second step, ensuring thus the most efficient homogeneity and facilitating the QC/QA process. Finally the measuring cell may be filled with a buffer or a preservation solution and sealed, to prevent any degradation of the active capture agents during the storage and shipping.

[0040] The input and output openings of the tube(s) may be sealed or may be covered with slits to allow an easier handling and protect the content of the measuring cell against any environmental contamination. These seals or slits will break or slide upon insertion of the measuring cell into the detection system unit or at the insertion of the sample into the tube. The measuring cell may also be sealed to preserve the content's integrity until it is used.

[0041] The measuring cell may or may not comprise a primary light connecting element(s) and/or a secondary light connecting element(s) and/or a fluid dispensing element(s). These elements may or may not be integrated in the measuring cell. In one example, the at least one measuring cell is provided with one primary light connecting element, one secondary light connecting element and a fluidic element.

[0042] The measuring cell can be packaged in a user friendly cartridge to be inserted in the detection system.

AN ANALYTICAL SYSTEM USING THE MEASURING CELLS

[0043] An exchangeable measuring cell (packaged in a cartridge unit) may be coupled to at least one light emitting element and at least one light detecting element. Further light connecting elements may be part of the detection system unit as well as a liquid dispensing unit, a sample reservoir and a waste reservoir.

[0044] An analytical system using the measuring cell of the present invention is shown in Figure 1. The light emitted by a light emitting element(s) (Figure 1, (101)) is connected to one or more measuring cell (Figure 1, (105)) through a primary light connecting element(s) (Figure 1, (102)). The light travels through the measuring cell(s) before being connected out of the measuring cell(s) and into a light detection element(s) (Figure 1, (104)) by a secondary light connecting element(s) (Figure 1, (103)). The sample of interest is directed to the measuring cell(s) and its flow through the measuring cell(s) is regulated by the fluid dispensing element(s) (Figure 1, (106)). Upon binding of the target(s) contained in the sample to the capture agent(s) bound to the inner surface of the tube(s) of the measuring cell(s), the amount of light guided through the tube or at least one property of this light is changed proportionally to the amount of target(s) bound to the capture agent(s).

[0045] In one embodiment, by inserting the measuring cell, packaged in the exchangeable cartridge unit, into the detection system, the entrance and exit covers slide off the measuring cell(s) and/or the seals of the measuring cell(s) are automatically broken, allowing thus the introduction of the sample into the measuring cell(s). A fluid dispensing element may be used to facilitate the sample flow through the measuring cell(s). The flow of the sample through the measuring cell(s) may be driven by gravity, capillary forces, by electrophoresis or pressure or a combination of these. For gaseous samples, the sample handling system may be comprised of a device that increases the flow through the measuring cells.

[0046] The light emitted by the at least one light emitting element is connected to the measuring cell(s) of the exchangeable cartridge unit through the at least one primary light connecting elements. The light travels through the at least one measuring cell before being connected out of the at least one measuring cell and into the at least one light detecting element by the at least one secondary light connecting elements.

[0047] When the target contained in the sample binds to the capture agent(s) immobilized on the inner surface of the tube, the change of the amount of light guided through the tube, or the change of at least one other property of this light, is measured. For example, the intensity at various wavelengths of the light guided through a measuring cell is changed by the interaction of this light with the target, and/or with the capture agent, and/or with the second binding agent, and/or with the amplification agent bound to the inner surface of the measuring cell(s). Other optical processes such as scattering, or such as the interaction between two of the above species, or between one of the above species and one interstitial layer may also change at least one property of the transmitted light. The amount of target bound to the capture agents can then be determined or computed by measuring these changes.

The light emitting element

[0048] Depending on the application, the at least one light emitting element may be emitting monochromatically or polychromatically in the visible and/or in the infrared and/or in the UV (e.g. Jameco Electronics Belmont, CA 94002). It may be a simple light emitting diode or a laser diode or even a white light source (Newport Corporation, Irvine, CA 92606) or a Vertical Cavity Surface Emitting Laser. It may be an array of light emitting diodes or lasers or white light

sources such that they can be inserted into the tubes. The wavelength(s) of interest may be selected through the at least one primary light connecting element that also serve the purpose of coupling the light into the tube.

The light connecting elements

[0049] The primary light connecting element transmits the light from the at least one light emitting element into at least one tube of the measuring cell and the secondary light connecting element transmits the light out of the at least one tube of the measuring cell into the at least one light detecting element. The light connecting element and the fluidic element which regulates the flow of the sample through the tube of the measuring cell may be a single element with dual purpose. More specifically, for liquid samples and measuring tubes made out of Teflon AF, the tube (pre cut to size) is connected to glass Brewster windows that serve the purposes of guiding light into and out of the tube (light connecting elements) as well as guiding the sample into and out of the tube (fluidic dispensing elements).

[0050] The primary and secondary light connecting elements serve different purposes such as connecting light from the at least one light emitting element into the at least one measuring cell and out of the at least one measuring cell onto the at least one light detecting element. They can also serve other purposes such as focusing light into separate tubes (lenses, lenslet arrays, Control Optics, Chino, CA 91710), such as tailoring the properties of the light (wavelength and intensity filters Newport Corporation, Irvine, CA 92606), such as partially reflecting the light back and forth in the tube or such as coupling light into the tube or out of the tube with a grating index coupler. The nature of the primary and the secondary light connecting elements are selected depending on the optical detection process that is used, e.g. fluorescence, absorption, Raman scattering.

[0051] The primary and secondary light connecting elements may be a multiplicity of the above described elements for each measuring cell. Besides connecting light into the measuring cell, the purpose of the connecting elements may be to ensure sample handling as well. These light connecting elements may or may not be integrated in the measuring cell.

The light detecting element

[0052] The detector, which may be a camera (Jameco Electronics Belmont, CA 94002) or a photomultiplier tube or a photodiode or a series of light detecting elements for a multiplicity of measuring cells, monitors the properties and/or the intensity of the light exiting each measuring cell. From the changes at specific wavelengths, of the intensity or of the properties of this light, the processing circuit calculates the concentration in the sample of biologically or chemically relevant targets.

The fluid dispensing element

[0053] The fluid dispensing element dispenses the sample to the at least one measuring cell from the sample reservoir and from the at least one measuring cell to the disposal reservoir; the fluid dispensing element may be used to facilitate the sample flow through the measuring cell(s). The flow of the sample through the measuring cell(s) may be driven by gravity, capillary forces, by electrophoresis or pressure or a combination of these. For gaseous samples, the sample handling system may be comprised of a device that increases the flow through the measuring cells. The fluid dispensing element may also be serving other purposes such as introducing different solutions into the tube (secondary binding agent, amplification agent, buffer, optical fluid), such as regulating the sample flow or such as performing sample preparation, including filtering, mixing or sample dilution. In one example, the sample flow is controlled via capillarity from the input opening of the tube to the output opening of the tube. Furthermore, the fluid dispensing element can be used to fill the cell(s) with an index fluid having a refractive index high enough to render the tube or the tube with its surrounding material a light guide.

[0054] The fluidic element or part of it may also serve other purposes such as introducing different samples into the tube (second binding agent, amplification agent, buffers), such as regulating the sample flow or such as performing sample preparation, including sample filtering, sample mixing or sample dilution. In one example, the sample flow is controlled via gravity from the input opening of the tube to the output opening of the tube. In addition, the fluidic element may also be used to introduce one or more fluids with a defined refractive index into the tube to control its light guiding properties.

A METHODS OF USING THE MEASURING CELL ANALYTICAL SYSTEM

[0055] A tube filled with gas or liquid may be turned into an optical waveguide by a specific design of its optical properties or by a specific choice of the optical properties of the fluid. A change in the optical properties of the fluid filling the tube or a change of the properties of the interface between the tube and the fluid may induce a change in the amount or in the characteristics of the guided light. The method described here uses the above principle to detect a target in a fluid sample: the inner surface of the tube is engineered such that the target will be immobilized or bound to this surface when the sample is flowed through the tube. The optical characteristics of the target, or of an agent bound to the target (e.g. for specificity or amplification), or the interaction of the target, or of any agent, with the inner surface of the tube, or with any other agent, may generate a variation in the amount or in the properties of the guided light, which can be detected. This variation is proportional to the amount of targets bound to the inner surface of the tube.

[0056] A capture agent is a molecule or a part of a molecule that is capable of binding a target, i.e. capable of immobilizing for a certain period of time another molecule or another part of a molecule contained in a sample. Examples of targets are explosives, pathogens, bacteria, viruses, DNA strands or proteins. Examples of capture agents are molecules/polymers with specific end-groups such as biotin or amine reactive terminals or more complex species such as antibodies, DNA strands. For the method to detect the cleavages of parts of the target(s) (kinase, protease) processes, a cleaving and/or digesting agent can be introduced into the measuring cell after the target is immobilized on the inner surface of the measuring cell in a first step. Methods for immobilizing antibodies on surfaces are known in the art and are described, for example, in Harlow, E. and D. Lane, *Antibodies: A Laboratory Manual*, (1988) Cold Spring Harbor Laboratory, Cold Spring Harbor, N.Y. which is incorporated herein by reference. In addition the company Biacore (www.biacore.com) has accumulated protocols for numerous immobilization methods. Biacore makes this information available to the public via the internet or by publications which can be ordered.

[0057] In order to increase the sensitivity of the detection or to allow for specific types of detections, a second binding agent(s) may interact with the target(s). The second binding

agent(s) may also serve as a second filter, by lowering the influence of non-specific binding to the capture agent(s). It may be labeled with a fluorescent dye or with an absorbing molecule such that the interaction of the guided light with this dye or with this molecule results in a change of the properties of the guided light. In order to further increase the sensitivity of the assay, an amplification agent(s) may be bound to the second agent(s) serving a signal amplification purpose and a further filter. Examples of a second binding agent(s) are secondary antibodies conjugated to HRP (horseradish peroxidase) with the corresponding amplification agent being a signal enhancement substrate (e.g. Tetra methyl Benzidine) (Molecular Probes Inc. Eugene, OR 97402). Washing steps may be used to wash off excess of sample, second binding agent(s) or amplification agent(s).

[0058] With gaseous samples and with liquid samples, which are partially light transparent, the measurement can occur simultaneously with the sample flow and can run continuously through the measuring cell. Additional automated fluidic devices may allow for additional assay steps for the sample preparation as well as for targets and for agents that require rinsing and/or signal amplification after their immobilization/incubation.

WHAT IS CLAIMED IS:

1. A measuring cell comprising a tube capable of guiding light, wherein the tube is from about 1 to about 1000 mm in length, has an inner diameter of from about 5 to about 1000 microns and comprises
 - a) an input opening,
 - b) an output opening, and
 - c) an inner surface comprising thereon at least one binding agent capable of binding a target from a fluid sample introduced to the tube through said input opening, and which by its physical properties or by its physical structure causes the tube to be a light guiding tube.
2. The measuring cell of claim 1, wherein the tube is from about 5 to about 15 mm in length.
3. The measuring cell of claim 1, wherein the tube has an inner diameter from about 50 to about 400-microns.
4. The measuring cell of claim 1 wherein the tube is a light guiding tube by reason of being fabricated of a material having a lower refractive index than the refractive index of the fluid sample.
5. The measuring cell of claim 4, wherein the tube is a hollow fiber made from Teflon AF[®].
6. The measuring cell of claim 4, wherein the tube is a hollow fiber made from fused silica.
7. The measuring cell of claim 1 wherein the tube is a light guiding tube by reason of being fabricated of a multilayer tube wherein the layer exposed to the interior of the tube is the inner surface and has a lower refractive index than the refractive index of the fluid sample.

8. The measuring cell of claim 7 wherein the inner surface is an inner sleeve.
9. The measuring cell of claim 7 wherein the inner surface is chemical coating.
10. The measuring cell of claim 7 wherein the tube is a hollow fiber with Teflon AF[®] on the inner surface.
11. The measuring cell of claim 1 wherein the tube is a light guiding tube by reason of being fabricated of a photonic bandgap crystal.
12. The measuring cell of claim 1, wherein the sample is liquid.
13. The measuring cell of claim 11, wherein the sample is gaseous.
14. The measuring cell of claim 1, wherein inner surface of the tube capable of guiding light comprises thereon a plurality of capture agents.
15. The measuring cell of claim 14, wherein the plurality of capture agents is capable of binding a plurality of targets.
16. The measuring cell of claim 1, wherein the capture agent is chemically bonded to the inner surface of the tube.
17. The measuring cell of claim 1, wherein the capture agent is adsorbed to the inner surface of the tube.
18. The measuring cell of claim 1, wherein inner surface of the tube capable of guiding light comprises thereon an interstitial layer between the inner surface of the tube and the plurality of capture agents.

19. The measuring cell of claim 18, wherein the capture agent is chemically bonded to the interstitial layer.
20. The measuring cell of claim 18, wherein the capture agent is adsorbed to an interstitial layer.
21. The measuring cell of claim 1, wherein the capture agent is an antibody.
22. The measuring cell of claim 1, wherein the inner surface of the tube is coated with an additional layer which interacts with the at least one bound target in such a way that it changes a property of the light guided through the tube.
23. A measuring cell comprising a plurality of tubes capable of guiding light, wherein each tube is from about 1 to about 1000 mm in length, has an inner diameter of from about 5 to about 1000 microns and comprises
 - d) an input opening,
 - e) an output opening, and
 - f) an inner surface comprising thereon a binding agent capable of binding a target from a fluid sample introduced to the tube through said input opening, and
 - g) which by its physical properties or by its physical structure causes the tube to be a light guiding tube.
24. The measuring cell of claim 23, wherein the plurality of tubes are configured in a bundle.
25. The measuring cell of claim 23, wherein the plurality of tubes are configured in an array.
26. The measuring cell of claim 25, wherein the array is configured in a 96-well plate.
27. The measuring cell of claim 26 where an optical plate is set against the bottom of the 96-well plate to block the bottom output of the tubing.

28. The measuring cell of claim 27 where the optical plate is reflecting the emission light.

29. The measuring cell of claim 27 where the optical plate is transparent.

30. A detection system for detecting a target present in a fluid sample comprising
a measuring cell of claim 1 containing a fluid sample;
means for feeding an initial light signal to the light guiding tube, which signal is
capable of being changed by the target bound to the capture agent on the inner surface of the
tube, to produce an altered light signal; and
means for reading the altered light signal from the light guiding tube.

31. A system comprising:

- a) a light source;
- b) a primary light connecting element for feeding the light from the light source to a
measuring cell comprising a tube capable of guiding light, wherein the tube comprises
 - i) an input opening,
 - ii) an output opening, and
 - iii) an inner surface comprising thereon a binding agent capable of binding a
target from a fluid sample introduced to the tube through said input opening,
and which by its physical properties or by its physical structure causes the tube
to be a light guiding tube;
- c) a secondary light connecting element for feeding the light from the light guiding tube
to a detecting element; and
- d) a fluid dispensing element;

wherein the fluid dispensing element dispenses the sample to the measuring cell;

further wherein the light emitted by the light emitting element is transmitted to the measuring
cell by primary light connecting element;

further wherein the light guided through the measuring cell is transmitted to the light
detecting element by the secondary light connecting element;

further wherein the amount of light or the variation of property of the light detected by the
light detecting element relates to the amount or to a change of structure and/or properties

of the target bound to the capture agent on the inner surface of the tube of the measuring cell.

32. The system of claim 31, where one of the primary and the secondary light connecting element or both are also liquid dispensing elements.
33. The system of claim 31, where one of the primary light connecting element and the secondary light connecting element or both are integrated into the measuring cell.
34. The system of claim 31, where the liquid dispensing element is capable of transferring liquid to and from the measuring cell.
35. The system of claim 31, further comprising a sample reservoir.
36. The system of claim 31, further comprising a disposal reservoir.
37. The system of claim 31, wherein the flow of the sample is regulated.
38. The system of claim 31, wherein the flow of the sample is regulated by pressure or by gravity or by capillary forces or by electrophoresis.
39. A method for detecting a target in a fluid sample, which method comprises:
 - a) introducing the sample to a measuring cell using a fluid dispensing element, wherein the measuring cell comprises a tube capable of guiding light, wherein the tube comprises:
 - i. an input opening;
 - ii. an output opening;
 - iii. an inner surface coated with a binding agent capable of binding a target of a sample; conducting light from a light emitting element, into the measuring cell using a primary light connecting element, wherein the light is then guided through the tube of the

- measuring cell wherein target from the sample is bound to the capture agent on the inner surface of the tube to produce a modified light signal;
- b) connecting light present in the modified light signal, using a secondary light connecting element to a light detecting element;
 - c) detecting the modified light signal or a variation of at least one property of the light present with the light detecting element;
 - d) correlating the detected amount of light or variation of the light with the presence of target bound to capture agent bound to the inner surface of the tube.
40. The method of claim 39, wherein the sample undergoes sample preparation steps before being introduced into the measuring cell.
41. The method of claim 39, wherein the fluid sample has a refractive index high enough to render the tube a light guide.
42. The method of claim 41, wherein the optical fluid is introduced at any step of the method or between any step of the method or both.
43. The method of claim 41, wherein the sample refractive index is rendered high enough by the addition of a high refractive index organic liquid.
44. The method of claim 39, wherein a cleaving and/or digesting agent is introduced into the measuring cell after the target is immobilized on the inner surface of the measuring cell, and wherein the cleaving and/or digesting agent modifies the structure of the bound target and thereby alters the light signal.
45. The method of claim 39, wherein a second binding agent is introduced into the measuring cell, using a fluid dispensing element, after the target is immobilized on the inner surface of the measuring cell in a first step, and wherein the second binding agent is captured by the bound target and thereby alters the light signal.

46. The method of claim 45, further comprising a washing step between immobilization or detection steps.
47. The method of claim 45, wherein the second binding agent has optical properties that enhance detection.
48. The method of claim 45, wherein the second binding agent emits light or absorbs light generated by the light emitting element.
49. The method of claim 45, wherein the interaction of the second binding agent with the bound target and/or with any agent and/or any layer bound or immobilized on the inner surface of the tube changes the optical properties of the second binding agent and/or of the bound target and/or of any agent and/or any layer bound or immobilized on the inner surface of the tube.
50. The method of claim 47, further comprising the step of introducing an amplification agent to the measuring cell, where the amplification agent binds to the second binding agent.
51. The method of claim 50, further comprising a washing step between any immobilization or detection step.
52. The method of claim 50, wherein the second binding agent and/or the amplification agent has optical properties that enhance detection.
53. The method of claim 50, wherein the second binding agent and/or the amplification agent emits light or absorbs light generated by the light emitting element.
54. The method of claim 50, wherein the interaction of the amplification agent with the bound target and/or with any agent and/or any layer bound or immobilized on the inner

surface of the tube changes the optical properties of the amplification agent and/or of the bound target and/or of any agent and/or any layer bound or immobilized on the inner surface of the tube.

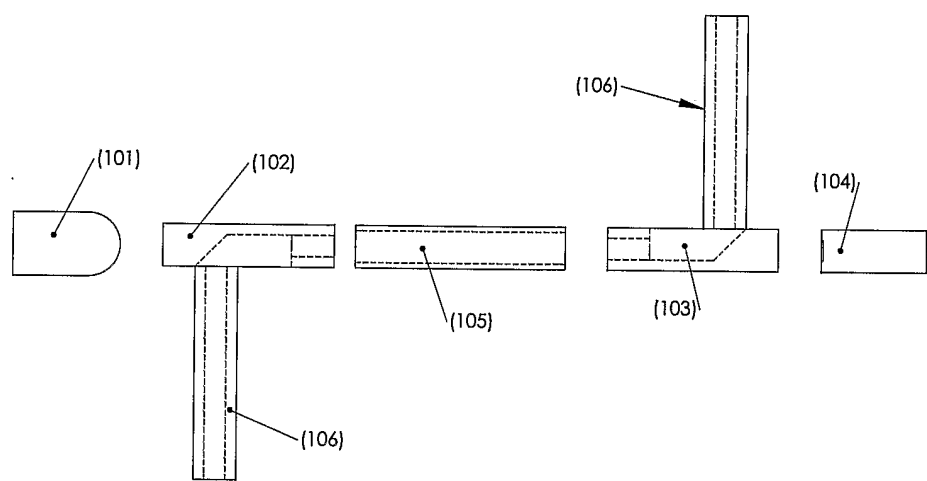


FIG. 1

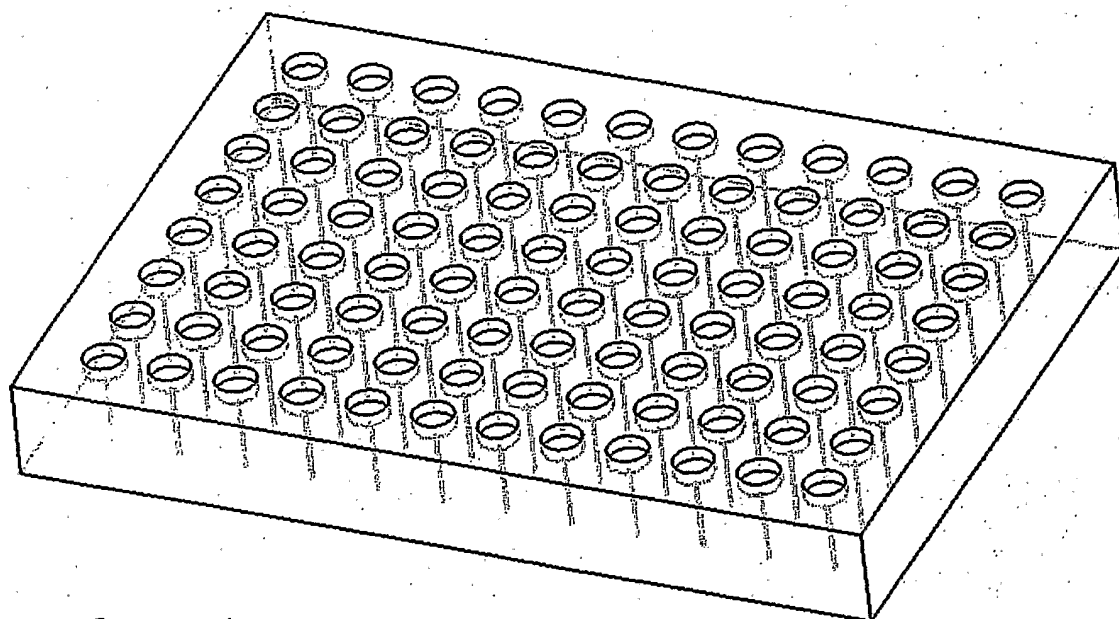


Figure 2

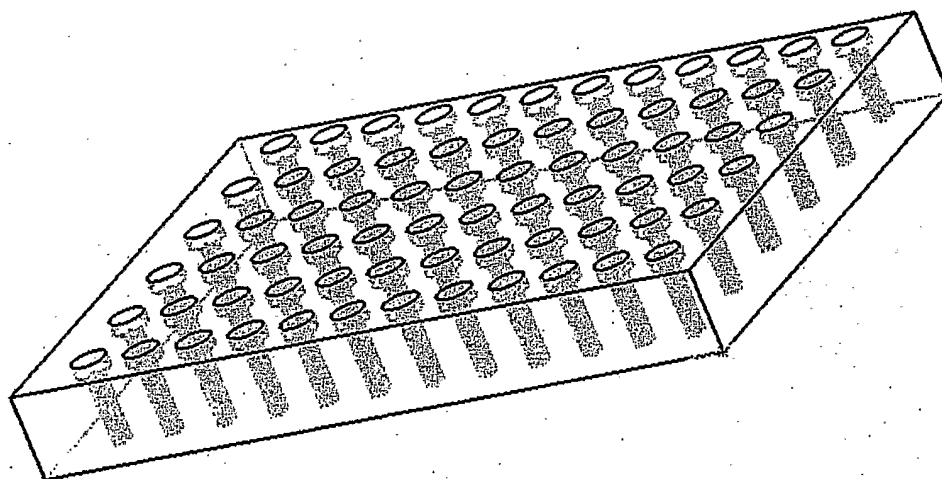


Figure 3