

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
17 February 2011 (17.02.2011)


(10) International Publication Number  
**WO 2011/017756 A1**

- (51) **International Patent Classification:**  
GOIL 7/08 (2006.01)
- (21) **International Application Number:**  
PCT/AU20 10/00 1024
- (22) **International Filing Date:**  
11 August 2010 (11.08.2010)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**  
2009903814 13 August 2009 (13.08.2009) AU  
2010901240 23 March 2010 (23.03.2010) AU
- (71) **Applicant (for all designated States except US):** ULTIMATE MEDICAL PTY. LTD. [AU/AU]; 484 Swan Street, Richmond, Victoria 3121 (AU).
- (72) **Inventor; and**
- (75) **Inventor/Applicant (for US only):** ESNOUF, Philip, Stuart [AU/AU]; 484 Swan Street, Richmond, Victoria 3121 (AU).
- (74) **Agents:** PRYOR, Geoffrey, Charles et al; Davies Collison Cave, 1 Nicholson Street, Melbourne, Victoria 3000 (AU).

- (81) **Designated States (unless otherwise indicated, for every kind of national protection available):** AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, **BH**, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, **DK**, DM, DO, DZ, EC, EE, EG, ES, **FI**, GB, GD, GE, GH, GM, GT, HN, **HR**, HU, **ID**, **IL**, **IN**, **IS**, **JP**, KE, KG, **KM**, KN, **KP**, **KR**, KZ, LA, LC, **LK**, **LR**, LS, **LT**, LU, LY, MA, MD, ME, MG, **MK**, MN, MW, MX, MY, MZ, NA, NG, **NI**, NO, NZ, OM, PE, PG, **PH**, **PL**, **PT**, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, **TH**, **TJ**, **TM**, TN, **TR**, **TT**, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) **Designated States (unless otherwise indicated, for every kind of regional protection available):** ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, **IT**, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Published:**  
— with international search report (Art. 21(3))

(54) **Title:** PRESSURE INDICATOR

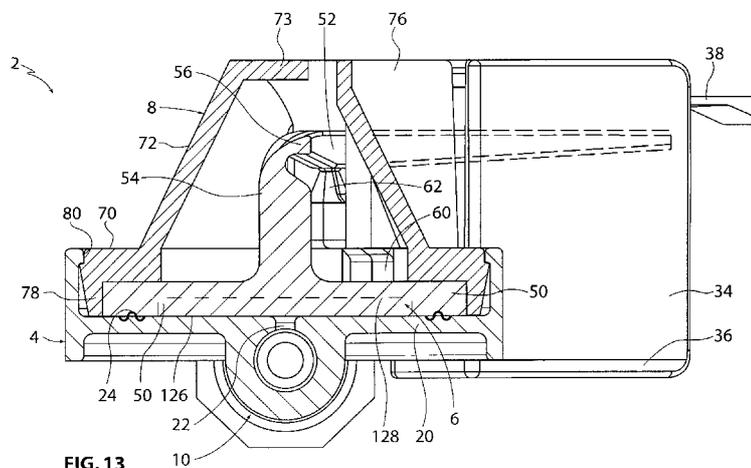

(57) **Abstract:** A pressure indicator: a body having a pressure chamber which has an inlet for communication with a fluid; a resilient diaphragm having a periphery sealed against the body and having one side thereof exposed to the fluid within the chamber; an indicating arm having an inner end which is integrally formed with the other side of the diaphragm and an outer end arm which is adjacent to a scale, the arrangement being such that pressure of the fluid within the chamber causes resilient deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber.

WO 2011/017756 A1

- 1 -

## PRESSURE INDICATOR

This invention relates to a pressure indicator.

5 There are many applications where a low cost pressure indicator is required for  
indicating the pressure of a liquid or gas. Sometimes the liquid or gas is flowing and at  
other times it is hydrostatic.

10 In the medical field, contamination is also a serious problem and it would be highly  
desirable for pressure indicators to be available which were inexpensive so that they could  
be discarded after a single use.

Medical applications include monitoring of the pressure of injectable fluids in  
typical situations as follows:

15 (i) Injections

During the injection of therapeutic agents into human tissue high pressures should  
be avoided where this indicates that the site of the injection is other than intended. Arterial  
injection produces pulsatile pressures of >100 mmHg. Injection into nerves  
characteristically produce static pressures of >1000 mmHg. Injection into tendon's and  
20 other non porous tissues may produce even higher pressures. There is often a need for the  
physician or nurse to be aware of such pressures as the tactile force applied to a syringe is  
not a consistent guide to the pressures generated due to variation in piston diameter  
between syringes of differing capacity,

(ii) Flow Rate Monitoring

25 If a fluid is injected through a fixed resistance then the pressure provides an  
indication of flow rate which is desirable during the injection of antibiotics,  
chemotherapeutic agents and radiological dyes. Such a pressure gauge can be calibrated to  
show the desired flow rate and hence the physician or nurse can easily inject the agent  
within the manufacturer's guidelines.

30 (iii) Pressure monitoring for ancillary equipment

Many medical devices require pressure monitoring as part of their functionality.

- 2 -

The pneumatic pressure devices commonly used to force fluid from Intravenous fluid bags require a pressure gauge for correct pressurisation. Filling of various catheters placed in body cavities arteries etc. These have balloons that are inflated to provide mechanical force to seal or expand against the walls for such cavities or vessels.

5 (iv) Measurement of airway pressure

Various airway management devices (including resuscitation bags) provide positive pressure ventilation for patients lungs, monitoring of this pressure is desirable to avoid barotrauma to the lungs.

10 The characteristics that are important for such a device include:

(i) Cost

Low cost requires low cost components and as well as ease of manufacture.

(ii) Ease of Use

15 Pressure indication that is easily read and preferably with an analogue indicating scale for easy interpretation.

(iii) Minimal Dead Space

If the gauge is used for the injection of fluids it is important that the internal mechanism of the gauge has minimal dead space as this tends to introduce air into the injection system. Further, the therapeutic agent may be of great value and hence it is  
20 undesirable for it to fill the gauge's deadspace and hence to be unavailable for injection. Finally the presence of air in the gauge can blunt the response of the gauge to pressure change.

(iv) Compact Design

It is important that the gauge be of the minimum size practical as in many  
25 applications it is undesirable to have a bulky or heavy device attached to a syringe or other system.

(v) Accuracy

It is important for such a gauge to have appropriate level of accuracy. +/- 7.5% has  
30 been achieved.

- 3 -

It is a general object of the invention to provide a pressure indicator which at least partially satisfies all or some of the criteria above.

According to the present invention there is provided a pressure indicator:

5 a body having a pressure chamber which has an inlet for communication with a fluid;

a resilient diaphragm having a periphery sealed against the body and having one side thereof exposed to the fluid within the chamber;

10 an indicating arm having an inner end which is integrally formed with the other side of the diaphragm and an outer end arm which is adjacent to a scale,

the arrangement being such that pressure of the fluid within the chamber causes resilient deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber.

15 Preferably, the chamber has an outlet and said fluid under pressure, in use, flows from the inlet to the outlet through the chamber.

Preferably, the indicator includes a fulcrum which serves to cause rotation of the arm on resilient deformation of the diaphragm.

20

Preferably, the fulcrum is integrally formed with the diaphragm.

Preferably, the diaphragm, arm and fulcrum are injection moulded from plastics material.

25

Preferably, the indicator includes a first housing coupled to the body, the diaphragm being arranged to resiliently expand into the first housing when the pressure of the fluid increases.

30 Preferably, the first housing includes formations which interlock with complementary formations on the body and wherein, in use, the periphery of the

- 4 -

diaphragm is clamped between the body and the first housing.

Preferably, the fulcrum extends from a mounting point inwardly adjacent to the periphery of the diaphragm.

5

Preferably, the first housing includes guide means which engage or are engagable with the fulcrum to limit displacement of the fulcrum when the diaphragm expands.

Preferably, the indicator includes a second housing, the outer end of the indicating  
10 arm being located within the second housing.

Preferably, the second housing is integrally formed with the body.

The invention also provides a resilient diaphragm for use in a pressure indicator  
15 having a periphery which is, in use, exposed to the fluid within a chamber, and an indicating arm having an inner end which is integrally formed with the diaphragm and an outer end arm which is adjacent, in use, to a scale.

The invention also provides a pressure indicator:  
20 a body having a pressure chamber which has an inlet for communication with a fluid under pressure;

a resilient diaphragm having a periphery sealed against the body and having one side thereof exposed to the fluid within the chamber;

an indicating arm having an inner end which is integrally formed with the other  
25 side of the diaphragm and an outer end arm which is adjacent to a scale;

a first housing includes formations which interlock with complementary formations on the body and wherein, in use, the periphery of the diaphragm is clamped between the body and the first housing,

the arrangement being such that pressure within the chamber causes resilient  
30 deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber,

- 5 -

characterised in that the indicator is formed from only three components.

The invention also provides a pressure indicator:

a body having a pressure chamber which has an inlet for communication with fluid  
5 under positive or negative pressure relative to atmosphere;

a resilient diaphragm having a periphery sealed against the body and having one  
side thereof exposed to the fluid within the chamber;

an indicating arm having an inner end which is integrally formed with the other  
side of the diaphragm and an outer end arm which is adjacent to a scale,

10 the arrangement being such that pressure within the chamber causes resilient  
deformation of the diaphragm which in turn causes the outer end of the arm to move  
relative to the scale thereby indicating the pressure of the fluid in the chamber.

The invention will now be further described with reference to the accompanying  
15 drawings, in which:

Figure 1 is an isometric view of a pressure indicator of the invention;

Figure 2 is an underside isometric view of the indicator;

Figure 3 is an exploded view of the indicator;

Figure 4 is a side view of the indicator;

20 Figure 5 is another side view of the indicator;

Figure 6 is a plan view of the indicator;

Figure 7 is an underside view of the indicator;

Figure 8 is a cross-sectional view along the line 8-8;

Figure 9 is a cross-sectional view along the line 9-9;

25 Figure 10 is a cross-sectional view along the line 10-10;

Figure 11 is an enlarged plan view;

Figure 12 is a cross-sectional view along the line 12-12;

Figure 13 is an enlarged side view;

Figure 14 is a side view of the diaphragm;

30 Figure 15 is another side view of the diaphragm;

Figure 16 is a fragmentary view of part of the housing;

- 6 -

Figure 17 is a fragmentary underside view of the housing;

Figure 18 is a schematic plan view of the housing and part of the diaphragm;

Figure 19 is a side view of the indicator;

Figure 20 shows the indicator in its final assembled position;

5 Figure 21 shows the indicator with the diaphragm deflected;

Figure 22 is a graph showing the deflection of the diaphragm as a function of pressure;

Figure 23 is a diagram showing deflection of the indicator as a function of deflection of the diaphragm; and

10 Figure 24 is an enlarged side view of a modified indicator of the invention.

The drawings show a pressure indicating device 2 of the invention which is especially suited for single use medical applications such as indicating the pressure at which a liquid is injected into a patient via a syringe. Typically the pressure of the fluid  
15 needs to be in the range from 0 to 25psi.

The indicating device 2 of the invention is made from three components which include a main body 4, diaphragm assembly 6 and diaphragm housing 8 as best seen in the exploded view of Figure 3.

20

The main body 4 is preferably injection moulded from plastics material such as clear polycarbonate. The main body 4 includes a conduit 10 which has an inlet 12 formed as a male Luer connector and an outlet 14 formed as a female Luer connector. The inlet and outlets could be interchanged. The conduit 10 is integrally formed with a cup-shaped  
25 body 16 which includes a cylindrical wall 18 and base wall 20. The base wall 20 includes a port 22 which communicates with the interior of the conduit 10. The base wall 20 is essentially flat or planar but it does include an annular projecting rib 24 located somewhat inwardly from the cylindrical wall 18. The cylindrical wall 18 includes an inwardly projecting lip 25 on its upper edge.

30

- 7 -

The main body 4 is integrally formed with an indicator housing 30 which is formed at an angle of about 45° relative to the axis of the conduit 10 as seen in Figure 8. This orientation makes it easier to view the pressure indication as will be described in more detail below. The indicator housing 30 includes two parallel sidewalls 32 and 34 joined by a bottom wall 36. The housing includes a top wall 38 which is moulded in a position where it is generally parallel to the bottom wall 36 and connected to the upper corners of the sidewalls 32 and 34 by means of an integral hinge 40. This is the preferred way of forming the top wall because it would be difficult to injection mould the main body 4 with a fixed top wall joining the upper edges of the sidewalls 32 and 34. One or other of the walls 32 or 34 could be moulded with a pressure scale (not shown) which in use is adjacent to the indicating arm of the device so as to enable the pressure to be read. Alternatively, the scale could be printed onto one or other of these walls. Normally it is preferred that the scale be printed onto the sidewall 34 so that an operator can view the position of the indicating arm through the sidewall 32 against the scale so as to obtain a pressure reading.

15

The diaphragm assembly 6 will now be described in more detail with reference to Figures 3, 14 and 15. The diaphragm assembly is injection moulded from silicone rubber preferably having a Shore A hardness in the range 50 to 55. It includes a diaphragm 50 in the form of a circular disc preferably of uniform thickness, the thickness typically being in the range from 1.5mm to 2.5mm and preferably about 2mm. The diaphragm is integrally moulded with an indicating arm 52 which is joined to the centre of the diaphragm 50 by means of an upstanding post 54 via an integral hinge 56. The diaphragm assembly 6 includes a bracket 58 which is also integrally moulded with the diaphragm 50 and the indicating arm 52. The bracket 58 includes a lower leg which is connected to the diaphragm 50 inwardly adjacent to the periphery of the diaphragm, as best seen in Figure 15. The bracket includes a second leg 62 which is joined to the underside of the indicating arm 52 and serves as a fulcrum about which the indicating arm 52 can rotate, as will be described in more detail below. As can be seen from Figure 14, the first leg 60 is somewhat wider than the second leg 62. Also, the first leg 60 includes first and second blind bores 64 and 66.

30

- 8 -

The diaphragm housing 8 will now be described in more detail with reference to Figures 3, 13, 16, 17 and 18.

The diaphragm housing 8 is injection moulded from clear polycarbonate as an integral moulding. It includes an annular base 70 from which extends a hollow frustoconical projection 72 which is partly closed by means of a top wall 73. As can best be seen from Figure 3, the frustoconical projection 72 includes a gap which is bounded by two flanges 74 and 76 which extend from the annular base 70 to the top wall 73. The housing 8 includes a tapered flange 78 which extends downwardly from the outer periphery of the base 70, as best seen in Figure 13. In addition, the outer peripheral edge of the annular base 70 includes a rebate 80.

The arrangement and dimensions of the three components are such that the diaphragm 50 is clamped between the main body 4 and the housing 8 with the indicating arm 52 projecting between the flanges 74 and into the indicator housing 30. More particularly, it will be seen from Figure 13 that the diaphragm 50 rests on the base wall 20 of the main body 4. Its outer peripheral region engages the underside of the annular base 70 of the housing 8 and the outer peripheral wall engages the inner periphery of the flange 78. During assembly, the diaphragm assembly is first fitted into the diaphragm housing 8 so that the indicating arm 52 projects outwardly between the flanges 74 and 76. The indicating arm 52 is aligned relative to the sidewalls 32 and 34 so that the diaphragm housing 8 and diaphragm assembly 6 can be lowered so that the indicating arm 52 enters the indicator housing 30 between the sidewalls 32 and 34. The diaphragm housing 8 and main body 4 are then pressed together so that the tapered flange is snap fit into the cylindrical 18 and the lip 25 interlocks with the rebate 80 so that the diaphragm housing 8 and main body 4 are interlocked with the diaphragm 50 sealingly engaged therebetween. It will be seen from Figure 13 that the rib 24 presses into the underside of the diaphragm 50 and resiliently deforms it so as to enhance the seal between the outer region of the diaphragm 50 and the base wall 20 of the main body 4.

- 9 -

After the three components have been fitted together, as described above, the top wall 38 can be rotated into its final position. This is schematically illustrated in Figures 19 and 20 where the top wall has been rotated anti-clockwise through approximately 180° so that the top wall 38 closes the gap between the sidewalls 32 and 34 and is sufficiently long so that it effectively closes the gap between the flanges 74 and 76. This protects the indicating arm 52 from being inadvertently displaced. The top wall 38 includes laterally extending projections 90 and 92 which interlock with complementary projections 94 and 96 formed adjacent to the upper edges of the sidewalls 32 and 34.

In use of the pressure indicating device 2 of the invention, fluid under pressure is located within the conduit 10. The fluid can be static or flowing. The port 22 communicates the pressurised fluid with the underside of the diaphragm 50 and, depending on the pressure of the fluid, the diaphragm 50 will resiliently deform, as schematically illustrated in Figure 20. It will be appreciated that as the diaphragm 50 deflects upwardly, the indicating arm 52 will be caused to rotate in a generally clockwise direction as seen in Figure 20. The extent of deflection of the indicating arm 52 is proportional to the extent of deflection of the diaphragm 50. Deflection of the diaphragm 50 is also generally proportional to the pressure within the conduit 10, as will be described in more detail below.

20

It will be appreciated that the second leg 62 which serves as the fulcrum for the indicating arm 52 is not completely independent of movement of the diaphragm 50 since it forms part of the bracket 58 which is moulded integrally with the diaphragm 50. The illustrated device includes components which serve to stabilise the position of the indicating arm 52 so as to tend to make deflection of the indicating arm 52 more truly proportional to the pressure within the conduit 10. In the illustrated arrangement, the width of the first leg 60 is such that it is snugly received between inner flanges 100 and 102 which can be regarded as being contiguous with the flanges 74 and 76 respectively. The flanges 100 and 102 have inwardly directed conical pins 104 and 106 formed therewith. The arrangement is such that the conical pins 104 and 106 are received within the bores 64 and 66 respectively as shown in the schematic plan view of Figure 18. This

30

- 10 -

serves to further fix the position of the legs 60 and 62 relative to the main body 4 and diaphragm housing 8 so as to minimise movement of the fulcrum for the indicating arm 52.

A prototype of the pressure indicating device 2 has been constructed and tested. In the prototype, the diaphragm 50 had a nominal diameter of 18mm and the length of the indicating arm 52 about 22mm as measured from the centre line of the post 54.

The deflection of the diaphragm depends on the thickness of the diaphragm as well as its hardness. Table 1 below shows the typical deflection at the end of the indicating arm 52 for diaphragms of different thicknesses. In each case the hardness was Shore A 50.

<b>Diaphragm Thickness (mm)</b>	<b>Deflection of indicator at 25psi (mm)</b>
1.6	12.8
1.8	8.4
2.0	5.8

Figure 22 shows the average deflection of the diaphragm 50 as a function of the pressure within the conduit 10. Figure 23 is a diagram showing the theoretical deflection at the tip of the indicating arm 52 as a function of deflection of the diaphragm. It will be seen that the relationship is approximately linear.

In the illustrated arrangement, the main body 4 is formed with a conduit 10 which has an inlet and outlet which is appropriate for pressure measurement where the fluid under pressure flows through the conduit. It would be possible to block one of the outlets where the device was to be used for measurement of a fluid which is not flowing through the device. Alternatively, the main body 4 could be moulded with a single inlet port without an outlet.

The pressure indicator 2 described above is a compact and inexpensive device for indicating pressures. It is capable of indicating positive pressures, that is to say pressures above atmospheric. It is also possible to indicate negative pressures, that is to say

- 11 -

pressures which are less than atmospheric. In other words, when there is a negative pressure at the port 22 the diaphragm 50 will be resiliently deformed in a direction towards the port 22. It is possible to modify the arrangement by changing the shape of the base wall 20 in order to accommodate greater degrees of resilient deformation of the diaphragm 50 when subjected to negative pressures.

Figure 24 illustrates a modified indicator 120 which is modified slightly so that it can indicate positive as well as negative pressures. In this embodiment, the same reference numerals have been used to denote parts which are the same as or correspond to those of the earlier embodiment. More particularly, Figure 24 corresponds to Figure 13 of the previous embodiment. It will be seen that the base wall 20 includes a concave dish formation 122 which can permit a greater degree of downward resilient flexure of the diaphragm 50 when the pressure within the port 22 is less than atmospheric. In this embodiment, the indicator arm 52 is arranged so that it occupies a central position within the indicator housing 30 when at rest or subject to zero pressure in the port 22. When positive pressures are applied in the port 22, the diaphragm 50 flexes upwardly so that the indicator arm 52 moves downwardly so as to indicate positive pressures against the scale 124 which is applied to or on the sidewalls 32 or 34 or both of them. When, however, a negative pressure is applied to the port 22, the diaphragm 50 is deflected downwardly so that the indicator arm 52 moves upwardly so as to indicate negative pressures against the scale 124.

As indicated above, the modified indicator 120 is specially designed so that it can readily indicate positive as well as negative pressures. A modification can be readily made to the device shown in Figures 1 to 23 so that it is better able to indicate both positive and negative pressures. More particularly, the lower face 126 of the diaphragm 50 can be partially removed, say for instance at broken line 128 shown in Figure 13. If the disc of material bounded by the broken line 128 were removed this would create a gap between the stepped lower face of the diaphragm 50 and the base wall 20 which would enable a greater degree of downward deflection of the diaphragm 50 and hence the modified device would also be better able to indicate positive as well as negative pressures.

- 12 -

Many modifications will be apparent to those skilled in the art without departing from the spirit and scope of the invention.

- 13 -

## LIST OF PARTS

	pressure indicating device	2
	main body	4
5	diaphragm assembly	6
	diaphragm housing	8
	conduit	10
	inlet	12
	outlet	14
10	cup-shaped body	16
	cylindrical wall	18
	base wall	20
	port	22
	annular rib	24
15	inwardly projecting lip	25
	indicator housing	30
	sidewalls	32, 34
	bottom wall	36
	top wall	38
20	hinge	40
	diaphragm	50
	indicating arm	52
	upstanding post	54
	hinge	56
25	bracket	58
	first leg	60
	second leg	62
	1st and 2nd blind bores	64, 66
	annular base	70
30	frustoconical projection	72
	top wall	73

- 14 -

	flanges	74, 76
	tapered flange	78
	rebate	80
	laterally extending projection	90, 92
5	projections	94, 96
	inner flanges	100, 102
	pins	104, 106
	indicator	120
	concave dish formation	122
10	scale	124
	lower face	126
	broken line	128

## CLAIMS:

1. A pressure indicator:  
a body having a pressure chamber which has an inlet for communication with a  
5 fluid;  
a resilient diaphragm having a periphery sealed against the body and having one  
side thereof exposed to the fluid within the chamber;  
an indicating arm having an inner end which is integrally formed with the other  
side of the diaphragm and an outer end arm which is adjacent to a scale,  
10 the arrangement being such that pressure of the fluid within the chamber causes  
resilient deformation of the diaphragm which in turn causes the outer end of the arm to  
move relative to the scale thereby indicating the pressure of the fluid in the chamber.
2. An indicator as claimed in claim 1 wherein the chamber has an outlet and said fluid  
15 under pressure, in use, flows from the inlet to the outlet through the chamber.
3. An indicator as claimed in claim 1 or 2 wherein the indicator includes a fulcrum  
which serves to cause rotation of the arm on resilient deformation of the diaphragm.
- 20 4. An indicator as claimed in claim 3 wherein the fulcrum is integrally formed with  
the diaphragm.
5. An indicator as claimed in claim 4 wherein the diaphragm, arm and fulcrum are  
injection moulded from plastics material.  
25
6. An indicator as claimed in claim 5, wherein the indicator includes a first housing  
coupled to the body, the diaphragm being arranged to resiliently deflect into the first  
housing when the pressure of the fluid increases above atmospheric pressure.
- 30 7. An indicator as claimed in claim 5 or 6 wherein the body has a base wall and  
wherein said one side of the diaphragm is spaced from the base wall so that the diaphragm

- 16 -

can resiliently deflect towards said base wall when the pressure of the fluid decreases below atmospheric pressure.

8. An indicator as claimed in claim 6 or 7 wherein the first housing includes  
5 formations which interlock with complementary formations on the body and wherein, in use, the periphery of the diaphragm is clamped between the body and the first housing.

9. An indicator as claimed in claim 6, 7 or 8 wherein the fulcrum extends from a mounting point inwardly adjacent to the periphery of the diaphragm.

10

10. An indicator as claimed in claim 9 wherein the first housing includes guide means which engage or are engagable with the fulcrum to limit displacement of the fulcrum when the diaphragm expands.

15 11. An indicator as claimed in any one of claims 7 to 10 including a second housing, the outer end of the indicating arm being located within the second housing.

12. An indicator as claimed in claim 11 wherein the second housing is integrally formed with the body.

20

13. A resilient diaphragm for use in a pressure indicator having a periphery which is, in use, exposed to the fluid within a chamber, and an indicating arm having an inner end which is integrally formed with the diaphragm and an outer end arm which is adjacent, in use, to a scale.

25

14. A pressure indicator:

a body having a pressure chamber which has an inlet for communication with a fluid under pressure;

a resilient diaphragm having a periphery sealed against the body and having one  
30 side thereof exposed to the fluid within the chamber;

an indicating arm having an inner end which is integrally formed with the other

- 17 -

side of the diaphragm and an outer end arm which is adjacent to a scale;

a first housing includes formations which interlock with complementary formations on the body and wherein, in use, the periphery of the diaphragm is clamped between the body and the first housing,

5 the arrangement being such that pressure within the chamber causes resilient deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber, characterised in that the indicator is formed from only three components.

10 15. A pressure indicator:

a body having a pressure chamber which has an inlet for communication with fluid under positive or negative pressure relative to atmosphere;

a resilient diaphragm having a periphery sealed against the body and having one side thereof exposed to the fluid within the chamber;

15 an indicating arm having an inner end which is integrally formed with the other side of the diaphragm and an outer end arm which is adjacent to a scale,

the arrangement being such that pressure within the chamber causes resilient deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber.


20

16. A resilient diaphragm for a pressure indicator, said diaphragm having a periphery which is, in use, sealed against a body having a pressure chamber therein and one side of the diaphragm is subjected, in use, to the pressure within the chamber, the diaphragm including:


25 an indicating arm having an inner end which is integrally formed with the other side of the diaphragm and an outer end arm which is, in use, adjacent to a scale,

the arrangement being such that, in use, pressure within the chamber causes resilient deformation of the diaphragm which in turn causes the outer end of the arm to move relative to the scale thereby indicating the pressure of the fluid in the chamber.




30

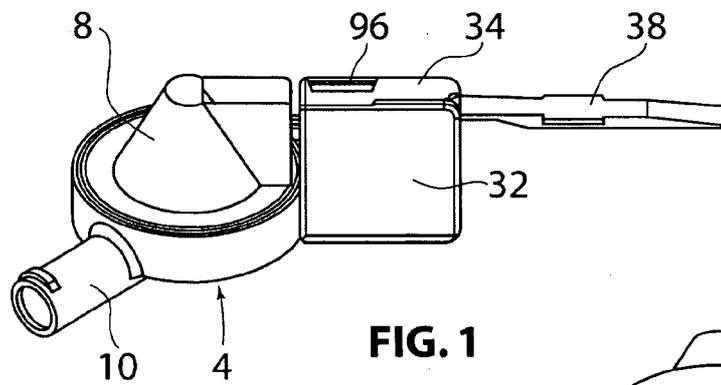


**FIG. 1**

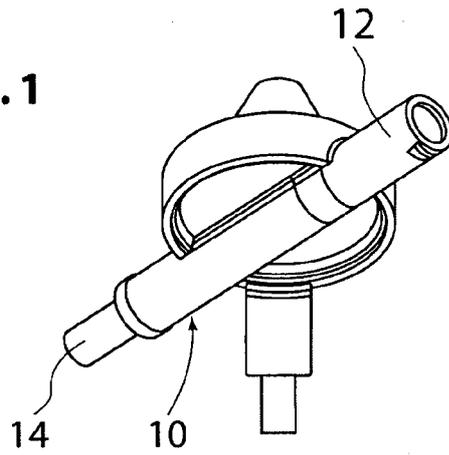


**FIG. 2**

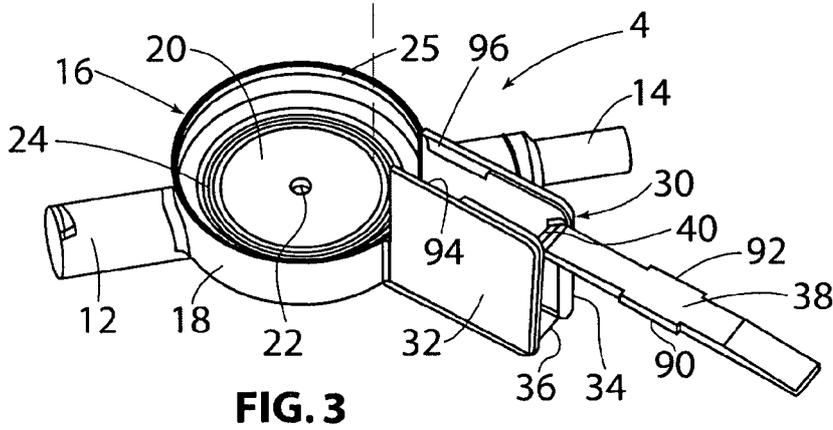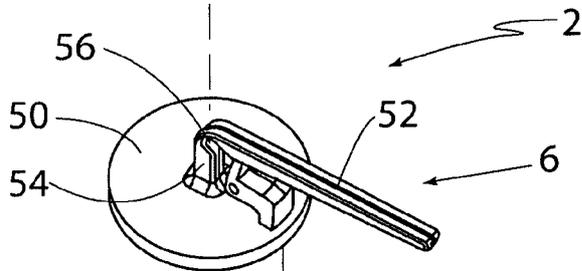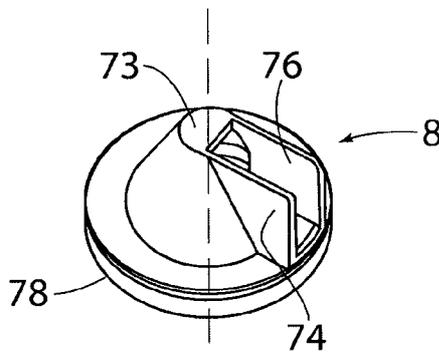

**FIG. 3**

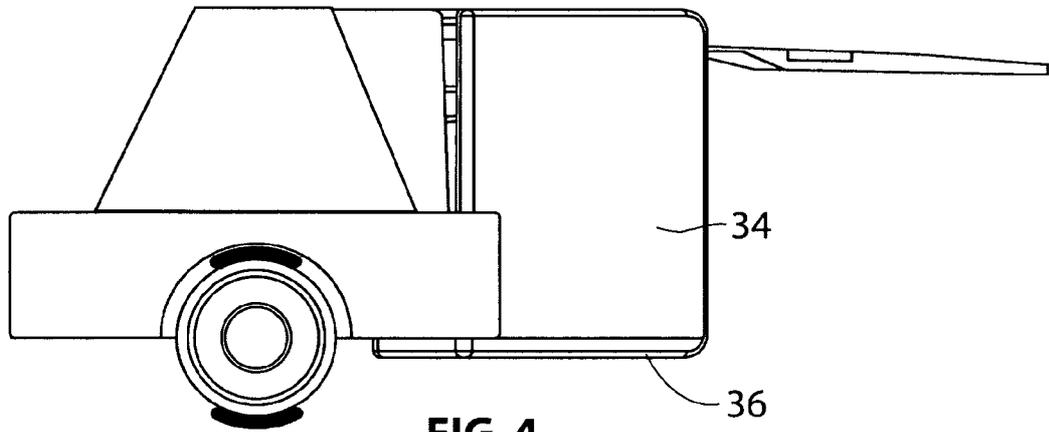

**FIG. 4**

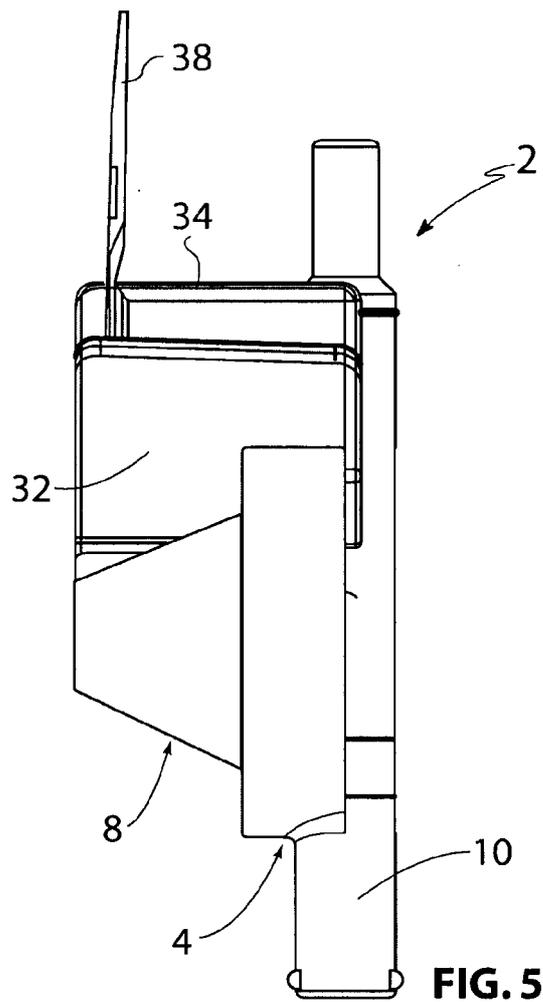

**FIG. 5**



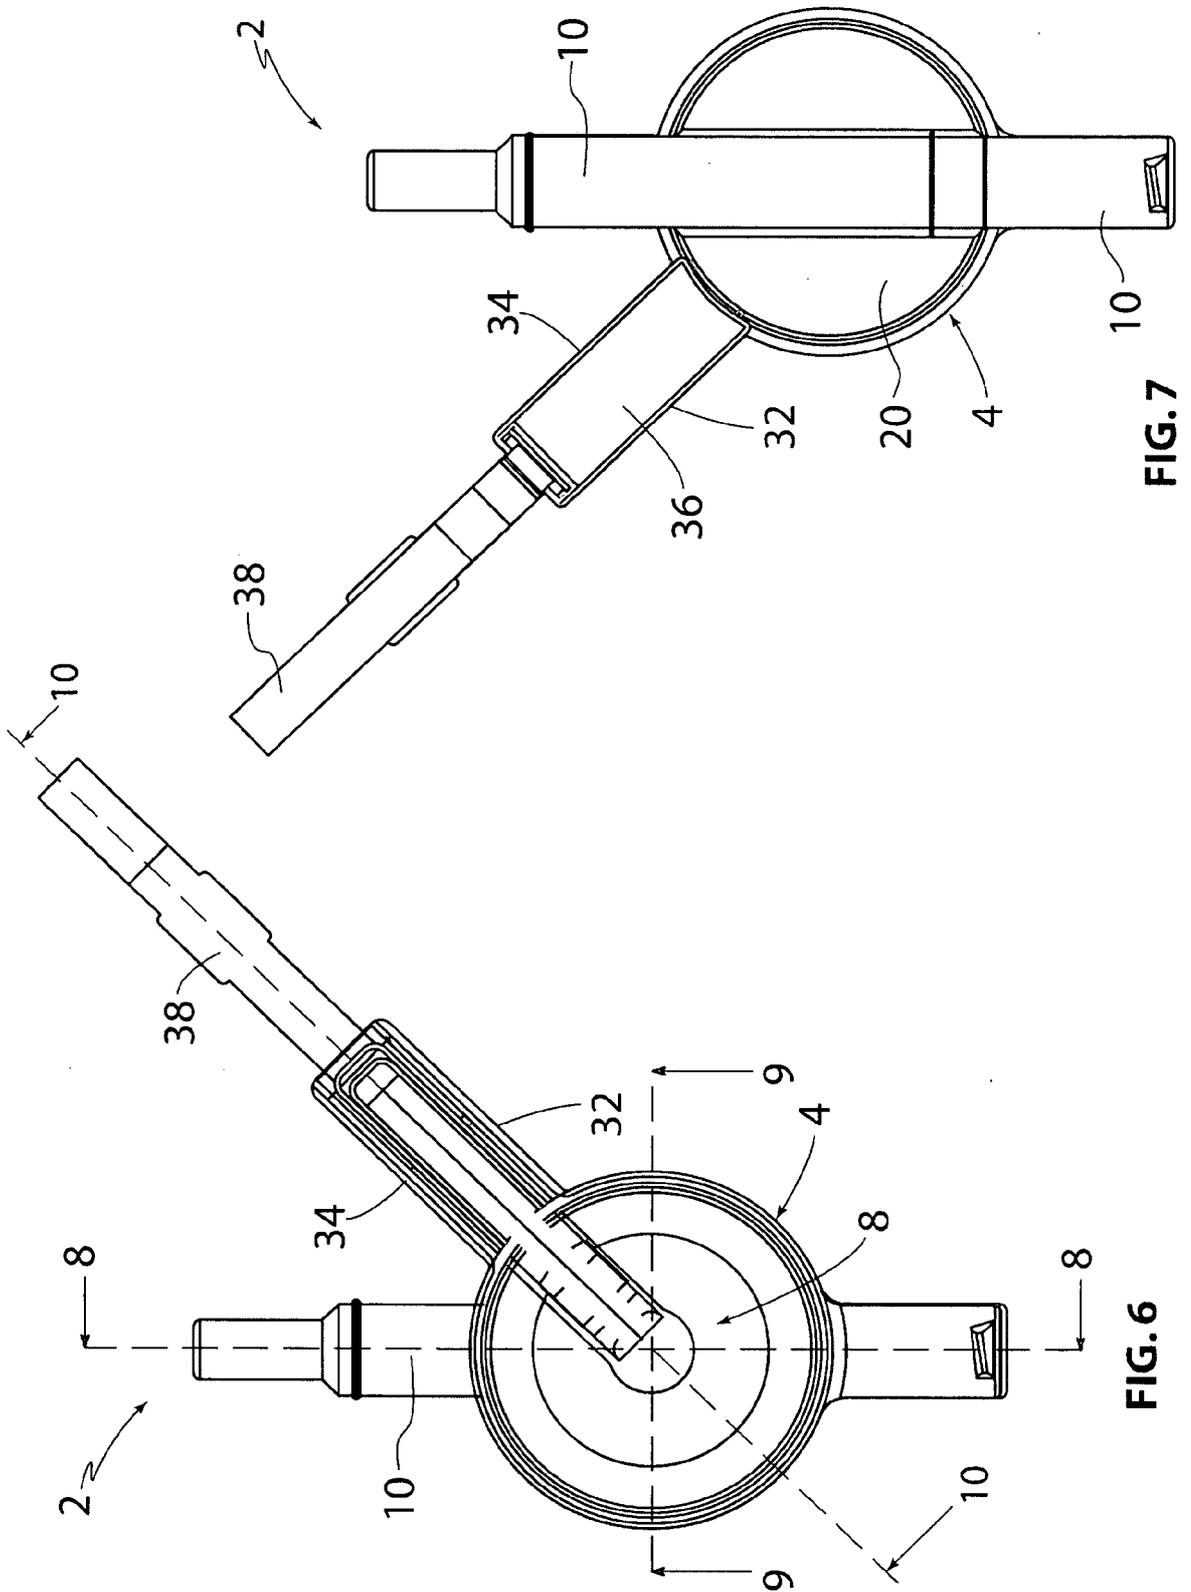


FIG. 7


FIG. 6

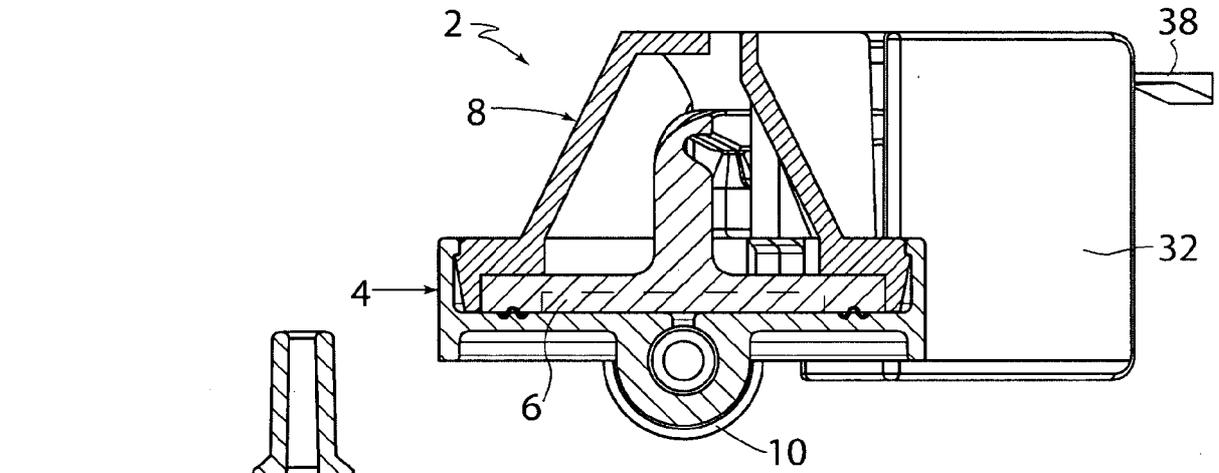


**FIG. 9**

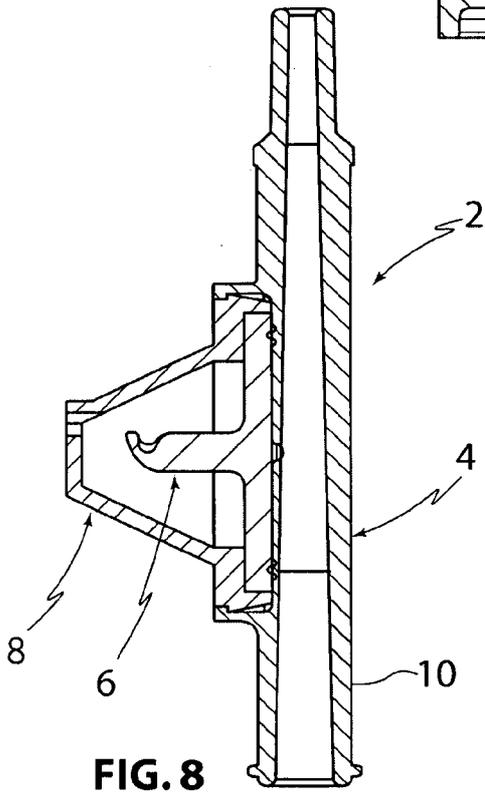

**FIG. 8**

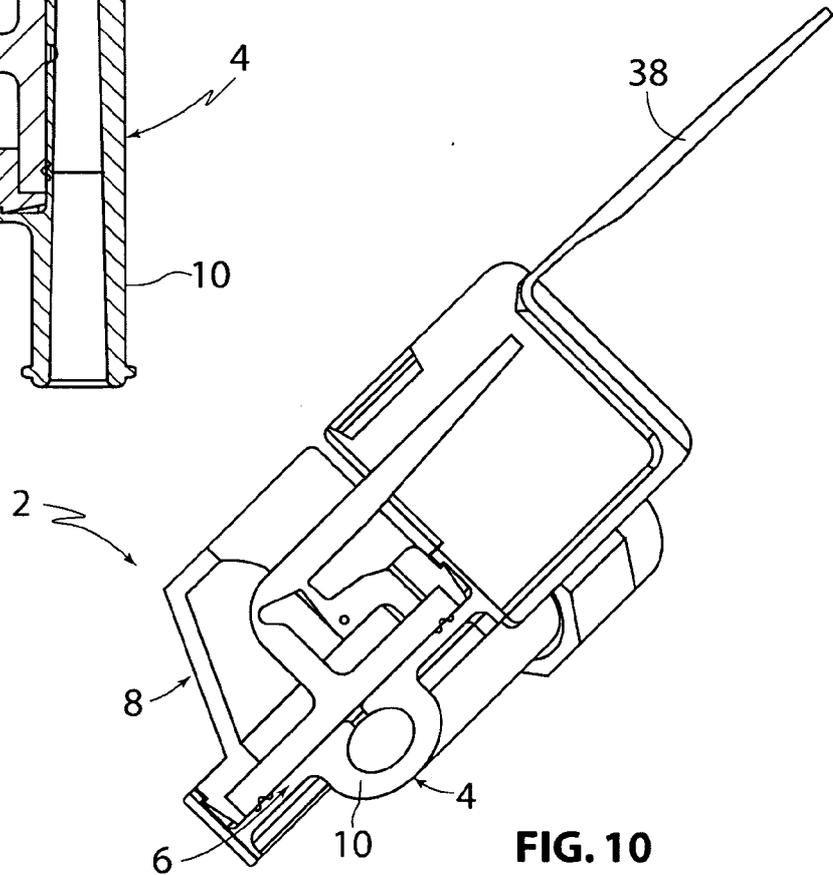

**FIG. 10**

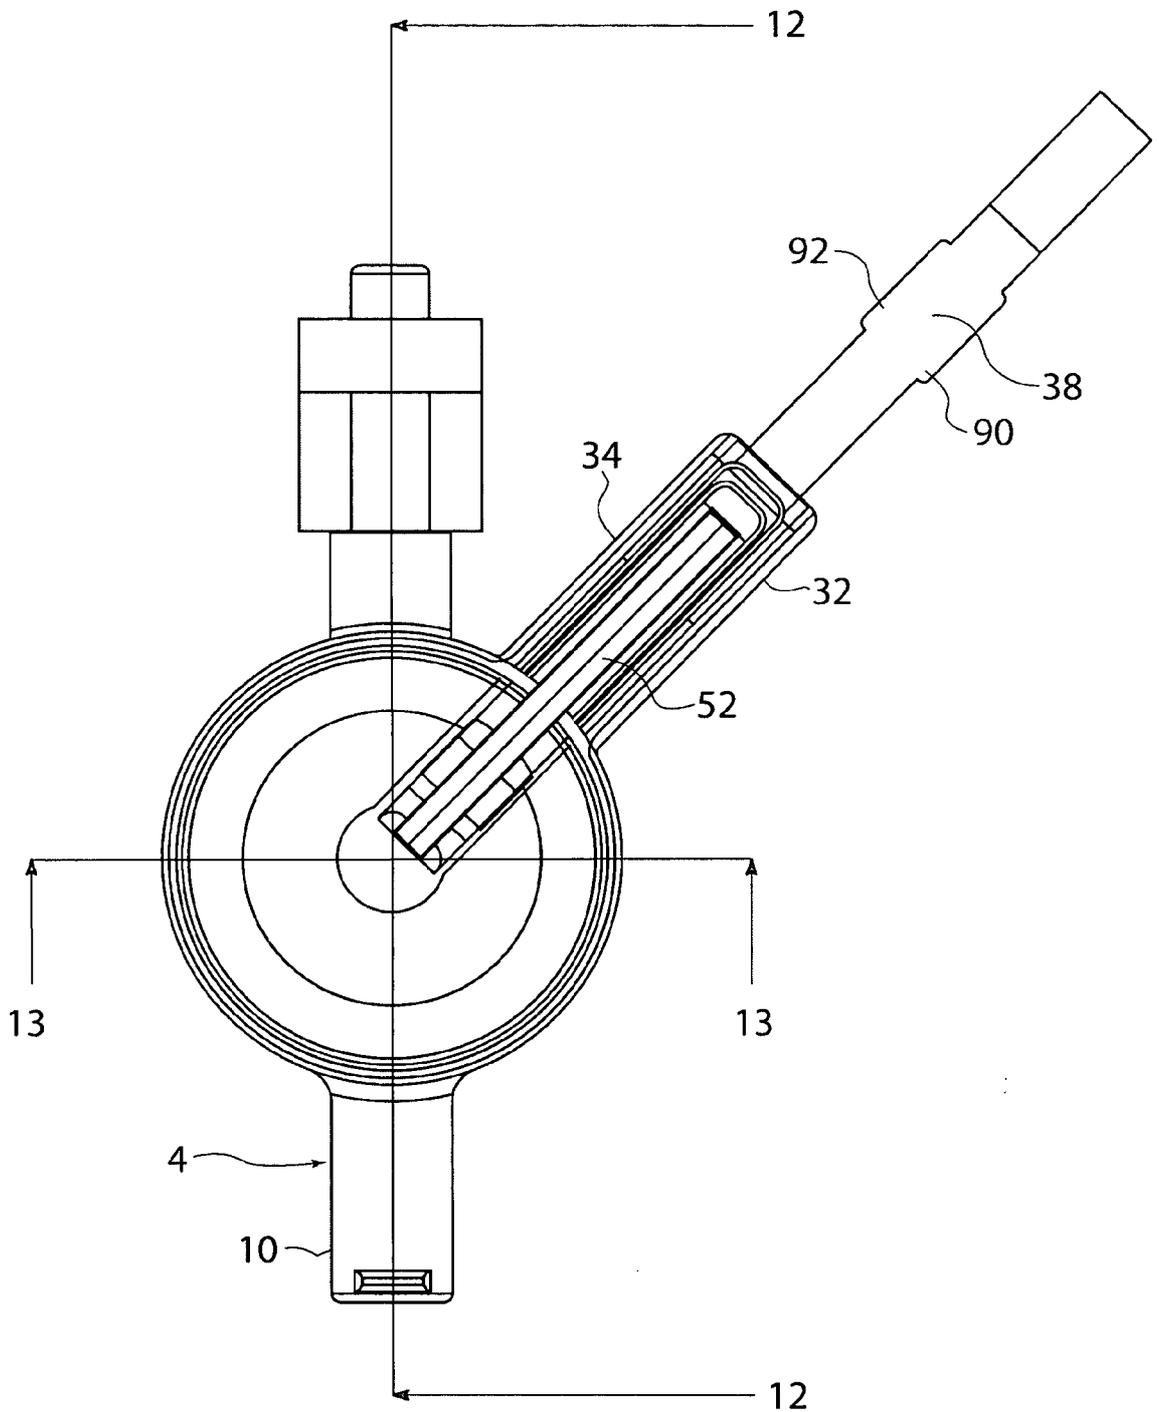

**FIG. 11**

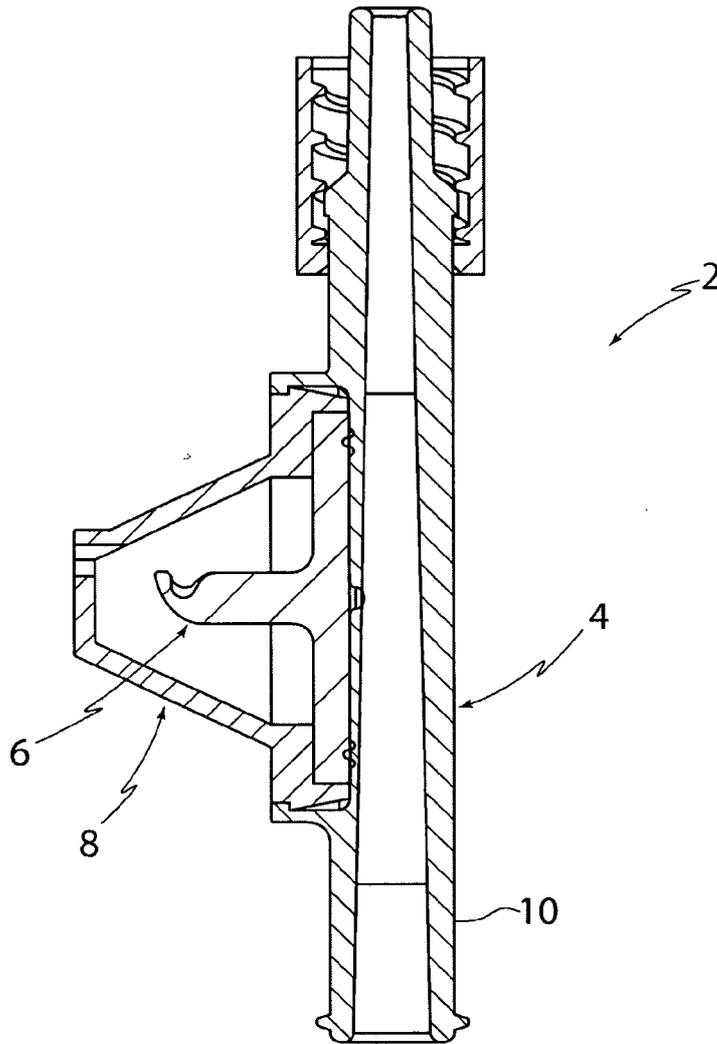
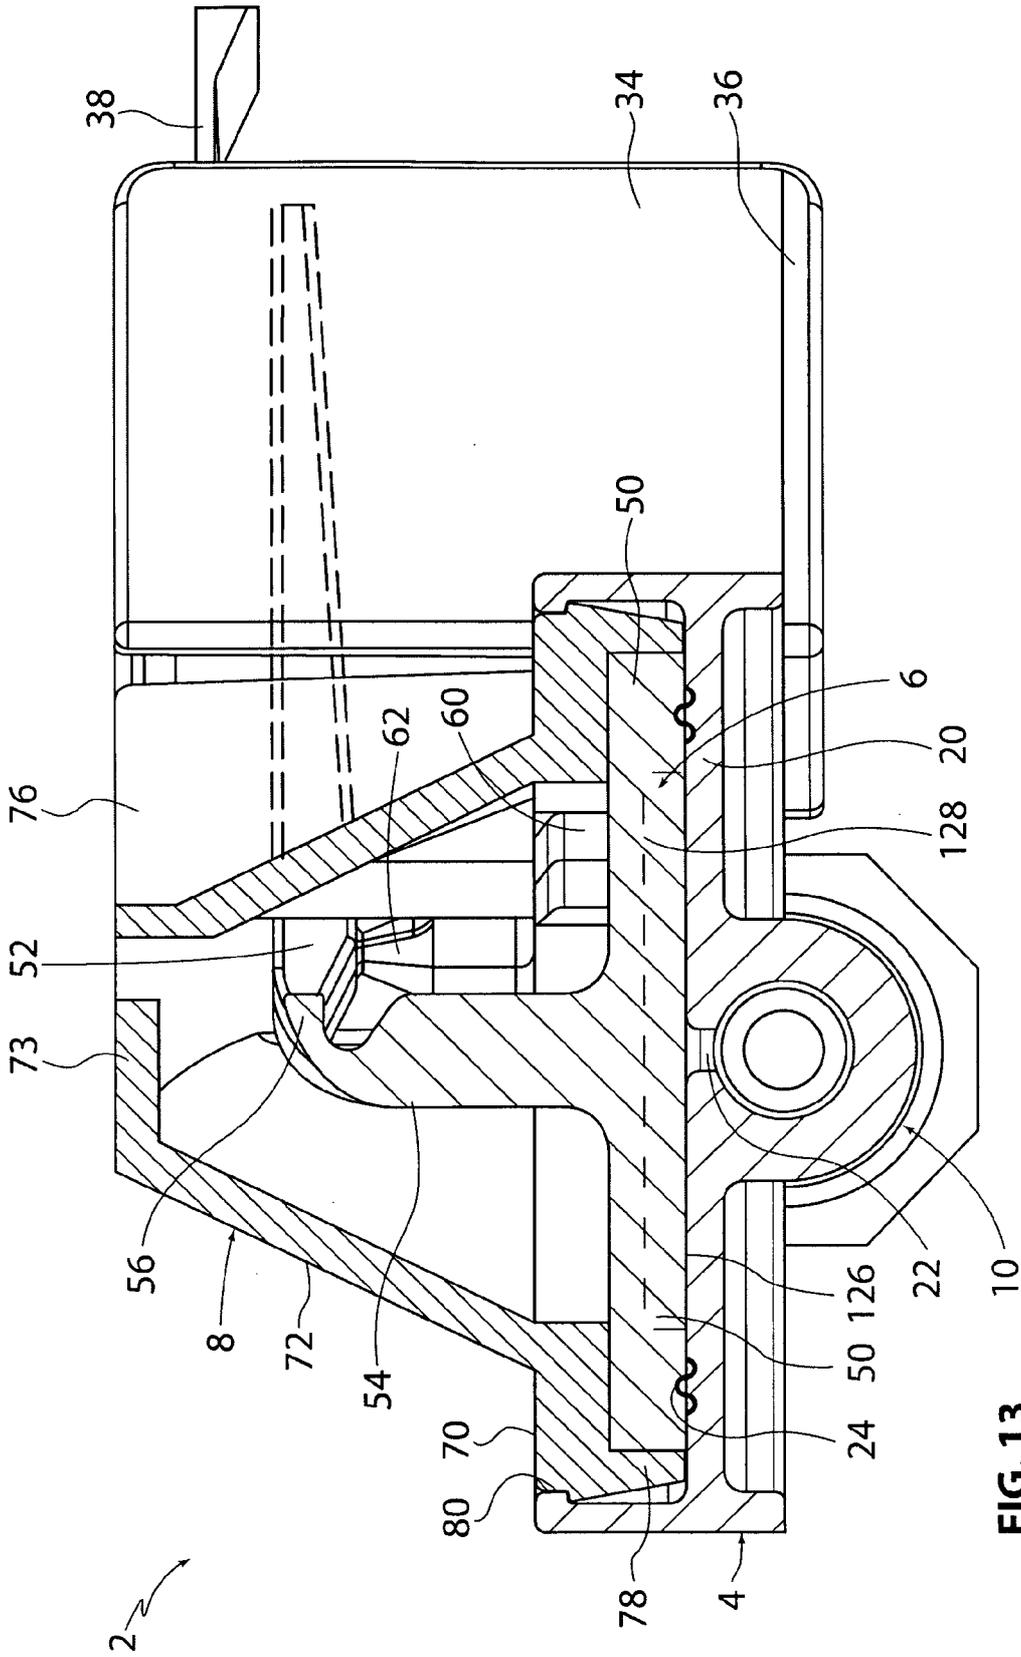


FIG. 12



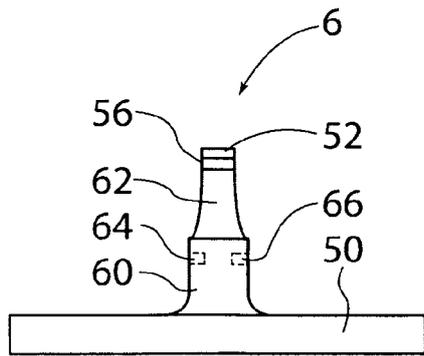


FIG. 14

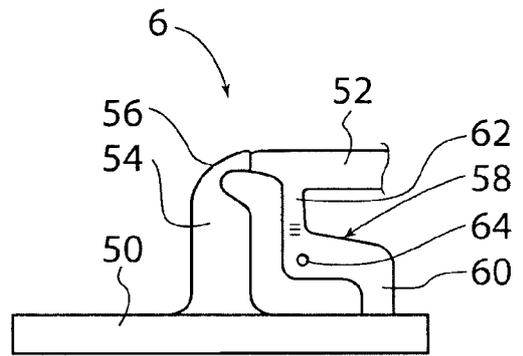


FIG. 15

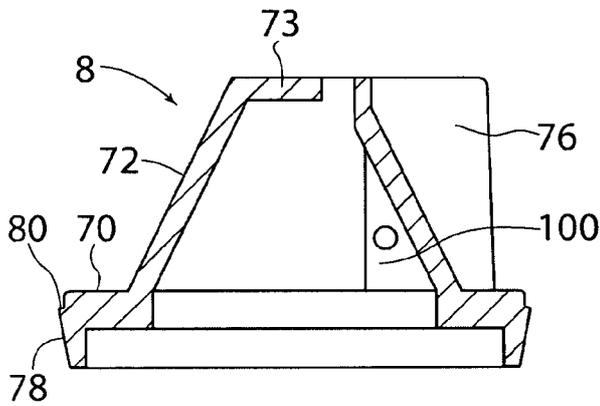


FIG. 16

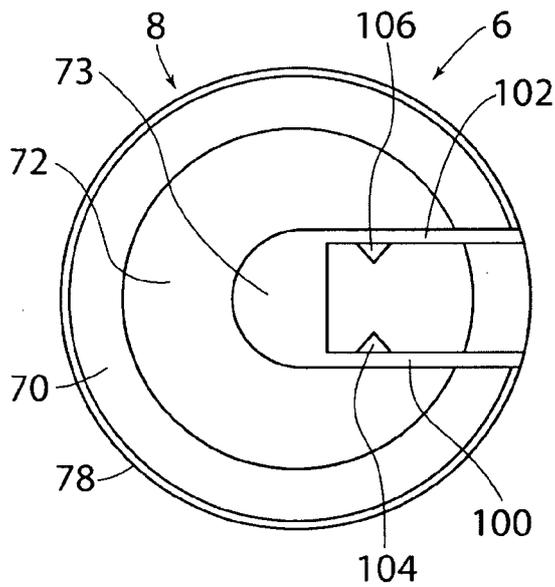


FIG. 17



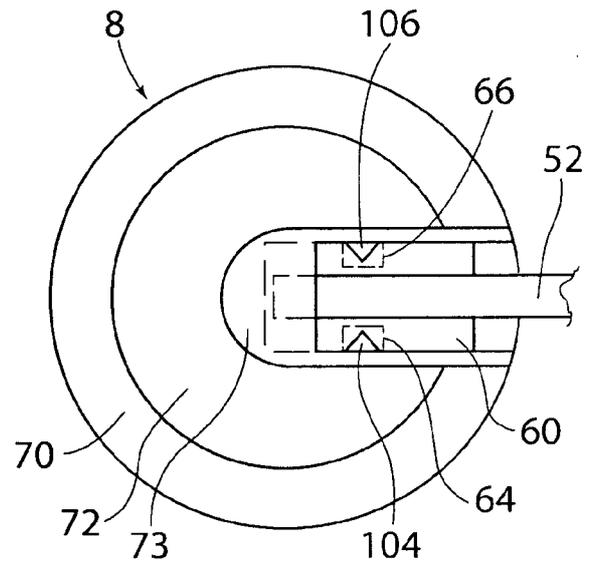



FIG. 18

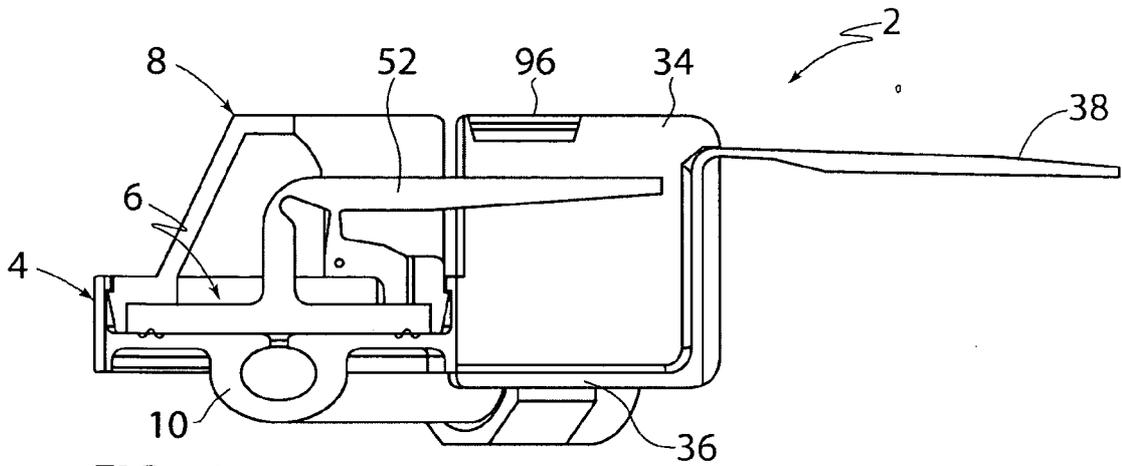

**FIG. 19**

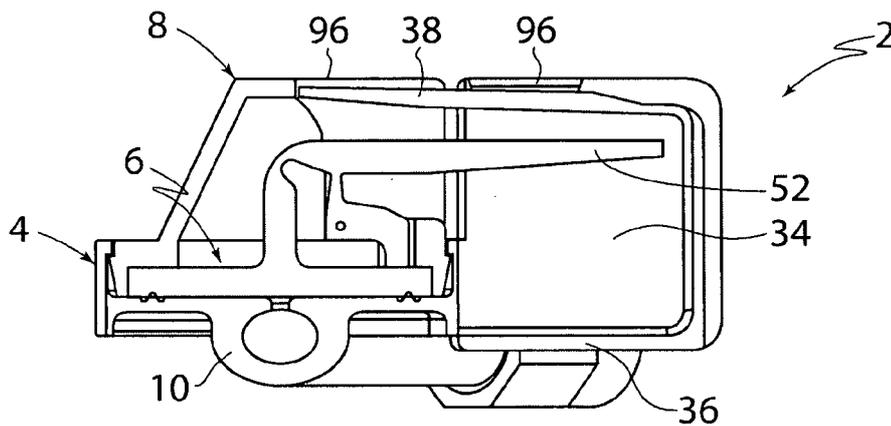

**FIG. 20**

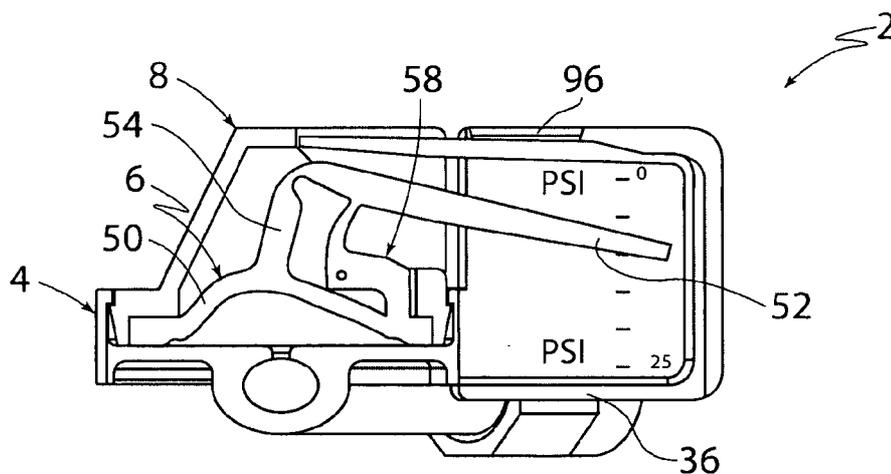

**FIG. 21**

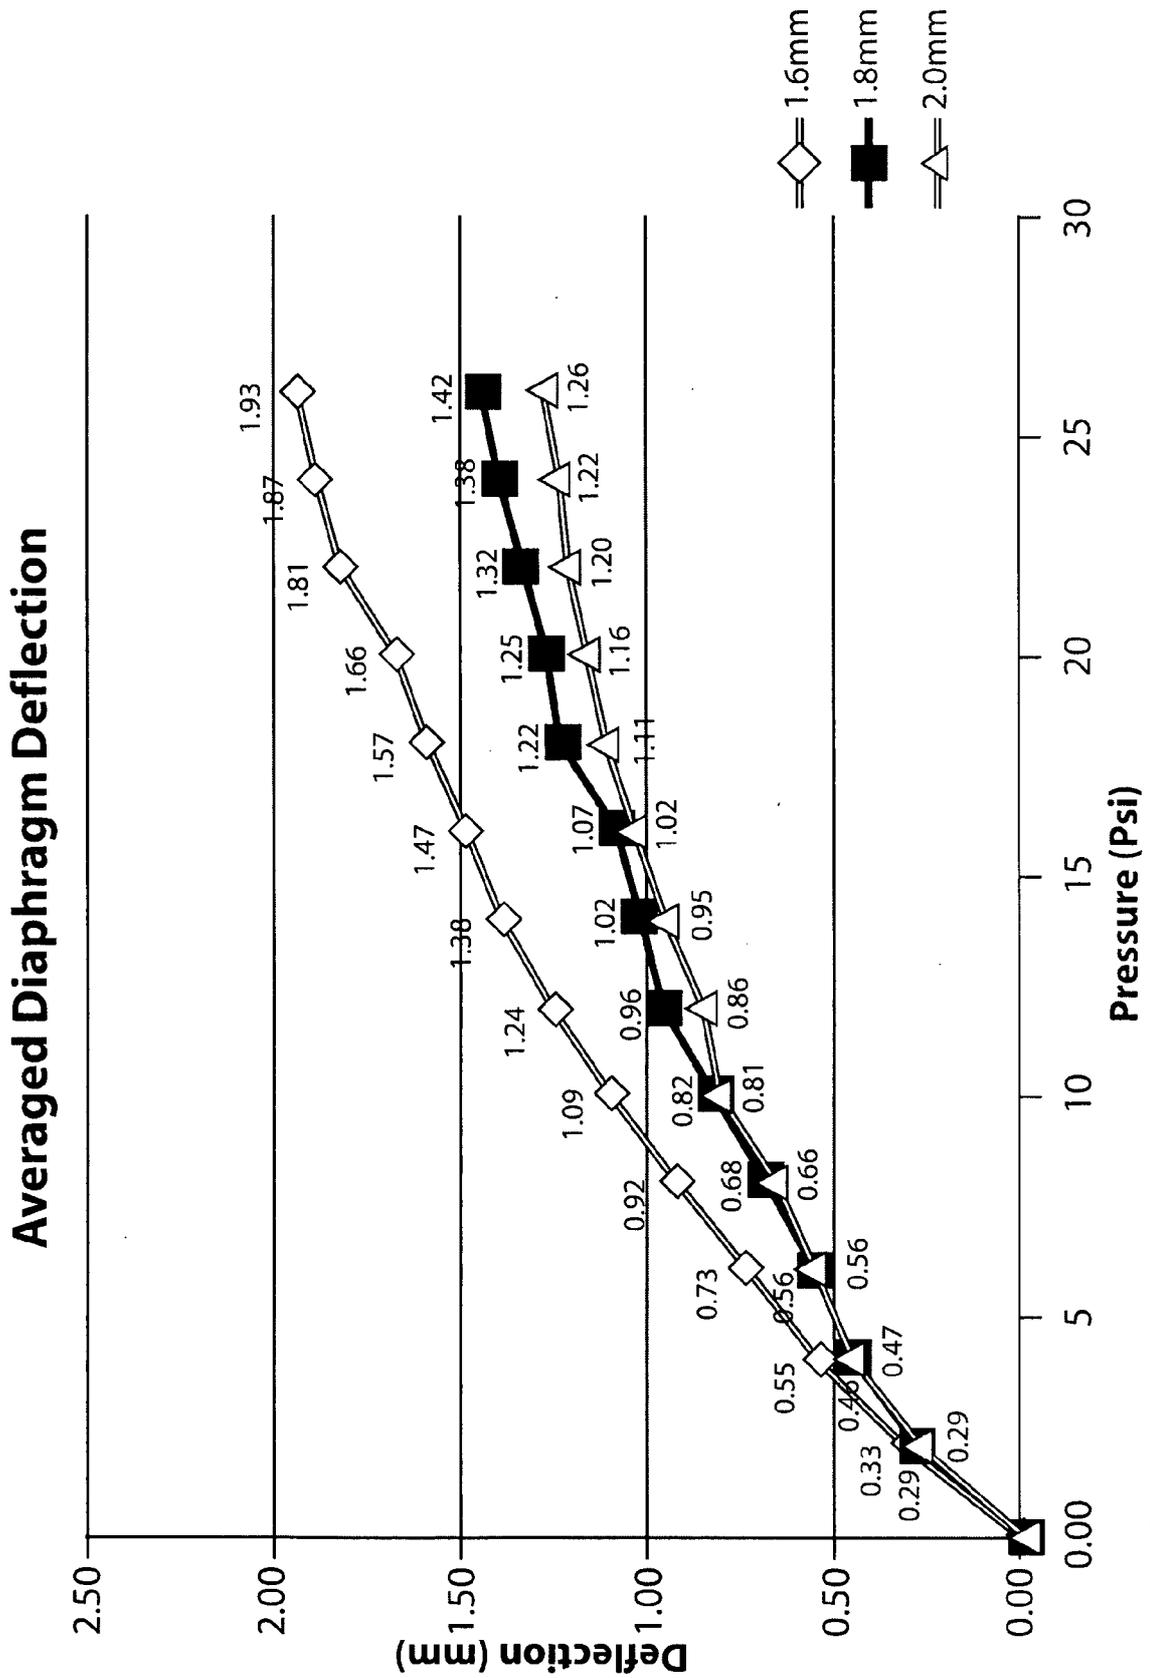


FIG. 22

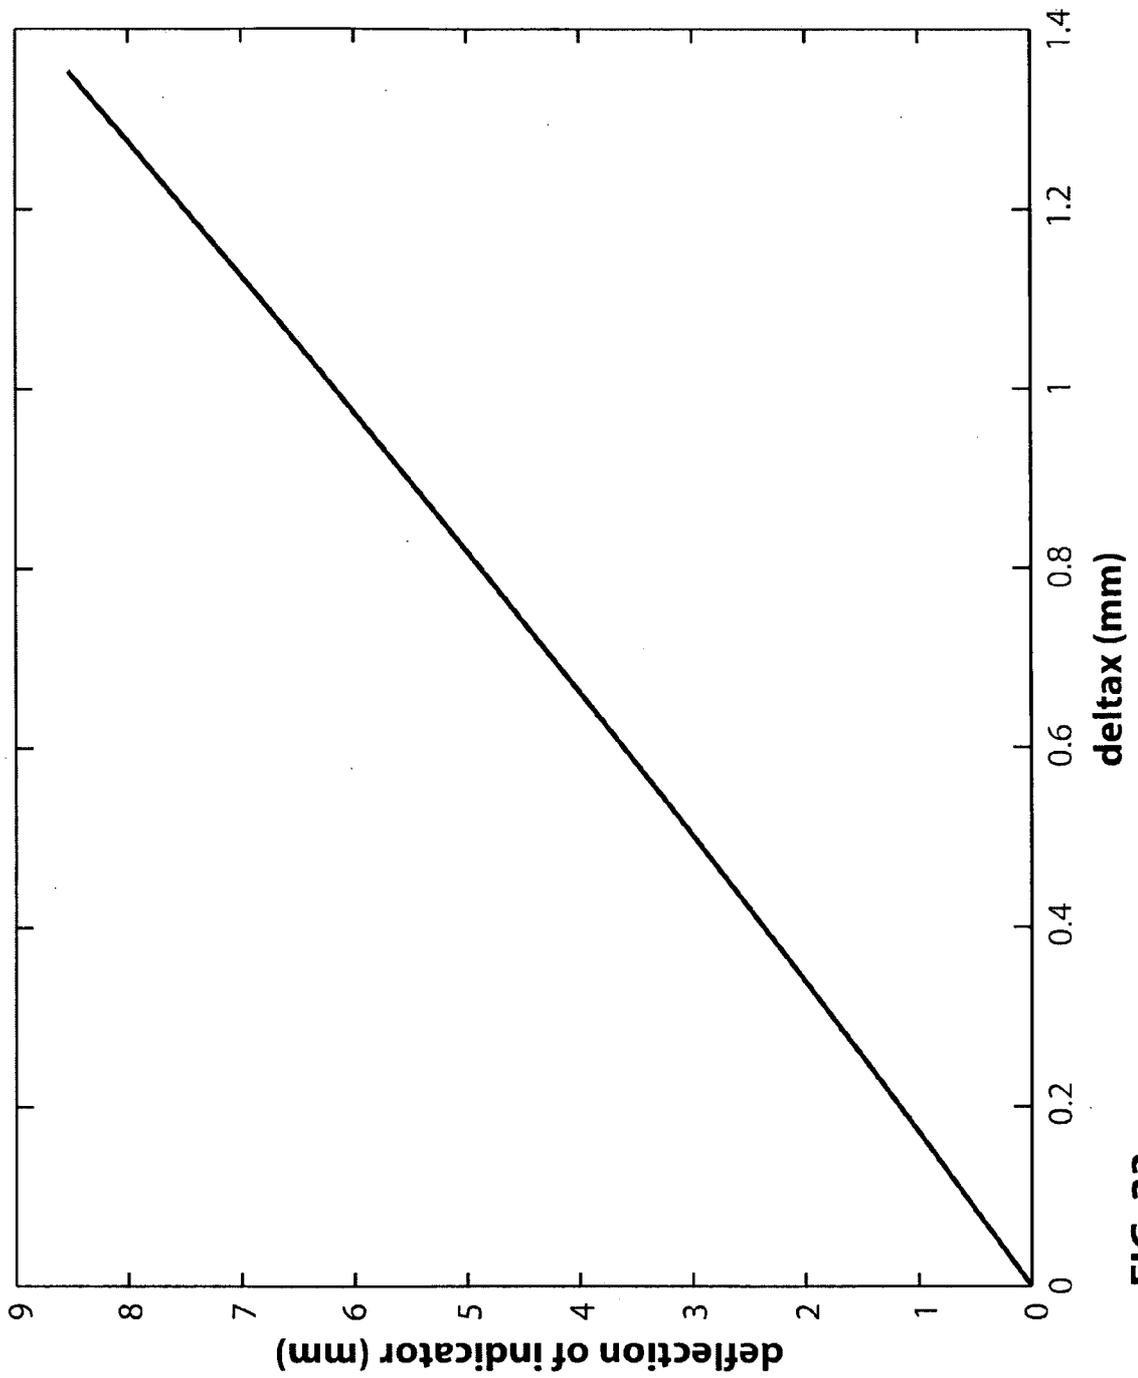


FIG. 23

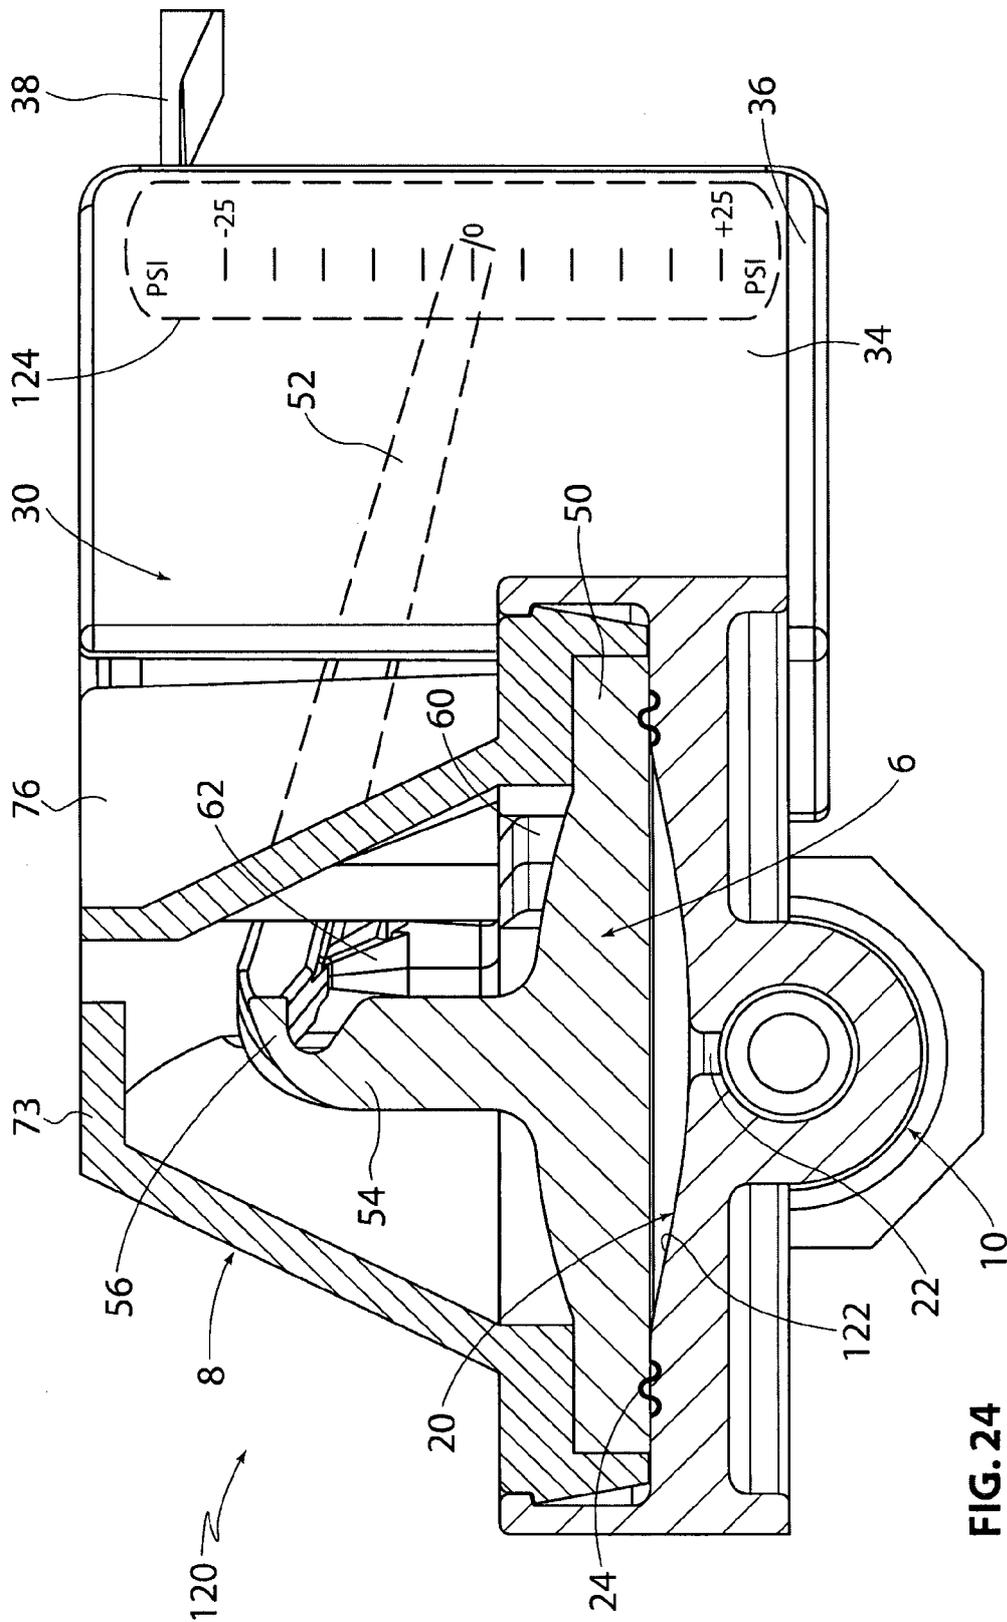


FIG. 24

## INTERNATIONAL SEARCH REPORT

International application No

PCT/AU20 10/00 1024

## A CLASSIFICATION OF SUBJECT MATTER

Int Cl

GOIL 7/08 (2006 01)

According to International Patent Classification (IPC) or to both national classification and IPC

## B FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPODOC, WPI IPC GOIL with keywords pressure, diaphragm, bellow, membrane, scale, mark, dial meter, point, ruling, graduation, indicate, measure, display, guage, chamber, volume, space

## C DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No
X	US 5935084 A (SOUTHWORTH) 10 August 1999 Figures 2, 5, 7, 9 and 10	1-3, 13-16
A	US 4096759 A (DESOR) 27 June 1978	1-3, 5, 13, 15, 16
A	US 2252874 A (VISCHER Jr.) 19 August 1941	1-3, 13, 15, 16

Further documents are listed in the continuation of Box C

See patent family annex

♦ Special categories of cited documents		
"A" document defining the general state of the art which is not considered to be of particular relevance	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention	
"E" earlier application or patent but published on or after the international filing date	"X" document of particular relevance, the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone	
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"Y" document of particular relevance, the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art	
"O" document referring to an oral disclosure, use, exhibition or other means	"&" document member of the same patent family	
"P" document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search  
07 October 2010

Date of mailing of the international search report

1 f OCT 2010

Name and mailing address of the ISA/AU  
AUSTRALIAN PATENT OFFICE  
PO BOX 200, WODEN ACT 2606, AUSTRALIA  
E-mail address pct@ipaustaliagov au  
Facsimile No +61 2 6283 7999Authorized officer  
**KURT TOBLER**  
AUSTRALIAN PATENT OFFICE  
(ISO 9001 Quality Certified Service)  
Telephone No +61 2 6283 2469

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

**PCT/AU20 10/00 1024**

This Annex lists the known "A" publication level patent family members relating to the patent documents cited in the above-mentioned international search report. The Australian Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

Patent Document Cited in Search Report		Patent Family Member					
US	5935084	EP	0904728	EP	1552784	JP	2008249728
		JP	11218455				
US	4096759	DE	2609882	FR	2344005	GB	1537003
<b>US</b>	2252874	NONE					
Due to data integration issues this family listing may not include 10 digit Australian applications filed since May 2001.							
END OF ANNEX							