

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2017/103330 A1

(43) International Publication Date

22 June 2017 (22.06.2017)

(51) International Patent Classification:

A61B 3/16 (2006.01)

(21) International Application Number:

PCT/FI2016/050871

(22) International Filing Date:

14 December 2016 (14.12.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

20155973 18 December 2015 (18.12.2015) FI

(71) Applicant: ICARE FINLAND OY [FI/FI]; Äyritie 22, 01510 Vantaa (FI).

(72) Inventors: MÄKKELI, Pauliina; Komentajankatu 6 D 32, 02600 Espoo (FI). HAULISTO, Rami; Maarukankuja 1 C 29, 01480 Vantaa (FI). RAUDASOJA, Matti; Pähkinätie 5 D 23, 01710 Vantaa (FI). PUKKI, Jussi; Kivihaantie 9 B 23, 00310 Helsinki (FI). HERRANEN, Teemu; Solistintie 2 B 5, 05810 Hyvinkää (FI). KUKKONEN, Ari; Kutomotie 8c A 26, 00380 Helsinki (FI). SALKOLA, Mika; Luukintie 22, 02940 Espoo (FI).

(74) Agent: BOCO IP OY AB; Itämerenkatu 5, 00180 Helsinki (FI).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

**Published:**

- with international search report (Art. 21(3))
- with amended claims (Art. 19(1))

(54) Title: APPARATUS FOR MEASURING INTRAOCULAR PRESSURE

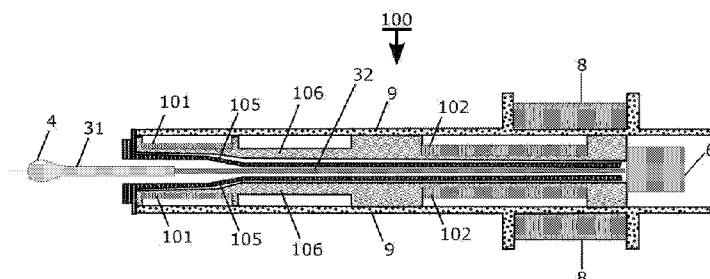


Figure 1 C

(57) **Abstract:** The apparatus of the invention for measuring intraocular pressure comprises a functional part (100) with a tubular probe base (105) and a probe (3) contactable with a surface of an eye to derive an intraocular pressure in the eye from variations in a velocity of the probe (3). The probe (3) is inside the tubular probe base (105). The probe (3) is partly formed of magnetic material. An induction coil (101, 102) gives the probe (3) a specific velocity. The apparatus also has means for measuring the variations in a velocity of the probe (3), means for processing and displaying the measurement data, and controlling operations. The apparatus is mainly characterized by means (6) for holding the probe (3) inside the tubular probe base (105), and means for releasing the probe (3) for the measurement.

## APPARATUS FOR MEASURING INTRAOCULAR PRESSURE

## TECHNICAL FIELD

The invention is concerned with an apparatus for measuring intraocular pressure. It

5 comprises a functional part with a tubular probe base and a probe contactable with a surface of an eye to derive an intraocular pressure in the eye from variations in a velocity of the probe, which is inside the tubular probe base. The probe is partly of magnetic material. An induction coil gives the probe a specific velocity. The apparatus also has means for measuring the variations in a velocity of the probe, means for processing and

10 displaying the measurement data, controlling operations, means for holding the probe (3) inside the tubular probe base, and means for releasing the probe for the measurement.

## BACKGROUND

Tonometry is a method for measuring intraocular pressure and the apparatus used for

15 the measurements is called tonometer. Various types of tonometers exist. In contact tonometry, there is a physical contact with the cornea during measurement. A probe is directed against the surface of the cornea, the elasticity of which is measured using various methods. The Goldmann tonometer and the Schiötz tonometer are examples of tonometers.

20 Two of the most commonly used principles are the measurement of the force required to flatten a certain area of the surface of the eye, or the measurement of the diameter of the area that is flattened by a known force. These methods require the patient's co-operation and cannot be applied without general anaesthesia.

Methods, such as those presented in US patent publications, 5148807, 5279300, and

25 5299573, in which the surface of the cornea is not touched, the intraocular pressure is instead measured with the aid of a water or air jet, or various kinds of waves, have also been developed. These methods are technically complex and thus expensive. Meters operating on the air-jet principle are widely used by opticians, but their cost has prevented them from being more extensively used by general practitioners.

Rebound tonometry is a type of contact tonometry, wherein a probe, which is partly of magnetic material is accelerated towards an eye by means of an inductive coil system. Upon contact with the cornea of the eye, the probe starts to decelerate and rebounds from the eye. As a result, a voltage is induced in an other coil and the intraocular pressure 5 is calculated from measurement data of parameters of the moving.

US patent 6, 093,147 is mentioned as prior art for such a tonometer. It comprises a probe, which is propelled at a constant velocity in the horizontal direction to impact the eye and includes a device for continuously determining the velocity of the probe. The tonometer disclosed is suitable for horizontal measurements.

10 The problem with the rebound tonometers of prior art is that measurements, in which the probe in the tonometer apparatus moves in an inclined direction, are not possible to make securely since the probe tend to fall from the apparatus when it is inclined. This means that the measurements have to be done with the patient in upright position if the probe is not prevented from falling by e.g. mechanical means and/or by regulating the driving 15 current and using a wide probe holder, which prevents the probe from falling from the device.

However, in some situations, it is necessary to perform intraocular pressure measurements when the patient is in a non-vertical position, such as during eye surgery. Consequently, an inclined measurement, especially a vertical measurement, is a very 20 useful and desired feature in tonometry.

US patent publication 5176139 discloses a method based on rebound technology, in which a freely-falling ball is dropped onto the eyelid and the height of the ball's rebound is measured. The amount of the ball rebound varies depending on the amount of intraocular pressure and the latter is judged against the amount of the ball rebound. The 25 method solves the above problem mechanically by having a spring lock to prevent the ball from falling and keep it in the top most position. Upon depressing the spring lock, the ball is released for the measurement. The patient can be either recumbent (by leaning back) or sitting during the measurement.

CN patent publication 104274153A is mentioned as prior art for a soft touch intraocular 30 pressure horizontal or vertical measuring device and method, the device comprising a small magnetic needle pressure measuring probe, a front end device, and a driving

adjusting circuit. The device has a magnetic induction coil connected with an electric solenoid skeleton that is provided with a permanent magnet and an iron core. When the power is on, the probe can be prevented from falling during a vertical measurement by introducing currents in the coils.

5 There is, however, need for a tonometer device, wherein the probe stays inside the tonometer whether the power is on or off. Also, there is need for a tonometer device, wherein the movement of a rebound type probe can be more easily controlled in all kind of measurements.

## 10 SUMMARY

The apparatus of the invention for measuring intraocular pressure comprises a functional part with a tubular probe base and a probe contactable with a surface of an eye to derive an intraocular pressure in the eye from variations in a velocity of the probe. The probe is inside the tubular probe base. The probe is partly of magnetic material. An induction coil 15 gives the probe a specific velocity. The apparatus also has means for measuring the variations in a velocity of the probe, means for processing and displaying the measurement data, controlling operations, means for holding the probe inside the tubular probe base, and means for releasing the probe for the measurement. The apparatus is mainly characterized in that the means for holding the probe is a magnetic circuit and the 20 means for releasing the probe is a magnetic coil.

The preferable embodiments of the invention have the features of the subclaims.

With inclined measurements is meant measurements in which the measurements are performed with the tonometer in such a position that the probe is during measurement moving in a direction forming an angle compared to the horizontal plane. Vertical 25 measurements, wherein this angle is 90°, is to be seen as a special case of an inclined measurement, in which the measurements are performed with the tonometer in such a position that the probe is moving vertically during measurement (i.e. perpendicularly to the horizontal plane).

Currently, in the rebound tonometer apparatuses of prior art, the probe does not fall from 30 the tonometer when the power is on even if the apparatus is inclined because the

measuring coil is pulling the probe back. However, the clinicians performing the measurement might not remember to switch the power on before inclining the apparatus for the measurement, which is a risk for the patient to get the probe in the eye if there is no additional means to prevent the probe from falling.

5 In the apparatus of the present invention, vertical and other inclined measurements are risk-free thanks to the inventive means for holding the probe inside the tonometer in a probe base. The probe stays inside the probe base of the tonometer independently of whether the power is on or off.

10 The means for holding the probe inside the probe base can e.g. be a magnetic circuit like in the invention, or it can be a mechanical lock, or a friction brake.

15 In the developing of the apparatus of the invention, the focus has been in the control of the influence of gravity on the probe. With the apparatus of the invention, an inclined/vertical measurement can be performed by decreasing the driving current as a function of the inclination degree because the influence of gravity on the probe also changes as a function of the inclination degree.

The intraocular pressure is determined from the movement parameters, which are examined from the induced voltage in the measuring coil.

20 The improvement of the invention of holding the probe inside the probe base during inclined/vertical measurement also when the power is off improves the usability of the device. Yet, the invention retains the apparatus' as a simple, economical, and precise measuring basic construction by means of which intraocular pressure also can be measured in patients incapable of co-operating. In addition, the apparatus of the invention is also suitable for extensive screening campaigns, as the measurements are rapid and require neither local anaesthesia nor specially trained operators. The position of the 25 apparatus during the measurements is now more flexible including the possibility for both horizontal and inclined/vertical measurements in a secure way.

Next, the invention will be described by means of some example embodiments and accompanying figures to which the invention is not restricted.

## FIGURES

Figure 1A presents a first type of a probe that can be used in the embodiments of a tonometer of the invention

5

Figure 1B presents a second type of a probe that can be used in the embodiments of a tonometer of the invention

Figure 1C presents a first embodiment of a tonometer of the invention, wherein the holding mechanism is a magnet and the releasing actuator is a magnetic coil

10

Figure 2 presents a second embodiment of a tonometer of the invention, wherein the holding mechanism is a magnet and the releasing actuator is a magnetic coil

Figure 3 presents a third embodiment of a tonometer of the invention, wherein the holding mechanism is a magnet and the releasing actuator is a magnetic coil

Figure 4 presents a fourth embodiment of a tonometer of the invention, wherein the holding mechanism is a magnet and the releasing actuator is a magnetic coil

20

Figure 4B is a cross-sectional view of the magnet and the releasing actuator of figure 4

Figure 5 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnet and the releasing actuator is a magnetic coil

25

Figure 6 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnet and the releasing actuator is a magnetic coil

Figure 7 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnet and the releasing actuator is a magnetic coil

30

Figure 8 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnet and the releasing actuator is a magnetic coil

Figure 9 presents a tonometer, wherein the holding mechanism is a friction brake caused by a solid object and the releasing actuator is a piezoelectric element, a pneumatic membrane, a hydraulic membrane or a magnetic coil

5 Figure 10 presents a tonometer, wherein the holding mechanism is a mechanical catch and the releasing actuator is a piezoelectric element, a pneumatic membrane, a hydraulic membrane or a magnetic coil

10 DETAILED DESCRIPTION

Figure 1A presents a probe 3 that can be used in the embodiments of an apparatus of the invention for measuring intraocular pressure, i.e. in a tonometer. The probe 3 is formed of a rear part 32 of magnetic material, such as steel, and a front part 31 of non-15 magnetic material, such as a plastic material. The front part 31 of the probe 3 has a tip 4, which impacts the eye in the measurement of the intraocular pressure.

Figure 1B presents a probe 3 that can be used in the embodiments of an apparatus of the invention for measuring intraocular pressure, i.e. in a tonometer. The probe 3 is partly 20 of magnetic material and the probe 3 has a tip 4, which impacts the eye in the measurement of the intraocular pressure.

Figure 1C presents a first embodiment of a functional part 100 of the tonometer of the invention, wherein the probe 3 of figure 1A and figure 1B can be used.

25 The functional part 100 together with other components belonging to a tonometer are inside a tonometer case. Examples of other components in the tonometer are means for adjusting the distance from which the probe is launched for impacting the eye, batteries, from which the apparatus gets its operating power, a circuit board on which the electronics 30 of the apparatus are assembled, a display, a processing unit, and a socket, to which an external recharging device can be connected. The means for adjusting the distance can be an adjustable forehead support. Only the functional part 100 of the tonometer is presented in the figures. The above components of a tonometer are closer presented in WO publication 03/105681.

The functional part 100 has a frame pipe 9, inside which there is an inner tube around the probe 3, which is partly of magnetic material. The inner tube is hereafter referred to as the probe base 105.

5 The probe 3 is accelerated towards an eye by means of a driving inductive coil system 101 in the front end of the probe base 105. The force pushing the probe 3 is generated in the coil 101 by a voltage fed to the coil 101. So power is supplied to the front coil 101 causing the probe 3 to start moving and to impact the eye. Upon contact with the cornea of the eye, the probe 3 starts to decelerate and rebounds from the eye.

10 As a result, a voltage, which is dependent on the intraocular pressure, is induced in another coil 102. The coils 101 and 102 are mounted on a coil frame 106.

15 This voltage and other parameters, such as the speed of the probe 3, are detected by the rear coil 102 and recorded and processed with a data processing unit (not shown). The intraocular pressure is calculated by means of an algorithm from the measurement data of parameters of the moving probe 3 and the result is presented on a display of the tonometer.

20 The tonometer of the invention might also comprise means for correcting the measurement results in proportion to how much kinetic energy is lost or gained in the impact and rebound of the probe.

25 Instead of the front coil 101 giving the probe 3 the launching power, it is possible to use the rear coil 102.

One of the coils 101 and 102 are intended to operate also as a retainer for holding the probe 3 in place when the power is switched on in the tonometer.

30 After the impact has occurred and the measurement result has been obtained, there is a risk that the probe 3 detaches due to movements of the tonometer or for other reasons. This is prevented in the embodiment of figure 1C of the invention by using a magnetic circuit 6 (such as a magnet), which magnetic circuit 6 can be located behind the rear part of the probe base 105 (in the opposite end of the apparatus than the tip 4 of the probe 3).

The magnetic circuit 6 holds the probe 3 inside the probe base 105 in any position of the apparatus once the probe 3 is loaded into the probe base 105.

The magnetic circuit 6 can consist of a permanent magnet. Means for releasing the probe, 5 such as a releasing coil 8, is placed around the frame pipe 9 in order to cancel the effect of the magnetic circuit 6 during measurement. Consequently, the probe 3 can move. The frame pipe 9 works as a case in the functional part 100 of the apparatus.

When current is flown into the releasing coil 8 during measurement, the resulting 10 magnetic field compensates the effect of the magnetic field of the magnetic circuit 6 and the probe 3 can move.

The control functions of the releasing coil 8 is integrated into the electric circuit board of 15 the tonometer. The releasing coil 8 gets its power from the power supply and the currents flow in the releasing coil 8 and the driving coil 101 flow during a measurement.

The position, shape, dimensions, material, layers and turns of the magnetic coil are not fixed and can be adapted suitable case by case. Similarly, the position, shape, dimensions, material and grade of the magnet 6 are not fixed and can be adapted suitable 20 case by case.

Figure 2 presents a second embodiment of a tonometer of the invention. In this embodiment, the releasing coil 8 is wrapped around the frame pipe 9 like in the first 25 embodiment of figure 1B but the frame pipe is split into two parts, i.e. a rear frame part 9A and a front frame part 9B.

Figure 3 presents a third embodiment of a tonometer of the invention. The frame pipe 9 30 is in one part like that in figure 1C. A centralizing part 10 between the frame pipe 9 and the magnetic circuit 6 facilitates the mounting and keeping of the magnet 6 in place.

The embodiment of figure 4 otherwise corresponds to that of figure 1C but the releasing coil 8 is directly wound around the magnet 6, whereby the means 6 for holding the probe 3 inside the probe base 105 are integrated with the means 8 for releasing the probe 3.

5

Figure 4B is a cross-sectional view of the magnet 6 around which the releasing coil 8 has been wound.

10 Figure 5 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnet and the releasing actuator is a magnetic coil.

A magnet 6 generates a magnetic field and the probe 3 turns parallel to the field. Because of the turning, the probe touches the probe base 105, which causes friction between the 15 contact areas of the probe 3 and the probe base 105. The friction prevents the probe 3 from moving and falling out from the device. During a measurement, current flows into the releasing coil 8 and the produced magnetic field compensates the effect of the magnetic circuit 6. Consequently, the probe can move.

20

Figure 6 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnetic circuit 6 and the releasing actuator is a magnetic coil 8. Here the magnetic circuit 6 is on the frame pipe 9 of the functional part 100 and the releasing coil 8 is inside the frame pipe 9. The releasing coil 8 is outside the rear part of the coil frame 106.

25

Figure 7 presents a tonometer, wherein the holding mechanism is a friction brake caused by a magnetic circuit 6 and the releasing actuator is a magnetic coil 8. Here the position of the magnetic circuit 6 is like in figure 6 around the releasing coil 8 with the frame pipe 9 there between, but the magnetic circuit 6 and the releasing coil 8 are in the front part of 30 the functional part 100 between the driving coil 101 and the measuring coil 102.

Figure 8 presents a tonometer, wherein the holding mechanism is a friction brake caused by a holding magnet and the releasing actuator is a magnetic coil. The releasing coil 8, which is around the magnet 6 is outside the rear part of the functional part 100, the combination being mounted on the frame pipe 9.

5 A magnet 6 generates a magnetic field which is guided via a magnetic material 11 placed in the vicinity of the magnet 6. The magnetic field affects the probe 3 and it tries to turn parallel to the field. Because of the turning, the probe 3 touches the probe base 105, which causes friction between the contact areas of the probe base 105 and the probe 3.

10 10 The friction prevents the probe 3 from moving and falling out from the device. During a measurement, current flows in the releasing coil 8 and a produced magnetic field compensates the effect of the magnet 6. Consequently, the probe 3 can move.

Figure 9 presents a tonometer, wherein the holding mechanism is a friction brake caused  
15 by a solid object and the releasing actuator is a piezoelectric element, a pneumatic membrane, a hydraulic membrane or a magnetic coil.

A solid object 12 is in contact with the probe 3 and causes friction between the contact areas of the probe 3 and the solid object 12. The friction holds the probe 3 so that it can  
20 not move or fall out from the device. During the measurement, the releasing actuator 8' shifts the solid object 12 so that it does not touch the probe 3 anymore. Consequently, there is no friction and the probe 3 can move.

The releasing actuator 8' is on the frame pipe 9 at the rear part of the functional part 100 and the solid object touches the rear end of the probe 3, which is partly inside the  
25 releasing actuator 8'.

Figure 10 presents a tonometer, wherein the holding mechanism is a mechanical catch and the releasing actuator is a piezoelectric element, a pneumatic membrane, a hydraulic membrane or a magnetic coil.

30 There is a notch 13 in the rear part of the probe 3. A solid object 12' is placed on the notch 13 and these work together as a mechanical catch. The catch prevents the probe

3 from moving and falling out from the device. During the measurement, the releasing actuator 8' lifts the solid object 12' and the probe 3 can move.

The releasing actuator 8' is on the frame pipe 9 at the rear part of the functional part 100 and the mechanical catch is at the rear end of the probe 3.

5

10

## CLAIMS

1. An apparatus for measuring intraocular pressure, which comprises a functional part (100) with  
a tubular probe base (105),  
5 a probe (3) contactable with a surface of an eye to derive an intraocular pressure in the eye from variations in a velocity of the probe, the probe (3) being inside the tubular probe base (105), and the probe (3) being partly of magnetic material,  
an induction coil (101, 102) for giving the probe (3) a specific velocity,  
means for measuring the variations in a velocity of the probe (3),  
10 means for processing and displaying the measurement data,  
controlling operations,  
means (6) for holding the probe (3) inside the tubular probe base (105), and  
means (8) for releasing the probe (3) for the measurement,  
characterized in that the means (6) for holding the probe (3) is a magnetic  
15 circuit and the means (8) for releasing the probe (3) is a magnetic coil.
2. An apparatus according to Claim 1, characterized in that the magnetic circuit (6) is located behind the rear part of the probe base (105) and the means (8) for releasing the probe (3) is located at the rear part of the probe base (105).  
20
3. An apparatus according to Claim 1, characterized in that the magnetic circuit (6) is located behind the rear part of the probe base (105) and the means (8) for releasing the probe (3) are located at the rear part of the probe base (105), and further characterized by a centralized part (10) between the frame pipe (9) and the magnetic  
25 circuit (6), which centralized part (10) keeps the magnetic circuit (6) in place.
4. An apparatus according to Claim 1, characterized in that the means (6) for holding the probe (3) inside the tubular probe base (105) and the means (8) for releasing the probe (3) are integrated, whereby the means (8) for releasing the probe (3) are wound in the form of a releasing coil around the means (6) for holding the probe (3) inside the tubular probe base (105).  
30

5. An apparatus according to any of the above claims, characterized in that one of the means (101, 102) is intended also to operate, when the power is switched on in the apparatus, as a retainer for holding the probe (3) in place.
- 5 6. An apparatus according to any of the above claims, characterized in that it includes means for correcting the measurement results in proportion to how much kinetic energy is lost or gained in the impact and rebound of the probe (3).

10

## AMENDED CLAIMS

received by the International Bureau on 29 May 2017 (29.05.2017)

1. An apparatus for measuring intraocular pressure, which comprises a functional part (100) with  
a tubular probe base (105),  
5 a probe (3) contactable with a surface of an eye to derive an intraocular pressure in the eye from variations in a velocity of the probe, the probe (3) being inside the tubular probe base (105), and the probe (3) being partly of magnetic material, an induction coil (101, 102) for giving the probe (3) a specific velocity, means for measuring the variations in a velocity of the probe (3),  
10 means for processing and displaying the measurement data, controlling operations, means (6) for holding the probe (3) inside the tubular probe base (105), and means (8) for releasing the probe (3) for the measurement,  
characterized in that the means (6) for holding the probe (3) is a magnetic circuit, which is located behind the rear part of the probe base (105) in the opposite end of the apparatus than the tip (4) of the probe (3), and the means (8) for releasing the probe (3) is a magnetic coil.  
15
2. An apparatus according to Claim 1, characterized in that the means (8) for releasing the probe (3) is located at the rear part of the probe base (105).  
20
3. An apparatus according to Claim 1, characterized in that the means (8) for releasing the probe (3) are located at the rear part of the probe base (105), and further characterized by a centralized part (10) between the frame pipe (9) and the magnetic circuit (6), which centralized part (10) keeps the magnetic circuit (6) in place.  
25
4. An apparatus according to Claim 1, characterized in that the means (6) for holding the probe (3) inside the tubular probe base (105) and the means (8) for releasing the probe (3) are integrated, whereby the means (8) for releasing the probe (3) are wound in the form of a releasing coil around the means (6) for holding the probe (3) inside the tubular probe base (105).  
30

5. An apparatus according to any of the above claims, characterized in that one of the means (101, 102) is intended also to operate, when the power is switched on in the apparatus, as a retainer for holding the probe (3) in place.
- 5 6. An apparatus according to any of the above claims, characterized in that it includes means for correcting the measurement results in proportion to how much kinetic energy is lost or gained in the impact and rebound of the probe (3).

10

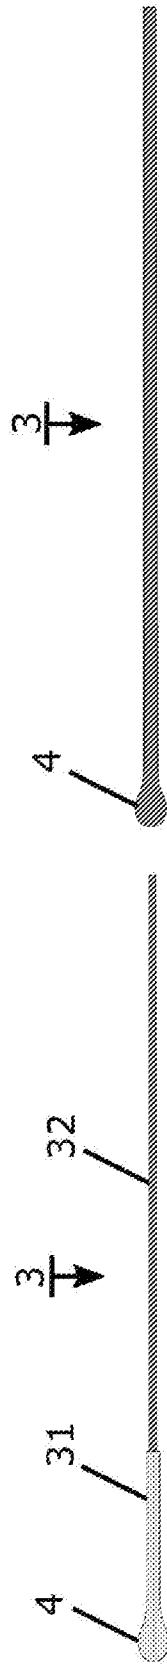


Figure 1 A

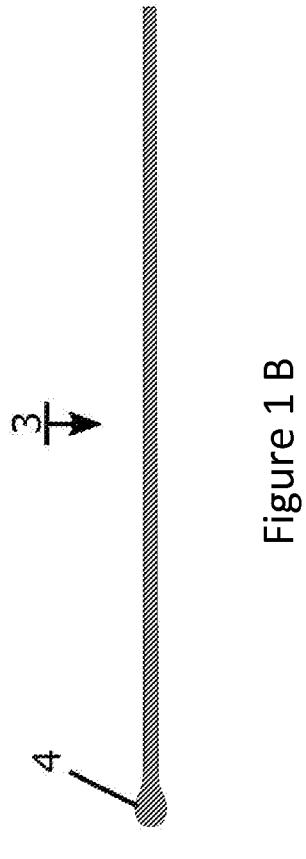


Figure 1 B

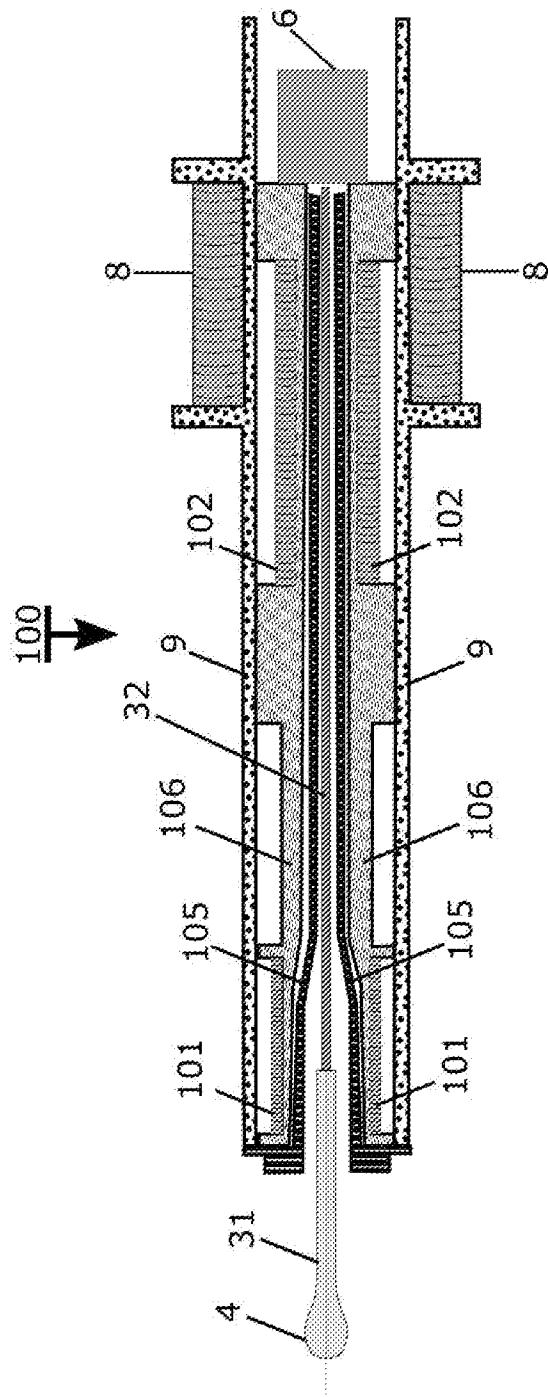


Figure 1 C

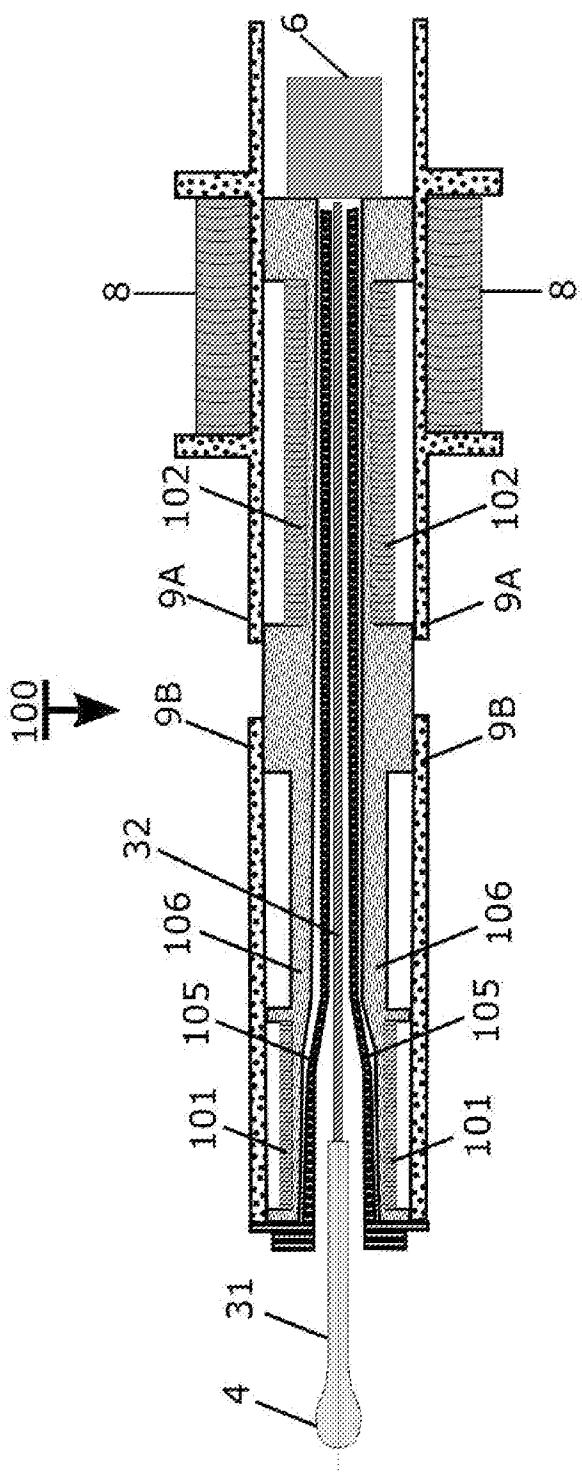


Figure 2

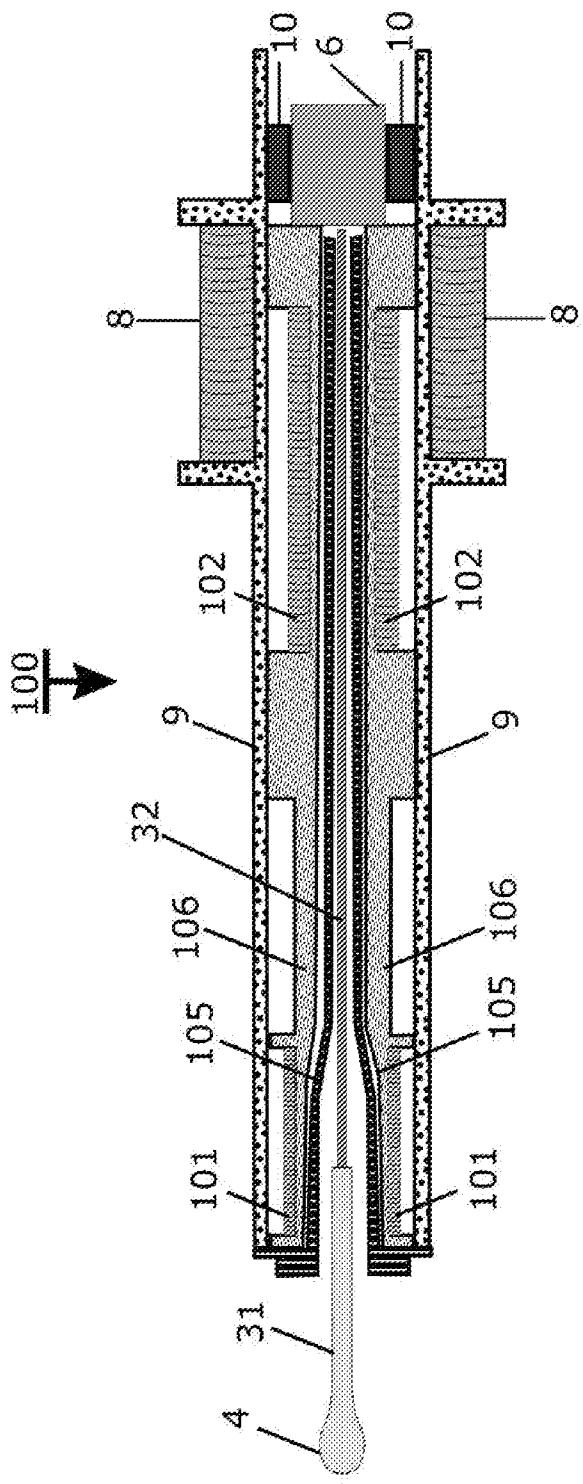


Figure 3

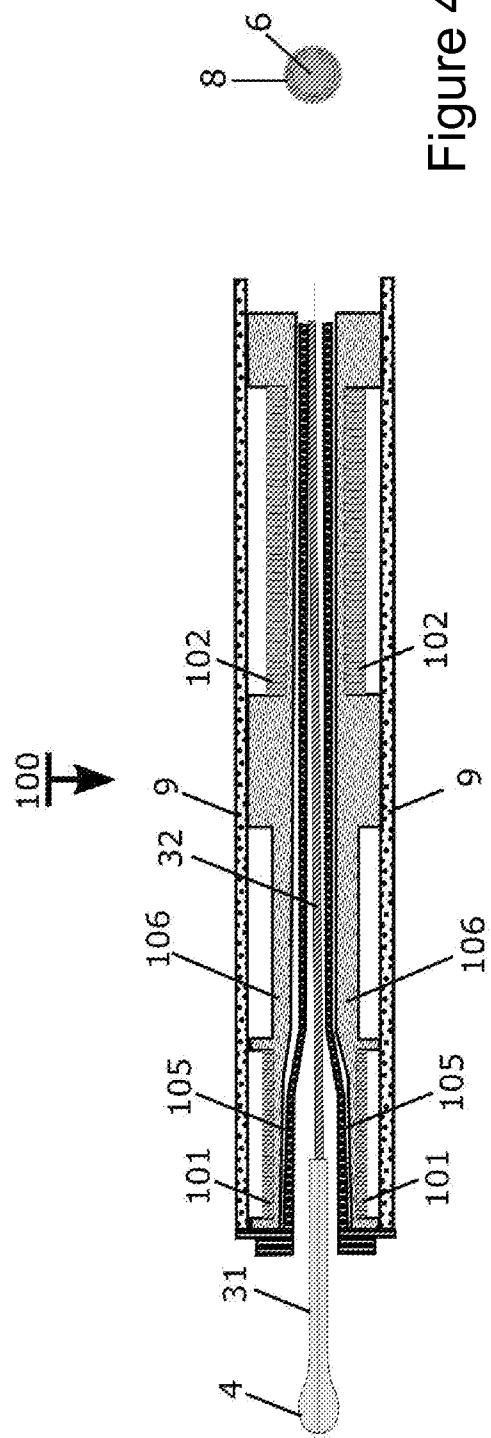


Figure 4B

Figure 4

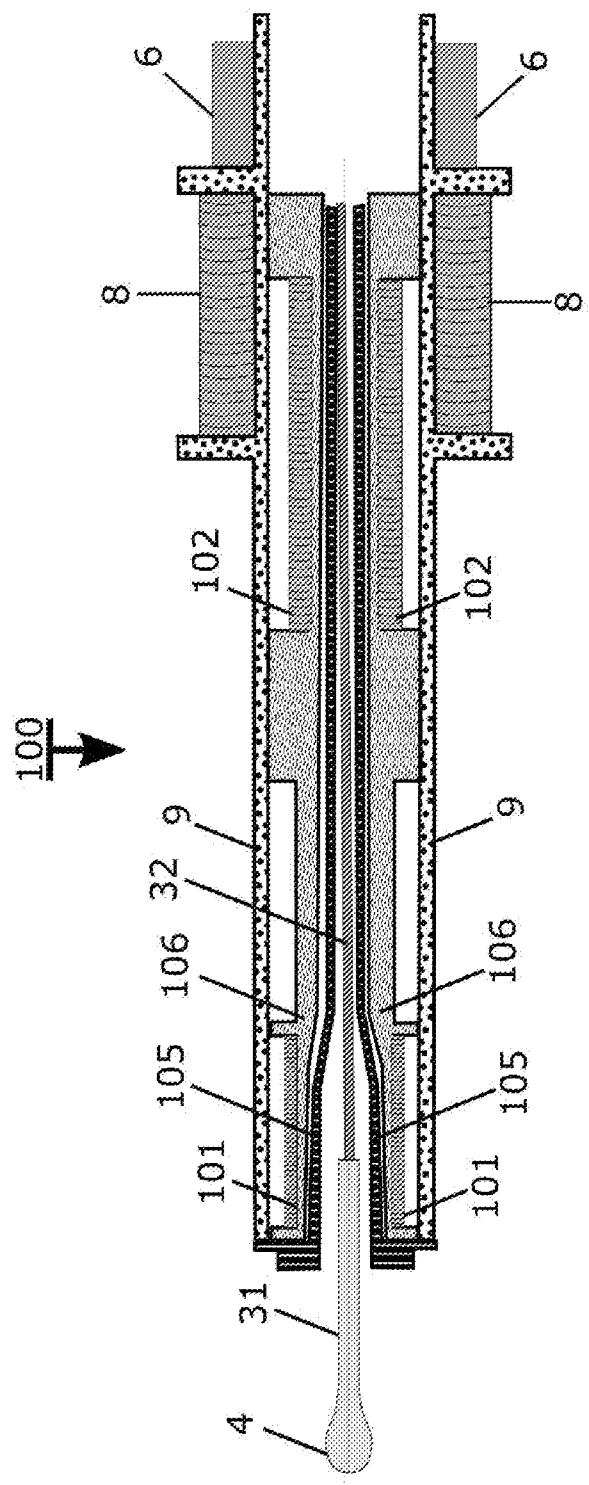


Figure 5

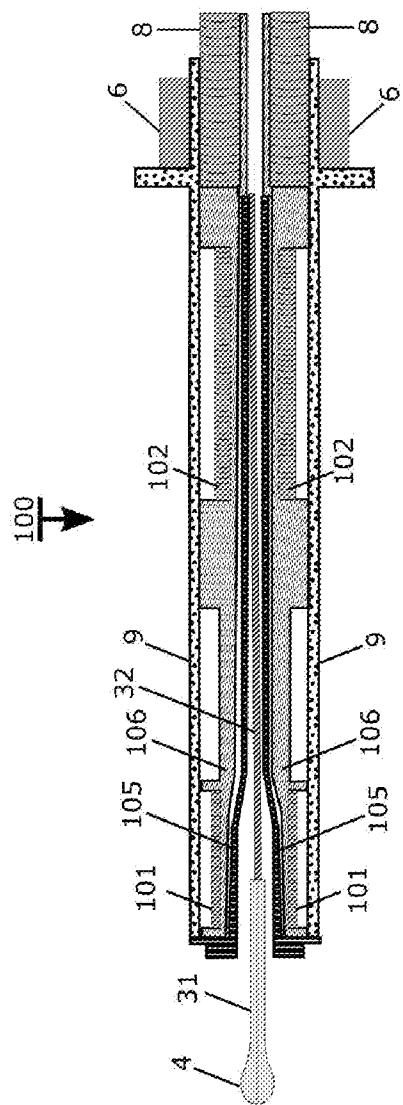


Figure 6

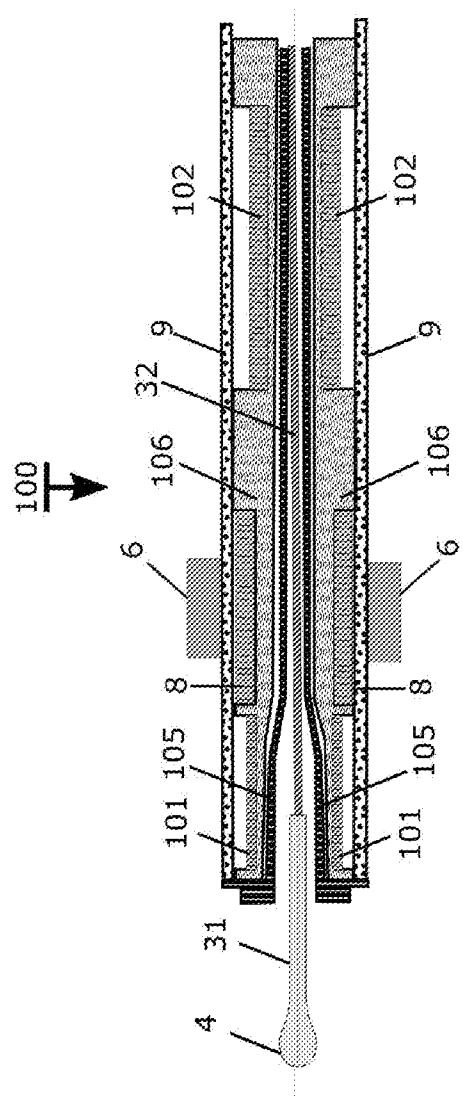


Figure 7

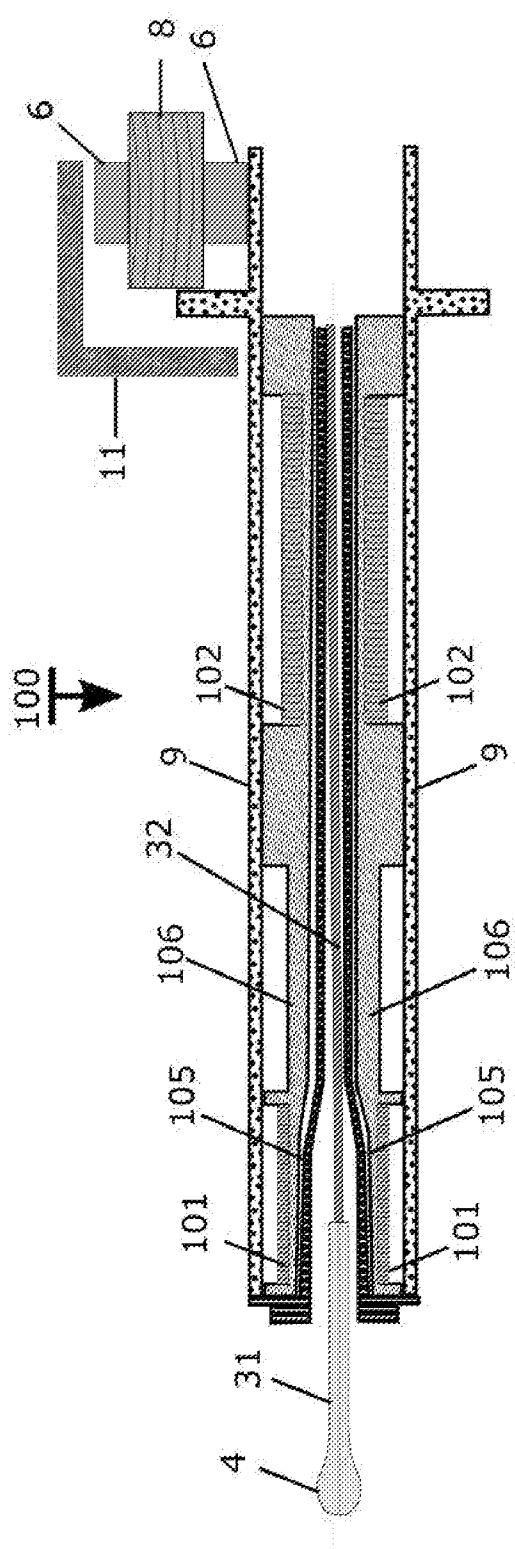


Figure 8

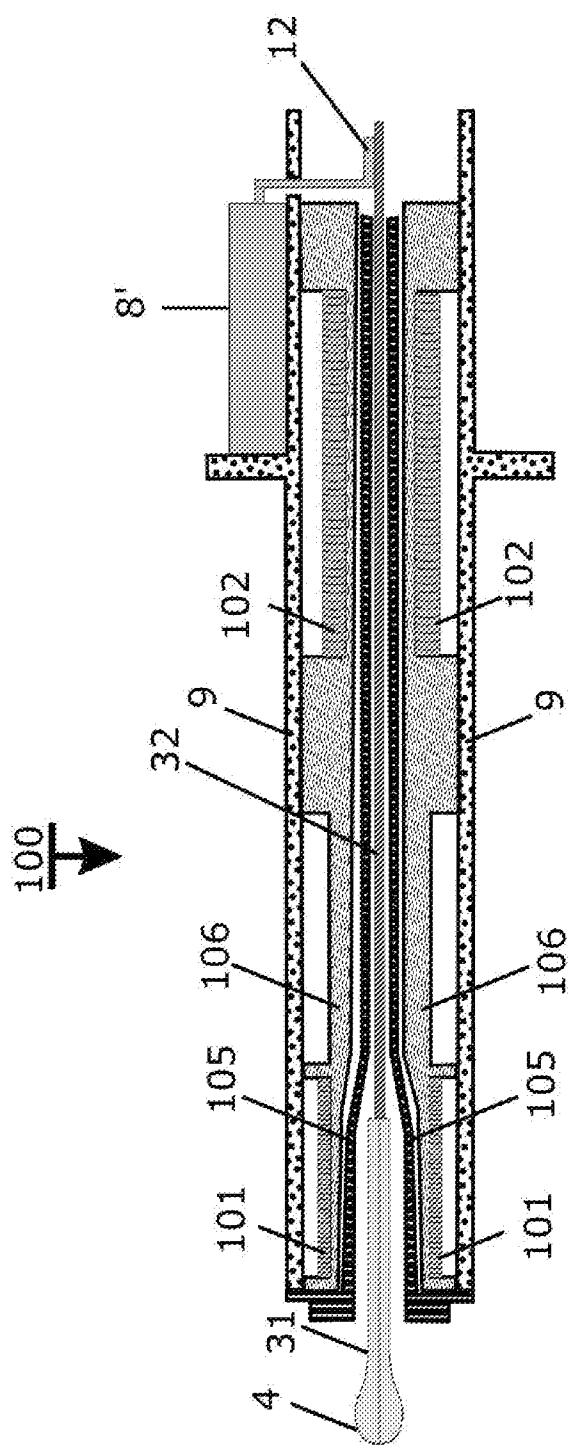


Figure 9

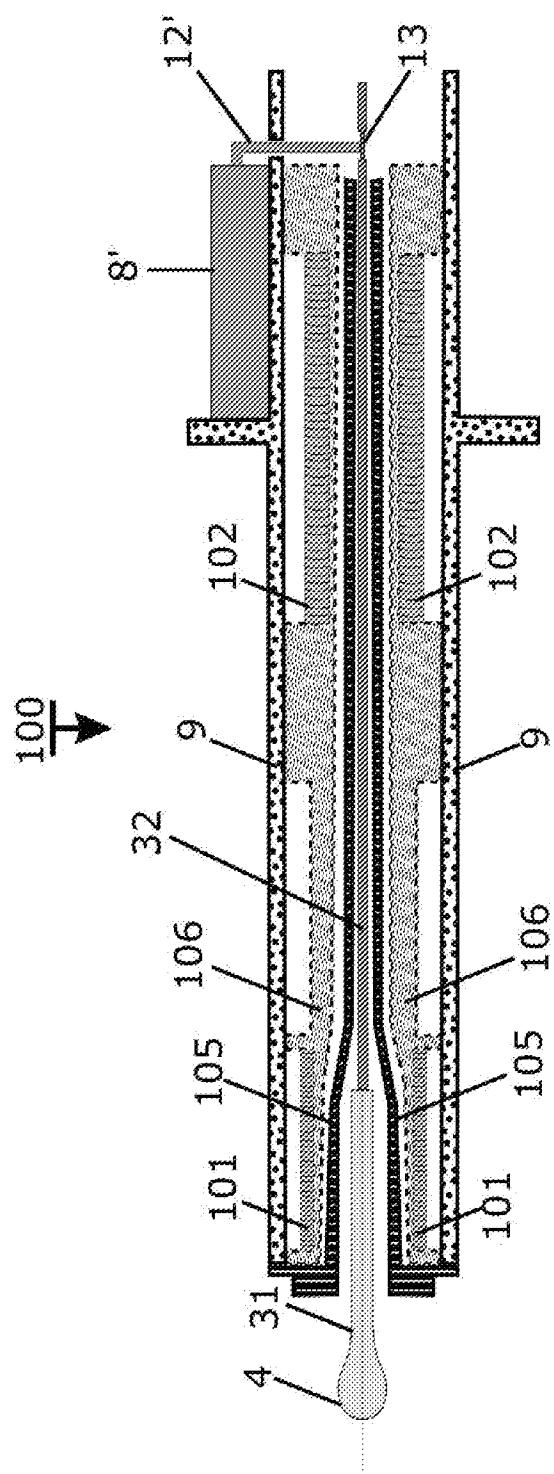


Figure 10

# INTERNATIONAL SEARCH REPORT

International application No  
PCT/FI2016/050871

**A. CLASSIFICATION OF SUBJECT MATTER**  
INV. A61B3/16  
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 03/105681 A1 (TIOLAT OY [FI]; KONTIOLA ANTTI [FI]) 24 December 2003 (2003-12-24) cited in the application pages 4-7 ----- US 6 093 147 A (KONTIOLA ANTTI [FI]) 25 July 2000 (2000-07-25) cited in the application column 2, line 41 - column 3, line 24; claims 1-3,5 -----	1-6
A	WO 2006/067266 A1 (TIOLAT OY [FI]; KONTIOLA ANTTI [FI]) 29 June 2006 (2006-06-29) claim 1 -----	1
X	US 2005/137473 A1 (KONTIOLA ANTTI [FI]) 23 June 2005 (2005-06-23) paragraphs [0015] - [0035] -----	1-6



Further documents are listed in the continuation of Box C.



See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier application or patent but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
15 March 2017	27/03/2017
Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer  Martelli, Luca

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No
PCT/FI2016/050871

Patent document cited in search report	Publication date	Patent family member(s)		Publication date
WO 03105681	A1 24-12-2003	AT 383809 T AT 387138 T AU 2003239630 A1 AU 2003244665 A1 DE 60318705 T2 DE 60319392 T2 DK 1513442 T3 DK 1545294 T3 EP 1513442 A1 EP 1545294 A1 ES 2300583 T3 ES 2300592 T3 FI 20021172 A JP 4478014 B2 JP 4478015 B2 JP 2005529670 A JP 2005529671 A WO 03105680 A1 WO 03105681 A1		15-02-2008 15-03-2008 31-12-2003 31-12-2003 08-01-2009 02-04-2009 26-05-2008 30-06-2008 16-03-2005 29-06-2005 16-06-2008 16-06-2008 18-12-2003 09-06-2010 09-06-2010 06-10-2005 06-10-2005 24-12-2003 24-12-2003
US 6093147	A 25-07-2000	NONE		
WO 2006067266	A1 29-06-2006	AT 497720 T CN 101083934 A DK 1853156 T3 EP 1853156 A1 ES 2356381 T3 FI 20041641 A JP 4866367 B2 JP 2008523939 A PT 1853156 E US 2009306493 A1 WO 2006067266 A1		15-02-2011 05-12-2007 02-05-2011 14-11-2007 07-04-2011 22-06-2006 01-02-2012 10-07-2008 05-04-2011 10-12-2009 29-06-2006
US 2005137473	A1 23-06-2005	NONE		